

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR041219\
 Data File : PR037128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 17:25
 Operator : SM\SJ
 Sample : K2316-07RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 20190175-AMND-COMP-CS-2RE

Manual Integrations
 APPROVED

mohammad
 4/15/2019 4:44:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 04:10:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.390	3.463	19599687	73370979	12.302m	12.525m
2) SA Decachlor...	10.026	8.316	19554581	78846703	10.437	9.878m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR041219\
Data File : PR037128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 17:25
Operator : SM\SJ
Sample : K2316-07RE
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
20190175-AMND-COMP-CS-2RE


Manual Integrations
APPROVED

mohammad
4/15/2019 4:44:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 04:10:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

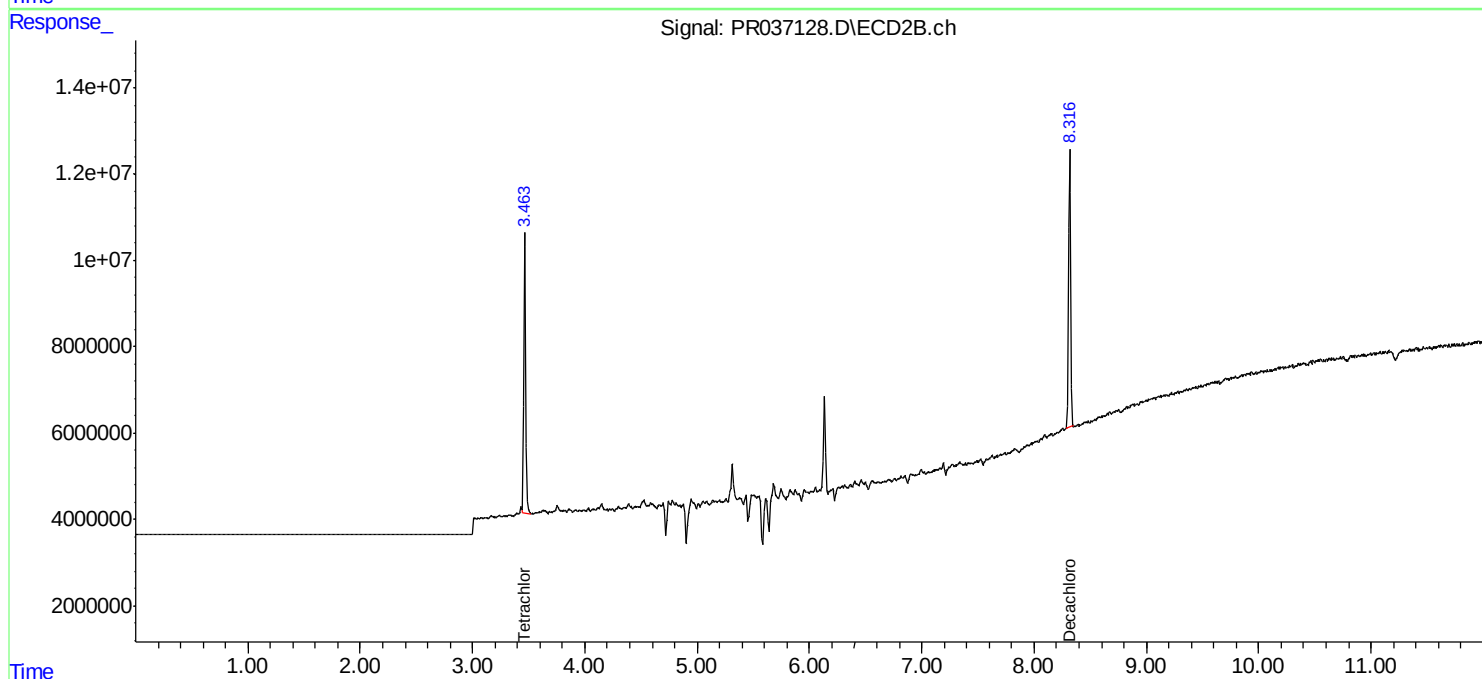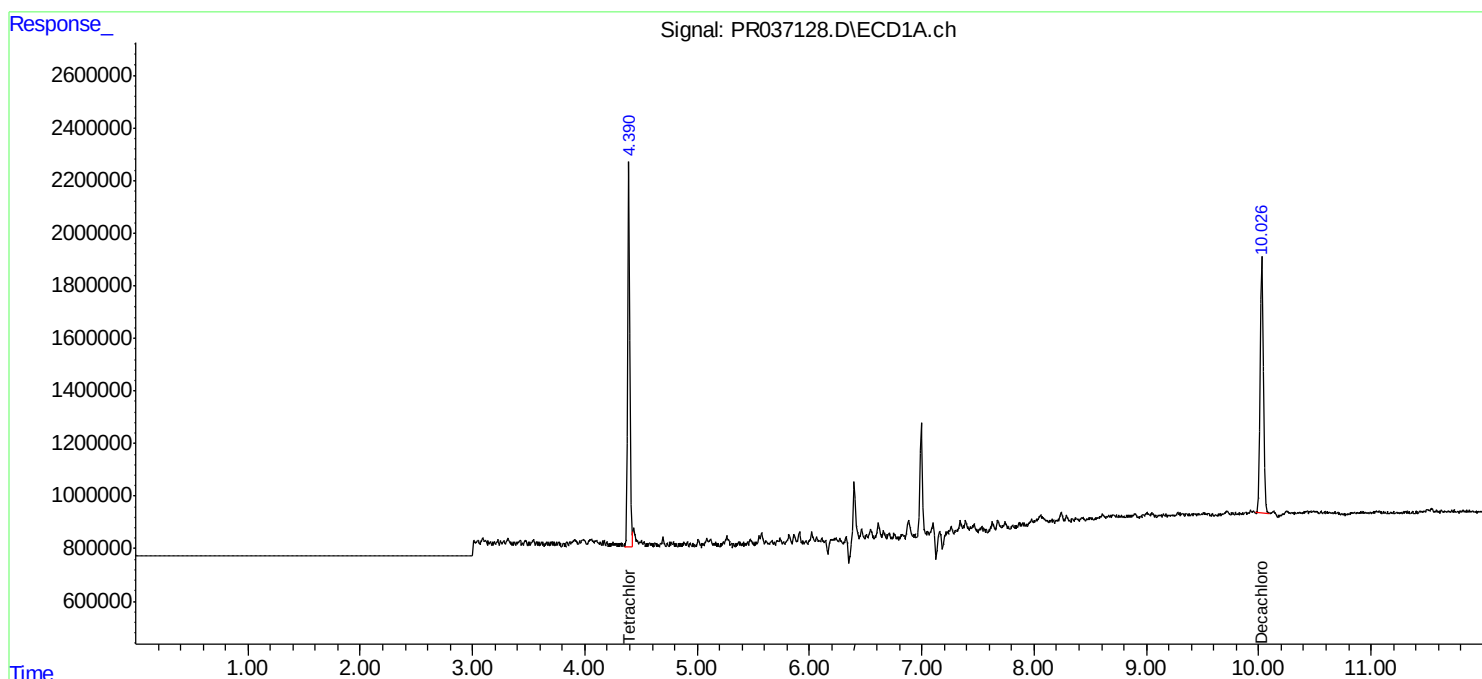

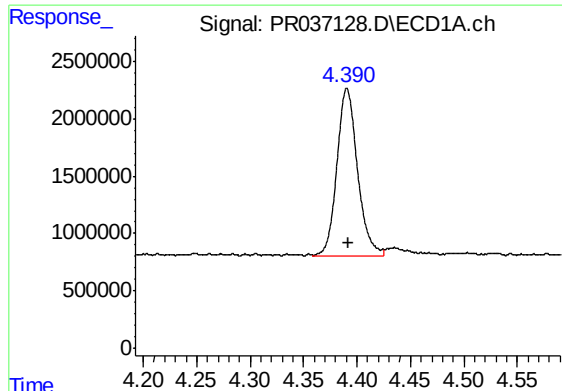


#1 Tetrachloro-m-xylene

R.T.: 4.390 min
Delta R.T.: -0.002 min
Response: 19599687
Conc: 12.30 ng/ml m

Instrument :
ECD_R
ClientSampleId :
20190175-AMND-COMP-CS-2RE


Manual Integrations
APPROVED

mohammad
4/15/2019 4:44:40 PM

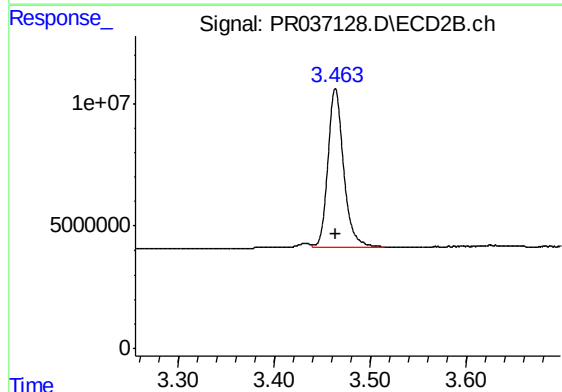


#1 Tetrachloro-m-xylene

R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 73370979
Conc: 12.53 ng/ml m

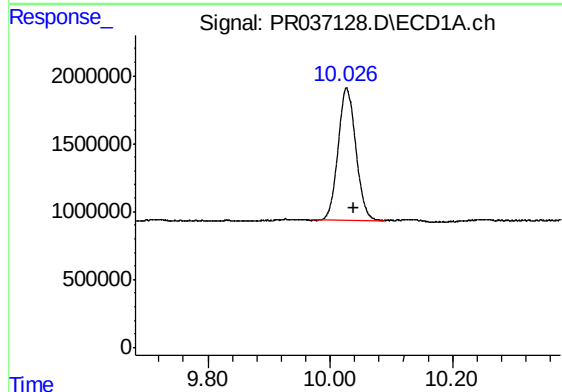

#2 Decachlorobiphenyl

R.T.: 10.026 min
Delta R.T.: -0.012 min
Response: 19554581
Conc: 10.44 ng/ml

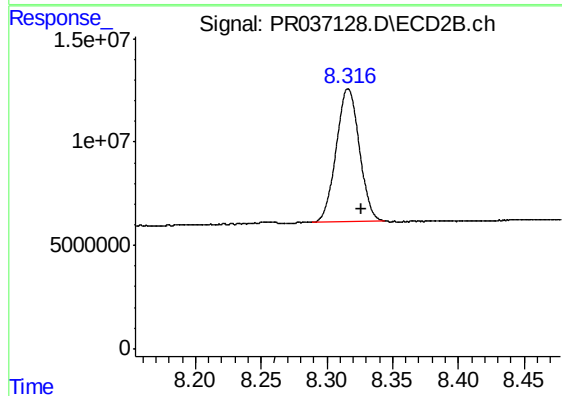

#2 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.010 min
Response: 78846703
Conc: 9.88 ng/ml m