

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 20:09
 Operator : SM\SJ
 Sample : K1560-11
 Misc : AR1232 MDL 25PPB
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:53:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.363	3.408	29326228	118.0E6	23.442	24.615
2)	SA Decachlor...	9.996	8.247	40288213	198.1E6	30.462	34.019
Target Compounds							
3)	L1 AR-1016-1	5.525	4.452	631043	2442649	14.645	13.415
4)	L1 AR-1016-2	5.546	4.468	1169011	3708876	16.882	13.146
5)	L1 AR-1016-3	5.607	4.638	689979	1709662	17.109	11.891 #
6)	L1 AR-1016-4	5.705	4.681	446044	1809774	13.582	16.358
7)	L1 AR-1016-5	5.998	4.886	437571	5464722	12.761	35.950 #
8)	L2 AR-1221-1	0.000	3.611	0	1560036	N.D.	30.638 #
9)	L2 AR-1221-2	4.665	3.697	563683	2344268	62.327	63.127
10)	L2 AR-1221-3	4.735	3.769	782750	3365187	25.539	27.483
11)	L3 AR-1232-1	4.735	3.769	782750	3365187	26.760	28.764
12)	L3 AR-1232-2	5.258	4.468	427081	3708876	25.275	26.832
13)	L3 AR-1232-3	5.546	4.638	1169011	1709662	34.582	24.354 #
14)	L3 AR-1232-4	5.705	4.721	446044	1979252	28.416	33.169
15)	L3 AR-1232-5	5.794	4.886	436833	5464722	37.350	80.077 #
16)	L4 AR-1242-1	5.525	4.452	631043	2442649	18.444	16.669
17)	L4 AR-1242-2	5.546	4.468	1169011	3708876	21.075	16.256
18)	L4 AR-1242-3	5.607	4.638	689979	1709662	20.962	14.786 #
19)	L4 AR-1242-4	5.705	4.721	446044	1979252	16.910	18.008
20)	L4 AR-1242-5	6.436	5.227	1889824	7117096	58.729	42.952 #
21)	L5 AR-1248-1	5.525	4.452	631043	2442649	27.548	24.265
22)	L5 AR-1248-2	5.794	4.681	436833	1809774	12.476	13.261
23)	L5 AR-1248-3	5.998	4.721	437571	1979252	10.696	14.140 #
24)	L5 AR-1248-4	6.374	4.886	5063448	5464722	103.432	30.707 #
25)	L5 AR-1248-5	6.436	5.250	1889824	21553426	40.007	110.184 #
26)	L6 AR-1254-1	6.374	5.227	5063448	7117096	92.685	20.661 #
27)	L6 AR-1254-2	6.592	5.374	3039511	13621099	35.468	45.479 #
28)	L6 AR-1254-3	6.970	5.767	2086404	6075444	22.937	12.828 #
29)	L6 AR-1254-4	7.237	5.984	345713	621333	5.159	1.772 #
30)	L6 AR-1254-5	0.000	6.394	0	4261955	N.D.	9.624 #
31)	L7 AR-1260-1	7.137	5.888	892127	75385	13.520	0.258 #
32)	L7 AR-1260-2	0.000	6.069	0	5923434	N.D.	12.861 #
33)	L7 AR-1260-3	0.000	6.212	0	221001	N.D.	0.620 #
34)	L7 AR-1260-4	0.000	6.700	0	1434541	N.D.	4.707 #
35)	L7 AR-1260-5	0.000	6.927	0	369378	N.D.	0.426 #
36)	L8 AR-1262-1	0.000	6.496	0	5634755	N.D.	22.483 #
37)	L8 AR-1262-2	0.000	6.927	0	369378	N.D.	0.294 #
38)	L8 AR-1262-3	0.000	7.258	0	43253636	N.D.	78.892 #
39)	L8 AR-1262-4	0.000	7.258	0	43253636	N.D.	48.186 #
40)	L8 AR-1262-5	0.000	7.764	0	589463	N.D.	1.541 #
41)	L9 AR-1268-1	0.000	7.258	0	43253636	N.D.	35.136 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 20:09
 Operator : SM\SJ
 Sample : K1560-11
 Misc : AR1232 MDL 25PPB
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:53:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.258	0	43253636	N.D.	40.847 #
43) L9	AR-1268-3	0.000	7.467	0	12963665	N.D.	14.628 #
44) L9	AR-1268-4	0.000	7.764	0	589463	N.D.	1.625 #
45) L9	AR-1268-5	0.000	8.027	0	4929459	N.D.	1.938 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
Data File : PR037302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 20:09
Operator : SM\SJ
Sample : K1560-11
Misc : AR1232 MDL 25PPB
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:53:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

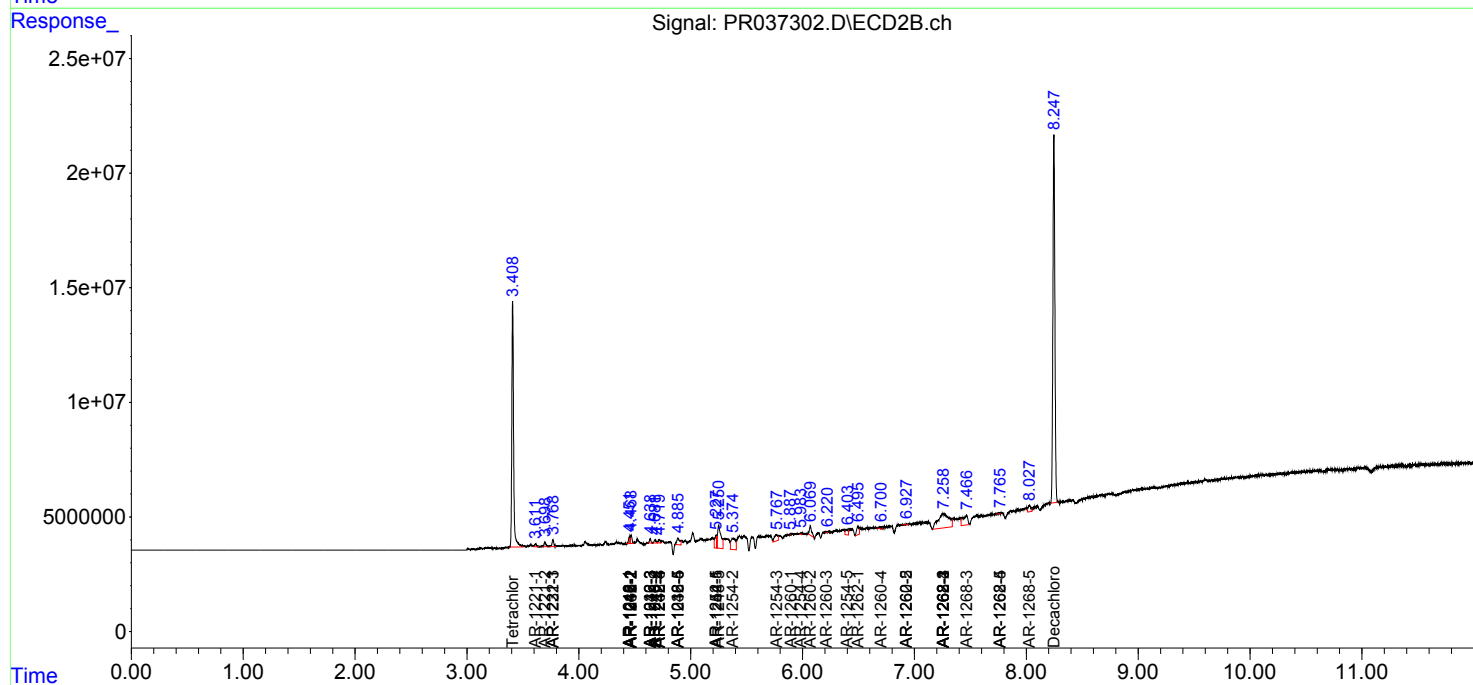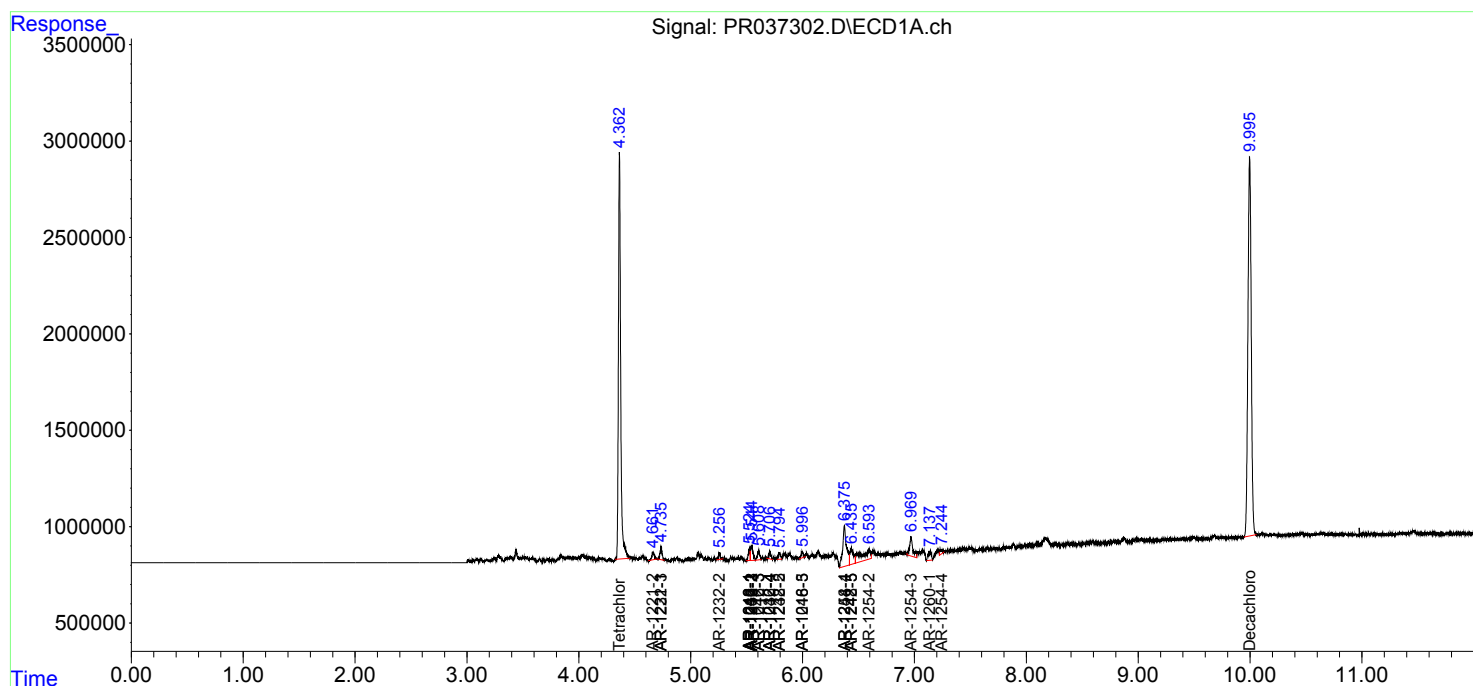


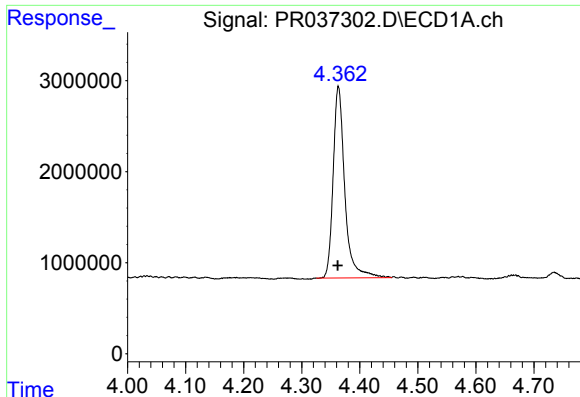

#1 Tetrachloro-m-xylene


R.T.: 4.363 min
Delta R.T.: 0.001 min
Response: 29326228
Conc: 23.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

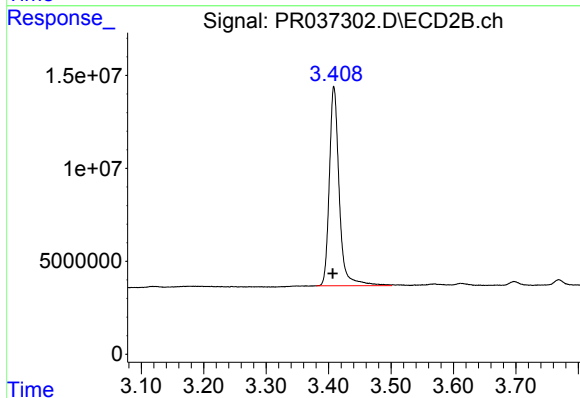


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: 0.002 min
Response: 118039665
Conc: 24.61 ng/ml

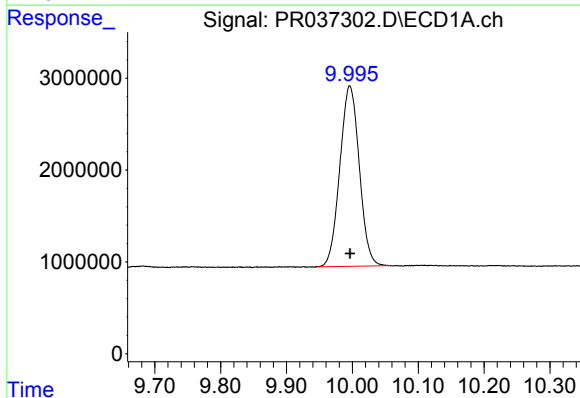


#2 Decachlorobiphenyl

R.T.: 9.996 min
Delta R.T.: 0.000 min
Response: 40288213
Conc: 30.46 ng/ml

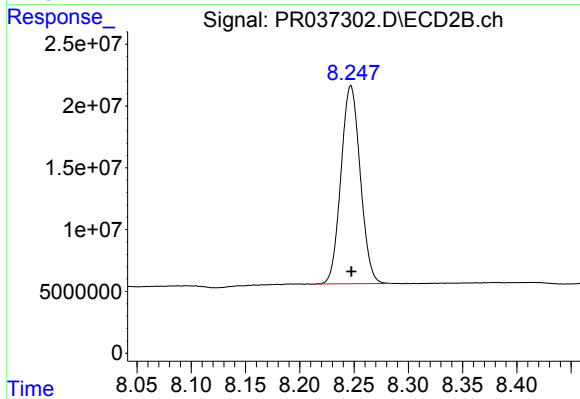

#2 Decachlorobiphenyl


R.T.: 8.247 min
Delta R.T.: 0.000 min
Response: 198134250
Conc: 34.02 ng/ml

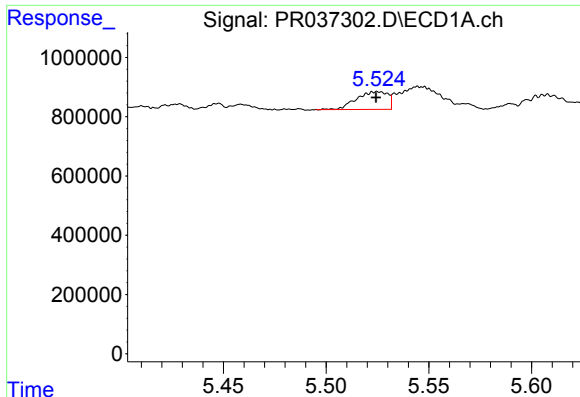

#3 AR-1016-1


R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 631043
Conc: 14.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

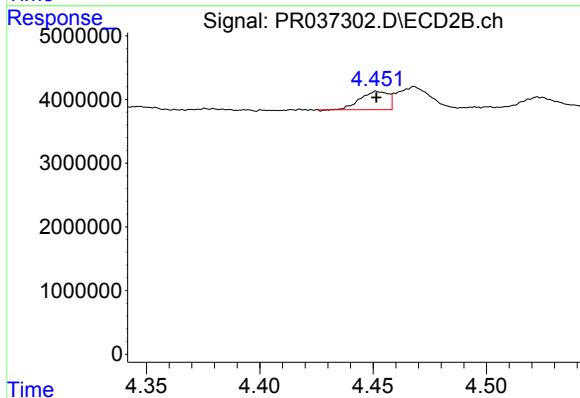


#3 AR-1016-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2442649
Conc: 13.42 ng/ml

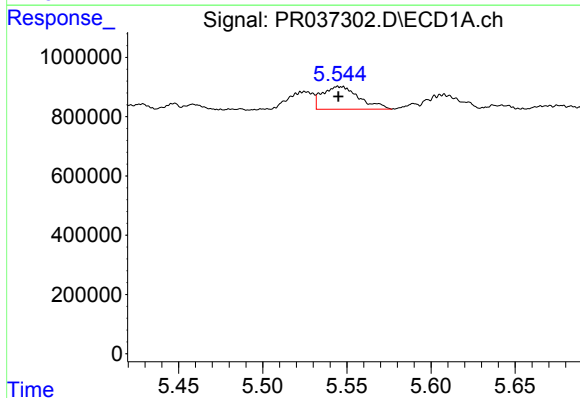


#4 AR-1016-2

R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 1169011
Conc: 16.88 ng/ml

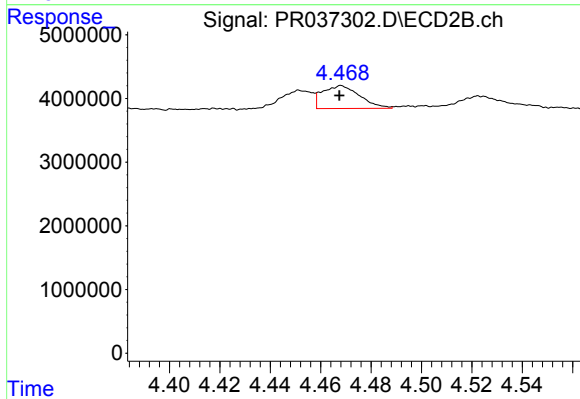

#4 AR-1016-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 3708876
Conc: 13.15 ng/ml

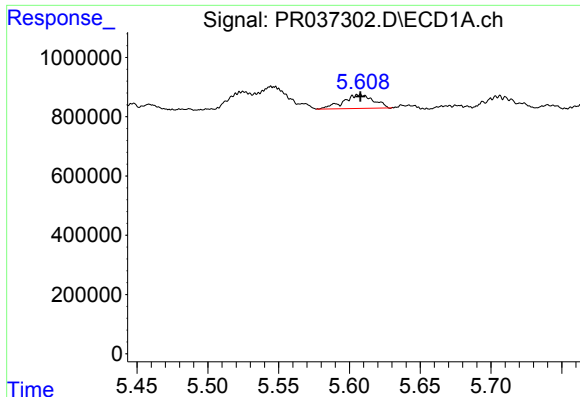

#5 AR-1016-3


R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 689979
Conc: 17.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

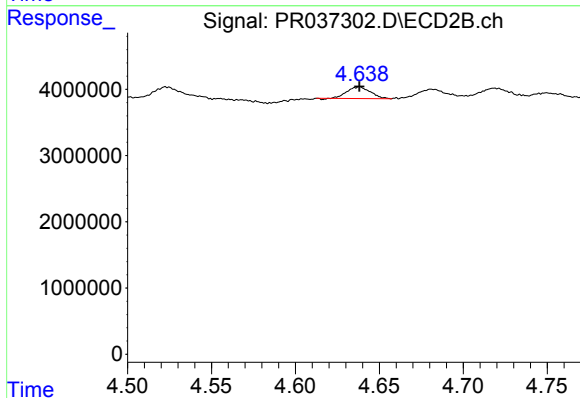


#5 AR-1016-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 1709662
Conc: 11.89 ng/ml

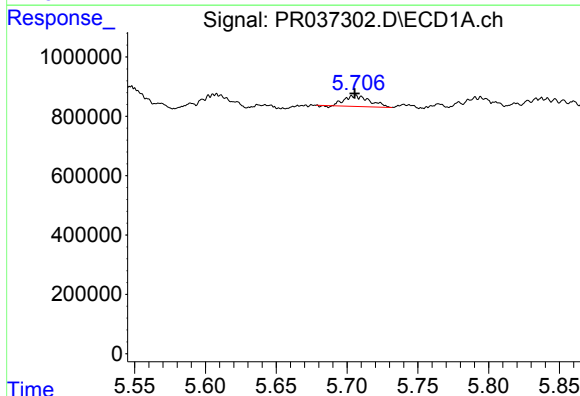


#6 AR-1016-4

R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 446044
Conc: 13.58 ng/ml

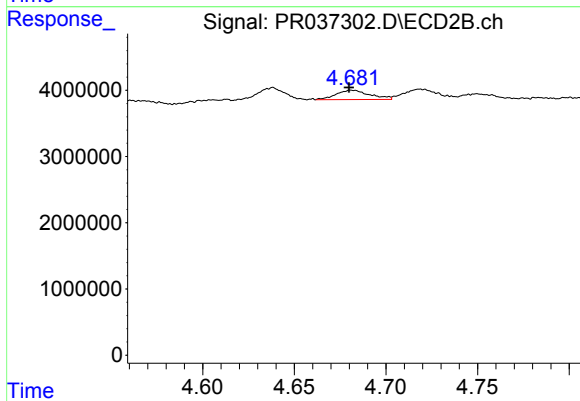

#6 AR-1016-4


R.T.: 4.681 min
Delta R.T.: 0.001 min
Response: 1809774
Conc: 16.36 ng/ml

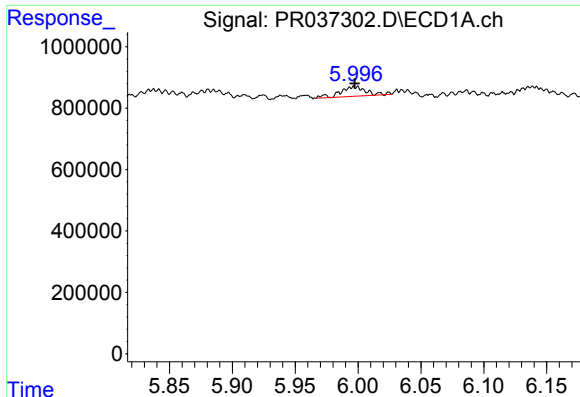

#7 AR-1016-5


R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 437571
Conc: 12.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

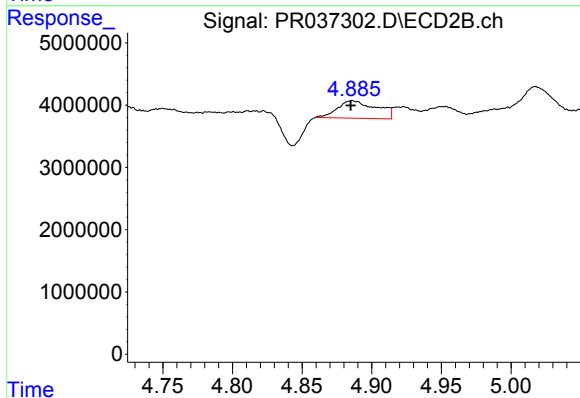


#7 AR-1016-5

R.T.: 4.886 min
Delta R.T.: 0.001 min
Response: 5464722
Conc: 35.95 ng/ml

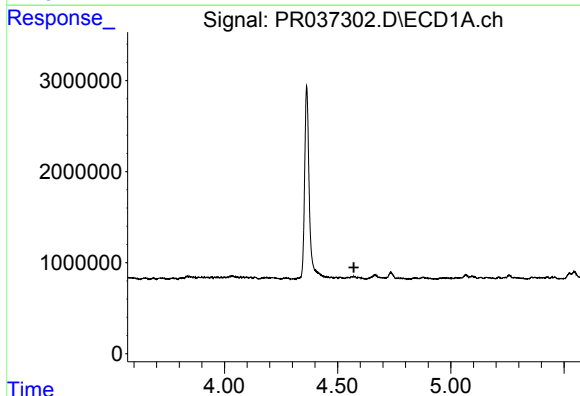


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

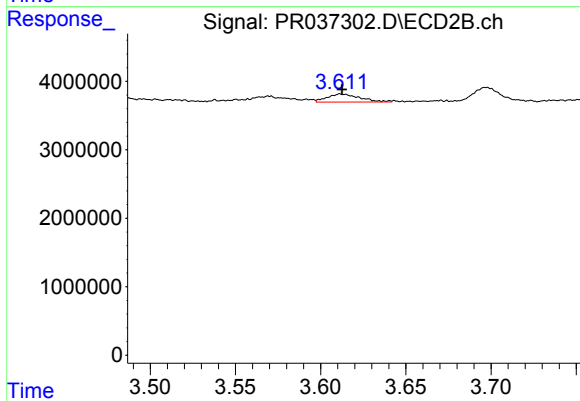

#8 AR-1221-1


R.T.: 3.611 min
Delta R.T.: -0.001 min
Response: 1560036
Conc: 30.64 ng/ml

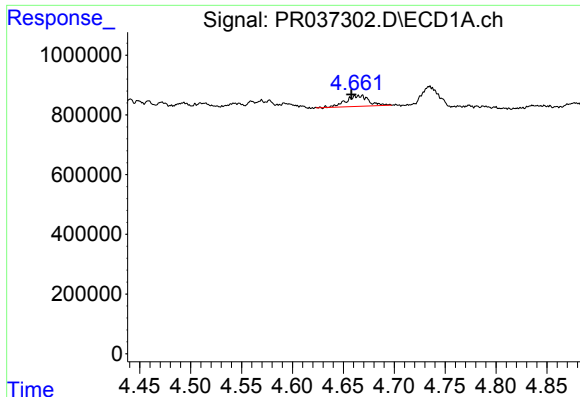

#9 AR-1221-2


R.T.: 4.665 min
Delta R.T.: 0.007 min
Response: 563683
Conc: 62.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

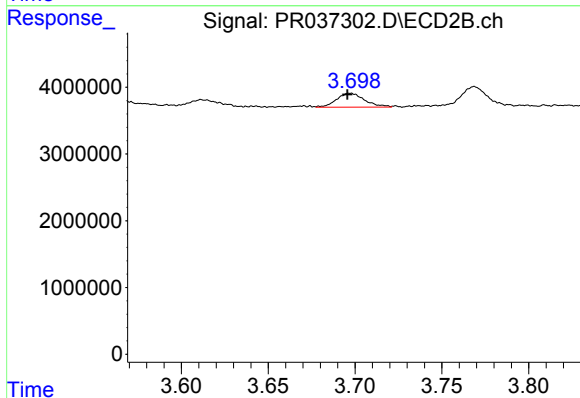


#9 AR-1221-2

R.T.: 3.697 min
Delta R.T.: 0.002 min
Response: 2344268
Conc: 63.13 ng/ml

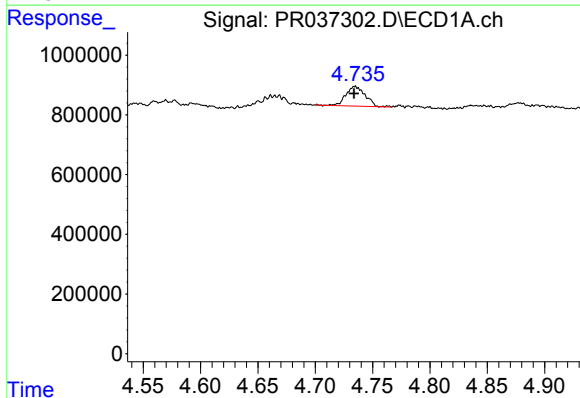


#10 AR-1221-3

R.T.: 4.735 min
Delta R.T.: 0.000 min
Response: 782750
Conc: 25.54 ng/ml

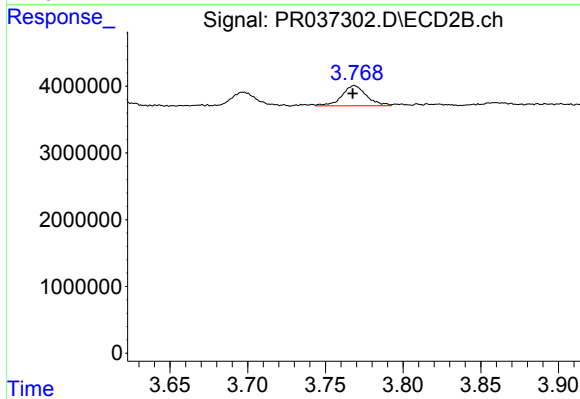

#10 AR-1221-3


R.T.: 3.769 min
Delta R.T.: 0.001 min
Response: 3365187
Conc: 27.48 ng/ml

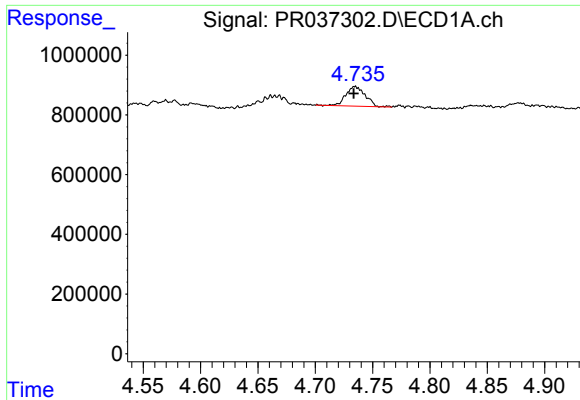

#11 AR-1232-1


R.T.: 4.735 min
Delta R.T.: 0.000 min
Response: 782750
Conc: 26.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

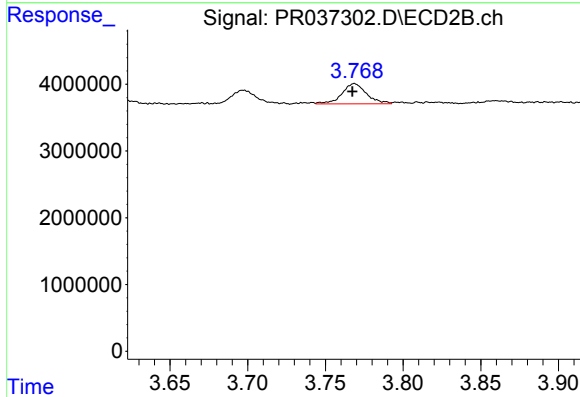


#11 AR-1232-1

R.T.: 3.769 min
Delta R.T.: 0.001 min
Response: 3365187
Conc: 28.76 ng/ml

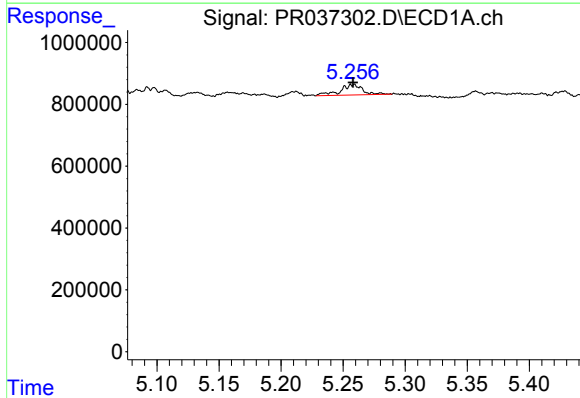


#12 AR-1232-2

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 427081
Conc: 25.27 ng/ml

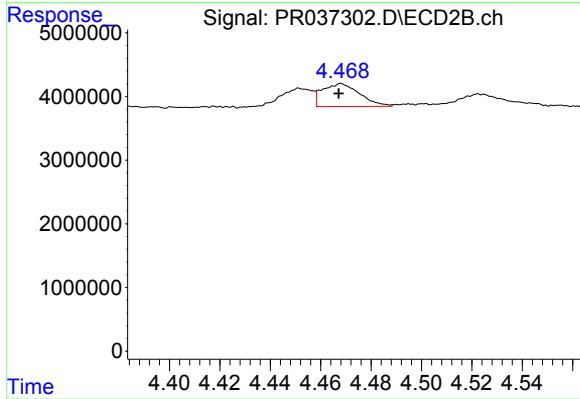

#12 AR-1232-2


R.T.: 4.468 min
Delta R.T.: 0.001 min
Response: 3708876
Conc: 26.83 ng/ml

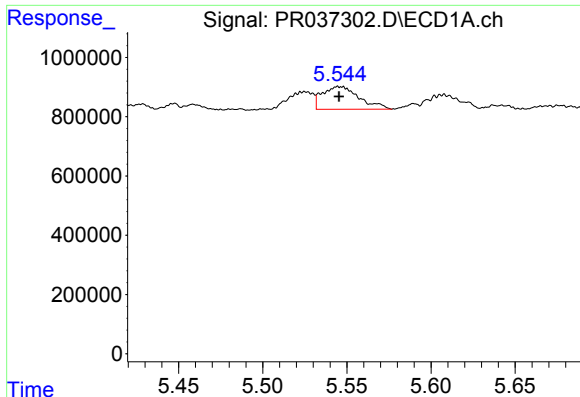

#13 AR-1232-3


R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 1169011
Conc: 34.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

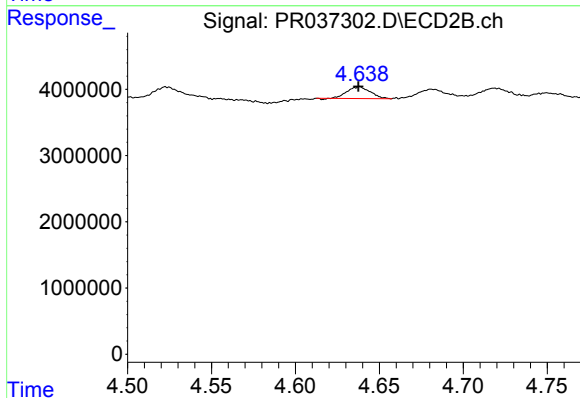


#13 AR-1232-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 1709662
Conc: 24.35 ng/ml

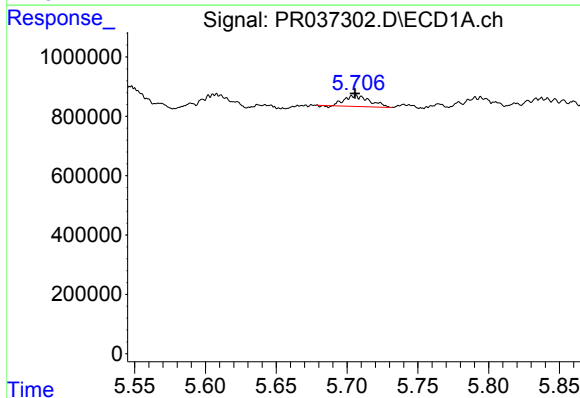


#14 AR-1232-4

R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 446044
Conc: 28.42 ng/ml

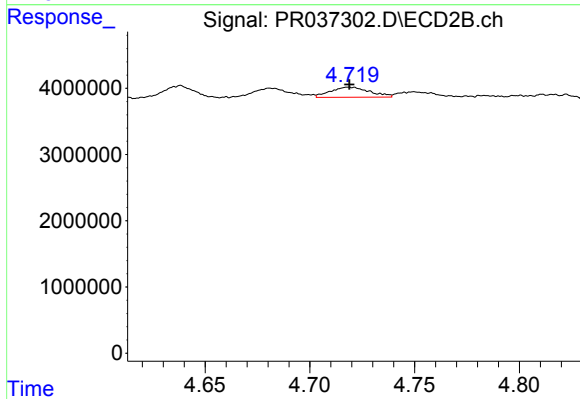

#14 AR-1232-4


R.T.: 4.721 min
Delta R.T.: 0.002 min
Response: 1979252
Conc: 33.17 ng/ml

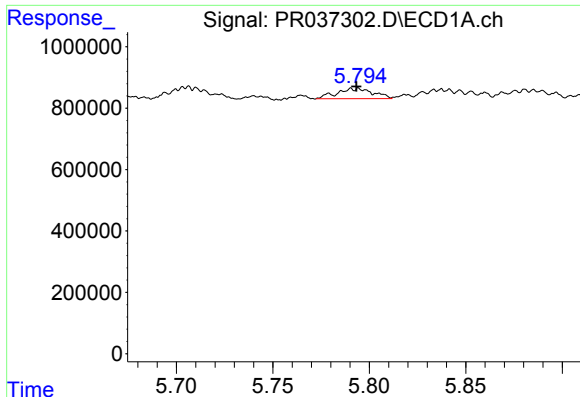

#15 AR-1232-5


R.T.: 5.794 min
Delta R.T.: 0.001 min
Response: 436833
Conc: 37.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

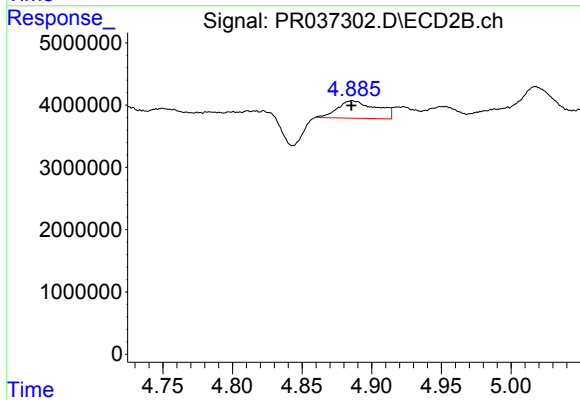


#15 AR-1232-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 5464722
Conc: 80.08 ng/ml

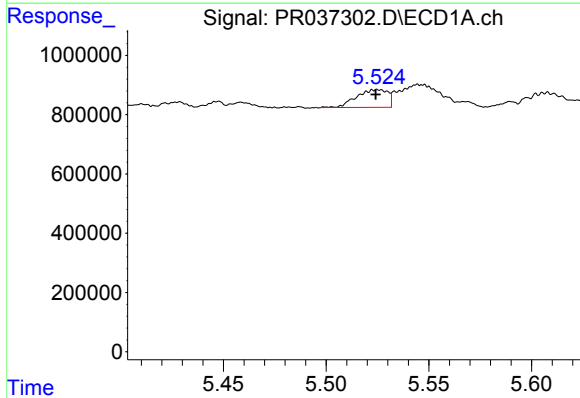


#16 AR-1242-1

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 631043
Conc: 18.44 ng/ml

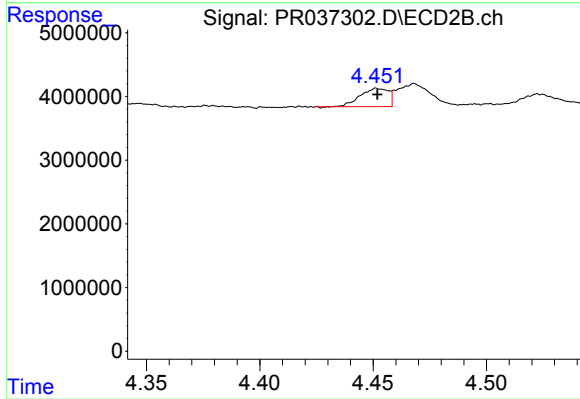

#16 AR-1242-1


R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2442649
Conc: 16.67 ng/ml

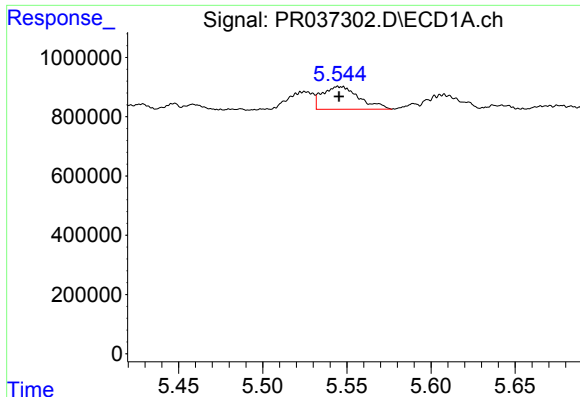

#17 AR-1242-2


R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 1169011
Conc: 21.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

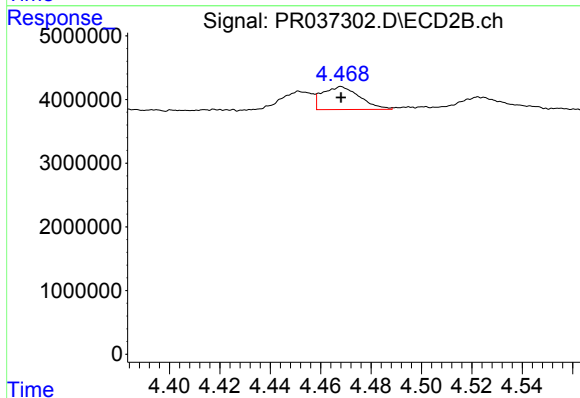


#17 AR-1242-2

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 3708876
Conc: 16.26 ng/ml

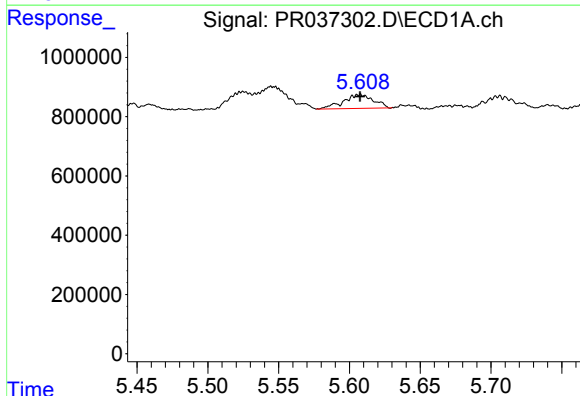


#18 AR-1242-3

R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 689979
Conc: 20.96 ng/ml

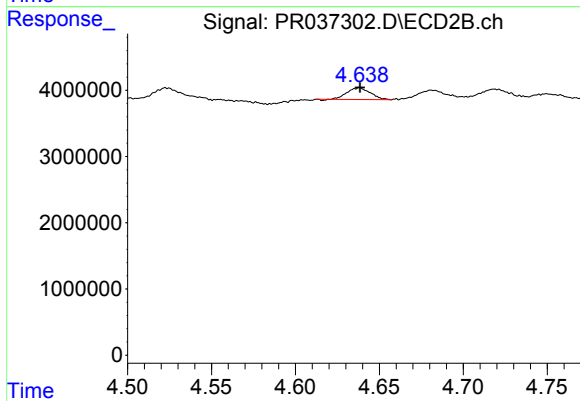

#18 AR-1242-3


R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 1709662
Conc: 14.79 ng/ml

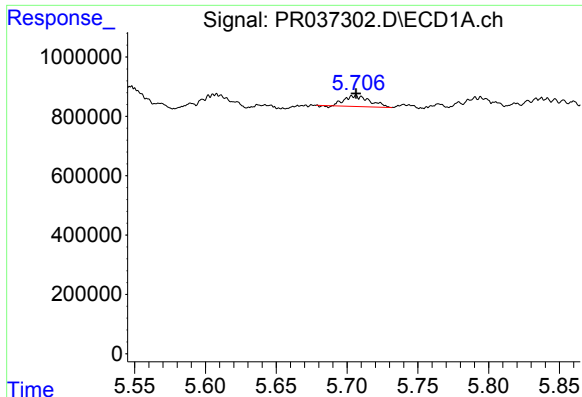

#19 AR-1242-4


R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 446044
Conc: 16.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

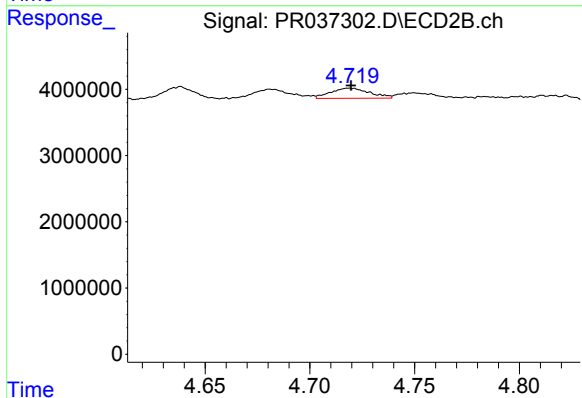


#19 AR-1242-4

R.T.: 4.721 min
Delta R.T.: 0.002 min
Response: 1979252
Conc: 18.01 ng/ml

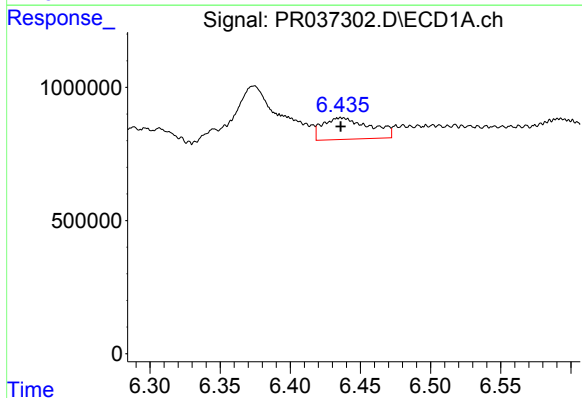


#20 AR-1242-5

R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 1889824
Conc: 58.73 ng/ml

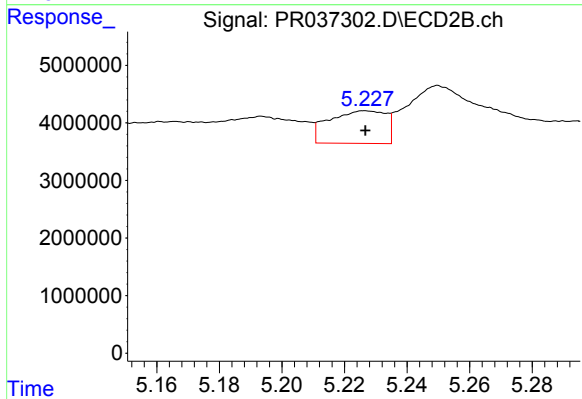

#20 AR-1242-5


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 7117096
Conc: 42.95 ng/ml

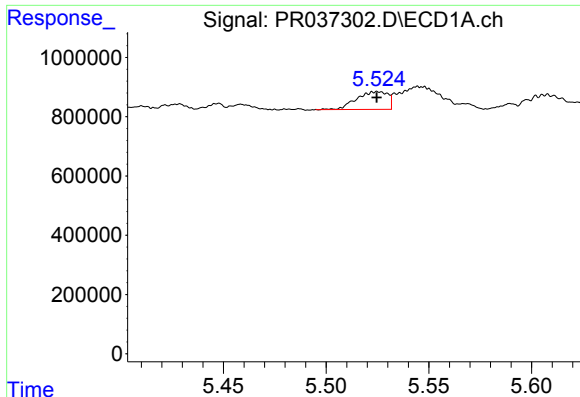

#21 AR-1248-1


R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 631043
Conc: 27.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

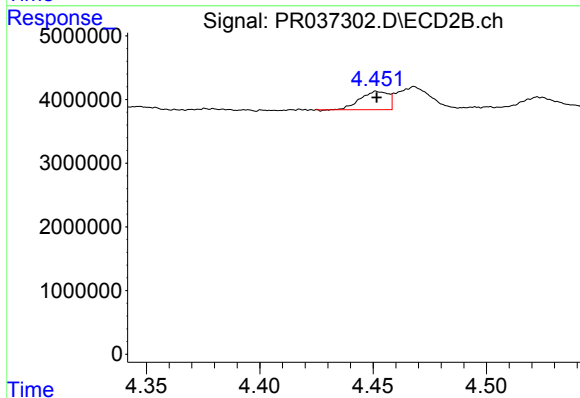


#21 AR-1248-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2442649
Conc: 24.27 ng/ml

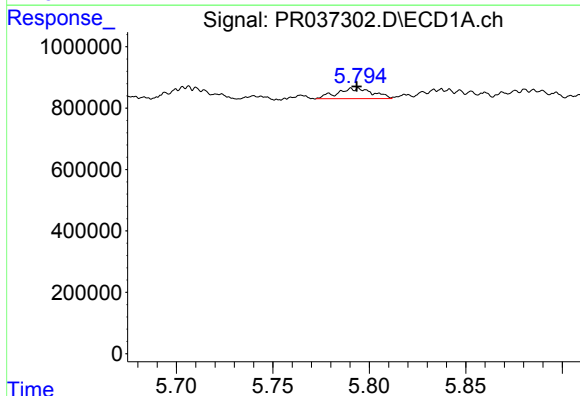


#22 AR-1248-2

R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 436833
Conc: 12.48 ng/ml

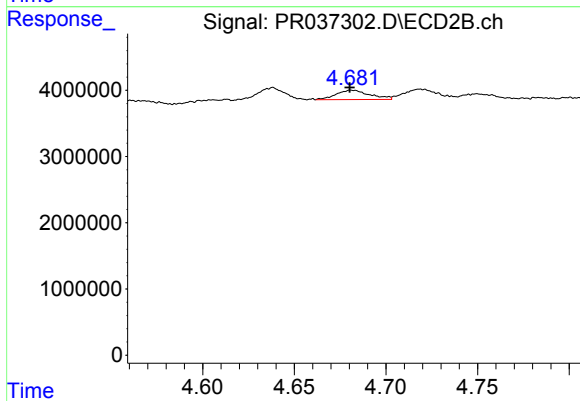

#22 AR-1248-2


R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 1809774
Conc: 13.26 ng/ml

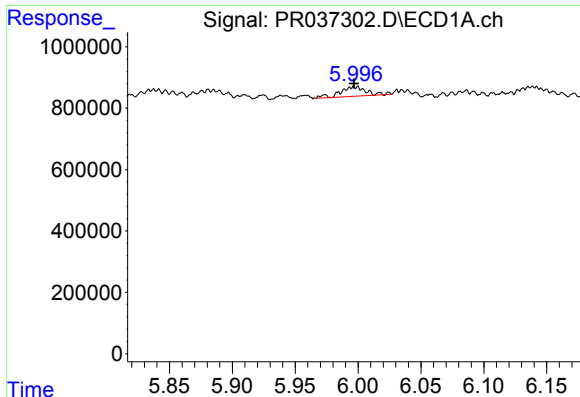

#23 AR-1248-3


R.T.: 5.998 min
Delta R.T.: 0.001 min
Response: 437571
Conc: 10.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

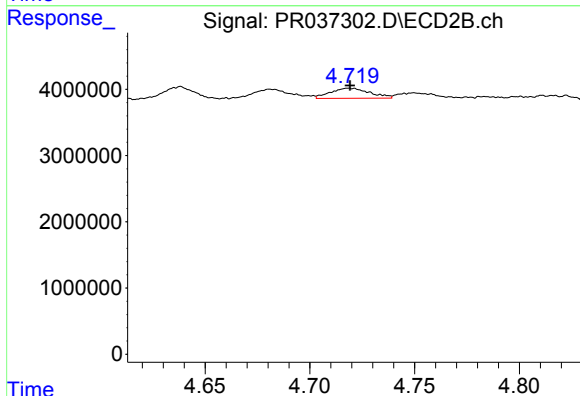


#23 AR-1248-3

R.T.: 4.721 min
Delta R.T.: 0.002 min
Response: 1979252
Conc: 14.14 ng/ml

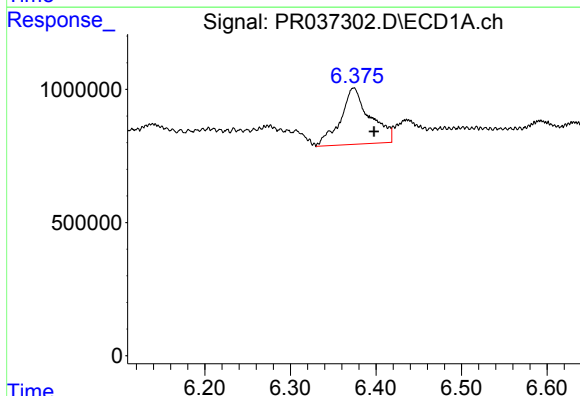


#24 AR-1248-4

R.T.: 6.374 min
Delta R.T.: -0.024 min
Response: 5063448
Conc: 103.43 ng/ml

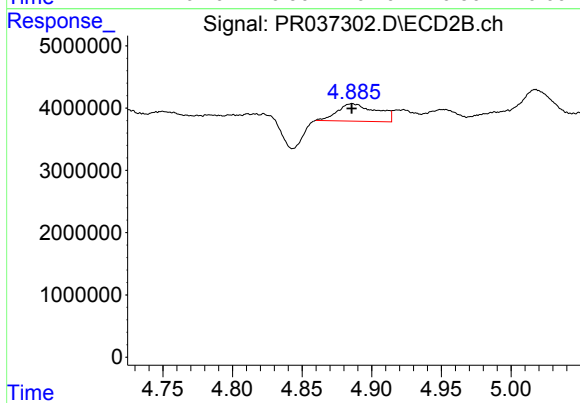

#24 AR-1248-4


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 5464722
Conc: 30.71 ng/ml

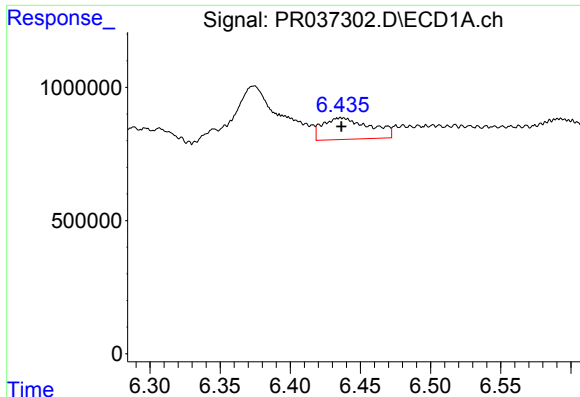

#25 AR-1248-5


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 1889824
Conc: 40.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

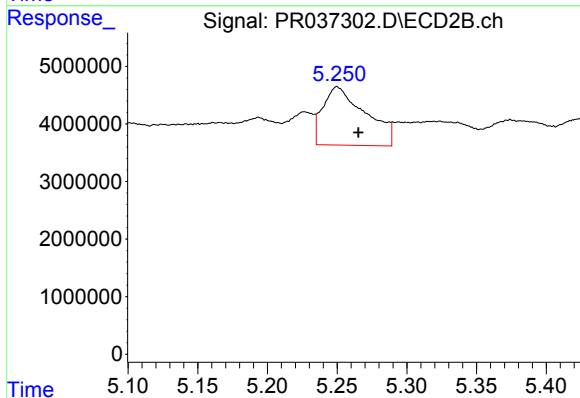


#25 AR-1248-5

R.T.: 5.250 min
Delta R.T.: -0.015 min
Response: 21553426
Conc: 110.18 ng/ml

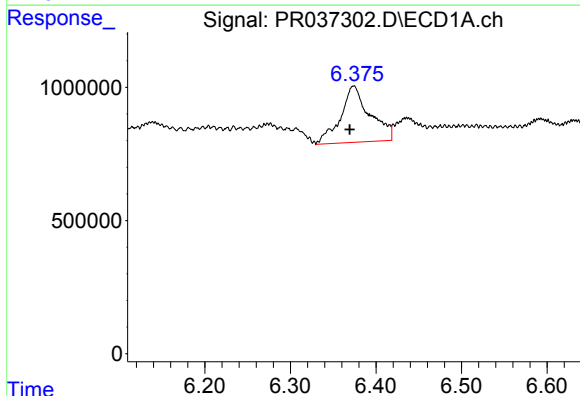


#26 AR-1254-1

R.T.: 6.374 min
Delta R.T.: 0.005 min
Response: 5063448
Conc: 92.68 ng/ml

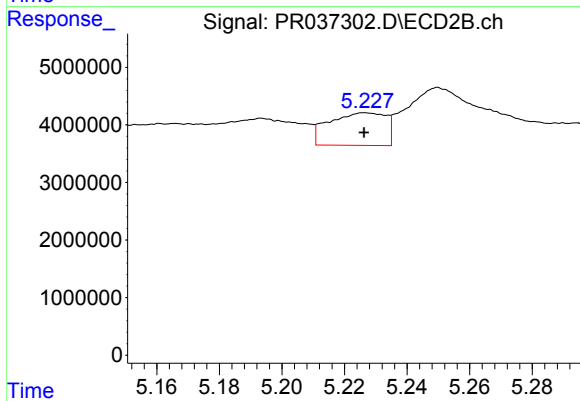

#26 AR-1254-1


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 7117096
Conc: 20.66 ng/ml

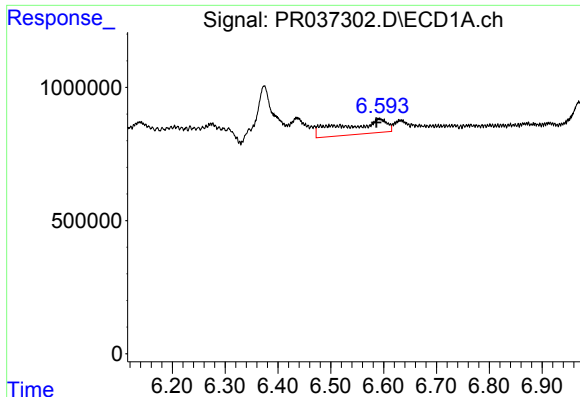

#27 AR-1254-2


R.T.: 6.592 min
Delta R.T.: 0.006 min
Response: 3039511
Conc: 35.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

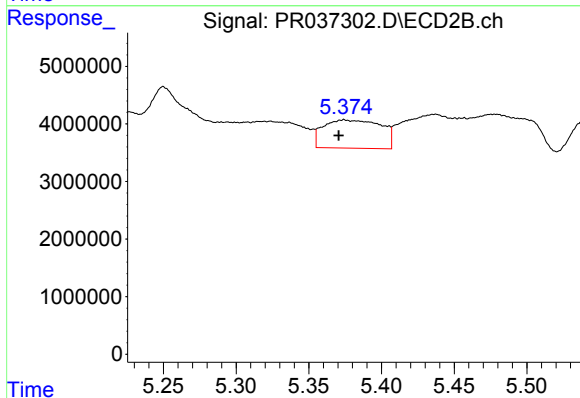


#27 AR-1254-2

R.T.: 5.374 min
Delta R.T.: 0.004 min
Response: 13621099
Conc: 45.48 ng/ml

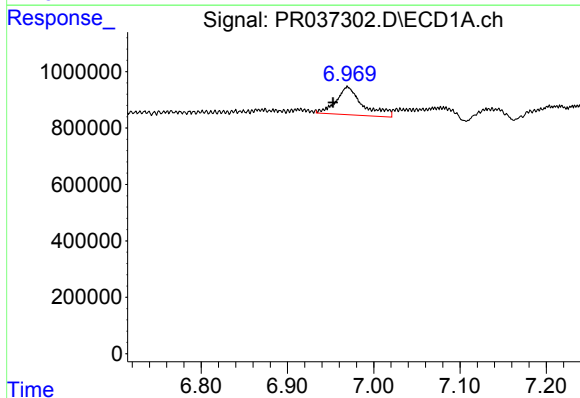


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: 0.017 min
Response: 2086404
Conc: 22.94 ng/ml

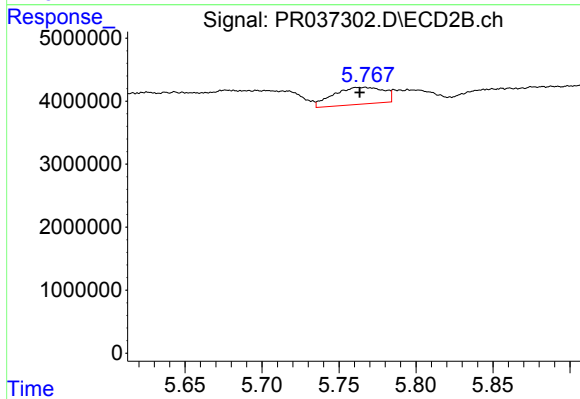

#28 AR-1254-3


R.T.: 5.767 min
Delta R.T.: 0.004 min
Response: 6075444
Conc: 12.83 ng/ml

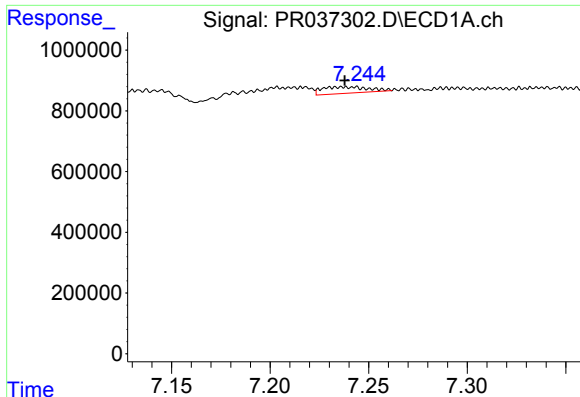

#29 AR-1254-4


R.T.: 7.237 min
Delta R.T.: -0.001 min
Response: 345713
Conc: 5.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

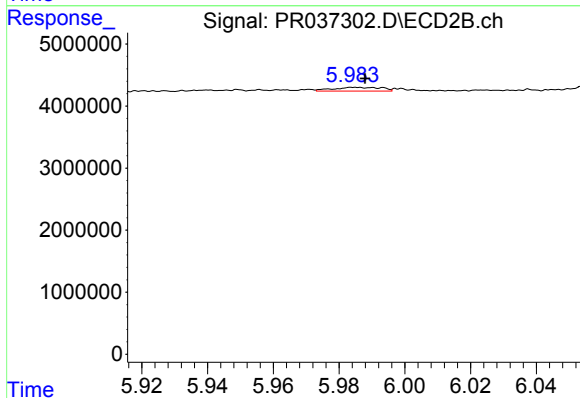


#29 AR-1254-4

R.T.: 5.984 min
Delta R.T.: -0.004 min
Response: 621333
Conc: 1.77 ng/ml

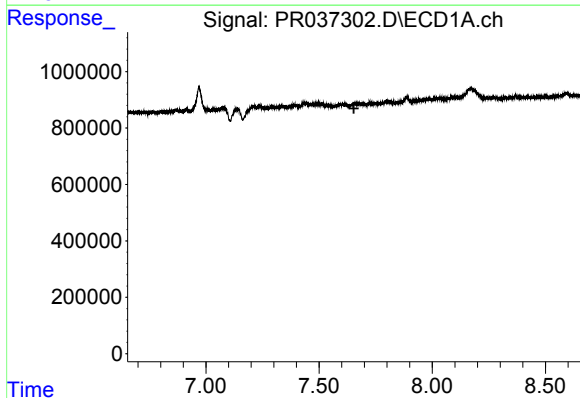


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

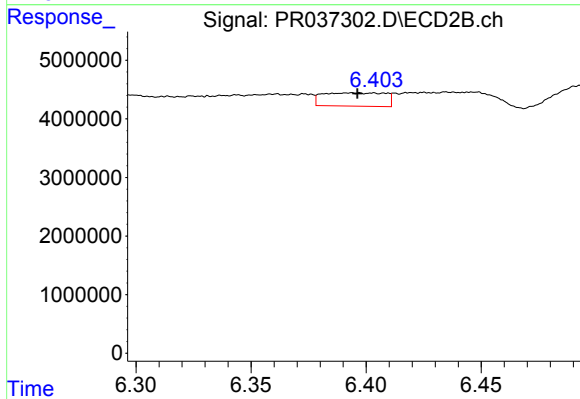

#30 AR-1254-5


R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 4261955
Conc: 9.62 ng/ml

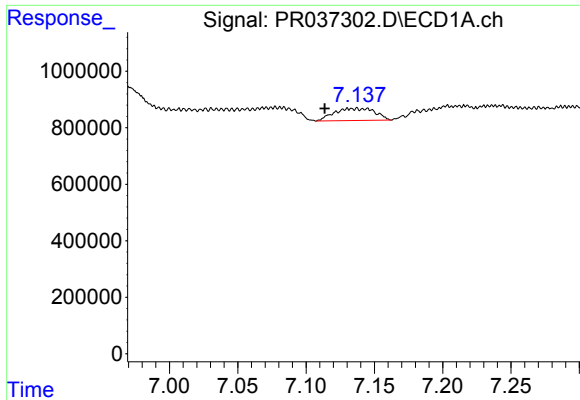

#31 AR-1260-1


R.T.: 7.137 min
Delta R.T.: 0.023 min
Response: 892127
Conc: 13.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

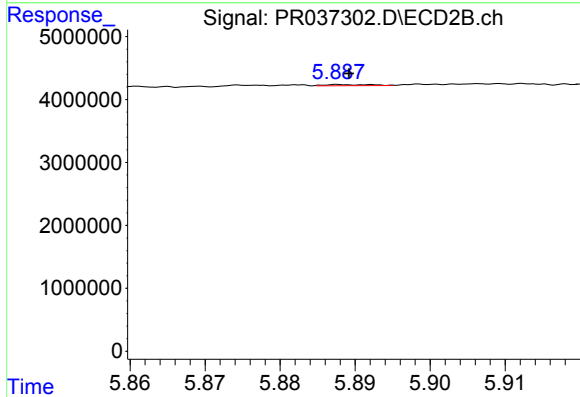


#31 AR-1260-1

R.T.: 5.888 min
Delta R.T.: -0.001 min
Response: 75385
Conc: 0.26 ng/ml

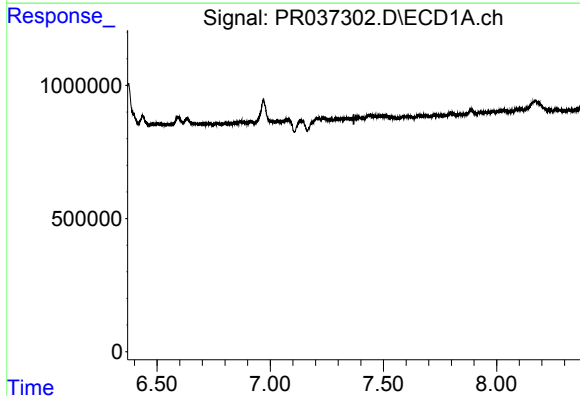


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

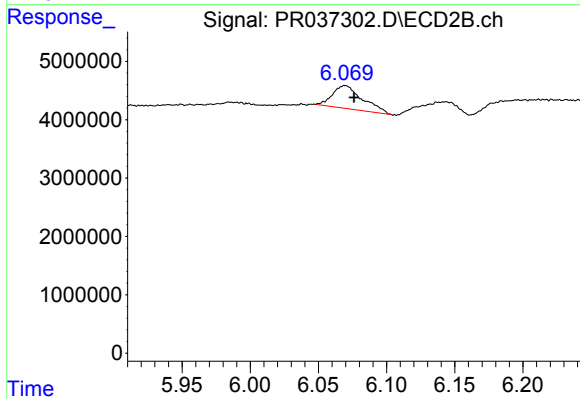

#32 AR-1260-2


R.T.: 6.069 min
Delta R.T.: -0.007 min
Response: 5923434
Conc: 12.86 ng/ml

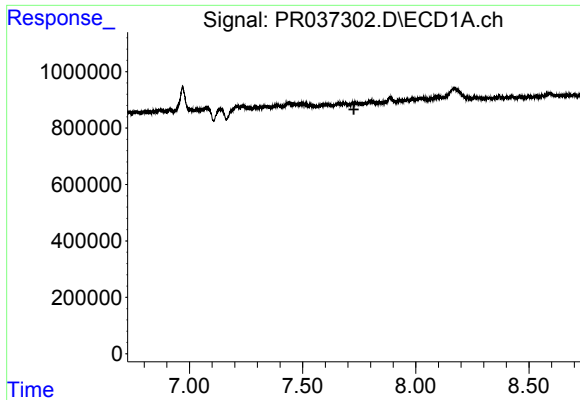

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

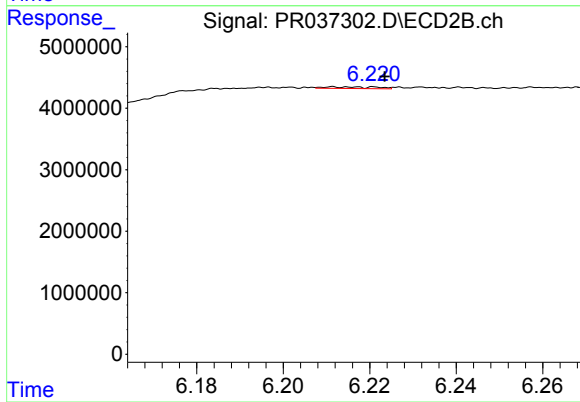


#33 AR-1260-3

R.T.: 6.212 min
Delta R.T.: -0.012 min
Response: 221001
Conc: 0.62 ng/ml

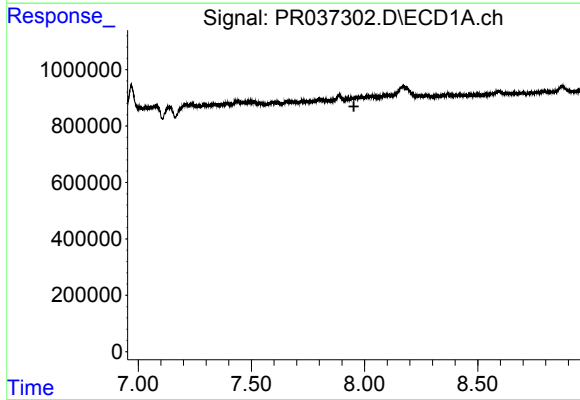


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

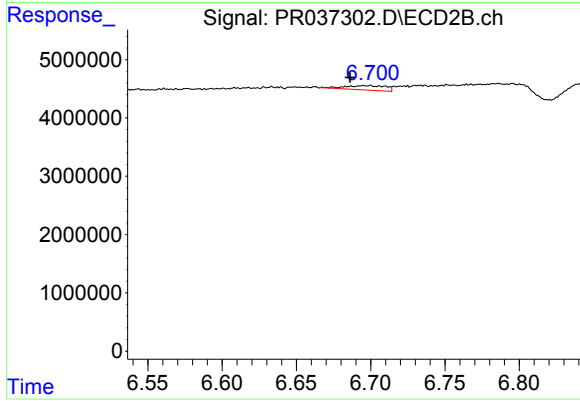

#34 AR-1260-4


R.T.: 6.700 min
Delta R.T.: 0.014 min
Response: 1434541
Conc: 4.71 ng/ml

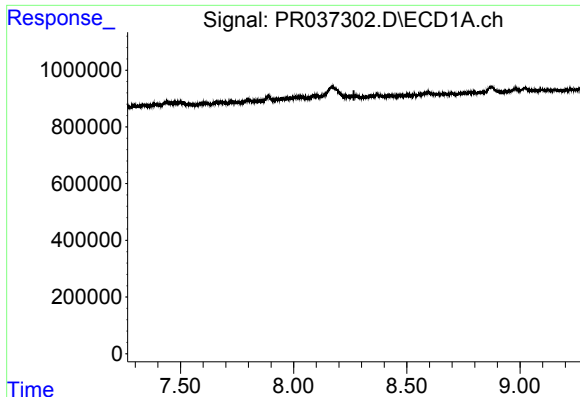

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

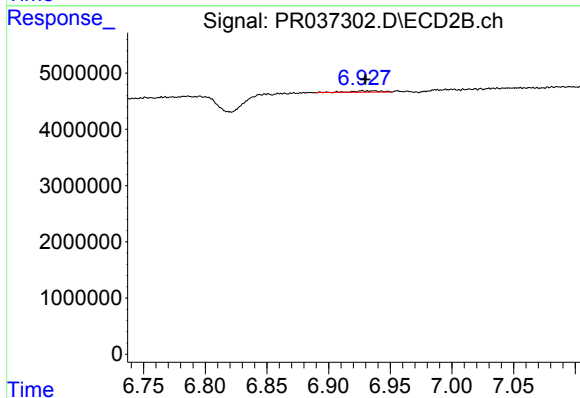


#35 AR-1260-5

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 369378
Conc: 0.43 ng/ml

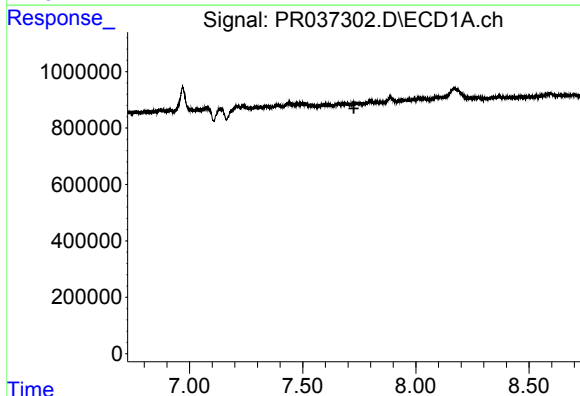


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

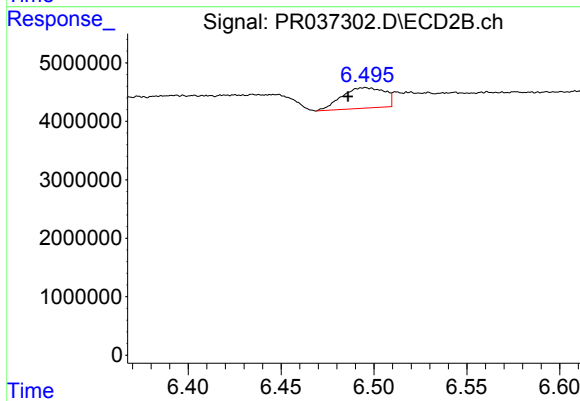

#36 AR-1262-1


R.T.: 6.496 min
Delta R.T.: 0.010 min
Response: 5634755
Conc: 22.48 ng/ml

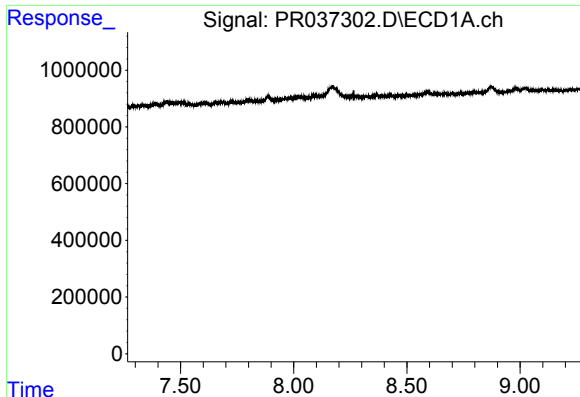

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

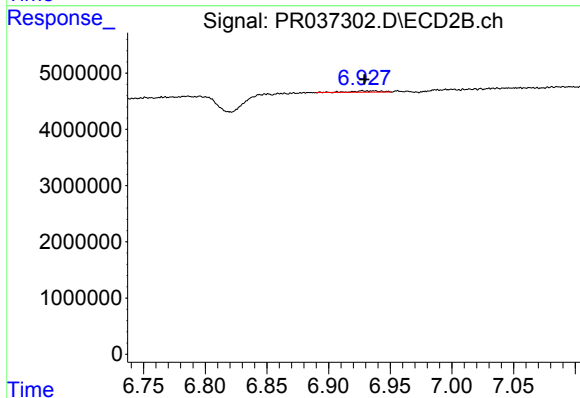


#37 AR-1262-2

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 369378
Conc: 0.29 ng/ml

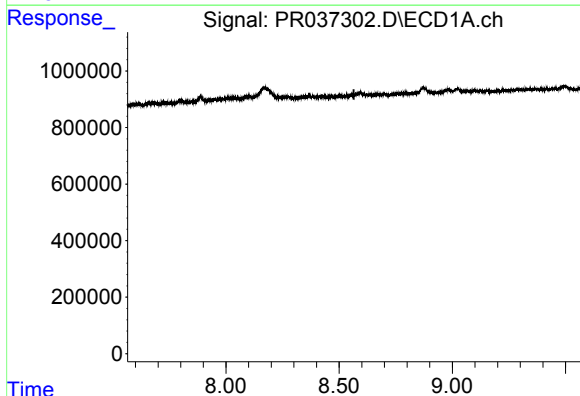


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

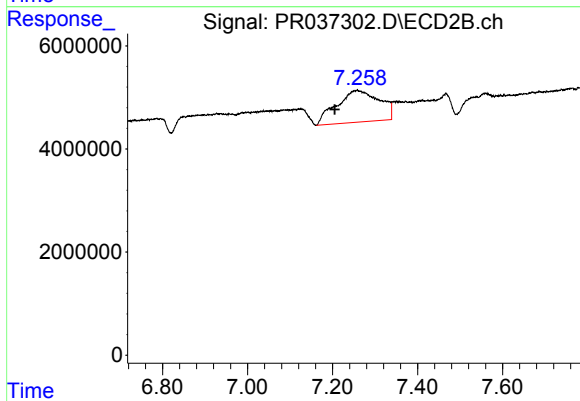

#38 AR-1262-3


R.T.: 7.258 min
Delta R.T.: 0.053 min
Response: 43253636
Conc: 78.89 ng/ml

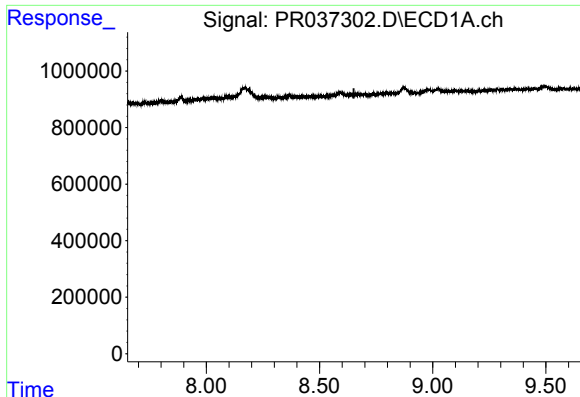

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

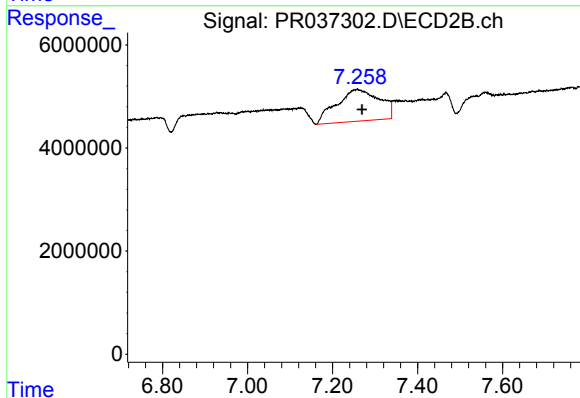


#39 AR-1262-4

R.T.: 7.258 min
Delta R.T.: -0.011 min
Response: 43253636
Conc: 48.19 ng/ml

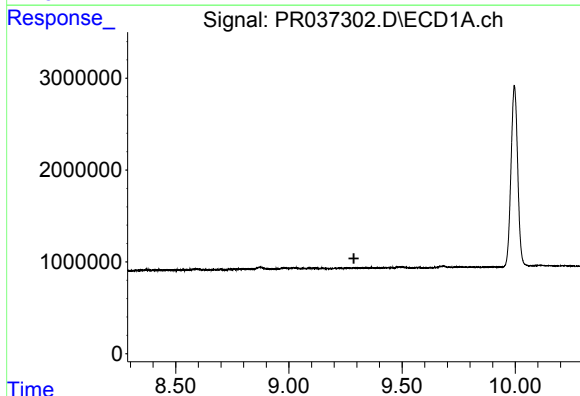


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

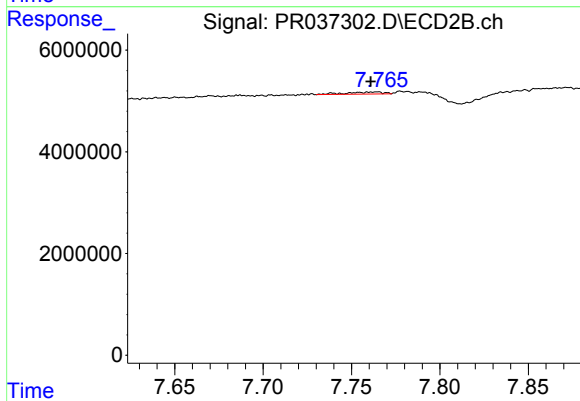

#40 AR-1262-5


R.T.: 7.764 min
Delta R.T.: 0.003 min
Response: 589463
Conc: 1.54 ng/ml

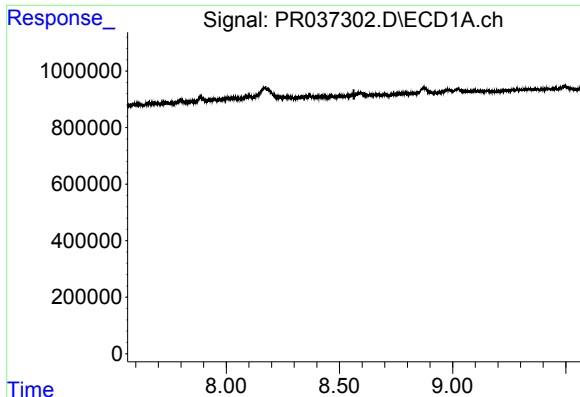

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

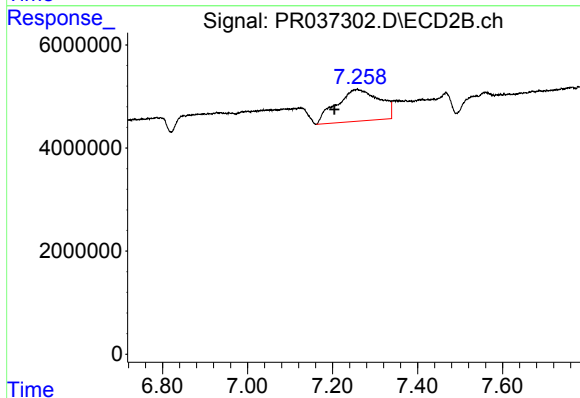


#41 AR-1268-1

R.T.: 7.258 min
Delta R.T.: 0.053 min
Response: 43253636
Conc: 35.14 ng/ml

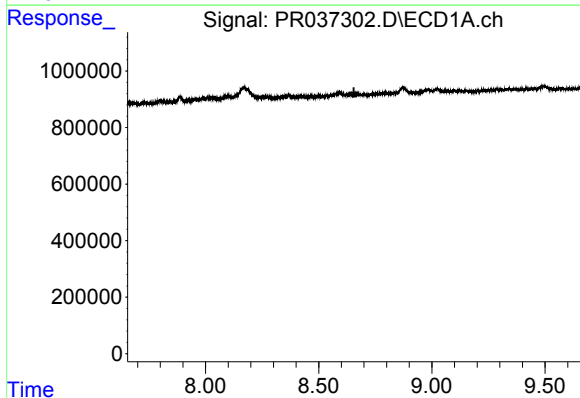


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

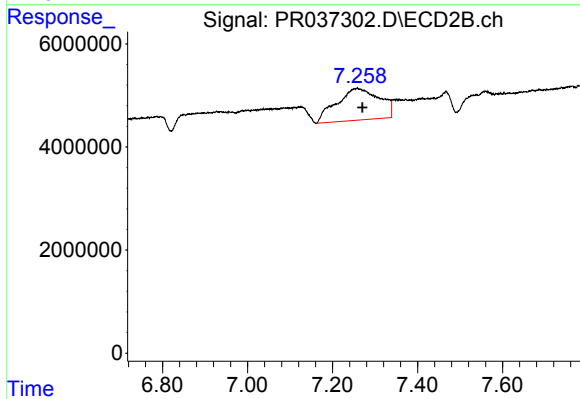

#42 AR-1268-2


R.T.: 7.258 min
Delta R.T.: -0.012 min
Response: 43253636
Conc: 40.85 ng/ml

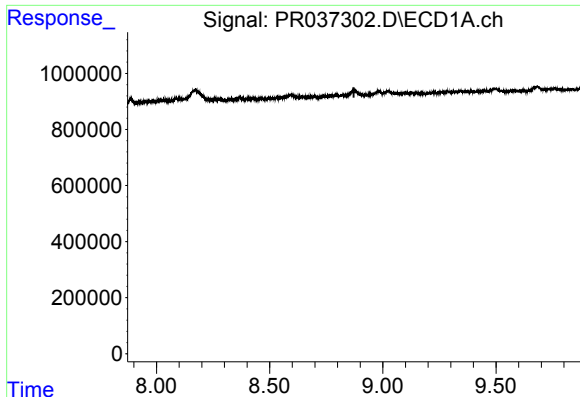

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

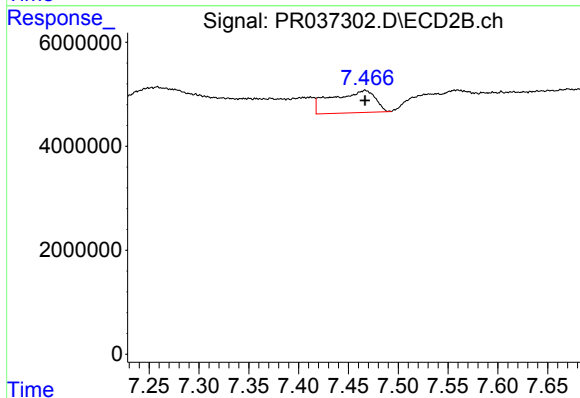


#43 AR-1268-3

R.T.: 7.467 min
Delta R.T.: 0.000 min
Response: 12963665
Conc: 14.63 ng/ml

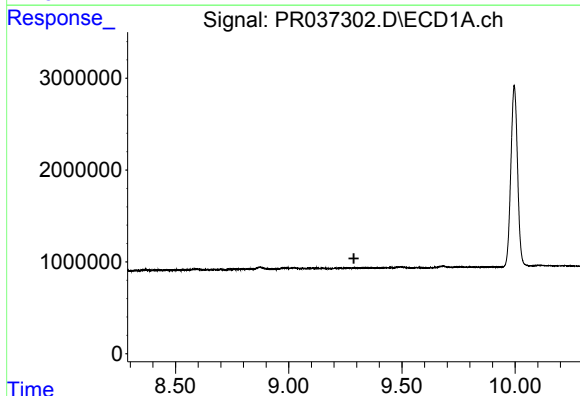


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

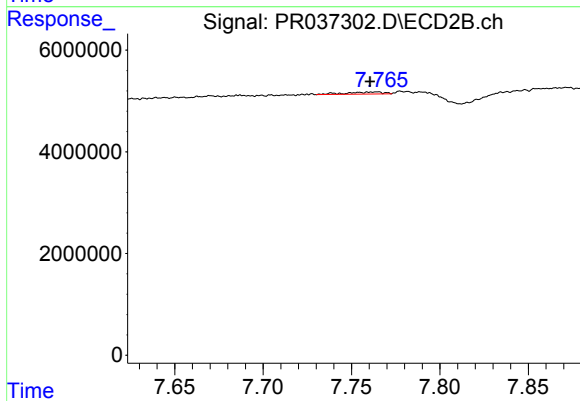

#44 AR-1268-4


R.T.: 7.764 min
Delta R.T.: 0.004 min
Response: 589463
Conc: 1.62 ng/ml

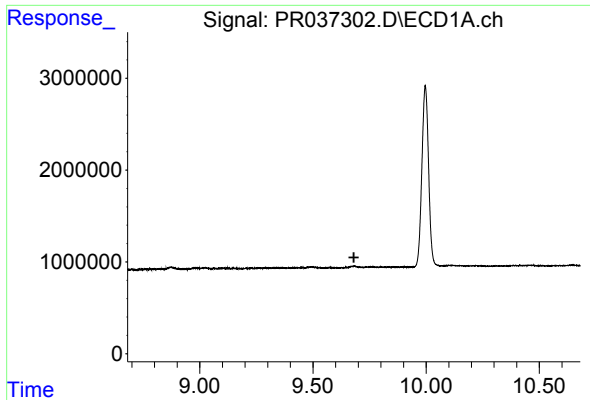

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

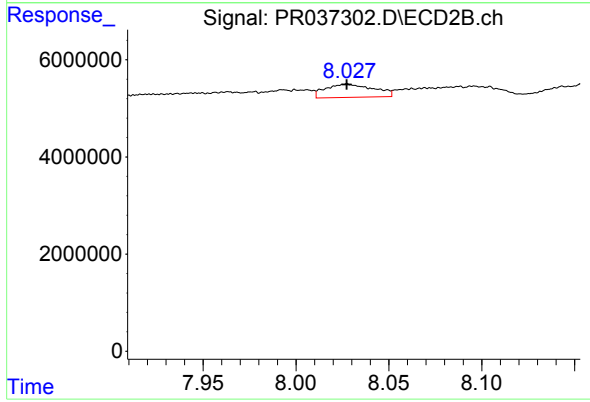

#45 AR-1268-5

R.T.: 8.027 min
Delta R.T.: 0.000 min
Response: 4929459
Conc: 1.94 ng/ml