

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 20:24
 Operator : SM\SJ
 Sample : K1560-12
 Misc : AR1242 MDL 25PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:53:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.364	3.410	31724502	129.2E6	25.359	26.940
2)	SA Decachlor...	9.996	8.248	43044146	208.4E6	32.545	35.788
Target Compounds							
3)	L1 AR-1016-1	5.545	4.452	3239676	5559888	75.186	30.535 #
4)	L1 AR-1016-2	5.545	4.468	3239676	8170286	46.784	28.960 #
5)	L1 AR-1016-3	5.607	4.638	1202052	3694916	29.807	25.698
6)	L1 AR-1016-4	5.706	4.681	1042476	4236329	31.744	38.291
7)	L1 AR-1016-5	5.997	4.886	1318753	18212716	38.459	119.813 #
8)	L2 AR-1221-1	0.000	3.612	0	328633	N.D.	6.454 #
9)	L2 AR-1221-2	4.666	3.698	775699	2878633	85.770	77.516
10)	L2 AR-1221-3	4.735	3.768	969785	3987267	31.642	32.563
11)	L3 AR-1232-1	4.735	3.768	969785	3987267	33.154	34.082
12)	L3 AR-1232-2	5.258	4.468	1044067	8170286	61.788	59.109
13)	L3 AR-1232-3	5.545	4.638	3239676	3694916	95.836	52.633 #
14)	L3 AR-1232-4	5.706	4.720	1042476	4440862	66.414	74.421
15)	L3 AR-1232-5	5.793	4.886	653151	18212716	55.846	266.877 #
16)	L4 AR-1242-1	5.545	4.452	3239676	5559888	94.687	37.942 #
17)	L4 AR-1242-2	5.545	4.468	3239676	8170286	58.404	35.809 #
18)	L4 AR-1242-3	5.607	4.638	1202052	3694916	36.520	31.955
19)	L4 AR-1242-4	5.706	4.720	1042476	4440862	39.522	40.404
20)	L4 AR-1242-5	6.436	5.249	2085015	134.3E6	64.795	810.380 #
21)	L5 AR-1248-1	5.545	4.452	3239676	5559888	141.425	55.232 #
22)	L5 AR-1248-2	5.793	4.681	653151	4236329	18.654	31.041 #
23)	L5 AR-1248-3	5.997	4.720	1318753	4440862	32.236	31.727
24)	L5 AR-1248-4	6.373	4.886	25740227	18212716	525.801	102.339 #
25)	L5 AR-1248-5	6.436	5.249	2085015	134.3E6	44.139	686.458 #
26)	L6 AR-1254-1	6.373	5.249	25740227	134.3E6	471.166	389.811
27)	L6 AR-1254-2	6.592	5.375	1354543	29504326	15.806	98.511 #
28)	L6 AR-1254-3	6.971	5.764	10685644	12281464	117.472	25.931 #
29)	L6 AR-1254-4	7.236	5.988	1494751	2239760	22.307	6.388 #
30)	L6 AR-1254-5	7.656	6.394	1764132	10304990	24.542	23.271
31)	L7 AR-1260-1	7.076	5.888	466670	395824	7.072	1.354 #
32)	L7 AR-1260-2	7.389	6.068	2418476	37564895	30.343	81.559 #
33)	L7 AR-1260-3	7.733	6.226	1525572	405250	24.380	1.137 #
34)	L7 AR-1260-4	7.888	6.686	2493674	3322179	33.515	10.901 #
35)	L7 AR-1260-5	0.000	6.930	0	1878617	N.D.	2.166 #
36)	L8 AR-1262-1	7.733	6.497	1525572	7522838	14.605	30.017 #
37)	L8 AR-1262-2	0.000	6.930	0	1878617	N.D.	1.496 #
38)	L8 AR-1262-3	8.591	7.237	1439489	1098.0E6	10.946	2002.707 #
39)	L8 AR-1262-4	8.591	7.237	1439489	1098.0E6	14.654	1223.216 #
40)	L8 AR-1262-5	0.000	7.763	0	362614	N.D.	0.948 #
41)	L9 AR-1268-1	8.591	7.237	1439489	1098.0E6	8.038	891.950 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 20:24
 Operator : SM\SJ
 Sample : K1560-12
 Misc : AR1242 MDL 25PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:53:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.591	7.237	1439489	1098.0E6	8.751	1036.918 #
43) L9	AR-1268-3	8.873	7.466	1841662	8904539	13.303	10.048
44) L9	AR-1268-4	0.000	7.763	0	362614	N.D.	1.000 #
45) L9	AR-1268-5	0.000	8.025	0	6020121	N.D.	2.366 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
Data File : PR037303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 20:24
Operator : SM\SJ
Sample : K1560-12
Misc : AR1242 MDL 25PPB
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:53:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

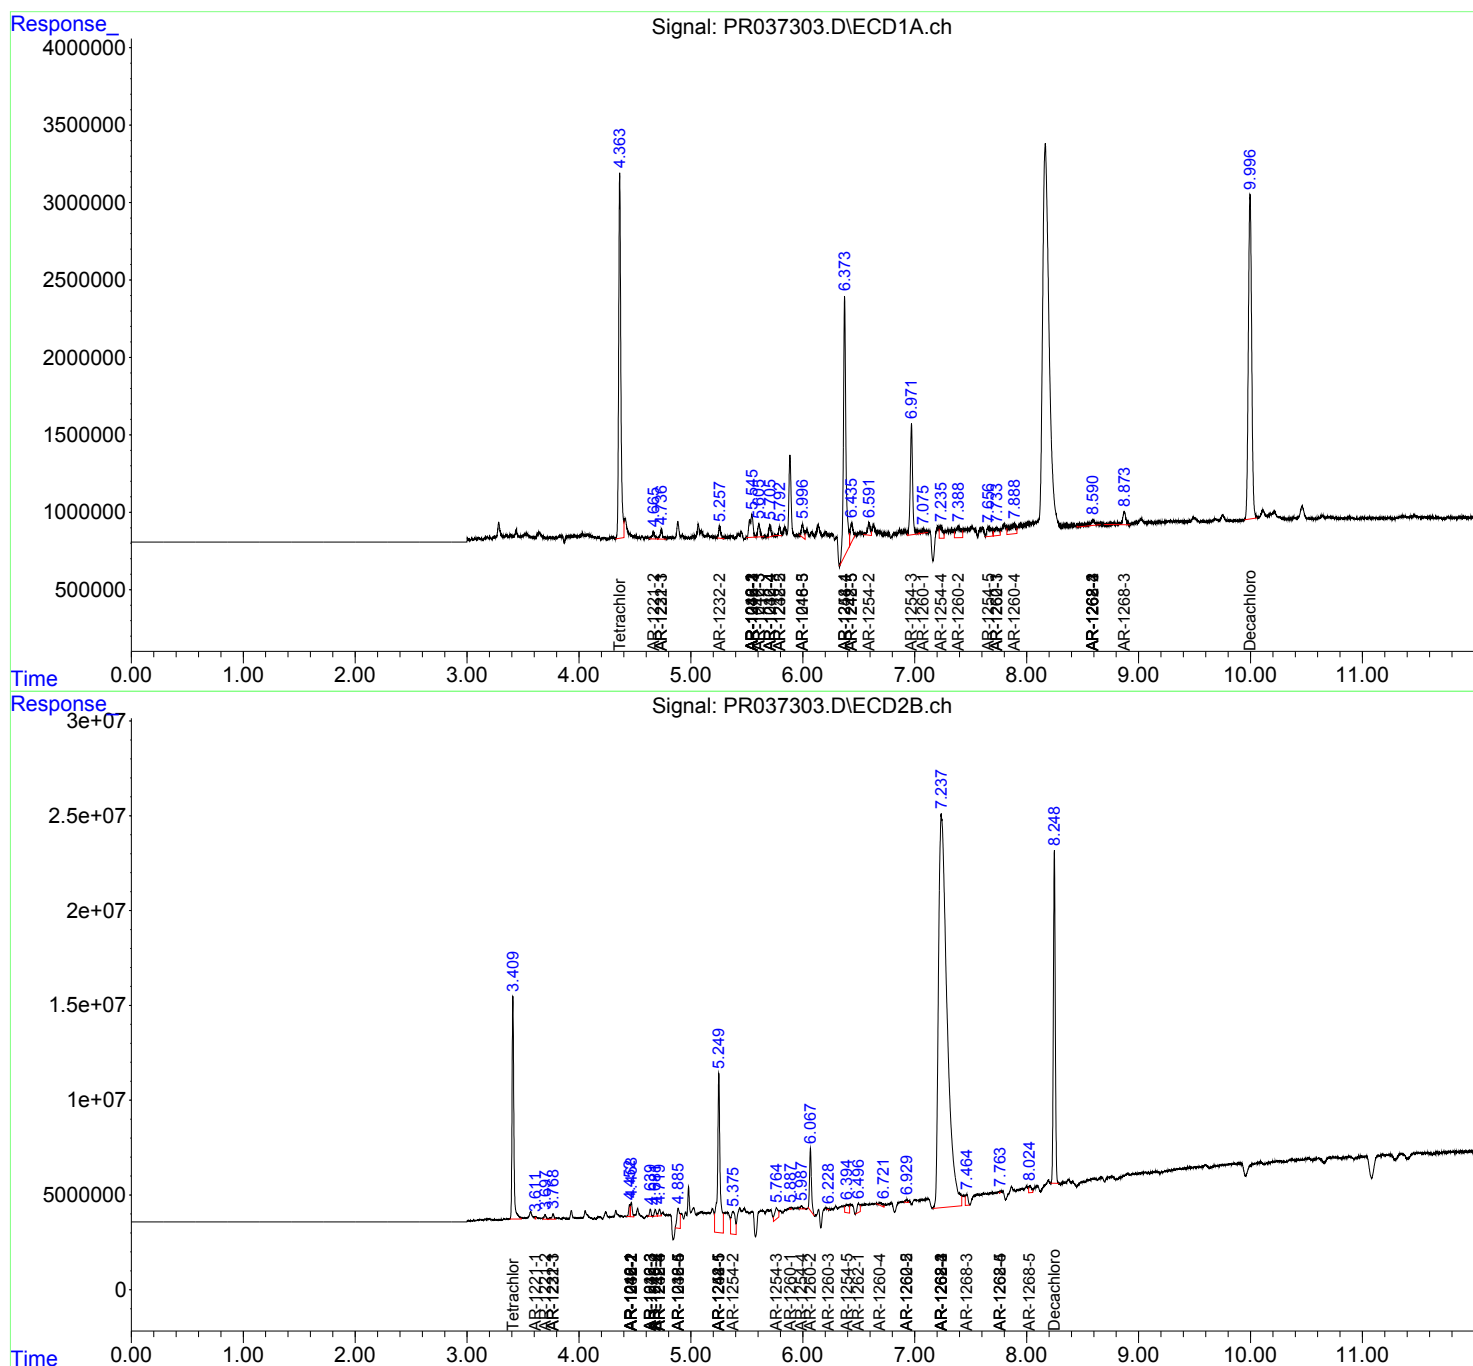


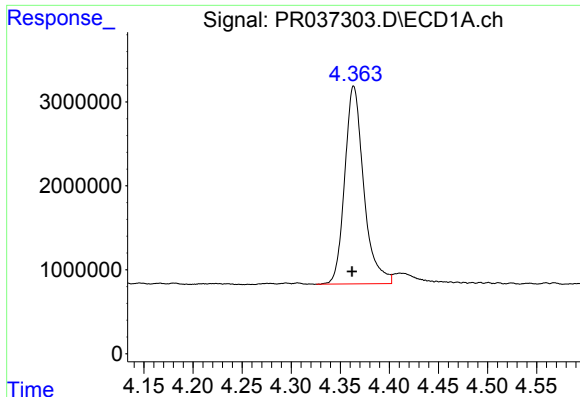

#1 Tetrachloro-m-xylene


R.T.: 4.364 min
Delta R.T.: 0.002 min
Response: 31724502
Conc: 25.36 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

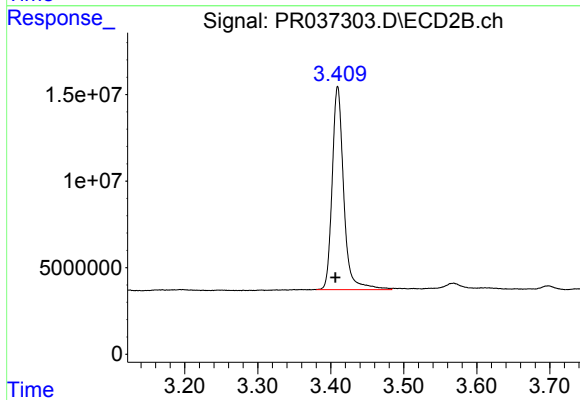


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.003 min
Response: 129190736
Conc: 26.94 ng/ml

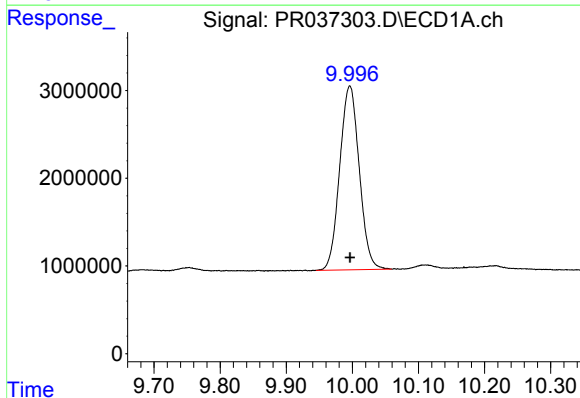


#2 Decachlorobiphenyl

R.T.: 9.996 min
Delta R.T.: 0.000 min
Response: 43044146
Conc: 32.55 ng/ml

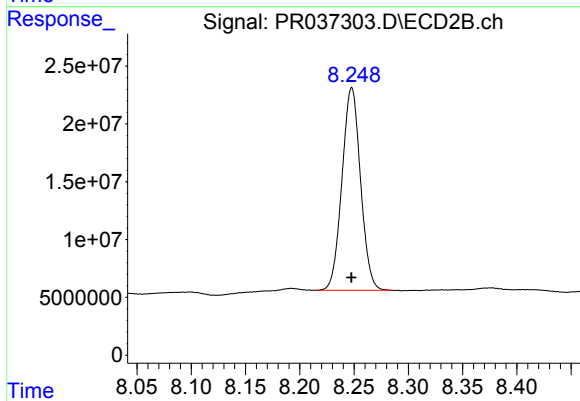

#2 Decachlorobiphenyl


R.T.: 8.248 min
Delta R.T.: 0.000 min
Response: 208436653
Conc: 35.79 ng/ml

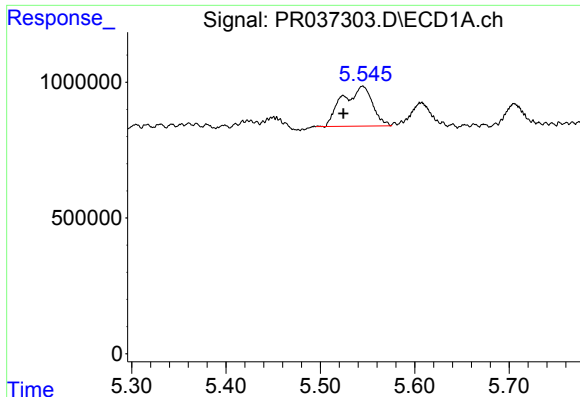

#3 AR-1016-1


R.T.: 5.545 min
Delta R.T.: 0.021 min
Response: 3239676
Conc: 75.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

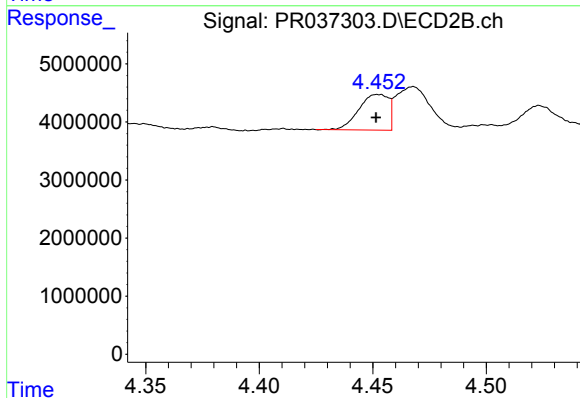


#3 AR-1016-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 5559888
Conc: 30.54 ng/ml

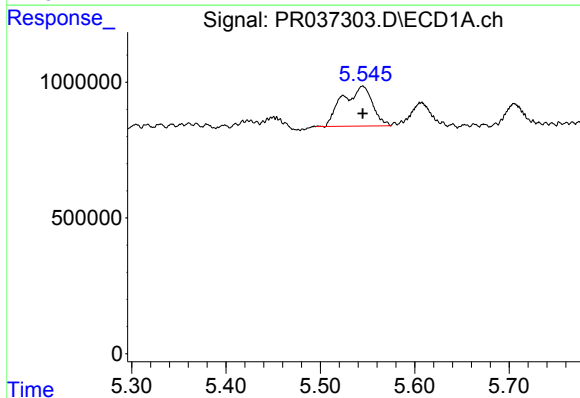


#4 AR-1016-2

R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 3239676
Conc: 46.78 ng/ml

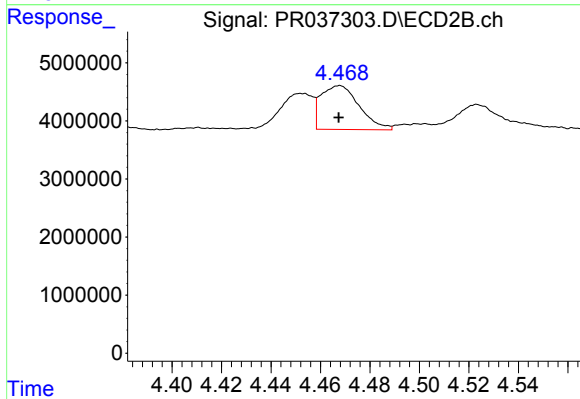

#4 AR-1016-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 8170286
Conc: 28.96 ng/ml

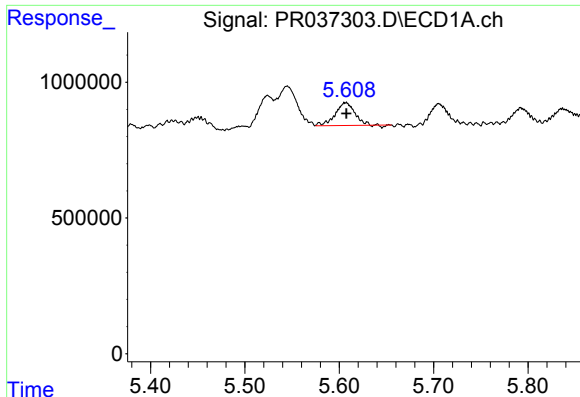

#5 AR-1016-3


R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 1202052
Conc: 29.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

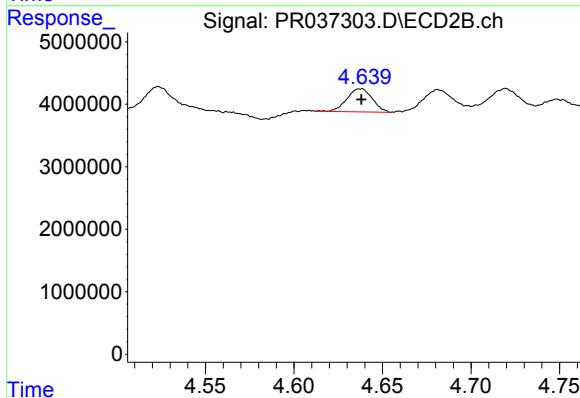


#5 AR-1016-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 3694916
Conc: 25.70 ng/ml

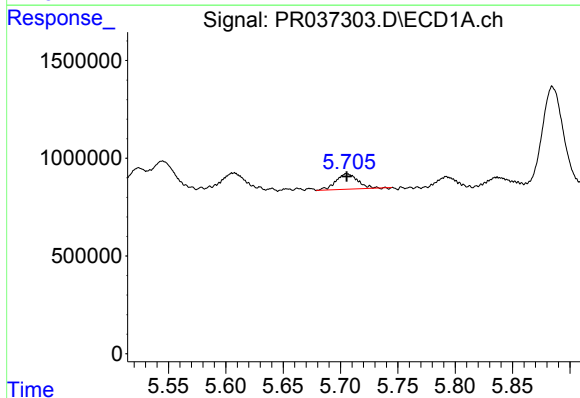


#6 AR-1016-4

R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 1042476
Conc: 31.74 ng/ml

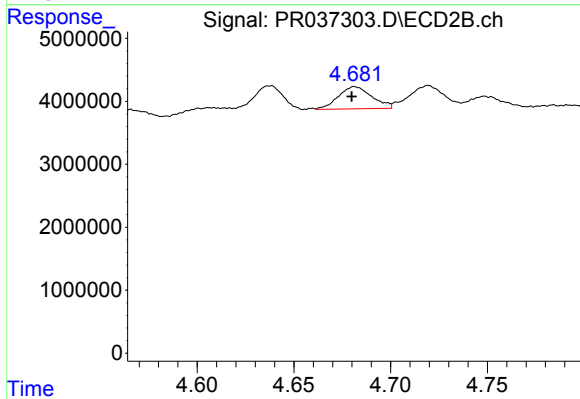

#6 AR-1016-4


R.T.: 4.681 min
Delta R.T.: 0.001 min
Response: 4236329
Conc: 38.29 ng/ml

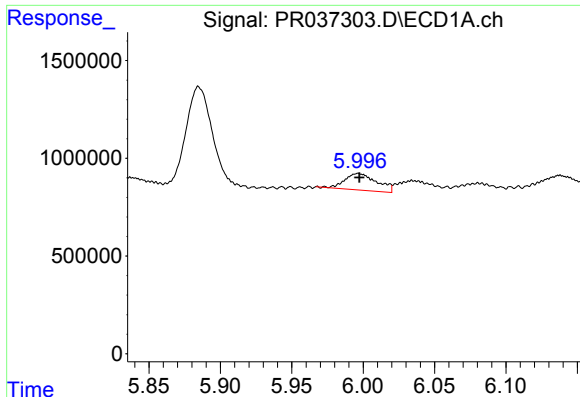

#7 AR-1016-5


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 1318753
Conc: 38.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

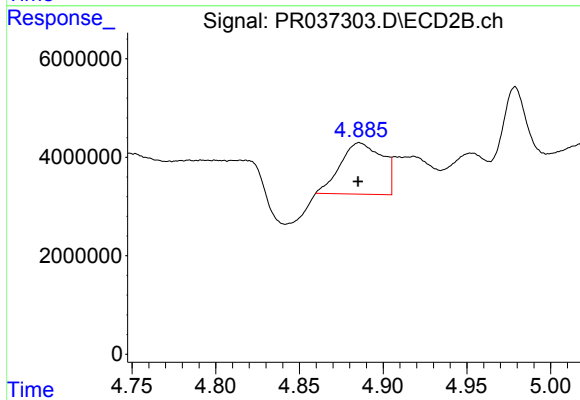


#7 AR-1016-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 18212716
Conc: 119.81 ng/ml

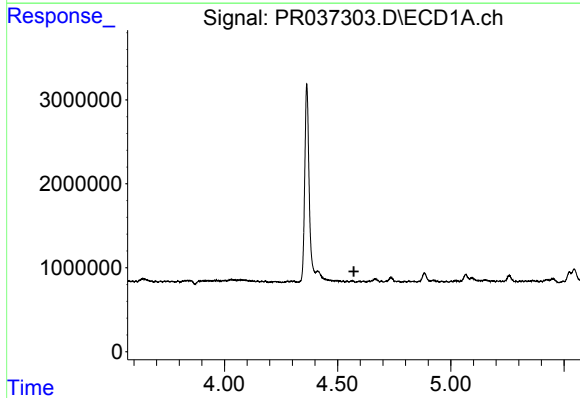


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

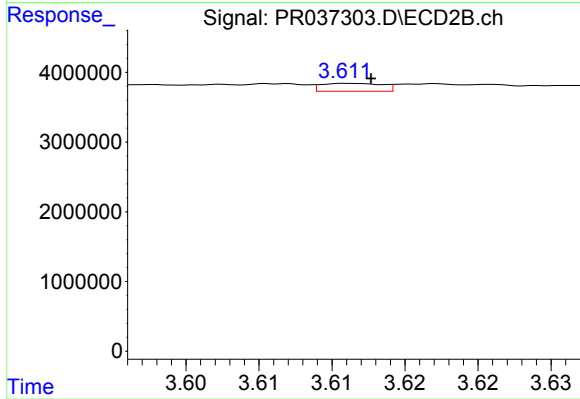

#8 AR-1221-1


R.T.: 3.612 min
Delta R.T.: -0.001 min
Response: 328633
Conc: 6.45 ng/ml

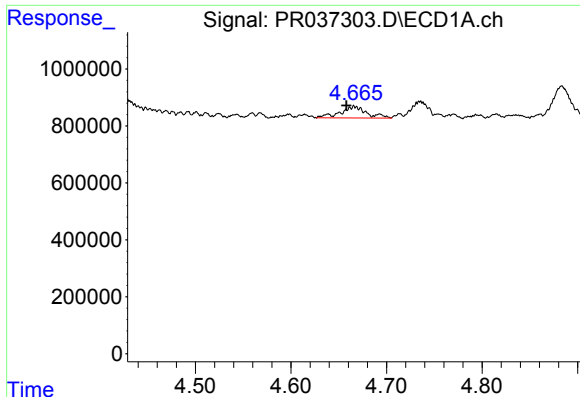

#9 AR-1221-2


R.T.: 4.666 min
Delta R.T.: 0.008 min
Response: 775699
Conc: 85.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

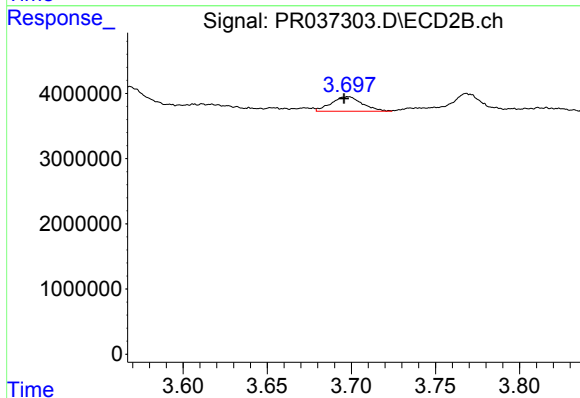


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.003 min
Response: 2878633
Conc: 77.52 ng/ml

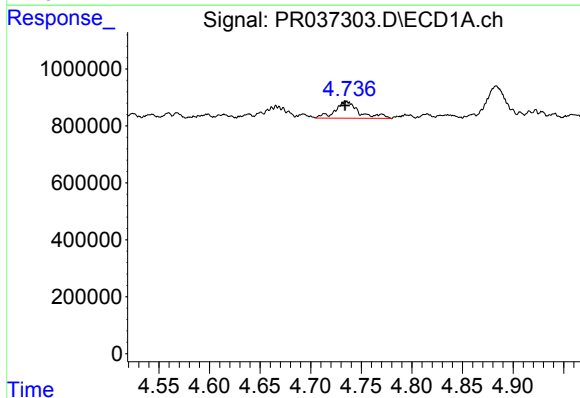


#10 AR-1221-3

R.T.: 4.735 min
Delta R.T.: 0.001 min
Response: 969785
Conc: 31.64 ng/ml

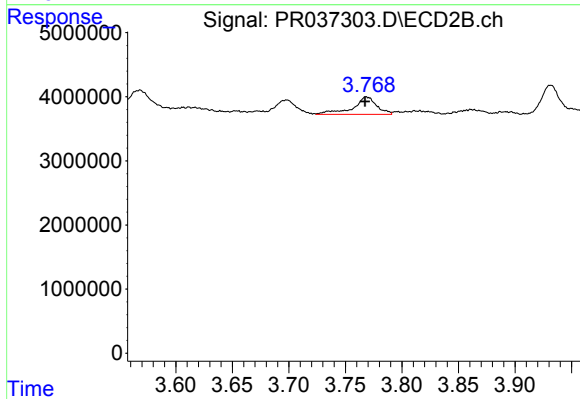

#10 AR-1221-3


R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 3987267
Conc: 32.56 ng/ml

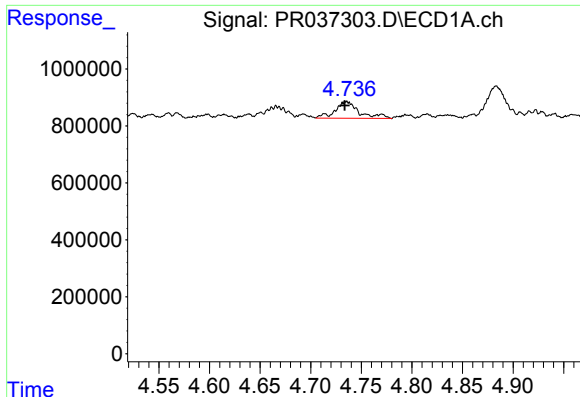

#11 AR-1232-1


R.T.: 4.735 min
Delta R.T.: 0.002 min
Response: 969785
Conc: 33.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

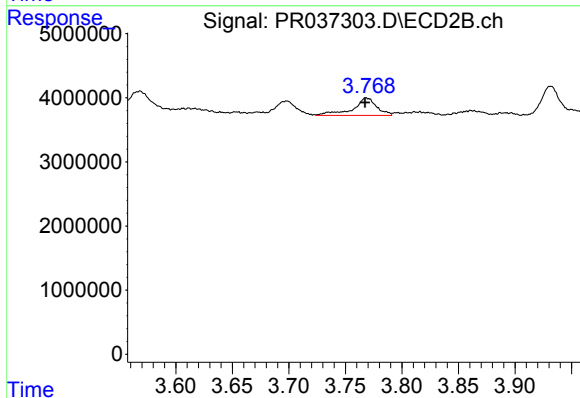


#11 AR-1232-1

R.T.: 3.768 min
Delta R.T.: 0.001 min
Response: 3987267
Conc: 34.08 ng/ml

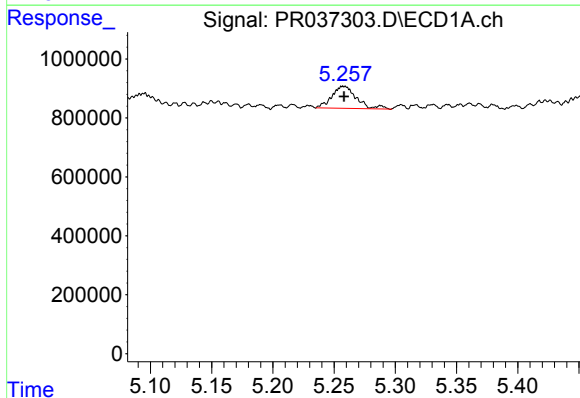


#12 AR-1232-2

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 1044067
Conc: 61.79 ng/ml

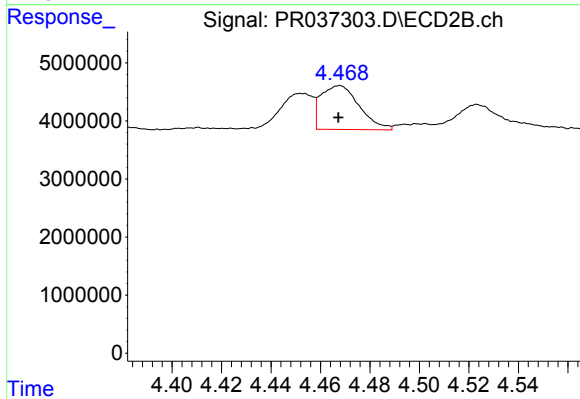

#12 AR-1232-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 8170286
Conc: 59.11 ng/ml

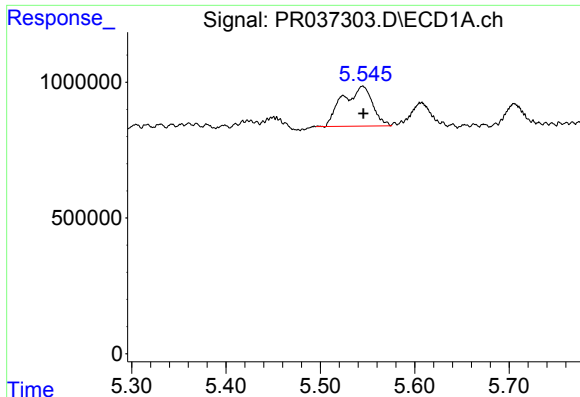

#13 AR-1232-3


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 3239676
Conc: 95.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

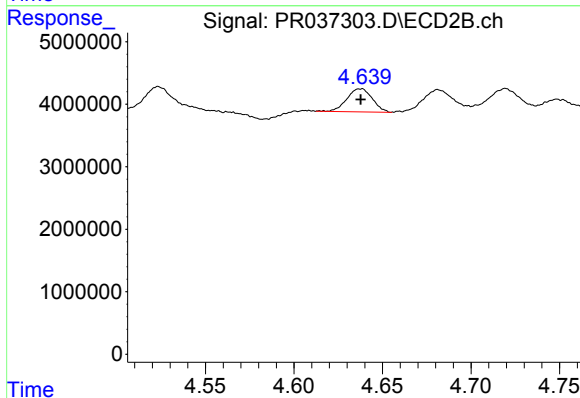


#13 AR-1232-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 3694916
Conc: 52.63 ng/ml

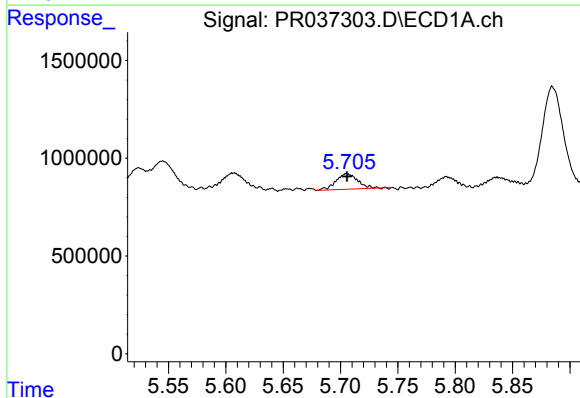


#14 AR-1232-4

R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 1042476
Conc: 66.41 ng/ml

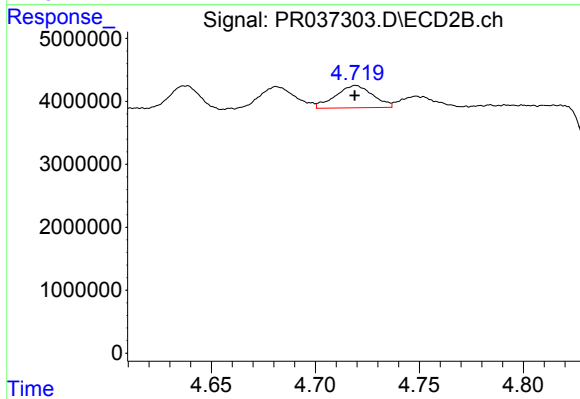

#14 AR-1232-4


R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 4440862
Conc: 74.42 ng/ml

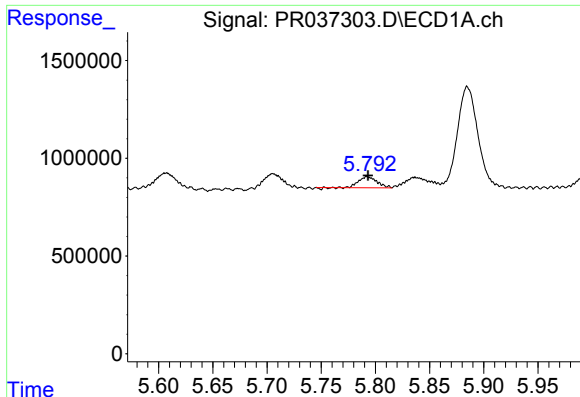

#15 AR-1232-5


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 653151
Conc: 55.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

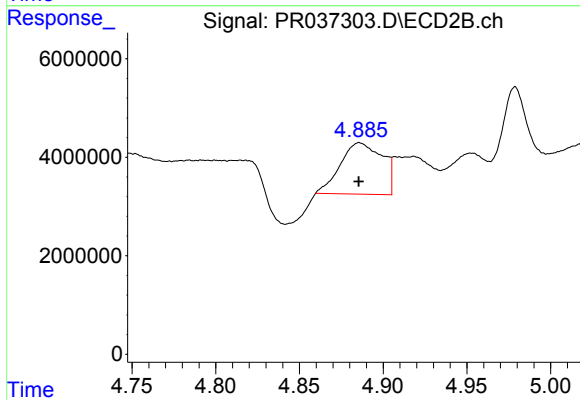


#15 AR-1232-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 18212716
Conc: 266.88 ng/ml

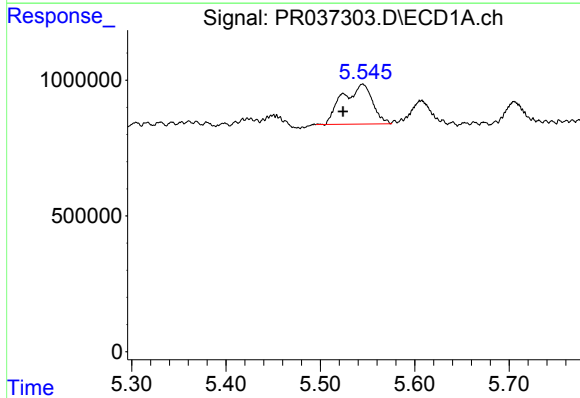


#16 AR-1242-1

R.T.: 5.545 min
Delta R.T.: 0.021 min
Response: 3239676
Conc: 94.69 ng/ml

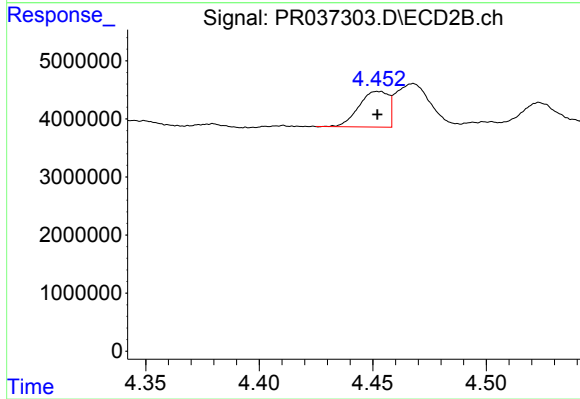

#16 AR-1242-1


R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 5559888
Conc: 37.94 ng/ml

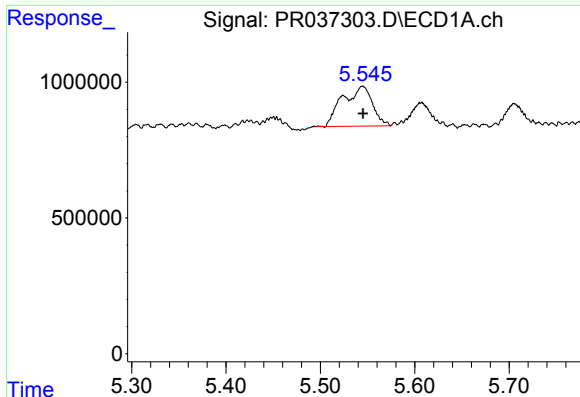

#17 AR-1242-2


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 3239676
Conc: 58.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

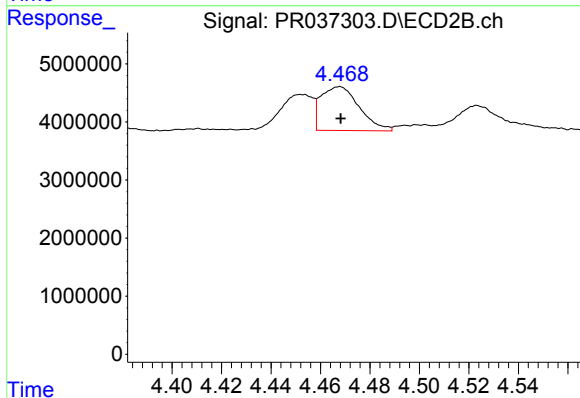


#17 AR-1242-2

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 8170286
Conc: 35.81 ng/ml

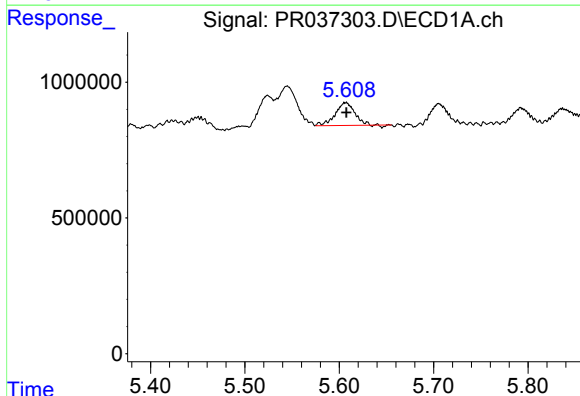


#18 AR-1242-3

R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 1202052
Conc: 36.52 ng/ml

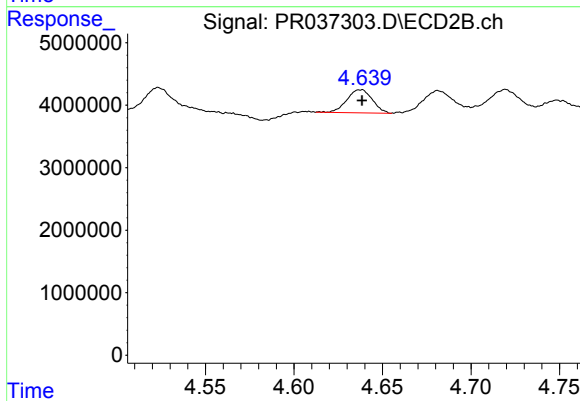

#18 AR-1242-3


R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 3694916
Conc: 31.95 ng/ml

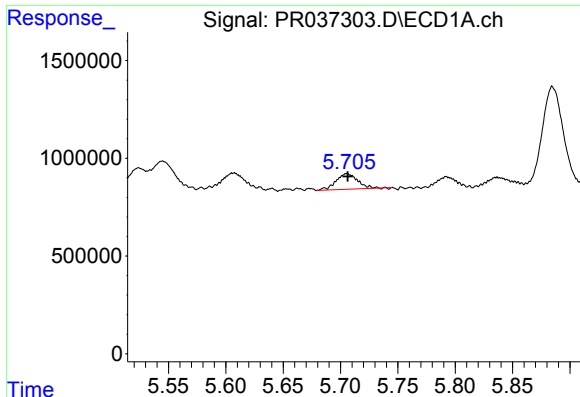

#19 AR-1242-4


R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 1042476
Conc: 39.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

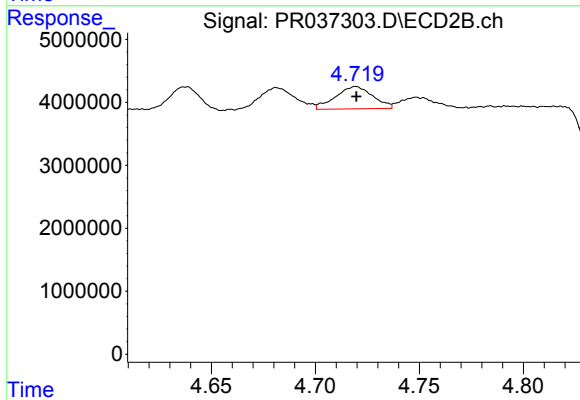


#19 AR-1242-4

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 4440862
Conc: 40.40 ng/ml

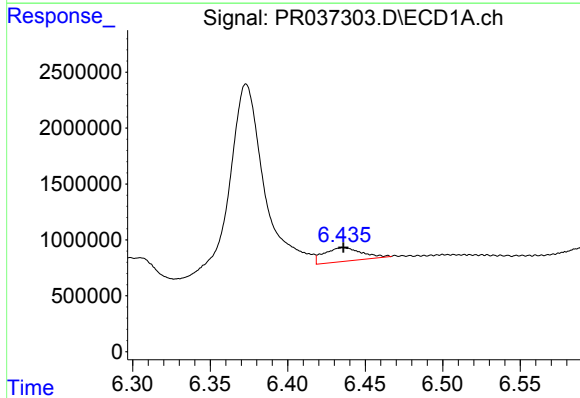


#20 AR-1242-5

R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 2085015
Conc: 64.79 ng/ml

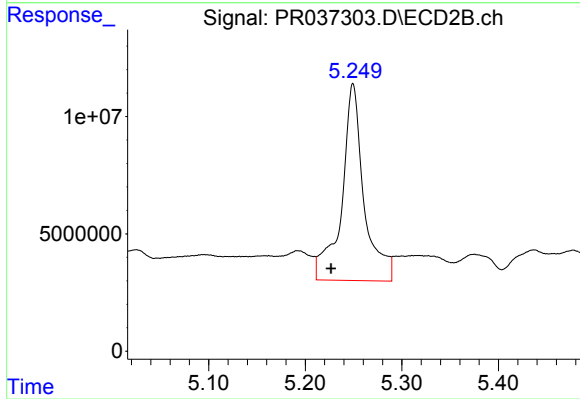

#20 AR-1242-5


R.T.: 5.249 min
Delta R.T.: 0.023 min
Response: 134279483
Conc: 810.38 ng/ml

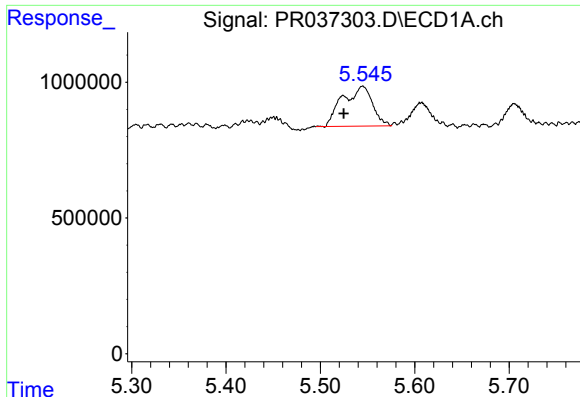

#21 AR-1248-1


R.T.: 5.545 min
Delta R.T.: 0.020 min
Response: 3239676
Conc: 141.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

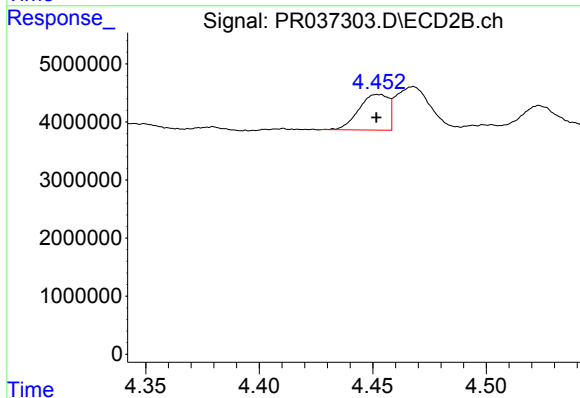


#21 AR-1248-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 5559888
Conc: 55.23 ng/ml

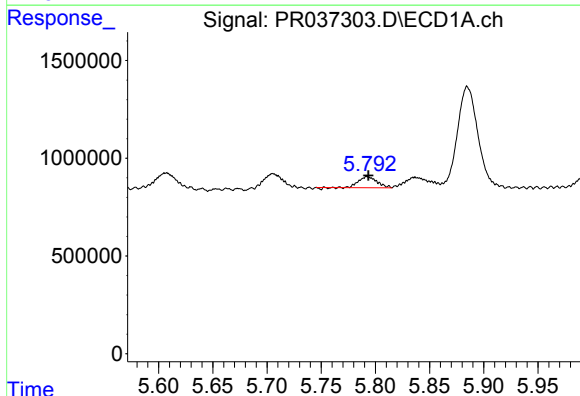


#22 AR-1248-2

R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 653151
Conc: 18.65 ng/ml

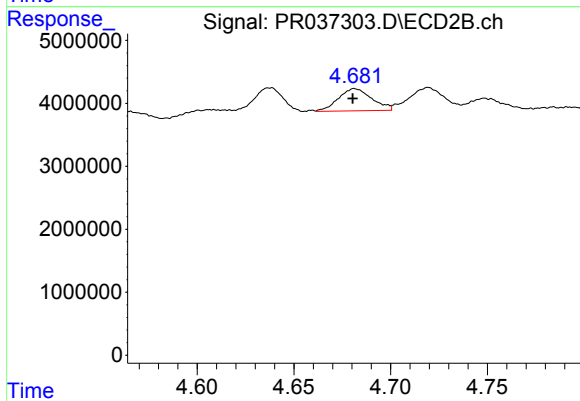

#22 AR-1248-2


R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 4236329
Conc: 31.04 ng/ml

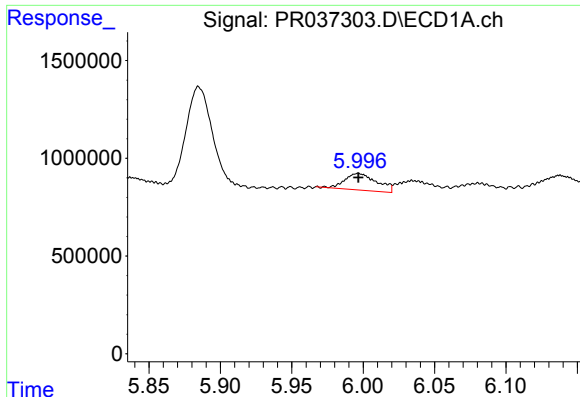

#23 AR-1248-3


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 1318753
Conc: 32.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

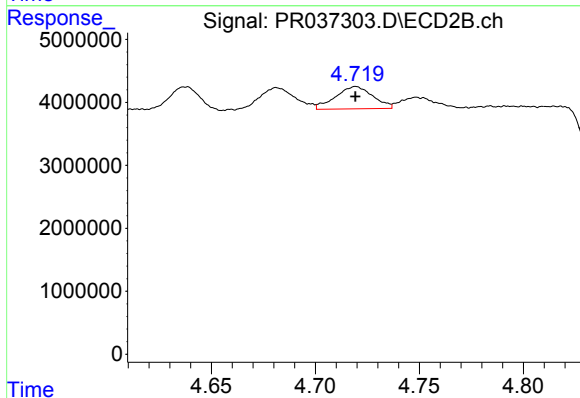


#23 AR-1248-3

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 4440862
Conc: 31.73 ng/ml

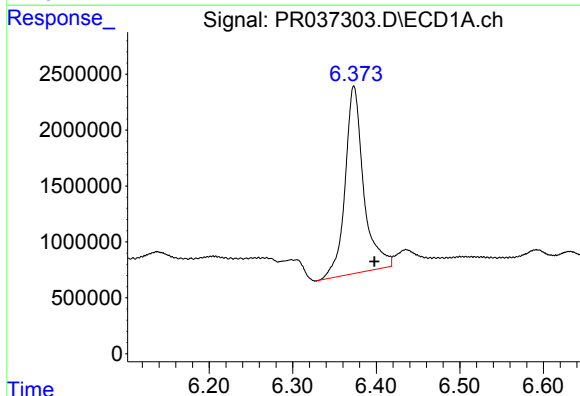


#24 AR-1248-4

R.T.: 6.373 min
Delta R.T.: -0.025 min
Response: 25740227
Conc: 525.80 ng/ml

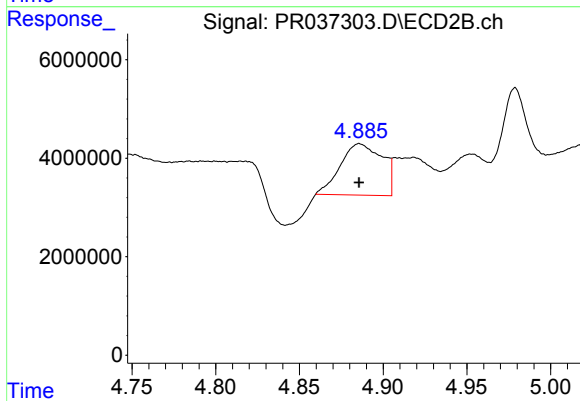

#24 AR-1248-4


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 18212716
Conc: 102.34 ng/ml

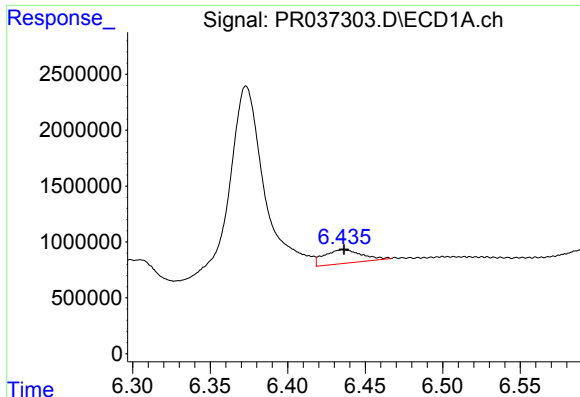

#25 AR-1248-5


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 2085015
Conc: 44.14 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

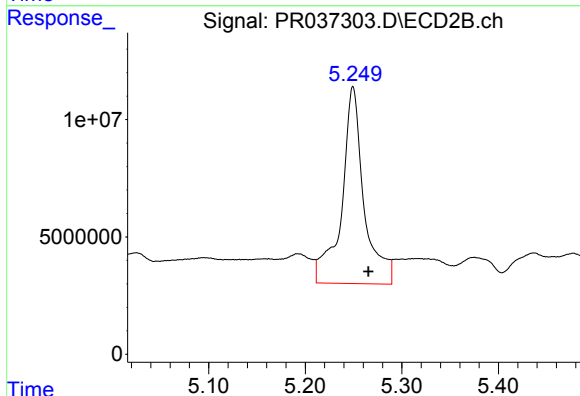


#25 AR-1248-5

R.T.: 5.249 min
Delta R.T.: -0.016 min
Response: 134279483
Conc: 686.46 ng/ml

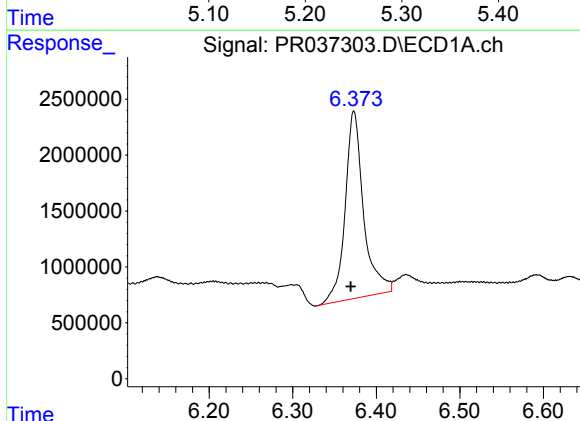


#26 AR-1254-1

R.T.: 6.373 min
Delta R.T.: 0.004 min
Response: 25740227
Conc: 471.17 ng/ml

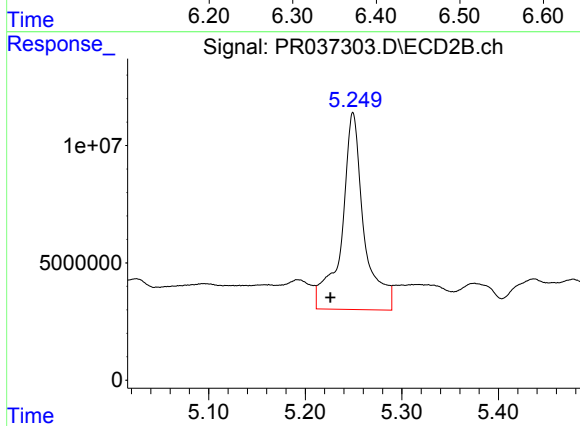

#26 AR-1254-1


R.T.: 5.249 min
Delta R.T.: 0.023 min
Response: 134279483
Conc: 389.81 ng/ml

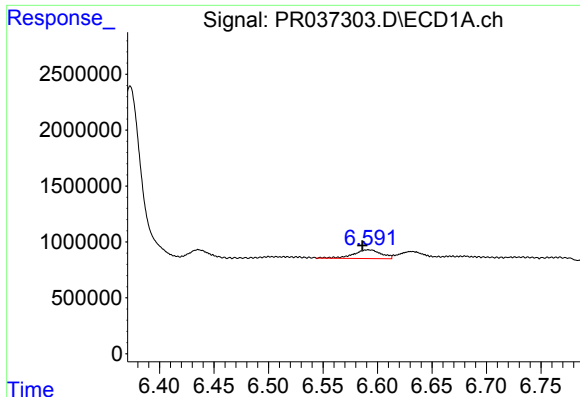

#27 AR-1254-2


R.T.: 6.592 min
Delta R.T.: 0.006 min
Response: 1354543
Conc: 15.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

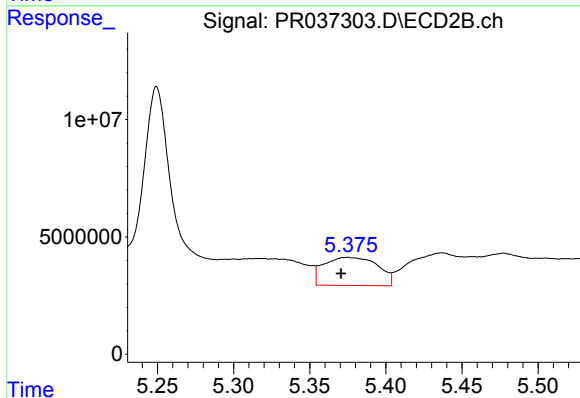


#27 AR-1254-2

R.T.: 5.375 min
Delta R.T.: 0.005 min
Response: 29504326
Conc: 98.51 ng/ml

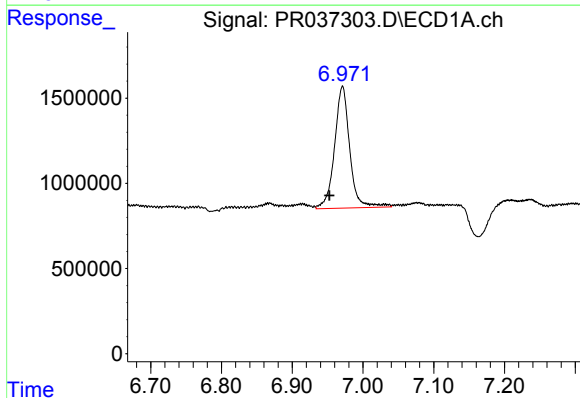


#28 AR-1254-3

R.T.: 6.971 min
Delta R.T.: 0.018 min
Response: 10685644
Conc: 117.47 ng/ml

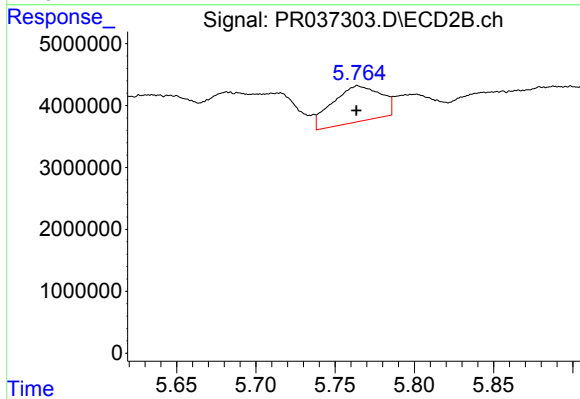

#28 AR-1254-3


R.T.: 5.764 min
Delta R.T.: 0.000 min
Response: 12281464
Conc: 25.93 ng/ml

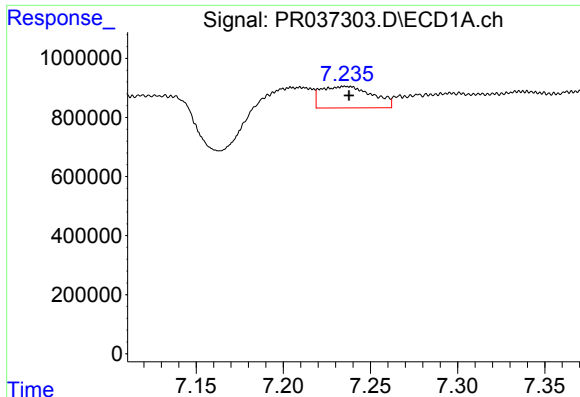

#29 AR-1254-4


R.T.: 7.236 min
Delta R.T.: -0.002 min
Response: 1494751
Conc: 22.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

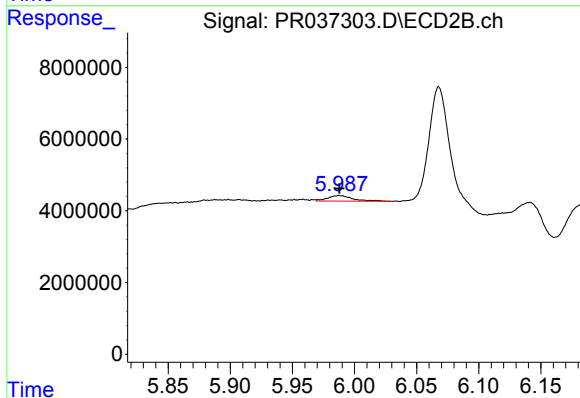


#29 AR-1254-4

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 2239760
Conc: 6.39 ng/ml

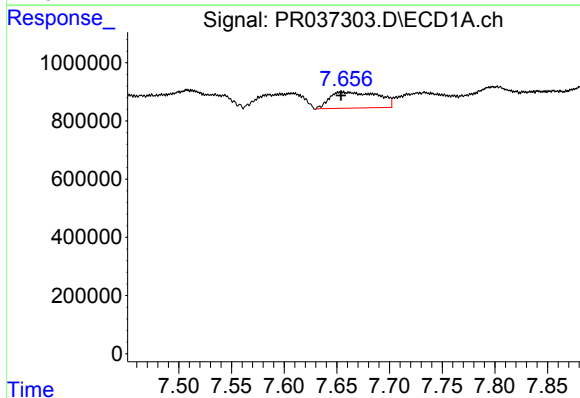


#30 AR-1254-5

R.T.: 7.656 min
Delta R.T.: 0.002 min
Response: 1764132
Conc: 24.54 ng/ml

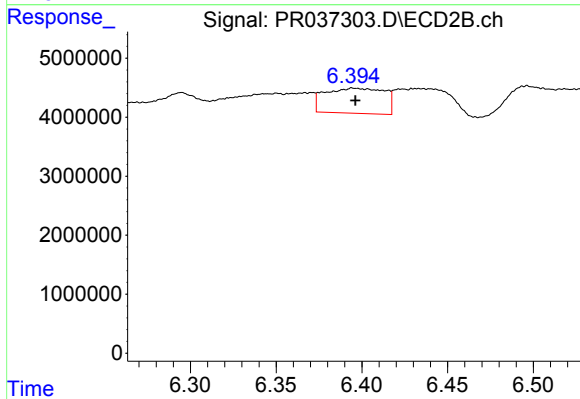

#30 AR-1254-5


R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 10304990
Conc: 23.27 ng/ml

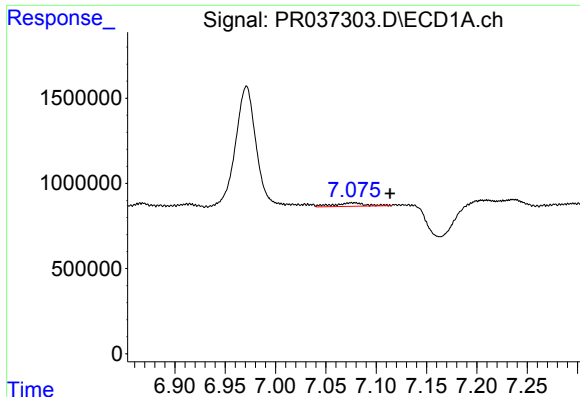

#31 AR-1260-1


R.T.: 7.076 min
Delta R.T.: -0.038 min
Response: 466670
Conc: 7.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

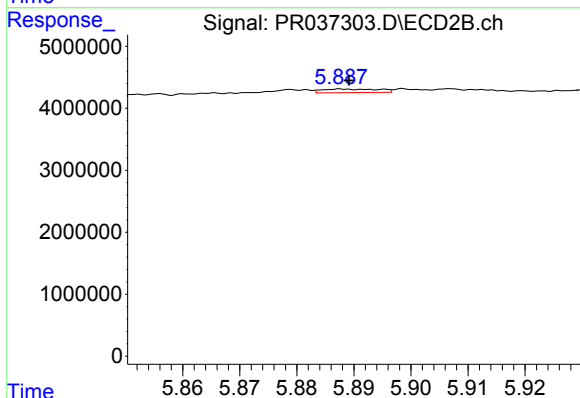


#31 AR-1260-1

R.T.: 5.888 min
Delta R.T.: -0.001 min
Response: 395824
Conc: 1.35 ng/ml

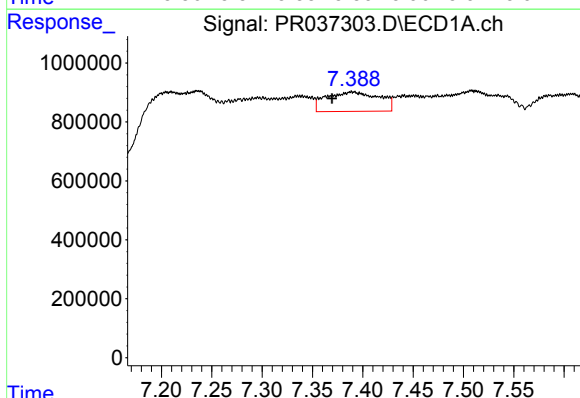


#32 AR-1260-2

R.T.: 7.389 min
Delta R.T.: 0.020 min
Response: 2418476
Conc: 30.34 ng/ml

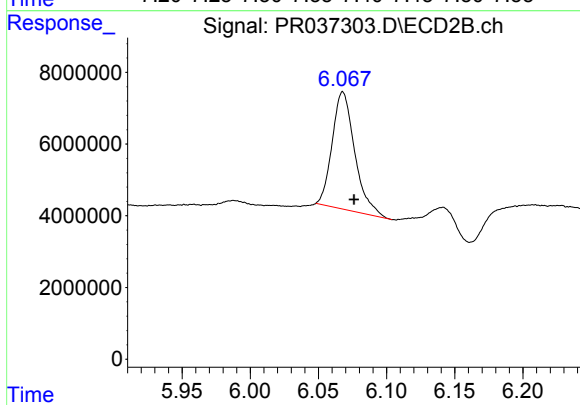

#32 AR-1260-2


R.T.: 6.068 min
Delta R.T.: -0.008 min
Response: 37564895
Conc: 81.56 ng/ml

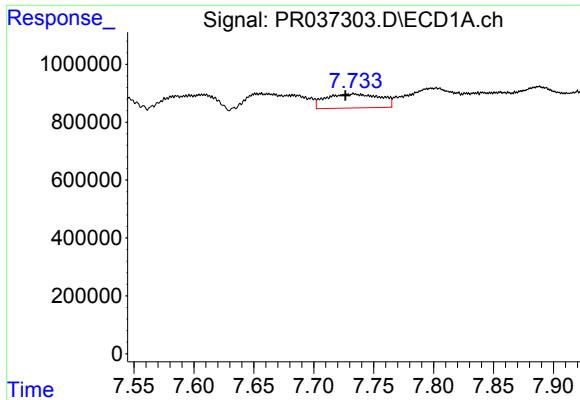

#33 AR-1260-3


R.T.: 7.733 min
Delta R.T.: 0.007 min
Response: 1525572
Conc: 24.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

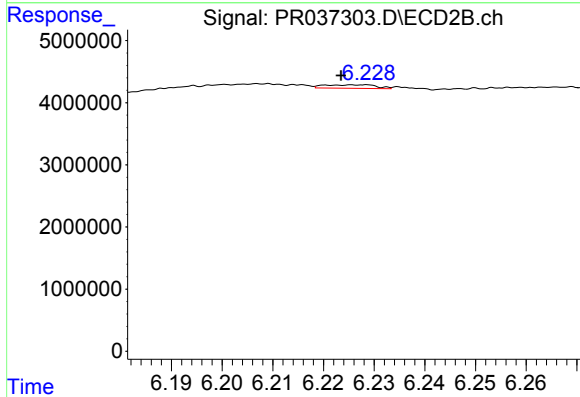


#33 AR-1260-3

R.T.: 6.226 min
Delta R.T.: 0.002 min
Response: 405250
Conc: 1.14 ng/ml

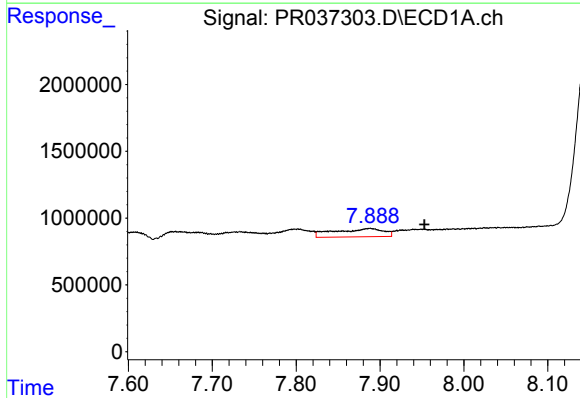


#34 AR-1260-4

R.T.: 7.888 min
Delta R.T.: -0.065 min
Response: 2493674
Conc: 33.52 ng/ml

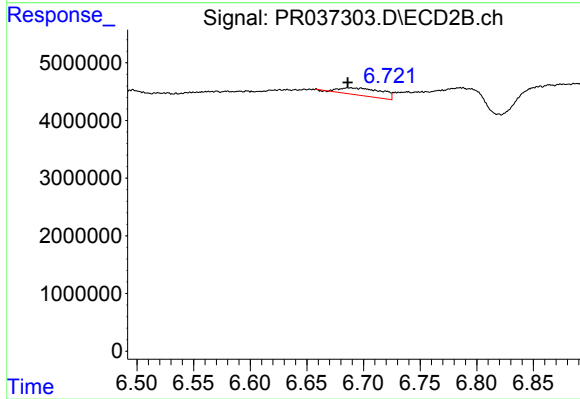

#34 AR-1260-4


R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 3322179
Conc: 10.90 ng/ml

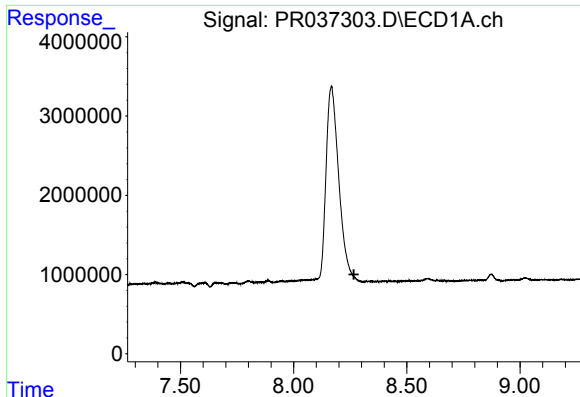

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

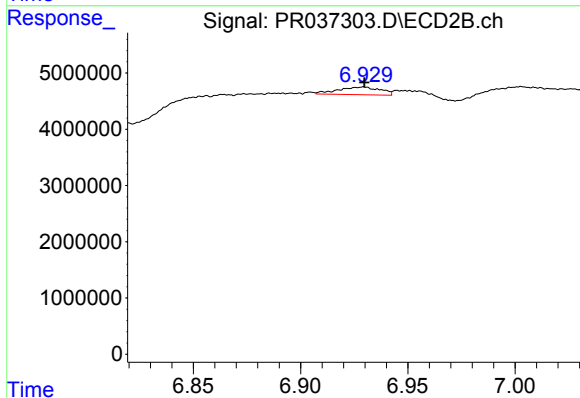


#35 AR-1260-5

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 1878617
Conc: 2.17 ng/ml

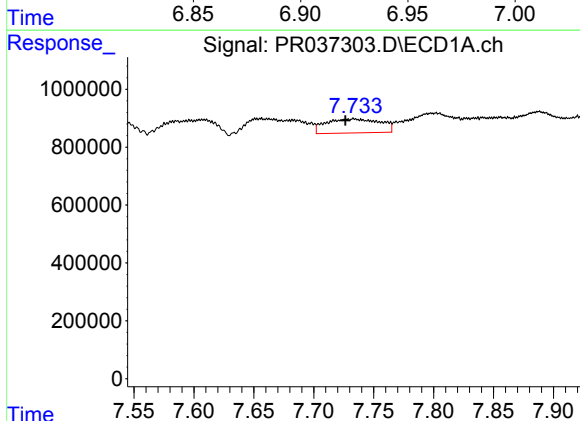


#36 AR-1262-1

R.T.: 7.733 min
Delta R.T.: 0.007 min
Response: 1525572
Conc: 14.61 ng/ml

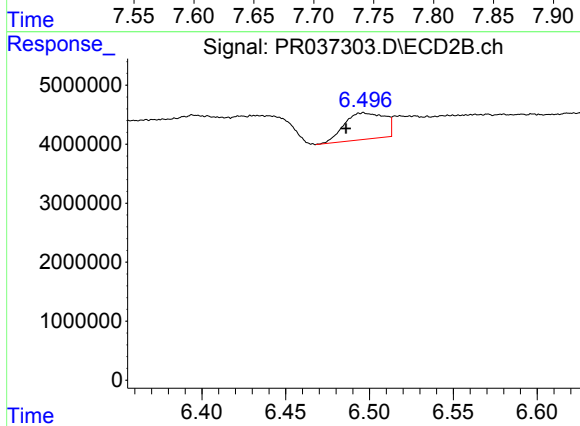

#36 AR-1262-1


R.T.: 6.497 min
Delta R.T.: 0.011 min
Response: 7522838
Conc: 30.02 ng/ml

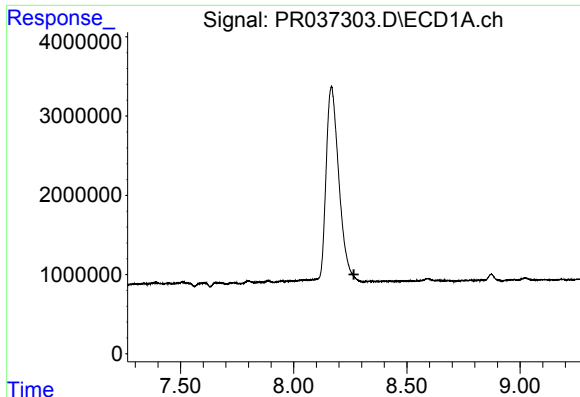

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

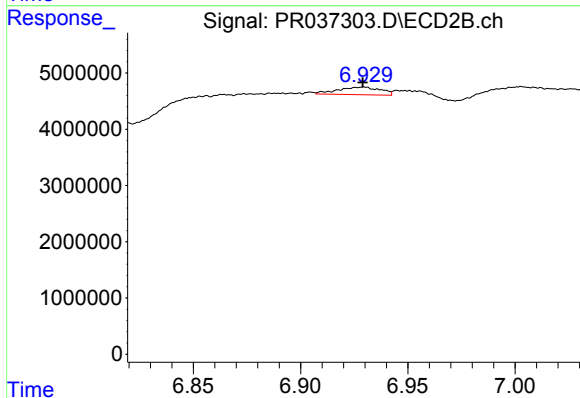


#37 AR-1262-2

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 1878617
Conc: 1.50 ng/ml

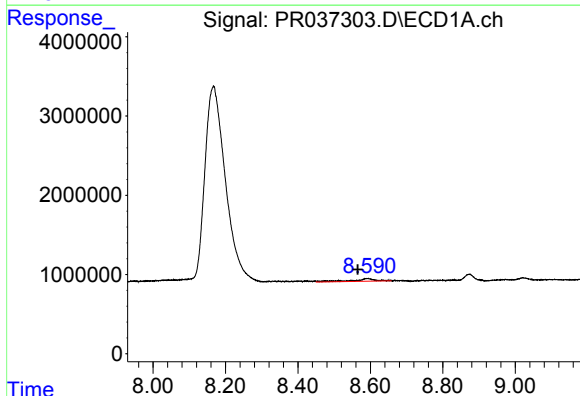


#38 AR-1262-3

R.T.: 8.591 min
Delta R.T.: 0.026 min
Response: 1439489
Conc: 10.95 ng/ml

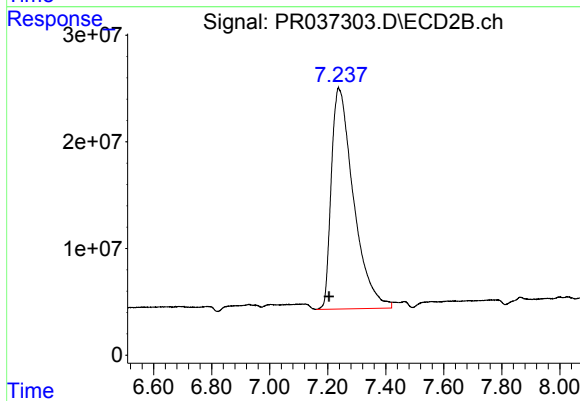

#38 AR-1262-3


R.T.: 7.237 min
Delta R.T.: 0.032 min
Response: 1098014416
Conc: 2002.71 ng/ml

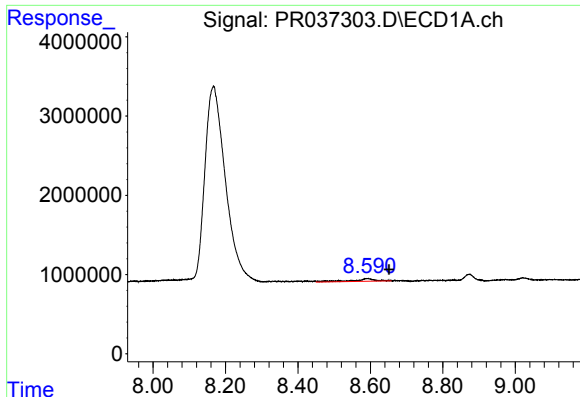

#39 AR-1262-4


R.T.: 8.591 min
Delta R.T.: -0.061 min
Response: 1439489
Conc: 14.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

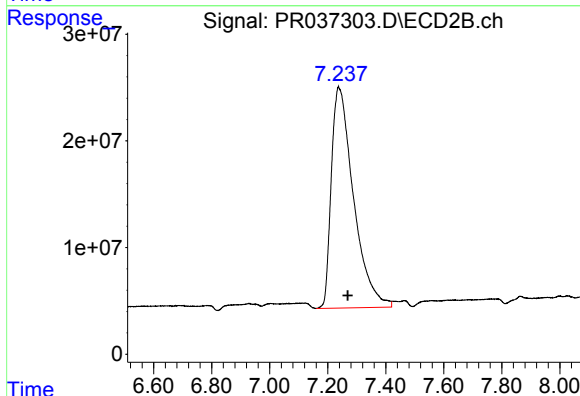


#39 AR-1262-4

R.T.: 7.237 min
Delta R.T.: -0.032 min
Response: 1098014416
Conc: 1223.22 ng/ml

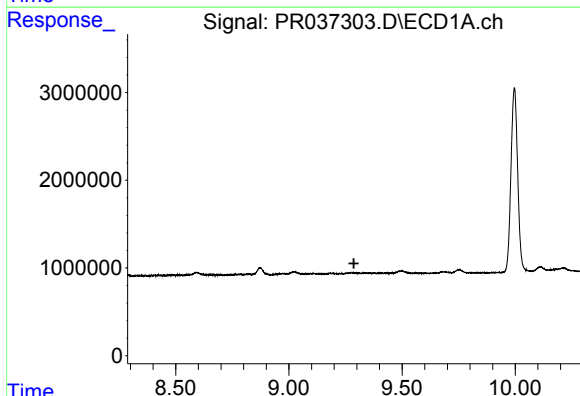


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.287 min
Response: 0
Conc: N.D.

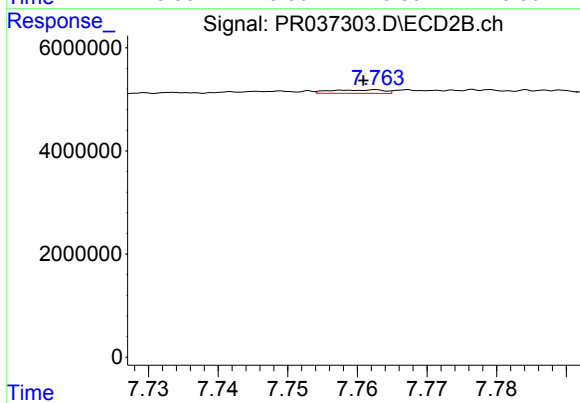

#40 AR-1262-5


R.T.: 7.763 min
Delta R.T.: 0.002 min
Response: 362614
Conc: 0.95 ng/ml

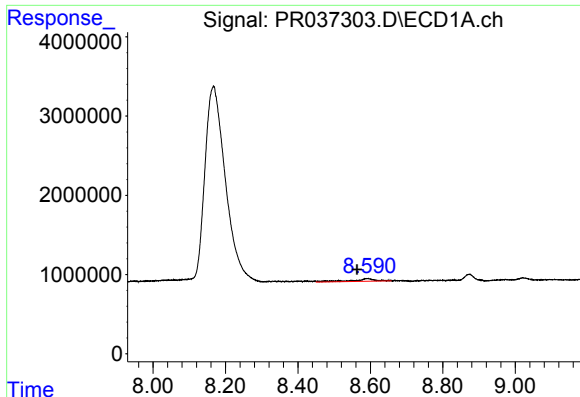

#41 AR-1268-1


R.T.: 8.591 min
Delta R.T.: 0.027 min
Response: 1439489
Conc: 8.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

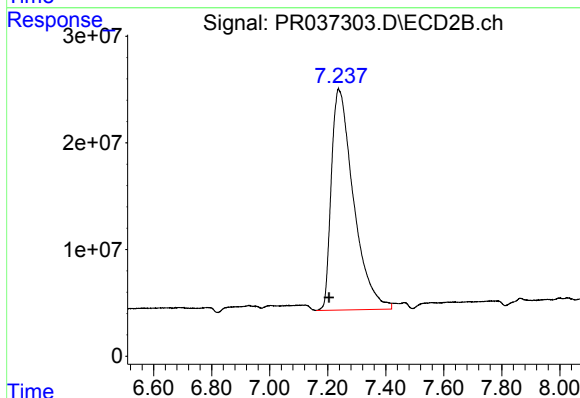


#41 AR-1268-1

R.T.: 7.237 min
Delta R.T.: 0.032 min
Response: 1098014416
Conc: 891.95 ng/ml

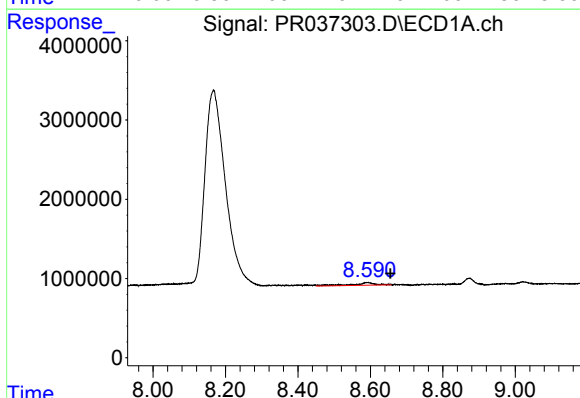


#42 AR-1268-2

R.T.: 8.591 min
Delta R.T.: -0.065 min
Response: 1439489
Conc: 8.75 ng/ml

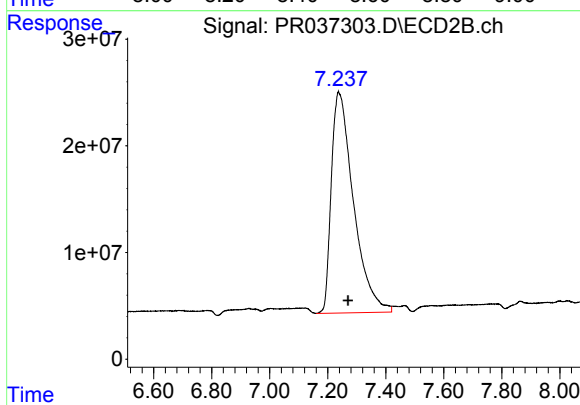

#42 AR-1268-2


R.T.: 7.237 min
Delta R.T.: -0.033 min
Response: 1098014416
Conc: 1036.92 ng/ml

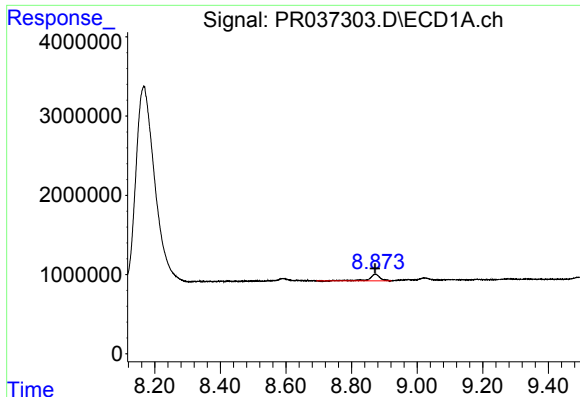

#43 AR-1268-3


R.T.: 8.873 min
Delta R.T.: 0.000 min
Response: 1841662
Conc: 13.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

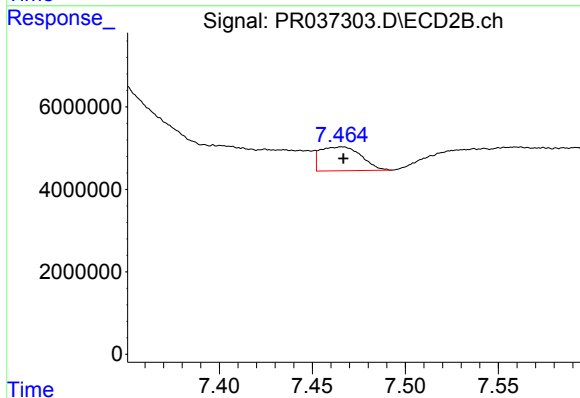


#43 AR-1268-3

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 8904539
Conc: 10.05 ng/ml

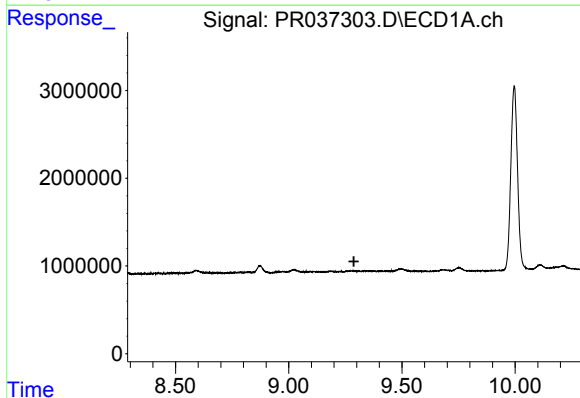


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.288 min
Response: 0
Conc: N.D.

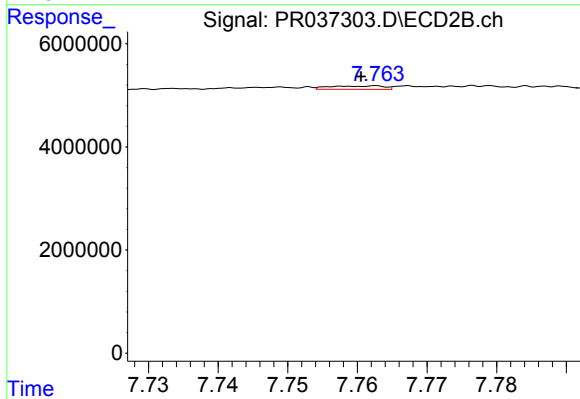

#44 AR-1268-4


R.T.: 7.763 min
Delta R.T.: 0.002 min
Response: 362614
Conc: 1.00 ng/ml

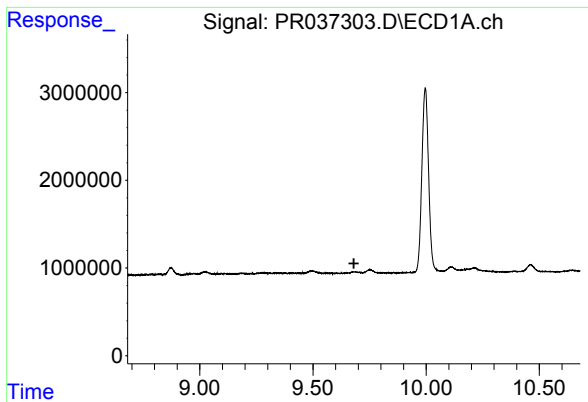

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

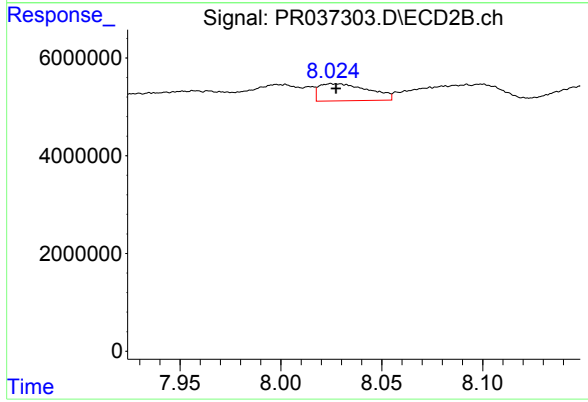

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.003 min
Response: 6020121
Conc: 2.37 ng/ml