

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 20:38
 Operator : SM\SJ
 Sample : K1560-13
 Misc : AR1248 MDL 25PPB
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:54:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.362	3.408	29324358	117.4E6	23.441	24.484
2)	SA Decachlor...	9.994	8.245	40545505	198.3E6	30.656	34.045
Target Compounds							
3)	L1 AR-1016-1	5.525	4.451	722355	3171873	16.764	17.420
4)	L1 AR-1016-2	5.545	4.467	1014643	3430801	14.652	12.161
5)	L1 AR-1016-3	5.608	4.639	532380	2305936	13.201	16.038
6)	L1 AR-1016-4	5.704	4.679	521252	4898160	15.873	44.273 #
7)	L1 AR-1016-5	5.995	4.884	1301173	6372597	37.946	41.922
8)	L2 AR-1221-1	0.000	3.577	0	328730	N.D.	6.456 #
9)	L2 AR-1221-2	4.668	3.696	631499	1627622	69.825	43.829 #
10)	L2 AR-1221-3	4.668	3.770	631499	217155	20.604	1.773 #
11)	L3 AR-1232-1	4.668	3.770	631499	217155	21.589	1.856 #
12)	L3 AR-1232-2	5.258	4.467	491081	3430801	29.062	24.820
13)	L3 AR-1232-3	5.545	4.639	1014643	2305936	30.015	32.847
14)	L3 AR-1232-4	5.704	4.719	521252	4773054	33.208	79.988 #
15)	L3 AR-1232-5	5.793	4.884	1114514	6372597	95.293	93.380
16)	L4 AR-1242-1	5.525	4.451	722355	3171873	21.113	21.645
17)	L4 AR-1242-2	5.545	4.467	1014643	3430801	18.292	15.037
18)	L4 AR-1242-3	5.608	4.639	532380	2305936	16.174	19.942
19)	L4 AR-1242-4	5.704	4.719	521252	4773054	19.761	43.427 #
20)	L4 AR-1242-5	6.435	5.226	1868514	10538958	58.067	63.603
21)	L5 AR-1248-1	5.525	4.451	722355	3171873	31.534	31.510
22)	L5 AR-1248-2	5.793	4.679	1114514	4898160	31.830	35.891
23)	L5 AR-1248-3	5.995	4.719	1301173	4773054	31.806	34.100
24)	L5 AR-1248-4	6.396	4.884	1688557	6372597	34.492	35.808
25)	L5 AR-1248-5	6.435	5.265	1868514	9566417	39.556	48.905
26)	L6 AR-1254-1	6.369	5.226	1606110	10538958	29.399	30.594
27)	L6 AR-1254-2	6.590	5.371	1727698	4989459	20.160	16.659
28)	L6 AR-1254-3	6.953	5.762	1663435	7043747	18.287	14.872
29)	L6 AR-1254-4	7.235	5.989	996326	3140016	14.869	8.955 #
30)	L6 AR-1254-5	0.000	6.395	0	1781284	N.D.	4.023 #
31)	L7 AR-1260-1	7.077	5.905	556239	1831784	8.430	6.267 #
32)	L7 AR-1260-2	0.000	6.071	0	2467440	N.D.	5.357 #
33)	L7 AR-1260-3	0.000	6.219	0	492114	N.D.	1.380 #
34)	L7 AR-1260-4	0.000	6.689	0	255799	N.D.	0.839 #
35)	L7 AR-1260-5	0.000	6.929	0	259151	N.D.	0.299 #
36)	L8 AR-1262-1	0.000	6.492	0	2538272	N.D.	10.128 #
37)	L8 AR-1262-2	0.000	6.929	0	259151	N.D.	0.206 #
38)	L8 AR-1262-3	0.000	7.258	0	26038708	N.D.	47.493 #
39)	L8 AR-1262-4	0.000	7.258	0	26038708	N.D.	29.008 #
40)	L8 AR-1262-5	0.000	7.774	0	1331763	N.D.	3.481 #
41)	L9 AR-1268-1	0.000	7.258	0	26038708	N.D.	21.152 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 20:38
 Operator : SM\SJ
 Sample : K1560-13
 Misc : AR1248 MDL 25PPB
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:54:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.258	0	26038708	N.D.	24.590 #
43) L9	AR-1268-3	0.000	7.465	0	6221455	N.D.	7.020 #
44) L9	AR-1268-4	0.000	7.774	0	1331763	N.D.	3.671 #
45) L9	AR-1268-5	0.000	8.025	0	12506456	N.D.	4.916 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
Data File : PR037304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 20:38
Operator : SM\SJ
Sample : K1560-13
Misc : AR1248 MDL 25PPB
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:54:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

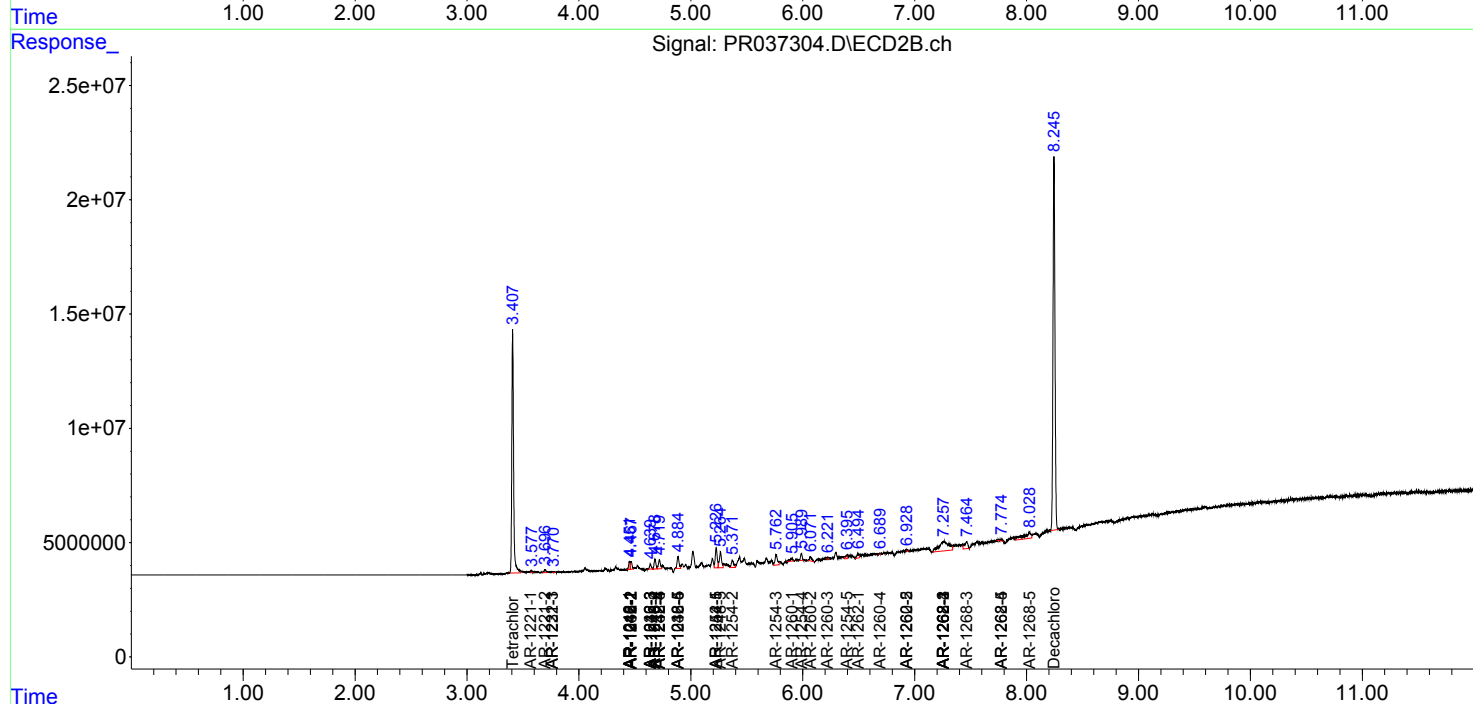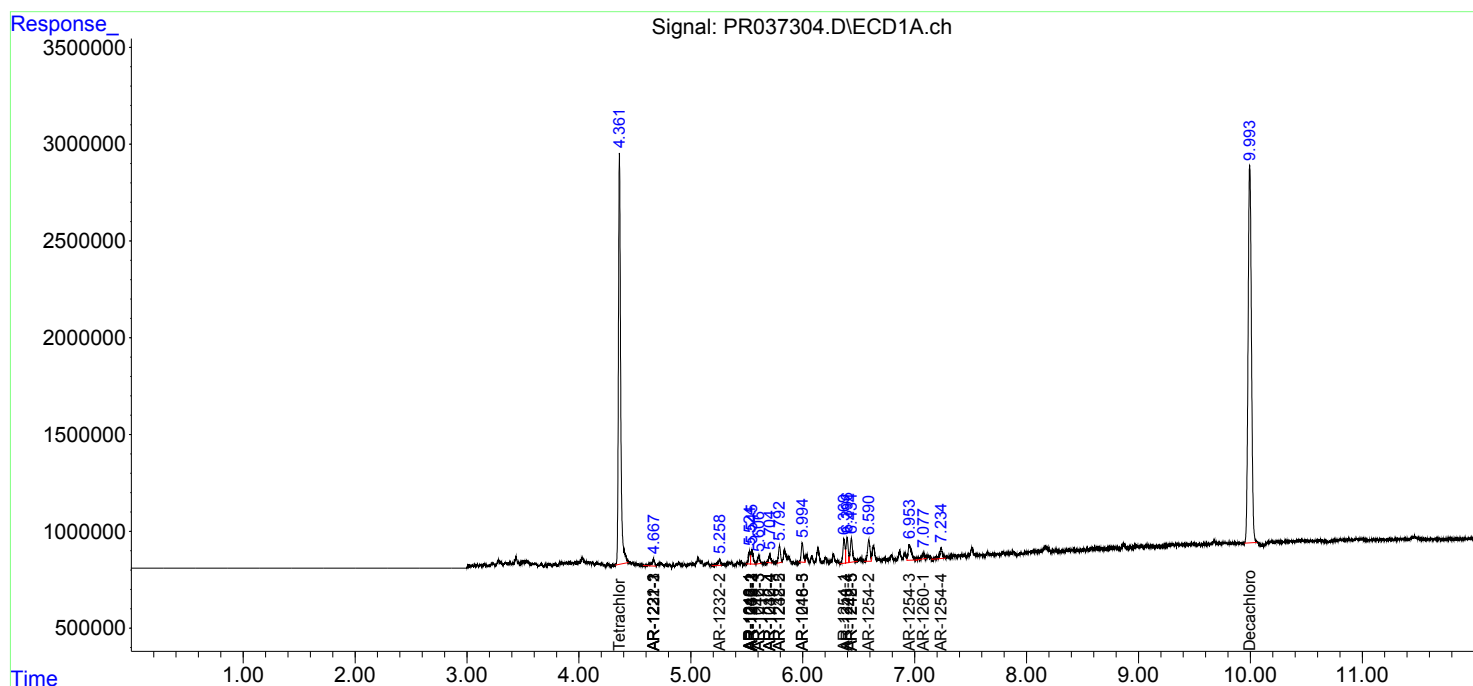


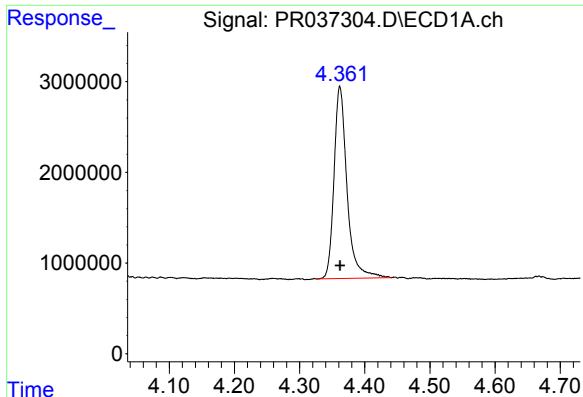

#1 Tetrachloro-m-xylene


R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 29324358
Conc: 23.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

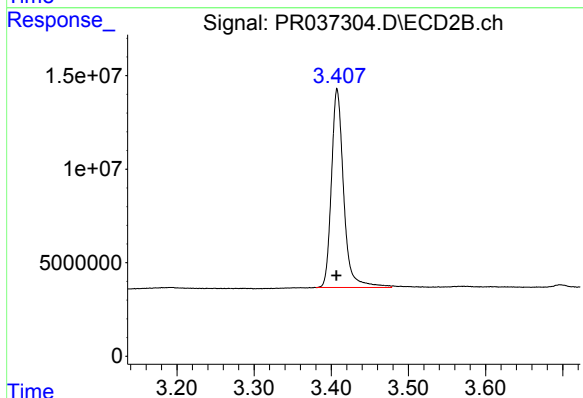


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: 0.001 min
Response: 117415240
Conc: 24.48 ng/ml

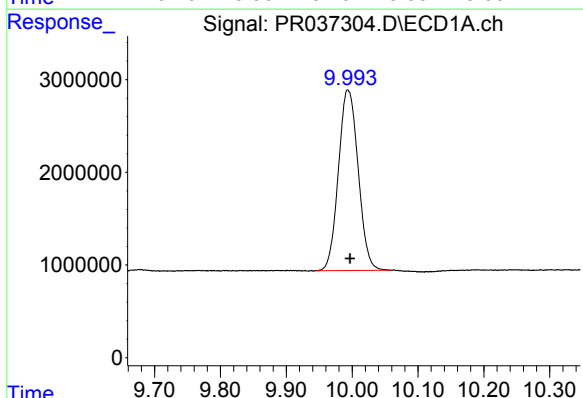


#2 Decachlorobiphenyl

R.T.: 9.994 min
Delta R.T.: -0.003 min
Response: 40545505
Conc: 30.66 ng/ml

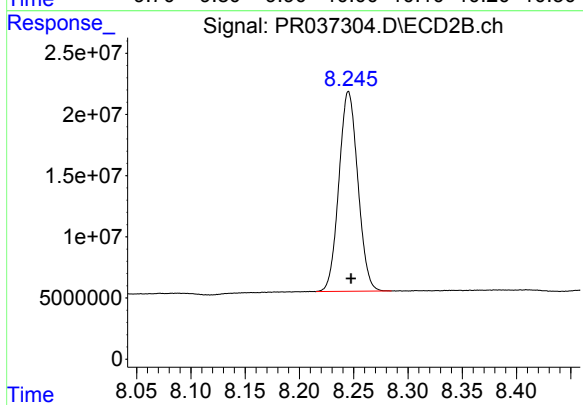

#2 Decachlorobiphenyl


R.T.: 8.245 min
Delta R.T.: -0.002 min
Response: 198284736
Conc: 34.04 ng/ml

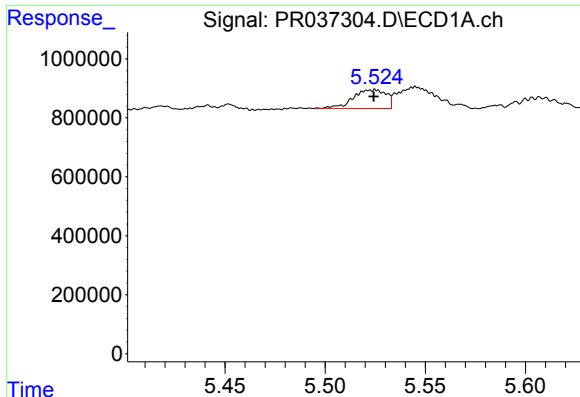

#3 AR-1016-1


R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 722355
Conc: 16.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

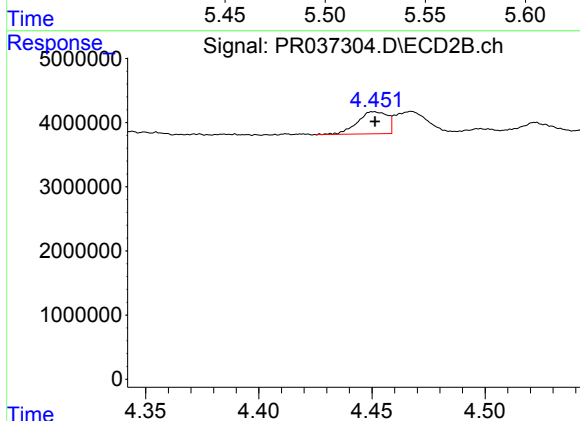


#3 AR-1016-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3171873
Conc: 17.42 ng/ml

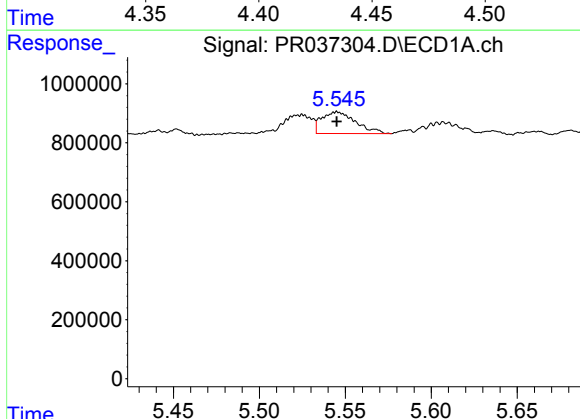


#4 AR-1016-2

R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 1014643
Conc: 14.65 ng/ml

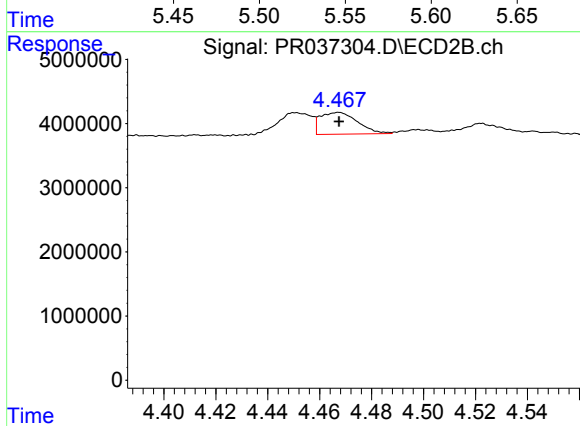

#4 AR-1016-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3430801
Conc: 12.16 ng/ml

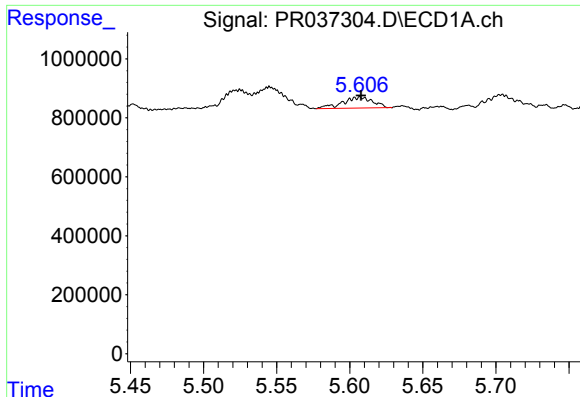

#5 AR-1016-3


R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 532380
Conc: 13.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

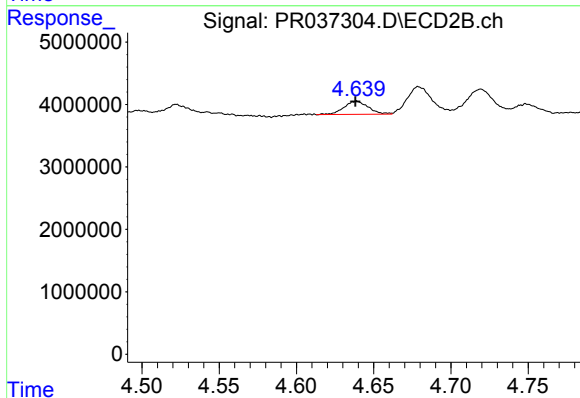


#5 AR-1016-3

R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 2305936
Conc: 16.04 ng/ml

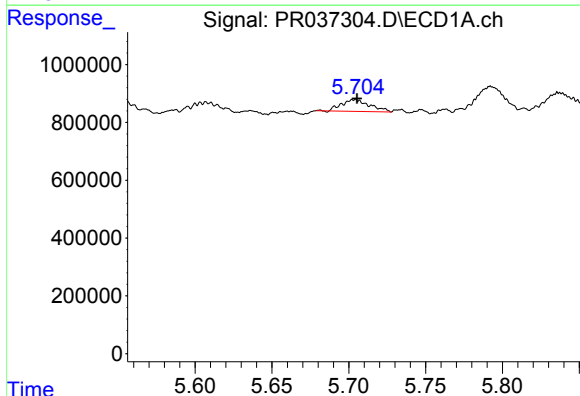


#6 AR-1016-4

R.T.: 5.704 min
Delta R.T.: -0.001 min
Response: 521252
Conc: 15.87 ng/ml

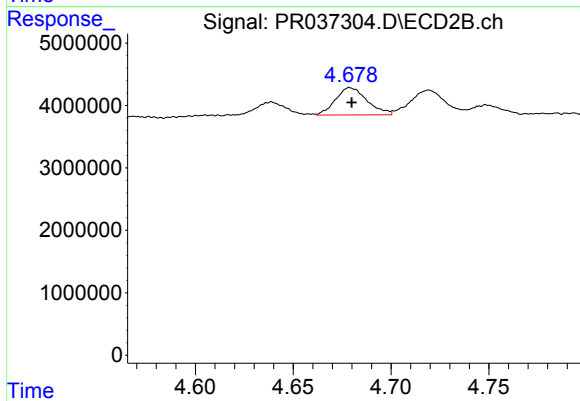

#6 AR-1016-4


R.T.: 4.679 min
Delta R.T.: 0.000 min
Response: 4898160
Conc: 44.27 ng/ml

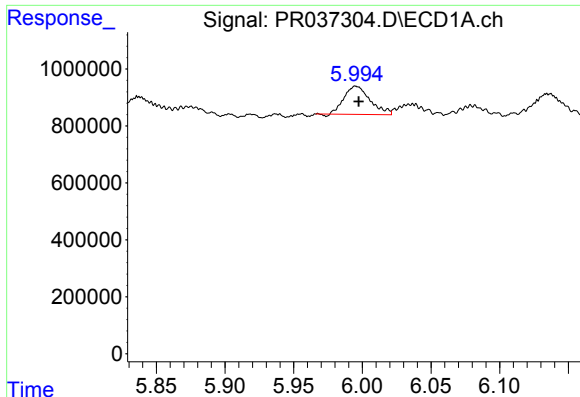

#7 AR-1016-5


R.T.: 5.995 min
Delta R.T.: -0.002 min
Response: 1301173
Conc: 37.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

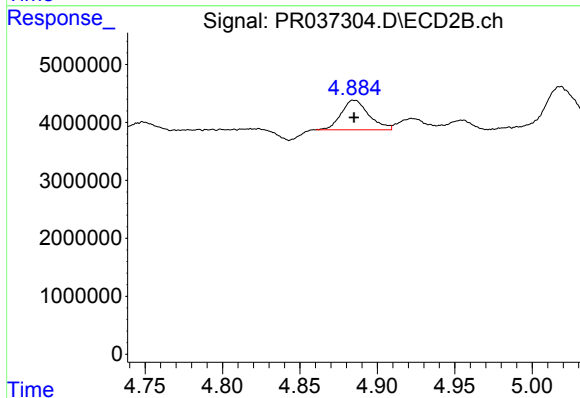


#7 AR-1016-5

R.T.: 4.884 min
Delta R.T.: 0.000 min
Response: 6372597
Conc: 41.92 ng/ml

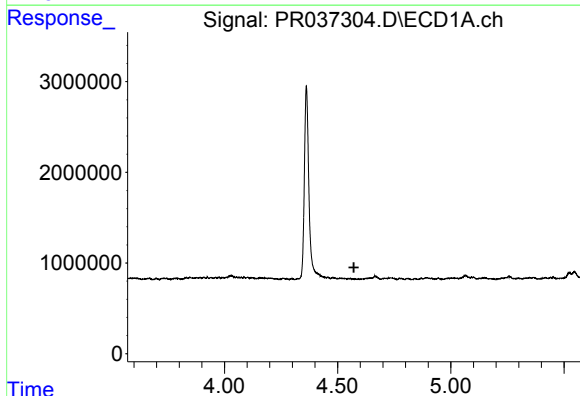


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

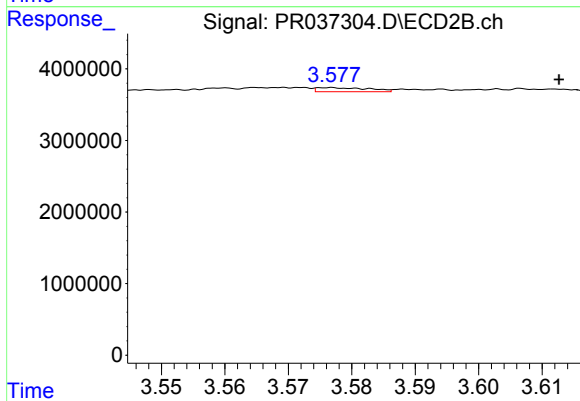

#8 AR-1221-1


R.T.: 3.577 min
Delta R.T.: -0.036 min
Response: 328730
Conc: 6.46 ng/ml

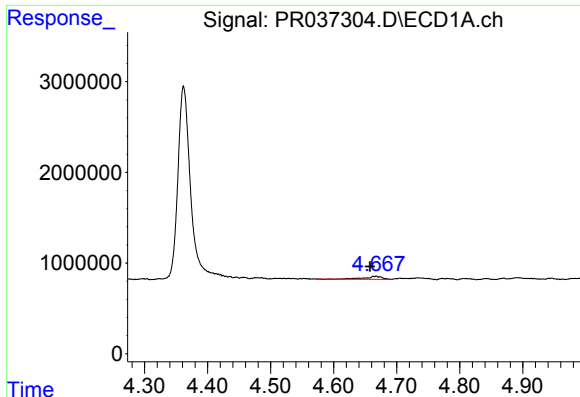

#9 AR-1221-2


R.T.: 4.668 min
Delta R.T.: 0.010 min
Response: 631499
Conc: 69.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

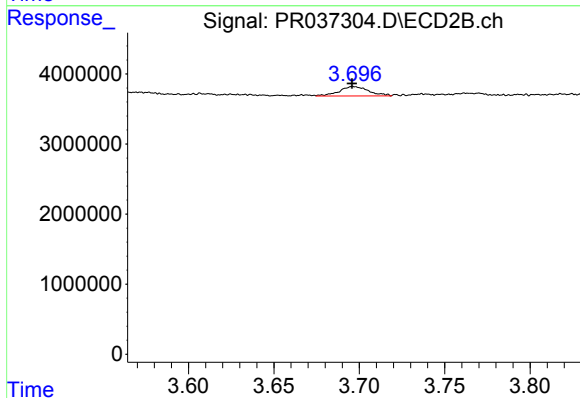


#9 AR-1221-2

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 1627622
Conc: 43.83 ng/ml

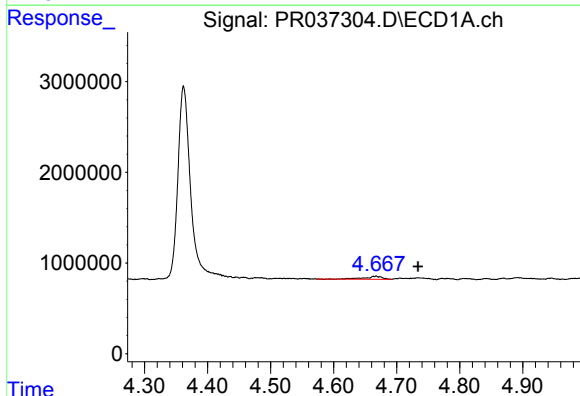


#10 AR-1221-3

R.T.: 4.668 min
Delta R.T.: -0.066 min
Response: 631499
Conc: 20.60 ng/ml

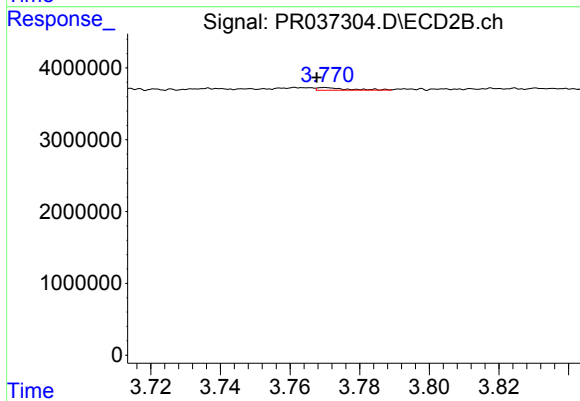

#10 AR-1221-3


R.T.: 3.770 min
Delta R.T.: 0.003 min
Response: 217155
Conc: 1.77 ng/ml

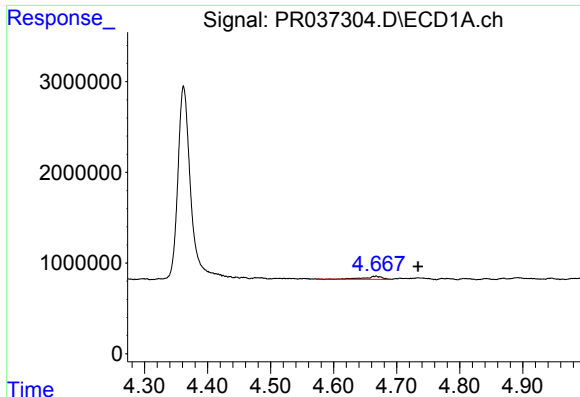

#11 AR-1232-1


R.T.: 4.668 min
Delta R.T.: -0.066 min
Response: 631499
Conc: 21.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

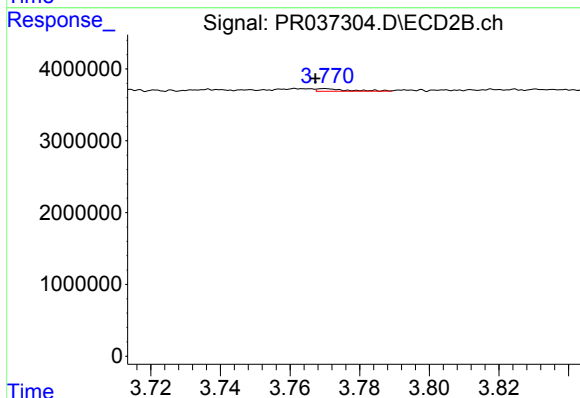


#11 AR-1232-1

R.T.: 3.770 min
Delta R.T.: 0.003 min
Response: 217155
Conc: 1.86 ng/ml

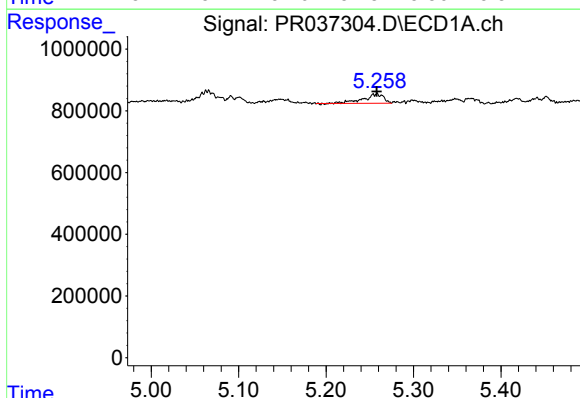


#12 AR-1232-2

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 491081
Conc: 29.06 ng/ml

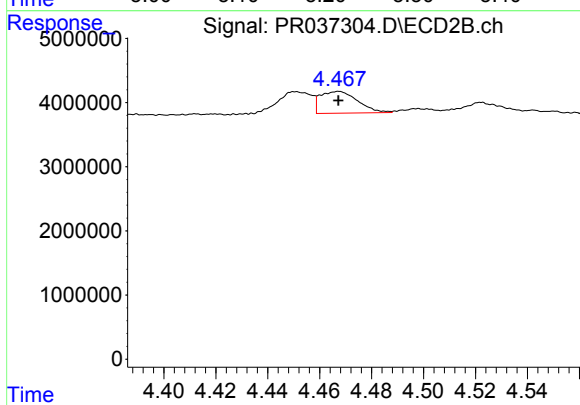

#12 AR-1232-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3430801
Conc: 24.82 ng/ml

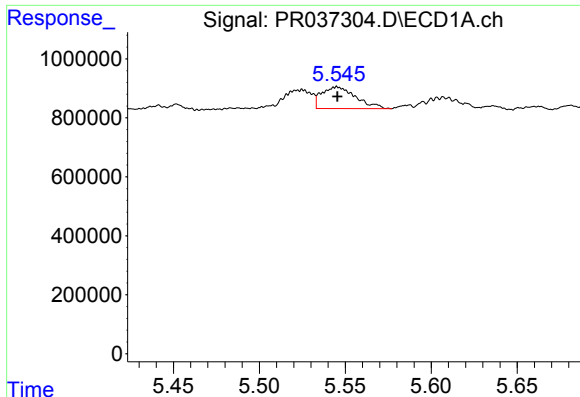

#13 AR-1232-3


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 1014643
Conc: 30.02 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

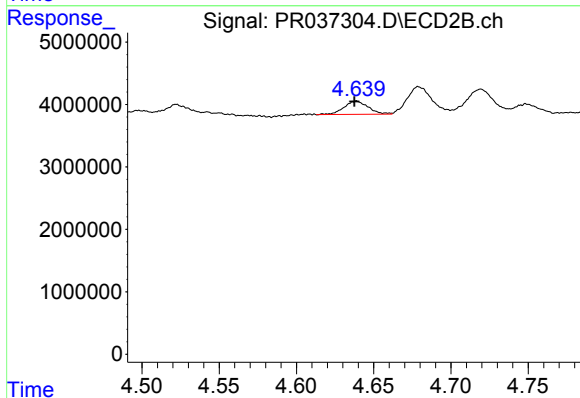


#13 AR-1232-3

R.T.: 4.639 min
Delta R.T.: 0.001 min
Response: 2305936
Conc: 32.85 ng/ml

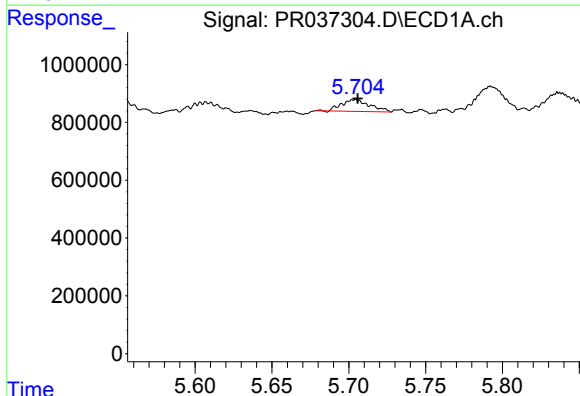


#14 AR-1232-4

R.T.: 5.704 min
Delta R.T.: -0.002 min
Response: 521252
Conc: 33.21 ng/ml

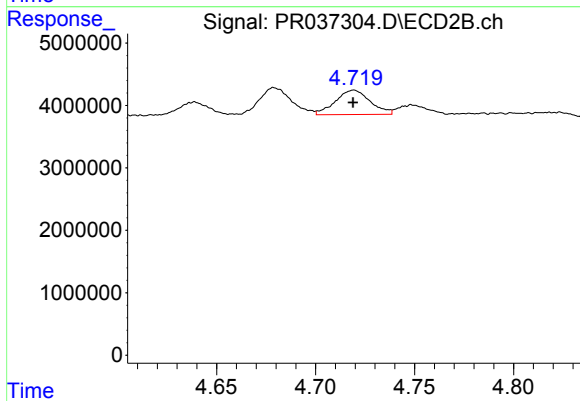

#14 AR-1232-4


R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 4773054
Conc: 79.99 ng/ml

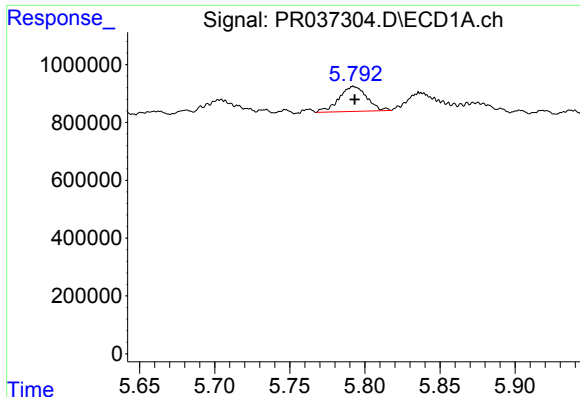

#15 AR-1232-5


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 1114514
Conc: 95.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

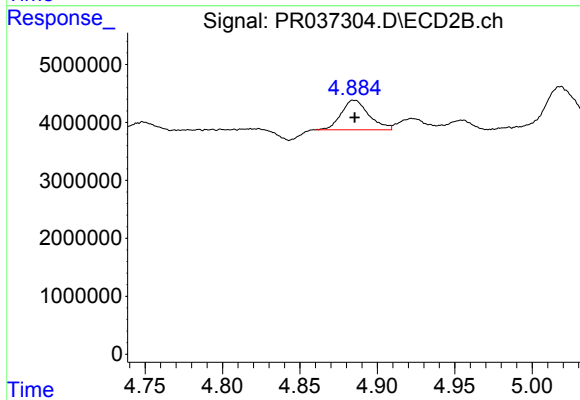


#15 AR-1232-5

R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 6372597
Conc: 93.38 ng/ml

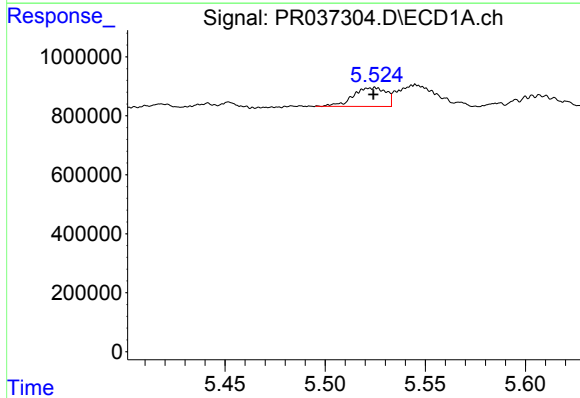


#16 AR-1242-1

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 722355
Conc: 21.11 ng/ml

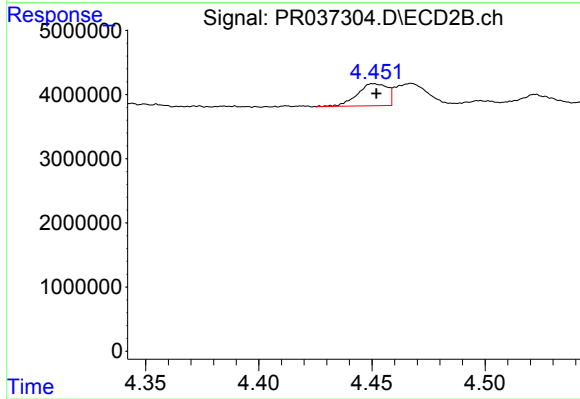

#16 AR-1242-1


R.T.: 4.451 min
Delta R.T.: -0.001 min
Response: 3171873
Conc: 21.65 ng/ml

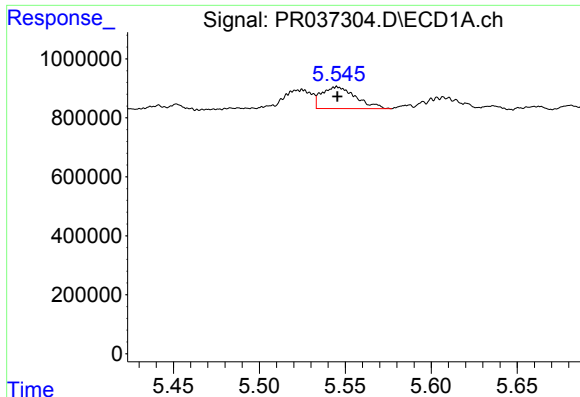

#17 AR-1242-2


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 1014643
Conc: 18.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

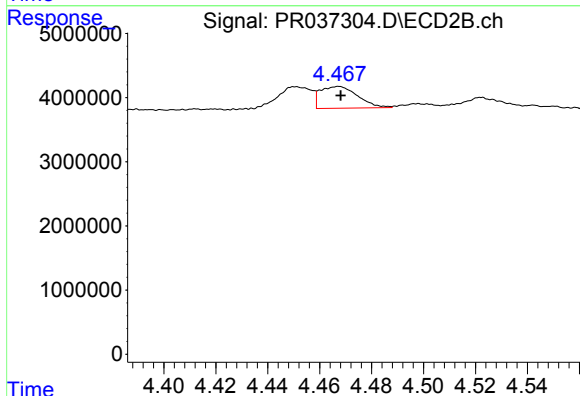


#17 AR-1242-2

R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3430801
Conc: 15.04 ng/ml

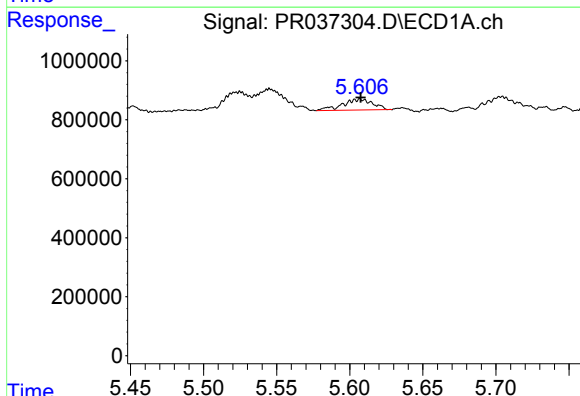


#18 AR-1242-3

R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 532380
Conc: 16.17 ng/ml

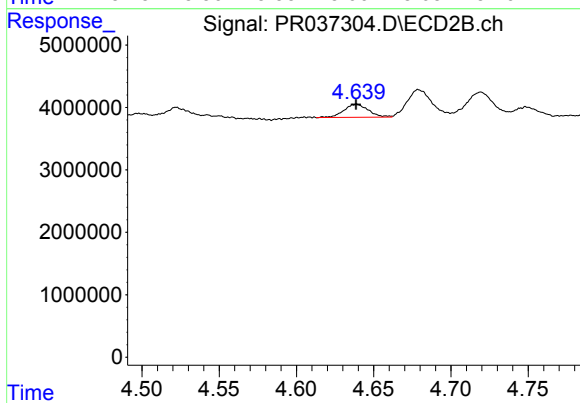

#18 AR-1242-3


R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 2305936
Conc: 19.94 ng/ml

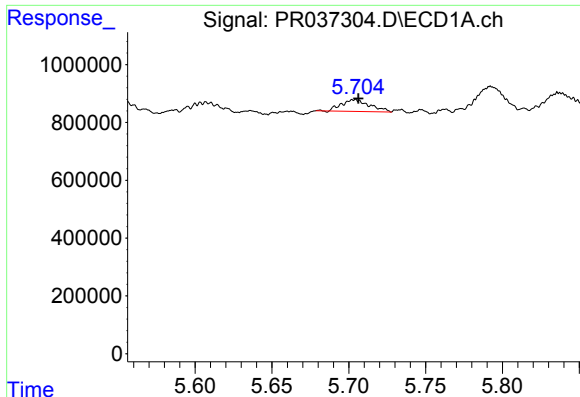

#19 AR-1242-4


R.T.: 5.704 min
Delta R.T.: -0.002 min
Response: 521252
Conc: 19.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

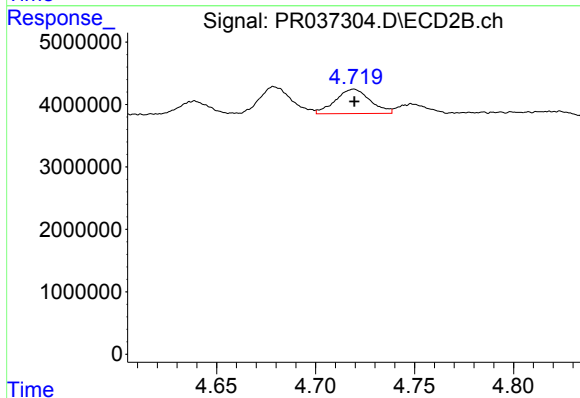


#19 AR-1242-4

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 4773054
Conc: 43.43 ng/ml

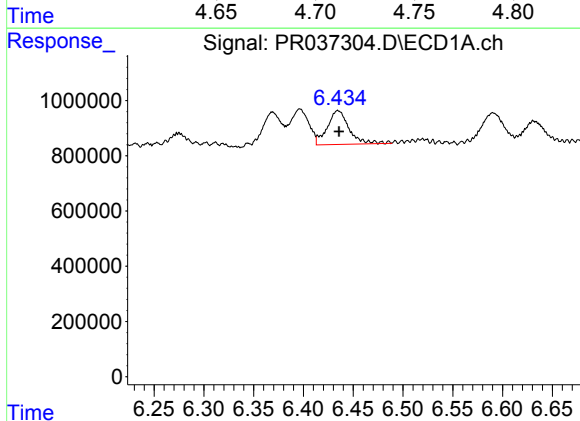


#20 AR-1242-5

R.T.: 6.435 min
Delta R.T.: -0.001 min
Response: 1868514
Conc: 58.07 ng/ml

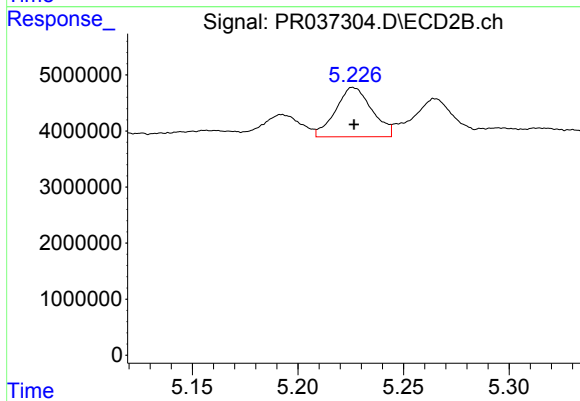

#20 AR-1242-5


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 10538958
Conc: 63.60 ng/ml

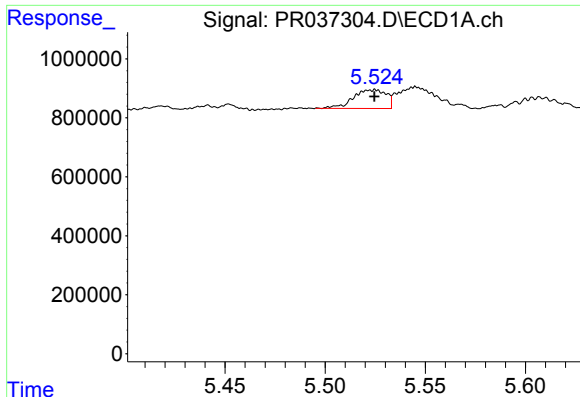

#21 AR-1248-1


R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 722355
Conc: 31.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

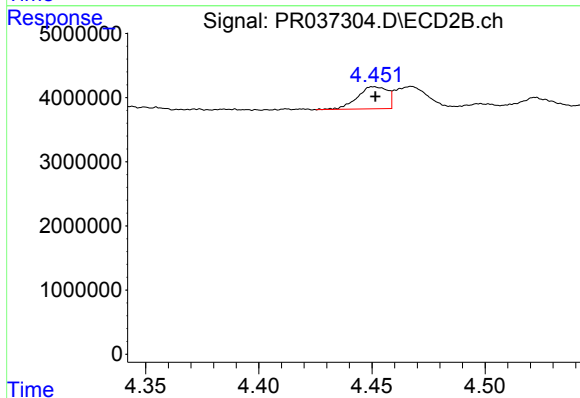


#21 AR-1248-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3171873
Conc: 31.51 ng/ml

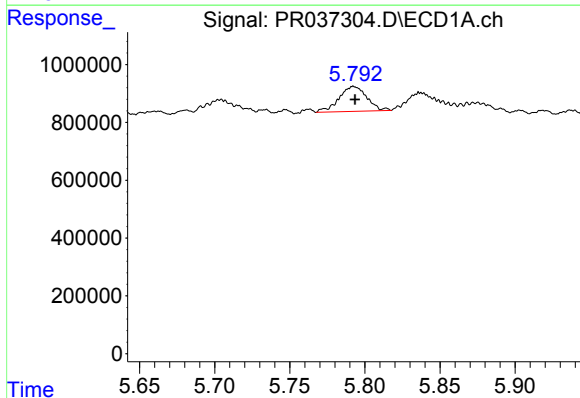


#22 AR-1248-2

R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 1114514
Conc: 31.83 ng/ml

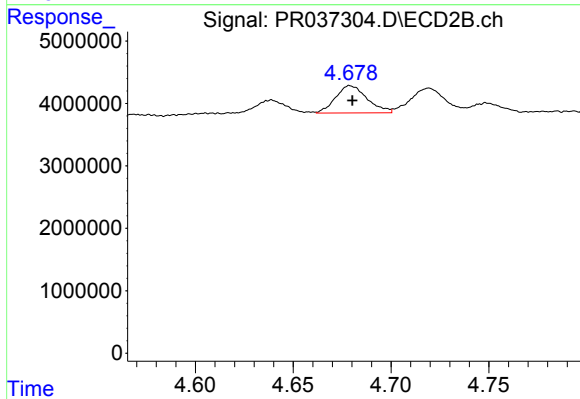

#22 AR-1248-2


R.T.: 4.679 min
Delta R.T.: -0.001 min
Response: 4898160
Conc: 35.89 ng/ml

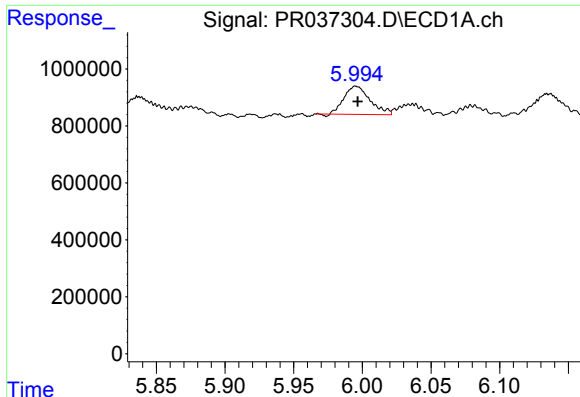

#23 AR-1248-3


R.T.: 5.995 min
Delta R.T.: -0.001 min
Response: 1301173
Conc: 31.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

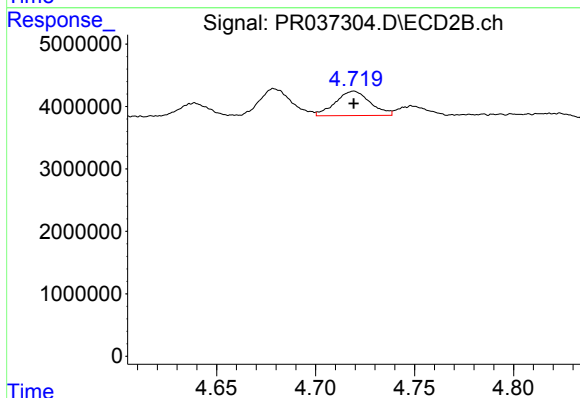


#23 AR-1248-3

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 4773054
Conc: 34.10 ng/ml

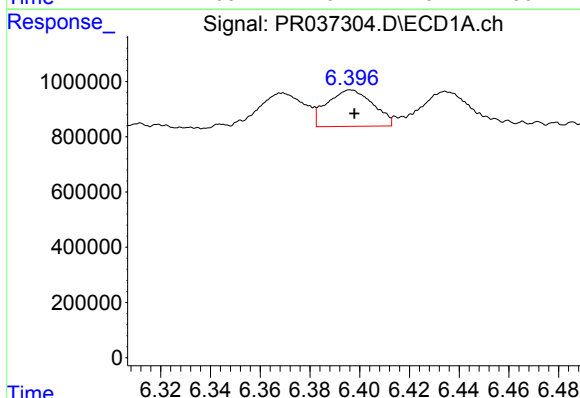


#24 AR-1248-4

R.T.: 6.396 min
Delta R.T.: -0.002 min
Response: 1688557
Conc: 34.49 ng/ml

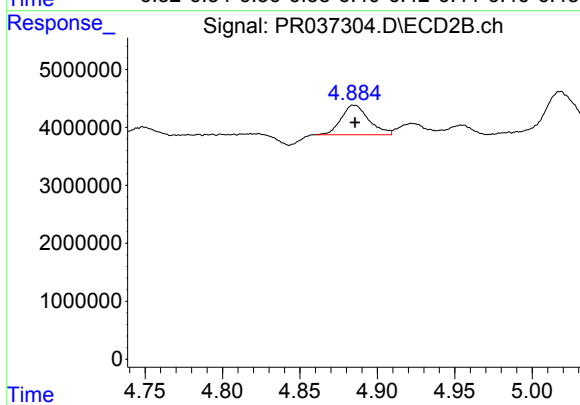

#24 AR-1248-4


R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 6372597
Conc: 35.81 ng/ml

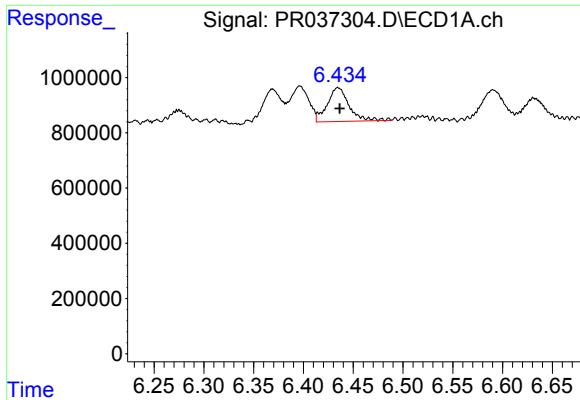

#25 AR-1248-5


R.T.: 6.435 min
Delta R.T.: -0.002 min
Response: 1868514
Conc: 39.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

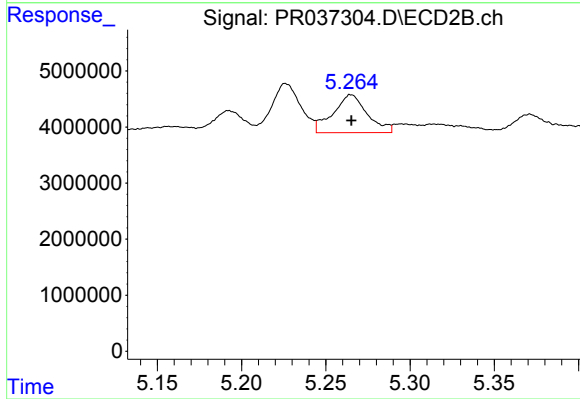


#25 AR-1248-5

R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 9566417
Conc: 48.91 ng/ml

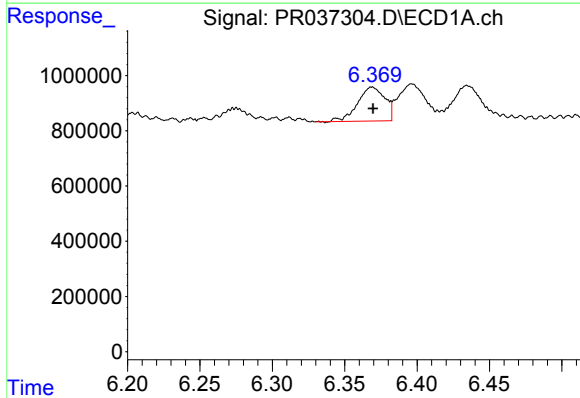


#26 AR-1254-1

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 1606110
Conc: 29.40 ng/ml

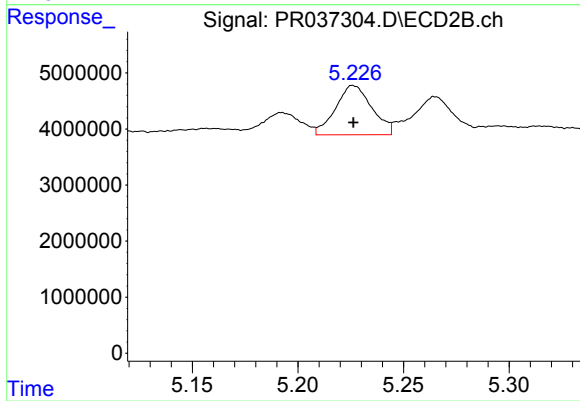

#26 AR-1254-1


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 10538958
Conc: 30.59 ng/ml

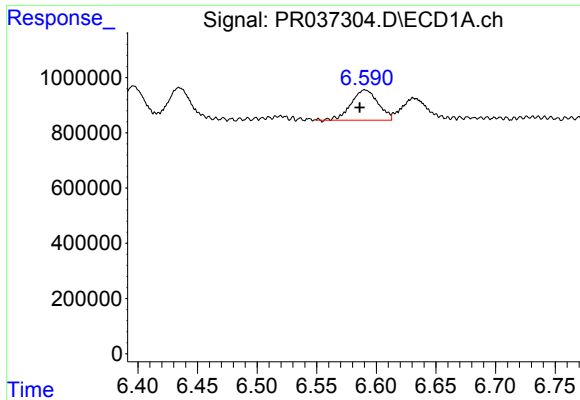

#27 AR-1254-2


R.T.: 6.590 min
Delta R.T.: 0.004 min
Response: 1727698
Conc: 20.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

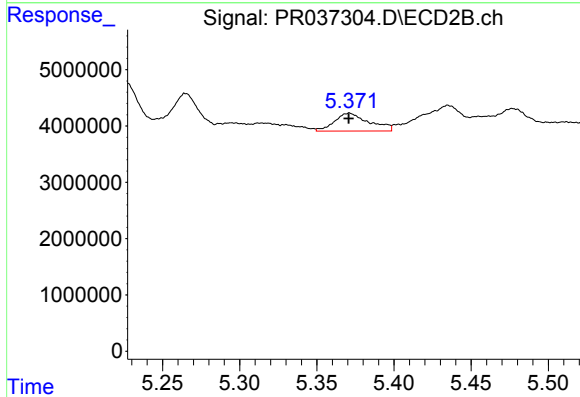


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 4989459
Conc: 16.66 ng/ml

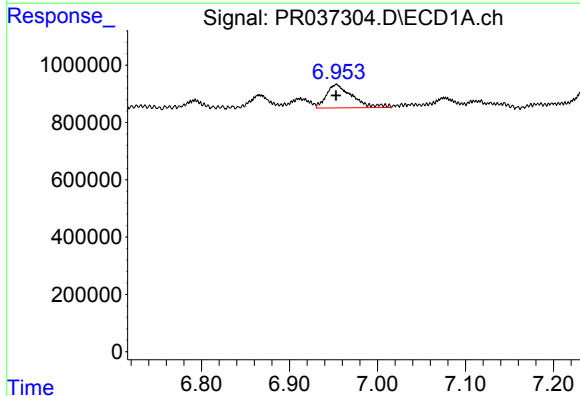


#28 AR-1254-3

R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 1663435
Conc: 18.29 ng/ml

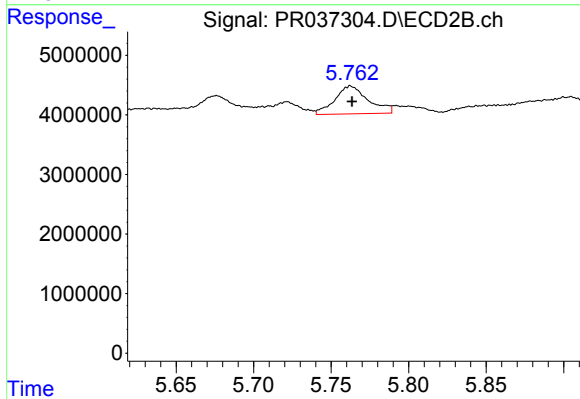

#28 AR-1254-3


R.T.: 5.762 min
Delta R.T.: -0.001 min
Response: 7043747
Conc: 14.87 ng/ml

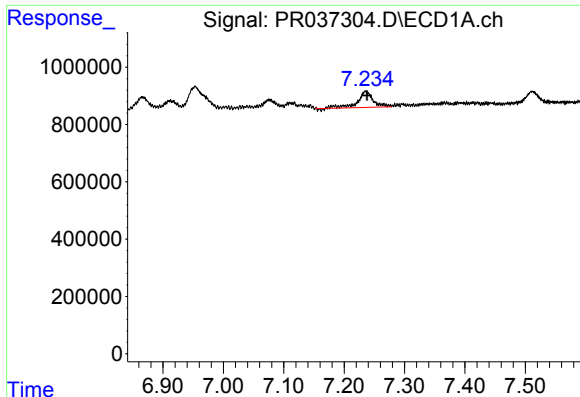

#29 AR-1254-4


R.T.: 7.235 min
Delta R.T.: -0.002 min
Response: 996326
Conc: 14.87 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

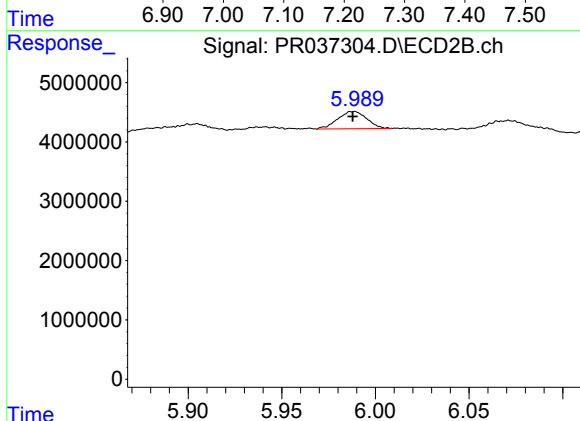


#29 AR-1254-4

R.T.: 5.989 min
Delta R.T.: 0.001 min
Response: 3140016
Conc: 8.95 ng/ml

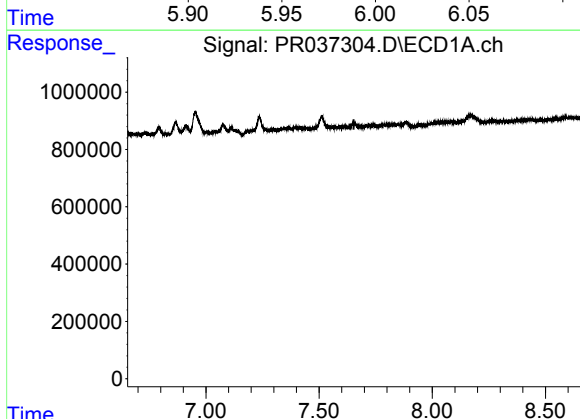


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

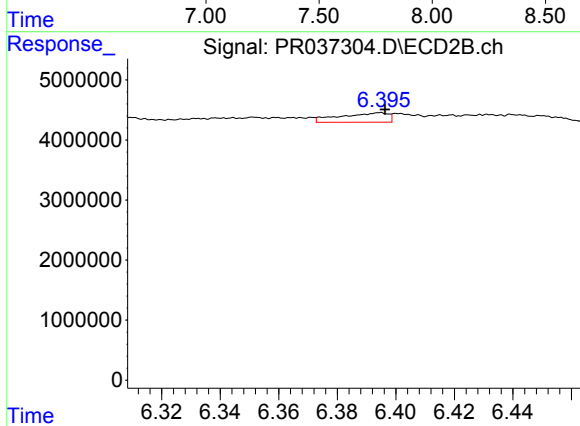

#30 AR-1254-5


R.T.: 6.395 min
Delta R.T.: -0.002 min
Response: 1781284
Conc: 4.02 ng/ml

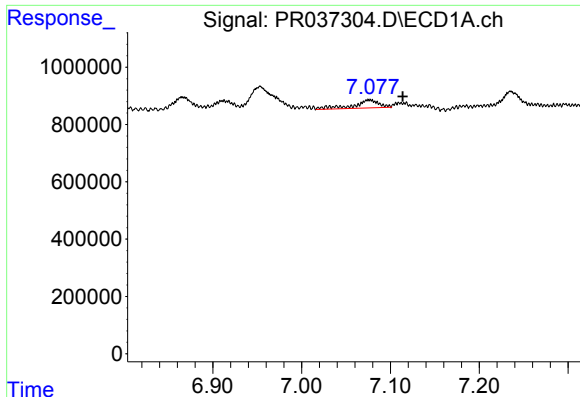

#31 AR-1260-1


R.T.: 7.077 min
Delta R.T.: -0.037 min
Response: 556239
Conc: 8.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

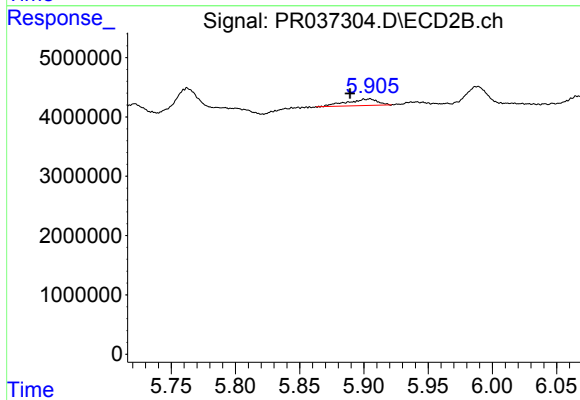


#31 AR-1260-1

R.T.: 5.905 min
Delta R.T.: 0.016 min
Response: 1831784
Conc: 6.27 ng/ml

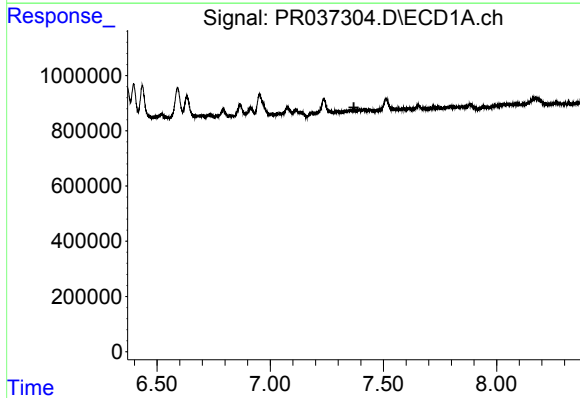


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

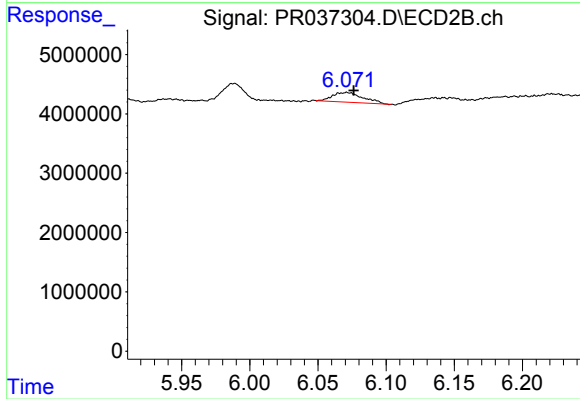

#32 AR-1260-2


R.T.: 6.071 min
Delta R.T.: -0.005 min
Response: 2467440
Conc: 5.36 ng/ml

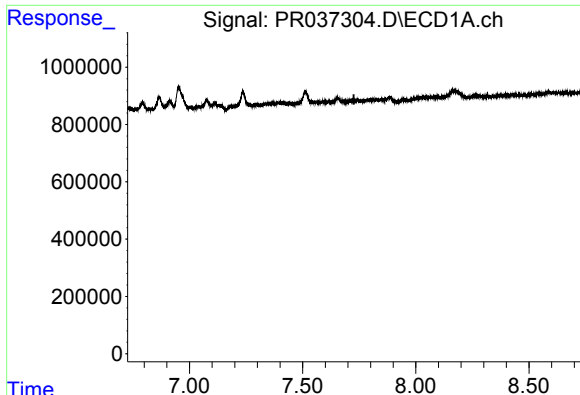

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

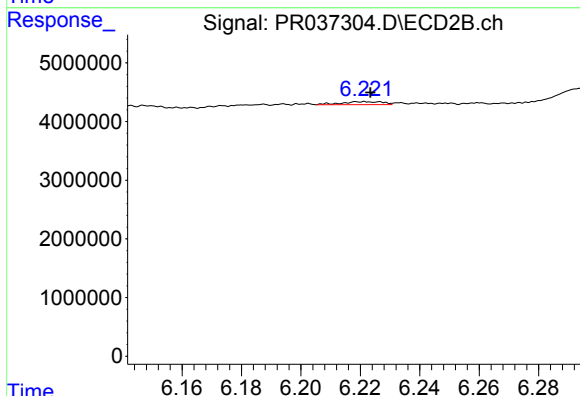


#33 AR-1260-3

R.T.: 6.219 min
Delta R.T.: -0.005 min
Response: 492114
Conc: 1.38 ng/ml

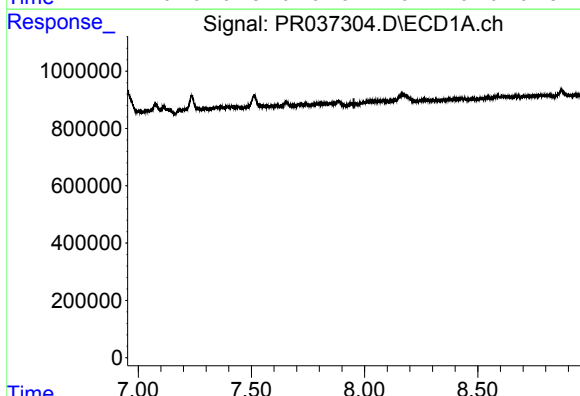


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

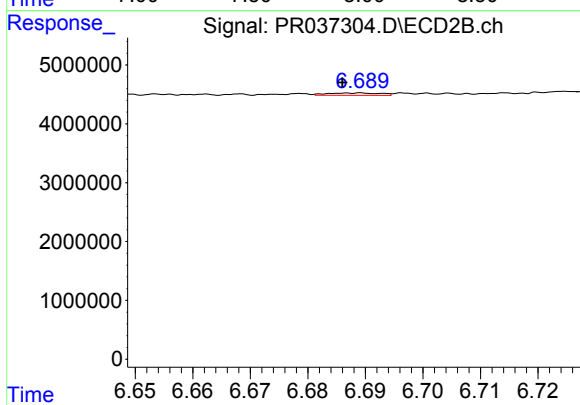

#34 AR-1260-4


R.T.: 6.689 min
Delta R.T.: 0.003 min
Response: 255799
Conc: 0.84 ng/ml

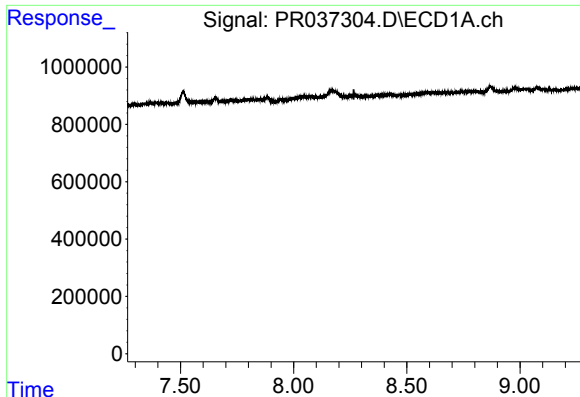

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

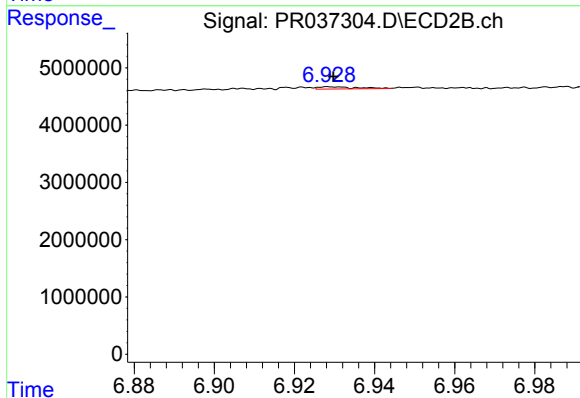


#35 AR-1260-5

R.T.: 6.929 min
Delta R.T.: -0.001 min
Response: 259151
Conc: 0.30 ng/ml

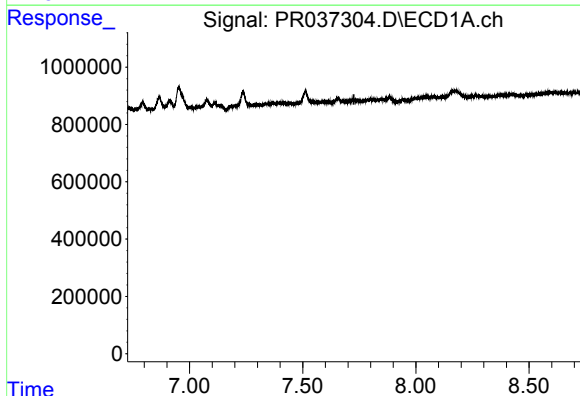


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

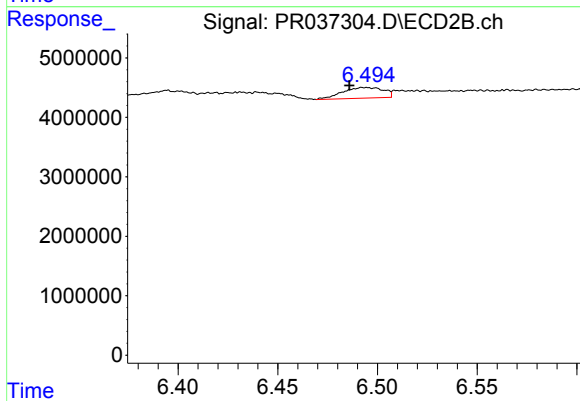

#36 AR-1262-1


R.T.: 6.492 min
Delta R.T.: 0.006 min
Response: 2538272
Conc: 10.13 ng/ml

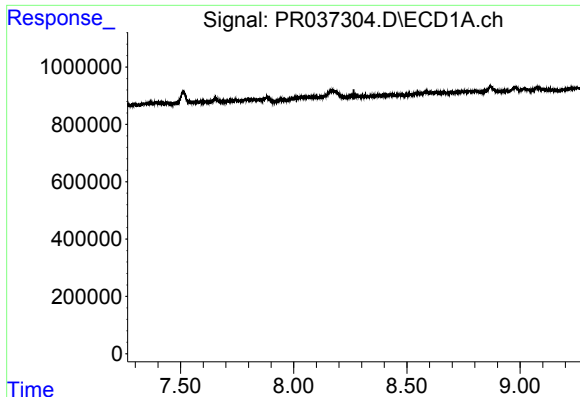

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

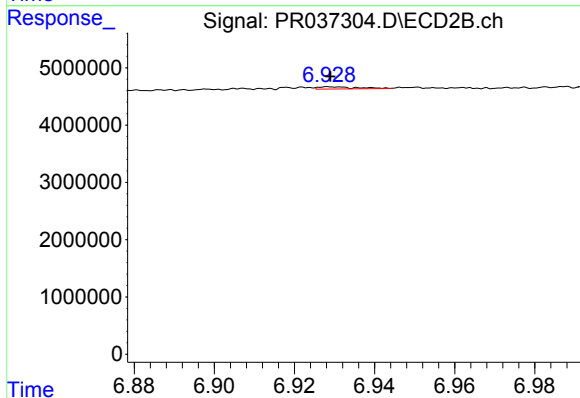


#37 AR-1262-2

R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 259151
Conc: 0.21 ng/ml

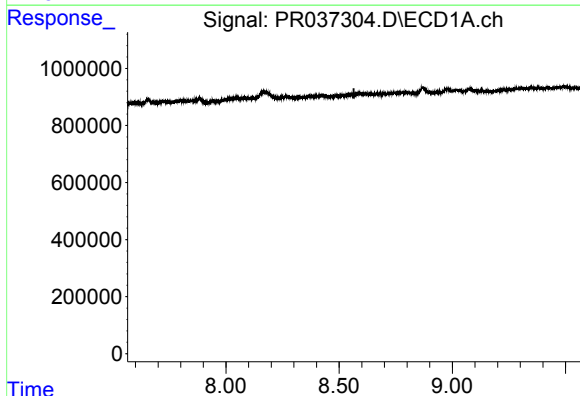


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

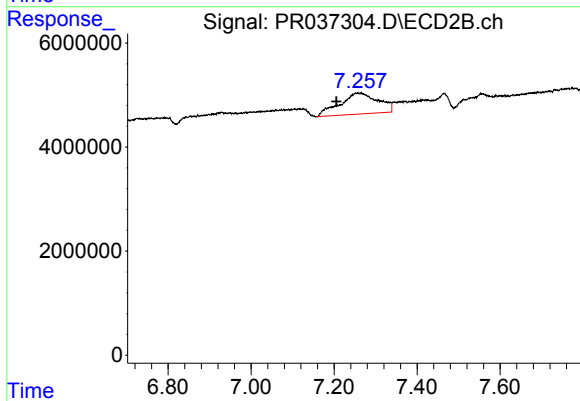

#38 AR-1262-3


R.T.: 7.258 min
Delta R.T.: 0.052 min
Response: 26038708
Conc: 47.49 ng/ml

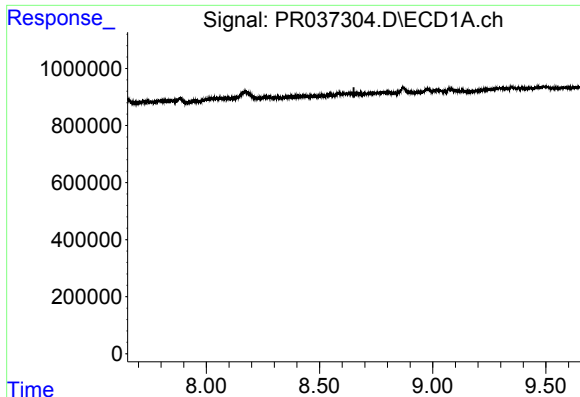

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

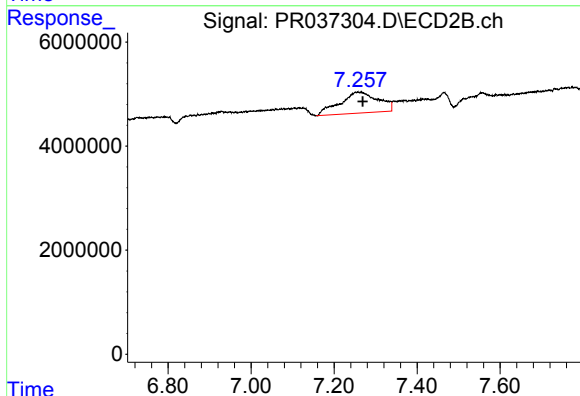


#39 AR-1262-4

R.T.: 7.258 min
Delta R.T.: -0.012 min
Response: 26038708
Conc: 29.01 ng/ml

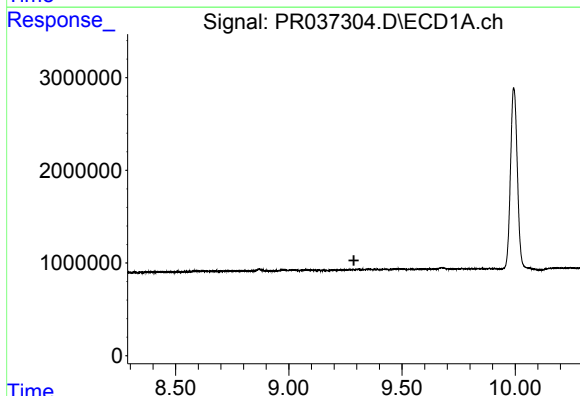


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

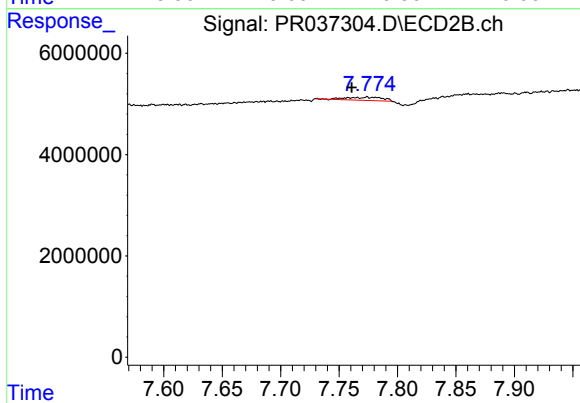

#40 AR-1262-5


R.T.: 7.774 min
Delta R.T.: 0.013 min
Response: 1331763
Conc: 3.48 ng/ml

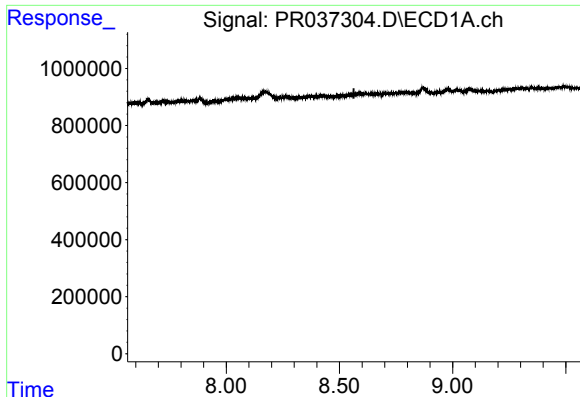

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

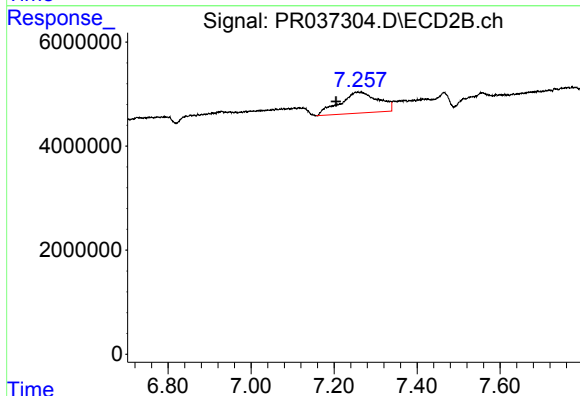


#41 AR-1268-1

R.T.: 7.258 min
Delta R.T.: 0.053 min
Response: 26038708
Conc: 21.15 ng/ml

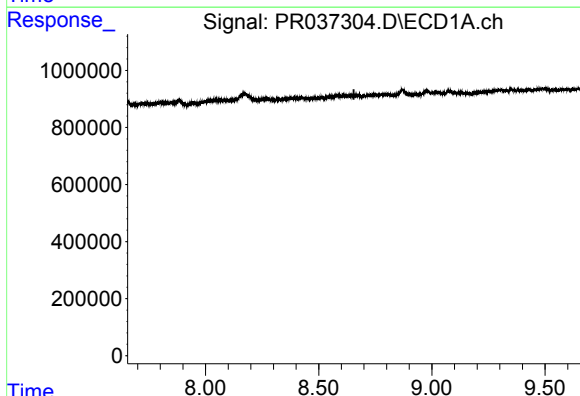


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

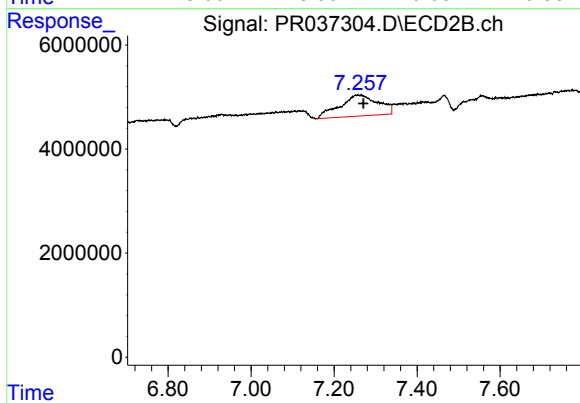

#42 AR-1268-2


R.T.: 7.258 min
Delta R.T.: -0.013 min
Response: 26038708
Conc: 24.59 ng/ml

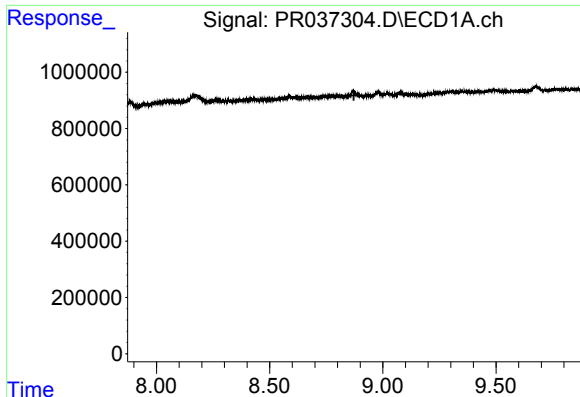

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

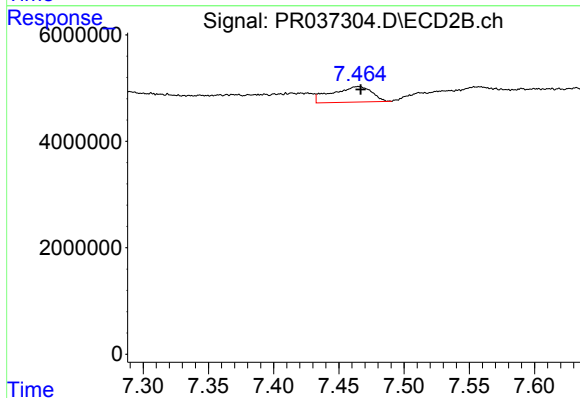


#43 AR-1268-3

R.T.: 7.465 min
Delta R.T.: -0.002 min
Response: 6221455
Conc: 7.02 ng/ml

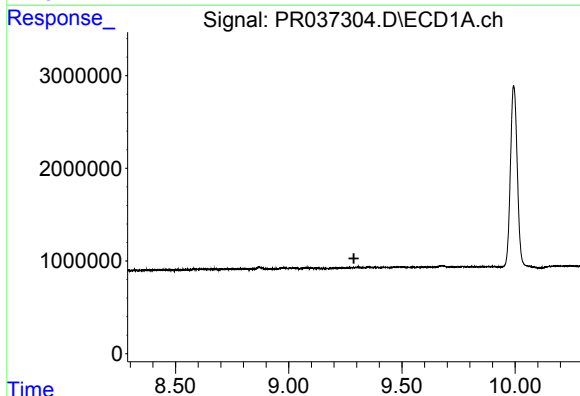


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

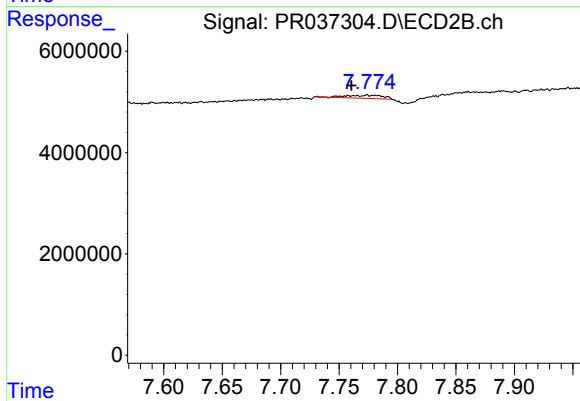

#44 AR-1268-4


R.T.: 7.774 min
Delta R.T.: 0.013 min
Response: 1331763
Conc: 3.67 ng/ml

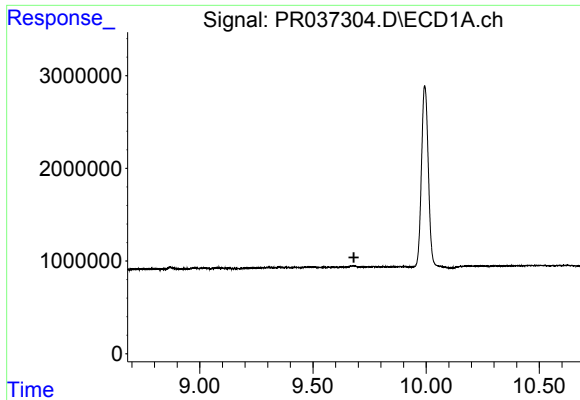

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

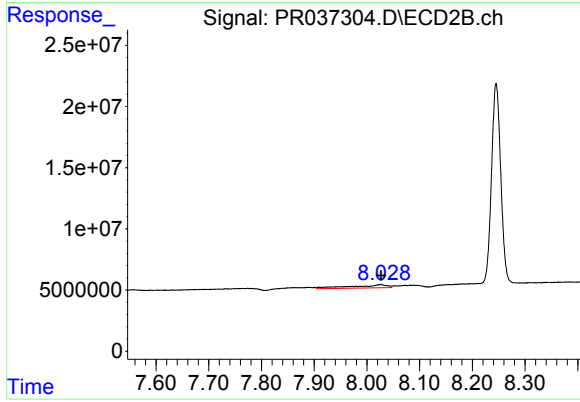

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.002 min
Response: 12506456
Conc: 4.92 ng/ml