

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 20:53
 Operator : SM\SJ
 Sample : K1560-14
 Misc : AR1254 MDL 25PPB
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:54:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.362	3.408	32482493	128.3E6	25.965	26.750
2)	SA Decachlor...	9.993	8.245	39999177	198.2E6	30.243	34.038
Target Compounds							
3)	L1 AR-1016-1	0.000	4.459	0	927952	N.D.	5.096 #
4)	L1 AR-1016-2	0.000	4.459	0	927952	N.D.	3.289 #
5)	L1 AR-1016-3	0.000	4.638	0	256523	N.D.	1.784 #
6)	L1 AR-1016-4	0.000	4.680	0	4255490	N.D.	38.464 #
7)	L1 AR-1016-5	5.995	4.885	677638	4494841	19.762	29.570 #
8)	L2 AR-1221-1	0.000	3.606	0	157866	N.D.	3.100 #
9)	L2 AR-1221-2	4.670	3.696	460771	1905288	50.948	51.306
10)	L2 AR-1221-3	4.670	3.752	460771	316377	15.034	2.584 #
11)	L3 AR-1232-1	4.670	3.752	460771	316377	15.752	2.704 #
12)	L3 AR-1232-2	0.000	4.459	0	927952	N.D.	6.713 #
13)	L3 AR-1232-3	0.000	4.638	0	256523	N.D.	3.654 #
14)	L3 AR-1232-4	0.000	4.718	0	1377331	N.D.	23.082 #
15)	L3 AR-1232-5	5.792	4.885	1136229	4494841	97.150	65.864 #
16)	L4 AR-1242-1	0.000	4.459	0	927952	N.D.	6.333 #
17)	L4 AR-1242-2	0.000	4.459	0	927952	N.D.	4.067 #
18)	L4 AR-1242-3	0.000	4.638	0	256523	N.D.	2.218 #
19)	L4 AR-1242-4	0.000	4.718	0	1377331	N.D.	12.531 #
20)	L4 AR-1242-5	6.438	5.226	922983	20758925	28.683	125.281 #
21)	L5 AR-1248-1	0.000	4.459	0	927952	N.D.	9.218 #
22)	L5 AR-1248-2	5.792	4.680	1136229	4255490	32.450	31.182
23)	L5 AR-1248-3	5.995	4.718	677638	1377331	16.564	9.840 #
24)	L5 AR-1248-4	6.396	4.885	1273126	4494841	26.006	25.257
25)	L5 AR-1248-5	6.438	5.297	922983	2173751	19.539	11.113 #
26)	L6 AR-1254-1	6.370	5.226	2994874	20758925	54.820	60.263
27)	L6 AR-1254-2	6.585	5.371	3409979	13470014	39.791	44.975
28)	L6 AR-1254-3	6.952	5.763	3661471	17723055	40.252	37.420
29)	L6 AR-1254-4	7.236	5.988	2521979	12077002	37.637	34.442
30)	L6 AR-1254-5	7.653	6.395	2904721	24527418	40.410	55.388 #
31)	L7 AR-1260-1	7.112	5.889	1419703	7251590	21.515	24.811
32)	L7 AR-1260-2	7.367	6.074	1645294	11382015	20.643	24.712
33)	L7 AR-1260-3	0.000	6.222	0	6641917	N.D.	18.631 #
34)	L7 AR-1260-4	7.943	6.684	1119749	1723908	15.050	5.657 #
35)	L7 AR-1260-5	8.265	6.928	699919	2439301	4.840	2.813 #
36)	L8 AR-1262-1	0.000	6.491	0	4797128	N.D.	19.141 #
37)	L8 AR-1262-2	8.265	6.928	699919	2439301	3.601	1.942 #
38)	L8 AR-1262-3	8.586	7.265	564057	35041508	4.289	63.913 #
39)	L8 AR-1262-4	8.586	7.265	564057	35041508	5.742	39.037 #
40)	L8 AR-1262-5	0.000	7.759	0	826417	N.D.	2.160 #
41)	L9 AR-1268-1	8.586	7.265	564057	35041508	3.150	28.465 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 20:53
 Operator : SM\SJ
 Sample : K1560-14
 Misc : AR1254 MDL 25PPB
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:54:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.586	7.265	564057	35041508	3.429	33.092 #
43) L9	AR-1268-3	0.000	7.465	0	9170946	N.D.	10.348 #
44) L9	AR-1268-4	0.000	7.759	0	826417	N.D.	2.278 #
45) L9	AR-1268-5	0.000	8.027	0	12435958	N.D.	4.888 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
Data File : PR037305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 20:53
Operator : SM\SJ
Sample : K1560-14
Misc : AR1254 MDL 25PPB
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:54:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

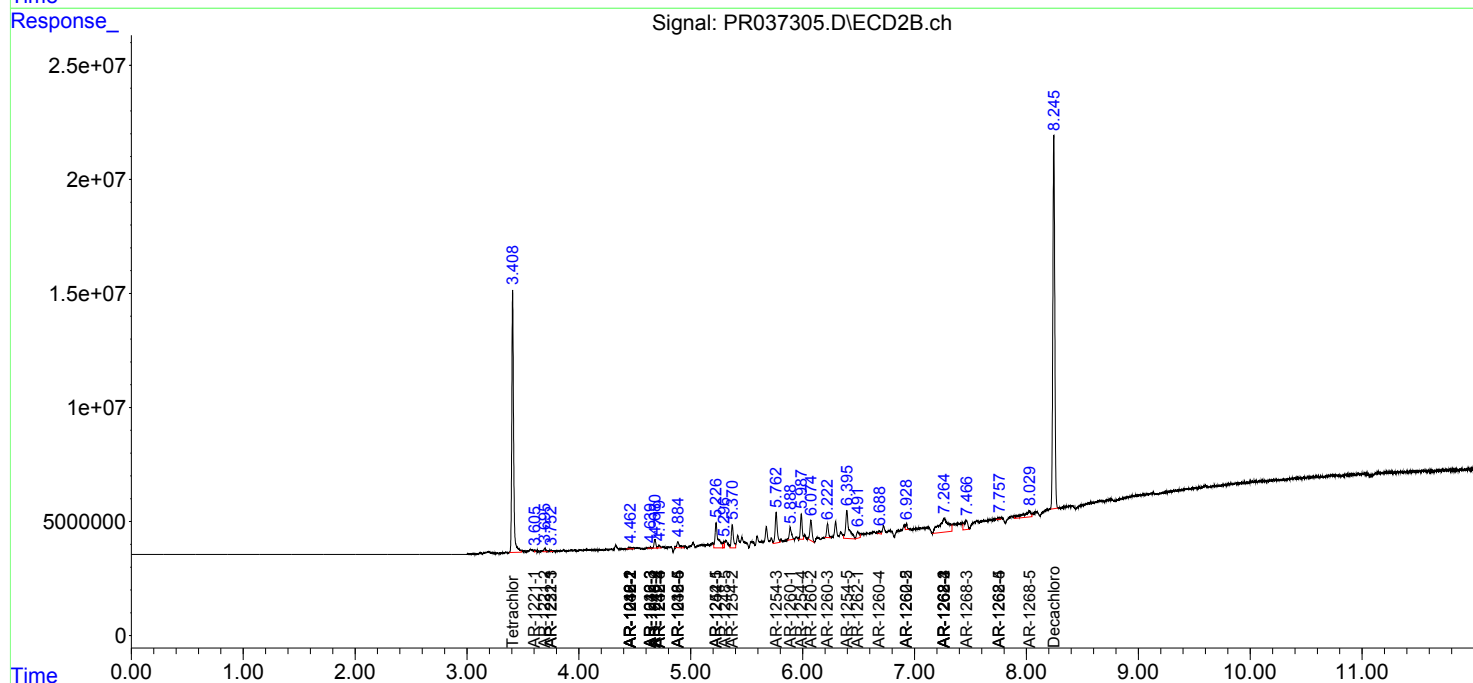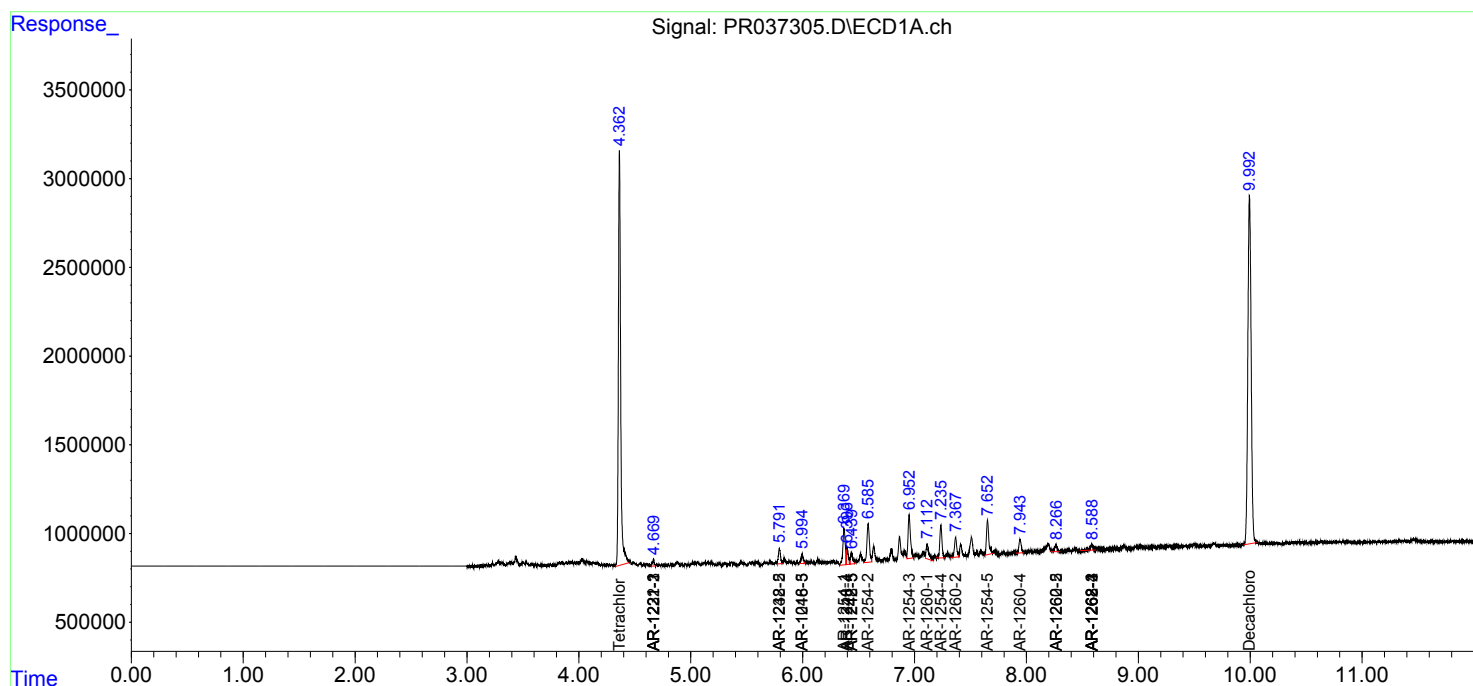


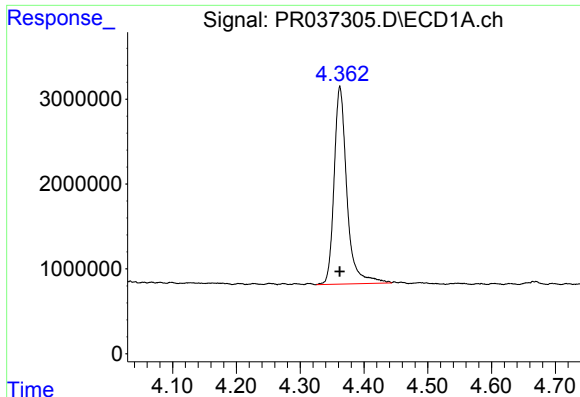

#1 Tetrachloro-m-xylene


R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 32482493
Conc: 25.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

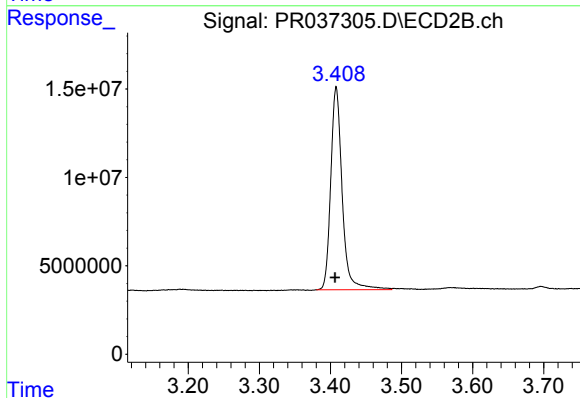


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: 0.002 min
Response: 128279966
Conc: 26.75 ng/ml

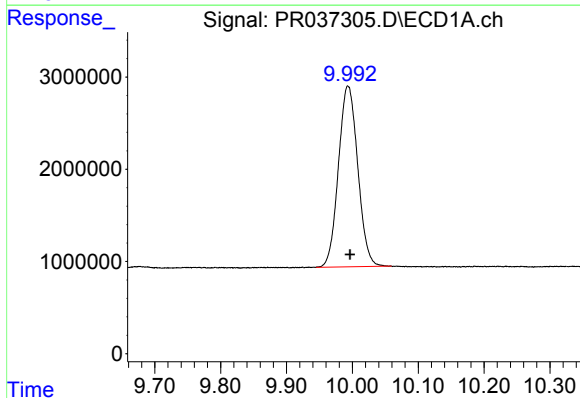


#2 Decachlorobiphenyl

R.T.: 9.993 min
Delta R.T.: -0.003 min
Response: 39999177
Conc: 30.24 ng/ml

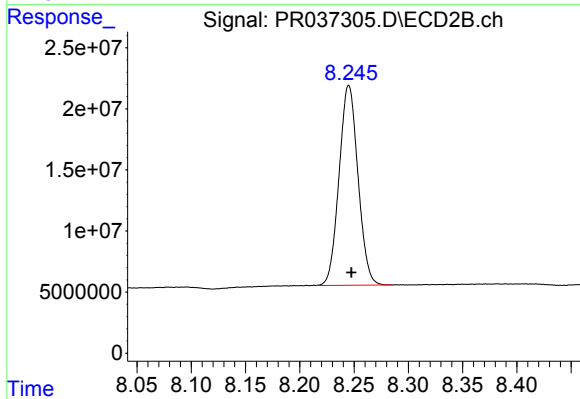

#2 Decachlorobiphenyl


R.T.: 8.245 min
Delta R.T.: -0.002 min
Response: 198245555
Conc: 34.04 ng/ml

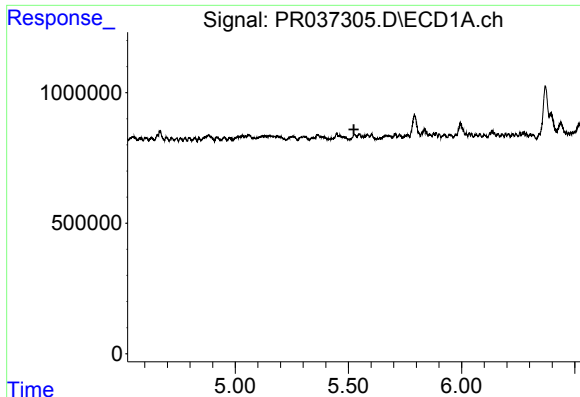

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

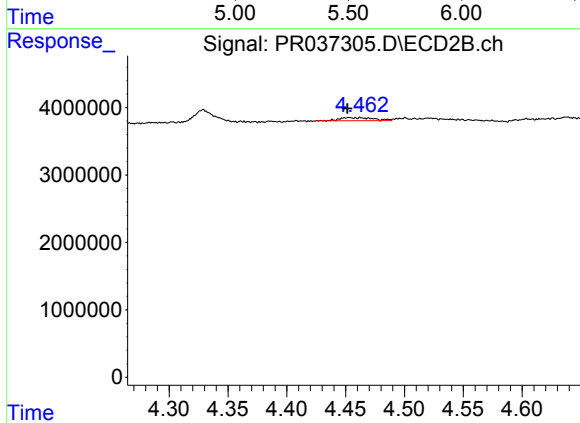


#3 AR-1016-1

R.T.: 4.459 min
Delta R.T.: 0.007 min
Response: 927952
Conc: 5.10 ng/ml

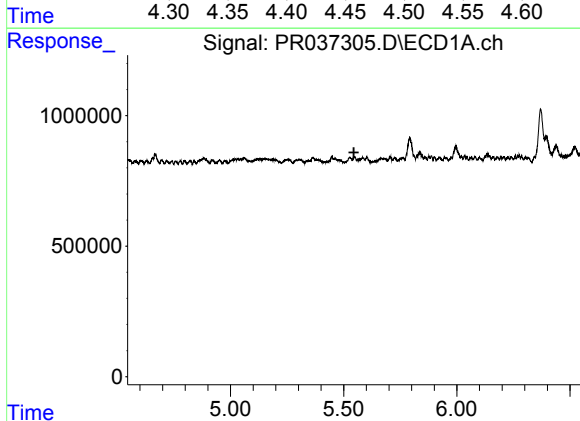


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

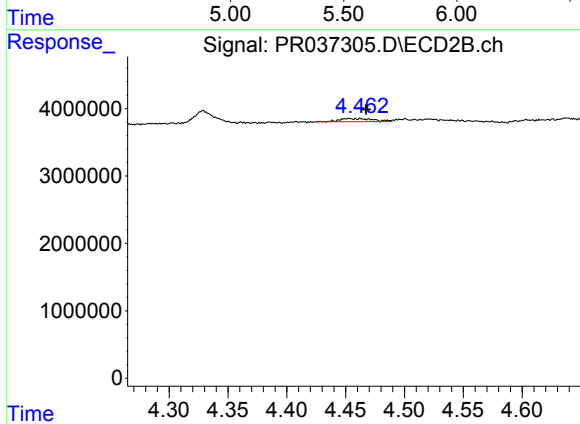

#4 AR-1016-2


R.T.: 4.459 min
Delta R.T.: -0.009 min
Response: 927952
Conc: 3.29 ng/ml

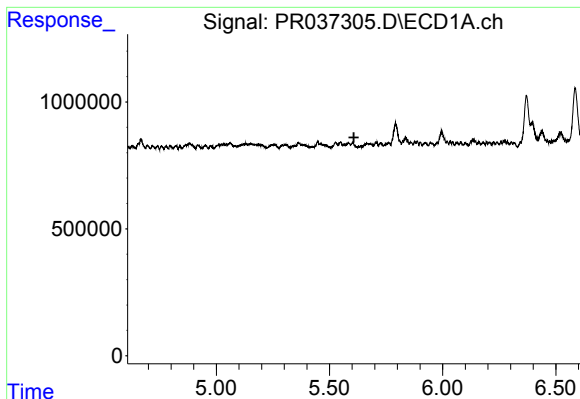

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

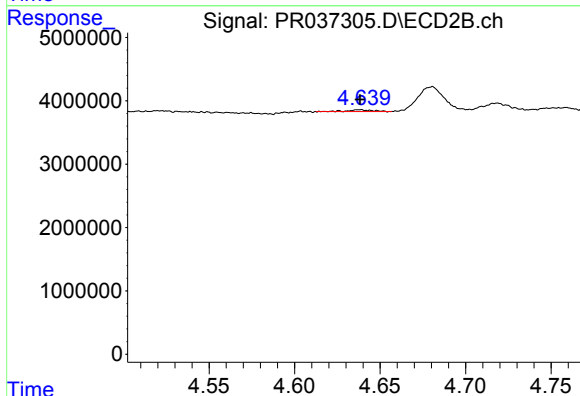


#5 AR-1016-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 256523
Conc: 1.78 ng/ml

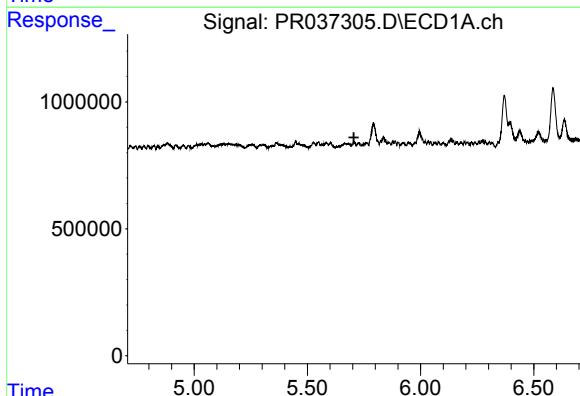


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

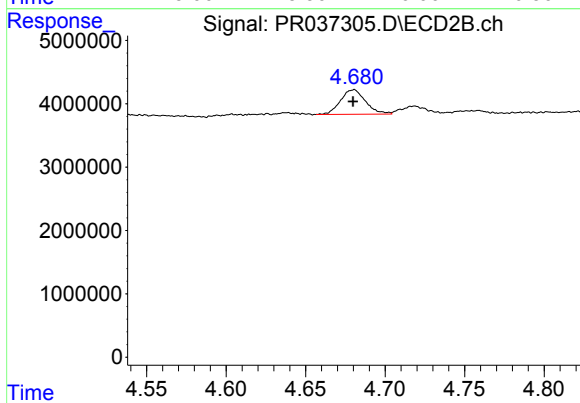

#6 AR-1016-4


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 4255490
Conc: 38.46 ng/ml

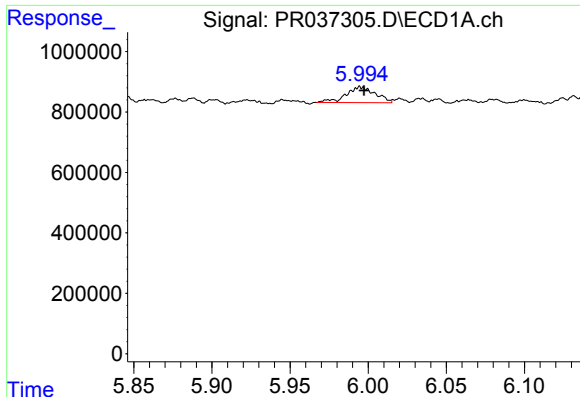

#7 AR-1016-5


R.T.: 5.995 min
Delta R.T.: -0.002 min
Response: 677638
Conc: 19.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

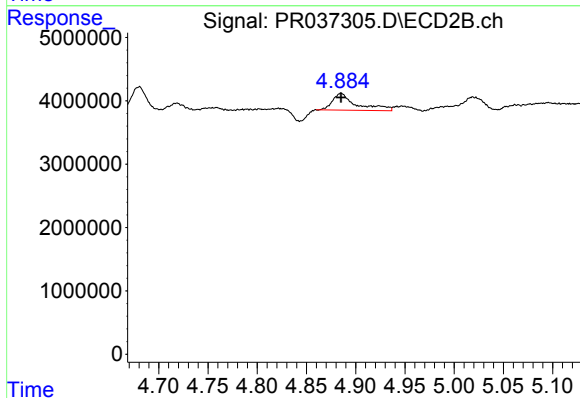


#7 AR-1016-5

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 4494841
Conc: 29.57 ng/ml

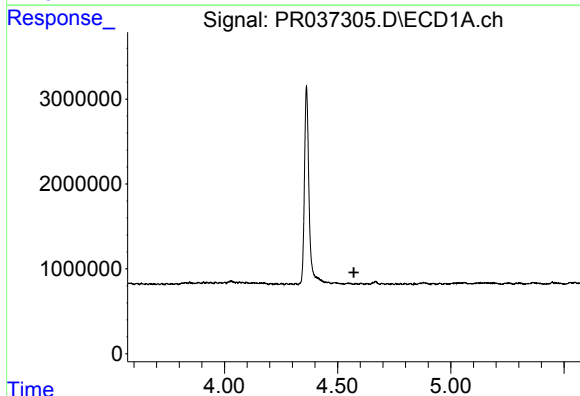


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

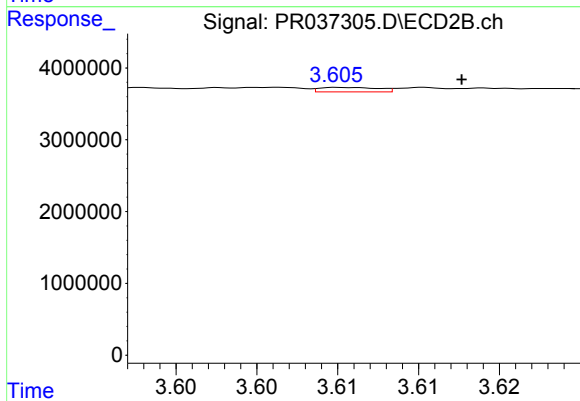

#8 AR-1221-1


R.T.: 3.606 min
Delta R.T.: -0.007 min
Response: 157866
Conc: 3.10 ng/ml

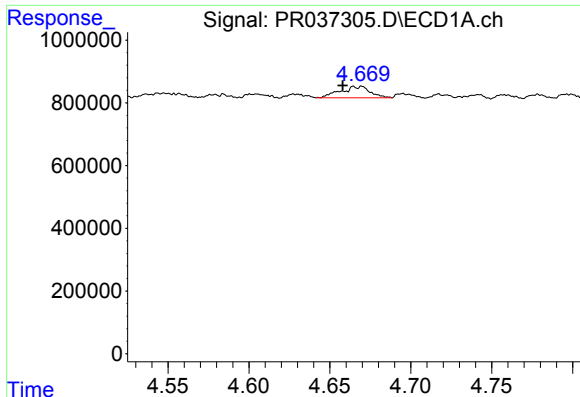

#9 AR-1221-2


R.T.: 4.670 min
Delta R.T.: 0.012 min
Response: 460771
Conc: 50.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

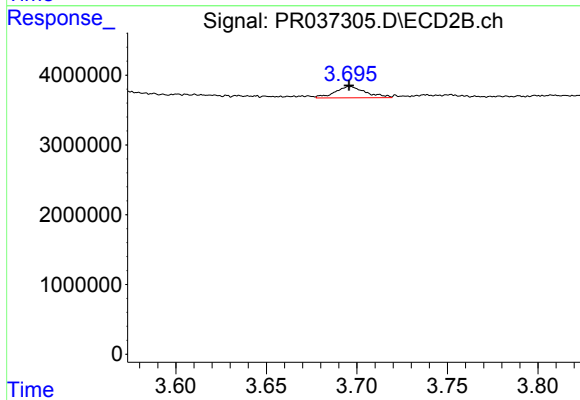


#9 AR-1221-2

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 1905288
Conc: 51.31 ng/ml

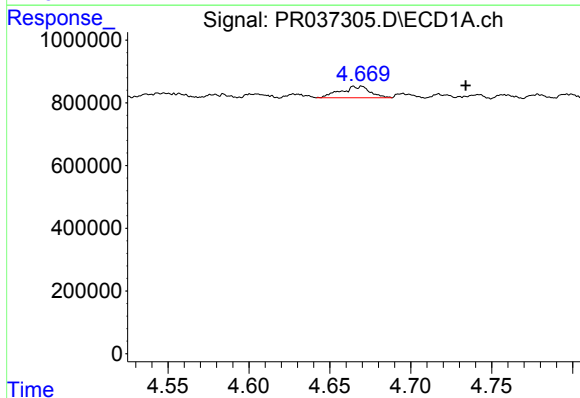


#10 AR-1221-3

R.T.: 4.670 min
Delta R.T.: -0.064 min
Response: 460771
Conc: 15.03 ng/ml

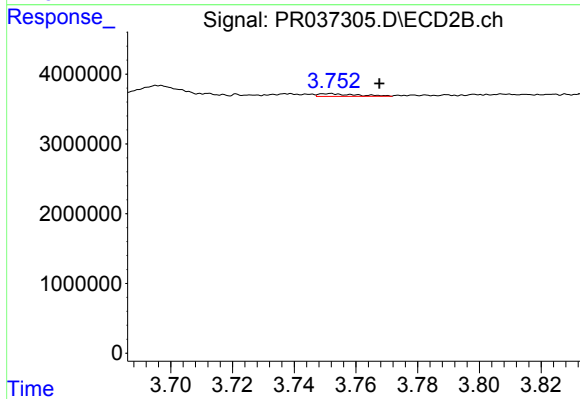

#10 AR-1221-3


R.T.: 3.752 min
Delta R.T.: -0.016 min
Response: 316377
Conc: 2.58 ng/ml

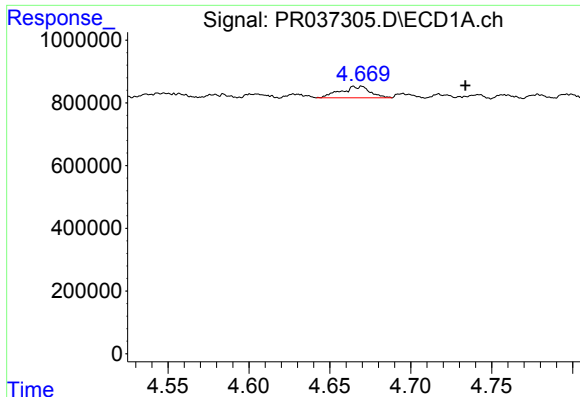

#11 AR-1232-1


R.T.: 4.670 min
Delta R.T.: -0.064 min
Response: 460771
Conc: 15.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

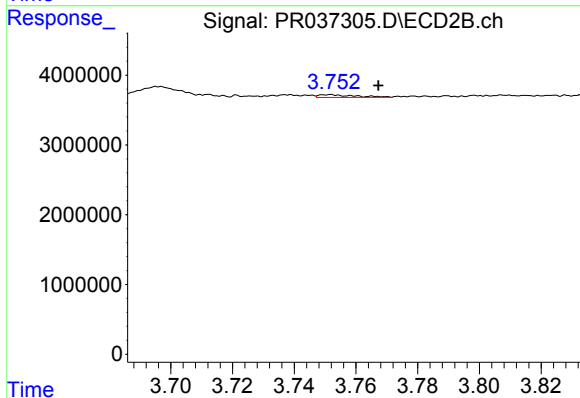


#11 AR-1232-1

R.T.: 3.752 min
Delta R.T.: -0.015 min
Response: 316377
Conc: 2.70 ng/ml

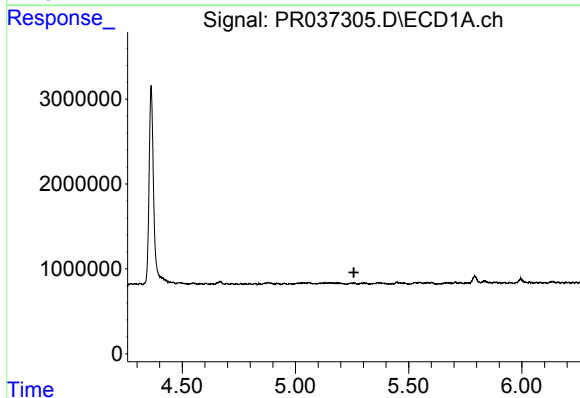


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

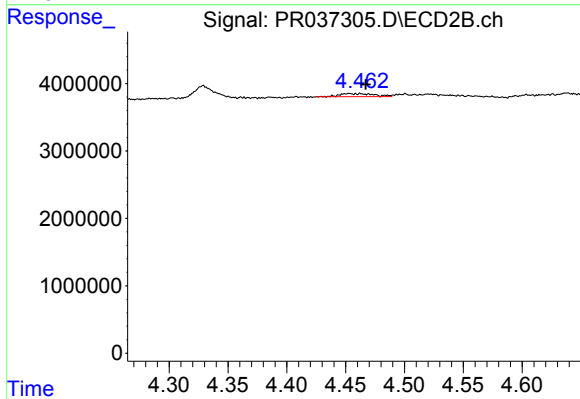

#12 AR-1232-2


R.T.: 4.459 min
Delta R.T.: -0.009 min
Response: 927952
Conc: 6.71 ng/ml

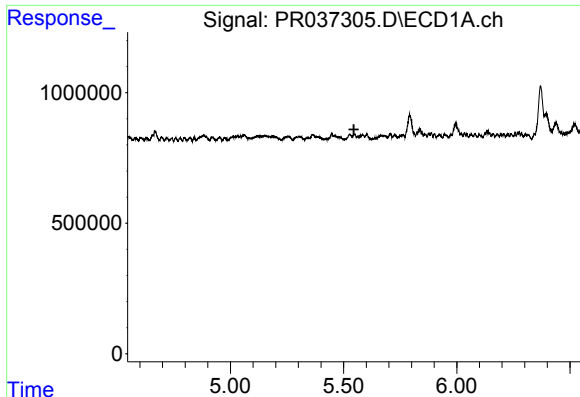

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

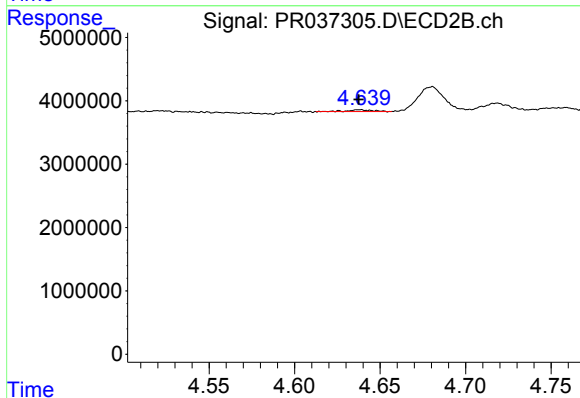


#13 AR-1232-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 256523
Conc: 3.65 ng/ml

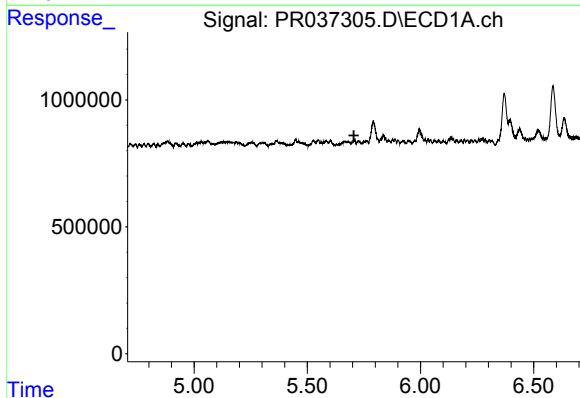


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

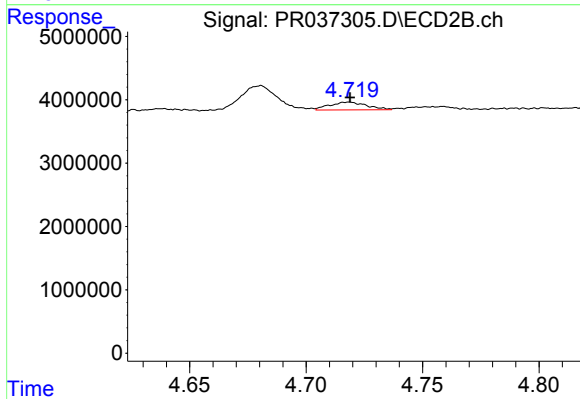

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 1377331
Conc: 23.08 ng/ml

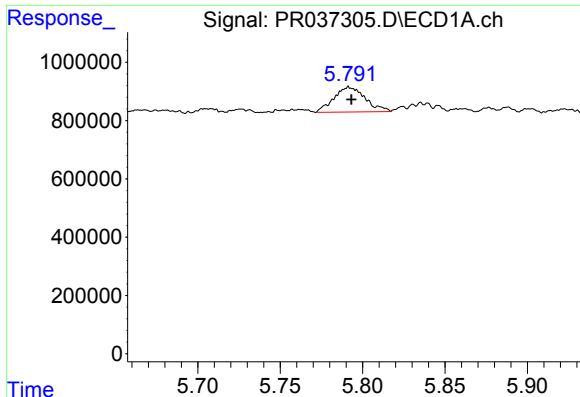

#15 AR-1232-5


R.T.: 5.792 min
Delta R.T.: -0.002 min
Response: 1136229
Conc: 97.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

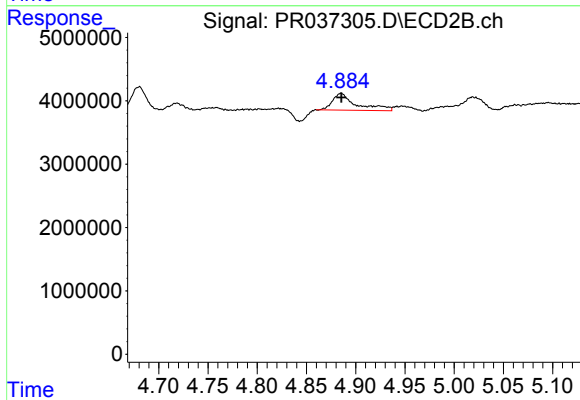


#15 AR-1232-5

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 4494841
Conc: 65.86 ng/ml

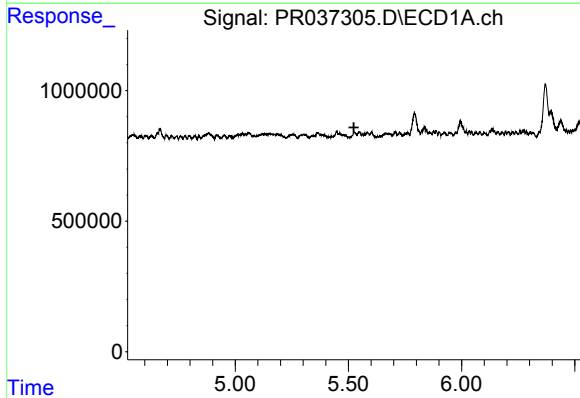


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

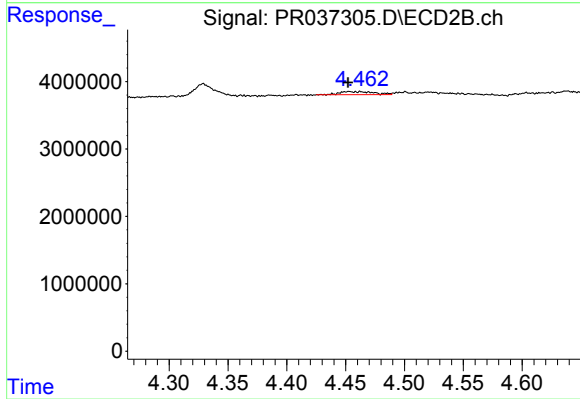

#16 AR-1242-1


R.T.: 4.459 min
Delta R.T.: 0.007 min
Response: 927952
Conc: 6.33 ng/ml

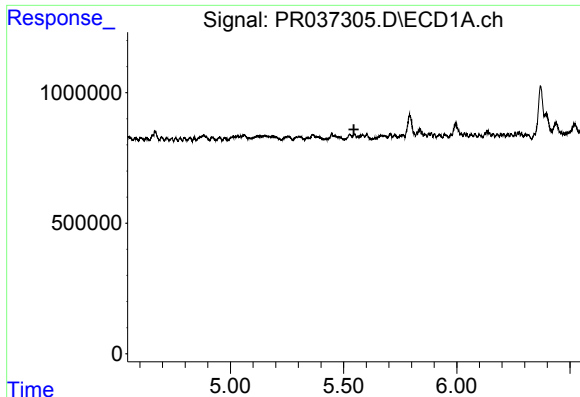

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

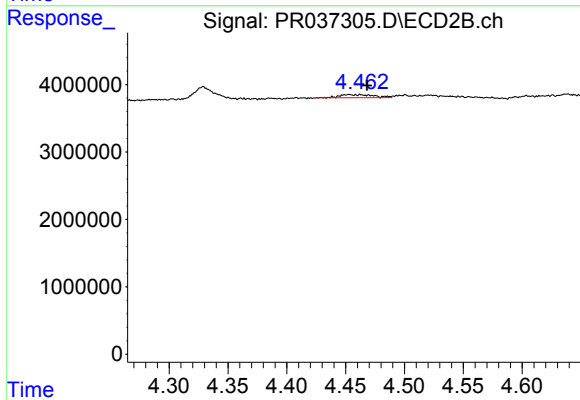


#17 AR-1242-2

R.T.: 4.459 min
Delta R.T.: -0.010 min
Response: 927952
Conc: 4.07 ng/ml

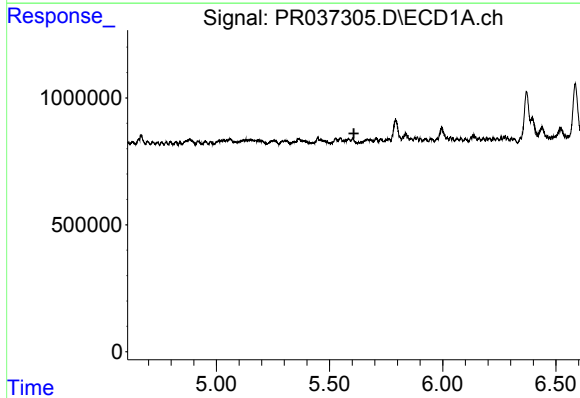


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

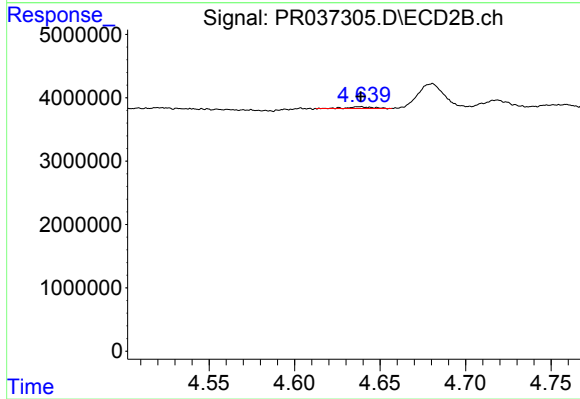

#18 AR-1242-3


R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 256523
Conc: 2.22 ng/ml

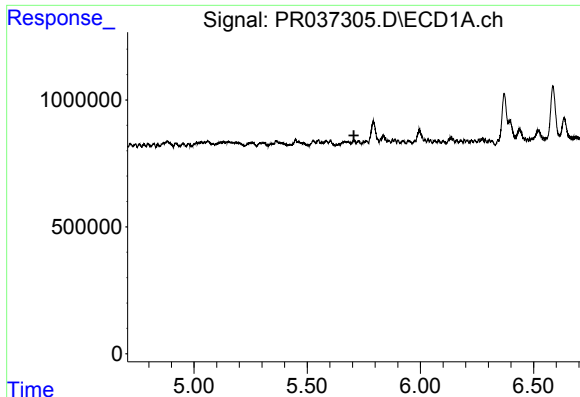

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

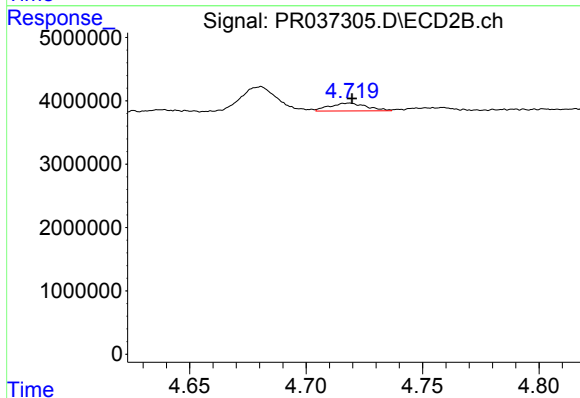


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 1377331
Conc: 12.53 ng/ml

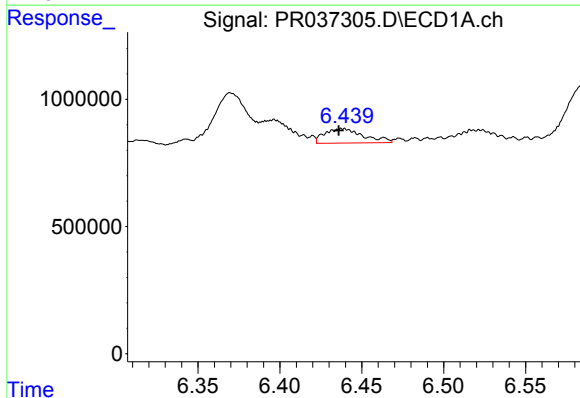


#20 AR-1242-5

R.T.: 6.438 min
Delta R.T.: 0.002 min
Response: 922983
Conc: 28.68 ng/ml

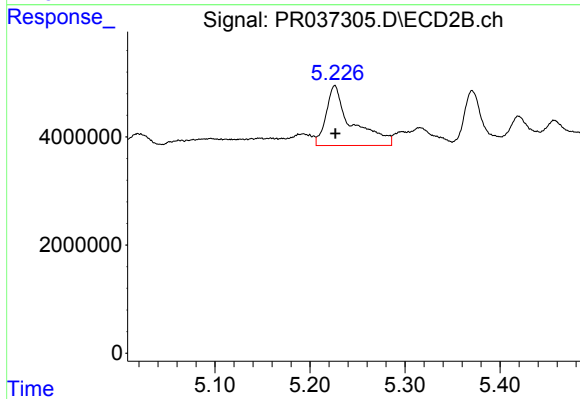

#20 AR-1242-5


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 20758925
Conc: 125.28 ng/ml

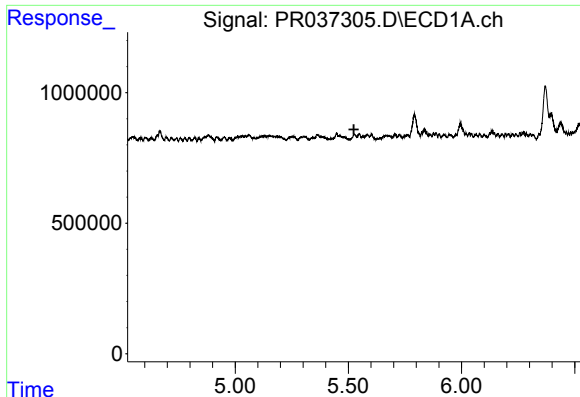

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

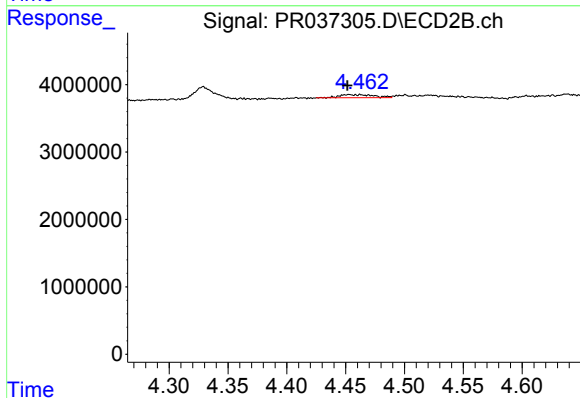


#21 AR-1248-1

R.T.: 4.459 min
Delta R.T.: 0.007 min
Response: 927952
Conc: 9.22 ng/ml

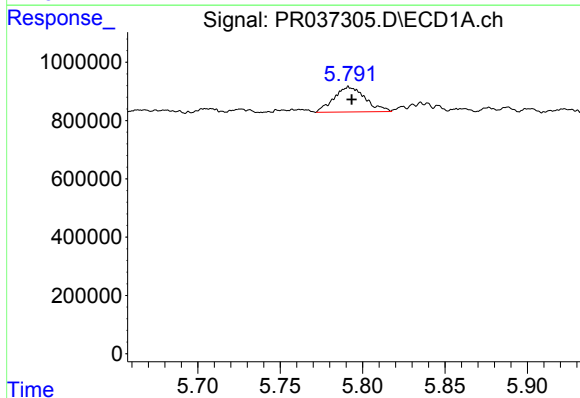


#22 AR-1248-2

R.T.: 5.792 min
Delta R.T.: -0.002 min
Response: 1136229
Conc: 32.45 ng/ml

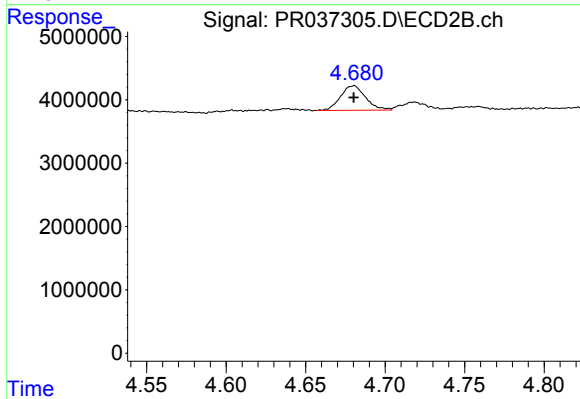

#22 AR-1248-2


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 4255490
Conc: 31.18 ng/ml

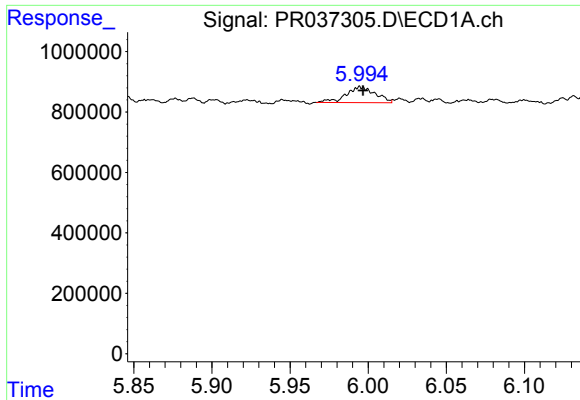

#23 AR-1248-3


R.T.: 5.995 min
Delta R.T.: -0.002 min
Response: 677638
Conc: 16.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

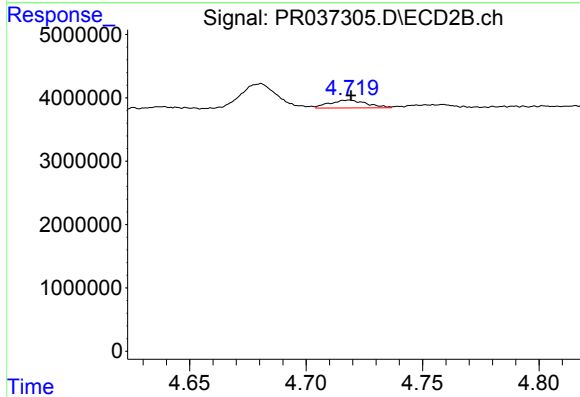


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 1377331
Conc: 9.84 ng/ml

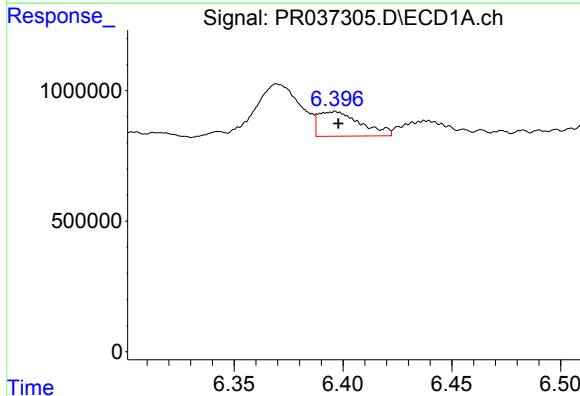


#24 AR-1248-4

R.T.: 6.396 min
Delta R.T.: -0.002 min
Response: 1273126
Conc: 26.01 ng/ml

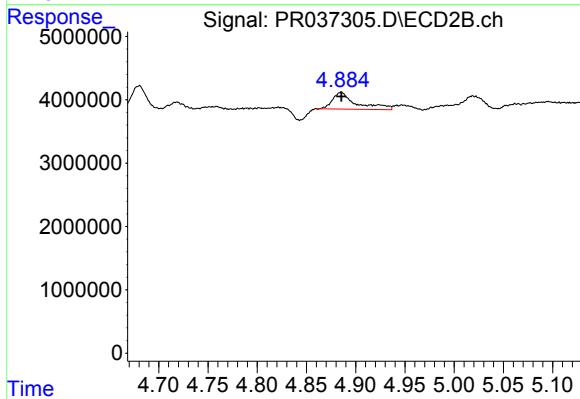

#24 AR-1248-4


R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 4494841
Conc: 25.26 ng/ml

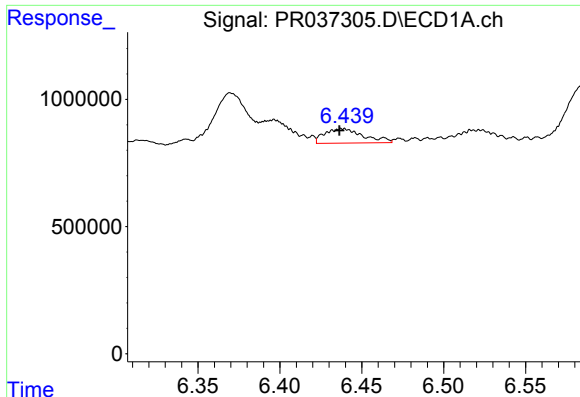

#25 AR-1248-5


R.T.: 6.438 min
Delta R.T.: 0.002 min
Response: 922983
Conc: 19.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

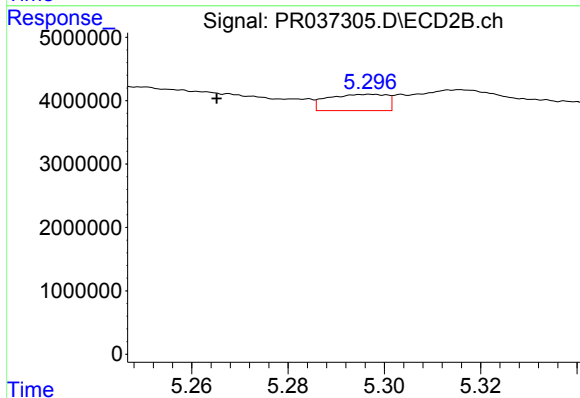


#25 AR-1248-5

R.T.: 5.297 min
Delta R.T.: 0.032 min
Response: 2173751
Conc: 11.11 ng/ml

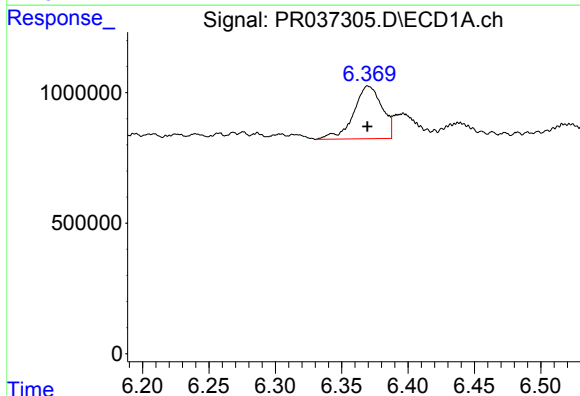


#26 AR-1254-1

R.T.: 6.370 min
Delta R.T.: 0.000 min
Response: 2994874
Conc: 54.82 ng/ml

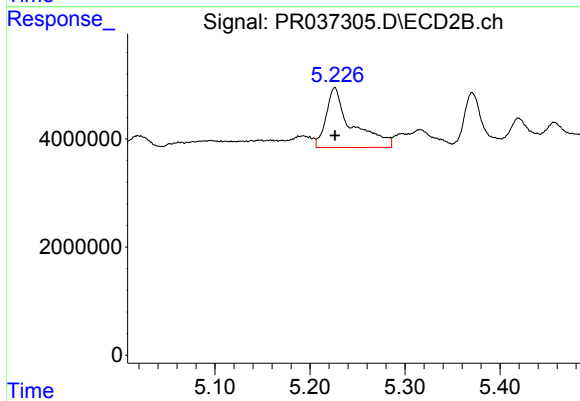

#26 AR-1254-1


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 20758925
Conc: 60.26 ng/ml

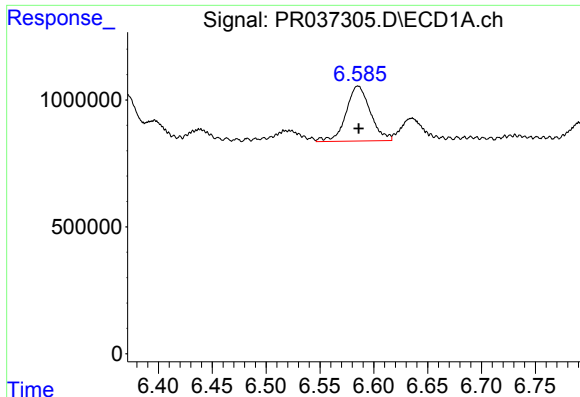

#27 AR-1254-2


R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 3409979
Conc: 39.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

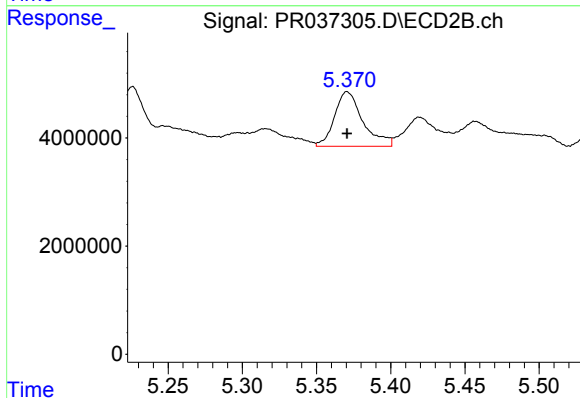


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 13470014
Conc: 44.97 ng/ml

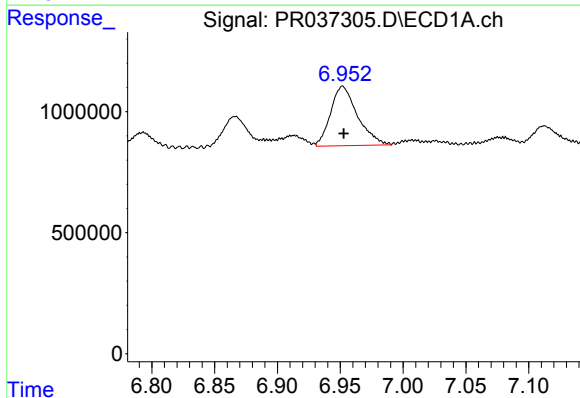


#28 AR-1254-3

R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 3661471
Conc: 40.25 ng/ml

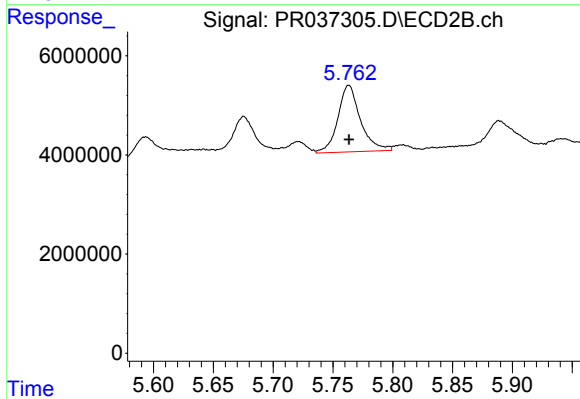

#28 AR-1254-3


R.T.: 5.763 min
Delta R.T.: 0.000 min
Response: 17723055
Conc: 37.42 ng/ml

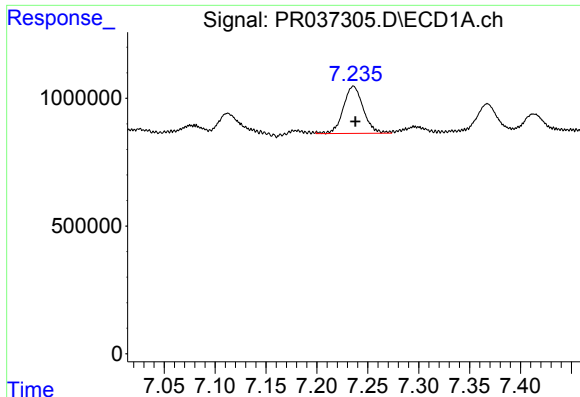

#29 AR-1254-4


R.T.: 7.236 min
Delta R.T.: -0.002 min
Response: 2521979
Conc: 37.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

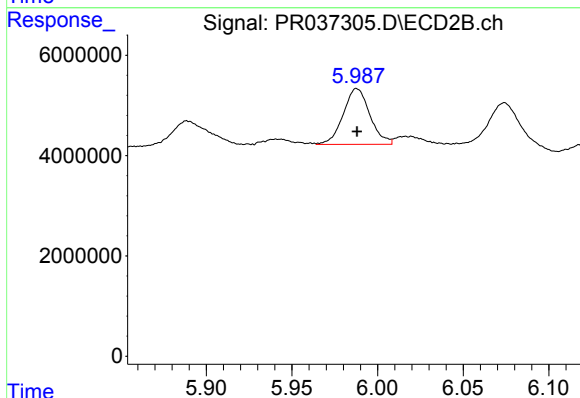


#29 AR-1254-4

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 12077002
Conc: 34.44 ng/ml

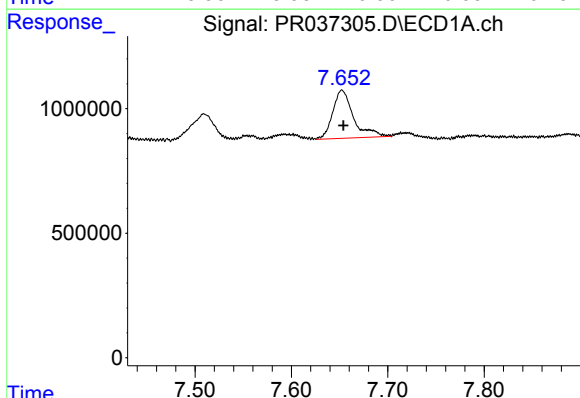


#30 AR-1254-5

R.T.: 7.653 min
Delta R.T.: -0.001 min
Response: 2904721
Conc: 40.41 ng/ml

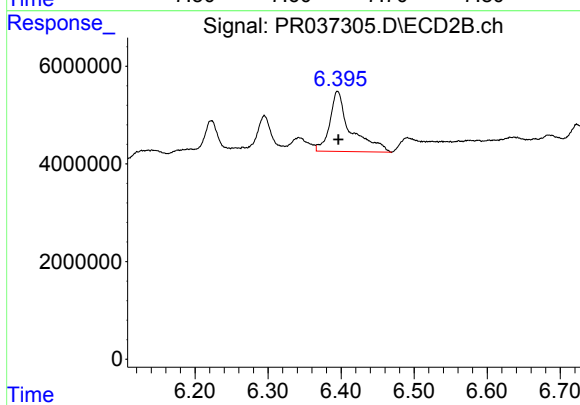

#30 AR-1254-5


R.T.: 6.395 min
Delta R.T.: -0.001 min
Response: 24527418
Conc: 55.39 ng/ml

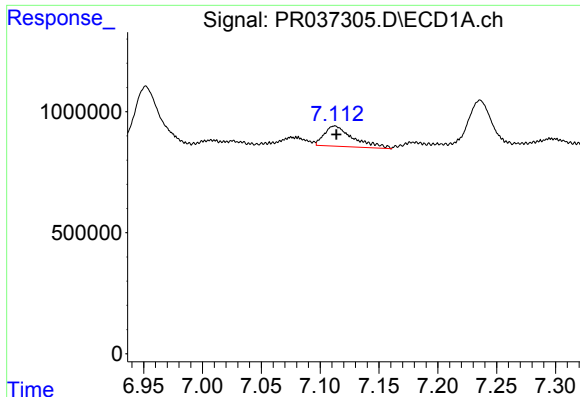

#31 AR-1260-1


R.T.: 7.112 min
Delta R.T.: -0.001 min
Response: 1419703
Conc: 21.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

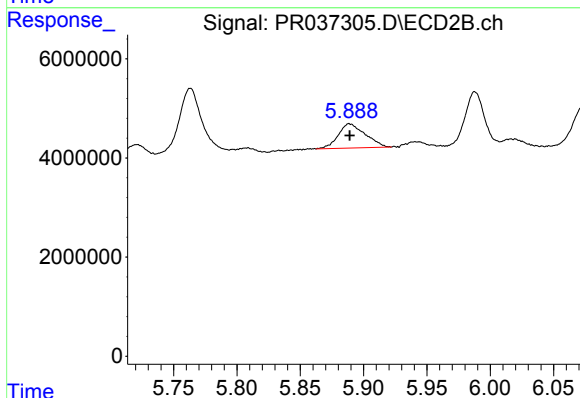


#31 AR-1260-1

R.T.: 5.889 min
Delta R.T.: 0.000 min
Response: 7251590
Conc: 24.81 ng/ml

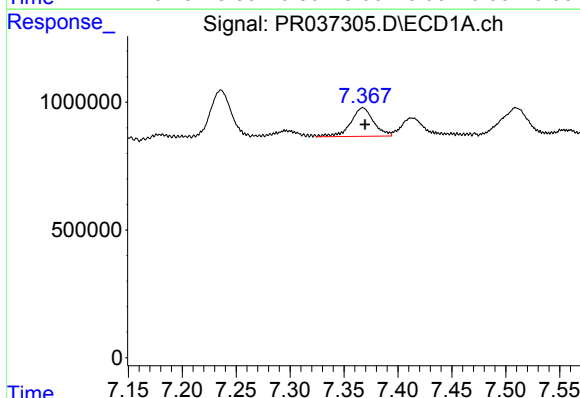


#32 AR-1260-2

R.T.: 7.367 min
Delta R.T.: -0.002 min
Response: 1645294
Conc: 20.64 ng/ml

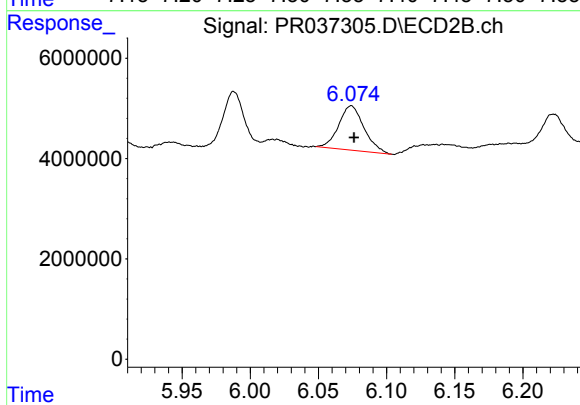

#32 AR-1260-2


R.T.: 6.074 min
Delta R.T.: -0.002 min
Response: 11382015
Conc: 24.71 ng/ml

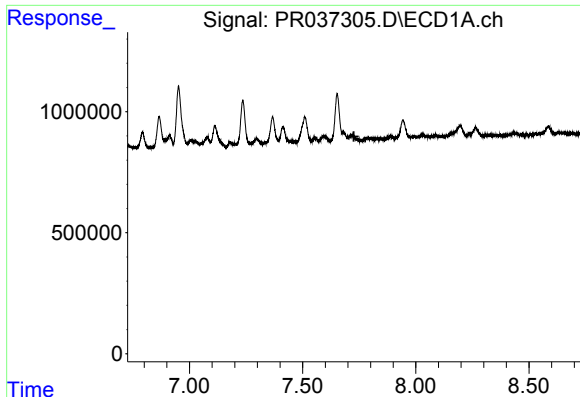

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

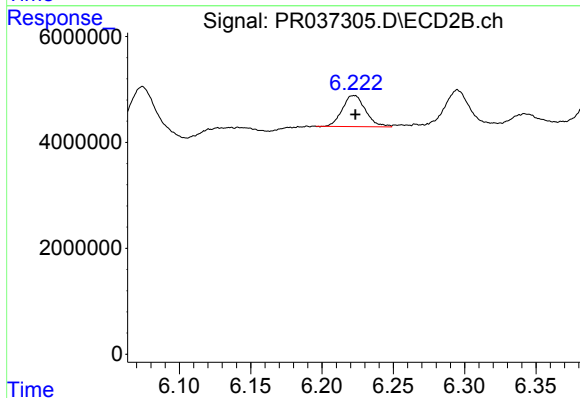


#33 AR-1260-3

R.T.: 6.222 min
Delta R.T.: -0.001 min
Response: 6641917
Conc: 18.63 ng/ml

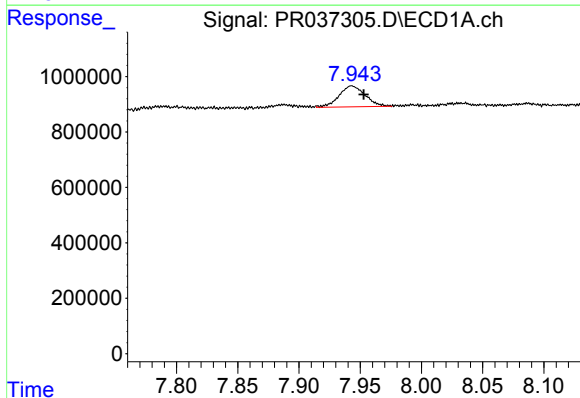


#34 AR-1260-4

R.T.: 7.943 min
Delta R.T.: -0.010 min
Response: 1119749
Conc: 15.05 ng/ml

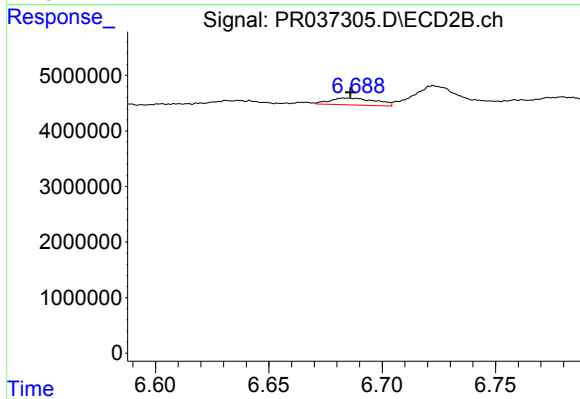

#34 AR-1260-4


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 1723908
Conc: 5.66 ng/ml

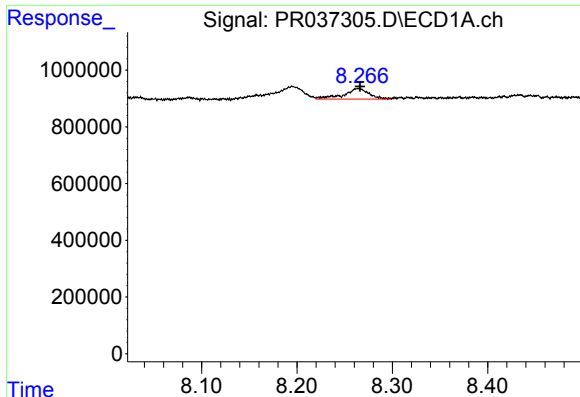

#35 AR-1260-5


R.T.: 8.265 min
Delta R.T.: -0.001 min
Response: 699919
Conc: 4.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

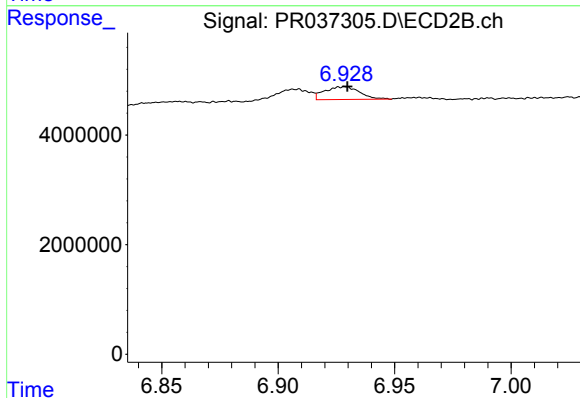


#35 AR-1260-5

R.T.: 6.928 min
Delta R.T.: -0.001 min
Response: 2439301
Conc: 2.81 ng/ml

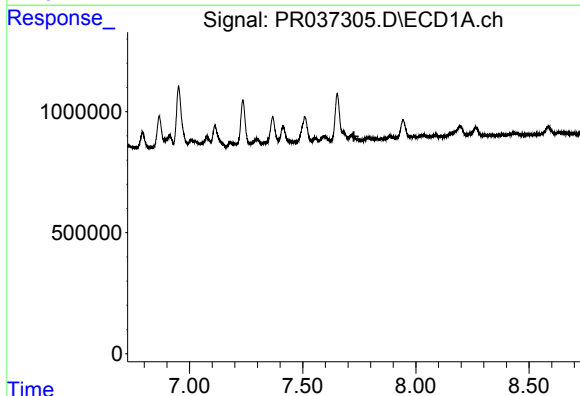


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.726 min
Response: 0
Conc: N.D.

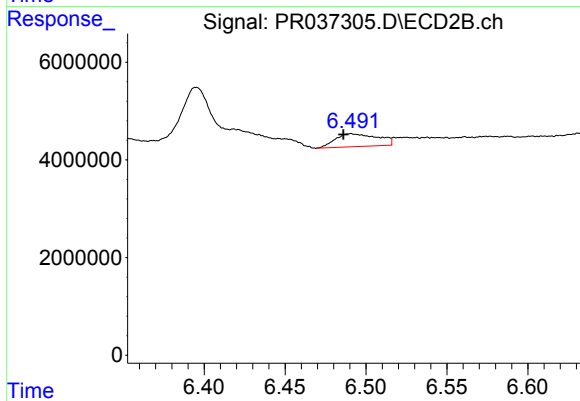

#36 AR-1262-1


R.T.: 6.491 min
Delta R.T.: 0.005 min
Response: 4797128
Conc: 19.14 ng/ml

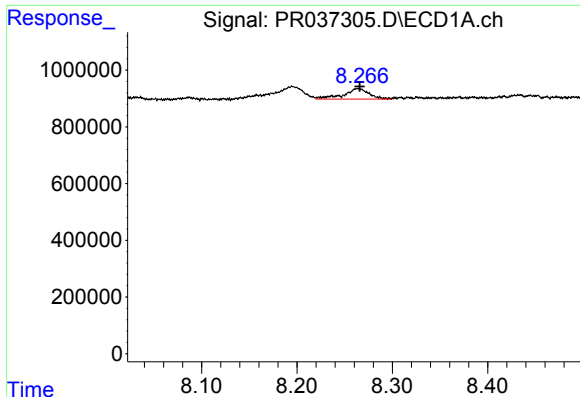

#37 AR-1262-2


R.T.: 8.265 min
Delta R.T.: -0.001 min
Response: 699919
Conc: 3.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

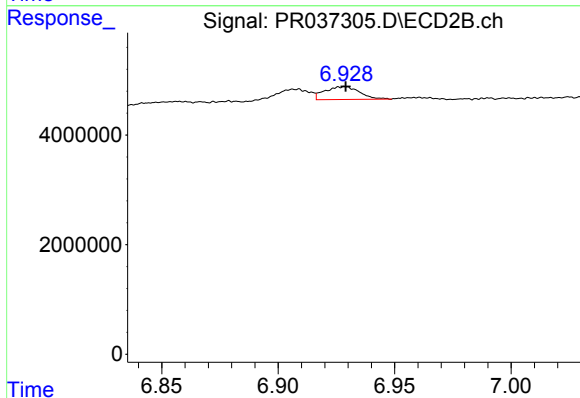


#37 AR-1262-2

R.T.: 6.928 min
Delta R.T.: 0.000 min
Response: 2439301
Conc: 1.94 ng/ml

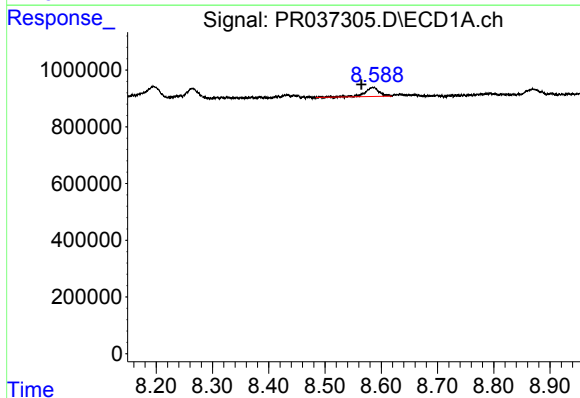


#38 AR-1262-3

R.T.: 8.586 min
Delta R.T.: 0.021 min
Response: 564057
Conc: 4.29 ng/ml

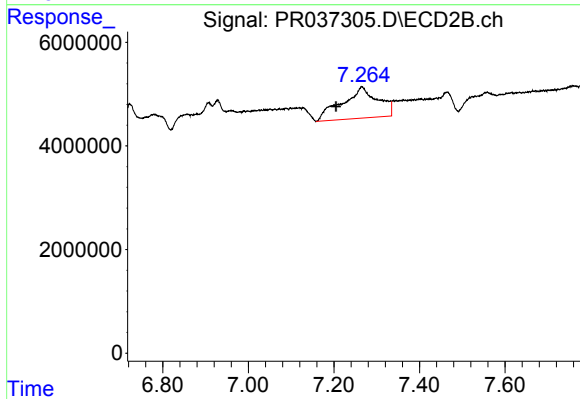

#38 AR-1262-3


R.T.: 7.265 min
Delta R.T.: 0.060 min
Response: 35041508
Conc: 63.91 ng/ml

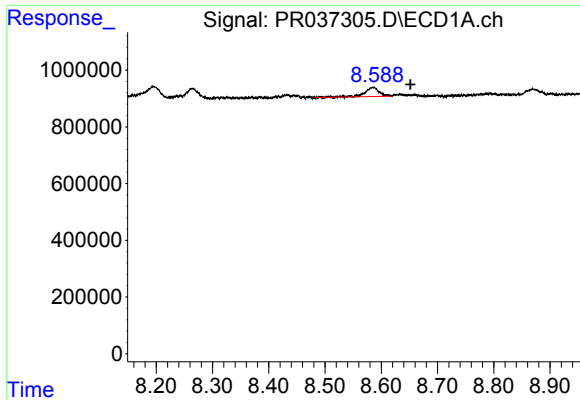

#39 AR-1262-4


R.T.: 8.586 min
Delta R.T.: -0.066 min
Response: 564057
Conc: 5.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

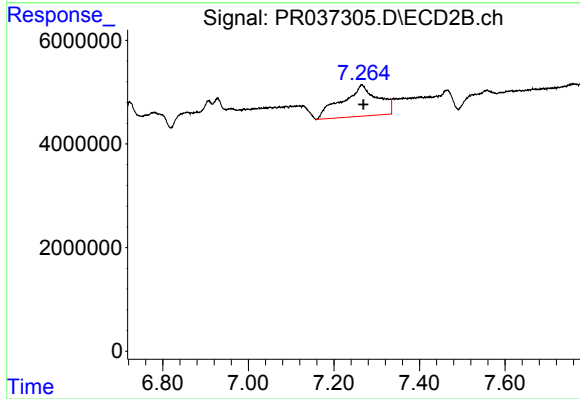


#39 AR-1262-4

R.T.: 7.265 min
Delta R.T.: -0.004 min
Response: 35041508
Conc: 39.04 ng/ml

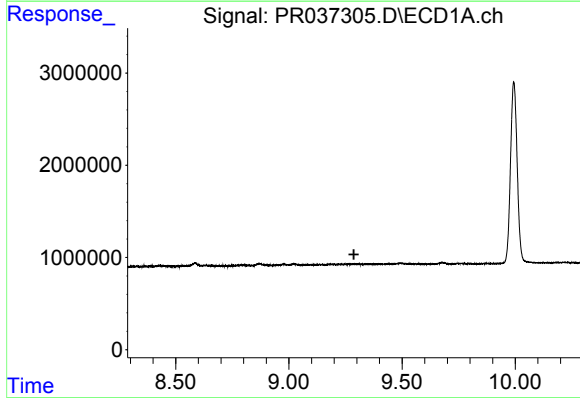


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.287 min
Response: 0
Conc: N.D.

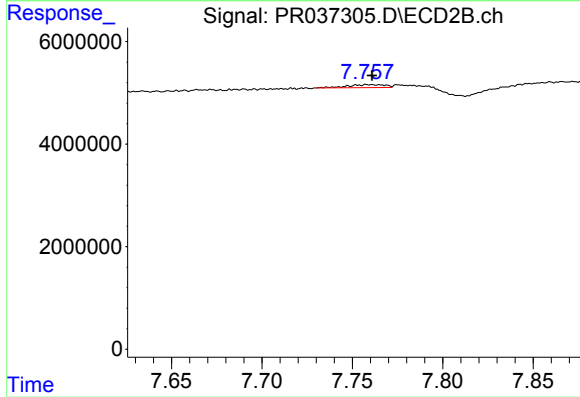

#40 AR-1262-5


R.T.: 7.759 min
Delta R.T.: -0.002 min
Response: 826417
Conc: 2.16 ng/ml

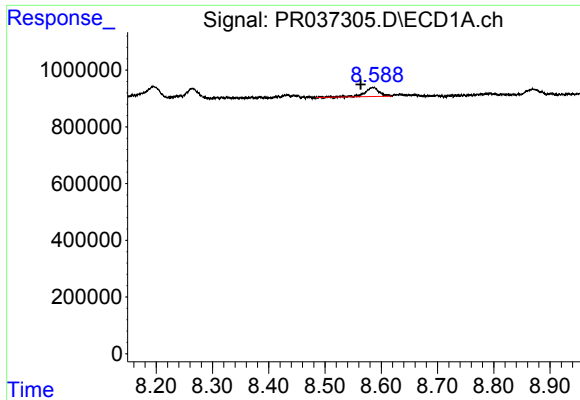

#41 AR-1268-1


R.T.: 8.586 min
Delta R.T.: 0.022 min
Response: 564057
Conc: 3.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

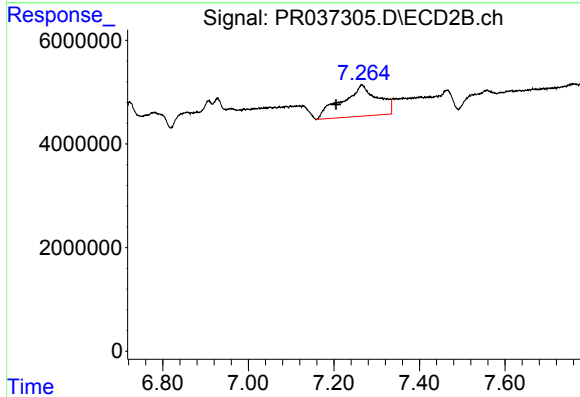


#41 AR-1268-1

R.T.: 7.265 min
Delta R.T.: 0.060 min
Response: 35041508
Conc: 28.47 ng/ml

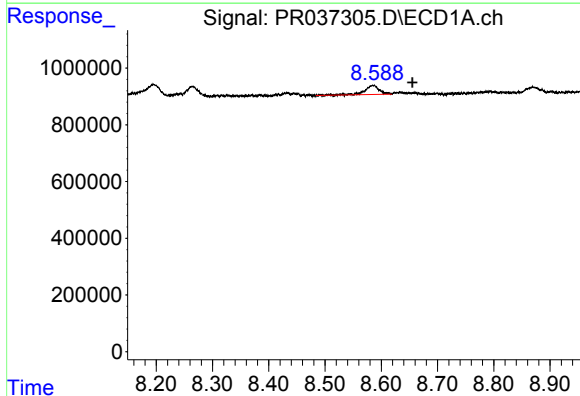


#42 AR-1268-2

R.T.: 8.586 min
Delta R.T.: -0.069 min
Response: 564057
Conc: 3.43 ng/ml

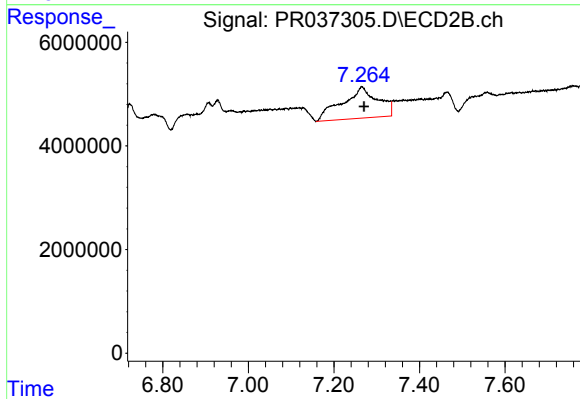

#42 AR-1268-2


R.T.: 7.265 min
Delta R.T.: -0.005 min
Response: 35041508
Conc: 33.09 ng/ml

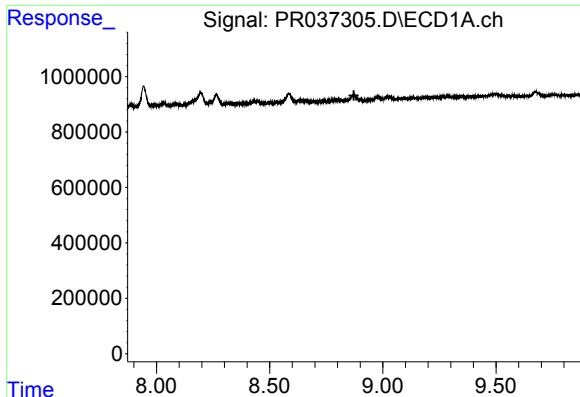

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

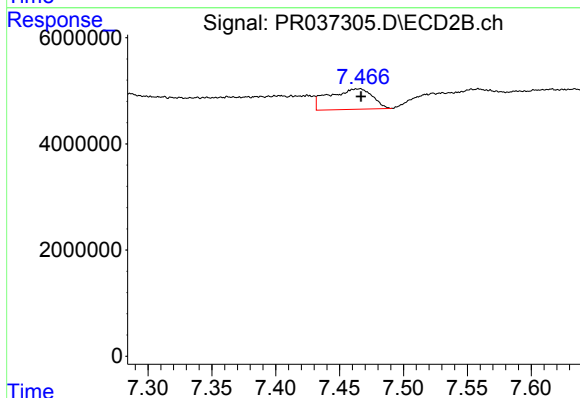


#43 AR-1268-3

R.T.: 7.465 min
Delta R.T.: -0.001 min
Response: 9170946
Conc: 10.35 ng/ml

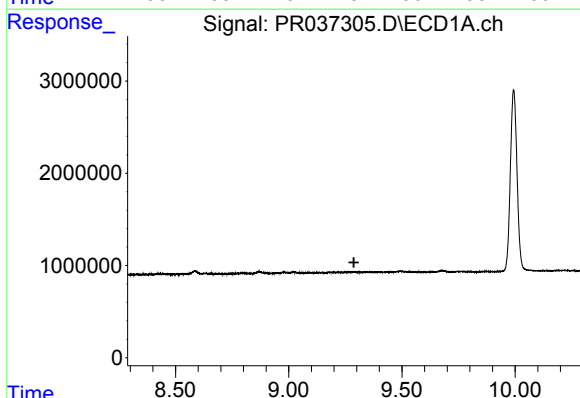


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

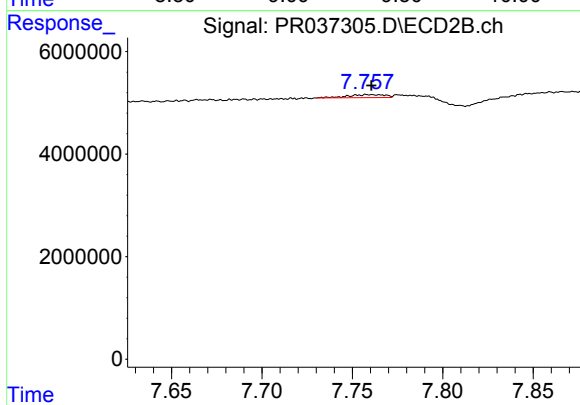

#44 AR-1268-4


R.T.: 7.759 min
Delta R.T.: -0.002 min
Response: 826417
Conc: 2.28 ng/ml

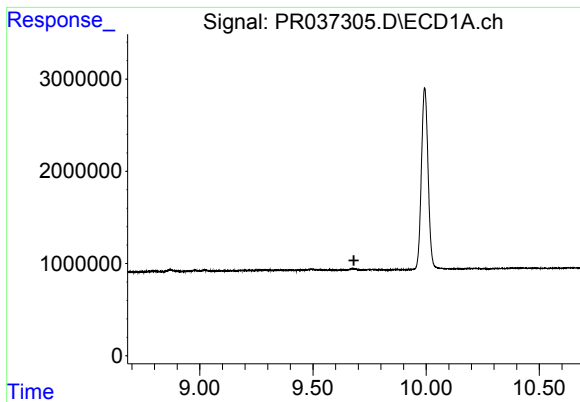

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

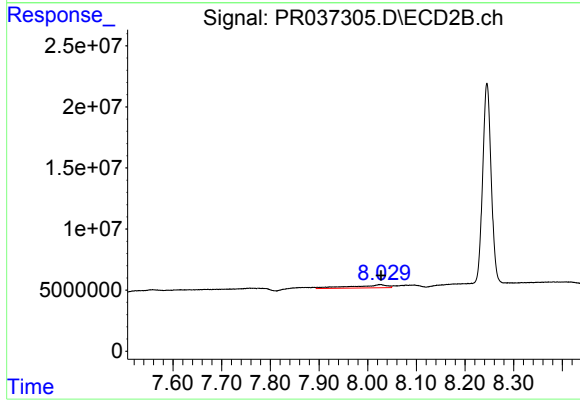

#45 AR-1268-5

R.T.: 8.027 min
Delta R.T.: 0.000 min
Response: 12435958
Conc: 4.89 ng/ml