

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 21:07
 Operator : SM\SJ
 Sample : K1560-15
 Misc : AR1262 MDL 25PPB
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:55:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.361	3.408	39966531	159.3E6	31.948	33.227
2)	SA Decachlor...	9.993	8.244	46373967	232.1E6	35.063	39.854
Target Compounds							
3)	L1 AR-1016-1	0.000	4.454	0	604742	N.D.	3.321 #
4)	L1 AR-1016-2	0.000	4.468	0	178923	N.D.	0.634 #
5)	L1 AR-1016-3	0.000	4.639	0	357506	N.D.	2.486 #
6)	L1 AR-1016-4	0.000	4.688	0	1549128	N.D.	14.002 #
7)	L1 AR-1016-5	0.000	4.886	0	935631	N.D.	6.155 #
8)	L2 AR-1221-1	0.000	3.608	0	242541	N.D.	4.763 #
9)	L2 AR-1221-2	4.665	3.698	579906	2617265	64.121	70.478
10)	L2 AR-1221-3	4.665	3.740	579906	188384	18.921	1.538 #
11)	L3 AR-1232-1	4.665	3.740	579906	188384	19.825	1.610 #
12)	L3 AR-1232-2	0.000	4.468	0	178923	N.D.	1.294 #
13)	L3 AR-1232-3	0.000	4.639	0	357506	N.D.	5.093 #
14)	L3 AR-1232-4	0.000	4.715	0	394623	N.D.	6.613 #
15)	L3 AR-1232-5	0.000	4.886	0	935631	N.D.	13.710 #
16)	L4 AR-1242-1	0.000	4.454	0	604742	N.D.	4.127 #
17)	L4 AR-1242-2	0.000	4.468	0	178923	N.D.	0.784 #
18)	L4 AR-1242-3	0.000	4.639	0	357506	N.D.	3.092 #
19)	L4 AR-1242-4	0.000	4.715	0	394623	N.D.	3.590 #
20)	L4 AR-1242-5	6.440	5.227	526085	5846358	16.349	35.283 #
21)	L5 AR-1248-1	0.000	4.454	0	604742	N.D.	6.008 #
22)	L5 AR-1248-2	0.000	4.688	0	1549128	N.D.	11.351 #
23)	L5 AR-1248-3	0.000	4.715	0	394623	N.D.	2.819 #
24)	L5 AR-1248-4	6.411	4.886	232570	935631	4.751	5.257
25)	L5 AR-1248-5	6.440	5.248	526085	13668495	11.137	69.875 #
26)	L6 AR-1254-1	6.372	5.227	3039149	5846358	55.631	16.972 #
27)	L6 AR-1254-2	6.584	5.371	791883	11270574	9.240	37.631 #
28)	L6 AR-1254-3	6.969	5.776	1552662	13027305	17.069	27.506 #
29)	L6 AR-1254-4	7.235	5.986	1690683	568869	25.231	1.622 #
30)	L6 AR-1254-5	7.650	6.394	3341409	15067706	46.485	34.026 #
31)	L7 AR-1260-1	7.112	5.888	3373444	11128983	51.123	38.077 #
32)	L7 AR-1260-2	7.367	6.074	3785742	20375969	47.498	44.239
33)	L7 AR-1260-3	7.724	6.223	4468686	14803828	71.413	41.526 #
34)	L7 AR-1260-4	7.951	6.685	4405799	20212266	59.214	66.321
35)	L7 AR-1260-5	8.263	6.927	7571370	45599977	52.353	52.580
36)	L8 AR-1262-1	7.724	6.485	4468686	13904208	42.782	55.479 #
37)	L8 AR-1262-2	8.263	6.927	7571370	45599977	38.950	36.307
38)	L8 AR-1262-3	8.561	7.202	5700272	29868300	43.345	54.478 #
39)	L8 AR-1262-4	8.651	7.267	4177900	58274700	42.532	64.920 #
40)	L8 AR-1262-5	9.284	7.758	2887615	15652753	41.825	40.909
41)	L9 AR-1268-1	8.561	7.202	5700272	29868300	31.829	24.263

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 21:07
 Operator : SM\SJ
 Sample : K1560-15
 Misc : AR1262 MDL 25PPB
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:55:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.651	7.267	4177900	58274700	25.398	55.032 #
43) L9	AR-1268-3	8.869	7.465	899165	10688916	6.495	12.061 #
44) L9	AR-1268-4	9.284	7.758	2887615	15652753	46.286	43.146
45) L9	AR-1268-5	9.675	8.024	1305461	18611120	2.864	7.315 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
Data File : PR037306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 21:07
Operator : SM\SJ
Sample : K1560-15
Misc : AR1262 MDL 25PPB
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:55:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

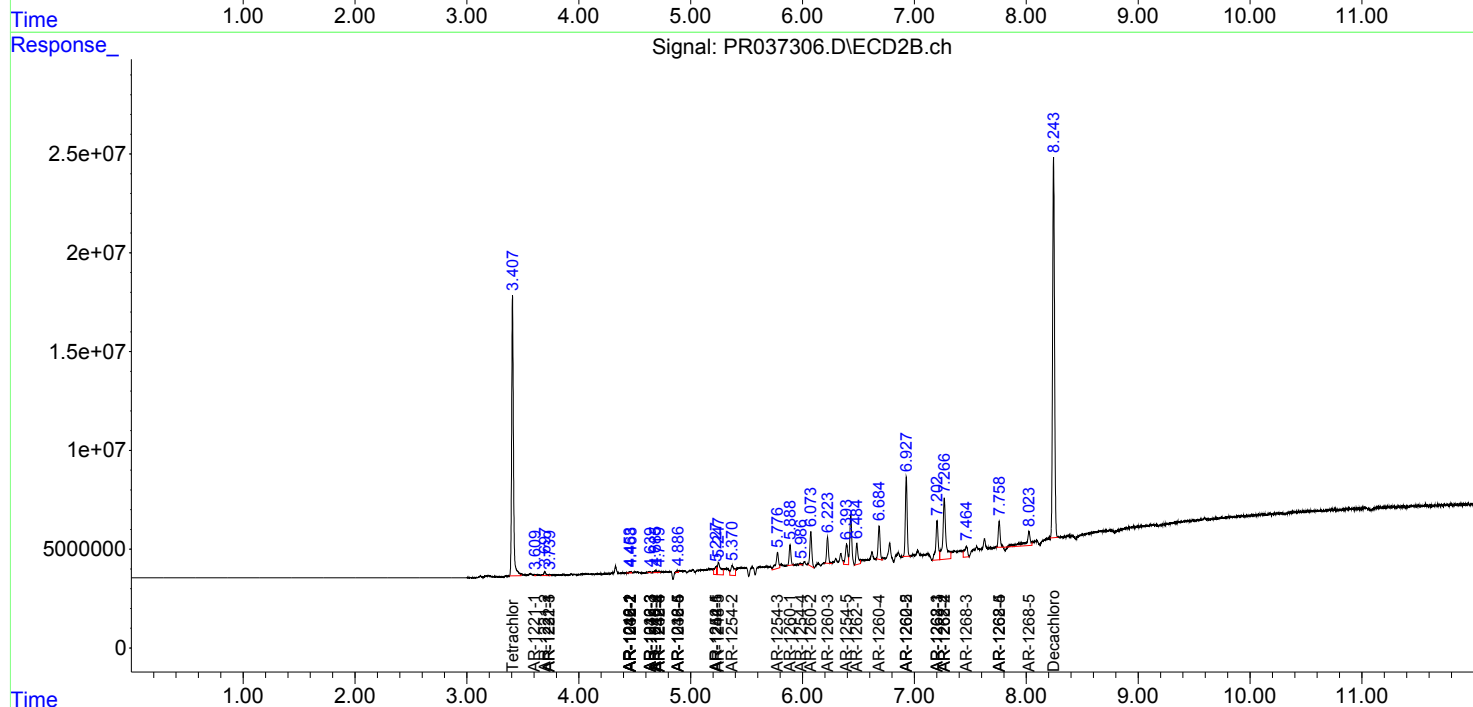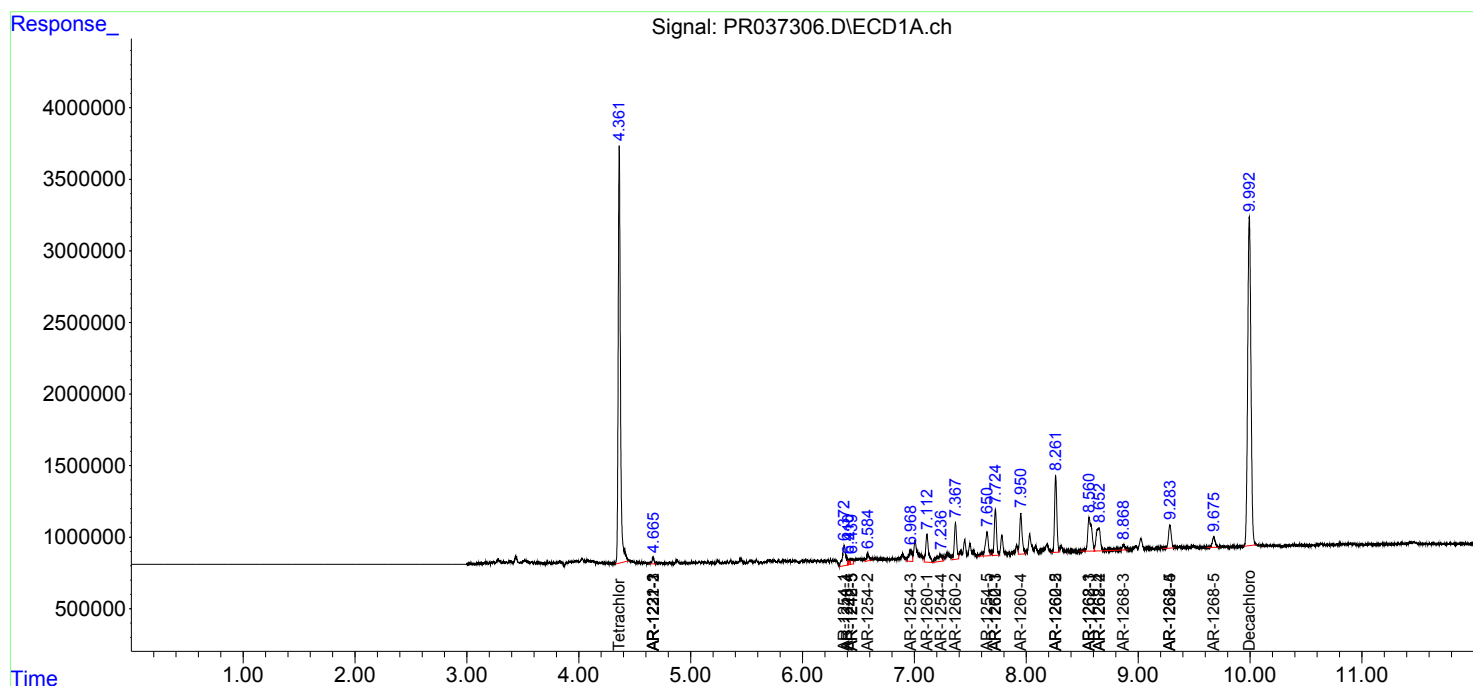


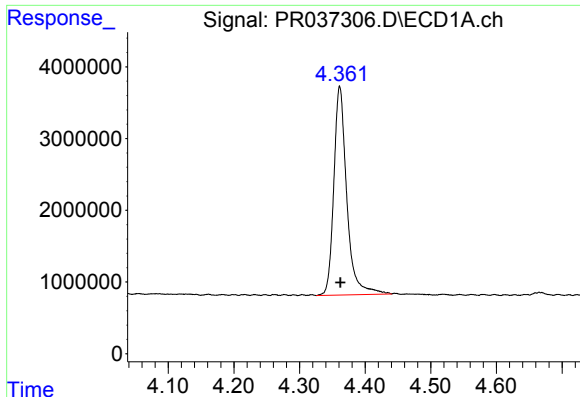

#1 Tetrachloro-m-xylene


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 39966531
Conc: 31.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

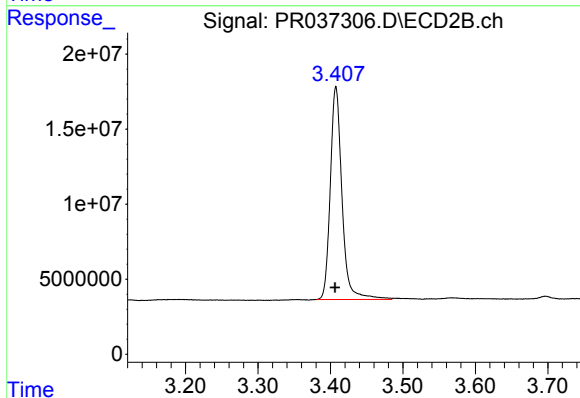


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: 0.001 min
Response: 159340248
Conc: 33.23 ng/ml

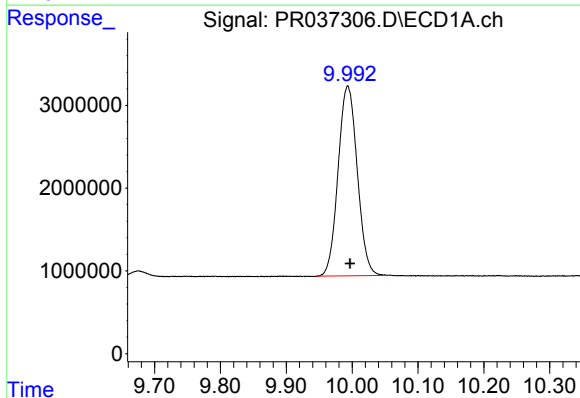


#2 Decachlorobiphenyl

R.T.: 9.993 min
Delta R.T.: -0.003 min
Response: 46373967
Conc: 35.06 ng/ml

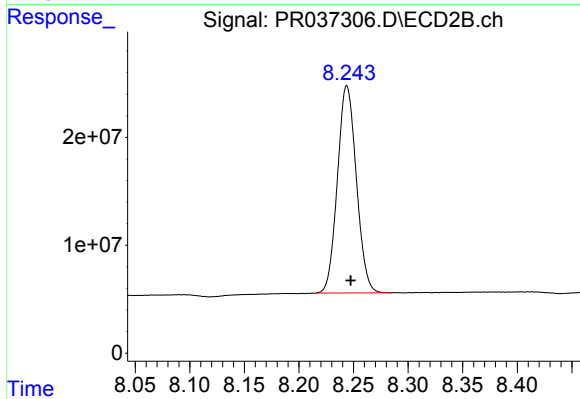

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 232118835
Conc: 39.85 ng/ml

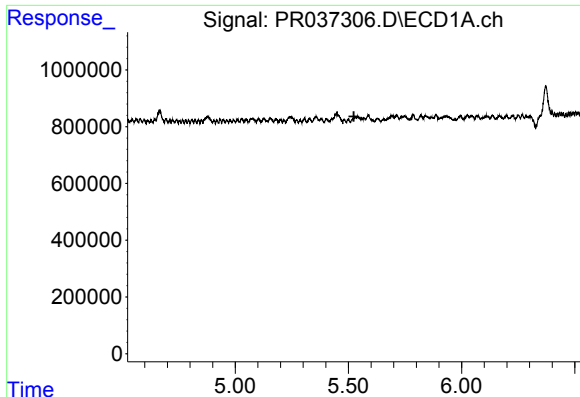

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

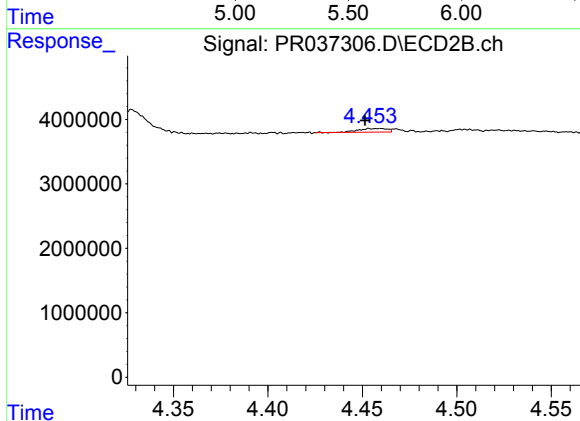


#3 AR-1016-1

R.T.: 4.454 min
Delta R.T.: 0.002 min
Response: 604742
Conc: 3.32 ng/ml

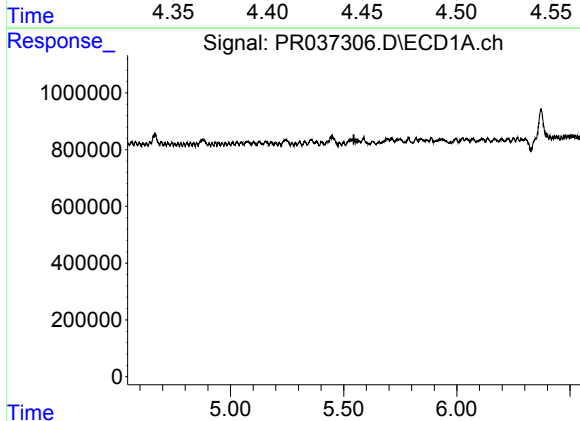


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

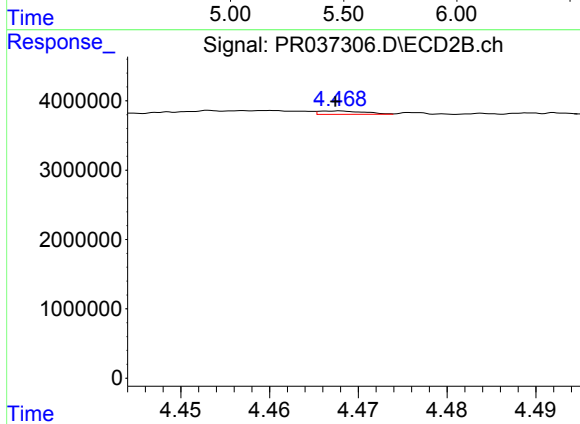

#4 AR-1016-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 178923
Conc: 0.63 ng/ml

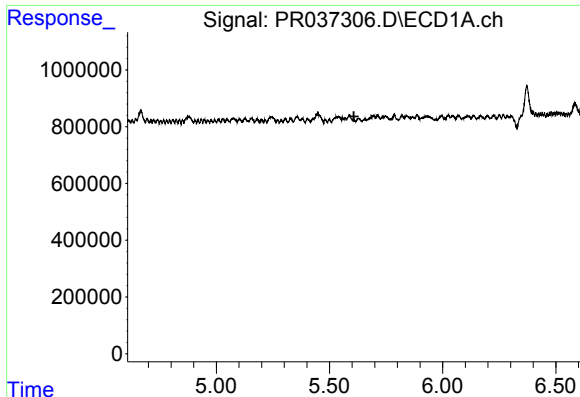

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

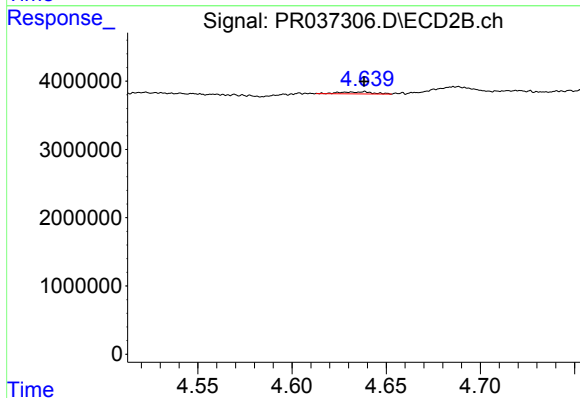


#5 AR-1016-3

R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 357506
Conc: 2.49 ng/ml

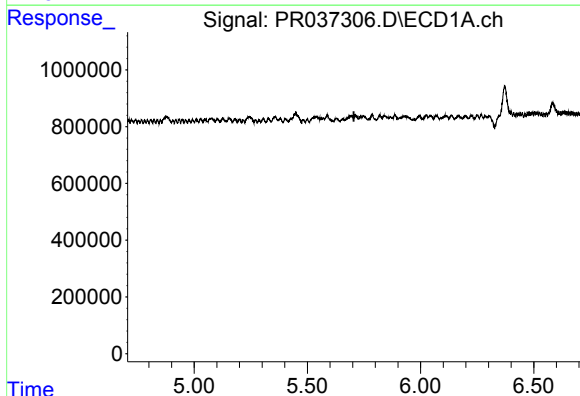


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

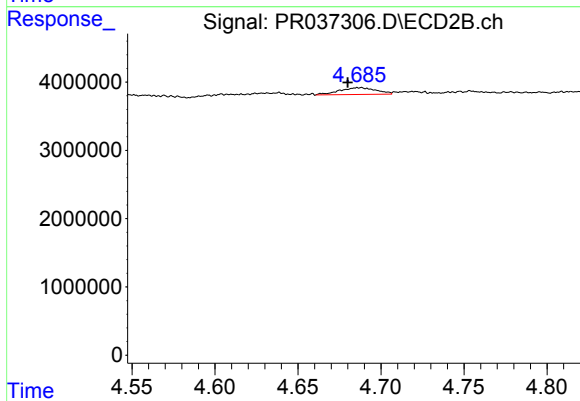

#6 AR-1016-4


R.T.: 4.688 min
Delta R.T.: 0.009 min
Response: 1549128
Conc: 14.00 ng/ml

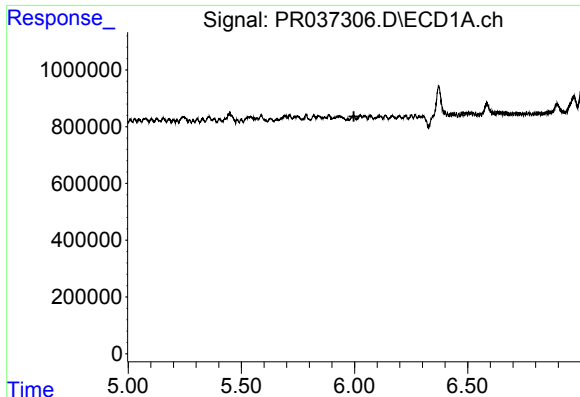

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

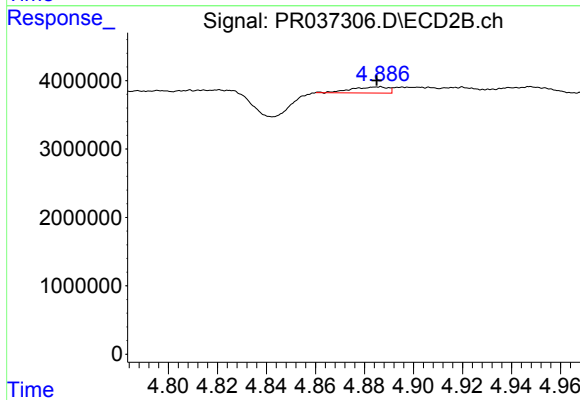


#7 AR-1016-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 935631
Conc: 6.16 ng/ml

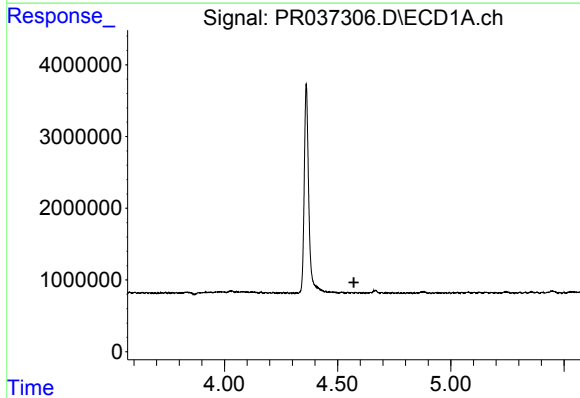


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

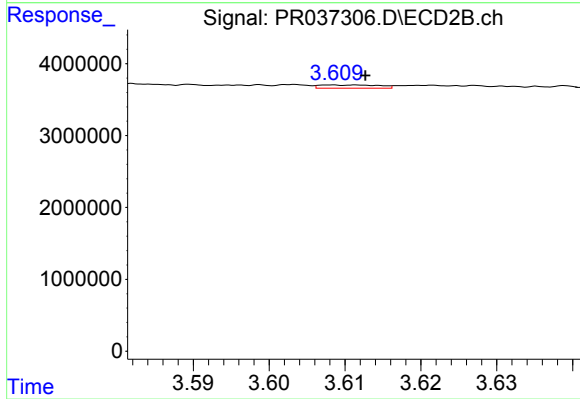

#8 AR-1221-1


R.T.: 3.608 min
Delta R.T.: -0.004 min
Response: 242541
Conc: 4.76 ng/ml

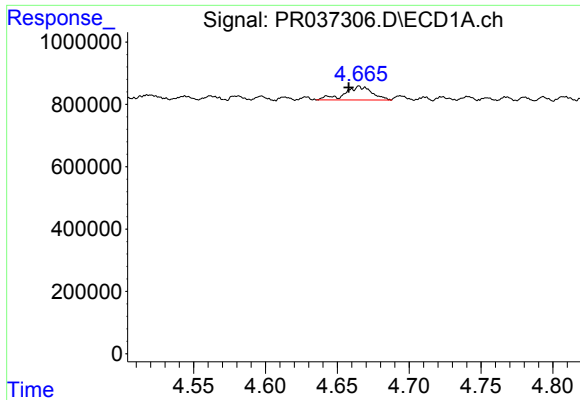

#9 AR-1221-2


R.T.: 4.665 min
Delta R.T.: 0.007 min
Response: 579906
Conc: 64.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

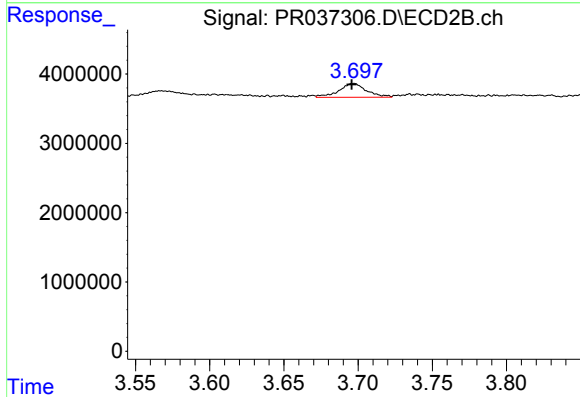


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.002 min
Response: 2617265
Conc: 70.48 ng/ml

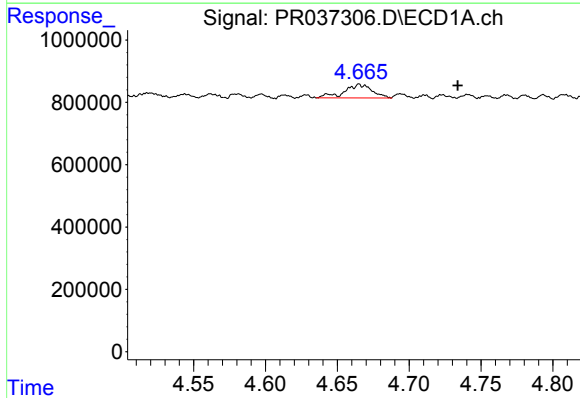


#10 AR-1221-3

R.T.: 4.665 min
Delta R.T.: -0.069 min
Response: 579906
Conc: 18.92 ng/ml

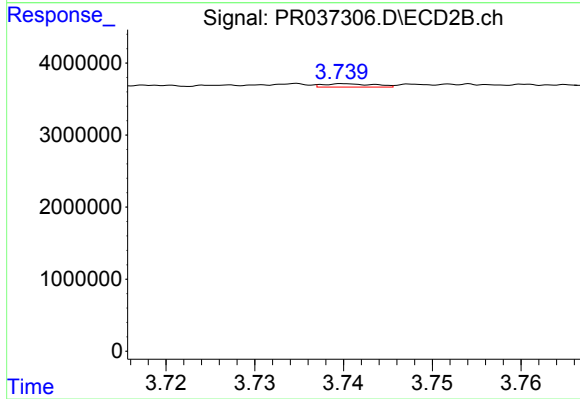

#10 AR-1221-3


R.T.: 3.740 min
Delta R.T.: -0.027 min
Response: 188384
Conc: 1.54 ng/ml

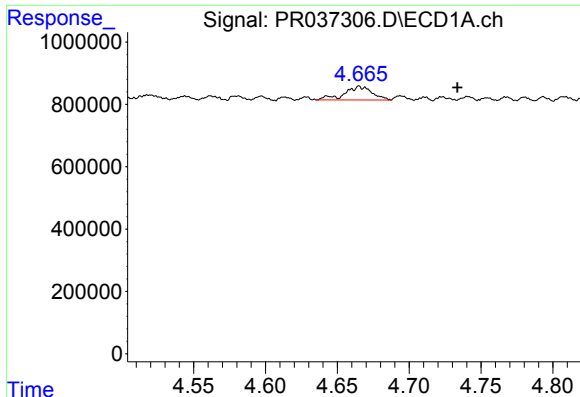

#11 AR-1232-1


R.T.: 4.665 min
Delta R.T.: -0.068 min
Response: 579906
Conc: 19.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

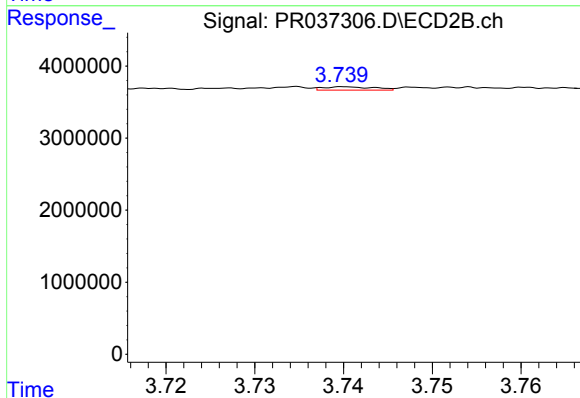


#11 AR-1232-1

R.T.: 3.740 min
Delta R.T.: -0.027 min
Response: 188384
Conc: 1.61 ng/ml

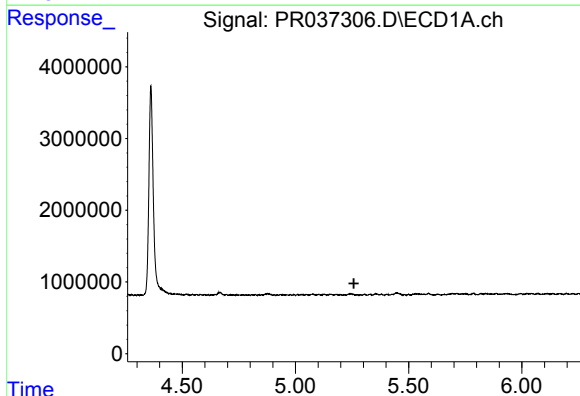


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

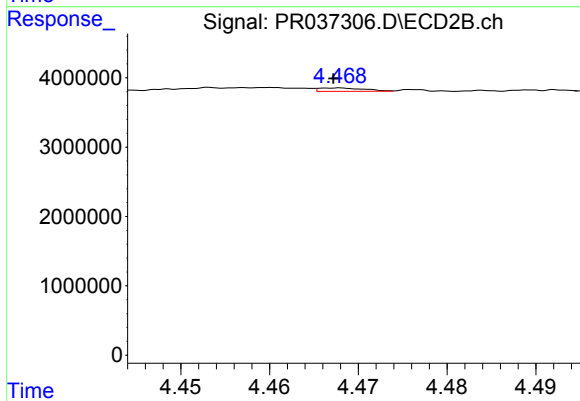

#12 AR-1232-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 178923
Conc: 1.29 ng/ml

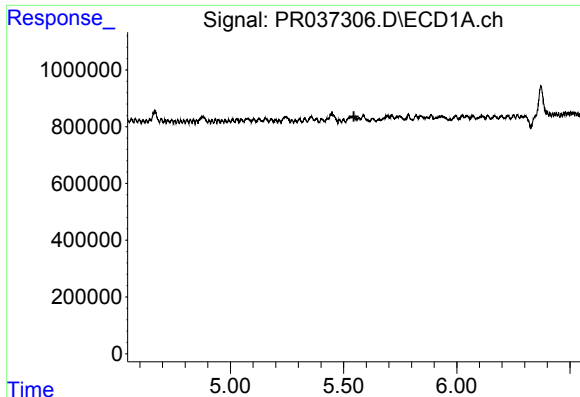

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

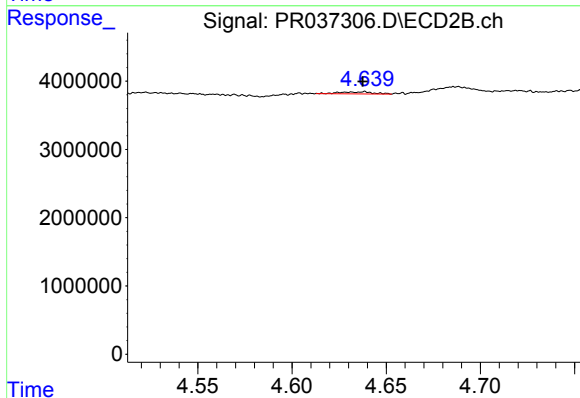


#13 AR-1232-3

R.T.: 4.639 min
Delta R.T.: 0.001 min
Response: 357506
Conc: 5.09 ng/ml

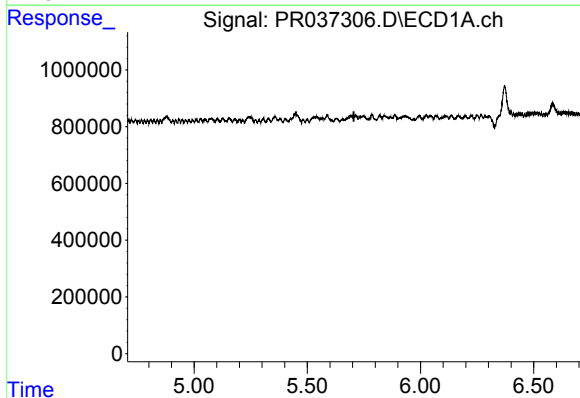


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

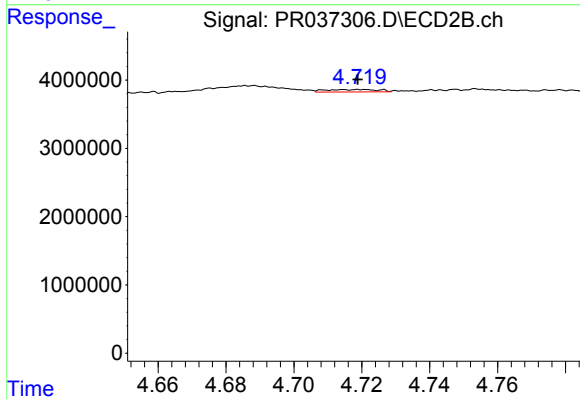

#14 AR-1232-4


R.T.: 4.715 min
Delta R.T.: -0.004 min
Response: 394623
Conc: 6.61 ng/ml

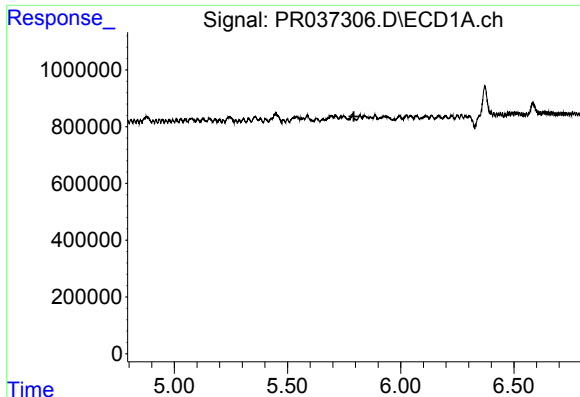

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

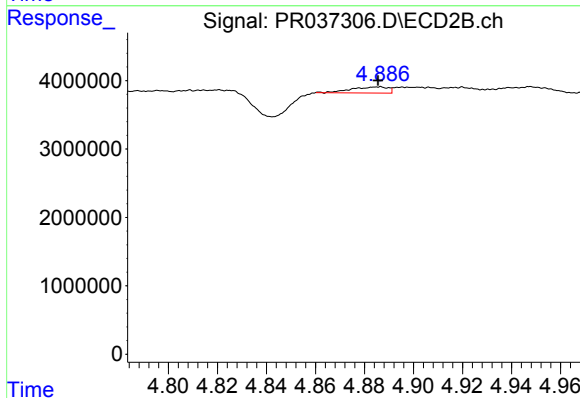


#15 AR-1232-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 935631
Conc: 13.71 ng/ml

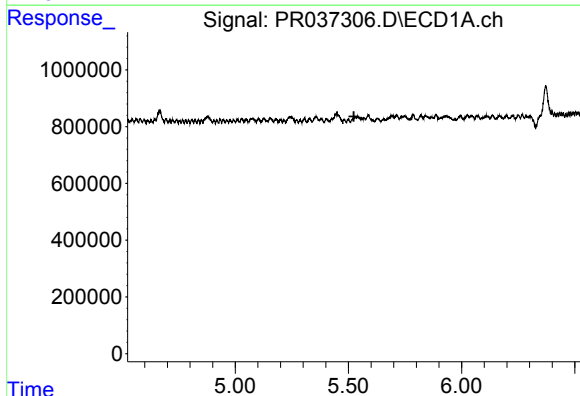


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

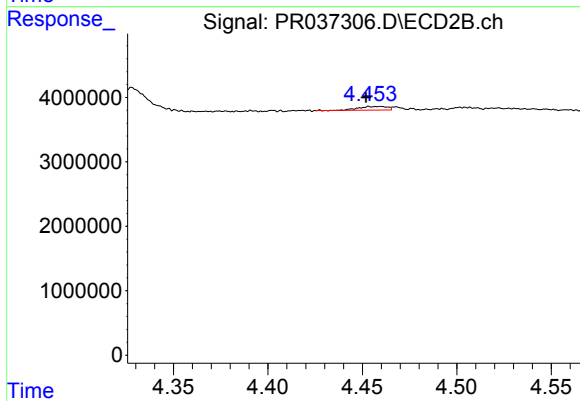

#16 AR-1242-1


R.T.: 4.454 min
Delta R.T.: 0.002 min
Response: 604742
Conc: 4.13 ng/ml

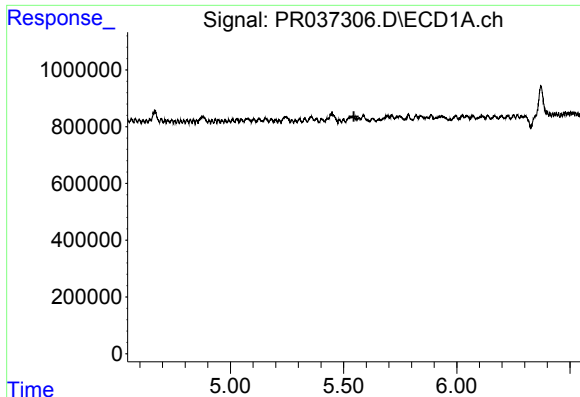

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

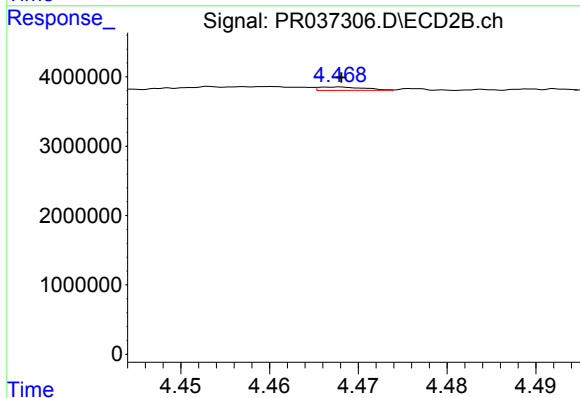


#17 AR-1242-2

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 178923
Conc: 0.78 ng/ml

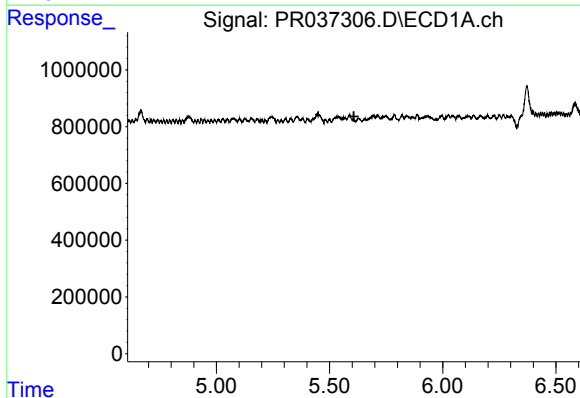


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

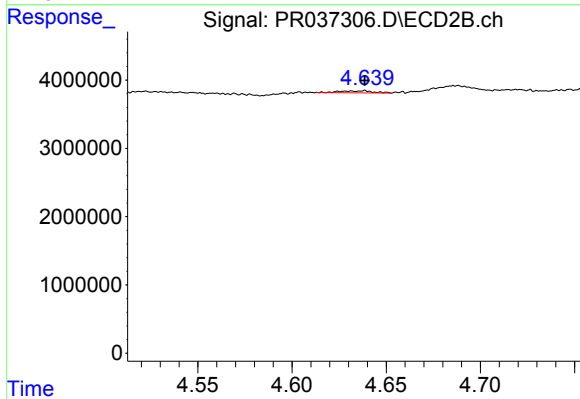

#18 AR-1242-3


R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 357506
Conc: 3.09 ng/ml

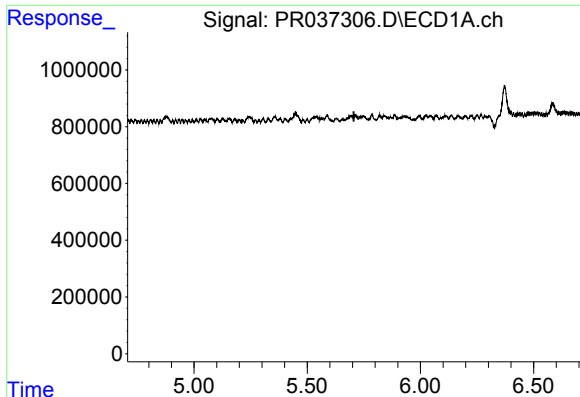

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

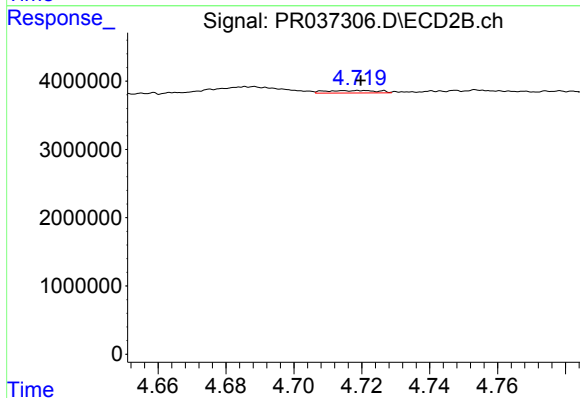


#19 AR-1242-4

R.T.: 4.715 min
Delta R.T.: -0.005 min
Response: 394623
Conc: 3.59 ng/ml

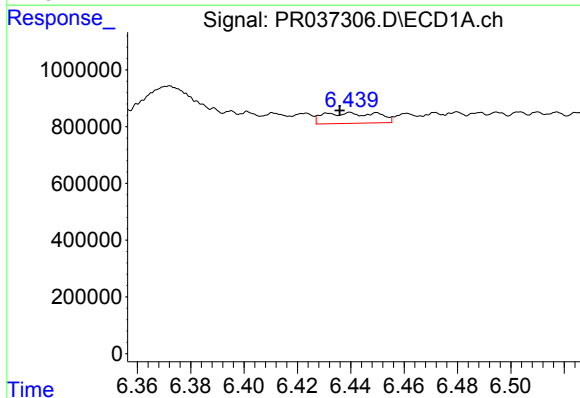


#20 AR-1242-5

R.T.: 6.440 min
Delta R.T.: 0.004 min
Response: 526085
Conc: 16.35 ng/ml

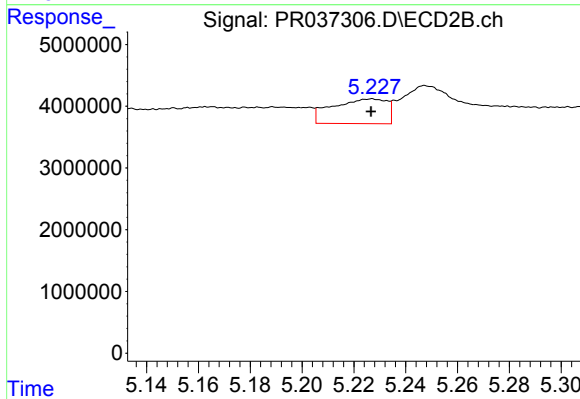

#20 AR-1242-5


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 5846358
Conc: 35.28 ng/ml

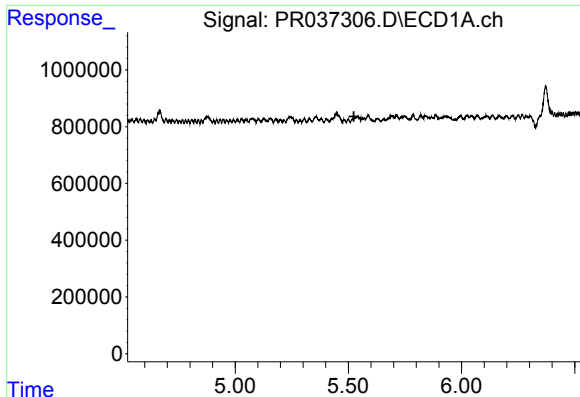

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

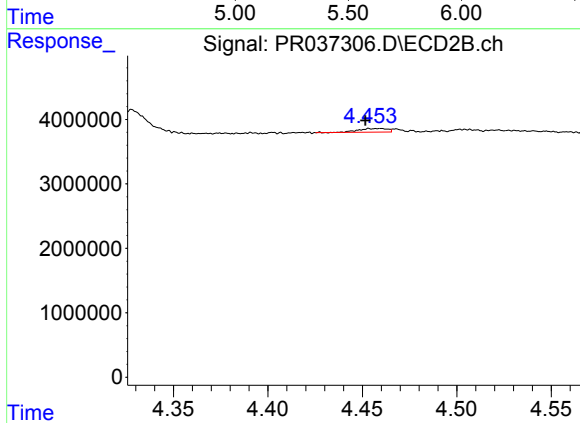


#21 AR-1248-1

R.T.: 4.454 min
Delta R.T.: 0.002 min
Response: 604742
Conc: 6.01 ng/ml

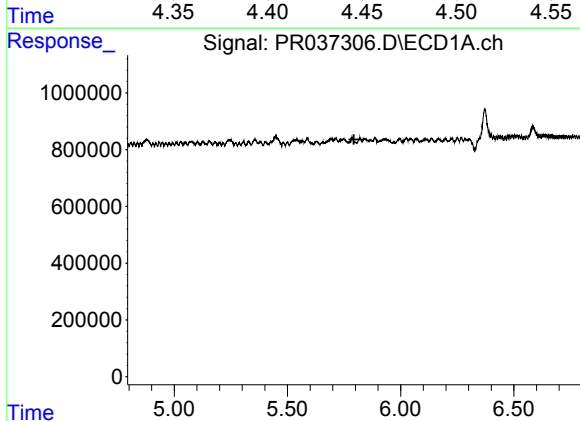


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

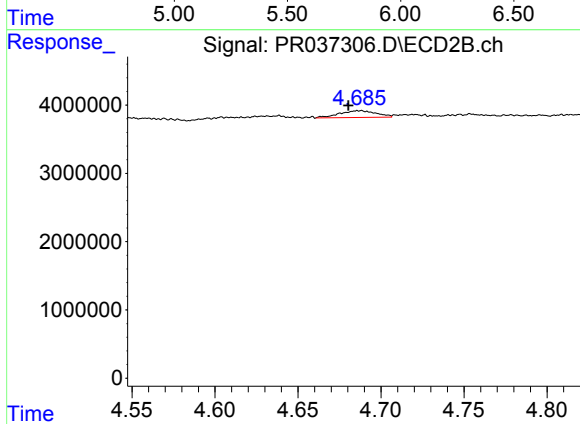

#22 AR-1248-2


R.T.: 4.688 min
Delta R.T.: 0.008 min
Response: 1549128
Conc: 11.35 ng/ml

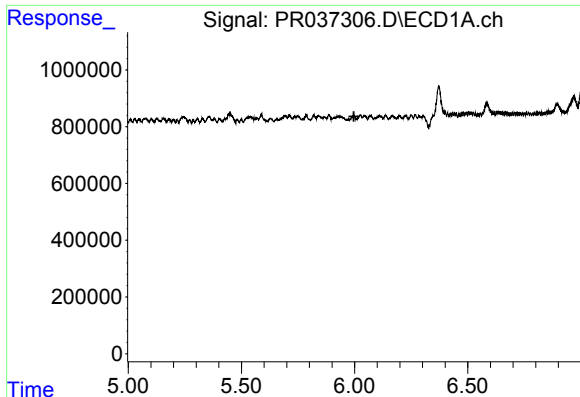

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

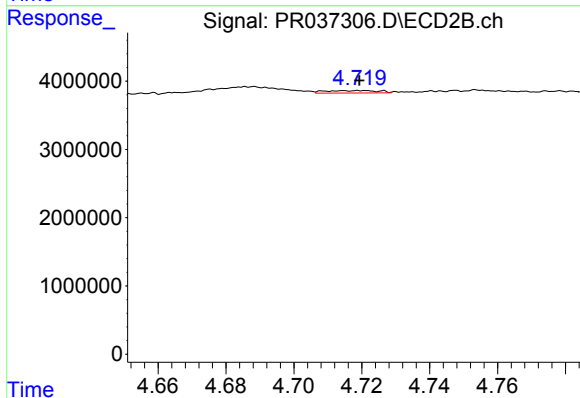


#23 AR-1248-3

R.T.: 4.715 min
Delta R.T.: -0.004 min
Response: 394623
Conc: 2.82 ng/ml

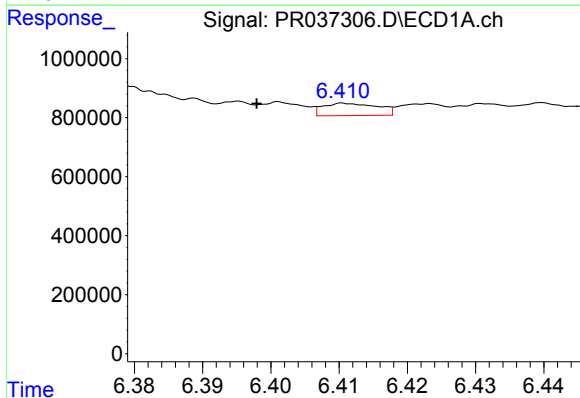


#24 AR-1248-4

R.T.: 6.411 min
Delta R.T.: 0.013 min
Response: 232570
Conc: 4.75 ng/ml

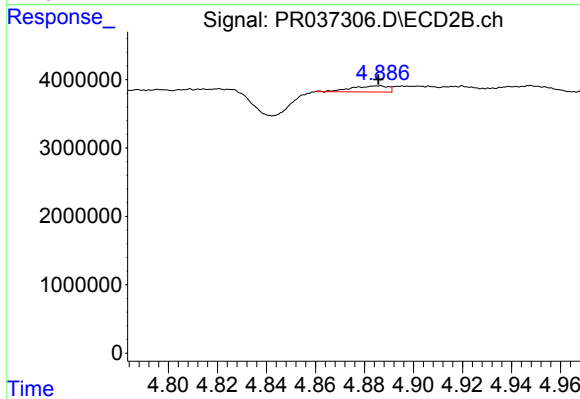

#24 AR-1248-4


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 935631
Conc: 5.26 ng/ml

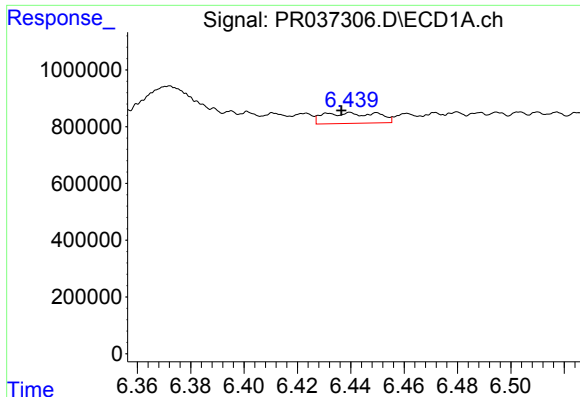

#25 AR-1248-5


R.T.: 6.440 min
Delta R.T.: 0.003 min
Response: 526085
Conc: 11.14 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

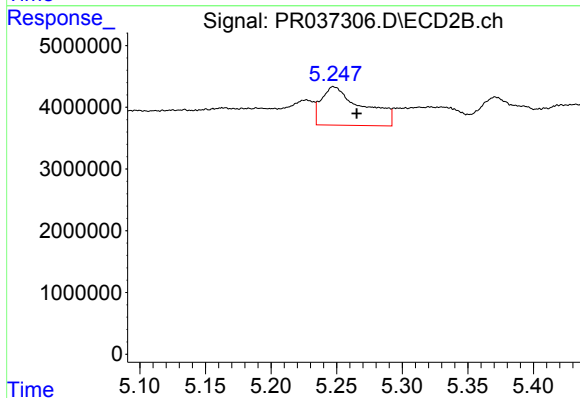


#25 AR-1248-5

R.T.: 5.248 min
Delta R.T.: -0.017 min
Response: 13668495
Conc: 69.88 ng/ml

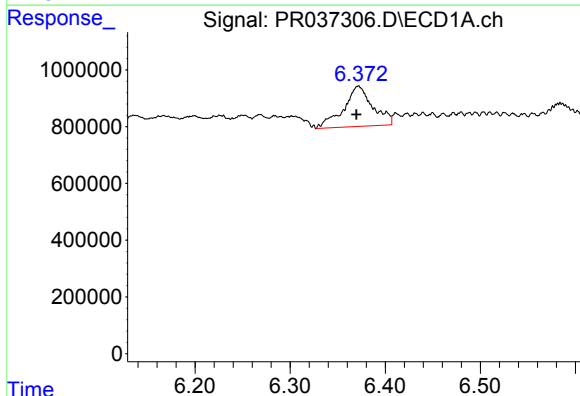


#26 AR-1254-1

R.T.: 6.372 min
Delta R.T.: 0.002 min
Response: 3039149
Conc: 55.63 ng/ml

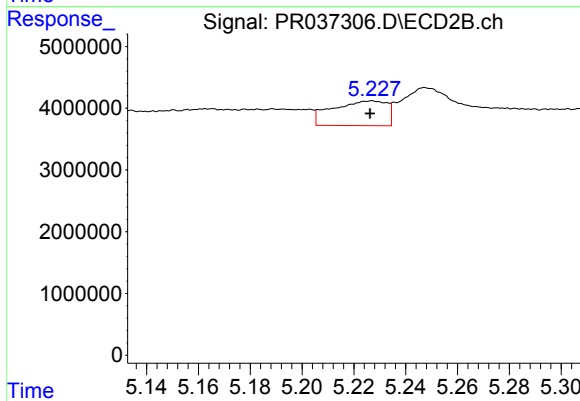

#26 AR-1254-1


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 5846358
Conc: 16.97 ng/ml

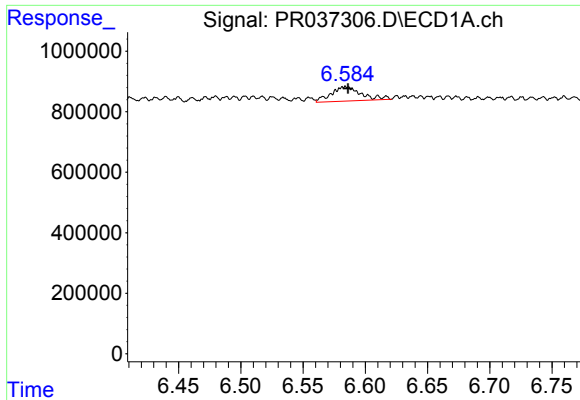

#27 AR-1254-2


R.T.: 6.584 min
Delta R.T.: -0.002 min
Response: 791883
Conc: 9.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

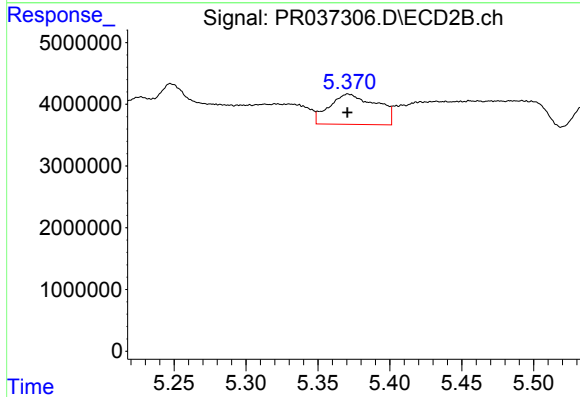


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 11270574
Conc: 37.63 ng/ml

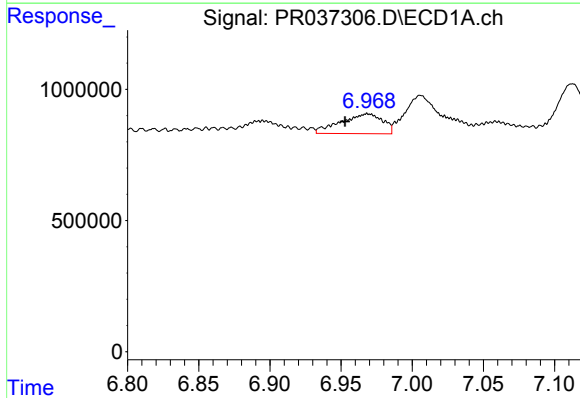


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: 0.016 min
Response: 1552662
Conc: 17.07 ng/ml

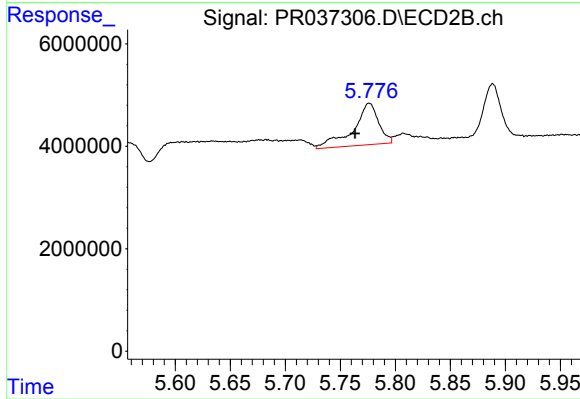

#28 AR-1254-3


R.T.: 5.776 min
Delta R.T.: 0.013 min
Response: 13027305
Conc: 27.51 ng/ml

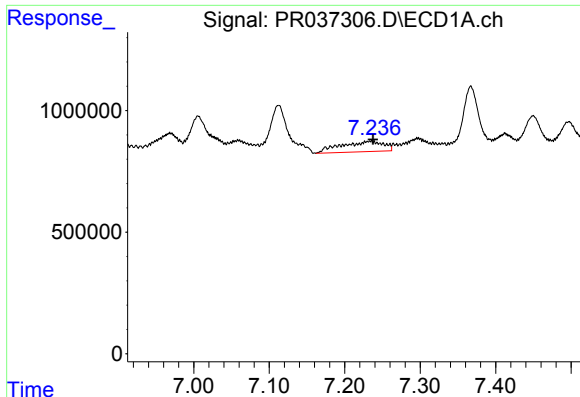

#29 AR-1254-4


R.T.: 7.235 min
Delta R.T.: -0.003 min
Response: 1690683
Conc: 25.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

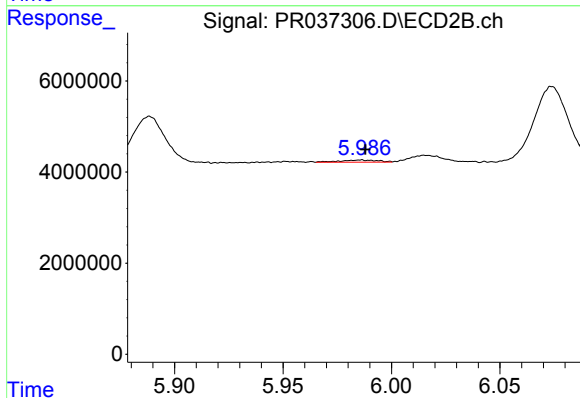


#29 AR-1254-4

R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 568869
Conc: 1.62 ng/ml

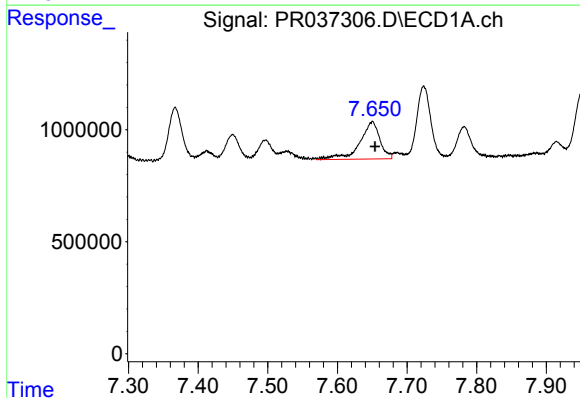


#30 AR-1254-5

R.T.: 7.650 min
Delta R.T.: -0.004 min
Response: 3341409
Conc: 46.49 ng/ml

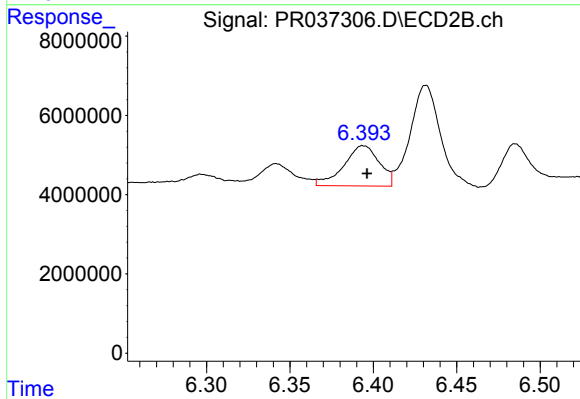

#30 AR-1254-5


R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 15067706
Conc: 34.03 ng/ml

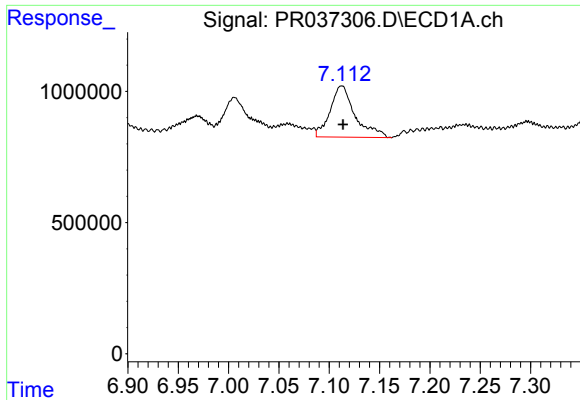

#31 AR-1260-1


R.T.: 7.112 min
Delta R.T.: -0.001 min
Response: 3373444
Conc: 51.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

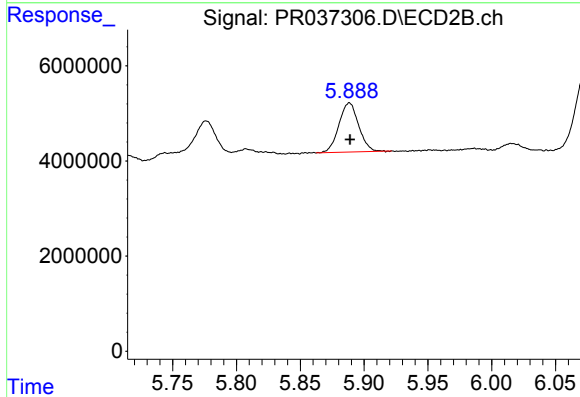


#31 AR-1260-1

R.T.: 5.888 min
Delta R.T.: 0.000 min
Response: 11128983
Conc: 38.08 ng/ml

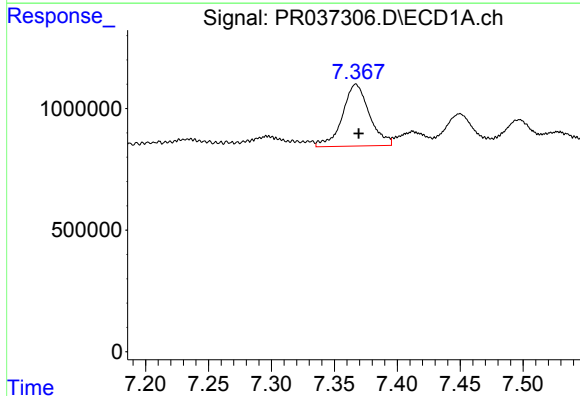


#32 AR-1260-2

R.T.: 7.367 min
Delta R.T.: -0.002 min
Response: 3785742
Conc: 47.50 ng/ml

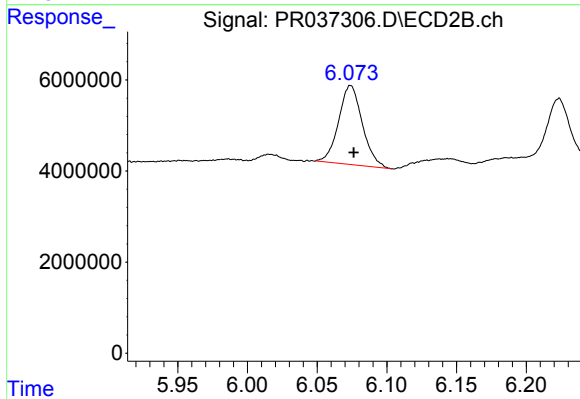

#32 AR-1260-2


R.T.: 6.074 min
Delta R.T.: -0.002 min
Response: 20375969
Conc: 44.24 ng/ml

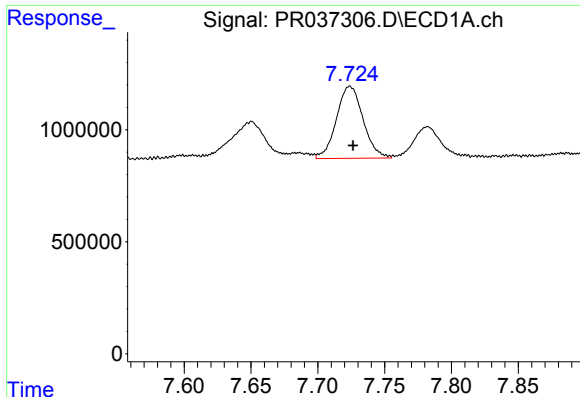

#33 AR-1260-3


R.T.: 7.724 min
Delta R.T.: -0.002 min
Response: 4468686
Conc: 71.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

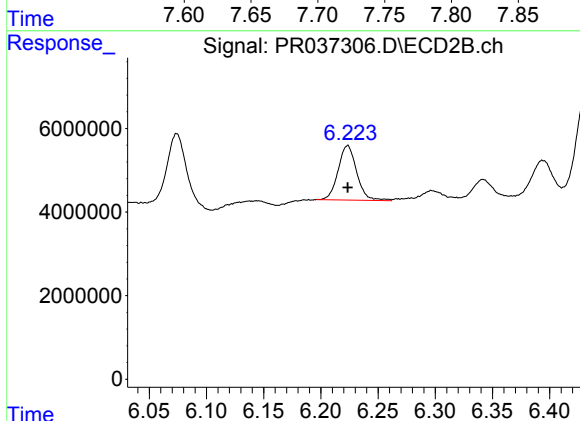


#33 AR-1260-3

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 14803828
Conc: 41.53 ng/ml

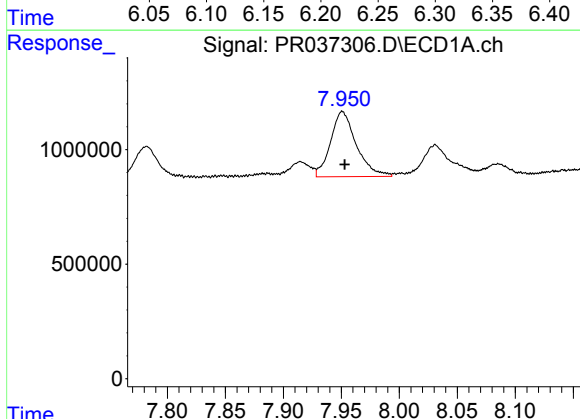


#34 AR-1260-4

R.T.: 7.951 min
Delta R.T.: -0.002 min
Response: 4405799
Conc: 59.21 ng/ml

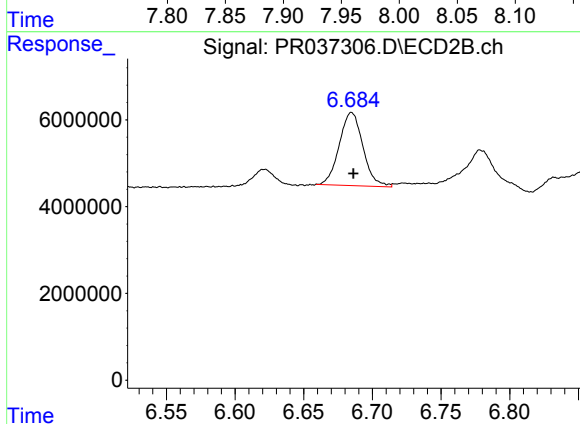

#34 AR-1260-4


R.T.: 6.685 min
Delta R.T.: -0.001 min
Response: 20212266
Conc: 66.32 ng/ml

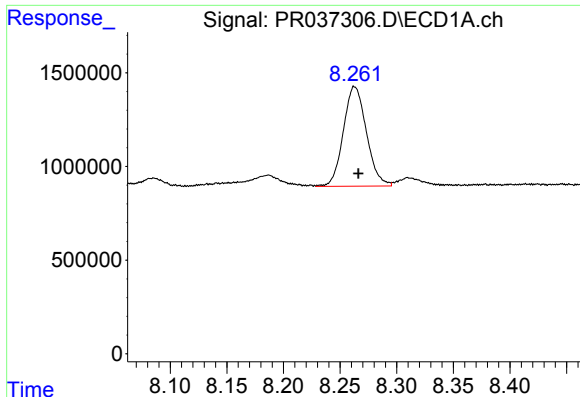

#35 AR-1260-5


R.T.: 8.263 min
Delta R.T.: -0.003 min
Response: 7571370
Conc: 52.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

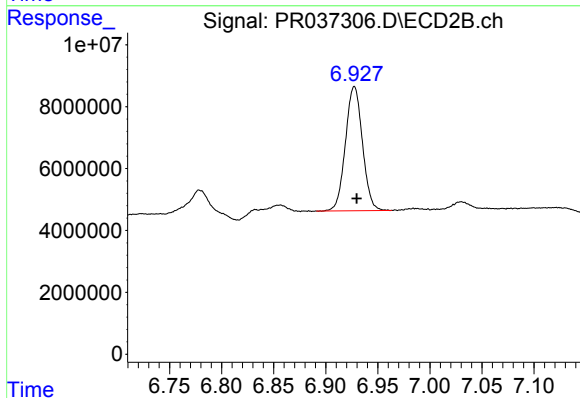


#35 AR-1260-5

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 45599977
Conc: 52.58 ng/ml

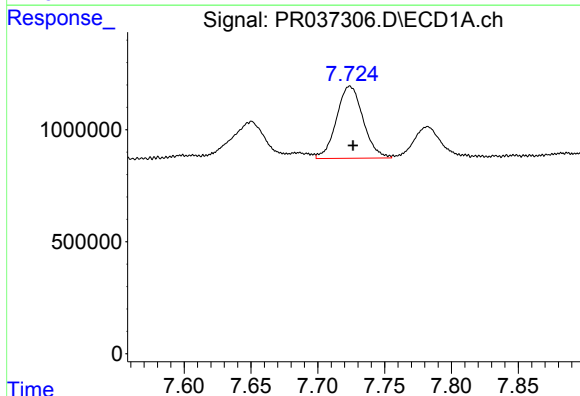


#36 AR-1262-1

R.T.: 7.724 min
Delta R.T.: -0.002 min
Response: 4468686
Conc: 42.78 ng/ml

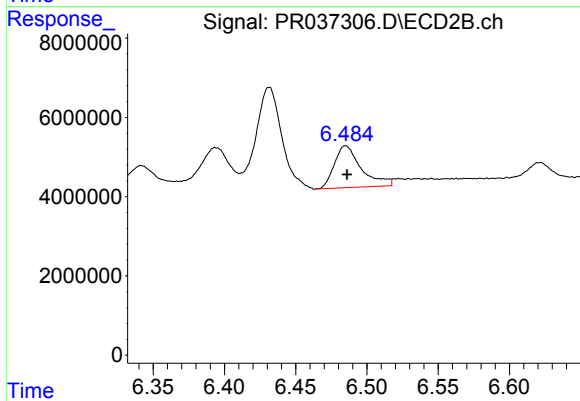

#36 AR-1262-1


R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 13904208
Conc: 55.48 ng/ml

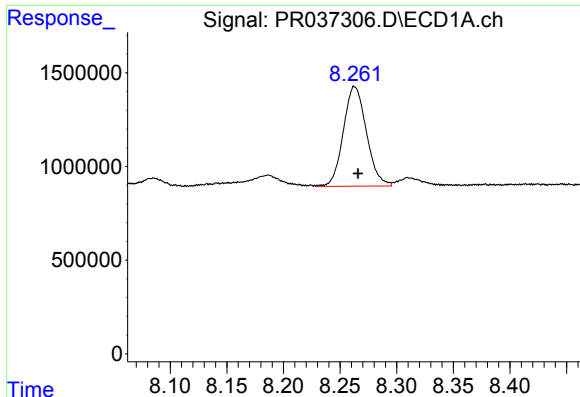

#37 AR-1262-2


R.T.: 8.263 min
Delta R.T.: -0.003 min
Response: 7571370
Conc: 38.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

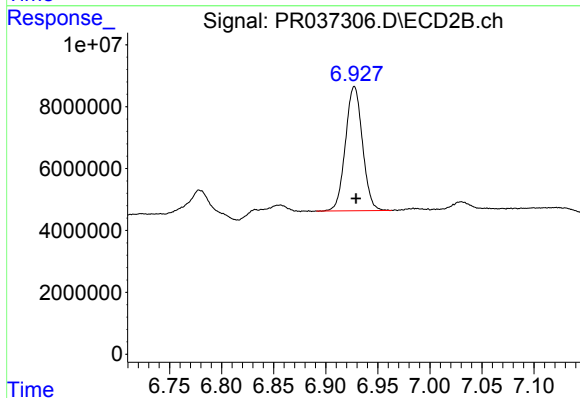


#37 AR-1262-2

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 45599977
Conc: 36.31 ng/ml

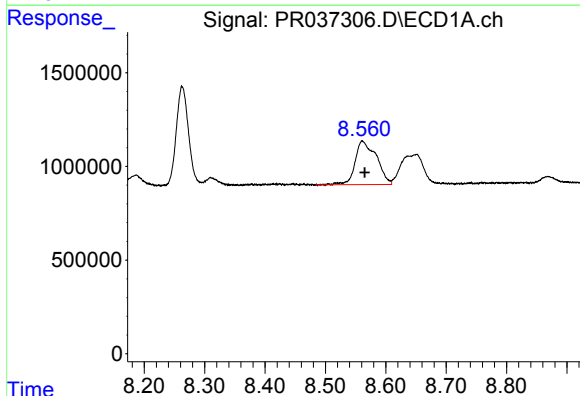


#38 AR-1262-3

R.T.: 8.561 min
Delta R.T.: -0.004 min
Response: 5700272
Conc: 43.34 ng/ml

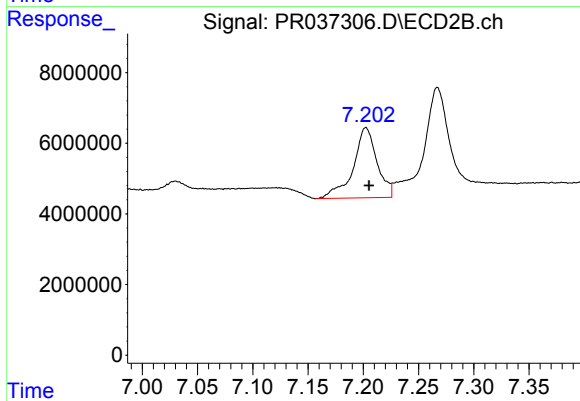

#38 AR-1262-3


R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 29868300
Conc: 54.48 ng/ml

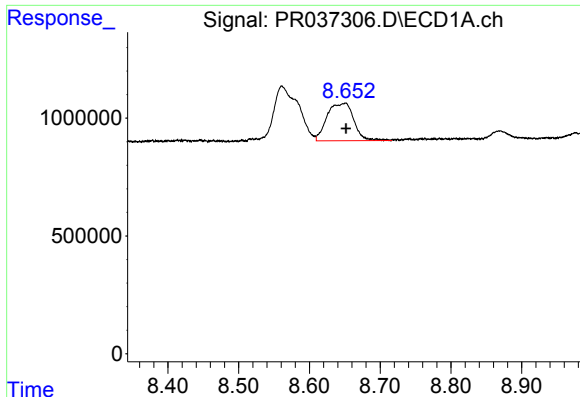

#39 AR-1262-4


R.T.: 8.651 min
Delta R.T.: 0.000 min
Response: 4177900
Conc: 42.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

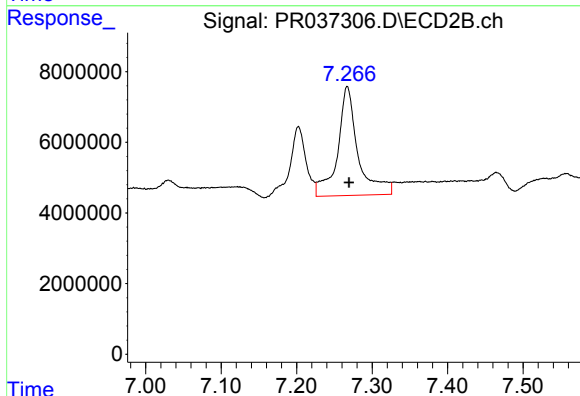


#39 AR-1262-4

R.T.: 7.267 min
Delta R.T.: -0.002 min
Response: 58274700
Conc: 64.92 ng/ml

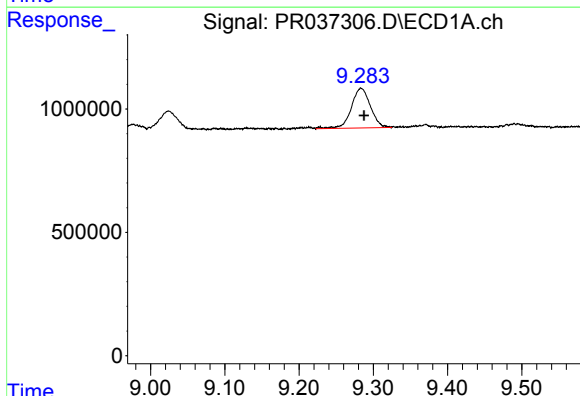


#40 AR-1262-5

R.T.: 9.284 min
Delta R.T.: -0.004 min
Response: 2887615
Conc: 41.82 ng/ml

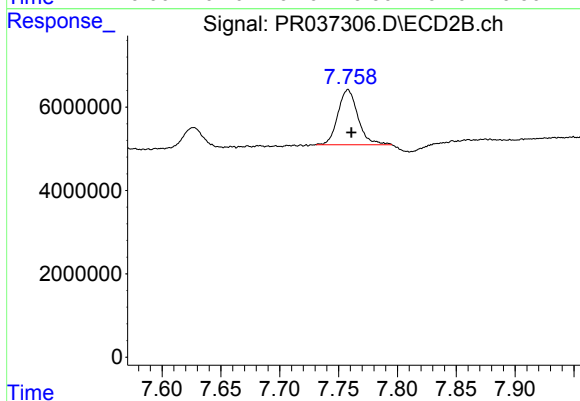

#40 AR-1262-5


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 15652753
Conc: 40.91 ng/ml

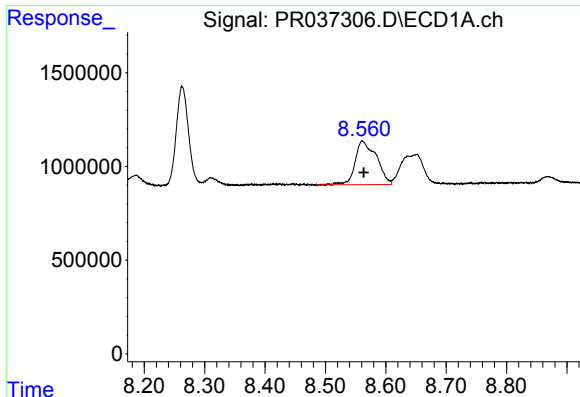

#41 AR-1268-1


R.T.: 8.561 min
Delta R.T.: -0.003 min
Response: 5700272
Conc: 31.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

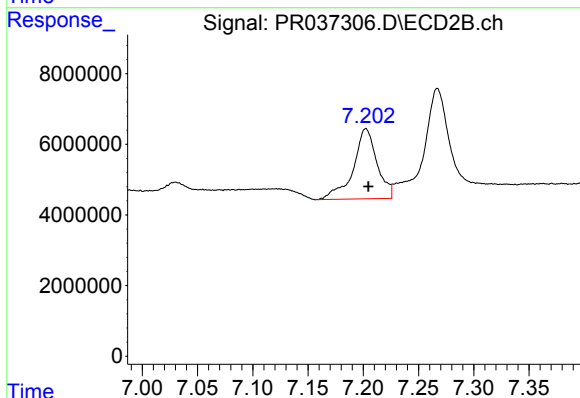


#41 AR-1268-1

R.T.: 7.202 min
Delta R.T.: -0.002 min
Response: 29868300
Conc: 24.26 ng/ml

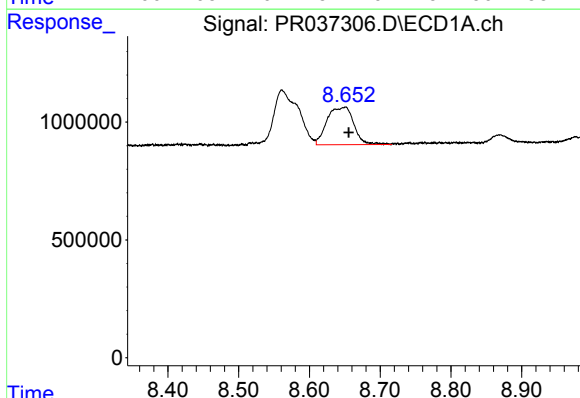


#42 AR-1268-2

R.T.: 8.651 min
Delta R.T.: -0.004 min
Response: 4177900
Conc: 25.40 ng/ml

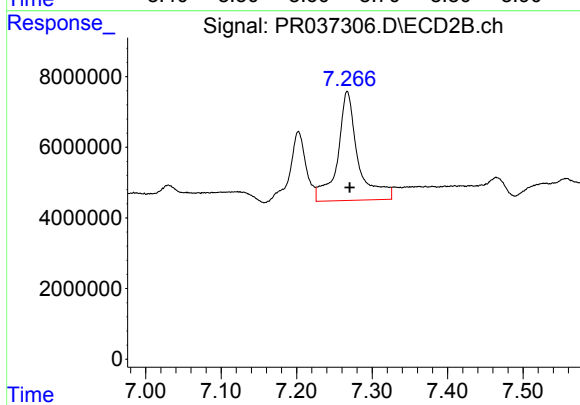

#42 AR-1268-2


R.T.: 7.267 min
Delta R.T.: -0.003 min
Response: 58274700
Conc: 55.03 ng/ml

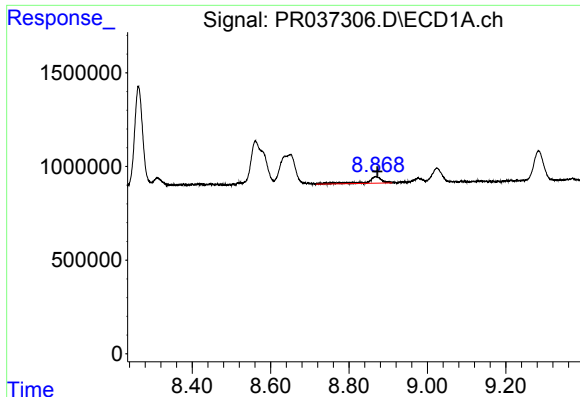

#43 AR-1268-3


R.T.: 8.869 min
Delta R.T.: -0.003 min
Response: 899165
Conc: 6.50 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

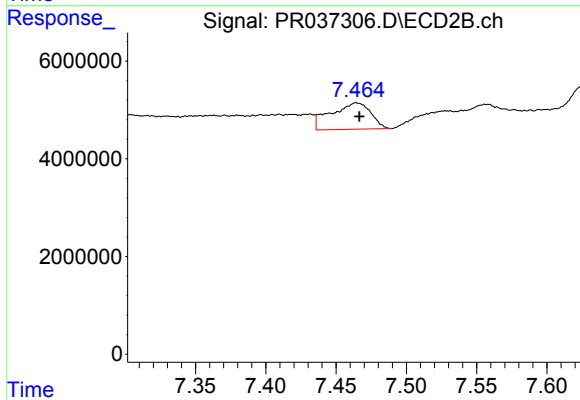


#43 AR-1268-3

R.T.: 7.465 min
Delta R.T.: -0.002 min
Response: 10688916
Conc: 12.06 ng/ml

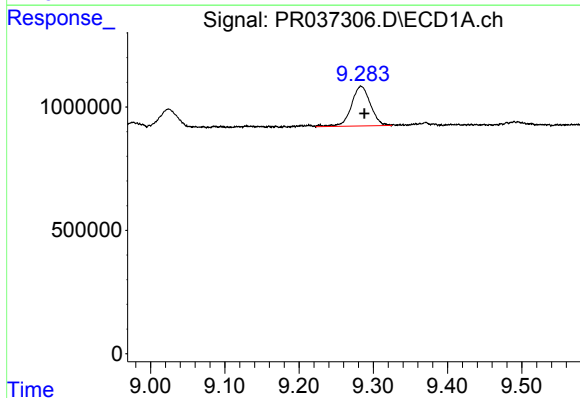


#44 AR-1268-4

R.T.: 9.284 min
Delta R.T.: -0.004 min
Response: 2887615
Conc: 46.29 ng/ml

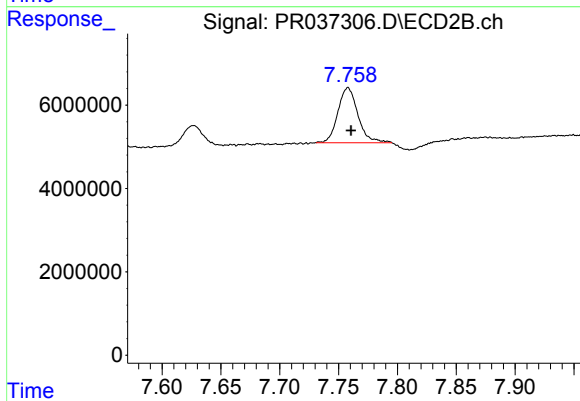

#44 AR-1268-4


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 15652753
Conc: 43.15 ng/ml

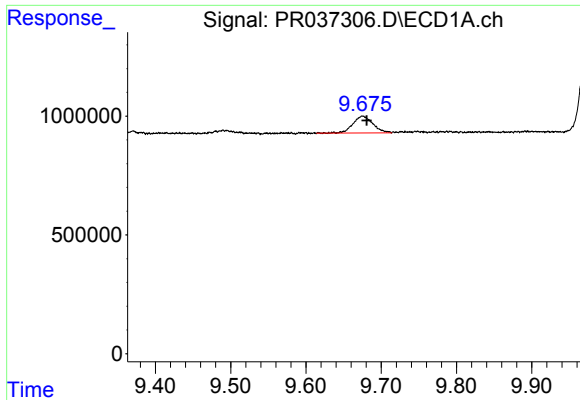

#45 AR-1268-5

R.T.: 9.675 min
Delta R.T.: -0.005 min
Response: 1305461
Conc: 2.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

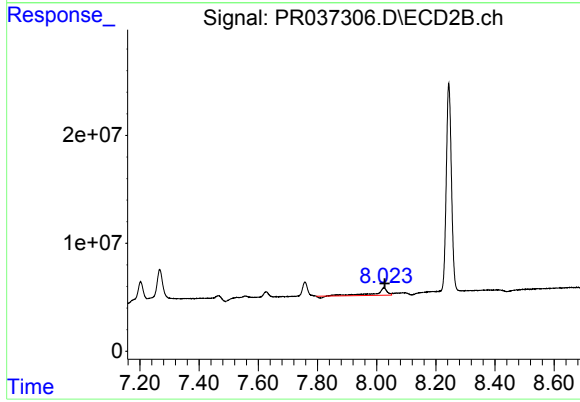

#45 AR-1268-5

R.T.: 8.024 min
Delta R.T.: -0.003 min
Response: 18611120
Conc: 7.32 ng/ml