

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 21:22
 Operator : SM\SJ
 Sample : K1560-16
 Misc : AR1268 MDL 25PPB
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:56:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.362	3.408	32515158	127.5E6	25.991	26.580
2)	SA Decachlor...	9.992	8.245	43909493	219.0E6	33.200	37.599
Target Compounds							
3)	L1 AR-1016-1	0.000	4.454	0	135350	N.D.	0.743 #
4)	L1 AR-1016-2	0.000	4.454	0	135350	N.D.	0.480 #
5)	L1 AR-1016-3	0.000	4.611	0	20883	N.D.	0.145 #
6)	L1 AR-1016-4	0.000	4.690	0	1261204	N.D.	11.400 #
7)	L1 AR-1016-5	0.000	4.885	0	6127976	N.D.	40.313 #
8)	L2 AR-1221-1	0.000	3.603	0	28097	N.D.	0.552 #
9)	L2 AR-1221-2	4.666	3.697	550407	1882094	60.859	50.681
10)	L2 AR-1221-3	4.666	3.763	550407	55353	17.958	0.452 #
11)	L3 AR-1232-1	4.666	3.763	550407	55353	18.817	0.473 #
12)	L3 AR-1232-2	0.000	4.454	0	135350	N.D.	0.979 #
13)	L3 AR-1232-3	0.000	4.611	0	20883	N.D.	0.297 #
14)	L3 AR-1232-4	0.000	4.722	0	276793	N.D.	4.639 #
15)	L3 AR-1232-5	0.000	4.885	0	6127976	N.D.	89.795 #
16)	L4 AR-1242-1	0.000	4.454	0	135350	N.D.	0.924 #
17)	L4 AR-1242-2	0.000	4.454	0	135350	N.D.	0.593 #
18)	L4 AR-1242-3	0.000	4.611	0	20883	N.D.	0.181 #
19)	L4 AR-1242-4	0.000	4.722	0	276793	N.D.	2.518 #
20)	L4 AR-1242-5	6.441	5.249	537716	56452976	16.710	340.695 #
21)	L5 AR-1248-1	0.000	4.454	0	135350	N.D.	1.345 #
22)	L5 AR-1248-2	0.000	4.690	0	1261204	N.D.	9.241 #
23)	L5 AR-1248-3	0.000	4.722	0	276793	N.D.	1.977 #
24)	L5 AR-1248-4	6.420	4.885	871748	6127976	17.807	34.434 #
25)	L5 AR-1248-5	6.441	5.249	537716	56452976	11.383	288.596 #
26)	L6 AR-1254-1	6.373	5.249	7865452	56452976	143.974	163.882
27)	L6 AR-1254-2	6.526	5.381	450858	26560828	5.261	88.683 #
28)	L6 AR-1254-3	6.969	5.774	12076442	12133512	132.761	25.619 #
29)	L6 AR-1254-4	7.207	5.978	1834276	382737	27.374	1.092 #
30)	L6 AR-1254-5	7.723	6.398	2330710	2577480	32.425	5.821 #
31)	L7 AR-1260-1	0.000	5.890	0	255622	N.D.	0.875 #
32)	L7 AR-1260-2	0.000	6.068	0	12949267	N.D.	28.115 #
33)	L7 AR-1260-3	7.723	6.226	2330710	384340	37.246	1.078 #
34)	L7 AR-1260-4	7.965	6.678	1780974	10268305	23.936	33.693 #
35)	L7 AR-1260-5	8.262	6.927	954676	5312707	6.601	6.126
36)	L8 AR-1262-1	7.723	6.491	2330710	4068672	22.313	16.234 #
37)	L8 AR-1262-2	8.262	6.927	954676	5312707	4.911	4.230
38)	L8 AR-1262-3	8.560	7.205	7499356	77486582	57.025	141.330 #
39)	L8 AR-1262-4	8.653	7.267	6978738	202.1E6	71.046	225.137 #
40)	L8 AR-1262-5	9.284	7.758	2760717	13992109	39.987	36.569
41)	L9 AR-1268-1	8.560	7.205	7499356	77486582	41.874	62.945 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
 Data File : PR037307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 21:22
 Operator : SM\SJ
 Sample : K1560-16
 Misc : AR1268 MDL 25PPB
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:56:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.653	7.267	6978738	202.1E6	42.425	190.848 #
43) L9	AR-1268-3	8.868	7.465	6436485	38287172	46.494	43.202
44) L9	AR-1268-4	9.284	7.758	2760717	13992109	44.252	38.569
45) L9	AR-1268-5	9.676	8.025	17779322	98556529	39.001	38.738



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042219\
Data File : PR037307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 21:22
Operator : SM\SJ
Sample : K1560-16
Misc : AR1268 MDL 25PPB
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:56:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

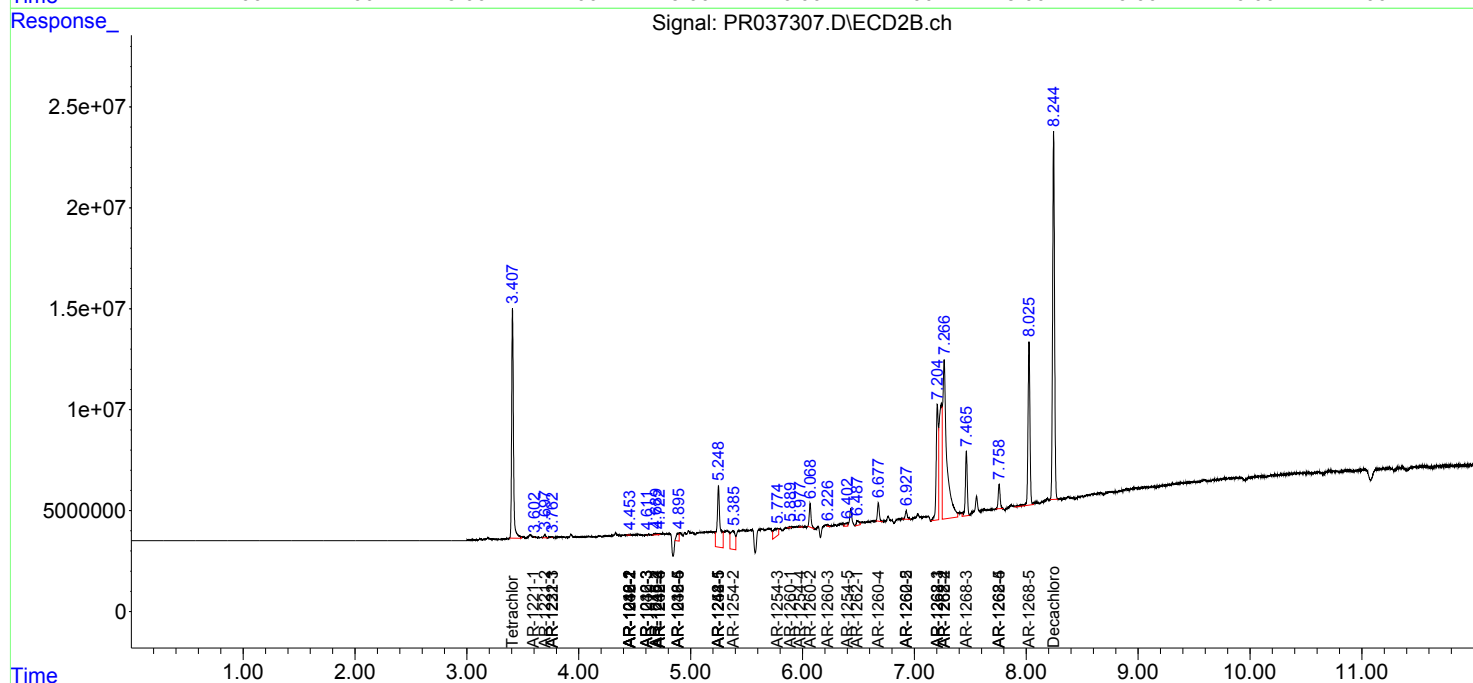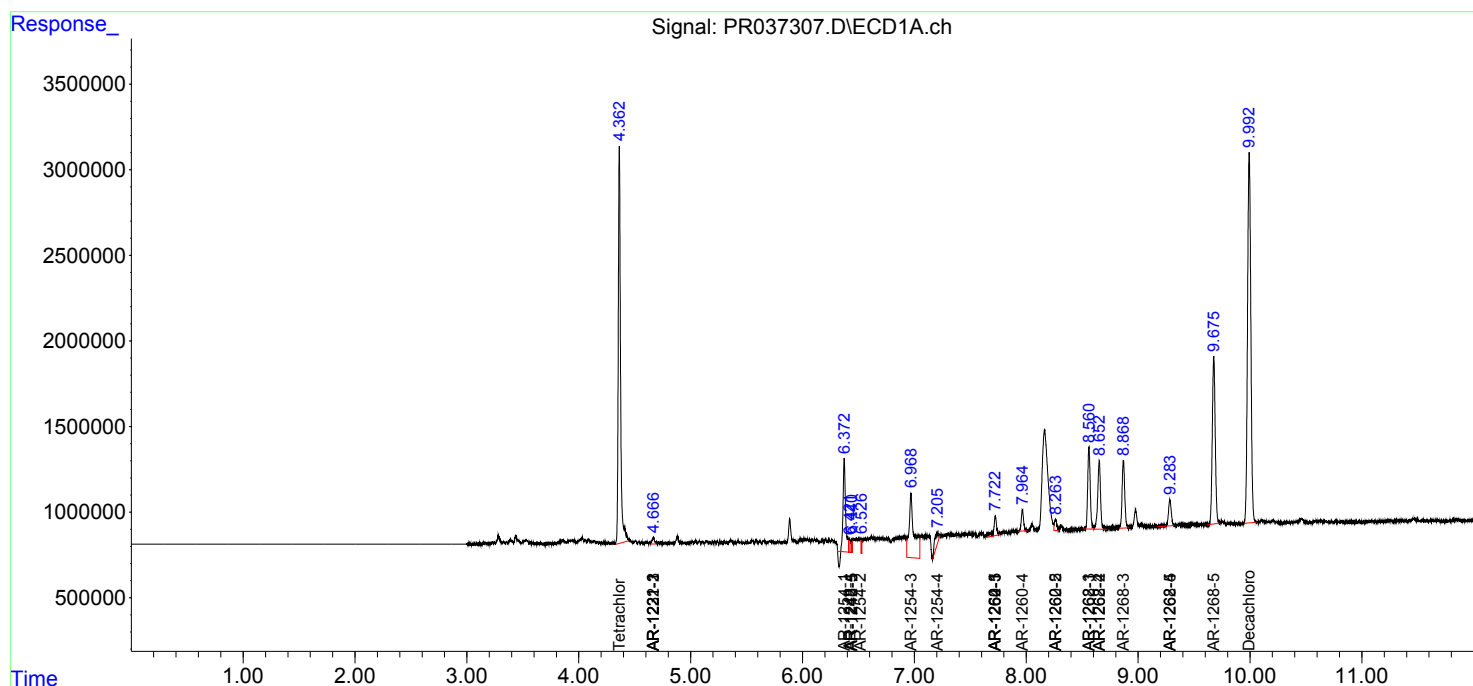


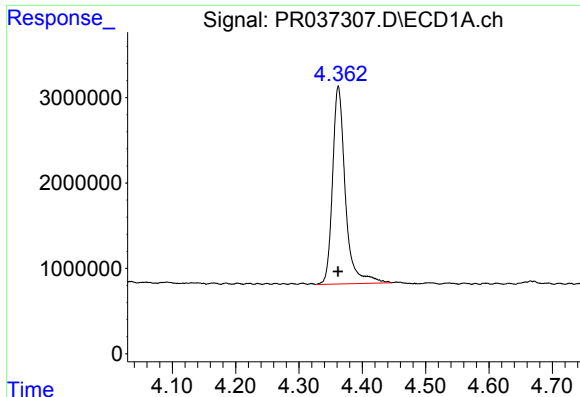

#1 Tetrachloro-m-xylene


R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 32515158
Conc: 25.99 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

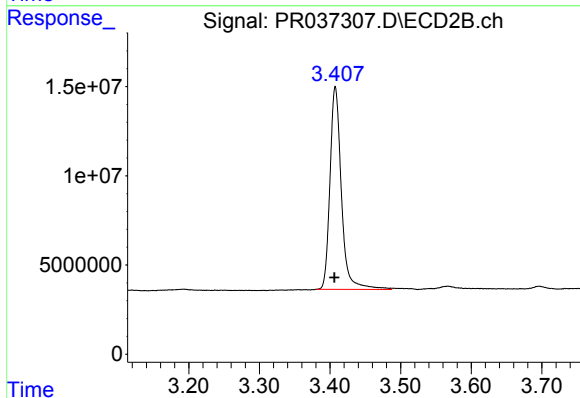


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: 0.001 min
Response: 127463290
Conc: 26.58 ng/ml

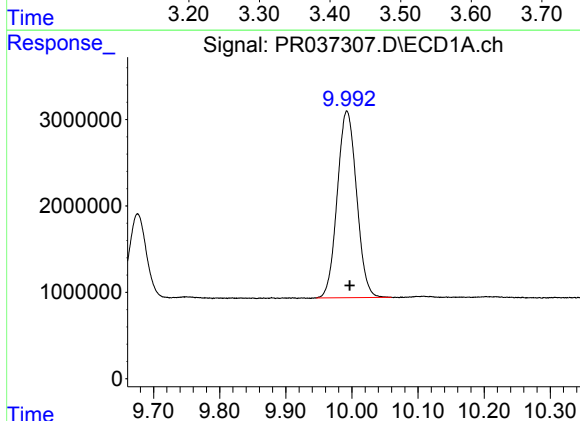


#2 Decachlorobiphenyl

R.T.: 9.992 min
Delta R.T.: -0.004 min
Response: 43909493
Conc: 33.20 ng/ml

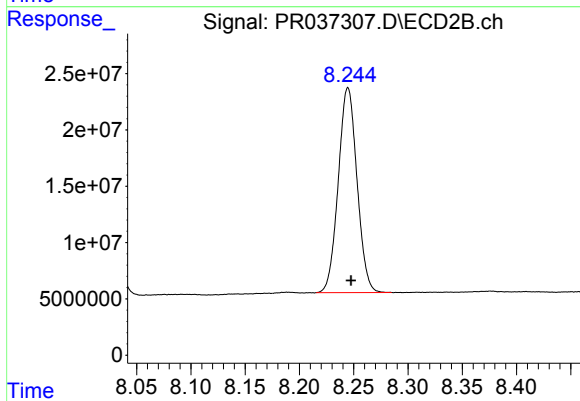

#2 Decachlorobiphenyl


R.T.: 8.245 min
Delta R.T.: -0.003 min
Response: 218988764
Conc: 37.60 ng/ml

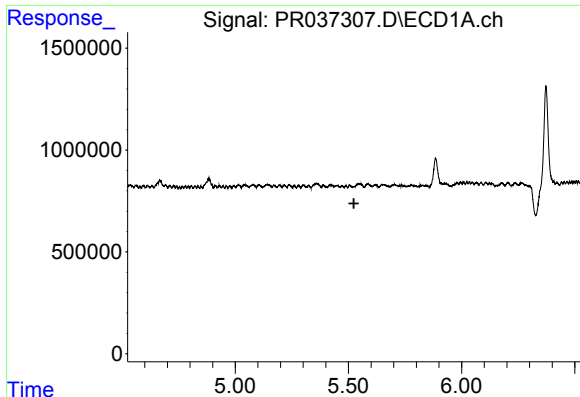

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

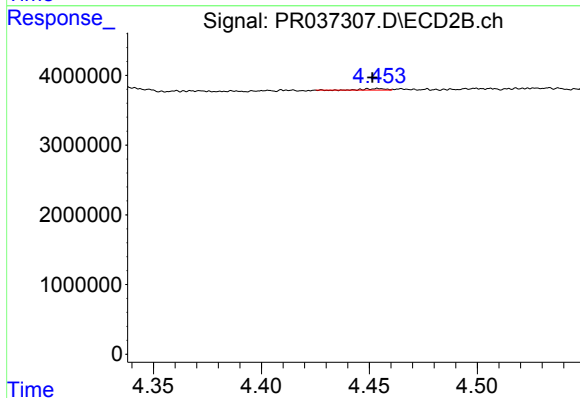


#3 AR-1016-1

R.T.: 4.454 min
Delta R.T.: 0.003 min
Response: 135350
Conc: 0.74 ng/ml

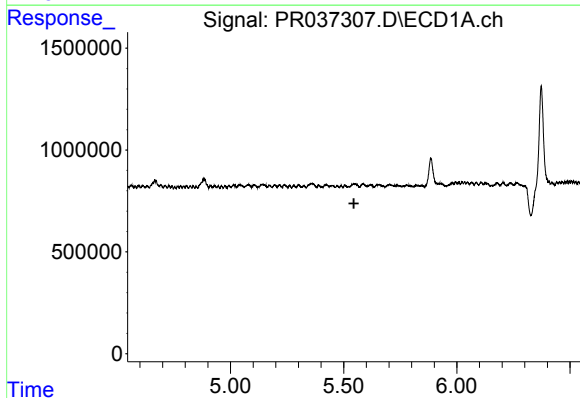


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

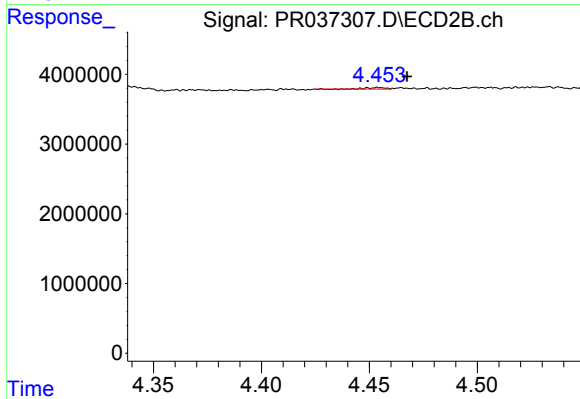

#4 AR-1016-2


R.T.: 4.454 min
Delta R.T.: -0.013 min
Response: 135350
Conc: 0.48 ng/ml

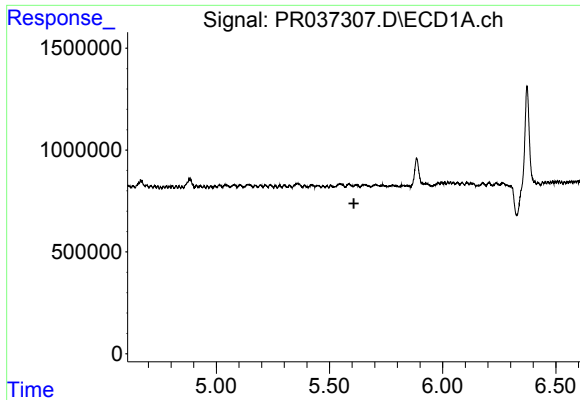

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

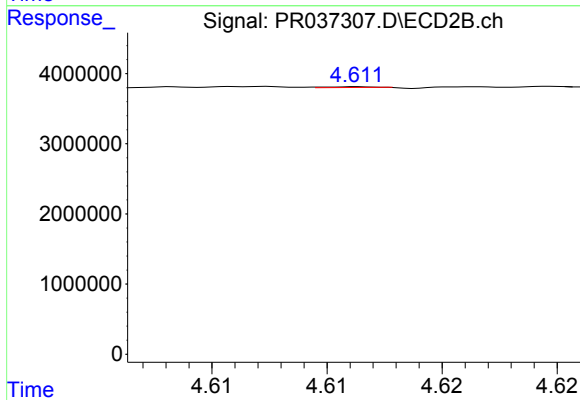


#5 AR-1016-3

R.T.: 4.611 min
Delta R.T.: -0.027 min
Response: 20883
Conc: 0.15 ng/ml

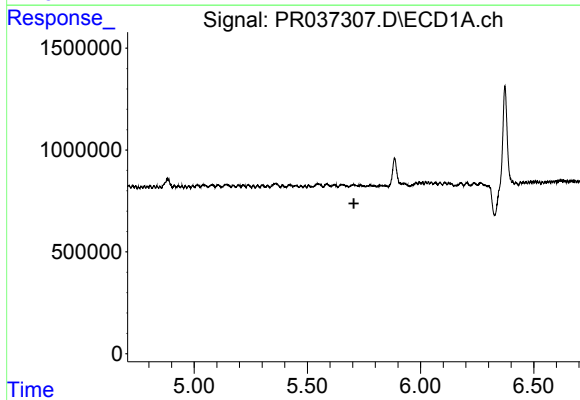


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

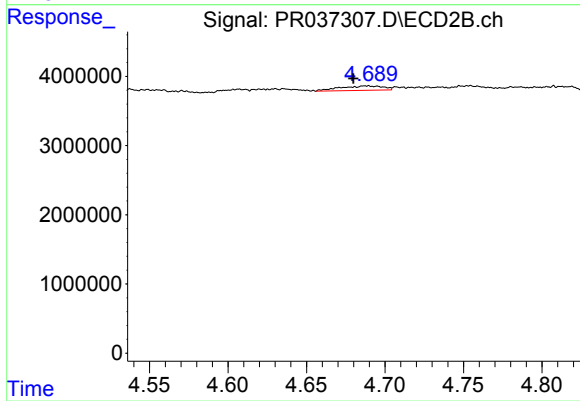

#6 AR-1016-4


R.T.: 4.690 min
Delta R.T.: 0.010 min
Response: 1261204
Conc: 11.40 ng/ml

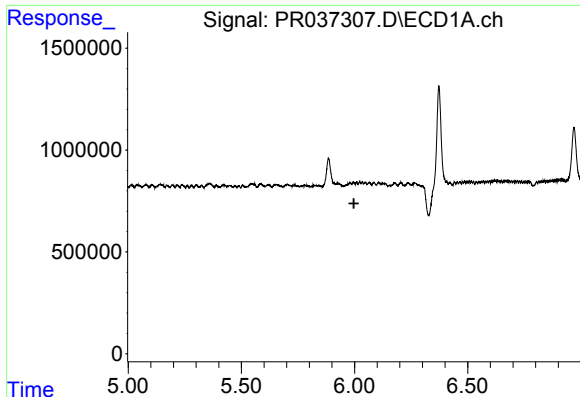

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

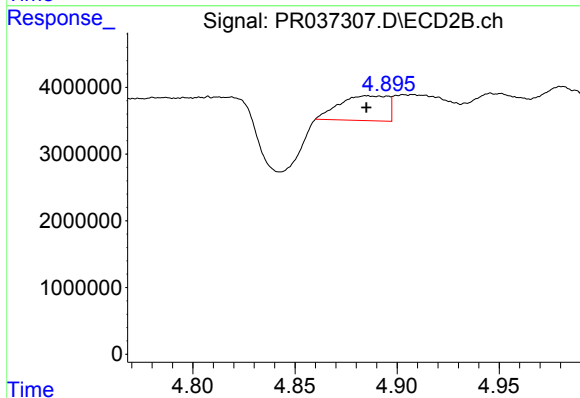


#7 AR-1016-5

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 6127976
Conc: 40.31 ng/ml

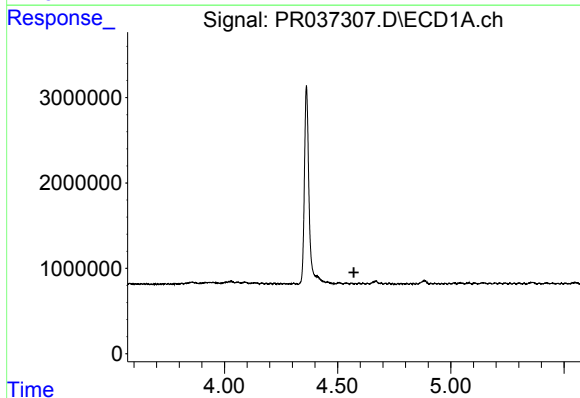


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

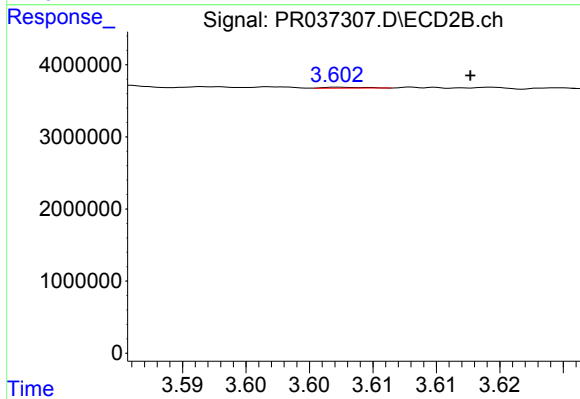

#8 AR-1221-1


R.T.: 3.603 min
Delta R.T.: -0.010 min
Response: 28097
Conc: 0.55 ng/ml

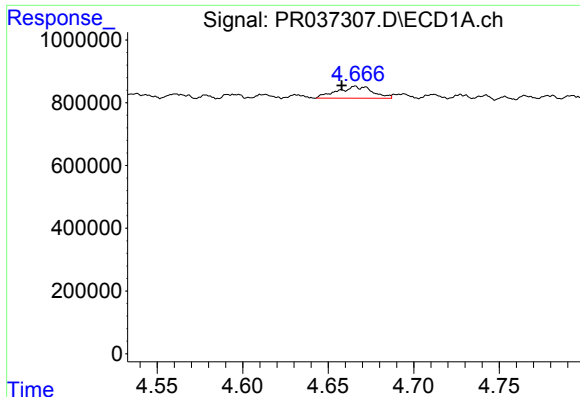

#9 AR-1221-2


R.T.: 4.666 min
Delta R.T.: 0.008 min
Response: 550407
Conc: 60.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

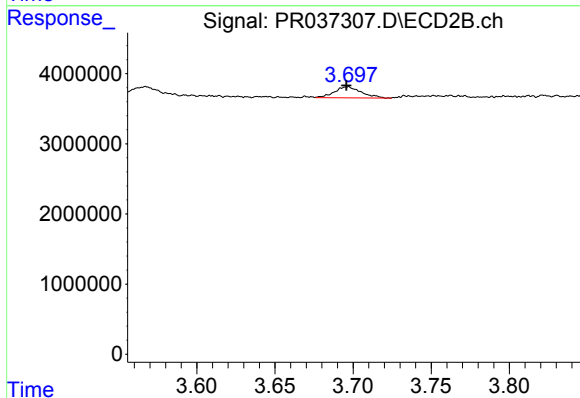


#9 AR-1221-2

R.T.: 3.697 min
Delta R.T.: 0.001 min
Response: 1882094
Conc: 50.68 ng/ml

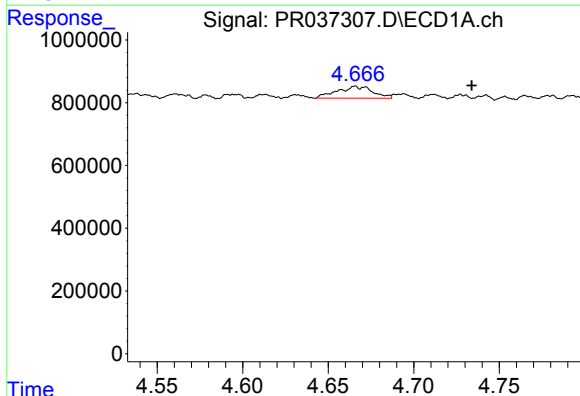


#10 AR-1221-3

R.T.: 4.666 min
Delta R.T.: -0.068 min
Response: 550407
Conc: 17.96 ng/ml

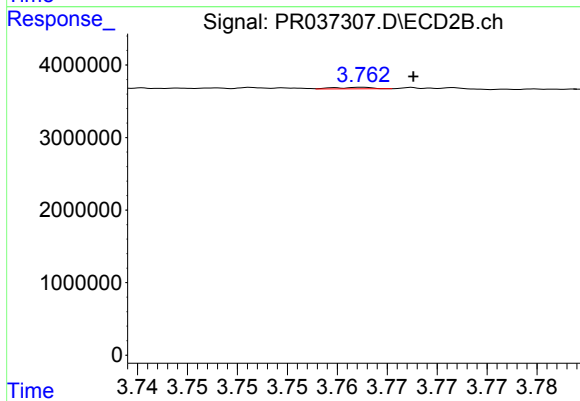

#10 AR-1221-3


R.T.: 3.763 min
Delta R.T.: -0.005 min
Response: 55353
Conc: 0.45 ng/ml

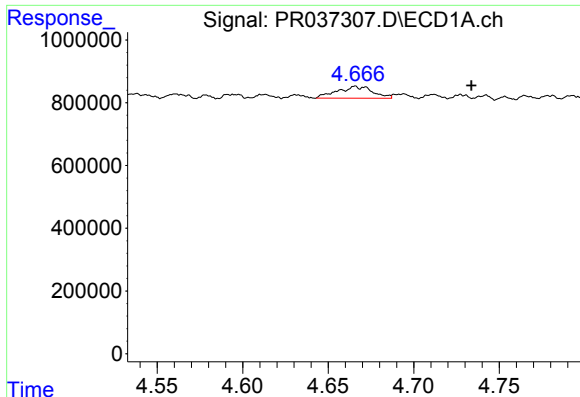

#11 AR-1232-1


R.T.: 4.666 min
Delta R.T.: -0.068 min
Response: 550407
Conc: 18.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

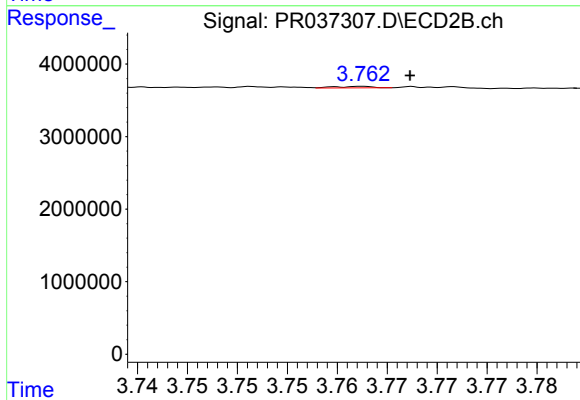


#11 AR-1232-1

R.T.: 3.763 min
Delta R.T.: -0.005 min
Response: 55353
Conc: 0.47 ng/ml

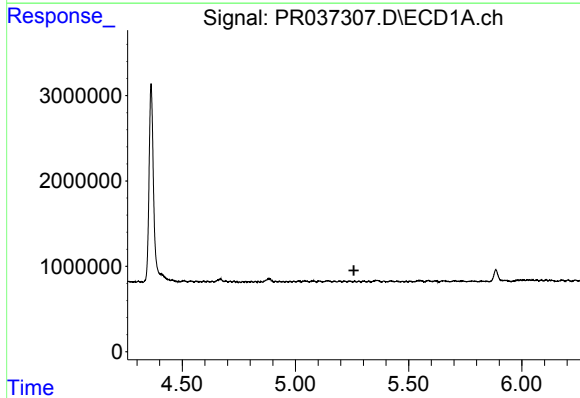


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

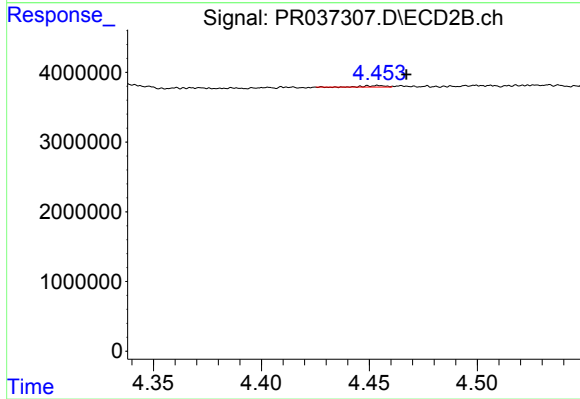

#12 AR-1232-2


R.T.: 4.454 min
Delta R.T.: -0.013 min
Response: 135350
Conc: 0.98 ng/ml

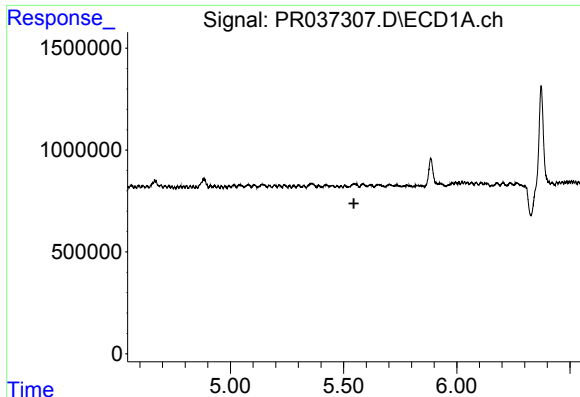

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

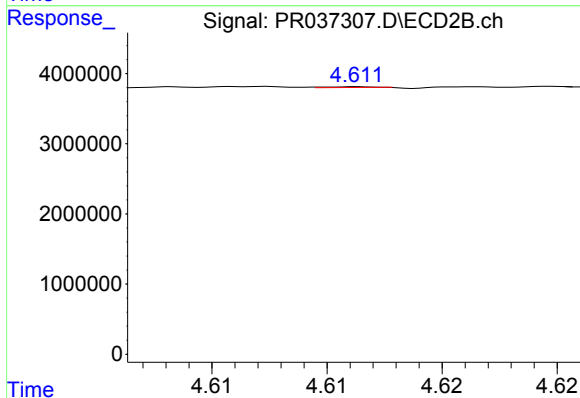


#13 AR-1232-3

R.T.: 4.611 min
Delta R.T.: -0.026 min
Response: 20883
Conc: 0.30 ng/ml

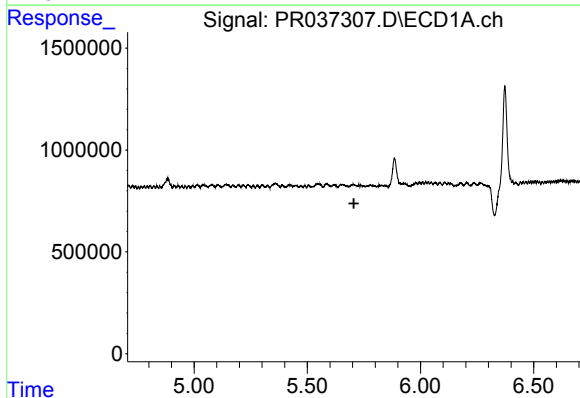


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

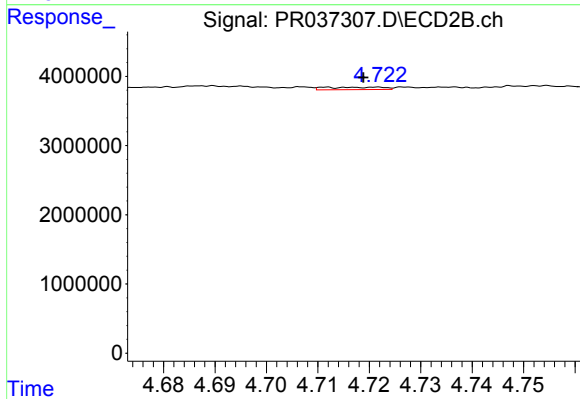

#14 AR-1232-4


R.T.: 4.722 min
Delta R.T.: 0.003 min
Response: 276793
Conc: 4.64 ng/ml

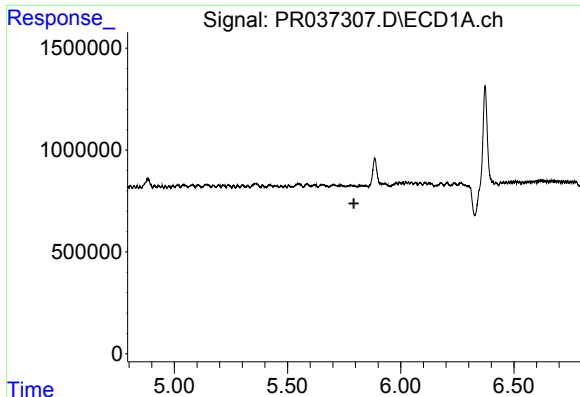

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

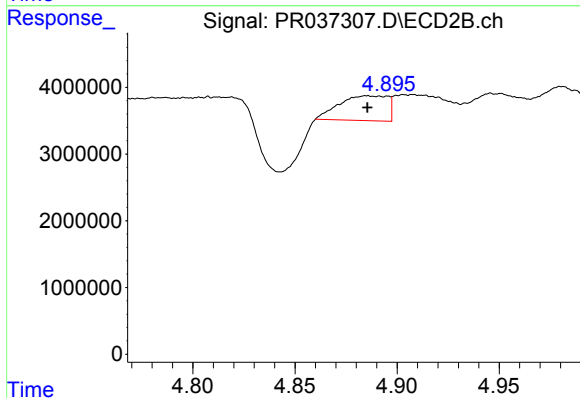


#15 AR-1232-5

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 6127976
Conc: 89.80 ng/ml

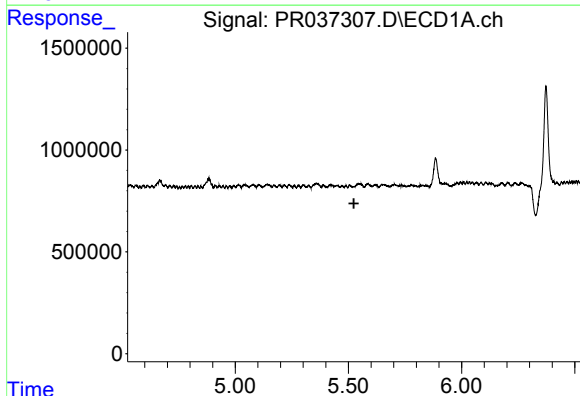


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

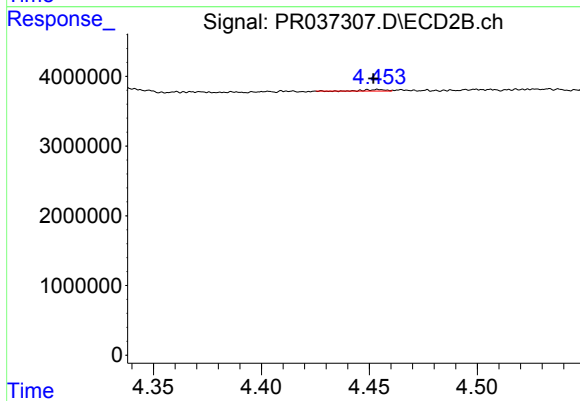

#16 AR-1242-1


R.T.: 4.454 min
Delta R.T.: 0.002 min
Response: 135350
Conc: 0.92 ng/ml

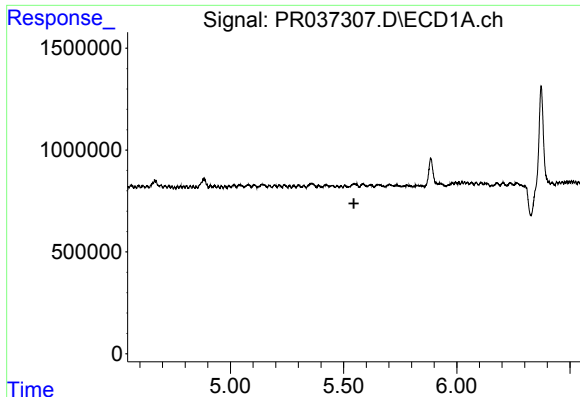

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

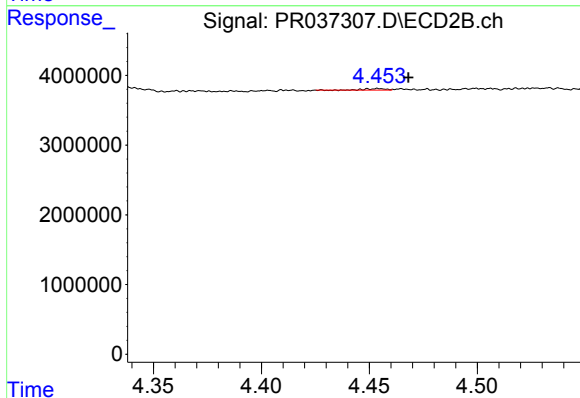


#17 AR-1242-2

R.T.: 4.454 min
Delta R.T.: -0.014 min
Response: 135350
Conc: 0.59 ng/ml

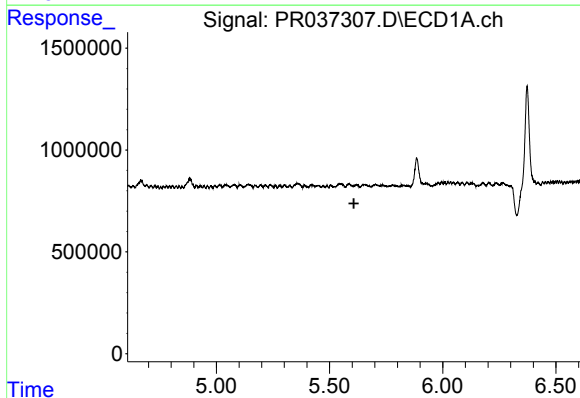


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

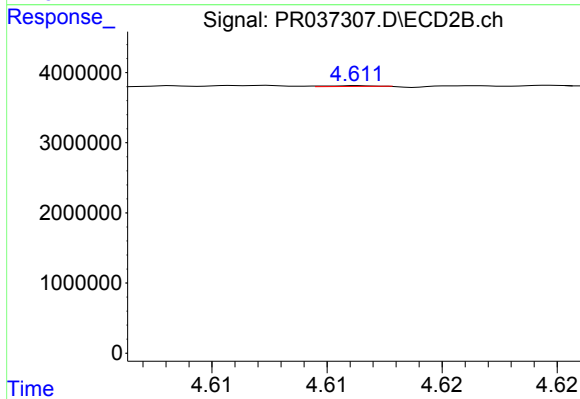

#18 AR-1242-3


R.T.: 4.611 min
Delta R.T.: -0.027 min
Response: 20883
Conc: 0.18 ng/ml

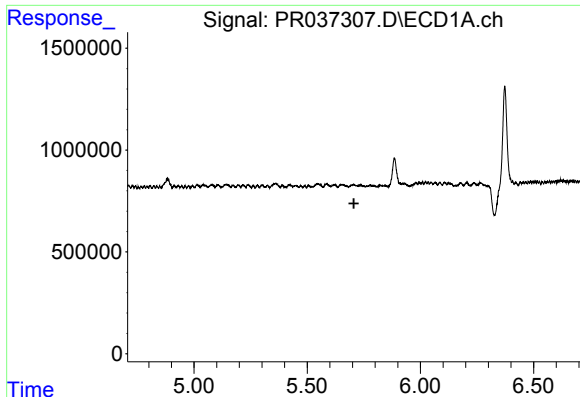

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

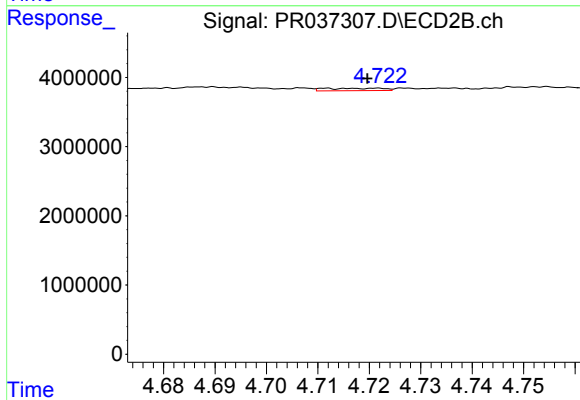


#19 AR-1242-4

R.T.: 4.722 min
Delta R.T.: 0.002 min
Response: 276793
Conc: 2.52 ng/ml

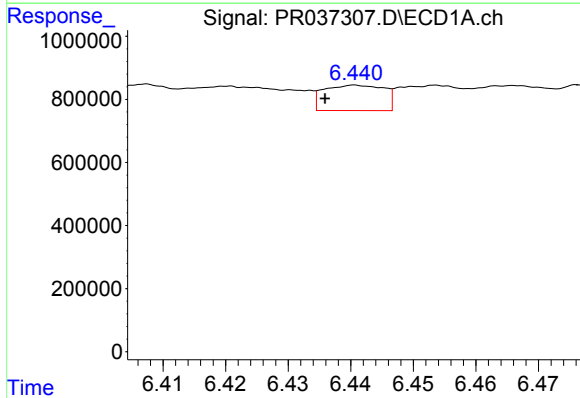


#20 AR-1242-5

R.T.: 6.441 min
Delta R.T.: 0.005 min
Response: 537716
Conc: 16.71 ng/ml

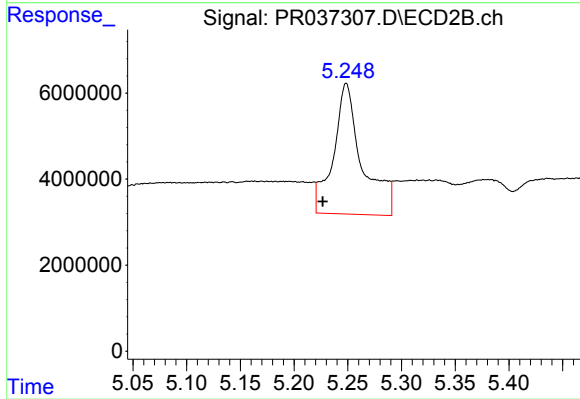

#20 AR-1242-5


R.T.: 5.249 min
Delta R.T.: 0.022 min
Response: 56452976
Conc: 340.69 ng/ml

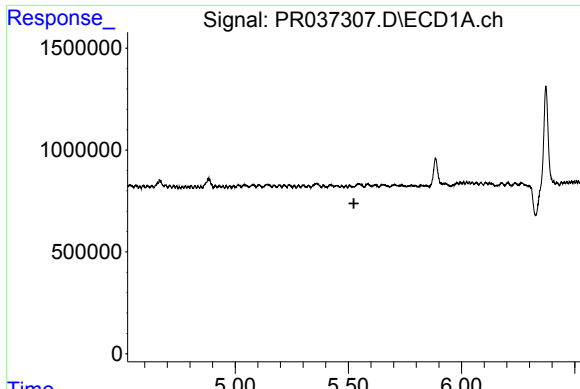

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

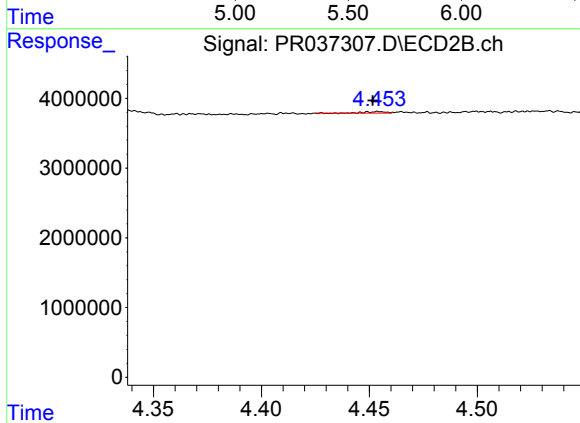


#21 AR-1248-1

R.T.: 4.454 min
Delta R.T.: 0.002 min
Response: 135350
Conc: 1.34 ng/ml

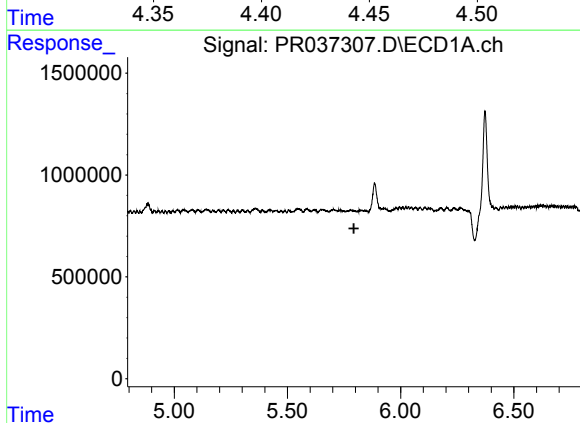


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

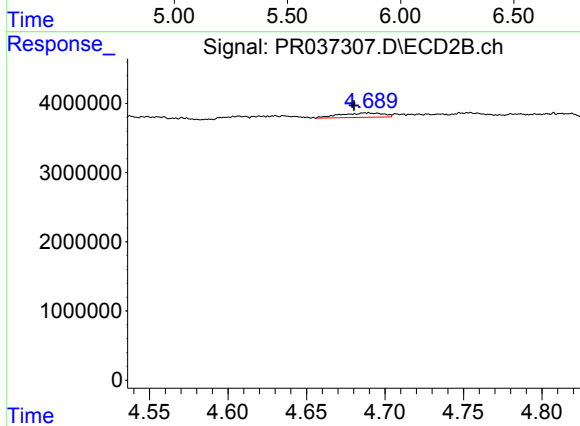

#22 AR-1248-2


R.T.: 4.690 min
Delta R.T.: 0.009 min
Response: 1261204
Conc: 9.24 ng/ml

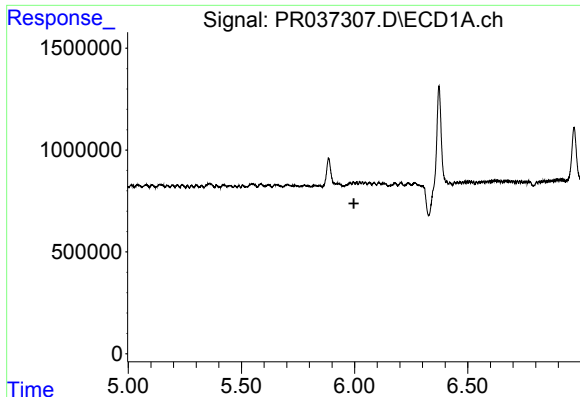

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

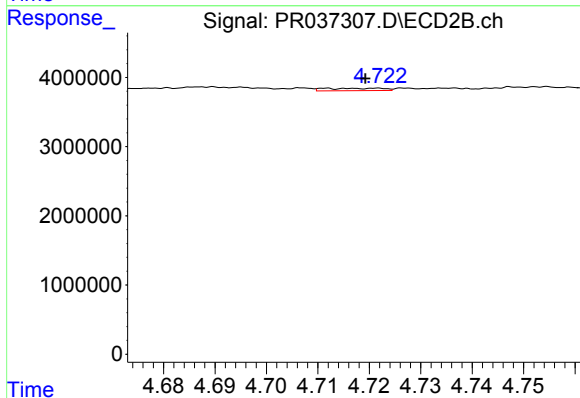


#23 AR-1248-3

R.T.: 4.722 min
Delta R.T.: 0.002 min
Response: 276793
Conc: 1.98 ng/ml

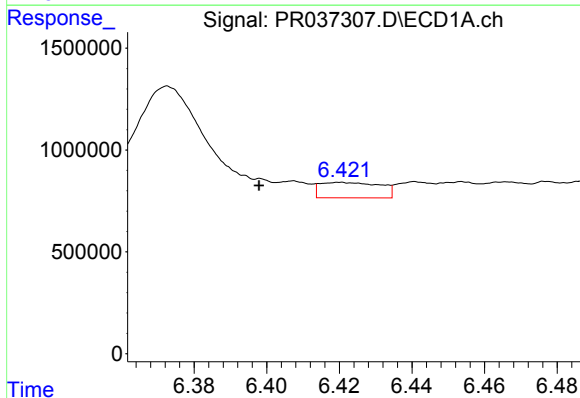


#24 AR-1248-4

R.T.: 6.420 min
Delta R.T.: 0.022 min
Response: 871748
Conc: 17.81 ng/ml

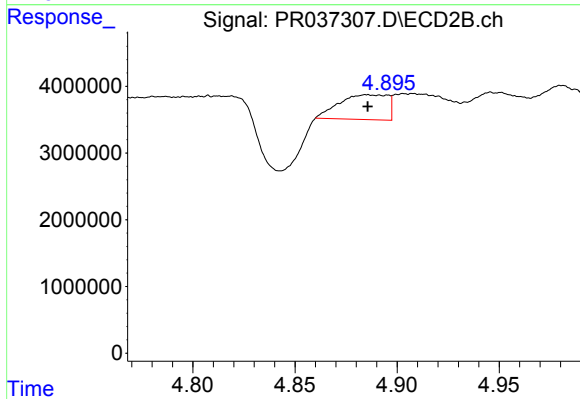

#24 AR-1248-4


R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 6127976
Conc: 34.43 ng/ml

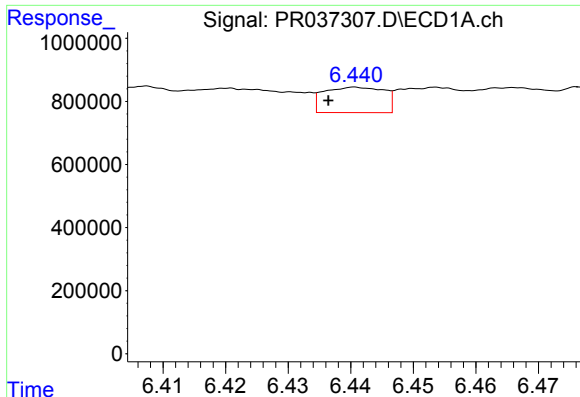

#25 AR-1248-5


R.T.: 6.441 min
Delta R.T.: 0.005 min
Response: 537716
Conc: 11.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

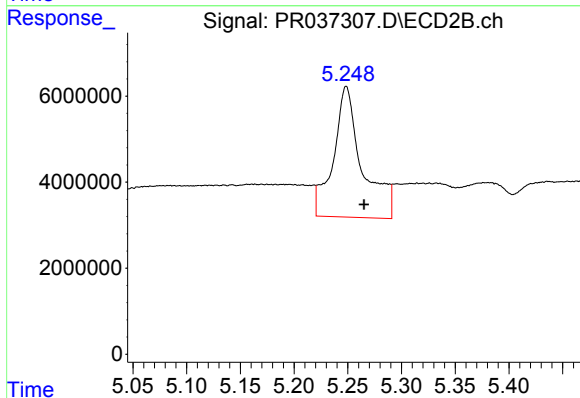


#25 AR-1248-5

R.T.: 5.249 min
Delta R.T.: -0.017 min
Response: 56452976
Conc: 288.60 ng/ml

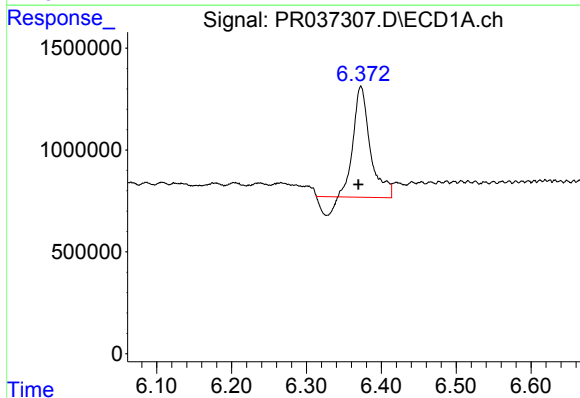


#26 AR-1254-1

R.T.: 6.373 min
Delta R.T.: 0.003 min
Response: 7865452
Conc: 143.97 ng/ml

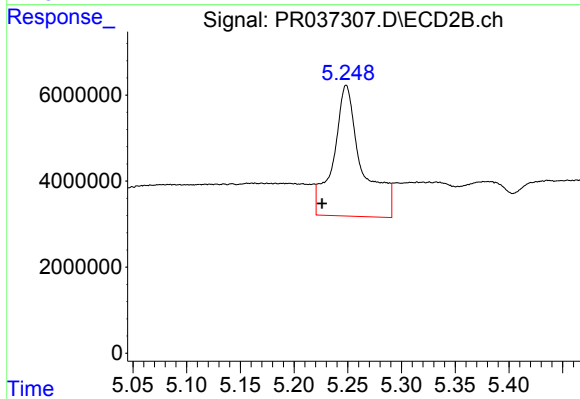

#26 AR-1254-1


R.T.: 5.249 min
Delta R.T.: 0.022 min
Response: 56452976
Conc: 163.88 ng/ml

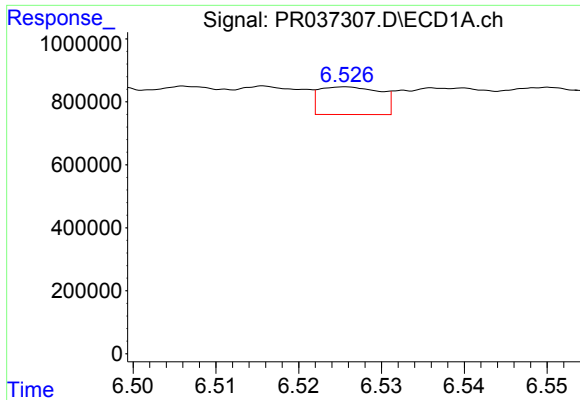

#27 AR-1254-2


R.T.: 6.526 min
Delta R.T.: -0.060 min
Response: 450858
Conc: 5.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

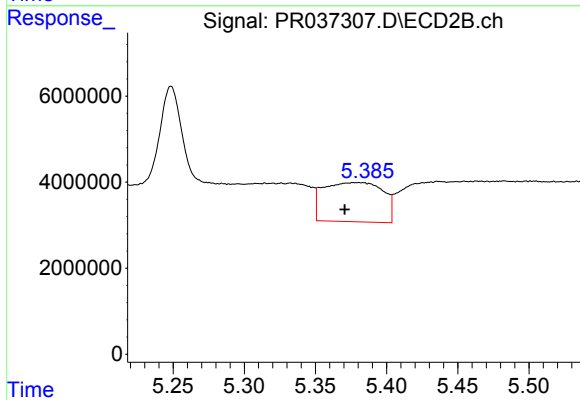


#27 AR-1254-2

R.T.: 5.381 min
Delta R.T.: 0.010 min
Response: 26560828
Conc: 88.68 ng/ml

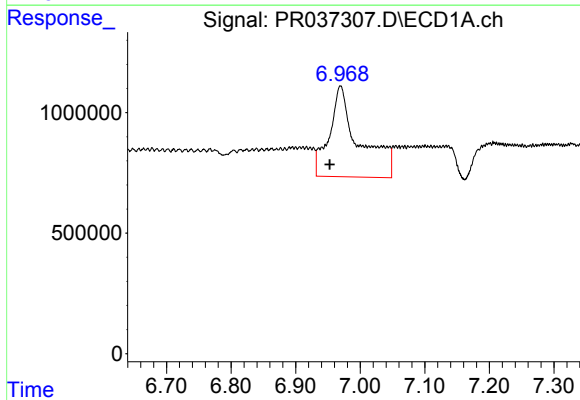


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: 0.017 min
Response: 12076442
Conc: 132.76 ng/ml

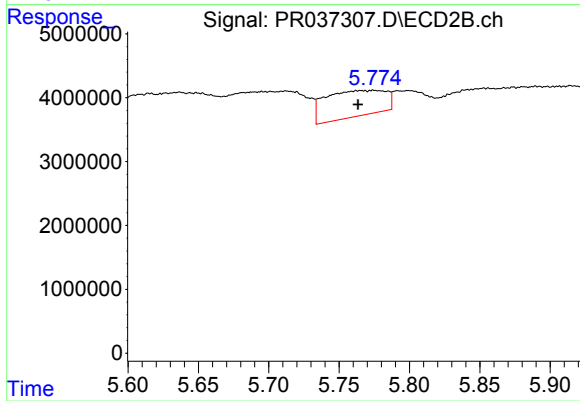

#28 AR-1254-3


R.T.: 5.774 min
Delta R.T.: 0.011 min
Response: 12133512
Conc: 25.62 ng/ml

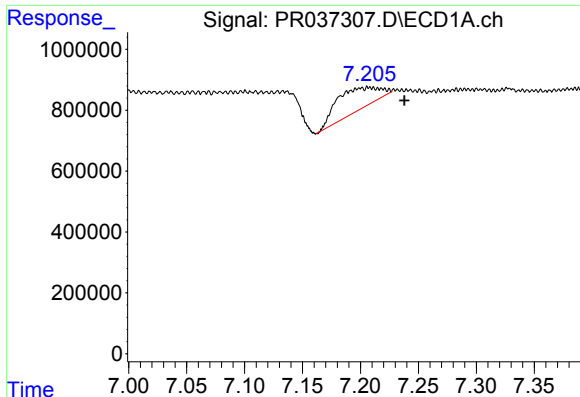

#29 AR-1254-4


R.T.: 7.207 min
Delta R.T.: -0.030 min
Response: 1834276
Conc: 27.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

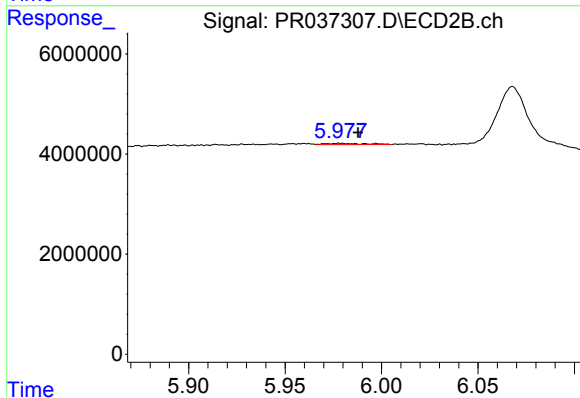


#29 AR-1254-4

R.T.: 5.978 min
Delta R.T.: -0.010 min
Response: 382737
Conc: 1.09 ng/ml

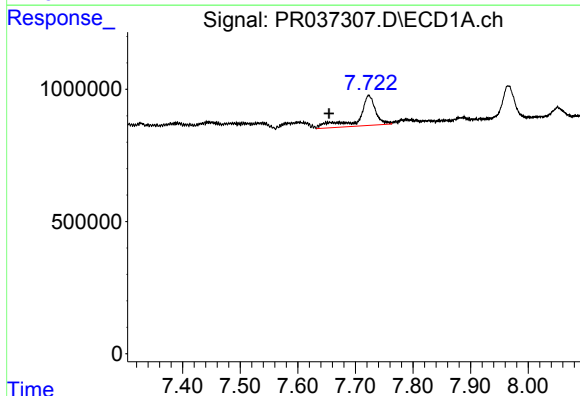


#30 AR-1254-5

R.T.: 7.723 min
Delta R.T.: 0.069 min
Response: 2330710
Conc: 32.42 ng/ml

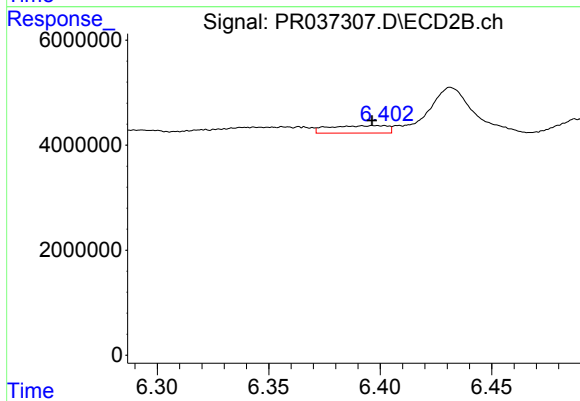

#30 AR-1254-5


R.T.: 6.398 min
Delta R.T.: 0.002 min
Response: 2577480
Conc: 5.82 ng/ml

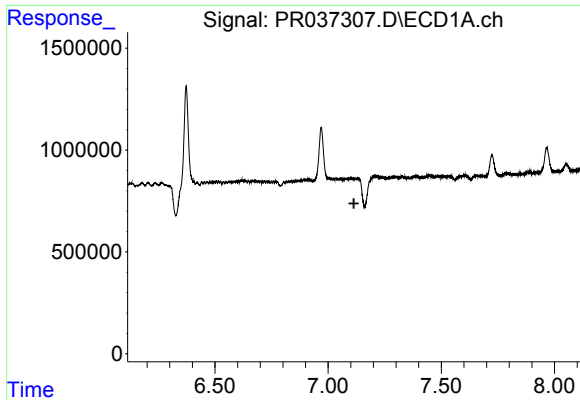

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

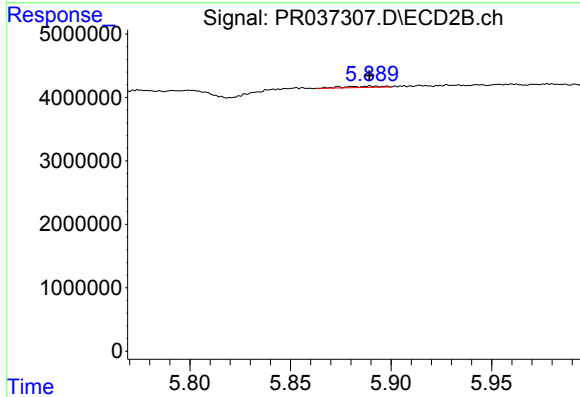


#31 AR-1260-1

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 255622
Conc: 0.87 ng/ml

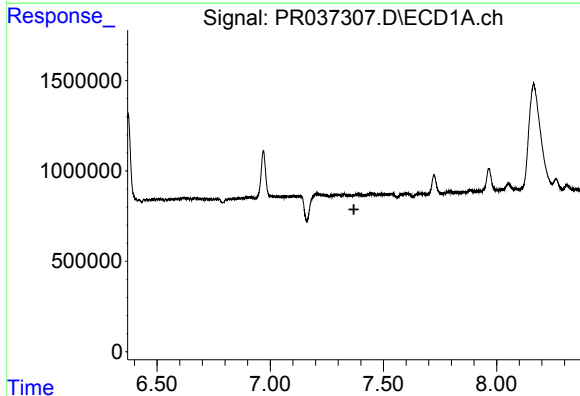


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

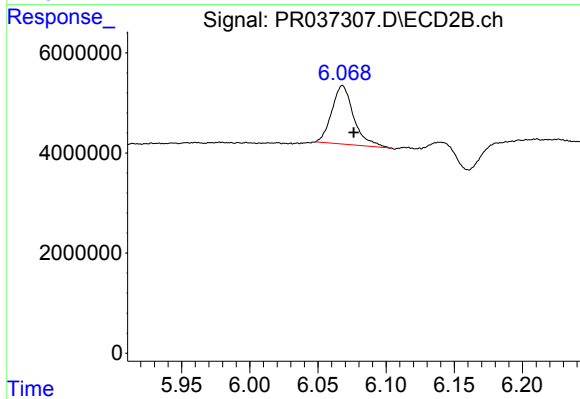

#32 AR-1260-2


R.T.: 6.068 min
Delta R.T.: -0.008 min
Response: 12949267
Conc: 28.11 ng/ml

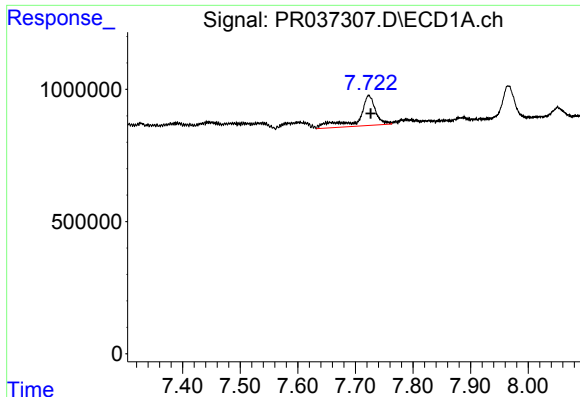

#33 AR-1260-3


R.T.: 7.723 min
Delta R.T.: -0.003 min
Response: 2330710
Conc: 37.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

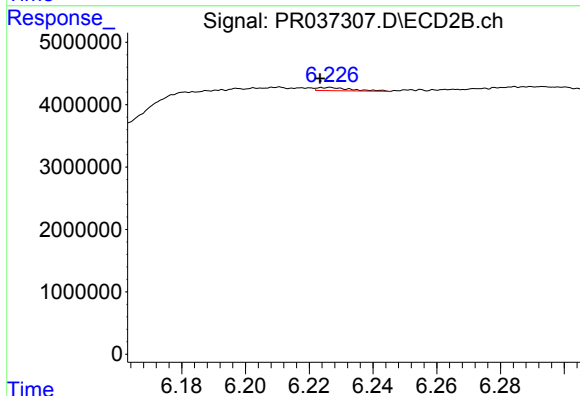


#33 AR-1260-3

R.T.: 6.226 min
Delta R.T.: 0.003 min
Response: 384340
Conc: 1.08 ng/ml

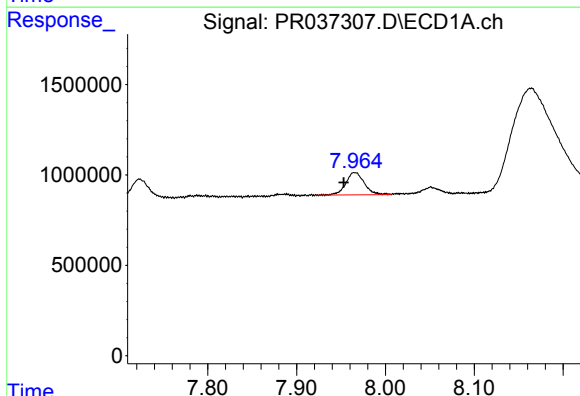


#34 AR-1260-4

R.T.: 7.965 min
Delta R.T.: 0.012 min
Response: 1780974
Conc: 23.94 ng/ml

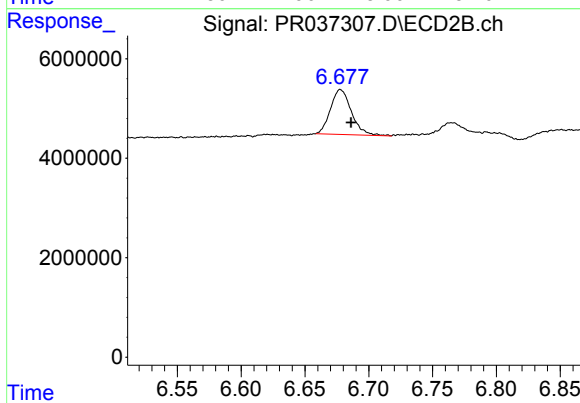

#34 AR-1260-4


R.T.: 6.678 min
Delta R.T.: -0.008 min
Response: 10268305
Conc: 33.69 ng/ml

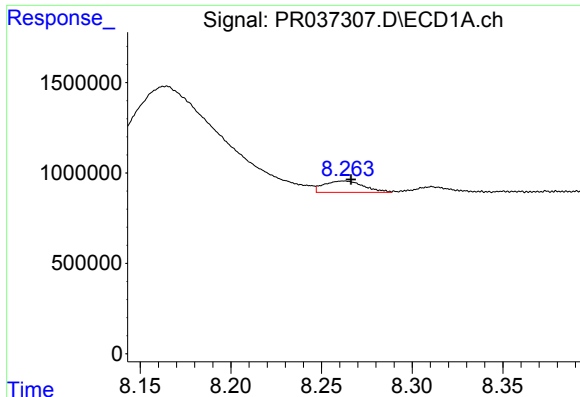

#35 AR-1260-5


R.T.: 8.262 min
Delta R.T.: -0.004 min
Response: 954676
Conc: 6.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

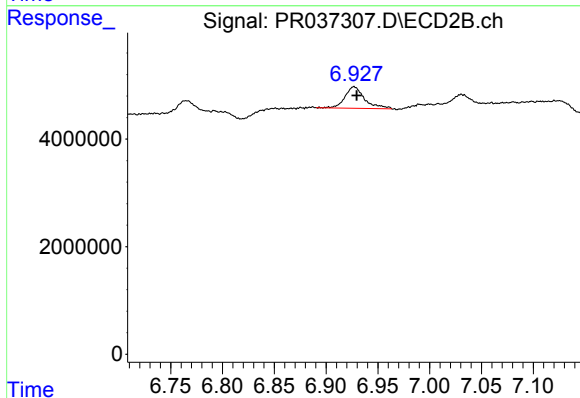


#35 AR-1260-5

R.T.: 6.927 min
Delta R.T.: -0.003 min
Response: 5312707
Conc: 6.13 ng/ml

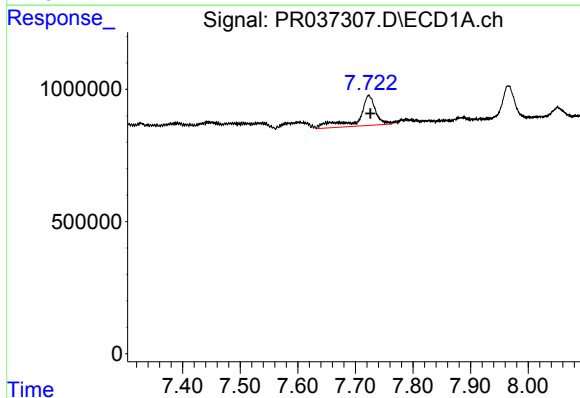


#36 AR-1262-1

R.T.: 7.723 min
Delta R.T.: -0.003 min
Response: 2330710
Conc: 22.31 ng/ml

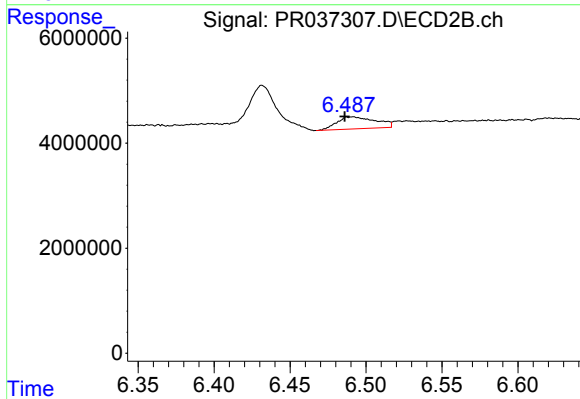

#36 AR-1262-1


R.T.: 6.491 min
Delta R.T.: 0.005 min
Response: 4068672
Conc: 16.23 ng/ml

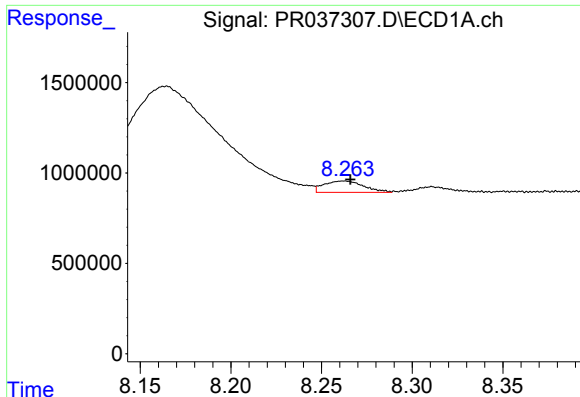

#37 AR-1262-2


R.T.: 8.262 min
Delta R.T.: -0.003 min
Response: 954676
Conc: 4.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

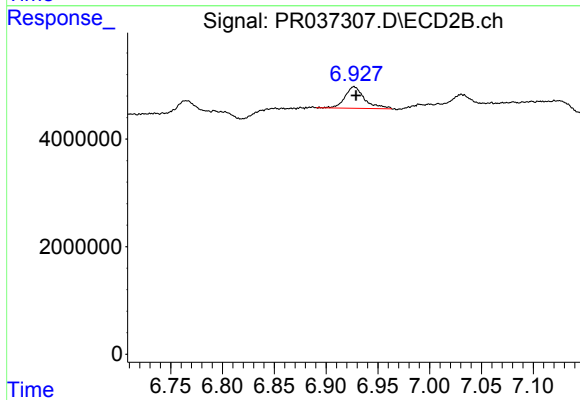


#37 AR-1262-2

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 5312707
Conc: 4.23 ng/ml

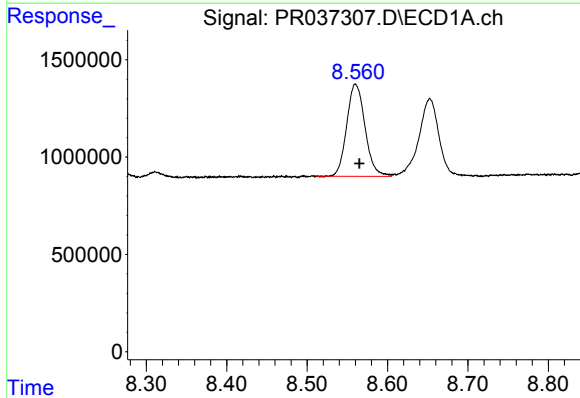


#38 AR-1262-3

R.T.: 8.560 min
Delta R.T.: -0.005 min
Response: 7499356
Conc: 57.02 ng/ml

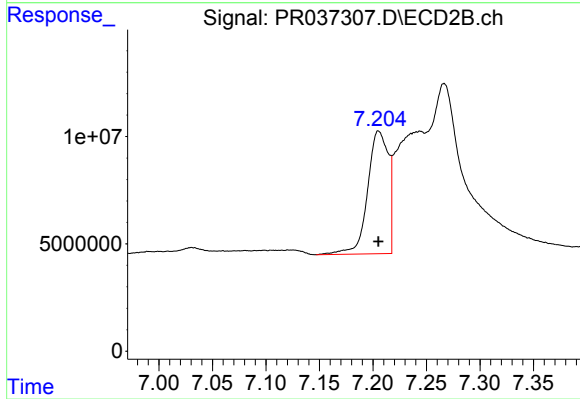

#38 AR-1262-3


R.T.: 7.205 min
Delta R.T.: 0.000 min
Response: 77486582
Conc: 141.33 ng/ml

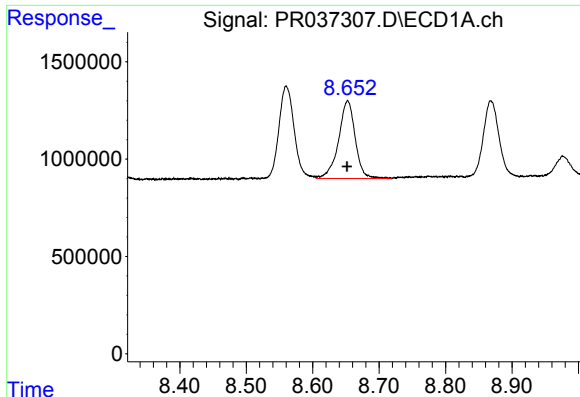

#39 AR-1262-4


R.T.: 8.653 min
Delta R.T.: 0.000 min
Response: 6978738
Conc: 71.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

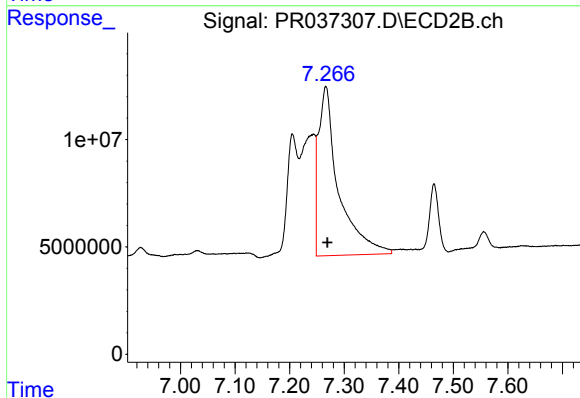


#39 AR-1262-4

R.T.: 7.267 min
Delta R.T.: -0.003 min
Response: 202092739
Conc: 225.14 ng/ml

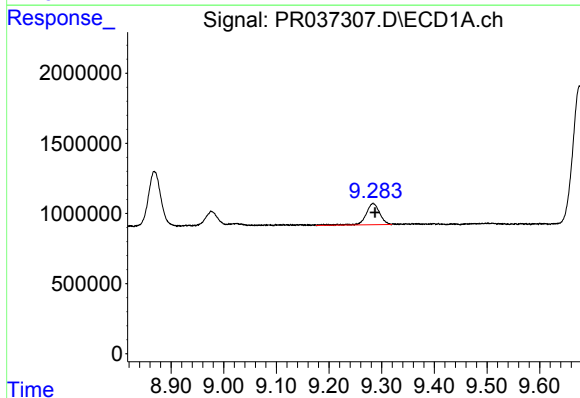


#40 AR-1262-5

R.T.: 9.284 min
Delta R.T.: -0.004 min
Response: 2760717
Conc: 39.99 ng/ml

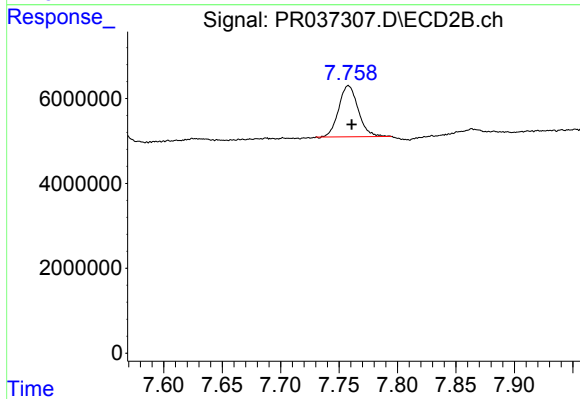

#40 AR-1262-5


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 13992109
Conc: 36.57 ng/ml

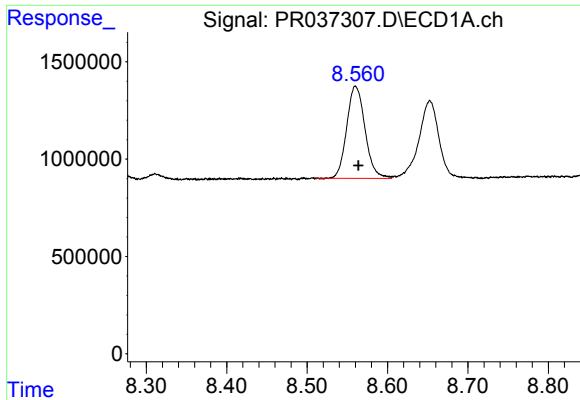

#41 AR-1268-1


R.T.: 8.560 min
Delta R.T.: -0.004 min
Response: 7499356
Conc: 41.87 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

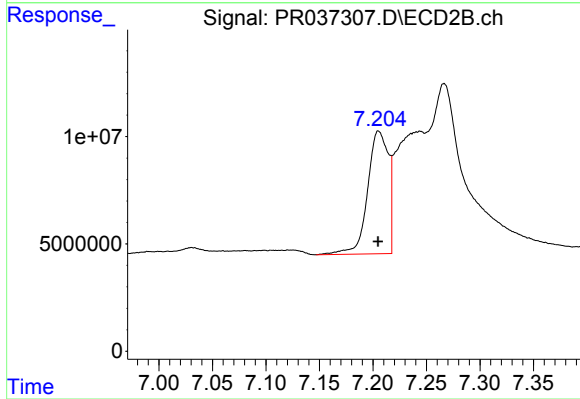


#41 AR-1268-1

R.T.: 7.205 min
Delta R.T.: 0.000 min
Response: 77486582
Conc: 62.94 ng/ml

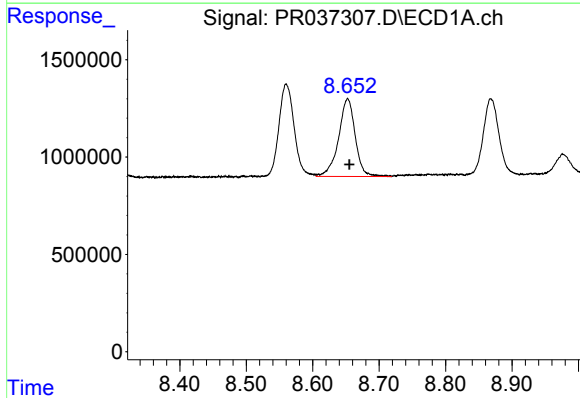


#42 AR-1268-2

R.T.: 8.653 min
Delta R.T.: -0.003 min
Response: 6978738
Conc: 42.42 ng/ml

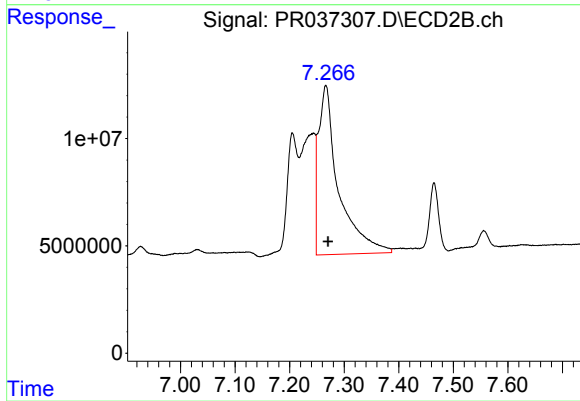

#42 AR-1268-2


R.T.: 7.267 min
Delta R.T.: -0.004 min
Response: 202092739
Conc: 190.85 ng/ml

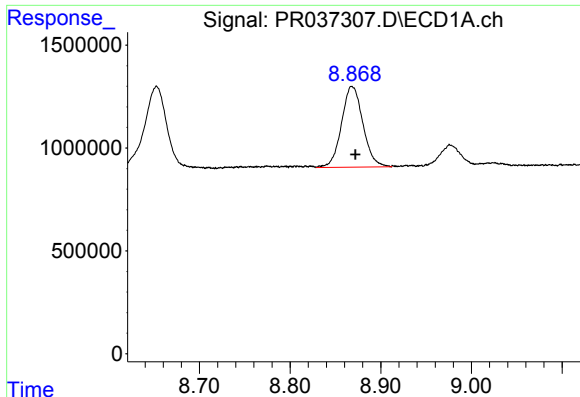

#43 AR-1268-3


R.T.: 8.868 min
Delta R.T.: -0.004 min
Response: 6436485
Conc: 46.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

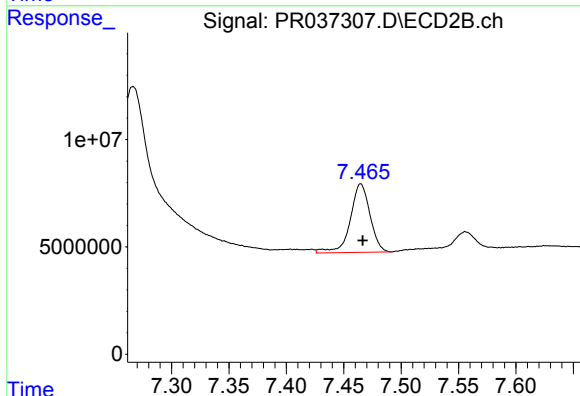


#43 AR-1268-3

R.T.: 7.465 min
Delta R.T.: -0.002 min
Response: 38287172
Conc: 43.20 ng/ml

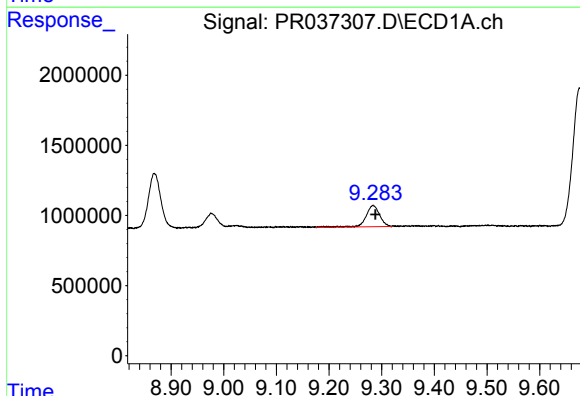


#44 AR-1268-4

R.T.: 9.284 min
Delta R.T.: -0.004 min
Response: 2760717
Conc: 44.25 ng/ml

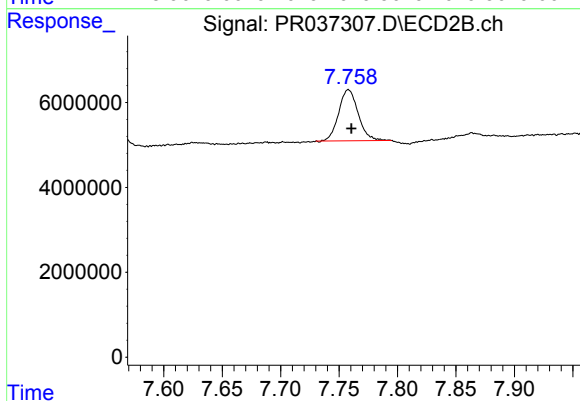

#44 AR-1268-4


R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 13992109
Conc: 38.57 ng/ml

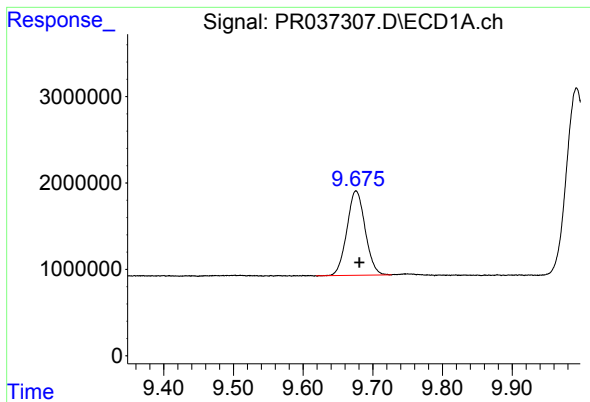

#45 AR-1268-5

R.T.: 9.676 min
Delta R.T.: -0.005 min
Response: 17779322
Conc: 39.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

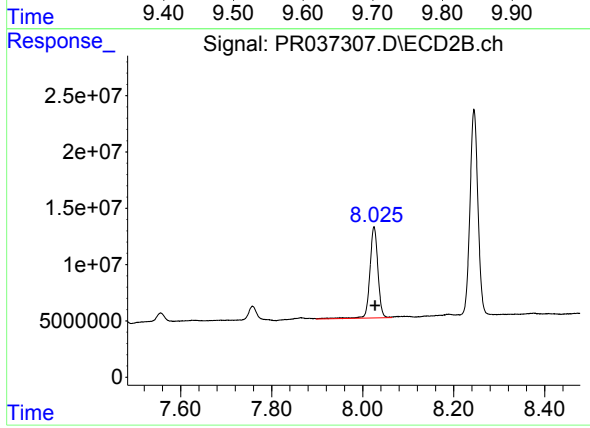

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.002 min
Response: 98556529
Conc: 38.74 ng/ml