

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 17:37
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1660 MDL 25PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 21:58:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.359	3.407	24079860	95737222	19.248	19.964
2)	SA Decachlor...	9.988	8.245	26152921	124.0E6	19.774	21.283
Target Compounds							
3)	L1 AR-1016-1	5.521	4.450	1289468	5195284	29.926	28.533
4)	L1 AR-1016-2	5.541	4.466	2023889	7954291	29.227	28.194
5)	L1 AR-1016-3	5.603	4.637	1316189	3662192	32.637	25.470
6)	L1 AR-1016-4	5.701	4.678	837745	3054888	25.510	27.612
7)	L1 AR-1016-5	5.992	4.883	1181448	4485142	34.455	29.506
8)	L2 AR-1221-1	0.000	3.615	0	100791	N.D.	1.979 #
9)	L2 AR-1221-2	4.663	3.695	654330	1819969	72.350	49.009 #
10)	L2 AR-1221-3	4.731	3.767	886002	2616454	28.908	21.368 #
11)	L3 AR-1232-1	4.731	3.767	886002	2616454	30.290	22.365 #
12)	L3 AR-1232-2	5.254	4.466	1559411	7954291	92.286	57.546 #
13)	L3 AR-1232-3	5.541	4.637	2023889	3662192	59.870	52.167
14)	L3 AR-1232-4	5.701	4.718	837745	3855146	53.371	64.606
15)	L3 AR-1232-5	5.788	4.883	856460	4485142	73.229	65.722
16)	L4 AR-1242-1	5.521	4.450	1289468	5195284	37.688	35.454
17)	L4 AR-1242-2	5.541	4.466	2023889	7954291	36.486	34.863
18)	L4 AR-1242-3	5.603	4.637	1316189	3662192	39.988	31.672
19)	L4 AR-1242-4	5.701	4.718	837745	3855146	31.760	35.075
20)	L4 AR-1242-5	6.432	5.226	465662	6386681	14.471	38.544 #
21)	L5 AR-1248-1	5.521	4.450	1289468	5195284	56.291	51.610
22)	L5 AR-1248-2	5.788	4.678	856460	3054888	24.460	22.384
23)	L5 AR-1248-3	5.992	4.718	1181448	3855146	28.880	27.542
24)	L5 AR-1248-4	6.366	4.883	2084683	4485142	42.584	25.202 #
25)	L5 AR-1248-5	6.432	5.261	465662	2429161	9.858	12.418 #
26)	L6 AR-1254-1	6.366	5.226	2084683	6386681	38.159	18.540 #
27)	L6 AR-1254-2	6.580	5.369	919933	5623620	10.735	18.777 #
28)	L6 AR-1254-3	6.953	5.774	1129879	8721996	12.421	18.416 #
29)	L6 AR-1254-4	7.231	5.985	745081	670237	11.119	1.911 #
30)	L6 AR-1254-5	7.646	6.393	3406535	16583272	47.391	37.449
31)	L7 AR-1260-1	7.107	5.888	2443209	9496134	37.026	32.490
32)	L7 AR-1260-2	7.362	6.074	2891225	16161218	36.275	35.088
33)	L7 AR-1260-3	7.719	6.222	1919359	11217303	30.673	31.465
34)	L7 AR-1260-4	7.945	6.684	2266286	9640582	30.459	31.633
35)	L7 AR-1260-5	8.258	6.926	3920733	24899028	27.110	28.711
36)	L8 AR-1262-1	7.719	6.484	1919359	7785643	18.375	31.066 #
37)	L8 AR-1262-2	8.258	6.926	3920733	24899028	20.170	19.825
38)	L8 AR-1262-3	8.577	7.202	2647928	12863288	20.135	23.462
39)	L8 AR-1262-4	8.630	7.266	1584247	25183164	16.128	28.055 #
40)	L8 AR-1262-5	9.279	7.758	1512610	6283016	21.909	16.421 #
41)	L9 AR-1268-1	8.577	7.202	2647928	12863288	14.785	10.449 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 17:37
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1660 MDL 25PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 21:58:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.630	7.266	1584247	25183164	9.631	23.782 #
43) L9	AR-1268-3	0.000	7.464	0	6554258	N.D.	7.396 #
44) L9	AR-1268-4	9.279	7.758	1512610	6283016	24.246	17.319 #
45) L9	AR-1268-5	0.000	8.026	0	7308037	N.D.	2.872 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
Data File : PR037326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 17:37
Operator : SM\SJ
Sample : K1560-03
Misc : AR1660 MDL 25PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 21:58:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

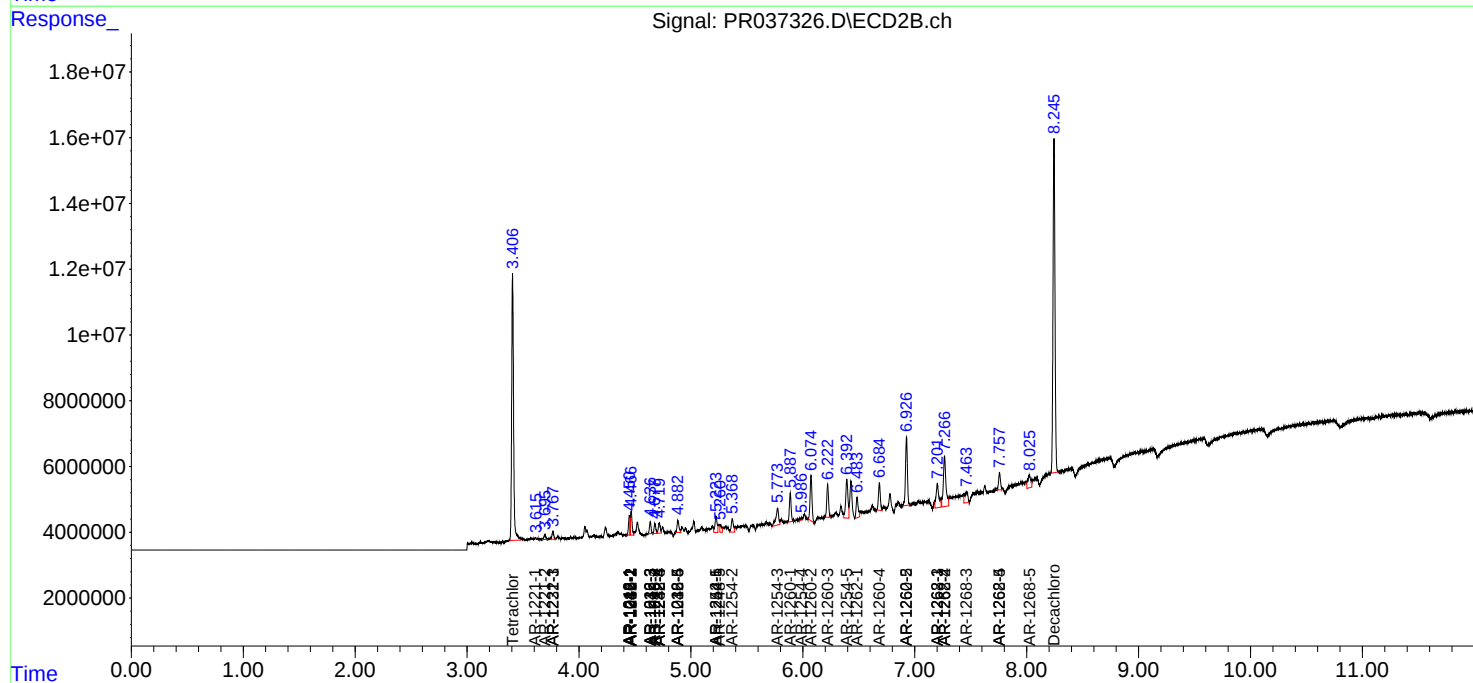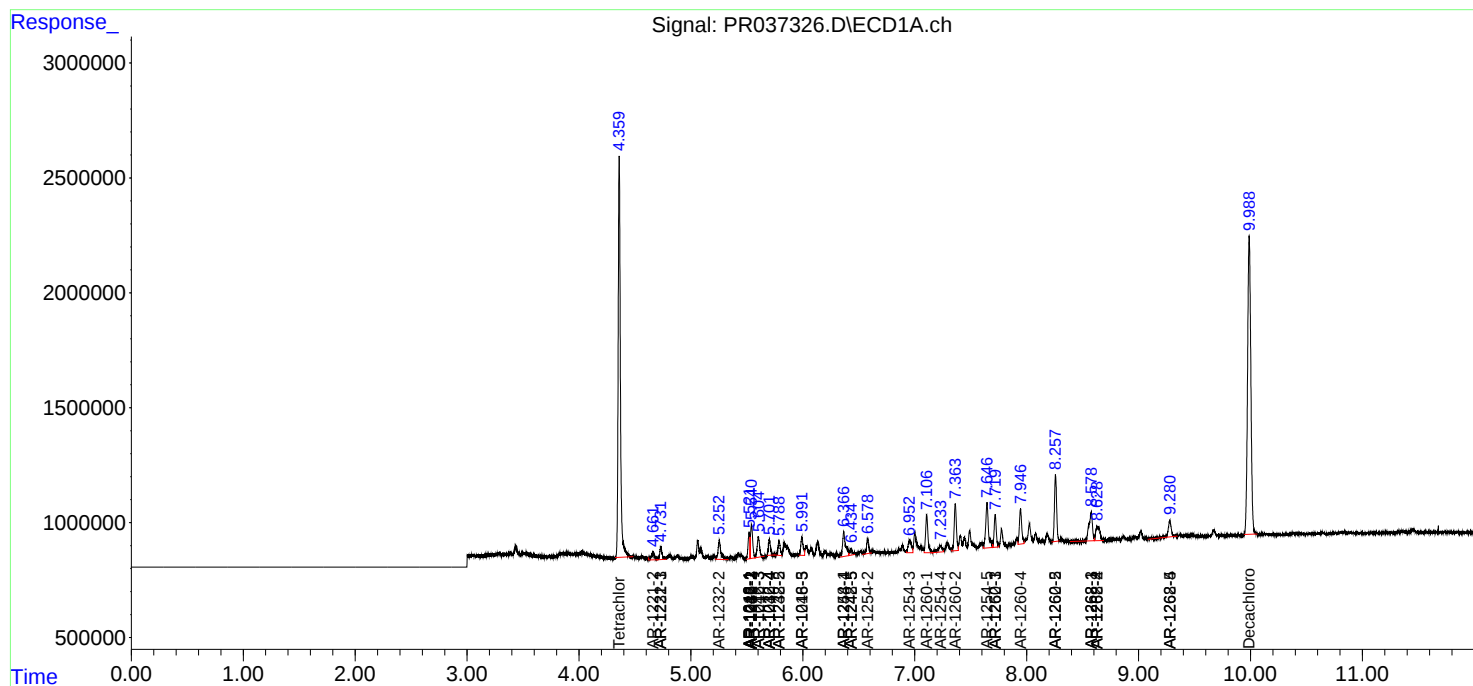


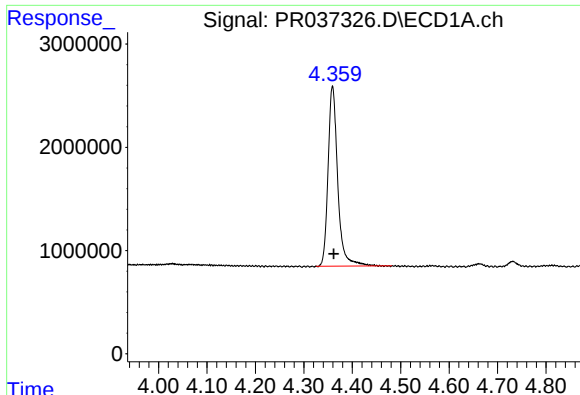

#1 Tetrachloro-m-xylene


R.T.: 4.359 min
Delta R.T.: -0.003 min
Response: 24079860
Conc: 19.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

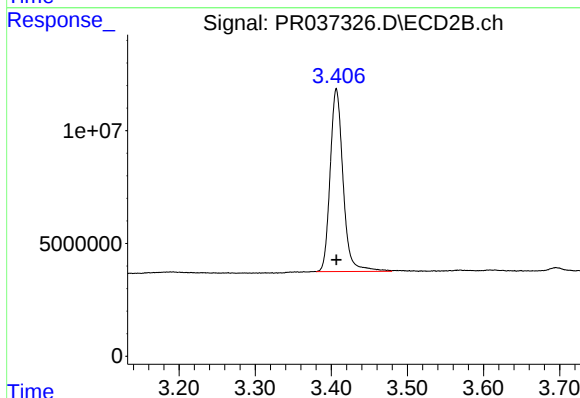


#1 Tetrachloro-m-xylene

R.T.: 3.407 min
Delta R.T.: 0.000 min
Response: 95737222
Conc: 19.96 ng/ml

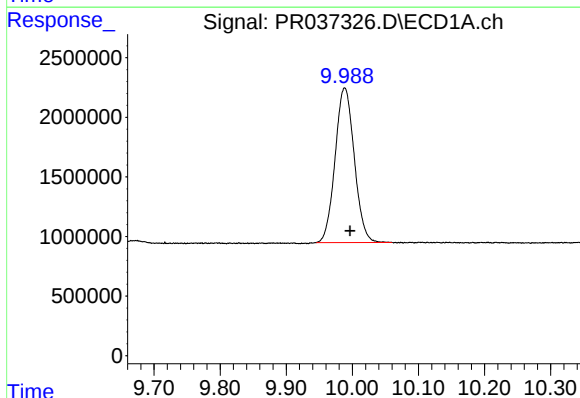


#2 Decachlorobiphenyl

R.T.: 9.988 min
Delta R.T.: -0.008 min
Response: 26152921
Conc: 19.77 ng/ml

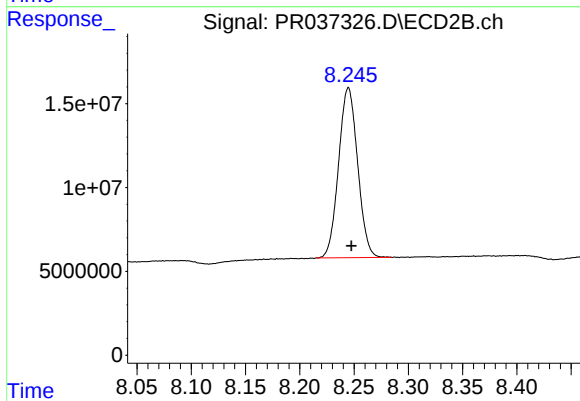

#2 Decachlorobiphenyl


R.T.: 8.245 min
Delta R.T.: -0.003 min
Response: 123960011
Conc: 21.28 ng/ml

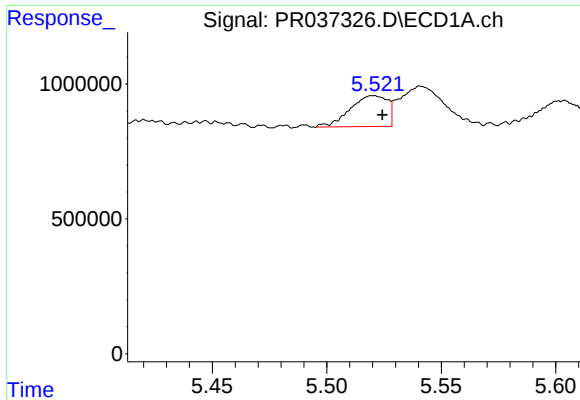

#3 AR-1016-1


R.T.: 5.521 min
Delta R.T.: -0.003 min
Response: 1289468
Conc: 29.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

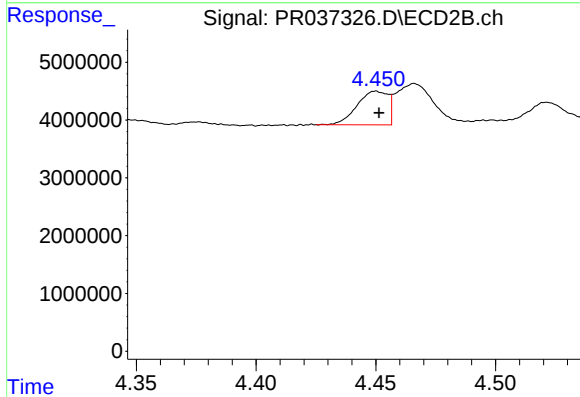


#3 AR-1016-1

R.T.: 4.450 min
Delta R.T.: -0.001 min
Response: 5195284
Conc: 28.53 ng/ml

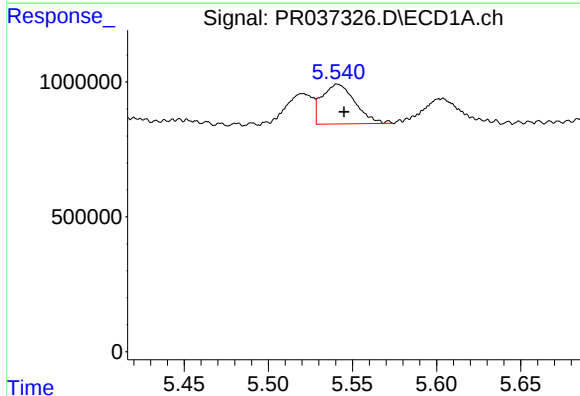


#4 AR-1016-2

R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 2023889
Conc: 29.23 ng/ml

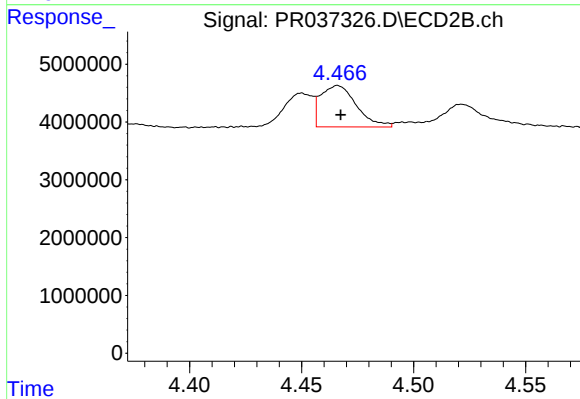

#4 AR-1016-2


R.T.: 4.466 min
Delta R.T.: -0.001 min
Response: 7954291
Conc: 28.19 ng/ml

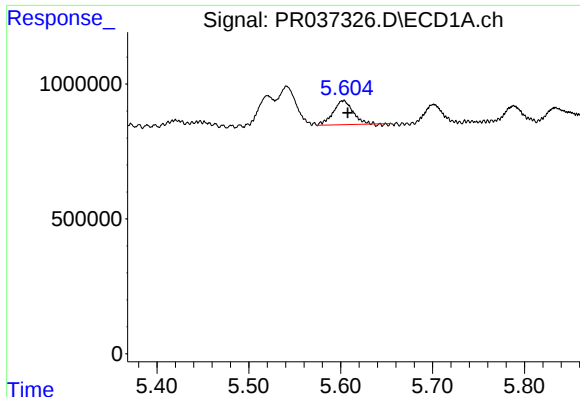

#5 AR-1016-3


R.T.: 5.603 min
Delta R.T.: -0.005 min
Response: 1316189
Conc: 32.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

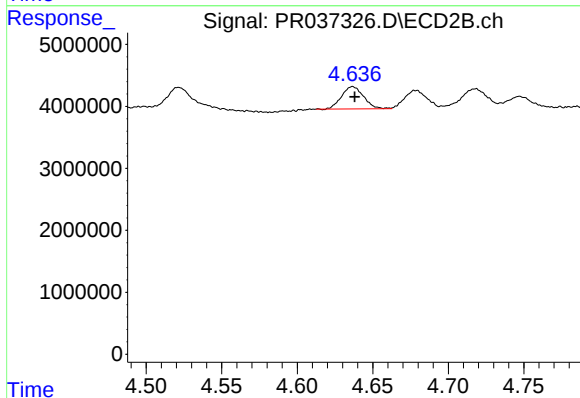


#5 AR-1016-3

R.T.: 4.637 min
Delta R.T.: -0.002 min
Response: 3662192
Conc: 25.47 ng/ml

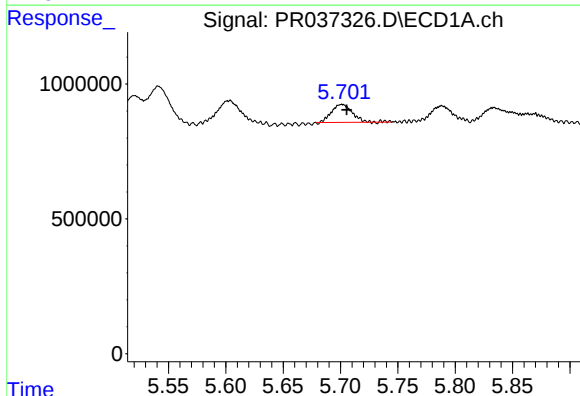


#6 AR-1016-4

R.T.: 5.701 min
Delta R.T.: -0.004 min
Response: 837745
Conc: 25.51 ng/ml

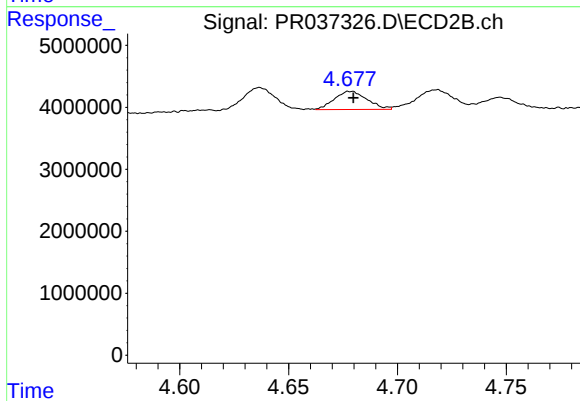

#6 AR-1016-4


R.T.: 4.678 min
Delta R.T.: -0.002 min
Response: 3054888
Conc: 27.61 ng/ml

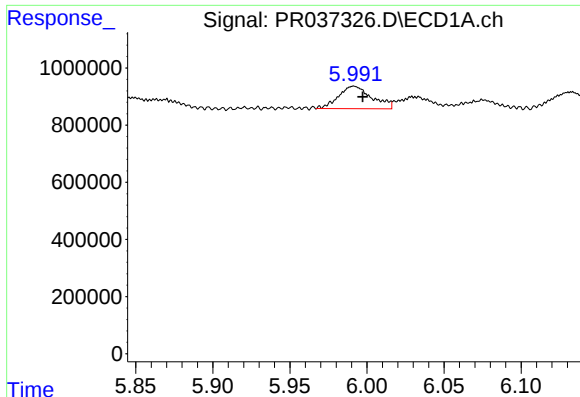

#7 AR-1016-5


R.T.: 5.992 min
Delta R.T.: -0.006 min
Response: 1181448
Conc: 34.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

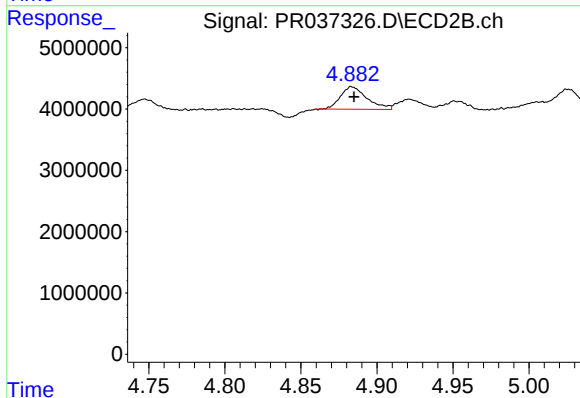


#7 AR-1016-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 4485142
Conc: 29.51 ng/ml

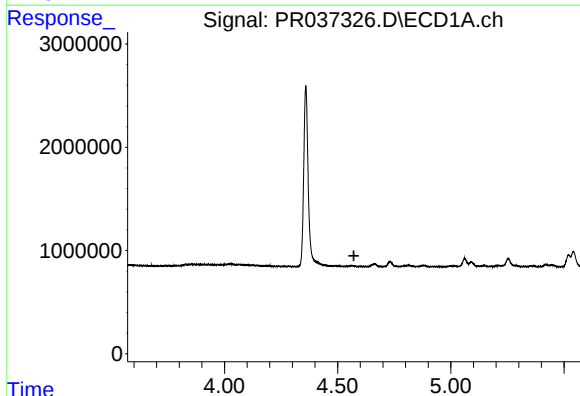


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

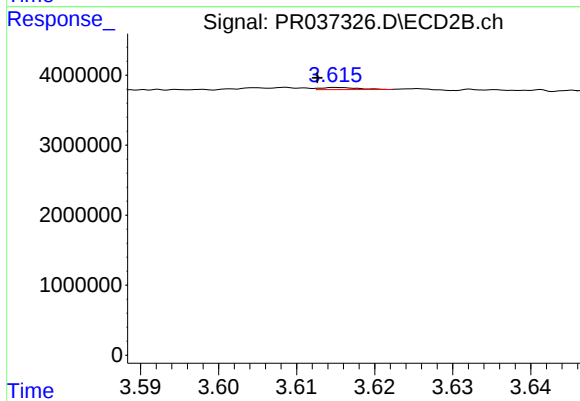

#8 AR-1221-1


R.T.: 3.615 min
Delta R.T.: 0.003 min
Response: 100791
Conc: 1.98 ng/ml

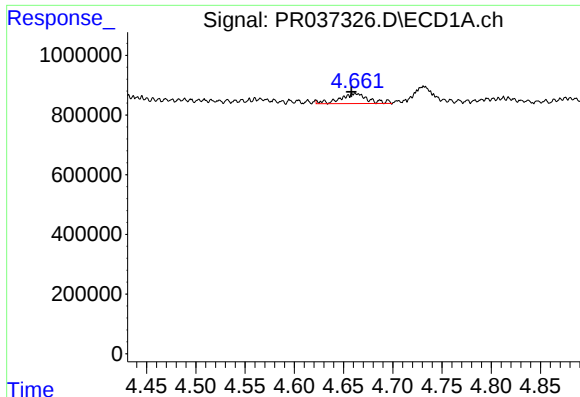

#9 AR-1221-2


R.T.: 4.663 min
Delta R.T.: 0.005 min
Response: 654330
Conc: 72.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

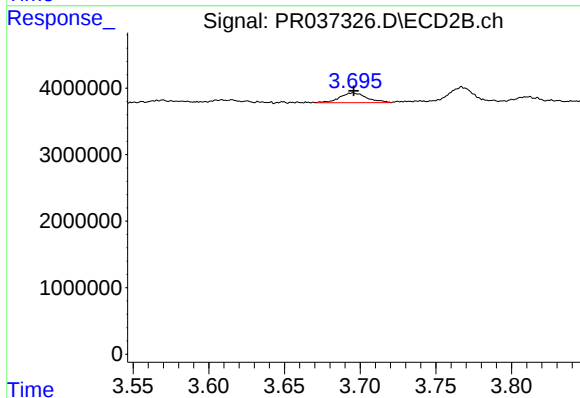


#9 AR-1221-2

R.T.: 3.695 min
Delta R.T.: 0.000 min
Response: 1819969
Conc: 49.01 ng/ml

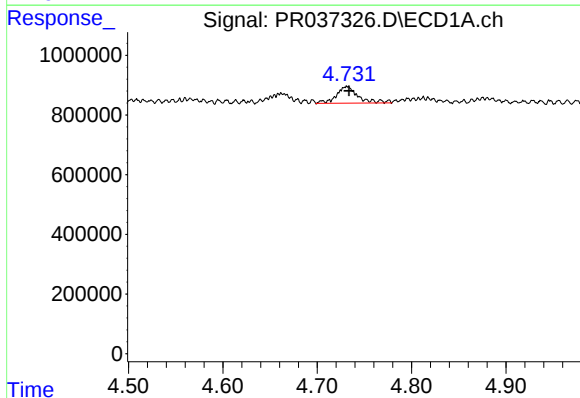


#10 AR-1221-3

R.T.: 4.731 min
Delta R.T.: -0.003 min
Response: 886002
Conc: 28.91 ng/ml

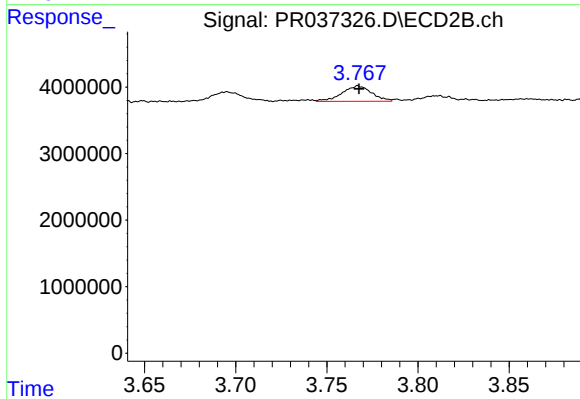

#10 AR-1221-3


R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 2616454
Conc: 21.37 ng/ml

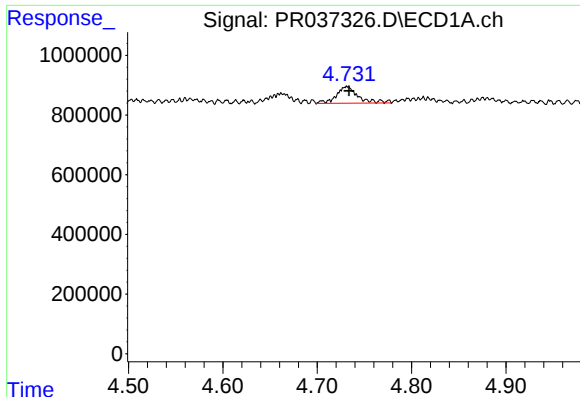

#11 AR-1232-1


R.T.: 4.731 min
Delta R.T.: -0.002 min
Response: 886002
Conc: 30.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

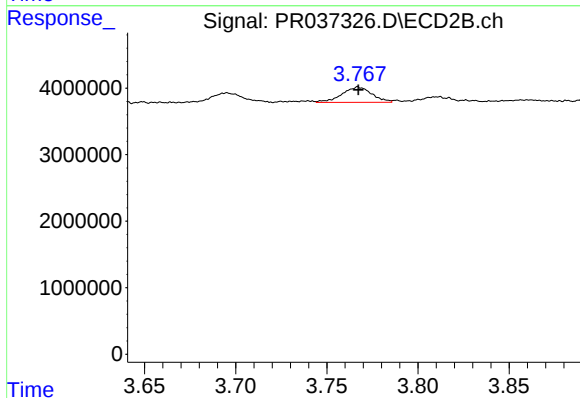


#11 AR-1232-1

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 2616454
Conc: 22.36 ng/ml

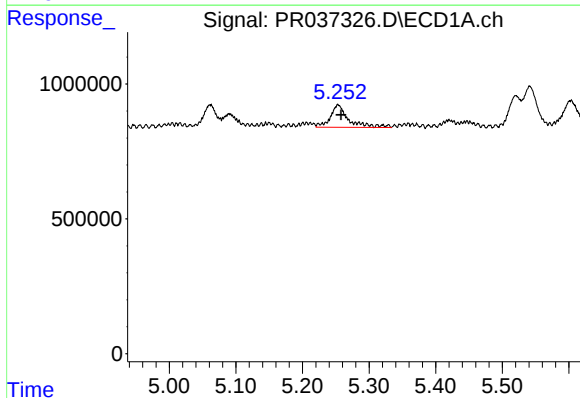


#12 AR-1232-2

R.T.: 5.254 min
Delta R.T.: -0.004 min
Response: 1559411
Conc: 92.29 ng/ml

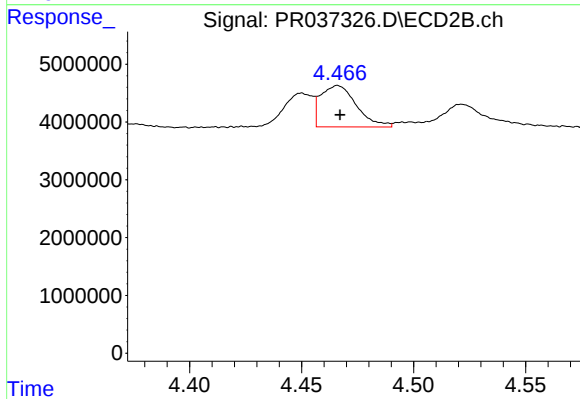

#12 AR-1232-2


R.T.: 4.466 min
Delta R.T.: -0.001 min
Response: 7954291
Conc: 57.55 ng/ml

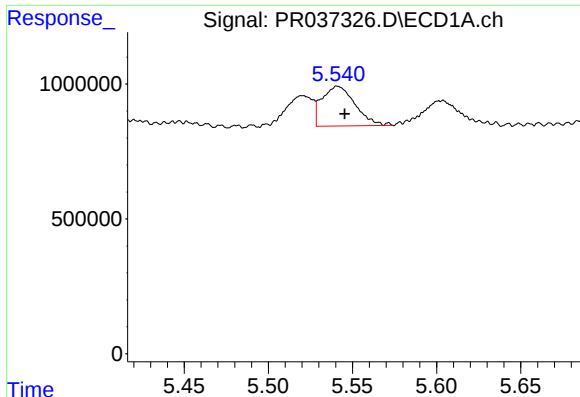

#13 AR-1232-3


R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 2023889
Conc: 59.87 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

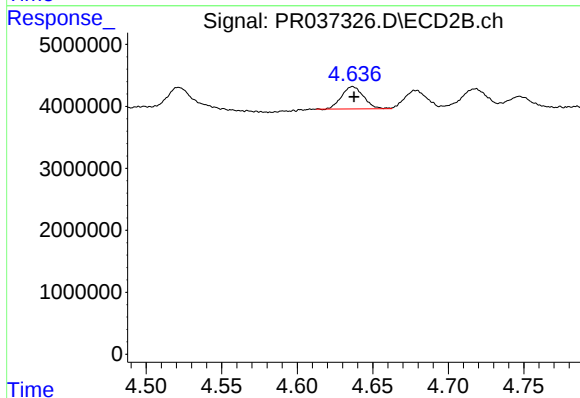


#13 AR-1232-3

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 3662192
Conc: 52.17 ng/ml

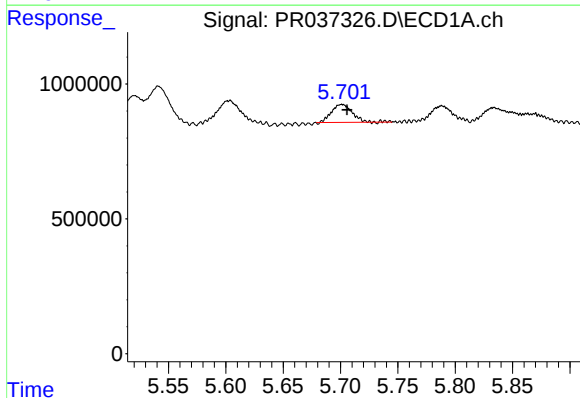


#14 AR-1232-4

R.T.: 5.701 min
Delta R.T.: -0.005 min
Response: 837745
Conc: 53.37 ng/ml

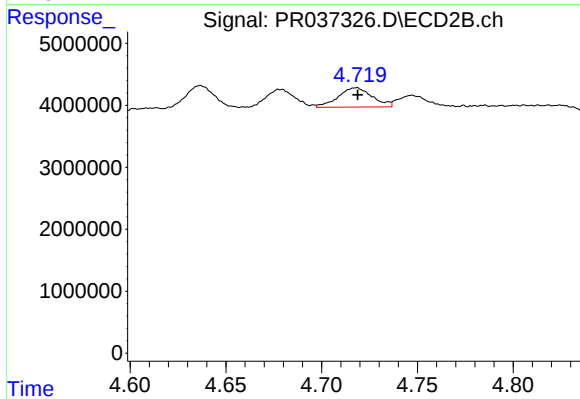

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 3855146
Conc: 64.61 ng/ml

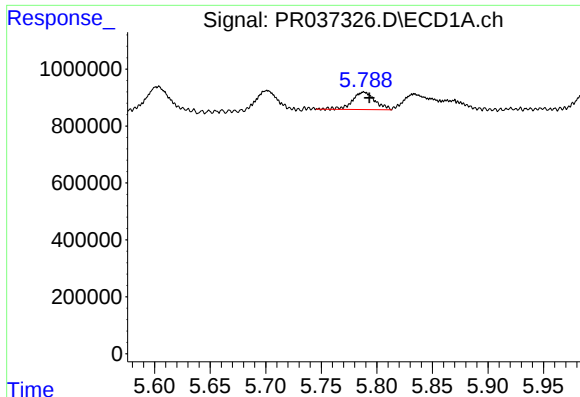

#15 AR-1232-5


R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 856460
Conc: 73.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

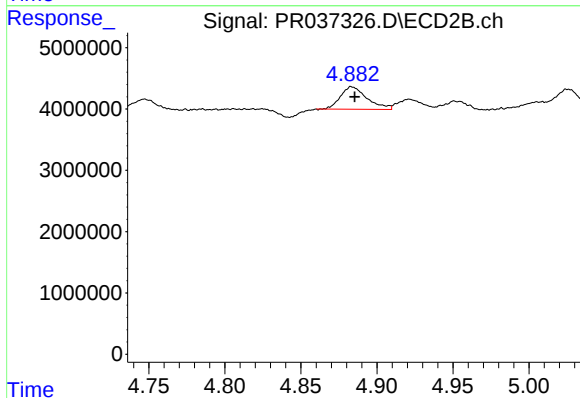


#15 AR-1232-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 4485142
Conc: 65.72 ng/ml

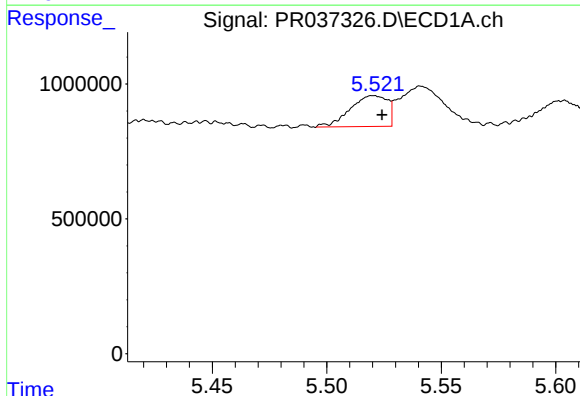


#16 AR-1242-1

R.T.: 5.521 min
Delta R.T.: -0.003 min
Response: 1289468
Conc: 37.69 ng/ml

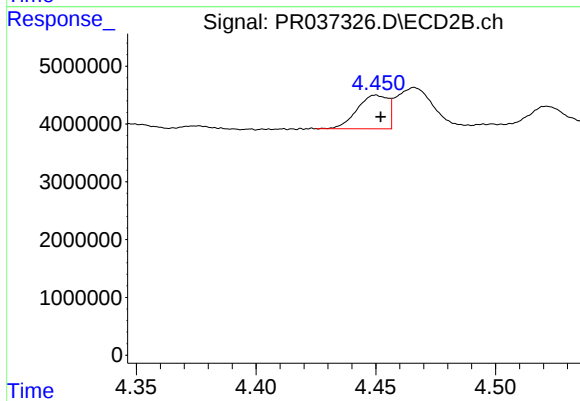

#16 AR-1242-1


R.T.: 4.450 min
Delta R.T.: -0.002 min
Response: 5195284
Conc: 35.45 ng/ml

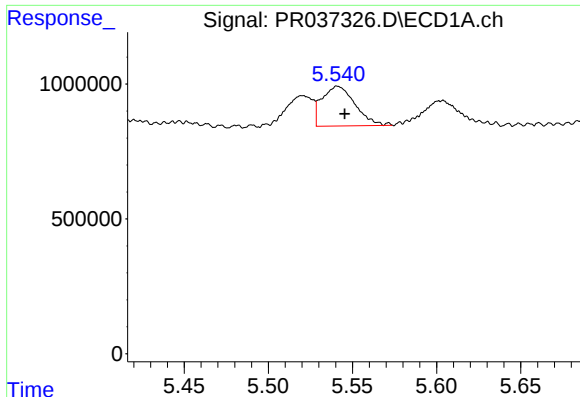

#17 AR-1242-2


R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 2023889
Conc: 36.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

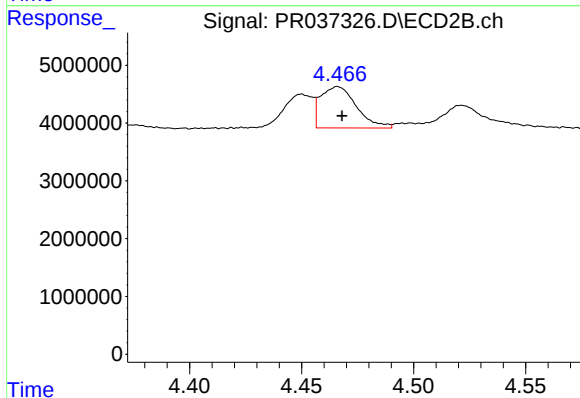


#17 AR-1242-2

R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 7954291
Conc: 34.86 ng/ml

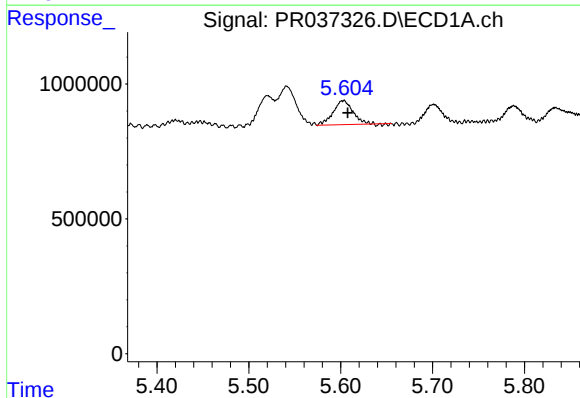


#18 AR-1242-3

R.T.: 5.603 min
Delta R.T.: -0.005 min
Response: 1316189
Conc: 39.99 ng/ml

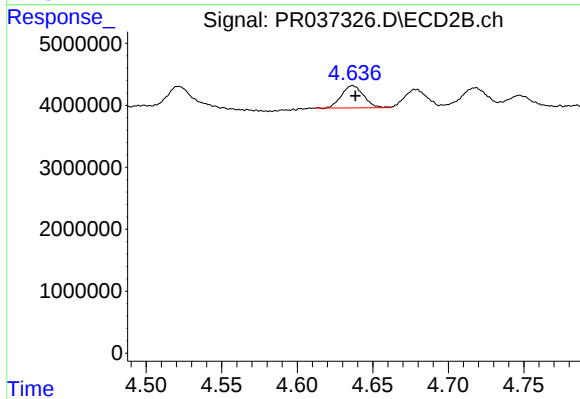

#18 AR-1242-3


R.T.: 4.637 min
Delta R.T.: -0.002 min
Response: 3662192
Conc: 31.67 ng/ml

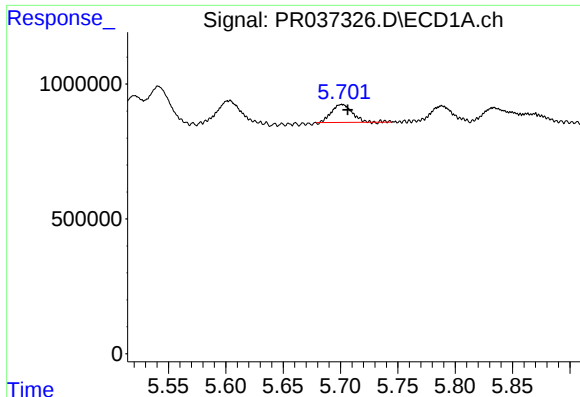

#19 AR-1242-4


R.T.: 5.701 min
Delta R.T.: -0.005 min
Response: 837745
Conc: 31.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

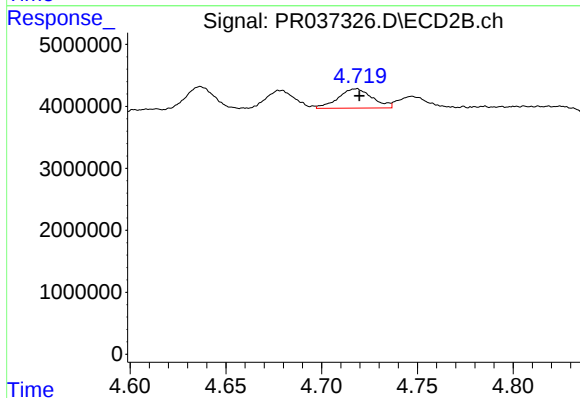


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 3855146
Conc: 35.08 ng/ml

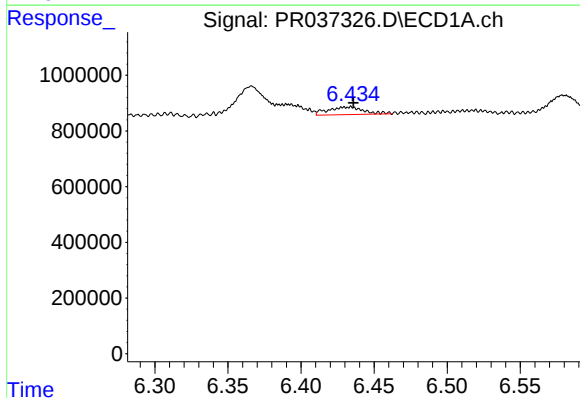


#20 AR-1242-5

R.T.: 6.432 min
Delta R.T.: -0.004 min
Response: 465662
Conc: 14.47 ng/ml

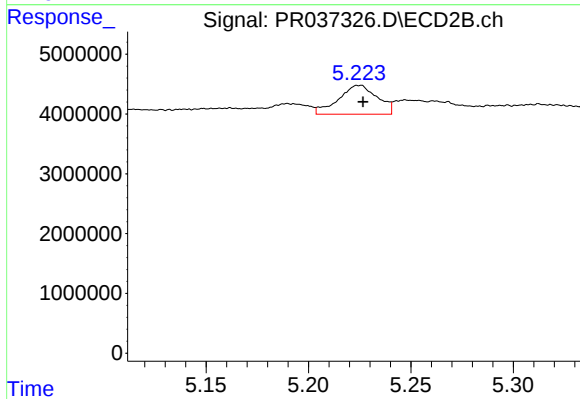

#20 AR-1242-5


R.T.: 5.226 min
Delta R.T.: -0.001 min
Response: 6386681
Conc: 38.54 ng/ml

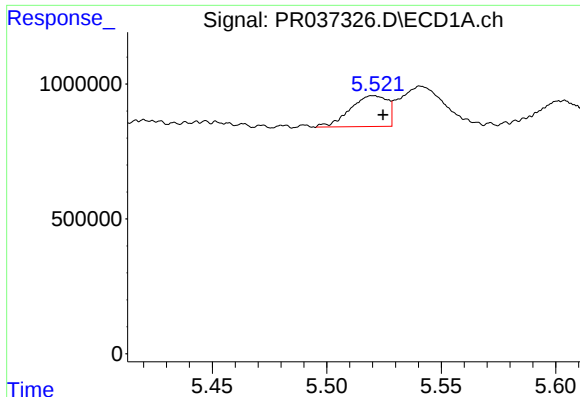

#21 AR-1248-1


R.T.: 5.521 min
Delta R.T.: -0.004 min
Response: 1289468
Conc: 56.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

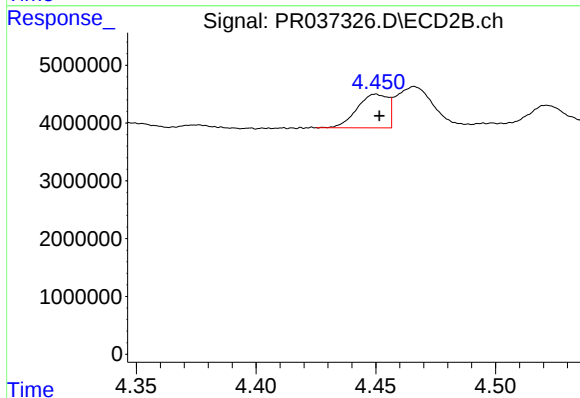


#21 AR-1248-1

R.T.: 4.450 min
Delta R.T.: -0.002 min
Response: 5195284
Conc: 51.61 ng/ml

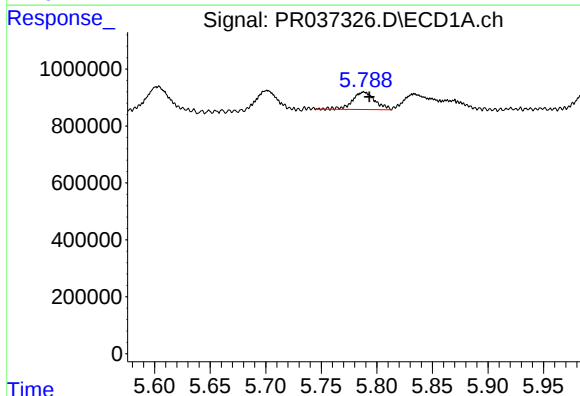


#22 AR-1248-2

R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 856460
Conc: 24.46 ng/ml

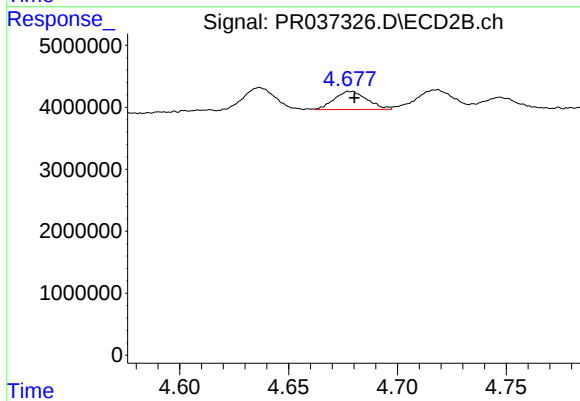

#22 AR-1248-2


R.T.: 4.678 min
Delta R.T.: -0.002 min
Response: 3054888
Conc: 22.38 ng/ml

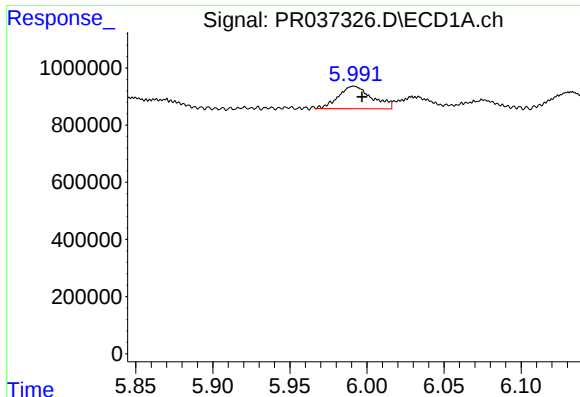

#23 AR-1248-3


R.T.: 5.992 min
Delta R.T.: -0.005 min
Response: 1181448
Conc: 28.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

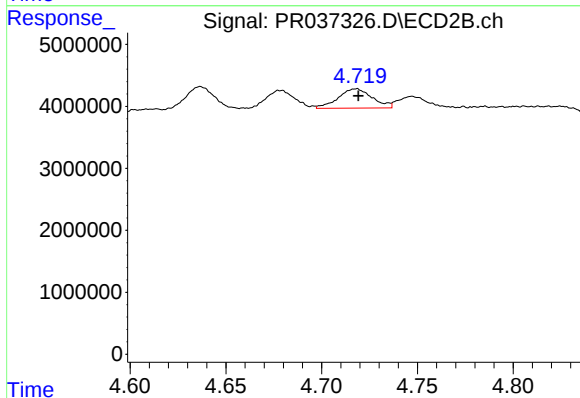


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 3855146
Conc: 27.54 ng/ml

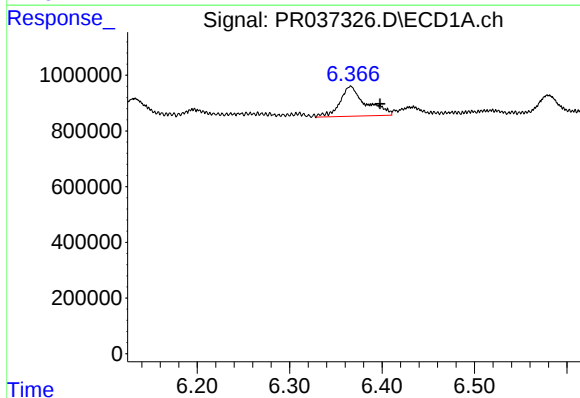


#24 AR-1248-4

R.T.: 6.366 min
Delta R.T.: -0.032 min
Response: 2084683
Conc: 42.58 ng/ml

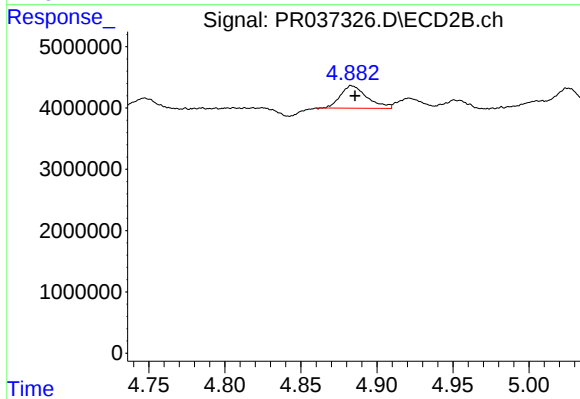

#24 AR-1248-4


R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 4485142
Conc: 25.20 ng/ml

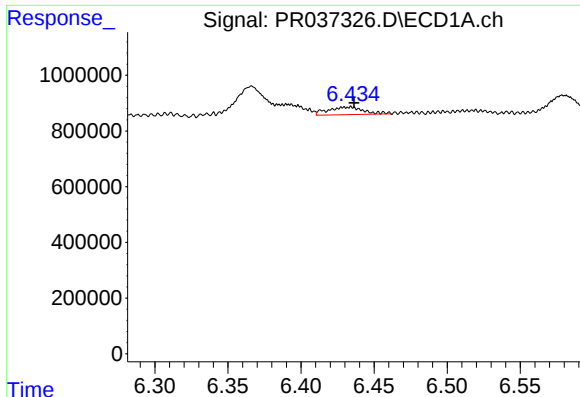

#25 AR-1248-5


R.T.: 6.432 min
Delta R.T.: -0.004 min
Response: 465662
Conc: 9.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

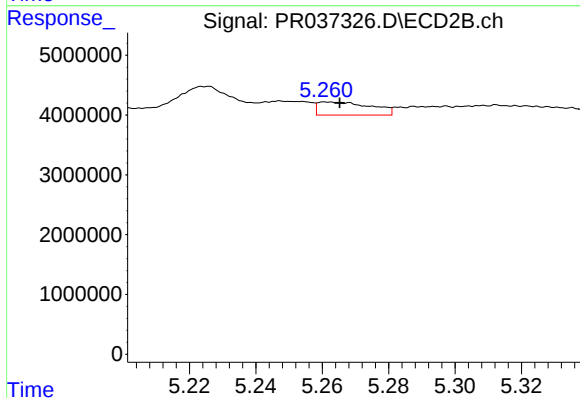


#25 AR-1248-5

R.T.: 5.261 min
Delta R.T.: -0.004 min
Response: 2429161
Conc: 12.42 ng/ml

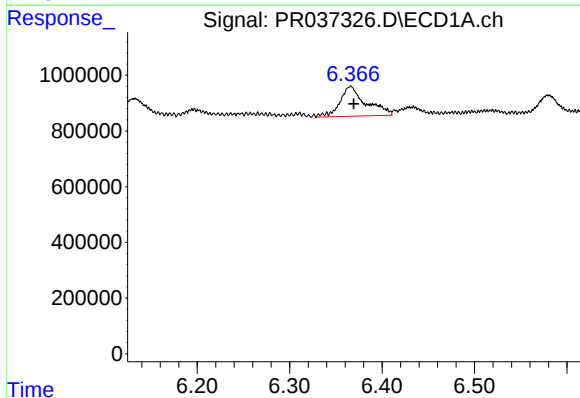


#26 AR-1254-1

R.T.: 6.366 min
Delta R.T.: -0.004 min
Response: 2084683
Conc: 38.16 ng/ml

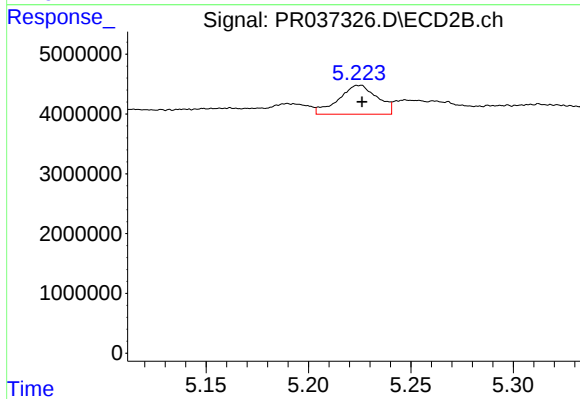

#26 AR-1254-1


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 6386681
Conc: 18.54 ng/ml

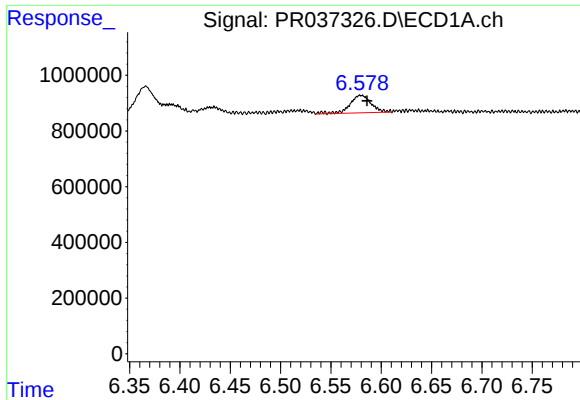

#27 AR-1254-2


R.T.: 6.580 min
Delta R.T.: -0.006 min
Response: 919933
Conc: 10.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

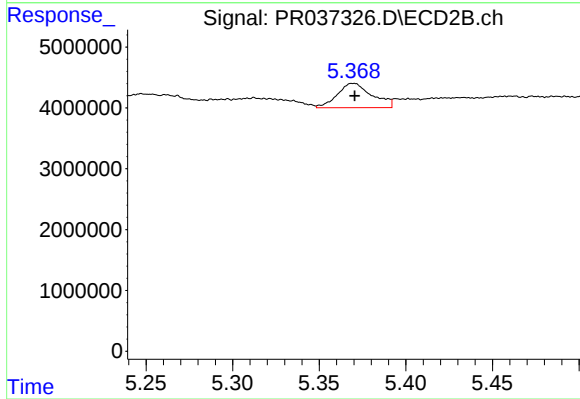


#27 AR-1254-2

R.T.: 5.369 min
Delta R.T.: -0.001 min
Response: 5623620
Conc: 18.78 ng/ml

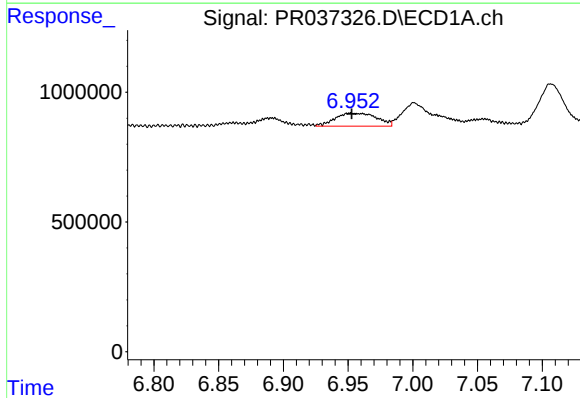


#28 AR-1254-3

R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 1129879
Conc: 12.42 ng/ml

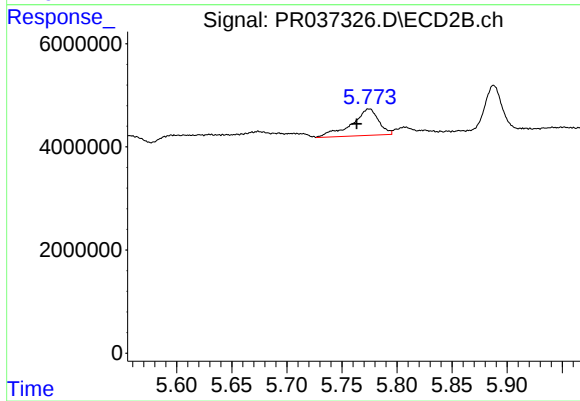

#28 AR-1254-3


R.T.: 5.774 min
Delta R.T.: 0.011 min
Response: 8721996
Conc: 18.42 ng/ml

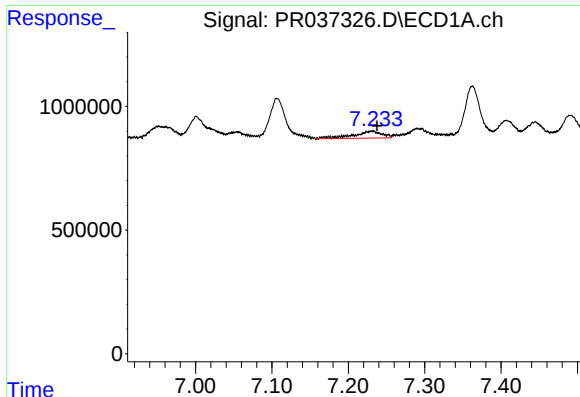

#29 AR-1254-4


R.T.: 7.231 min
Delta R.T.: -0.007 min
Response: 745081
Conc: 11.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

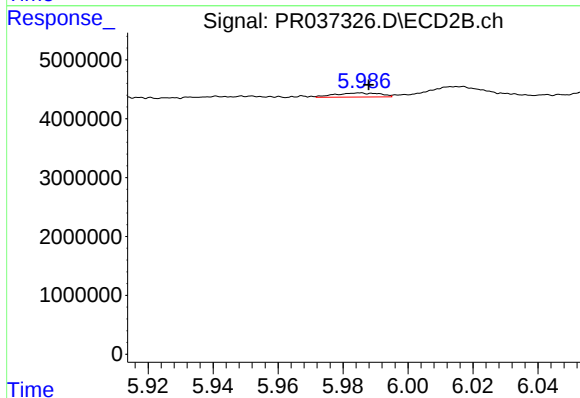


#29 AR-1254-4

R.T.: 5.985 min
Delta R.T.: -0.002 min
Response: 670237
Conc: 1.91 ng/ml

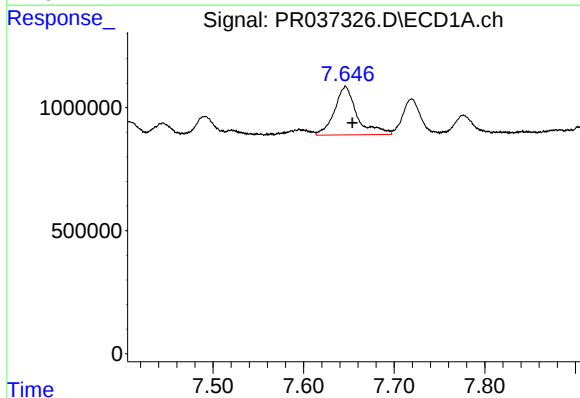


#30 AR-1254-5

R.T.: 7.646 min
Delta R.T.: -0.008 min
Response: 3406535
Conc: 47.39 ng/ml

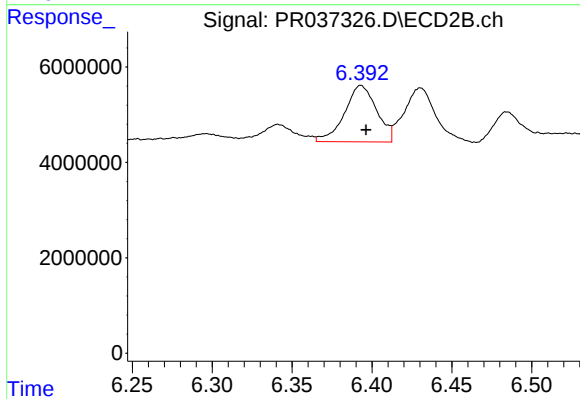

#30 AR-1254-5


R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 16583272
Conc: 37.45 ng/ml

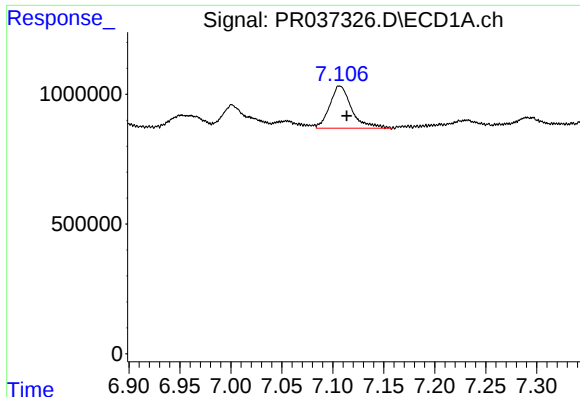

#31 AR-1260-1


R.T.: 7.107 min
Delta R.T.: -0.007 min
Response: 2443209
Conc: 37.03 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

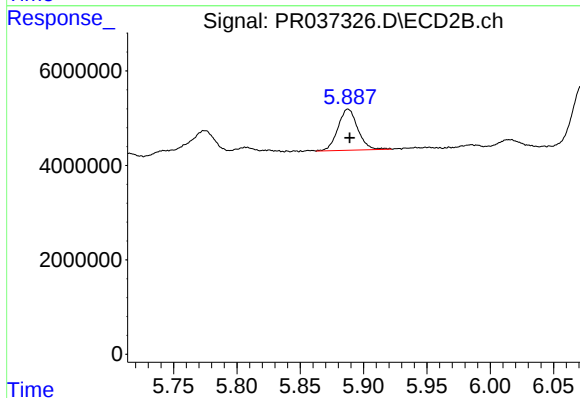


#31 AR-1260-1

R.T.: 5.888 min
Delta R.T.: -0.002 min
Response: 9496134
Conc: 32.49 ng/ml

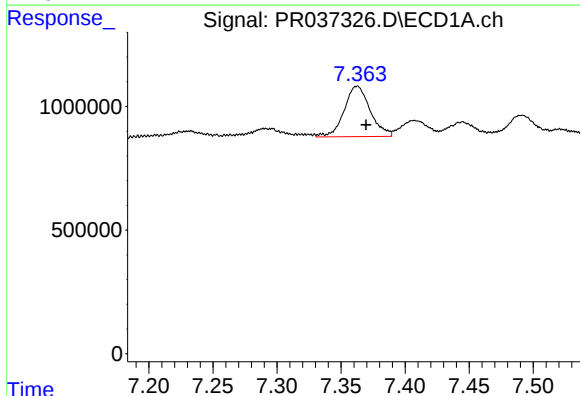


#32 AR-1260-2

R.T.: 7.362 min
Delta R.T.: -0.007 min
Response: 2891225
Conc: 36.27 ng/ml

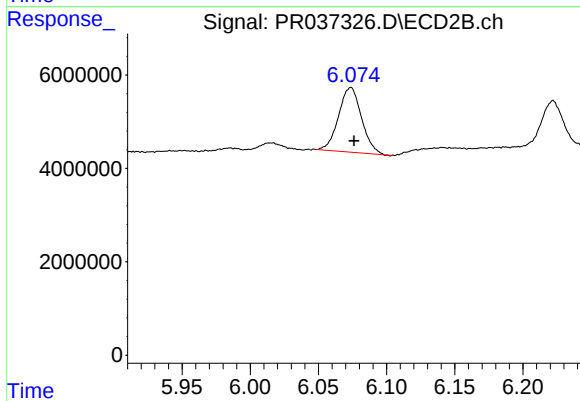

#32 AR-1260-2


R.T.: 6.074 min
Delta R.T.: -0.002 min
Response: 16161218
Conc: 35.09 ng/ml

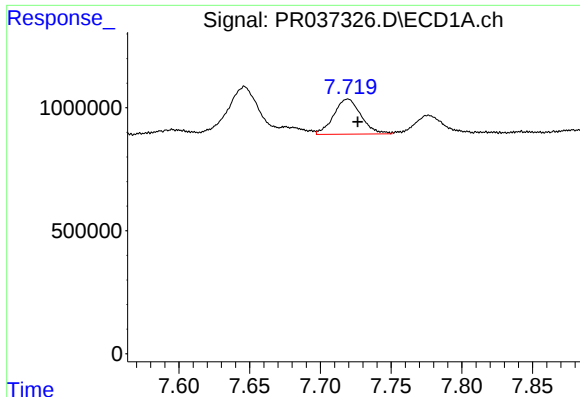

#33 AR-1260-3


R.T.: 7.719 min
Delta R.T.: -0.007 min
Response: 1919359
Conc: 30.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

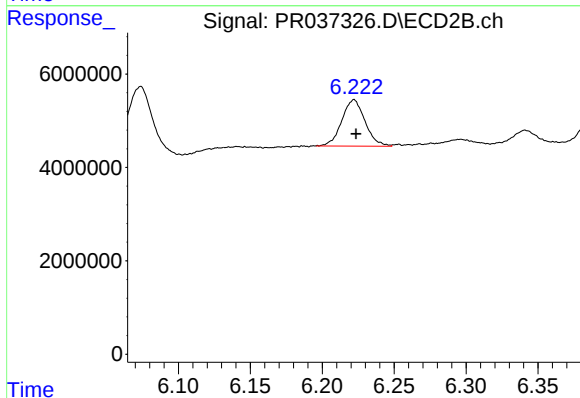


#33 AR-1260-3

R.T.: 6.222 min
Delta R.T.: -0.001 min
Response: 11217303
Conc: 31.47 ng/ml

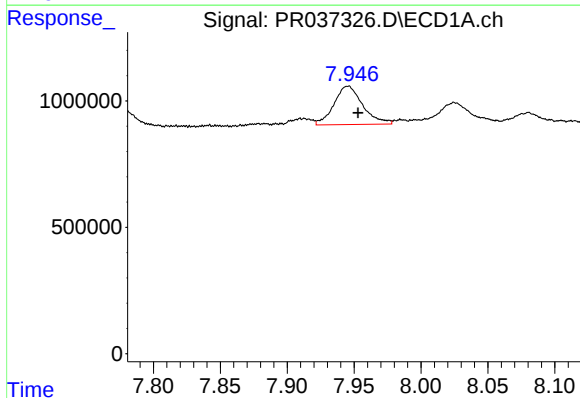


#34 AR-1260-4

R.T.: 7.945 min
Delta R.T.: -0.008 min
Response: 2266286
Conc: 30.46 ng/ml

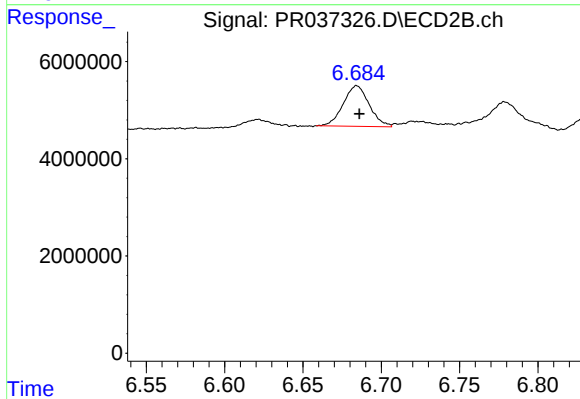

#34 AR-1260-4


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 9640582
Conc: 31.63 ng/ml

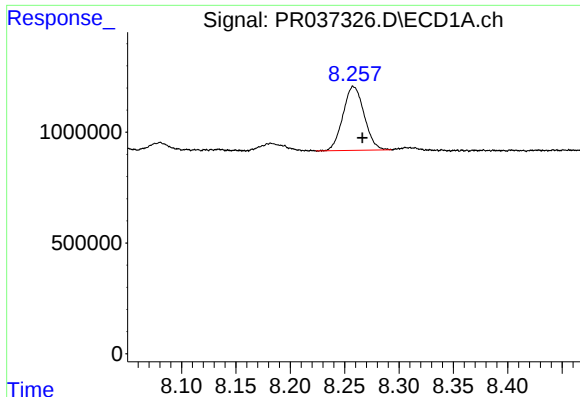

#35 AR-1260-5


R.T.: 8.258 min
Delta R.T.: -0.008 min
Response: 3920733
Conc: 27.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

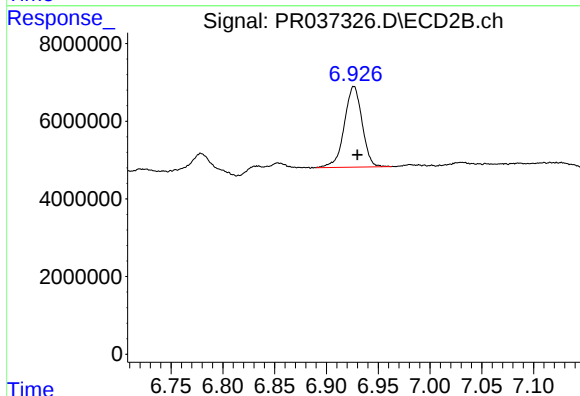


#35 AR-1260-5

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 24899028
Conc: 28.71 ng/ml

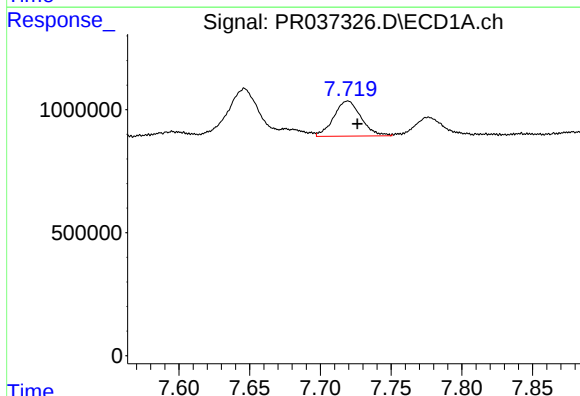


#36 AR-1262-1

R.T.: 7.719 min
Delta R.T.: -0.007 min
Response: 1919359
Conc: 18.38 ng/ml

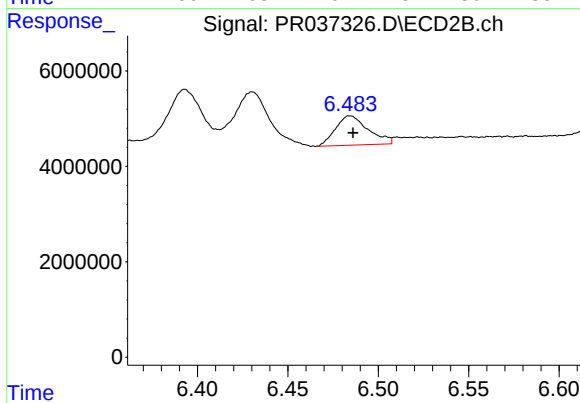

#36 AR-1262-1


R.T.: 6.484 min
Delta R.T.: -0.002 min
Response: 7785643
Conc: 31.07 ng/ml

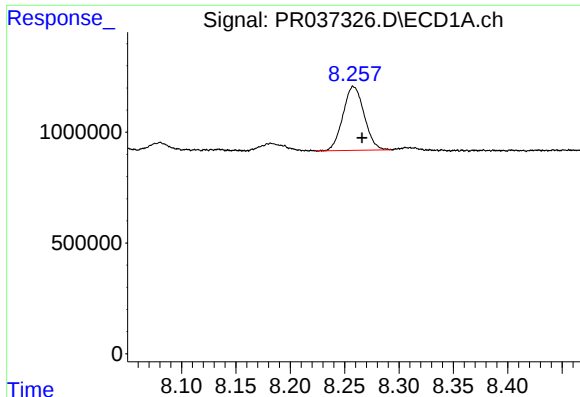

#37 AR-1262-2


R.T.: 8.258 min
Delta R.T.: -0.008 min
Response: 3920733
Conc: 20.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

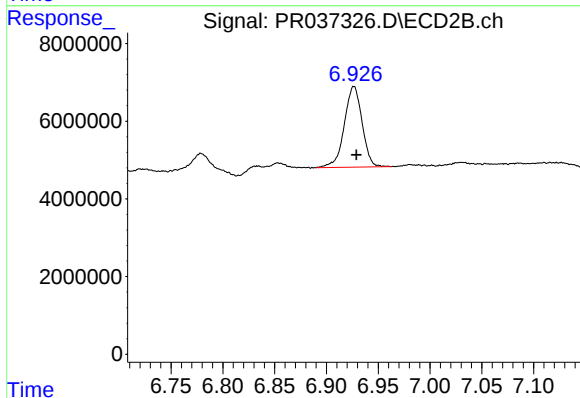


#37 AR-1262-2

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 24899028
Conc: 19.82 ng/ml

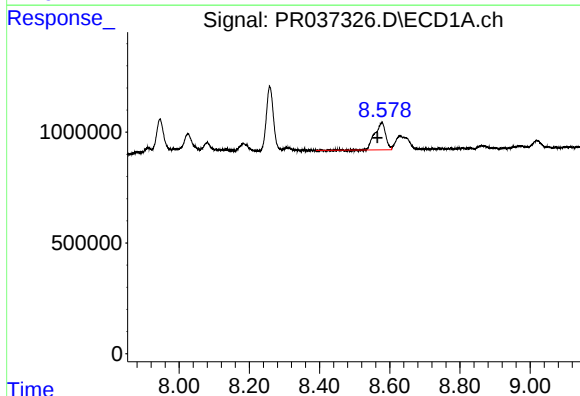


#38 AR-1262-3

R.T.: 8.577 min
Delta R.T.: 0.012 min
Response: 2647928
Conc: 20.13 ng/ml

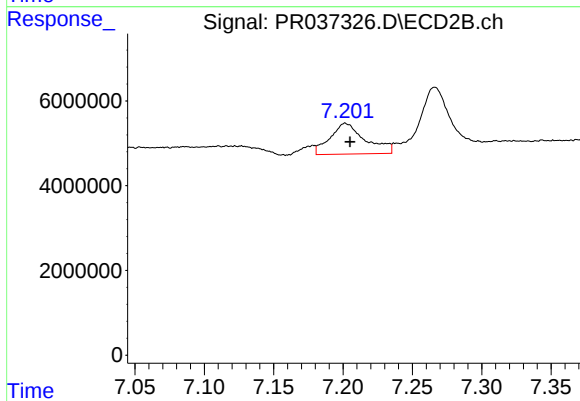

#38 AR-1262-3


R.T.: 7.202 min
Delta R.T.: -0.004 min
Response: 12863288
Conc: 23.46 ng/ml

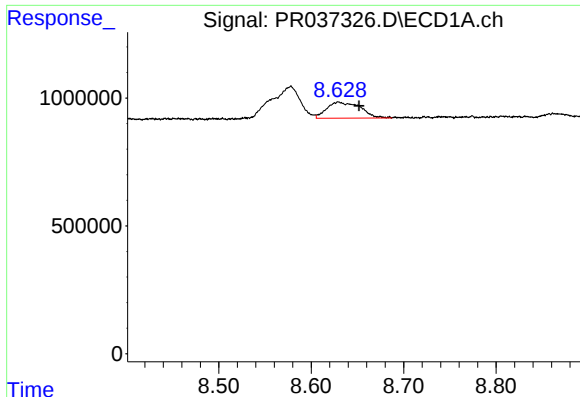

#39 AR-1262-4


R.T.: 8.630 min
Delta R.T.: -0.022 min
Response: 1584247
Conc: 16.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

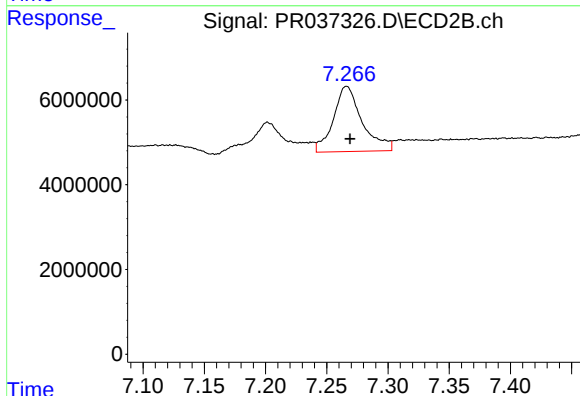


#39 AR-1262-4

R.T.: 7.266 min
Delta R.T.: -0.003 min
Response: 25183164
Conc: 28.05 ng/ml

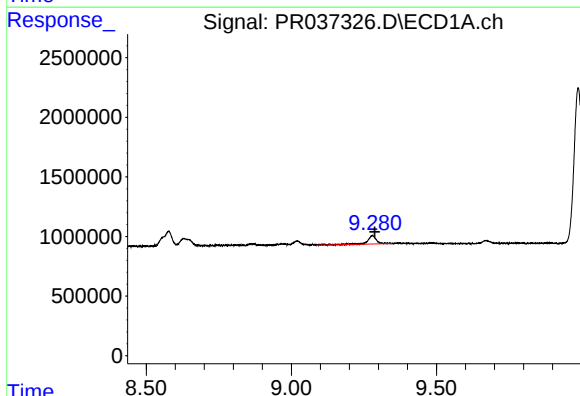


#40 AR-1262-5

R.T.: 9.279 min
Delta R.T.: -0.008 min
Response: 1512610
Conc: 21.91 ng/ml

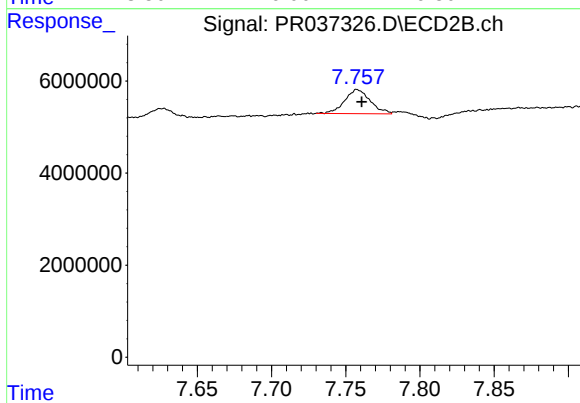

#40 AR-1262-5


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 6283016
Conc: 16.42 ng/ml

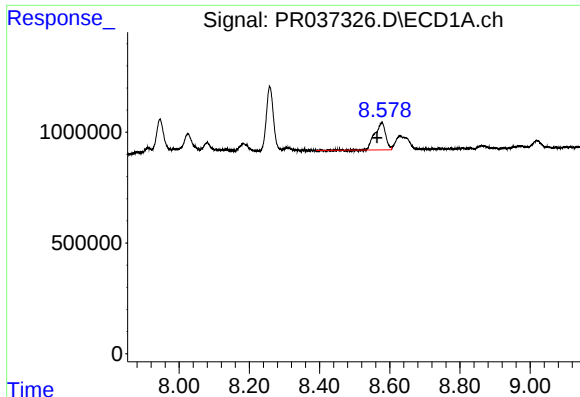

#41 AR-1268-1


R.T.: 8.577 min
Delta R.T.: 0.014 min
Response: 2647928
Conc: 14.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

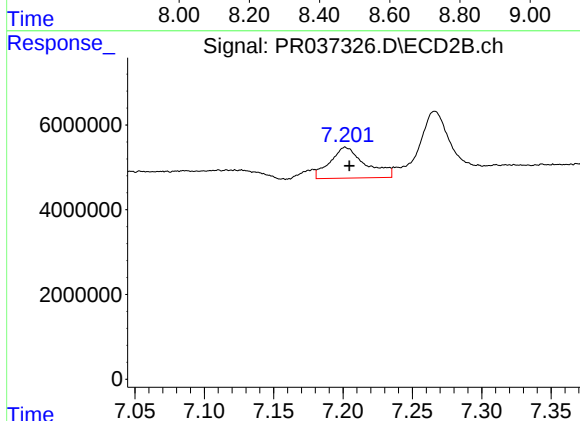


#41 AR-1268-1

R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 12863288
Conc: 10.45 ng/ml

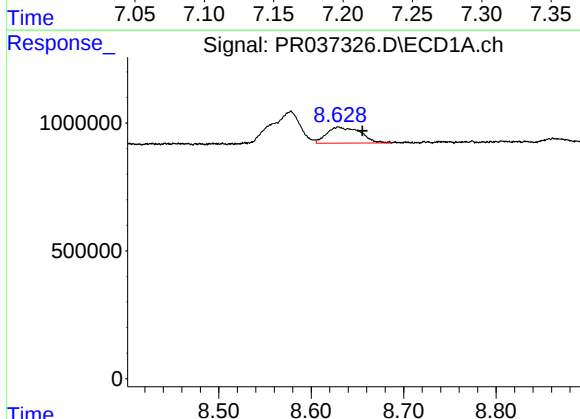


#42 AR-1268-2

R.T.: 8.630 min
Delta R.T.: -0.026 min
Response: 1584247
Conc: 9.63 ng/ml

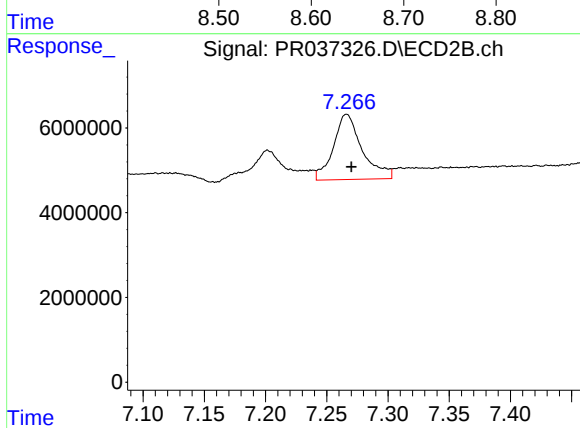

#42 AR-1268-2


R.T.: 7.266 min
Delta R.T.: -0.004 min
Response: 25183164
Conc: 23.78 ng/ml

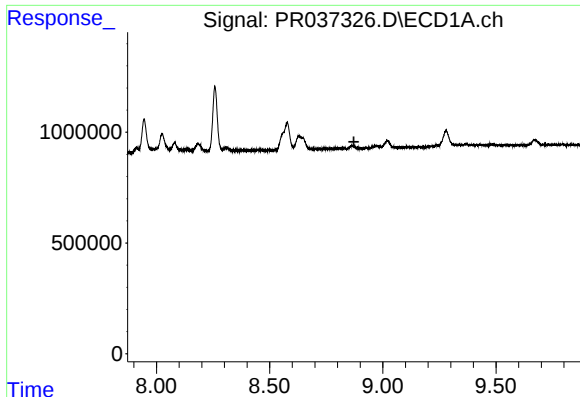

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

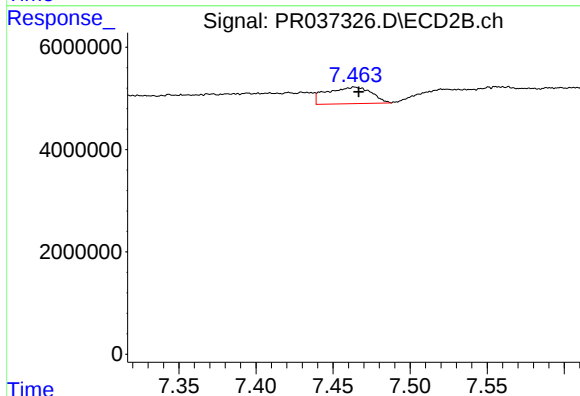


#43 AR-1268-3

R.T.: 7.464 min
Delta R.T.: -0.003 min
Response: 6554258
Conc: 7.40 ng/ml

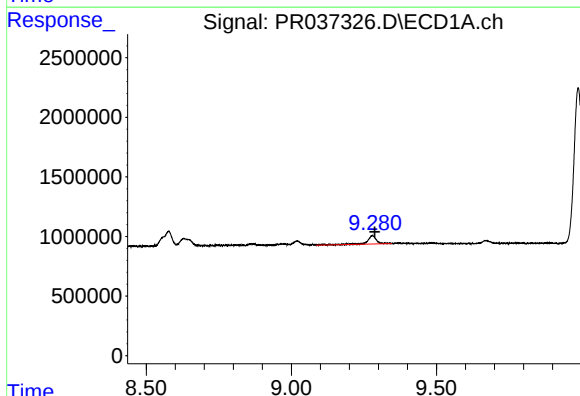


#44 AR-1268-4

R.T.: 9.279 min
Delta R.T.: -0.009 min
Response: 1512610
Conc: 24.25 ng/ml

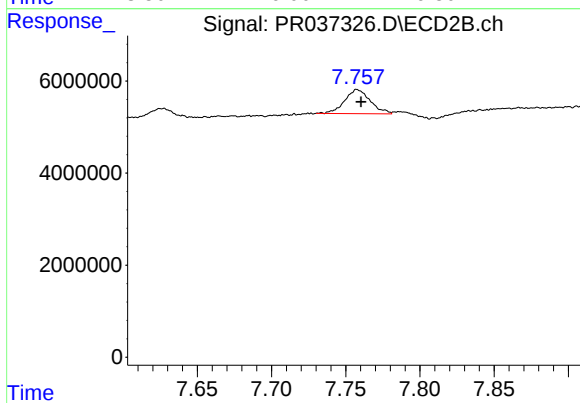

#44 AR-1268-4


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 6283016
Conc: 17.32 ng/ml

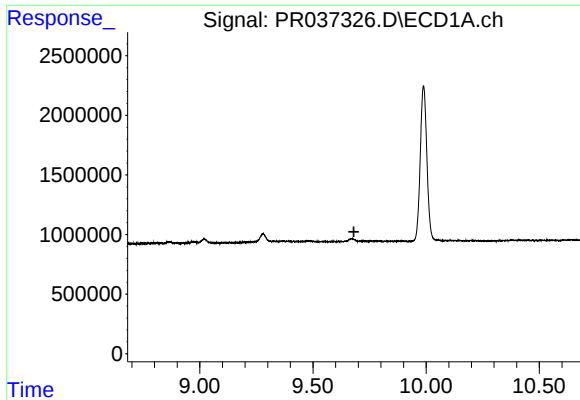

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

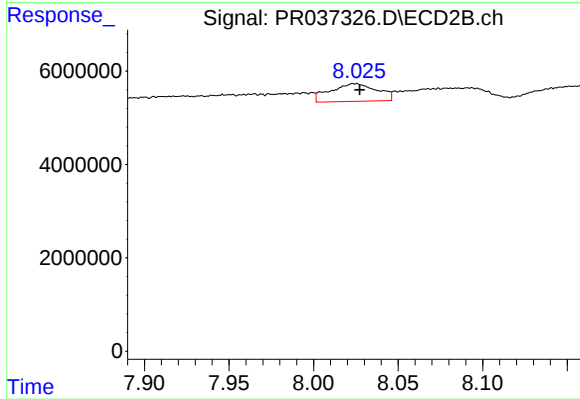

#45 AR-1268-5

R.T.: 8.026 min
Delta R.T.: -0.002 min
Response: 7308037
Conc: 2.87 ng/ml