

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 18:06
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1232 MDL 25PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 22:00:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.408	24052211	93104657	19.226	19.415
2)	SA Decachlor...	9.986	8.244	29309404	141.4E6	22.161	24.285
Target Compounds							
3)	L1 AR-1016-1	5.521	4.467	539438	5581632	12.519	30.655 #
4)	L1 AR-1016-2	5.541	4.467	959912	5581632	13.862	19.784 #
5)	L1 AR-1016-3	5.599	4.636	456346	1459161	11.316	10.148
6)	L1 AR-1016-4	5.700	4.681	520344	1612369	15.845	14.574
7)	L1 AR-1016-5	5.993	4.885	501451	3218978	14.624	21.176 #
8)	L2 AR-1221-1	0.000	3.615	0	1182094	N.D.	23.215 #
9)	L2 AR-1221-2	4.664	3.696	608786	1658288	67.314	44.655 #
10)	L2 AR-1221-3	4.732	3.769	903970	2132791	29.494	17.418 #
11)	L3 AR-1232-1	4.732	3.769	903970	2132791	30.904	18.230 #
12)	L3 AR-1232-2	5.254	4.467	529682	5581632	31.347	40.381 #
13)	L3 AR-1232-3	5.541	4.636	959912	1459161	28.396	20.785 #
14)	L3 AR-1232-4	5.700	4.717	520344	1388572	33.150	23.270 #
15)	L3 AR-1232-5	0.000	4.885	0	3218978	N.D.	47.169 #
16)	L4 AR-1242-1	5.521	4.467	539438	5581632	15.766	38.090 #
17)	L4 AR-1242-2	5.541	4.467	959912	5581632	17.305	24.464 #
18)	L4 AR-1242-3	5.599	4.636	456346	1459161	13.864	12.619
19)	L4 AR-1242-4	5.700	4.717	520344	1388572	19.727	12.634 #
20)	L4 AR-1242-5	6.430	5.226	995351	5853652	30.932	35.327
21)	L5 AR-1248-1	5.521	4.467	539438	5581632	23.549	55.448 #
22)	L5 AR-1248-2	0.000	4.681	0	1612369	N.D.	11.814 #
23)	L5 AR-1248-3	5.993	4.717	501451	1388572	12.258	9.920
24)	L5 AR-1248-4	6.368	4.885	4196548	3218978	85.724	18.088 #
25)	L5 AR-1248-5	6.430	5.248	995351	18775485	21.071	95.983 #
26)	L6 AR-1254-1	6.368	5.226	4196548	5853652	76.816	16.993 #
27)	L6 AR-1254-2	6.588	5.372	682269	7197449	7.961	24.031 #
28)	L6 AR-1254-3	6.964	5.763	1319151	6458096	14.502	13.636
29)	L6 AR-1254-4	7.232	5.987	1724111	606186	25.730	1.729 #
30)	L6 AR-1254-5	0.000	6.394	0	2896752	N.D.	6.542 #
31)	L7 AR-1260-1	0.000	5.901	0	472238	N.D.	1.616 #
32)	L7 AR-1260-2	0.000	6.067	0	4591144	N.D.	9.968 #
33)	L7 AR-1260-3	0.000	6.290	0	3296316	N.D.	9.246 #
34)	L7 AR-1260-4	0.000	6.699	0	708919	N.D.	2.326 #
35)	L7 AR-1260-5	0.000	6.926	0	346499	N.D.	0.400 #
36)	L8 AR-1262-1	0.000	6.492	0	4317016	N.D.	17.225 #
37)	L8 AR-1262-2	0.000	6.926	0	346499	N.D.	0.276 #
38)	L8 AR-1262-3	0.000	7.249	0	36009547	N.D.	65.679 #
39)	L8 AR-1262-4	0.000	7.249	0	36009547	N.D.	40.116 #
40)	L8 AR-1262-5	0.000	7.764	0	393247	N.D.	1.028 #
41)	L9 AR-1268-1	0.000	7.249	0	36009547	N.D.	29.252 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 18:06
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1232 MDL 25PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 22:00:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.249	0	36009547	N.D.	34.006 #
43) L9	AR-1268-3	0.000	7.464	0	12037831	N.D.	13.583 #
44) L9	AR-1268-4	0.000	7.764	0	393247	N.D.	1.084 #
45) L9	AR-1268-5	0.000	8.024	0	2696176	N.D.	1.060 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
Data File : PR037328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 18:06
Operator : SM\SJ
Sample : K1560-03
Misc : AR1232 MDL 25PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 22:00:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

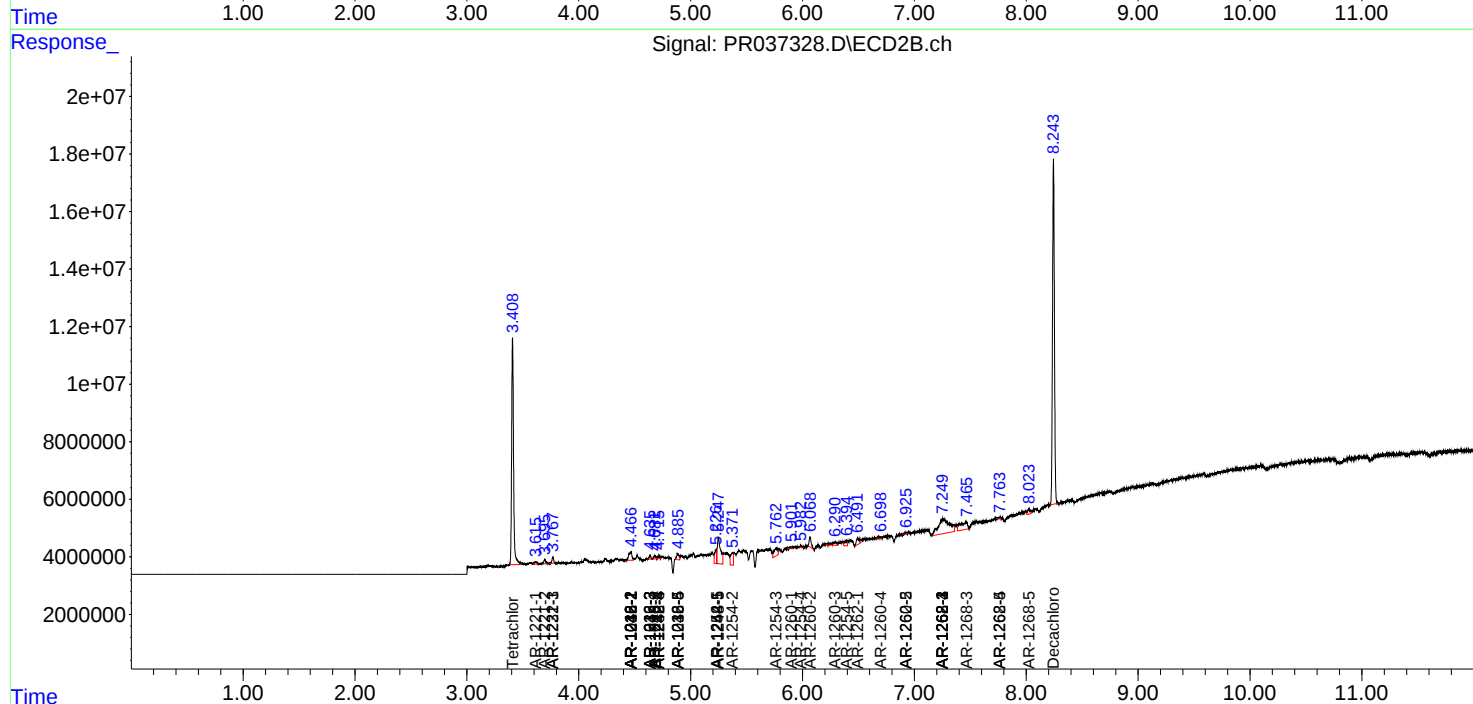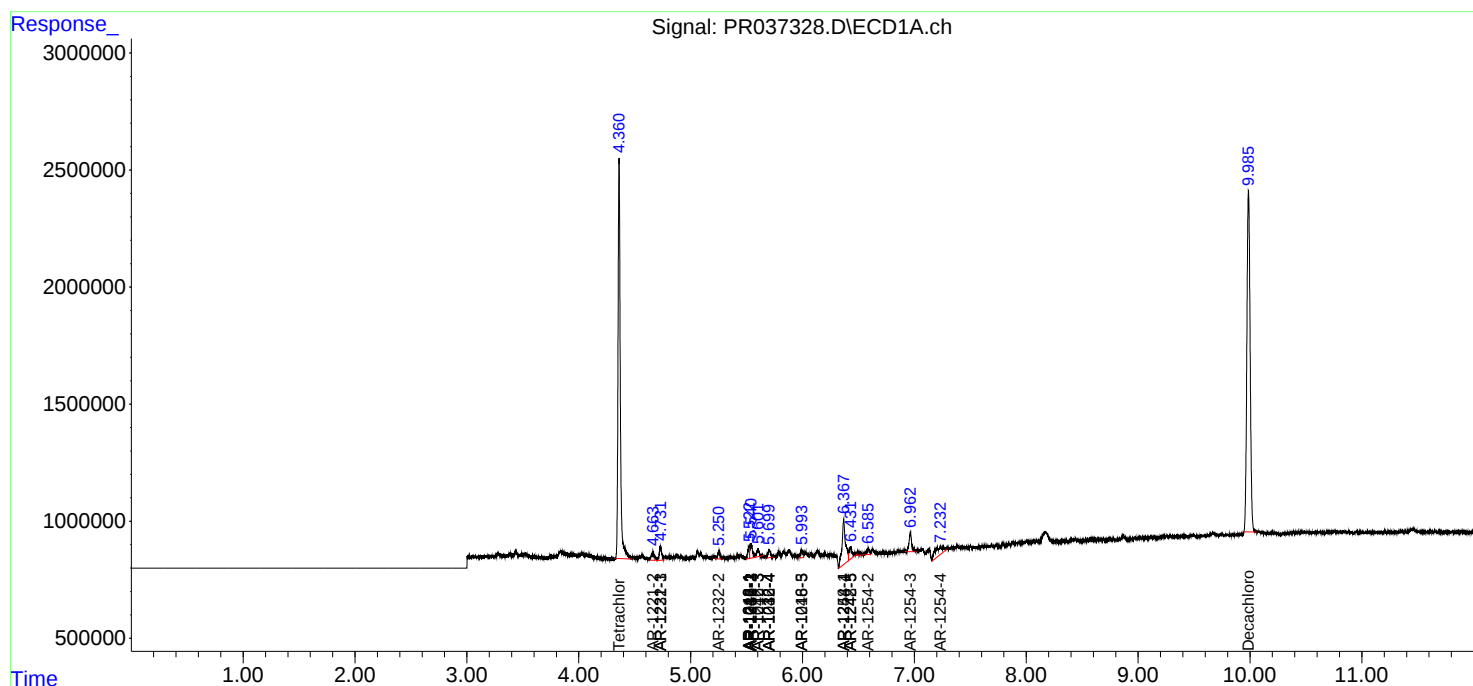


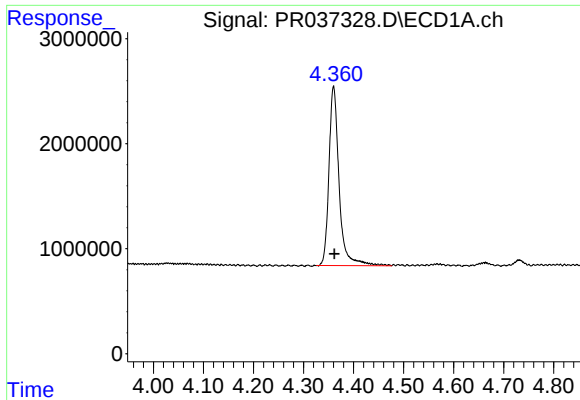

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 24052211
Conc: 19.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

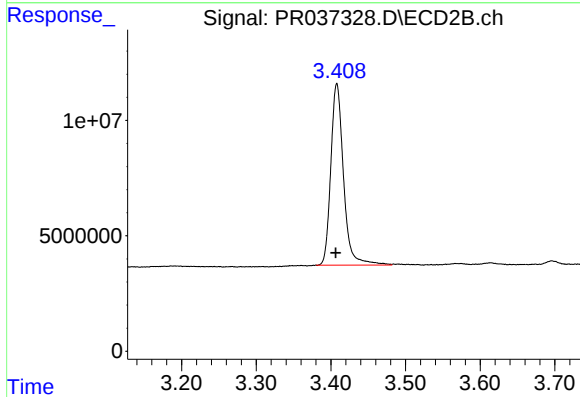


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: 0.002 min
Response: 93104657
Conc: 19.41 ng/ml

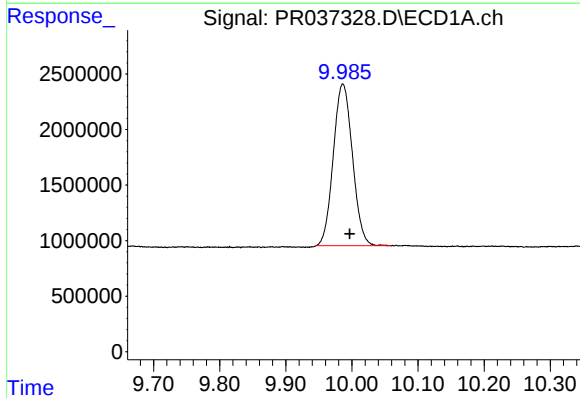


#2 Decachlorobiphenyl

R.T.: 9.986 min
Delta R.T.: -0.010 min
Response: 29309404
Conc: 22.16 ng/ml

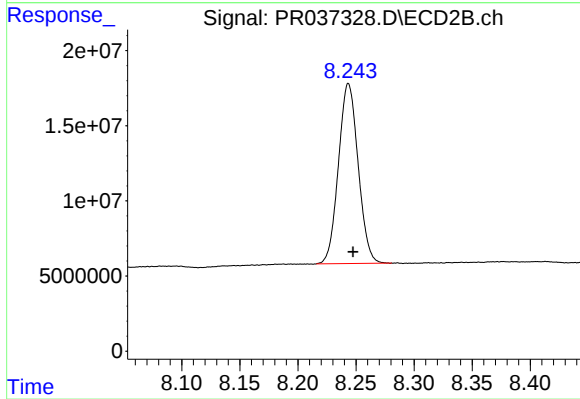

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 141439460
Conc: 24.28 ng/ml

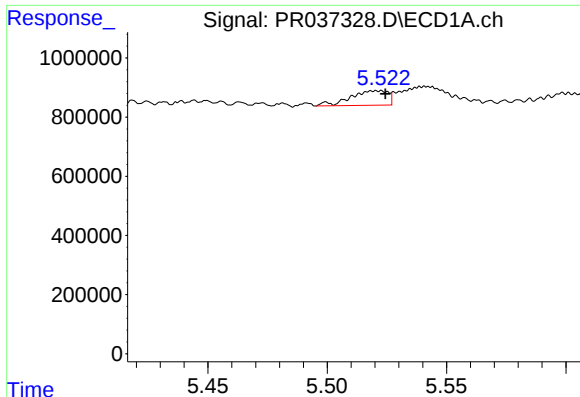

#3 AR-1016-1


R.T.: 5.521 min
Delta R.T.: -0.004 min
Response: 539438
Conc: 12.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

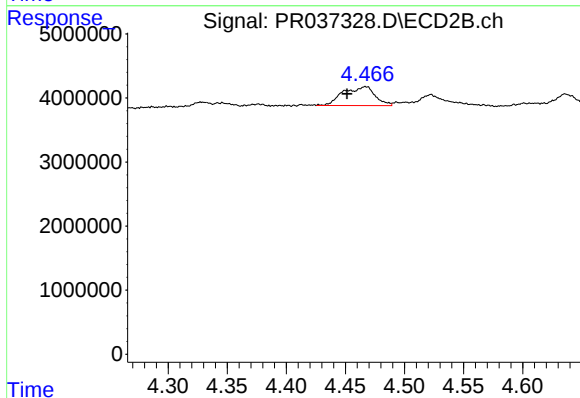


#3 AR-1016-1

R.T.: 4.467 min
Delta R.T.: 0.016 min
Response: 5581632
Conc: 30.65 ng/ml

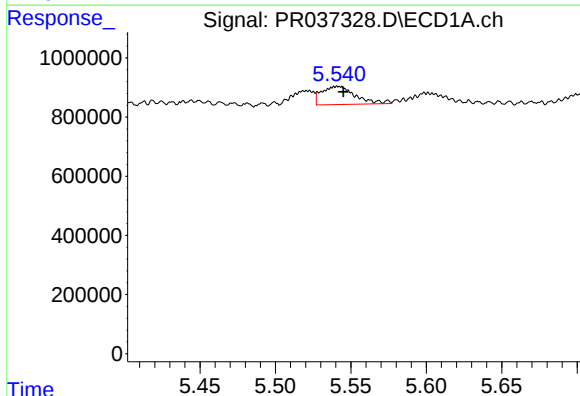


#4 AR-1016-2

R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 959912
Conc: 13.86 ng/ml

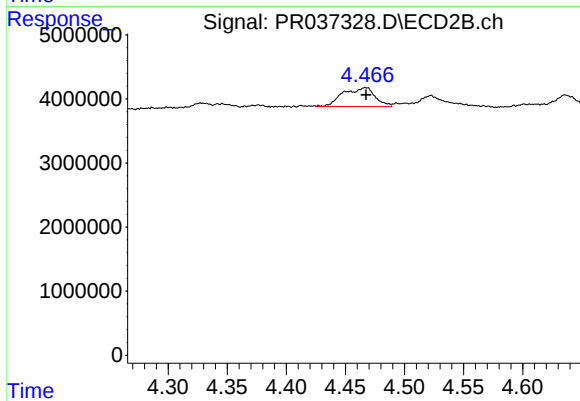

#4 AR-1016-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 5581632
Conc: 19.78 ng/ml

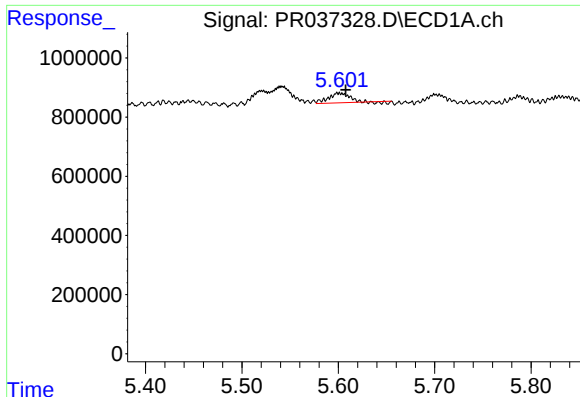

#5 AR-1016-3


R.T.: 5.599 min
Delta R.T.: -0.008 min
Response: 456346
Conc: 11.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

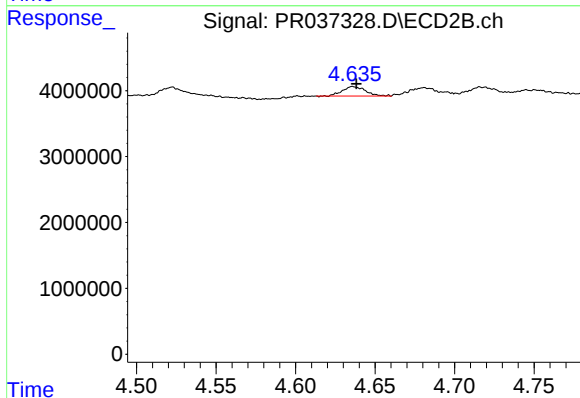


#5 AR-1016-3

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 1459161
Conc: 10.15 ng/ml

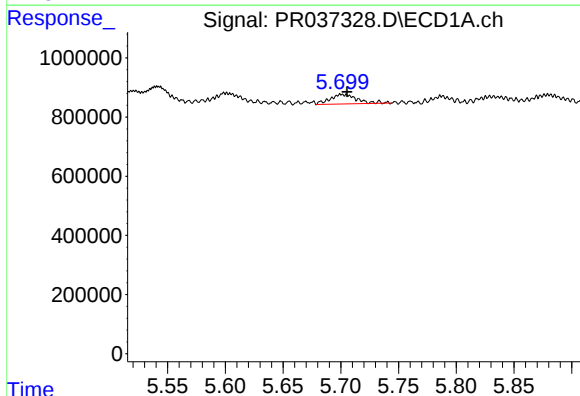


#6 AR-1016-4

R.T.: 5.700 min
Delta R.T.: -0.005 min
Response: 520344
Conc: 15.84 ng/ml

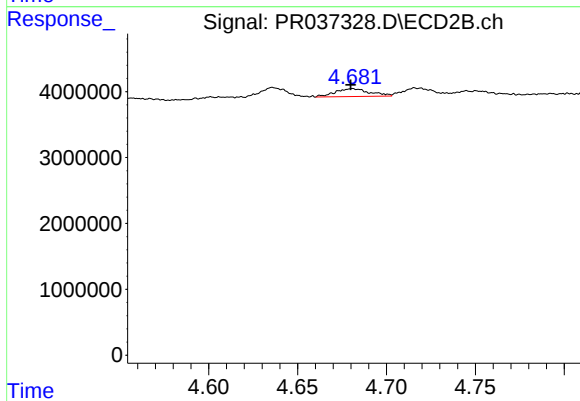

#6 AR-1016-4


R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 1612369
Conc: 14.57 ng/ml

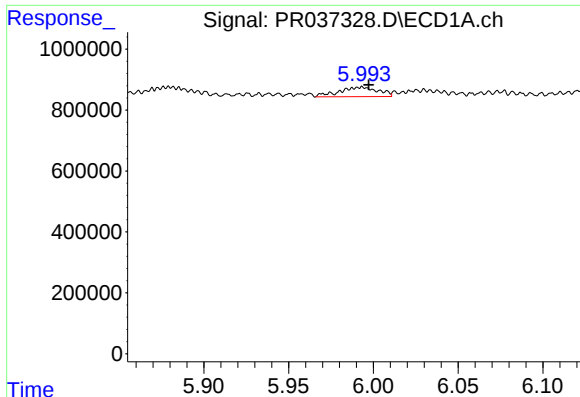

#7 AR-1016-5


R.T.: 5.993 min
Delta R.T.: -0.004 min
Response: 501451
Conc: 14.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

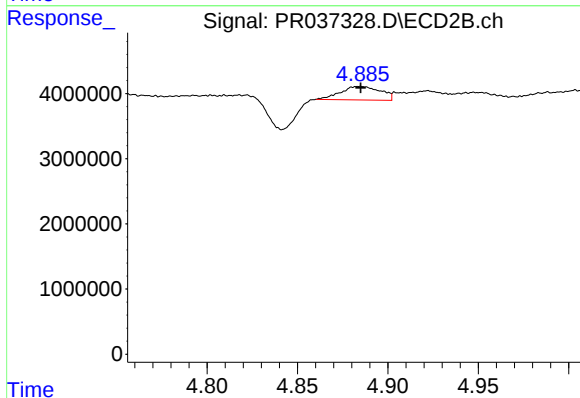


#7 AR-1016-5

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 3218978
Conc: 21.18 ng/ml

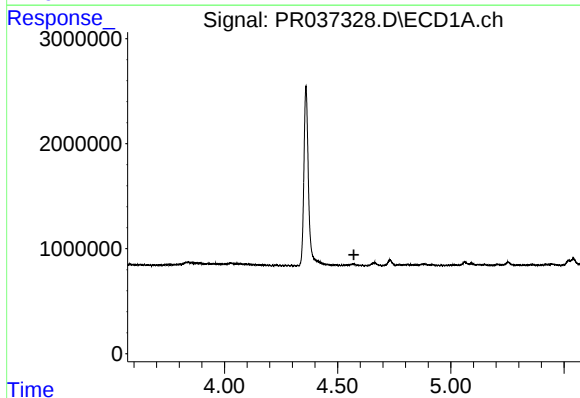


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

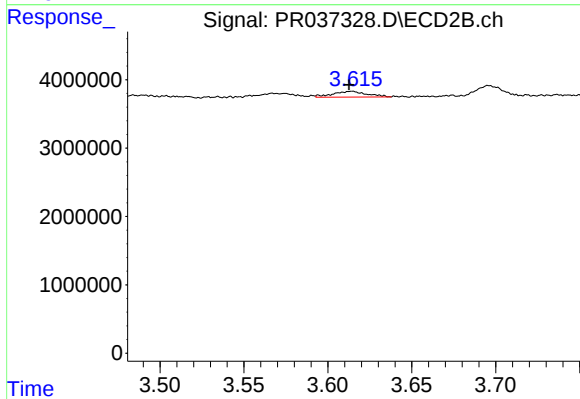

#8 AR-1221-1


R.T.: 3.615 min
Delta R.T.: 0.002 min
Response: 1182094
Conc: 23.22 ng/ml

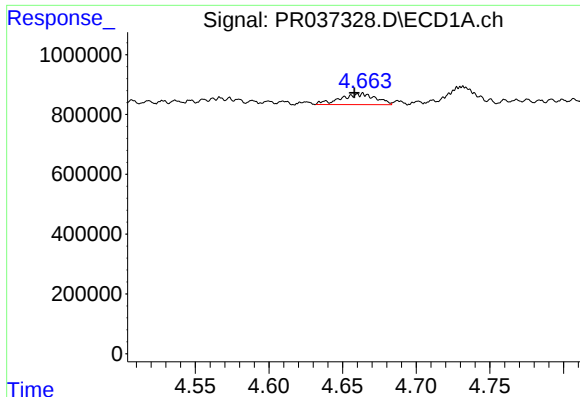

#9 AR-1221-2


R.T.: 4.664 min
Delta R.T.: 0.006 min
Response: 608786
Conc: 67.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

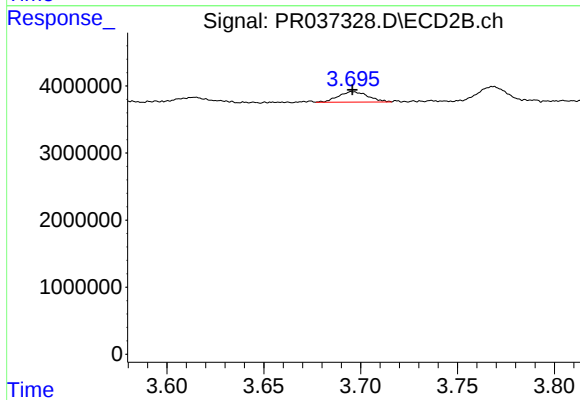


#9 AR-1221-2

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 1658288
Conc: 44.65 ng/ml

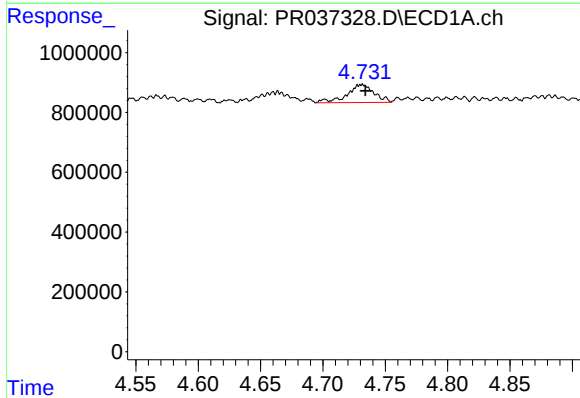


#10 AR-1221-3

R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 903970
Conc: 29.49 ng/ml

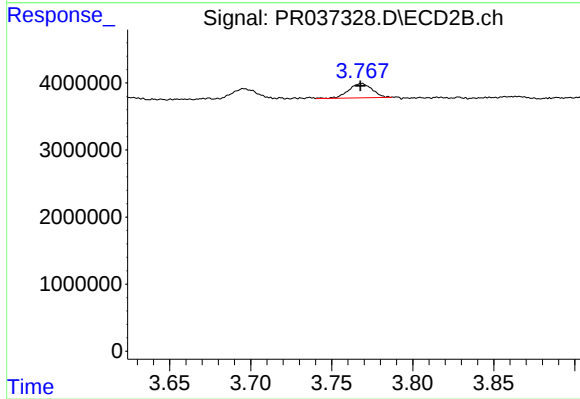

#10 AR-1221-3


R.T.: 3.769 min
Delta R.T.: 0.000 min
Response: 2132791
Conc: 17.42 ng/ml

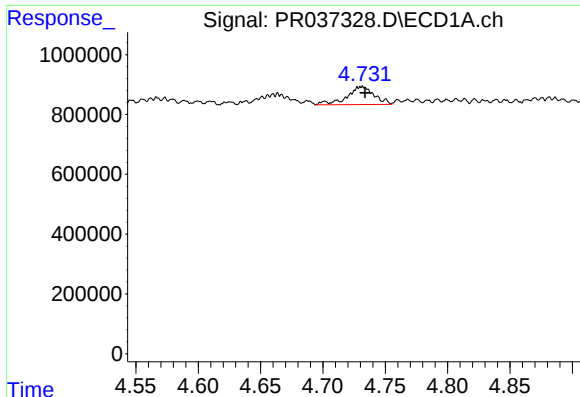

#11 AR-1232-1


R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 903970
Conc: 30.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

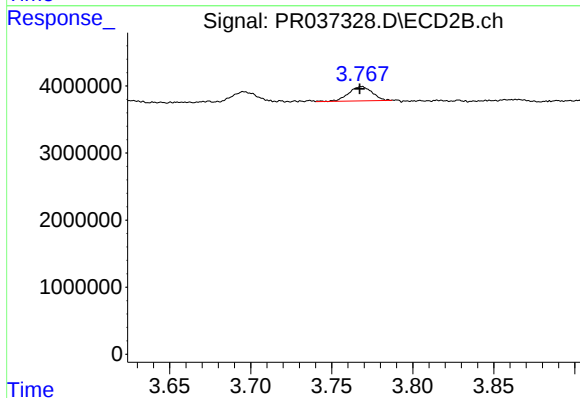


#11 AR-1232-1

R.T.: 3.769 min
Delta R.T.: 0.001 min
Response: 2132791
Conc: 18.23 ng/ml

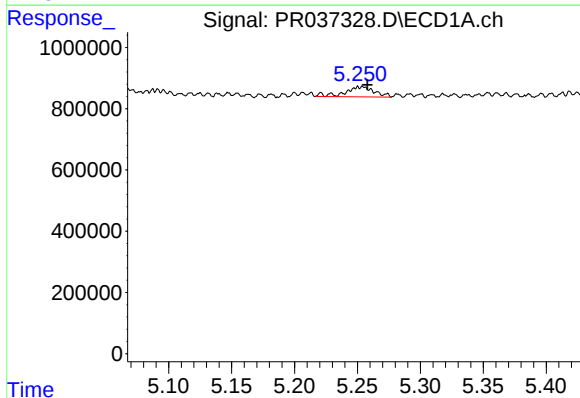


#12 AR-1232-2

R.T.: 5.254 min
Delta R.T.: -0.004 min
Response: 529682
Conc: 31.35 ng/ml

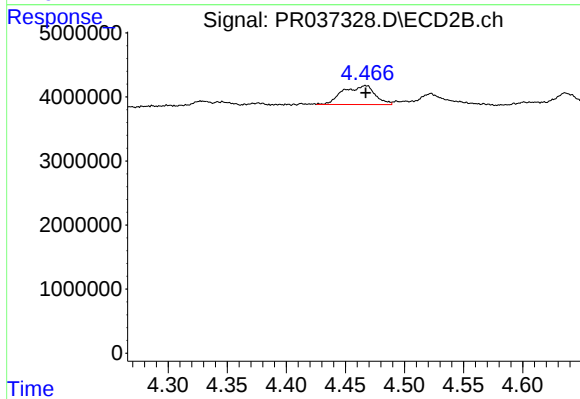

#12 AR-1232-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 5581632
Conc: 40.38 ng/ml

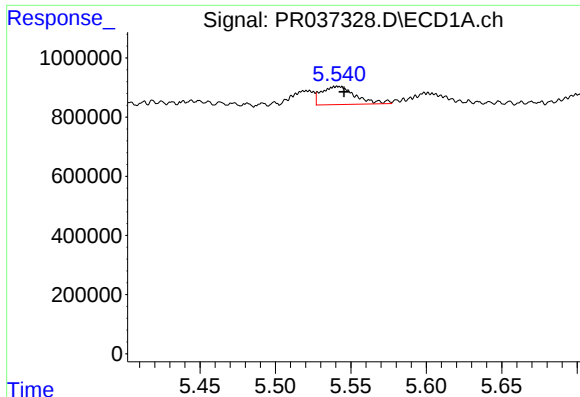

#13 AR-1232-3


R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 959912
Conc: 28.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

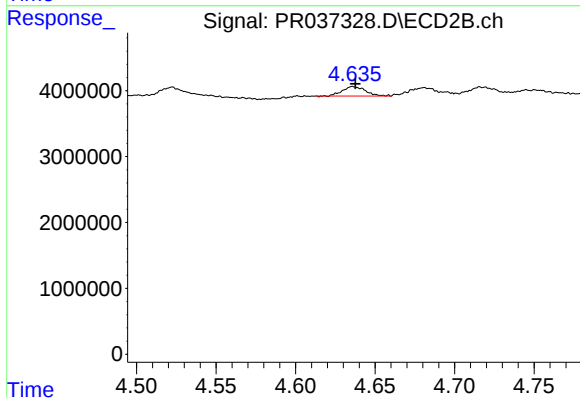


#13 AR-1232-3

R.T.: 4.636 min
Delta R.T.: -0.001 min
Response: 1459161
Conc: 20.79 ng/ml

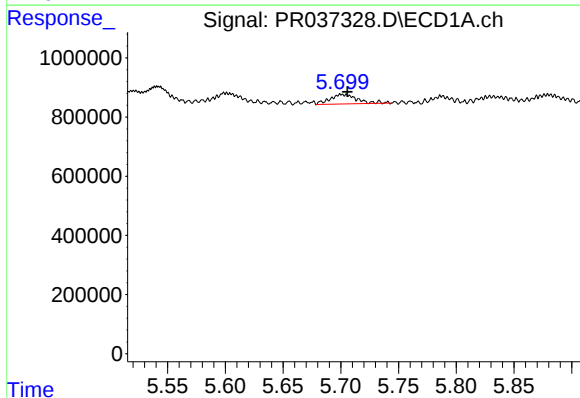


#14 AR-1232-4

R.T.: 5.700 min
Delta R.T.: -0.005 min
Response: 520344
Conc: 33.15 ng/ml

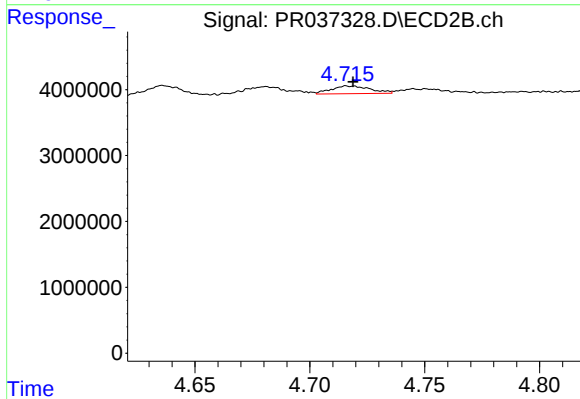

#14 AR-1232-4


R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 1388572
Conc: 23.27 ng/ml

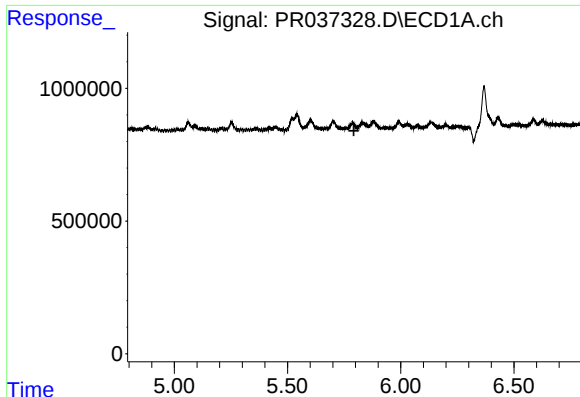

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

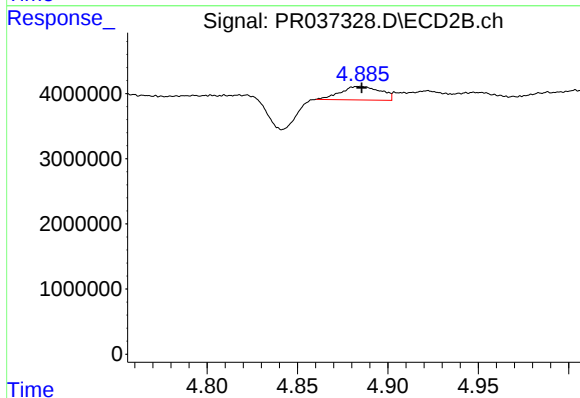


#15 AR-1232-5

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 3218978
Conc: 47.17 ng/ml

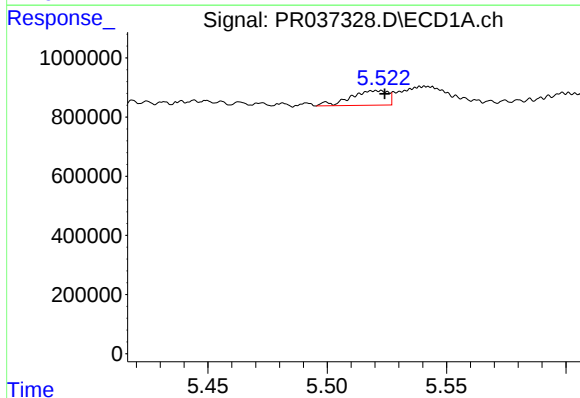


#16 AR-1242-1

R.T.: 5.521 min
Delta R.T.: -0.003 min
Response: 539438
Conc: 15.77 ng/ml

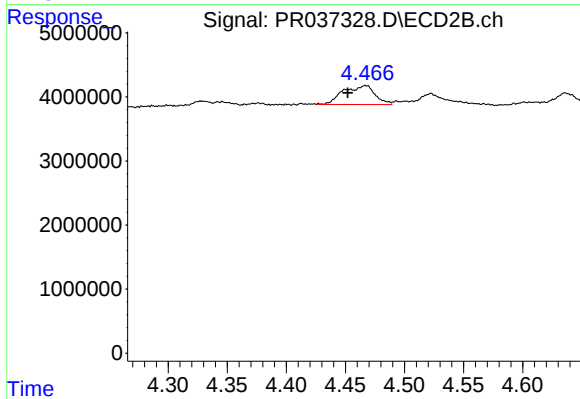

#16 AR-1242-1


R.T.: 4.467 min
Delta R.T.: 0.015 min
Response: 5581632
Conc: 38.09 ng/ml

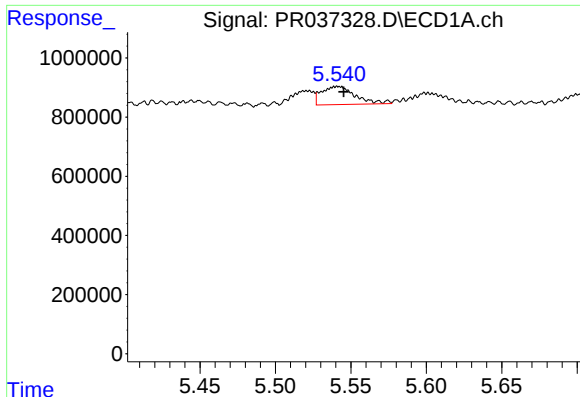

#17 AR-1242-2


R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 959912
Conc: 17.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

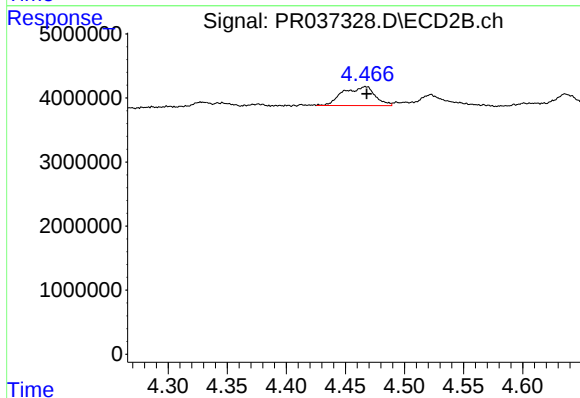


#17 AR-1242-2

R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 5581632
Conc: 24.46 ng/ml

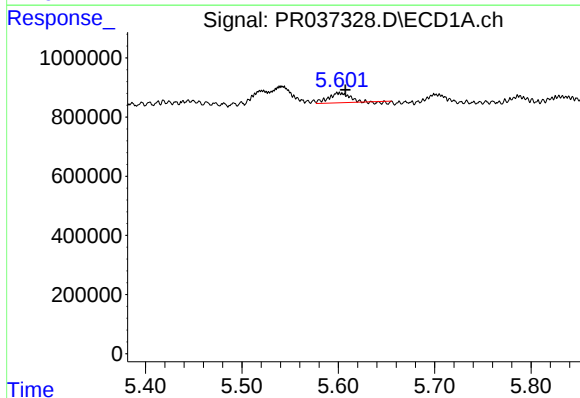


#18 AR-1242-3

R.T.: 5.599 min
Delta R.T.: -0.008 min
Response: 456346
Conc: 13.86 ng/ml

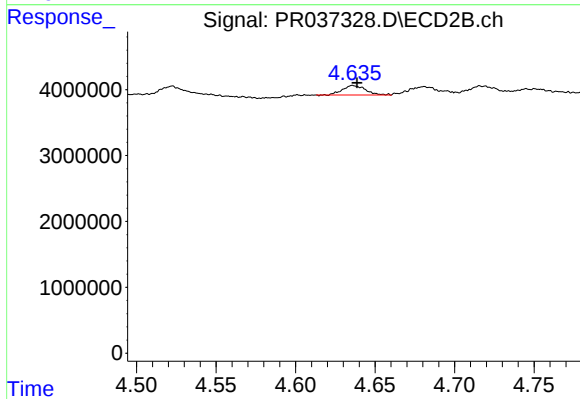

#18 AR-1242-3


R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 1459161
Conc: 12.62 ng/ml

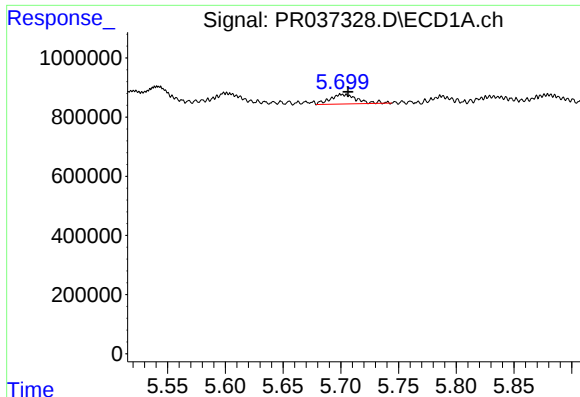

#19 AR-1242-4


R.T.: 5.700 min
Delta R.T.: -0.006 min
Response: 520344
Conc: 19.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

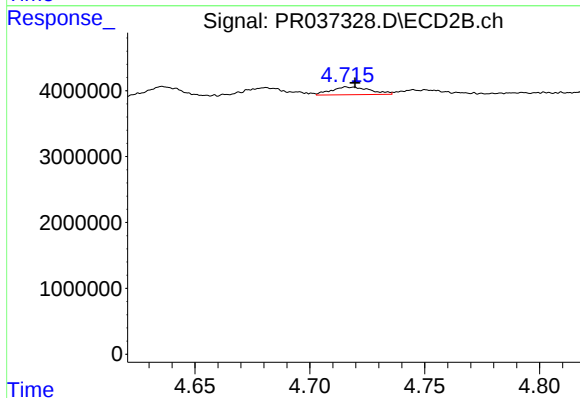


#19 AR-1242-4

R.T.: 4.717 min
Delta R.T.: -0.003 min
Response: 1388572
Conc: 12.63 ng/ml

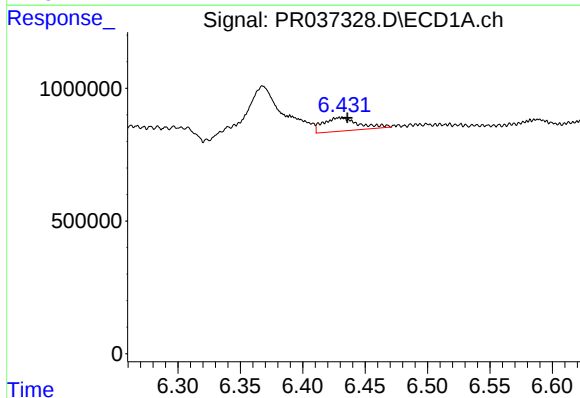


#20 AR-1242-5

R.T.: 6.430 min
Delta R.T.: -0.006 min
Response: 995351
Conc: 30.93 ng/ml

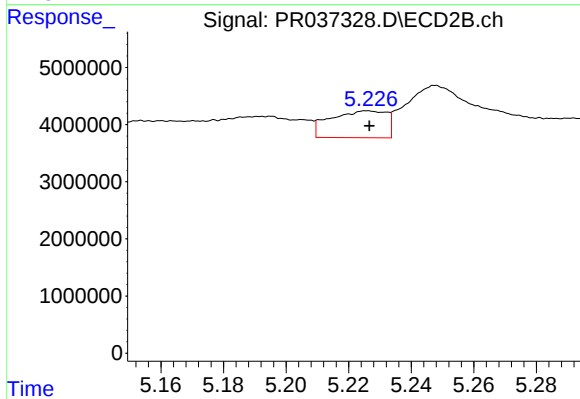

#20 AR-1242-5


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 5853652
Conc: 35.33 ng/ml

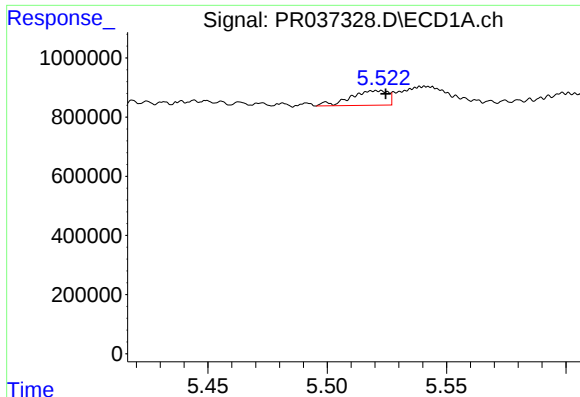

#21 AR-1248-1


R.T.: 5.521 min
Delta R.T.: -0.004 min
Response: 539438
Conc: 23.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

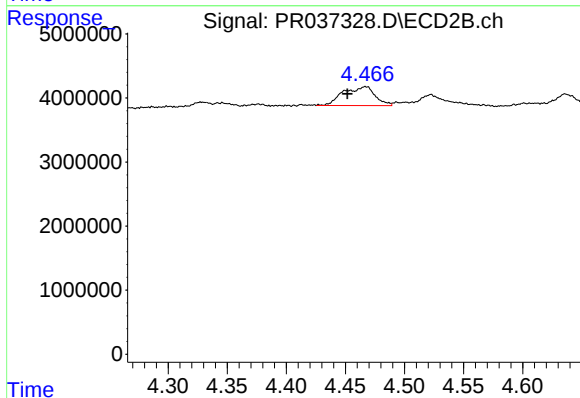


#21 AR-1248-1

R.T.: 4.467 min
Delta R.T.: 0.016 min
Response: 5581632
Conc: 55.45 ng/ml

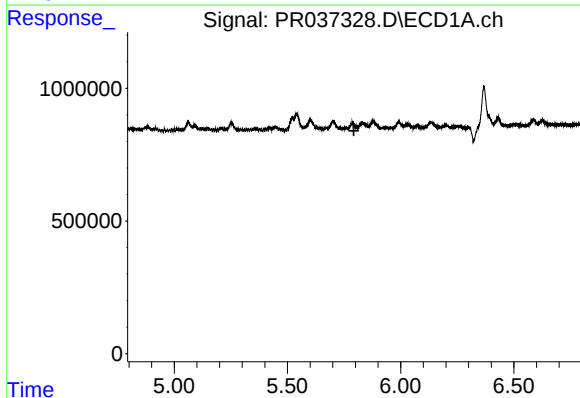


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.793 min
Response: 0
Conc: N.D.

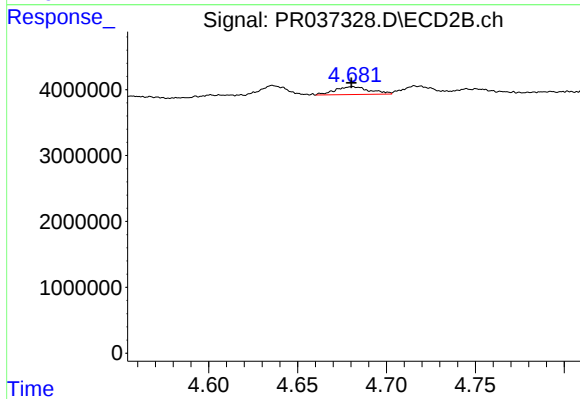

#22 AR-1248-2


R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 1612369
Conc: 11.81 ng/ml

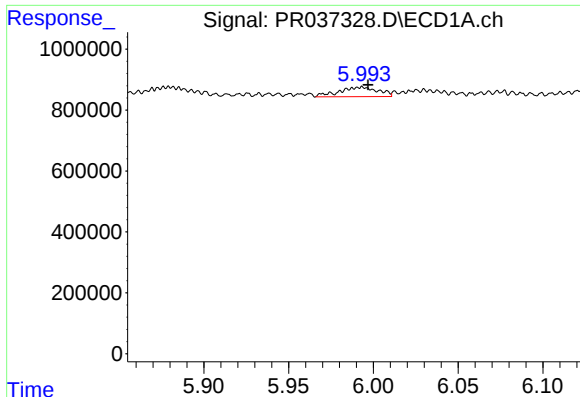

#23 AR-1248-3


R.T.: 5.993 min
Delta R.T.: -0.004 min
Response: 501451
Conc: 12.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

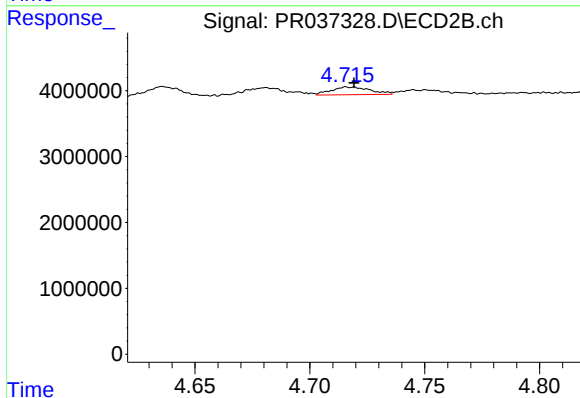


#23 AR-1248-3

R.T.: 4.717 min
Delta R.T.: -0.003 min
Response: 1388572
Conc: 9.92 ng/ml

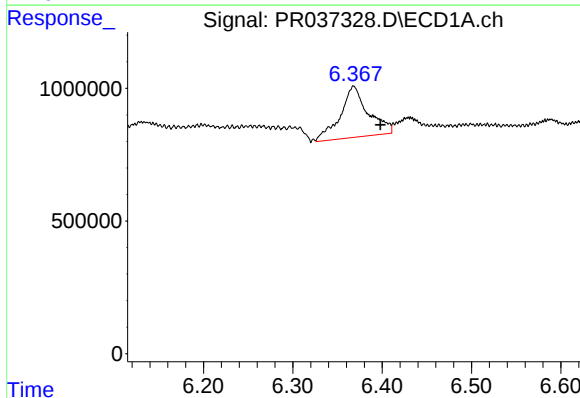


#24 AR-1248-4

R.T.: 6.368 min
Delta R.T.: -0.030 min
Response: 4196548
Conc: 85.72 ng/ml

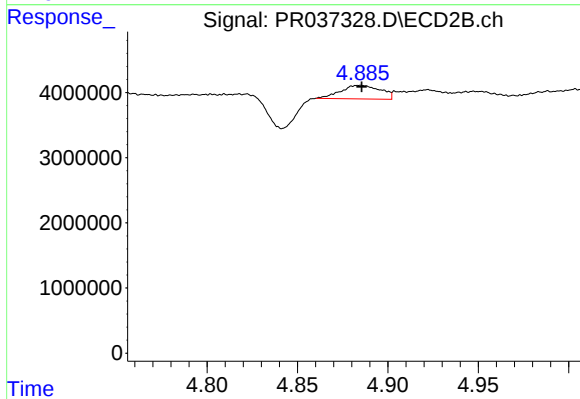

#24 AR-1248-4


R.T.: 4.885 min
Delta R.T.: -0.001 min
Response: 3218978
Conc: 18.09 ng/ml

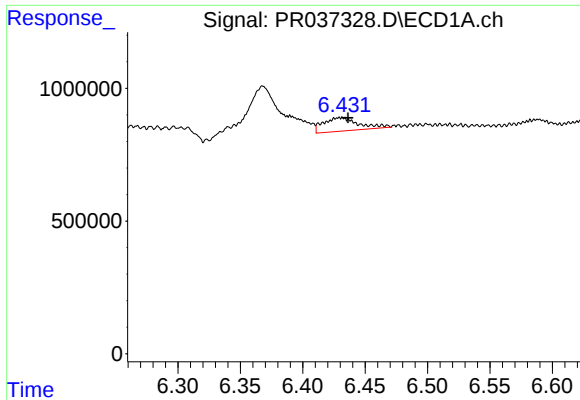

#25 AR-1248-5


R.T.: 6.430 min
Delta R.T.: -0.007 min
Response: 995351
Conc: 21.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

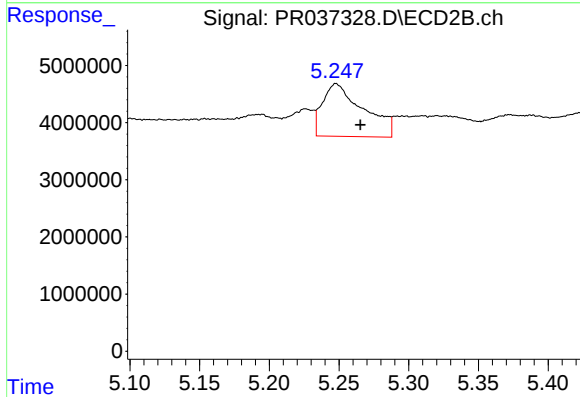


#25 AR-1248-5

R.T.: 5.248 min
Delta R.T.: -0.017 min
Response: 18775485
Conc: 95.98 ng/ml

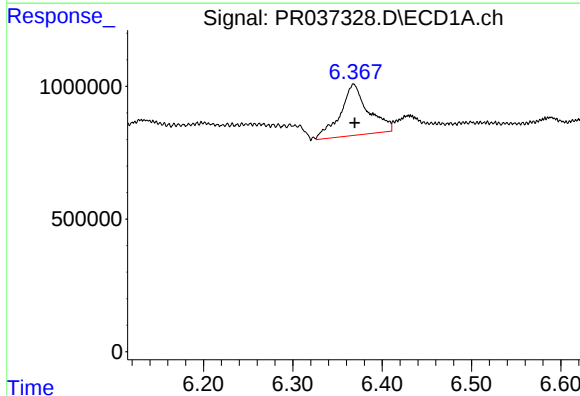


#26 AR-1254-1

R.T.: 6.368 min
Delta R.T.: -0.001 min
Response: 4196548
Conc: 76.82 ng/ml

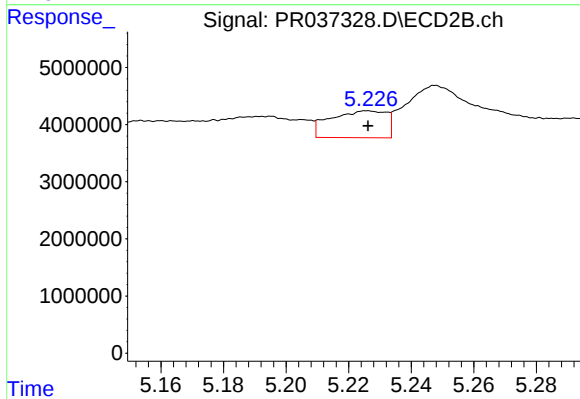

#26 AR-1254-1


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 5853652
Conc: 16.99 ng/ml

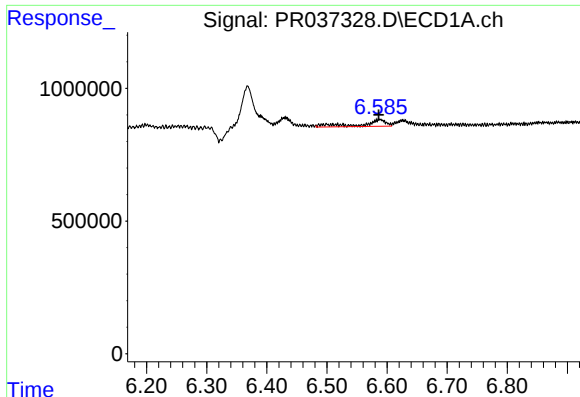

#27 AR-1254-2


R.T.: 6.588 min
Delta R.T.: 0.002 min
Response: 682269
Conc: 7.96 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

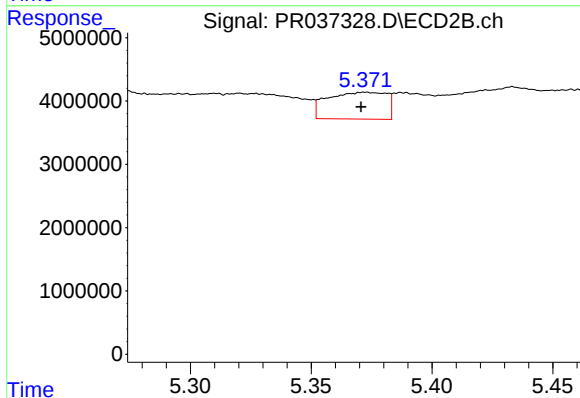


#27 AR-1254-2

R.T.: 5.372 min
Delta R.T.: 0.002 min
Response: 7197449
Conc: 24.03 ng/ml

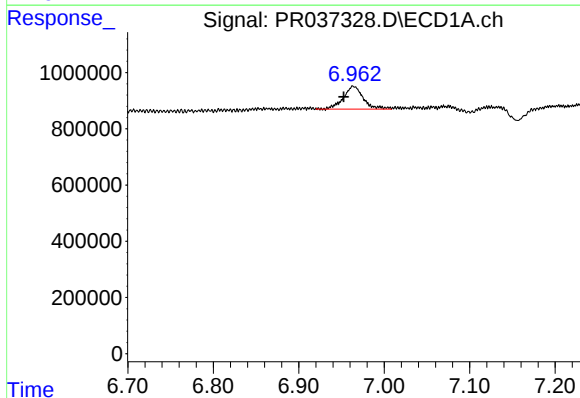


#28 AR-1254-3

R.T.: 6.964 min
Delta R.T.: 0.011 min
Response: 1319151
Conc: 14.50 ng/ml

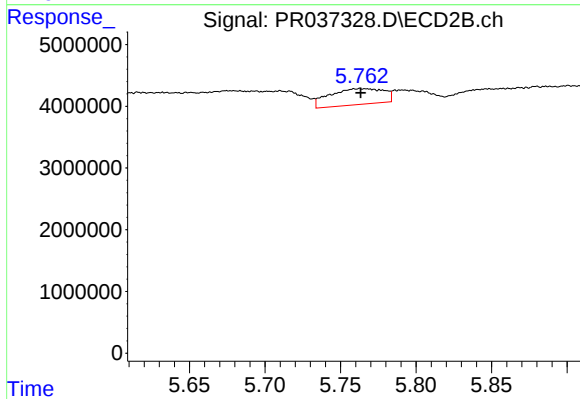

#28 AR-1254-3


R.T.: 5.763 min
Delta R.T.: 0.000 min
Response: 6458096
Conc: 13.64 ng/ml

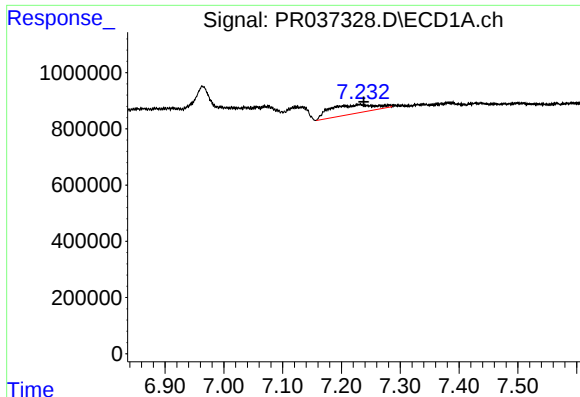

#29 AR-1254-4


R.T.: 7.232 min
Delta R.T.: -0.005 min
Response: 1724111
Conc: 25.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

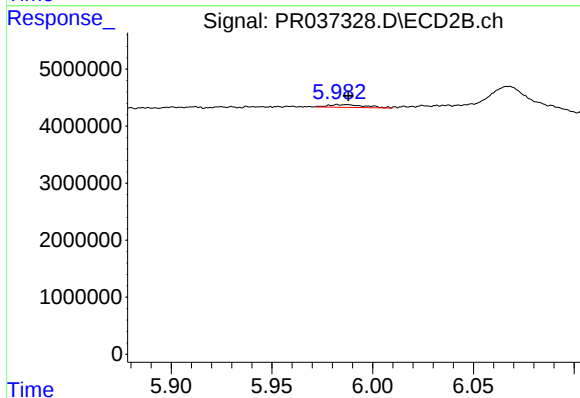


#29 AR-1254-4

R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 606186
Conc: 1.73 ng/ml

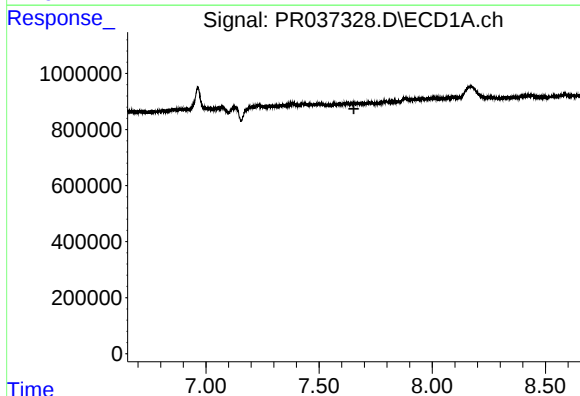


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

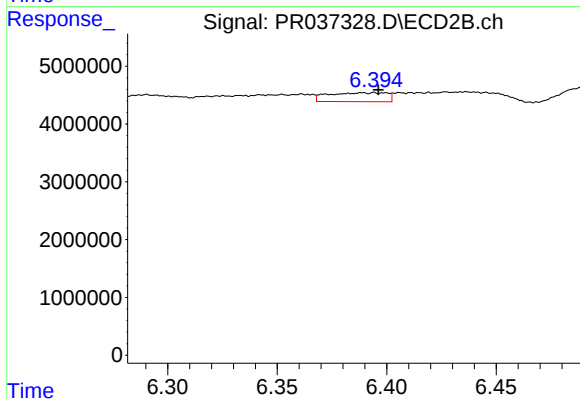

#30 AR-1254-5


R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 2896752
Conc: 6.54 ng/ml

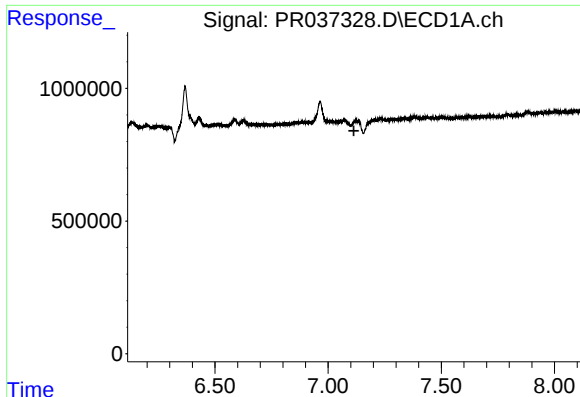

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

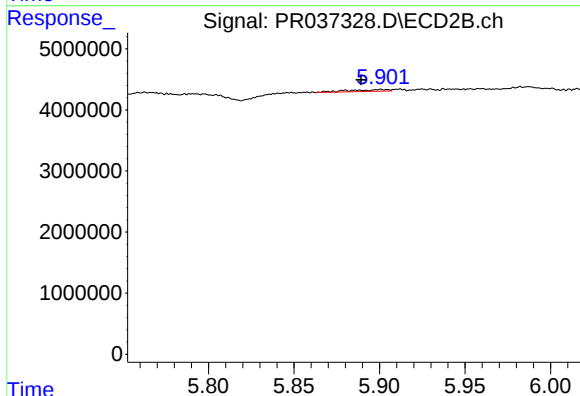


#31 AR-1260-1

R.T.: 5.901 min
Delta R.T.: 0.011 min
Response: 472238
Conc: 1.62 ng/ml

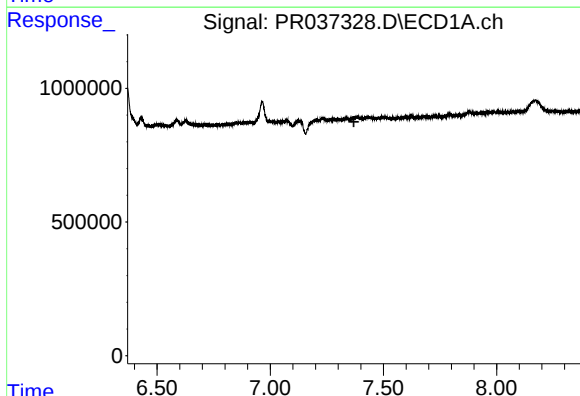


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

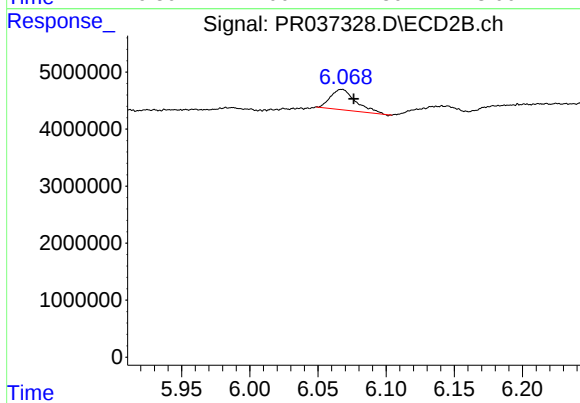

#32 AR-1260-2


R.T.: 6.067 min
Delta R.T.: -0.009 min
Response: 4591144
Conc: 9.97 ng/ml

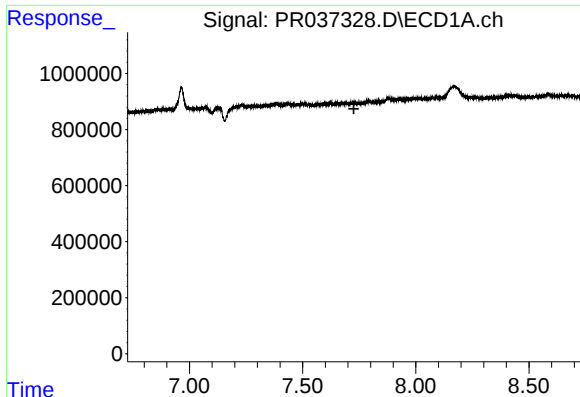

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

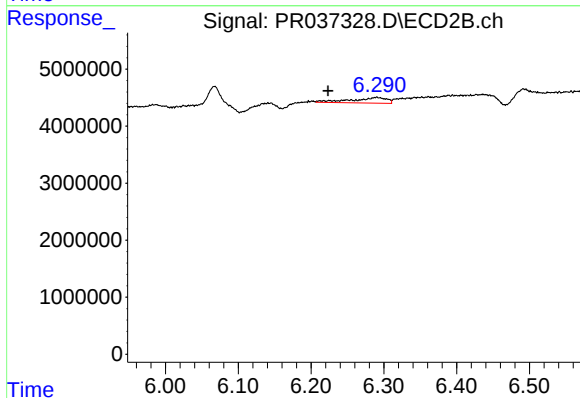


#33 AR-1260-3

R.T.: 6.290 min
Delta R.T.: 0.067 min
Response: 3296316
Conc: 9.25 ng/ml

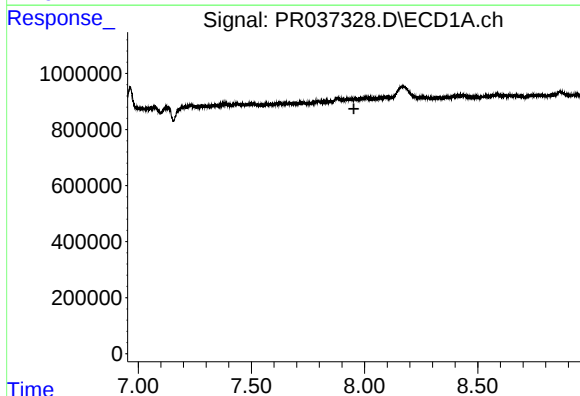


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

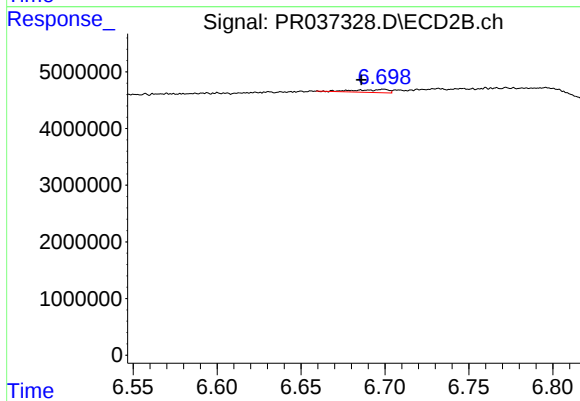

#34 AR-1260-4


R.T.: 6.699 min
Delta R.T.: 0.013 min
Response: 708919
Conc: 2.33 ng/ml

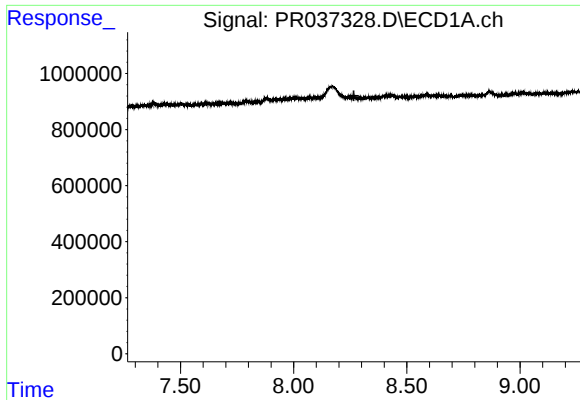

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

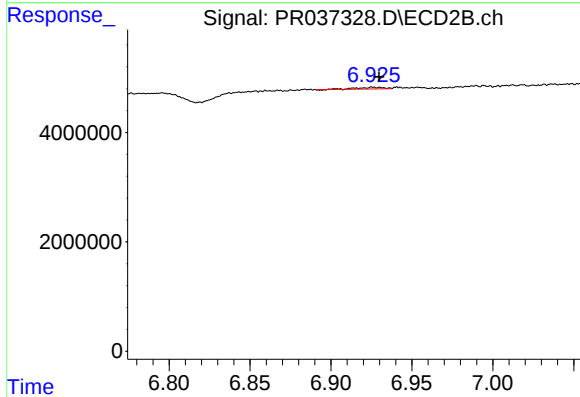


#35 AR-1260-5

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 346499
Conc: 0.40 ng/ml

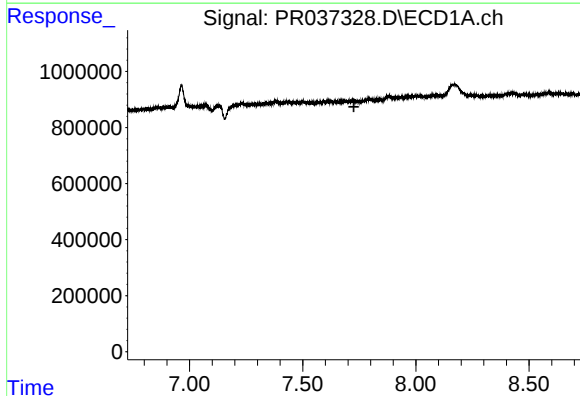


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

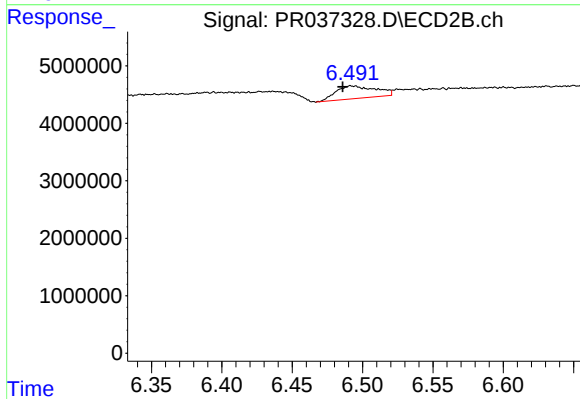

#36 AR-1262-1


R.T.: 6.492 min
Delta R.T.: 0.006 min
Response: 4317016
Conc: 17.23 ng/ml

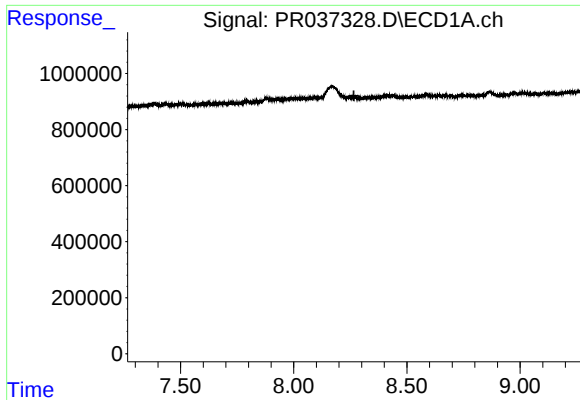

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

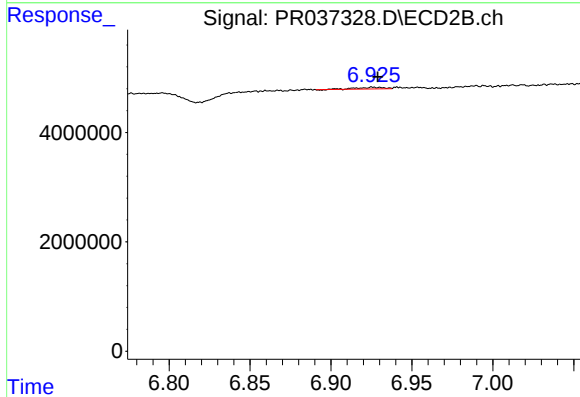


#37 AR-1262-2

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 346499
Conc: 0.28 ng/ml

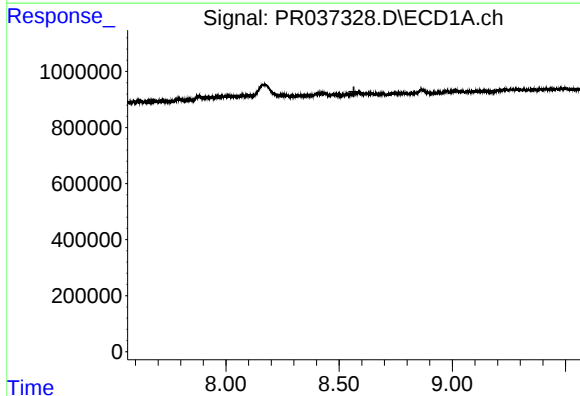


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

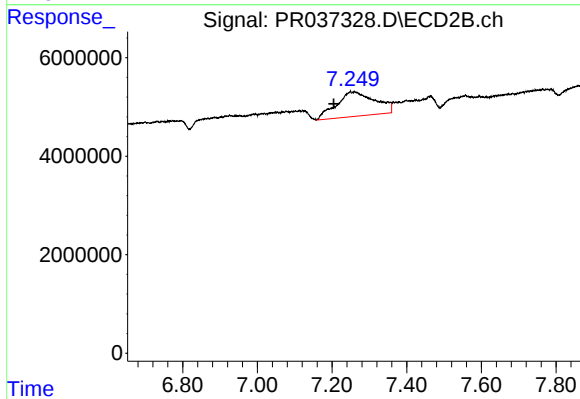

#38 AR-1262-3


R.T.: 7.249 min
Delta R.T.: 0.044 min
Response: 36009547
Conc: 65.68 ng/ml

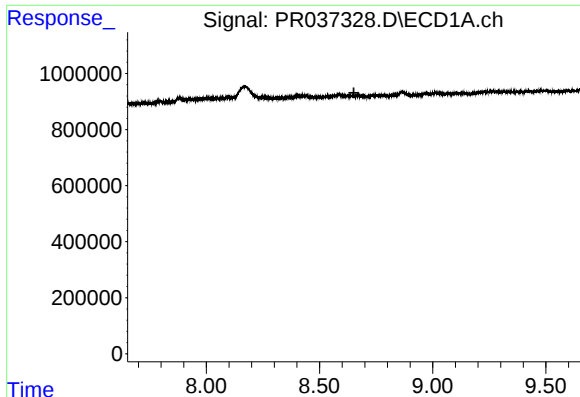

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

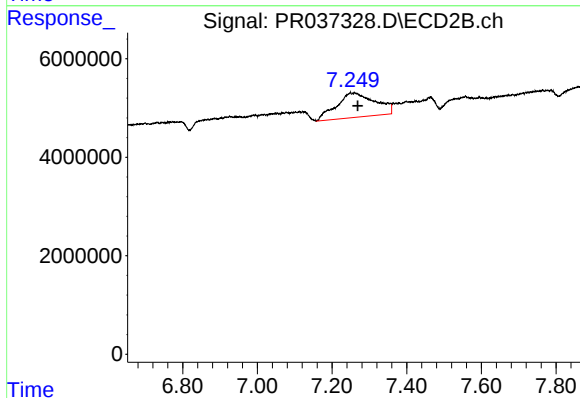


#39 AR-1262-4

R.T.: 7.249 min
Delta R.T.: -0.020 min
Response: 36009547
Conc: 40.12 ng/ml

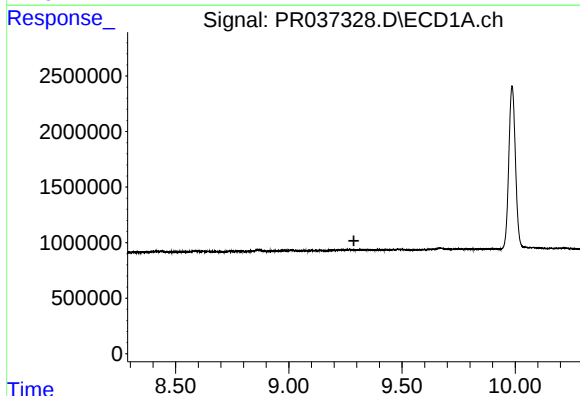


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

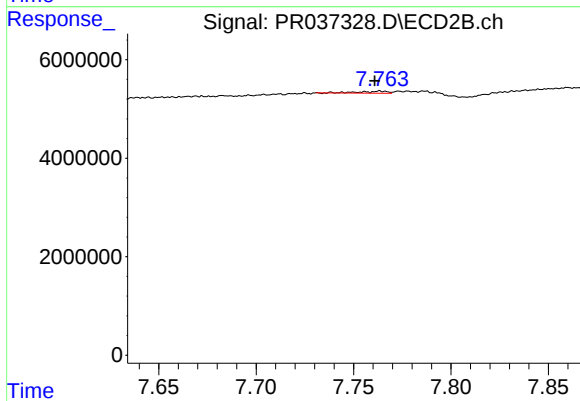

#40 AR-1262-5


R.T.: 7.764 min
Delta R.T.: 0.003 min
Response: 393247
Conc: 1.03 ng/ml

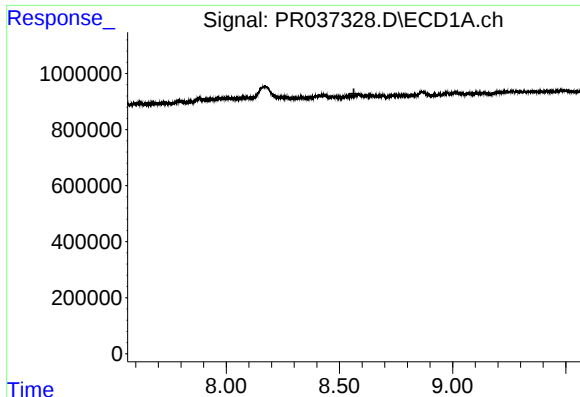

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

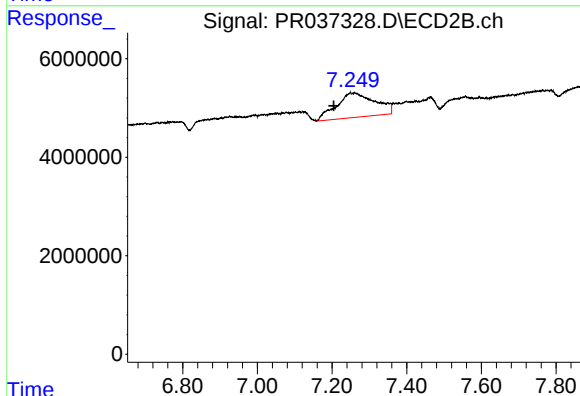


#41 AR-1268-1

R.T.: 7.249 min
Delta R.T.: 0.044 min
Response: 36009547
Conc: 29.25 ng/ml

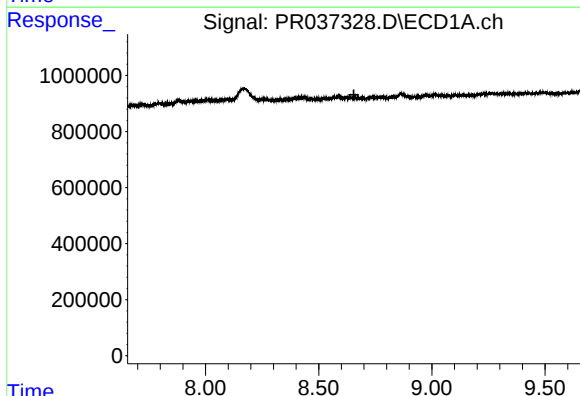


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

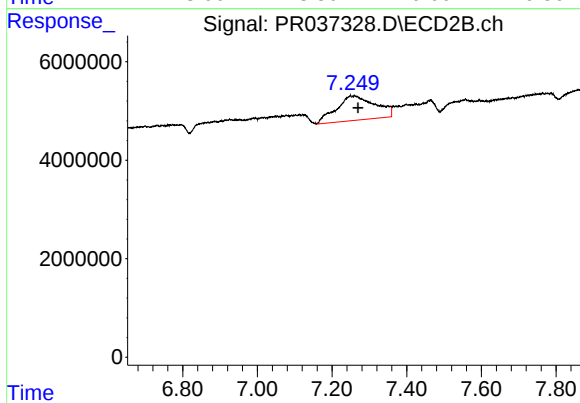

#42 AR-1268-2


R.T.: 7.249 min
Delta R.T.: -0.021 min
Response: 36009547
Conc: 34.01 ng/ml

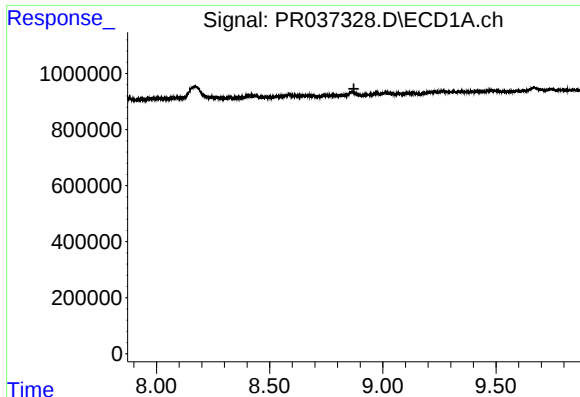

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

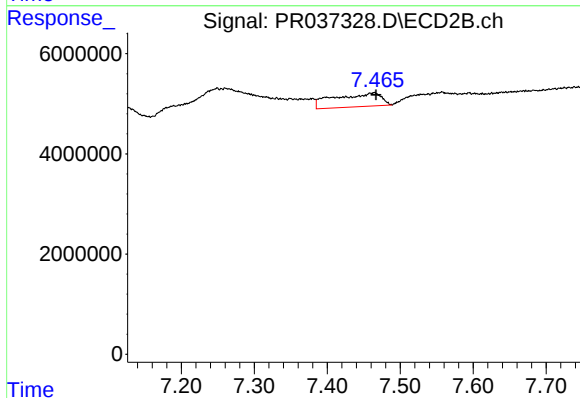


#43 AR-1268-3

R.T.: 7.464 min
Delta R.T.: -0.002 min
Response: 12037831
Conc: 13.58 ng/ml

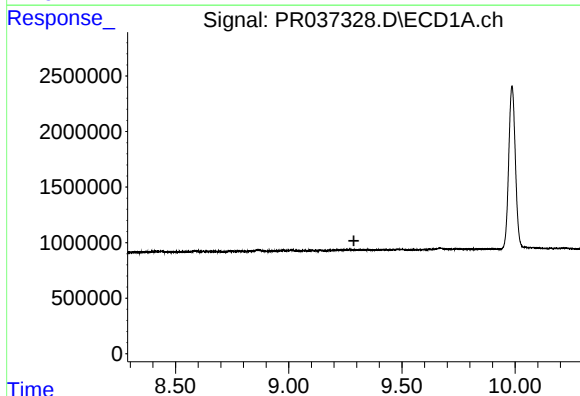


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

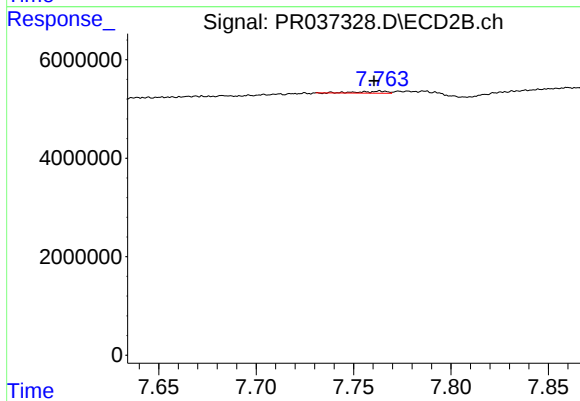

#44 AR-1268-4


R.T.: 7.764 min
Delta R.T.: 0.003 min
Response: 393247
Conc: 1.08 ng/ml

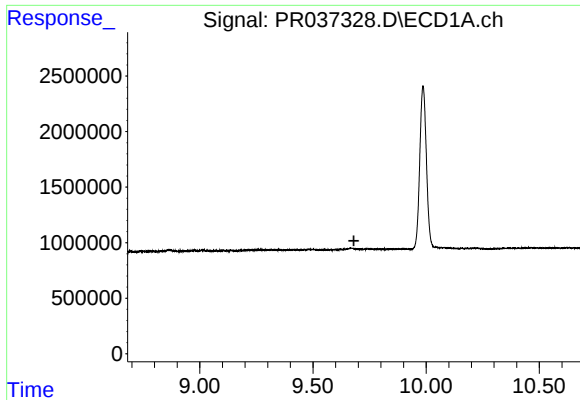

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

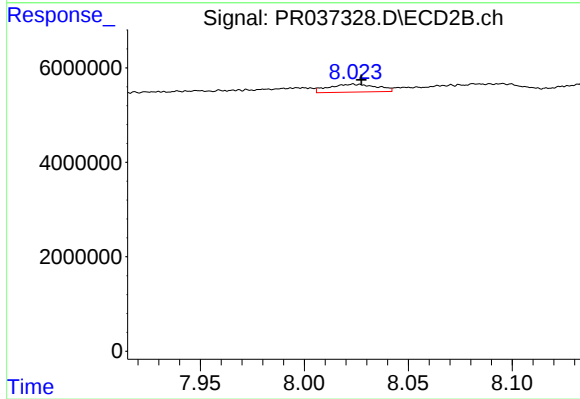

#45 AR-1268-5

R.T.: 8.024 min
Delta R.T.: -0.004 min
Response: 2696176
Conc: 1.06 ng/ml