

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037329.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 18:21
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1242 MDL 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 22:01:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.359	3.408	26434466	103.7E6	21.131	21.620
2)	SA Decachlor...	9.986	8.244	29372433	142.0E6	22.208	24.386
Target Compounds							
3)	L1 AR-1016-1	5.519	4.452	957891	4349054	22.231	23.885
4)	L1 AR-1016-2	5.540	4.465	1531677	6244664	22.119	22.135
5)	L1 AR-1016-3	5.601	4.638	1082595	3375779	26.845	23.478
6)	L1 AR-1016-4	5.700	4.680	757942	3651753	23.080	33.007 #
7)	L1 AR-1016-5	5.990	4.884	675264	3802930	19.693	25.018 #
8)	L2 AR-1221-1	0.000	3.617	0	531719	N.D.	10.443 #
9)	L2 AR-1221-2	4.659	3.695	651738	2569772	72.063	69.199
10)	L2 AR-1221-3	4.730	3.769	581988	2989882	18.989	24.418 #
11)	L3 AR-1232-1	4.730	3.769	581988	2989882	19.896	25.556 #
12)	L3 AR-1232-2	5.252	4.465	1273361	6244664	75.358	45.178 #
13)	L3 AR-1232-3	5.540	4.638	1531677	3375779	45.310	48.087
14)	L3 AR-1232-4	5.700	4.718	757942	3469890	48.287	58.150
15)	L3 AR-1232-5	5.786	4.884	523545	3802930	44.764	55.726
16)	L4 AR-1242-1	5.519	4.452	957891	4349054	27.997	29.679
17)	L4 AR-1242-2	5.540	4.465	1531677	6244664	27.613	27.370
18)	L4 AR-1242-3	5.601	4.638	1082595	3375779	32.891	29.195
19)	L4 AR-1242-4	5.700	4.718	757942	3469890	28.735	31.570
20)	L4 AR-1242-5	6.429	5.224	1027761	7210493	31.939	43.515 #
21)	L5 AR-1248-1	5.519	4.452	957891	4349054	41.816	43.204
22)	L5 AR-1248-2	5.786	4.680	523545	3651753	14.952	26.758 #
23)	L5 AR-1248-3	5.990	4.718	675264	3469890	16.506	24.790 #
24)	L5 AR-1248-4	6.390	4.884	908652	3802930	18.561	21.369
25)	L5 AR-1248-5	6.429	5.263	1027761	9873702	21.757	50.476 #
26)	L6 AR-1254-1	6.366	5.224	1173915	7210493	21.488	20.932
27)	L6 AR-1254-2	6.587	5.371	759365	5468972	8.861	18.260 #
28)	L6 AR-1254-3	6.961	5.764	876312	4624688	9.634	9.765
29)	L6 AR-1254-4	7.233	5.986	1001763	1416224	14.950	4.039 #
30)	L6 AR-1254-5	0.000	6.397	0	1853067	N.D.	4.185 #
31)	L7 AR-1260-1	7.122	5.883	586614	154931	8.890	0.530 #
32)	L7 AR-1260-2	0.000	6.066	0	3474569	N.D.	7.544 #
33)	L7 AR-1260-3	0.000	6.217	0	488302	N.D.	1.370 #
34)	L7 AR-1260-4	0.000	6.691	0	466423	N.D.	1.530 #
35)	L7 AR-1260-5	0.000	6.919	0	43089	N.D.	0.050 #
36)	L8 AR-1262-1	0.000	6.493	0	5667201	N.D.	22.613 #
37)	L8 AR-1262-2	0.000	6.919	0	43089	N.D.	0.034 #
38)	L8 AR-1262-3	0.000	7.202	0	1825118	N.D.	3.329 #
39)	L8 AR-1262-4	0.000	7.268	0	828106	N.D.	0.923 #
40)	L8 AR-1262-5	0.000	7.759	0	472650	N.D.	1.235 #
41)	L9 AR-1268-1	0.000	7.202	0	1825118	N.D.	1.483 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
Data File : PR037329.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 18:21
Operator : SM\SJ
Sample : K1560-03
Misc : AR1242 MDL 25PPB
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 22:01:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.272	0	704233	N.D.	0.665 #
43) L9	AR-1268-3	0.000	7.463	0	7013942	N.D.	7.914 #
44) L9	AR-1268-4	0.000	7.759	0	472650	N.D.	1.303 #
45) L9	AR-1268-5	0.000	8.025	0	4419734	N.D.	1.737 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

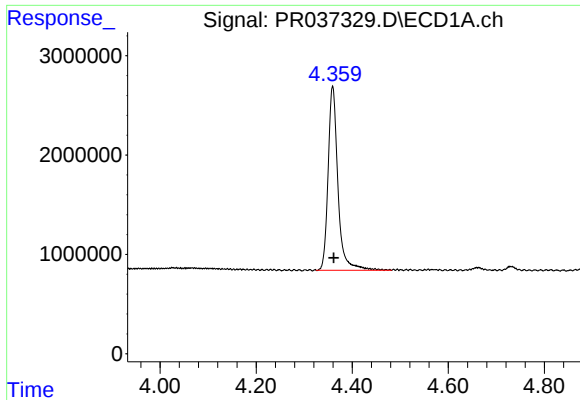

#1 Tetrachloro-m-xylene


R.T.: 4.359 min
Delta R.T.: -0.003 min
Response: 26434466
Conc: 21.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

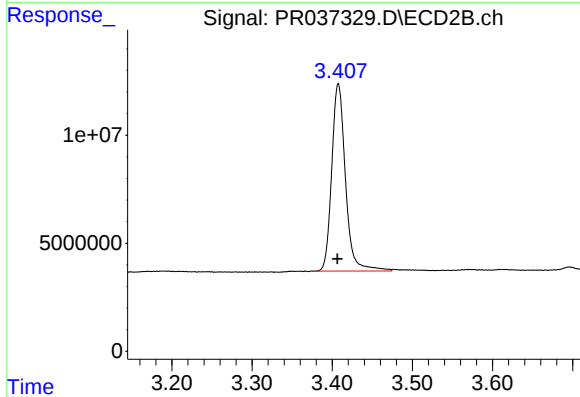


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: 0.001 min
Response: 103681261
Conc: 21.62 ng/ml

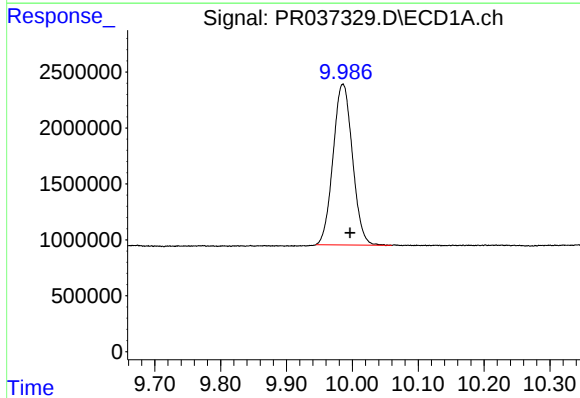


#2 Decachlorobiphenyl

R.T.: 9.986 min
Delta R.T.: -0.011 min
Response: 29372433
Conc: 22.21 ng/ml

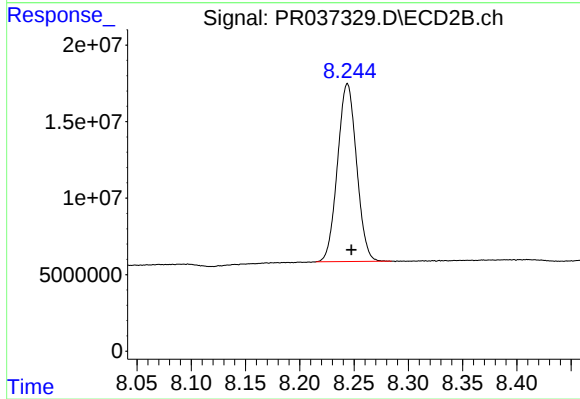

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 142032483
Conc: 24.39 ng/ml

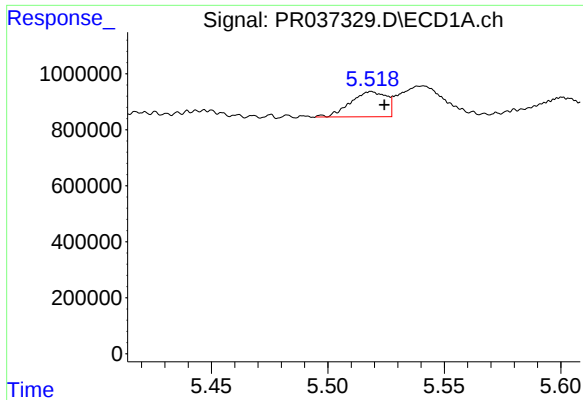

#3 AR-1016-1


R.T.: 5.519 min
Delta R.T.: -0.006 min
Response: 957891
Conc: 22.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

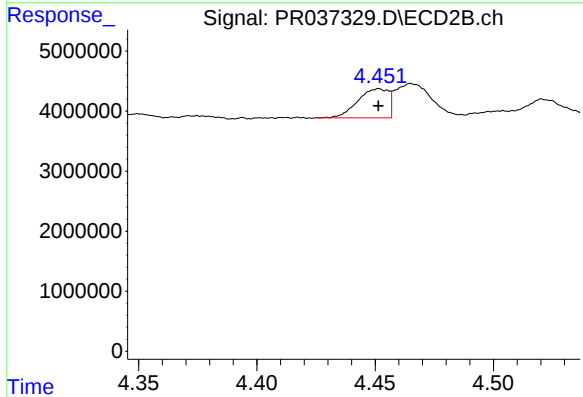


#3 AR-1016-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 4349054
Conc: 23.89 ng/ml

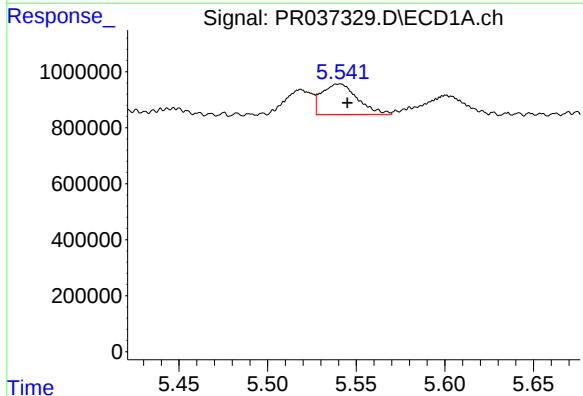


#4 AR-1016-2

R.T.: 5.540 min
Delta R.T.: -0.005 min
Response: 1531677
Conc: 22.12 ng/ml

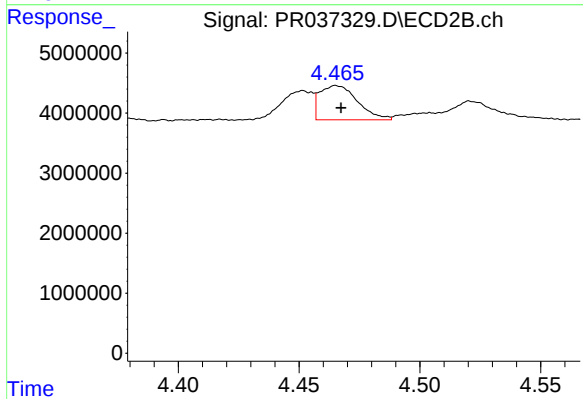

#4 AR-1016-2


R.T.: 4.465 min
Delta R.T.: -0.002 min
Response: 6244664
Conc: 22.13 ng/ml

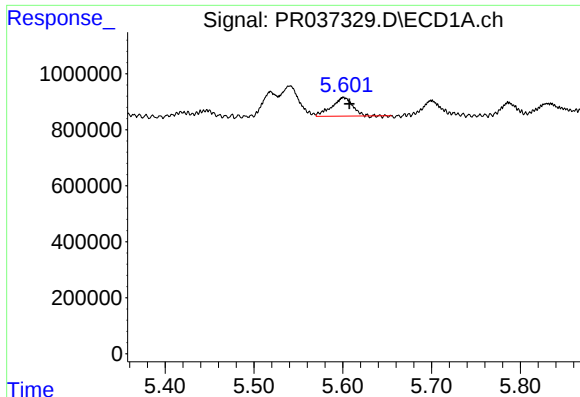

#5 AR-1016-3


R.T.: 5.601 min
Delta R.T.: -0.007 min
Response: 1082595
Conc: 26.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

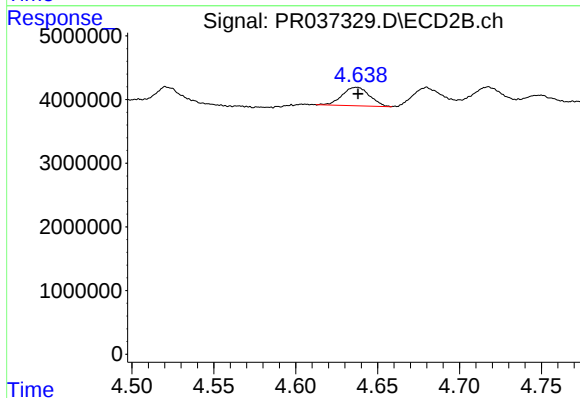


#5 AR-1016-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 3375779
Conc: 23.48 ng/ml

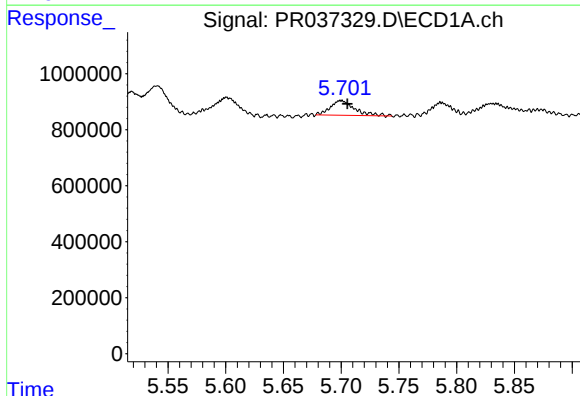


#6 AR-1016-4

R.T.: 5.700 min
Delta R.T.: -0.006 min
Response: 757942
Conc: 23.08 ng/ml

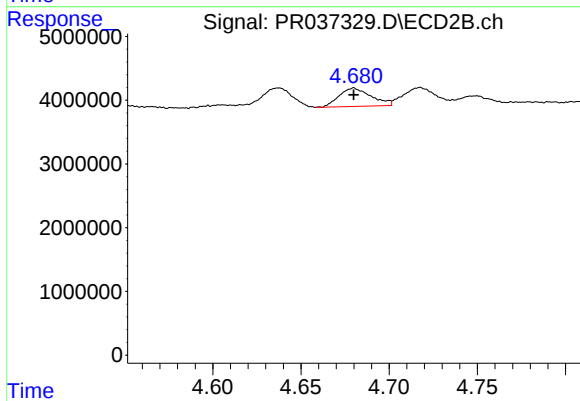

#6 AR-1016-4


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 3651753
Conc: 33.01 ng/ml

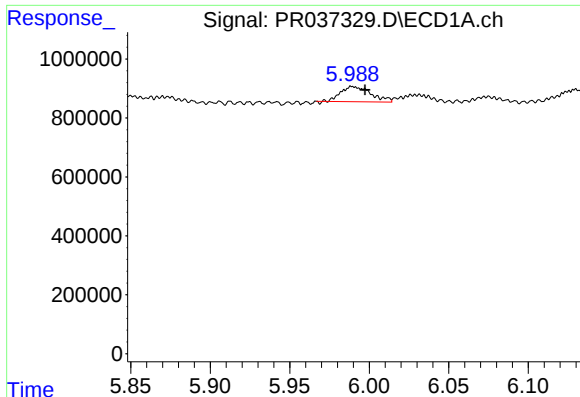

#7 AR-1016-5


R.T.: 5.990 min
Delta R.T.: -0.008 min
Response: 675264
Conc: 19.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

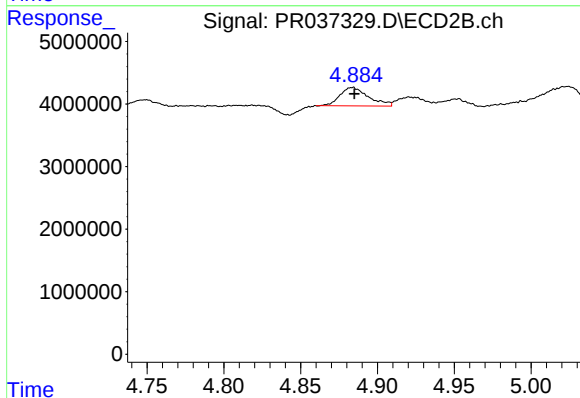


#7 AR-1016-5

R.T.: 4.884 min
Delta R.T.: 0.000 min
Response: 3802930
Conc: 25.02 ng/ml

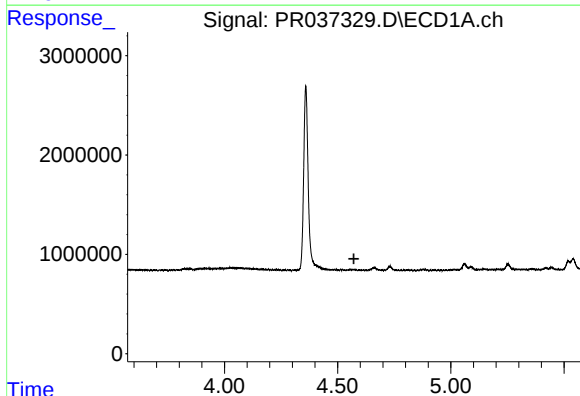


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

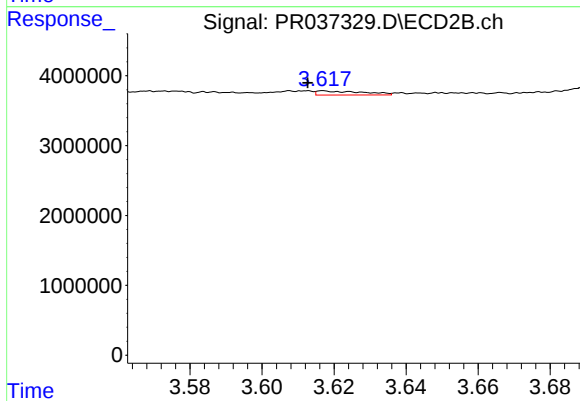

#8 AR-1221-1


R.T.: 3.617 min
Delta R.T.: 0.004 min
Response: 531719
Conc: 10.44 ng/ml

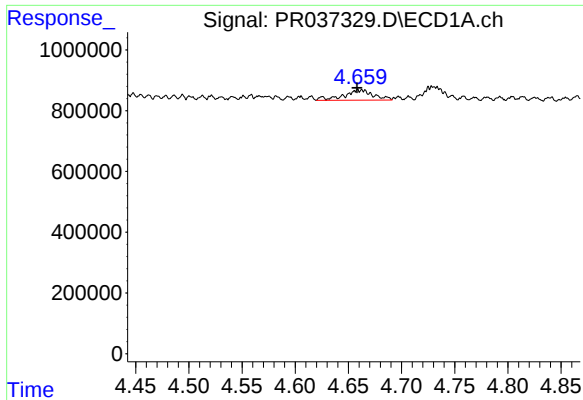

#9 AR-1221-2


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 651738
Conc: 72.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

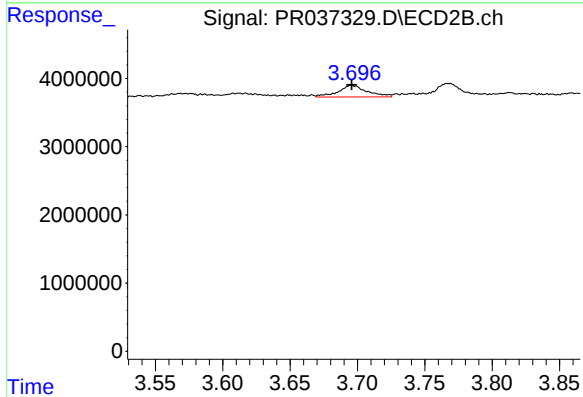


#9 AR-1221-2

R.T.: 3.695 min
Delta R.T.: 0.000 min
Response: 2569772
Conc: 69.20 ng/ml

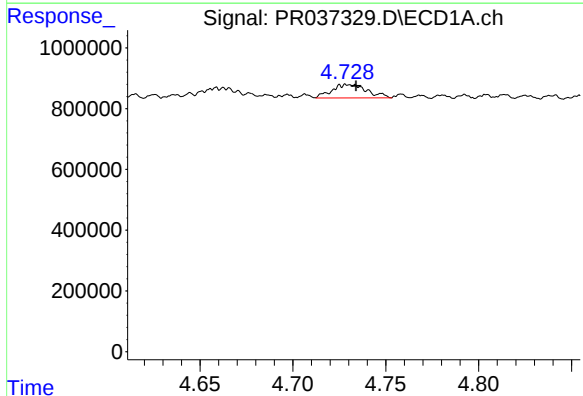


#10 AR-1221-3

R.T.: 4.730 min
Delta R.T.: -0.004 min
Response: 581988
Conc: 18.99 ng/ml

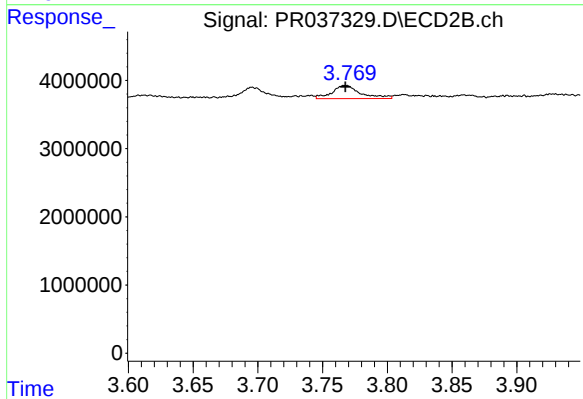

#10 AR-1221-3


R.T.: 3.769 min
Delta R.T.: 0.001 min
Response: 2989882
Conc: 24.42 ng/ml

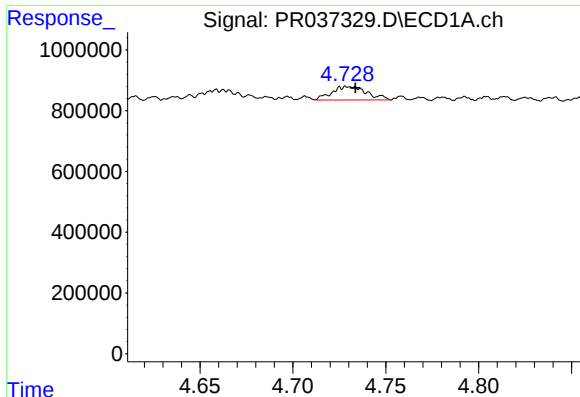

#11 AR-1232-1


R.T.: 4.730 min
Delta R.T.: -0.004 min
Response: 581988
Conc: 19.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

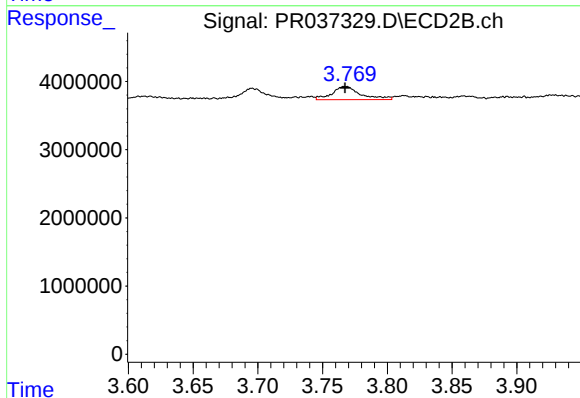


#11 AR-1232-1

R.T.: 3.769 min
Delta R.T.: 0.002 min
Response: 2989882
Conc: 25.56 ng/ml

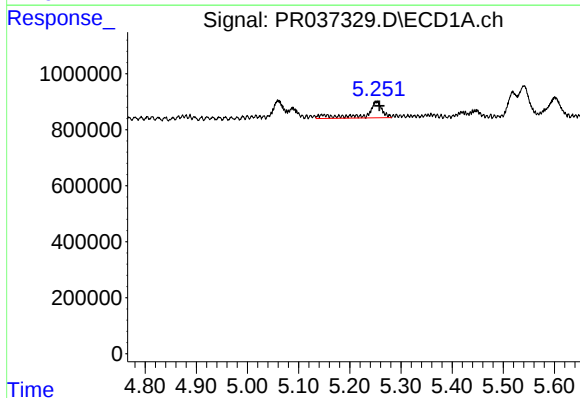


#12 AR-1232-2

R.T.: 5.252 min
Delta R.T.: -0.006 min
Response: 1273361
Conc: 75.36 ng/ml

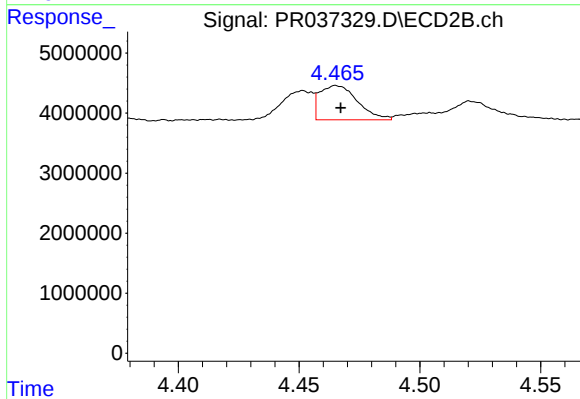

#12 AR-1232-2


R.T.: 4.465 min
Delta R.T.: -0.002 min
Response: 6244664
Conc: 45.18 ng/ml

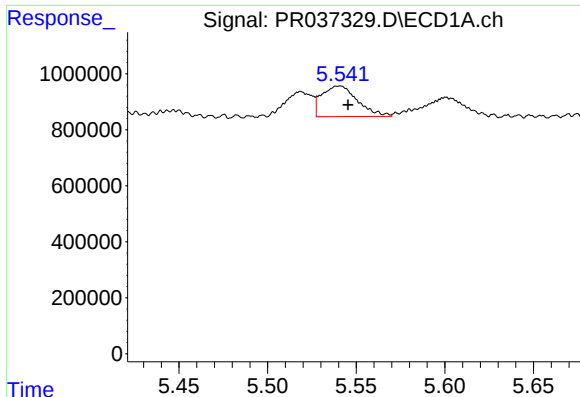

#13 AR-1232-3


R.T.: 5.540 min
Delta R.T.: -0.005 min
Response: 1531677
Conc: 45.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

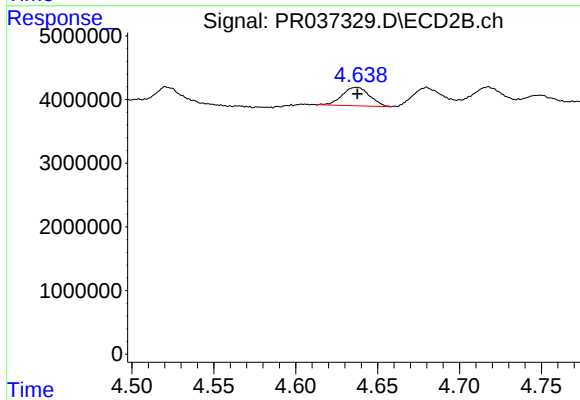


#13 AR-1232-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 3375779
Conc: 48.09 ng/ml

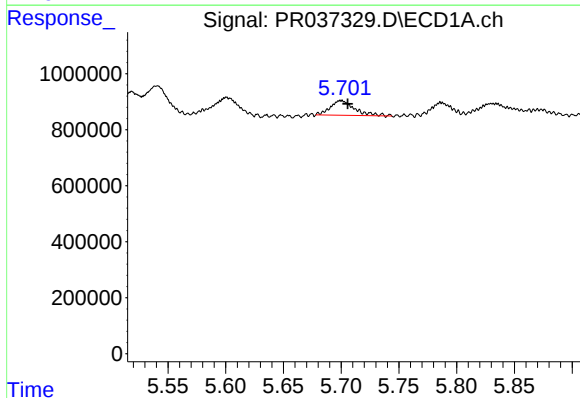


#14 AR-1232-4

R.T.: 5.700 min
Delta R.T.: -0.006 min
Response: 757942
Conc: 48.29 ng/ml

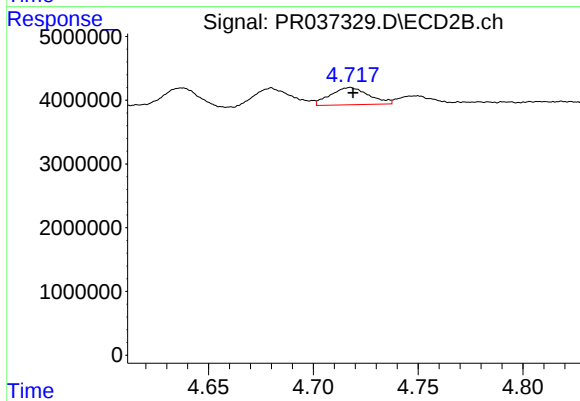

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 3469890
Conc: 58.15 ng/ml

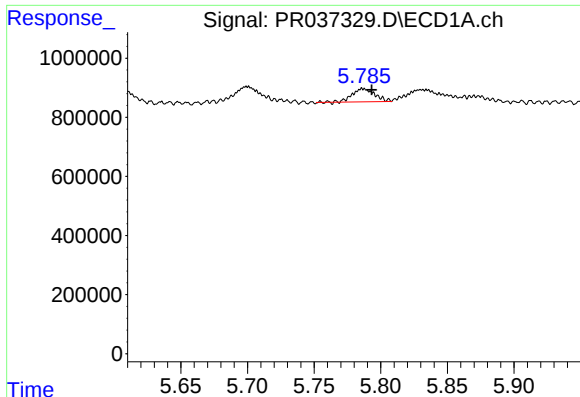

#15 AR-1232-5


R.T.: 5.786 min
Delta R.T.: -0.007 min
Response: 523545
Conc: 44.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

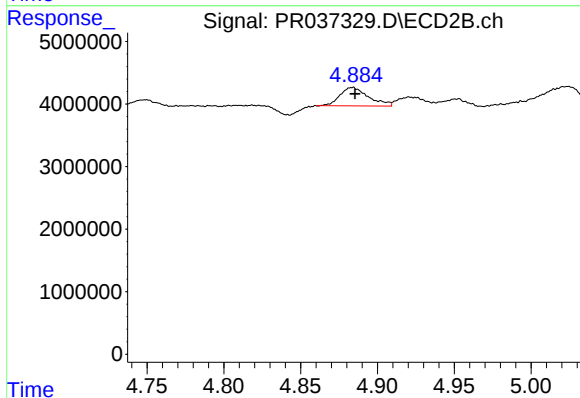


#15 AR-1232-5

R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 3802930
Conc: 55.73 ng/ml

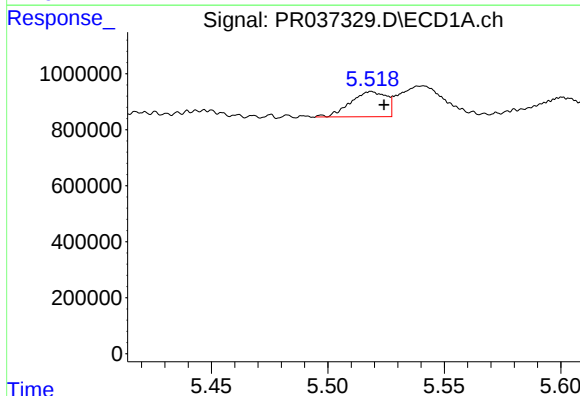


#16 AR-1242-1

R.T.: 5.519 min
Delta R.T.: -0.006 min
Response: 957891
Conc: 28.00 ng/ml

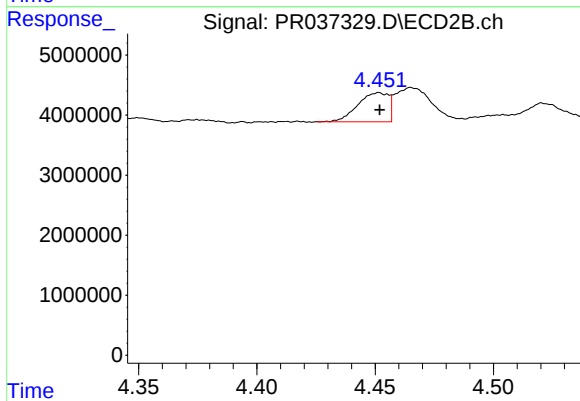

#16 AR-1242-1


R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 4349054
Conc: 29.68 ng/ml

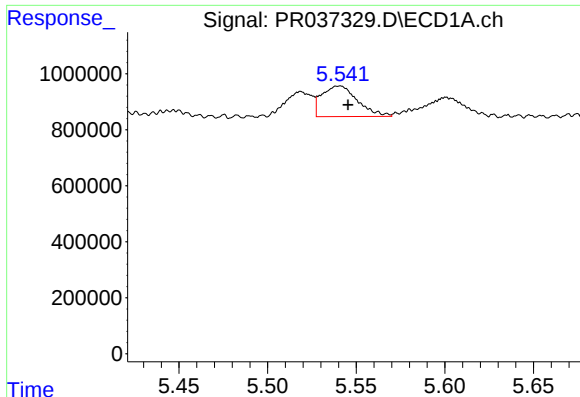

#17 AR-1242-2


R.T.: 5.540 min
Delta R.T.: -0.005 min
Response: 1531677
Conc: 27.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

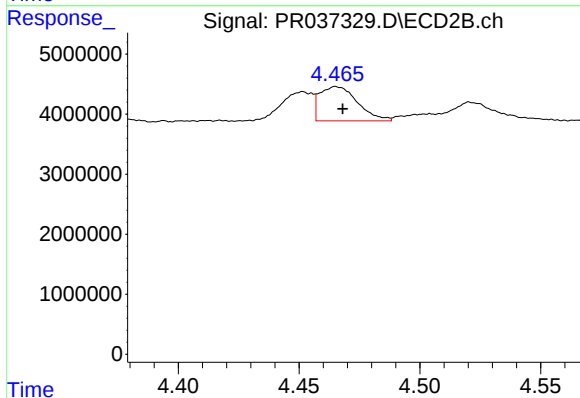


#17 AR-1242-2

R.T.: 4.465 min
Delta R.T.: -0.003 min
Response: 6244664
Conc: 27.37 ng/ml

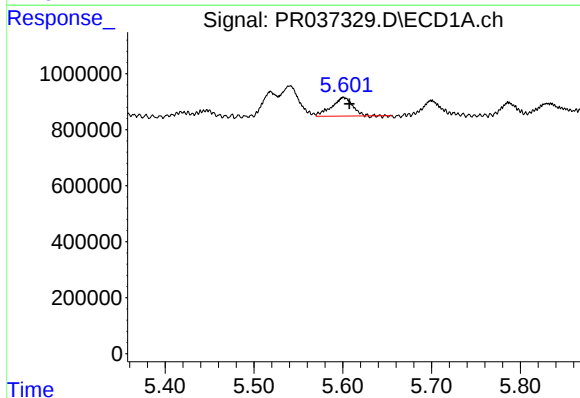


#18 AR-1242-3

R.T.: 5.601 min
Delta R.T.: -0.007 min
Response: 1082595
Conc: 32.89 ng/ml

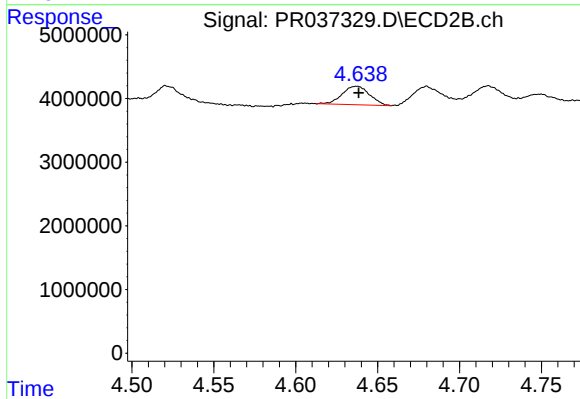

#18 AR-1242-3


R.T.: 4.638 min
Delta R.T.: -0.001 min
Response: 3375779
Conc: 29.19 ng/ml

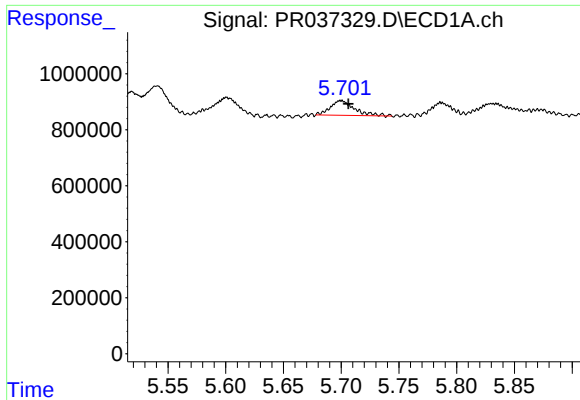

#19 AR-1242-4


R.T.: 5.700 min
Delta R.T.: -0.007 min
Response: 757942
Conc: 28.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

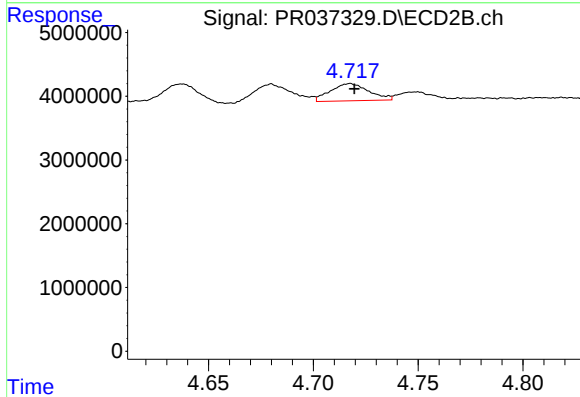


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 3469890
Conc: 31.57 ng/ml

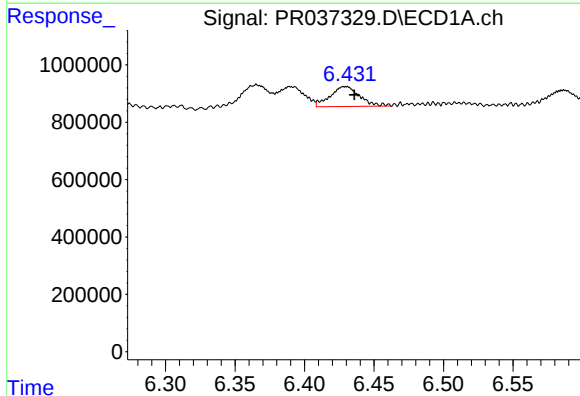


#20 AR-1242-5

R.T.: 6.429 min
Delta R.T.: -0.006 min
Response: 1027761
Conc: 31.94 ng/ml

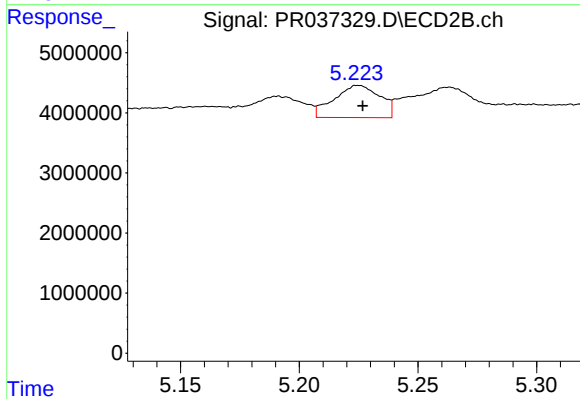

#20 AR-1242-5


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 7210493
Conc: 43.52 ng/ml

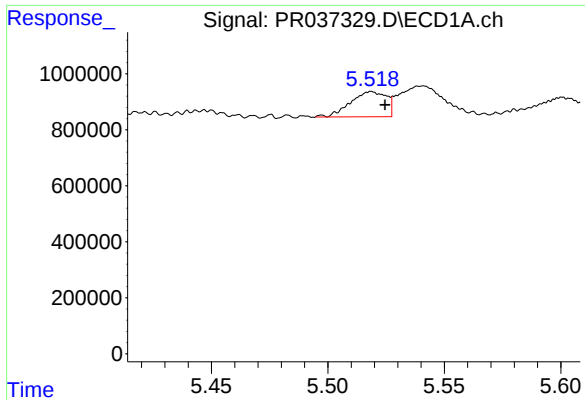

#21 AR-1248-1


R.T.: 5.519 min
Delta R.T.: -0.006 min
Response: 957891
Conc: 41.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

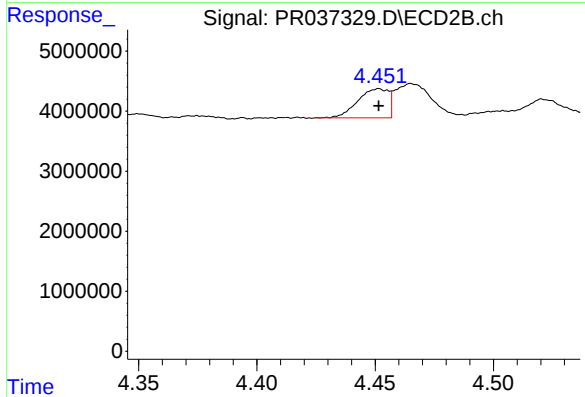


#21 AR-1248-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 4349054
Conc: 43.20 ng/ml

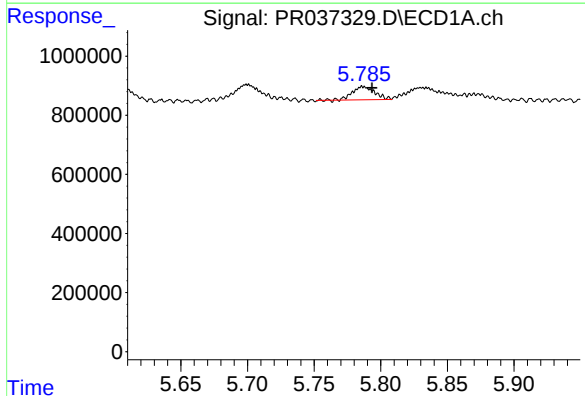


#22 AR-1248-2

R.T.: 5.786 min
Delta R.T.: -0.007 min
Response: 523545
Conc: 14.95 ng/ml

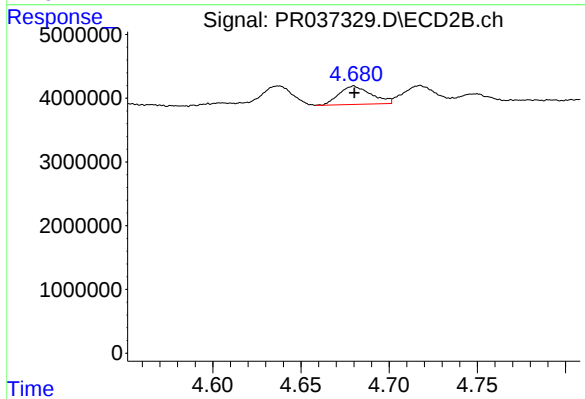

#22 AR-1248-2


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 3651753
Conc: 26.76 ng/ml

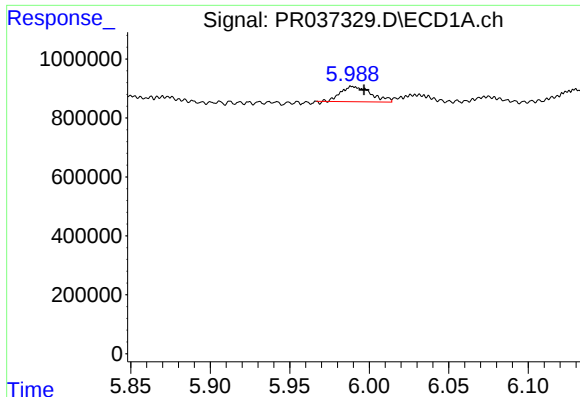

#23 AR-1248-3


R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 675264
Conc: 16.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

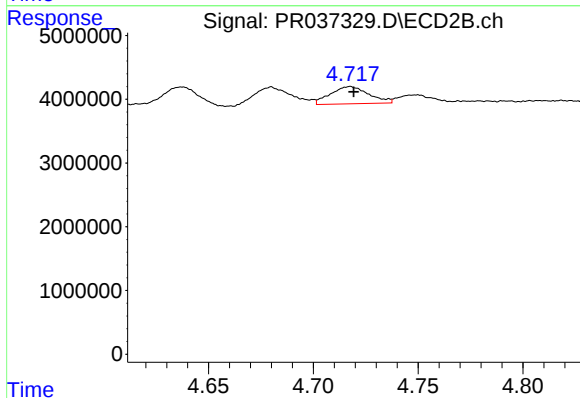


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 3469890
Conc: 24.79 ng/ml

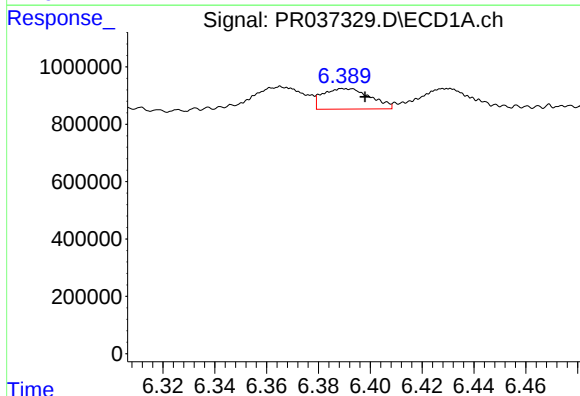


#24 AR-1248-4

R.T.: 6.390 min
Delta R.T.: -0.008 min
Response: 908652
Conc: 18.56 ng/ml

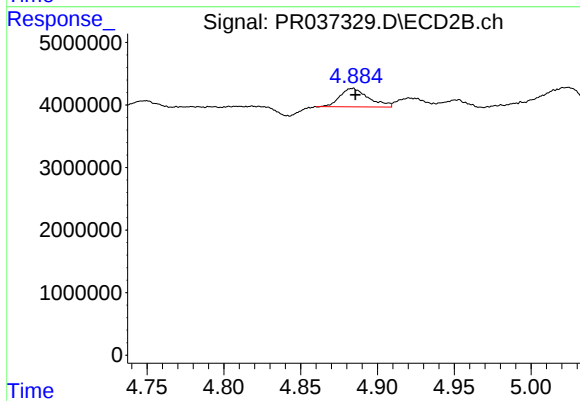

#24 AR-1248-4


R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 3802930
Conc: 21.37 ng/ml

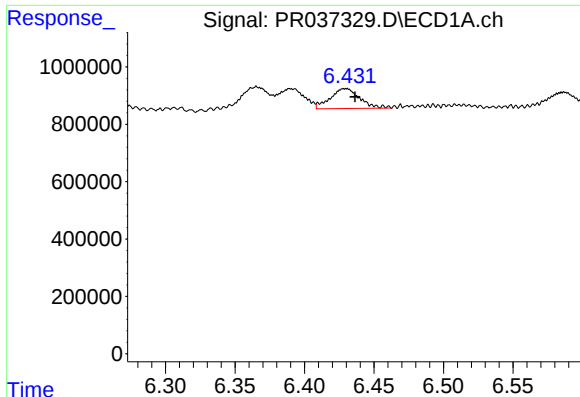

#25 AR-1248-5


R.T.: 6.429 min
Delta R.T.: -0.007 min
Response: 1027761
Conc: 21.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

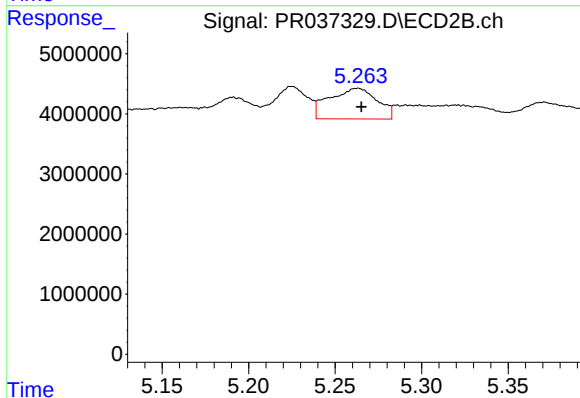


#25 AR-1248-5

R.T.: 5.263 min
Delta R.T.: -0.002 min
Response: 9873702
Conc: 50.48 ng/ml

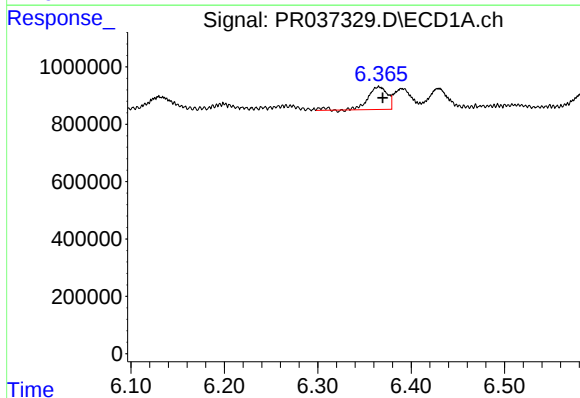


#26 AR-1254-1

R.T.: 6.366 min
Delta R.T.: -0.004 min
Response: 1173915
Conc: 21.49 ng/ml

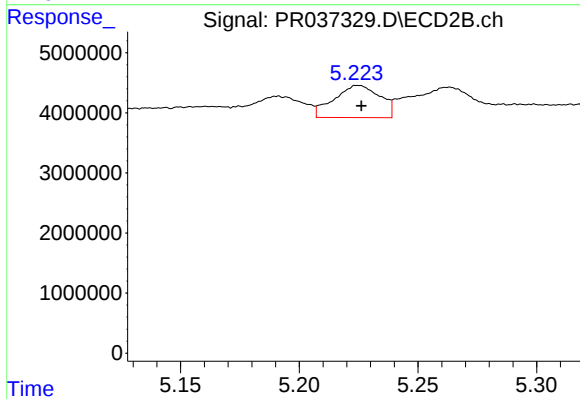

#26 AR-1254-1


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 7210493
Conc: 20.93 ng/ml

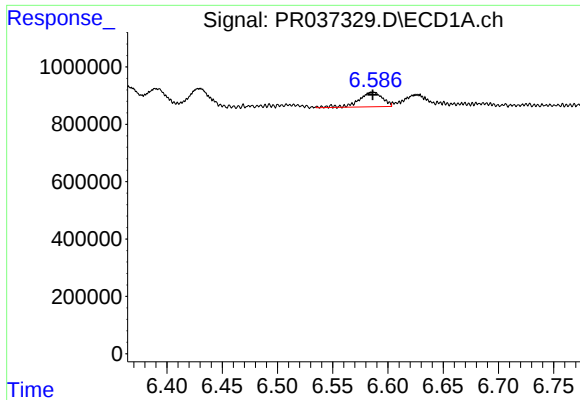

#27 AR-1254-2


R.T.: 6.587 min
Delta R.T.: 0.000 min
Response: 759365
Conc: 8.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

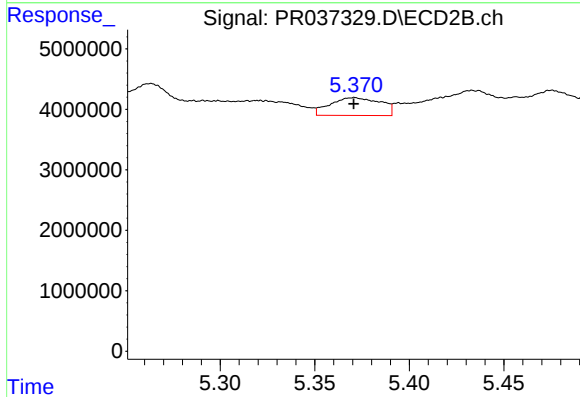


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 5468972
Conc: 18.26 ng/ml

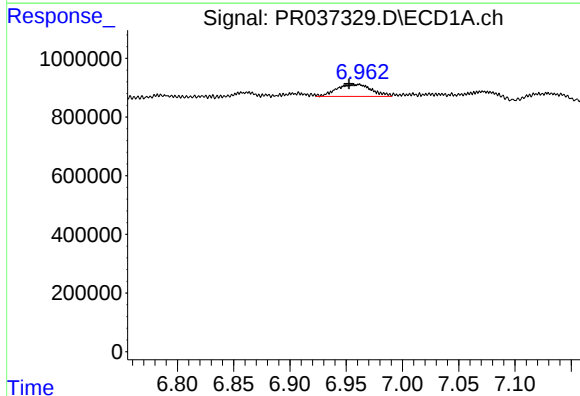


#28 AR-1254-3

R.T.: 6.961 min
Delta R.T.: 0.009 min
Response: 876312
Conc: 9.63 ng/ml

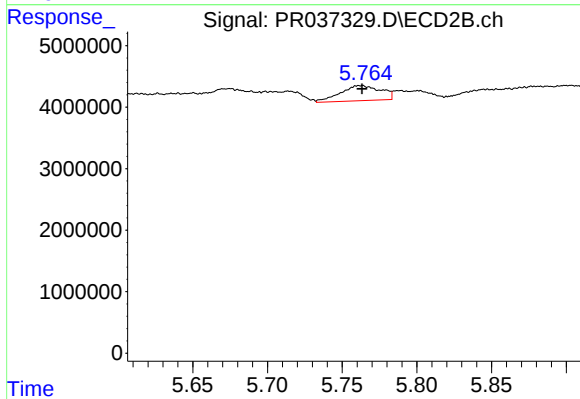

#28 AR-1254-3


R.T.: 5.764 min
Delta R.T.: 0.000 min
Response: 4624688
Conc: 9.76 ng/ml

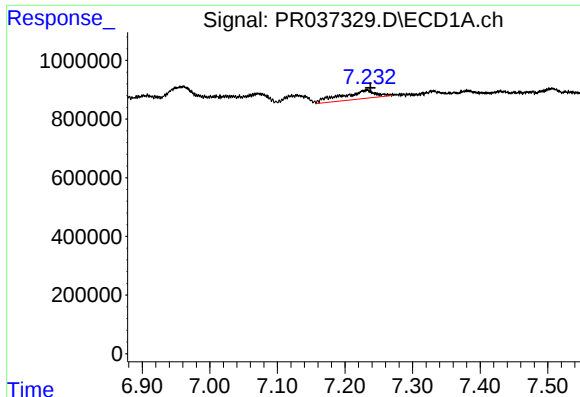

#29 AR-1254-4


R.T.: 7.233 min
Delta R.T.: -0.005 min
Response: 1001763
Conc: 14.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

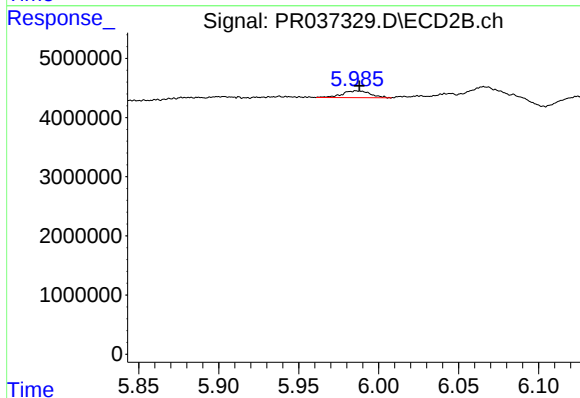


#29 AR-1254-4

R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 1416224
Conc: 4.04 ng/ml

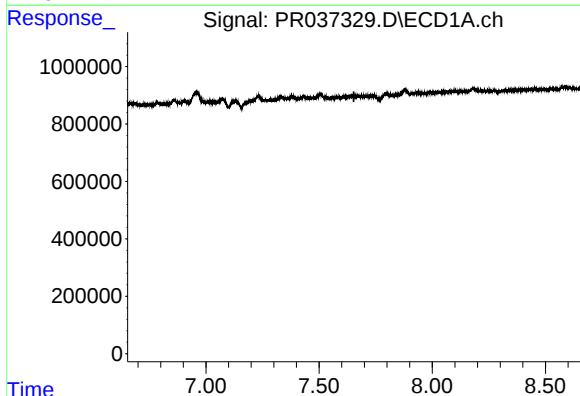


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

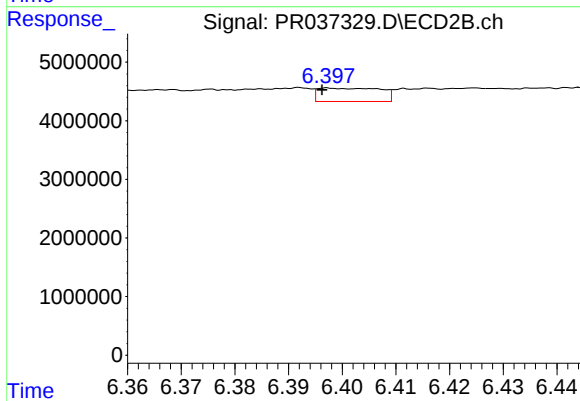

#30 AR-1254-5


R.T.: 6.397 min
Delta R.T.: 0.001 min
Response: 1853067
Conc: 4.18 ng/ml

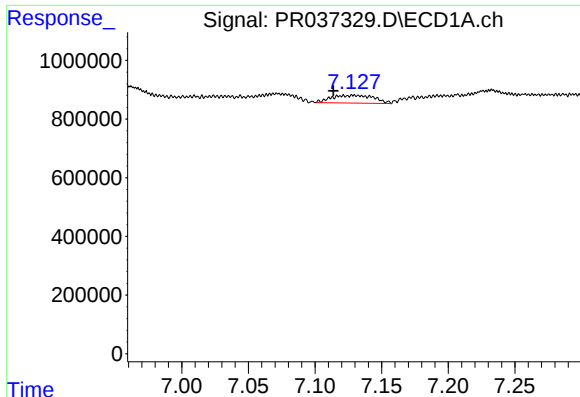

#31 AR-1260-1


R.T.: 7.122 min
Delta R.T.: 0.008 min
Response: 586614
Conc: 8.89 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

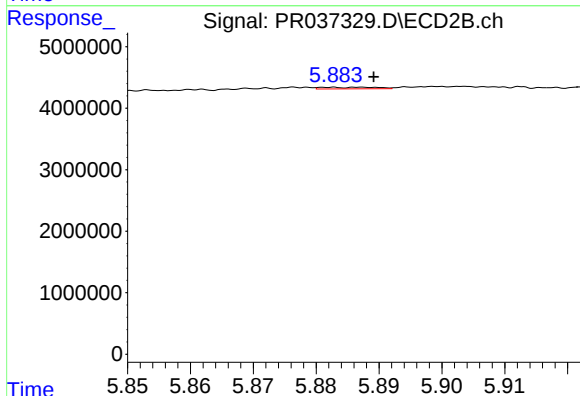


#31 AR-1260-1

R.T.: 5.883 min
Delta R.T.: -0.007 min
Response: 154931
Conc: 0.53 ng/ml

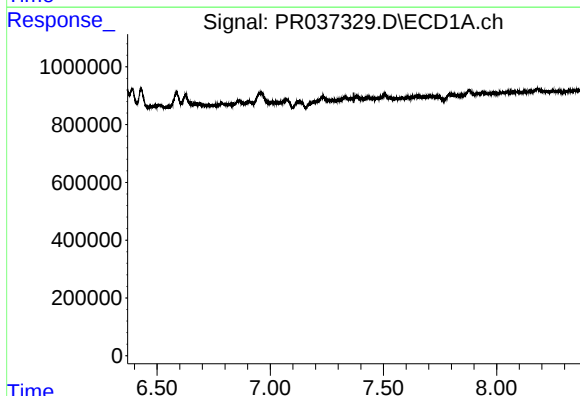


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

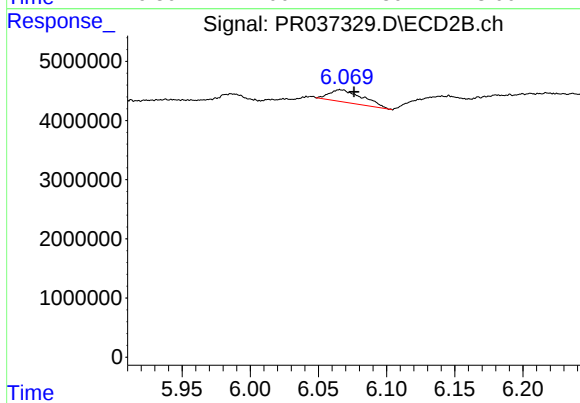

#32 AR-1260-2


R.T.: 6.066 min
Delta R.T.: -0.011 min
Response: 3474569
Conc: 7.54 ng/ml

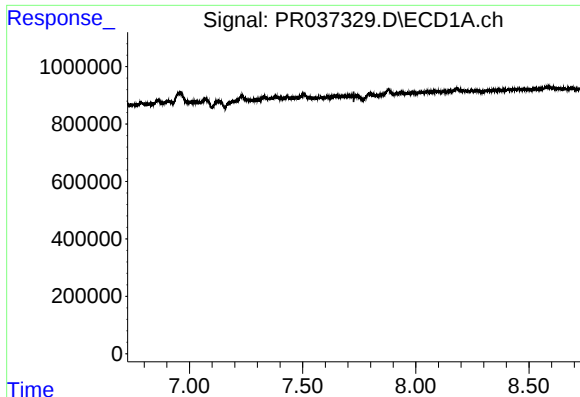

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

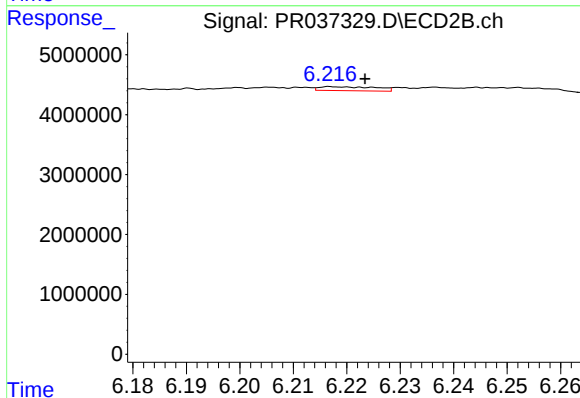


#33 AR-1260-3

R.T.: 6.217 min
Delta R.T.: -0.006 min
Response: 488302
Conc: 1.37 ng/ml

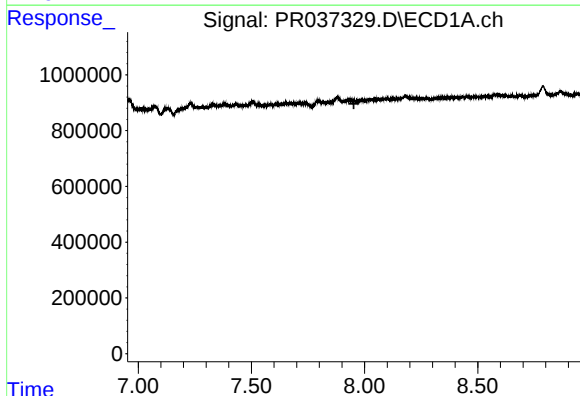


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

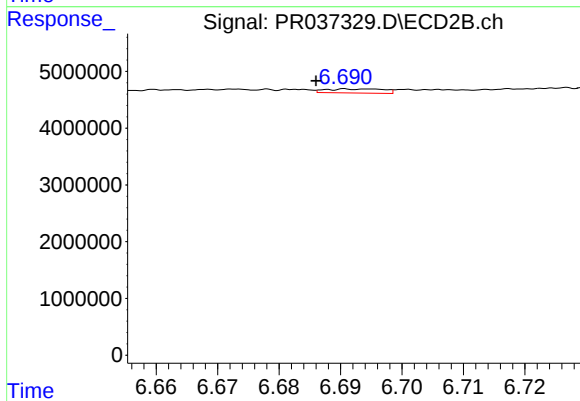

#34 AR-1260-4


R.T.: 6.691 min
Delta R.T.: 0.005 min
Response: 466423
Conc: 1.53 ng/ml

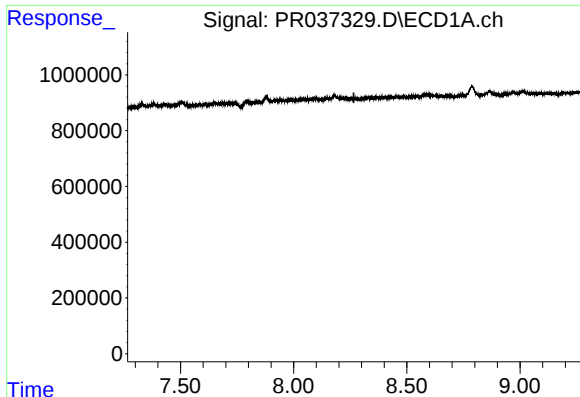

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

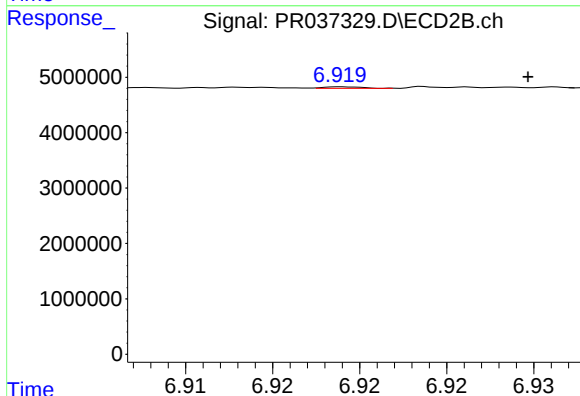


#35 AR-1260-5

R.T.: 6.919 min
Delta R.T.: -0.010 min
Response: 43089
Conc: 0.05 ng/ml

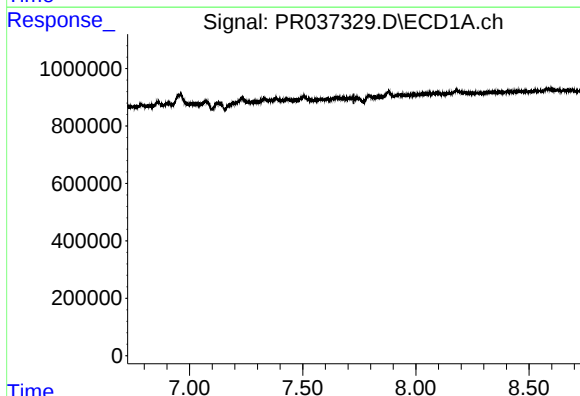


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

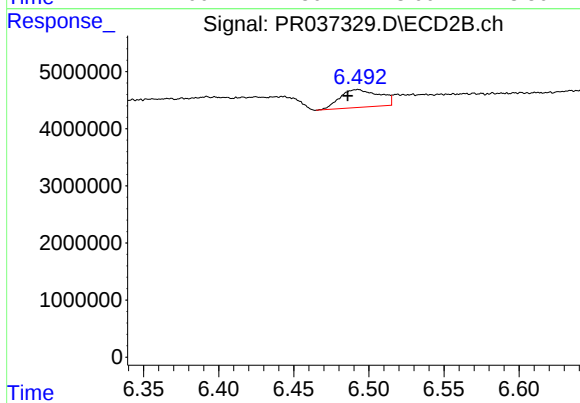

#36 AR-1262-1


R.T.: 6.493 min
Delta R.T.: 0.007 min
Response: 5667201
Conc: 22.61 ng/ml

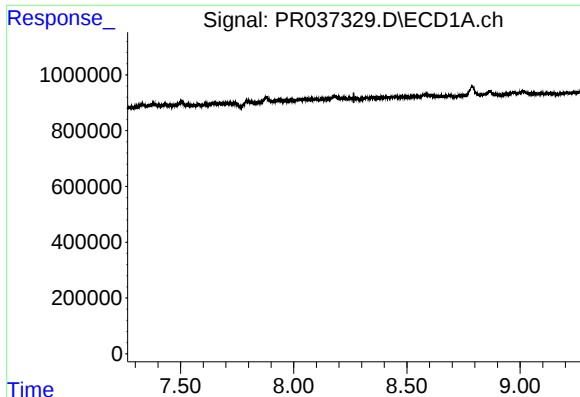

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

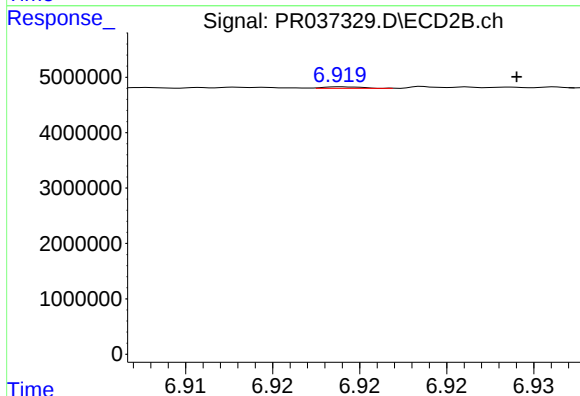


#37 AR-1262-2

R.T.: 6.919 min
Delta R.T.: -0.010 min
Response: 43089
Conc: 0.03 ng/ml

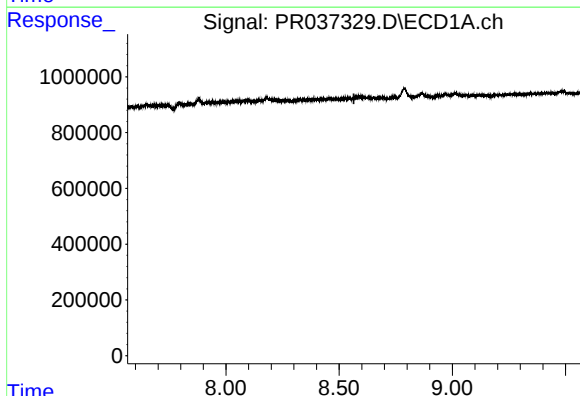


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

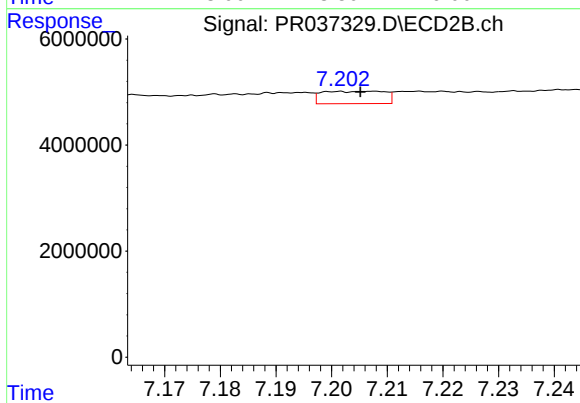

#38 AR-1262-3


R.T.: 7.202 min
Delta R.T.: -0.004 min
Response: 1825118
Conc: 3.33 ng/ml

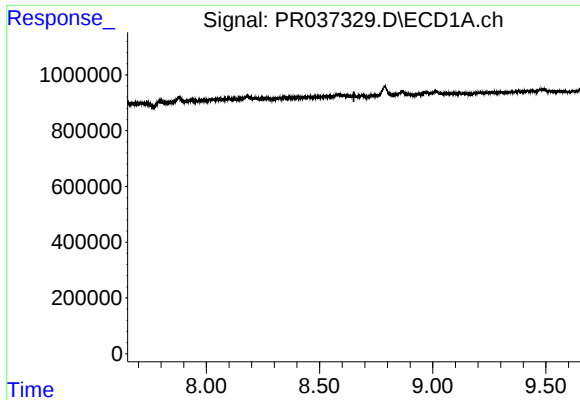

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

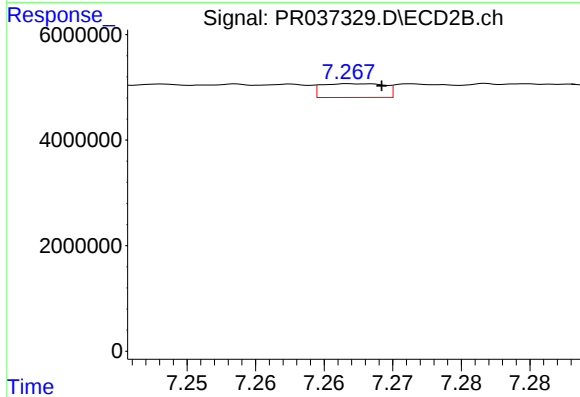


#39 AR-1262-4

R.T.: 7.268 min
Delta R.T.: -0.002 min
Response: 828106
Conc: 0.92 ng/ml

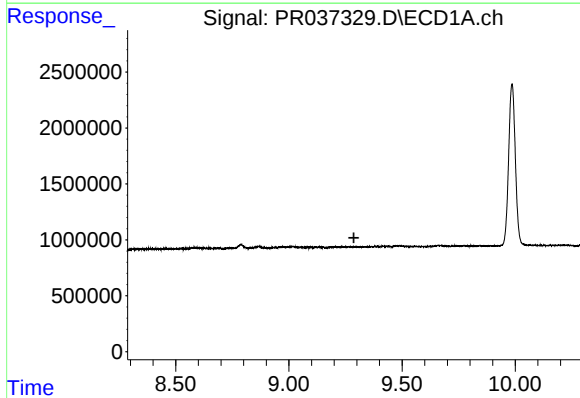


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

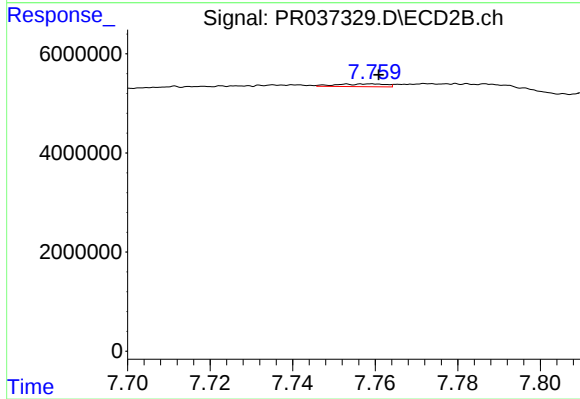

#40 AR-1262-5


R.T.: 7.759 min
Delta R.T.: -0.002 min
Response: 472650
Conc: 1.24 ng/ml

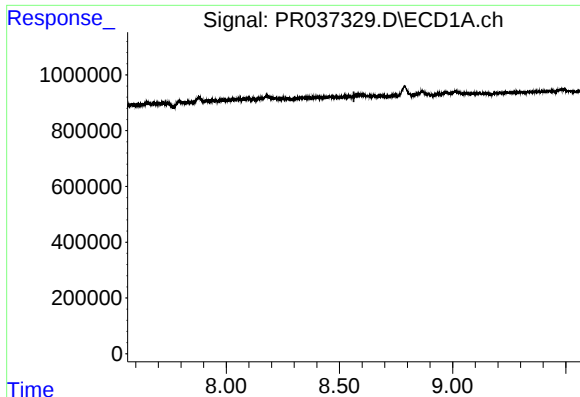

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

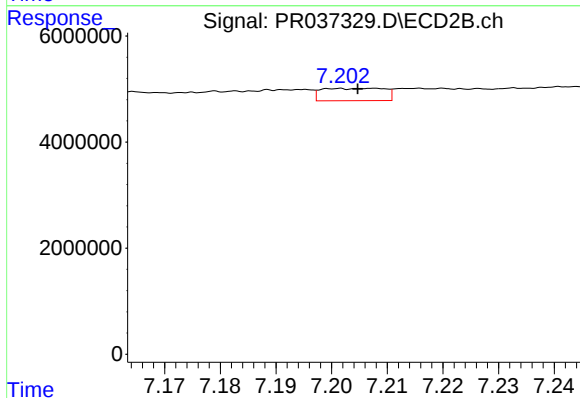


#41 AR-1268-1

R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 1825118
Conc: 1.48 ng/ml

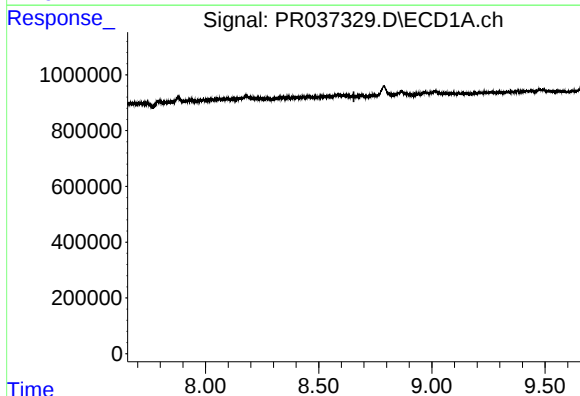


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

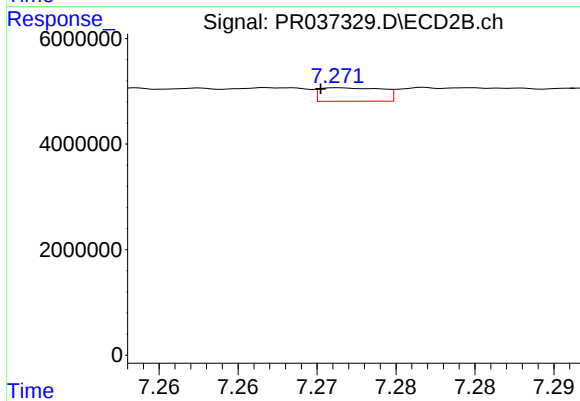

#42 AR-1268-2


R.T.: 7.272 min
Delta R.T.: 0.002 min
Response: 704233
Conc: 0.67 ng/ml

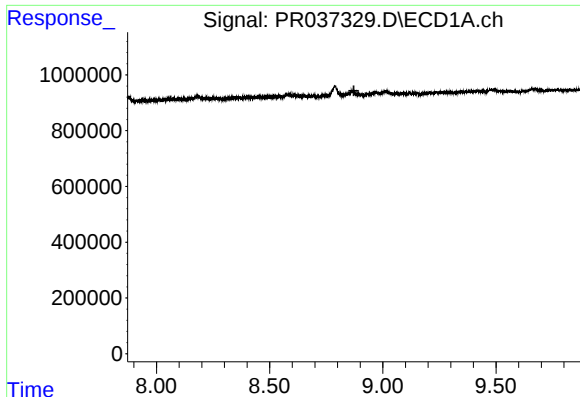

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

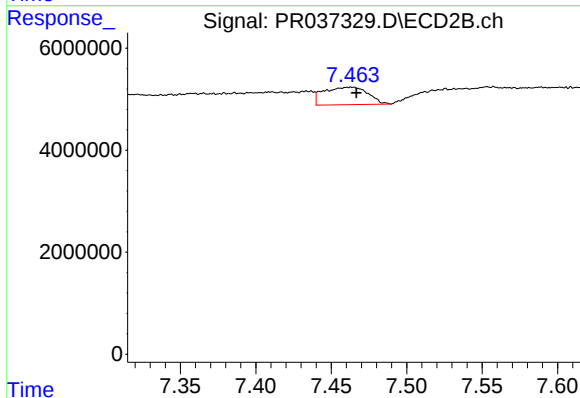


#43 AR-1268-3

R.T.: 7.463 min
Delta R.T.: -0.004 min
Response: 7013942
Conc: 7.91 ng/ml

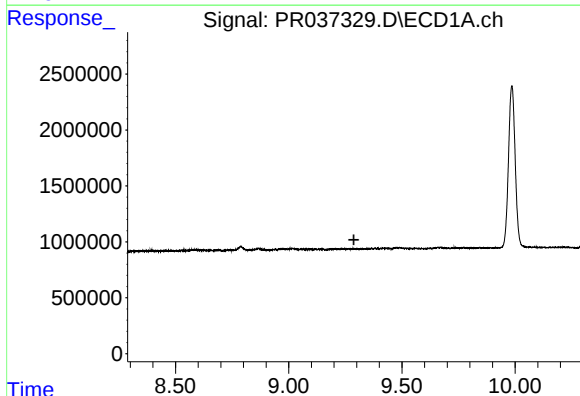


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

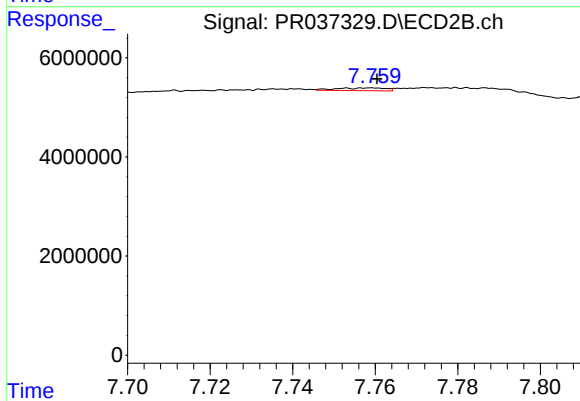

#44 AR-1268-4


R.T.: 7.759 min
Delta R.T.: -0.002 min
Response: 472650
Conc: 1.30 ng/ml

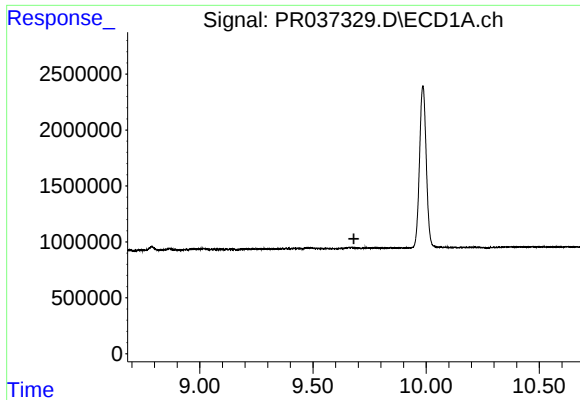

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

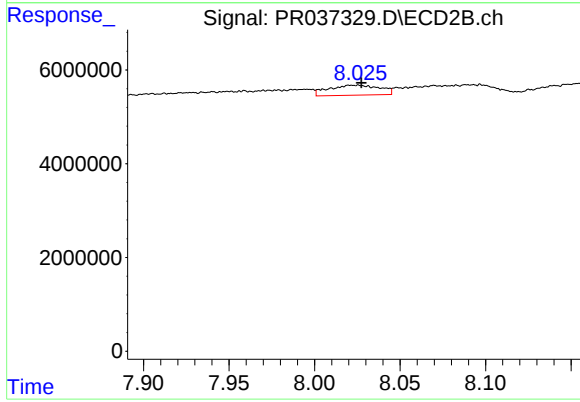

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.002 min
Response: 4419734
Conc: 1.74 ng/ml