

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 18:35
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1248 MDL 25PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 22:02:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.358	3.407	27348525	106.6E6	21.861	22.220
2)	SA Decachlor...	9.987	8.245	28653796	139.0E6	21.665	23.864
Target Compounds							
3)	L1 AR-1016-1	5.519	4.451	794386	3123023	18.436	17.152
4)	L1 AR-1016-2	5.541	4.465	1042131	3233604	15.049	11.462
5)	L1 AR-1016-3	5.601	4.637	767766	1828233	19.038	12.715 #
6)	L1 AR-1016-4	5.699	4.680	427259	4189581	13.010	37.868 #
7)	L1 AR-1016-5	5.990	4.883	1121117	6449663	32.695	42.429 #
8)	L2 AR-1221-1	0.000	3.569	0	406997	N.D.	7.993 #
9)	L2 AR-1221-2	4.663	3.696	524268	1603380	57.969	43.176 #
10)	L2 AR-1221-3	0.000	3.769	0	257004	N.D.	2.099 #
11)	L3 AR-1232-1	0.000	3.769	0	257004	N.D.	2.197 #
12)	L3 AR-1232-2	5.252	4.465	470521	3233604	27.846	23.394
13)	L3 AR-1232-3	5.541	4.637	1042131	1828233	30.828	26.043
14)	L3 AR-1232-4	5.699	4.718	427259	3989427	27.220	66.856 #
15)	L3 AR-1232-5	5.787	4.883	984643	6449663	84.189	94.509
16)	L4 AR-1242-1	5.519	4.451	794386	3123023	23.218	21.312
17)	L4 AR-1242-2	5.541	4.465	1042131	3233604	18.787	14.173
18)	L4 AR-1242-3	5.601	4.637	767766	1828233	23.326	15.811 #
19)	L4 AR-1242-4	5.699	4.718	427259	3989427	16.198	36.297 #
20)	L4 AR-1242-5	6.429	5.226	2026553	12404495	62.978	74.861
21)	L5 AR-1248-1	5.519	4.451	794386	3123023	34.678	31.024
22)	L5 AR-1248-2	5.787	4.680	984643	4189581	28.121	30.699
23)	L5 AR-1248-3	5.990	4.718	1121117	3989427	27.405	28.501
24)	L5 AR-1248-4	6.429	4.883	2026553	6449663	41.397	36.241
25)	L5 AR-1248-5	6.429	5.261	2026553	10640370	42.902	54.395 #
26)	L6 AR-1254-1	6.366	5.226	5295708	12404495	96.936	36.010 #
27)	L6 AR-1254-2	6.585	5.371	1657188	15821948	19.338	52.827 #
28)	L6 AR-1254-3	6.961	5.762	1983088	8801873	21.801	18.584
29)	L6 AR-1254-4	7.231	5.987	3131591	2662328	46.734	7.593 #
30)	L6 AR-1254-5	7.648	6.394	452323	1927011	6.293	4.352 #
31)	L7 AR-1260-1	7.130	5.899	1071249	1549392	16.234	5.301 #
32)	L7 AR-1260-2	7.380	6.067	2710683	4244790	34.009	9.216 #
33)	L7 AR-1260-3	0.000	6.218	0	583097	N.D.	1.636 #
34)	L7 AR-1260-4	0.000	6.685	0	107955	N.D.	0.354 #
35)	L7 AR-1260-5	0.000	6.932	0	234702	N.D.	0.271 #
36)	L8 AR-1262-1	0.000	6.493	0	4352947	N.D.	17.369 #
37)	L8 AR-1262-2	0.000	6.932	0	234702	N.D.	0.187 #
38)	L8 AR-1262-3	0.000	7.201	0	3921963	N.D.	7.153 #
39)	L8 AR-1262-4	0.000	7.264	0	28938894	N.D.	32.239 #
40)	L8 AR-1262-5	0.000	7.782	0	815274	N.D.	2.131 #
41)	L9 AR-1268-1	0.000	7.201	0	3921963	N.D.	3.186 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 18:35
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1248 MDL 25PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 22:02:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.264	0	28938894	N.D.	27.329 #
43) L9	AR-1268-3	0.000	7.466	0	9407286	N.D.	10.615 #
44) L9	AR-1268-4	0.000	7.782	0	815274	N.D.	2.247 #
45) L9	AR-1268-5	0.000	8.025	0	3944884	N.D.	1.551 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
Data File : PR037330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 18:35
Operator : SM\SJ
Sample : K1560-03
Misc : AR1248 MDL 25PPB
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 22:02:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

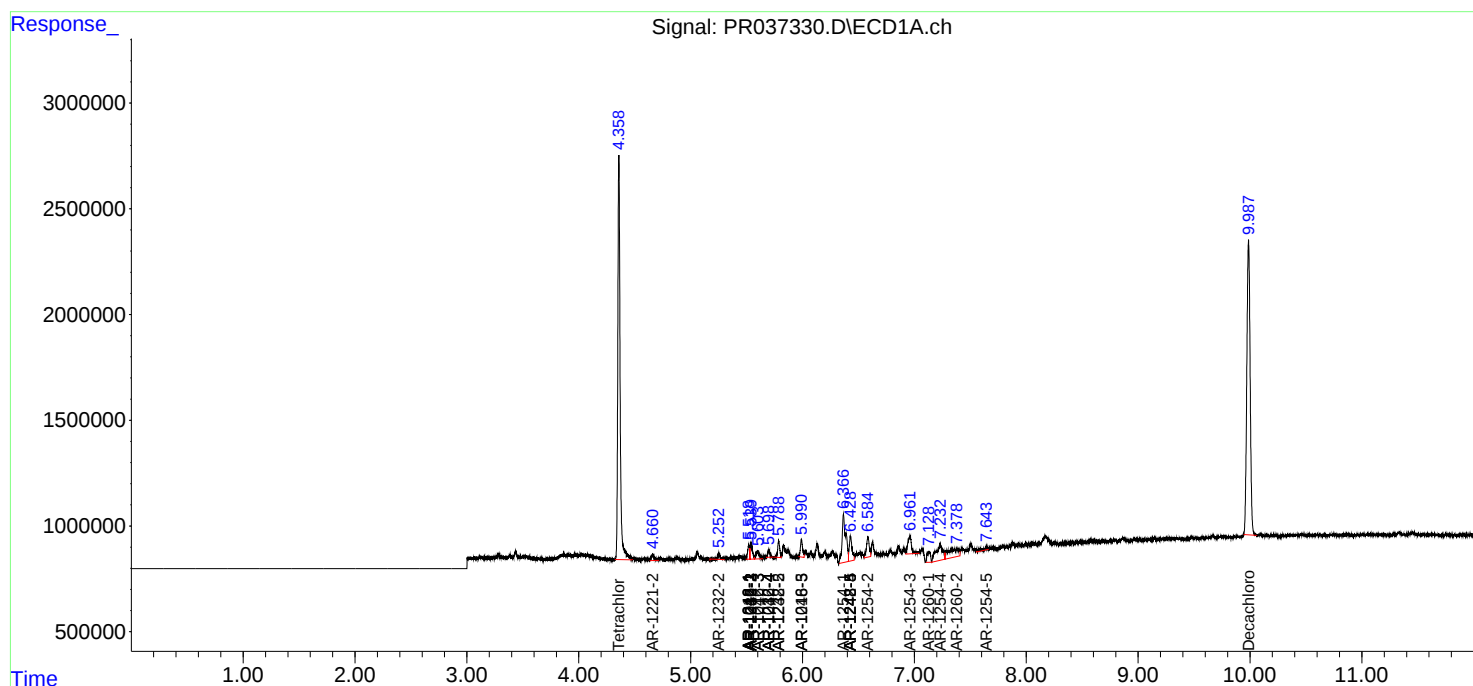


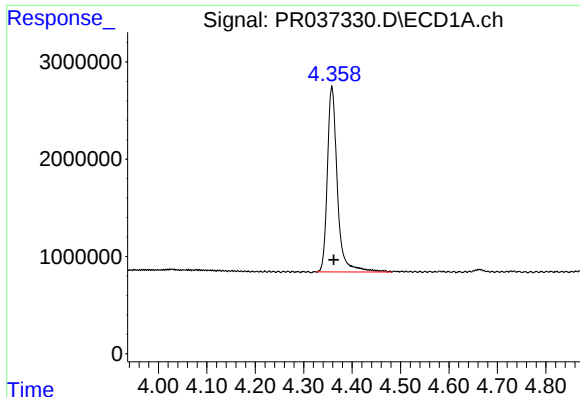

#1 Tetrachloro-m-xylene


R.T.: 4.358 min
Delta R.T.: -0.004 min
Response: 27348525
Conc: 21.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

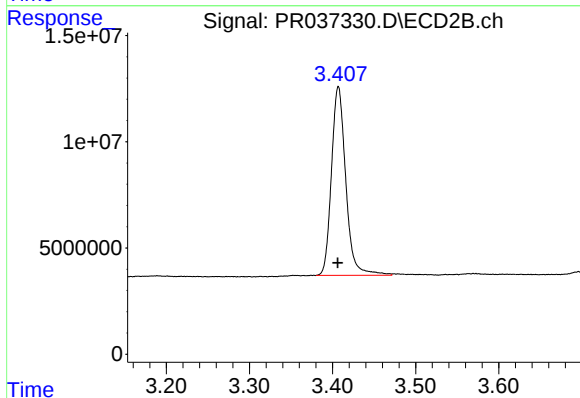


#1 Tetrachloro-m-xylene

R.T.: 3.407 min
Delta R.T.: 0.000 min
Response: 106555670
Conc: 22.22 ng/ml

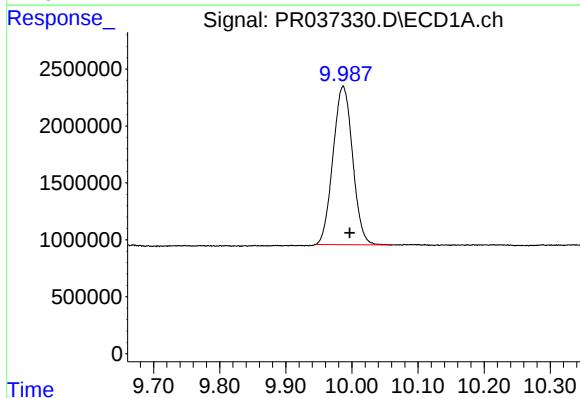


#2 Decachlorobiphenyl

R.T.: 9.987 min
Delta R.T.: -0.010 min
Response: 28653796
Conc: 21.67 ng/ml

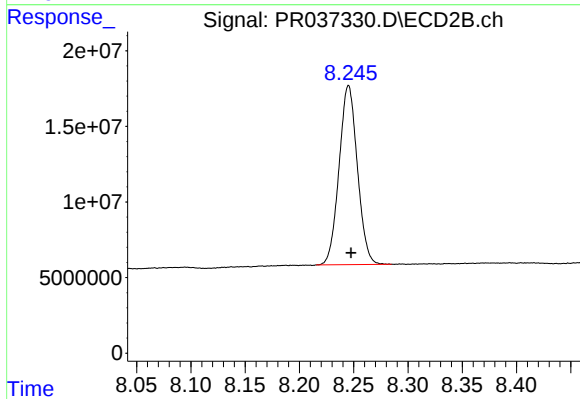

#2 Decachlorobiphenyl


R.T.: 8.245 min
Delta R.T.: -0.002 min
Response: 138992575
Conc: 23.86 ng/ml

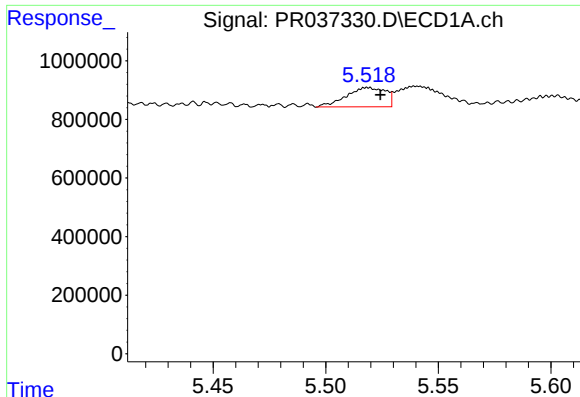

#3 AR-1016-1


R.T.: 5.519 min
Delta R.T.: -0.005 min
Response: 794386
Conc: 18.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

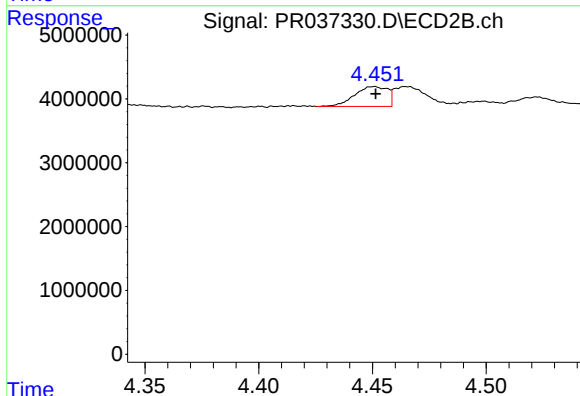


#3 AR-1016-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3123023
Conc: 17.15 ng/ml

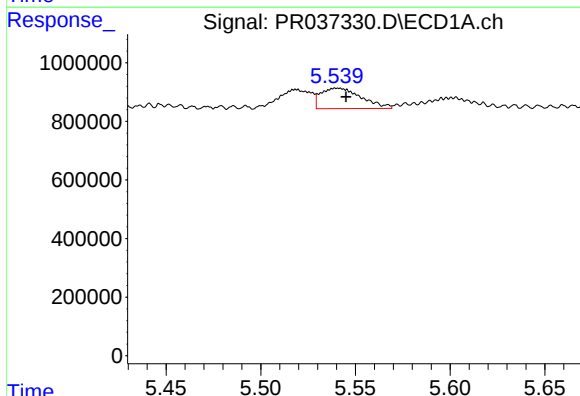


#4 AR-1016-2

R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 1042131
Conc: 15.05 ng/ml

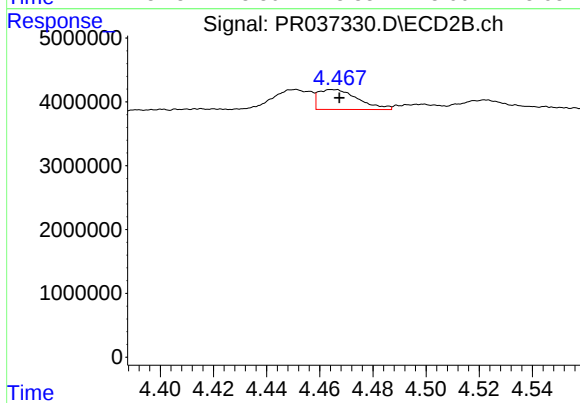

#4 AR-1016-2


R.T.: 4.465 min
Delta R.T.: -0.003 min
Response: 3233604
Conc: 11.46 ng/ml

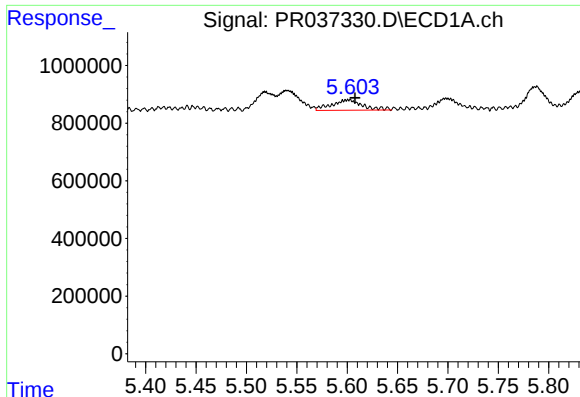

#5 AR-1016-3


R.T.: 5.601 min
Delta R.T.: -0.007 min
Response: 767766
Conc: 19.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

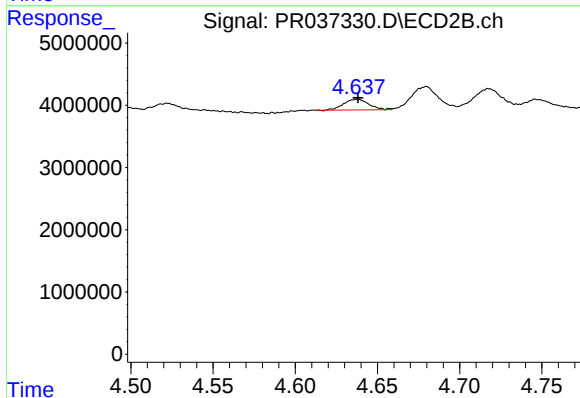


#5 AR-1016-3

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 1828233
Conc: 12.72 ng/ml

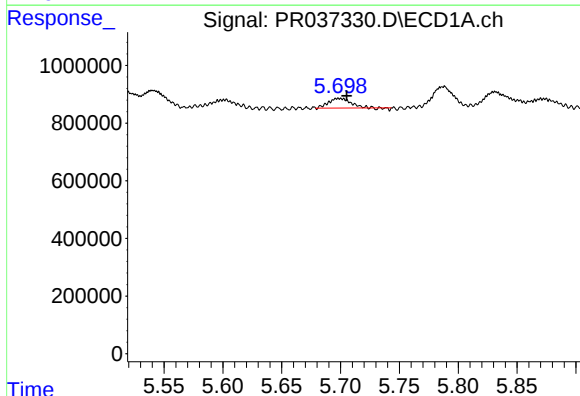


#6 AR-1016-4

R.T.: 5.699 min
Delta R.T.: -0.006 min
Response: 427259
Conc: 13.01 ng/ml

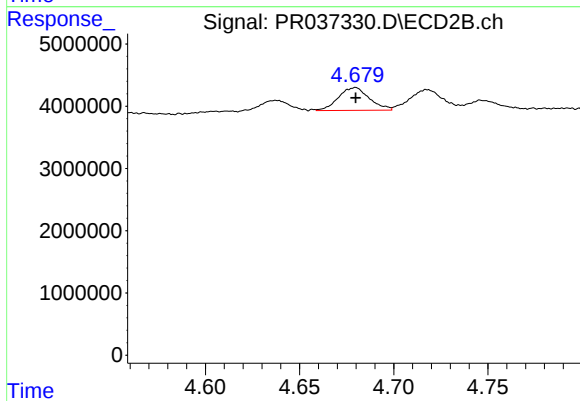

#6 AR-1016-4


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 4189581
Conc: 37.87 ng/ml

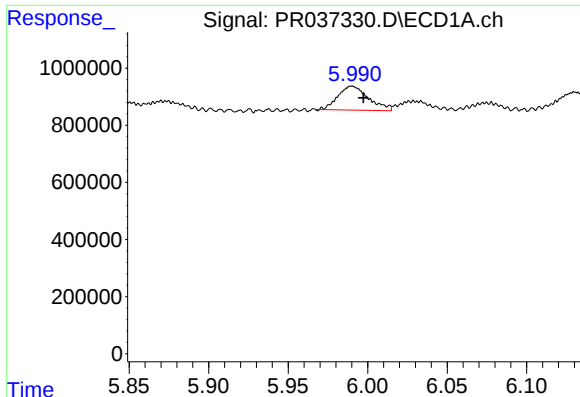

#7 AR-1016-5


R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 1121117
Conc: 32.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

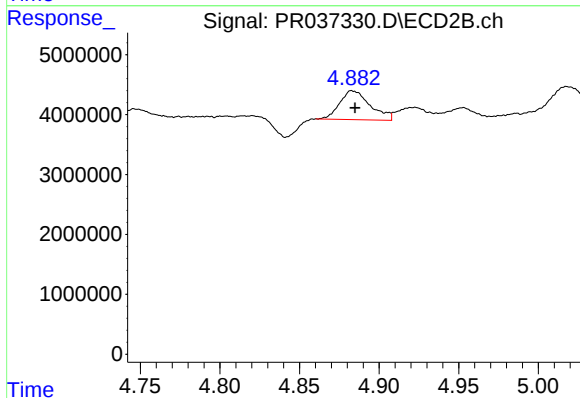


#7 AR-1016-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 6449663
Conc: 42.43 ng/ml

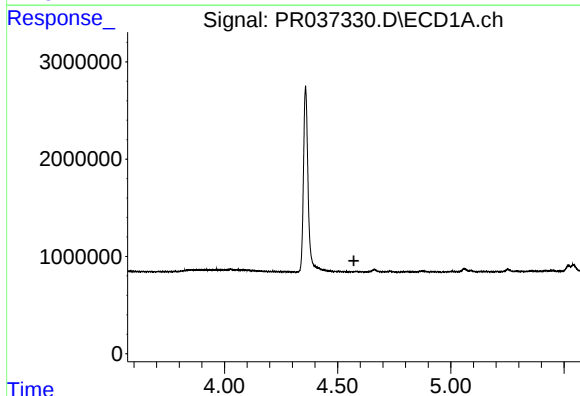


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

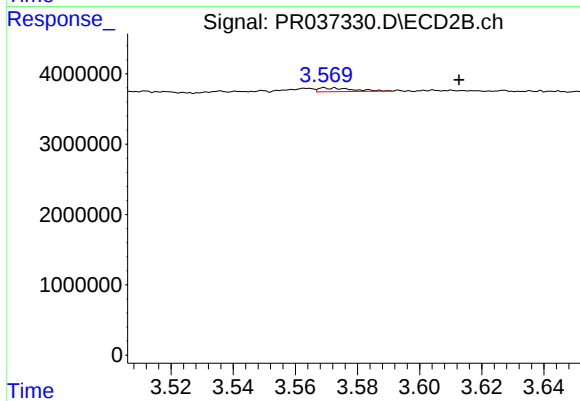

#8 AR-1221-1


R.T.: 3.569 min
Delta R.T.: -0.043 min
Response: 406997
Conc: 7.99 ng/ml

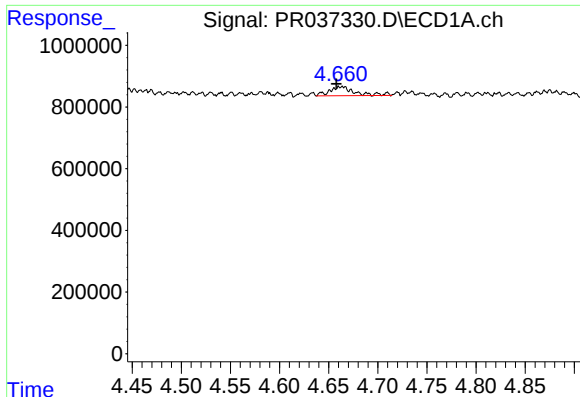

#9 AR-1221-2


R.T.: 4.663 min
Delta R.T.: 0.005 min
Response: 524268
Conc: 57.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

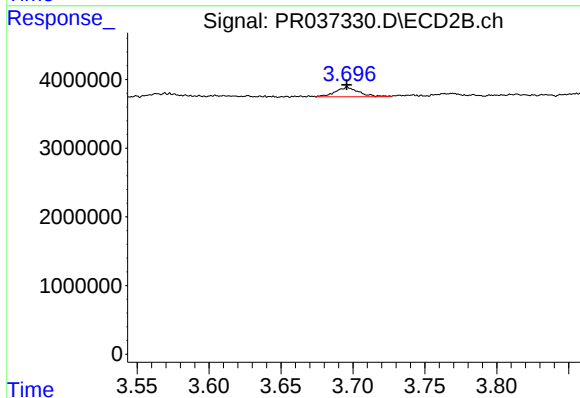


#9 AR-1221-2

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 1603380
Conc: 43.18 ng/ml

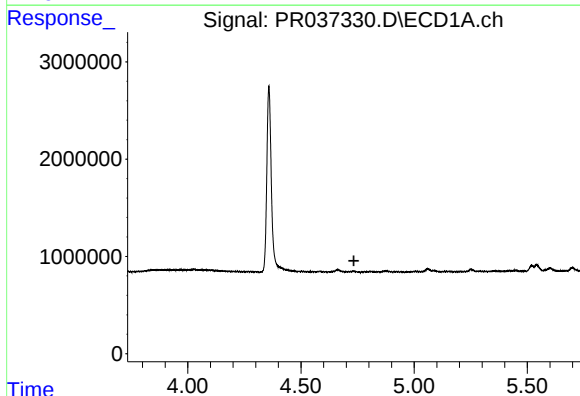


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

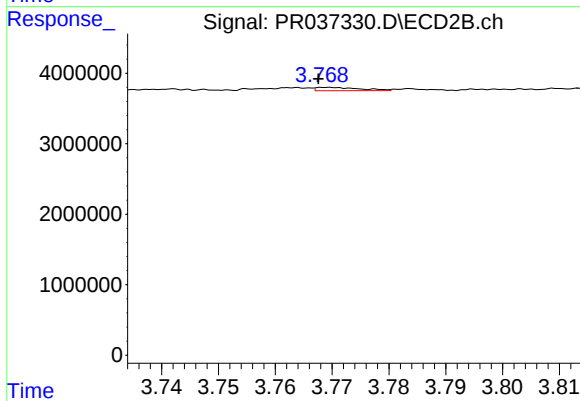

#10 AR-1221-3


R.T.: 3.769 min
Delta R.T.: 0.002 min
Response: 257004
Conc: 2.10 ng/ml

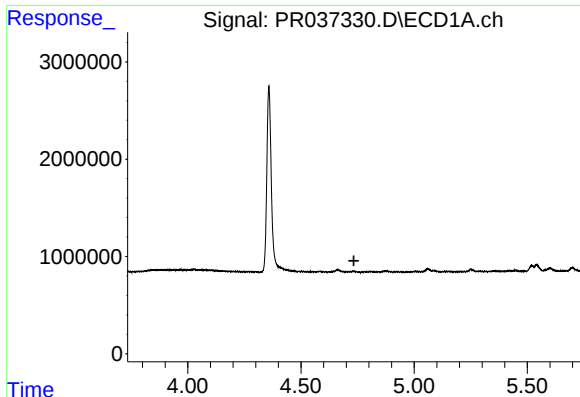

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

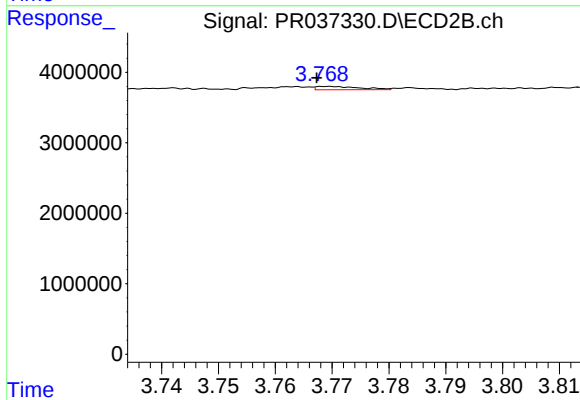


#11 AR-1232-1

R.T.: 3.769 min
Delta R.T.: 0.002 min
Response: 257004
Conc: 2.20 ng/ml

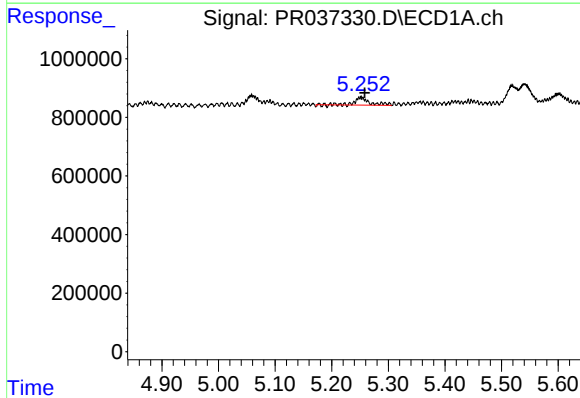


#12 AR-1232-2

R.T.: 5.252 min
Delta R.T.: -0.006 min
Response: 470521
Conc: 27.85 ng/ml

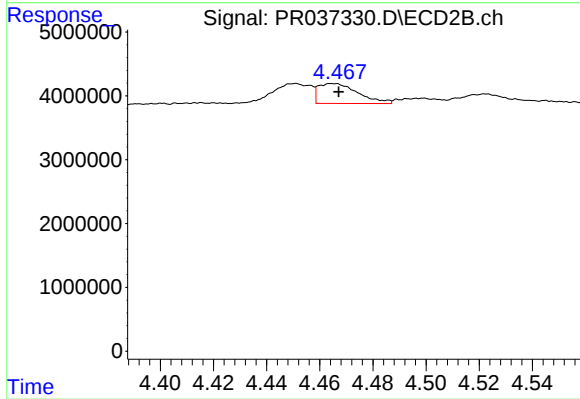

#12 AR-1232-2


R.T.: 4.465 min
Delta R.T.: -0.003 min
Response: 3233604
Conc: 23.39 ng/ml

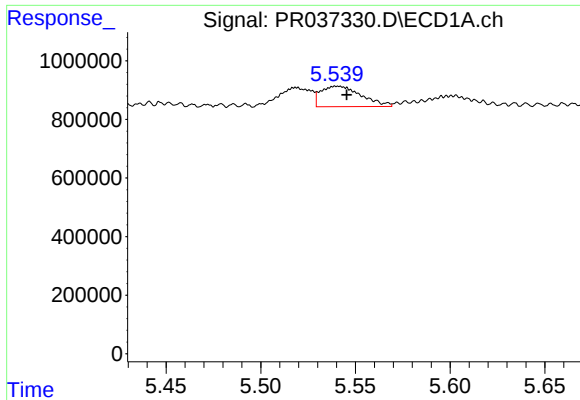

#13 AR-1232-3


R.T.: 5.541 min
Delta R.T.: -0.005 min
Response: 1042131
Conc: 30.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

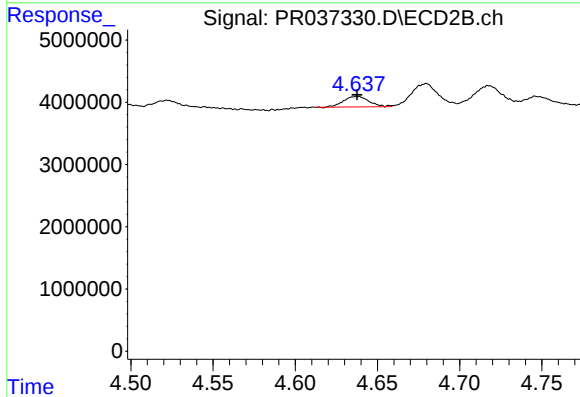


#13 AR-1232-3

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 1828233
Conc: 26.04 ng/ml

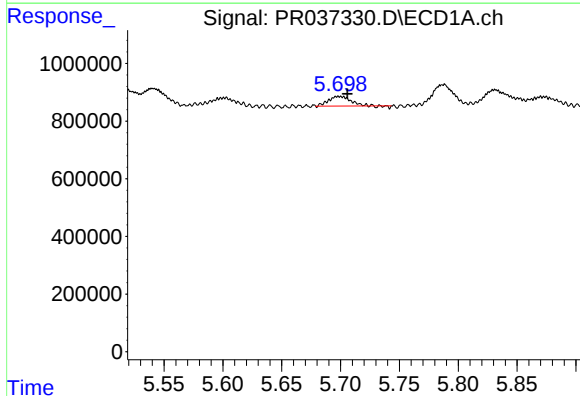


#14 AR-1232-4

R.T.: 5.699 min
Delta R.T.: -0.006 min
Response: 427259
Conc: 27.22 ng/ml

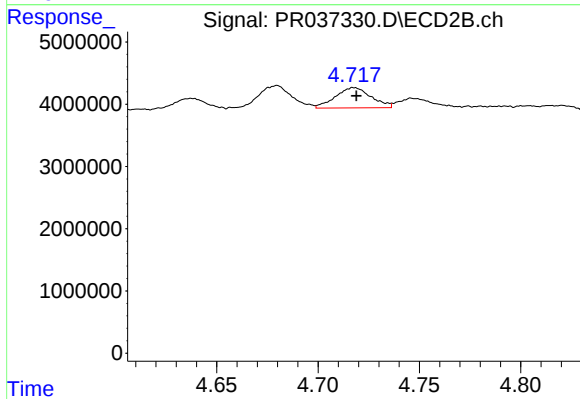

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 3989427
Conc: 66.86 ng/ml

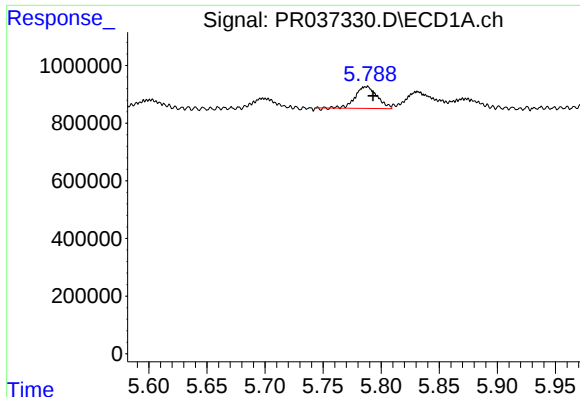

#15 AR-1232-5


R.T.: 5.787 min
Delta R.T.: -0.006 min
Response: 984643
Conc: 84.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

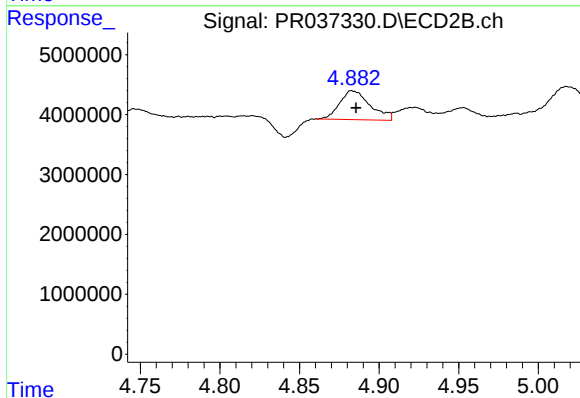


#15 AR-1232-5

R.T.: 4.883 min
Delta R.T.: -0.003 min
Response: 6449663
Conc: 94.51 ng/ml

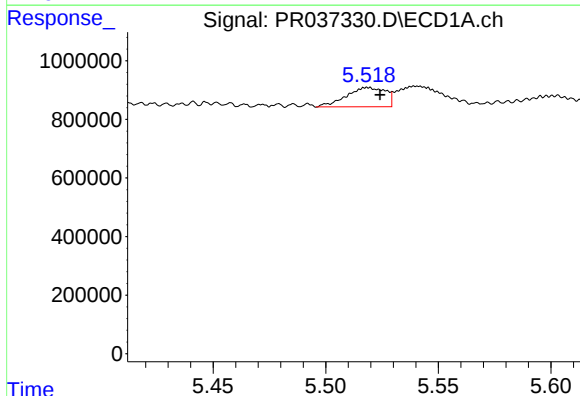


#16 AR-1242-1

R.T.: 5.519 min
Delta R.T.: -0.005 min
Response: 794386
Conc: 23.22 ng/ml

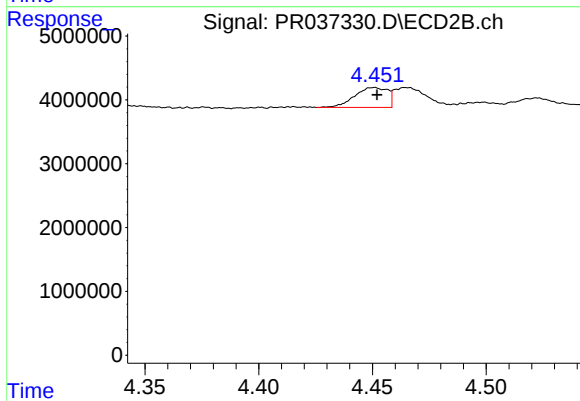

#16 AR-1242-1


R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3123023
Conc: 21.31 ng/ml

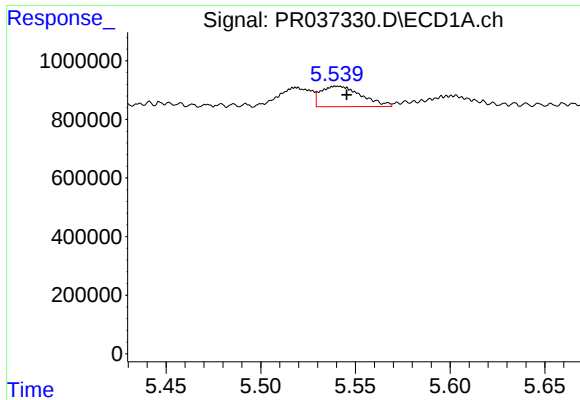

#17 AR-1242-2


R.T.: 5.541 min
Delta R.T.: -0.005 min
Response: 1042131
Conc: 18.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

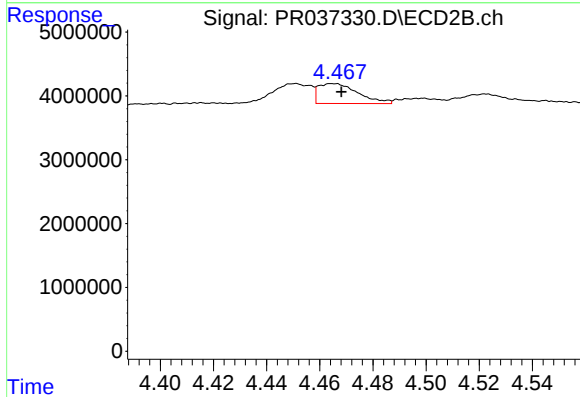


#17 AR-1242-2

R.T.: 4.465 min
Delta R.T.: -0.004 min
Response: 3233604
Conc: 14.17 ng/ml

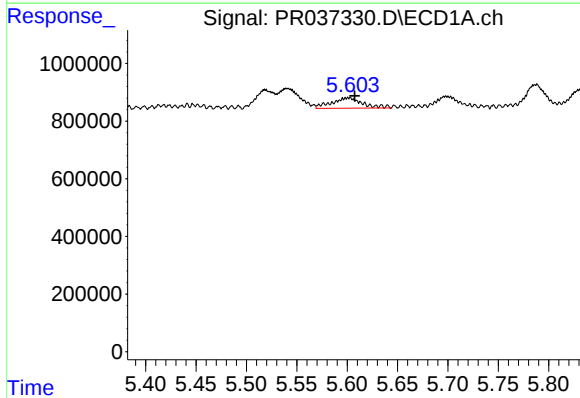


#18 AR-1242-3

R.T.: 5.601 min
Delta R.T.: -0.007 min
Response: 767766
Conc: 23.33 ng/ml

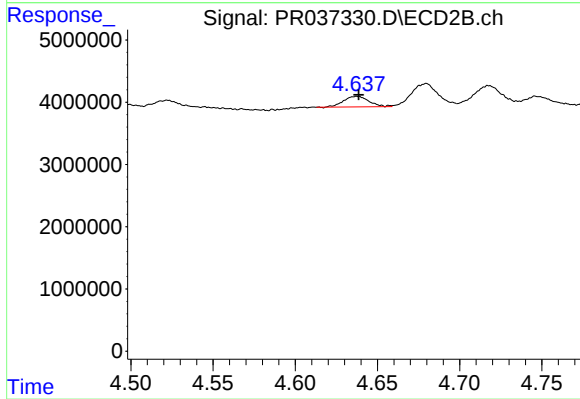

#18 AR-1242-3


R.T.: 4.637 min
Delta R.T.: -0.001 min
Response: 1828233
Conc: 15.81 ng/ml

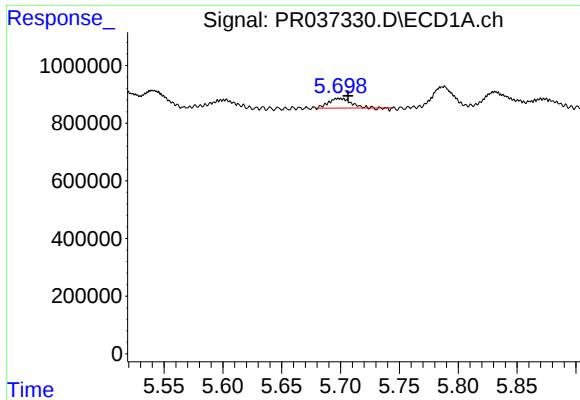

#19 AR-1242-4


R.T.: 5.699 min
Delta R.T.: -0.007 min
Response: 427259
Conc: 16.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

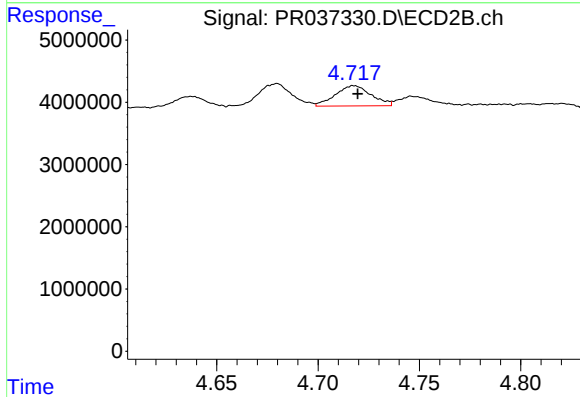


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 3989427
Conc: 36.30 ng/ml

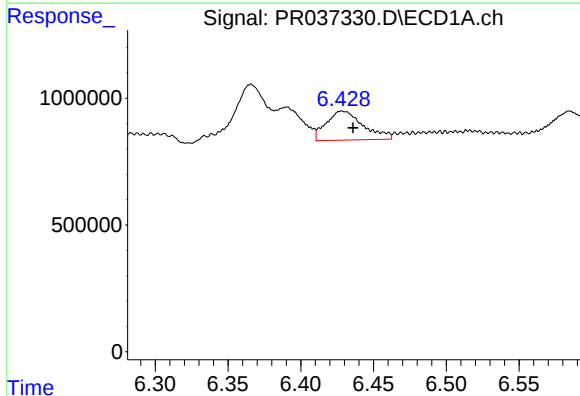


#20 AR-1242-5

R.T.: 6.429 min
Delta R.T.: -0.007 min
Response: 2026553
Conc: 62.98 ng/ml

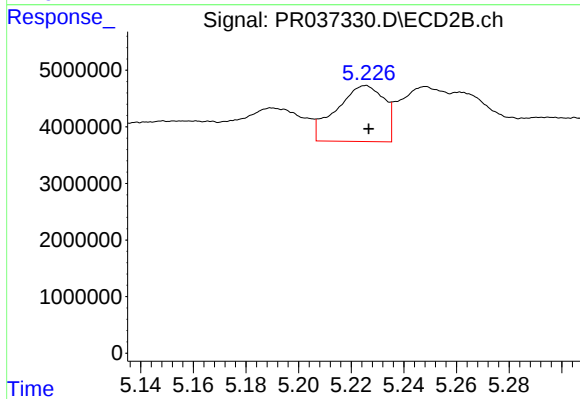

#20 AR-1242-5


R.T.: 5.226 min
Delta R.T.: -0.001 min
Response: 12404495
Conc: 74.86 ng/ml

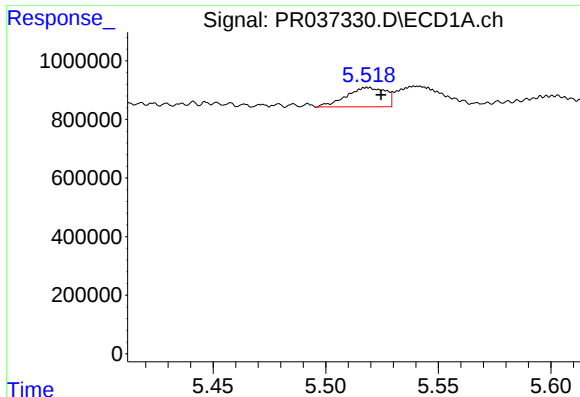

#21 AR-1248-1


R.T.: 5.519 min
Delta R.T.: -0.005 min
Response: 794386
Conc: 34.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

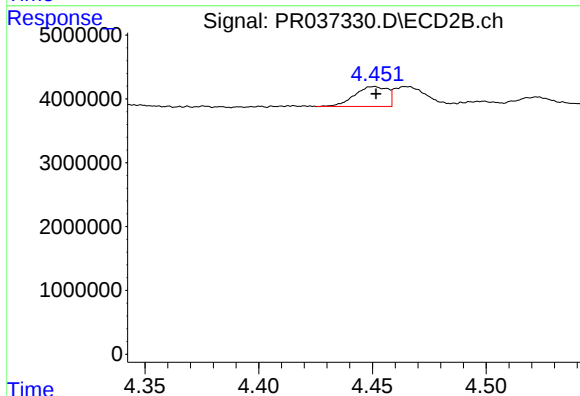


#21 AR-1248-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3123023
Conc: 31.02 ng/ml

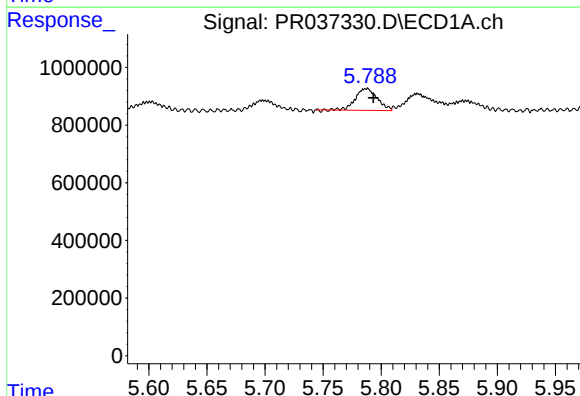


#22 AR-1248-2

R.T.: 5.787 min
Delta R.T.: -0.006 min
Response: 984643
Conc: 28.12 ng/ml

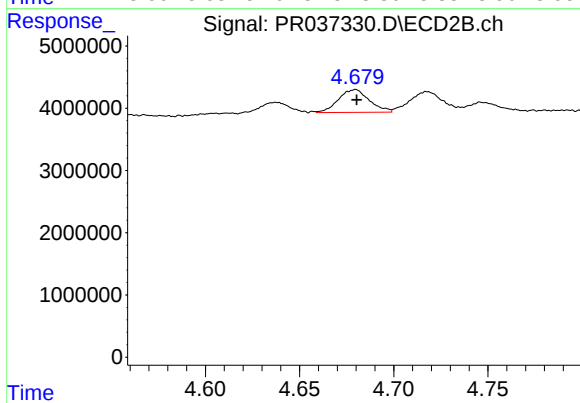

#22 AR-1248-2


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 4189581
Conc: 30.70 ng/ml

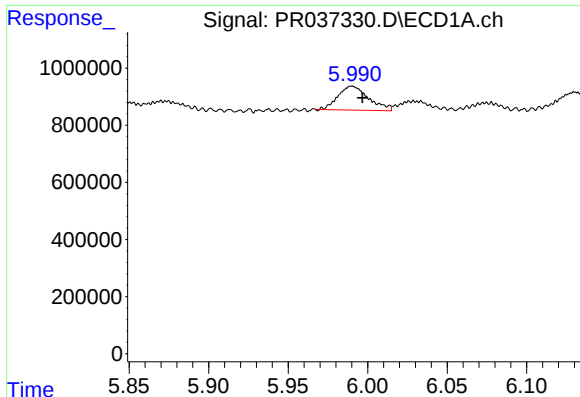

#23 AR-1248-3


R.T.: 5.990 min
Delta R.T.: -0.006 min
Response: 1121117
Conc: 27.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

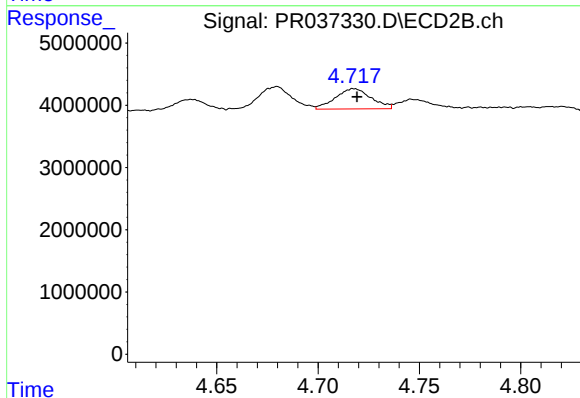


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 3989427
Conc: 28.50 ng/ml

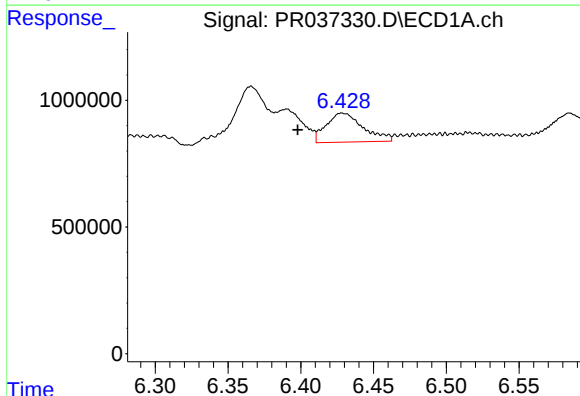


#24 AR-1248-4

R.T.: 6.429 min
Delta R.T.: 0.031 min
Response: 2026553
Conc: 41.40 ng/ml

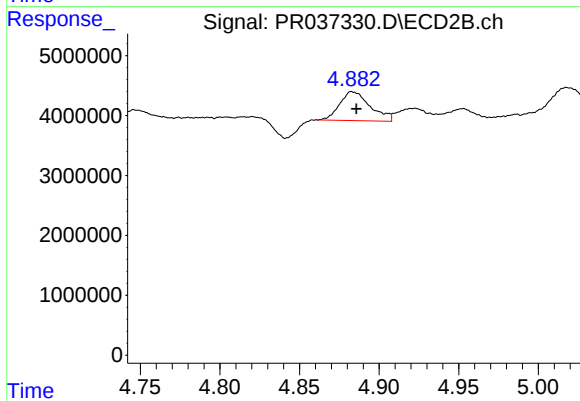

#24 AR-1248-4


R.T.: 4.883 min
Delta R.T.: -0.003 min
Response: 6449663
Conc: 36.24 ng/ml

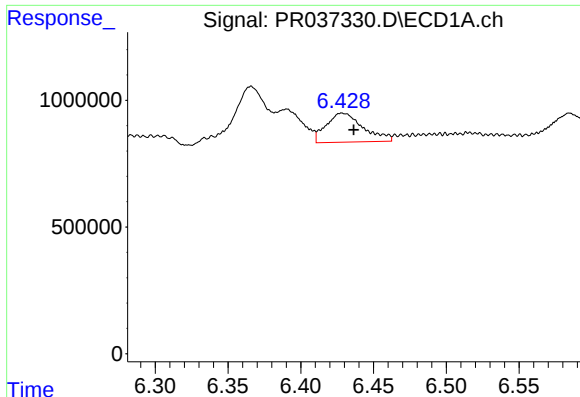

#25 AR-1248-5


R.T.: 6.429 min
Delta R.T.: -0.007 min
Response: 2026553
Conc: 42.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

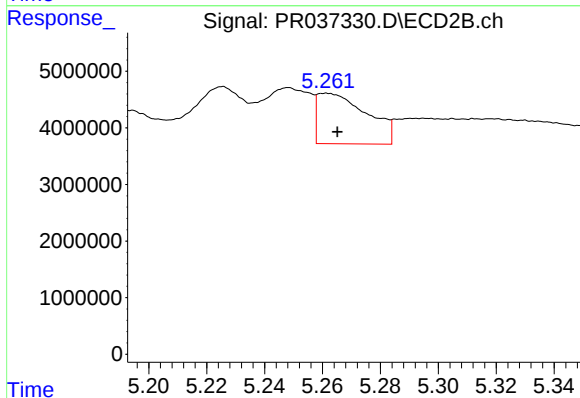


#25 AR-1248-5

R.T.: 5.261 min
Delta R.T.: -0.004 min
Response: 10640370
Conc: 54.40 ng/ml

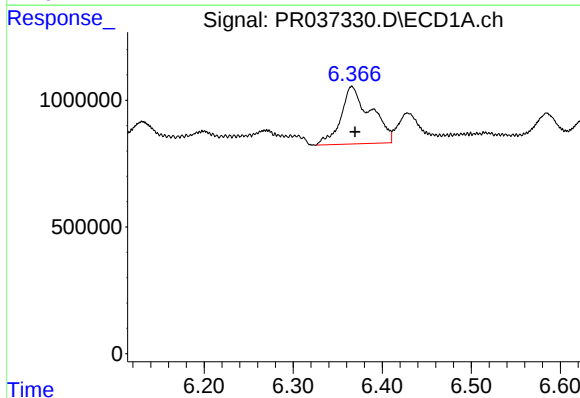


#26 AR-1254-1

R.T.: 6.366 min
Delta R.T.: -0.003 min
Response: 5295708
Conc: 96.94 ng/ml

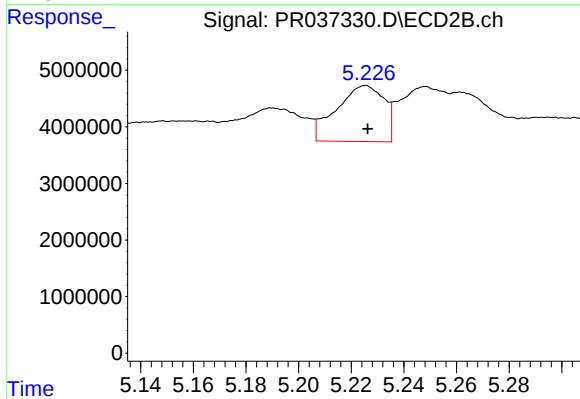

#26 AR-1254-1


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 12404495
Conc: 36.01 ng/ml

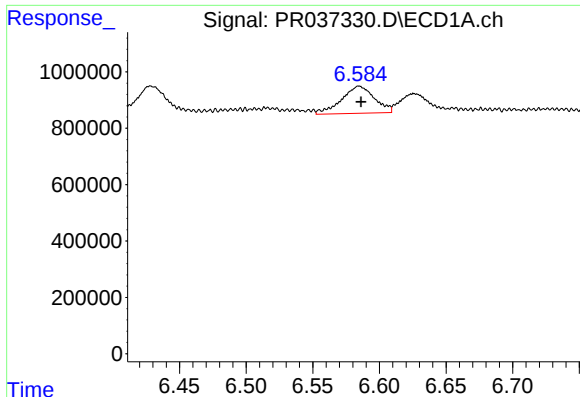

#27 AR-1254-2


R.T.: 6.585 min
Delta R.T.: -0.001 min
Response: 1657188
Conc: 19.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

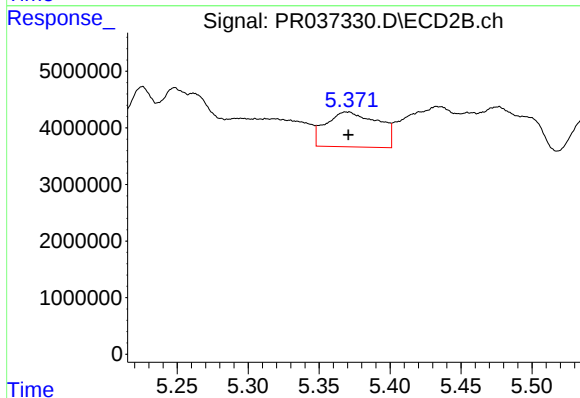


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 15821948
Conc: 52.83 ng/ml

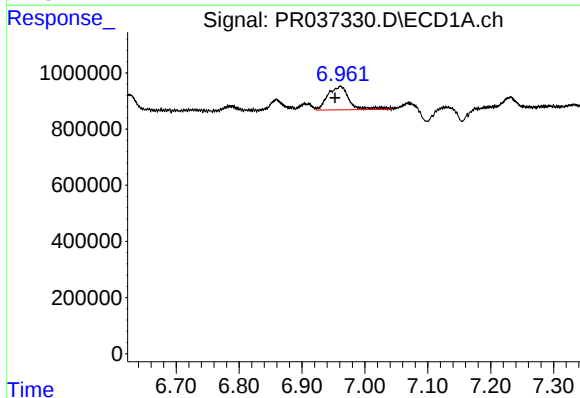


#28 AR-1254-3

R.T.: 6.961 min
Delta R.T.: 0.008 min
Response: 1983088
Conc: 21.80 ng/ml

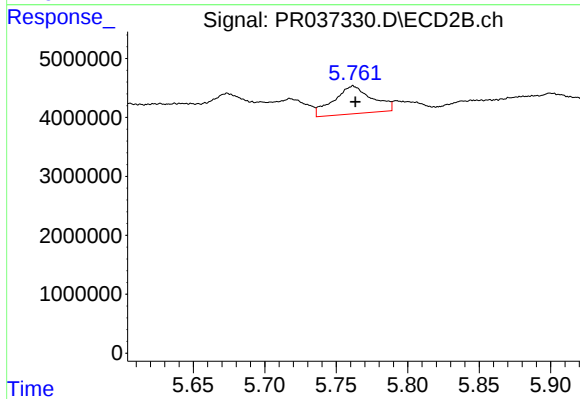

#28 AR-1254-3


R.T.: 5.762 min
Delta R.T.: -0.002 min
Response: 8801873
Conc: 18.58 ng/ml

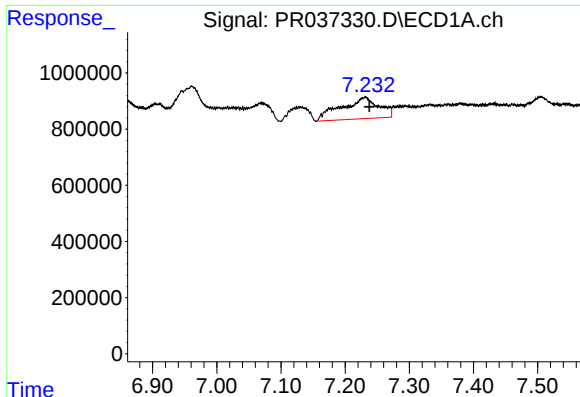

#29 AR-1254-4


R.T.: 7.231 min
Delta R.T.: -0.007 min
Response: 3131591
Conc: 46.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

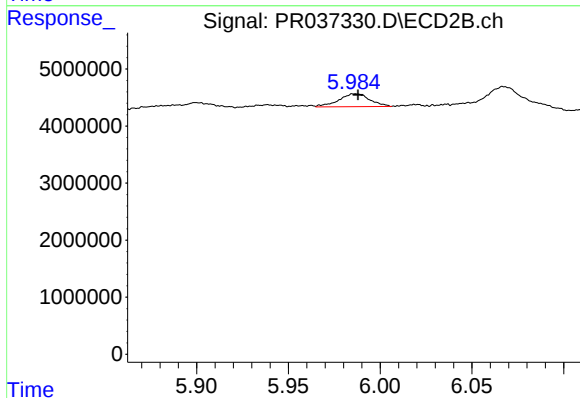


#29 AR-1254-4

R.T.: 5.987 min
Delta R.T.: -0.001 min
Response: 2662328
Conc: 7.59 ng/ml

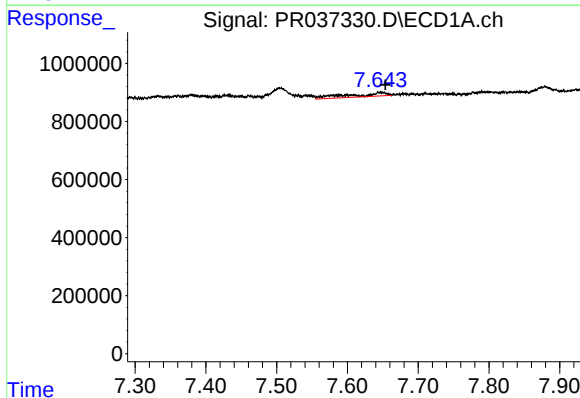


#30 AR-1254-5

R.T.: 7.648 min
Delta R.T.: -0.006 min
Response: 452323
Conc: 6.29 ng/ml

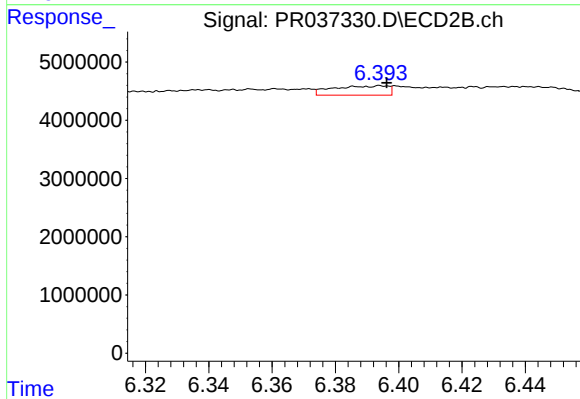

#30 AR-1254-5


R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 1927011
Conc: 4.35 ng/ml

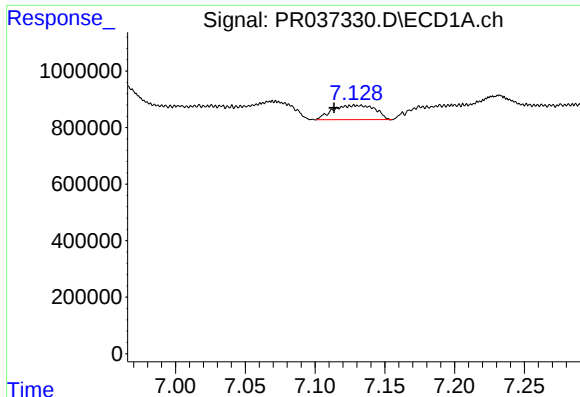

#31 AR-1260-1


R.T.: 7.130 min
Delta R.T.: 0.017 min
Response: 1071249
Conc: 16.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

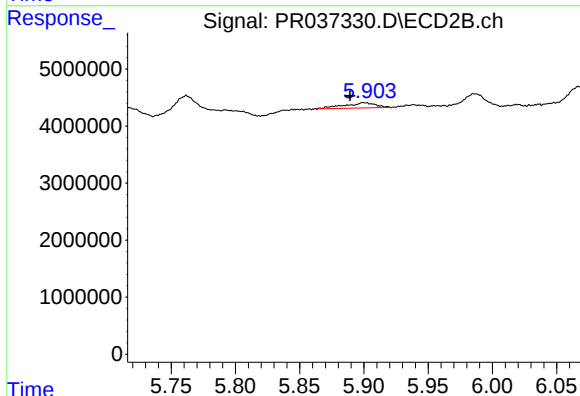


#31 AR-1260-1

R.T.: 5.899 min
Delta R.T.: 0.010 min
Response: 1549392
Conc: 5.30 ng/ml

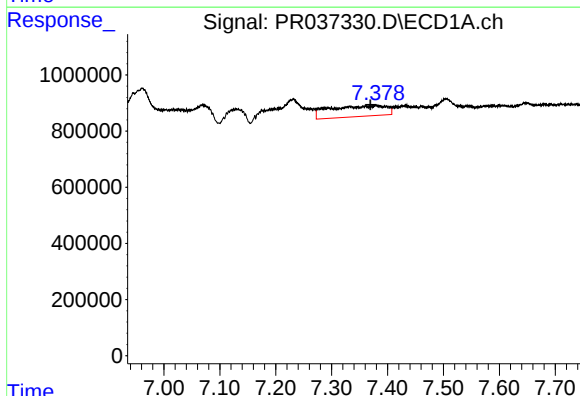


#32 AR-1260-2

R.T.: 7.380 min
Delta R.T.: 0.011 min
Response: 2710683
Conc: 34.01 ng/ml

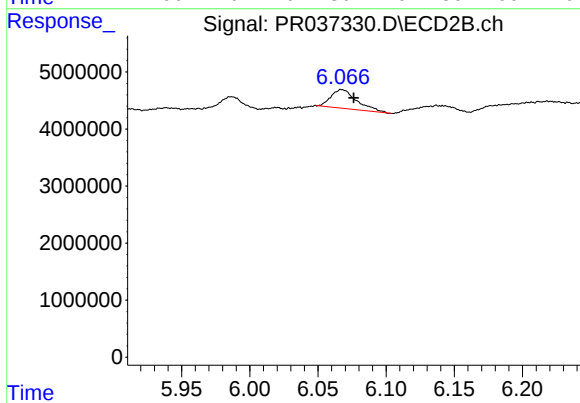

#32 AR-1260-2


R.T.: 6.067 min
Delta R.T.: -0.009 min
Response: 4244790
Conc: 9.22 ng/ml

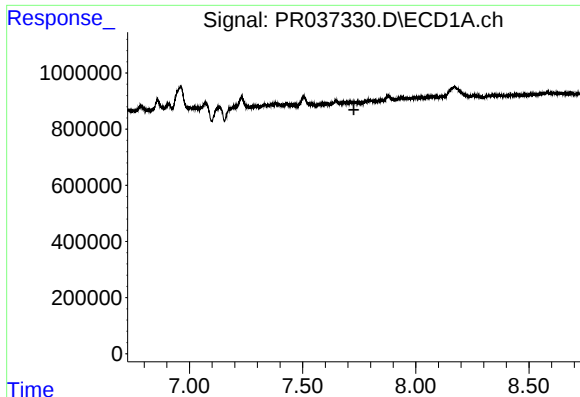

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

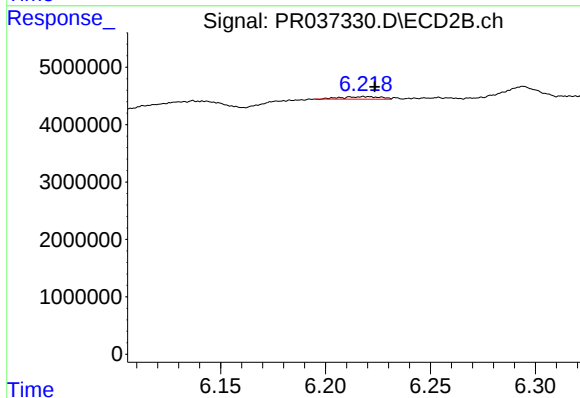


#33 AR-1260-3

R.T.: 6.218 min
Delta R.T.: -0.005 min
Response: 583097
Conc: 1.64 ng/ml

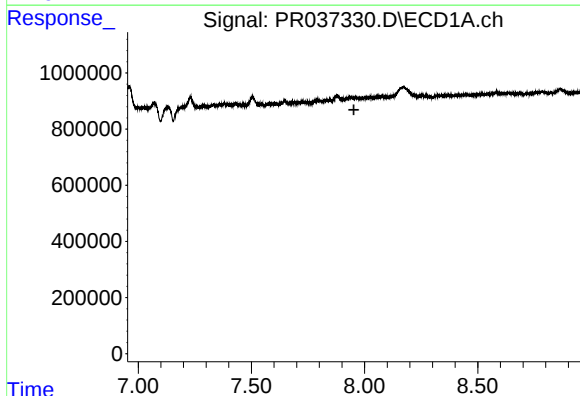


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

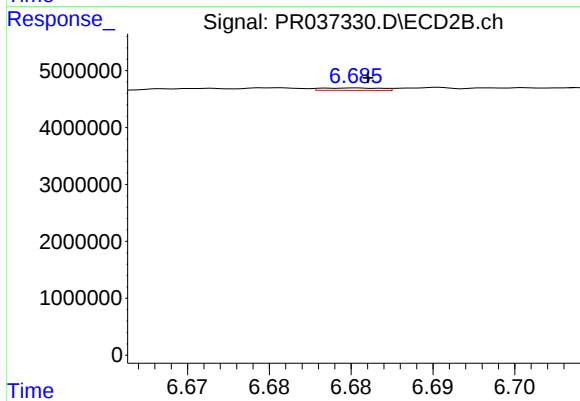

#34 AR-1260-4


R.T.: 6.685 min
Delta R.T.: 0.000 min
Response: 107955
Conc: 0.35 ng/ml

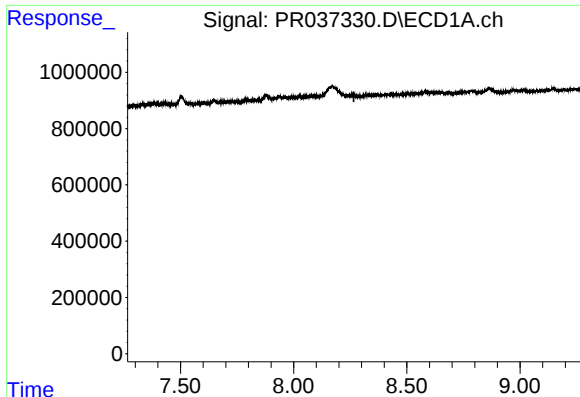

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

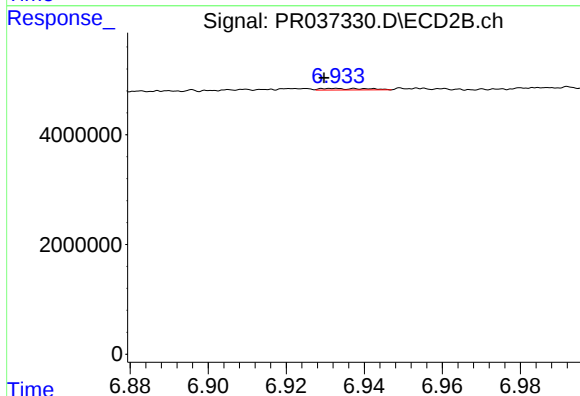


#35 AR-1260-5

R.T.: 6.932 min
Delta R.T.: 0.002 min
Response: 234702
Conc: 0.27 ng/ml

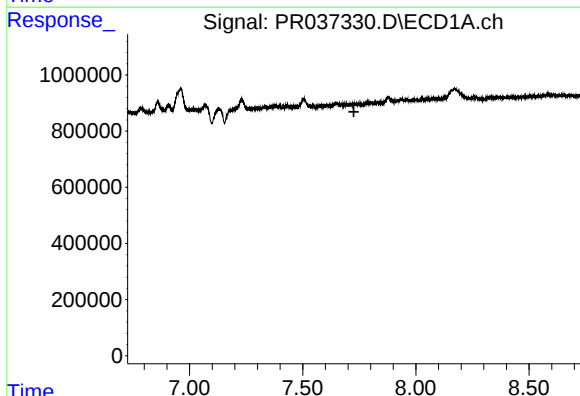


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

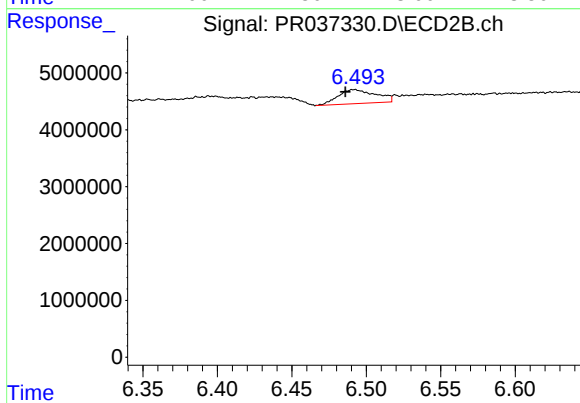

#36 AR-1262-1


R.T.: 6.493 min
Delta R.T.: 0.007 min
Response: 4352947
Conc: 17.37 ng/ml

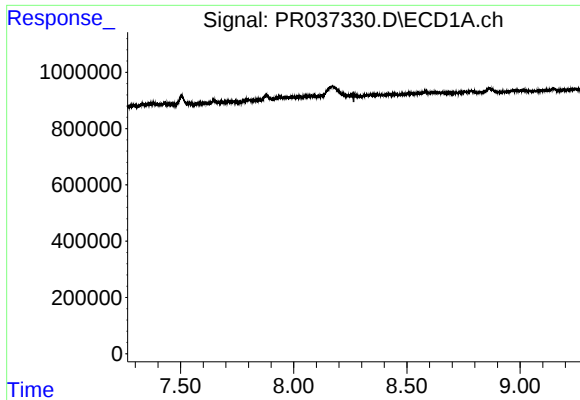

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

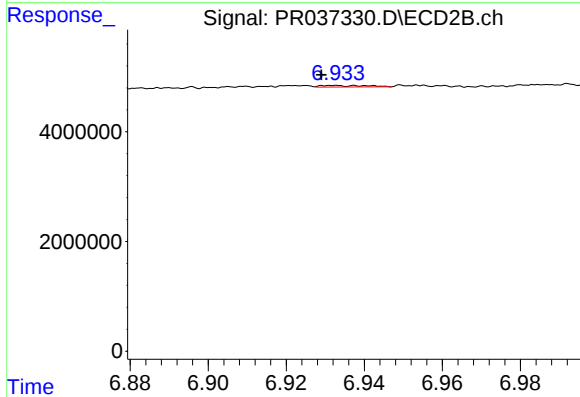


#37 AR-1262-2

R.T.: 6.932 min
Delta R.T.: 0.003 min
Response: 234702
Conc: 0.19 ng/ml

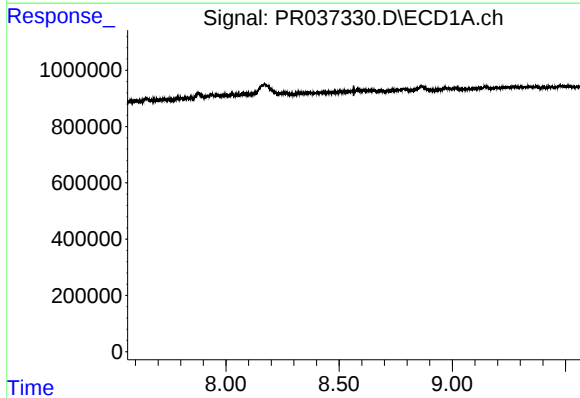


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

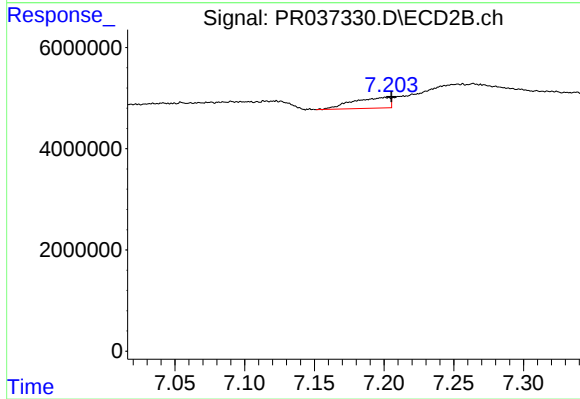

#38 AR-1262-3


R.T.: 7.201 min
Delta R.T.: -0.004 min
Response: 3921963
Conc: 7.15 ng/ml

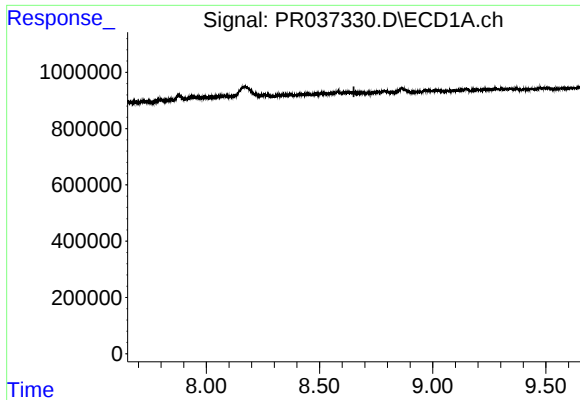

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

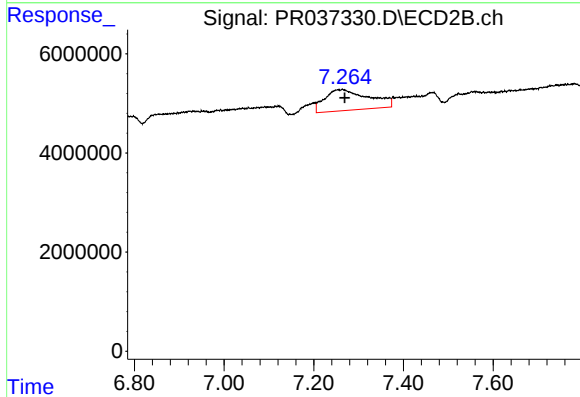


#39 AR-1262-4

R.T.: 7.264 min
Delta R.T.: -0.005 min
Response: 28938894
Conc: 32.24 ng/ml

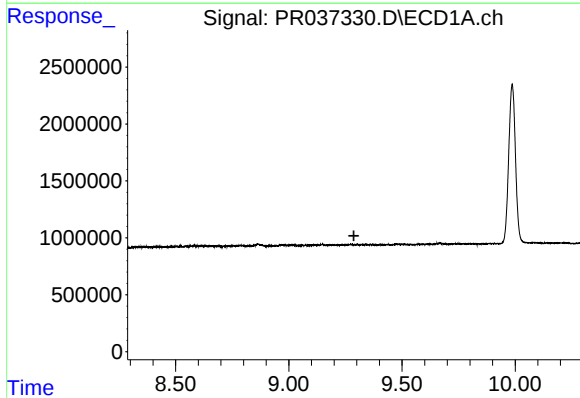


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

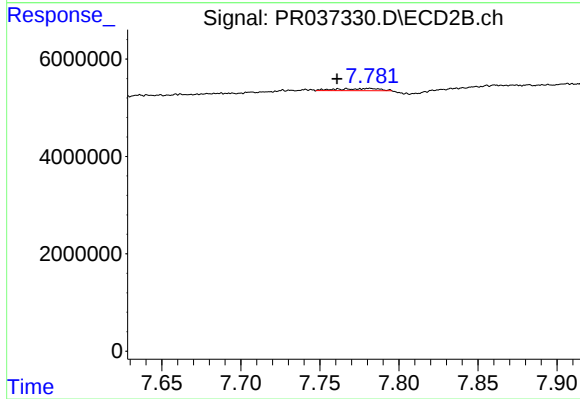

#40 AR-1262-5


R.T.: 7.782 min
Delta R.T.: 0.021 min
Response: 815274
Conc: 2.13 ng/ml

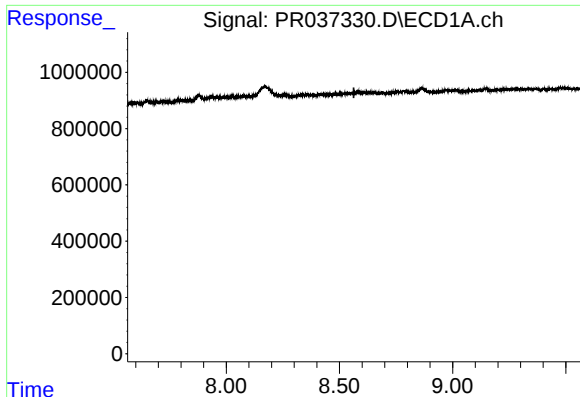

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

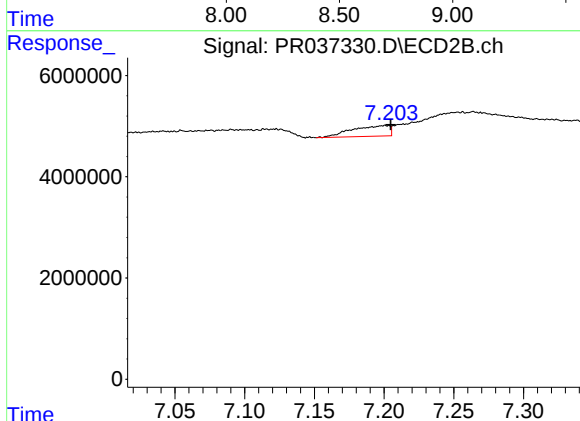


#41 AR-1268-1

R.T.: 7.201 min
Delta R.T.: -0.003 min
Response: 3921963
Conc: 3.19 ng/ml

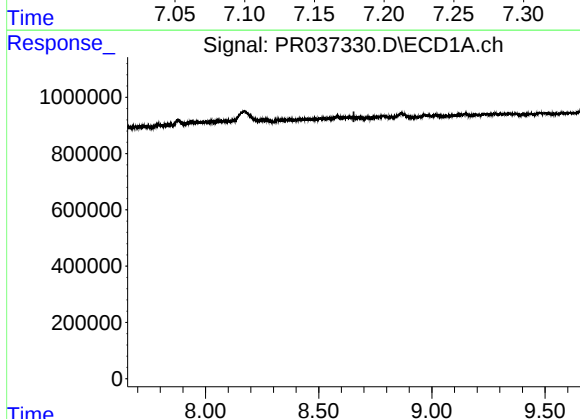


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

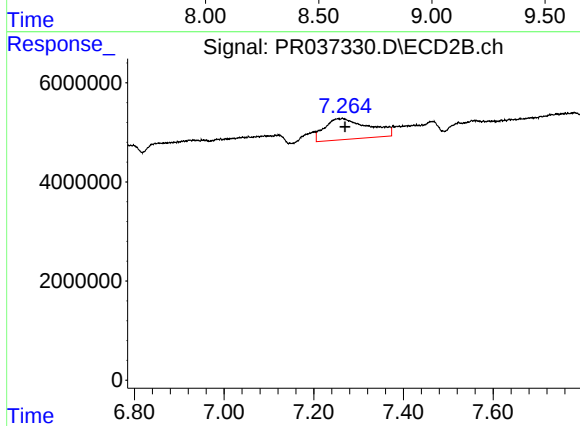

#42 AR-1268-2


R.T.: 7.264 min
Delta R.T.: -0.006 min
Response: 28938894
Conc: 27.33 ng/ml

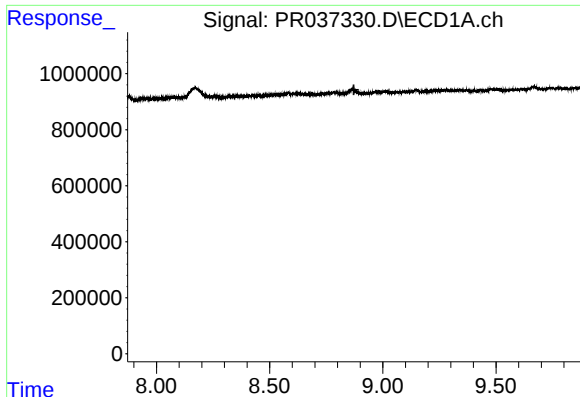

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

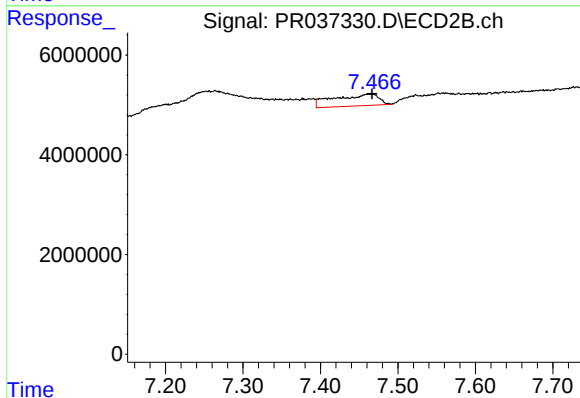


#43 AR-1268-3

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 9407286
Conc: 10.61 ng/ml

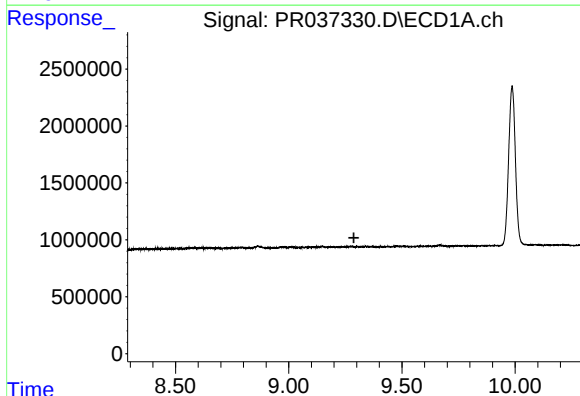


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

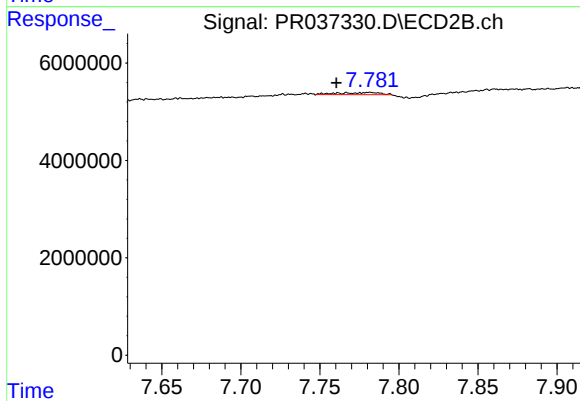

#44 AR-1268-4


R.T.: 7.782 min
Delta R.T.: 0.021 min
Response: 815274
Conc: 2.25 ng/ml

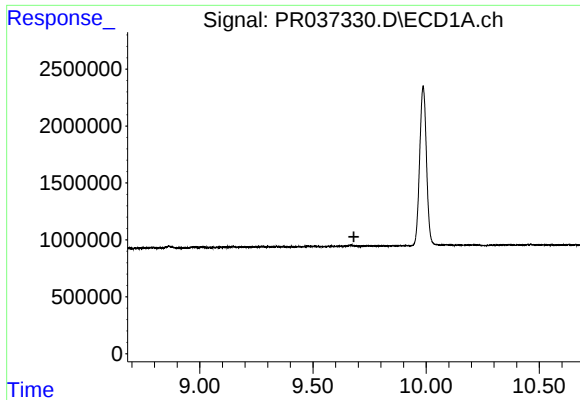

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

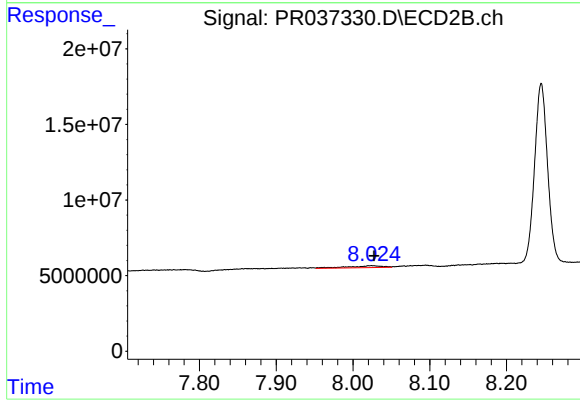

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.003 min
Response: 3944884
Conc: 1.55 ng/ml