

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 18:50
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1254 MDL 25PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 22:02:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.359	3.407	28033657	108.8E6	22.409	22.697
2)	SA Decachlor...	9.986	8.244	29342580	140.4E6	22.186	24.107
Target Compounds							
3)	L1 AR-1016-1	0.000	4.458	0	543887	N.D.	2.987 #
4)	L1 AR-1016-2	0.000	4.469	0	115424	N.D.	0.409 #
6)	L1 AR-1016-4	0.000	4.678	0	3747322	N.D.	33.871 #
7)	L1 AR-1016-5	5.990	4.882	523681	3031683	15.272	19.944 #
8)	L2 AR-1221-1	0.000	3.614	0	266993	N.D.	5.244 #
9)	L2 AR-1221-2	0.000	3.698	0	1601798	N.D.	43.134 #
10)	L2 AR-1221-3	0.000	3.768	0	110598	N.D.	0.903 #
11)	L3 AR-1232-1	0.000	3.768	0	110598	N.D.	0.945 #
12)	L3 AR-1232-2	0.000	4.469	0	115424	N.D.	0.835 #
14)	L3 AR-1232-4	0.000	4.716	0	1192765	N.D.	19.989 #
15)	L3 AR-1232-5	5.788	4.882	769891	3031683	65.827	44.424 #
16)	L4 AR-1242-1	0.000	4.458	0	543887	N.D.	3.712 #
17)	L4 AR-1242-2	0.000	4.469	0	115424	N.D.	0.506 #
19)	L4 AR-1242-4	0.000	4.716	0	1192765	N.D.	10.852 #
20)	L4 AR-1242-5	6.431	5.225	937427	12759394	29.132	77.003 #
21)	L5 AR-1248-1	0.000	4.458	0	543887	N.D.	5.403 #
22)	L5 AR-1248-2	5.788	4.678	769891	3747322	21.988	27.458
23)	L5 AR-1248-3	5.990	4.716	523681	1192765	12.801	8.521 #
24)	L5 AR-1248-4	6.392	4.882	924118	3031683	18.877	17.035
25)	L5 AR-1248-5	6.431	5.248	937427	8869497	19.845	45.342 #
26)	L6 AR-1254-1	6.365	5.225	3148971	12759394	57.641	37.040 #
27)	L6 AR-1254-2	6.581	5.370	2620733	12983013	30.581	43.349 #
28)	L6 AR-1254-3	6.947	5.761	2953522	16854185	32.469	35.586
29)	L6 AR-1254-4	7.230	5.986	1984940	9009729	29.622	25.695
30)	L6 AR-1254-5	7.646	6.394	2121690	31022116	29.517	70.055 #
31)	L7 AR-1260-1	7.106	5.887	1610144	5357457	24.401	18.330
32)	L7 AR-1260-2	7.362	6.071	1439001	11238327	18.054	24.400 #
33)	L7 AR-1260-3	0.000	6.220	0	5792854	N.D.	16.249 #
34)	L7 AR-1260-4	7.936	6.687	1202991	1920685	16.168	6.302 #
35)	L7 AR-1260-5	8.254	6.926	531947	1290322	3.678	1.488 #
36)	L8 AR-1262-1	0.000	6.493	0	7762299	N.D.	30.972 #
37)	L8 AR-1262-2	8.254	6.926	531947	1290322	2.737	1.027 #
38)	L8 AR-1262-3	8.579	7.263	665293	63267791	5.059	115.396 #
39)	L8 AR-1262-4	0.000	7.263	0	63267791	N.D.	70.482 #
40)	L8 AR-1262-5	0.000	7.759	0	1257109	N.D.	3.286 #
41)	L9 AR-1268-1	8.579	7.263	665293	63267791	3.715	51.394 #
42)	L9 AR-1268-2	0.000	7.263	0	63267791	N.D.	59.747 #
43)	L9 AR-1268-3	0.000	7.460	0	22982359	N.D.	25.932 #
44)	L9 AR-1268-4	0.000	7.759	0	1257109	N.D.	3.465 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
Data File : PR037331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 18:50
Operator : SM\SJ
Sample : K1560-03
Misc : AR1254 MDL 25PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 22:02:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	0.000	8.025	0	44485331	N.D.	17.485 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
Data File : PR037331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 18:50
Operator : SM\SJ
Sample : K1560-03
Misc : AR1254 MDL 25PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 22:02:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

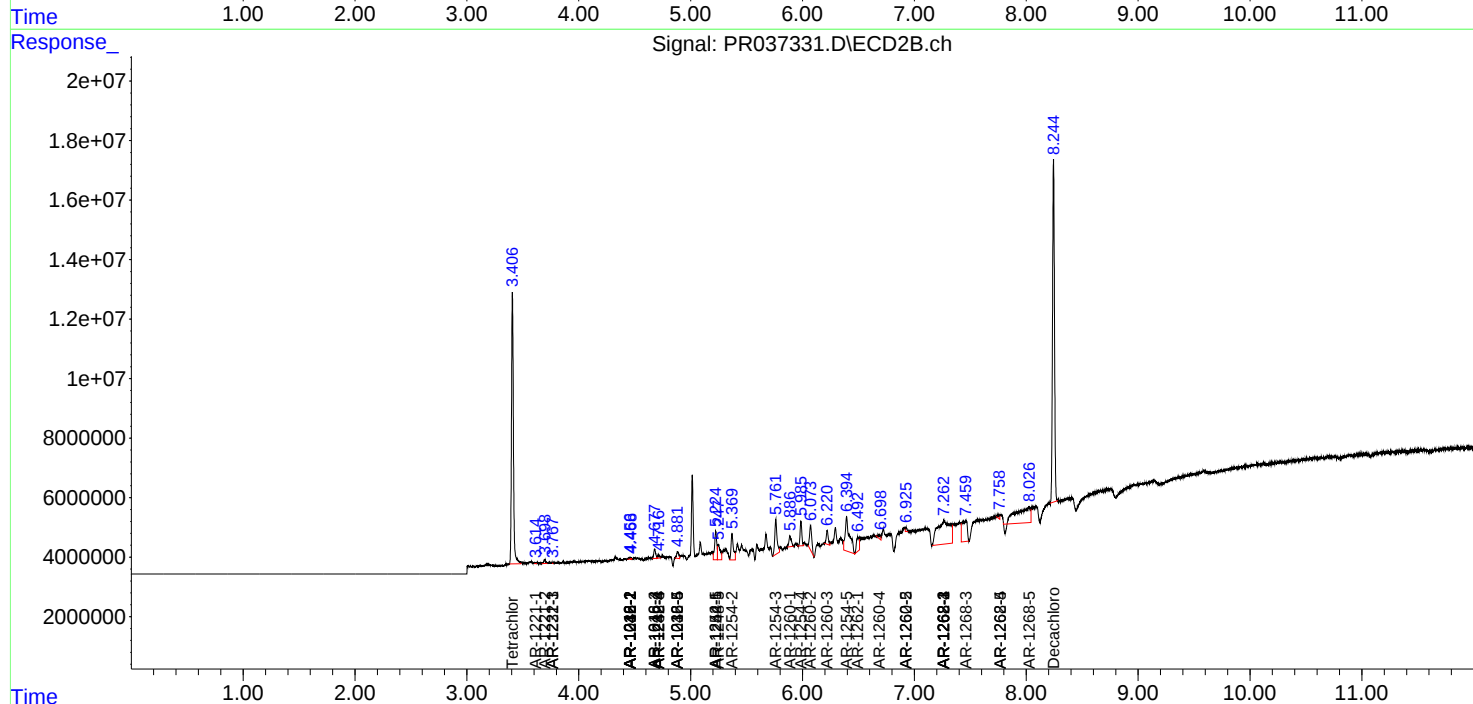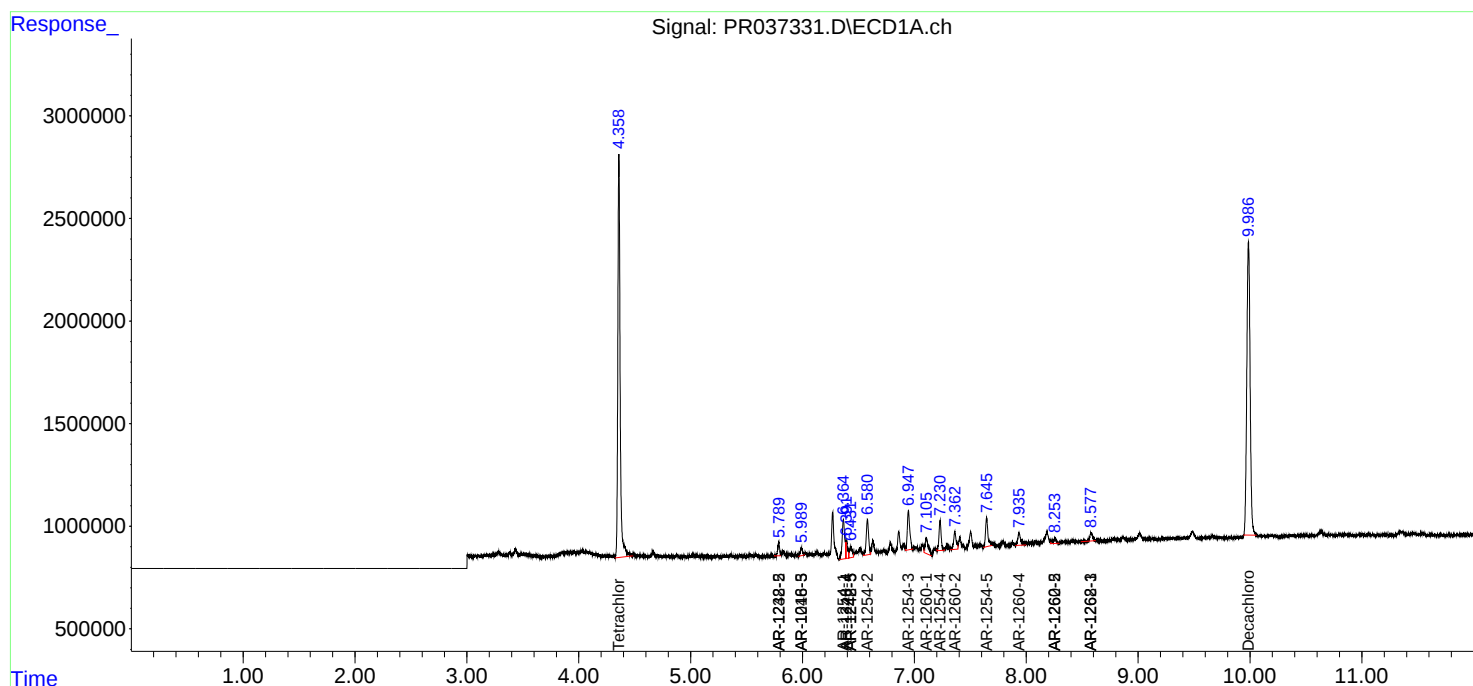


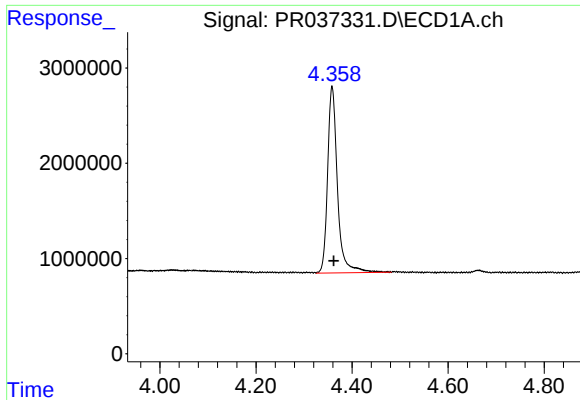

#1 Tetrachloro-m-xylene


R.T.: 4.359 min
Delta R.T.: -0.003 min
Response: 28033657
Conc: 22.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

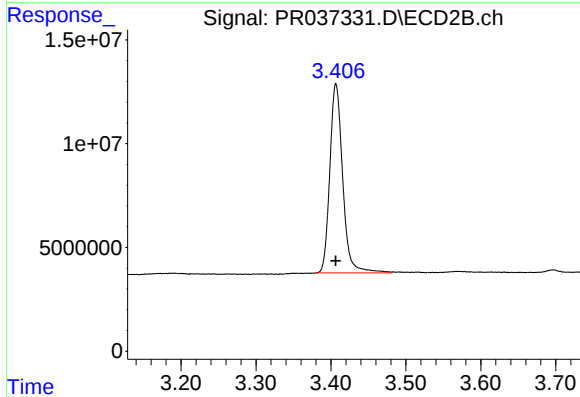


#1 Tetrachloro-m-xylene

R.T.: 3.407 min
Delta R.T.: 0.000 min
Response: 108845892
Conc: 22.70 ng/ml

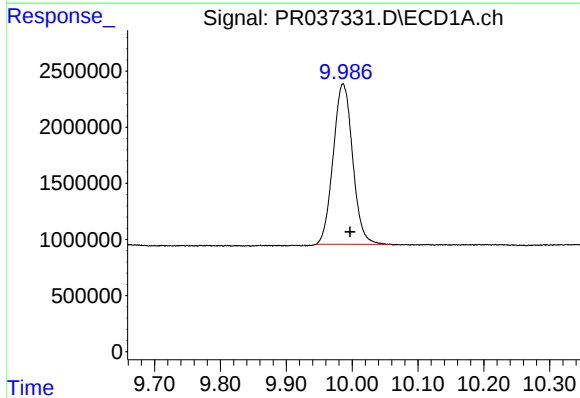


#2 Decachlorobiphenyl

R.T.: 9.986 min
Delta R.T.: -0.011 min
Response: 29342580
Conc: 22.19 ng/ml

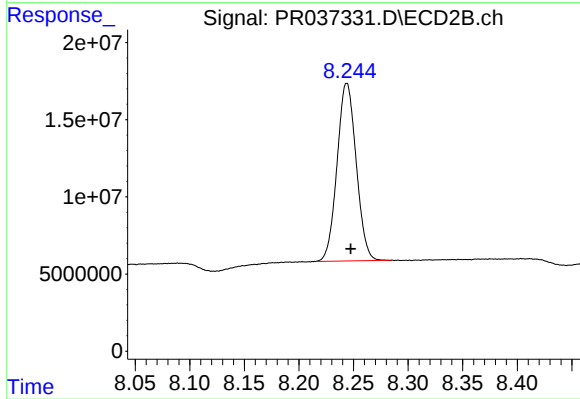

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 140405695
Conc: 24.11 ng/ml

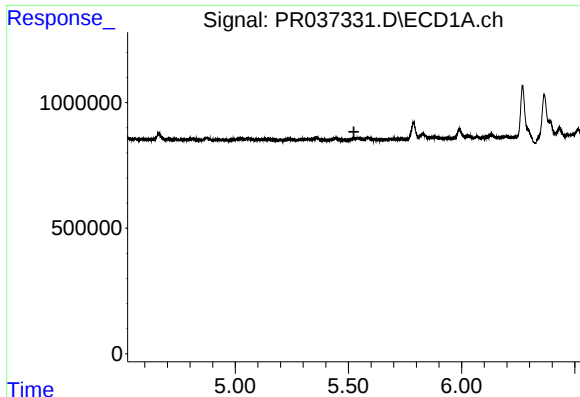

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

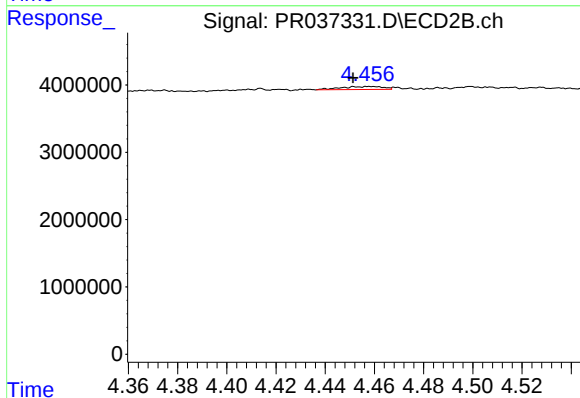


#3 AR-1016-1

R.T.: 4.458 min
Delta R.T.: 0.006 min
Response: 543887
Conc: 2.99 ng/ml

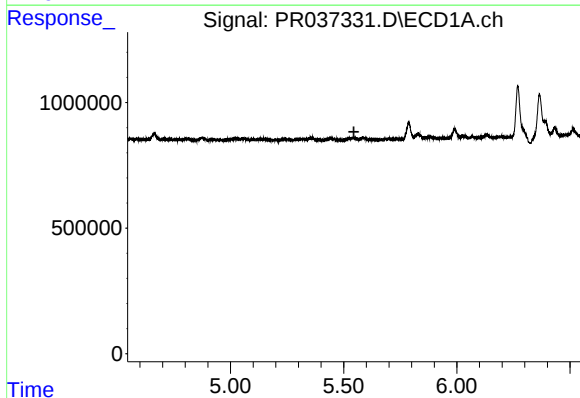


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

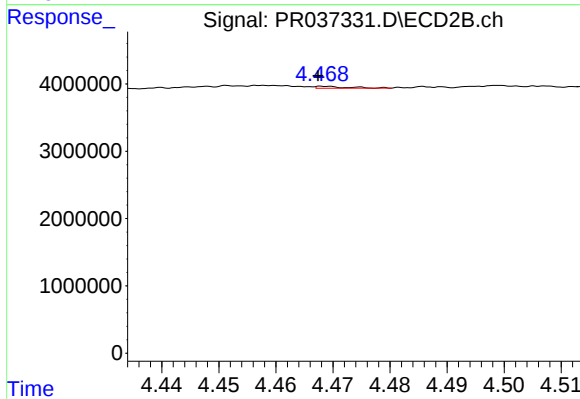

#4 AR-1016-2


R.T.: 4.469 min
Delta R.T.: 0.001 min
Response: 115424
Conc: 0.41 ng/ml

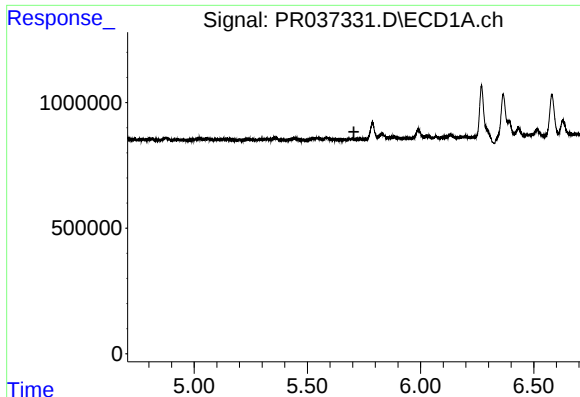

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

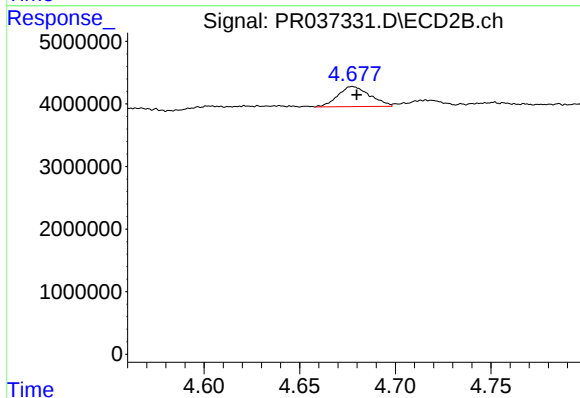


#6 AR-1016-4

R.T.: 4.678 min
Delta R.T.: -0.002 min
Response: 3747322
Conc: 33.87 ng/ml

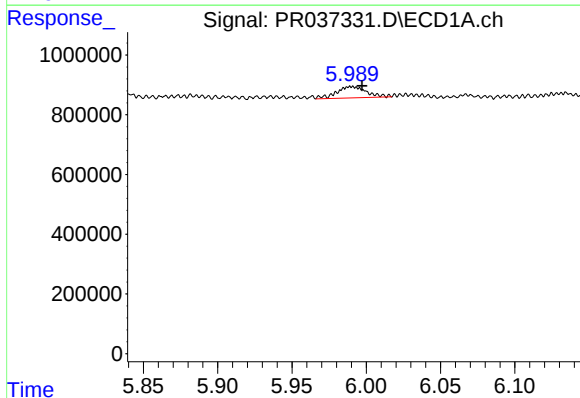


#7 AR-1016-5

R.T.: 5.990 min
Delta R.T.: -0.008 min
Response: 523681
Conc: 15.27 ng/ml

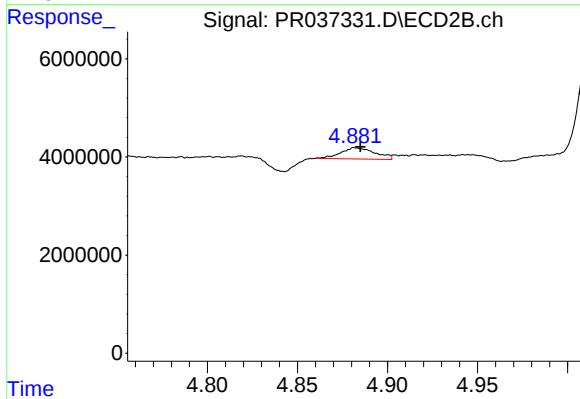

#7 AR-1016-5


R.T.: 4.882 min
Delta R.T.: -0.003 min
Response: 3031683
Conc: 19.94 ng/ml

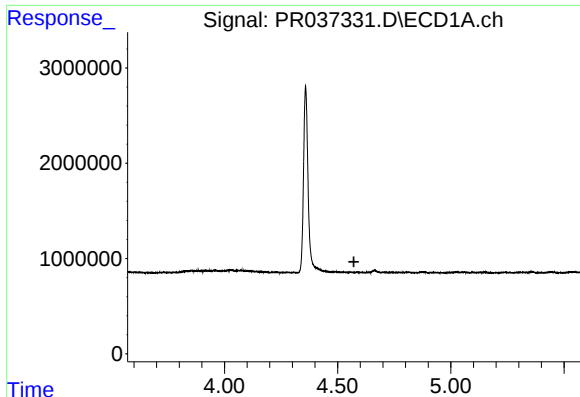

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

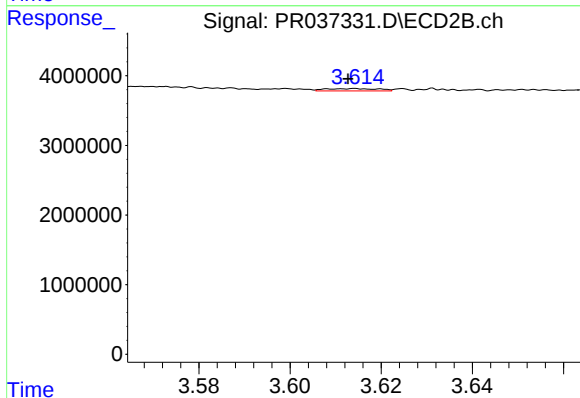


#8 AR-1221-1

R.T.: 3.614 min
Delta R.T.: 0.002 min
Response: 266993
Conc: 5.24 ng/ml

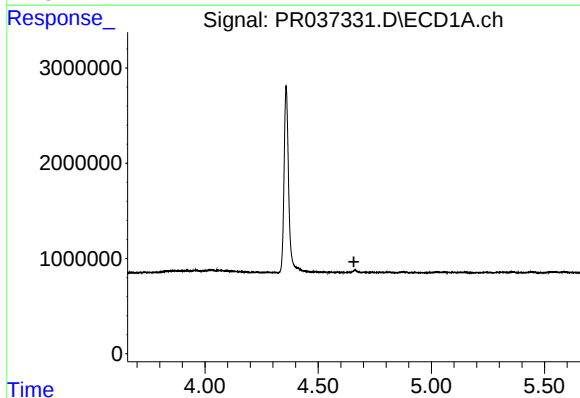


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.658 min
Response: 0
Conc: N.D.

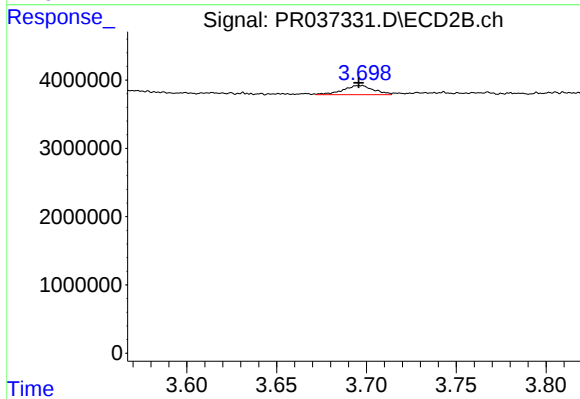

#9 AR-1221-2


R.T.: 3.698 min
Delta R.T.: 0.002 min
Response: 1601798
Conc: 43.13 ng/ml

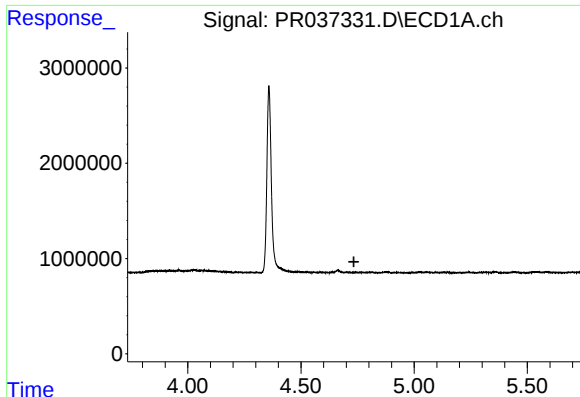

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

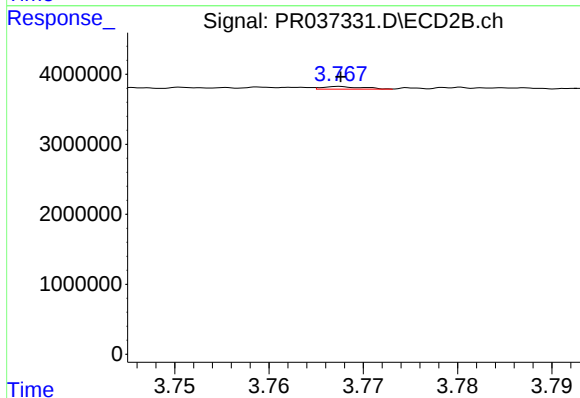


#10 AR-1221-3

R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 110598
Conc: 0.90 ng/ml

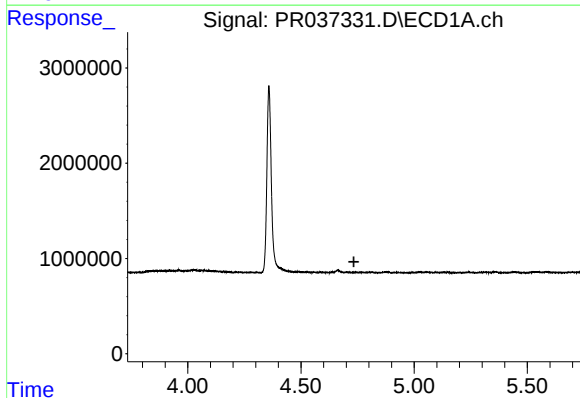


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

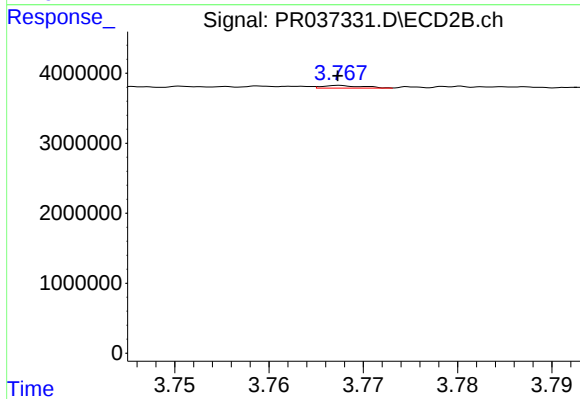

#11 AR-1232-1


R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 110598
Conc: 0.95 ng/ml

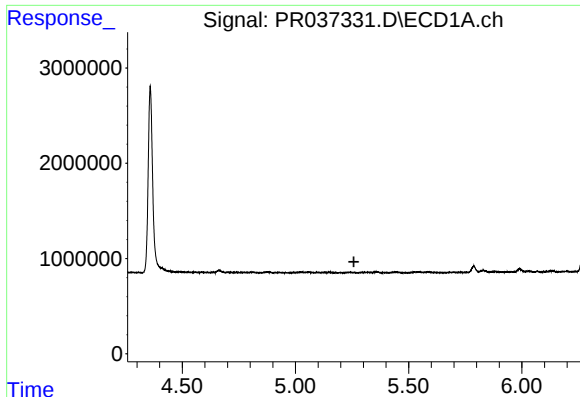

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

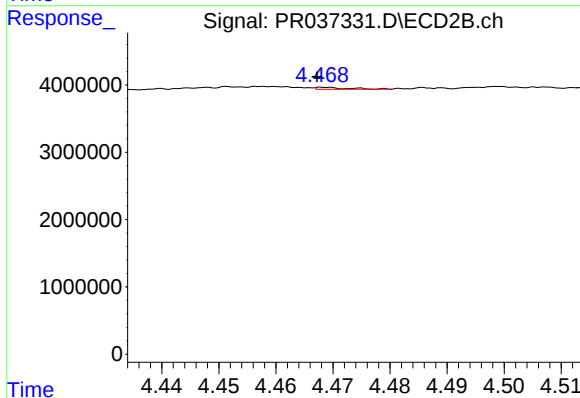


#12 AR-1232-2

R.T.: 4.469 min
Delta R.T.: 0.001 min
Response: 115424
Conc: 0.84 ng/ml

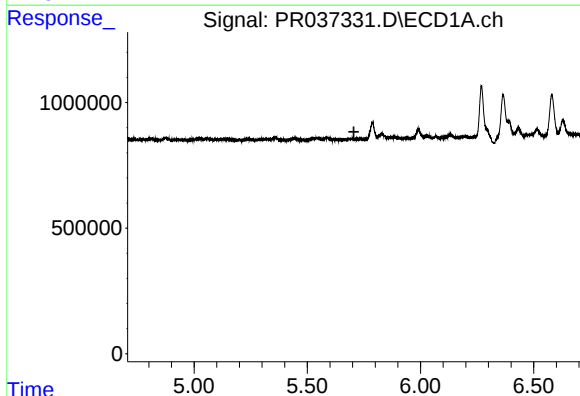


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

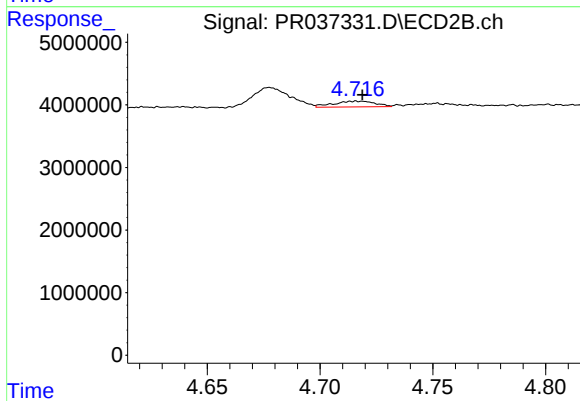

#14 AR-1232-4


R.T.: 4.716 min
Delta R.T.: -0.003 min
Response: 1192765
Conc: 19.99 ng/ml

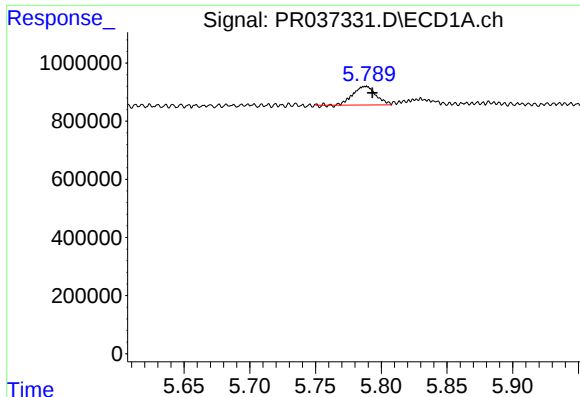

#15 AR-1232-5


R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 769891
Conc: 65.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

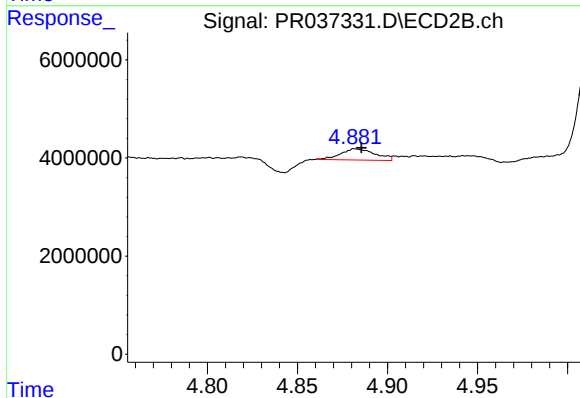


#15 AR-1232-5

R.T.: 4.882 min
Delta R.T.: -0.004 min
Response: 3031683
Conc: 44.42 ng/ml

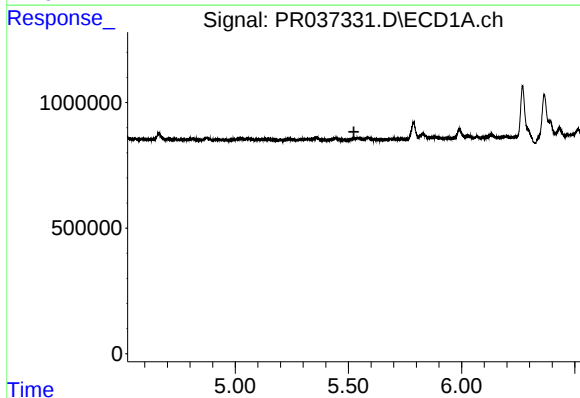


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

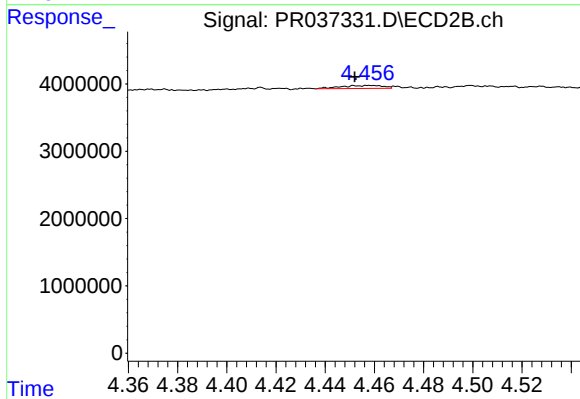

#16 AR-1242-1


R.T.: 4.458 min
Delta R.T.: 0.006 min
Response: 543887
Conc: 3.71 ng/ml

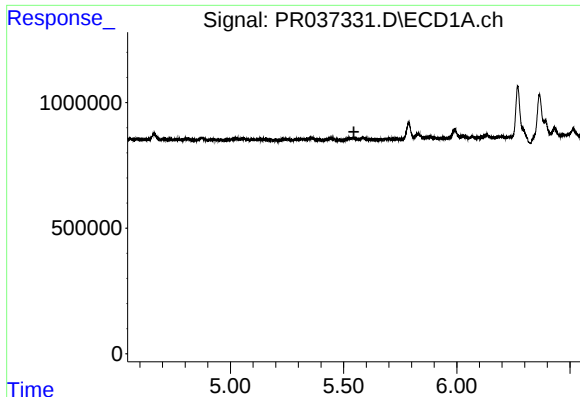

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

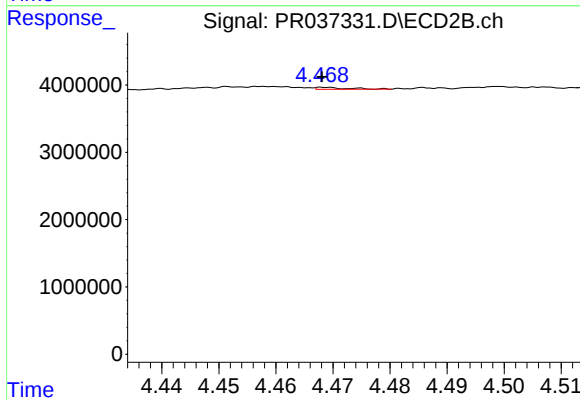


#17 AR-1242-2

R.T.: 4.469 min
Delta R.T.: 0.000 min
Response: 115424
Conc: 0.51 ng/ml

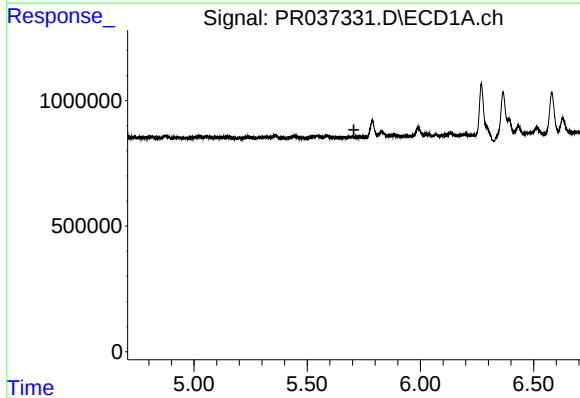


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

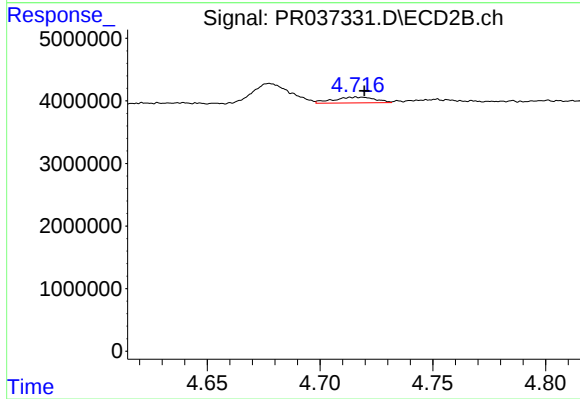

#19 AR-1242-4


R.T.: 4.716 min
Delta R.T.: -0.004 min
Response: 1192765
Conc: 10.85 ng/ml

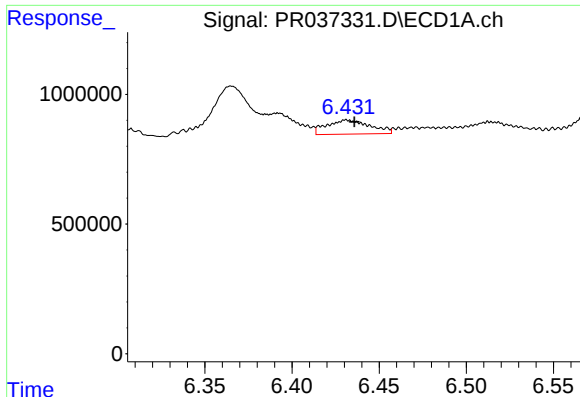

#20 AR-1242-5


R.T.: 6.431 min
Delta R.T.: -0.005 min
Response: 937427
Conc: 29.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

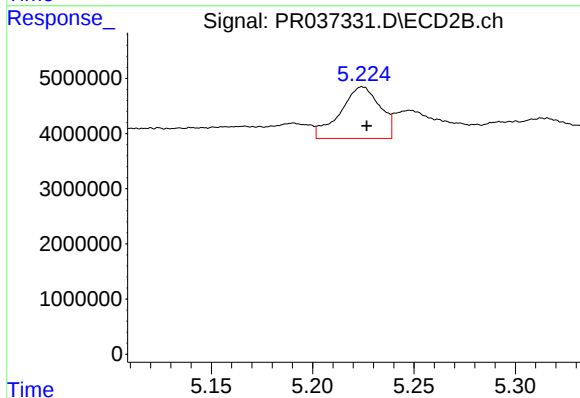


#20 AR-1242-5

R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 12759394
Conc: 77.00 ng/ml

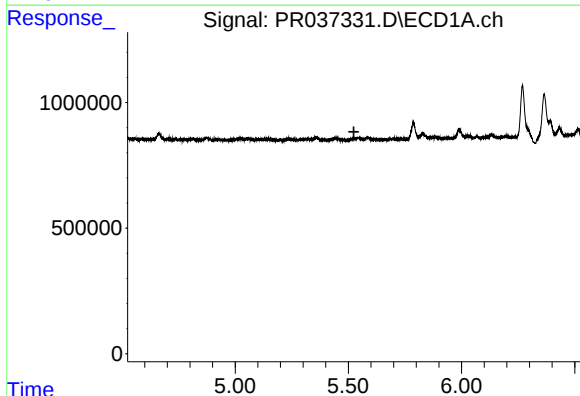


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.525 min
Response: 0
Conc: N.D.

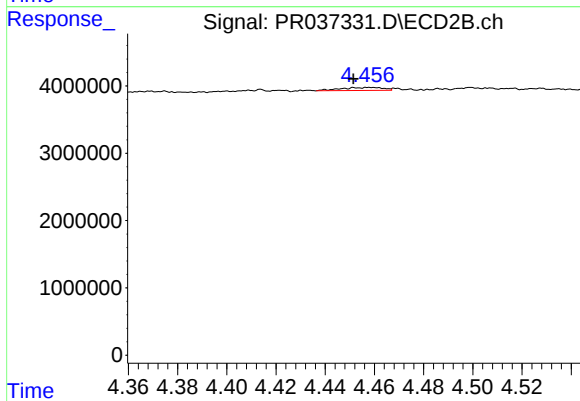

#21 AR-1248-1


R.T.: 4.458 min
Delta R.T.: 0.006 min
Response: 543887
Conc: 5.40 ng/ml

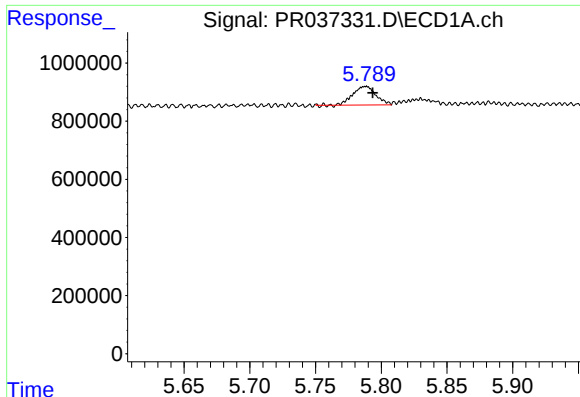

#22 AR-1248-2


R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 769891
Conc: 21.99 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

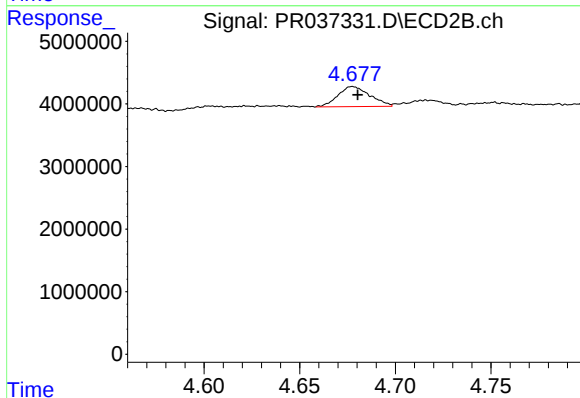


#22 AR-1248-2

R.T.: 4.678 min
Delta R.T.: -0.003 min
Response: 3747322
Conc: 27.46 ng/ml

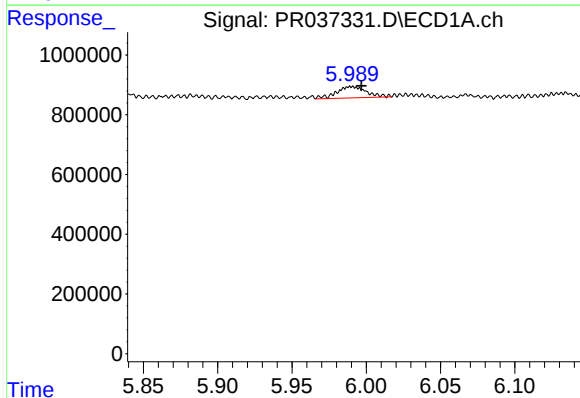


#23 AR-1248-3

R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 523681
Conc: 12.80 ng/ml

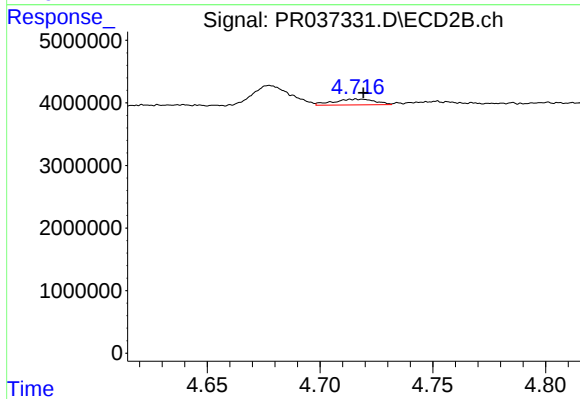

#23 AR-1248-3


R.T.: 4.716 min
Delta R.T.: -0.003 min
Response: 1192765
Conc: 8.52 ng/ml

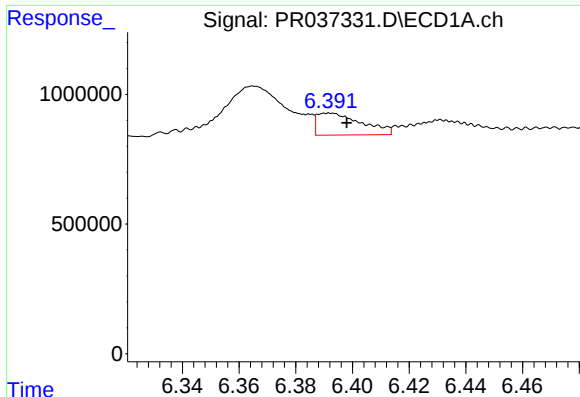

#24 AR-1248-4


R.T.: 6.392 min
Delta R.T.: -0.006 min
Response: 924118
Conc: 18.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

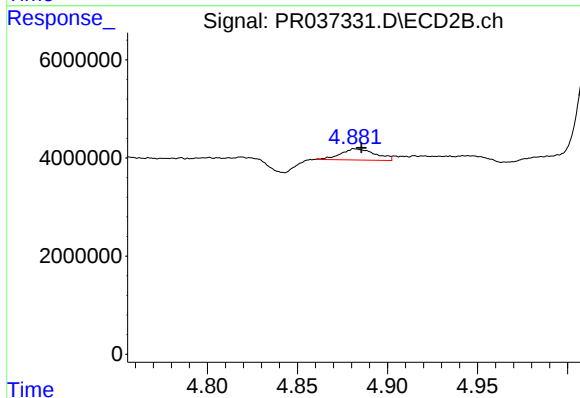


#24 AR-1248-4

R.T.: 4.882 min
Delta R.T.: -0.004 min
Response: 3031683
Conc: 17.04 ng/ml

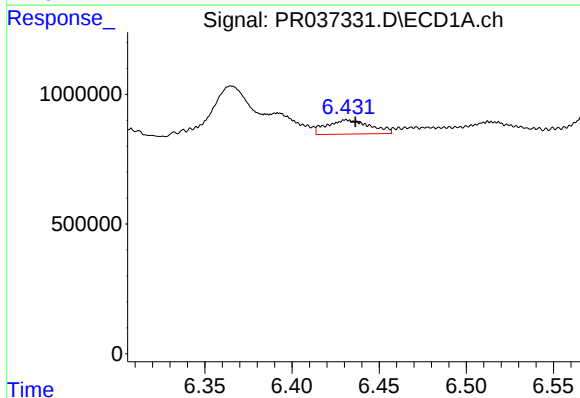


#25 AR-1248-5

R.T.: 6.431 min
Delta R.T.: -0.005 min
Response: 937427
Conc: 19.85 ng/ml

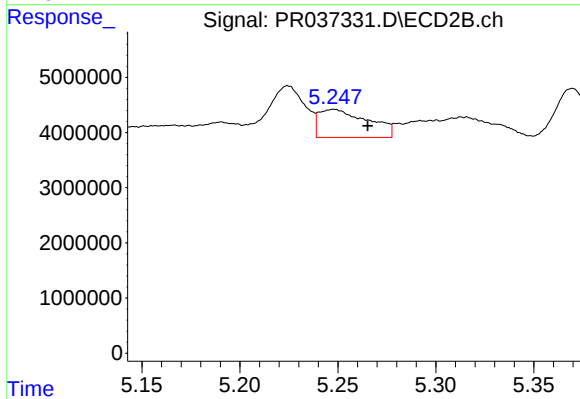

#25 AR-1248-5


R.T.: 5.248 min
Delta R.T.: -0.017 min
Response: 8869497
Conc: 45.34 ng/ml

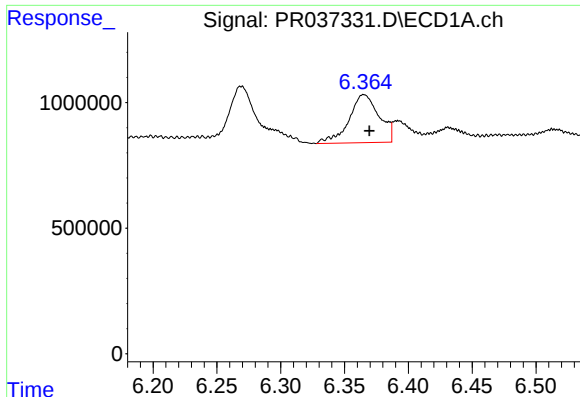

#26 AR-1254-1


R.T.: 6.365 min
Delta R.T.: -0.004 min
Response: 3148971
Conc: 57.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

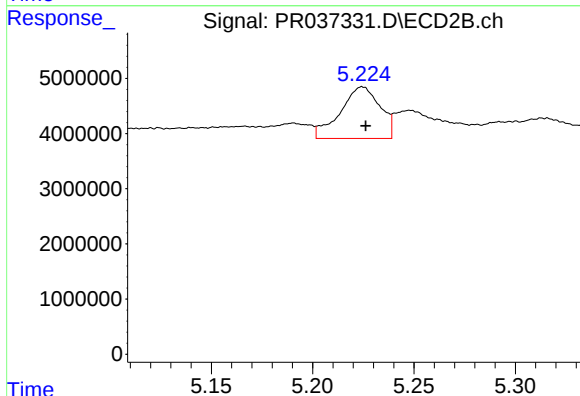


#26 AR-1254-1

R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 12759394
Conc: 37.04 ng/ml

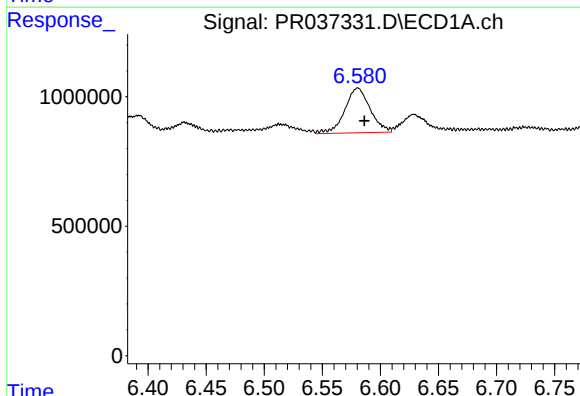


#27 AR-1254-2

R.T.: 6.581 min
Delta R.T.: -0.006 min
Response: 2620733
Conc: 30.58 ng/ml

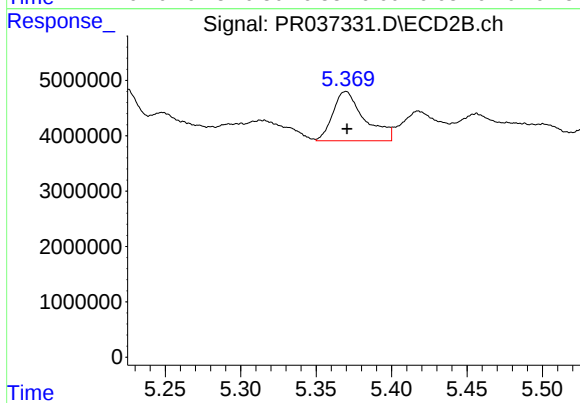

#27 AR-1254-2


R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 12983013
Conc: 43.35 ng/ml

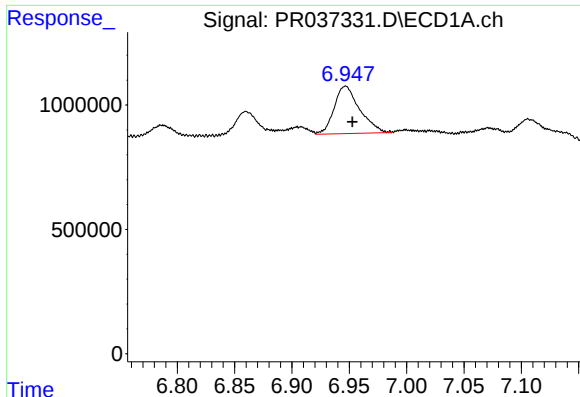

#28 AR-1254-3


R.T.: 6.947 min
Delta R.T.: -0.006 min
Response: 2953522
Conc: 32.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

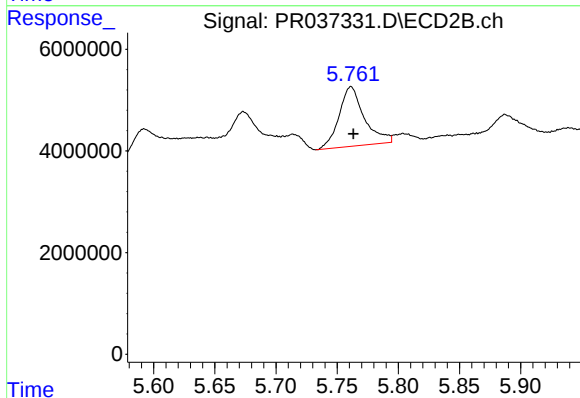


#28 AR-1254-3

R.T.: 5.761 min
Delta R.T.: -0.002 min
Response: 16854185
Conc: 35.59 ng/ml

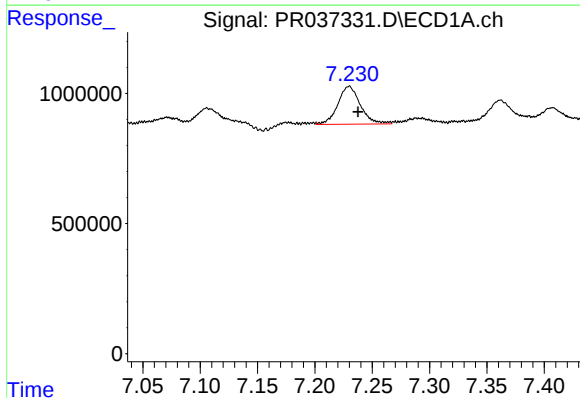


#29 AR-1254-4

R.T.: 7.230 min
Delta R.T.: -0.008 min
Response: 1984940
Conc: 29.62 ng/ml

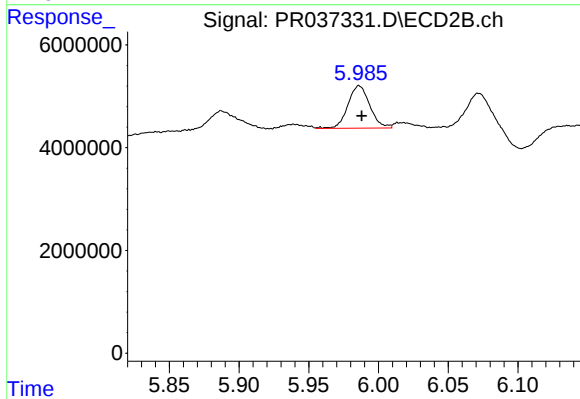

#29 AR-1254-4


R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 9009729
Conc: 25.69 ng/ml

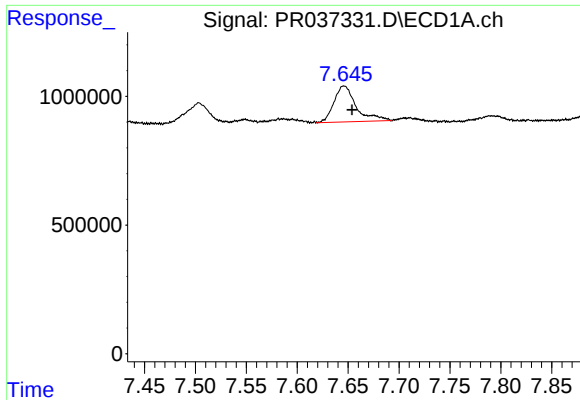

#30 AR-1254-5


R.T.: 7.646 min
Delta R.T.: -0.008 min
Response: 2121690
Conc: 29.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

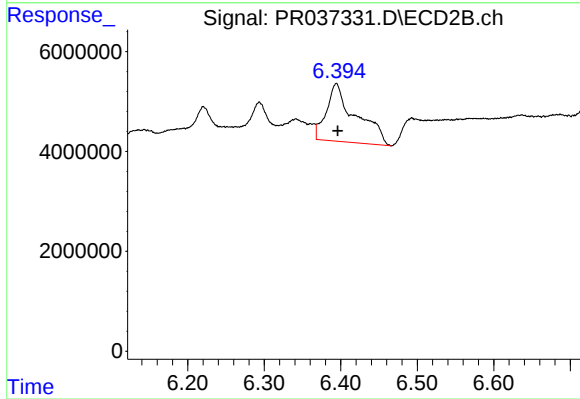


#30 AR-1254-5

R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 31022116
Conc: 70.05 ng/ml

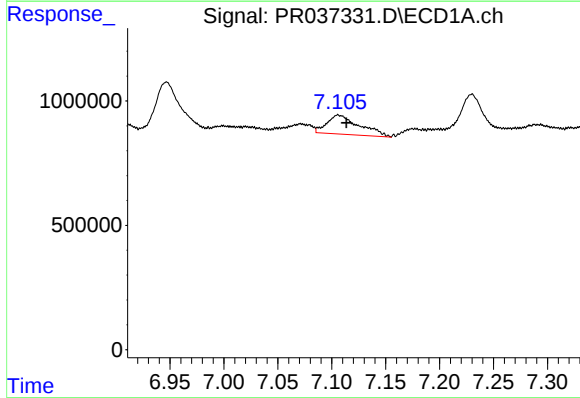


#31 AR-1260-1

R.T.: 7.106 min
Delta R.T.: -0.008 min
Response: 1610144
Conc: 24.40 ng/ml

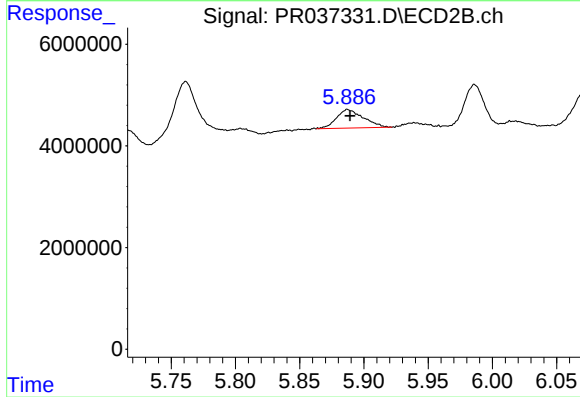

#31 AR-1260-1


R.T.: 5.887 min
Delta R.T.: -0.002 min
Response: 5357457
Conc: 18.33 ng/ml

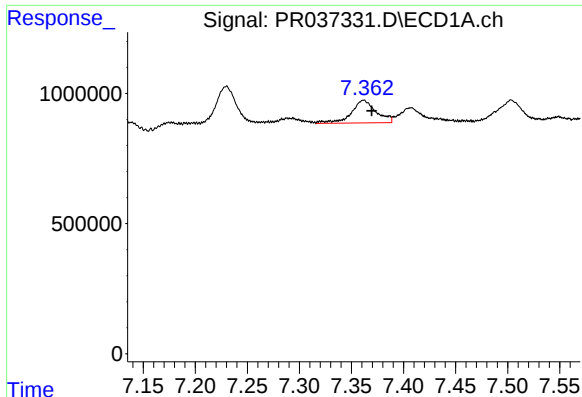

#32 AR-1260-2


R.T.: 7.362 min
Delta R.T.: -0.008 min
Response: 1439001
Conc: 18.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

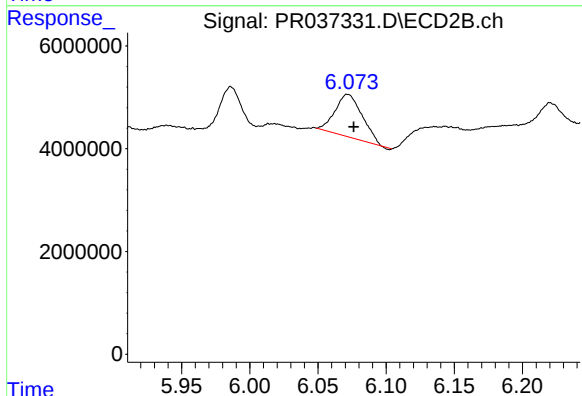


#32 AR-1260-2

R.T.: 6.071 min
Delta R.T.: -0.005 min
Response: 11238327
Conc: 24.40 ng/ml

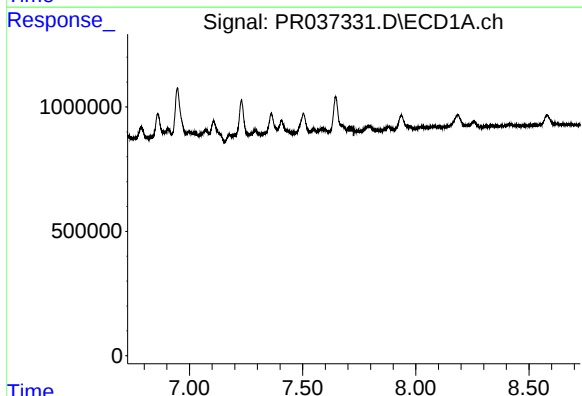


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.726 min
Response: 0
Conc: N.D.

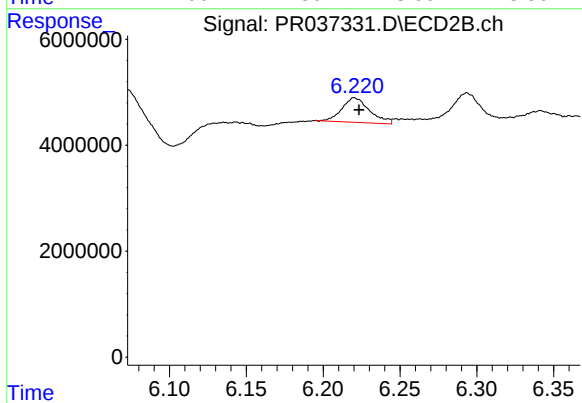

#33 AR-1260-3


R.T.: 6.220 min
Delta R.T.: -0.003 min
Response: 5792854
Conc: 16.25 ng/ml

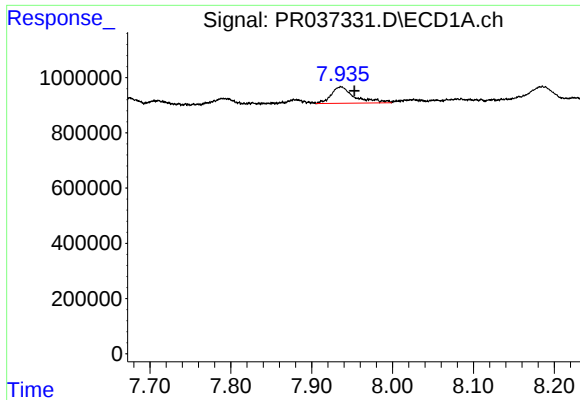

#34 AR-1260-4


R.T.: 7.936 min
Delta R.T.: -0.017 min
Response: 1202991
Conc: 16.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

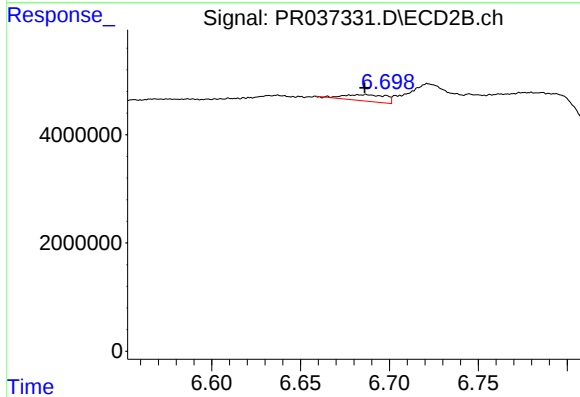


#34 AR-1260-4

R.T.: 6.687 min
Delta R.T.: 0.000 min
Response: 1920685
Conc: 6.30 ng/ml

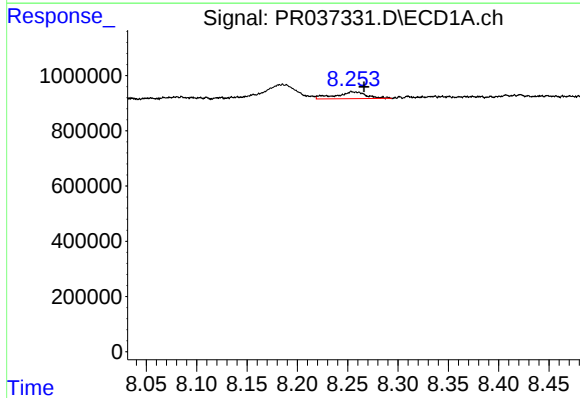


#35 AR-1260-5

R.T.: 8.254 min
Delta R.T.: -0.012 min
Response: 531947
Conc: 3.68 ng/ml

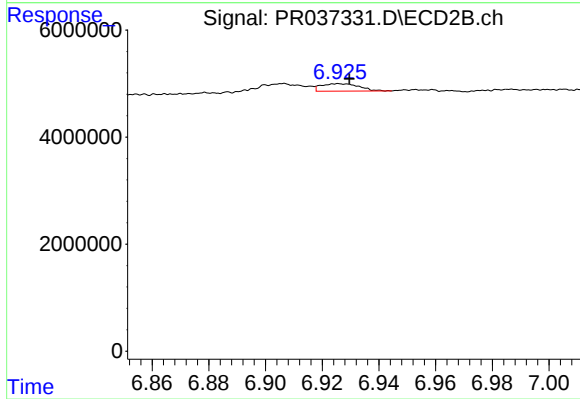

#35 AR-1260-5


R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 1290322
Conc: 1.49 ng/ml

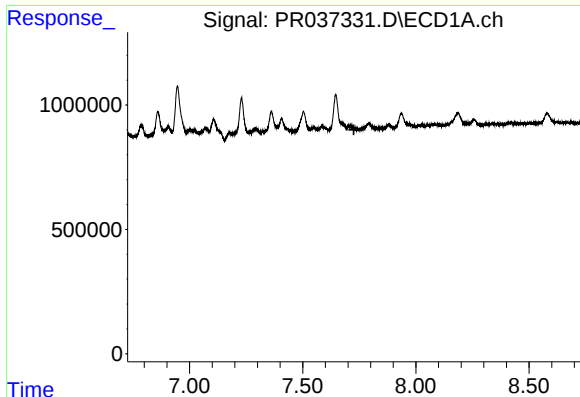

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

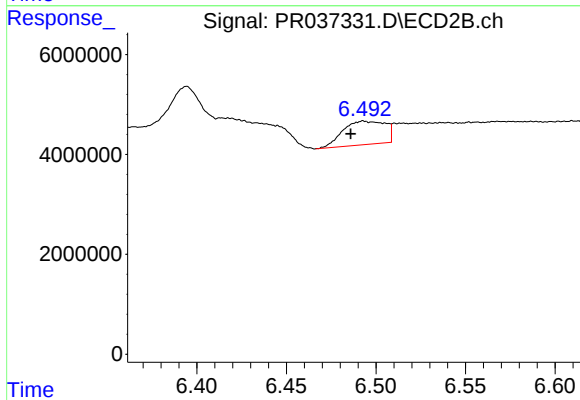


#36 AR-1262-1

R.T.: 6.493 min
Delta R.T.: 0.007 min
Response: 7762299
Conc: 30.97 ng/ml

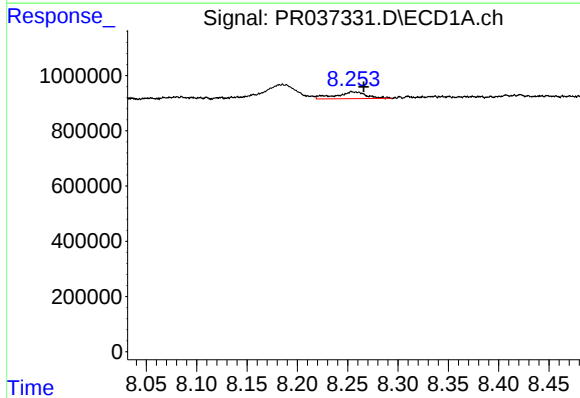


#37 AR-1262-2

R.T.: 8.254 min
Delta R.T.: -0.012 min
Response: 531947
Conc: 2.74 ng/ml

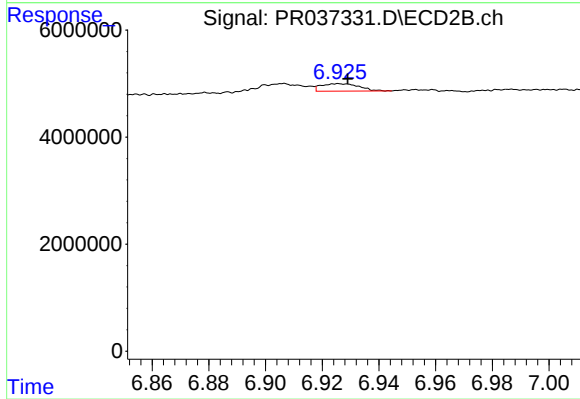

#37 AR-1262-2


R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 1290322
Conc: 1.03 ng/ml

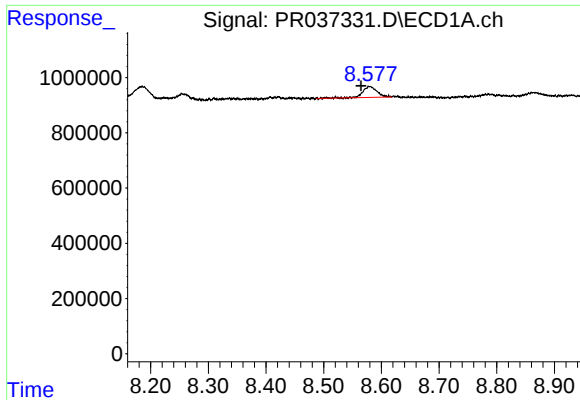

#38 AR-1262-3


R.T.: 8.579 min
Delta R.T.: 0.014 min
Response: 665293
Conc: 5.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

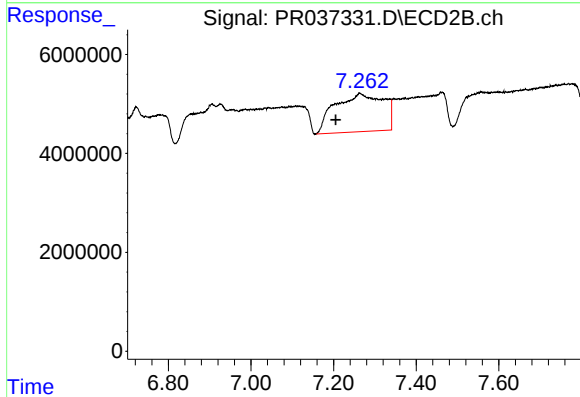


#38 AR-1262-3

R.T.: 7.263 min
Delta R.T.: 0.058 min
Response: 63267791
Conc: 115.40 ng/ml

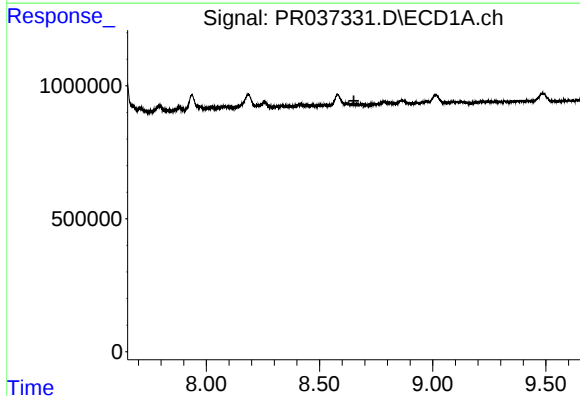


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.652 min
Response: 0
Conc: N.D.

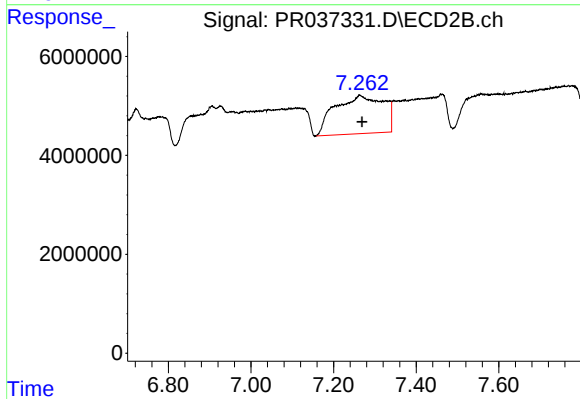

#39 AR-1262-4


R.T.: 7.263 min
Delta R.T.: -0.006 min
Response: 63267791
Conc: 70.48 ng/ml

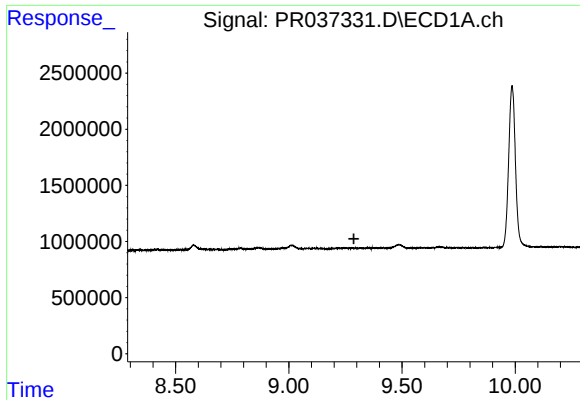

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

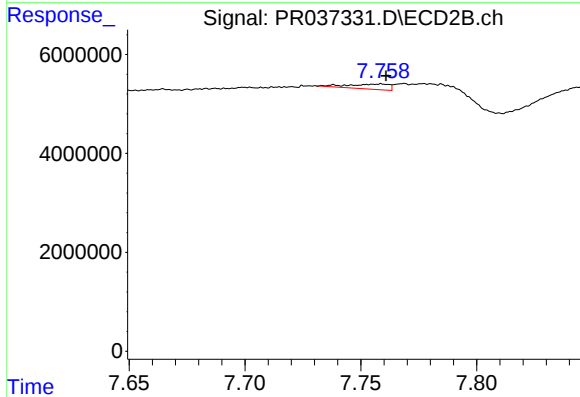


#40 AR-1262-5

R.T.: 7.759 min
Delta R.T.: -0.002 min
Response: 1257109
Conc: 3.29 ng/ml

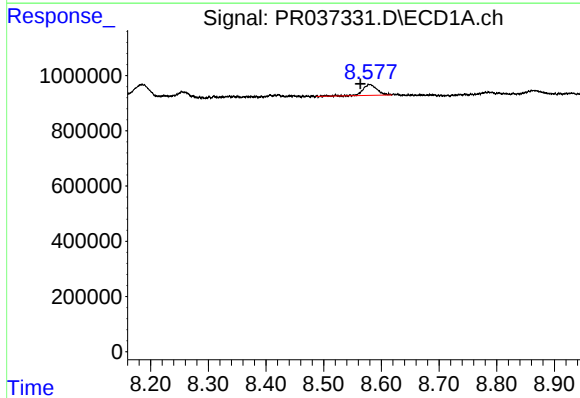


#41 AR-1268-1

R.T.: 8.579 min
Delta R.T.: 0.015 min
Response: 665293
Conc: 3.71 ng/ml

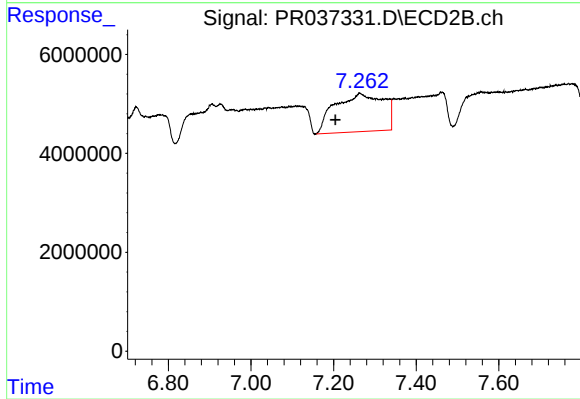

#41 AR-1268-1


R.T.: 7.263 min
Delta R.T.: 0.058 min
Response: 63267791
Conc: 51.39 ng/ml

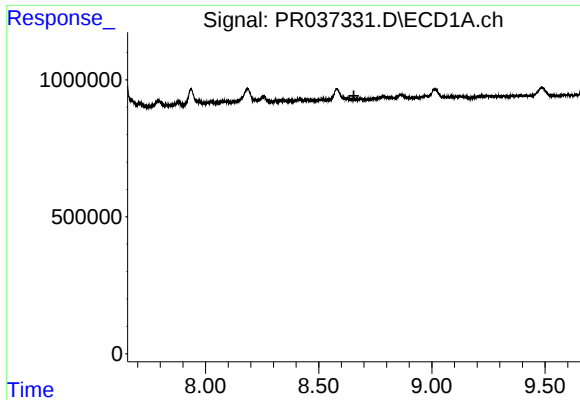

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

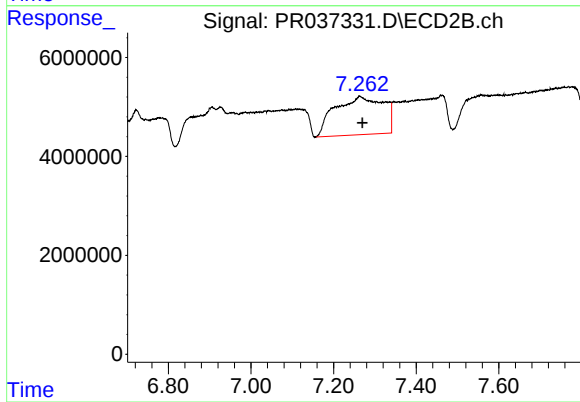


#42 AR-1268-2

R.T.: 7.263 min
Delta R.T.: -0.007 min
Response: 63267791
Conc: 59.75 ng/ml

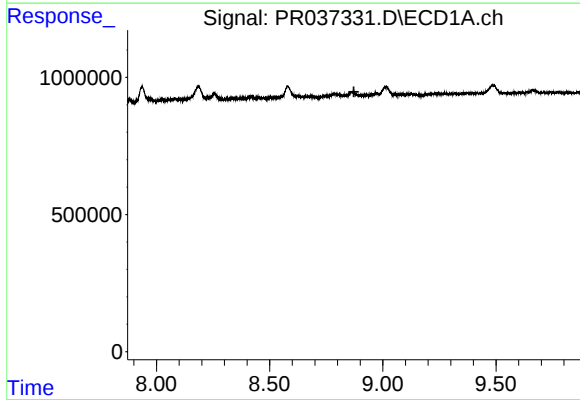


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

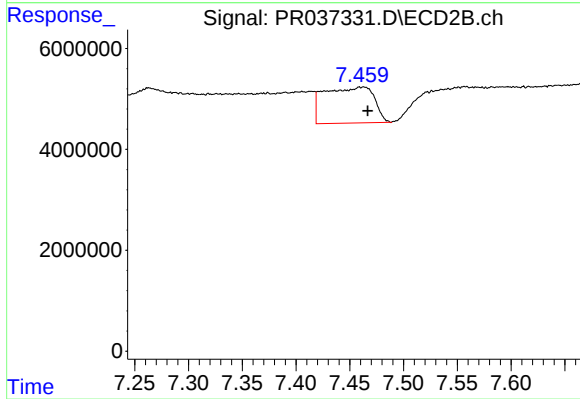

#43 AR-1268-3


R.T.: 7.460 min
Delta R.T.: -0.007 min
Response: 22982359
Conc: 25.93 ng/ml

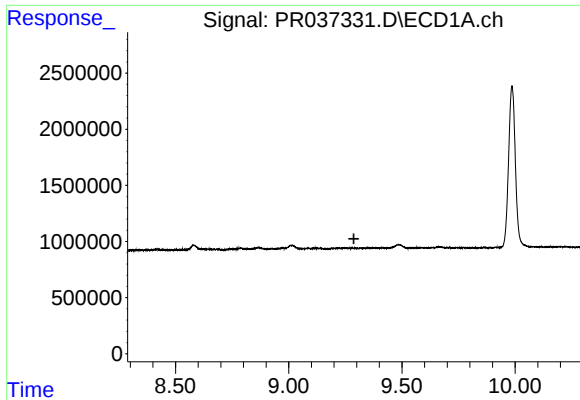

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.288 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

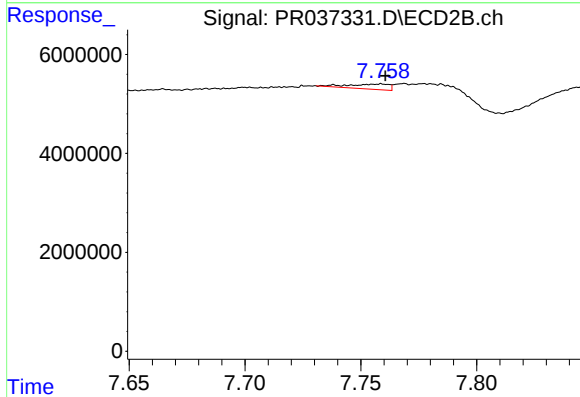


#44 AR-1268-4

R.T.: 7.759 min
Delta R.T.: -0.002 min
Response: 1257109
Conc: 3.47 ng/ml

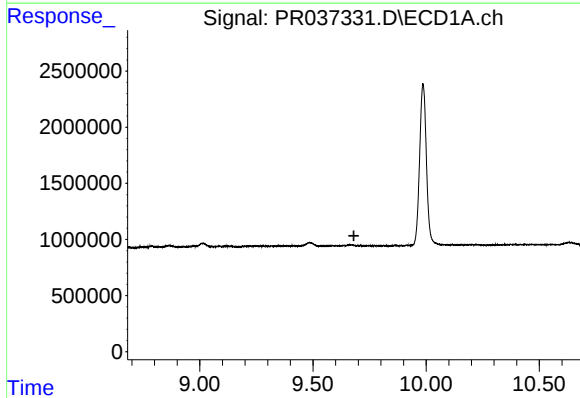

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.681 min
Response: 0
Conc: N.D.

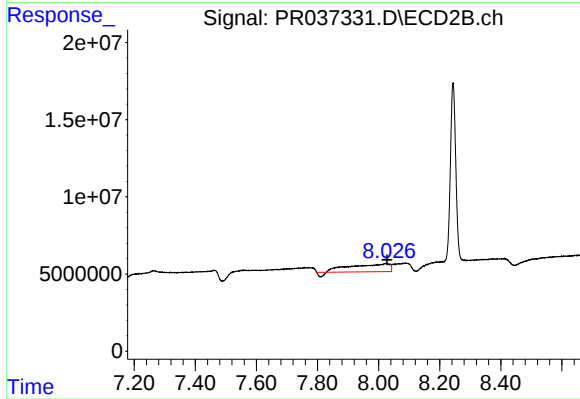

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.002 min
Response: 44485331
Conc: 17.49 ng/ml