

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 19:04
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1262 MDL 25PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 22:03:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.409	30011407	118.9E6	23.990	24.786
2)	SA Decachlor...	9.986	8.244	32788644	159.5E6	24.791	27.379
Target Compounds							
3)	L1 AR-1016-1	0.000	4.454	0	887178	N.D.	4.872 #
4)	L1 AR-1016-2	0.000	4.454	0	887178	N.D.	3.145 #
5)	L1 AR-1016-3	0.000	4.638	0	301518	N.D.	2.097 #
6)	L1 AR-1016-4	0.000	4.681	0	296242	N.D.	2.678 #
7)	L1 AR-1016-5	0.000	4.886	0	477988	N.D.	3.144 #
8)	L2 AR-1221-1	0.000	3.608	0	1479138	N.D.	29.049 #
9)	L2 AR-1221-2	4.664	3.698	511234	3357661	56.528	90.416 #
10)	L2 AR-1221-3	4.664	3.749	511234	800300	16.680	6.536 #
11)	L3 AR-1232-1	4.664	3.749	511234	800300	17.477	6.841 #
12)	L3 AR-1232-2	0.000	4.454	0	887178	N.D.	6.418 #
13)	L3 AR-1232-3	0.000	4.638	0	301518	N.D.	4.295 #
14)	L3 AR-1232-4	0.000	4.722	0	207687	N.D.	3.480 #
15)	L3 AR-1232-5	0.000	4.886	0	477988	N.D.	7.004 #
16)	L4 AR-1242-1	0.000	4.454	0	887178	N.D.	6.054 #
17)	L4 AR-1242-2	0.000	4.454	0	887178	N.D.	3.888 #
18)	L4 AR-1242-3	0.000	4.638	0	301518	N.D.	2.608 #
19)	L4 AR-1242-4	0.000	4.722	0	207687	N.D.	1.890 #
20)	L4 AR-1242-5	6.431	5.248	228254	17867262	7.093	107.829 #
21)	L5 AR-1248-1	0.000	4.454	0	887178	N.D.	8.813 #
22)	L5 AR-1248-2	0.000	4.681	0	296242	N.D.	2.171 #
23)	L5 AR-1248-3	0.000	4.722	0	207687	N.D.	1.484 #
24)	L5 AR-1248-4	6.368	4.886	2265035	477988	46.268	2.686 #
25)	L5 AR-1248-5	6.431	5.276	228254	2790989	4.832	14.268 #
26)	L6 AR-1254-1	6.368	5.248	2265035	17867262	41.461	51.868 #
27)	L6 AR-1254-2	6.578	5.371	568256	8213284	6.631	27.423 #
28)	L6 AR-1254-3	6.963	5.774	1399350	9223286	15.384	19.474 #
29)	L6 AR-1254-4	7.230	5.991	1115934	292312	16.654	0.834 #
30)	L6 AR-1254-5	7.643	6.393	1925039	12086148	26.781	27.293
31)	L7 AR-1260-1	7.107	5.887	2084127	8114616	31.584	27.763
32)	L7 AR-1260-2	7.361	6.073	2818657	16016980	35.364	34.775
33)	L7 AR-1260-3	7.718	6.222	2833863	11249159	45.287	31.555 #
34)	L7 AR-1260-4	7.945	6.683	3061761	14440963	41.150	47.384
35)	L7 AR-1260-5	8.257	6.926	4940749	31931351	34.163	36.819
36)	L8 AR-1262-1	7.718	6.485	2833863	10707793	27.131	42.725 #
37)	L8 AR-1262-2	8.257	6.926	4940749	31931351	25.417	25.424
38)	L8 AR-1262-3	8.556	7.202	3869779	25014927	29.426	45.626 #
39)	L8 AR-1262-4	8.645	7.266	2757005	46947842	28.067	52.301 #
40)	L8 AR-1262-5	9.277	7.758	2017193	10837051	29.218	28.323
41)	L9 AR-1268-1	8.556	7.202	3869779	25014927	21.608	20.320

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
 Data File : PR037332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 19:04
 Operator : SM\SJ
 Sample : K1560-03
 Misc : AR1262 MDL 25PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 22:03:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.645	7.266	2757005	46947842	16.760	44.336 #
43) L9	AR-1268-3	0.000	7.463	0	13168502	N.D.	14.859 #
44) L9	AR-1268-4	9.277	7.758	2017193	10837051	32.334	29.872
45) L9	AR-1268-5	9.669	8.025	890164	9401705	1.953	3.695 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042319\
Data File : PR037332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 19:04
Operator : SM\SJ
Sample : K1560-03
Misc : AR1262 MDL 25PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 22:03:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

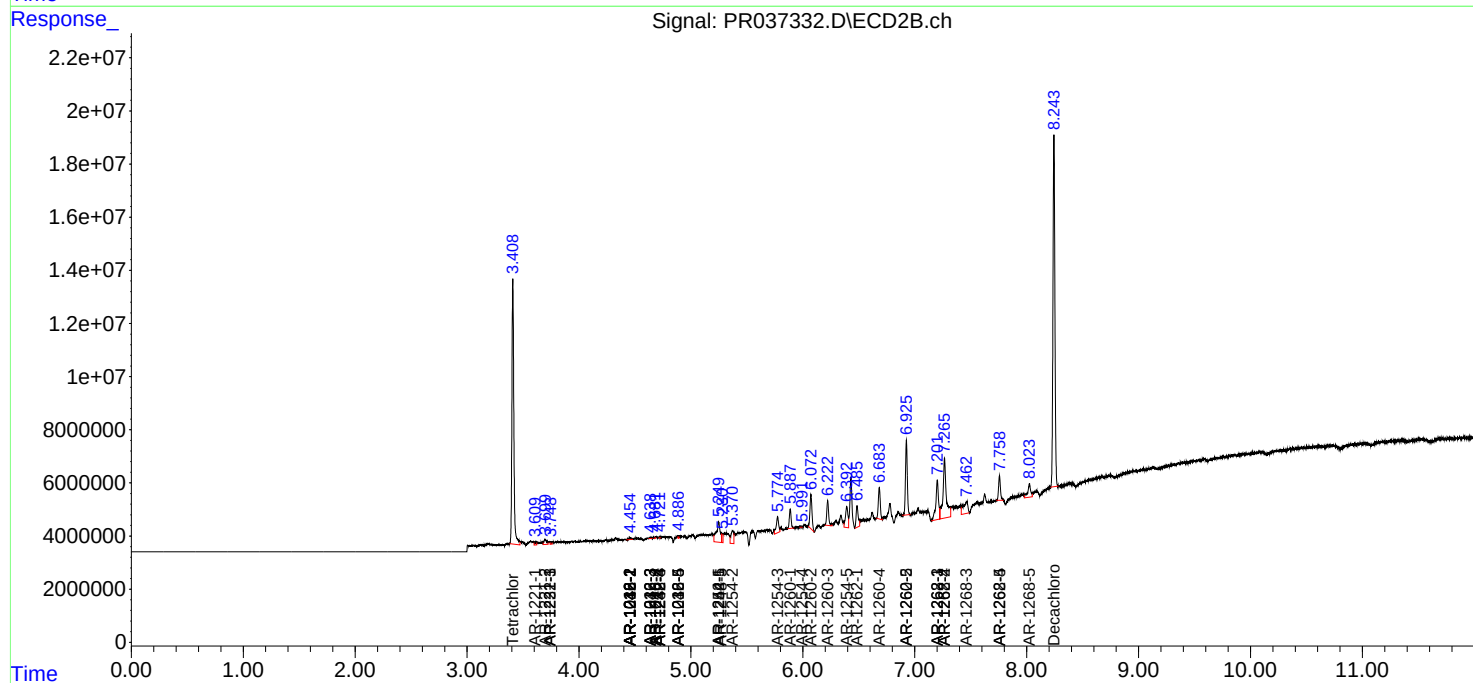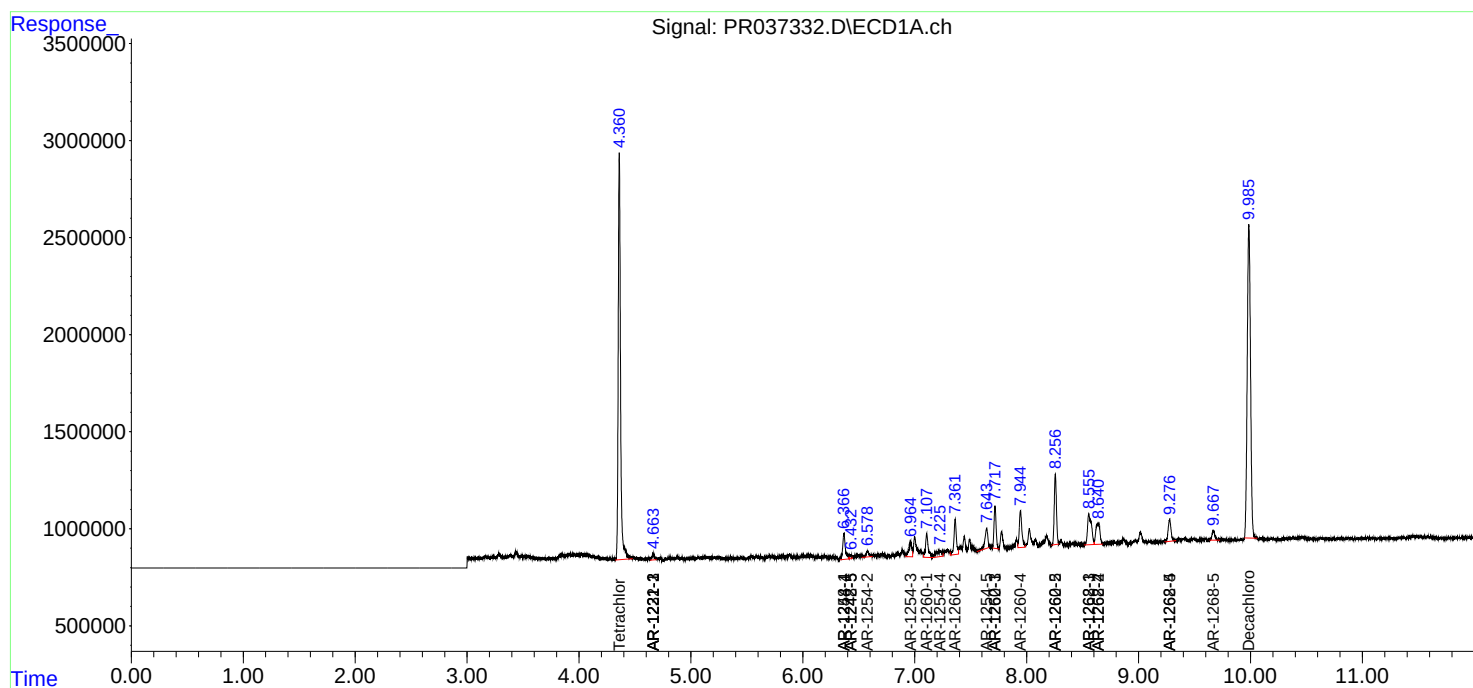


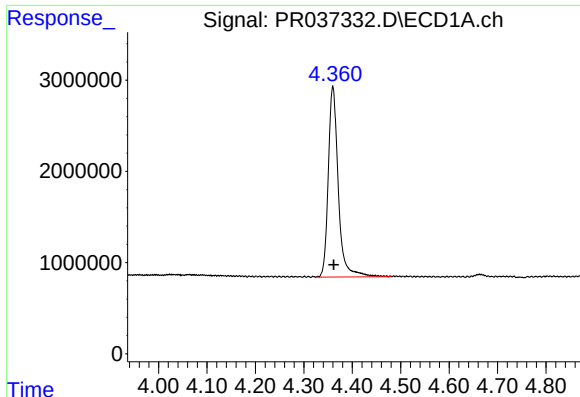

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 30011407
Conc: 23.99 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

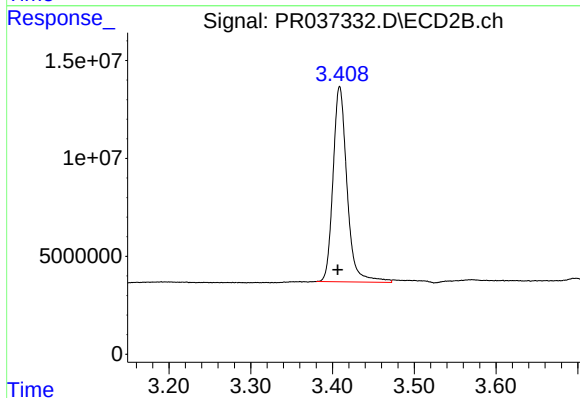


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: 0.002 min
Response: 118863031
Conc: 24.79 ng/ml

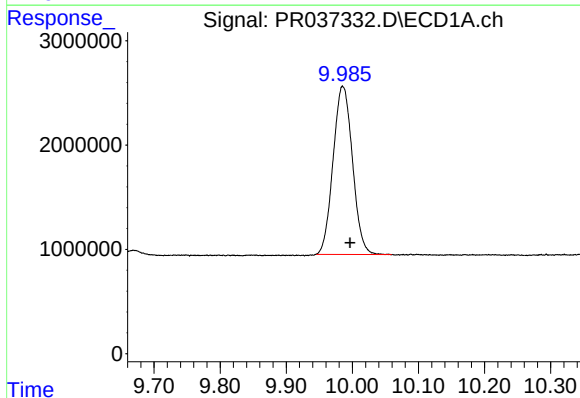


#2 Decachlorobiphenyl

R.T.: 9.986 min
Delta R.T.: -0.011 min
Response: 32788644
Conc: 24.79 ng/ml

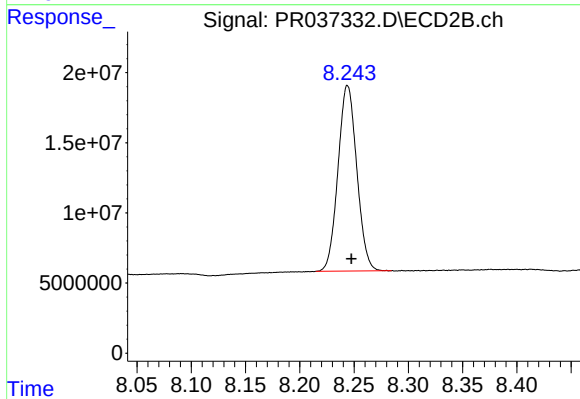

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.003 min
Response: 159462143
Conc: 27.38 ng/ml

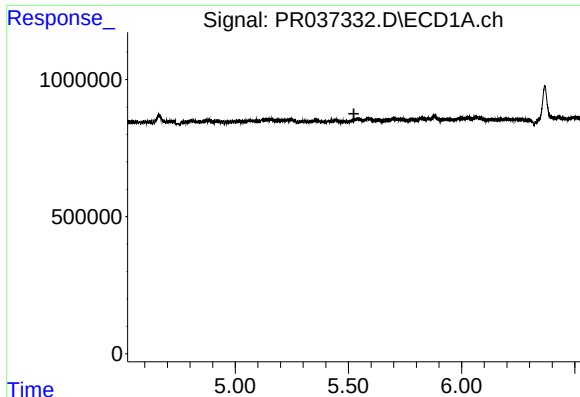

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

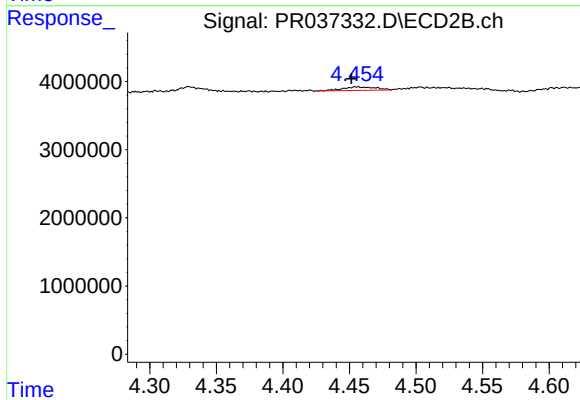


#3 AR-1016-1

R.T.: 4.454 min
Delta R.T.: 0.003 min
Response: 887178
Conc: 4.87 ng/ml

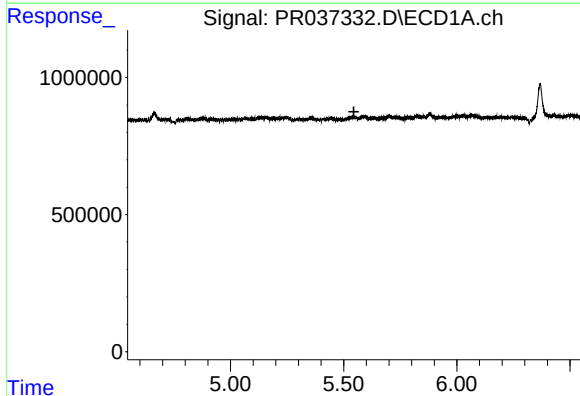


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

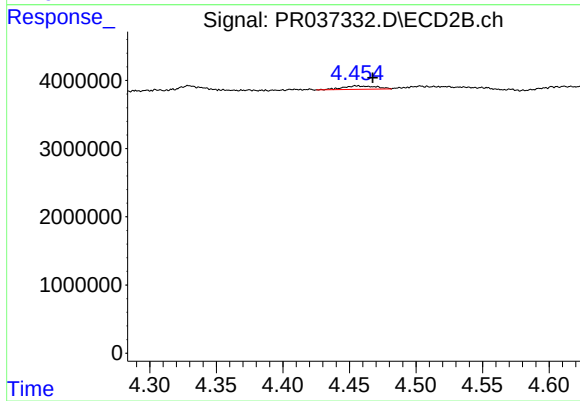

#4 AR-1016-2


R.T.: 4.454 min
Delta R.T.: -0.013 min
Response: 887178
Conc: 3.14 ng/ml

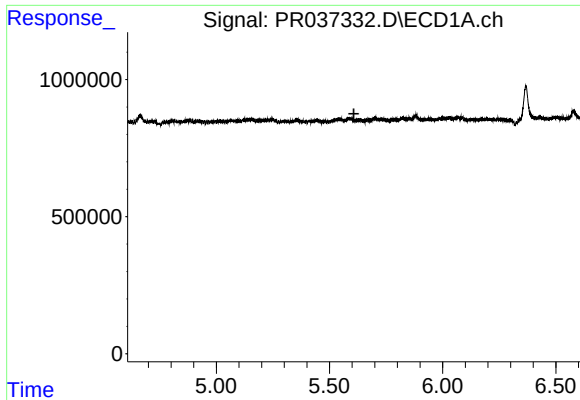

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

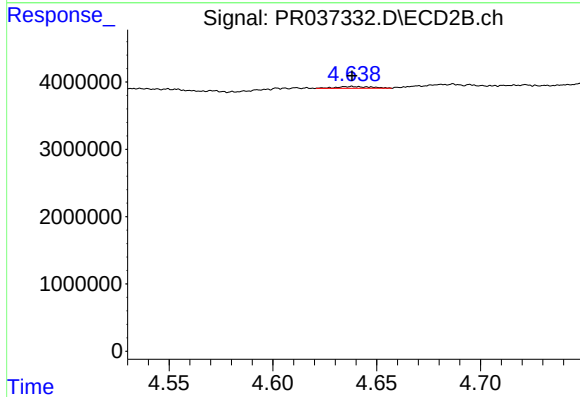


#5 AR-1016-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 301518
Conc: 2.10 ng/ml

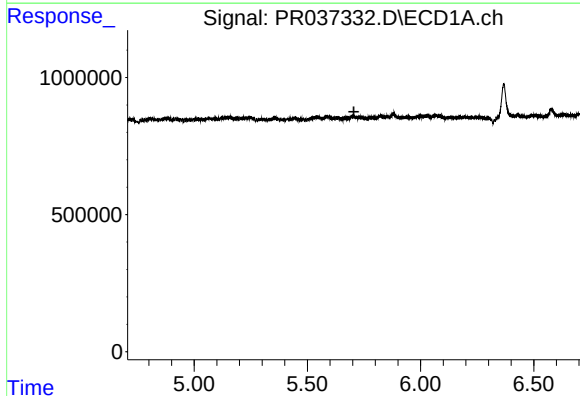


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

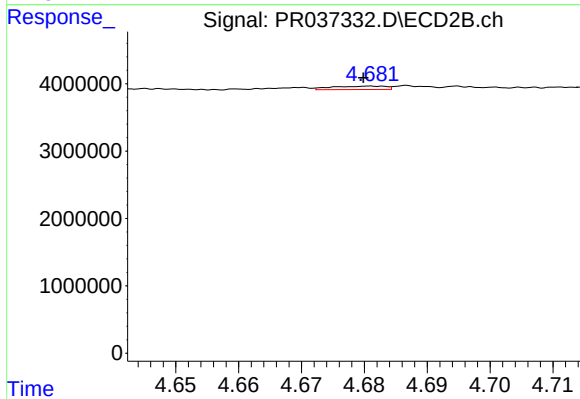

#6 AR-1016-4


R.T.: 4.681 min
Delta R.T.: 0.001 min
Response: 296242
Conc: 2.68 ng/ml

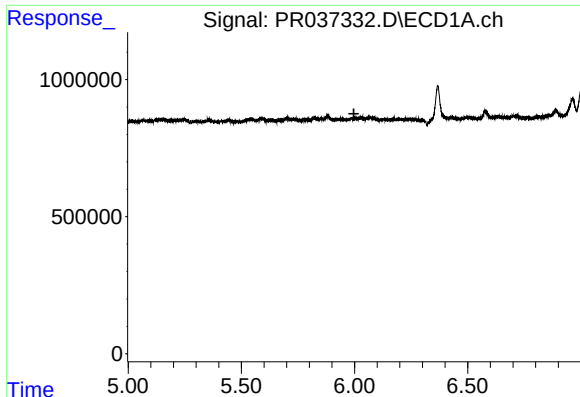

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

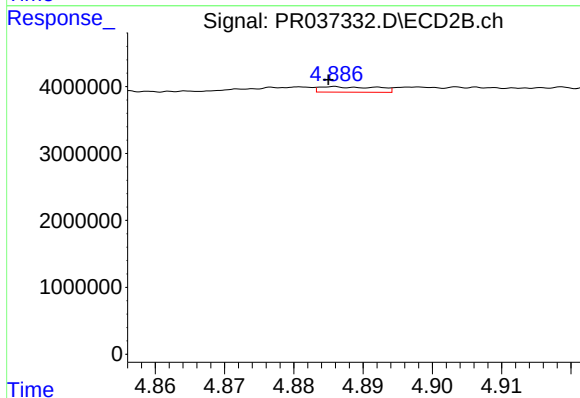


#7 AR-1016-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 477988
Conc: 3.14 ng/ml

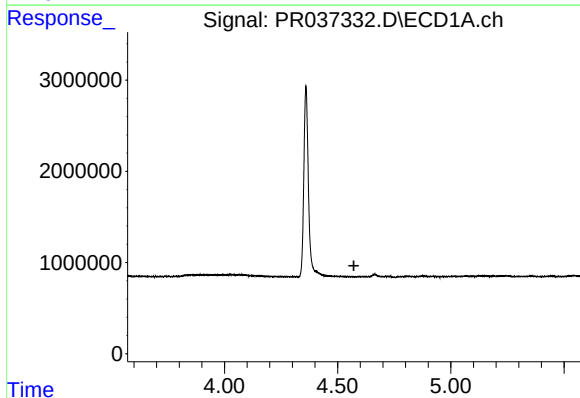


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

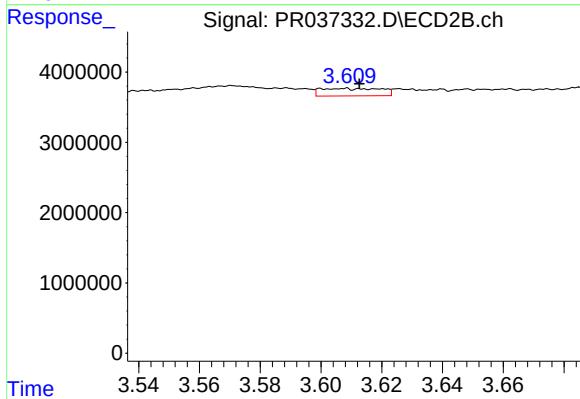

#8 AR-1221-1


R.T.: 3.608 min
Delta R.T.: -0.004 min
Response: 1479138
Conc: 29.05 ng/ml

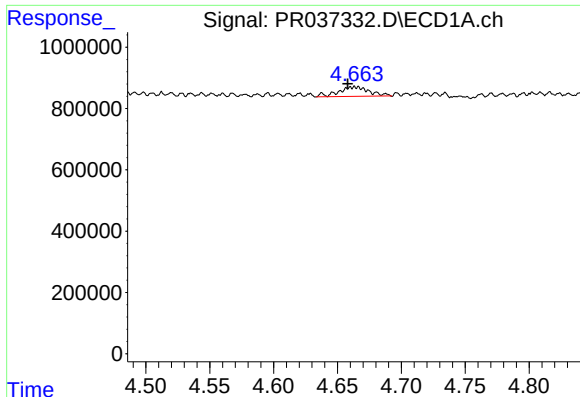

#9 AR-1221-2


R.T.: 4.664 min
Delta R.T.: 0.006 min
Response: 511234
Conc: 56.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

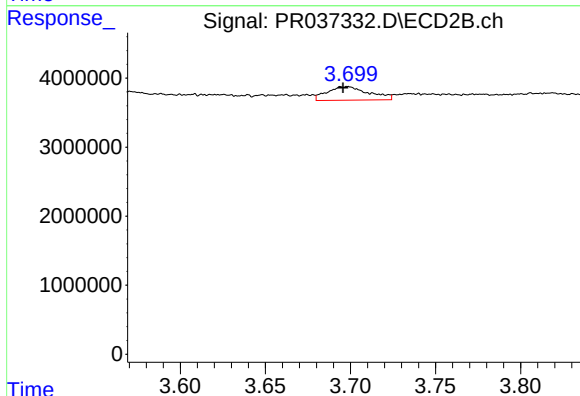


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.003 min
Response: 3357661
Conc: 90.42 ng/ml

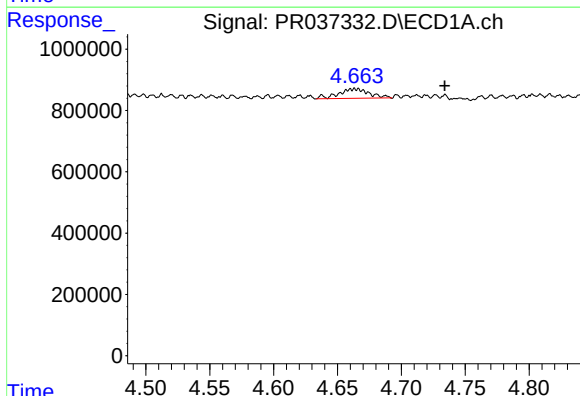


#10 AR-1221-3

R.T.: 4.664 min
Delta R.T.: -0.070 min
Response: 511234
Conc: 16.68 ng/ml

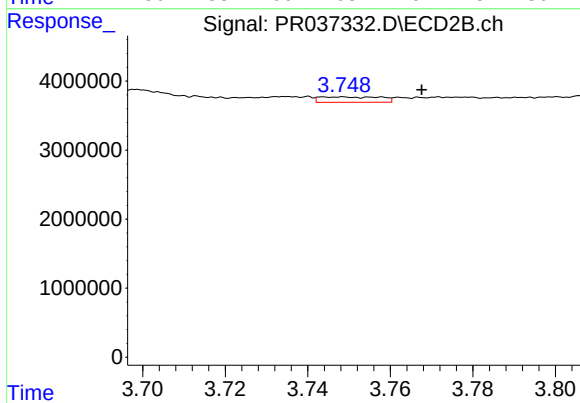

#10 AR-1221-3


R.T.: 3.749 min
Delta R.T.: -0.019 min
Response: 800300
Conc: 6.54 ng/ml

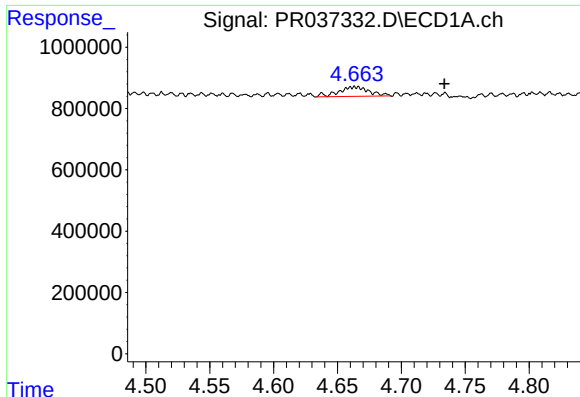

#11 AR-1232-1


R.T.: 4.664 min
Delta R.T.: -0.070 min
Response: 511234
Conc: 17.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

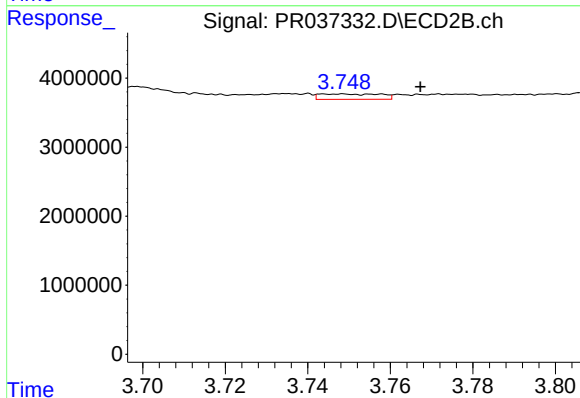


#11 AR-1232-1

R.T.: 3.749 min
Delta R.T.: -0.019 min
Response: 800300
Conc: 6.84 ng/ml

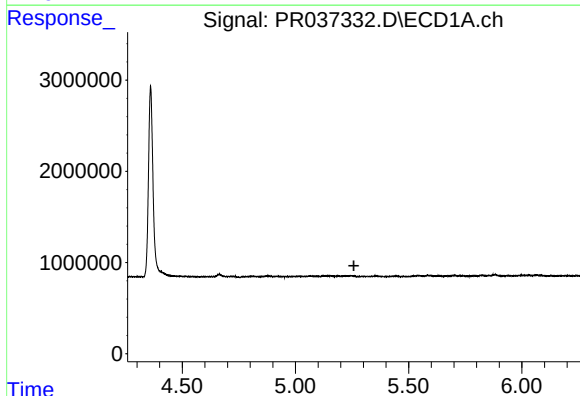


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

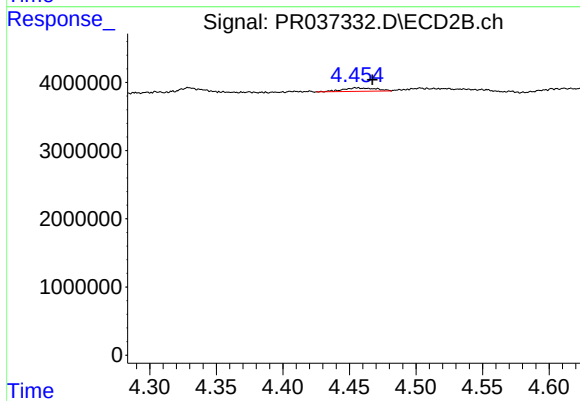

#12 AR-1232-2


R.T.: 4.454 min
Delta R.T.: -0.013 min
Response: 887178
Conc: 6.42 ng/ml

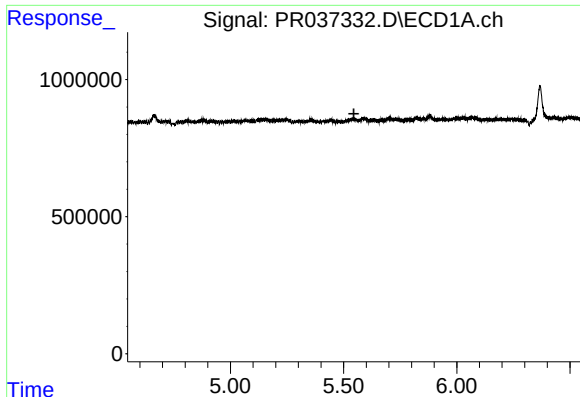

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

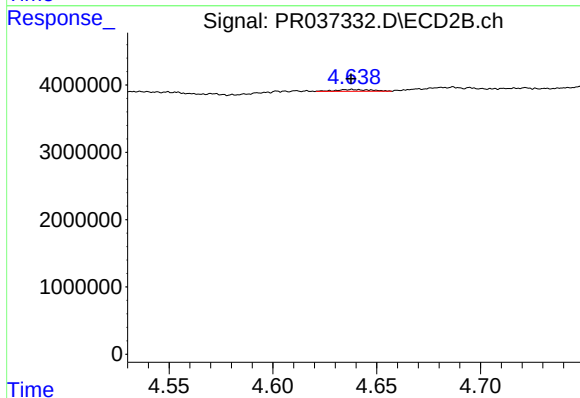


#13 AR-1232-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 301518
Conc: 4.30 ng/ml

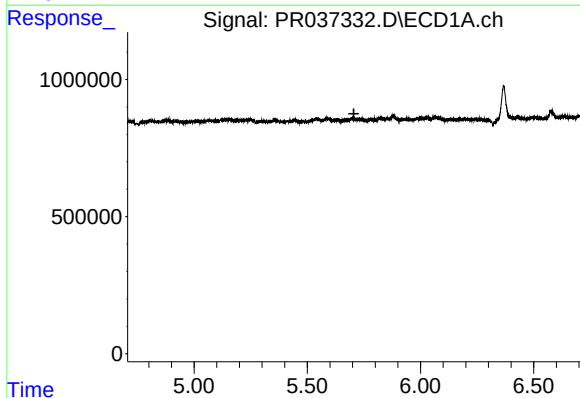


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

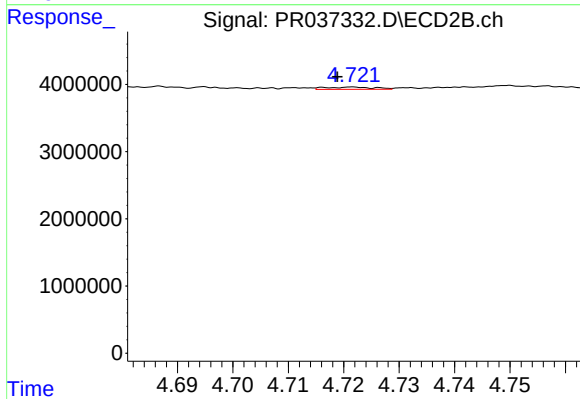

#14 AR-1232-4


R.T.: 4.722 min
Delta R.T.: 0.003 min
Response: 207687
Conc: 3.48 ng/ml

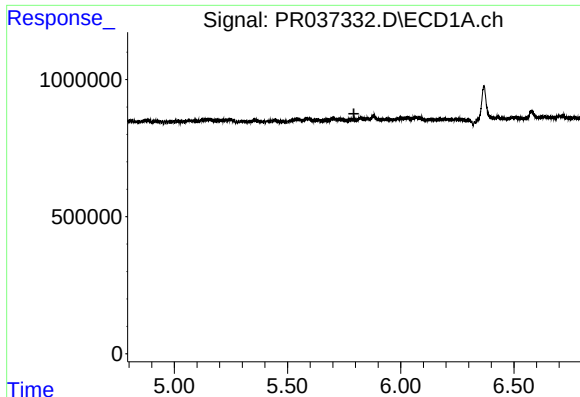

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

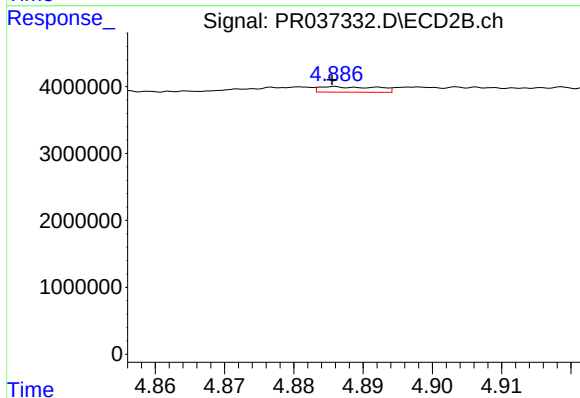


#15 AR-1232-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 477988
Conc: 7.00 ng/ml

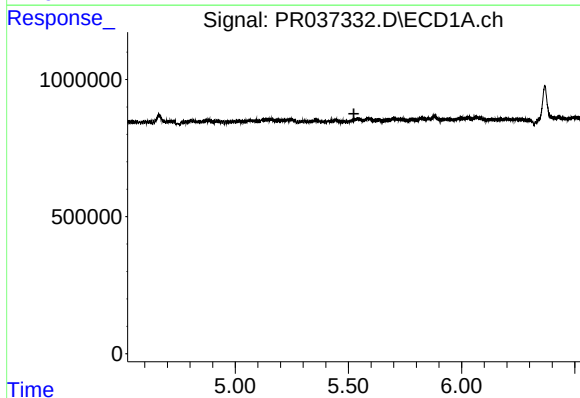


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

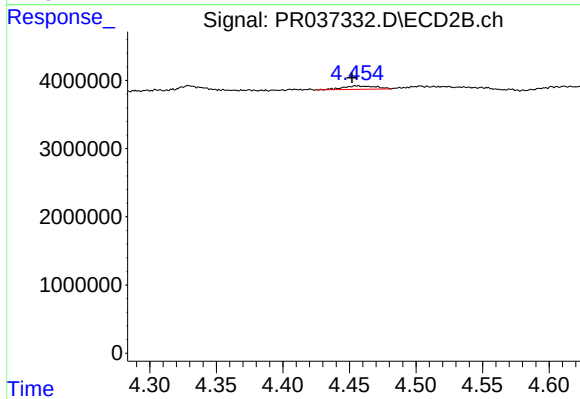

#16 AR-1242-1


R.T.: 4.454 min
Delta R.T.: 0.002 min
Response: 887178
Conc: 6.05 ng/ml

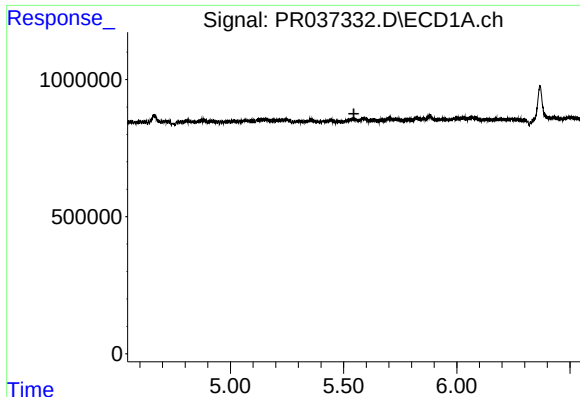

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

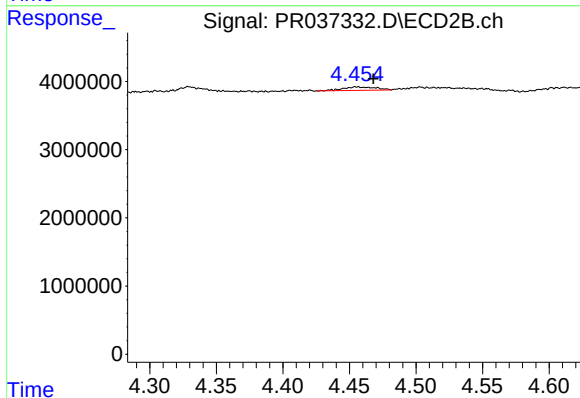


#17 AR-1242-2

R.T.: 4.454 min
Delta R.T.: -0.014 min
Response: 887178
Conc: 3.89 ng/ml

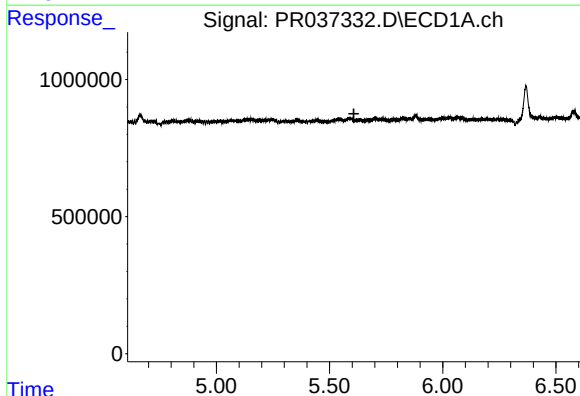


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 5.608 min
Response: 0
Conc: N.D.

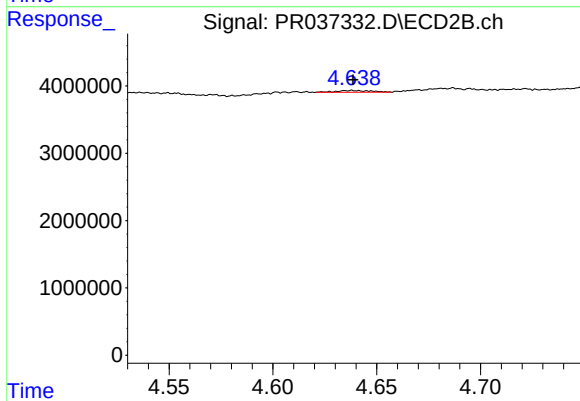

#18 AR-1242-3


R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 301518
Conc: 2.61 ng/ml

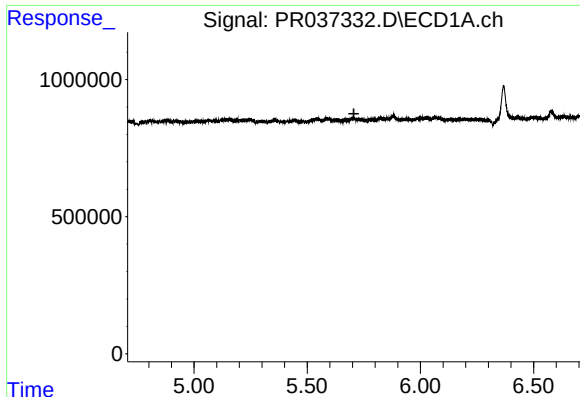

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

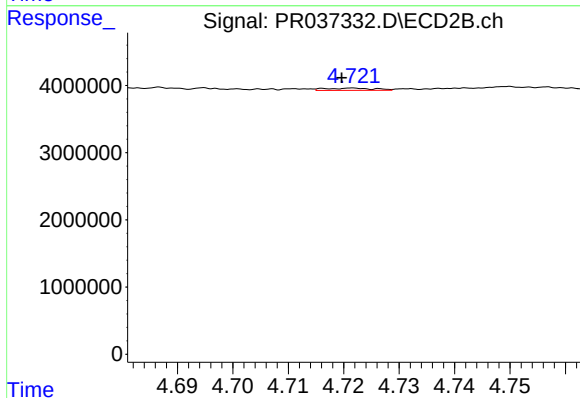


#19 AR-1242-4

R.T.: 4.722 min
Delta R.T.: 0.002 min
Response: 207687
Conc: 1.89 ng/ml

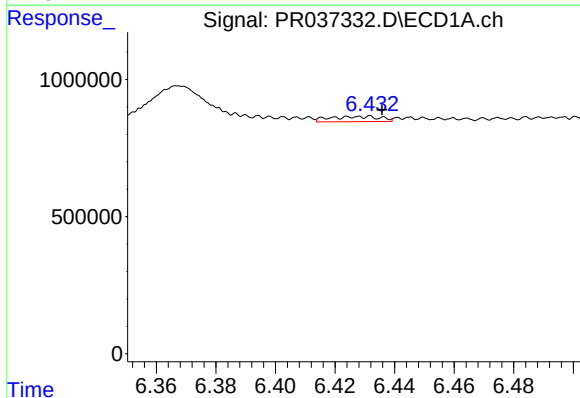


#20 AR-1242-5

R.T.: 6.431 min
Delta R.T.: -0.005 min
Response: 228254
Conc: 7.09 ng/ml

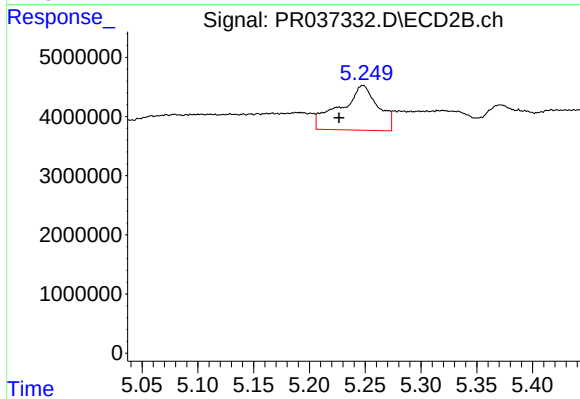

#20 AR-1242-5


R.T.: 5.248 min
Delta R.T.: 0.021 min
Response: 17867262
Conc: 107.83 ng/ml

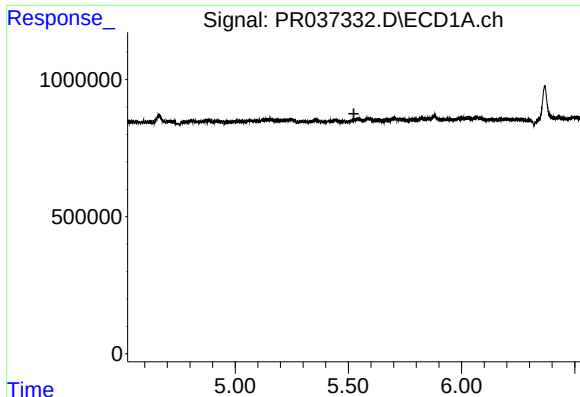

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

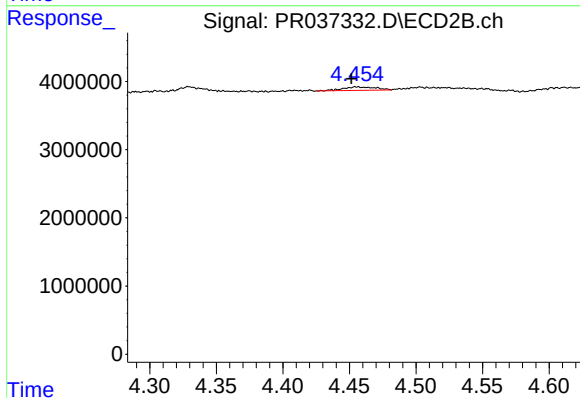


#21 AR-1248-1

R.T.: 4.454 min
Delta R.T.: 0.003 min
Response: 887178
Conc: 8.81 ng/ml

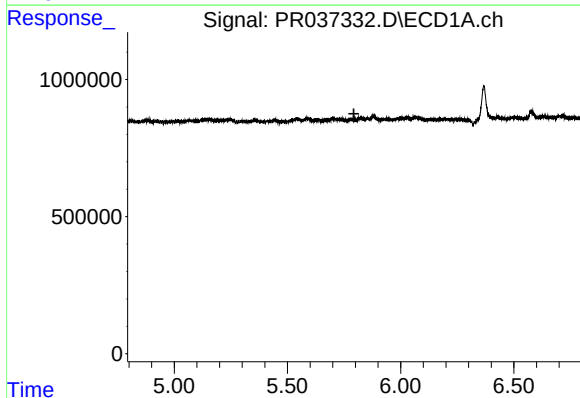


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

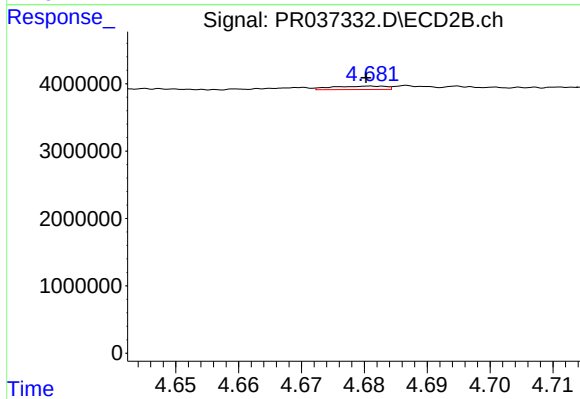

#22 AR-1248-2


R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 296242
Conc: 2.17 ng/ml

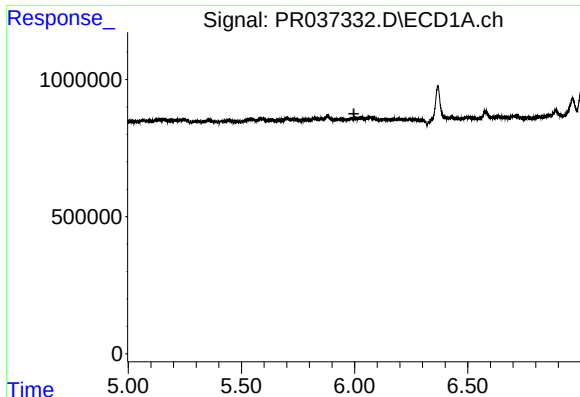

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

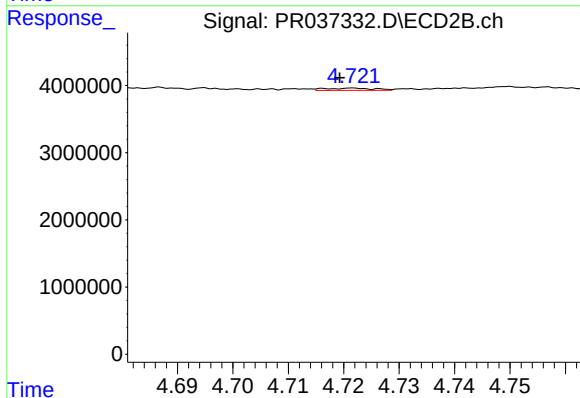


#23 AR-1248-3

R.T.: 4.722 min
Delta R.T.: 0.002 min
Response: 207687
Conc: 1.48 ng/ml

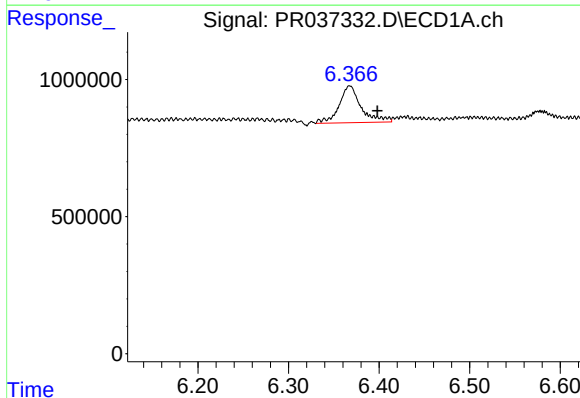


#24 AR-1248-4

R.T.: 6.368 min
Delta R.T.: -0.030 min
Response: 2265035
Conc: 46.27 ng/ml

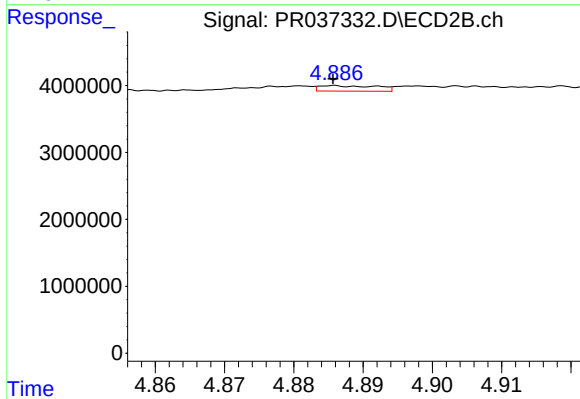

#24 AR-1248-4


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 477988
Conc: 2.69 ng/ml

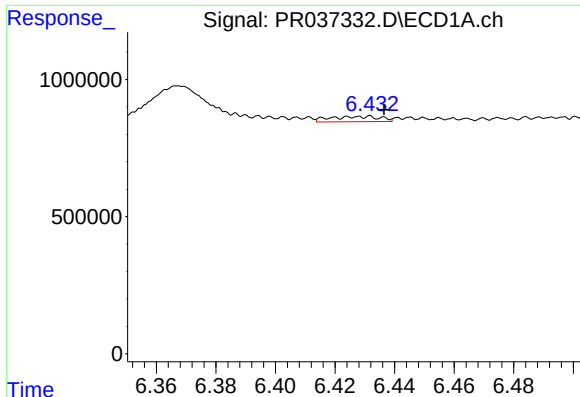

#25 AR-1248-5


R.T.: 6.431 min
Delta R.T.: -0.005 min
Response: 228254
Conc: 4.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

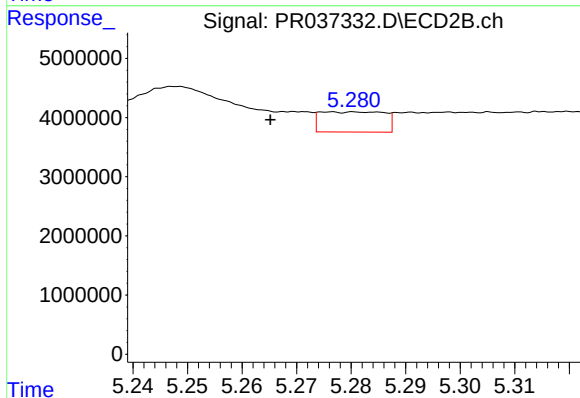


#25 AR-1248-5

R.T.: 5.276 min
Delta R.T.: 0.011 min
Response: 2790989
Conc: 14.27 ng/ml

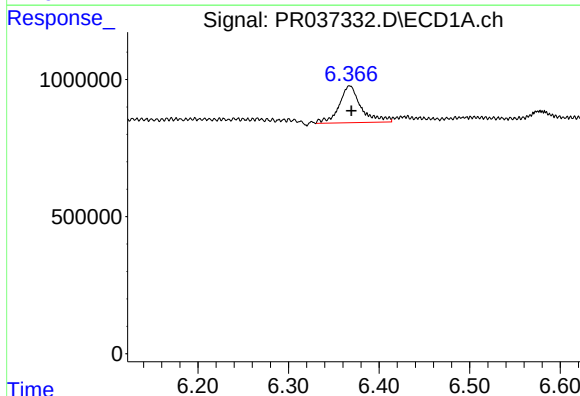


#26 AR-1254-1

R.T.: 6.368 min
Delta R.T.: -0.002 min
Response: 2265035
Conc: 41.46 ng/ml

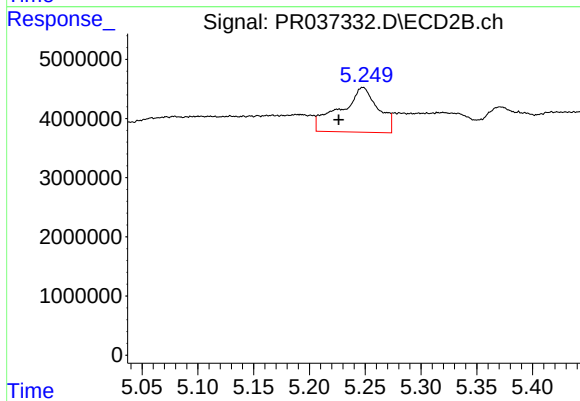

#26 AR-1254-1


R.T.: 5.248 min
Delta R.T.: 0.022 min
Response: 17867262
Conc: 51.87 ng/ml

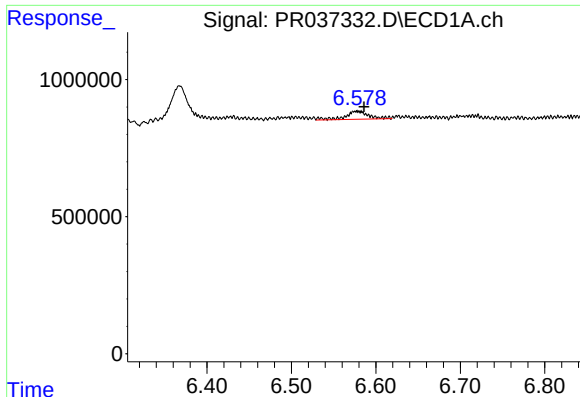

#27 AR-1254-2


R.T.: 6.578 min
Delta R.T.: -0.008 min
Response: 568256
Conc: 6.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

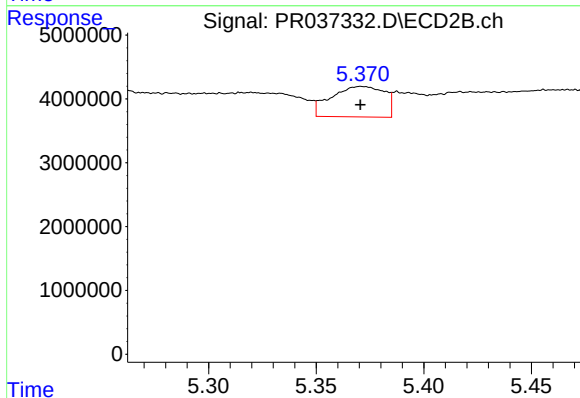


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 8213284
Conc: 27.42 ng/ml

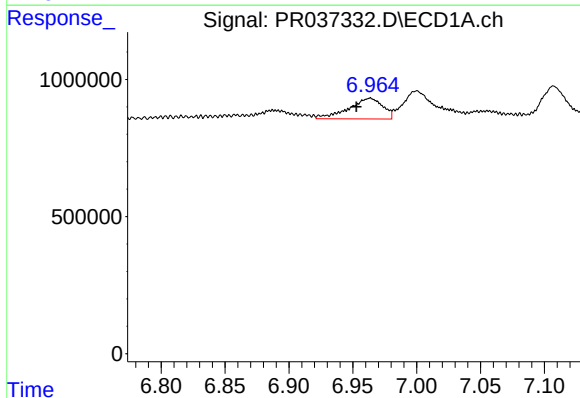


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: 0.011 min
Response: 1399350
Conc: 15.38 ng/ml

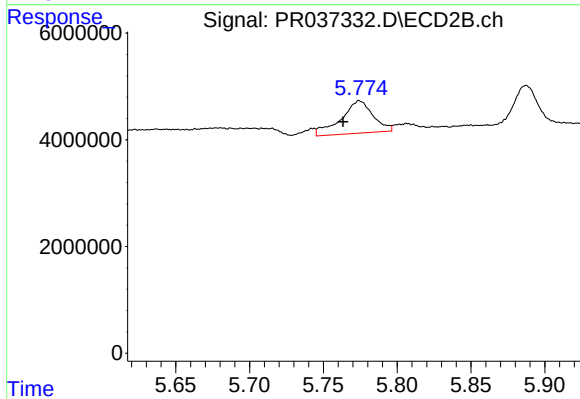

#28 AR-1254-3


R.T.: 5.774 min
Delta R.T.: 0.011 min
Response: 9223286
Conc: 19.47 ng/ml

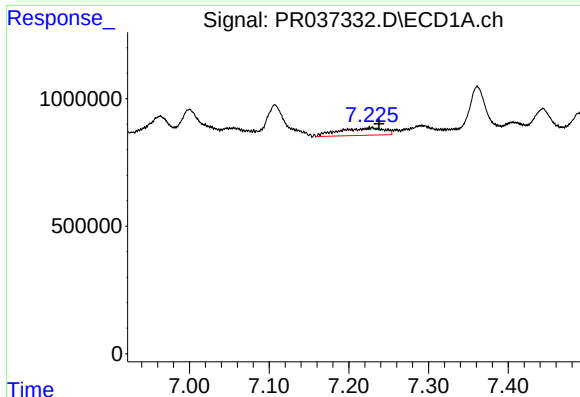

#29 AR-1254-4


R.T.: 7.230 min
Delta R.T.: -0.008 min
Response: 1115934
Conc: 16.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

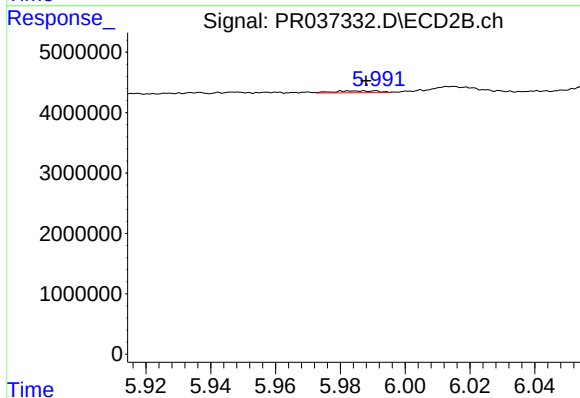


#29 AR-1254-4

R.T.: 5.991 min
Delta R.T.: 0.003 min
Response: 292312
Conc: 0.83 ng/ml

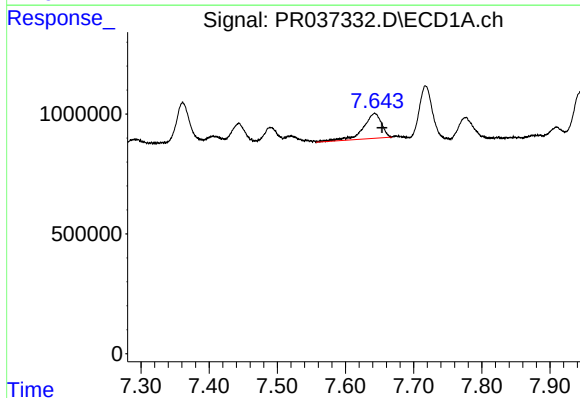


#30 AR-1254-5

R.T.: 7.643 min
Delta R.T.: -0.011 min
Response: 1925039
Conc: 26.78 ng/ml

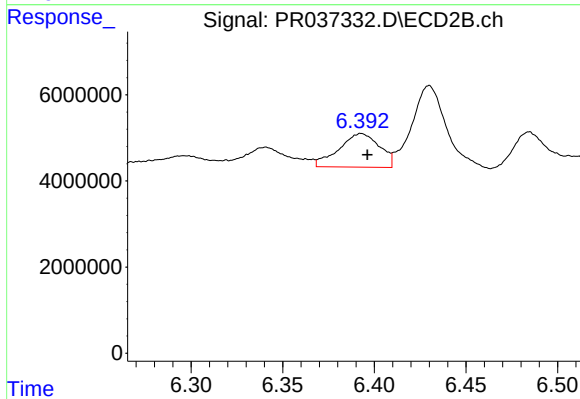

#30 AR-1254-5


R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 12086148
Conc: 27.29 ng/ml

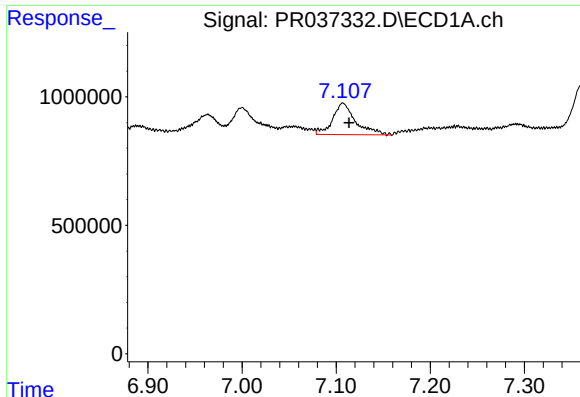

#31 AR-1260-1


R.T.: 7.107 min
Delta R.T.: -0.006 min
Response: 2084127
Conc: 31.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

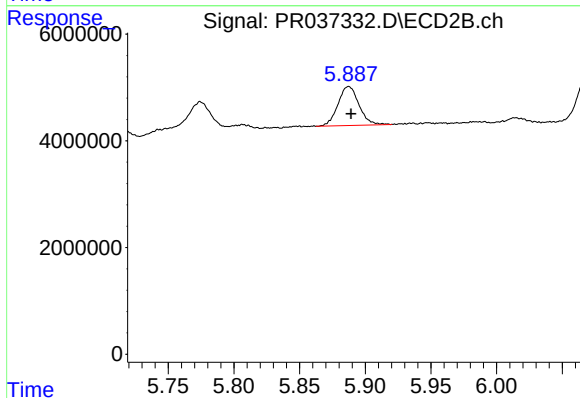


#31 AR-1260-1

R.T.: 5.887 min
Delta R.T.: -0.002 min
Response: 8114616
Conc: 27.76 ng/ml

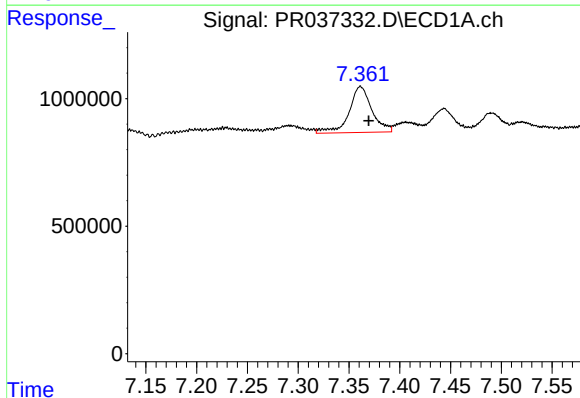


#32 AR-1260-2

R.T.: 7.361 min
Delta R.T.: -0.008 min
Response: 2818657
Conc: 35.36 ng/ml

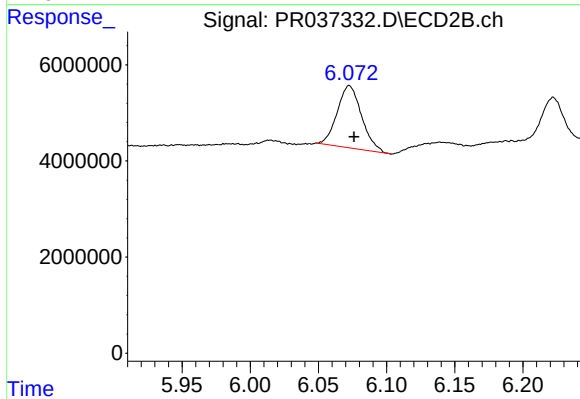

#32 AR-1260-2


R.T.: 6.073 min
Delta R.T.: -0.004 min
Response: 16016980
Conc: 34.78 ng/ml

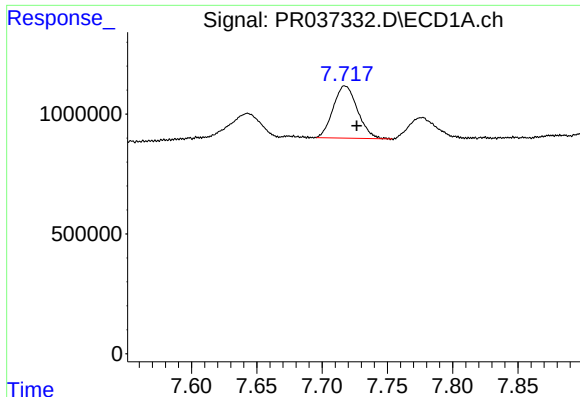

#33 AR-1260-3


R.T.: 7.718 min
Delta R.T.: -0.009 min
Response: 2833863
Conc: 45.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

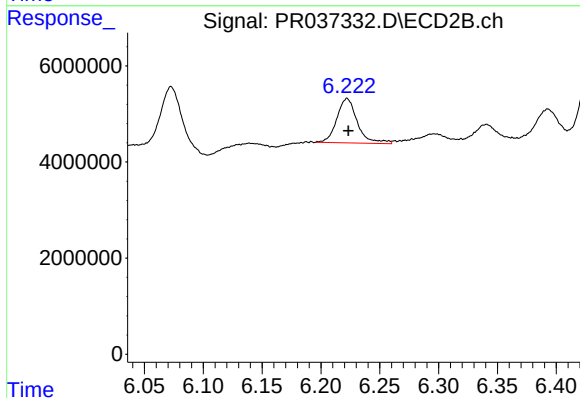


#33 AR-1260-3

R.T.: 6.222 min
Delta R.T.: -0.001 min
Response: 11249159
Conc: 31.55 ng/ml

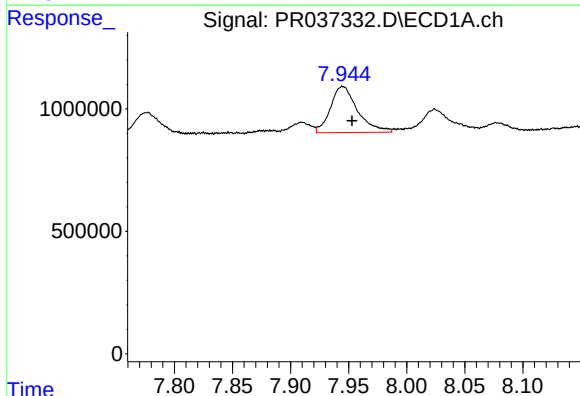


#34 AR-1260-4

R.T.: 7.945 min
Delta R.T.: -0.008 min
Response: 3061761
Conc: 41.15 ng/ml

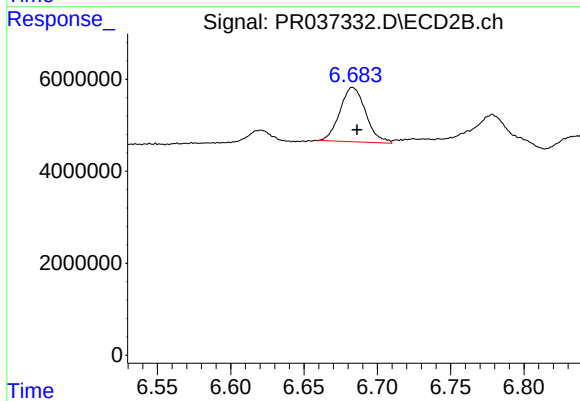

#34 AR-1260-4


R.T.: 6.683 min
Delta R.T.: -0.003 min
Response: 14440963
Conc: 47.38 ng/ml

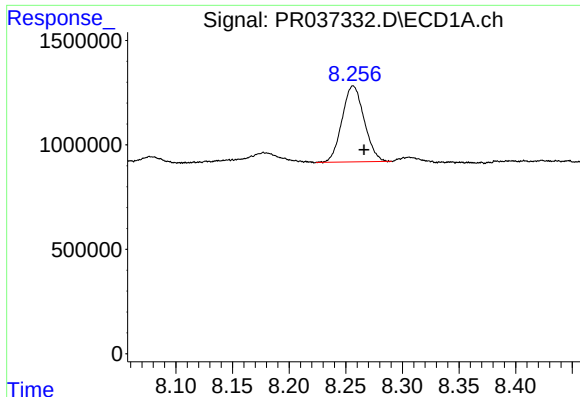

#35 AR-1260-5


R.T.: 8.257 min
Delta R.T.: -0.010 min
Response: 4940749
Conc: 34.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

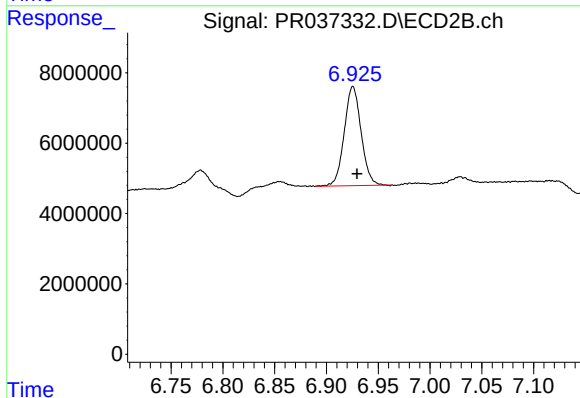


#35 AR-1260-5

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 31931351
Conc: 36.82 ng/ml

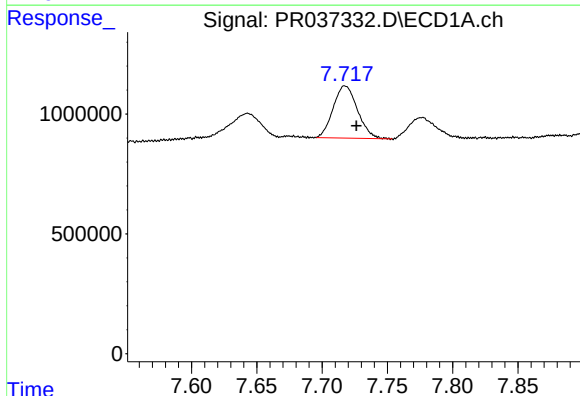


#36 AR-1262-1

R.T.: 7.718 min
Delta R.T.: -0.009 min
Response: 2833863
Conc: 27.13 ng/ml

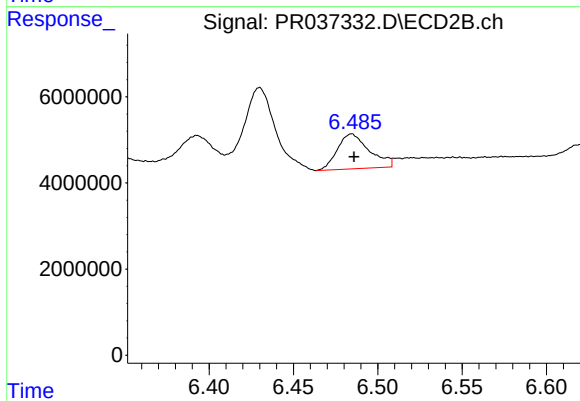

#36 AR-1262-1


R.T.: 6.485 min
Delta R.T.: -0.001 min
Response: 10707793
Conc: 42.73 ng/ml

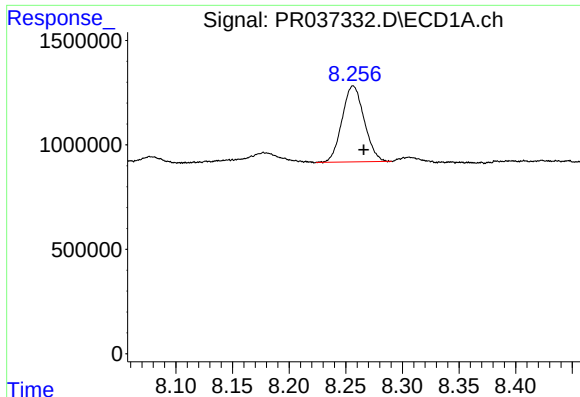

#37 AR-1262-2


R.T.: 8.257 min
Delta R.T.: -0.009 min
Response: 4940749
Conc: 25.42 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

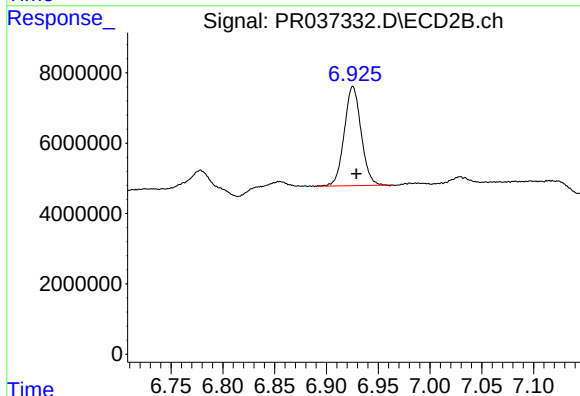


#37 AR-1262-2

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 31931351
Conc: 25.42 ng/ml

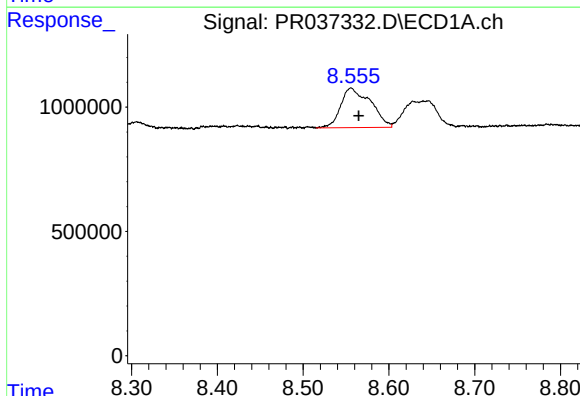


#38 AR-1262-3

R.T.: 8.556 min
Delta R.T.: -0.009 min
Response: 3869779
Conc: 29.43 ng/ml

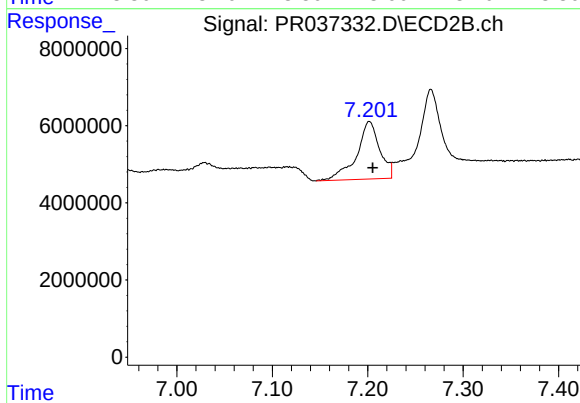

#38 AR-1262-3


R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 25014927
Conc: 45.63 ng/ml

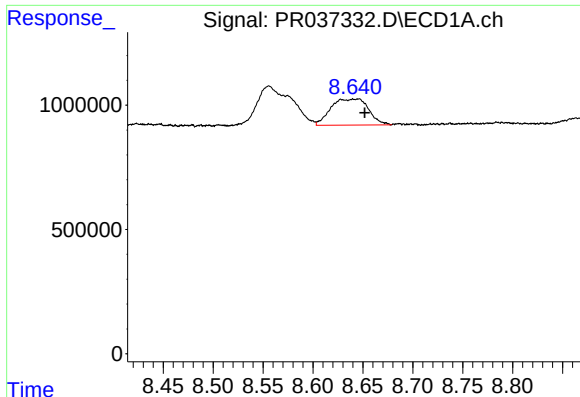

#39 AR-1262-4


R.T.: 8.645 min
Delta R.T.: -0.006 min
Response: 2757005
Conc: 28.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

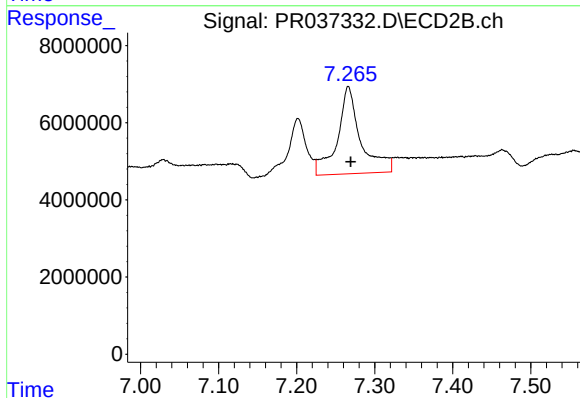


#39 AR-1262-4

R.T.: 7.266 min
Delta R.T.: -0.003 min
Response: 46947842
Conc: 52.30 ng/ml

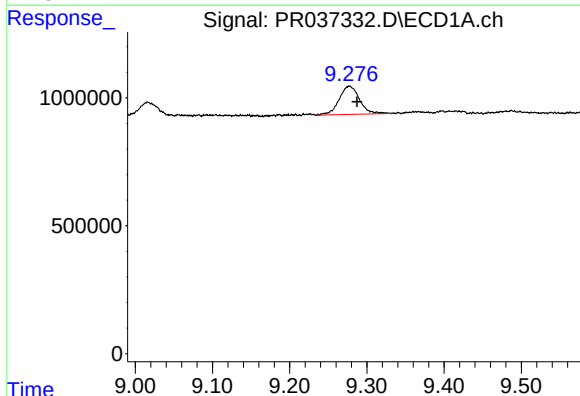


#40 AR-1262-5

R.T.: 9.277 min
Delta R.T.: -0.010 min
Response: 2017193
Conc: 29.22 ng/ml

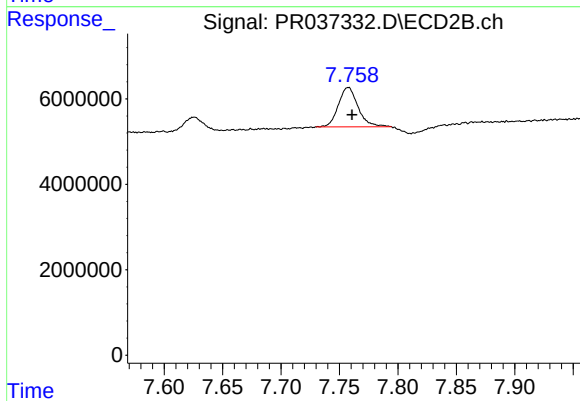

#40 AR-1262-5


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 10837051
Conc: 28.32 ng/ml

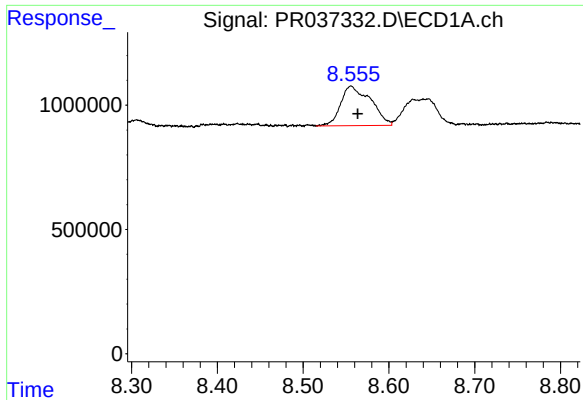

#41 AR-1268-1


R.T.: 8.556 min
Delta R.T.: -0.008 min
Response: 3869779
Conc: 21.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

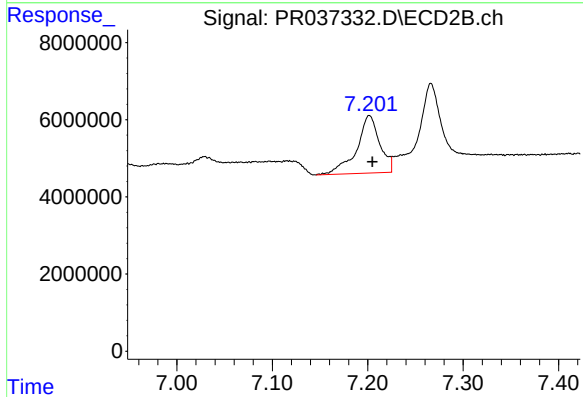


#41 AR-1268-1

R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 25014927
Conc: 20.32 ng/ml

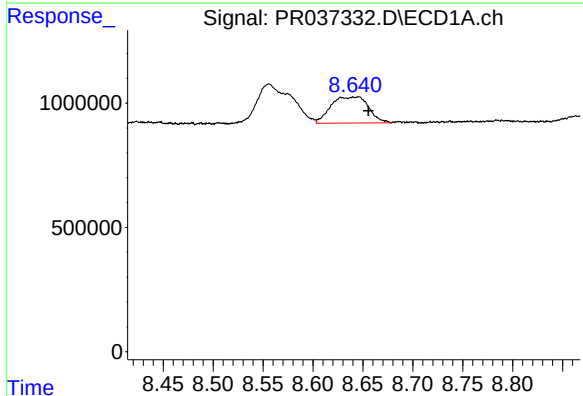


#42 AR-1268-2

R.T.: 8.645 min
Delta R.T.: -0.010 min
Response: 2757005
Conc: 16.76 ng/ml

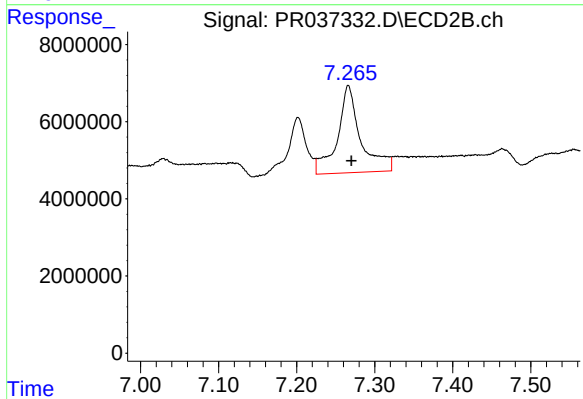

#42 AR-1268-2


R.T.: 7.266 min
Delta R.T.: -0.004 min
Response: 46947842
Conc: 44.34 ng/ml

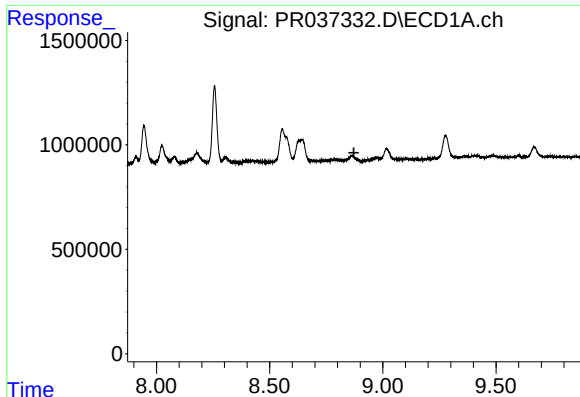

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

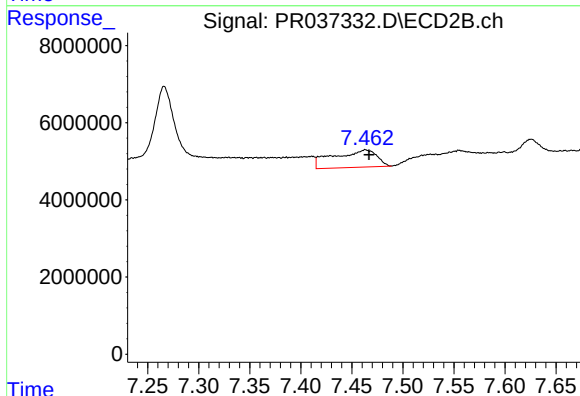


#43 AR-1268-3

R.T.: 7.463 min
Delta R.T.: -0.003 min
Response: 13168502
Conc: 14.86 ng/ml

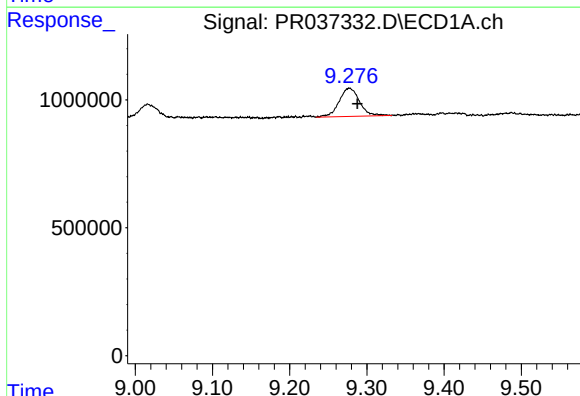


#44 AR-1268-4

R.T.: 9.277 min
Delta R.T.: -0.010 min
Response: 2017193
Conc: 32.33 ng/ml

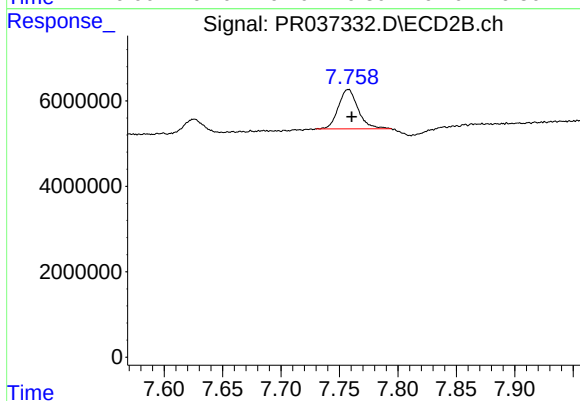

#44 AR-1268-4


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 10837051
Conc: 29.87 ng/ml

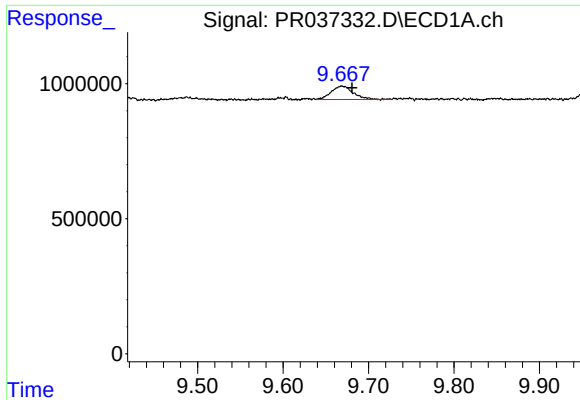

#45 AR-1268-5

R.T.: 9.669 min
Delta R.T.: -0.012 min
Response: 890164
Conc: 1.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

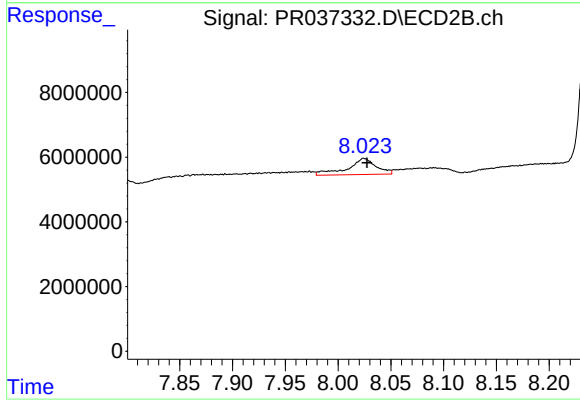

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.003 min
Response: 9401705
Conc: 3.70 ng/ml