

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
 Data File : PR037397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 14:53
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1660 MDL 25PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:40:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.359	3.407	29429735	117.9E6	23.525	24.589
2)	SA Decachlor...	9.985	8.244	28398432	136.4E6	21.472	23.423
Target Compounds							
3)	L1 AR-1016-1	5.520	4.450	1373764	5895627	31.882	32.379
4)	L1 AR-1016-2	5.540	4.466	2284041	9211723	32.984	32.652
5)	L1 AR-1016-3	5.602	4.634	1460763	1679553	36.222	11.681 #
6)	L1 AR-1016-4	5.701	4.680	1044509	4763526	31.806	43.056 #
7)	L1 AR-1016-5	5.991	4.883	1135367	4794128	33.111	31.538
8)	L2 AR-1221-1	0.000	3.613	0	417274	N.D.	8.195 #
9)	L2 AR-1221-2	4.659	3.695	494538	2181907	54.682	58.755
10)	L2 AR-1221-3	4.732	3.768	837811	3326570	27.336	27.167
11)	L3 AR-1232-1	4.732	3.768	837811	3326570	28.642	28.434
12)	L3 AR-1232-2	5.254	4.466	1223403	9211723	72.401	66.643
13)	L3 AR-1232-3	5.540	4.634	2284041	1679553	67.566	23.925 #
14)	L3 AR-1232-4	5.701	4.717	1044509	5343999	66.543	89.557 #
15)	L3 AR-1232-5	5.788	4.883	973273	4794128	83.217	70.250
16)	L4 AR-1242-1	5.520	4.450	1373764	5895627	40.152	40.233
17)	L4 AR-1242-2	5.540	4.466	2284041	9211723	41.176	40.374
18)	L4 AR-1242-3	5.602	4.634	1460763	1679553	44.380	14.525 #
19)	L4 AR-1242-4	5.701	4.717	1044509	5343999	39.599	48.621
20)	L4 AR-1242-5	6.428	5.224	950784	6672413	29.547	40.268 #
21)	L5 AR-1248-1	5.520	4.450	1373764	5895627	59.970	58.567
22)	L5 AR-1248-2	5.788	4.680	973273	4763526	27.796	34.904 #
23)	L5 AR-1248-3	5.991	4.717	1135367	5343999	27.753	38.179 #
24)	L5 AR-1248-4	6.391	4.883	777954	4794128	15.891	26.939 #
25)	L5 AR-1248-5	6.428	5.264	950784	3403898	20.128	17.401
26)	L6 AR-1254-1	6.364	5.224	1267764	6672413	23.206	19.370
27)	L6 AR-1254-2	6.579	5.370	1102814	5591799	12.869	18.670 #
28)	L6 AR-1254-3	6.963	5.774	1105488	9455275	12.153	19.964 #
29)	L6 AR-1254-4	7.229	5.987	526604	809553	7.859	2.309 #
30)	L6 AR-1254-5	7.646	6.394	3431927	18082479	47.745	40.834
31)	L7 AR-1260-1	7.107	5.887	2451951	10214364	37.158	34.948
32)	L7 AR-1260-2	7.362	6.073	2876607	18042431	36.091	39.173
33)	L7 AR-1260-3	7.718	6.222	2236829	12563465	35.746	35.241
34)	L7 AR-1260-4	7.944	6.684	2536964	10619258	34.097	34.844
35)	L7 AR-1260-5	8.256	6.927	4839746	26309682	33.465	30.337
36)	L8 AR-1262-1	7.718	6.484	2236829	9366816	21.415	37.375 #
37)	L8 AR-1262-2	8.256	6.927	4839746	26309682	24.898	20.948
38)	L8 AR-1262-3	8.575	7.202	4284487	11964131	32.579	21.822 #
39)	L8 AR-1262-4	8.627	7.266	2228494	25434457	22.687	28.335
40)	L8 AR-1262-5	9.278	7.758	1249714	6473647	18.101	16.919
41)	L9 AR-1268-1	8.575	7.202	4284487	11964131	23.923	9.719 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
 Data File : PR037397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 14:53
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1660 MDL 25PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:40:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.627	7.266	2228494	25434457	13.547	24.019 #
43) L9	AR-1268-3	0.000	7.463	0	6509790	N.D.	7.345 #
44) L9	AR-1268-4	9.278	7.758	1249714	6473647	20.032	17.844
45) L9	AR-1268-5	9.668	8.024	562669	4395969	1.234	1.728 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
Data File : PR037397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 14:53
Operator : SM\SJ
Sample : K2241-09
Misc : AR1660 MDL 25PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 00:40:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

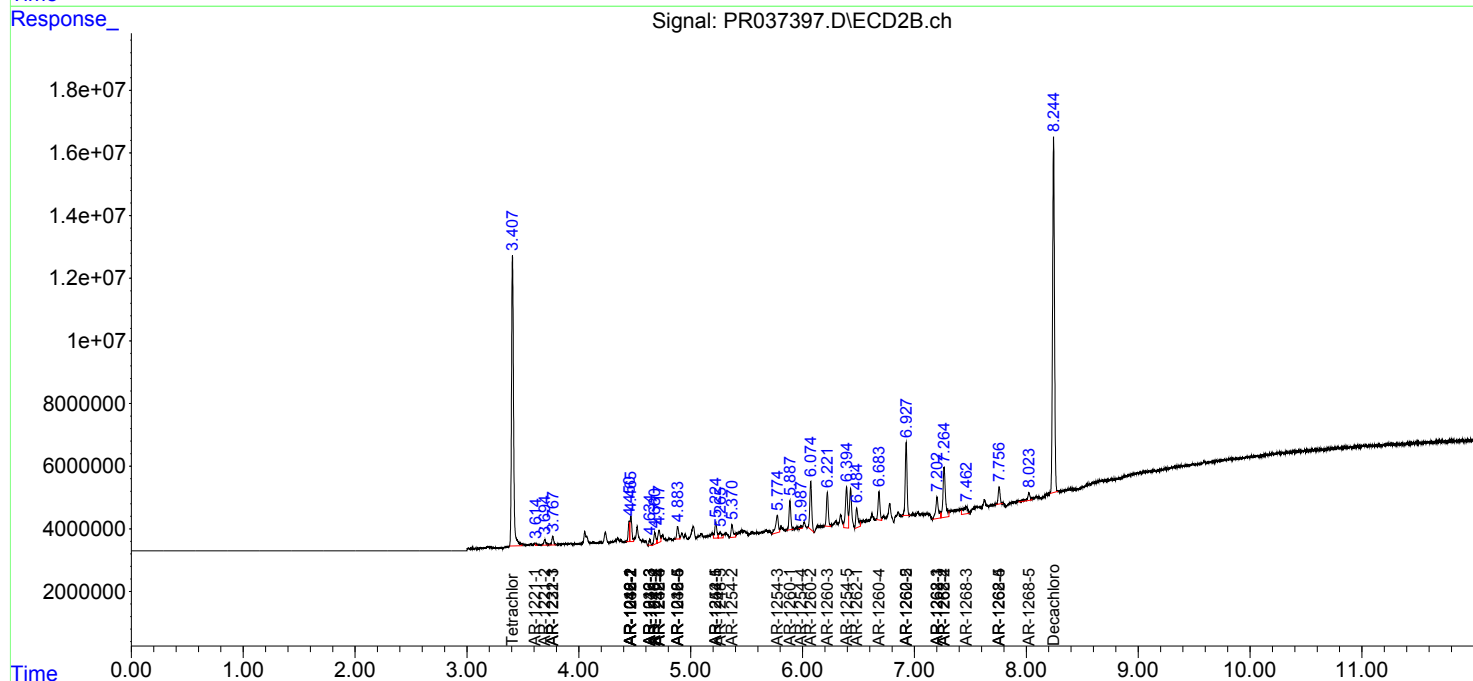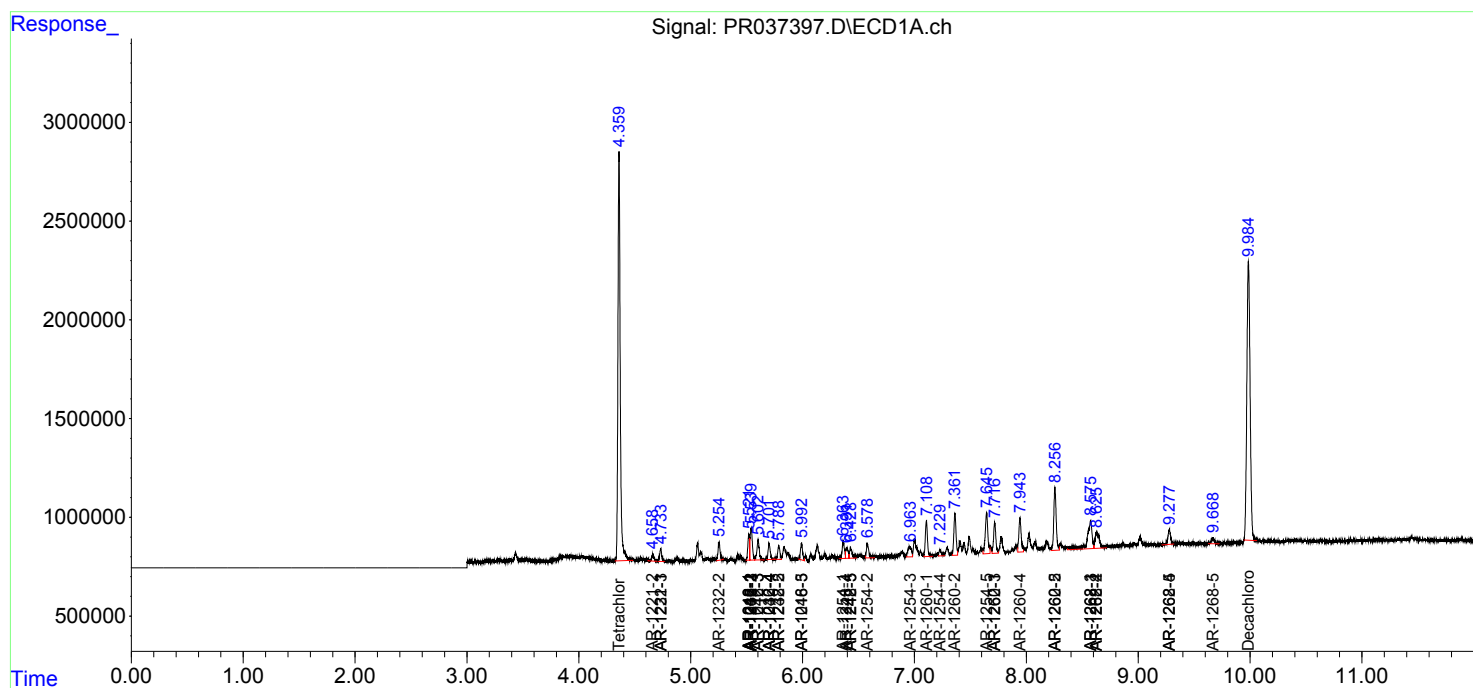


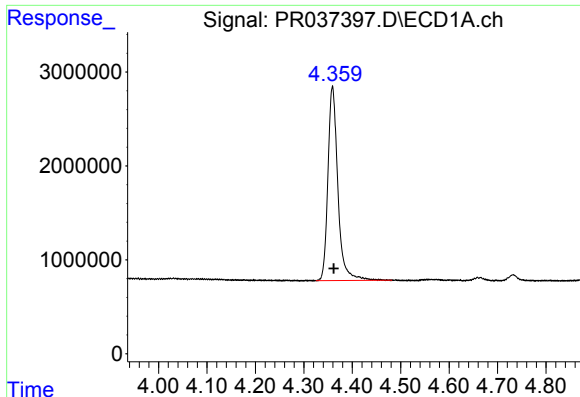

#1 Tetrachloro-m-xylene


R.T.: 4.359 min
Delta R.T.: -0.003 min
Response: 29429735
Conc: 23.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

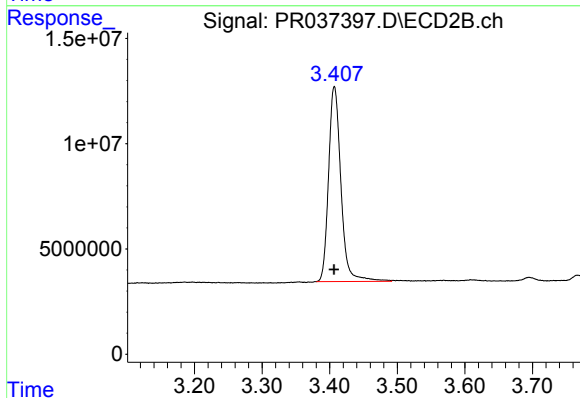


#1 Tetrachloro-m-xylene

R.T.: 3.407 min
Delta R.T.: 0.000 min
Response: 117916318
Conc: 24.59 ng/ml

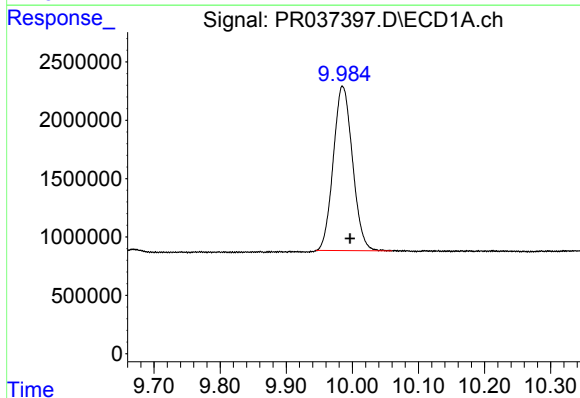


#2 Decachlorobiphenyl

R.T.: 9.985 min
Delta R.T.: -0.012 min
Response: 28398432
Conc: 21.47 ng/ml

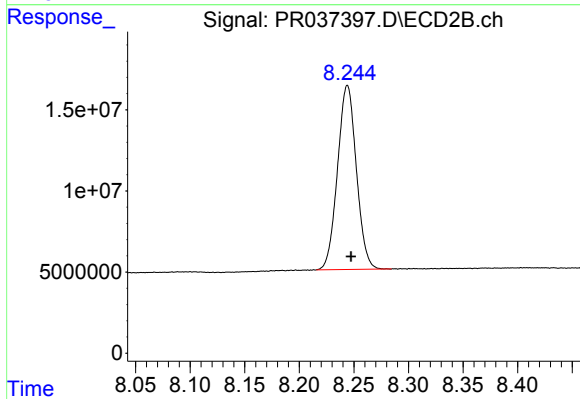

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.003 min
Response: 136420010
Conc: 23.42 ng/ml

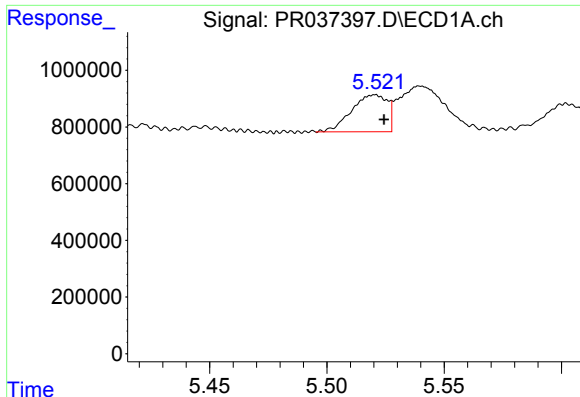

#3 AR-1016-1


R.T.: 5.520 min
Delta R.T.: -0.004 min
Response: 1373764
Conc: 31.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

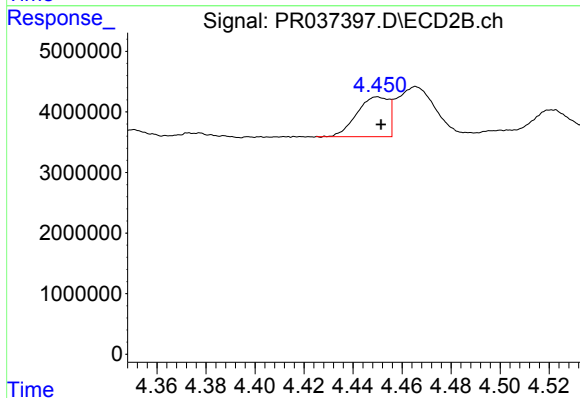


#3 AR-1016-1

R.T.: 4.450 min
Delta R.T.: -0.001 min
Response: 5895627
Conc: 32.38 ng/ml

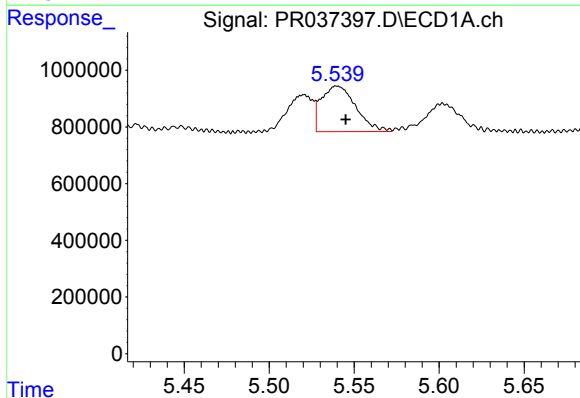


#4 AR-1016-2

R.T.: 5.540 min
Delta R.T.: -0.005 min
Response: 2284041
Conc: 32.98 ng/ml

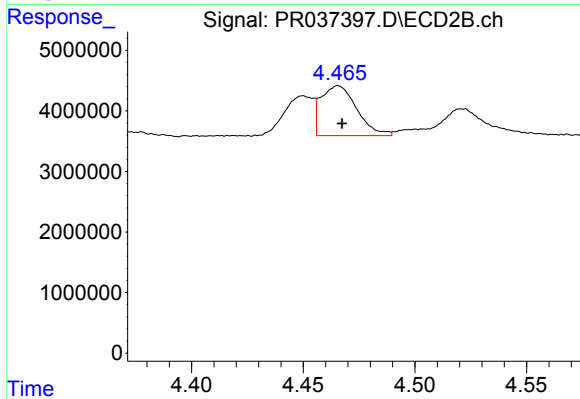

#4 AR-1016-2


R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 9211723
Conc: 32.65 ng/ml

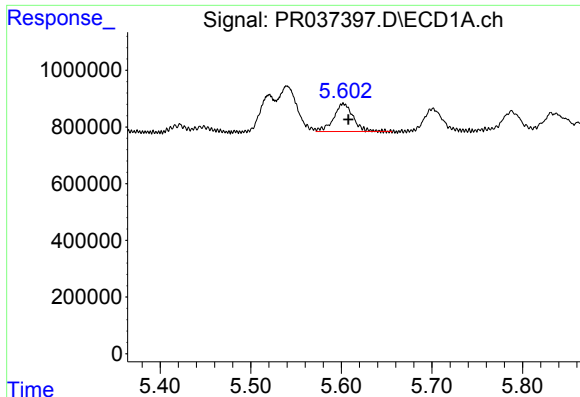

#5 AR-1016-3


R.T.: 5.602 min
Delta R.T.: -0.006 min
Response: 1460763
Conc: 36.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

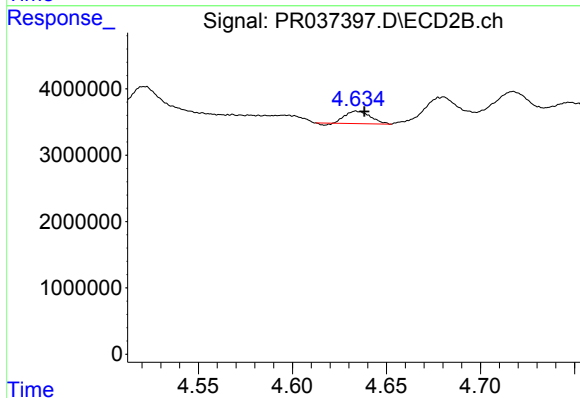


#5 AR-1016-3

R.T.: 4.634 min
Delta R.T.: -0.004 min
Response: 1679553
Conc: 11.68 ng/ml

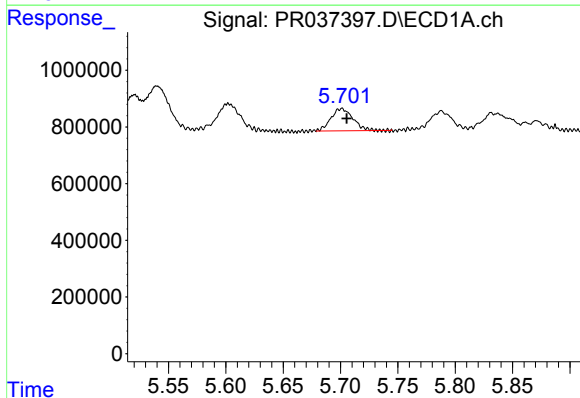


#6 AR-1016-4

R.T.: 5.701 min
Delta R.T.: -0.004 min
Response: 1044509
Conc: 31.81 ng/ml

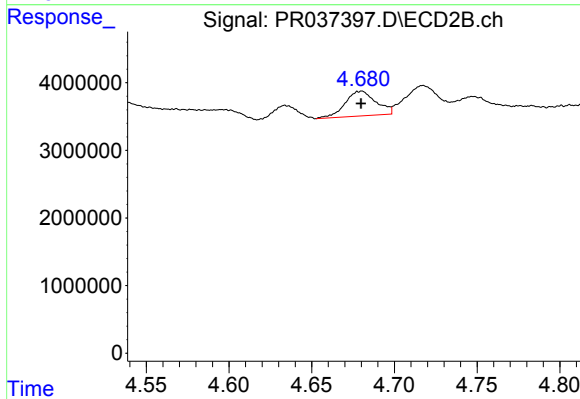

#6 AR-1016-4


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 4763526
Conc: 43.06 ng/ml

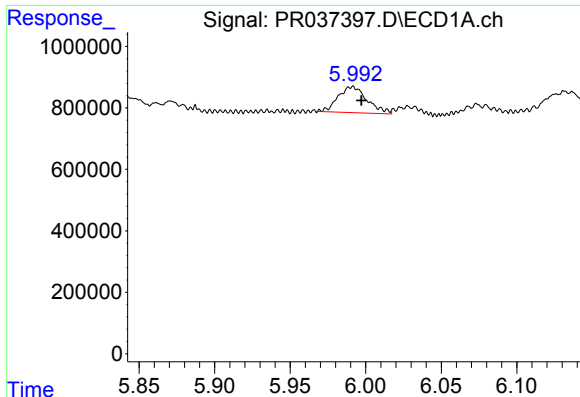

#7 AR-1016-5


R.T.: 5.991 min
Delta R.T.: -0.006 min
Response: 1135367
Conc: 33.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

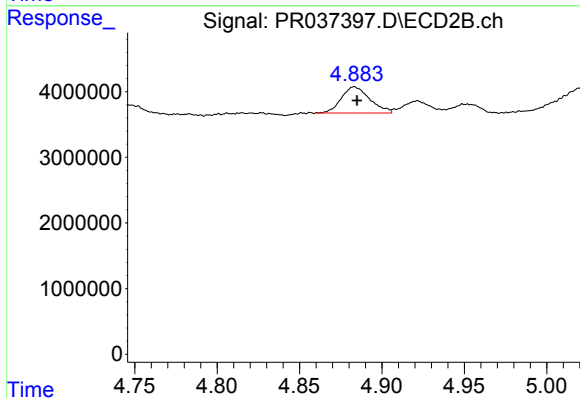


#7 AR-1016-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 4794128
Conc: 31.54 ng/ml

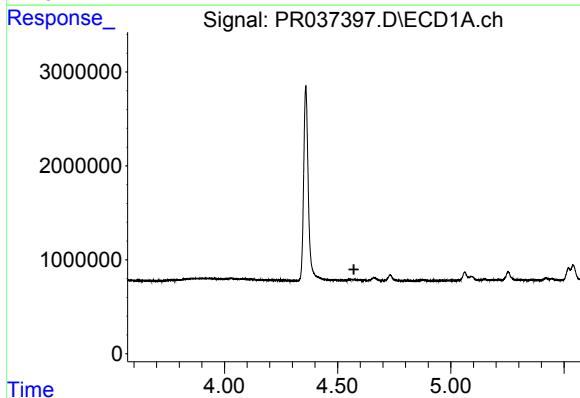


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

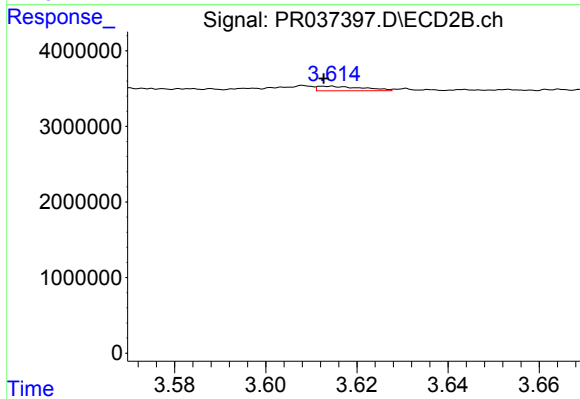

#8 AR-1221-1


R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 417274
Conc: 8.19 ng/ml

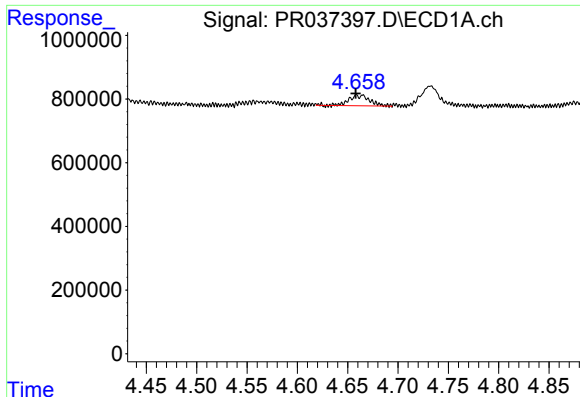

#9 AR-1221-2


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 494538
Conc: 54.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

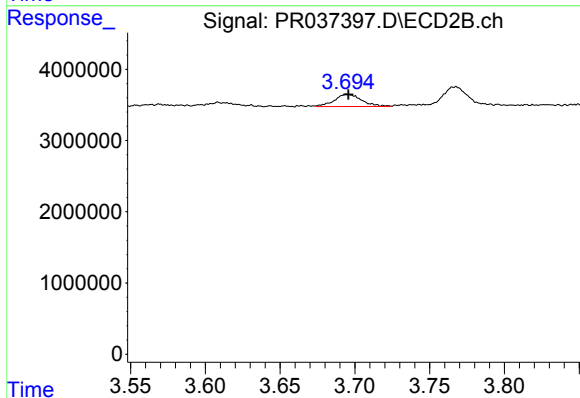


#9 AR-1221-2

R.T.: 3.695 min
Delta R.T.: 0.000 min
Response: 2181907
Conc: 58.75 ng/ml

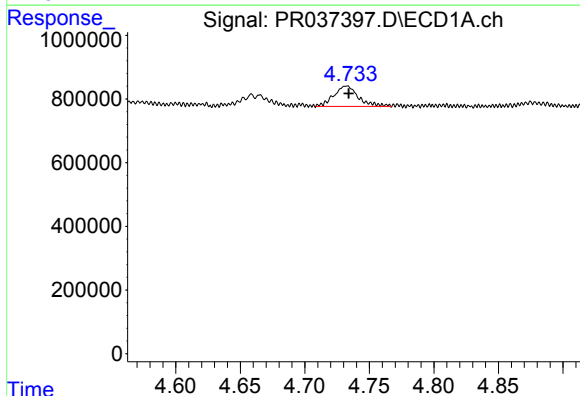


#10 AR-1221-3

R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 837811
Conc: 27.34 ng/ml

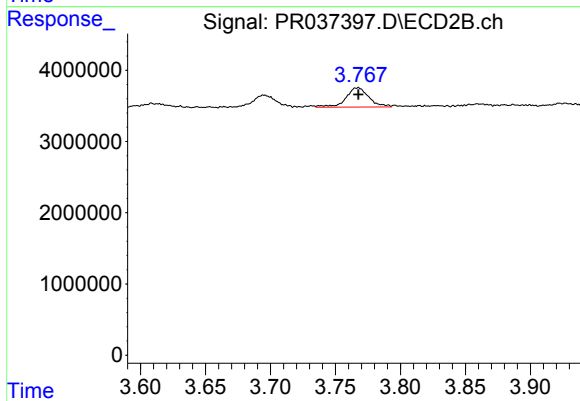

#10 AR-1221-3


R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 3326570
Conc: 27.17 ng/ml

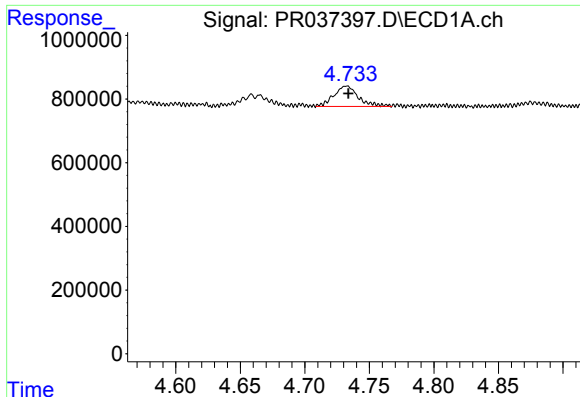

#11 AR-1232-1


R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 837811
Conc: 28.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

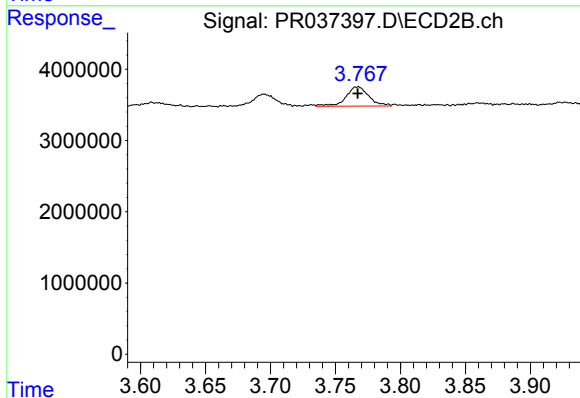


#11 AR-1232-1

R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 3326570
Conc: 28.43 ng/ml

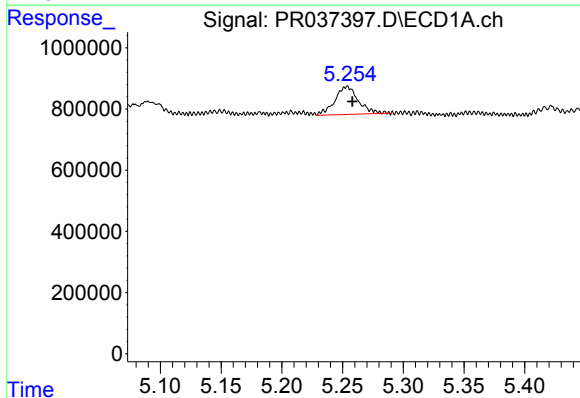


#12 AR-1232-2

R.T.: 5.254 min
Delta R.T.: -0.004 min
Response: 1223403
Conc: 72.40 ng/ml

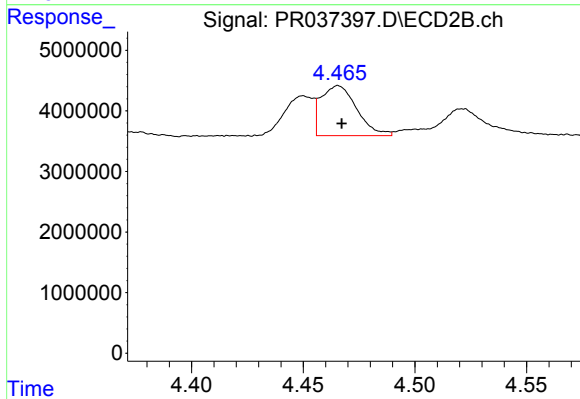

#12 AR-1232-2


R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 9211723
Conc: 66.64 ng/ml

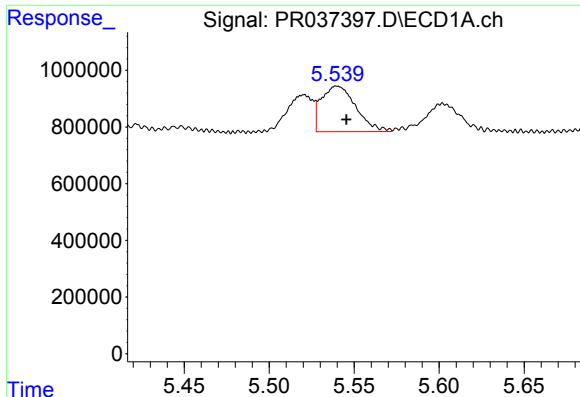

#13 AR-1232-3


R.T.: 5.540 min
Delta R.T.: -0.006 min
Response: 2284041
Conc: 67.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

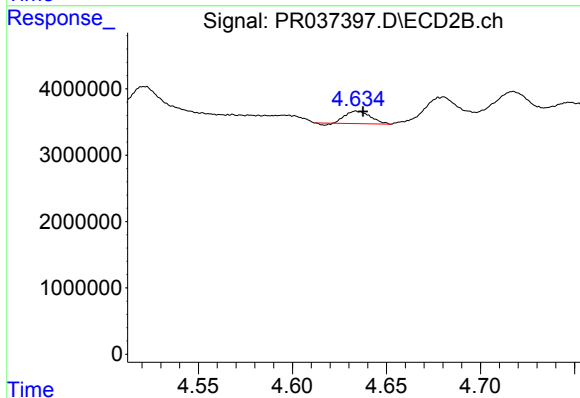


#13 AR-1232-3

R.T.: 4.634 min
Delta R.T.: -0.003 min
Response: 1679553
Conc: 23.92 ng/ml

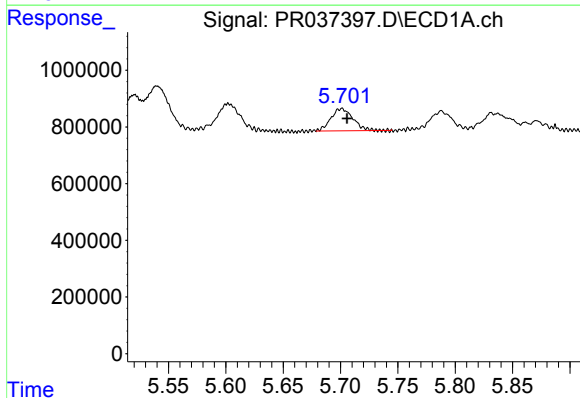


#14 AR-1232-4

R.T.: 5.701 min
Delta R.T.: -0.005 min
Response: 1044509
Conc: 66.54 ng/ml

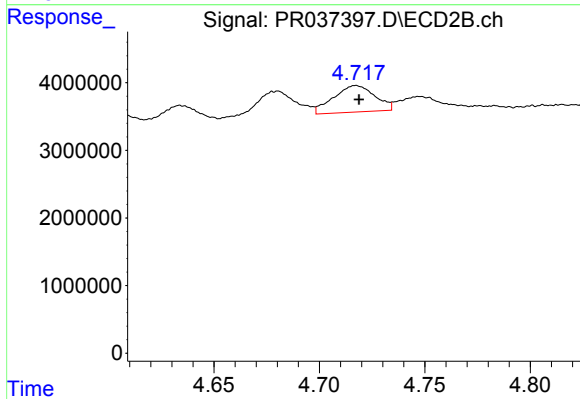

#14 AR-1232-4


R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 5343999
Conc: 89.56 ng/ml

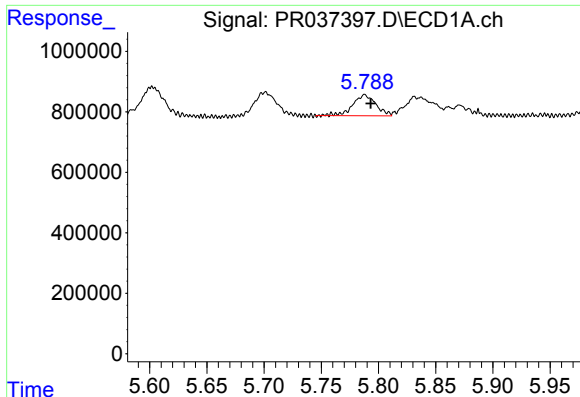

#15 AR-1232-5


R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 973273
Conc: 83.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

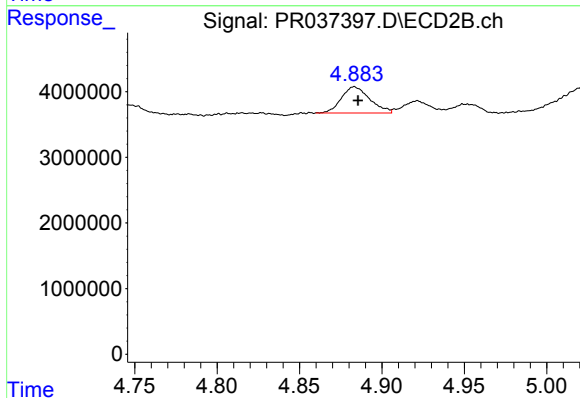


#15 AR-1232-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 4794128
Conc: 70.25 ng/ml

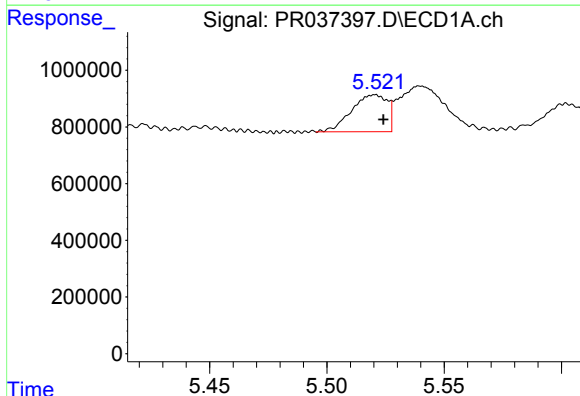


#16 AR-1242-1

R.T.: 5.520 min
Delta R.T.: -0.004 min
Response: 1373764
Conc: 40.15 ng/ml

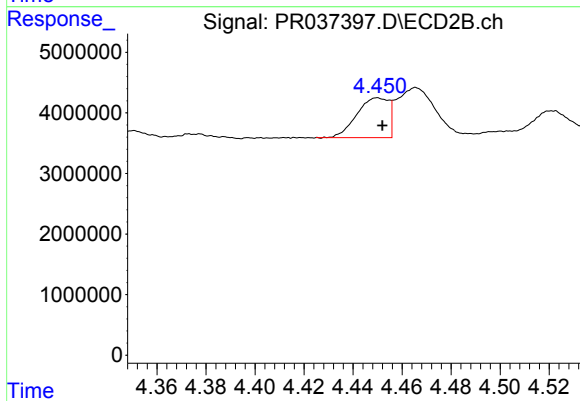

#16 AR-1242-1


R.T.: 4.450 min
Delta R.T.: -0.002 min
Response: 5895627
Conc: 40.23 ng/ml

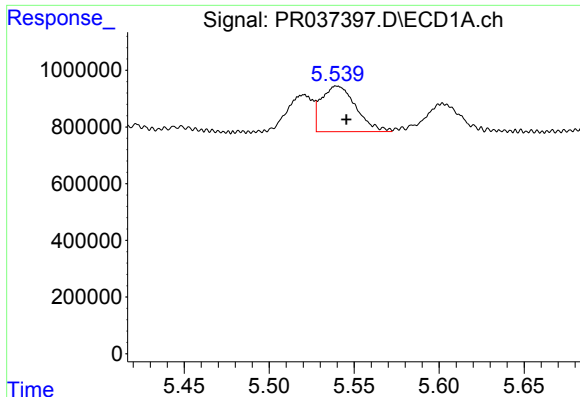

#17 AR-1242-2


R.T.: 5.540 min
Delta R.T.: -0.005 min
Response: 2284041
Conc: 41.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

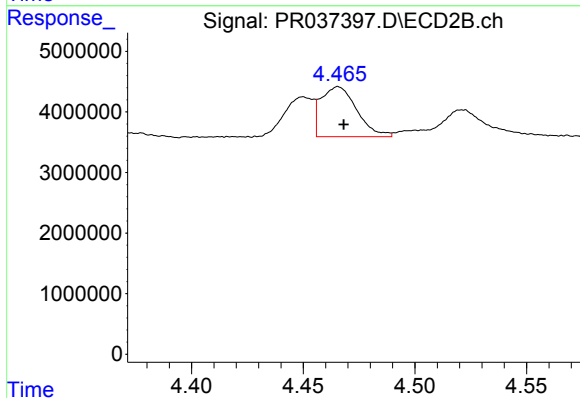


#17 AR-1242-2

R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 9211723
Conc: 40.37 ng/ml

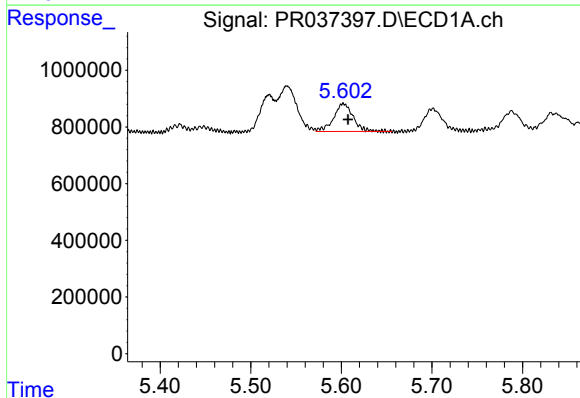


#18 AR-1242-3

R.T.: 5.602 min
Delta R.T.: -0.005 min
Response: 1460763
Conc: 44.38 ng/ml

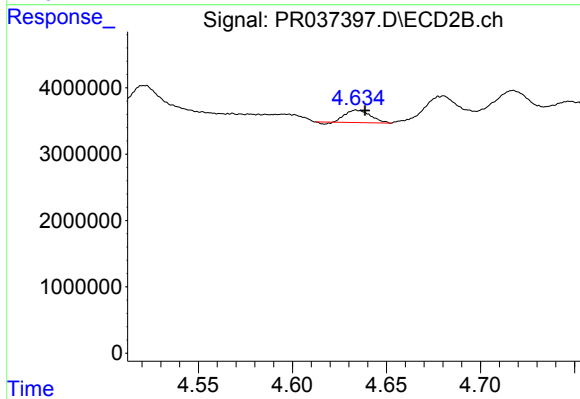

#18 AR-1242-3


R.T.: 4.634 min
Delta R.T.: -0.004 min
Response: 1679553
Conc: 14.53 ng/ml

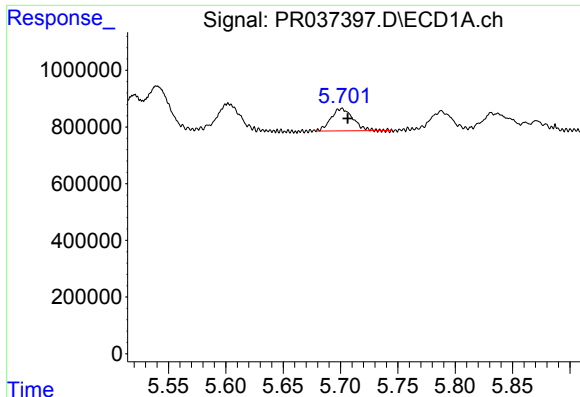

#19 AR-1242-4


R.T.: 5.701 min
Delta R.T.: -0.005 min
Response: 1044509
Conc: 39.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

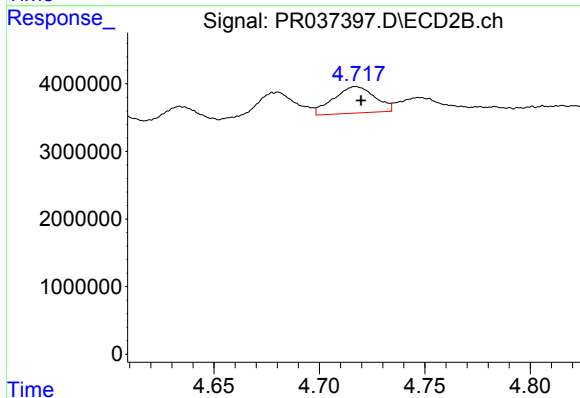


#19 AR-1242-4

R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 5343999
Conc: 48.62 ng/ml

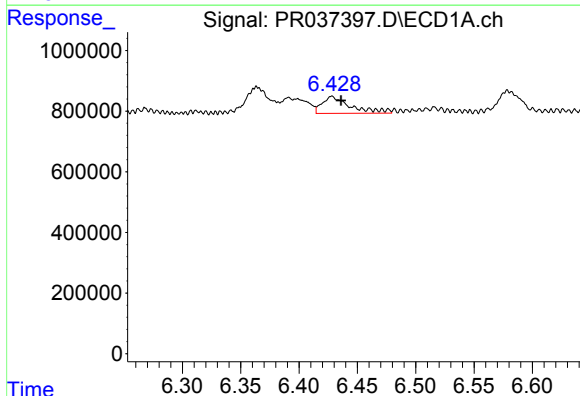


#20 AR-1242-5

R.T.: 6.428 min
Delta R.T.: -0.008 min
Response: 950784
Conc: 29.55 ng/ml

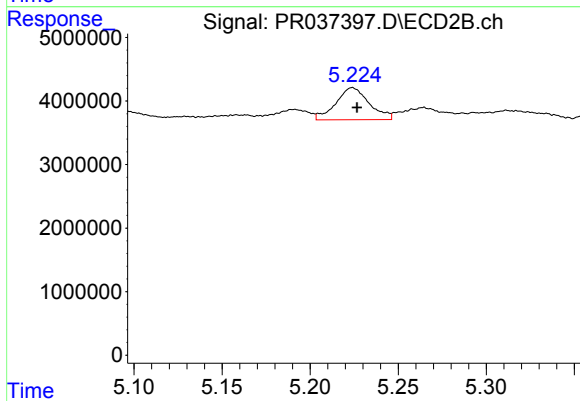

#20 AR-1242-5


R.T.: 5.224 min
Delta R.T.: -0.003 min
Response: 6672413
Conc: 40.27 ng/ml

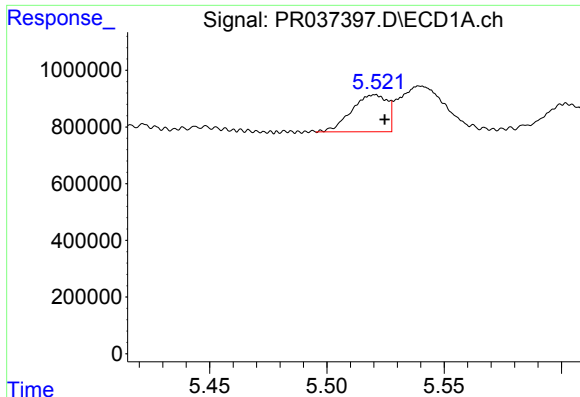

#21 AR-1248-1


R.T.: 5.520 min
Delta R.T.: -0.004 min
Response: 1373764
Conc: 59.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

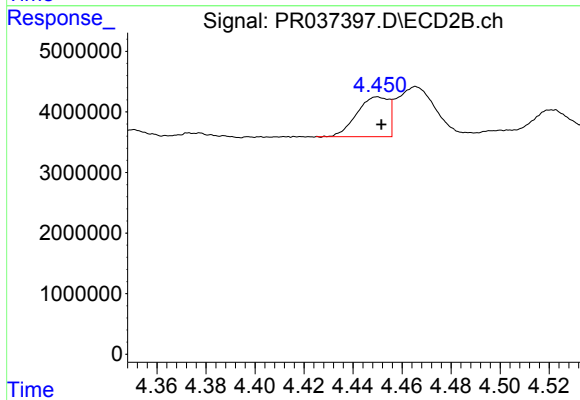


#21 AR-1248-1

R.T.: 4.450 min
Delta R.T.: -0.001 min
Response: 5895627
Conc: 58.57 ng/ml

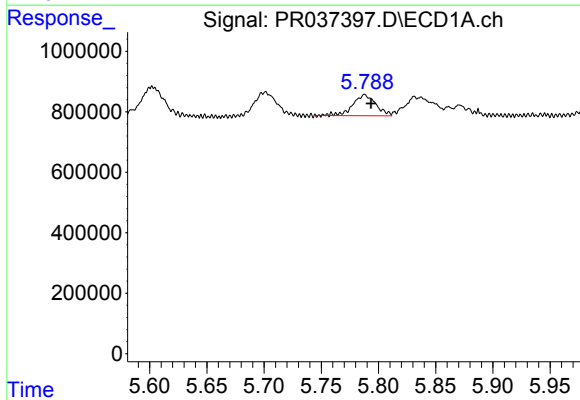


#22 AR-1248-2

R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 973273
Conc: 27.80 ng/ml

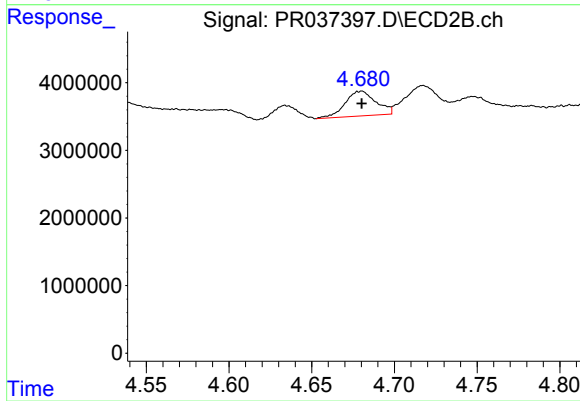

#22 AR-1248-2


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 4763526
Conc: 34.90 ng/ml

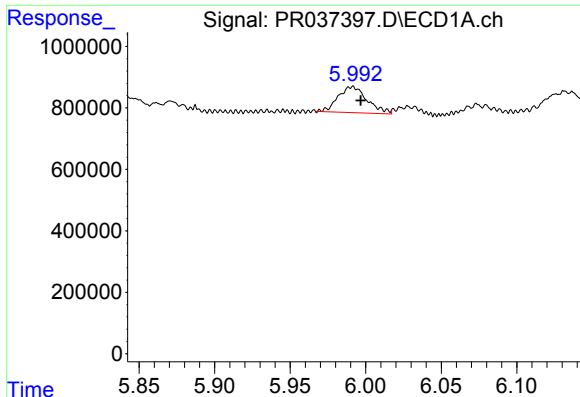

#23 AR-1248-3


R.T.: 5.991 min
Delta R.T.: -0.006 min
Response: 1135367
Conc: 27.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

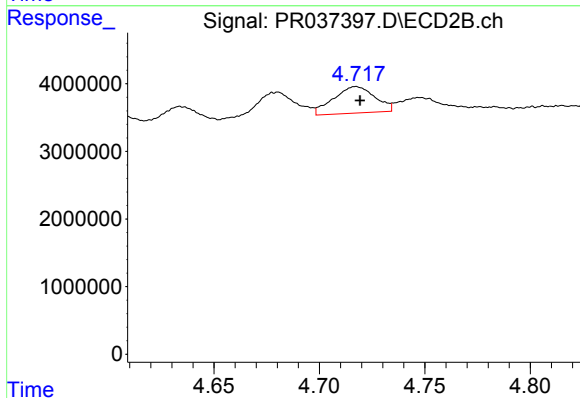


#23 AR-1248-3

R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 5343999
Conc: 38.18 ng/ml

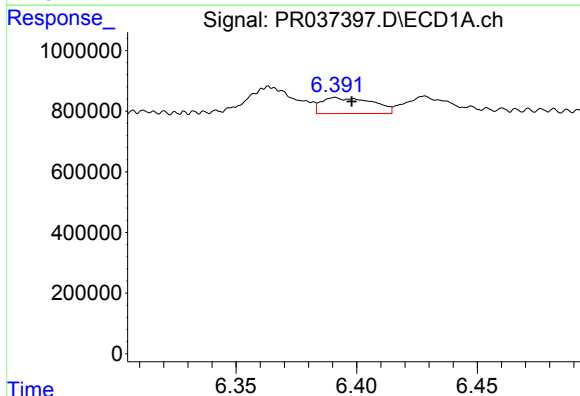


#24 AR-1248-4

R.T.: 6.391 min
Delta R.T.: -0.007 min
Response: 777954
Conc: 15.89 ng/ml

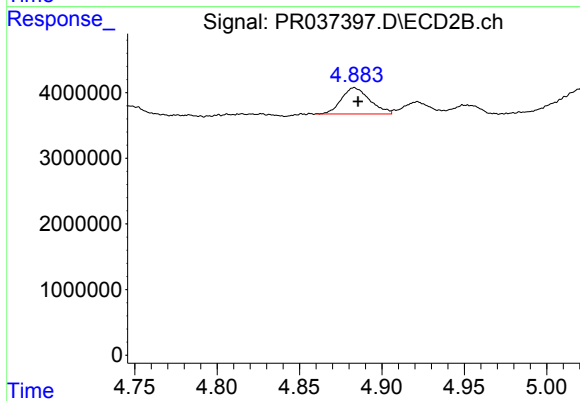

#24 AR-1248-4


R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 4794128
Conc: 26.94 ng/ml

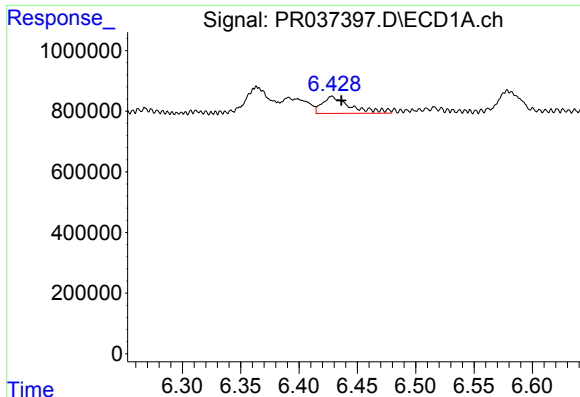

#25 AR-1248-5


R.T.: 6.428 min
Delta R.T.: -0.008 min
Response: 950784
Conc: 20.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

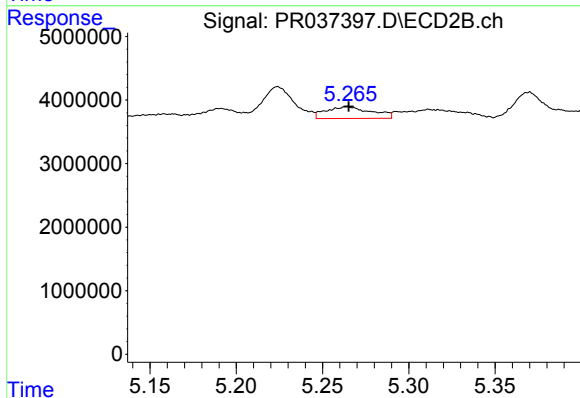


#25 AR-1248-5

R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 3403898
Conc: 17.40 ng/ml

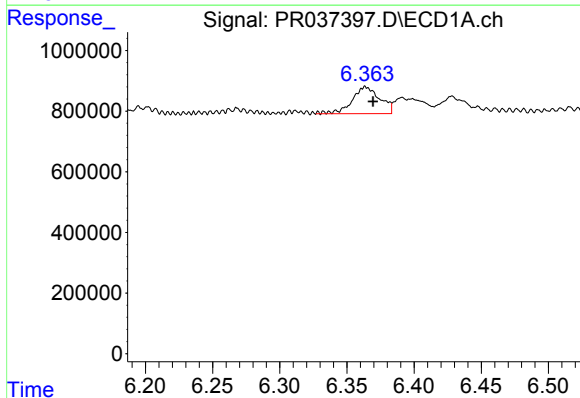


#26 AR-1254-1

R.T.: 6.364 min
Delta R.T.: -0.006 min
Response: 1267764
Conc: 23.21 ng/ml

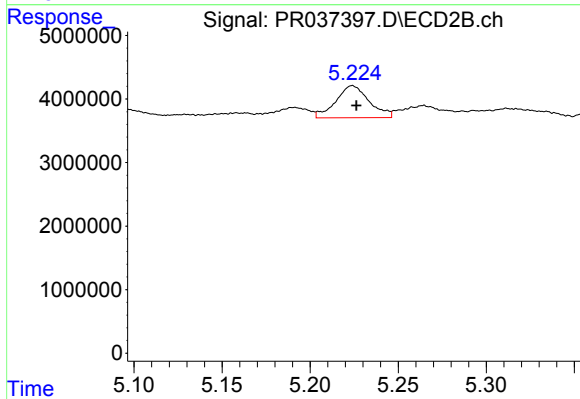

#26 AR-1254-1


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 6672413
Conc: 19.37 ng/ml

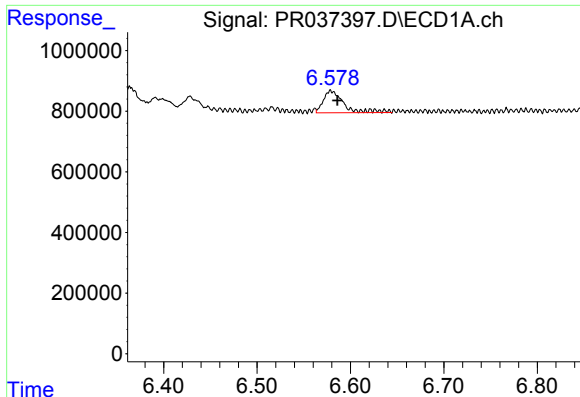

#27 AR-1254-2


R.T.: 6.579 min
Delta R.T.: -0.007 min
Response: 1102814
Conc: 12.87 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

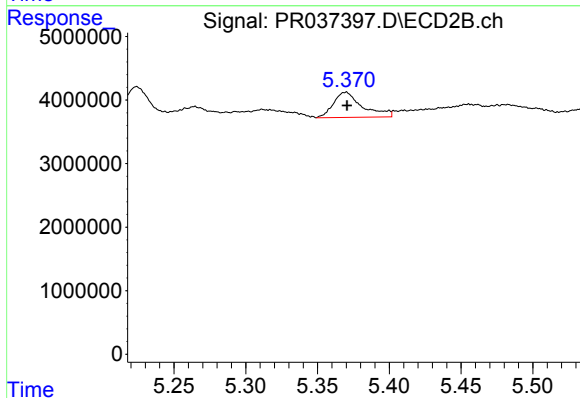


#27 AR-1254-2

R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 5591799
Conc: 18.67 ng/ml

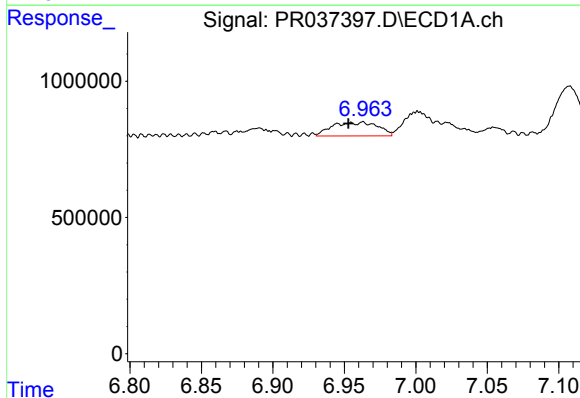


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: 0.010 min
Response: 1105488
Conc: 12.15 ng/ml

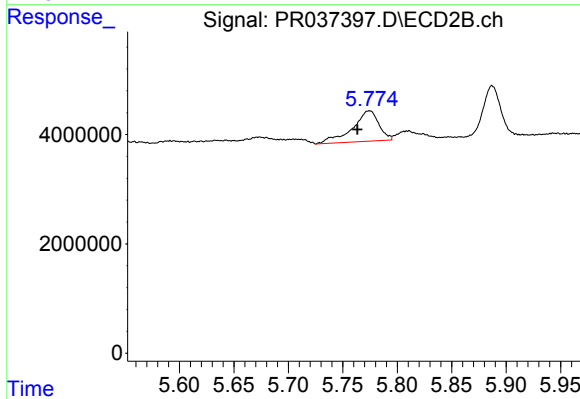

#28 AR-1254-3


R.T.: 5.774 min
Delta R.T.: 0.011 min
Response: 9455275
Conc: 19.96 ng/ml

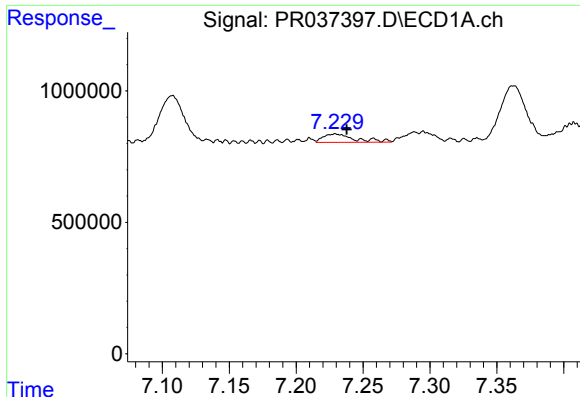

#29 AR-1254-4


R.T.: 7.229 min
Delta R.T.: -0.009 min
Response: 526604
Conc: 7.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

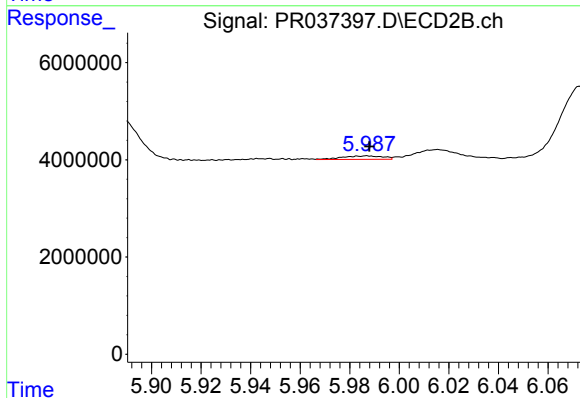


#29 AR-1254-4

R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 809553
Conc: 2.31 ng/ml

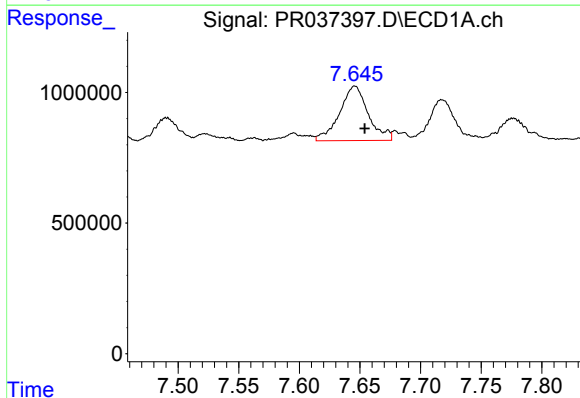


#30 AR-1254-5

R.T.: 7.646 min
Delta R.T.: -0.008 min
Response: 3431927
Conc: 47.74 ng/ml

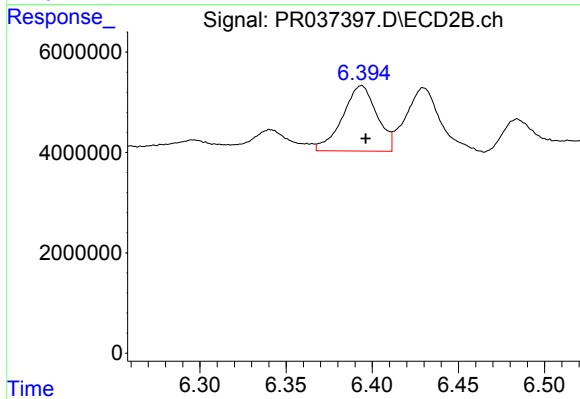

#30 AR-1254-5


R.T.: 6.394 min
Delta R.T.: -0.002 min
Response: 18082479
Conc: 40.83 ng/ml

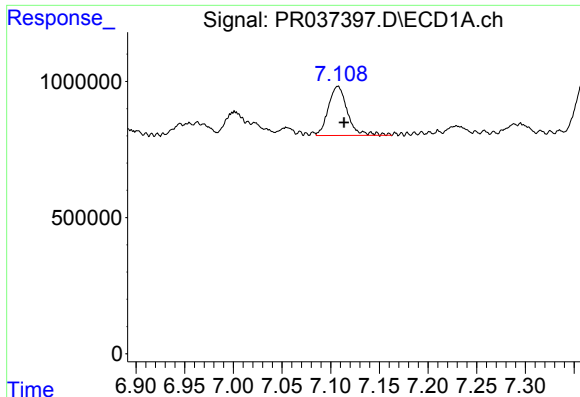

#31 AR-1260-1


R.T.: 7.107 min
Delta R.T.: -0.006 min
Response: 2451951
Conc: 37.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

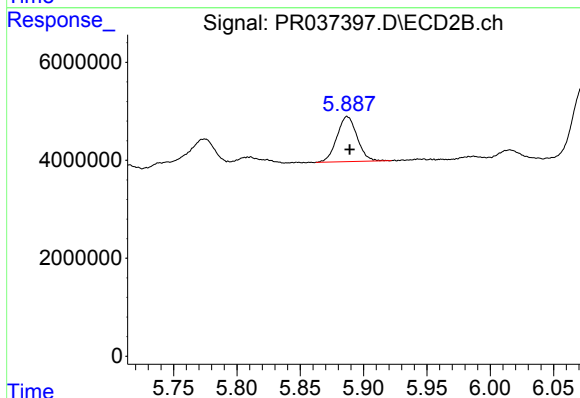


#31 AR-1260-1

R.T.: 5.887 min
Delta R.T.: -0.002 min
Response: 10214364
Conc: 34.95 ng/ml

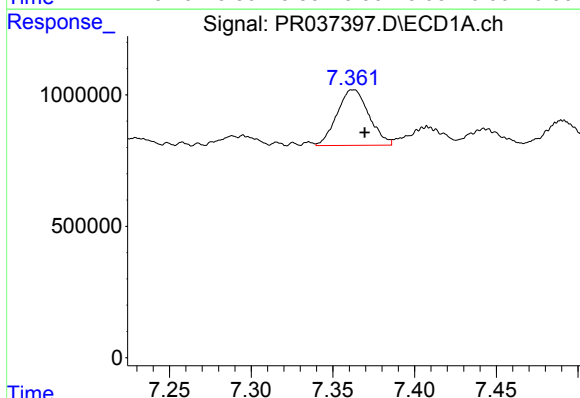


#32 AR-1260-2

R.T.: 7.362 min
Delta R.T.: -0.007 min
Response: 2876607
Conc: 36.09 ng/ml

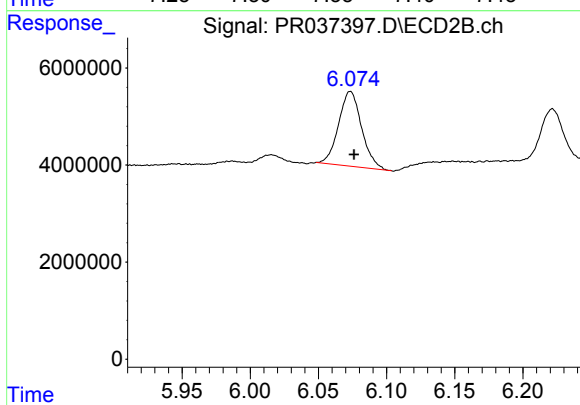

#32 AR-1260-2


R.T.: 6.073 min
Delta R.T.: -0.003 min
Response: 18042431
Conc: 39.17 ng/ml

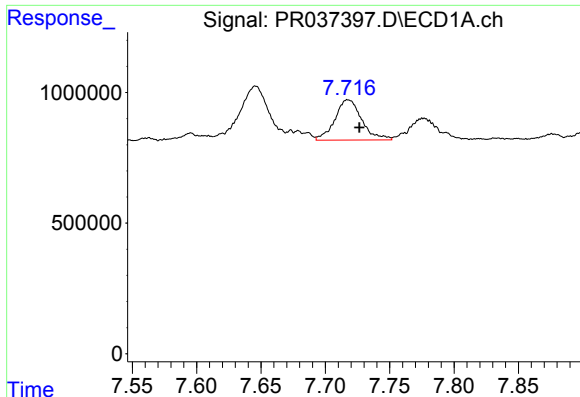

#33 AR-1260-3


R.T.: 7.718 min
Delta R.T.: -0.009 min
Response: 2236829
Conc: 35.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

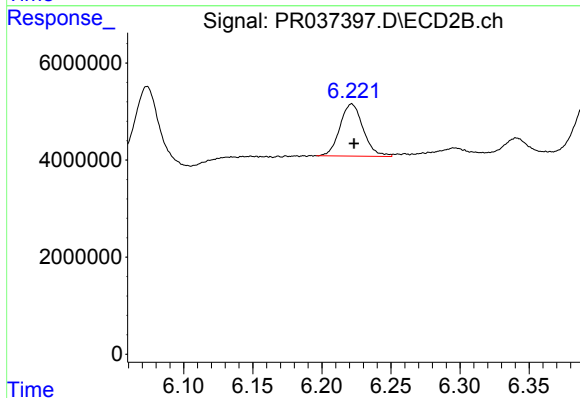


#33 AR-1260-3

R.T.: 6.222 min
Delta R.T.: -0.002 min
Response: 12563465
Conc: 35.24 ng/ml

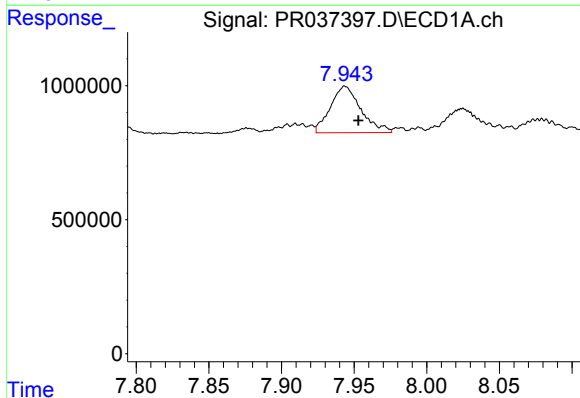


#34 AR-1260-4

R.T.: 7.944 min
Delta R.T.: -0.009 min
Response: 2536964
Conc: 34.10 ng/ml

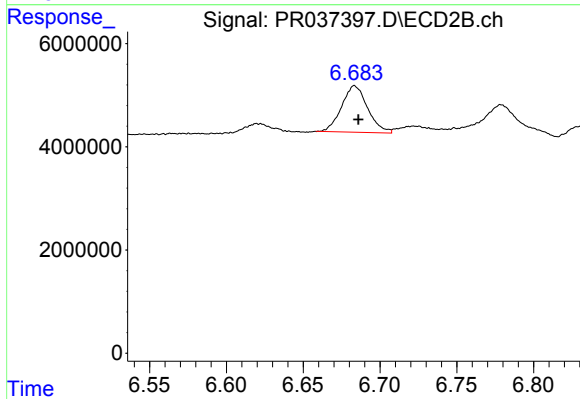

#34 AR-1260-4


R.T.: 6.684 min
Delta R.T.: -0.003 min
Response: 10619258
Conc: 34.84 ng/ml

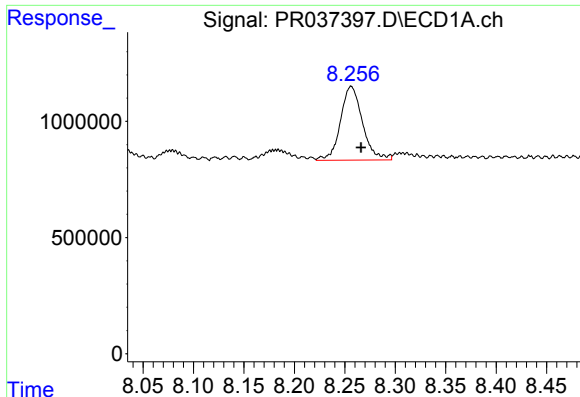

#35 AR-1260-5


R.T.: 8.256 min
Delta R.T.: -0.010 min
Response: 4839746
Conc: 33.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

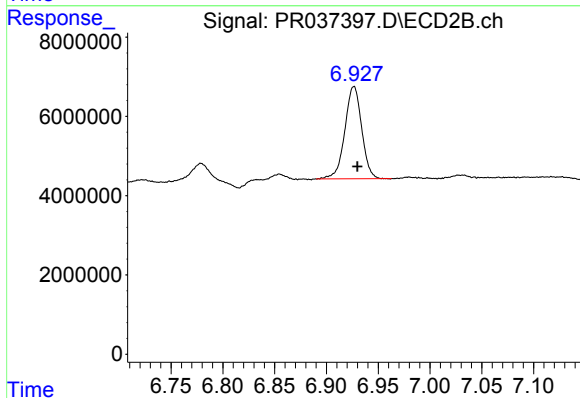


#35 AR-1260-5

R.T.: 6.927 min
Delta R.T.: -0.003 min
Response: 26309682
Conc: 30.34 ng/ml

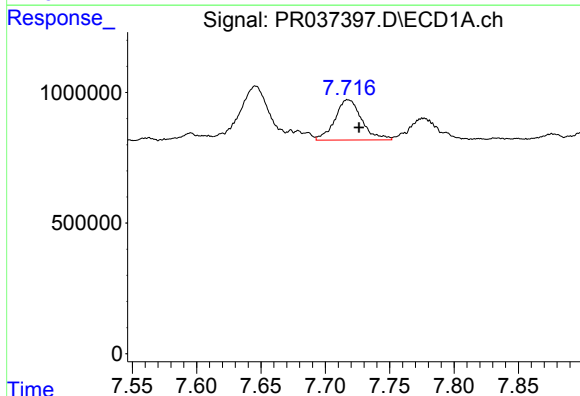


#36 AR-1262-1

R.T.: 7.718 min
Delta R.T.: -0.009 min
Response: 2236829
Conc: 21.41 ng/ml

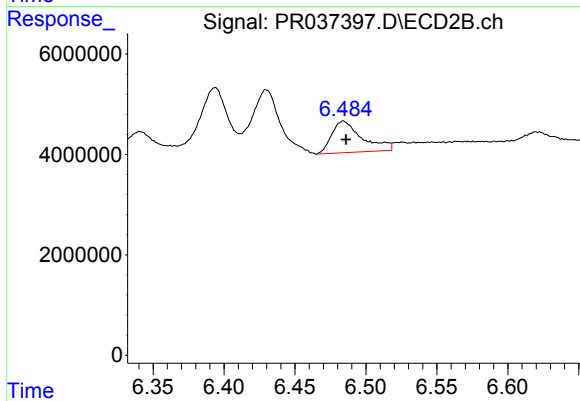

#36 AR-1262-1


R.T.: 6.484 min
Delta R.T.: -0.002 min
Response: 9366816
Conc: 37.37 ng/ml

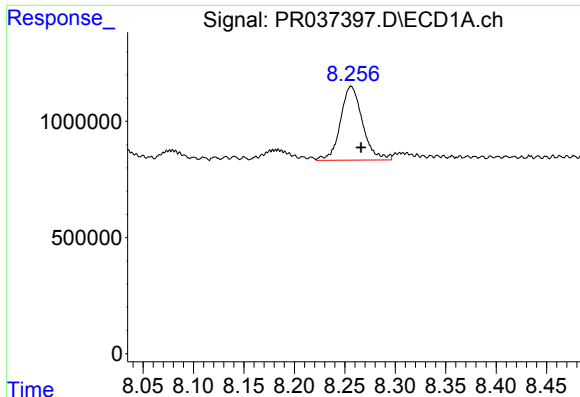

#37 AR-1262-2


R.T.: 8.256 min
Delta R.T.: -0.010 min
Response: 4839746
Conc: 24.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

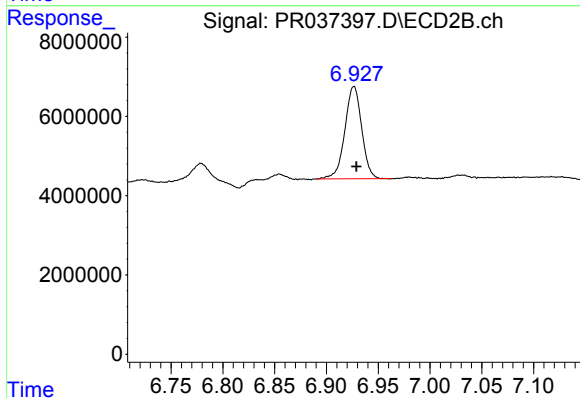


#37 AR-1262-2

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 26309682
Conc: 20.95 ng/ml

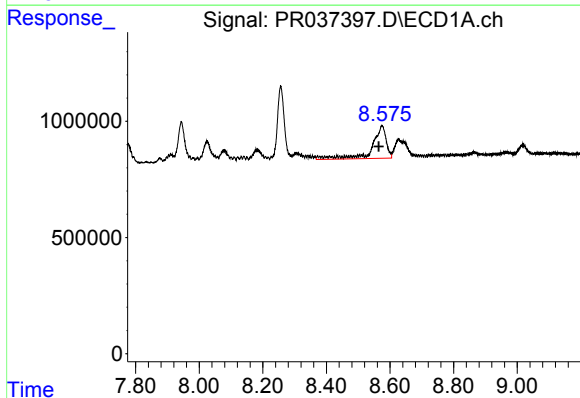


#38 AR-1262-3

R.T.: 8.575 min
Delta R.T.: 0.010 min
Response: 4284487
Conc: 32.58 ng/ml

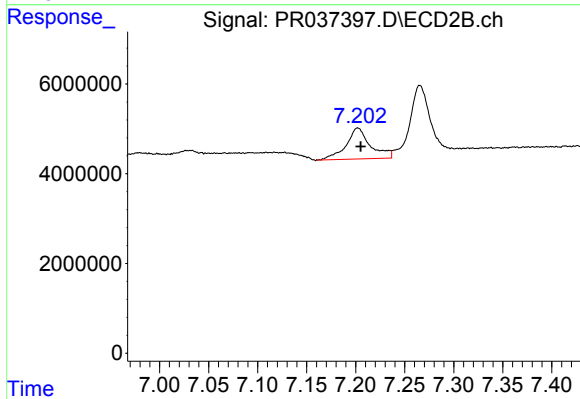

#38 AR-1262-3


R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 11964131
Conc: 21.82 ng/ml

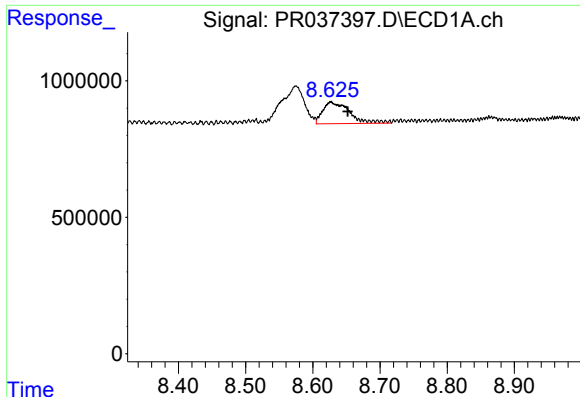

#39 AR-1262-4


R.T.: 8.627 min
Delta R.T.: -0.025 min
Response: 2228494
Conc: 22.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

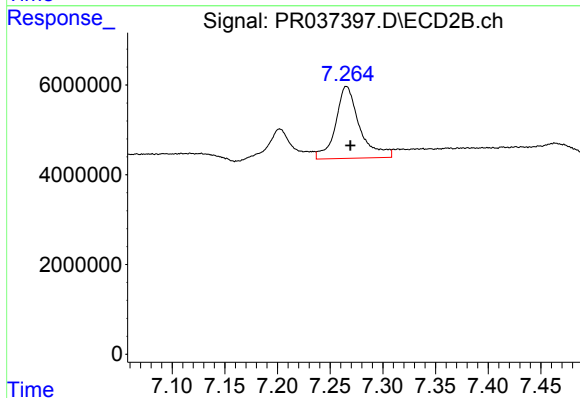


#39 AR-1262-4

R.T.: 7.266 min
Delta R.T.: -0.004 min
Response: 25434457
Conc: 28.33 ng/ml

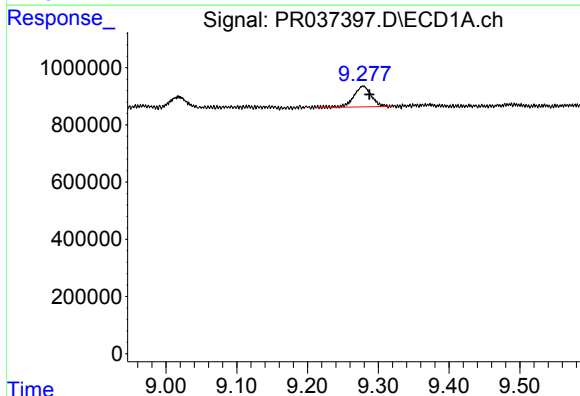


#40 AR-1262-5

R.T.: 9.278 min
Delta R.T.: -0.009 min
Response: 1249714
Conc: 18.10 ng/ml

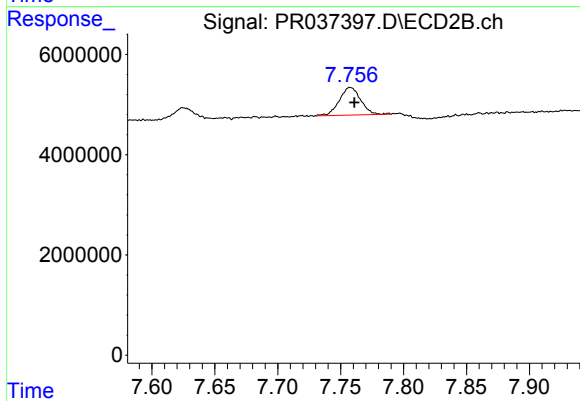

#40 AR-1262-5


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 6473647
Conc: 16.92 ng/ml

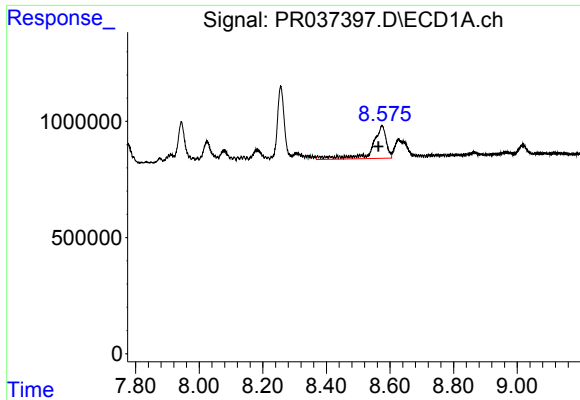

#41 AR-1268-1


R.T.: 8.575 min
Delta R.T.: 0.011 min
Response: 4284487
Conc: 23.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

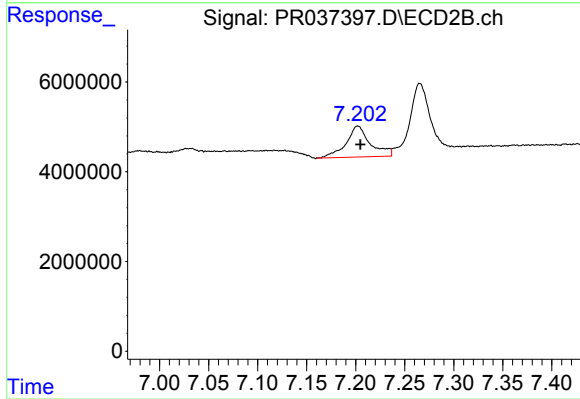


#41 AR-1268-1

R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 11964131
Conc: 9.72 ng/ml

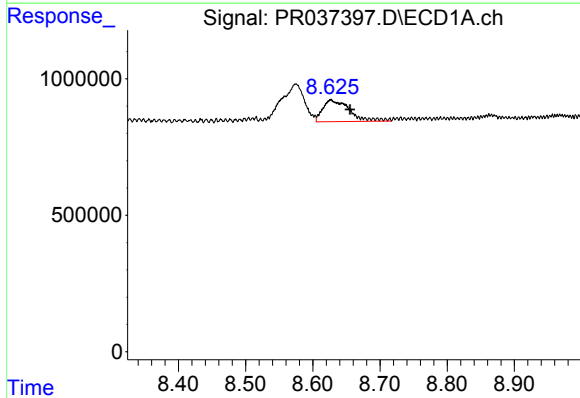


#42 AR-1268-2

R.T.: 8.627 min
Delta R.T.: -0.028 min
Response: 2228494
Conc: 13.55 ng/ml

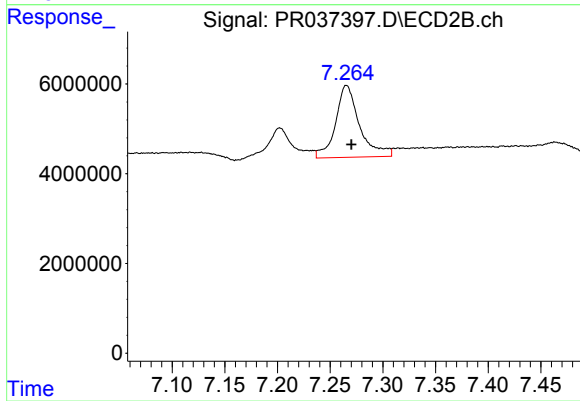

#42 AR-1268-2


R.T.: 7.266 min
Delta R.T.: -0.005 min
Response: 25434457
Conc: 24.02 ng/ml

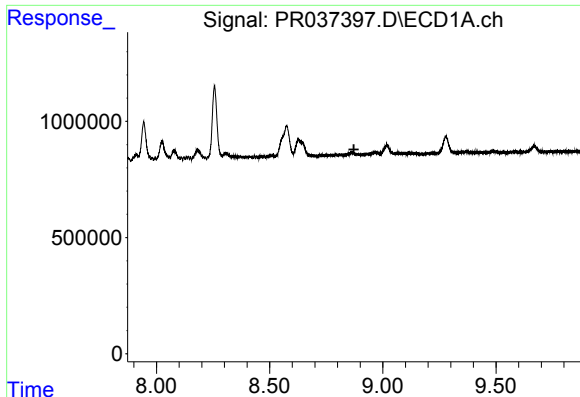

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

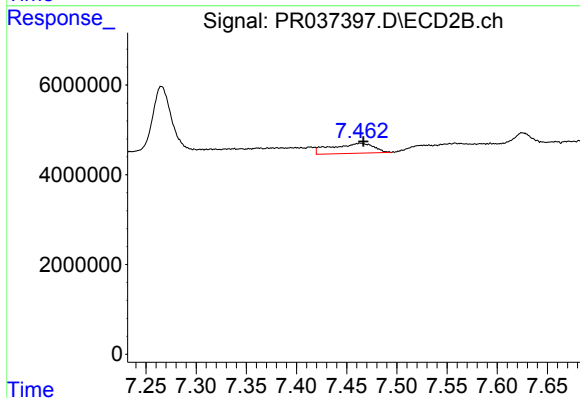


#43 AR-1268-3

R.T.: 7.463 min
Delta R.T.: -0.003 min
Response: 6509790
Conc: 7.35 ng/ml

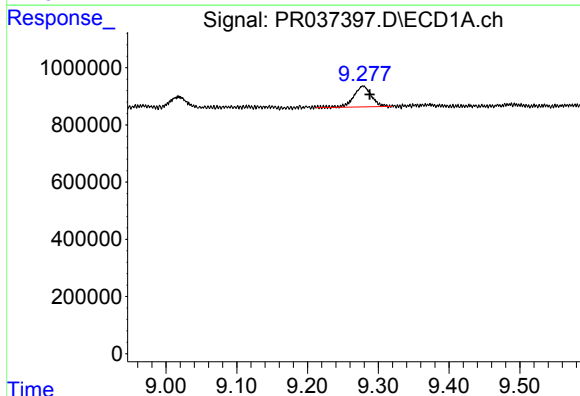


#44 AR-1268-4

R.T.: 9.278 min
Delta R.T.: -0.009 min
Response: 1249714
Conc: 20.03 ng/ml

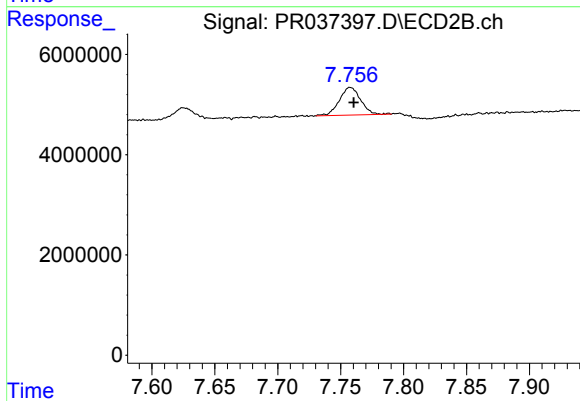

#44 AR-1268-4


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 6473647
Conc: 17.84 ng/ml

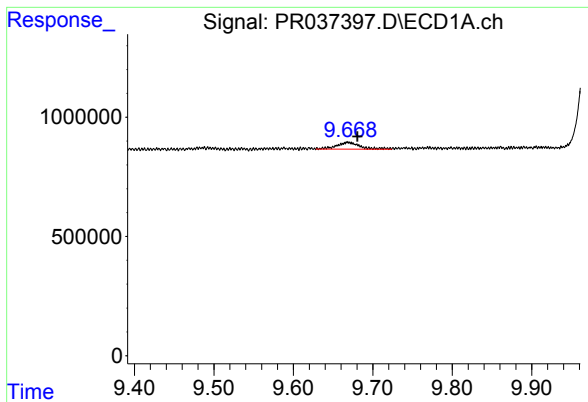

#45 AR-1268-5

R.T.: 9.668 min
Delta R.T.: -0.012 min
Response: 562669
Conc: 1.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

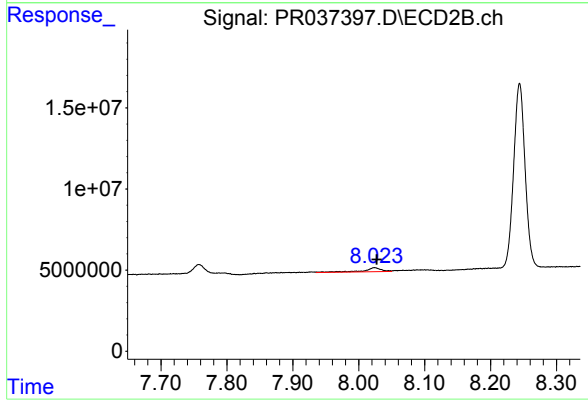

#45 AR-1268-5

R.T.: 8.024 min
Delta R.T.: -0.003 min
Response: 4395969
Conc: 1.73 ng/ml