

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
 Data File : PR037399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 15:22
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1232 MDL 25PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:41:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.357	3.406	31360117	126.4E6	25.068	26.363
2)	SA Decachlor...	9.983	8.244	29471706	145.2E6	22.283	24.928
Target Compounds							
3)	L1 AR-1016-1	5.518	4.452	462527	2319536	10.734	12.739
4)	L1 AR-1016-2	5.538	4.466	995436	3737287	14.375	13.247
5)	L1 AR-1016-3	5.599	4.636	721785	1204167	17.898	8.375 #
6)	L1 AR-1016-4	5.698	4.679	447203	1452947	13.618	13.133
7)	L1 AR-1016-5	5.991	4.884	430374	3639575	12.551	23.943 #
8)	L2 AR-1221-1	0.000	3.612	0	1451325	N.D.	28.503 #
9)	L2 AR-1221-2	4.657	3.694	760737	2447206	84.115	65.899
10)	L2 AR-1221-3	4.728	3.767	1101367	3809024	35.935	31.107
11)	L3 AR-1232-1	4.728	3.767	1101367	3809024	37.652	32.558
12)	L3 AR-1232-2	5.251	4.466	920061	3737287	54.450	27.038 #
13)	L3 AR-1232-3	5.538	4.636	995436	1204167	29.447	17.153 #
14)	L3 AR-1232-4	5.698	4.717	447203	1747476	28.490	29.285
15)	L3 AR-1232-5	5.788	4.884	398713	3639575	34.091	53.332 #
16)	L4 AR-1242-1	5.518	4.452	462527	2319536	13.518	15.829
17)	L4 AR-1242-2	5.538	4.466	995436	3737287	17.946	16.380
18)	L4 AR-1242-3	5.599	4.636	721785	1204167	21.929	10.414 #
19)	L4 AR-1242-4	5.698	4.717	447203	1747476	16.954	15.899
20)	L4 AR-1242-5	6.428	5.225	915220	6885439	28.442	41.554 #
21)	L5 AR-1248-1	5.518	4.452	462527	2319536	20.191	23.042
22)	L5 AR-1248-2	5.788	4.679	398713	1452947	11.387	10.646
23)	L5 AR-1248-3	5.991	4.717	430374	1747476	10.520	12.484
24)	L5 AR-1248-4	6.428	4.884	915220	3639575	18.695	20.451
25)	L5 AR-1248-5	6.428	5.247	915220	16718875	19.375	85.469 #
26)	L6 AR-1254-1	6.365	5.225	2602292	6885439	47.634	19.988 #
27)	L6 AR-1254-2	6.587	5.368	444596	12592776	5.188	42.046 #
28)	L6 AR-1254-3	6.964	5.761	1973382	5454978	21.694	11.518 #
29)	L6 AR-1254-4	7.240	5.987	154339	727646	2.303	2.075
30)	L6 AR-1254-5	0.000	6.392	0	3738461	N.D.	8.442 #
31)	L7 AR-1260-1	7.122	5.894	413182	66479	6.262	0.227 #
32)	L7 AR-1260-2	0.000	6.066	0	4234455	N.D.	9.194 #
33)	L7 AR-1260-3	0.000	6.215	0	187825	N.D.	0.527 #
34)	L7 AR-1260-4	0.000	6.689	0	458230	N.D.	1.504 #
35)	L7 AR-1260-5	0.000	6.926	0	159931	N.D.	0.184 #
36)	L8 AR-1262-1	0.000	6.493	0	2512745	N.D.	10.026 #
37)	L8 AR-1262-2	0.000	6.926	0	159931	N.D.	0.127 #
38)	L8 AR-1262-3	0.000	7.247	0	6065319	N.D.	11.063 #
39)	L8 AR-1262-4	0.000	7.247	0	6065319	N.D.	6.757 #
40)	L8 AR-1262-5	0.000	7.778	0	647870	N.D.	1.693 #
41)	L9 AR-1268-1	0.000	7.247	0	6065319	N.D.	4.927 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
Data File : PR037399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 15:22
Operator : SM\SJ
Sample : K2241-09
Misc : AR1232 MDL 25PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 00:41:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.247	0	6065319	N.D.	5.728 #
43)	L9 AR-1268-3	0.000	7.463	0	6894920	N.D.	7.780 #
44)	L9 AR-1268-4	0.000	7.778	0	647870	N.D.	1.786 #
45)	L9 AR-1268-5	0.000	8.025	0	6039799	N.D.	2.374 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-OT2-2019

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

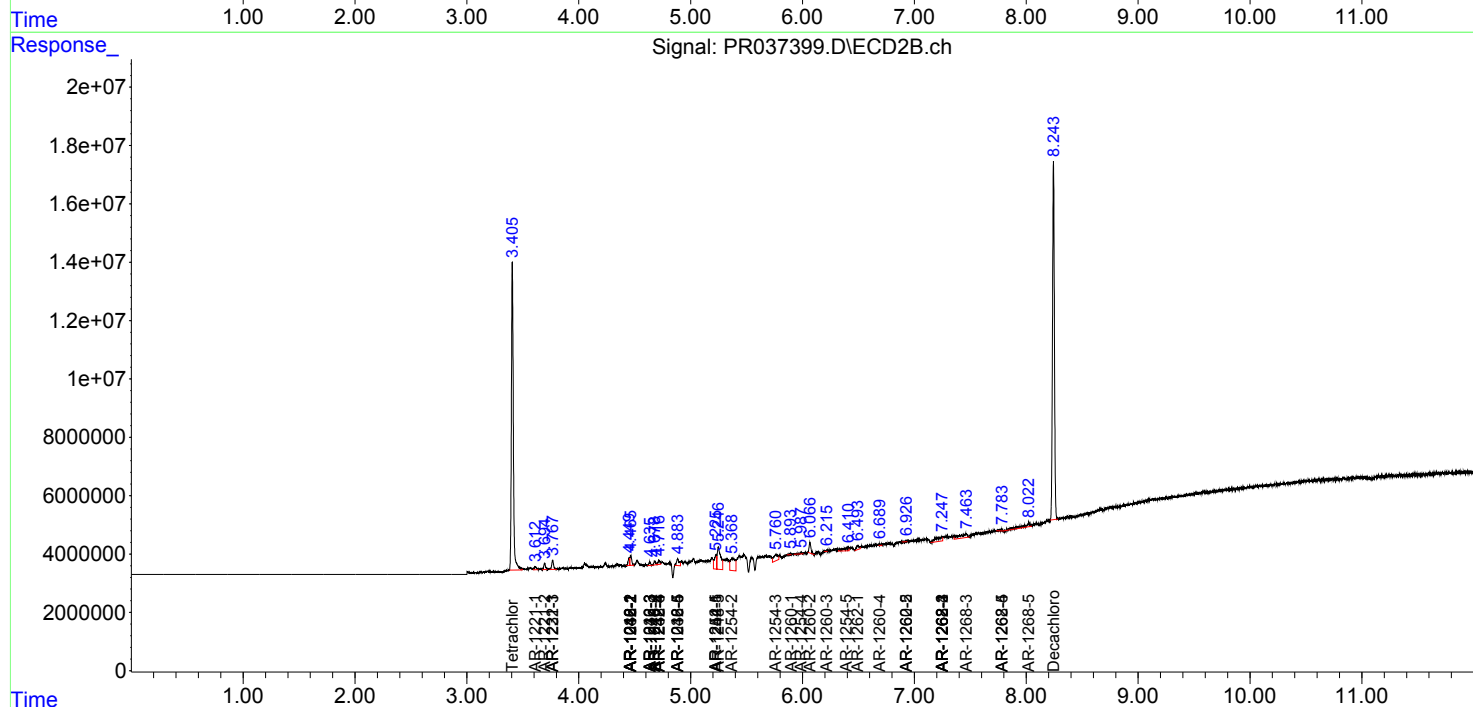


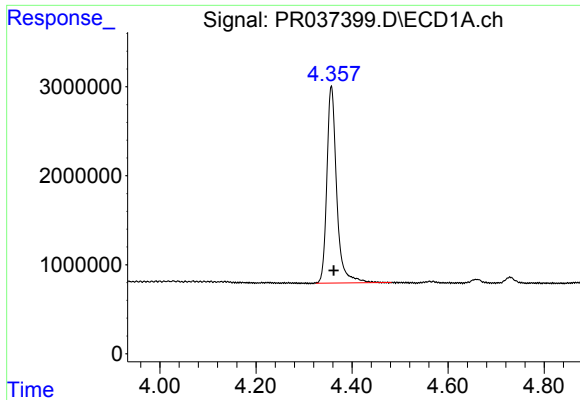

#1 Tetrachloro-m-xylene


R.T.: 4.357 min
Delta R.T.: -0.005 min
Response: 31360117
Conc: 25.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

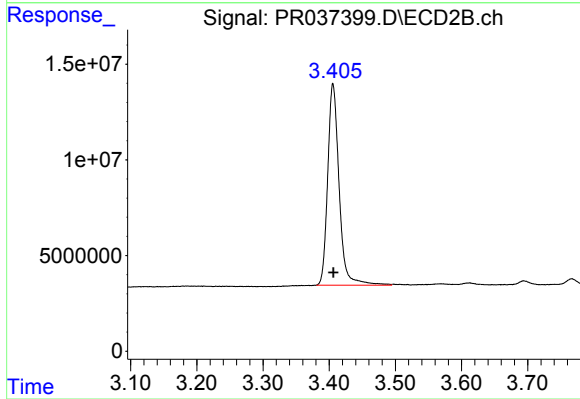


#1 Tetrachloro-m-xylene

R.T.: 3.406 min
Delta R.T.: 0.000 min
Response: 126423743
Conc: 26.36 ng/ml

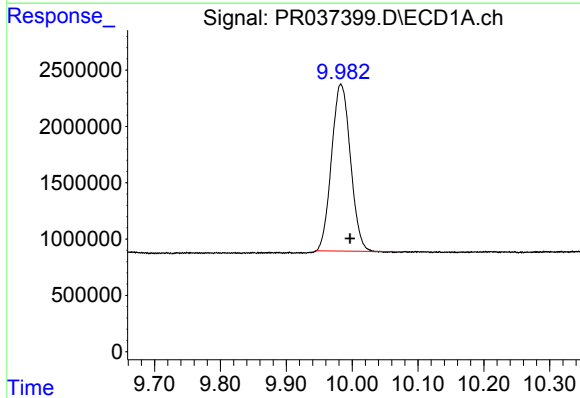


#2 Decachlorobiphenyl

R.T.: 9.983 min
Delta R.T.: -0.014 min
Response: 29471706
Conc: 22.28 ng/ml

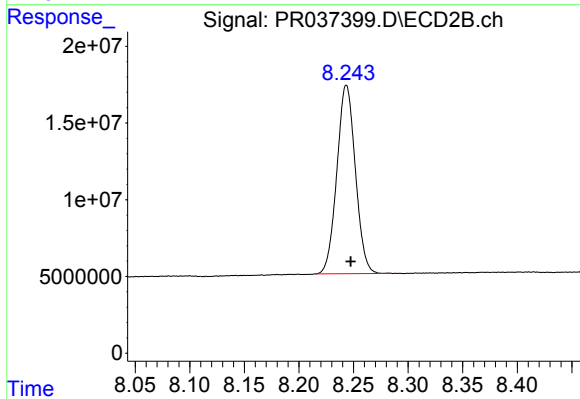

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 145185822
Conc: 24.93 ng/ml

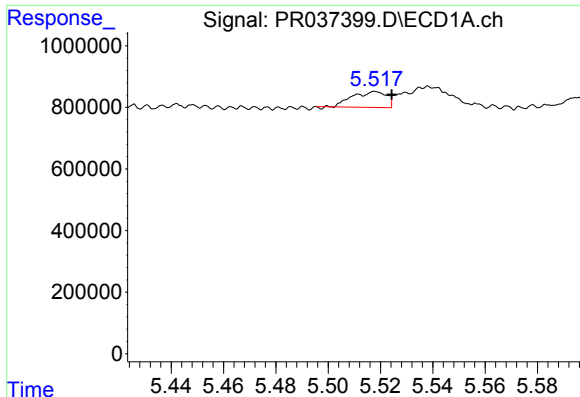

#3 AR-1016-1


R.T.: 5.518 min
Delta R.T.: -0.006 min
Response: 462527
Conc: 10.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

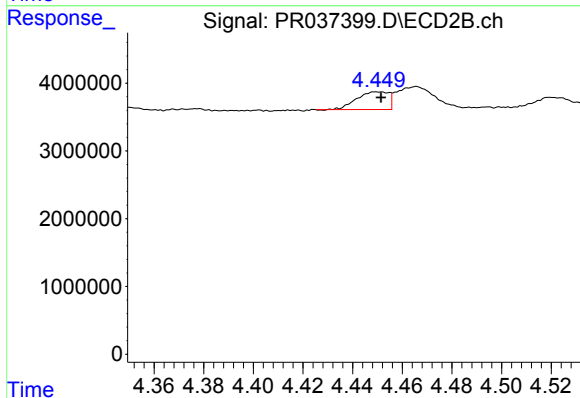


#3 AR-1016-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2319536
Conc: 12.74 ng/ml

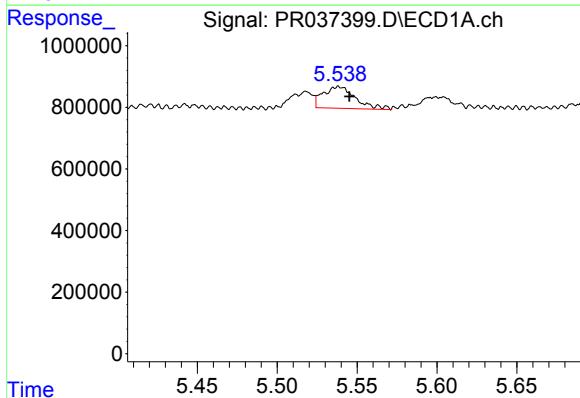


#4 AR-1016-2

R.T.: 5.538 min
Delta R.T.: -0.007 min
Response: 995436
Conc: 14.38 ng/ml

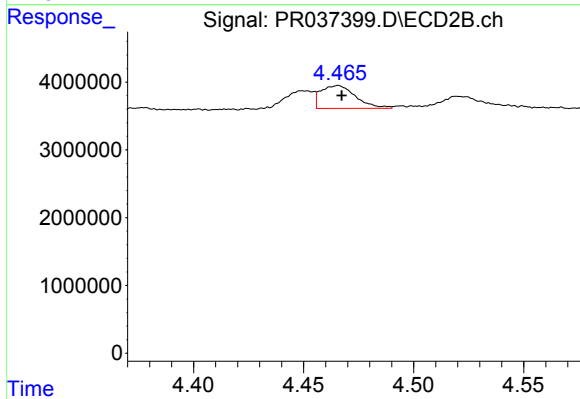

#4 AR-1016-2


R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 3737287
Conc: 13.25 ng/ml

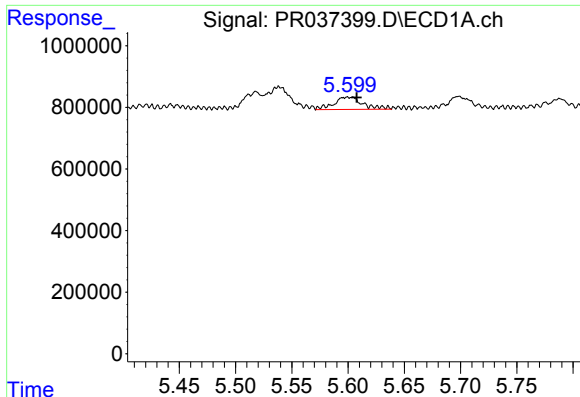

#5 AR-1016-3


R.T.: 5.599 min
Delta R.T.: -0.008 min
Response: 721785
Conc: 17.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

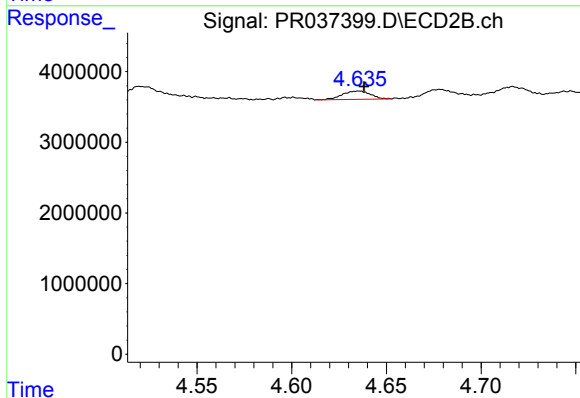


#5 AR-1016-3

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 1204167
Conc: 8.37 ng/ml

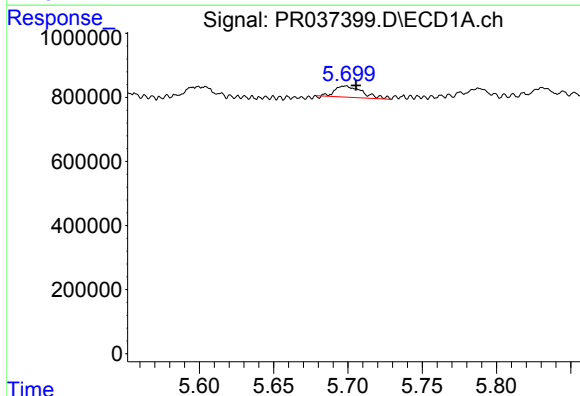


#6 AR-1016-4

R.T.: 5.698 min
Delta R.T.: -0.007 min
Response: 447203
Conc: 13.62 ng/ml

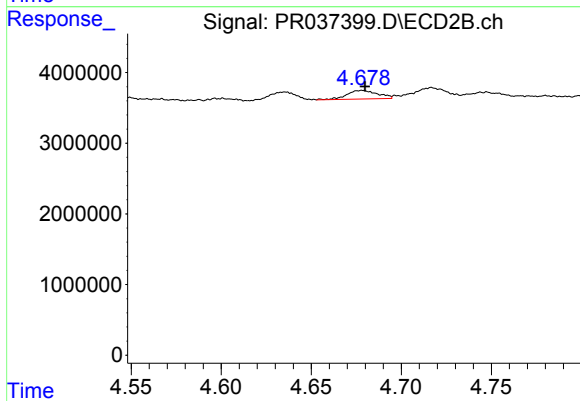

#6 AR-1016-4


R.T.: 4.679 min
Delta R.T.: -0.001 min
Response: 1452947
Conc: 13.13 ng/ml

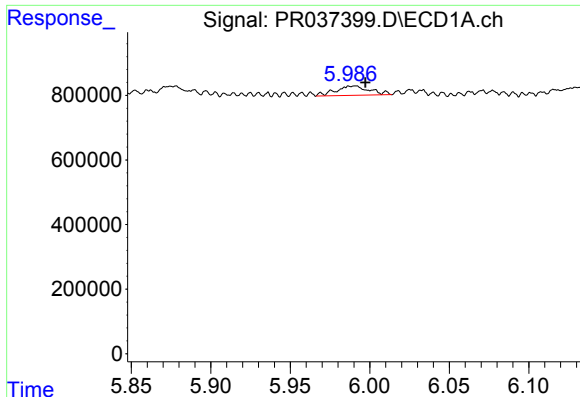

#7 AR-1016-5


R.T.: 5.991 min
Delta R.T.: -0.007 min
Response: 430374
Conc: 12.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

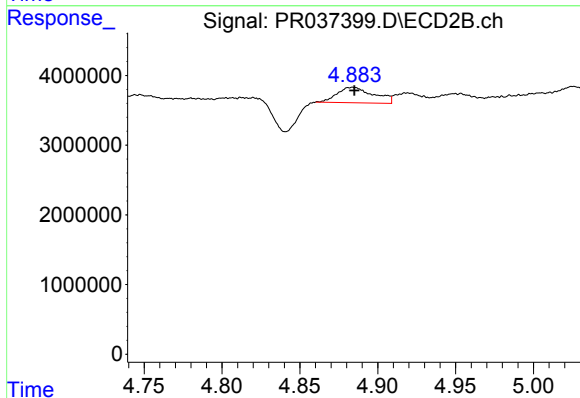


#7 AR-1016-5

R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 3639575
Conc: 23.94 ng/ml

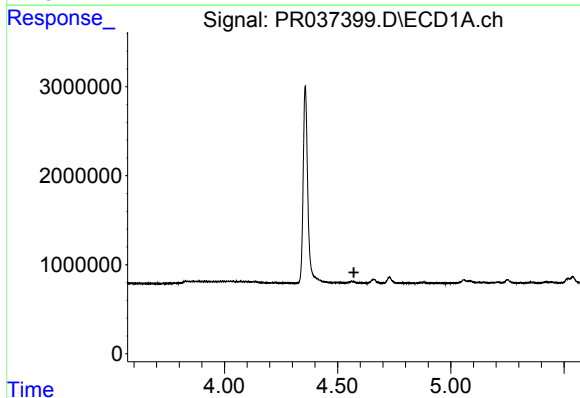


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

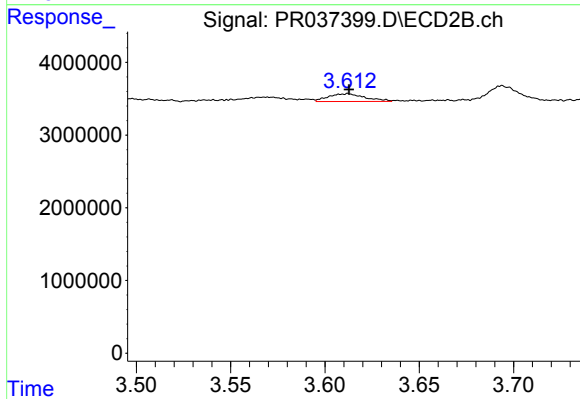

#8 AR-1221-1


R.T.: 3.612 min
Delta R.T.: 0.000 min
Response: 1451325
Conc: 28.50 ng/ml

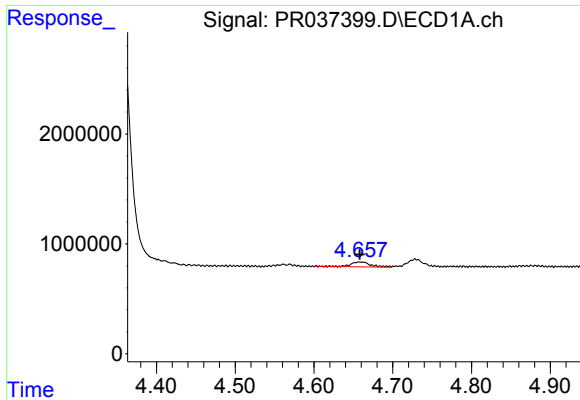

#9 AR-1221-2


R.T.: 4.657 min
Delta R.T.: 0.000 min
Response: 760737
Conc: 84.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

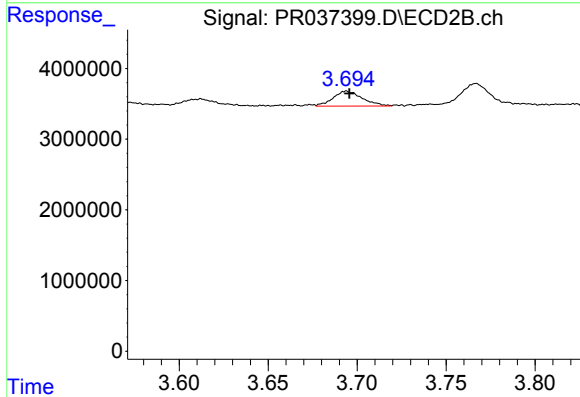


#9 AR-1221-2

R.T.: 3.694 min
Delta R.T.: -0.002 min
Response: 2447206
Conc: 65.90 ng/ml

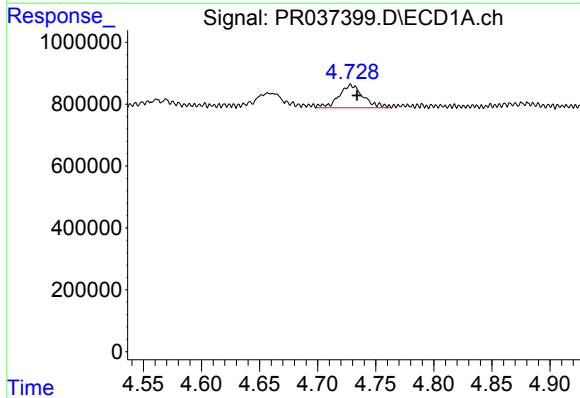


#10 AR-1221-3

R.T.: 4.728 min
Delta R.T.: -0.005 min
Response: 1101367
Conc: 35.93 ng/ml

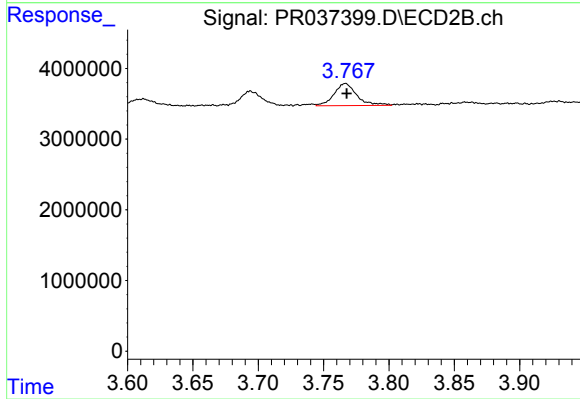

#10 AR-1221-3


R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 3809024
Conc: 31.11 ng/ml

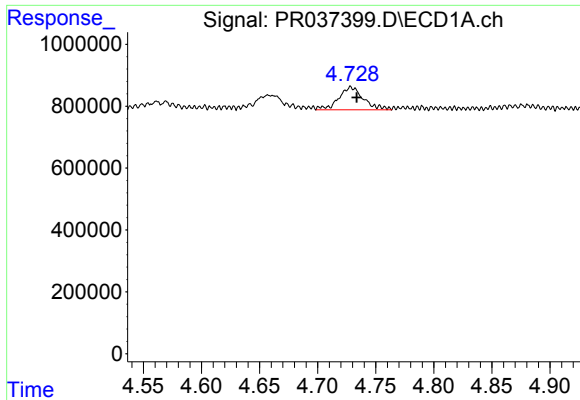

#11 AR-1232-1


R.T.: 4.728 min
Delta R.T.: -0.005 min
Response: 1101367
Conc: 37.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

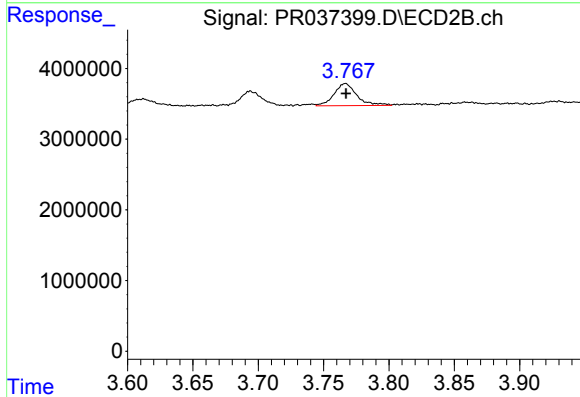


#11 AR-1232-1

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 3809024
Conc: 32.56 ng/ml

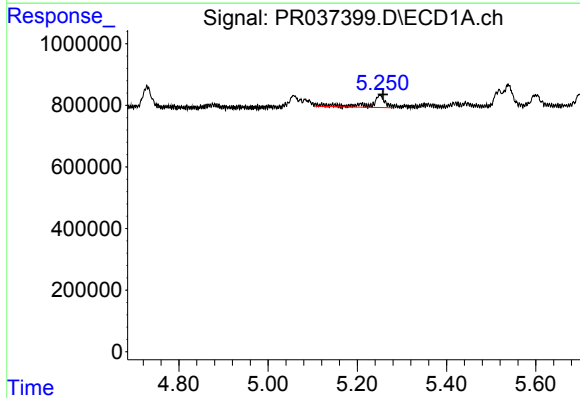


#12 AR-1232-2

R.T.: 5.251 min
Delta R.T.: -0.007 min
Response: 920061
Conc: 54.45 ng/ml

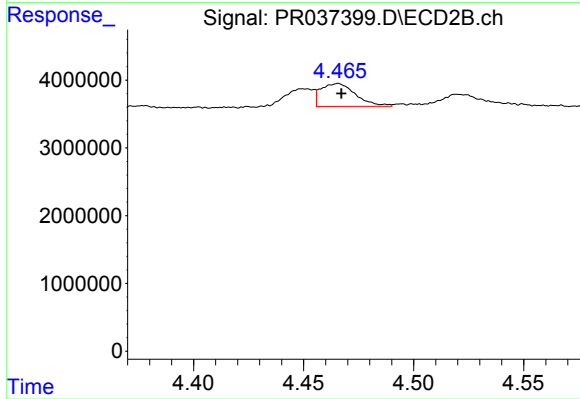

#12 AR-1232-2


R.T.: 4.466 min
Delta R.T.: -0.001 min
Response: 3737287
Conc: 27.04 ng/ml

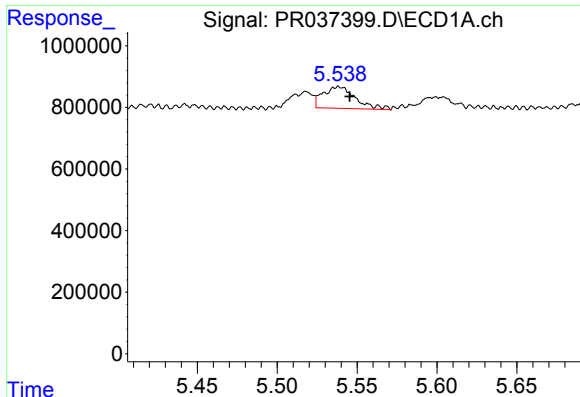

#13 AR-1232-3


R.T.: 5.538 min
Delta R.T.: -0.007 min
Response: 995436
Conc: 29.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

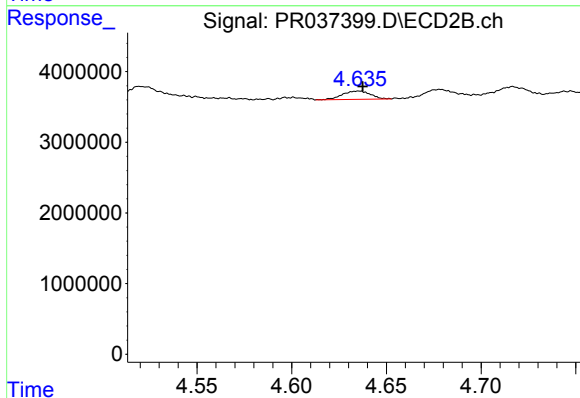


#13 AR-1232-3

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 1204167
Conc: 17.15 ng/ml

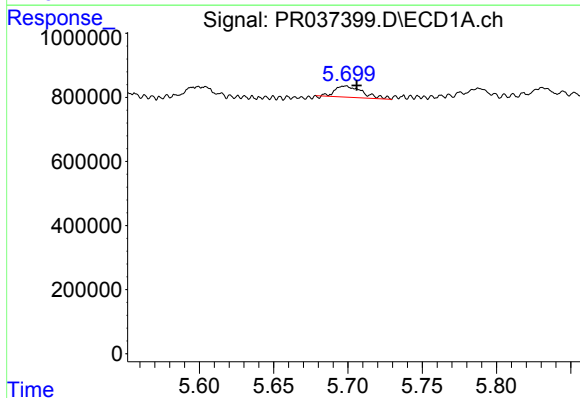


#14 AR-1232-4

R.T.: 5.698 min
Delta R.T.: -0.008 min
Response: 447203
Conc: 28.49 ng/ml

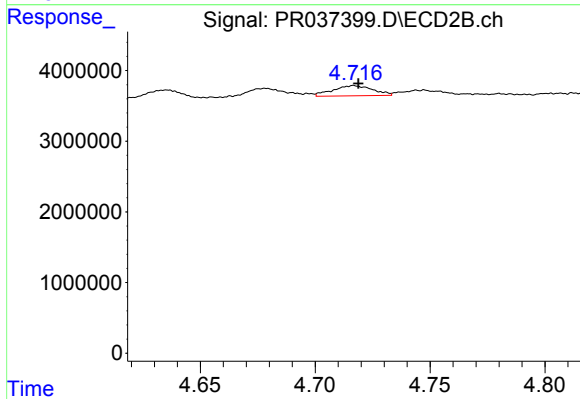

#14 AR-1232-4


R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 1747476
Conc: 29.28 ng/ml

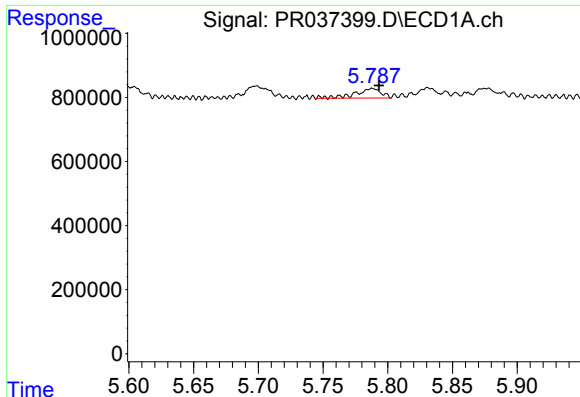

#15 AR-1232-5


R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 398713
Conc: 34.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

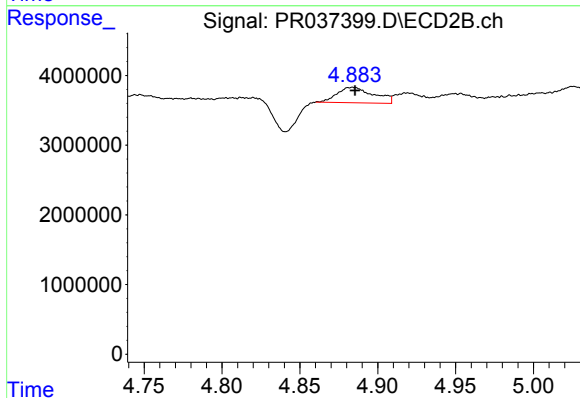


#15 AR-1232-5

R.T.: 4.884 min
Delta R.T.: -0.002 min
Response: 3639575
Conc: 53.33 ng/ml

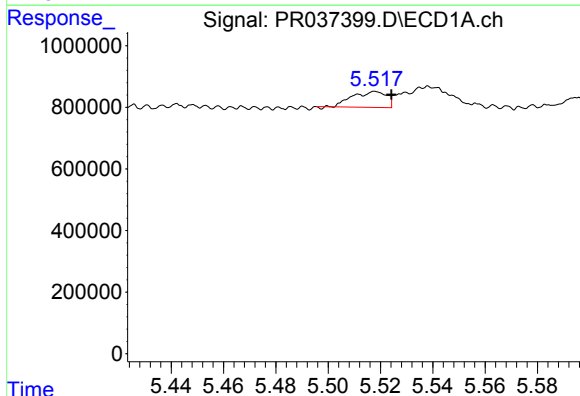


#16 AR-1242-1

R.T.: 5.518 min
Delta R.T.: -0.006 min
Response: 462527
Conc: 13.52 ng/ml

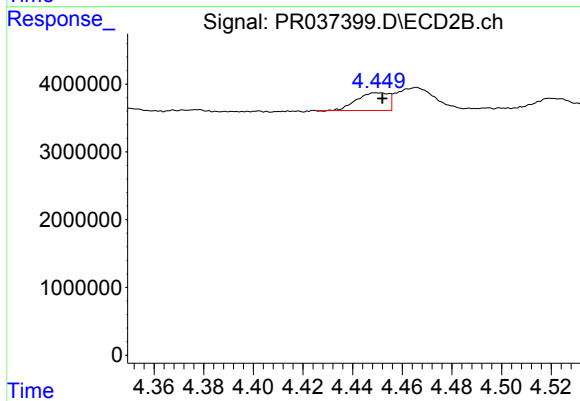

#16 AR-1242-1


R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2319536
Conc: 15.83 ng/ml

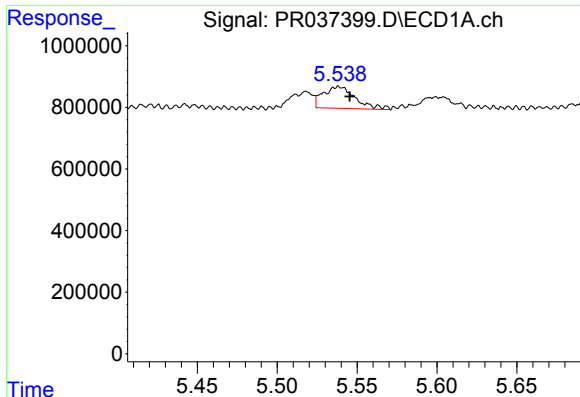

#17 AR-1242-2


R.T.: 5.538 min
Delta R.T.: -0.007 min
Response: 995436
Conc: 17.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

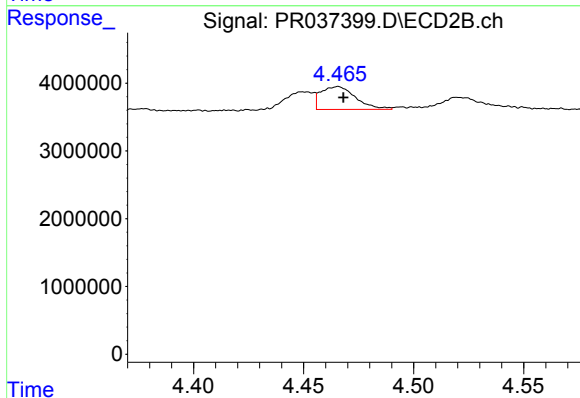


#17 AR-1242-2

R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 3737287
Conc: 16.38 ng/ml

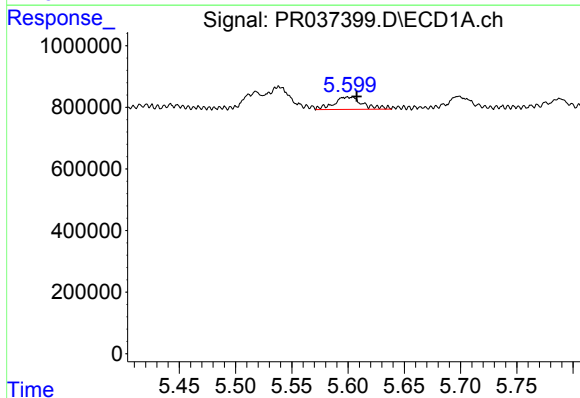


#18 AR-1242-3

R.T.: 5.599 min
Delta R.T.: -0.008 min
Response: 721785
Conc: 21.93 ng/ml

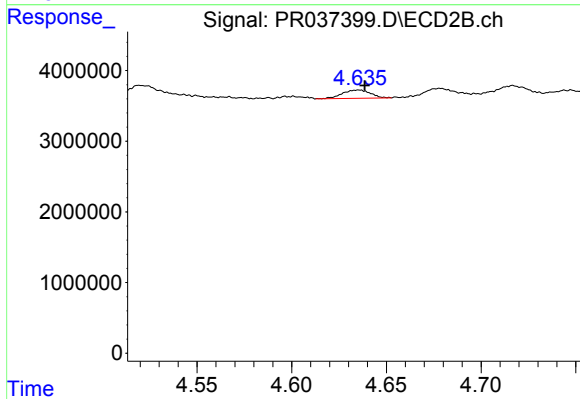

#18 AR-1242-3


R.T.: 4.636 min
Delta R.T.: -0.003 min
Response: 1204167
Conc: 10.41 ng/ml

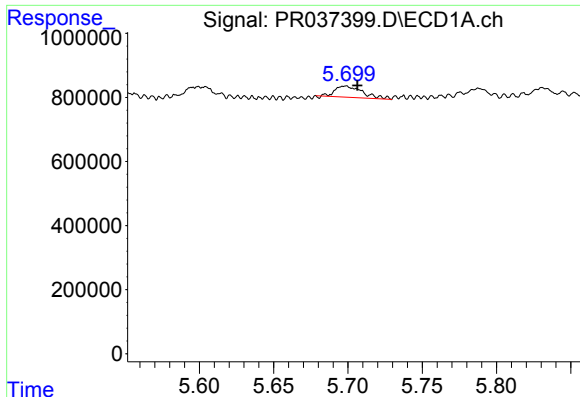

#19 AR-1242-4


R.T.: 5.698 min
Delta R.T.: -0.008 min
Response: 447203
Conc: 16.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

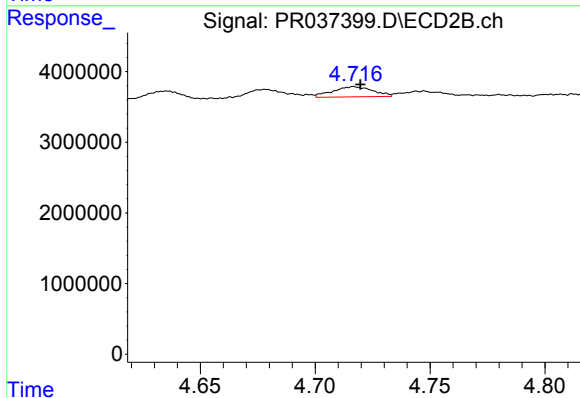


#19 AR-1242-4

R.T.: 4.717 min
Delta R.T.: -0.003 min
Response: 1747476
Conc: 15.90 ng/ml

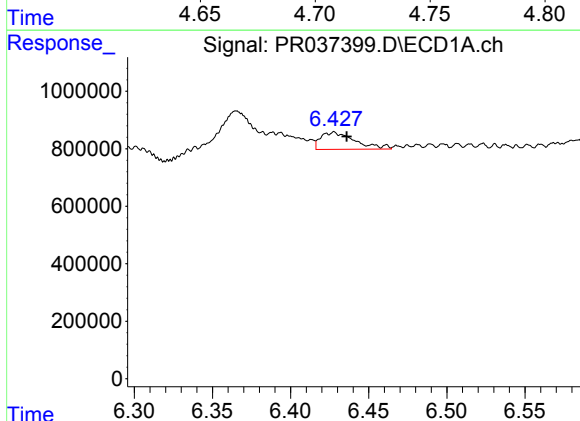


#20 AR-1242-5

R.T.: 6.428 min
Delta R.T.: -0.008 min
Response: 915220
Conc: 28.44 ng/ml

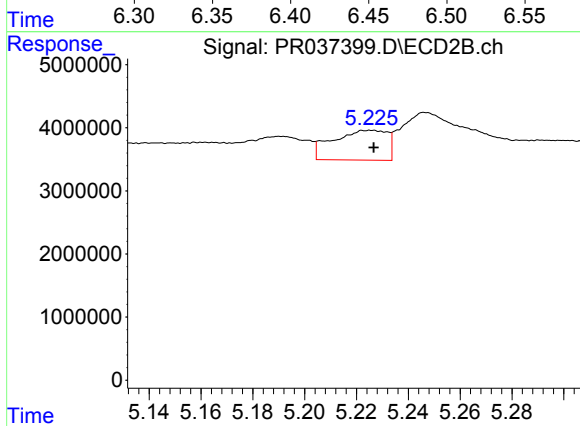

#20 AR-1242-5


R.T.: 5.225 min
Delta R.T.: -0.001 min
Response: 6885439
Conc: 41.55 ng/ml

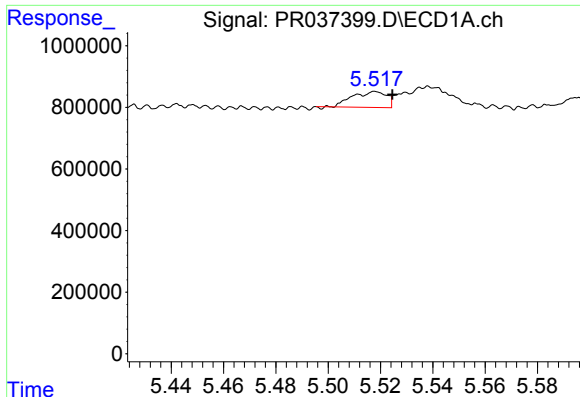

#21 AR-1248-1


R.T.: 5.518 min
Delta R.T.: -0.006 min
Response: 462527
Conc: 20.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

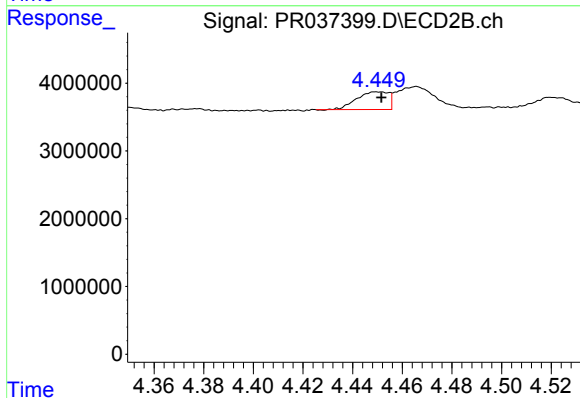


#21 AR-1248-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2319536
Conc: 23.04 ng/ml

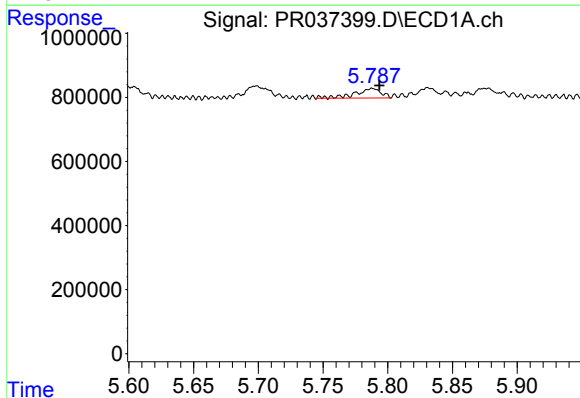


#22 AR-1248-2

R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 398713
Conc: 11.39 ng/ml

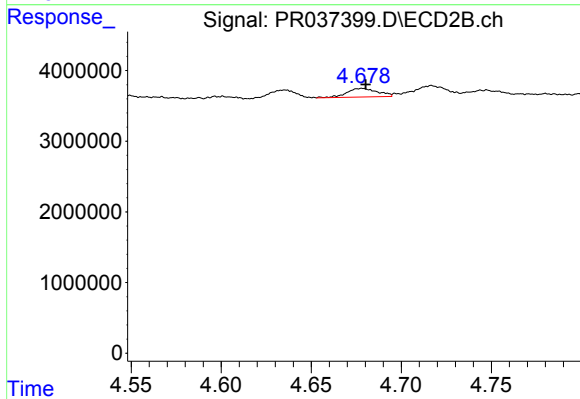

#22 AR-1248-2


R.T.: 4.679 min
Delta R.T.: -0.002 min
Response: 1452947
Conc: 10.65 ng/ml

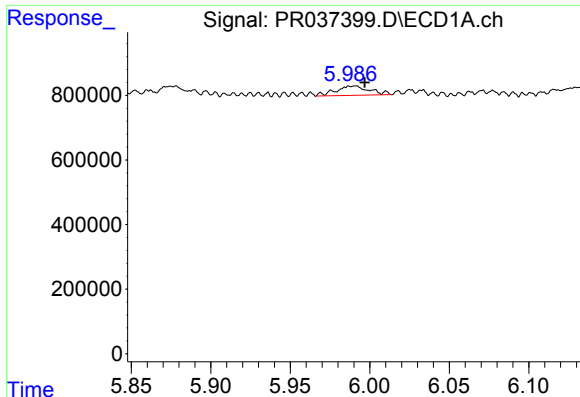

#23 AR-1248-3


R.T.: 5.991 min
Delta R.T.: -0.006 min
Response: 430374
Conc: 10.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

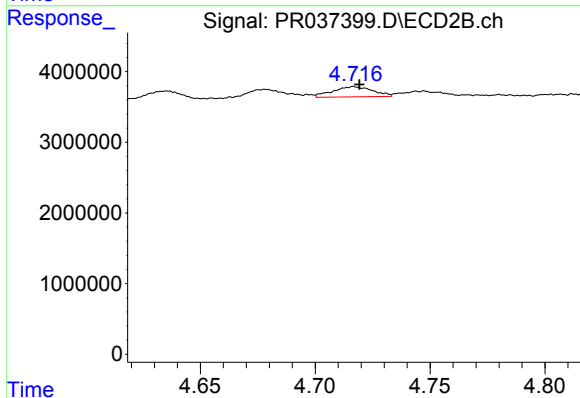


#23 AR-1248-3

R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 1747476
Conc: 12.48 ng/ml

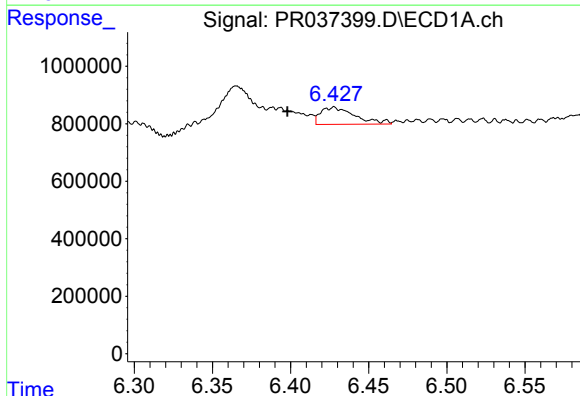


#24 AR-1248-4

R.T.: 6.428 min
Delta R.T.: 0.030 min
Response: 915220
Conc: 18.70 ng/ml

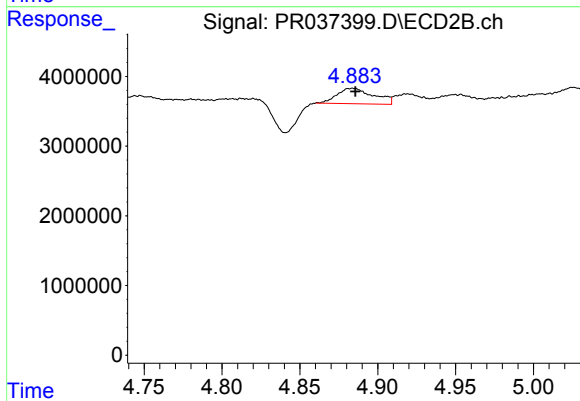

#24 AR-1248-4


R.T.: 4.884 min
Delta R.T.: -0.002 min
Response: 3639575
Conc: 20.45 ng/ml

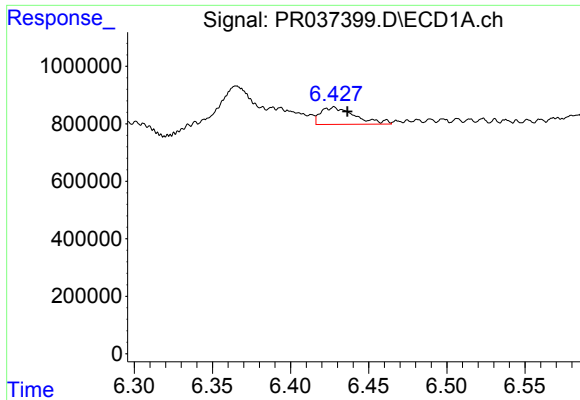

#25 AR-1248-5


R.T.: 6.428 min
Delta R.T.: -0.009 min
Response: 915220
Conc: 19.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

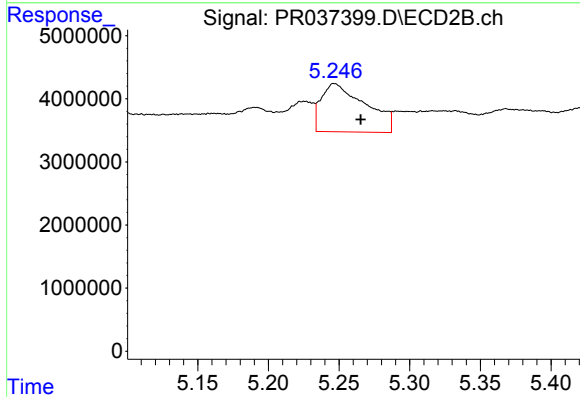


#25 AR-1248-5

R.T.: 5.247 min
Delta R.T.: -0.018 min
Response: 16718875
Conc: 85.47 ng/ml

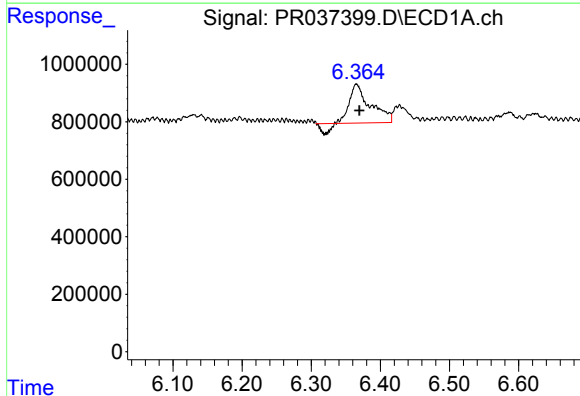


#26 AR-1254-1

R.T.: 6.365 min
Delta R.T.: -0.004 min
Response: 2602292
Conc: 47.63 ng/ml

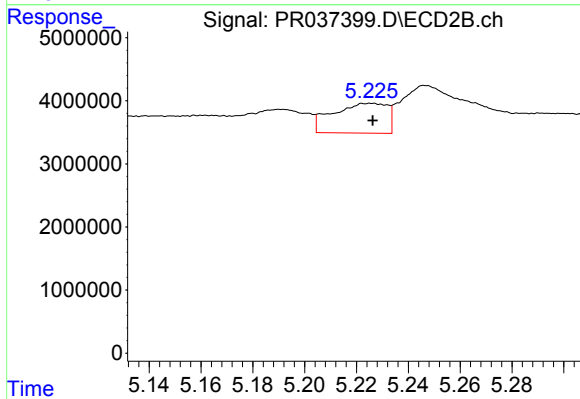

#26 AR-1254-1


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 6885439
Conc: 19.99 ng/ml

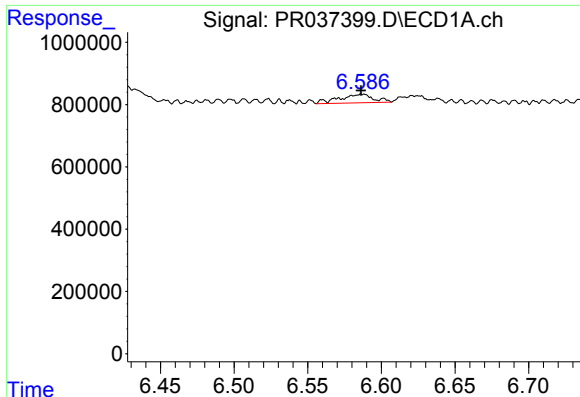

#27 AR-1254-2


R.T.: 6.587 min
Delta R.T.: 0.001 min
Response: 444596
Conc: 5.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

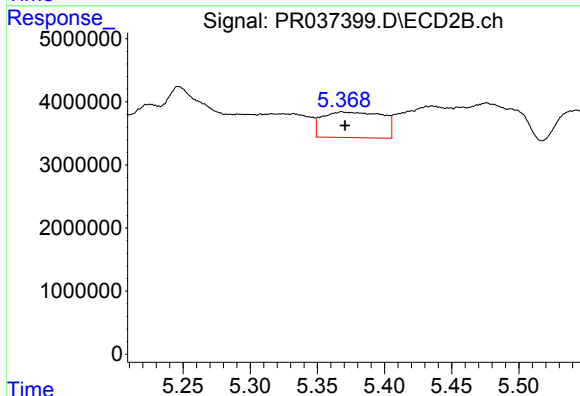


#27 AR-1254-2

R.T.: 5.368 min
Delta R.T.: -0.002 min
Response: 12592776
Conc: 42.05 ng/ml

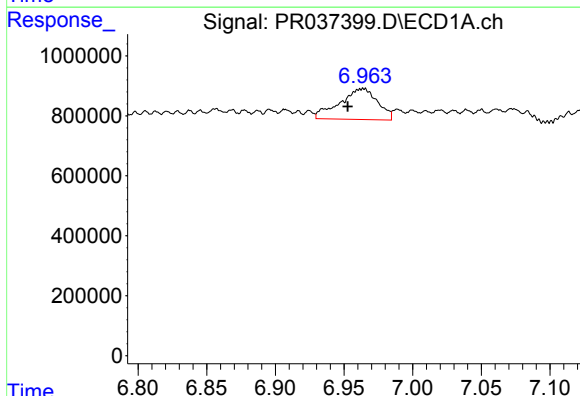


#28 AR-1254-3

R.T.: 6.964 min
Delta R.T.: 0.011 min
Response: 1973382
Conc: 21.69 ng/ml

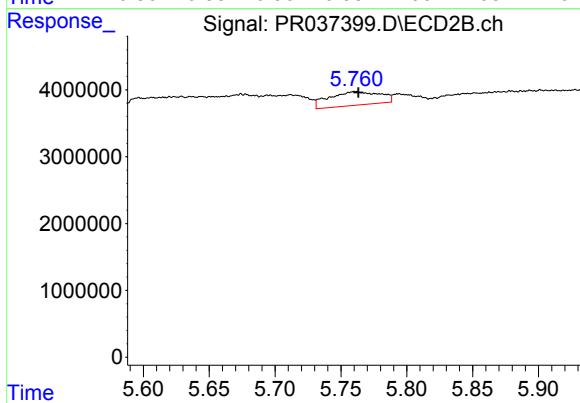

#28 AR-1254-3


R.T.: 5.761 min
Delta R.T.: -0.003 min
Response: 5454978
Conc: 11.52 ng/ml

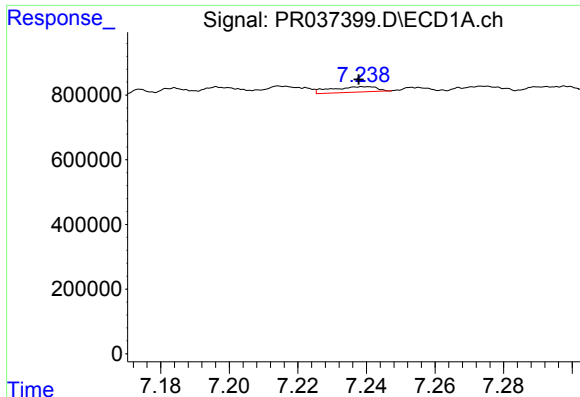

#29 AR-1254-4


R.T.: 7.240 min
Delta R.T.: 0.002 min
Response: 154339
Conc: 2.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

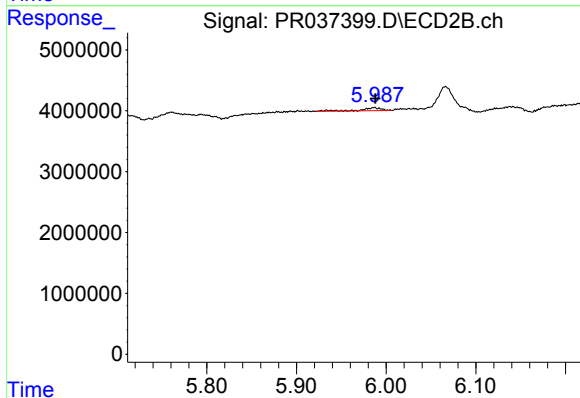


#29 AR-1254-4

R.T.: 5.987 min
Delta R.T.: -0.001 min
Response: 727646
Conc: 2.08 ng/ml

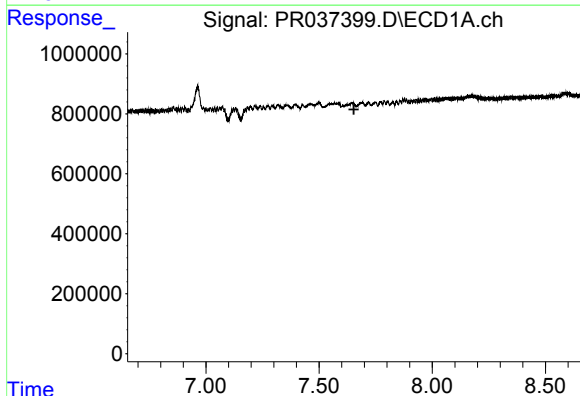


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

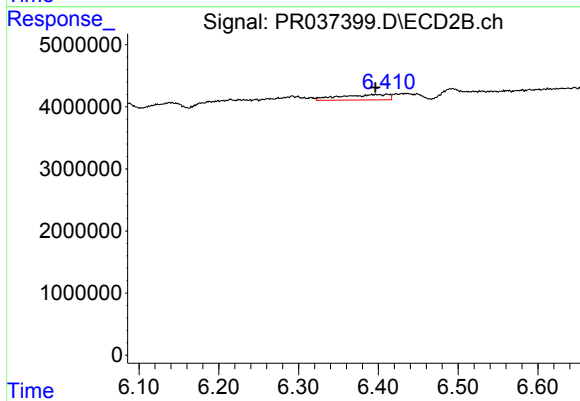

#30 AR-1254-5


R.T.: 6.392 min
Delta R.T.: -0.005 min
Response: 3738461
Conc: 8.44 ng/ml

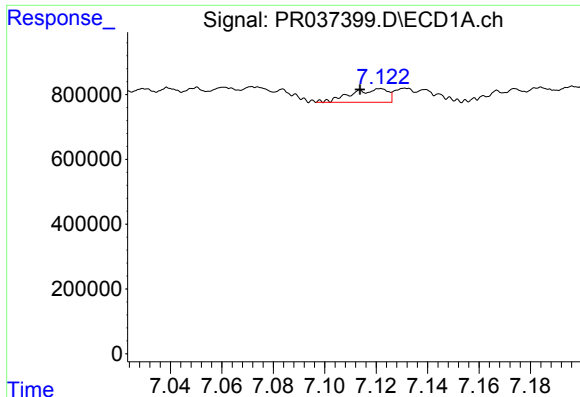

#31 AR-1260-1


R.T.: 7.122 min
Delta R.T.: 0.008 min
Response: 413182
Conc: 6.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

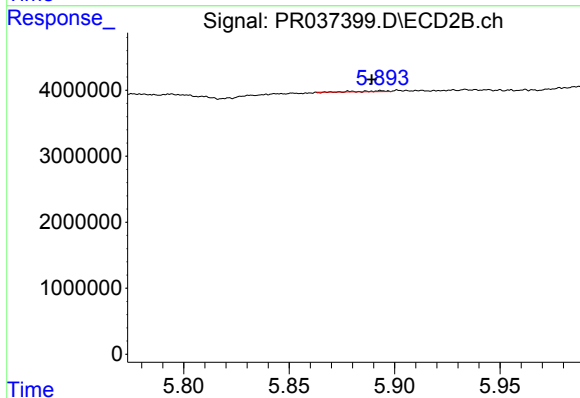


#31 AR-1260-1

R.T.: 5.894 min
Delta R.T.: 0.005 min
Response: 66479
Conc: 0.23 ng/ml

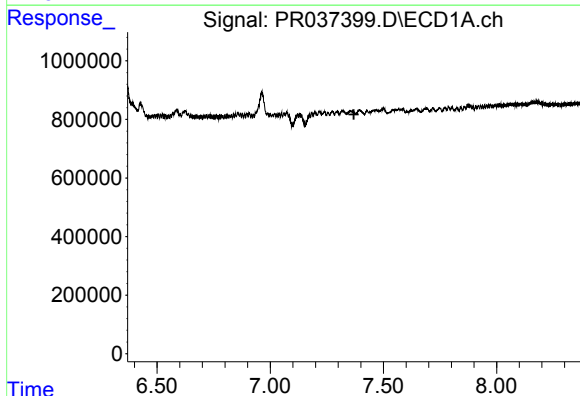


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

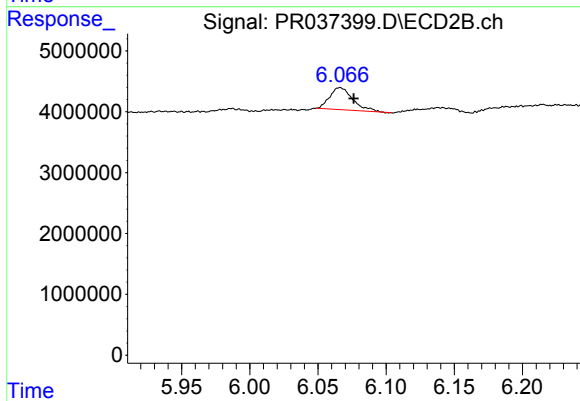

#32 AR-1260-2


R.T.: 6.066 min
Delta R.T.: -0.010 min
Response: 4234455
Conc: 9.19 ng/ml

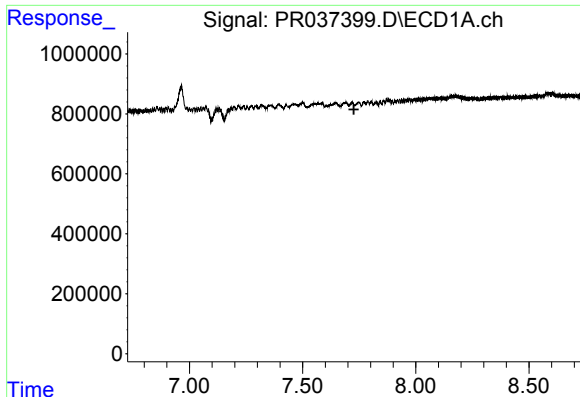

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

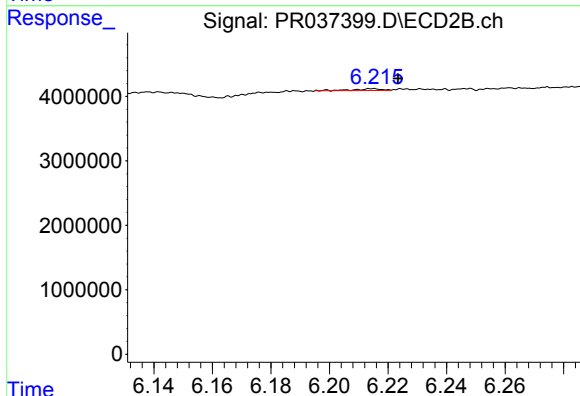


#33 AR-1260-3

R.T.: 6.215 min
Delta R.T.: -0.008 min
Response: 187825
Conc: 0.53 ng/ml

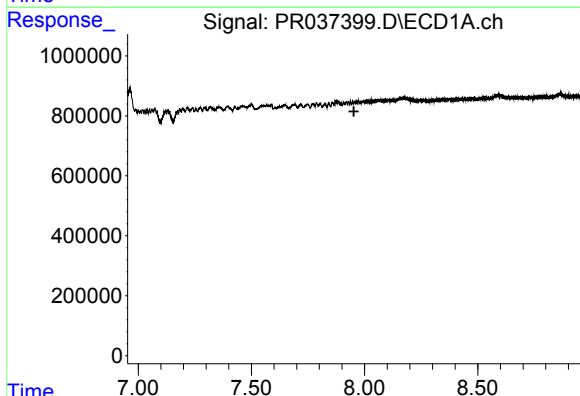


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

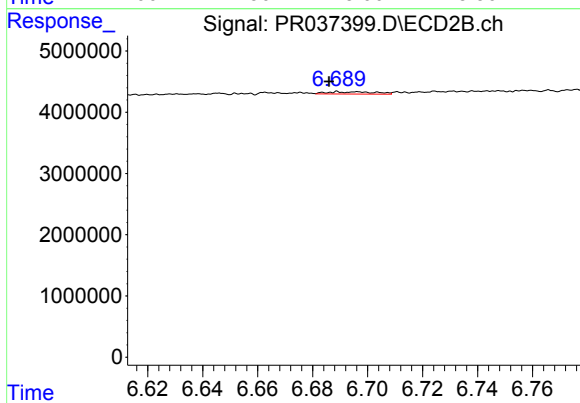

#34 AR-1260-4


R.T.: 6.689 min
Delta R.T.: 0.003 min
Response: 458230
Conc: 1.50 ng/ml

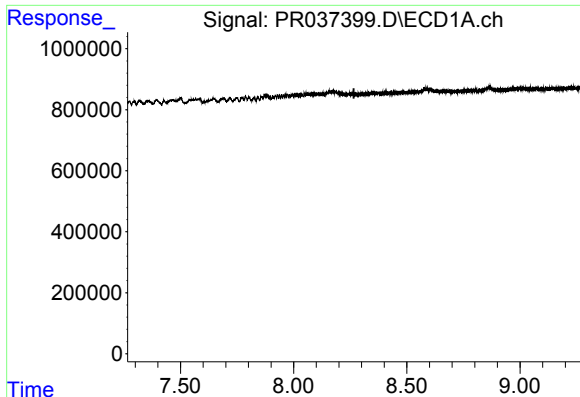

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

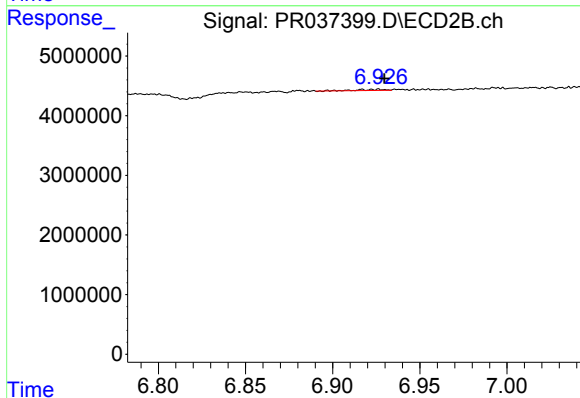


#35 AR-1260-5

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 159931
Conc: 0.18 ng/ml

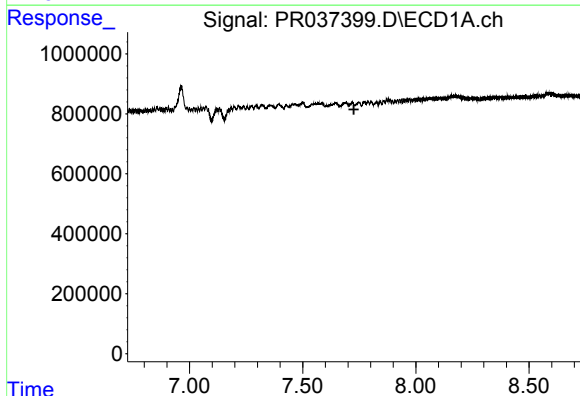


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

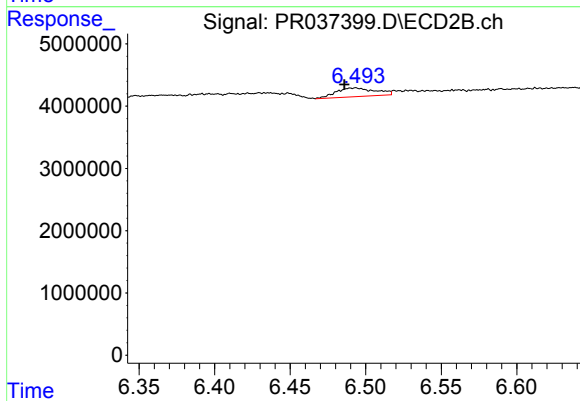

#36 AR-1262-1


R.T.: 6.493 min
Delta R.T.: 0.007 min
Response: 2512745
Conc: 10.03 ng/ml

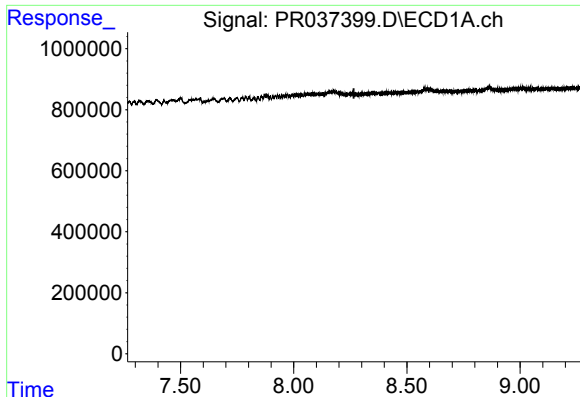

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

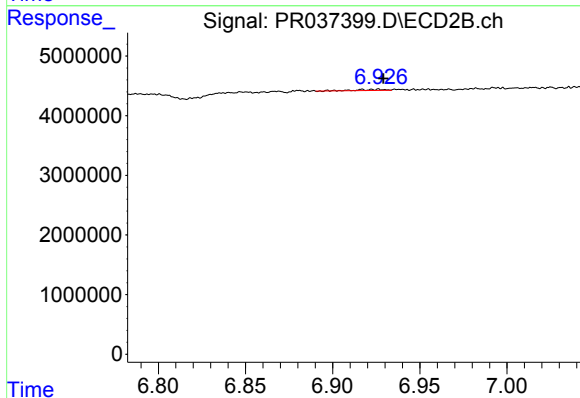


#37 AR-1262-2

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 159931
Conc: 0.13 ng/ml

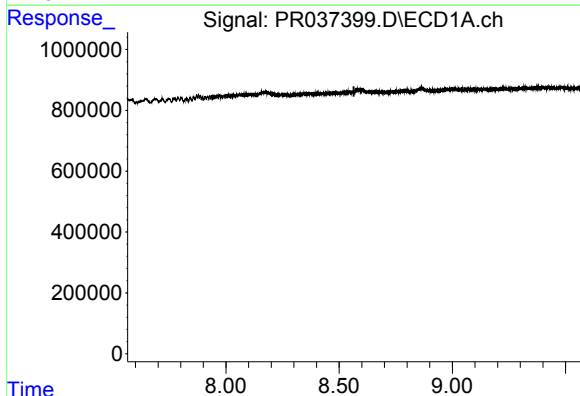


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

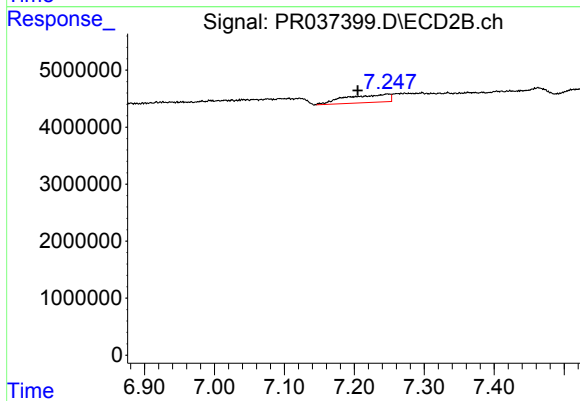

#38 AR-1262-3


R.T.: 7.247 min
Delta R.T.: 0.042 min
Response: 6065319
Conc: 11.06 ng/ml

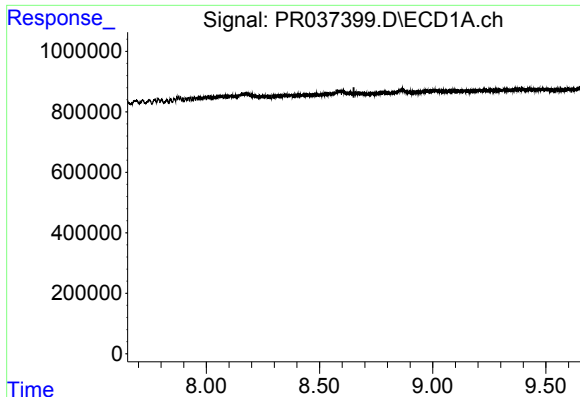

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

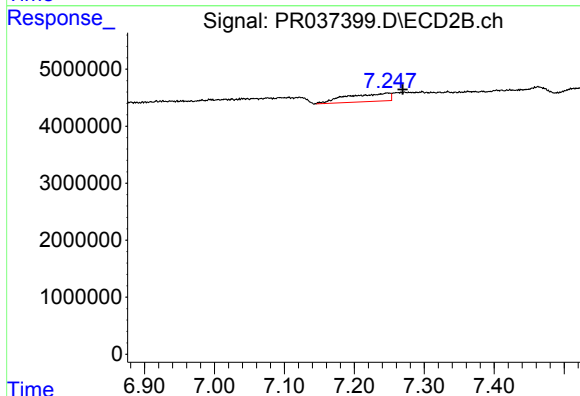


#39 AR-1262-4

R.T.: 7.247 min
Delta R.T.: -0.022 min
Response: 6065319
Conc: 6.76 ng/ml

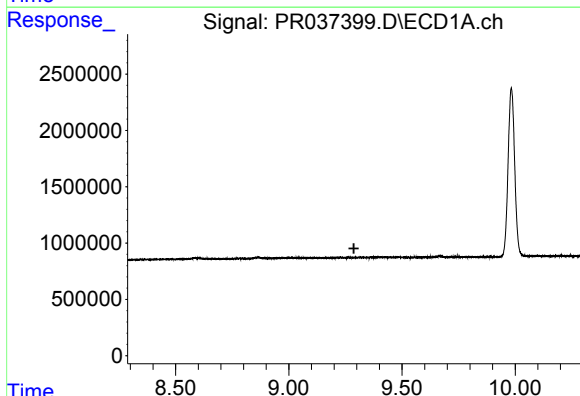


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

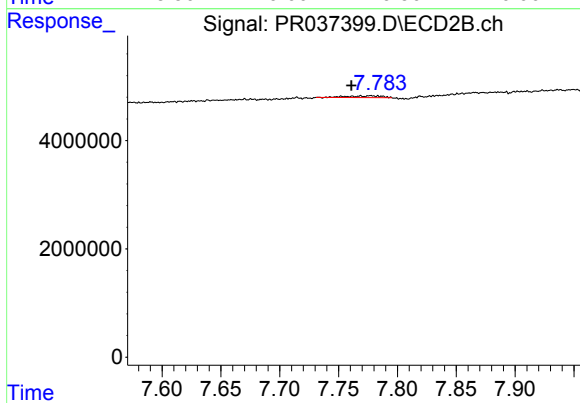

#40 AR-1262-5


R.T.: 7.778 min
Delta R.T.: 0.017 min
Response: 647870
Conc: 1.69 ng/ml

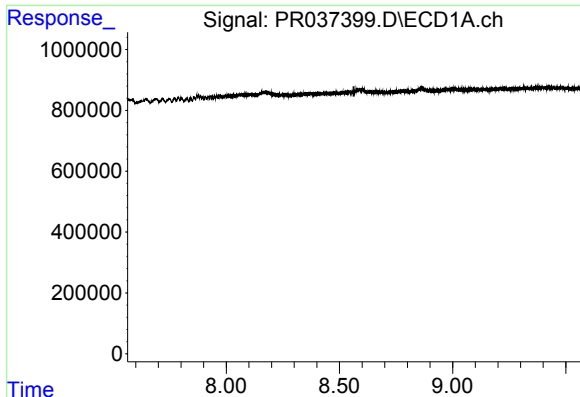

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

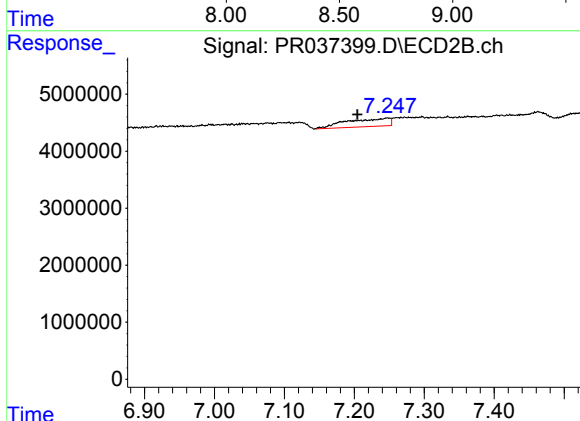


#41 AR-1268-1

R.T.: 7.247 min
Delta R.T.: 0.042 min
Response: 6065319
Conc: 4.93 ng/ml

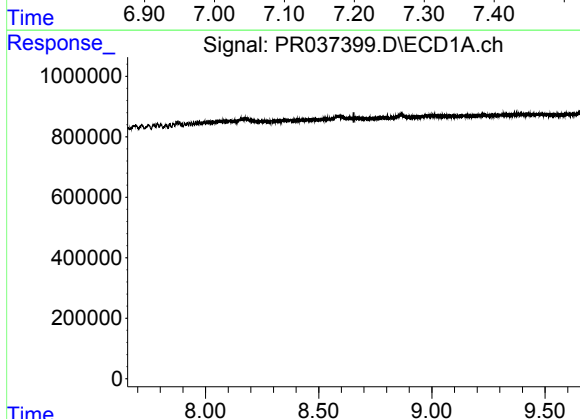


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

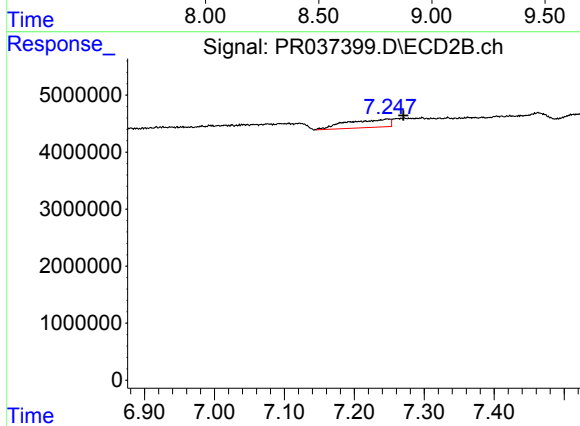

#42 AR-1268-2


R.T.: 7.247 min
Delta R.T.: -0.023 min
Response: 6065319
Conc: 5.73 ng/ml

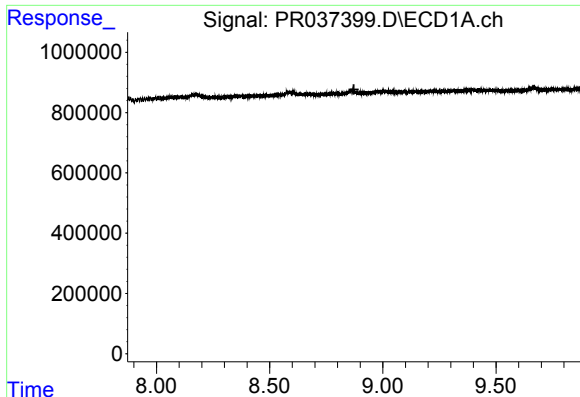

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

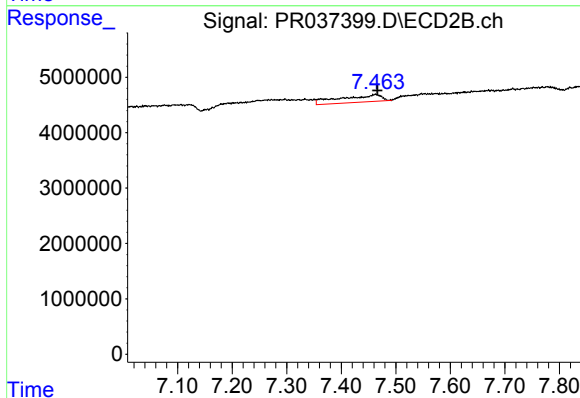


#43 AR-1268-3

R.T.: 7.463 min
Delta R.T.: -0.004 min
Response: 6894920
Conc: 7.78 ng/ml

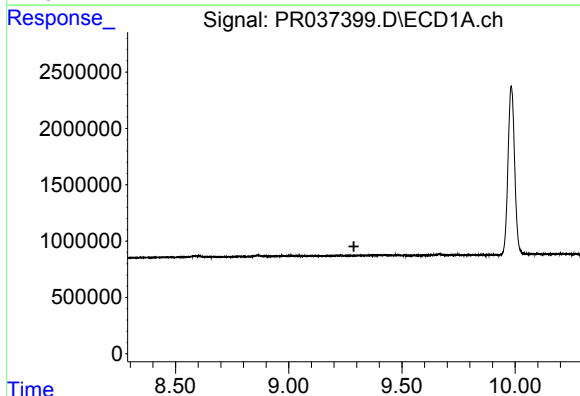


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

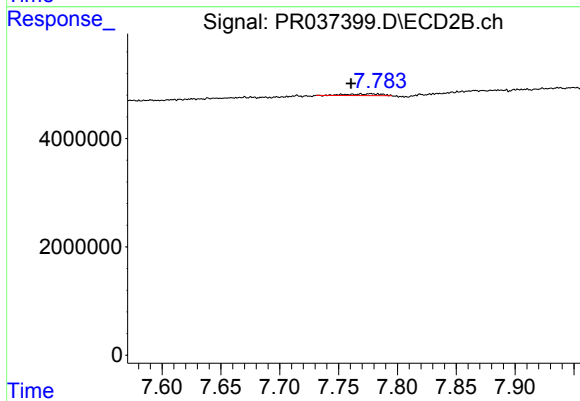

#44 AR-1268-4


R.T.: 7.778 min
Delta R.T.: 0.017 min
Response: 647870
Conc: 1.79 ng/ml

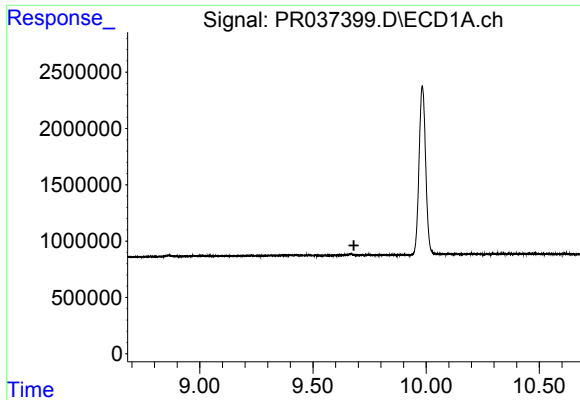

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

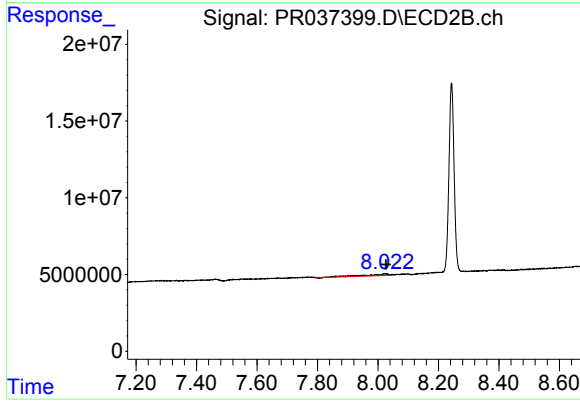

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.003 min
Response: 6039799
Conc: 2.37 ng/ml