

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR042519\  
 Data File : PR037402.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Apr 2019 16:07  
 Operator : SM\SJ  
 Sample : K2241-09  
 Misc : AR1242 MDL 25PPB  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 26 00:43:05 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR042219.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Mon Apr 22 17:27:39 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml  | ng/ml    |
|-----------------------------|-----------------|-------|-------|----------|---------|--------|----------|
| -----                       |                 |       |       |          |         |        |          |
| System Monitoring Compounds |                 |       |       |          |         |        |          |
| 1)                          | SA Tetrachlo... | 4.362 | 3.405 | 31467119 | 123.6E6 | 25.154 | 25.766   |
| 2)                          | SA Decachlor... | 9.991 | 8.246 | 29384877 | 142.3E6 | 22.218 | 24.424   |
| Target Compounds            |                 |       |       |          |         |        |          |
| 3)                          | L1 AR-1016-1    | 5.522 | 4.450 | 1256498  | 4842150 | 29.161 | 26.594   |
| 4)                          | L1 AR-1016-2    | 5.544 | 4.465 | 1718620  | 6848459 | 24.819 | 24.275   |
| 5)                          | L1 AR-1016-3    | 5.606 | 4.633 | 1236882  | 2814962 | 30.670 | 19.578 # |
| 6)                          | L1 AR-1016-4    | 5.703 | 4.678 | 707606   | 2879316 | 21.547 | 26.025   |
| 7)                          | L1 AR-1016-5    | 5.994 | 4.884 | 739477   | 3705177 | 21.565 | 24.375   |
| 8)                          | L2 AR-1221-1    | 0.000 | 3.610 | 0        | 386623  | N.D.   | 7.593 #  |
| 9)                          | L2 AR-1221-2    | 4.663 | 3.693 | 549639   | 2071804 | 60.774 | 55.790   |
| 10)                         | L2 AR-1221-3    | 4.735 | 3.764 | 789802   | 2591972 | 25.769 | 21.168   |
| 11)                         | L3 AR-1232-1    | 4.735 | 3.764 | 789802   | 2591972 | 27.001 | 22.155   |
| 12)                         | L3 AR-1232-2    | 5.258 | 4.465 | 1081937  | 6848459 | 64.029 | 49.546   |
| 13)                         | L3 AR-1232-3    | 5.544 | 4.633 | 1718620  | 2814962 | 50.840 | 40.098   |
| 14)                         | L3 AR-1232-4    | 5.703 | 4.717 | 707606   | 3520733 | 45.080 | 59.002 # |
| 15)                         | L3 AR-1232-5    | 5.791 | 4.884 | 700378   | 3705177 | 59.884 | 54.293   |
| 16)                         | L4 AR-1242-1    | 5.522 | 4.450 | 1256498  | 4842150 | 36.724 | 33.044   |
| 17)                         | L4 AR-1242-2    | 5.544 | 4.465 | 1718620  | 6848459 | 30.983 | 30.016   |
| 18)                         | L4 AR-1242-3    | 5.606 | 4.633 | 1236882  | 2814962 | 37.578 | 24.345 # |
| 19)                         | L4 AR-1242-4    | 5.703 | 4.717 | 707606   | 3520733 | 26.826 | 32.033   |
| 20)                         | L4 AR-1242-5    | 6.434 | 5.225 | 1229501  | 6768349 | 38.208 | 40.847   |
| 21)                         | L5 AR-1248-1    | 5.522 | 4.450 | 1256498  | 4842150 | 54.851 | 48.102   |
| 22)                         | L5 AR-1248-2    | 5.791 | 4.678 | 700378   | 2879316 | 20.003 | 21.098   |
| 23)                         | L5 AR-1248-3    | 5.994 | 4.717 | 739477   | 3520733 | 18.076 | 25.153 # |
| 24)                         | L5 AR-1248-4    | 6.396 | 4.884 | 1166770  | 3705177 | 23.834 | 20.820   |
| 25)                         | L5 AR-1248-5    | 6.434 | 5.263 | 1229501  | 6909238 | 26.028 | 35.321 # |
| 26)                         | L6 AR-1254-1    | 6.369 | 5.225 | 1314293  | 6768349 | 24.058 | 19.648   |
| 27)                         | L6 AR-1254-2    | 6.591 | 5.372 | 1124034  | 2104266 | 13.116 | 7.026 #  |
| 28)                         | L6 AR-1254-3    | 6.968 | 5.761 | 1029891  | 3570961 | 11.322 | 7.540 #  |
| 29)                         | L6 AR-1254-4    | 7.232 | 5.986 | 400154   | 1294802 | 5.972  | 3.693 #  |
| 30)                         | L6 AR-1254-5    | 0.000 | 6.396 | 0        | 1529284 | N.D.   | 3.453 #  |
| 31)                         | L7 AR-1260-1    | 0.000 | 5.883 | 0        | 162967  | N.D.   | 0.558 #  |
| 32)                         | L7 AR-1260-2    | 0.000 | 6.067 | 0        | 2856004 | N.D.   | 6.201 #  |
| 33)                         | L7 AR-1260-3    | 0.000 | 6.225 | 0        | 179569  | N.D.   | 0.504 #  |
| 34)                         | L7 AR-1260-4    | 0.000 | 6.689 | 0        | 163146  | N.D.   | 0.535 #  |
| 35)                         | L7 AR-1260-5    | 0.000 | 6.943 | 0        | 69858   | N.D.   | 0.081 #  |
| 36)                         | L8 AR-1262-1    | 0.000 | 6.494 | 0        | 2452641 | N.D.   | 9.786 #  |
| 37)                         | L8 AR-1262-2    | 0.000 | 6.943 | 0        | 69858   | N.D.   | 0.056 #  |
| 38)                         | L8 AR-1262-3    | 0.000 | 7.211 | 0        | 3961546 | N.D.   | 7.226 #  |
| 39)                         | L8 AR-1262-4    | 0.000 | 7.278 | 0        | 4329269 | N.D.   | 4.823 #  |
| 40)                         | L8 AR-1262-5    | 0.000 | 7.777 | 0        | 889781  | N.D.   | 2.325 #  |
| 41)                         | L9 AR-1268-1    | 0.000 | 7.211 | 0        | 3961546 | N.D.   | 3.218 #  |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR042519\  
 Data File : PR037402.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Apr 2019 16:07  
 Operator : SM\SJ  
 Sample : K2241-09  
 Misc : AR1242 MDL 25PPB  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 26 00:43:05 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR042219.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Mon Apr 22 17:27:39 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|        | Compound  | RT#1  | RT#2  | Resp#1 | Resp#2  | ng/ml | ng/ml   |
|--------|-----------|-------|-------|--------|---------|-------|---------|
| 42) L9 | AR-1268-2 | 0.000 | 7.278 | 0      | 4329269 | N.D.  | 4.088 # |
| 43) L9 | AR-1268-3 | 0.000 | 7.465 | 0      | 5478449 | N.D.  | 6.182 # |
| 44) L9 | AR-1268-4 | 0.000 | 7.777 | 0      | 889781  | N.D.  | 2.453 # |
| 45) L9 | AR-1268-5 | 0.000 | 8.028 | 0      | 3695557 | N.D.  | 1.453 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR042519\  
Data File : PR037402.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Apr 2019 16:07  
Operator : SM\SJ  
Sample : K2241-09  
Misc : AR1242 MDL 25PPB  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 26 00:43:05 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR042219.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Mon Apr 22 17:27:39 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

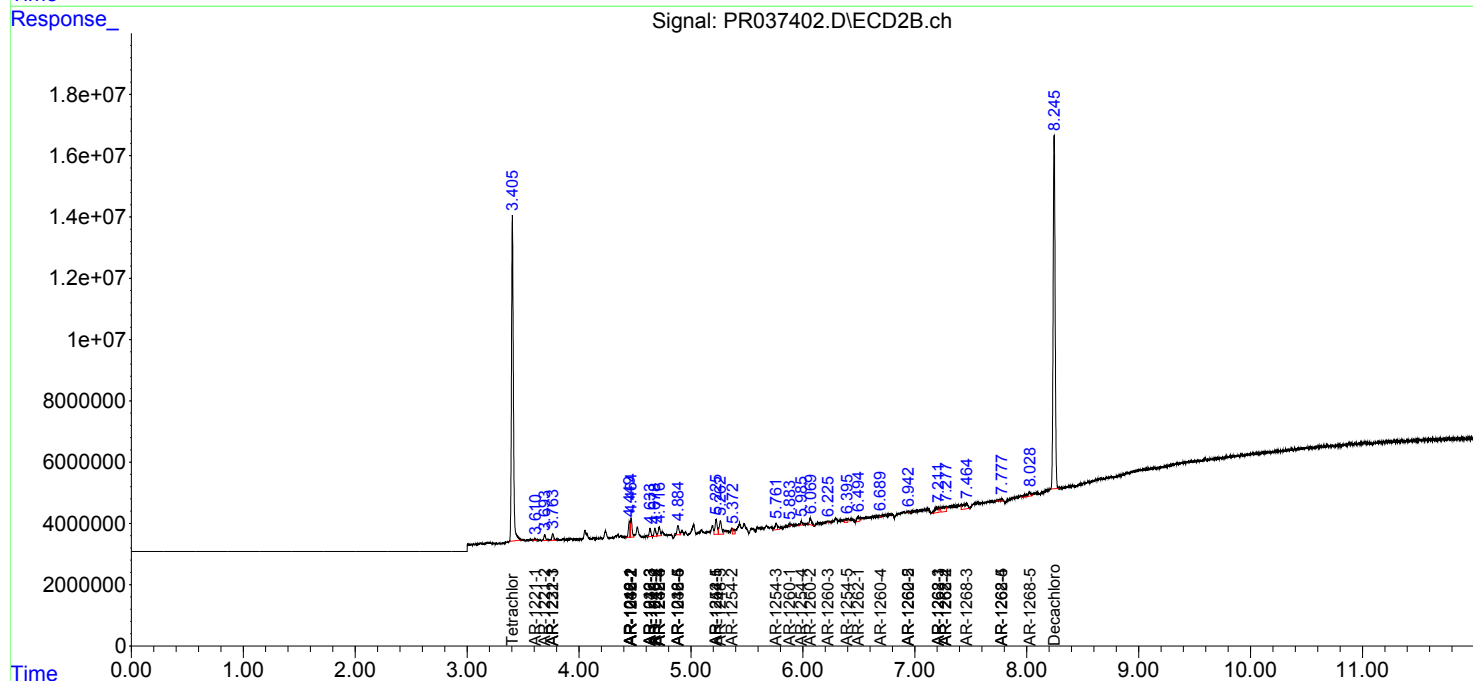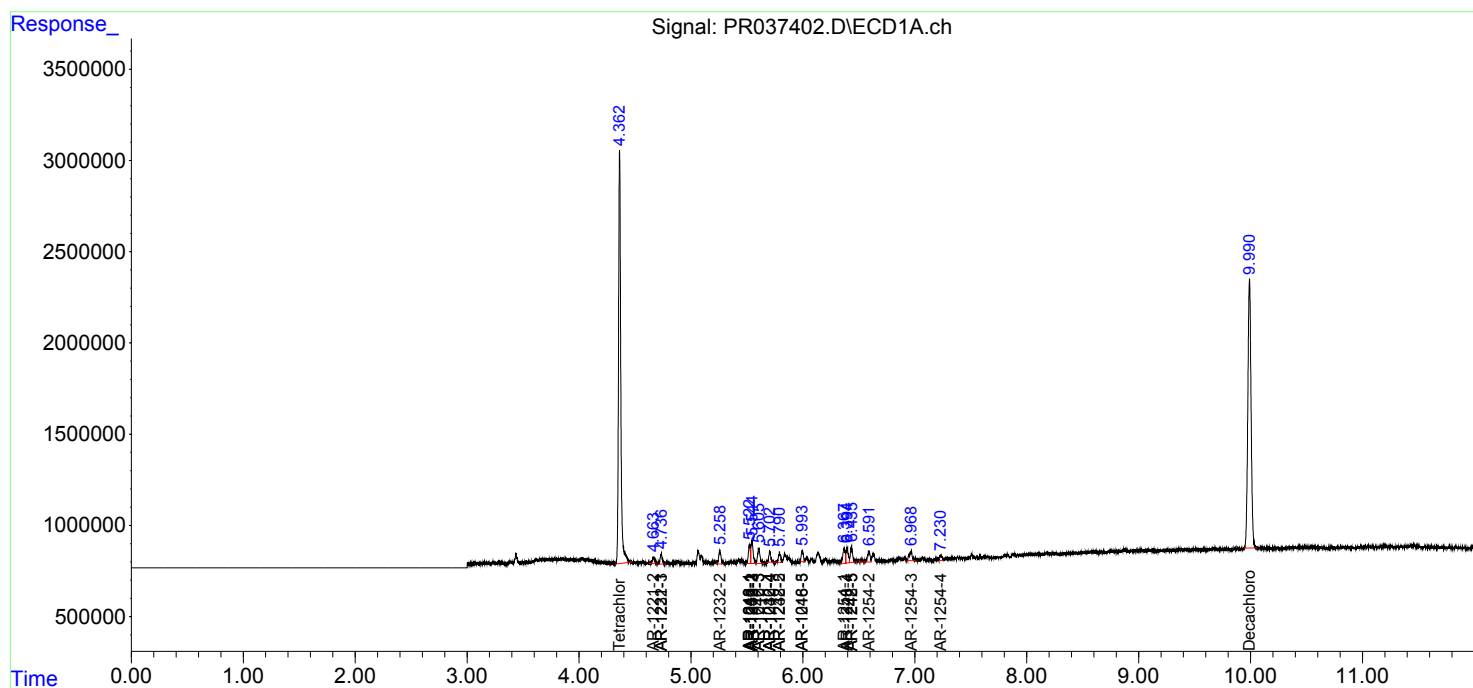


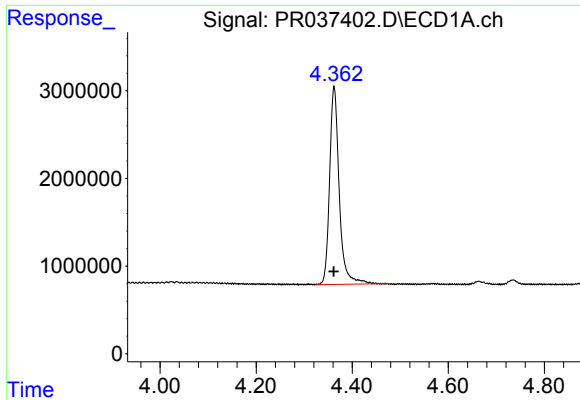

#1 Tetrachloro-m-xylene


R.T.: 4.362 min  
Delta R.T.: 0.000 min  
Response: 31467119  
Conc: 25.15 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

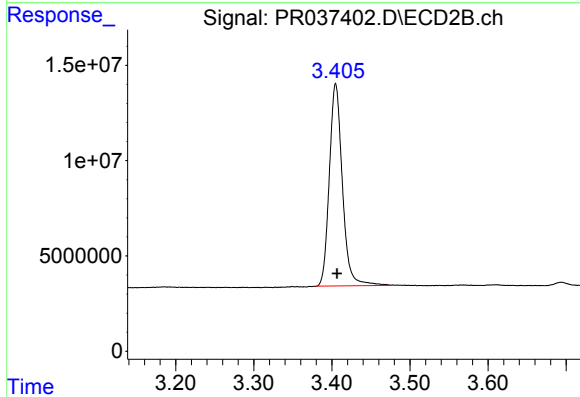


#1 Tetrachloro-m-xylene

R.T.: 3.405 min  
Delta R.T.: -0.002 min  
Response: 123560036  
Conc: 25.77 ng/ml

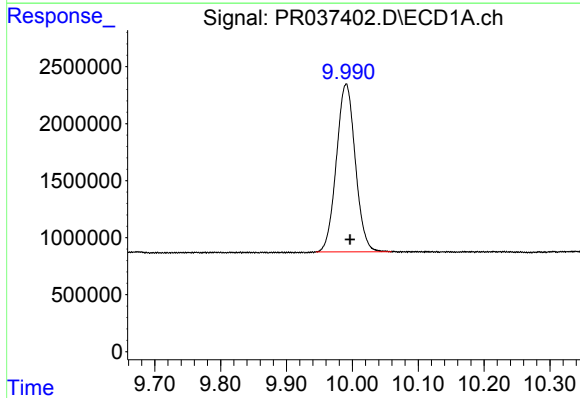


#2 Decachlorobiphenyl

R.T.: 9.991 min  
Delta R.T.: -0.006 min  
Response: 29384877  
Conc: 22.22 ng/ml

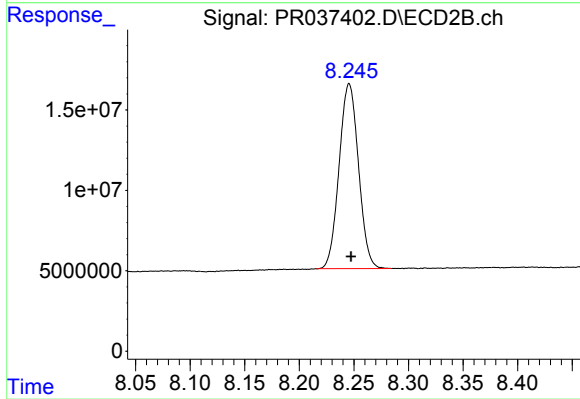

#2 Decachlorobiphenyl


R.T.: 8.246 min  
Delta R.T.: -0.002 min  
Response: 142250528  
Conc: 24.42 ng/ml

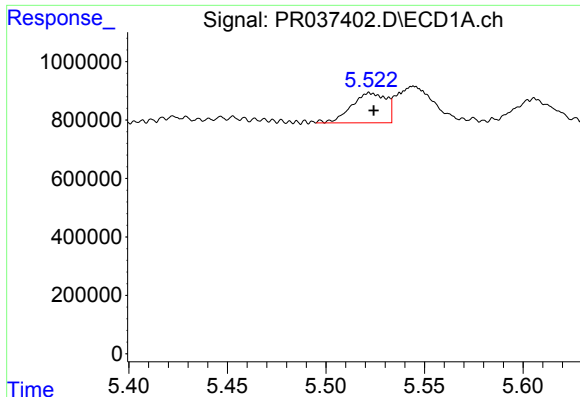

#3 AR-1016-1


R.T.: 5.522 min  
Delta R.T.: -0.002 min  
Response: 1256498  
Conc: 29.16 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

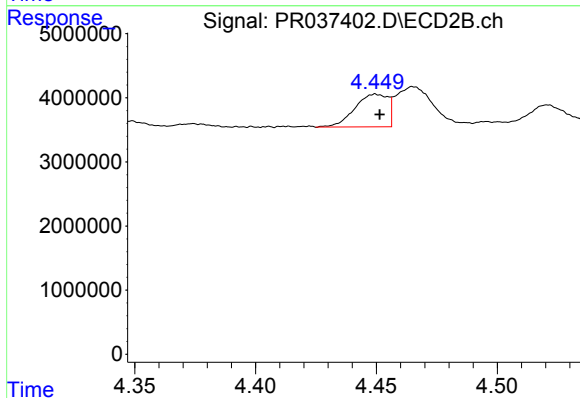


#3 AR-1016-1

R.T.: 4.450 min  
Delta R.T.: -0.002 min  
Response: 4842150  
Conc: 26.59 ng/ml

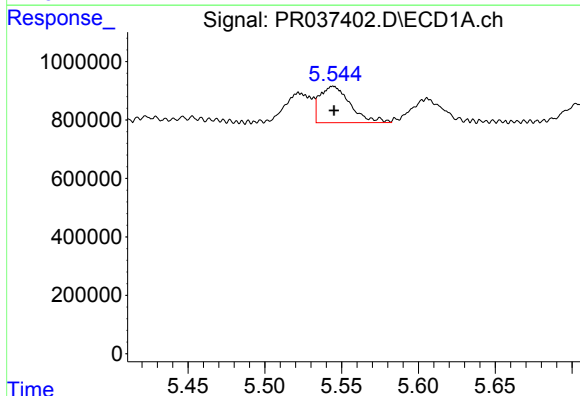


#4 AR-1016-2

R.T.: 5.544 min  
Delta R.T.: 0.000 min  
Response: 1718620  
Conc: 24.82 ng/ml

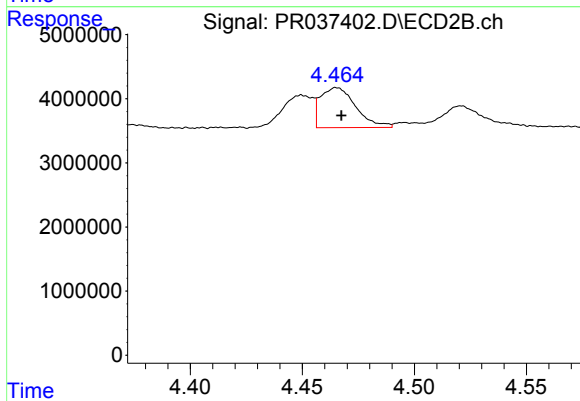

#4 AR-1016-2


R.T.: 4.465 min  
Delta R.T.: -0.002 min  
Response: 6848459  
Conc: 24.27 ng/ml

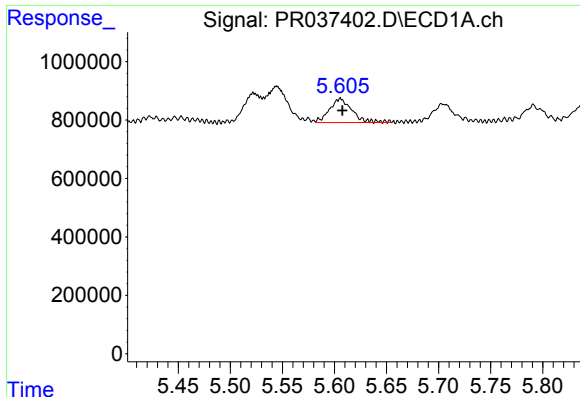

#5 AR-1016-3


R.T.: 5.606 min  
Delta R.T.: -0.002 min  
Response: 1236882  
Conc: 30.67 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

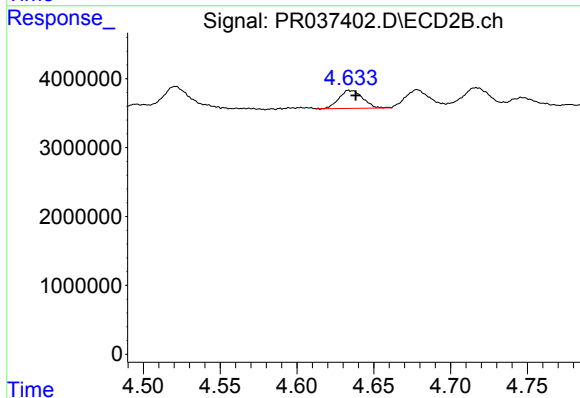


#5 AR-1016-3

R.T.: 4.633 min  
Delta R.T.: -0.005 min  
Response: 2814962  
Conc: 19.58 ng/ml

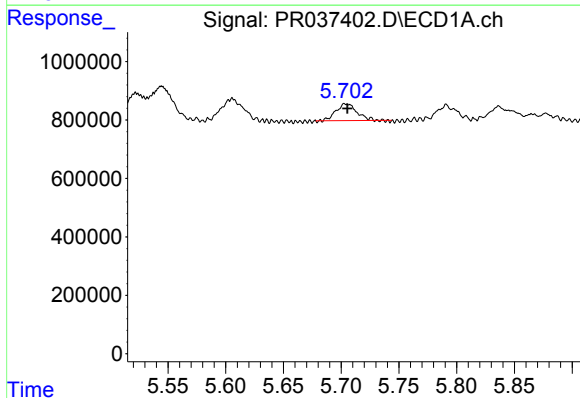


#6 AR-1016-4

R.T.: 5.703 min  
Delta R.T.: -0.002 min  
Response: 707606  
Conc: 21.55 ng/ml

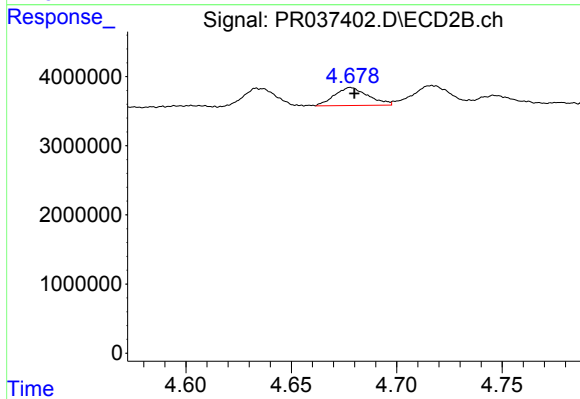

#6 AR-1016-4


R.T.: 4.678 min  
Delta R.T.: -0.002 min  
Response: 2879316  
Conc: 26.03 ng/ml

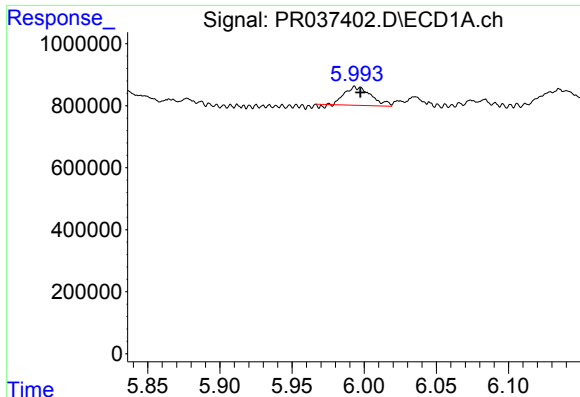

#7 AR-1016-5


R.T.: 5.994 min  
Delta R.T.: -0.004 min  
Response: 739477  
Conc: 21.57 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

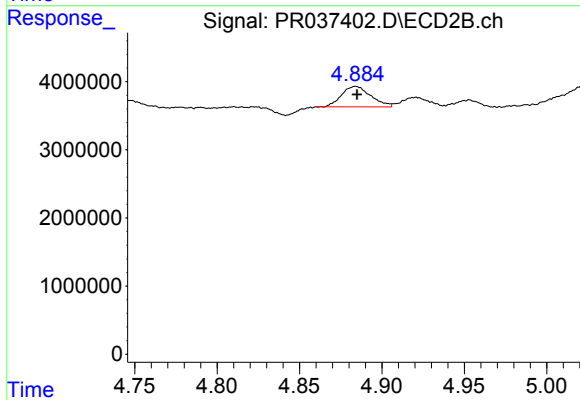


#7 AR-1016-5

R.T.: 4.884 min  
Delta R.T.: 0.000 min  
Response: 3705177  
Conc: 24.37 ng/ml

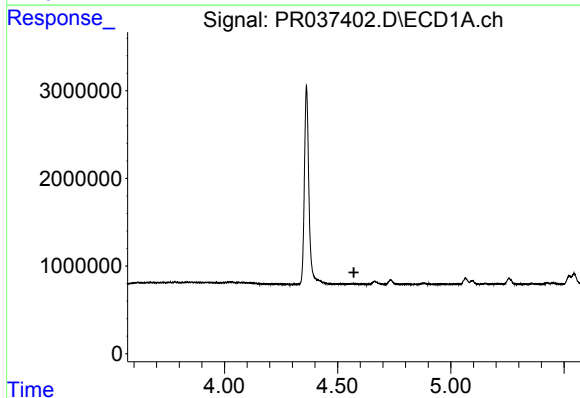


#8 AR-1221-1

R.T.: 0.000 min  
Exp R.T. : 4.572 min  
Response: 0  
Conc: N.D.

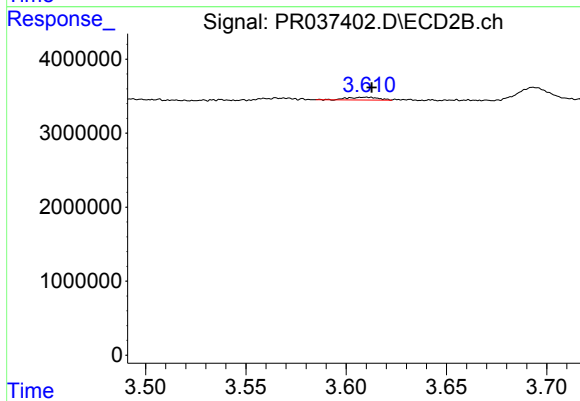

#8 AR-1221-1


R.T.: 3.610 min  
Delta R.T.: -0.003 min  
Response: 386623  
Conc: 7.59 ng/ml

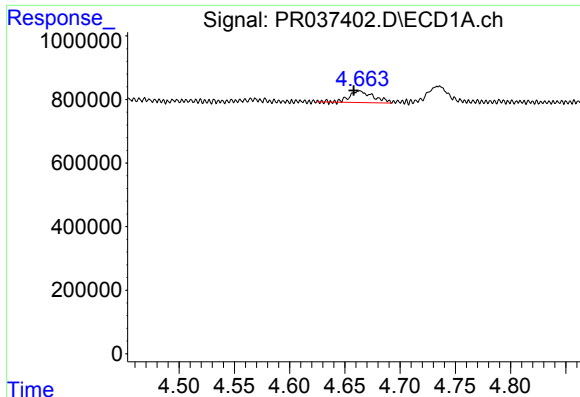

#9 AR-1221-2


R.T.: 4.663 min  
Delta R.T.: 0.005 min  
Response: 549639  
Conc: 60.77 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

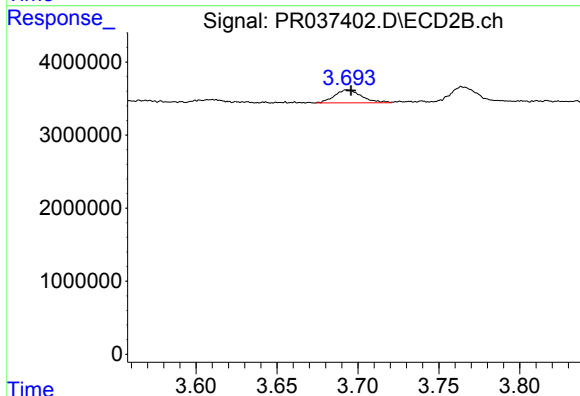


#9 AR-1221-2

R.T.: 3.693 min  
Delta R.T.: -0.002 min  
Response: 2071804  
Conc: 55.79 ng/ml

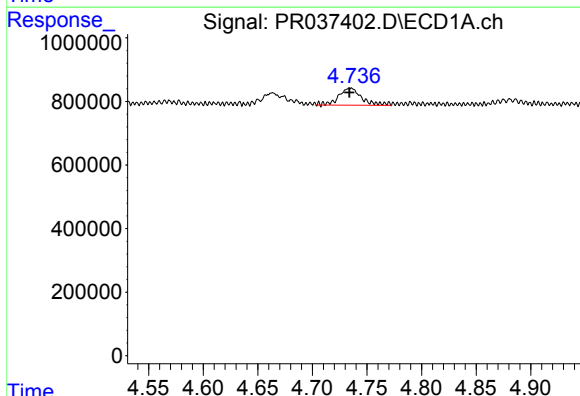


#10 AR-1221-3

R.T.: 4.735 min  
Delta R.T.: 0.001 min  
Response: 789802  
Conc: 25.77 ng/ml

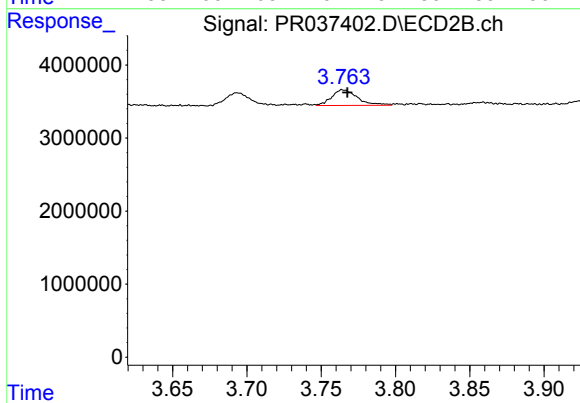

#10 AR-1221-3


R.T.: 3.764 min  
Delta R.T.: -0.004 min  
Response: 2591972  
Conc: 21.17 ng/ml

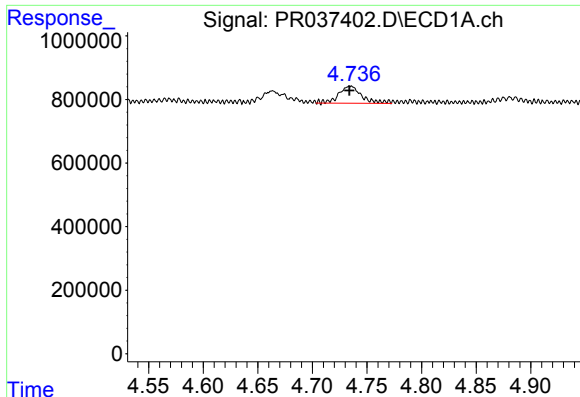

#11 AR-1232-1


R.T.: 4.735 min  
Delta R.T.: 0.002 min  
Response: 789802  
Conc: 27.00 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

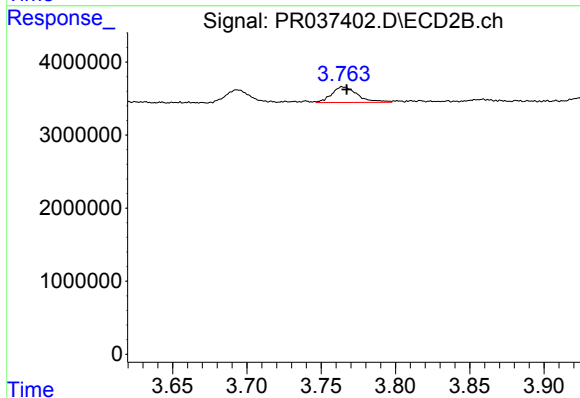


#11 AR-1232-1

R.T.: 3.764 min  
Delta R.T.: -0.003 min  
Response: 2591972  
Conc: 22.16 ng/ml

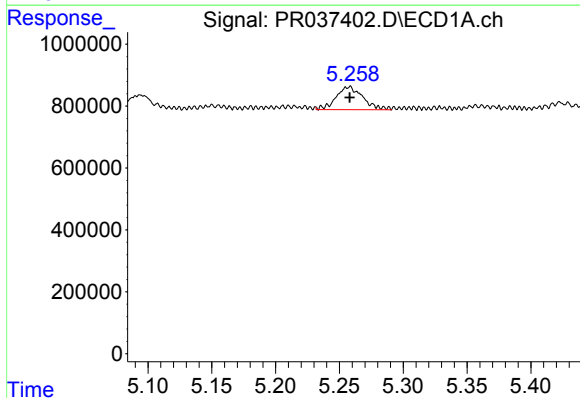


#12 AR-1232-2

R.T.: 5.258 min  
Delta R.T.: 0.000 min  
Response: 1081937  
Conc: 64.03 ng/ml

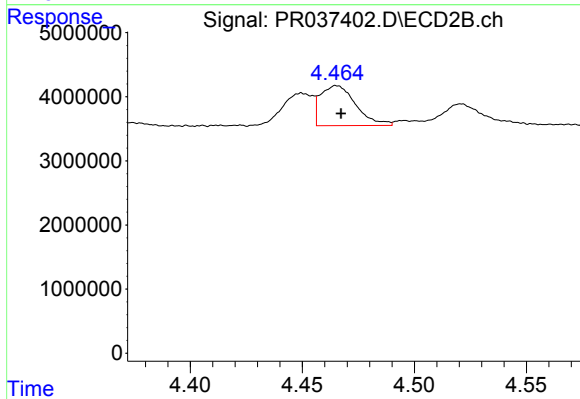

#12 AR-1232-2


R.T.: 4.465 min  
Delta R.T.: -0.002 min  
Response: 6848459  
Conc: 49.55 ng/ml

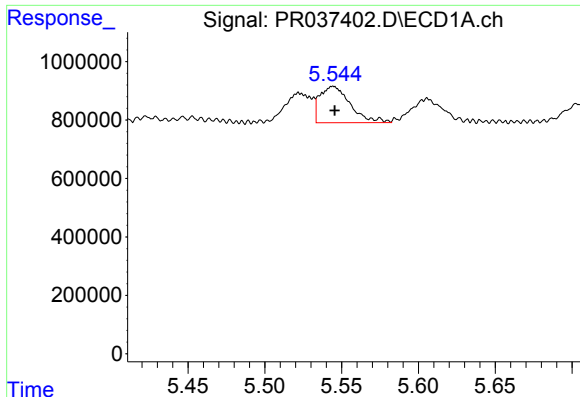

#13 AR-1232-3


R.T.: 5.544 min  
Delta R.T.: 0.000 min  
Response: 1718620  
Conc: 50.84 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

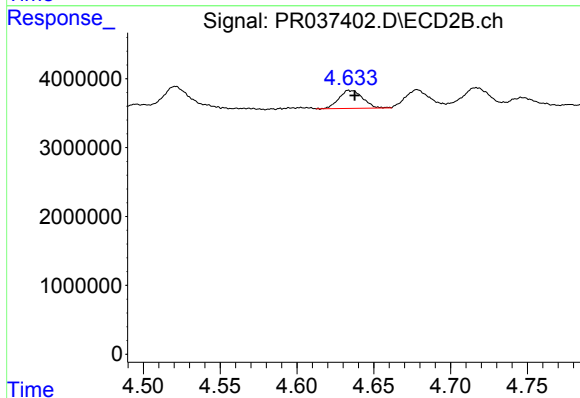


#13 AR-1232-3

R.T.: 4.633 min  
Delta R.T.: -0.004 min  
Response: 2814962  
Conc: 40.10 ng/ml

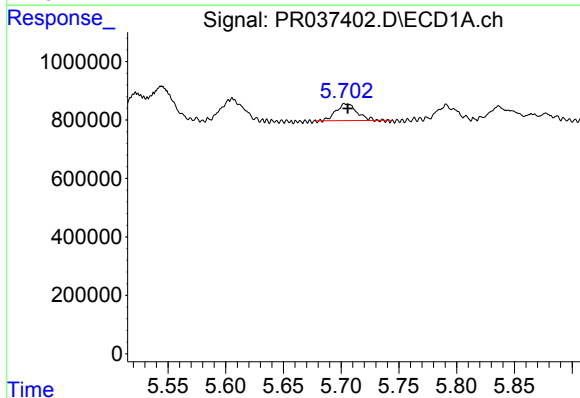


#14 AR-1232-4

R.T.: 5.703 min  
Delta R.T.: -0.002 min  
Response: 707606  
Conc: 45.08 ng/ml

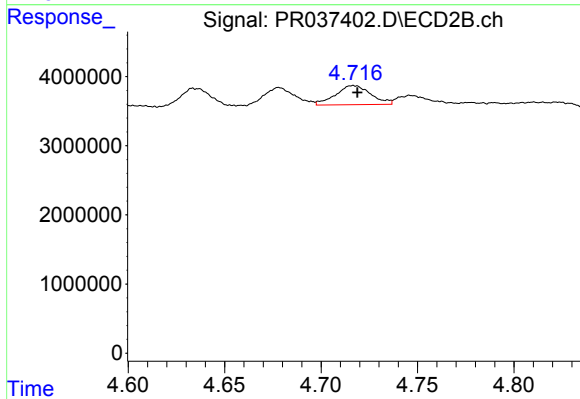

#14 AR-1232-4


R.T.: 4.717 min  
Delta R.T.: -0.002 min  
Response: 3520733  
Conc: 59.00 ng/ml

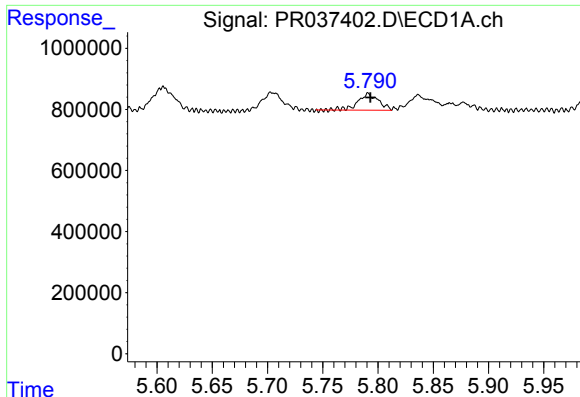

#15 AR-1232-5


R.T.: 5.791 min  
Delta R.T.: -0.002 min  
Response: 700378  
Conc: 59.88 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

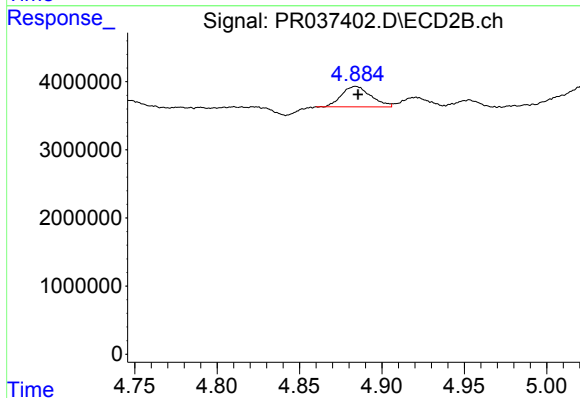


#15 AR-1232-5

R.T.: 4.884 min  
Delta R.T.: -0.001 min  
Response: 3705177  
Conc: 54.29 ng/ml

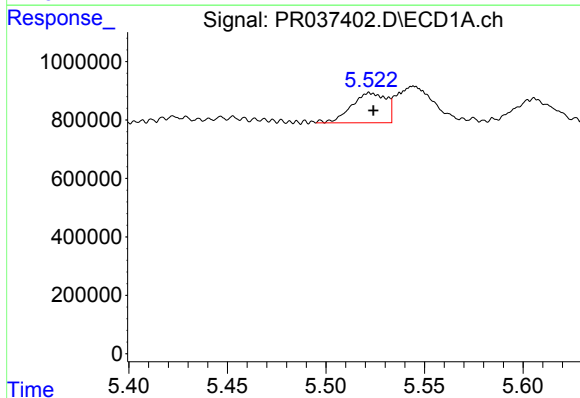


#16 AR-1242-1

R.T.: 5.522 min  
Delta R.T.: -0.002 min  
Response: 1256498  
Conc: 36.72 ng/ml

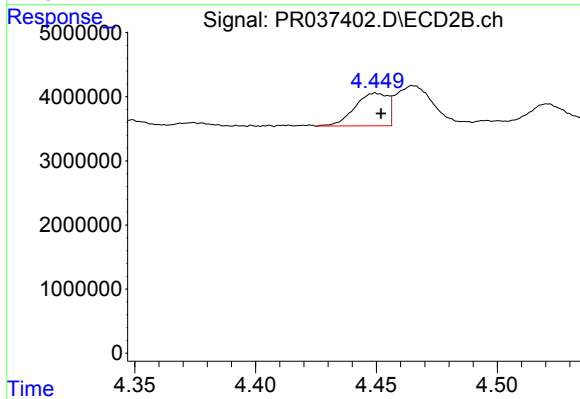

#16 AR-1242-1


R.T.: 4.450 min  
Delta R.T.: -0.002 min  
Response: 4842150  
Conc: 33.04 ng/ml

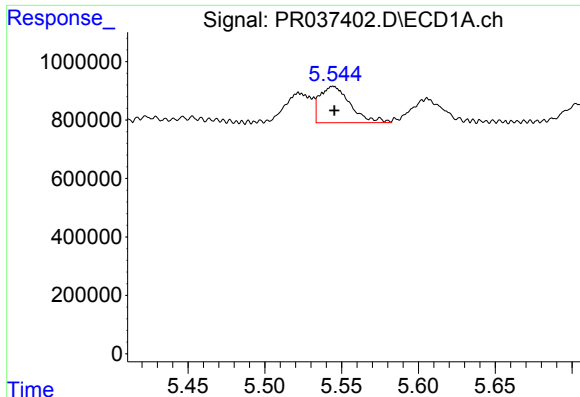

#17 AR-1242-2


R.T.: 5.544 min  
Delta R.T.: 0.000 min  
Response: 1718620  
Conc: 30.98 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

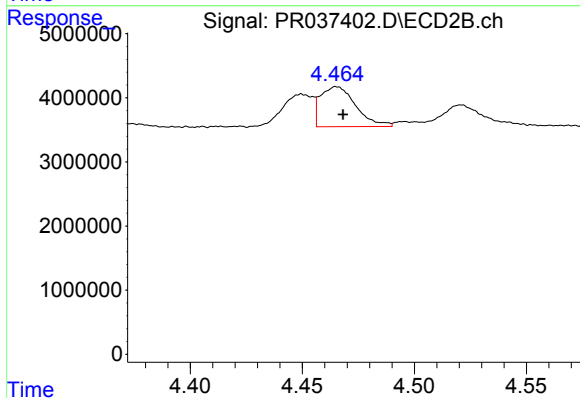


#17 AR-1242-2

R.T.: 4.465 min  
Delta R.T.: -0.003 min  
Response: 6848459  
Conc: 30.02 ng/ml

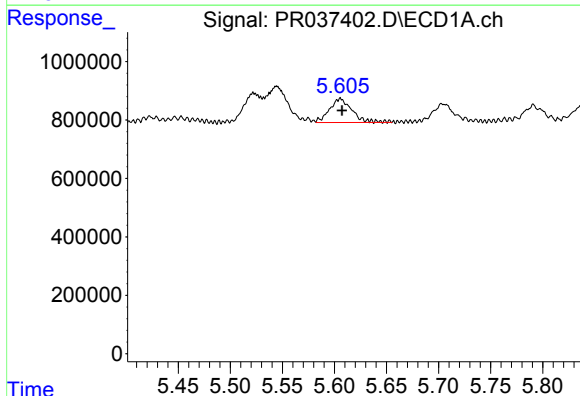


#18 AR-1242-3

R.T.: 5.606 min  
Delta R.T.: -0.002 min  
Response: 1236882  
Conc: 37.58 ng/ml

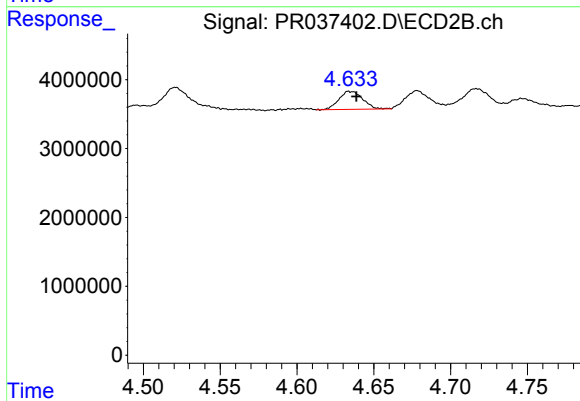

#18 AR-1242-3


R.T.: 4.633 min  
Delta R.T.: -0.005 min  
Response: 2814962  
Conc: 24.34 ng/ml

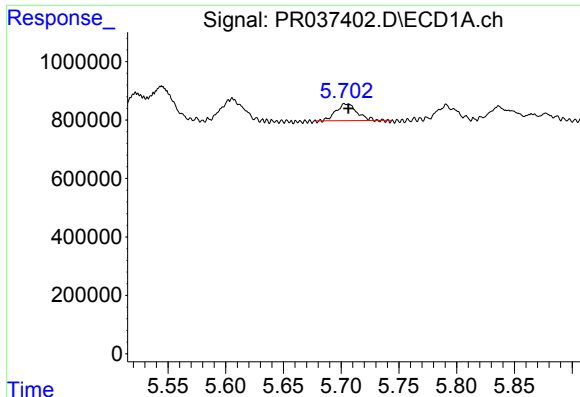

#19 AR-1242-4


R.T.: 5.703 min  
Delta R.T.: -0.003 min  
Response: 707606  
Conc: 26.83 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

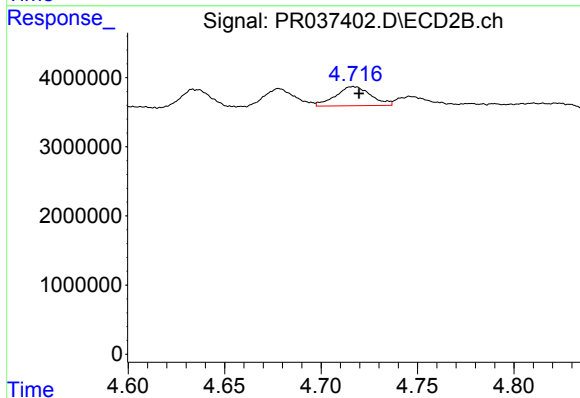


#19 AR-1242-4

R.T.: 4.717 min  
Delta R.T.: -0.003 min  
Response: 3520733  
Conc: 32.03 ng/ml

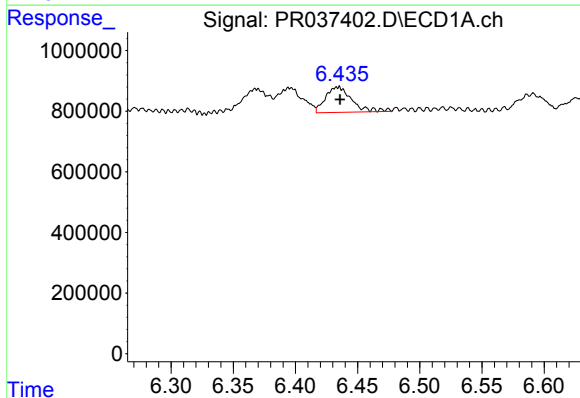


#20 AR-1242-5

R.T.: 6.434 min  
Delta R.T.: -0.002 min  
Response: 1229501  
Conc: 38.21 ng/ml

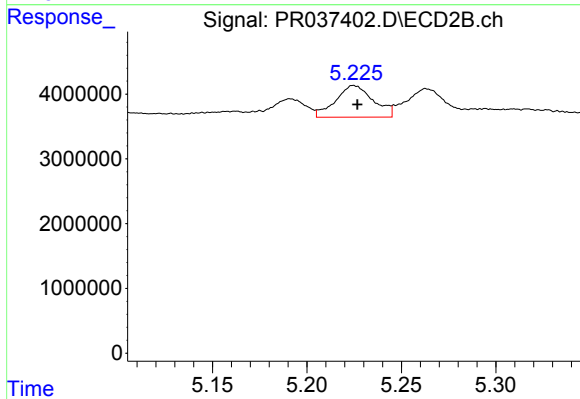

#20 AR-1242-5


R.T.: 5.225 min  
Delta R.T.: -0.002 min  
Response: 6768349  
Conc: 40.85 ng/ml

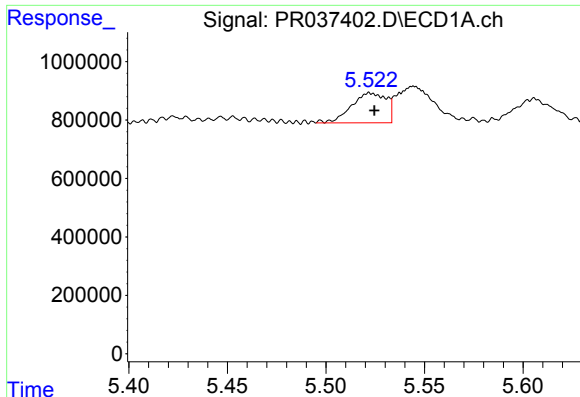

#21 AR-1248-1


R.T.: 5.522 min  
Delta R.T.: -0.002 min  
Response: 1256498  
Conc: 54.85 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

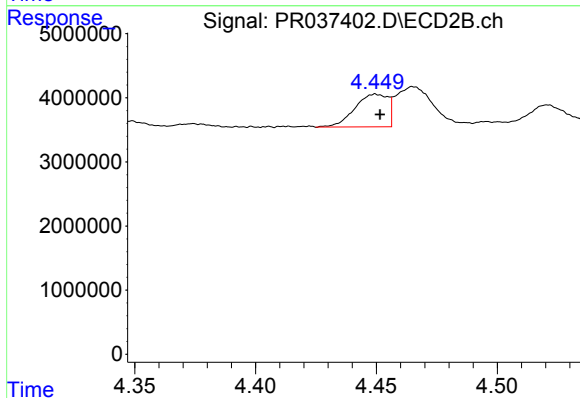


#21 AR-1248-1

R.T.: 4.450 min  
Delta R.T.: -0.002 min  
Response: 4842150  
Conc: 48.10 ng/ml

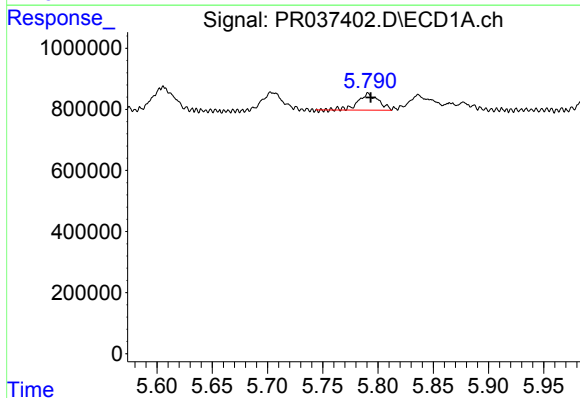


#22 AR-1248-2

R.T.: 5.791 min  
Delta R.T.: -0.002 min  
Response: 700378  
Conc: 20.00 ng/ml

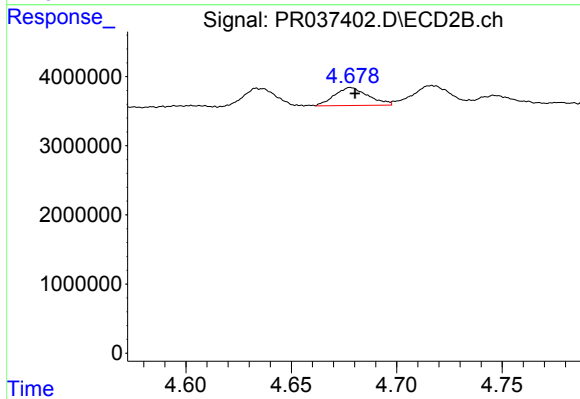

#22 AR-1248-2


R.T.: 4.678 min  
Delta R.T.: -0.002 min  
Response: 2879316  
Conc: 21.10 ng/ml

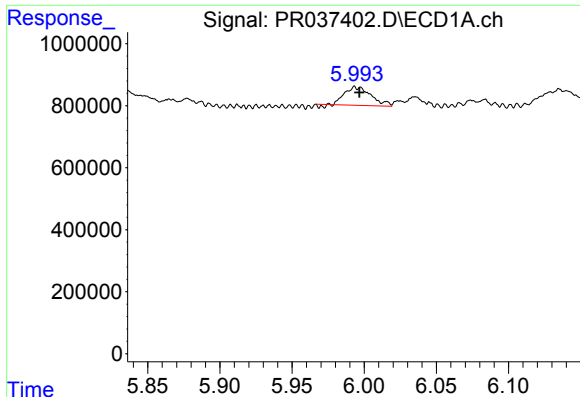

#23 AR-1248-3


R.T.: 5.994 min  
Delta R.T.: -0.003 min  
Response: 739477  
Conc: 18.08 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

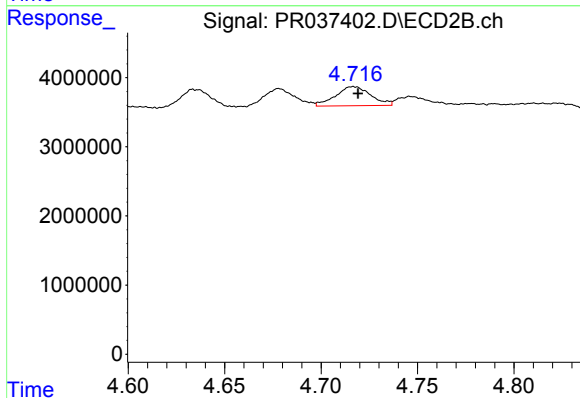


#23 AR-1248-3

R.T.: 4.717 min  
Delta R.T.: -0.003 min  
Response: 3520733  
Conc: 25.15 ng/ml

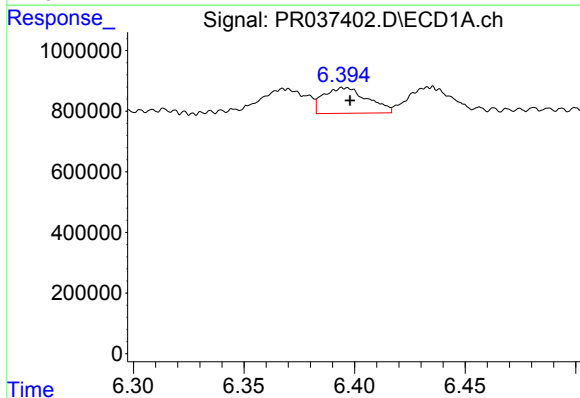


#24 AR-1248-4

R.T.: 6.396 min  
Delta R.T.: -0.002 min  
Response: 1166770  
Conc: 23.83 ng/ml

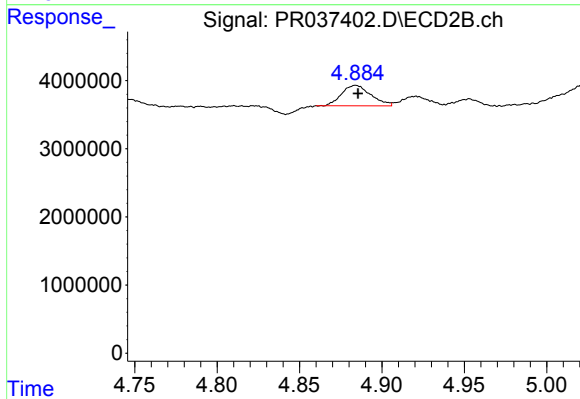

#24 AR-1248-4


R.T.: 4.884 min  
Delta R.T.: -0.002 min  
Response: 3705177  
Conc: 20.82 ng/ml

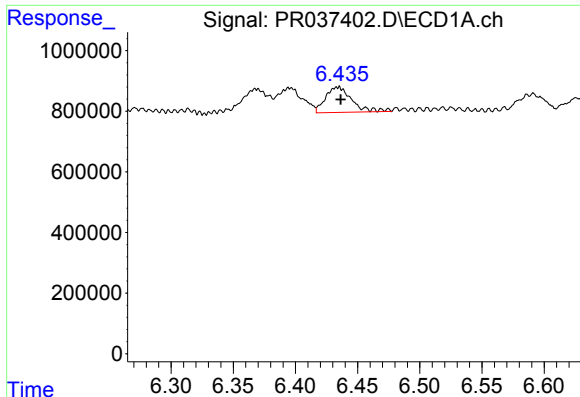

#25 AR-1248-5


R.T.: 6.434 min  
Delta R.T.: -0.002 min  
Response: 1229501  
Conc: 26.03 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

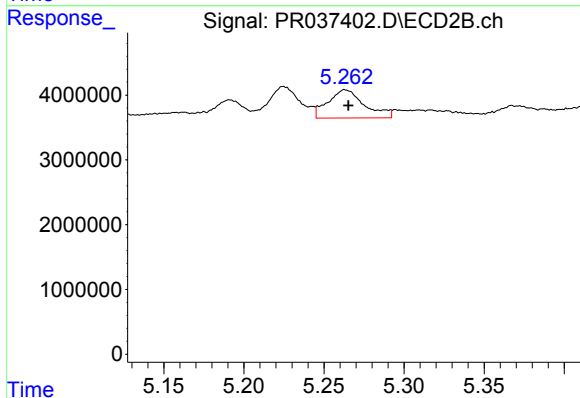


#25 AR-1248-5

R.T.: 5.263 min  
Delta R.T.: -0.002 min  
Response: 6909238  
Conc: 35.32 ng/ml

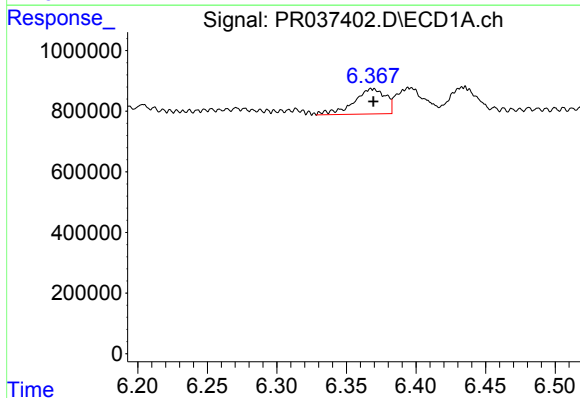


#26 AR-1254-1

R.T.: 6.369 min  
Delta R.T.: 0.000 min  
Response: 1314293  
Conc: 24.06 ng/ml

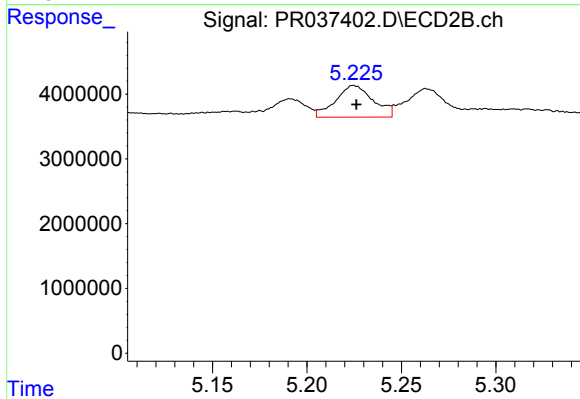

#26 AR-1254-1


R.T.: 5.225 min  
Delta R.T.: -0.002 min  
Response: 6768349  
Conc: 19.65 ng/ml

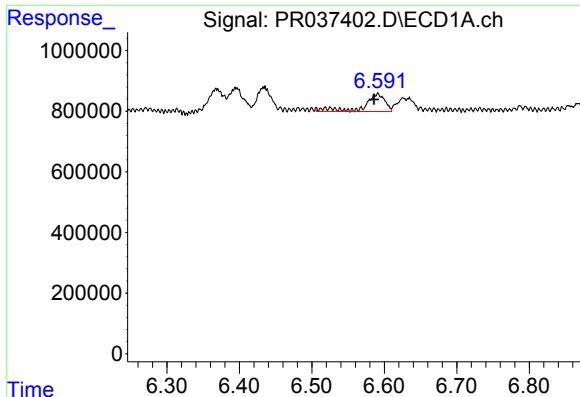

#27 AR-1254-2


R.T.: 6.591 min  
Delta R.T.: 0.005 min  
Response: 1124034  
Conc: 13.12 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

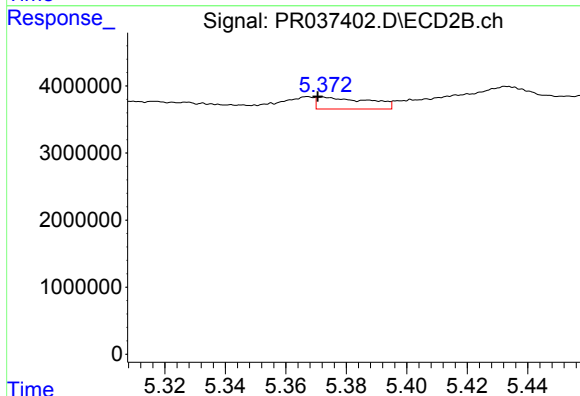


#27 AR-1254-2

R.T.: 5.372 min  
Delta R.T.: 0.002 min  
Response: 2104266  
Conc: 7.03 ng/ml

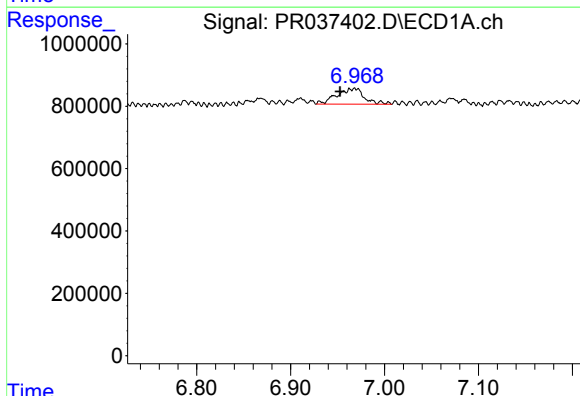


#28 AR-1254-3

R.T.: 6.968 min  
Delta R.T.: 0.016 min  
Response: 1029891  
Conc: 11.32 ng/ml

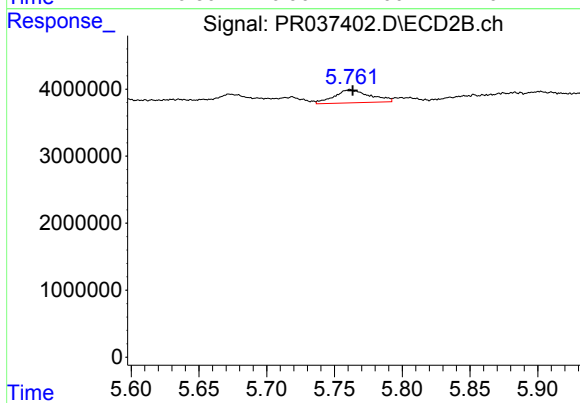

#28 AR-1254-3


R.T.: 5.761 min  
Delta R.T.: -0.002 min  
Response: 3570961  
Conc: 7.54 ng/ml

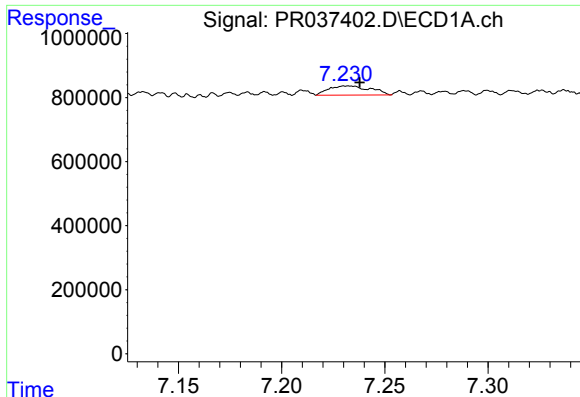

#29 AR-1254-4


R.T.: 7.232 min  
Delta R.T.: -0.006 min  
Response: 400154  
Conc: 5.97 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

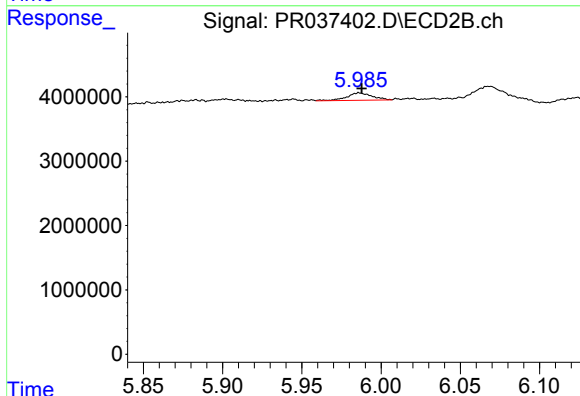


#29 AR-1254-4

R.T.: 5.986 min  
Delta R.T.: -0.002 min  
Response: 1294802  
Conc: 3.69 ng/ml

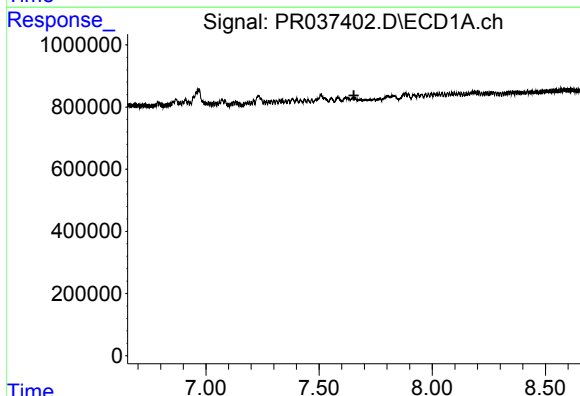


#30 AR-1254-5

R.T.: 0.000 min  
Exp R.T. : 7.654 min  
Response: 0  
Conc: N.D.

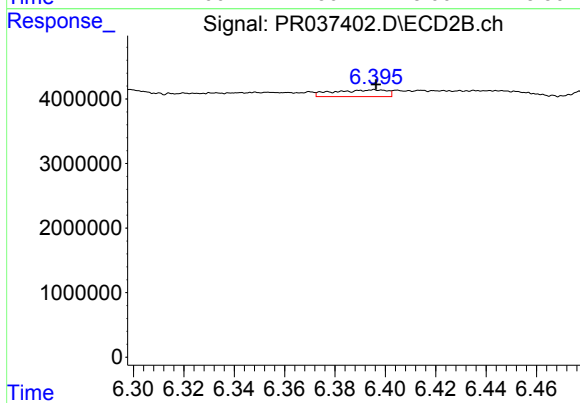

#30 AR-1254-5


R.T.: 6.396 min  
Delta R.T.: 0.000 min  
Response: 1529284  
Conc: 3.45 ng/ml

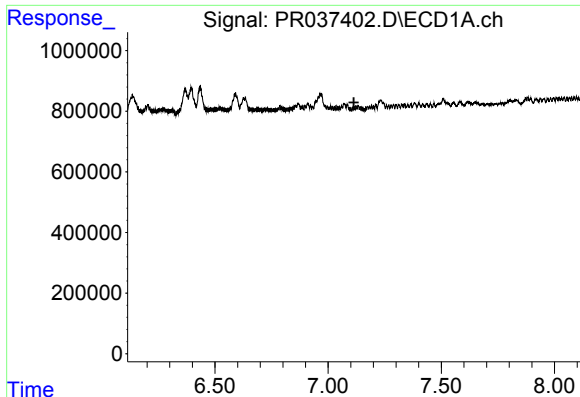

#31 AR-1260-1


R.T.: 0.000 min  
Exp R.T.: 7.114 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

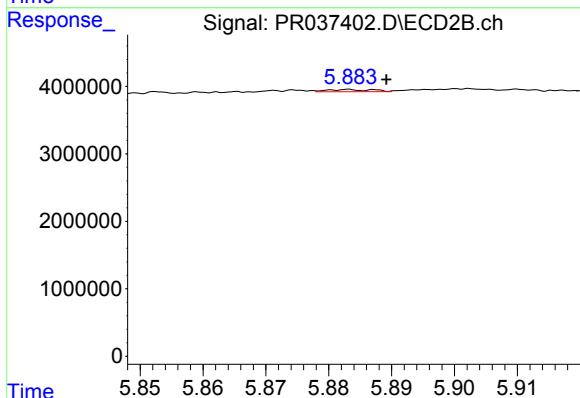


#31 AR-1260-1

R.T.: 5.883 min  
Delta R.T.: -0.006 min  
Response: 162967  
Conc: 0.56 ng/ml

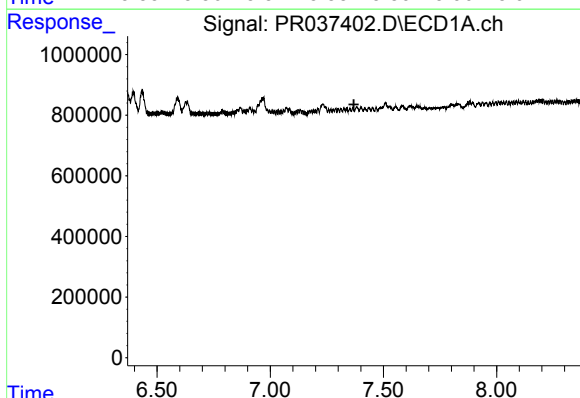


#32 AR-1260-2

R.T.: 0.000 min  
Exp R.T.: 7.369 min  
Response: 0  
Conc: N.D.

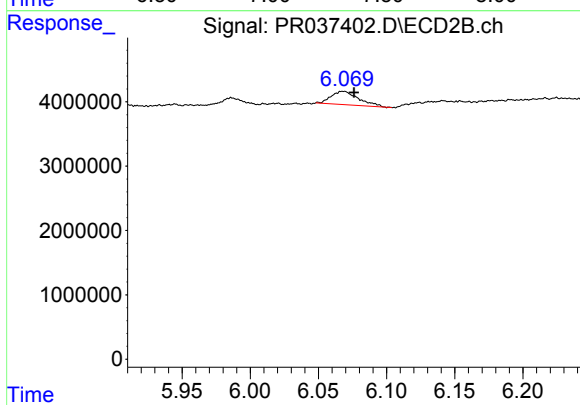

#32 AR-1260-2


R.T.: 6.067 min  
Delta R.T.: -0.009 min  
Response: 2856004  
Conc: 6.20 ng/ml

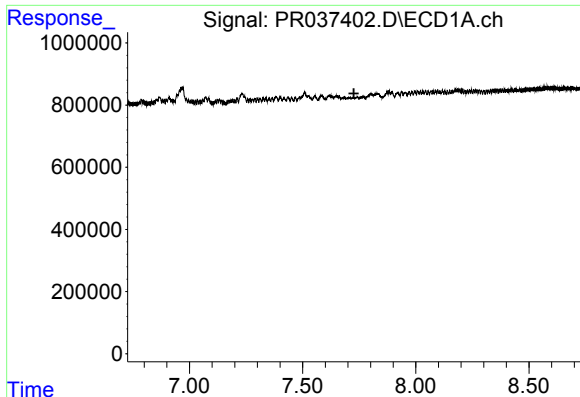

#33 AR-1260-3


R.T.: 0.000 min  
Exp R.T.: 7.726 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

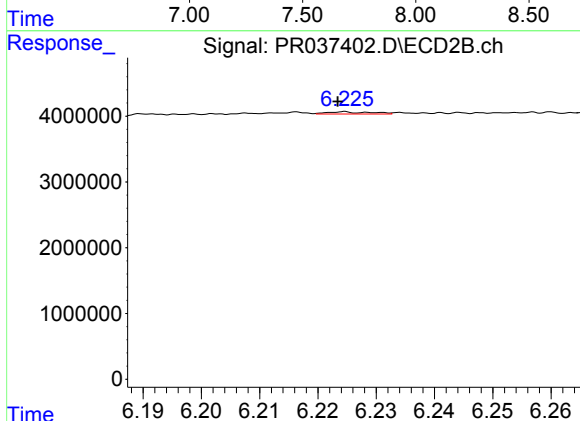


#33 AR-1260-3

R.T.: 6.225 min  
Delta R.T.: 0.001 min  
Response: 179569  
Conc: 0.50 ng/ml

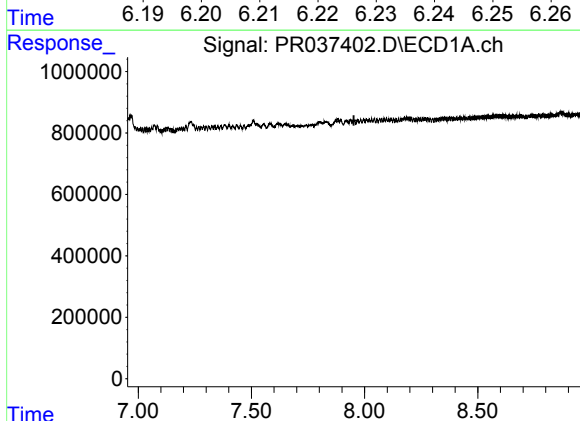


#34 AR-1260-4

R.T.: 0.000 min  
Exp R.T.: 7.953 min  
Response: 0  
Conc: N.D.

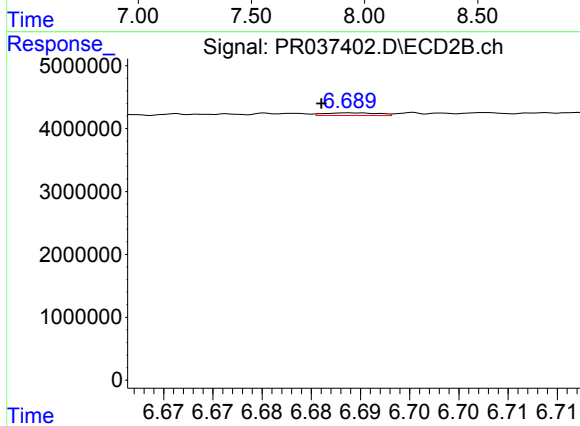

#34 AR-1260-4


R.T.: 6.689 min  
Delta R.T.: 0.003 min  
Response: 163146  
Conc: 0.54 ng/ml

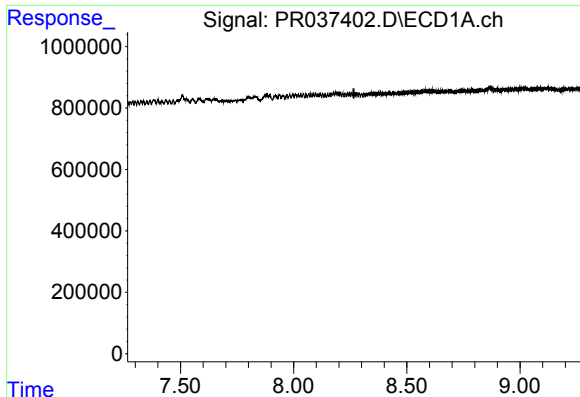

#35 AR-1260-5


R.T.: 0.000 min  
Exp R.T.: 8.266 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

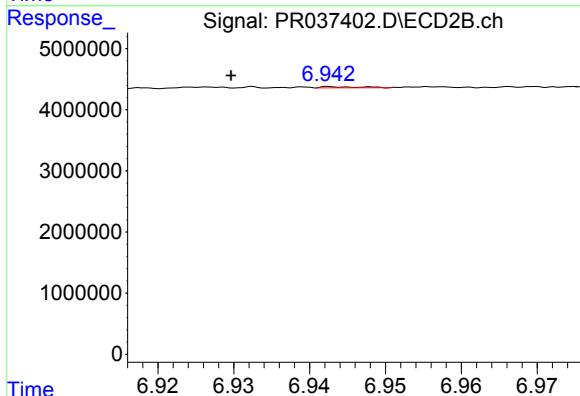


#35 AR-1260-5

R.T.: 6.943 min  
Delta R.T.: 0.013 min  
Response: 69858  
Conc: 0.08 ng/ml

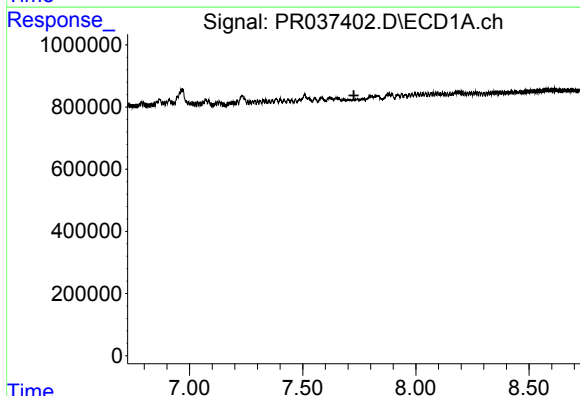


#36 AR-1262-1

R.T.: 0.000 min  
Exp R.T.: 7.726 min  
Response: 0  
Conc: N.D.

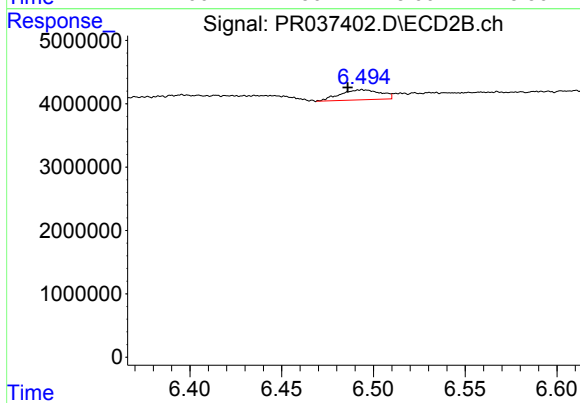

#36 AR-1262-1


R.T.: 6.494 min  
Delta R.T.: 0.008 min  
Response: 2452641  
Conc: 9.79 ng/ml

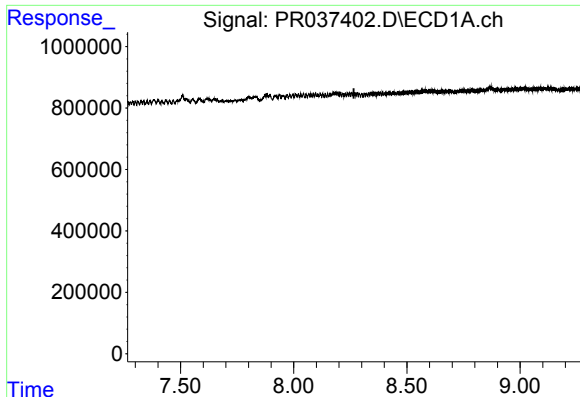

#37 AR-1262-2


R.T.: 0.000 min  
Exp R.T.: 8.266 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

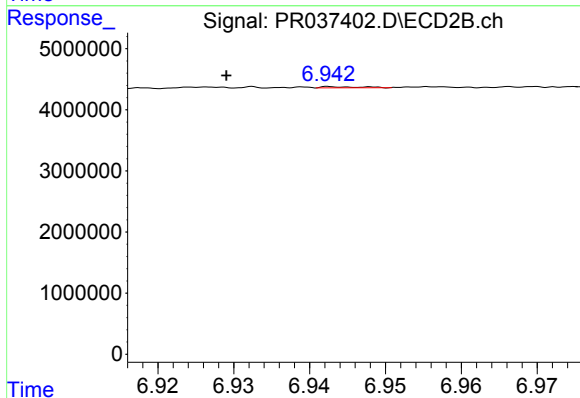


#37 AR-1262-2

R.T.: 6.943 min  
Delta R.T.: 0.014 min  
Response: 69858  
Conc: 0.06 ng/ml

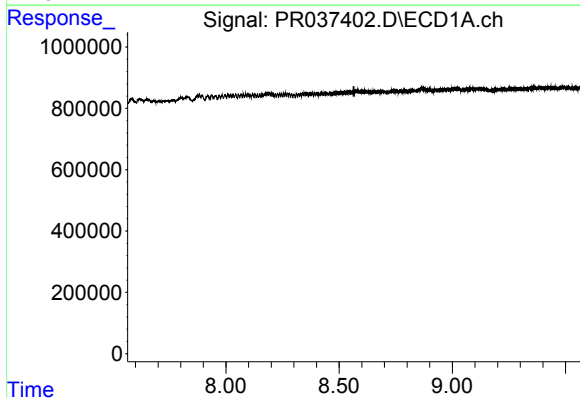


#38 AR-1262-3

R.T.: 0.000 min  
Exp R.T.: 8.565 min  
Response: 0  
Conc: N.D.

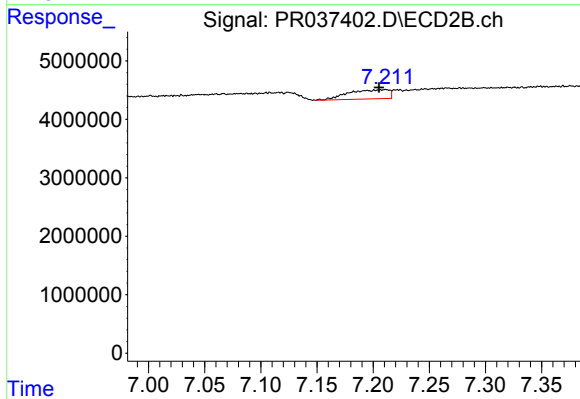

#38 AR-1262-3


R.T.: 7.211 min  
Delta R.T.: 0.006 min  
Response: 3961546  
Conc: 7.23 ng/ml

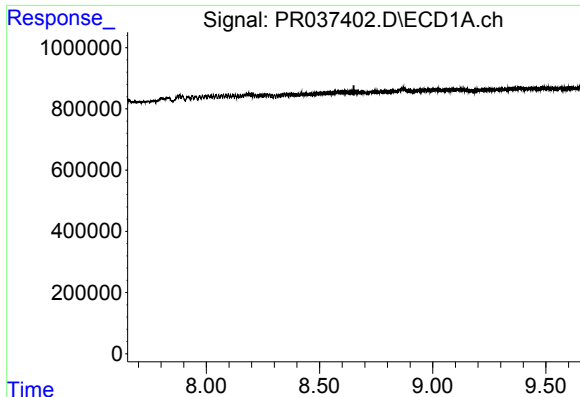

#39 AR-1262-4


R.T.: 0.000 min  
Exp R.T.: 8.652 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

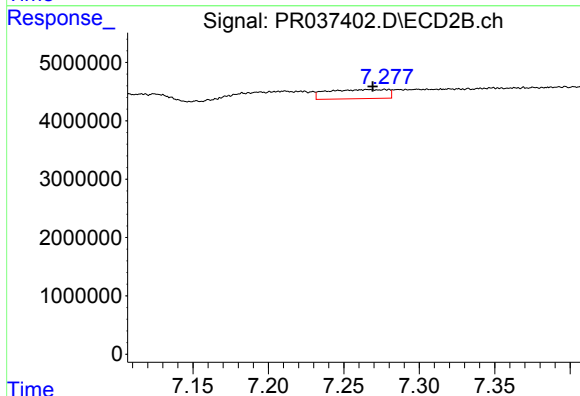


#39 AR-1262-4

R.T.: 7.278 min  
Delta R.T.: 0.008 min  
Response: 4329269  
Conc: 4.82 ng/ml

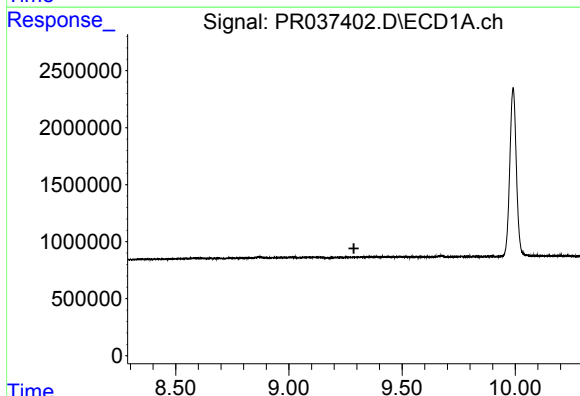


#40 AR-1262-5

R.T.: 0.000 min  
Exp R.T.: 9.287 min  
Response: 0  
Conc: N.D.

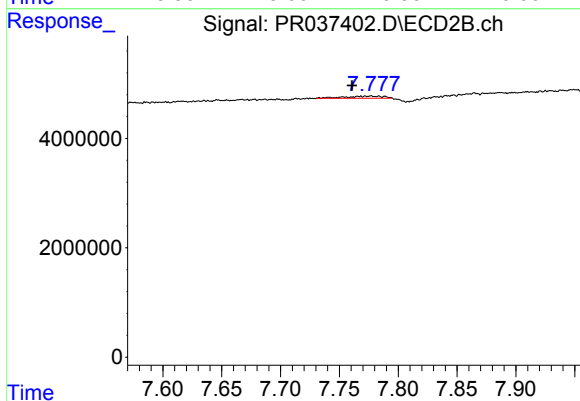

#40 AR-1262-5


R.T.: 7.777 min  
Delta R.T.: 0.016 min  
Response: 889781  
Conc: 2.33 ng/ml

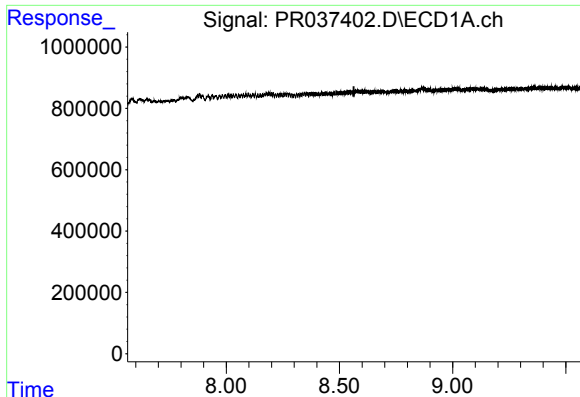

#41 AR-1268-1


R.T.: 0.000 min  
Exp R.T.: 8.564 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

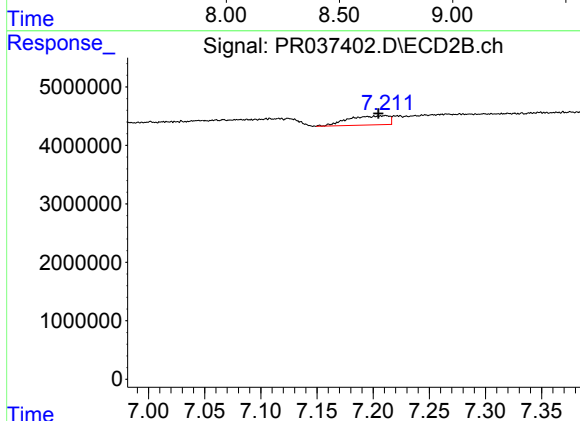


#41 AR-1268-1

R.T.: 7.211 min  
Delta R.T.: 0.006 min  
Response: 3961546  
Conc: 3.22 ng/ml

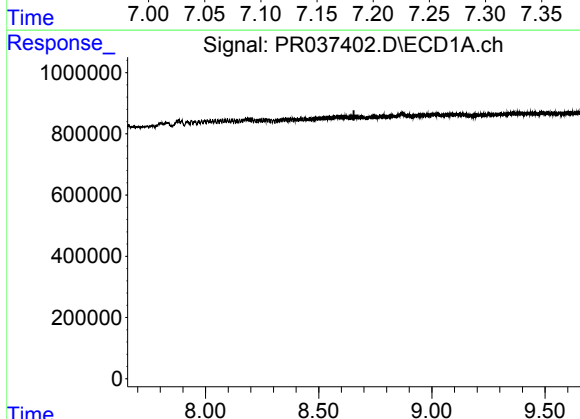


#42 AR-1268-2

R.T.: 0.000 min  
Exp R.T.: 8.655 min  
Response: 0  
Conc: N.D.

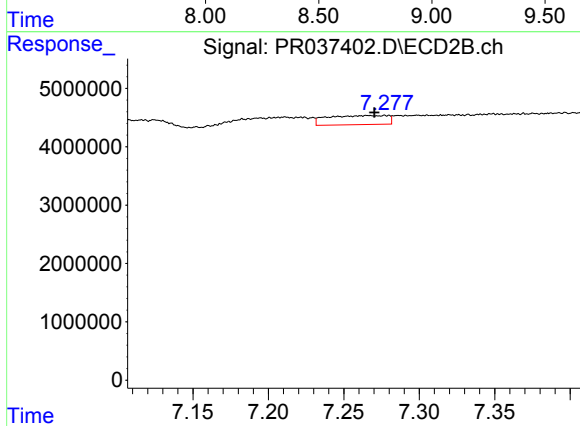

#42 AR-1268-2


R.T.: 7.278 min  
Delta R.T.: 0.007 min  
Response: 4329269  
Conc: 4.09 ng/ml

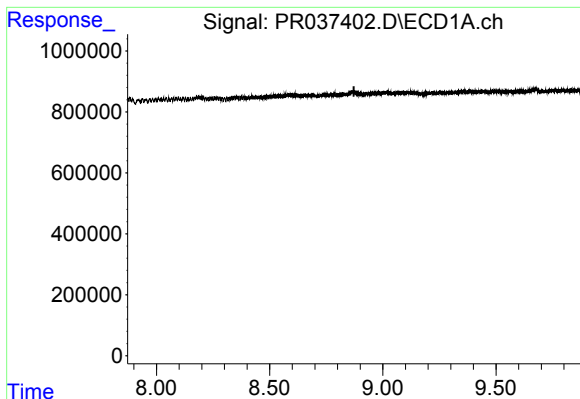

#43 AR-1268-3


R.T.: 0.000 min  
Exp R.T.: 8.872 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

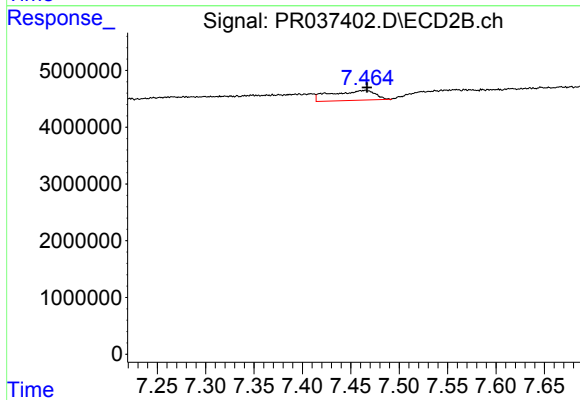


#43 AR-1268-3

R.T.: 7.465 min  
Delta R.T.: -0.002 min  
Response: 5478449  
Conc: 6.18 ng/ml

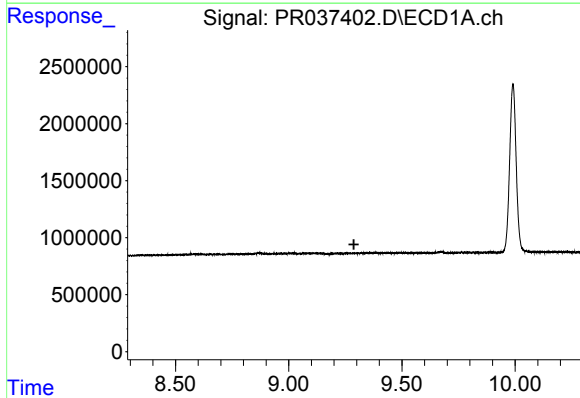


#44 AR-1268-4

R.T.: 0.000 min  
Exp R.T.: 9.288 min  
Response: 0  
Conc: N.D.

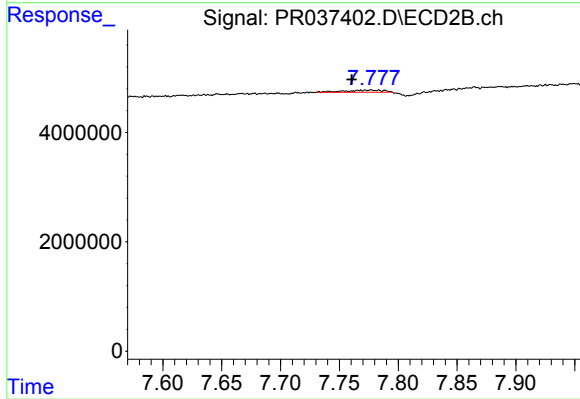

#44 AR-1268-4


R.T.: 7.777 min  
Delta R.T.: 0.017 min  
Response: 889781  
Conc: 2.45 ng/ml

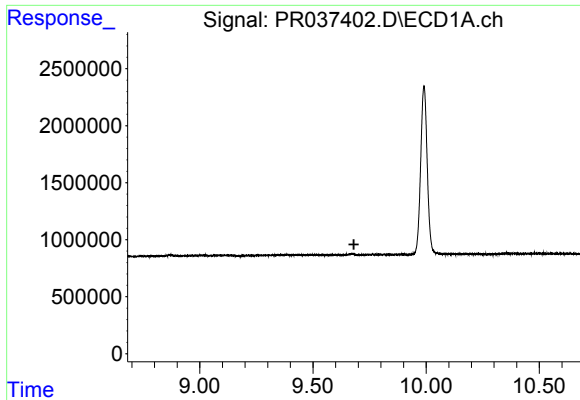

#45 AR-1268-5

R.T.: 0.000 min  
Exp R.T.: 9.681 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

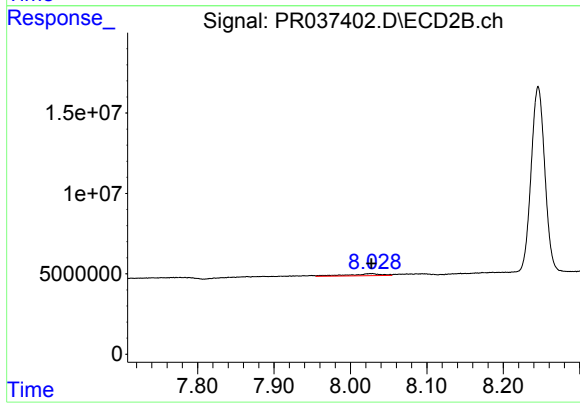

#45 AR-1268-5

R.T.: 8.028 min  
Delta R.T.: 0.000 min  
Response: 3695557  
Conc: 1.45 ng/ml