

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
 Data File : PR037403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 16:22
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1248 MDL 25PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:43:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.409	29508371	118.3E6	23.588	24.662
2)	SA Decachlor...	9.983	8.242	33931809	170.9E6	25.656	29.346
Target Compounds							
3)	L1 AR-1016-1	5.517	4.451	653687	3255498	15.171	17.879
4)	L1 AR-1016-2	5.540	4.467	1030479	3525813	14.881	12.497
5)	L1 AR-1016-3	5.602	4.638	617985	1326443	15.324	9.225 #
6)	L1 AR-1016-4	0.000	4.679	0	4399465	N.D.	39.766 #
7)	L1 AR-1016-5	5.990	4.884	1164733	6003445	33.967	39.494
8)	L2 AR-1221-1	0.000	3.567	0	263864	N.D.	5.182 #
9)	L2 AR-1221-2	4.668	3.698	401200	1488339	44.361	40.078
10)	L2 AR-1221-3	4.668	3.770	401200	455819	13.090	3.723 #
11)	L3 AR-1232-1	4.668	3.770	401200	455819	13.716	3.896 #
12)	L3 AR-1232-2	5.252	4.467	485221	3525813	28.716	25.508
13)	L3 AR-1232-3	5.540	4.638	1030479	1326443	30.483	18.895 #
14)	L3 AR-1232-4	0.000	4.718	0	4381213	N.D.	73.422 #
15)	L3 AR-1232-5	5.787	4.884	1234901	6003445	105.586	87.971
16)	L4 AR-1242-1	5.517	4.451	653687	3255498	19.106	22.216
17)	L4 AR-1242-2	5.540	4.467	1030479	3525813	18.577	15.453
18)	L4 AR-1242-3	5.602	4.638	617985	1326443	18.775	11.471 #
19)	L4 AR-1242-4	0.000	4.718	0	4381213	N.D.	39.862 #
20)	L4 AR-1242-5	6.430	5.225	1839050	10685776	57.151	64.489
21)	L5 AR-1248-1	5.517	4.451	653687	3255498	28.536	32.340
22)	L5 AR-1248-2	5.787	4.679	1234901	4399465	35.268	32.237
23)	L5 AR-1248-3	5.990	4.718	1164733	4381213	28.471	31.300
24)	L5 AR-1248-4	6.391	4.884	1896922	6003445	38.749	33.734
25)	L5 AR-1248-5	6.430	5.264	1839050	9322764	38.932	47.659
26)	L6 AR-1254-1	6.363	5.225	1767788	10685776	32.359	31.021
27)	L6 AR-1254-2	6.585	5.371	1554027	5171321	18.134	17.266
28)	L6 AR-1254-3	6.946	5.761	1709608	6305188	18.794	13.313 #
29)	L6 AR-1254-4	7.229	5.986	858980	3274403	12.819	9.338 #
30)	L6 AR-1254-5	0.000	6.393	0	2372701	N.D.	5.358 #
31)	L7 AR-1260-1	7.071	5.883	455680	484464	6.906	1.658 #
32)	L7 AR-1260-2	0.000	6.067	0	3323802	N.D.	7.216 #
33)	L7 AR-1260-3	0.000	6.223	0	588088	N.D.	1.650 #
34)	L7 AR-1260-4	0.000	6.685	0	78775	N.D.	0.258 #
35)	L7 AR-1260-5	0.000	6.925	0	245782	N.D.	0.283 #
36)	L8 AR-1262-1	0.000	6.489	0	1286666	N.D.	5.134 #
37)	L8 AR-1262-2	0.000	6.925	0	245782	N.D.	0.196 #
38)	L8 AR-1262-3	0.000	7.203	0	428095	N.D.	0.781 #
39)	L8 AR-1262-4	0.000	7.272	0	739524	N.D.	0.824 #
40)	L8 AR-1262-5	0.000	7.757	0	538393	N.D.	1.407 #
41)	L9 AR-1268-1	0.000	7.203	0	428095	N.D.	0.348 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
 Data File : PR037403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 16:22
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1248 MDL 25PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:43:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.272	0	739524	N.D.	0.698 #
43) L9	AR-1268-3	0.000	7.465	0	945001	N.D.	1.066 #
44) L9	AR-1268-4	0.000	7.757	0	538393	N.D.	1.484 #
45) L9	AR-1268-5	0.000	8.023	0	2222926	N.D.	0.874 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
Data File : PR037403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 16:22
Operator : SM\SJ
Sample : K2241-09
Misc : AR1248 MDL 25PPB
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 00:43:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

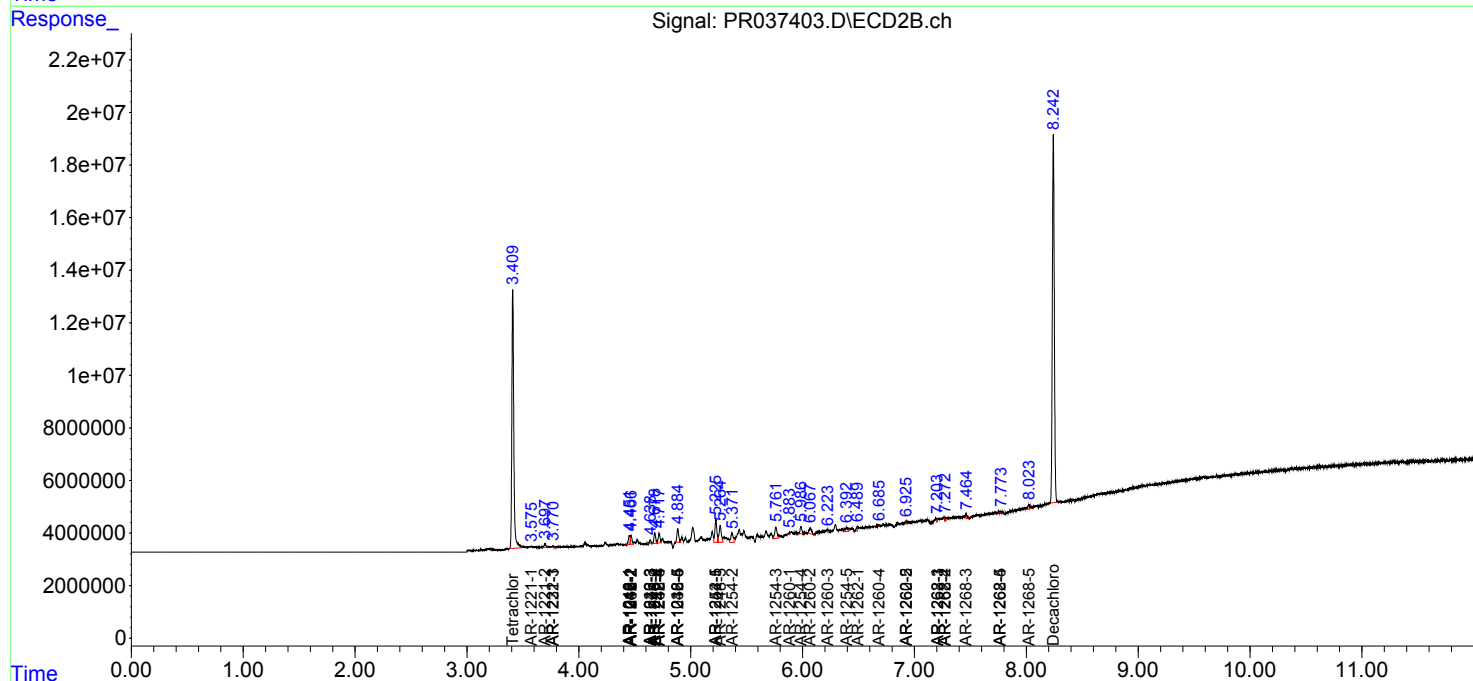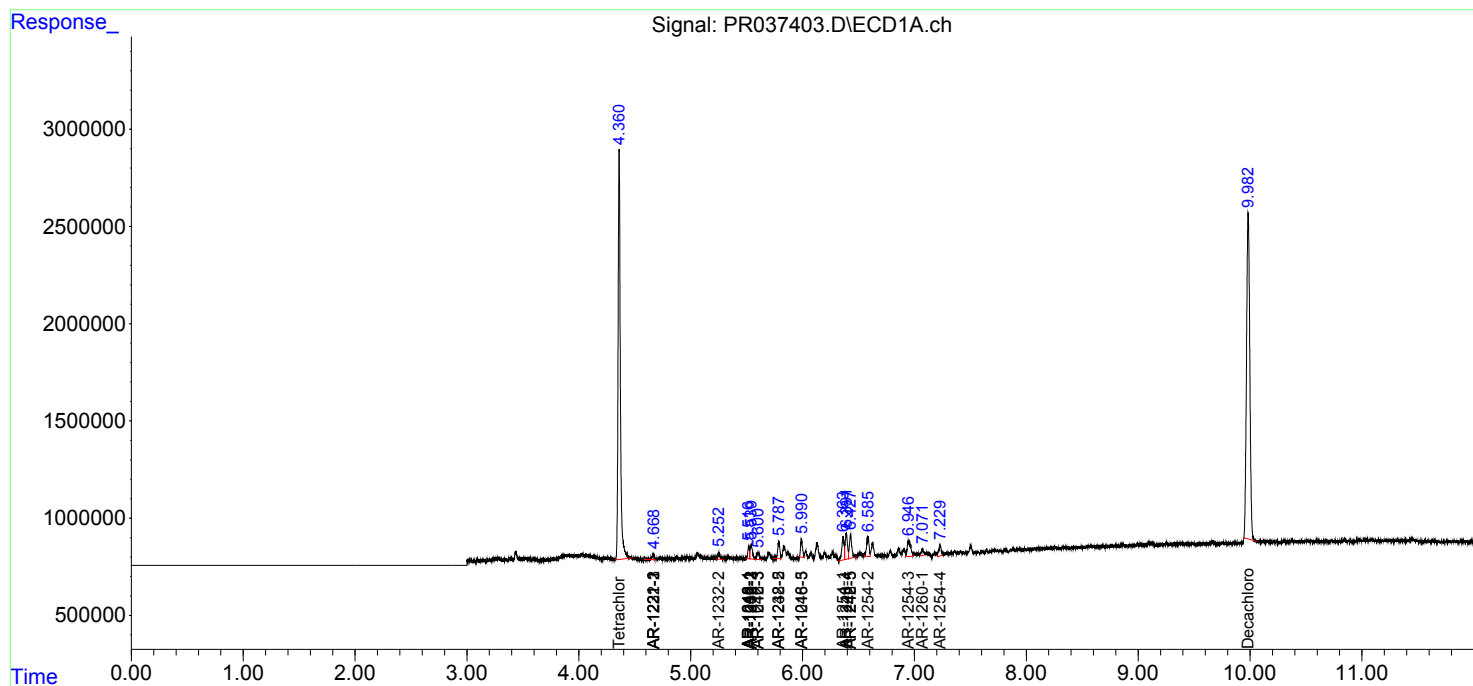


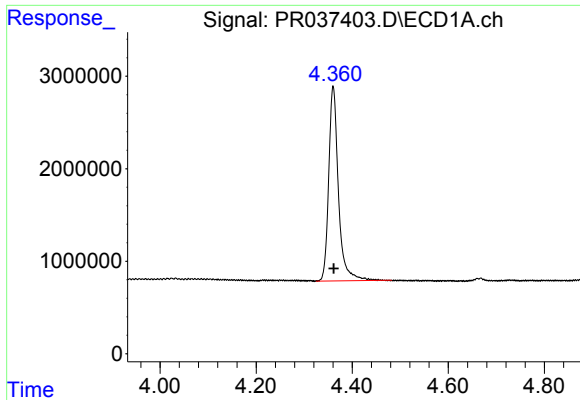

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 29508371
Conc: 23.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

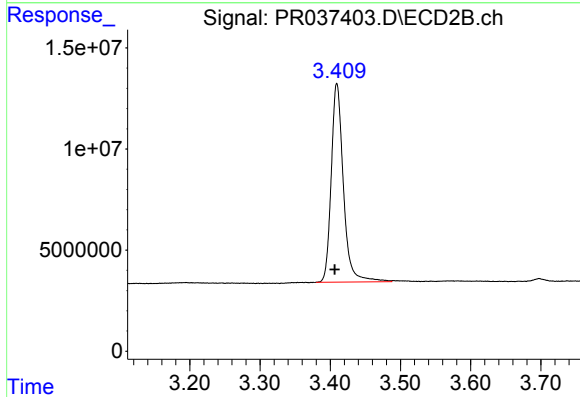


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: 0.003 min
Response: 118266016
Conc: 24.66 ng/ml

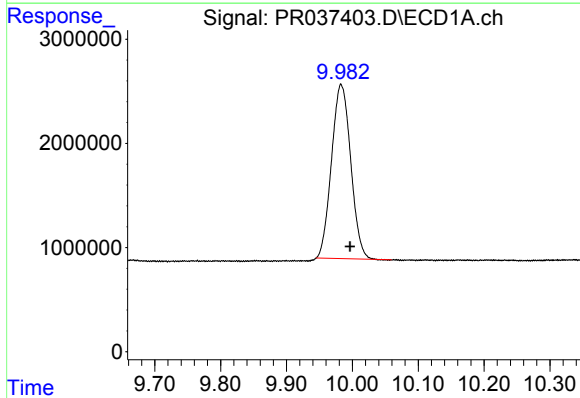


#2 Decachlorobiphenyl

R.T.: 9.983 min
Delta R.T.: -0.014 min
Response: 33931809
Conc: 25.66 ng/ml

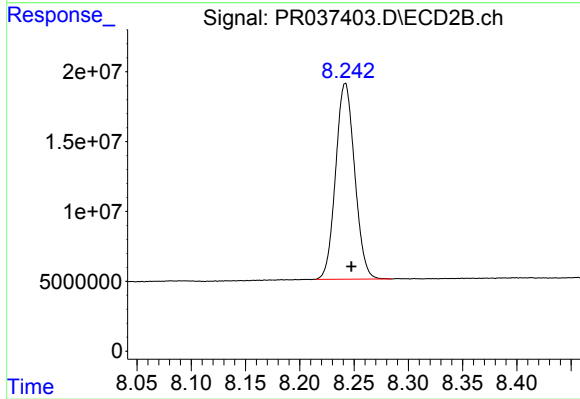

#2 Decachlorobiphenyl


R.T.: 8.242 min
Delta R.T.: -0.005 min
Response: 170920874
Conc: 29.35 ng/ml

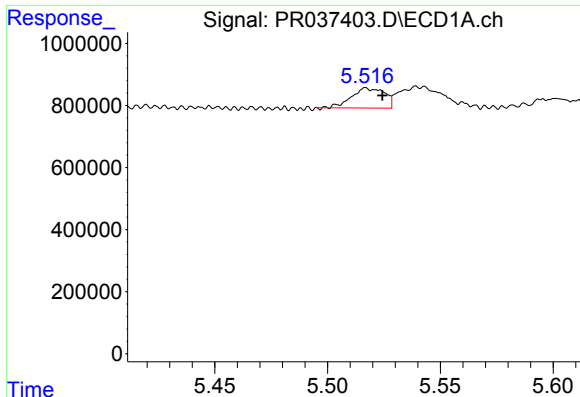

#3 AR-1016-1


R.T.: 5.517 min
Delta R.T.: -0.007 min
Response: 653687
Conc: 15.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

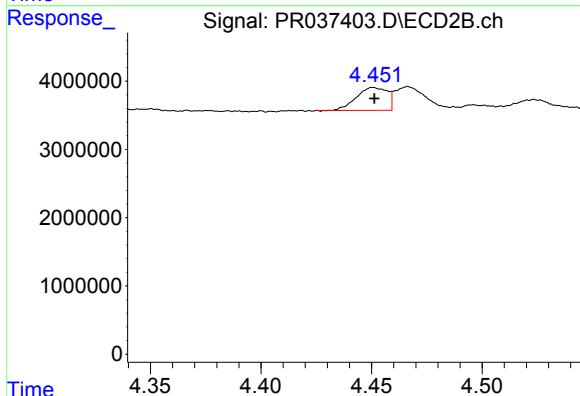


#3 AR-1016-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3255498
Conc: 17.88 ng/ml

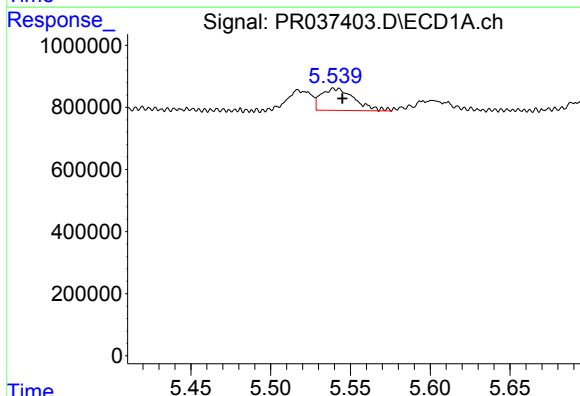


#4 AR-1016-2

R.T.: 5.540 min
Delta R.T.: -0.005 min
Response: 1030479
Conc: 14.88 ng/ml

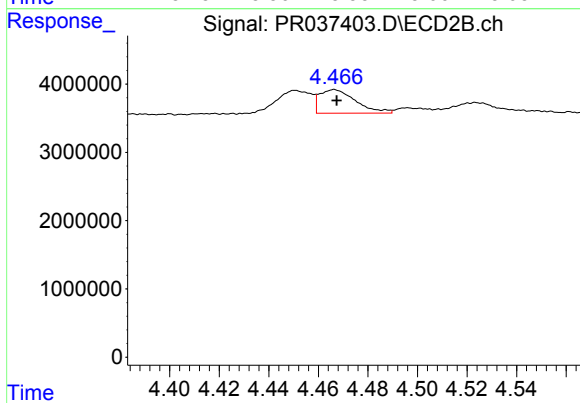

#4 AR-1016-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3525813
Conc: 12.50 ng/ml

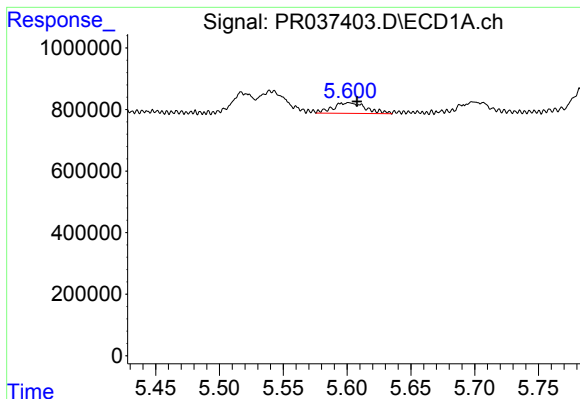

#5 AR-1016-3


R.T.: 5.602 min
Delta R.T.: -0.006 min
Response: 617985
Conc: 15.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

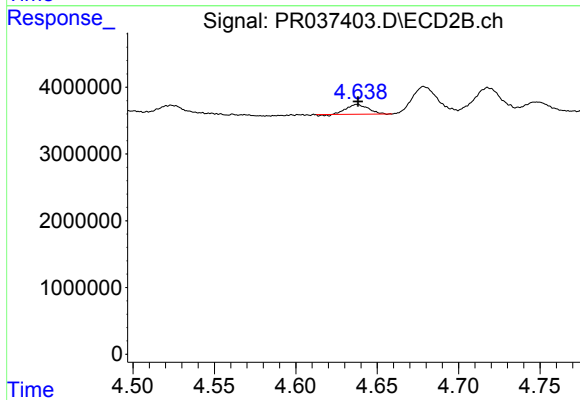


#5 AR-1016-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 1326443
Conc: 9.23 ng/ml

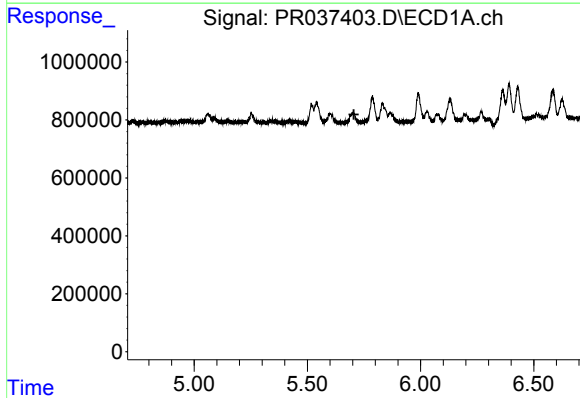


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.705 min
Response: 0
Conc: N.D.

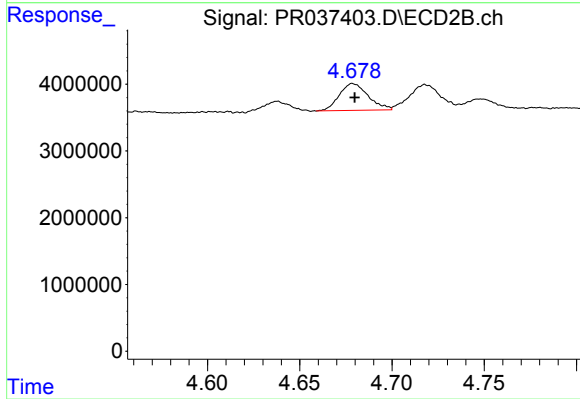

#6 AR-1016-4


R.T.: 4.679 min
Delta R.T.: -0.001 min
Response: 4399465
Conc: 39.77 ng/ml

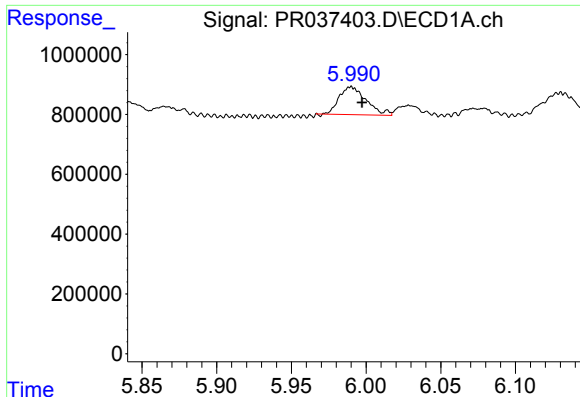

#7 AR-1016-5


R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 1164733
Conc: 33.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

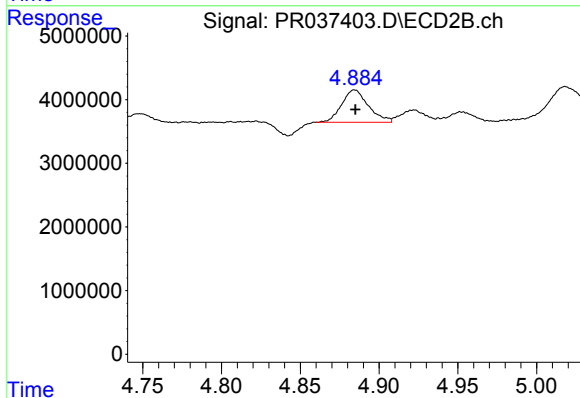


#7 AR-1016-5

R.T.: 4.884 min
Delta R.T.: 0.000 min
Response: 6003445
Conc: 39.49 ng/ml

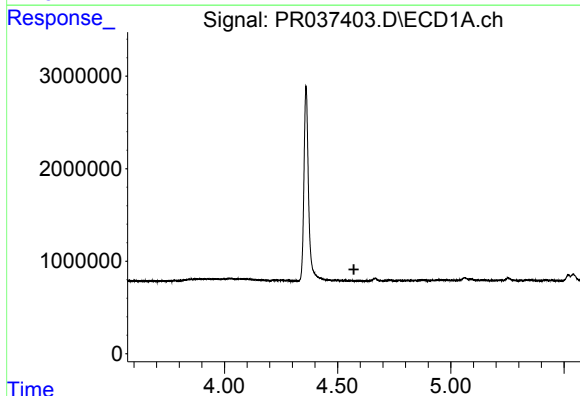


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

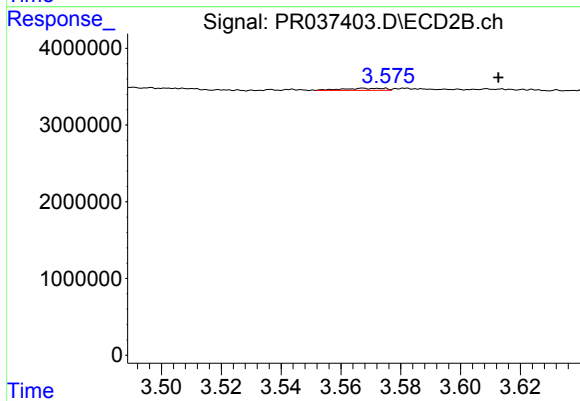

#8 AR-1221-1


R.T.: 3.567 min
Delta R.T.: -0.045 min
Response: 263864
Conc: 5.18 ng/ml

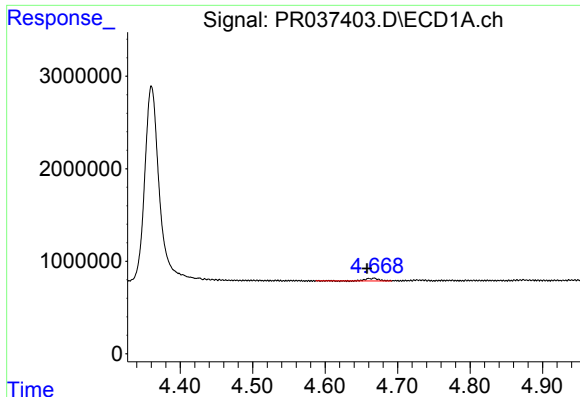

#9 AR-1221-2


R.T.: 4.668 min
Delta R.T.: 0.010 min
Response: 401200
Conc: 44.36 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

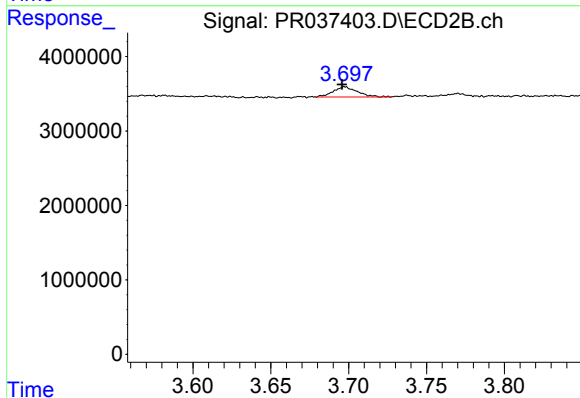


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.002 min
Response: 1488339
Conc: 40.08 ng/ml

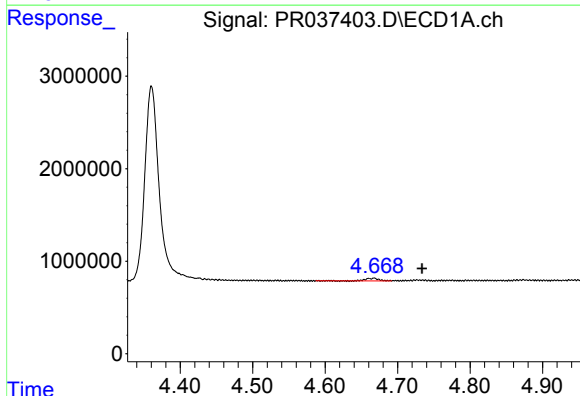


#10 AR-1221-3

R.T.: 4.668 min
Delta R.T.: -0.066 min
Response: 401200
Conc: 13.09 ng/ml

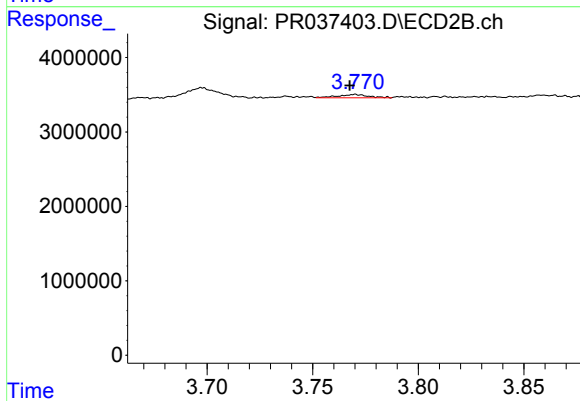

#10 AR-1221-3


R.T.: 3.770 min
Delta R.T.: 0.003 min
Response: 455819
Conc: 3.72 ng/ml

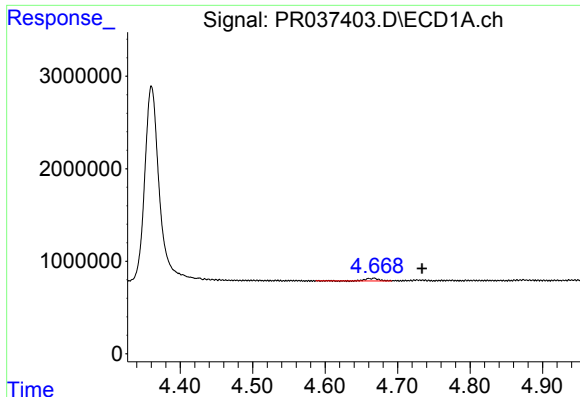

#11 AR-1232-1


R.T.: 4.668 min
Delta R.T.: -0.066 min
Response: 401200
Conc: 13.72 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

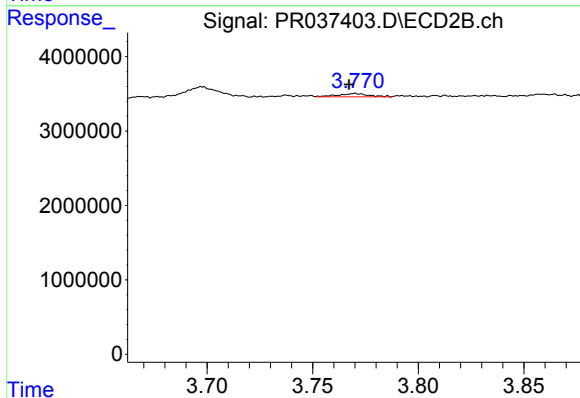


#11 AR-1232-1

R.T.: 3.770 min
Delta R.T.: 0.003 min
Response: 455819
Conc: 3.90 ng/ml

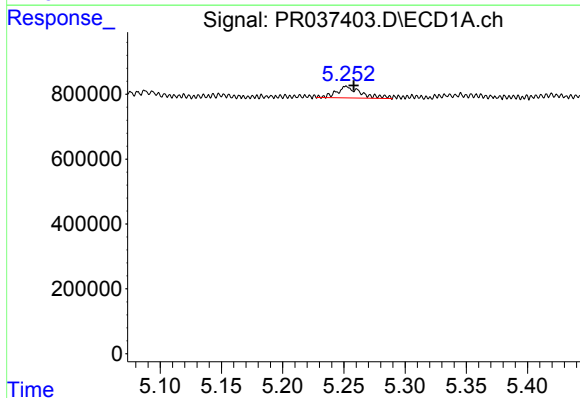


#12 AR-1232-2

R.T.: 5.252 min
Delta R.T.: -0.006 min
Response: 485221
Conc: 28.72 ng/ml

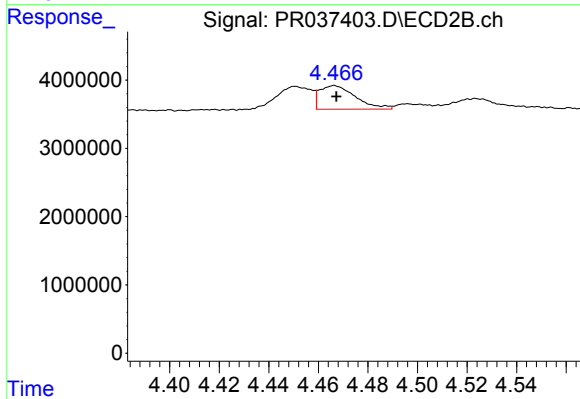

#12 AR-1232-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3525813
Conc: 25.51 ng/ml

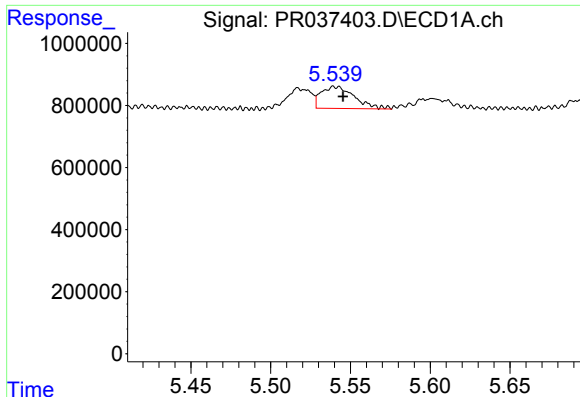

#13 AR-1232-3


R.T.: 5.540 min
Delta R.T.: -0.005 min
Response: 1030479
Conc: 30.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

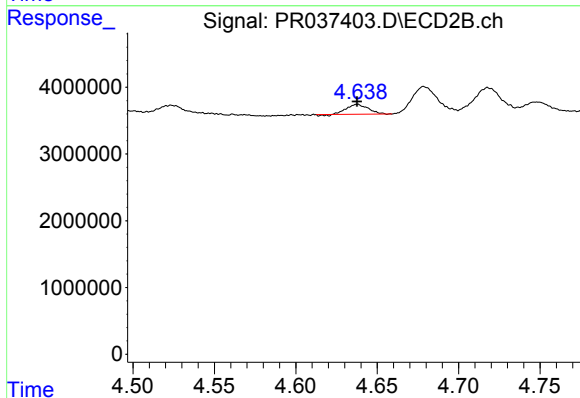


#13 AR-1232-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 1326443
Conc: 18.89 ng/ml

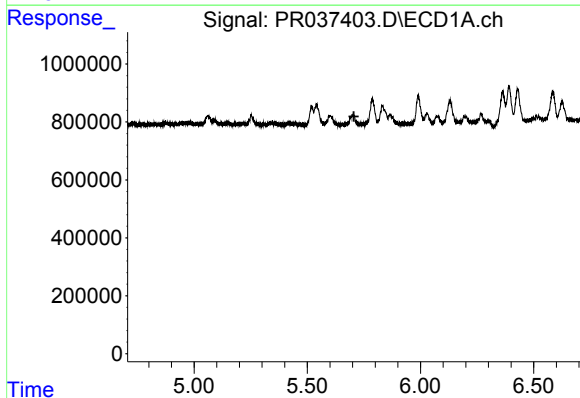


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.706 min
Response: 0
Conc: N.D.

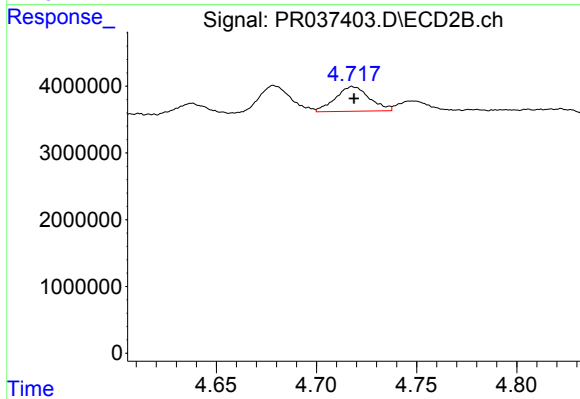

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 4381213
Conc: 73.42 ng/ml

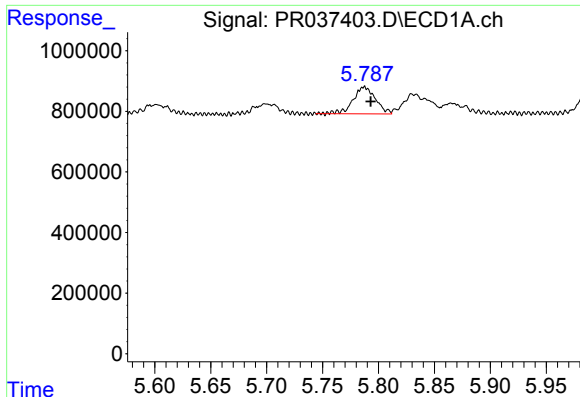

#15 AR-1232-5


R.T.: 5.787 min
Delta R.T.: -0.006 min
Response: 1234901
Conc: 105.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

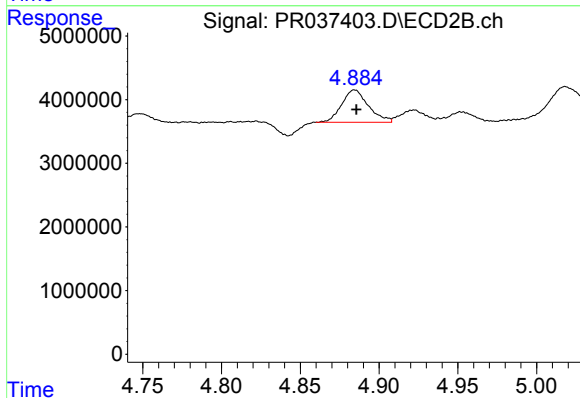


#15 AR-1232-5

R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 6003445
Conc: 87.97 ng/ml

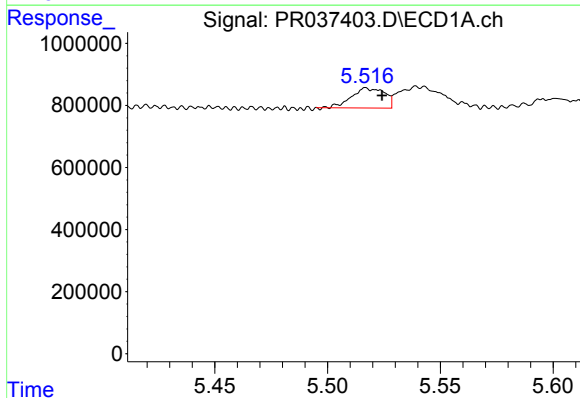


#16 AR-1242-1

R.T.: 5.517 min
Delta R.T.: -0.007 min
Response: 653687
Conc: 19.11 ng/ml

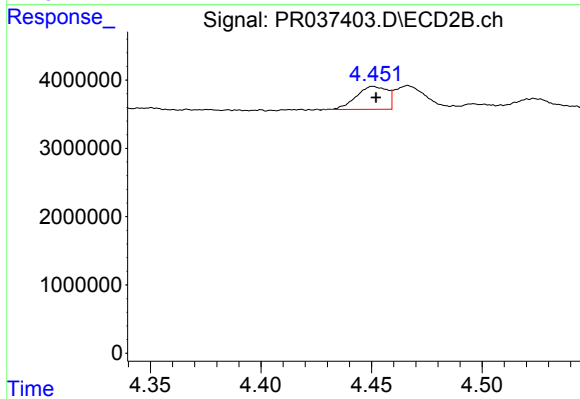

#16 AR-1242-1


R.T.: 4.451 min
Delta R.T.: -0.001 min
Response: 3255498
Conc: 22.22 ng/ml

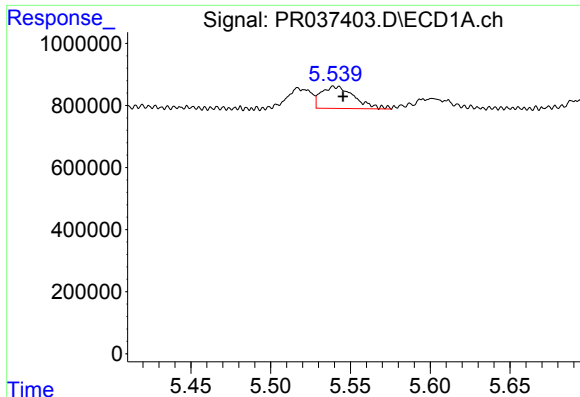

#17 AR-1242-2


R.T.: 5.540 min
Delta R.T.: -0.005 min
Response: 1030479
Conc: 18.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

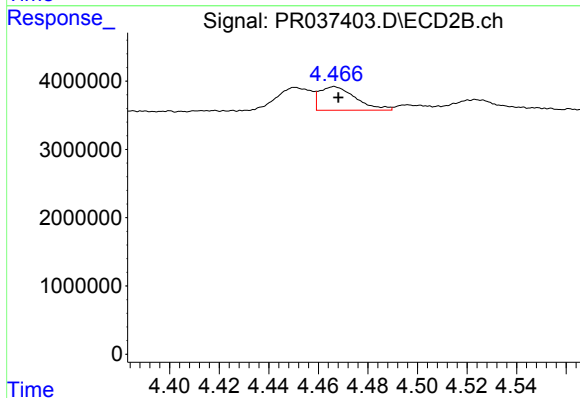


#17 AR-1242-2

R.T.: 4.467 min
Delta R.T.: -0.002 min
Response: 3525813
Conc: 15.45 ng/ml

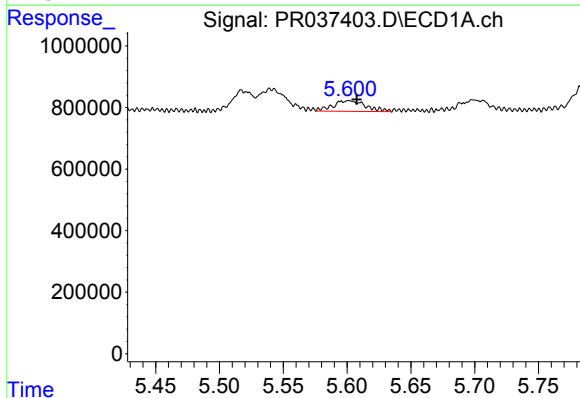


#18 AR-1242-3

R.T.: 5.602 min
Delta R.T.: -0.006 min
Response: 617985
Conc: 18.78 ng/ml

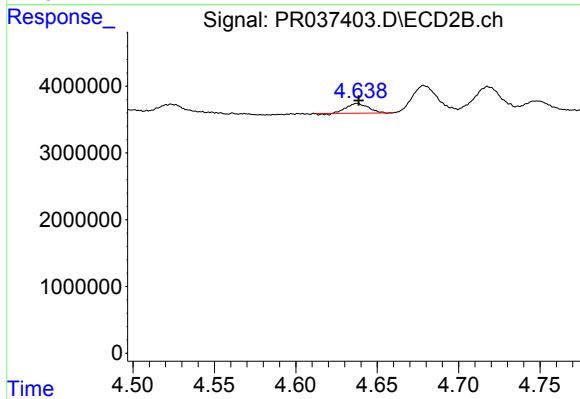

#18 AR-1242-3


R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 1326443
Conc: 11.47 ng/ml

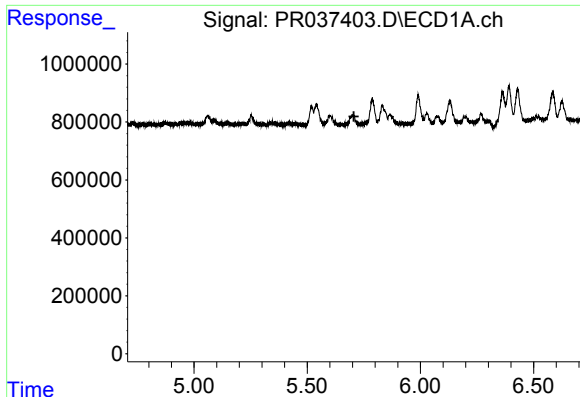

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

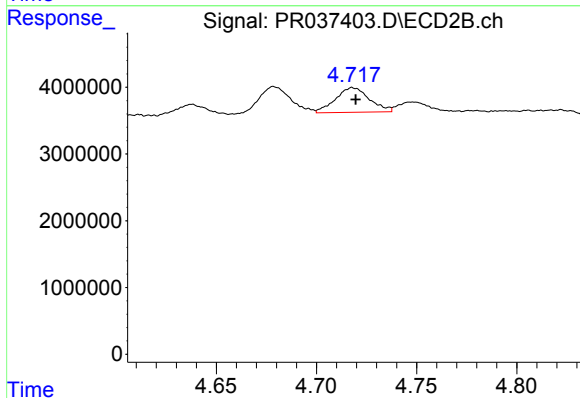


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 4381213
Conc: 39.86 ng/ml

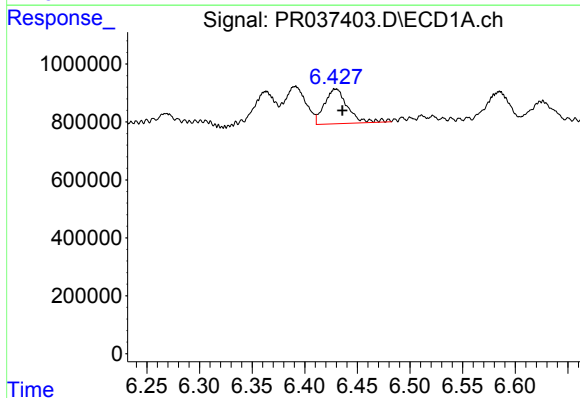


#20 AR-1242-5

R.T.: 6.430 min
Delta R.T.: -0.006 min
Response: 1839050
Conc: 57.15 ng/ml

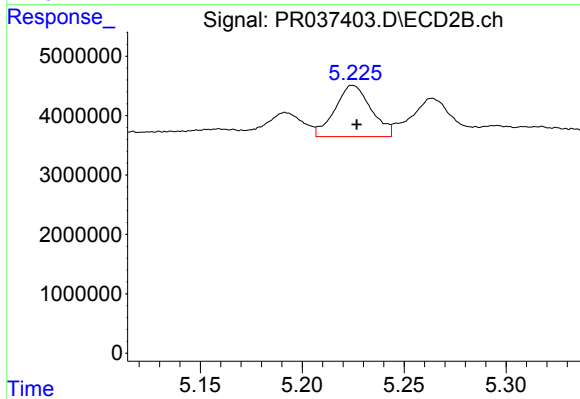

#20 AR-1242-5


R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 10685776
Conc: 64.49 ng/ml

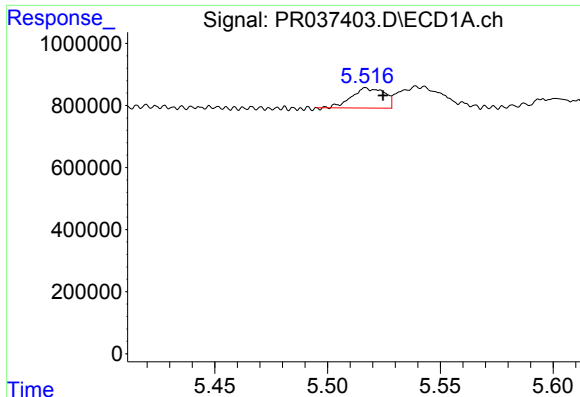

#21 AR-1248-1


R.T.: 5.517 min
Delta R.T.: -0.007 min
Response: 653687
Conc: 28.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

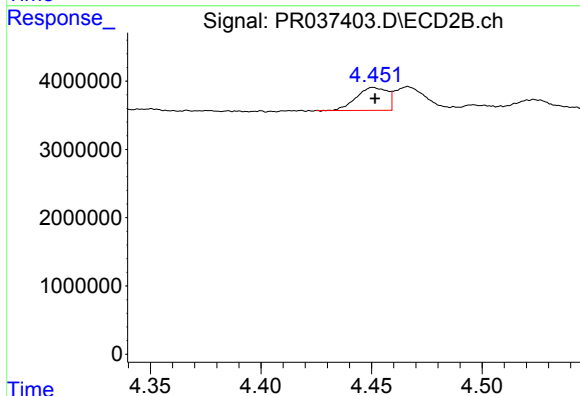


#21 AR-1248-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3255498
Conc: 32.34 ng/ml

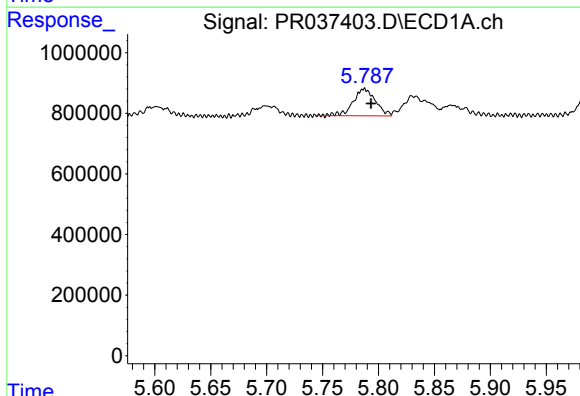


#22 AR-1248-2

R.T.: 5.787 min
Delta R.T.: -0.006 min
Response: 1234901
Conc: 35.27 ng/ml

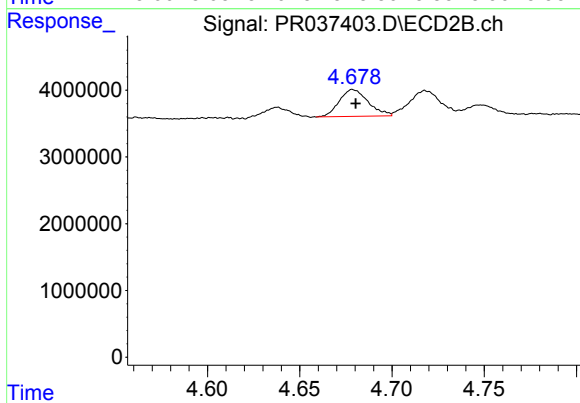

#22 AR-1248-2


R.T.: 4.679 min
Delta R.T.: -0.002 min
Response: 4399465
Conc: 32.24 ng/ml

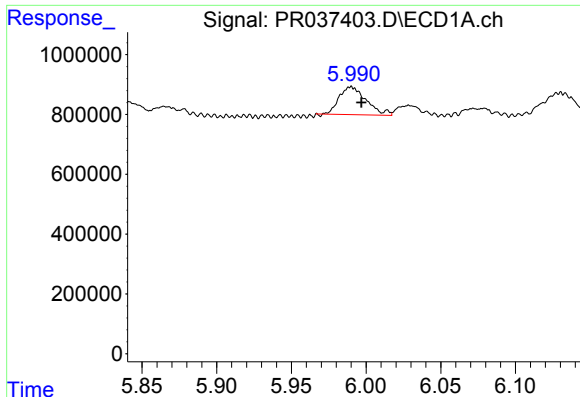

#23 AR-1248-3


R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 1164733
Conc: 28.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

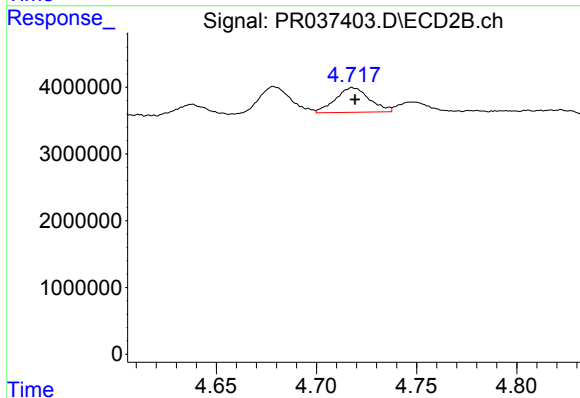


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 4381213
Conc: 31.30 ng/ml

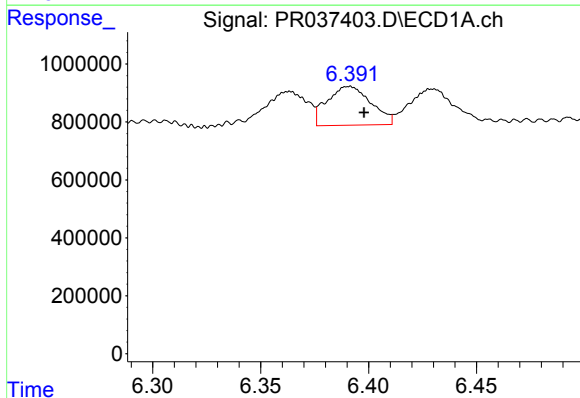


#24 AR-1248-4

R.T.: 6.391 min
Delta R.T.: -0.007 min
Response: 1896922
Conc: 38.75 ng/ml

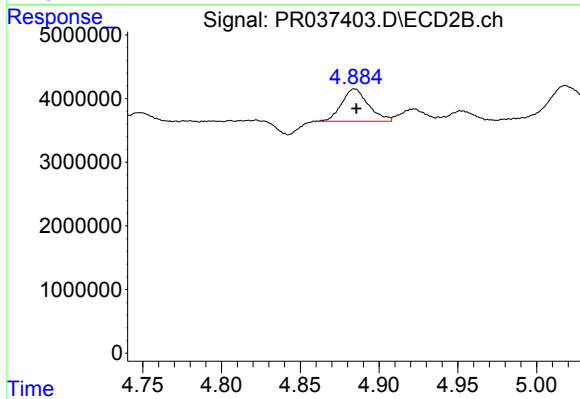

#24 AR-1248-4


R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 6003445
Conc: 33.73 ng/ml

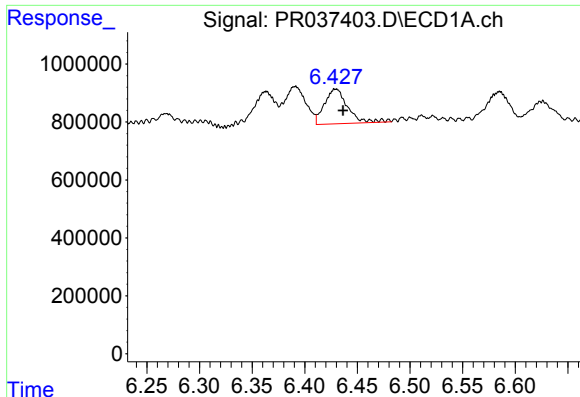

#25 AR-1248-5


R.T.: 6.430 min
Delta R.T.: -0.007 min
Response: 1839050
Conc: 38.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

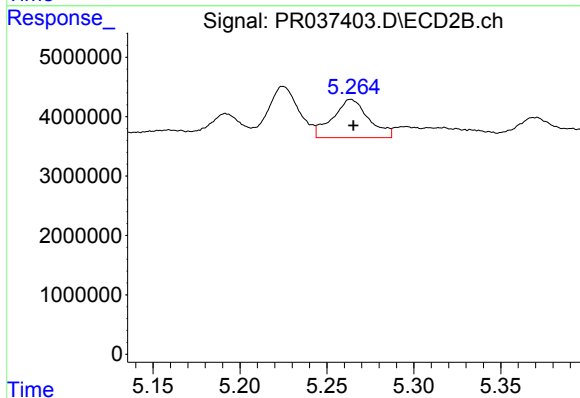


#25 AR-1248-5

R.T.: 5.264 min
Delta R.T.: -0.001 min
Response: 9322764
Conc: 47.66 ng/ml

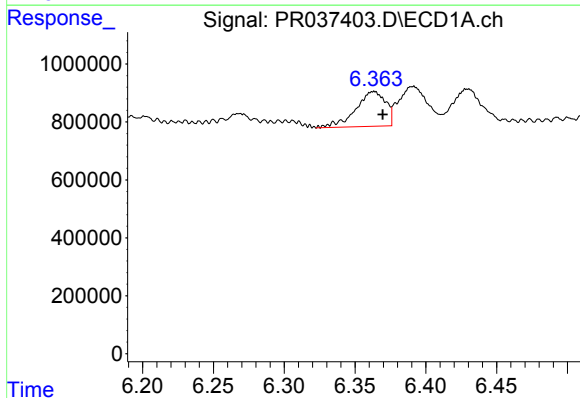


#26 AR-1254-1

R.T.: 6.363 min
Delta R.T.: -0.006 min
Response: 1767788
Conc: 32.36 ng/ml

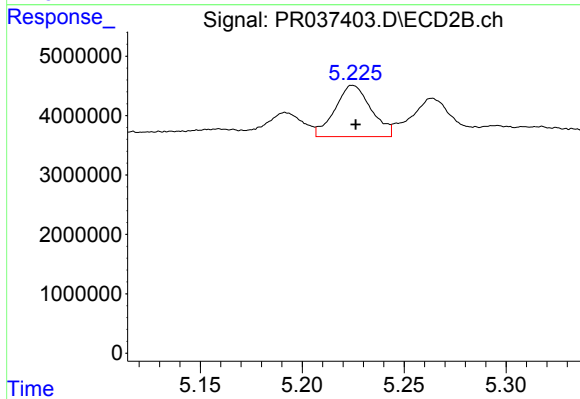

#26 AR-1254-1


R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 10685776
Conc: 31.02 ng/ml

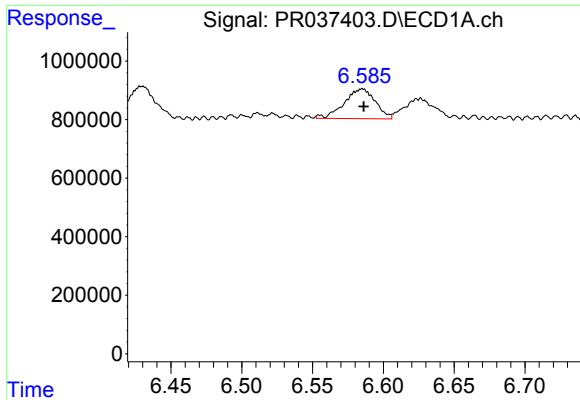

#27 AR-1254-2


R.T.: 6.585 min
Delta R.T.: -0.001 min
Response: 1554027
Conc: 18.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

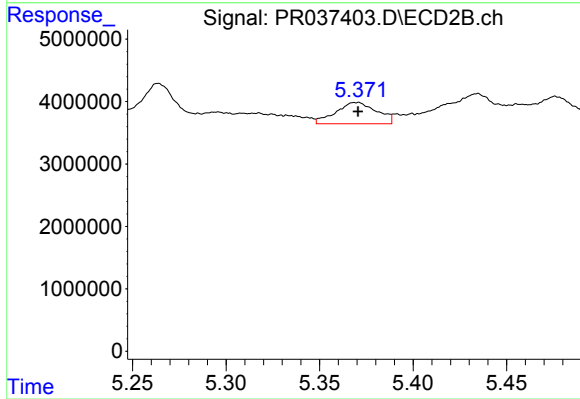


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 5171321
Conc: 17.27 ng/ml

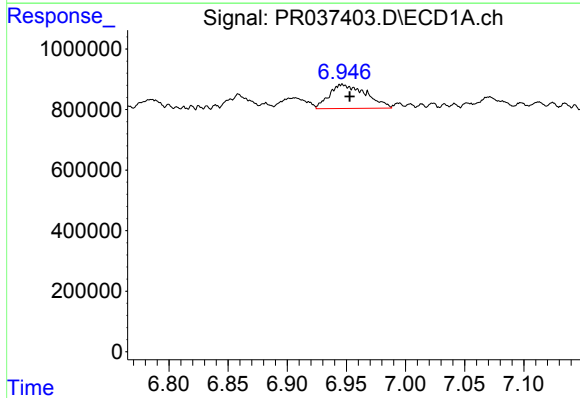


#28 AR-1254-3

R.T.: 6.946 min
Delta R.T.: -0.006 min
Response: 1709608
Conc: 18.79 ng/ml

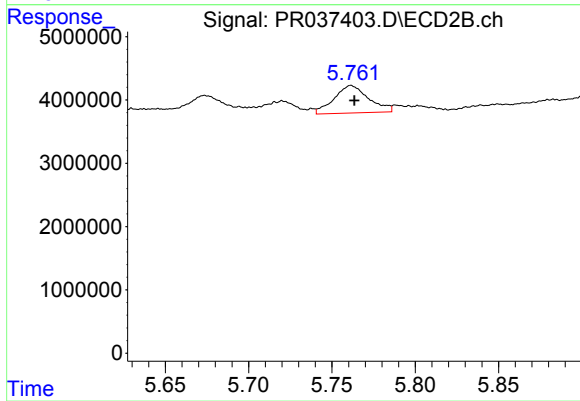

#28 AR-1254-3


R.T.: 5.761 min
Delta R.T.: -0.002 min
Response: 6305188
Conc: 13.31 ng/ml

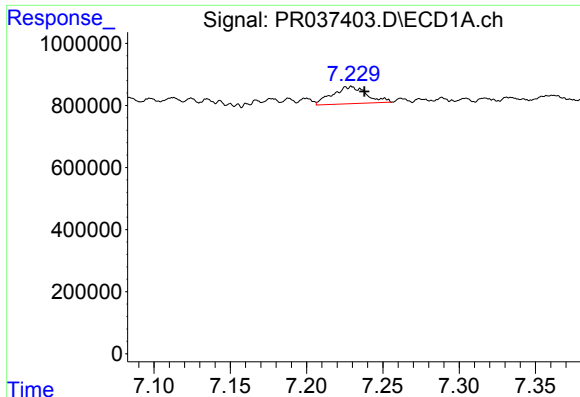

#29 AR-1254-4


R.T.: 7.229 min
Delta R.T.: -0.009 min
Response: 858980
Conc: 12.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

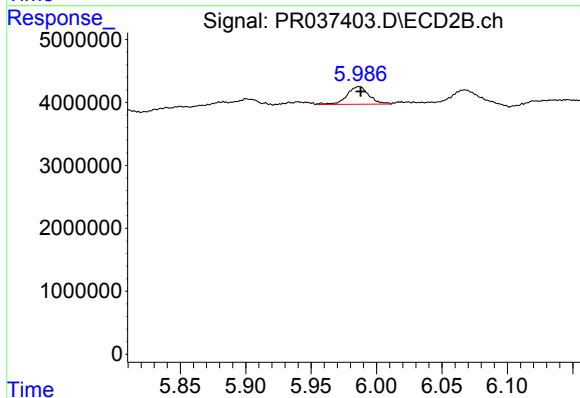


#29 AR-1254-4

R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 3274403
Conc: 9.34 ng/ml

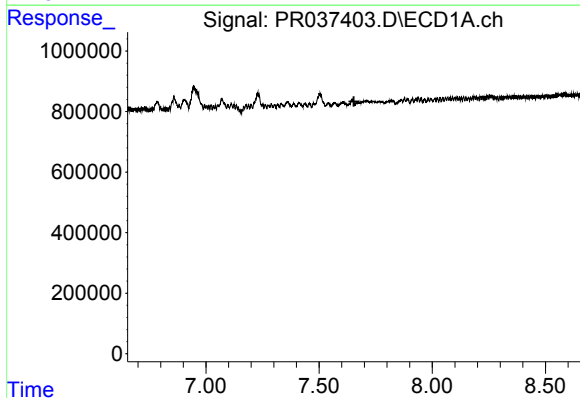


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

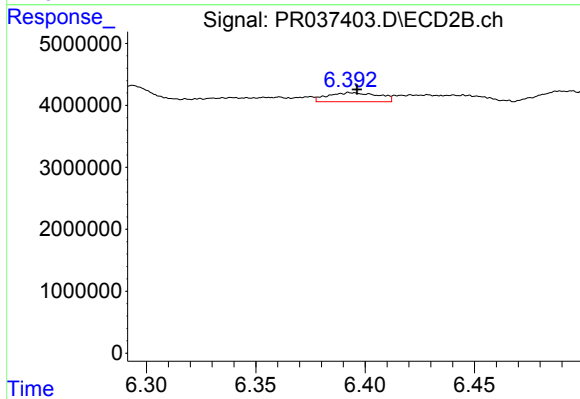

#30 AR-1254-5


R.T.: 6.393 min
Delta R.T.: -0.004 min
Response: 2372701
Conc: 5.36 ng/ml

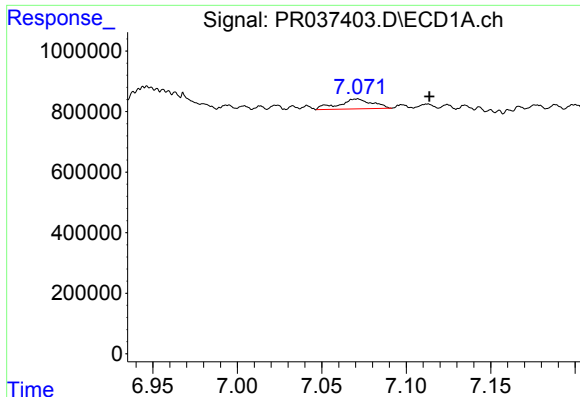

#31 AR-1260-1


R.T.: 7.071 min
Delta R.T.: -0.043 min
Response: 455680
Conc: 6.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

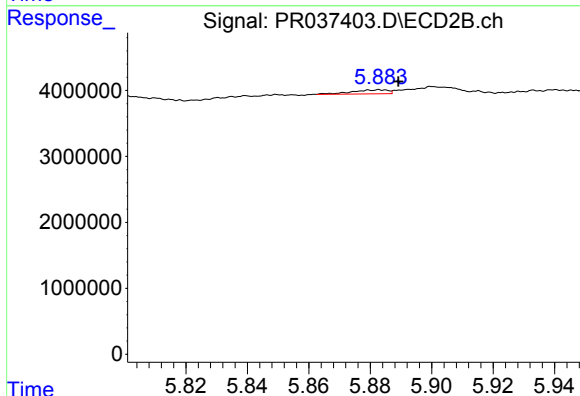


#31 AR-1260-1

R.T.: 5.883 min
Delta R.T.: -0.006 min
Response: 484464
Conc: 1.66 ng/ml

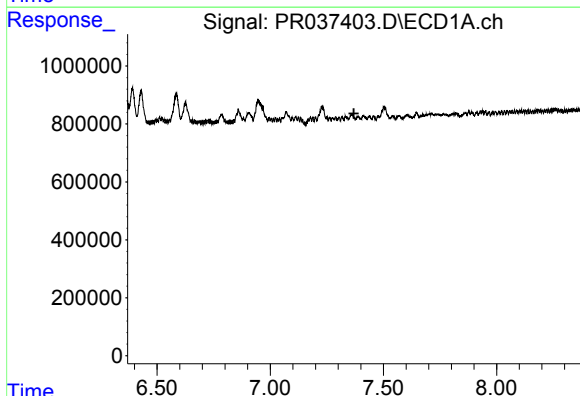


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

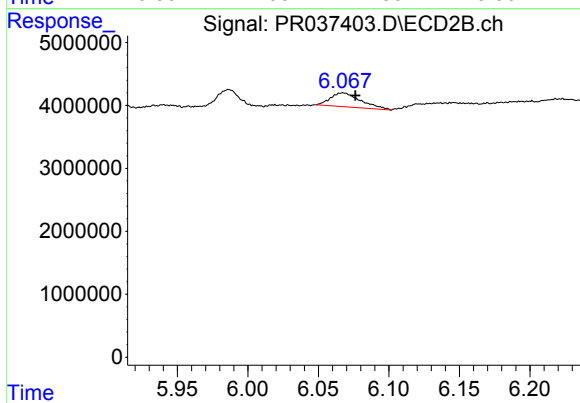

#32 AR-1260-2


R.T.: 6.067 min
Delta R.T.: -0.009 min
Response: 3323802
Conc: 7.22 ng/ml

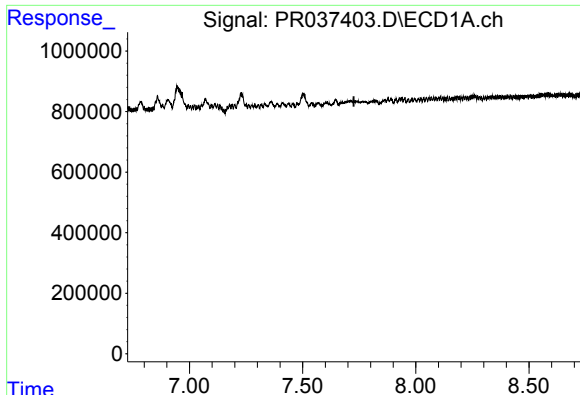

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

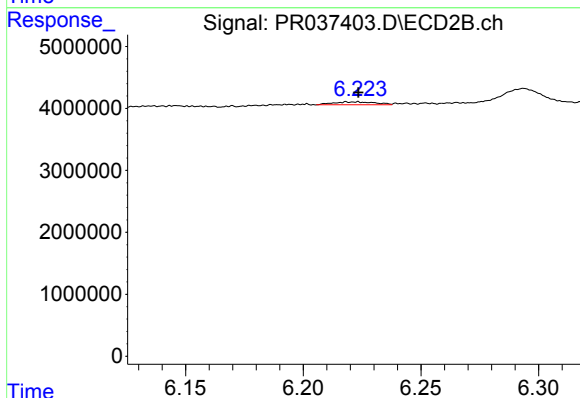


#33 AR-1260-3

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 588088
Conc: 1.65 ng/ml

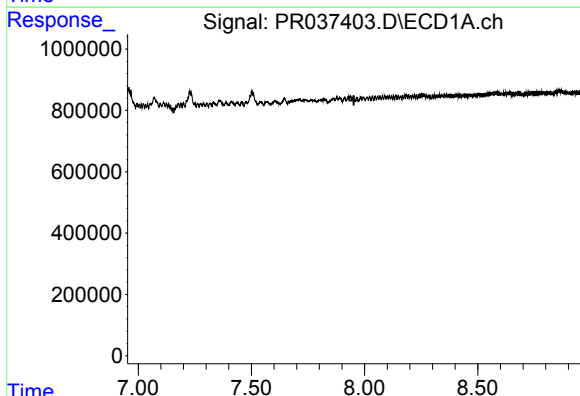


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

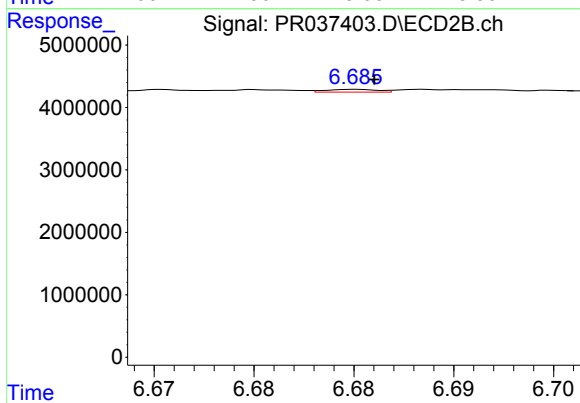

#34 AR-1260-4


R.T.: 6.685 min
Delta R.T.: 0.000 min
Response: 78775
Conc: 0.26 ng/ml

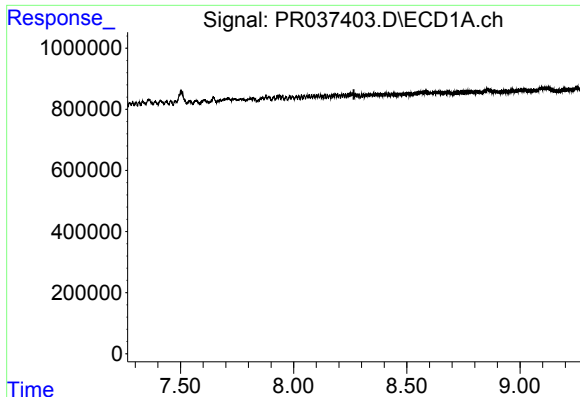

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

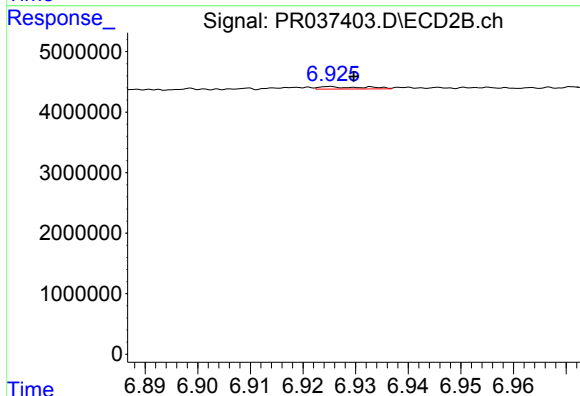


#35 AR-1260-5

R.T.: 6.925 min
Delta R.T.: -0.004 min
Response: 245782
Conc: 0.28 ng/ml

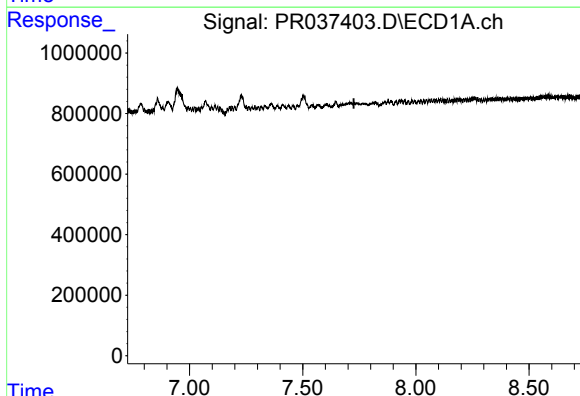


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

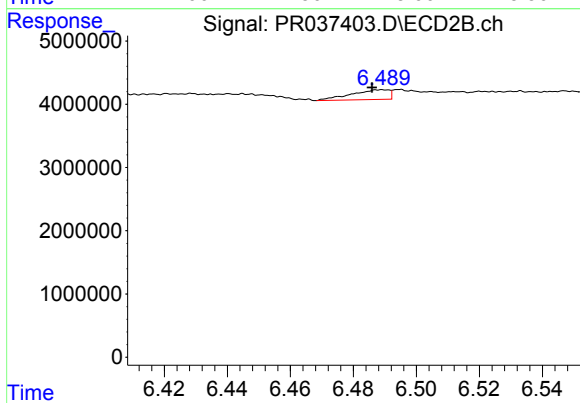

#36 AR-1262-1


R.T.: 6.489 min
Delta R.T.: 0.003 min
Response: 1286666
Conc: 5.13 ng/ml

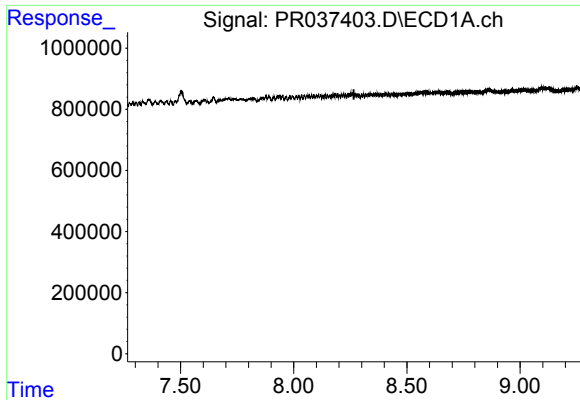

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

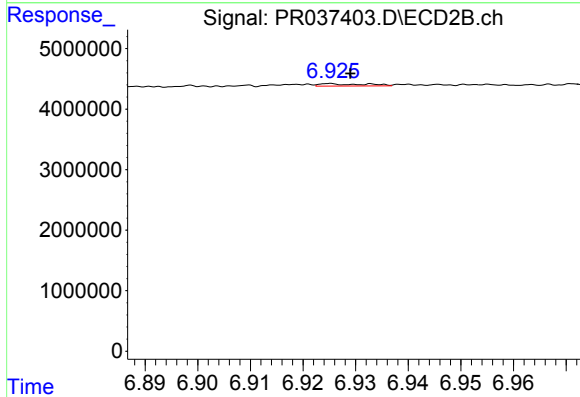


#37 AR-1262-2

R.T.: 6.925 min
Delta R.T.: -0.004 min
Response: 245782
Conc: 0.20 ng/ml

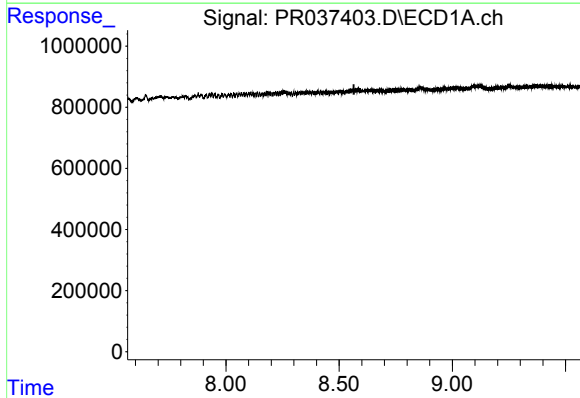


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

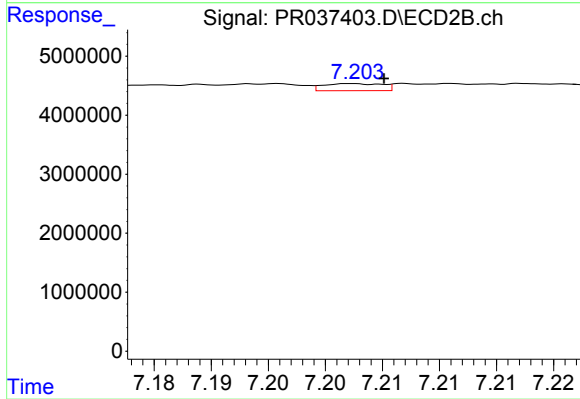

#38 AR-1262-3


R.T.: 7.203 min
Delta R.T.: -0.003 min
Response: 428095
Conc: 0.78 ng/ml

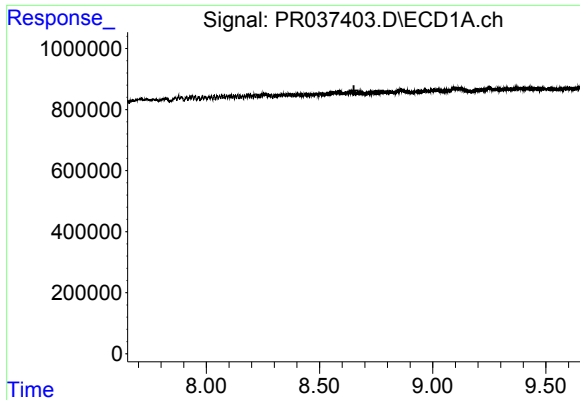

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

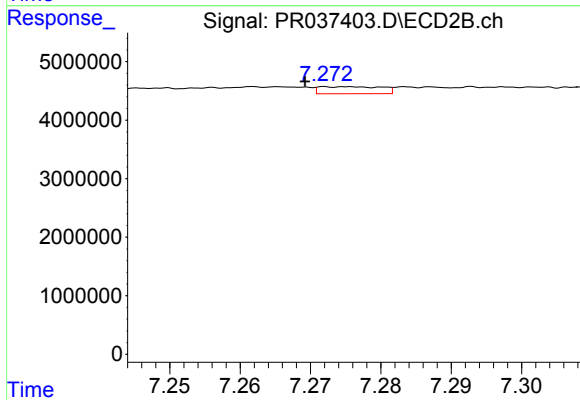


#39 AR-1262-4

R.T.: 7.272 min
Delta R.T.: 0.003 min
Response: 739524
Conc: 0.82 ng/ml

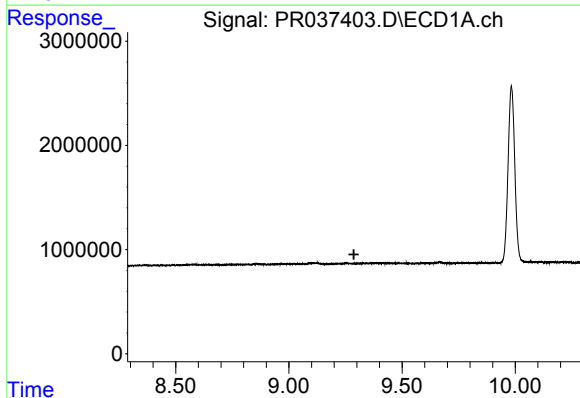


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

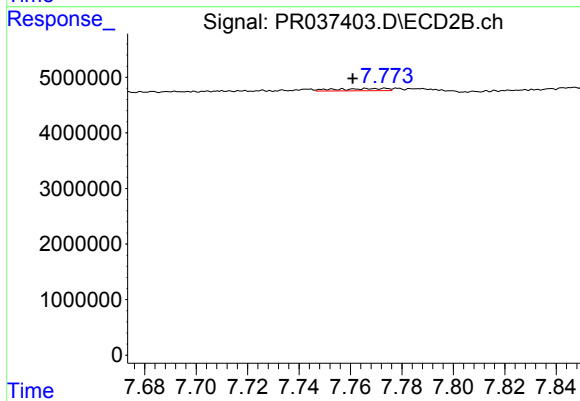

#40 AR-1262-5


R.T.: 7.757 min
Delta R.T.: -0.004 min
Response: 538393
Conc: 1.41 ng/ml

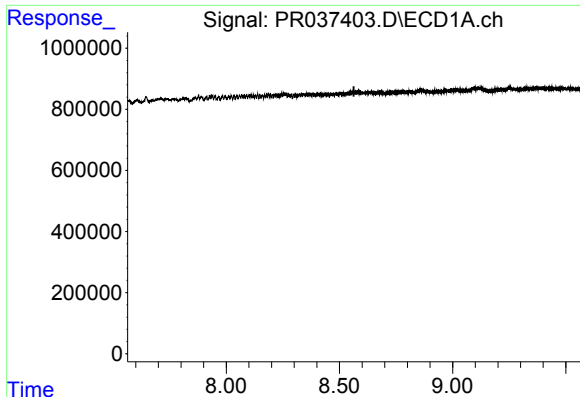

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

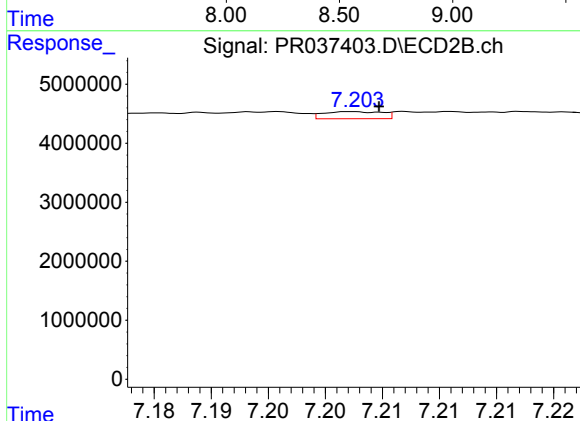


#41 AR-1268-1

R.T.: 7.203 min
Delta R.T.: -0.002 min
Response: 428095
Conc: 0.35 ng/ml

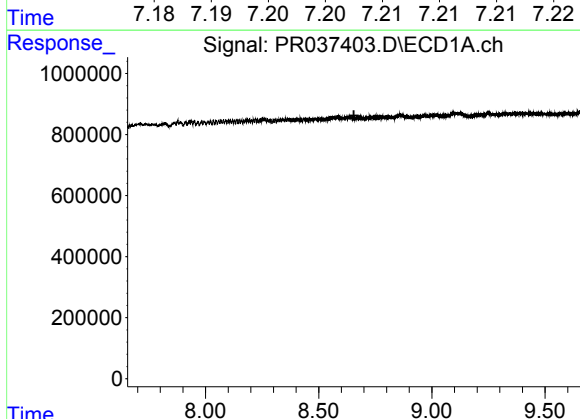


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

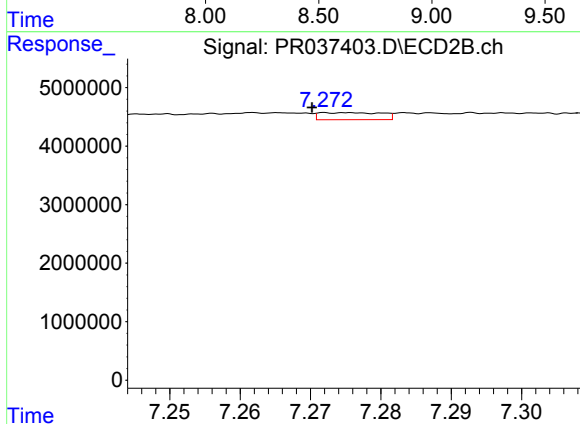

#42 AR-1268-2


R.T.: 7.272 min
Delta R.T.: 0.002 min
Response: 739524
Conc: 0.70 ng/ml

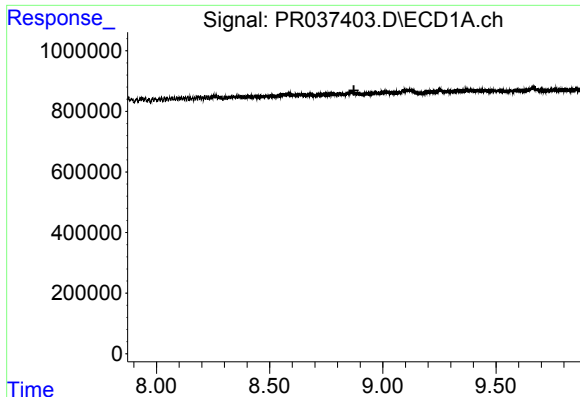

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

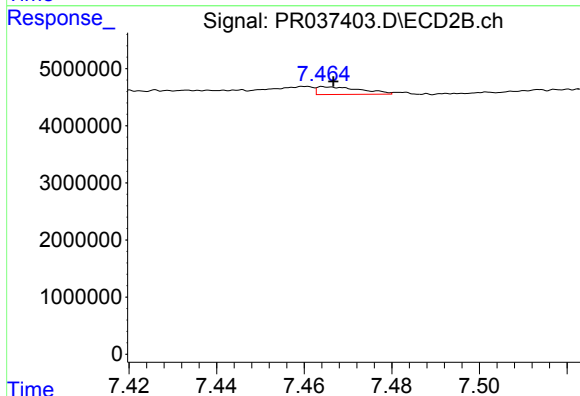


#43 AR-1268-3

R.T.: 7.465 min
Delta R.T.: -0.002 min
Response: 945001
Conc: 1.07 ng/ml

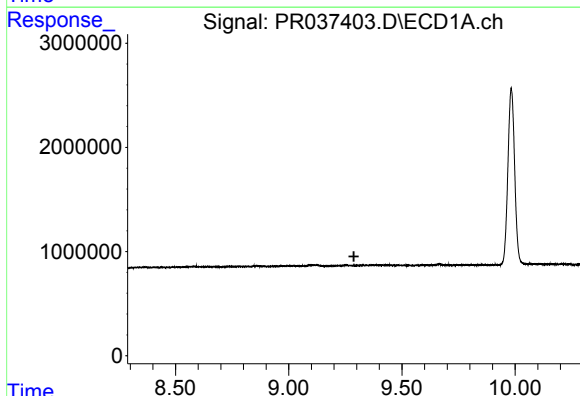


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

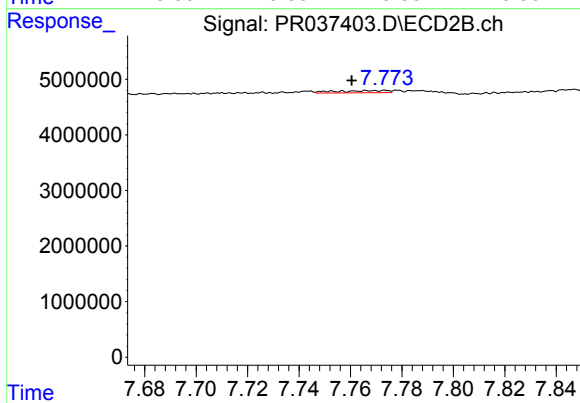

#44 AR-1268-4


R.T.: 7.757 min
Delta R.T.: -0.004 min
Response: 538393
Conc: 1.48 ng/ml

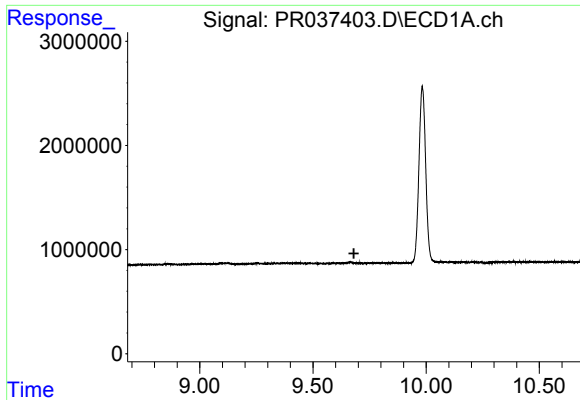

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

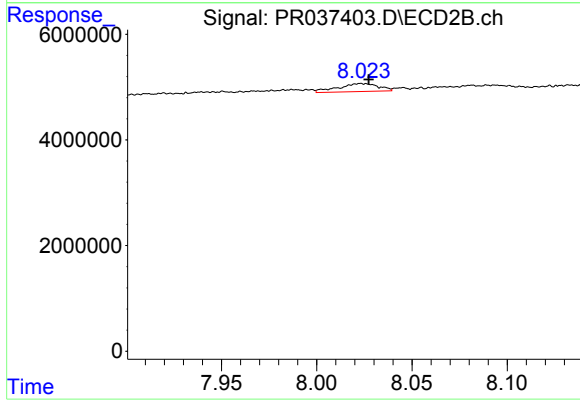

#45 AR-1268-5

R.T.: 8.023 min
Delta R.T.: -0.004 min
Response: 2222926
Conc: 0.87 ng/ml