

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR042519\  
 Data File : PR037404.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Apr 2019 16:36  
 Operator : SM\SJ  
 Sample : K2241-09  
 Misc : AR1254 MDL 25PPB  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 26 00:44:12 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR042219.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Mon Apr 22 17:27:39 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml     |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|-----------|
| -----                       |                 |       |       |          |          |        |           |
| System Monitoring Compounds |                 |       |       |          |          |        |           |
| 1)                          | SA Tetrachlo... | 4.357 | 3.406 | 34208031 | 134.7E6  | 27.345 | 28.093    |
| 2)                          | SA Decachlor... | 9.982 | 8.242 | 28994905 | 145.2E6  | 21.923 | 24.928    |
| Target Compounds            |                 |       |       |          |          |        |           |
| 3)                          | L1 AR-1016-1    | 0.000 | 4.453 | 0        | 645087   | N.D.   | 3.543 #   |
| 4)                          | L1 AR-1016-2    | 0.000 | 4.453 | 0        | 645087   | N.D.   | 2.287 #   |
| 5)                          | L1 AR-1016-3    | 0.000 | 4.677 | 0        | 4270318  | N.D.   | 29.700 #  |
| 6)                          | L1 AR-1016-4    | 0.000 | 4.677 | 0        | 4270318  | N.D.   | 38.598 #  |
| 7)                          | L1 AR-1016-5    | 5.990 | 4.883 | 568874   | 2910719  | 16.590 | 19.148    |
| 8)                          | L2 AR-1221-1    | 0.000 | 3.598 | 0        | 262401   | N.D.   | 5.153 #   |
| 9)                          | L2 AR-1221-2    | 4.660 | 3.696 | 835606   | 1844201  | 92.394 | 49.661 #  |
| 10)                         | L2 AR-1221-3    | 0.000 | 3.753 | 0        | 193510   | N.D.   | 1.580 #   |
| 11)                         | L3 AR-1232-1    | 0.000 | 3.753 | 0        | 193510   | N.D.   | 1.654 #   |
| 12)                         | L3 AR-1232-2    | 0.000 | 4.453 | 0        | 645087   | N.D.   | 4.667 #   |
| 13)                         | L3 AR-1232-3    | 0.000 | 4.677 | 0        | 4270318  | N.D.   | 60.829 #  |
| 14)                         | L3 AR-1232-4    | 0.000 | 4.715 | 0        | 1394208  | N.D.   | 23.365 #  |
| 15)                         | L3 AR-1232-5    | 5.786 | 4.883 | 1043278  | 2910719  | 89.202 | 42.652 #  |
| 16)                         | L4 AR-1242-1    | 0.000 | 4.453 | 0        | 645087   | N.D.   | 4.402 #   |
| 17)                         | L4 AR-1242-2    | 0.000 | 4.453 | 0        | 645087   | N.D.   | 2.827 #   |
| 18)                         | L4 AR-1242-3    | 0.000 | 4.677 | 0        | 4270318  | N.D.   | 36.931 #  |
| 19)                         | L4 AR-1242-4    | 0.000 | 4.715 | 0        | 1394208  | N.D.   | 12.685 #  |
| 20)                         | L4 AR-1242-5    | 6.430 | 5.224 | 892311   | 20227917 | 27.730 | 122.076 # |
| 21)                         | L5 AR-1248-1    | 0.000 | 4.453 | 0        | 645087   | N.D.   | 6.408 #   |
| 22)                         | L5 AR-1248-2    | 5.786 | 4.677 | 1043278  | 4270318  | 29.796 | 31.290    |
| 23)                         | L5 AR-1248-3    | 5.990 | 4.715 | 568874   | 1394208  | 13.906 | 9.961 #   |
| 24)                         | L5 AR-1248-4    | 6.388 | 4.883 | 1268935  | 2910719  | 25.921 | 16.356 #  |
| 25)                         | L5 AR-1248-5    | 6.430 | 5.295 | 892311   | 3683083  | 18.890 | 18.828    |
| 26)                         | L6 AR-1254-1    | 6.362 | 5.224 | 2888700  | 20227917 | 52.877 | 58.721    |
| 27)                         | L6 AR-1254-2    | 6.578 | 5.368 | 2834429  | 14966491 | 33.075 | 49.971 #  |
| 28)                         | L6 AR-1254-3    | 6.944 | 5.760 | 3708436  | 15778295 | 40.768 | 33.314    |
| 29)                         | L6 AR-1254-4    | 7.228 | 5.985 | 2942624  | 9770668  | 43.914 | 27.865 #  |
| 30)                         | L6 AR-1254-5    | 7.644 | 6.393 | 2501854  | 19891964 | 34.806 | 44.921 #  |
| 31)                         | L7 AR-1260-1    | 7.104 | 5.887 | 1925019  | 5741901  | 29.173 | 19.645 #  |
| 32)                         | L7 AR-1260-2    | 7.359 | 6.071 | 1805041  | 9060732  | 22.647 | 19.672    |
| 33)                         | L7 AR-1260-3    | 0.000 | 6.220 | 0        | 5865297  | N.D.   | 16.453 #  |
| 34)                         | L7 AR-1260-4    | 7.934 | 6.686 | 1075762  | 1085097  | 14.458 | 3.560 #   |
| 35)                         | L7 AR-1260-5    | 8.254 | 6.925 | 634289   | 1238428  | 4.386  | 1.428 #   |
| 36)                         | L8 AR-1262-1    | 0.000 | 6.490 | 0        | 2699588  | N.D.   | 10.772 #  |
| 37)                         | L8 AR-1262-2    | 8.254 | 6.925 | 634289   | 1238428  | 3.263  | 0.986 #   |
| 38)                         | L8 AR-1262-3    | 8.574 | 7.151 | 1276234  | 169195   | 9.704  | 0.309 #   |
| 39)                         | L8 AR-1262-4    | 0.000 | 7.264 | 0        | 12350701 | N.D.   | 13.759 #  |
| 40)                         | L8 AR-1262-5    | 0.000 | 7.770 | 0        | 526624   | N.D.   | 1.376 #   |
| 41)                         | L9 AR-1268-1    | 8.574 | 7.151 | 1276234  | 169195   | 7.126  | 0.137 #   |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR042519\  
 Data File : PR037404.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Apr 2019 16:36  
 Operator : SM\SJ  
 Sample : K2241-09  
 Misc : AR1254 MDL 25PPB  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 26 00:44:12 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR042219.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Mon Apr 22 17:27:39 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|        | Compound  | RT#1  | RT#2  | Resp#1 | Resp#2   | ng/ml | ng/ml    |
|--------|-----------|-------|-------|--------|----------|-------|----------|
| 42) L9 | AR-1268-2 | 0.000 | 7.264 | 0      | 12350701 | N.D.  | 11.663 # |
| 43) L9 | AR-1268-3 | 0.000 | 7.466 | 0      | 16229572 | N.D.  | 18.313 # |
| 44) L9 | AR-1268-4 | 0.000 | 7.770 | 0      | 526624   | N.D.  | 1.452 #  |
| 45) L9 | AR-1268-5 | 0.000 | 8.025 | 0      | 1874543  | N.D.  | 0.737 #  |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR042519\  
Data File : PR037404.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Apr 2019 16:36  
Operator : SM\SJ  
Sample : K2241-09  
Misc : AR1254 MDL 25PPB  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 26 00:44:12 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR042219.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Mon Apr 22 17:27:39 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

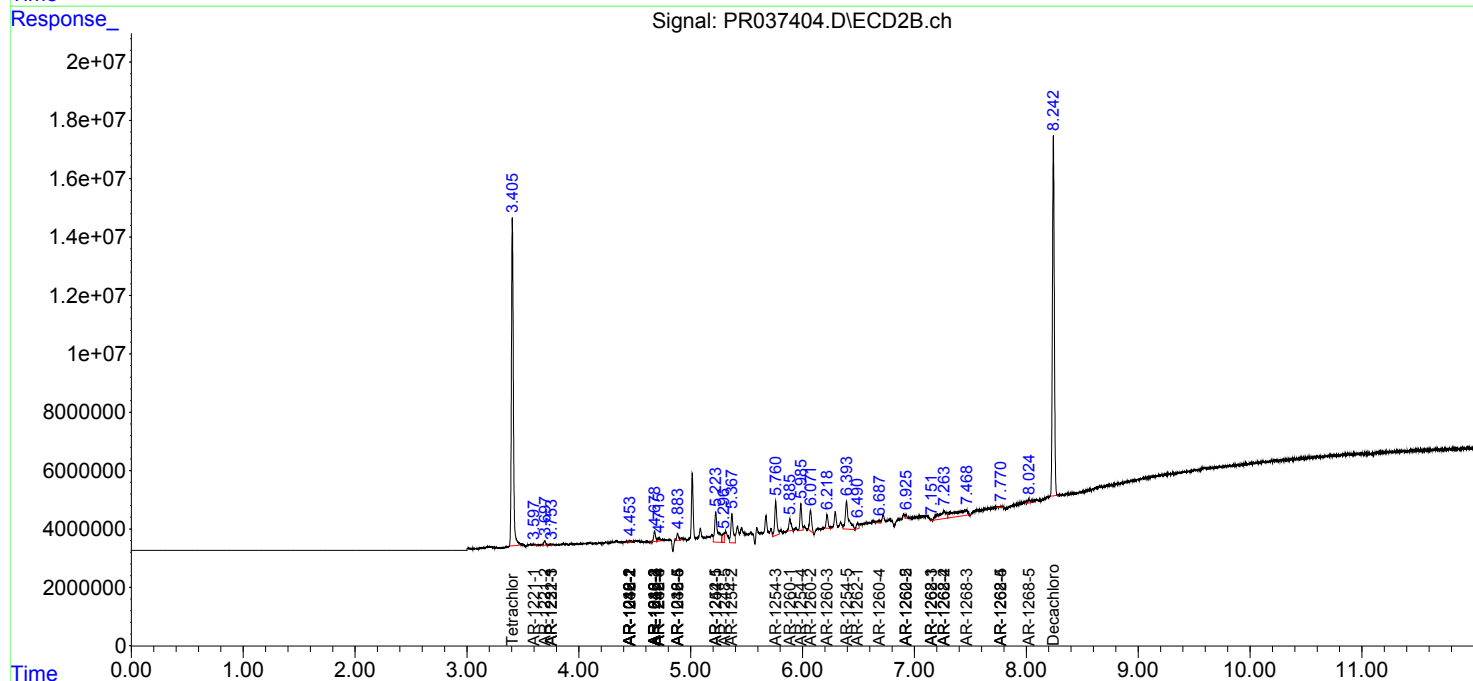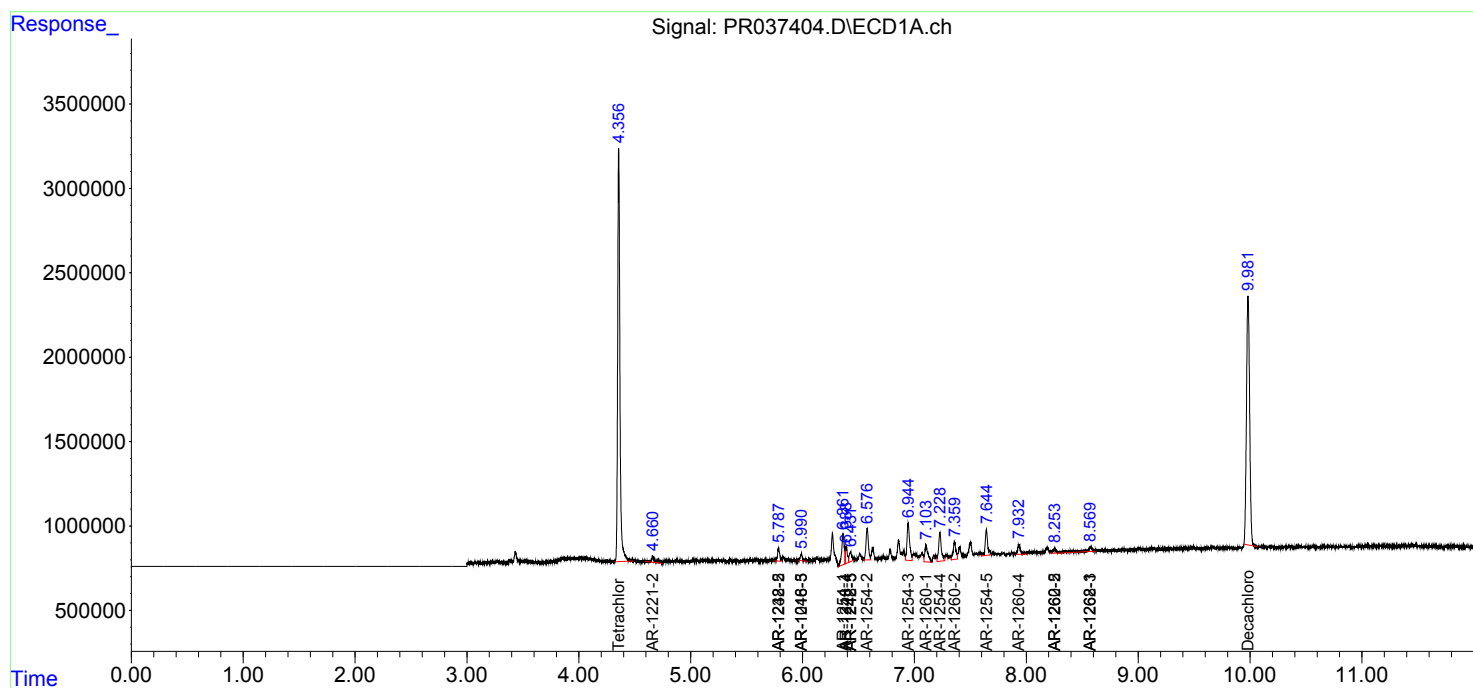


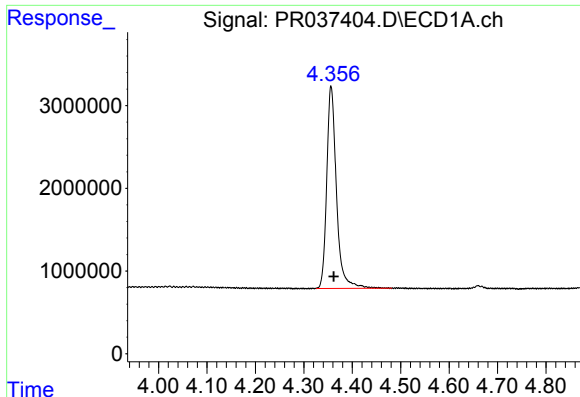

#1 Tetrachloro-m-xylene


R.T.: 4.357 min  
Delta R.T.: -0.005 min  
Response: 34208031  
Conc: 27.34 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

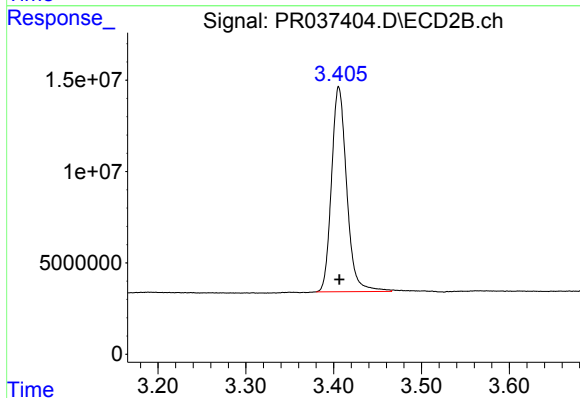


#1 Tetrachloro-m-xylene

R.T.: 3.406 min  
Delta R.T.: 0.000 min  
Response: 134720108  
Conc: 28.09 ng/ml

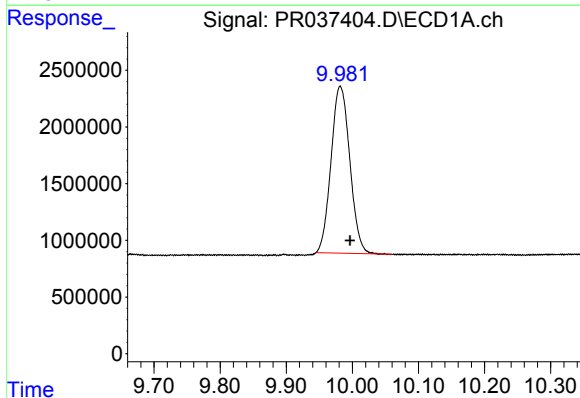


#2 Decachlorobiphenyl

R.T.: 9.982 min  
Delta R.T.: -0.015 min  
Response: 28994905  
Conc: 21.92 ng/ml

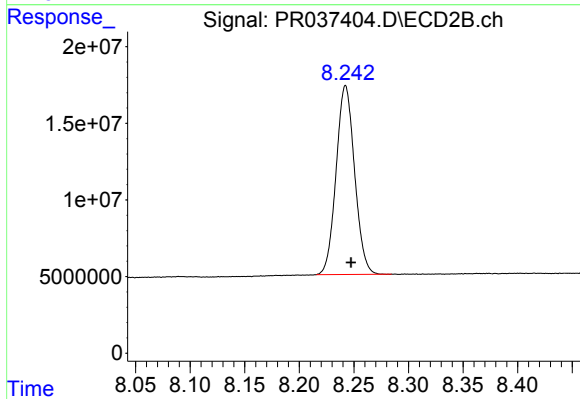

#2 Decachlorobiphenyl


R.T.: 8.242 min  
Delta R.T.: -0.005 min  
Response: 145184451  
Conc: 24.93 ng/ml

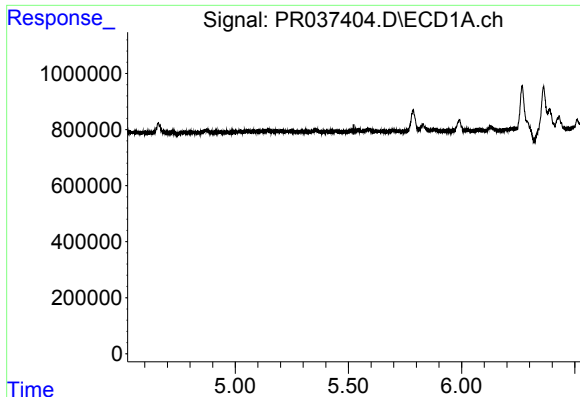

#3 AR-1016-1


R.T.: 0.000 min  
Exp R.T.: 5.524 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

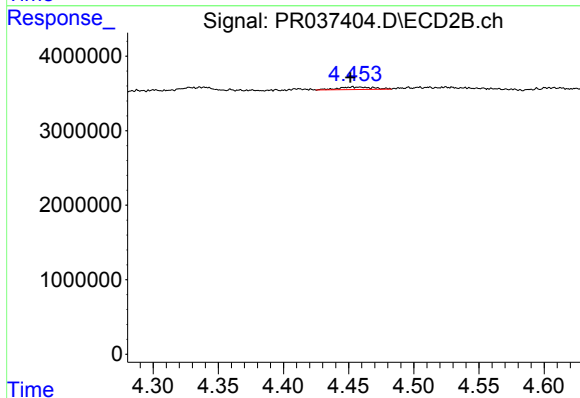


#3 AR-1016-1

R.T.: 4.453 min  
Delta R.T.: 0.002 min  
Response: 645087  
Conc: 3.54 ng/ml

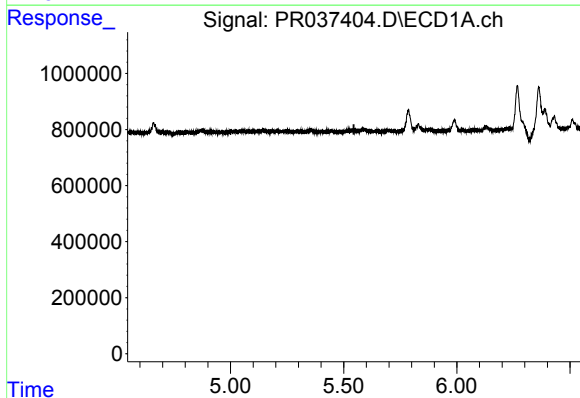


#4 AR-1016-2

R.T.: 0.000 min  
Exp R.T.: 5.545 min  
Response: 0  
Conc: N.D.

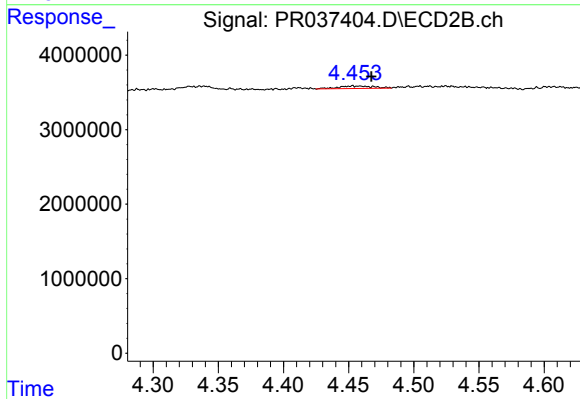

#4 AR-1016-2


R.T.: 4.453 min  
Delta R.T.: -0.014 min  
Response: 645087  
Conc: 2.29 ng/ml

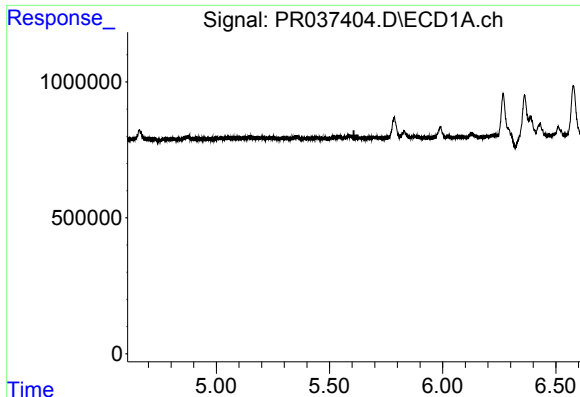

#5 AR-1016-3


R.T.: 0.000 min  
Exp R.T.: 5.608 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

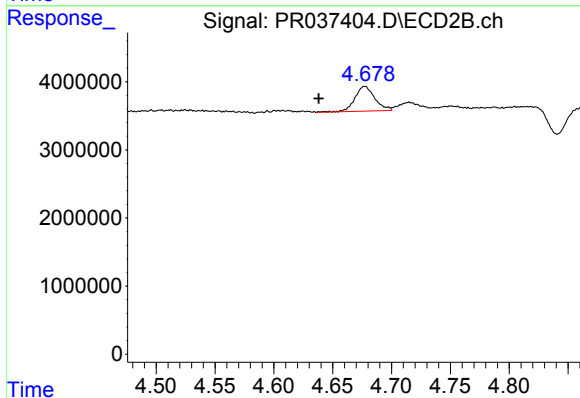


#5 AR-1016-3

R.T.: 4.677 min  
Delta R.T.: 0.039 min  
Response: 4270318  
Conc: 29.70 ng/ml

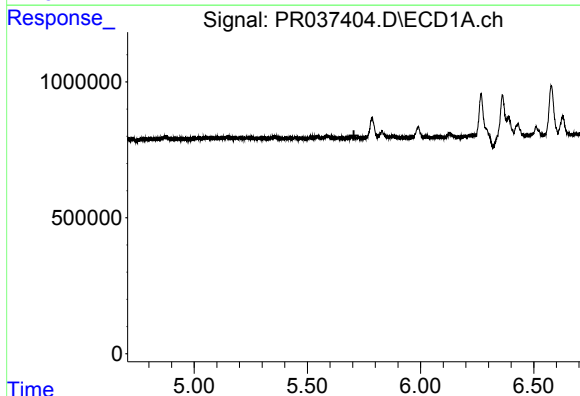


#6 AR-1016-4

R.T.: 0.000 min  
Exp R.T.: 5.705 min  
Response: 0  
Conc: N.D.

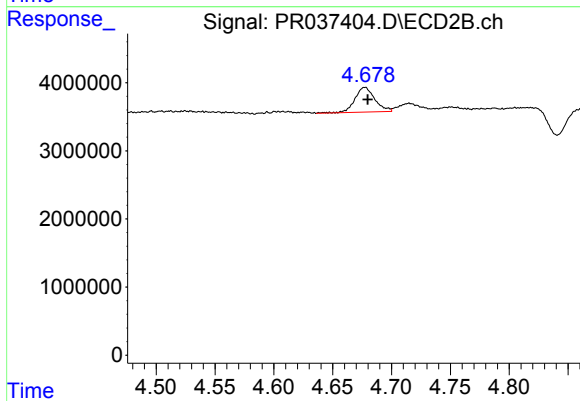

#6 AR-1016-4


R.T.: 4.677 min  
Delta R.T.: -0.003 min  
Response: 4270318  
Conc: 38.60 ng/ml

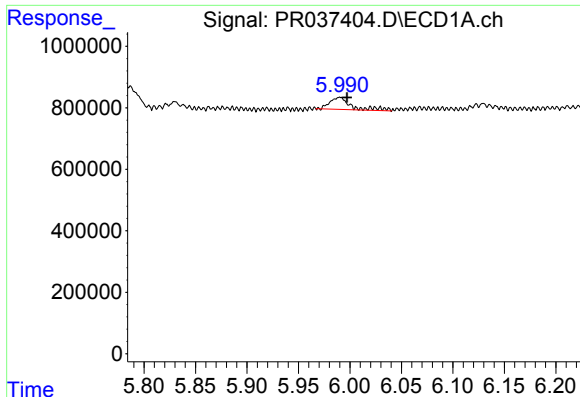

#7 AR-1016-5


R.T.: 5.990 min  
Delta R.T.: -0.008 min  
Response: 568874  
Conc: 16.59 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

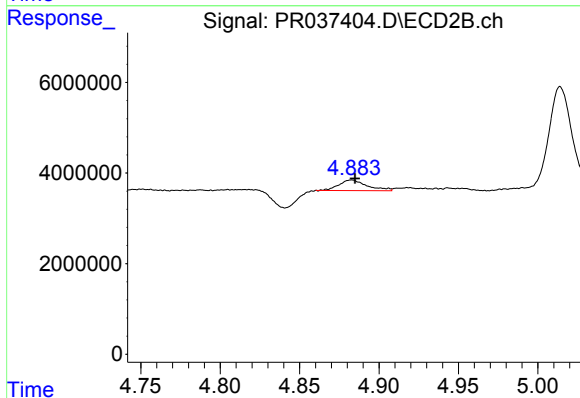


#7 AR-1016-5

R.T.: 4.883 min  
Delta R.T.: -0.002 min  
Response: 2910719  
Conc: 19.15 ng/ml

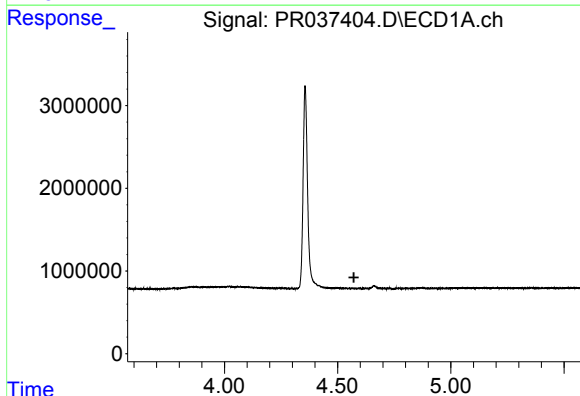


#8 AR-1221-1

R.T.: 0.000 min  
Exp R.T. : 4.572 min  
Response: 0  
Conc: N.D.

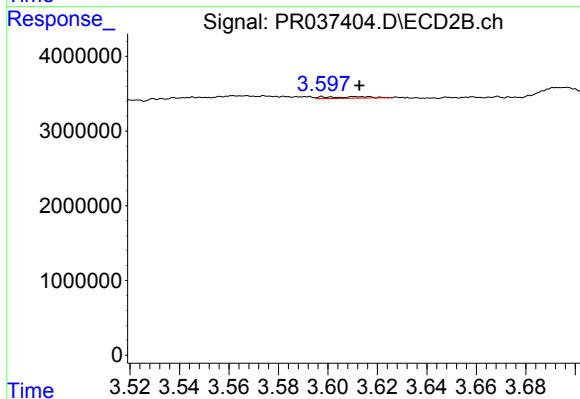

#8 AR-1221-1


R.T.: 3.598 min  
Delta R.T.: -0.015 min  
Response: 262401  
Conc: 5.15 ng/ml

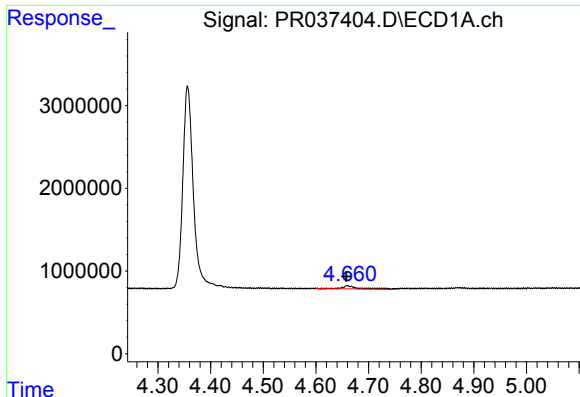

#9 AR-1221-2


R.T.: 4.660 min  
Delta R.T.: 0.002 min  
Response: 835606  
Conc: 92.39 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

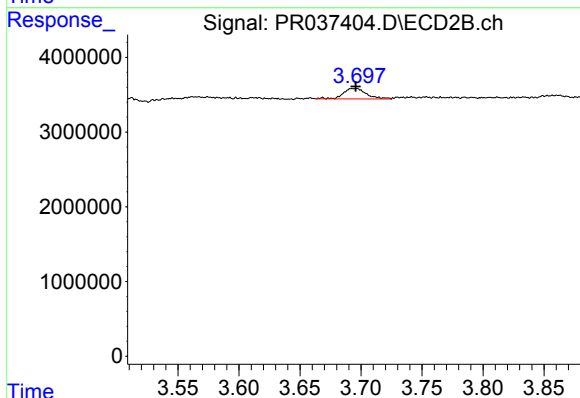


#9 AR-1221-2

R.T.: 3.696 min  
Delta R.T.: 0.000 min  
Response: 1844201  
Conc: 49.66 ng/ml

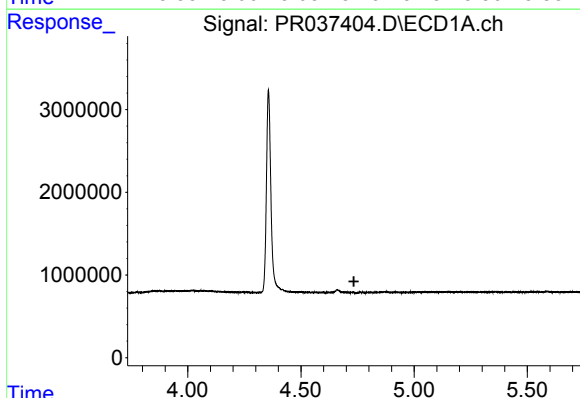

#10 AR-1221-3


R.T.: 0.000 min  
Exp R.T. : 4.734 min  
Response: 0  
Conc: N.D.

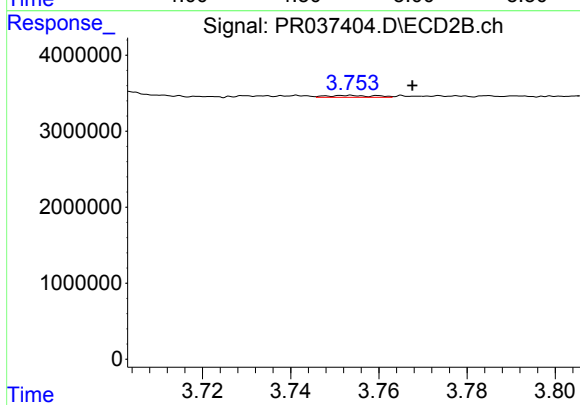

#10 AR-1221-3

R.T.: 3.753 min  
Delta R.T.: -0.014 min  
Response: 193510  
Conc: 1.58 ng/ml




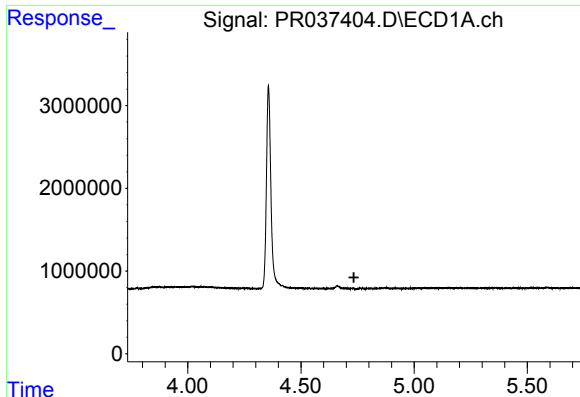

#11 AR-1232-1


R.T.: 0.000 min  
Exp R.T.: 4.734 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

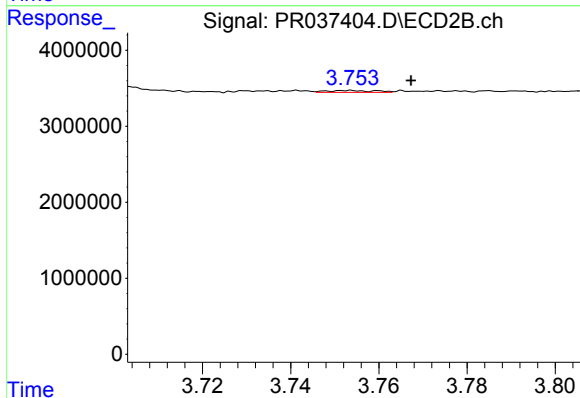


#11 AR-1232-1

R.T.: 3.753 min  
Delta R.T.: -0.014 min  
Response: 193510  
Conc: 1.65 ng/ml

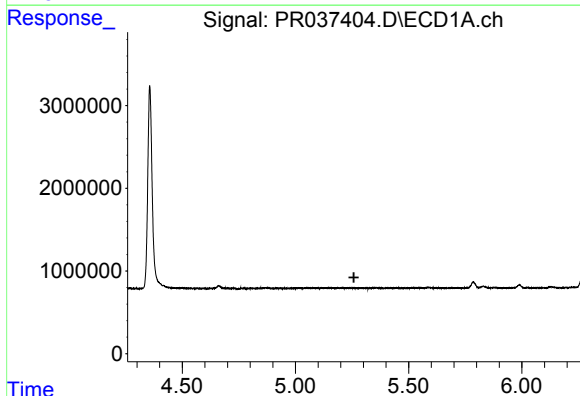


#12 AR-1232-2

R.T.: 0.000 min  
Exp R.T.: 5.258 min  
Response: 0  
Conc: N.D.

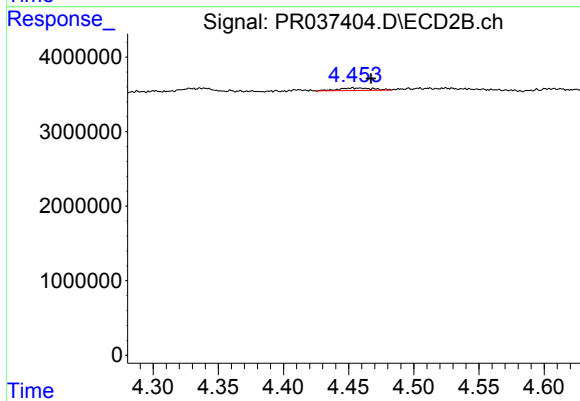

#12 AR-1232-2


R.T.: 4.453 min  
Delta R.T.: -0.014 min  
Response: 645087  
Conc: 4.67 ng/ml

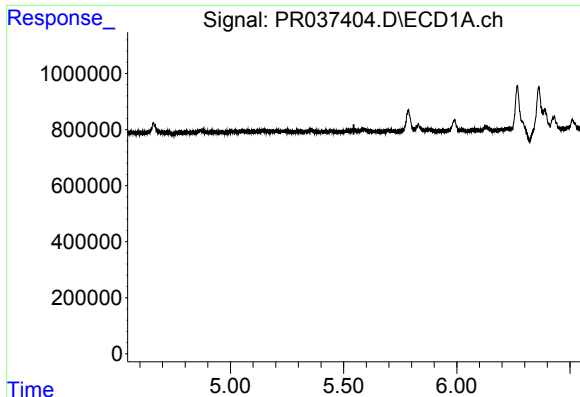

#13 AR-1232-3


R.T.: 0.000 min  
Exp R.T.: 5.545 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

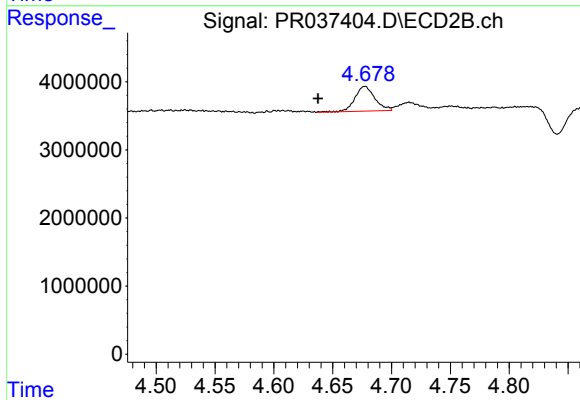


#13 AR-1232-3

R.T.: 4.677 min  
Delta R.T.: 0.040 min  
Response: 4270318  
Conc: 60.83 ng/ml

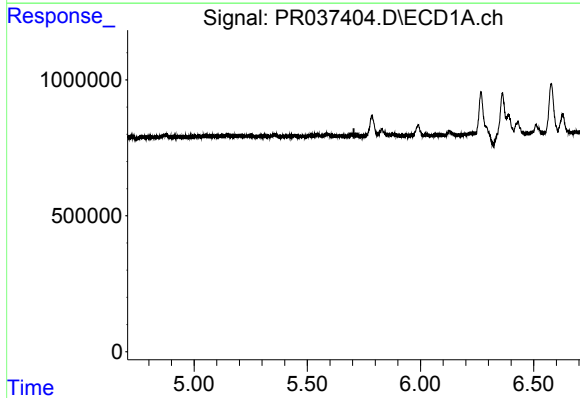


#14 AR-1232-4

R.T.: 0.000 min  
Exp R.T.: 5.706 min  
Response: 0  
Conc: N.D.

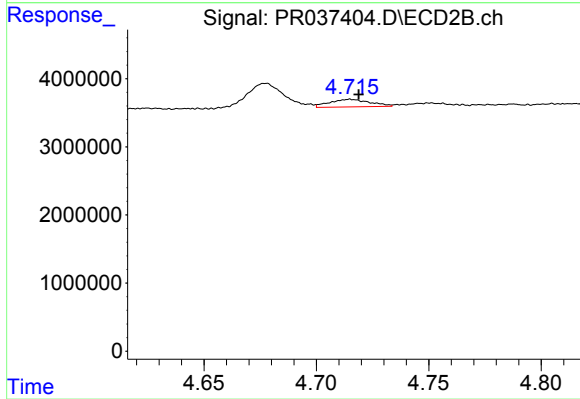

#14 AR-1232-4


R.T.: 4.715 min  
Delta R.T.: -0.004 min  
Response: 1394208  
Conc: 23.36 ng/ml

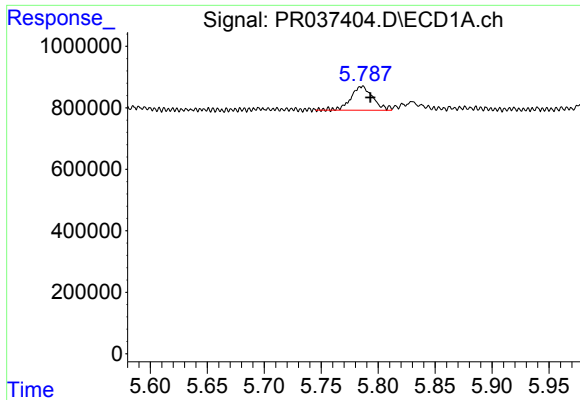

#15 AR-1232-5


R.T.: 5.786 min  
Delta R.T.: -0.008 min  
Response: 1043278  
Conc: 89.20 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

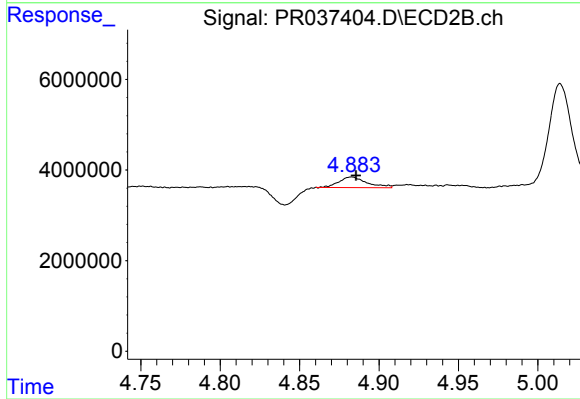


#15 AR-1232-5

R.T.: 4.883 min  
Delta R.T.: -0.003 min  
Response: 2910719  
Conc: 42.65 ng/ml

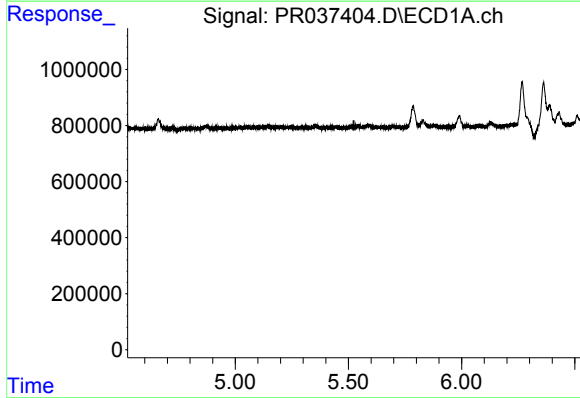


#16 AR-1242-1

R.T.: 0.000 min  
Exp R.T. : 5.524 min  
Response: 0  
Conc: N.D.

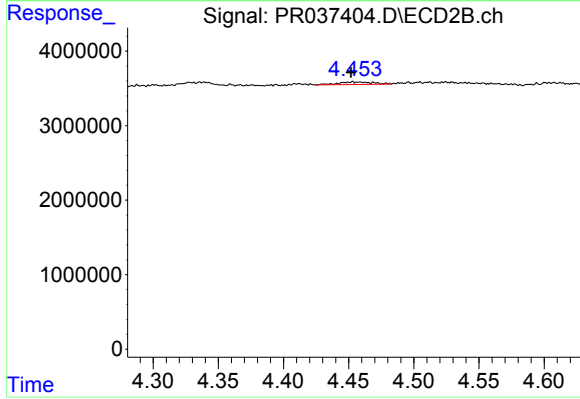

#16 AR-1242-1


R.T.: 4.453 min  
Delta R.T.: 0.001 min  
Response: 645087  
Conc: 4.40 ng/ml

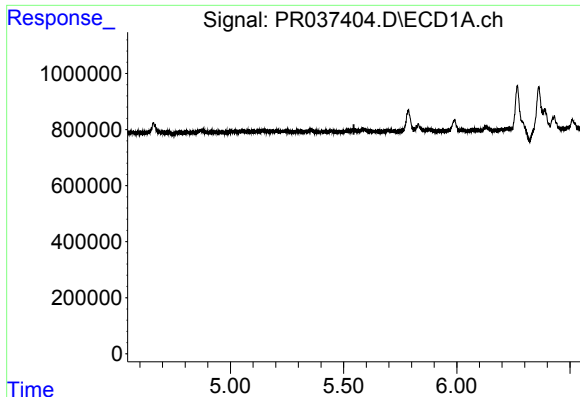

#17 AR-1242-2


R.T.: 0.000 min  
Exp R.T.: 5.545 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

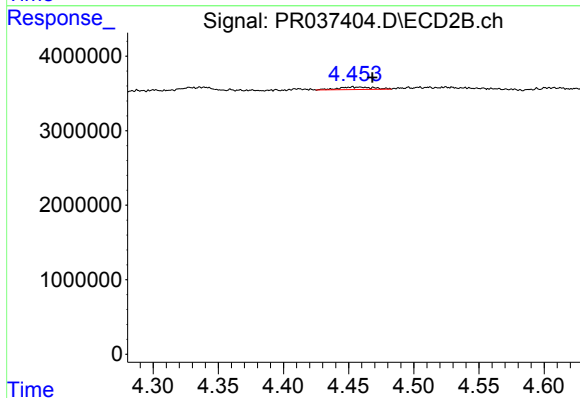


#17 AR-1242-2

R.T.: 4.453 min  
Delta R.T.: -0.015 min  
Response: 645087  
Conc: 2.83 ng/ml

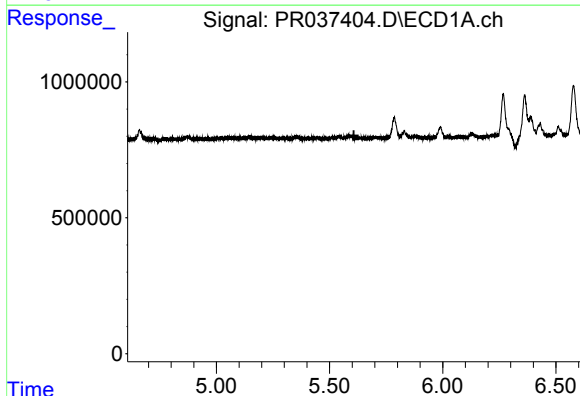


#18 AR-1242-3

R.T.: 0.000 min  
Exp R.T.: 5.608 min  
Response: 0  
Conc: N.D.

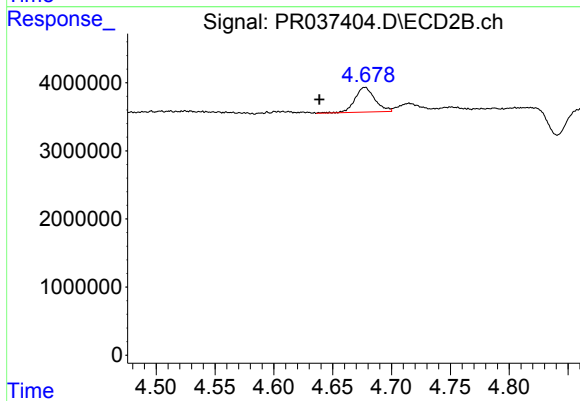

#18 AR-1242-3


R.T.: 4.677 min  
Delta R.T.: 0.039 min  
Response: 4270318  
Conc: 36.93 ng/ml

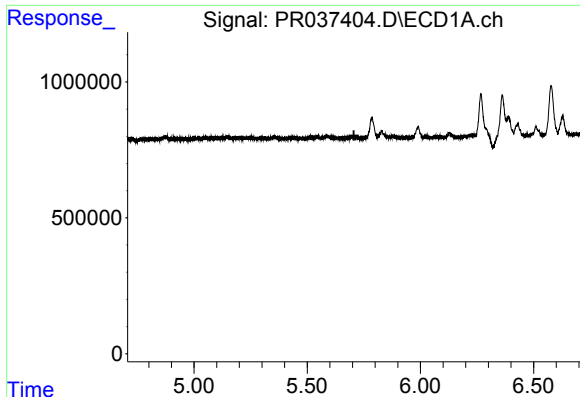

#19 AR-1242-4


R.T.: 0.000 min  
Exp R.T.: 5.706 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

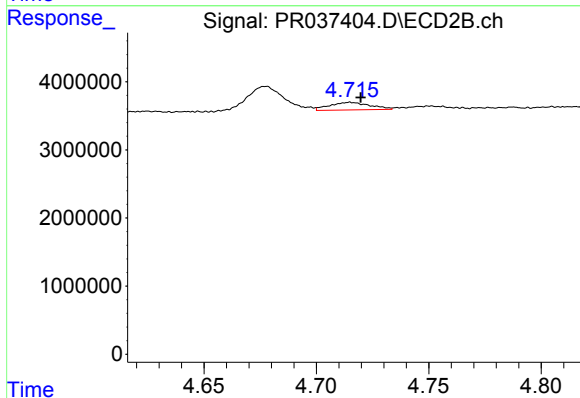


#19 AR-1242-4

R.T.: 4.715 min  
Delta R.T.: -0.005 min  
Response: 1394208  
Conc: 12.68 ng/ml

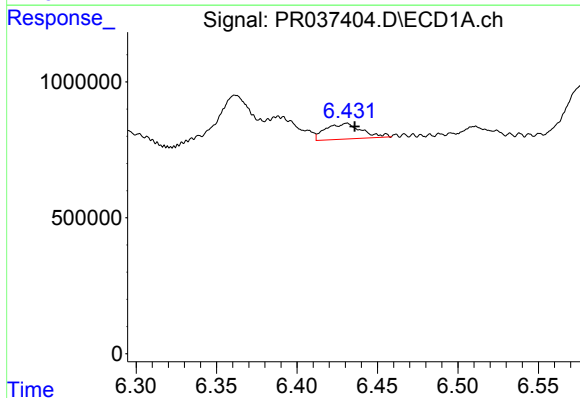


#20 AR-1242-5

R.T.: 6.430 min  
Delta R.T.: -0.006 min  
Response: 892311  
Conc: 27.73 ng/ml

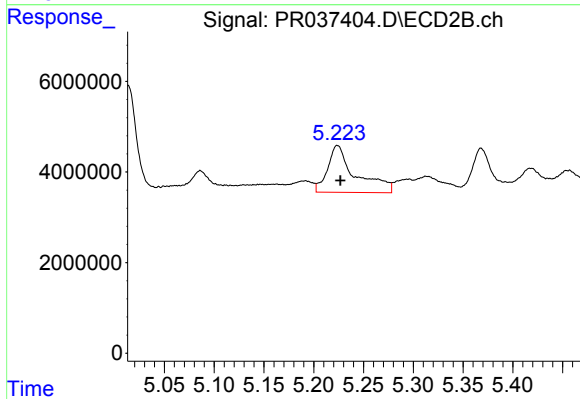

#20 AR-1242-5


R.T.: 5.224 min  
Delta R.T.: -0.003 min  
Response: 20227917  
Conc: 122.08 ng/ml

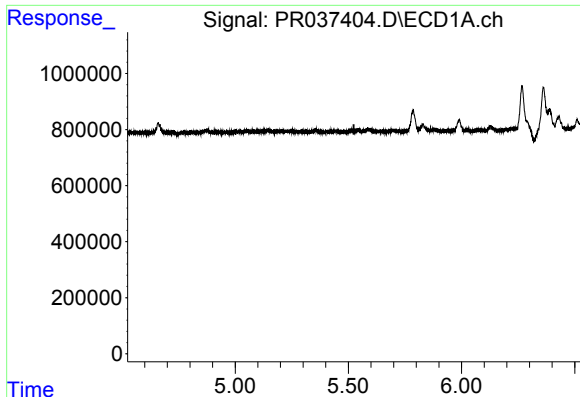

#21 AR-1248-1


R.T.: 0.000 min  
Exp R.T.: 5.525 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

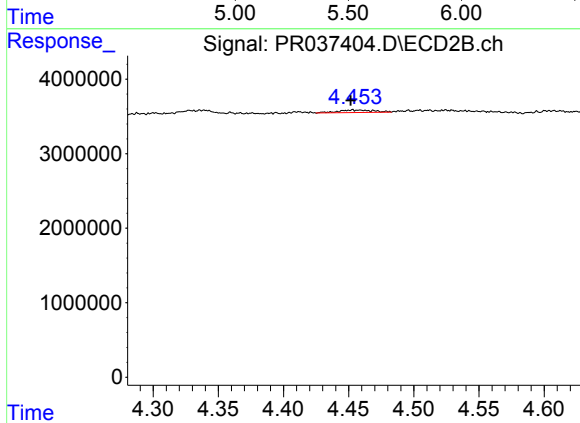


#21 AR-1248-1

R.T.: 4.453 min  
Delta R.T.: 0.001 min  
Response: 645087  
Conc: 6.41 ng/ml

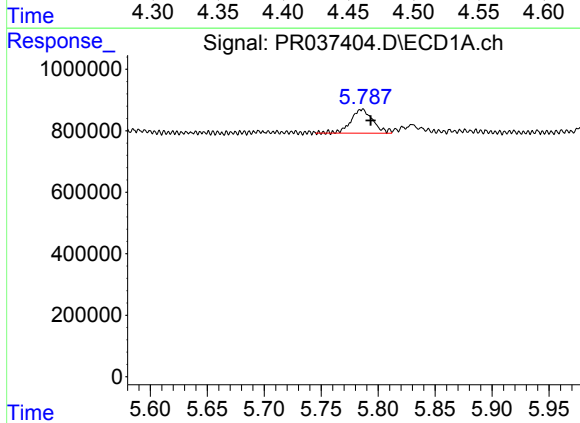


#22 AR-1248-2

R.T.: 5.786 min  
Delta R.T.: -0.008 min  
Response: 1043278  
Conc: 29.80 ng/ml

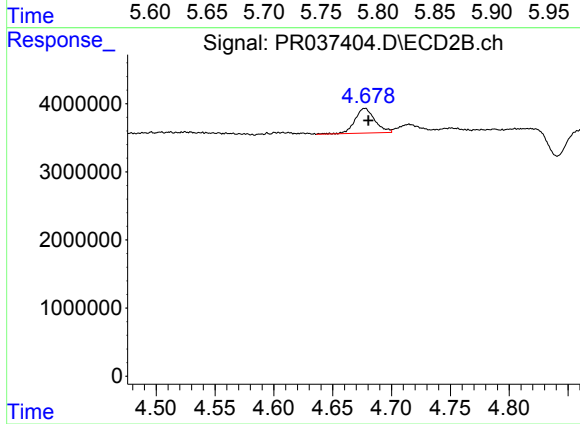

#22 AR-1248-2


R.T.: 4.677 min  
Delta R.T.: -0.003 min  
Response: 4270318  
Conc: 31.29 ng/ml

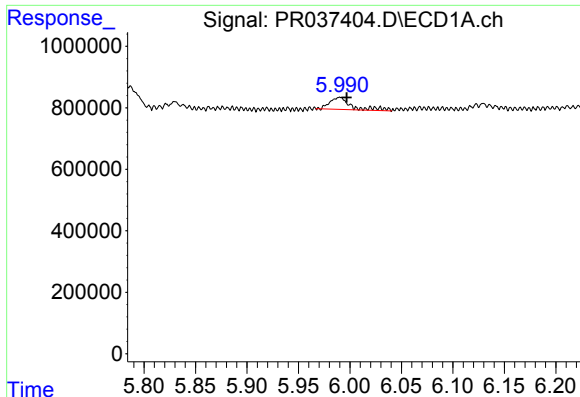

#23 AR-1248-3


R.T.: 5.990 min  
Delta R.T.: -0.007 min  
Response: 568874  
Conc: 13.91 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

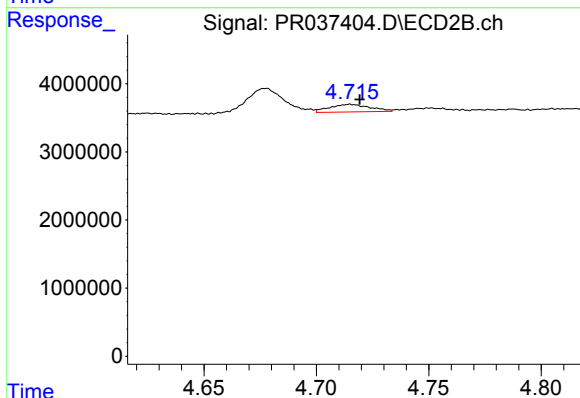


#23 AR-1248-3

R.T.: 4.715 min  
Delta R.T.: -0.004 min  
Response: 1394208  
Conc: 9.96 ng/ml

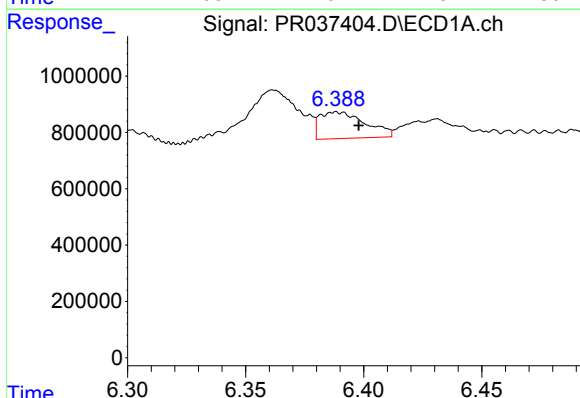


#24 AR-1248-4

R.T.: 6.388 min  
Delta R.T.: -0.010 min  
Response: 1268935  
Conc: 25.92 ng/ml

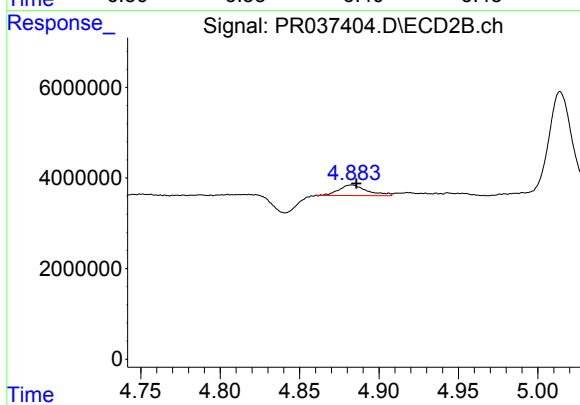

#24 AR-1248-4


R.T.: 4.883 min  
Delta R.T.: -0.003 min  
Response: 2910719  
Conc: 16.36 ng/ml

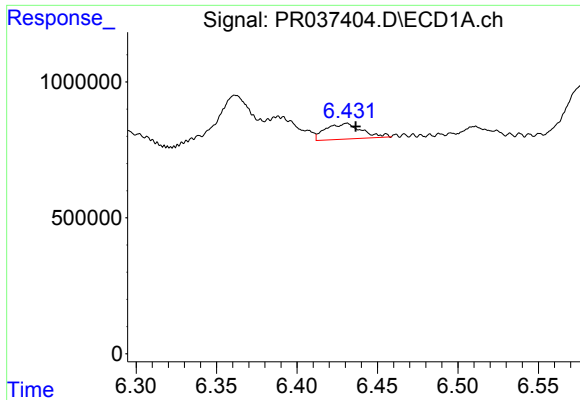

#25 AR-1248-5


R.T.: 6.430 min  
Delta R.T.: -0.006 min  
Response: 892311  
Conc: 18.89 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

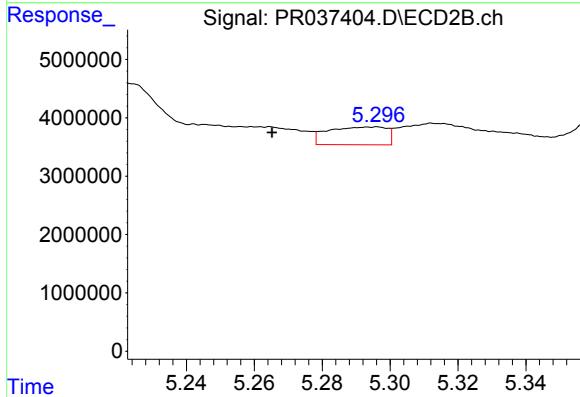


#25 AR-1248-5

R.T.: 5.295 min  
Delta R.T.: 0.030 min  
Response: 3683083  
Conc: 18.83 ng/ml

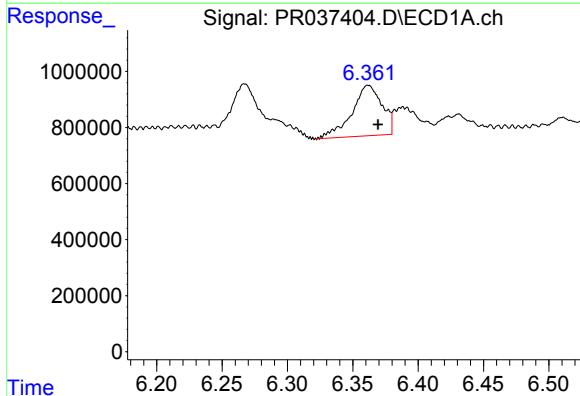

#26 AR-1254-1


R.T.: 6.362 min  
Delta R.T.: -0.007 min  
Response: 2888700  
Conc: 52.88 ng/ml

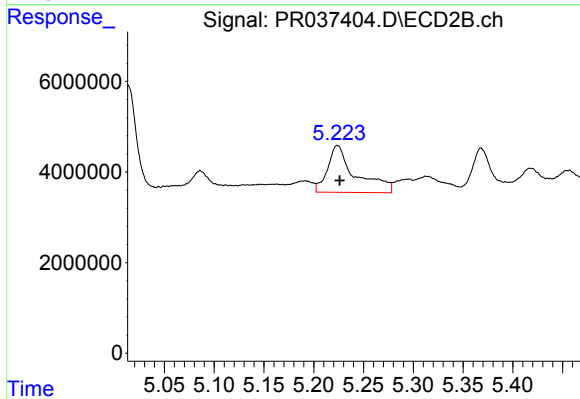

#26 AR-1254-1

R.T.: 5.224 min  
Delta R.T.: -0.002 min  
Response: 20227917  
Conc: 58.72 ng/ml




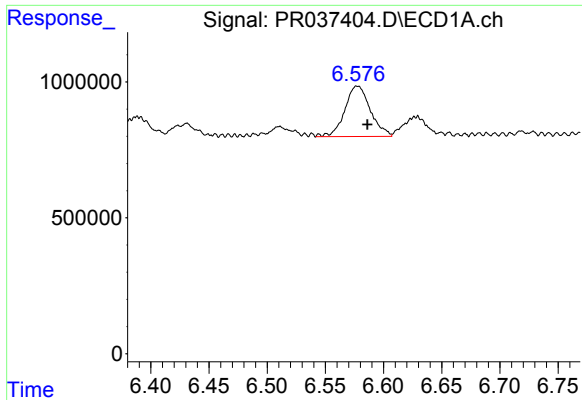

#27 AR-1254-2


R.T.: 6.578 min  
Delta R.T.: -0.008 min  
Response: 2834429  
Conc: 33.07 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

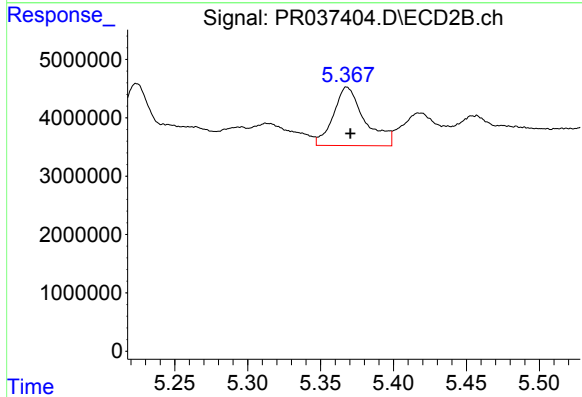


#27 AR-1254-2

R.T.: 5.368 min  
Delta R.T.: -0.002 min  
Response: 14966491  
Conc: 49.97 ng/ml

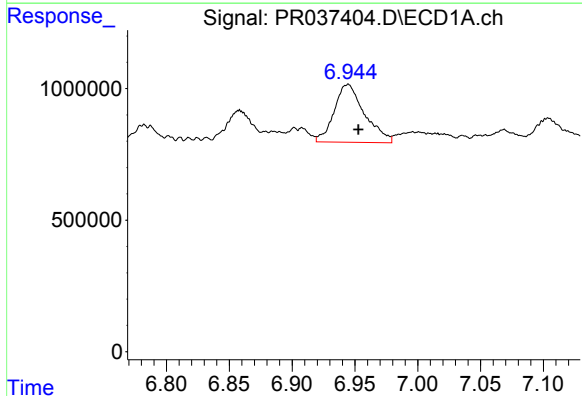


#28 AR-1254-3

R.T.: 6.944 min  
Delta R.T.: -0.008 min  
Response: 3708436  
Conc: 40.77 ng/ml

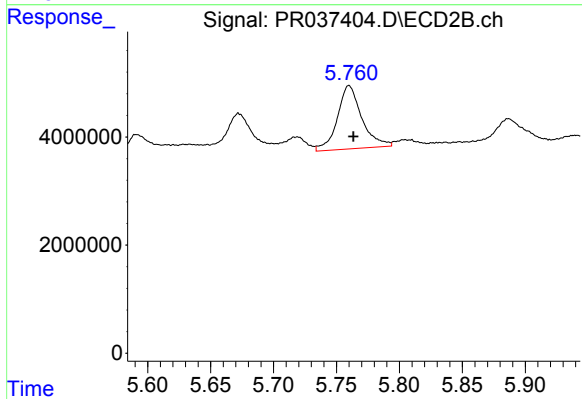

#28 AR-1254-3


R.T.: 5.760 min  
Delta R.T.: -0.003 min  
Response: 15778295  
Conc: 33.31 ng/ml

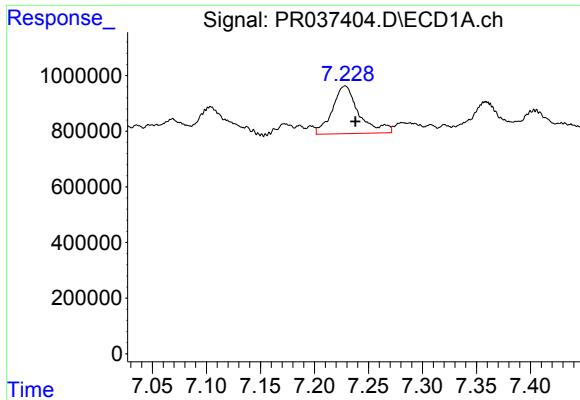

#29 AR-1254-4


R.T.: 7.228 min  
Delta R.T.: -0.010 min  
Response: 2942624  
Conc: 43.91 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

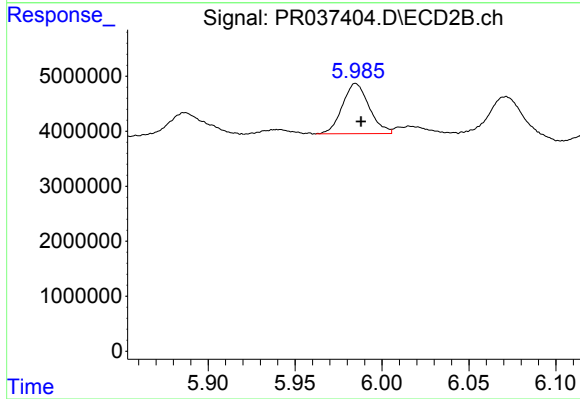


#29 AR-1254-4

R.T.: 5.985 min  
Delta R.T.: -0.003 min  
Response: 9770668  
Conc: 27.86 ng/ml

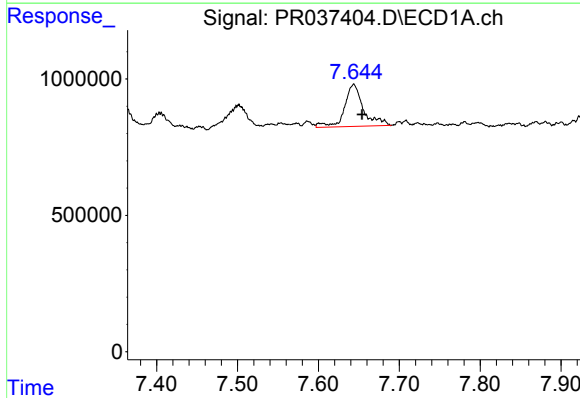


#30 AR-1254-5

R.T.: 7.644 min  
Delta R.T.: -0.010 min  
Response: 2501854  
Conc: 34.81 ng/ml

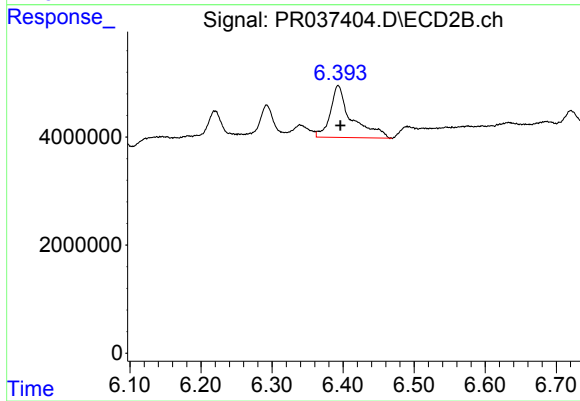

#30 AR-1254-5


R.T.: 6.393 min  
Delta R.T.: -0.003 min  
Response: 19891964  
Conc: 44.92 ng/ml

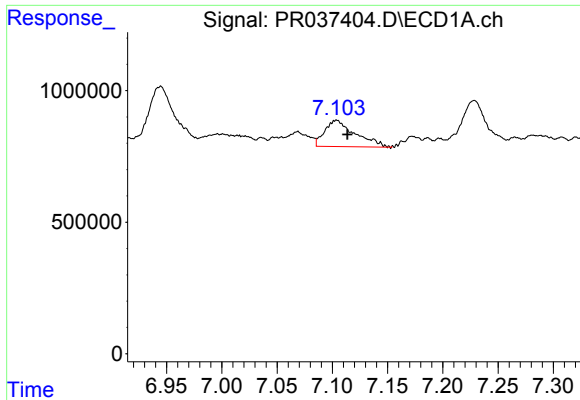

#31 AR-1260-1


R.T.: 7.104 min  
Delta R.T.: -0.010 min  
Response: 1925019  
Conc: 29.17 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

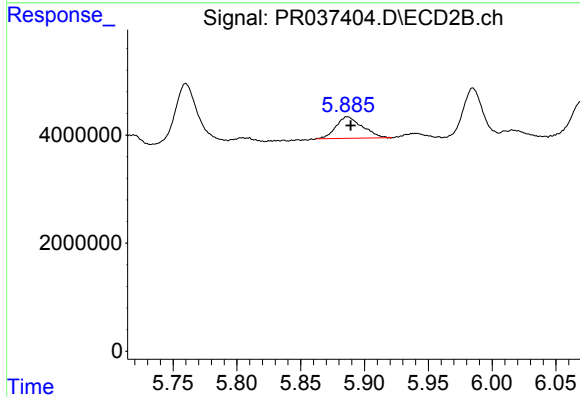


#31 AR-1260-1

R.T.: 5.887 min  
Delta R.T.: -0.002 min  
Response: 5741901  
Conc: 19.65 ng/ml

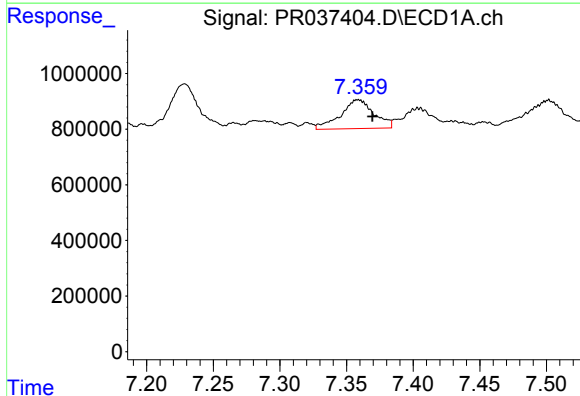


#32 AR-1260-2

R.T.: 7.359 min  
Delta R.T.: -0.011 min  
Response: 1805041  
Conc: 22.65 ng/ml

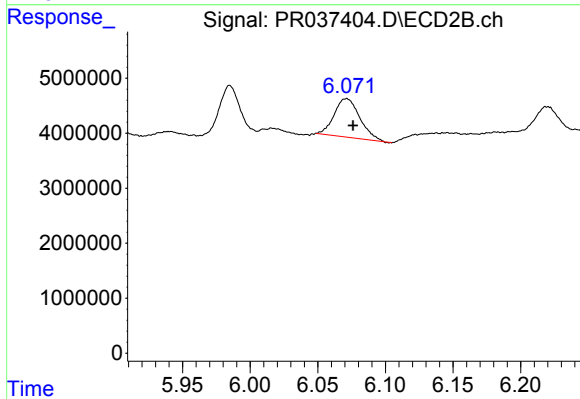

#32 AR-1260-2


R.T.: 6.071 min  
Delta R.T.: -0.005 min  
Response: 9060732  
Conc: 19.67 ng/ml

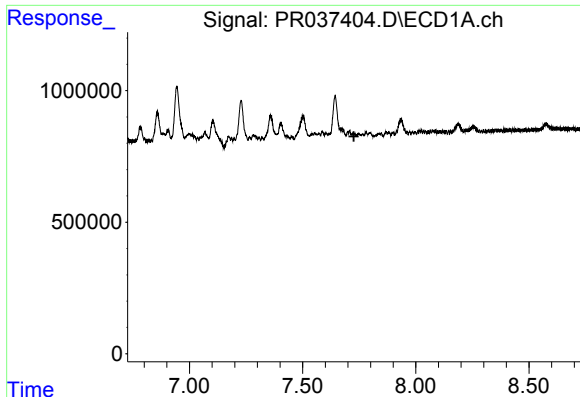

#33 AR-1260-3


R.T.: 0.000 min  
Exp R.T.: 7.726 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

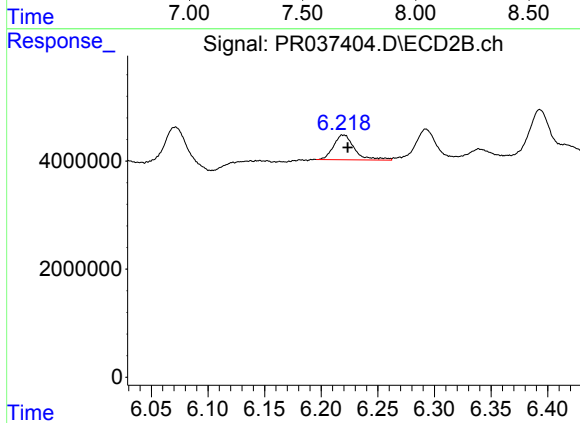


#33 AR-1260-3

R.T.: 6.220 min  
Delta R.T.: -0.004 min  
Response: 5865297  
Conc: 16.45 ng/ml

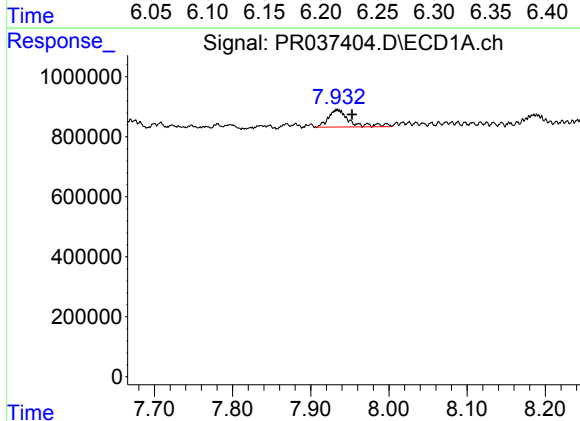


#34 AR-1260-4

R.T.: 7.934 min  
Delta R.T.: -0.019 min  
Response: 1075762  
Conc: 14.46 ng/ml

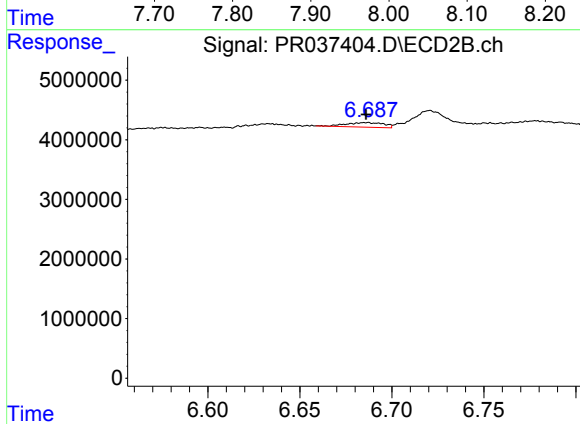

#34 AR-1260-4


R.T.: 6.686 min  
Delta R.T.: 0.000 min  
Response: 1085097  
Conc: 3.56 ng/ml

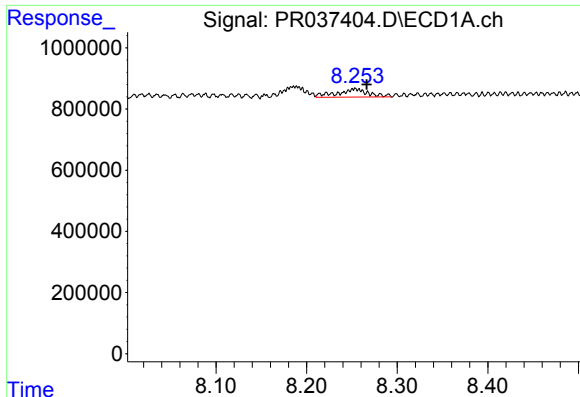

#35 AR-1260-5


R.T.: 8.254 min  
Delta R.T.: -0.012 min  
Response: 634289  
Conc: 4.39 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

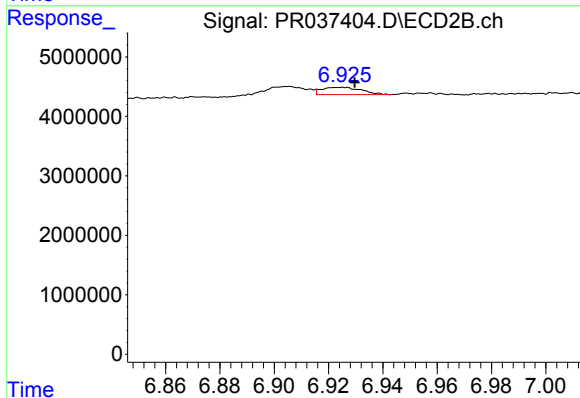


#35 AR-1260-5

R.T.: 6.925 min  
Delta R.T.: -0.005 min  
Response: 1238428  
Conc: 1.43 ng/ml

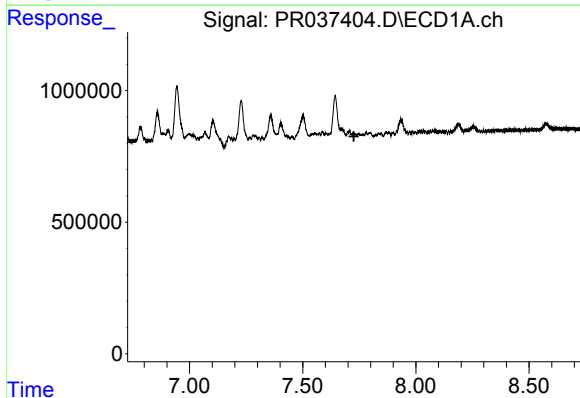


#36 AR-1262-1

R.T.: 0.000 min  
Exp R.T. : 7.726 min  
Response: 0  
Conc: N.D.

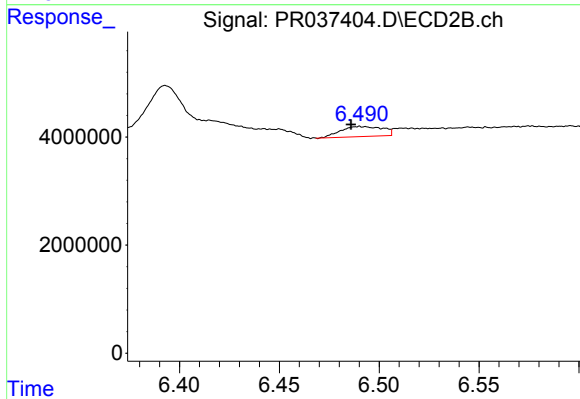

#36 AR-1262-1


R.T.: 6.490 min  
Delta R.T.: 0.005 min  
Response: 2699588  
Conc: 10.77 ng/ml

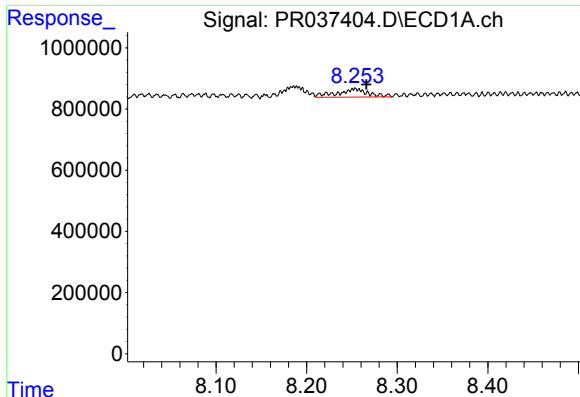

#37 AR-1262-2


R.T.: 8.254 min  
Delta R.T.: -0.012 min  
Response: 634289  
Conc: 3.26 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

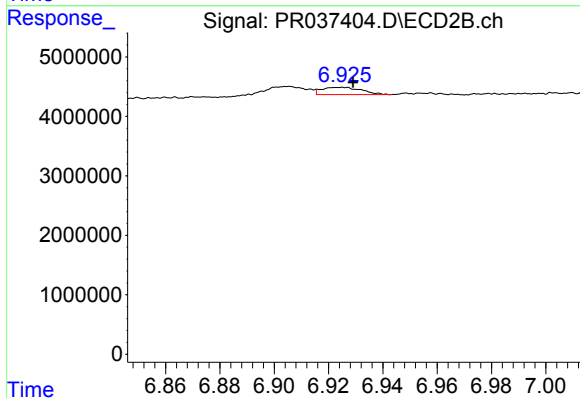


#37 AR-1262-2

R.T.: 6.925 min  
Delta R.T.: -0.004 min  
Response: 1238428  
Conc: 0.99 ng/ml

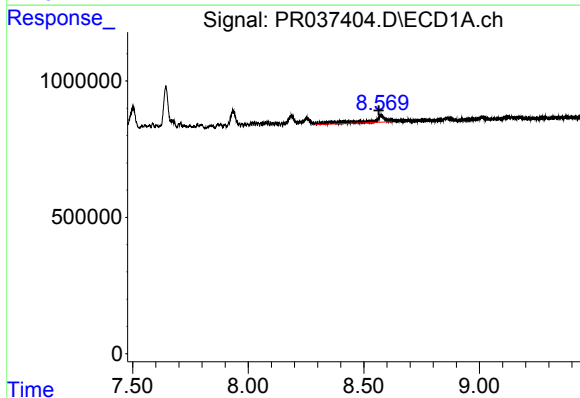


#38 AR-1262-3

R.T.: 8.574 min  
Delta R.T.: 0.009 min  
Response: 1276234  
Conc: 9.70 ng/ml

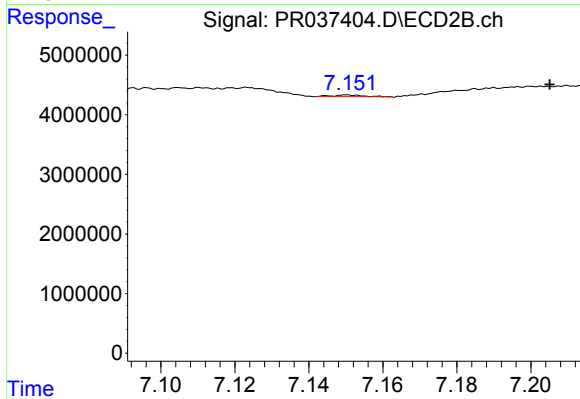

#38 AR-1262-3


R.T.: 7.151 min  
Delta R.T.: -0.054 min  
Response: 169195  
Conc: 0.31 ng/ml

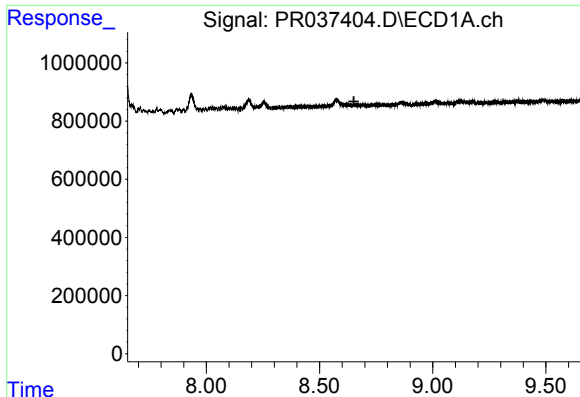

#39 AR-1262-4


R.T.: 0.000 min  
Exp R.T.: 8.652 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

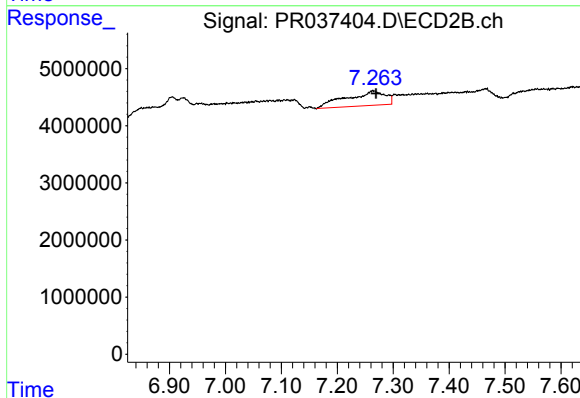


#39 AR-1262-4

R.T.: 7.264 min  
Delta R.T.: -0.005 min  
Response: 12350701  
Conc: 13.76 ng/ml

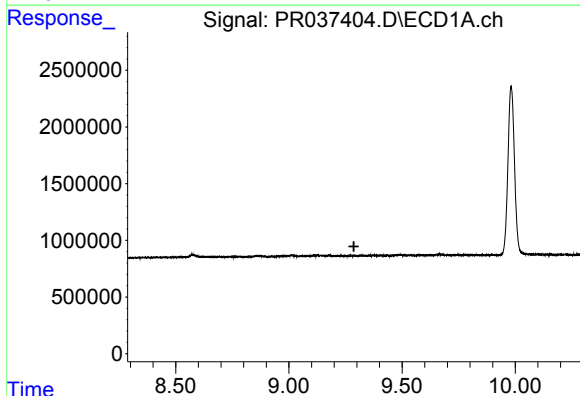


#40 AR-1262-5

R.T.: 0.000 min  
Exp R.T.: 9.287 min  
Response: 0  
Conc: N.D.

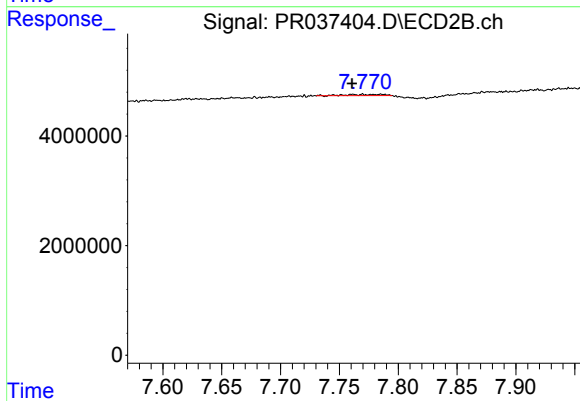

#40 AR-1262-5


R.T.: 7.770 min  
Delta R.T.: 0.009 min  
Response: 526624  
Conc: 1.38 ng/ml

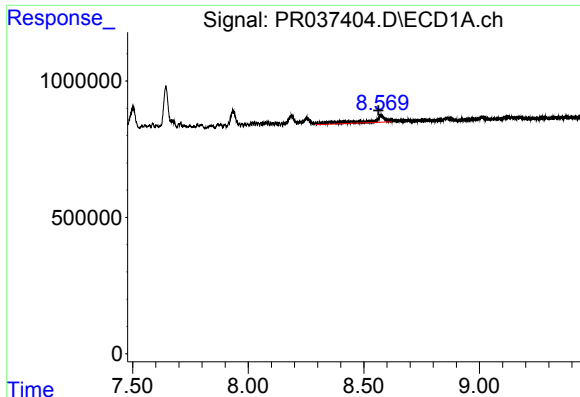

#41 AR-1268-1


R.T.: 8.574 min  
Delta R.T.: 0.011 min  
Response: 1276234  
Conc: 7.13 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

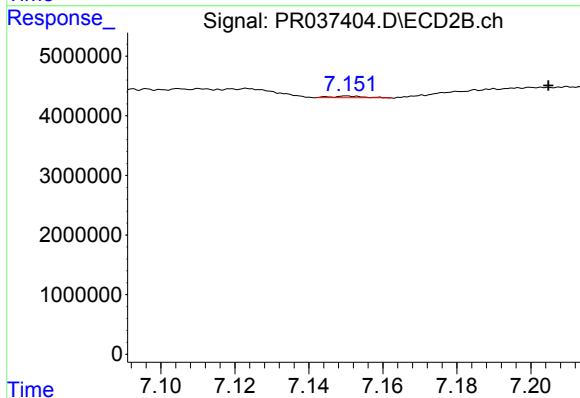


#41 AR-1268-1

R.T.: 7.151 min  
Delta R.T.: -0.054 min  
Response: 169195  
Conc: 0.14 ng/ml

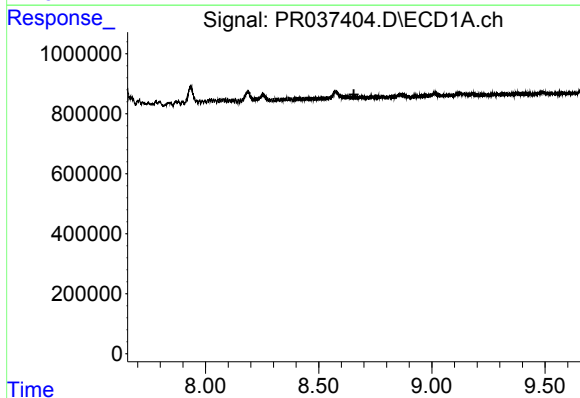

#42 AR-1268-2


R.T.: 0.000 min  
Exp R.T. : 8.655 min  
Response: 0  
Conc: N.D.

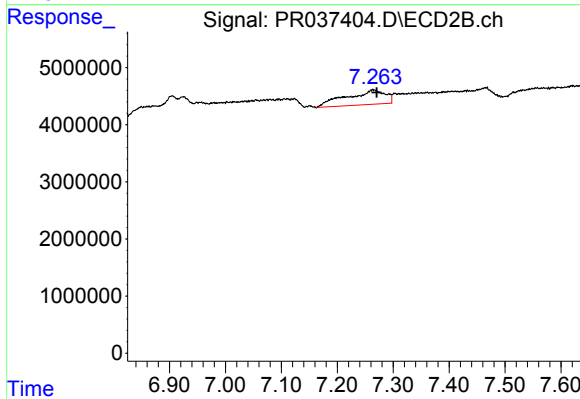

#42 AR-1268-2

R.T.: 7.264 min  
Delta R.T.: -0.006 min  
Response: 12350701  
Conc: 11.66 ng/ml




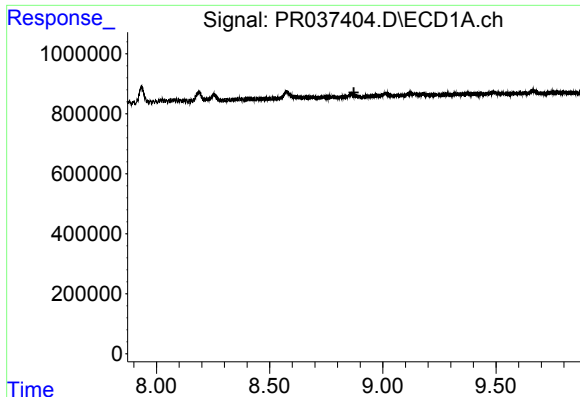

#43 AR-1268-3


R.T.: 0.000 min  
Exp R.T.: 8.872 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

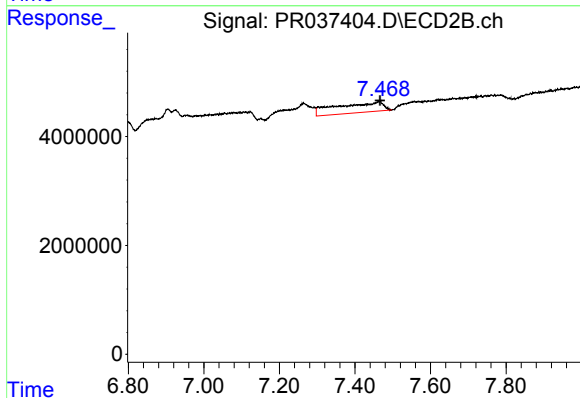


#43 AR-1268-3

R.T.: 7.466 min  
Delta R.T.: 0.000 min  
Response: 16229572  
Conc: 18.31 ng/ml

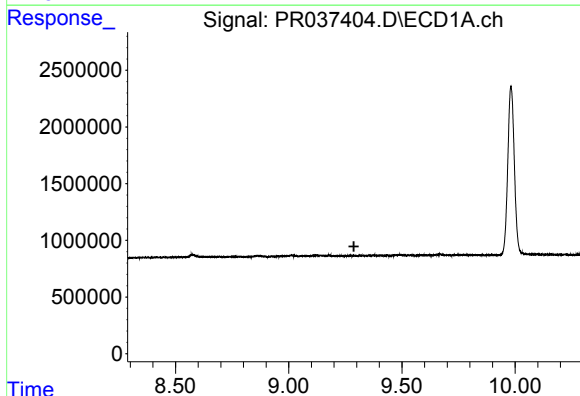


#44 AR-1268-4

R.T.: 0.000 min  
Exp R.T.: 9.288 min  
Response: 0  
Conc: N.D.

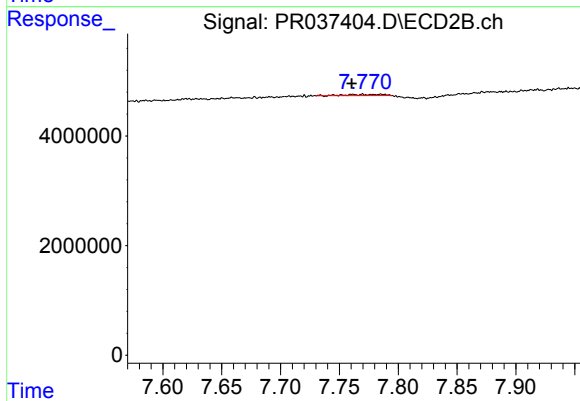

#44 AR-1268-4


R.T.: 7.770 min  
Delta R.T.: 0.009 min  
Response: 526624  
Conc: 1.45 ng/ml

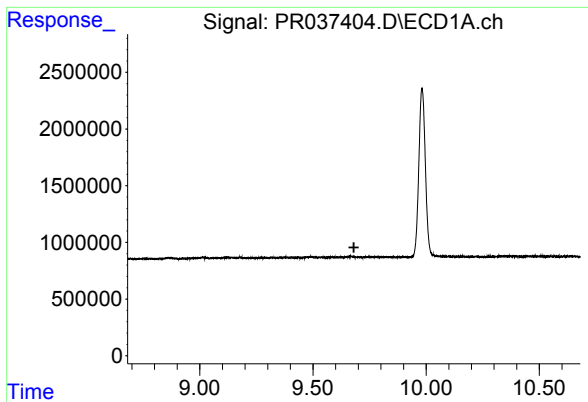

#45 AR-1268-5

R.T.: 0.000 min  
Exp R.T.: 9.681 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT2-2019

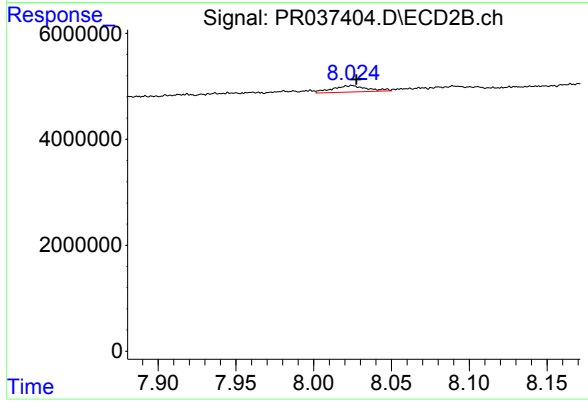

#45 AR-1268-5

R.T.: 8.025 min  
Delta R.T.: -0.003 min  
Response: 1874543  
Conc: 0.74 ng/ml