

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
 Data File : PR037405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 16:50
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1262 MDL 25PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:44:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.357	3.406	32146516	126.8E6	25.697	26.437
2)	SA Decachlor...	9.981	8.243	30001764	153.3E6	22.684	26.317
Target Compounds							
3)	L1 AR-1016-1	0.000	4.451	0	433800	N.D.	2.382 #
4)	L1 AR-1016-2	0.000	4.451	0	433800	N.D.	1.538 #
5)	L1 AR-1016-3	0.000	4.672	0	63035	N.D.	0.438 #
6)	L1 AR-1016-4	0.000	4.677	0	68737	N.D.	0.621 #
7)	L1 AR-1016-5	0.000	4.883	0	2298907	N.D.	15.123 #
8)	L2 AR-1221-1	0.000	3.565	0	1161250	N.D.	22.806 #
9)	L2 AR-1221-2	4.663	3.694	712845	1941245	78.820	52.274 #
10)	L2 AR-1221-3	0.000	3.754	0	28519	N.D.	0.233 #
11)	L3 AR-1232-1	0.000	3.754	0	28519	N.D.	0.244 #
12)	L3 AR-1232-2	0.000	4.451	0	433800	N.D.	3.138 #
13)	L3 AR-1232-3	0.000	4.604	0	64173	N.D.	0.914 #
14)	L3 AR-1232-4	0.000	4.721	0	134758	N.D.	2.258 #
15)	L3 AR-1232-5	0.000	4.883	0	2298907	N.D.	33.687 #
16)	L4 AR-1242-1	0.000	4.451	0	433800	N.D.	2.960 #
17)	L4 AR-1242-2	0.000	4.451	0	433800	N.D.	1.901 #
18)	L4 AR-1242-3	0.000	4.672	0	63035	N.D.	0.545 #
19)	L4 AR-1242-4	0.000	4.721	0	134758	N.D.	1.226 #
20)	L4 AR-1242-5	0.000	5.246	0	31143892	N.D.	187.954 #
21)	L5 AR-1248-1	0.000	4.451	0	433800	N.D.	4.309 #
22)	L5 AR-1248-2	0.000	4.677	0	68737	N.D.	0.504 #
23)	L5 AR-1248-3	0.000	4.721	0	134758	N.D.	0.963 #
24)	L5 AR-1248-4	6.366	4.883	4939697	2298907	100.904	12.918 #
25)	L5 AR-1248-5	0.000	5.276	0	5770350	N.D.	29.499 #
26)	L6 AR-1254-1	6.366	5.246	4939697	31143892	90.419	90.410
27)	L6 AR-1254-2	0.000	5.373	0	10097694	N.D.	33.715 #
28)	L6 AR-1254-3	6.962	5.773	2369207	10810045	26.046	22.824
29)	L6 AR-1254-4	7.245	5.996	431956	22189	6.446	0.063 #
30)	L6 AR-1254-5	7.716	6.429	1630099	10312600	22.678	23.288
31)	L7 AR-1260-1	0.000	5.894	0	191671	N.D.	0.656 #
32)	L7 AR-1260-2	0.000	6.066	0	6816257	N.D.	14.799 #
33)	L7 AR-1260-3	7.716	6.223	1630099	909920	26.050	2.552 #
34)	L7 AR-1260-4	7.958	6.676	1523127	6707620	20.471	22.009
35)	L7 AR-1260-5	8.254	6.925	762897	3623928	5.275	4.179
36)	L8 AR-1262-1	7.716	6.488	1630099	2449893	15.606	9.775 #
37)	L8 AR-1262-2	8.254	6.925	762897	3623928	3.925	2.885 #
38)	L8 AR-1262-3	8.552	7.201	5627199	37988058	42.789	69.288 #
39)	L8 AR-1262-4	8.644	7.266	5199787	45475763	52.935	50.661
40)	L8 AR-1262-5	9.275	7.756	1992995	10498861	28.867	27.439
41)	L9 AR-1268-1	8.552	7.201	5627199	37988058	31.421	30.859

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
 Data File : PR037405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 16:50
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1262 MDL 25PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 00:44:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.644	7.266	5199787	45475763	31.610	42.945 #
43) L9	AR-1268-3	8.860	7.463	4913465	26770888	35.492	30.207
44) L9	AR-1268-4	9.275	7.756	1992995	10498861	31.946	28.940
45) L9	AR-1268-5	9.666	8.024	12285851	67713196	26.950	26.615



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042519\
Data File : PR037405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 16:50
Operator : SM\SJ
Sample : K2241-09
Misc : AR1262 MDL 25PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 00:44:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

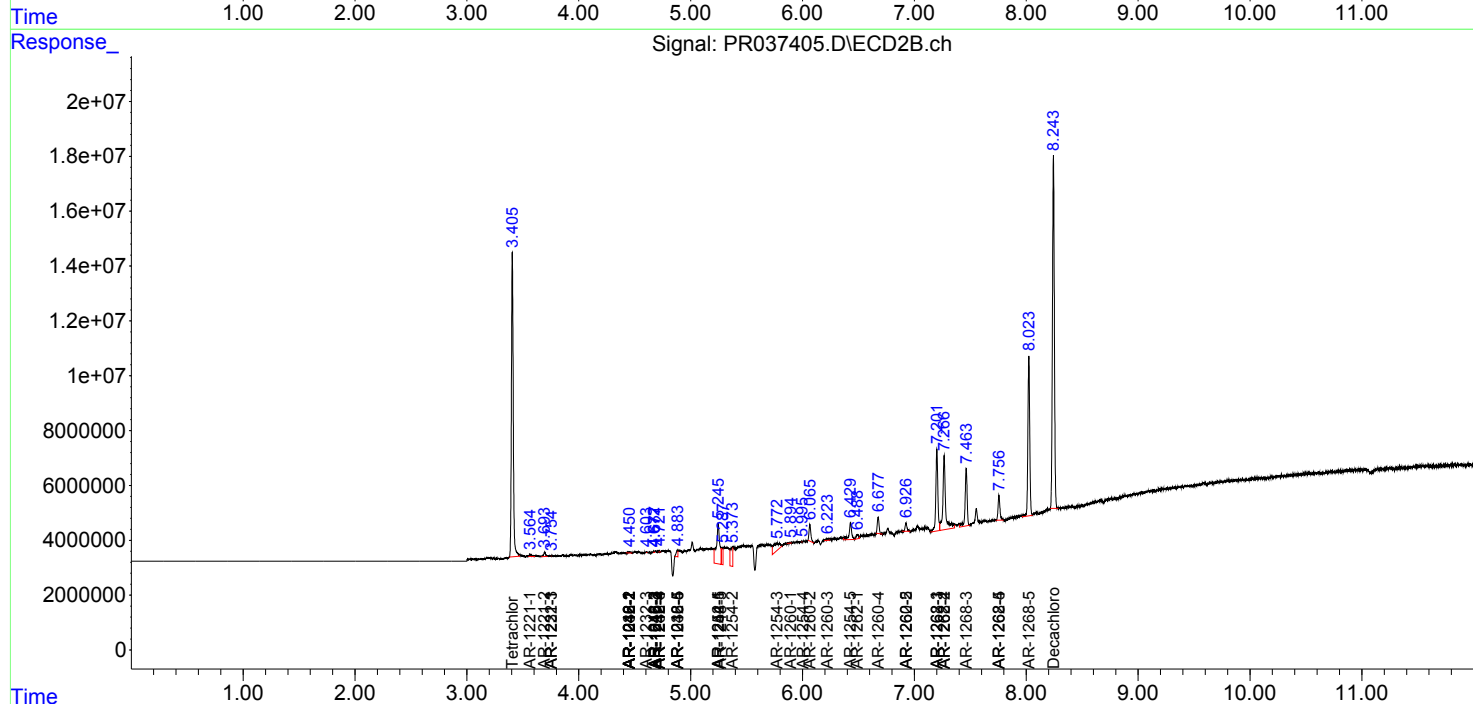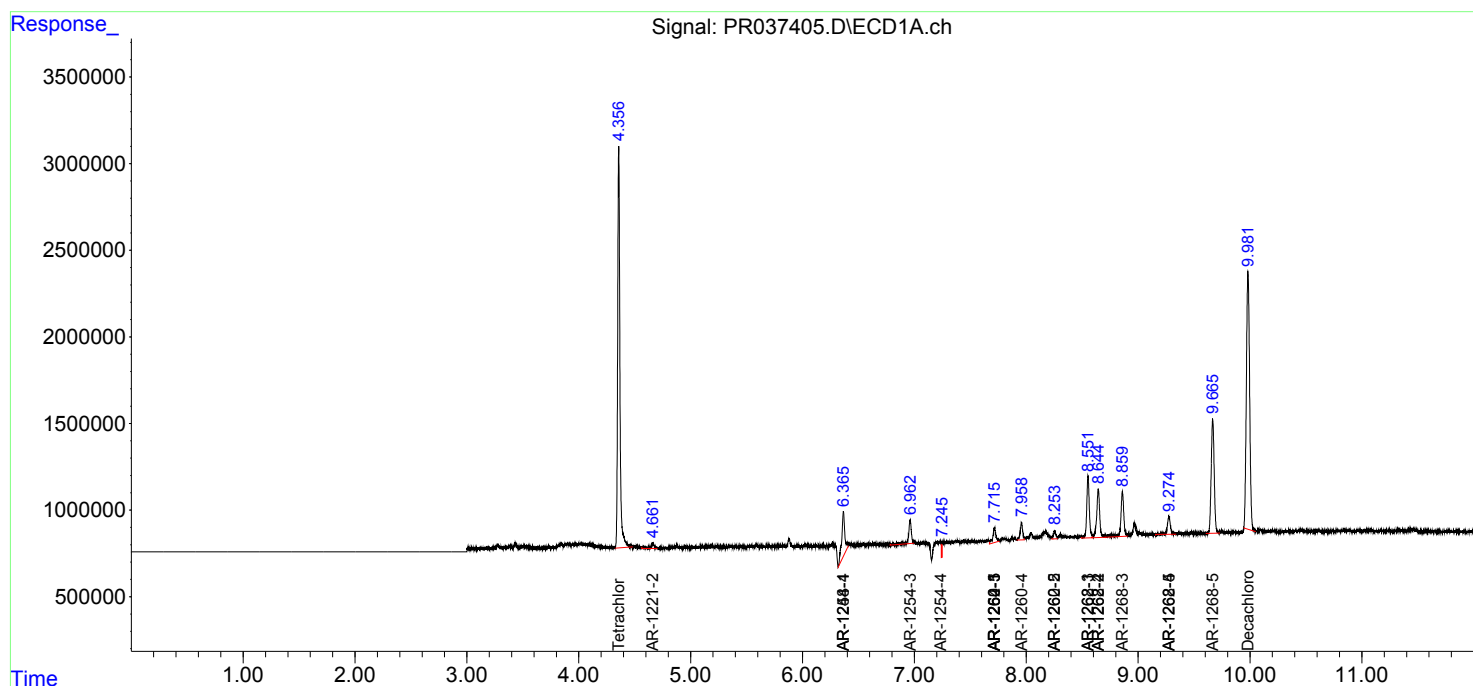


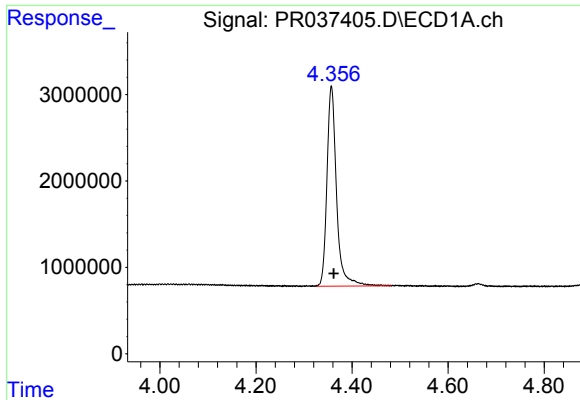

#1 Tetrachloro-m-xylene


R.T.: 4.357 min
Delta R.T.: -0.005 min
Response: 32146516
Conc: 25.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

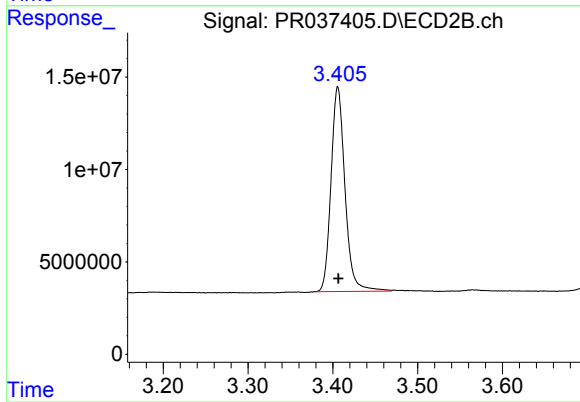


#1 Tetrachloro-m-xylene

R.T.: 3.406 min
Delta R.T.: 0.000 min
Response: 126781519
Conc: 26.44 ng/ml

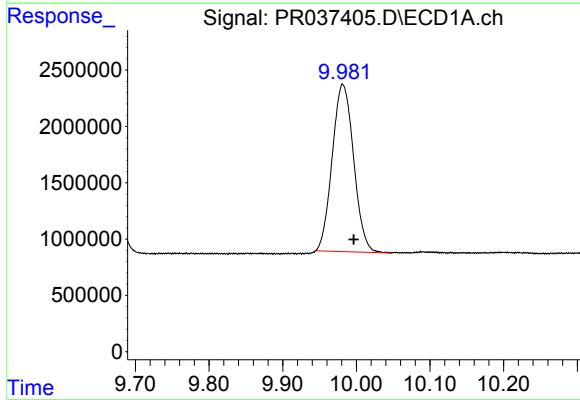


#2 Decachlorobiphenyl

R.T.: 9.981 min
Delta R.T.: -0.015 min
Response: 30001764
Conc: 22.68 ng/ml

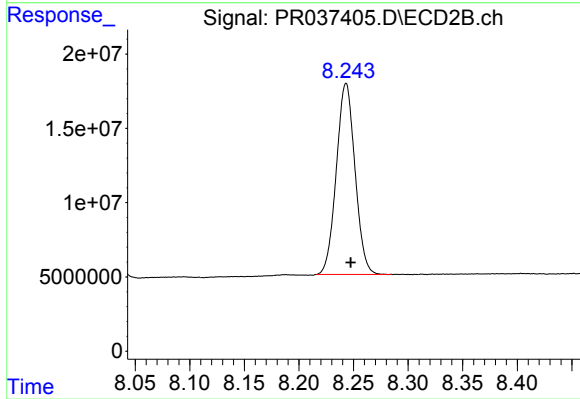

#2 Decachlorobiphenyl


R.T.: 8.243 min
Delta R.T.: -0.004 min
Response: 153278417
Conc: 26.32 ng/ml

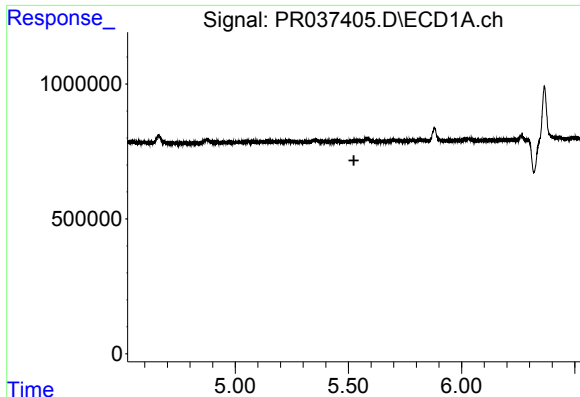

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

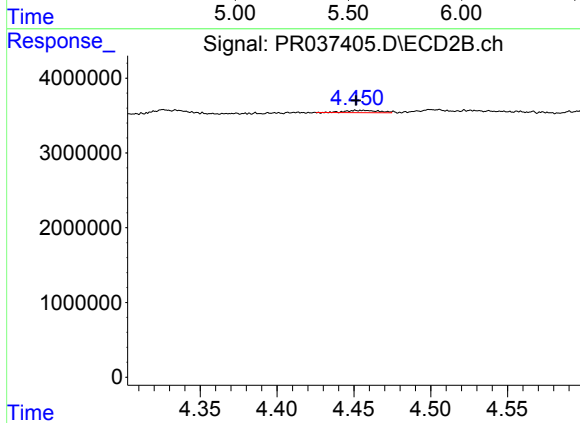


#3 AR-1016-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 433800
Conc: 2.38 ng/ml

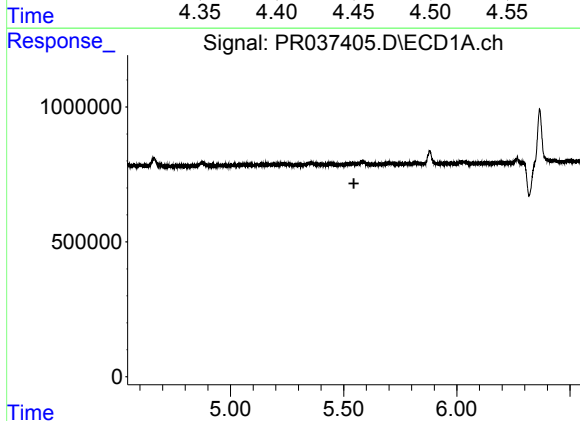


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

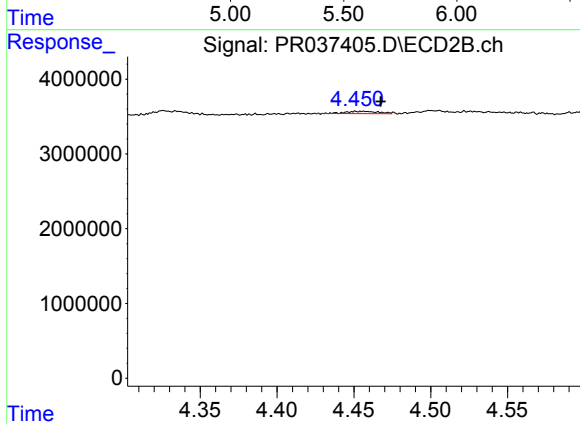

#4 AR-1016-2


R.T.: 4.451 min
Delta R.T.: -0.016 min
Response: 433800
Conc: 1.54 ng/ml

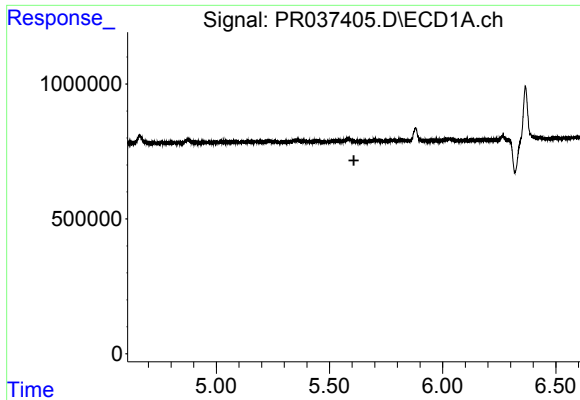

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

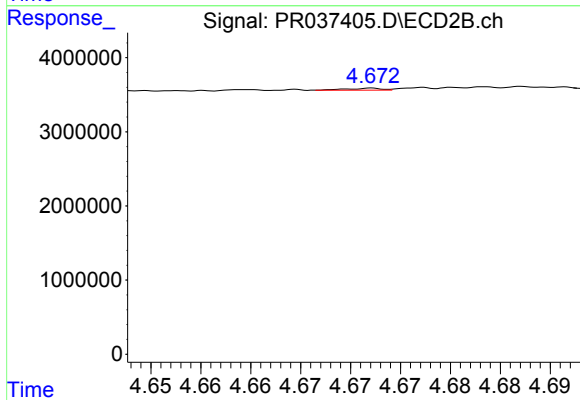


#5 AR-1016-3

R.T.: 4.672 min
Delta R.T.: 0.034 min
Response: 63035
Conc: 0.44 ng/ml

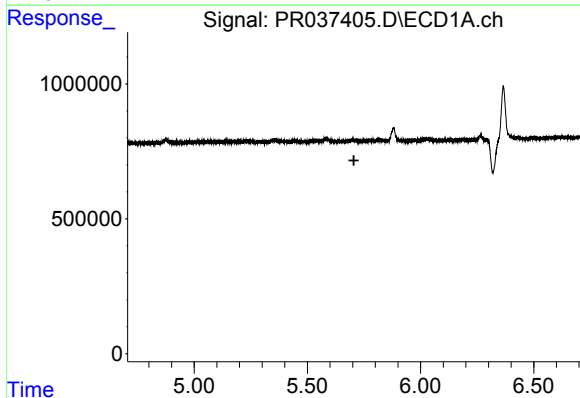


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

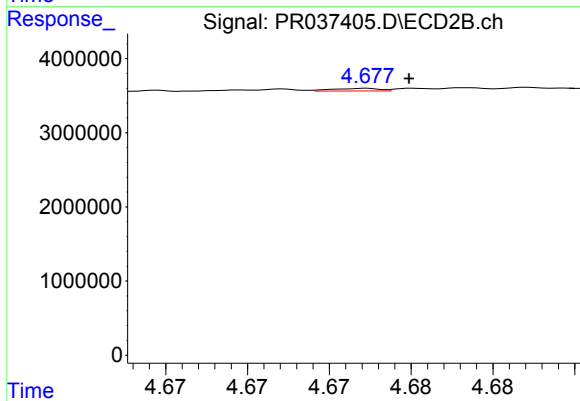

#6 AR-1016-4


R.T.: 4.677 min
Delta R.T.: -0.003 min
Response: 68737
Conc: 0.62 ng/ml

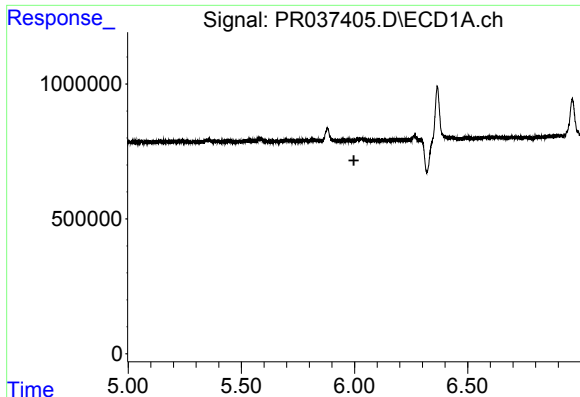

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

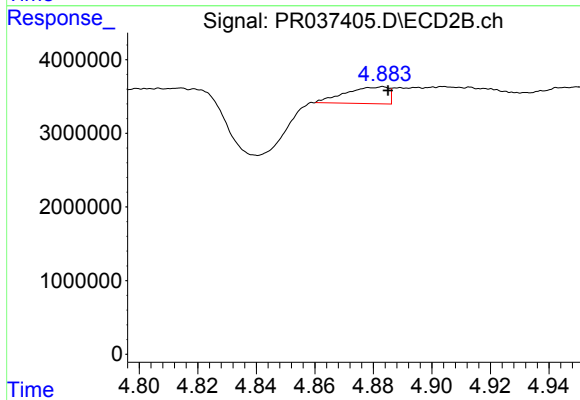


#7 AR-1016-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 2298907
Conc: 15.12 ng/ml

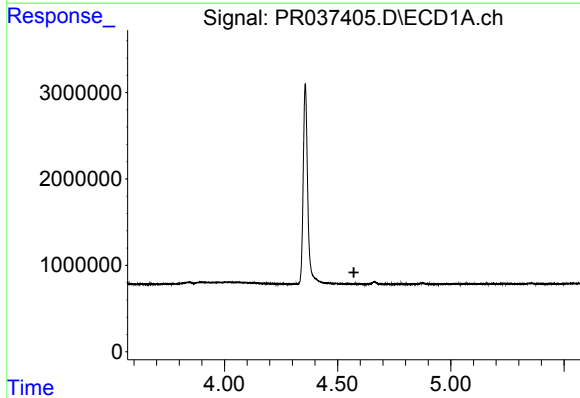


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

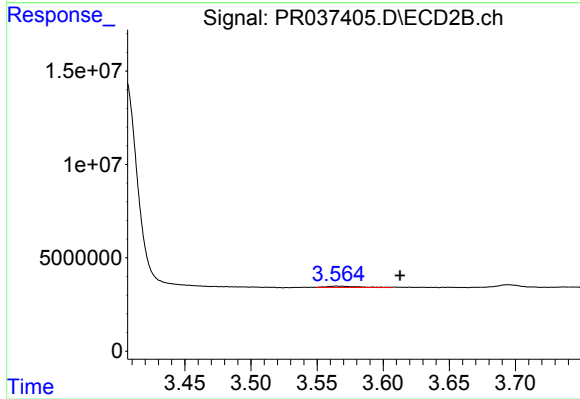

#8 AR-1221-1


R.T.: 3.565 min
Delta R.T.: -0.048 min
Response: 1161250
Conc: 22.81 ng/ml

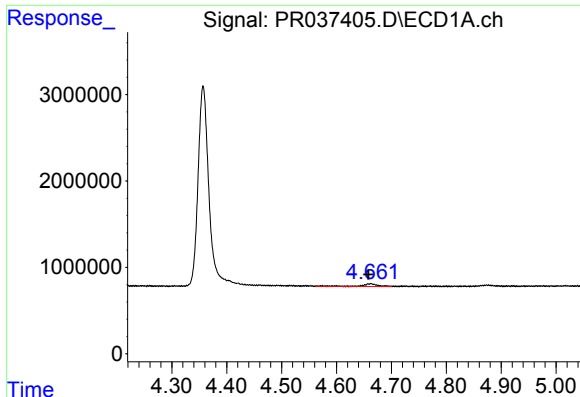

#9 AR-1221-2


R.T.: 4.663 min
Delta R.T.: 0.005 min
Response: 712845
Conc: 78.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

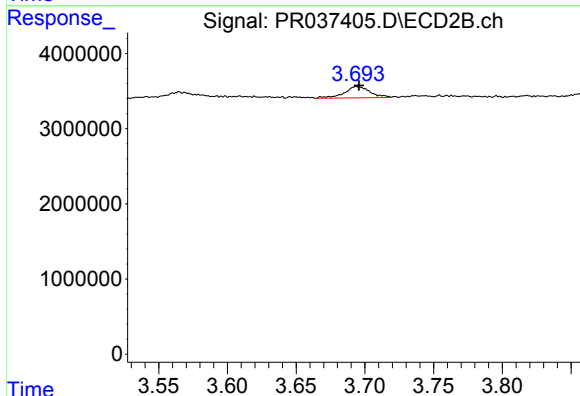


#9 AR-1221-2

R.T.: 3.694 min
Delta R.T.: -0.002 min
Response: 1941245
Conc: 52.27 ng/ml

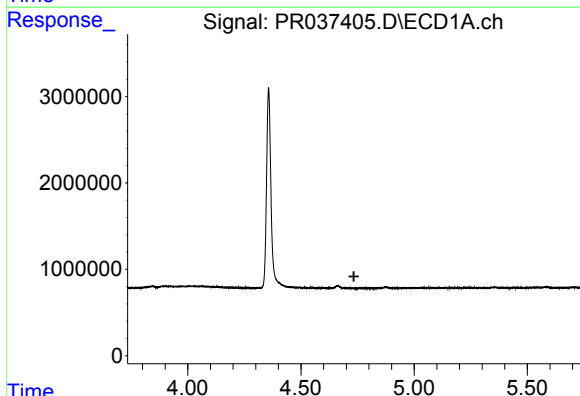


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

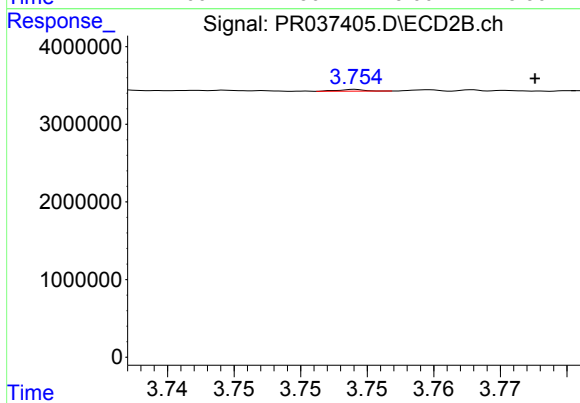

#10 AR-1221-3


R.T.: 3.754 min
Delta R.T.: -0.013 min
Response: 28519
Conc: 0.23 ng/ml

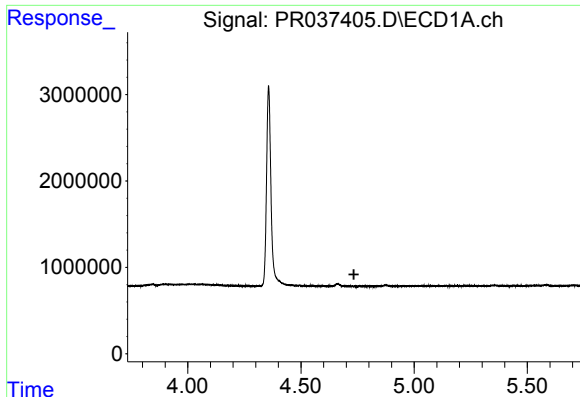

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

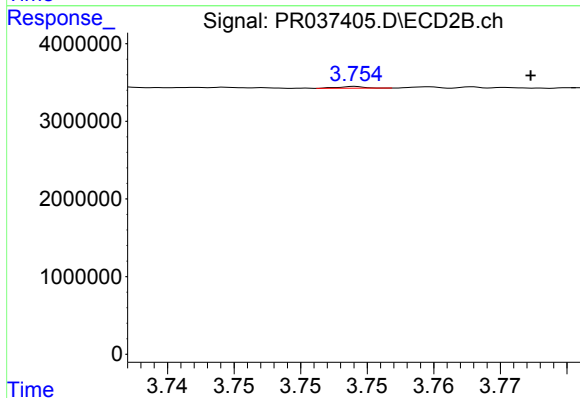


#11 AR-1232-1

R.T.: 3.754 min
Delta R.T.: -0.013 min
Response: 28519
Conc: 0.24 ng/ml

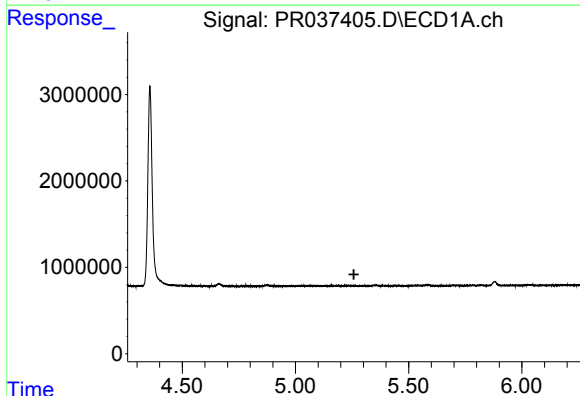


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

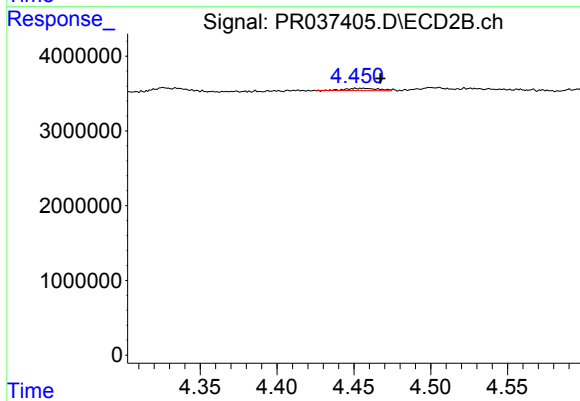

#12 AR-1232-2


R.T.: 4.451 min
Delta R.T.: -0.016 min
Response: 433800
Conc: 3.14 ng/ml

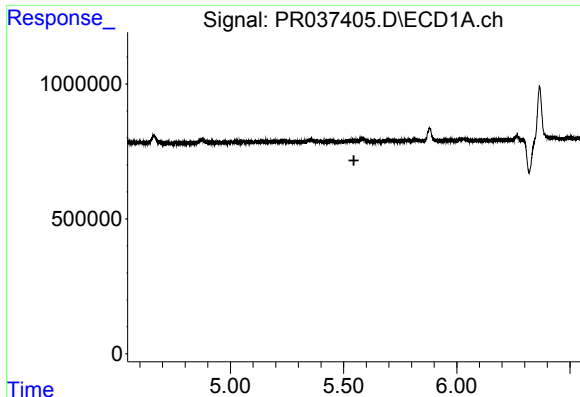

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

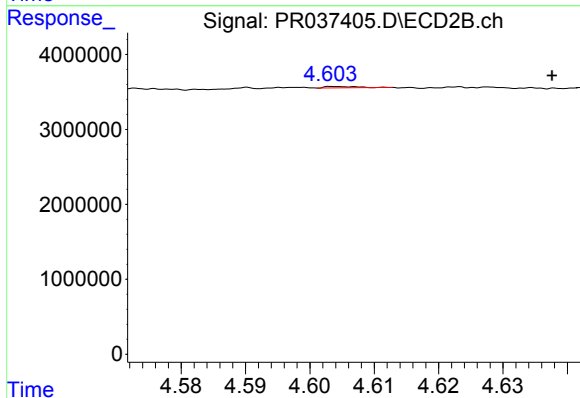


#13 AR-1232-3

R.T.: 4.604 min
Delta R.T.: -0.034 min
Response: 64173
Conc: 0.91 ng/ml

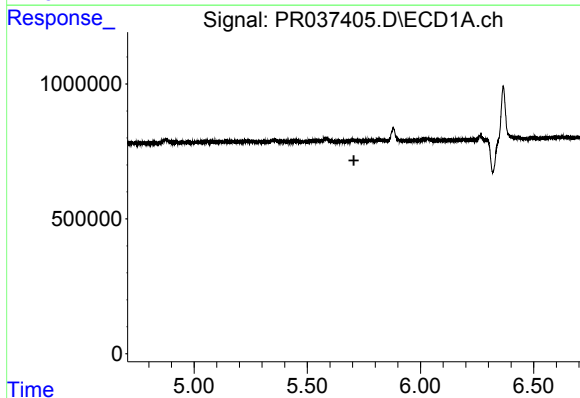


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

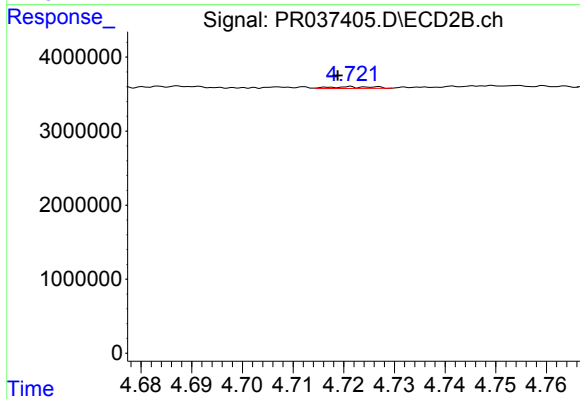

#14 AR-1232-4


R.T.: 4.721 min
Delta R.T.: 0.002 min
Response: 134758
Conc: 2.26 ng/ml

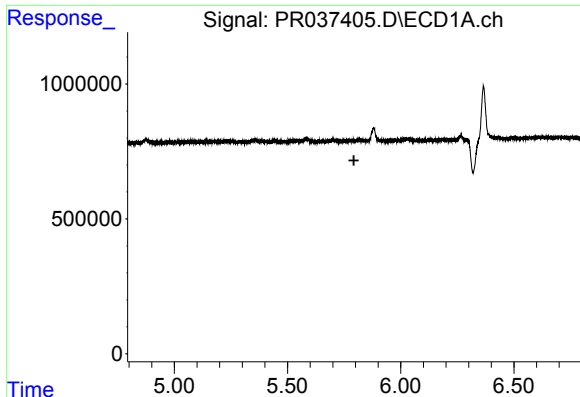

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

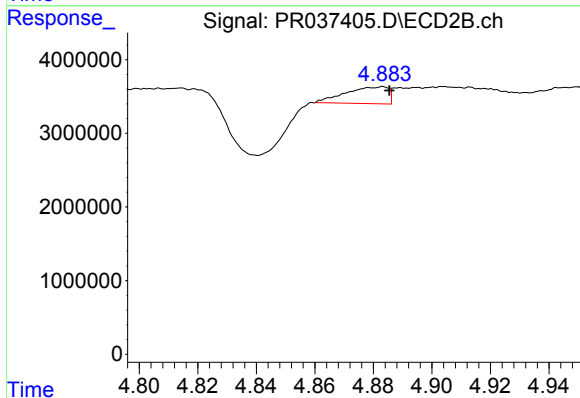


#15 AR-1232-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 2298907
Conc: 33.69 ng/ml

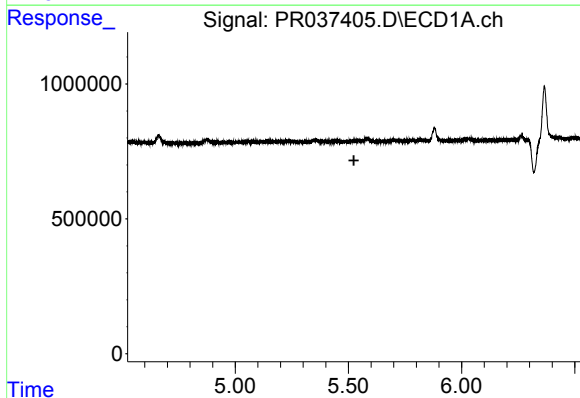


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

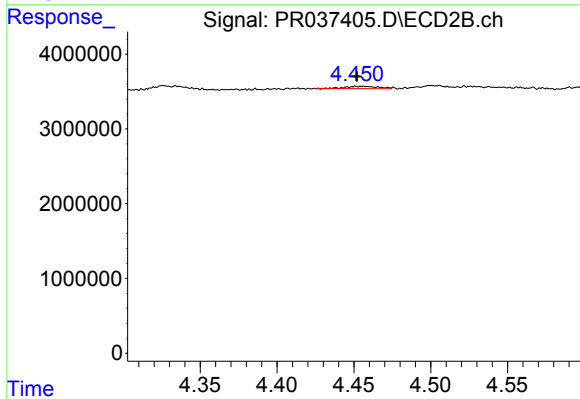

#16 AR-1242-1


R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 433800
Conc: 2.96 ng/ml

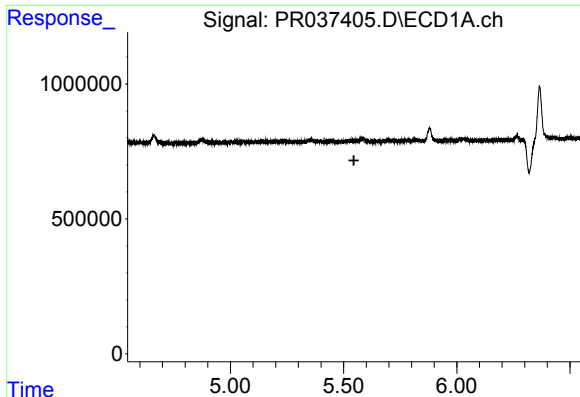

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

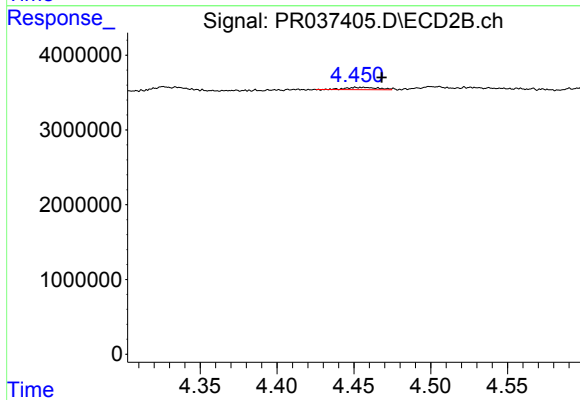


#17 AR-1242-2

R.T.: 4.451 min
Delta R.T.: -0.017 min
Response: 433800
Conc: 1.90 ng/ml

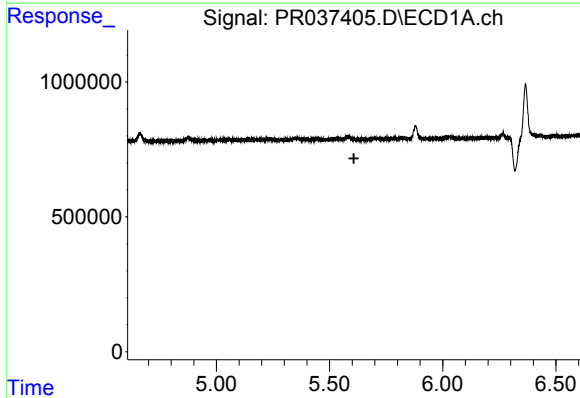


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

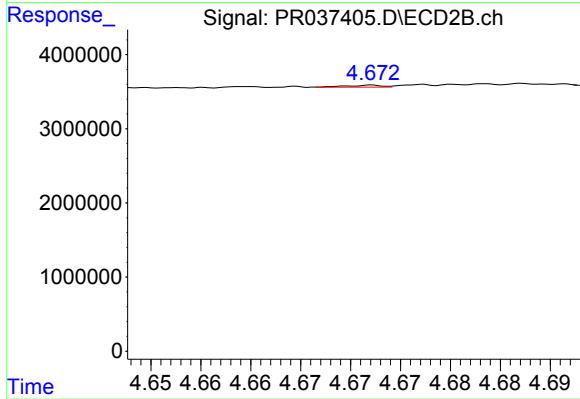

#18 AR-1242-3


R.T.: 4.672 min
Delta R.T.: 0.034 min
Response: 63035
Conc: 0.55 ng/ml

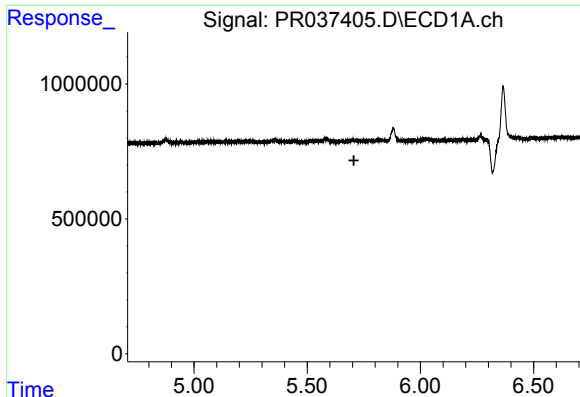

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

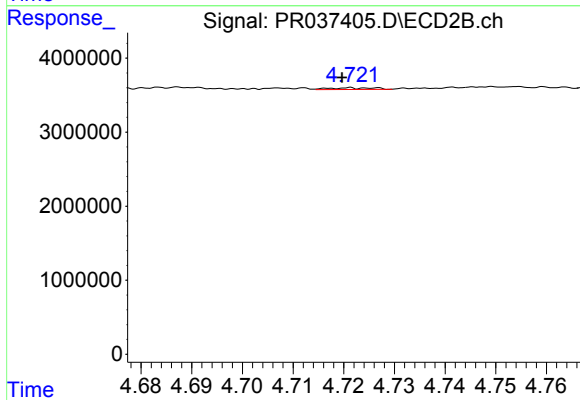


#19 AR-1242-4

R.T.: 4.721 min
Delta R.T.: 0.002 min
Response: 134758
Conc: 1.23 ng/ml

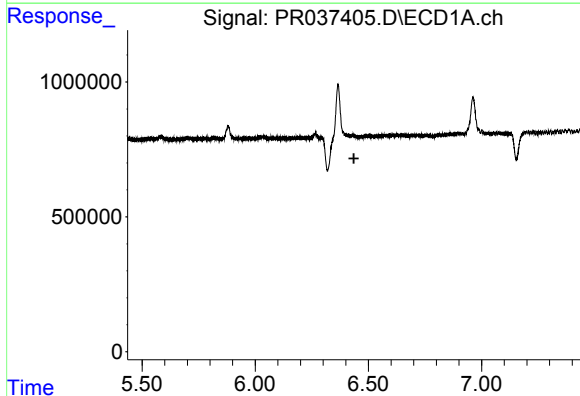


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

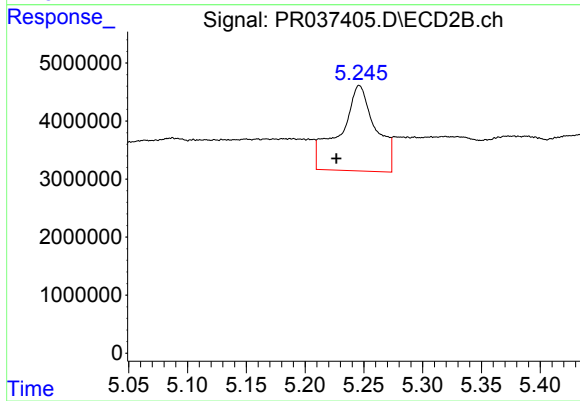

#20 AR-1242-5


R.T.: 5.246 min
Delta R.T.: 0.019 min
Response: 31143892
Conc: 187.95 ng/ml

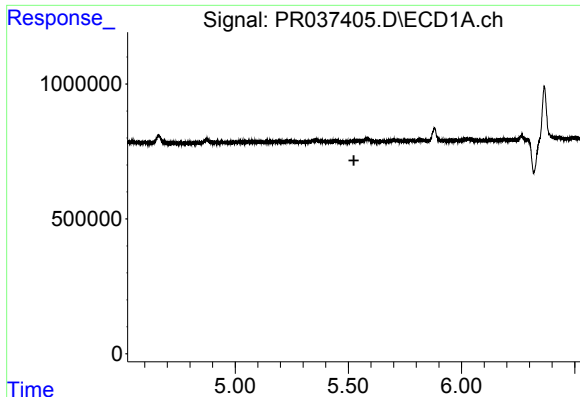

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

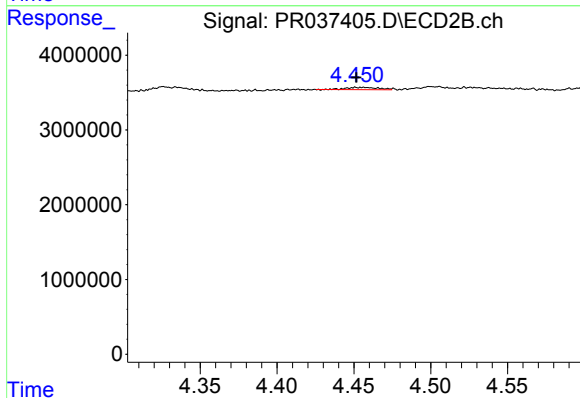


#21 AR-1248-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 433800
Conc: 4.31 ng/ml

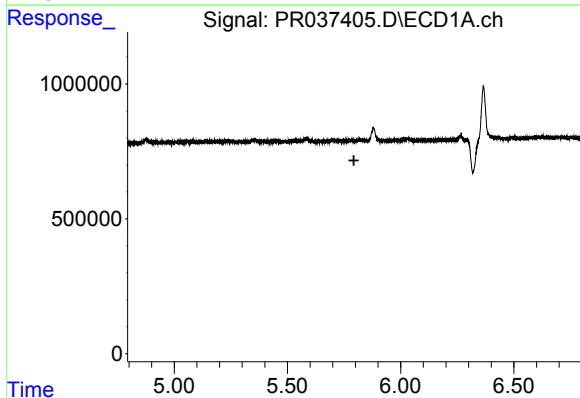


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

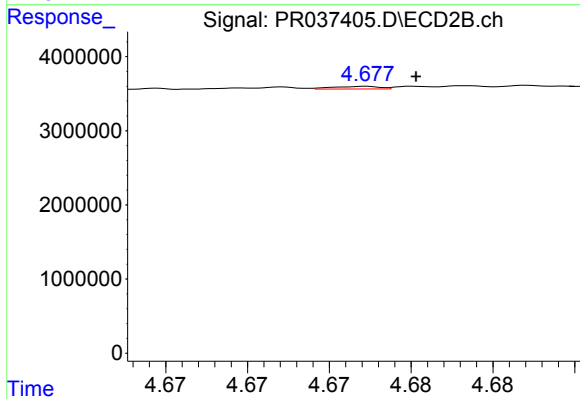

#22 AR-1248-2


R.T.: 4.677 min
Delta R.T.: -0.003 min
Response: 68737
Conc: 0.50 ng/ml

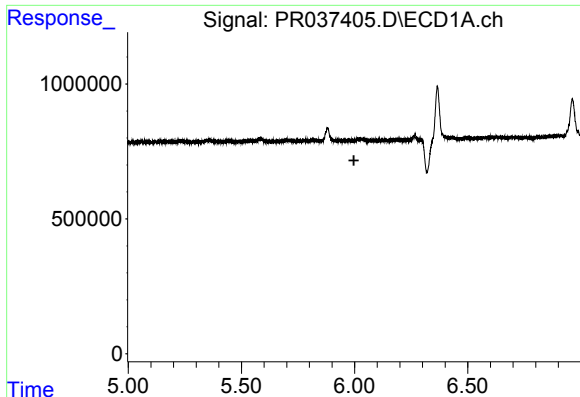

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

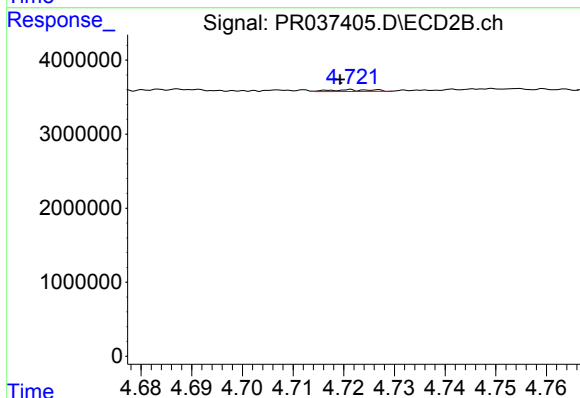


#23 AR-1248-3

R.T.: 4.721 min
Delta R.T.: 0.002 min
Response: 134758
Conc: 0.96 ng/ml

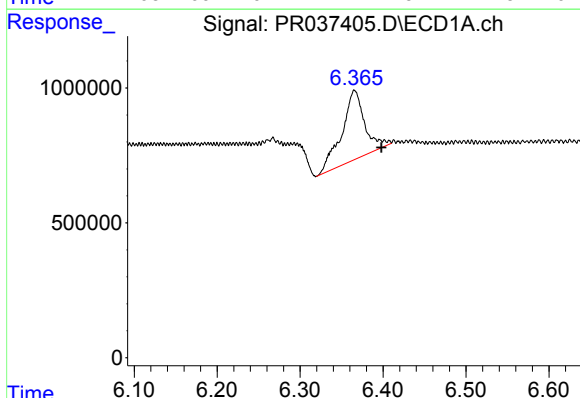


#24 AR-1248-4

R.T.: 6.366 min
Delta R.T.: -0.032 min
Response: 4939697
Conc: 100.90 ng/ml

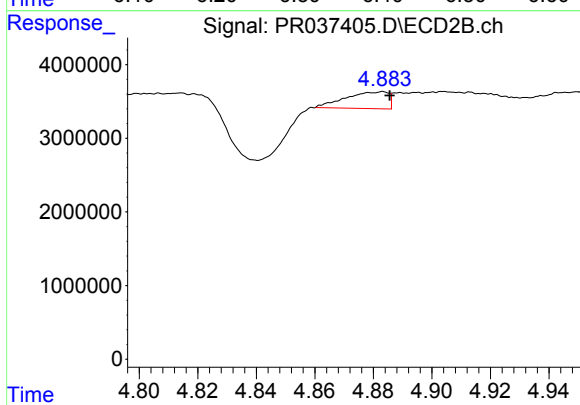

#24 AR-1248-4


R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 2298907
Conc: 12.92 ng/ml

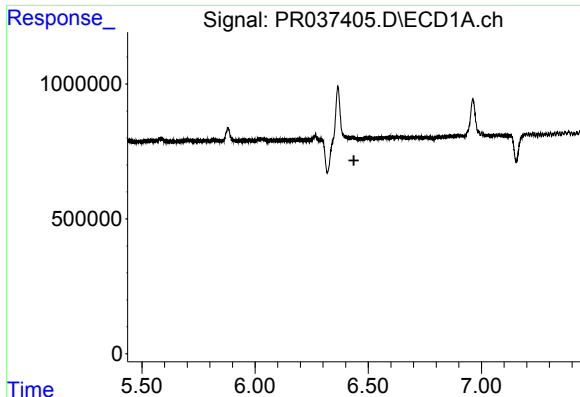

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

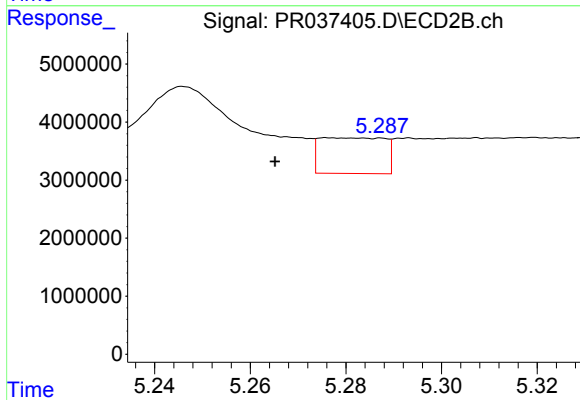


#25 AR-1248-5

R.T.: 5.276 min
Delta R.T.: 0.011 min
Response: 5770350
Conc: 29.50 ng/ml

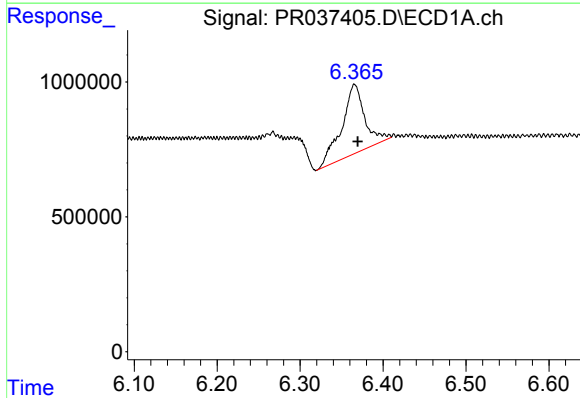


#26 AR-1254-1

R.T.: 6.366 min
Delta R.T.: -0.004 min
Response: 4939697
Conc: 90.42 ng/ml

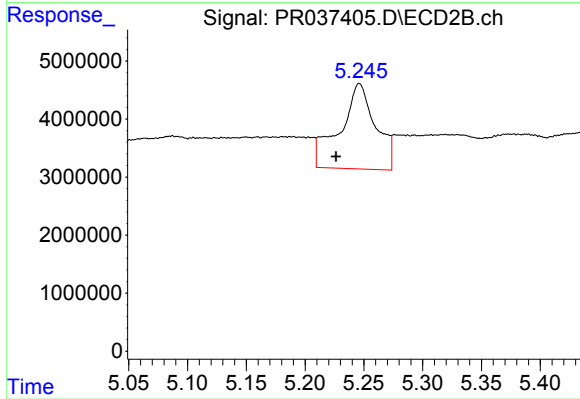

#26 AR-1254-1


R.T.: 5.246 min
Delta R.T.: 0.020 min
Response: 31143892
Conc: 90.41 ng/ml

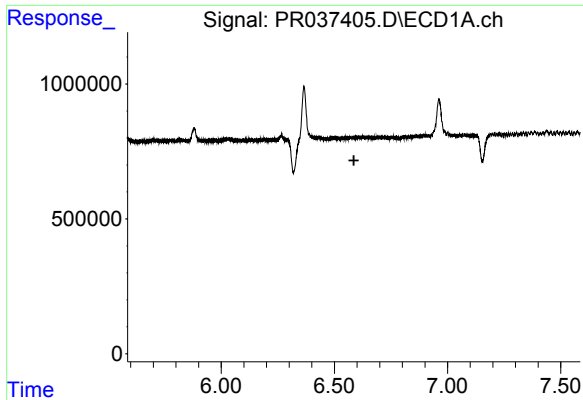

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

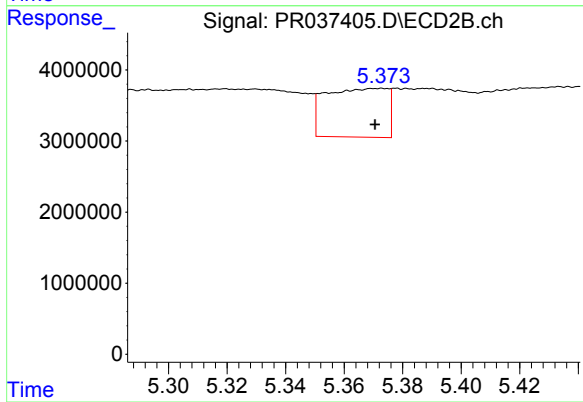


#27 AR-1254-2

R.T.: 5.373 min
Delta R.T.: 0.002 min
Response: 10097694
Conc: 33.71 ng/ml

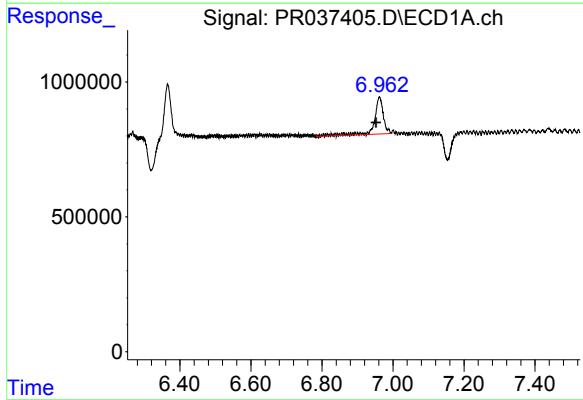


#28 AR-1254-3

R.T.: 6.962 min
Delta R.T.: 0.009 min
Response: 2369207
Conc: 26.05 ng/ml

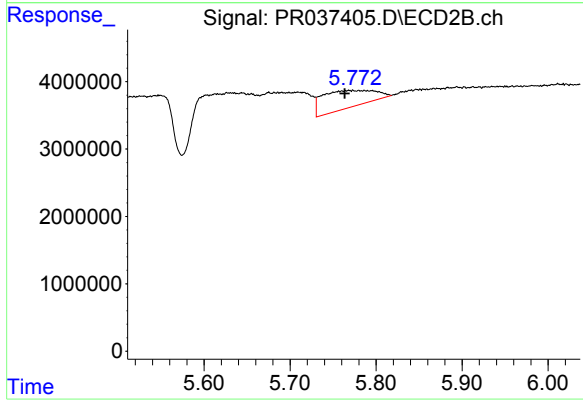

#28 AR-1254-3


R.T.: 5.773 min
Delta R.T.: 0.009 min
Response: 10810045
Conc: 22.82 ng/ml

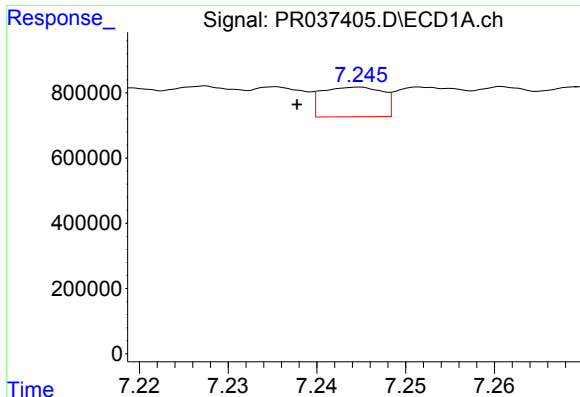

#29 AR-1254-4


R.T.: 7.245 min
Delta R.T.: 0.007 min
Response: 431956
Conc: 6.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

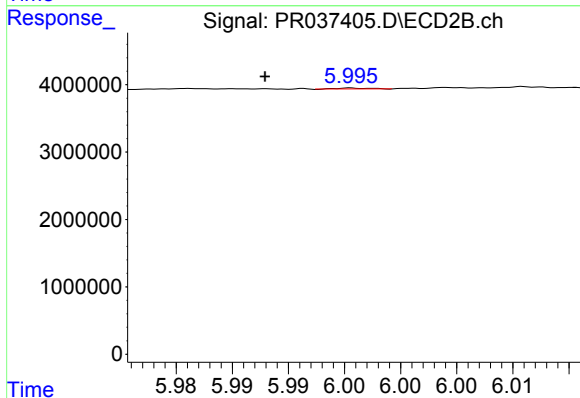


#29 AR-1254-4

R.T.: 5.996 min
Delta R.T.: 0.008 min
Response: 22189
Conc: 0.06 ng/ml

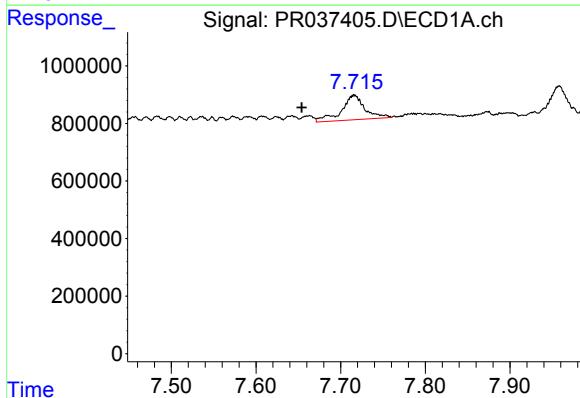


#30 AR-1254-5

R.T.: 7.716 min
Delta R.T.: 0.062 min
Response: 1630099
Conc: 22.68 ng/ml

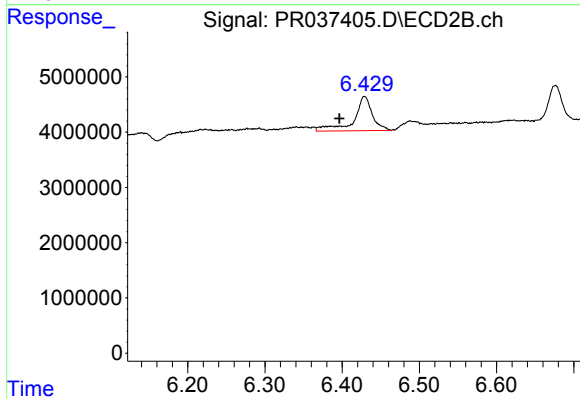

#30 AR-1254-5


R.T.: 6.429 min
Delta R.T.: 0.033 min
Response: 10312600
Conc: 23.29 ng/ml

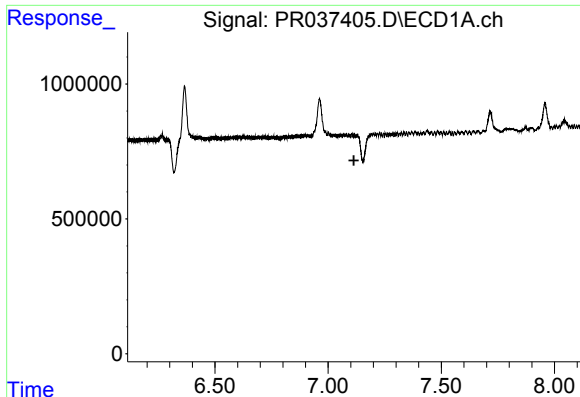

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

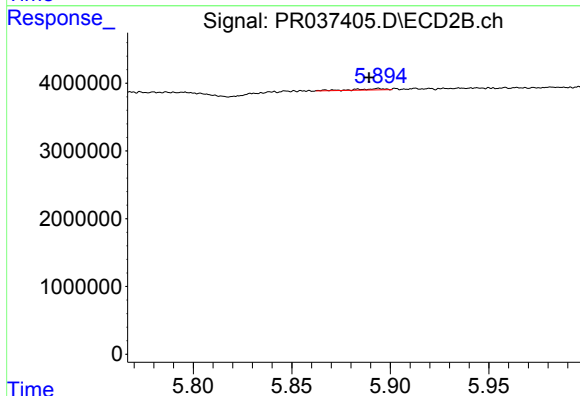


#31 AR-1260-1

R.T.: 5.894 min
Delta R.T.: 0.005 min
Response: 191671
Conc: 0.66 ng/ml

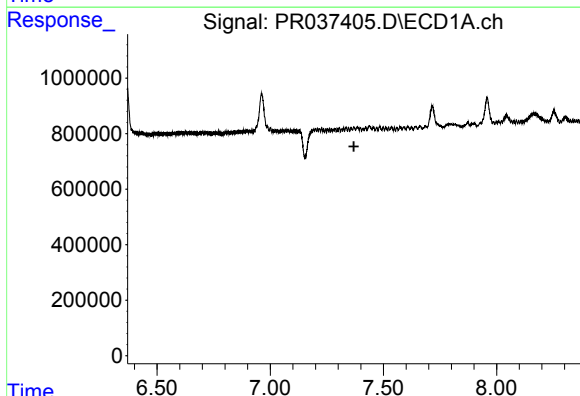


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

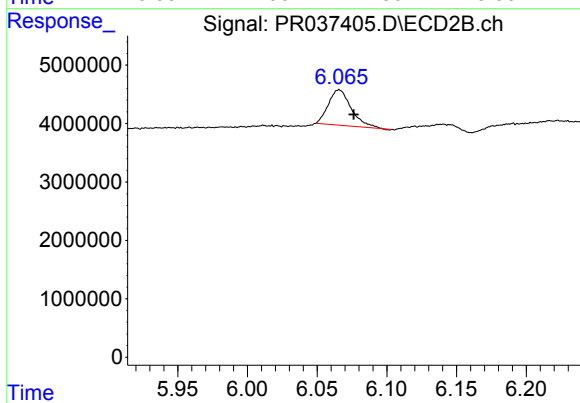

#32 AR-1260-2


R.T.: 6.066 min
Delta R.T.: -0.010 min
Response: 6816257
Conc: 14.80 ng/ml

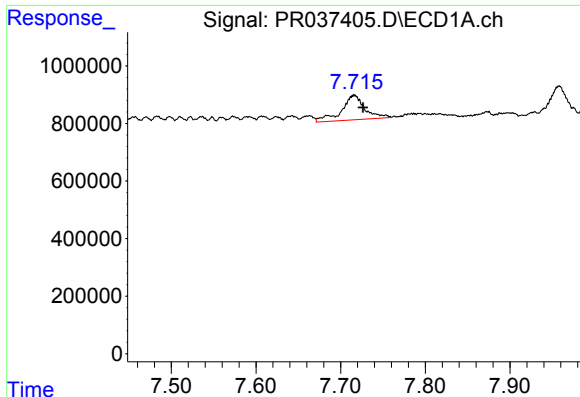

#33 AR-1260-3


R.T.: 7.716 min
Delta R.T.: -0.010 min
Response: 1630099
Conc: 26.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

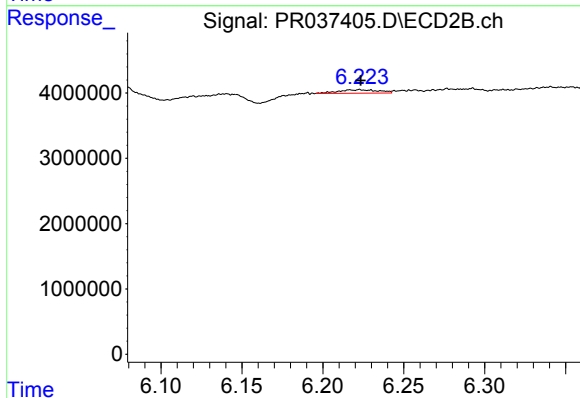


#33 AR-1260-3

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 909920
Conc: 2.55 ng/ml

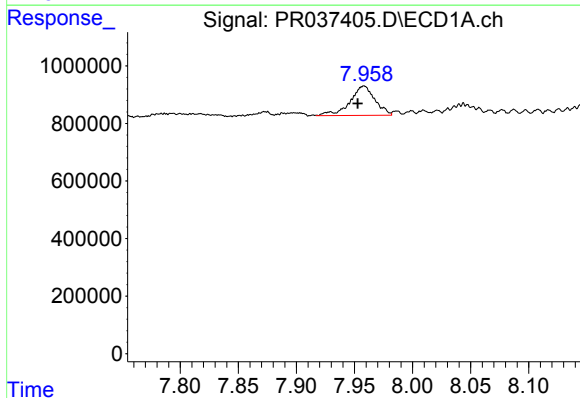


#34 AR-1260-4

R.T.: 7.958 min
Delta R.T.: 0.005 min
Response: 1523127
Conc: 20.47 ng/ml

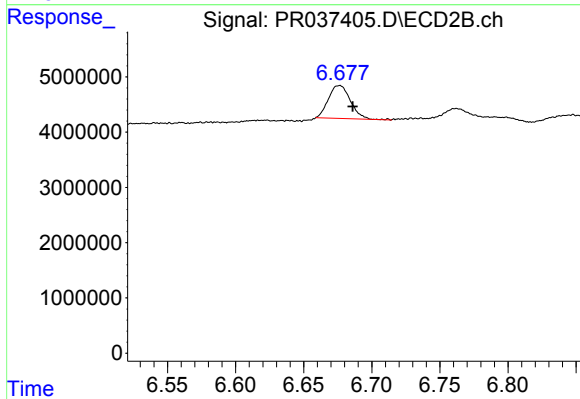

#34 AR-1260-4


R.T.: 6.676 min
Delta R.T.: -0.010 min
Response: 6707620
Conc: 22.01 ng/ml

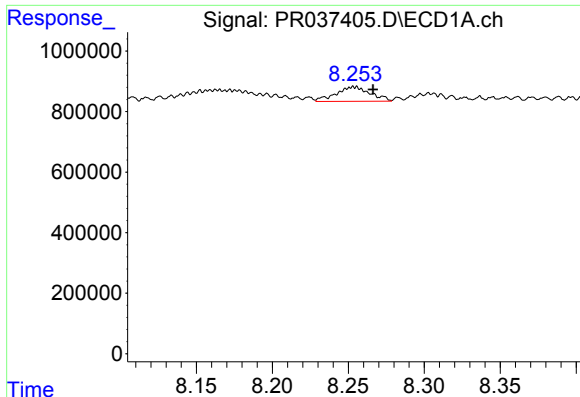

#35 AR-1260-5


R.T.: 8.254 min
Delta R.T.: -0.013 min
Response: 762897
Conc: 5.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

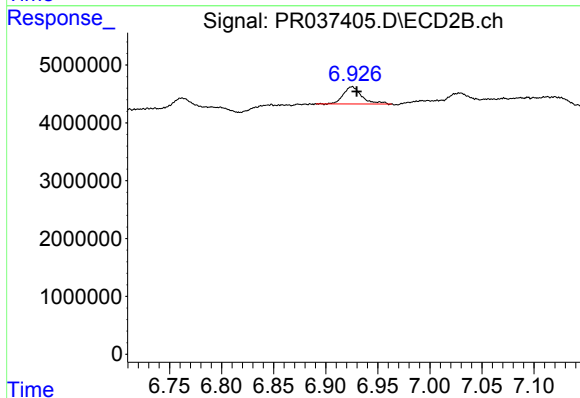


#35 AR-1260-5

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 3623928
Conc: 4.18 ng/ml

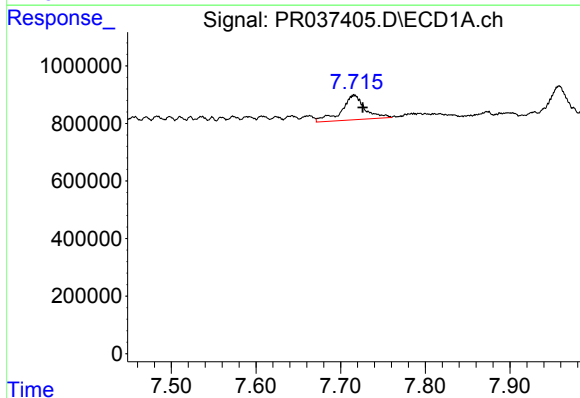


#36 AR-1262-1

R.T.: 7.716 min
Delta R.T.: -0.010 min
Response: 1630099
Conc: 15.61 ng/ml

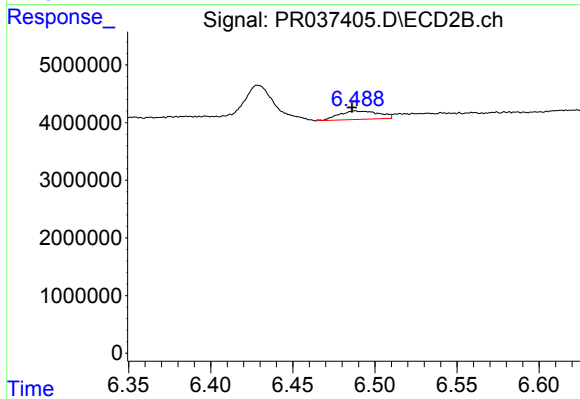

#36 AR-1262-1


R.T.: 6.488 min
Delta R.T.: 0.002 min
Response: 2449893
Conc: 9.78 ng/ml

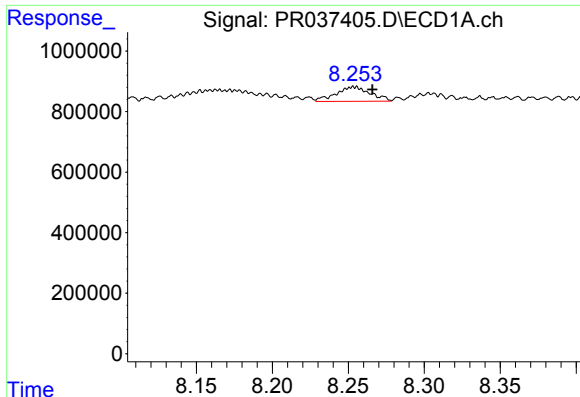

#37 AR-1262-2


R.T.: 8.254 min
Delta R.T.: -0.012 min
Response: 762897
Conc: 3.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

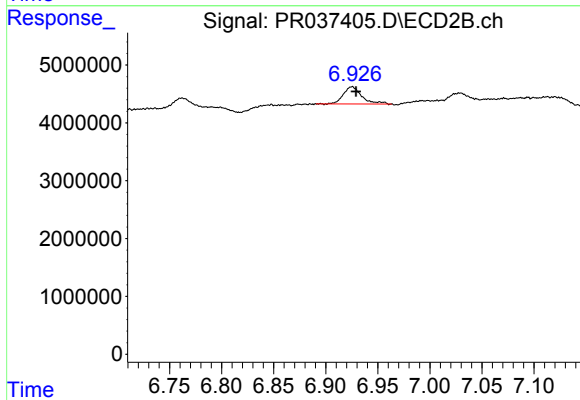


#37 AR-1262-2

R.T.: 6.925 min
Delta R.T.: -0.004 min
Response: 3623928
Conc: 2.89 ng/ml

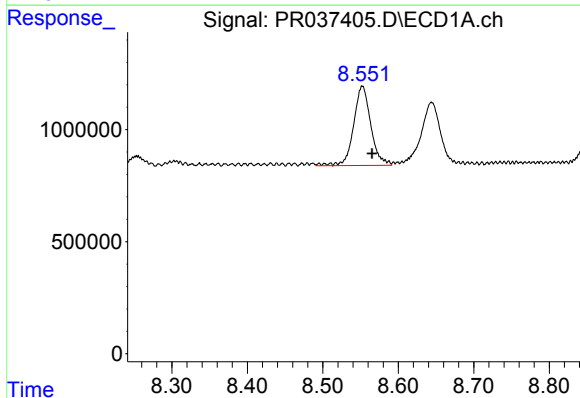


#38 AR-1262-3

R.T.: 8.552 min
Delta R.T.: -0.013 min
Response: 5627199
Conc: 42.79 ng/ml

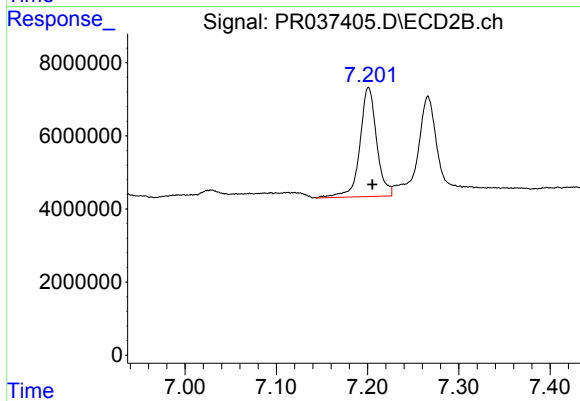

#38 AR-1262-3


R.T.: 7.201 min
Delta R.T.: -0.004 min
Response: 37988058
Conc: 69.29 ng/ml

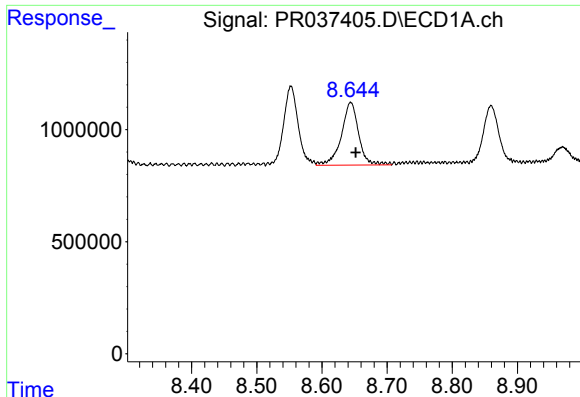

#39 AR-1262-4


R.T.: 8.644 min
Delta R.T.: -0.008 min
Response: 5199787
Conc: 52.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

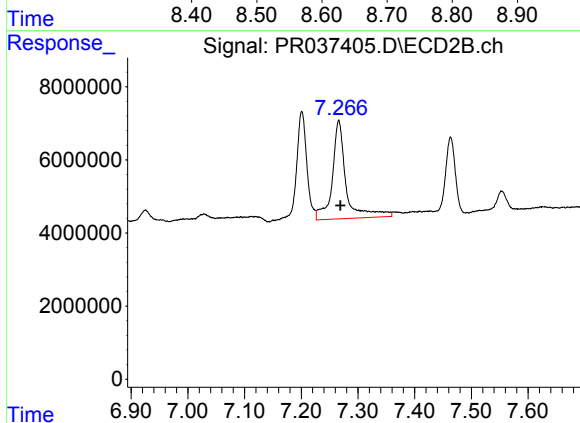


#39 AR-1262-4

R.T.: 7.266 min
Delta R.T.: -0.003 min
Response: 45475763
Conc: 50.66 ng/ml

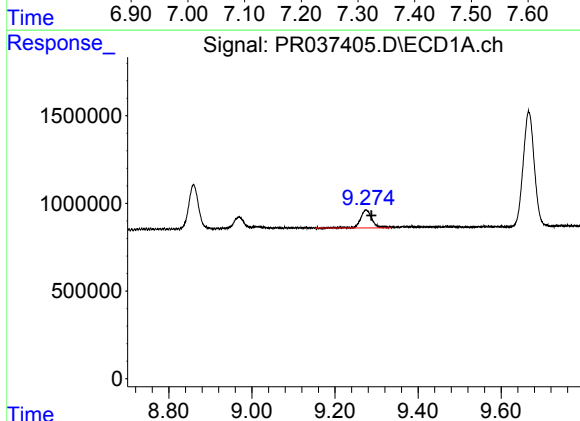


#40 AR-1262-5

R.T.: 9.275 min
Delta R.T.: -0.013 min
Response: 1992995
Conc: 28.87 ng/ml

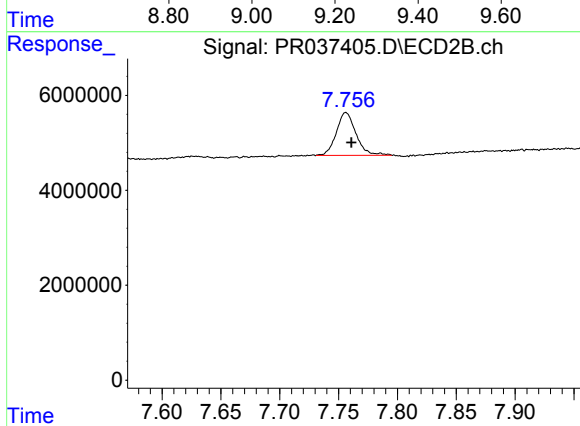

#40 AR-1262-5


R.T.: 7.756 min
Delta R.T.: -0.005 min
Response: 10498861
Conc: 27.44 ng/ml

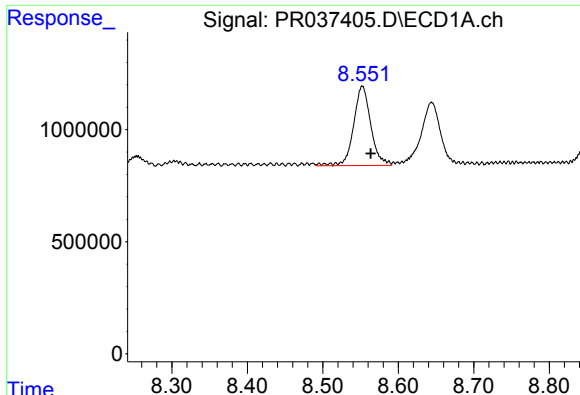

#41 AR-1268-1


R.T.: 8.552 min
Delta R.T.: -0.011 min
Response: 5627199
Conc: 31.42 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

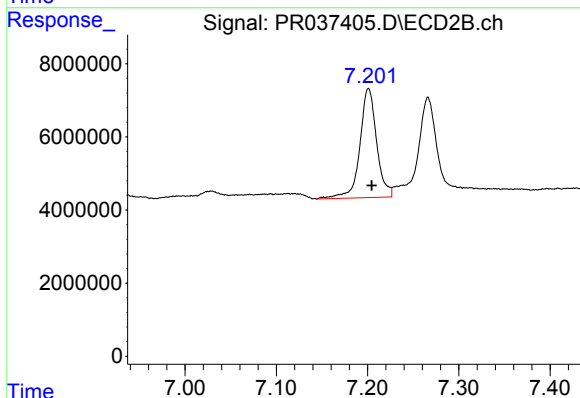


#41 AR-1268-1

R.T.: 7.201 min
Delta R.T.: -0.004 min
Response: 37988058
Conc: 30.86 ng/ml

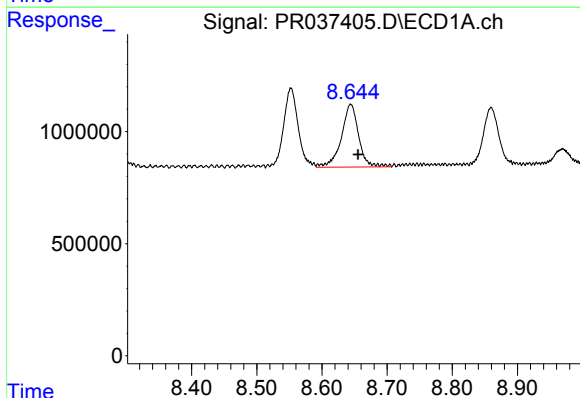


#42 AR-1268-2

R.T.: 8.644 min
Delta R.T.: -0.011 min
Response: 5199787
Conc: 31.61 ng/ml

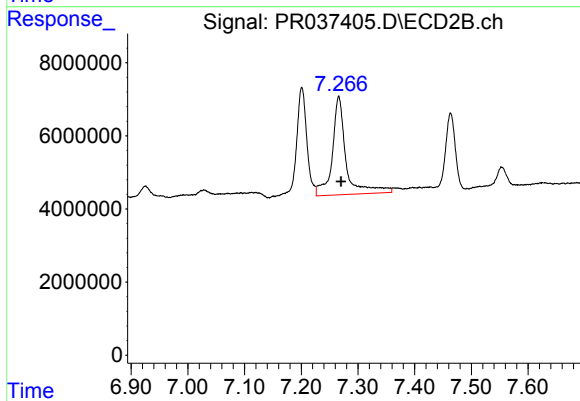

#42 AR-1268-2


R.T.: 7.266 min
Delta R.T.: -0.004 min
Response: 45475763
Conc: 42.95 ng/ml

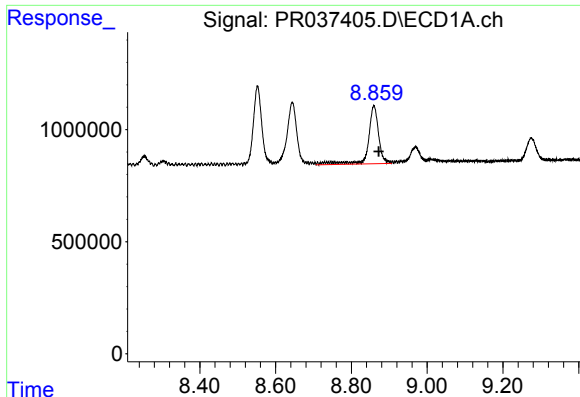

#43 AR-1268-3


R.T.: 8.860 min
Delta R.T.: -0.013 min
Response: 4913465
Conc: 35.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

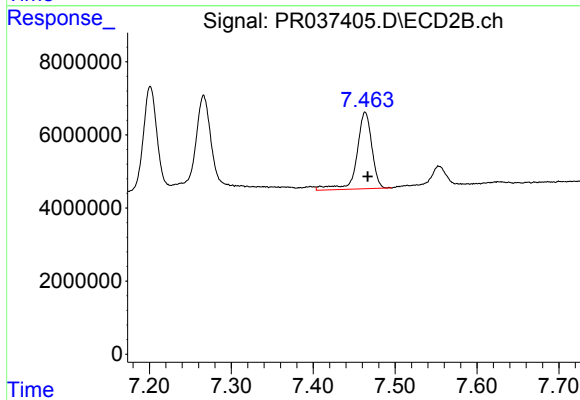


#43 AR-1268-3

R.T.: 7.463 min
Delta R.T.: -0.003 min
Response: 26770888
Conc: 30.21 ng/ml

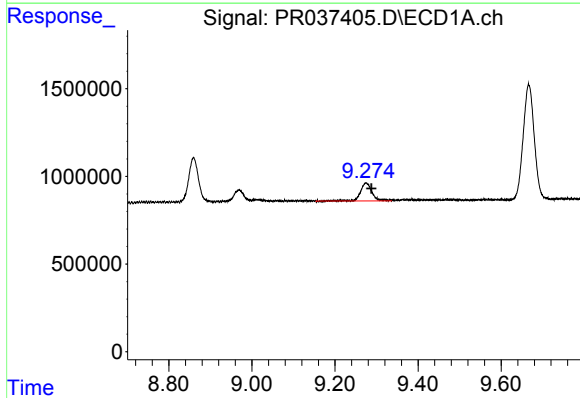


#44 AR-1268-4

R.T.: 9.275 min
Delta R.T.: -0.013 min
Response: 1992995
Conc: 31.95 ng/ml

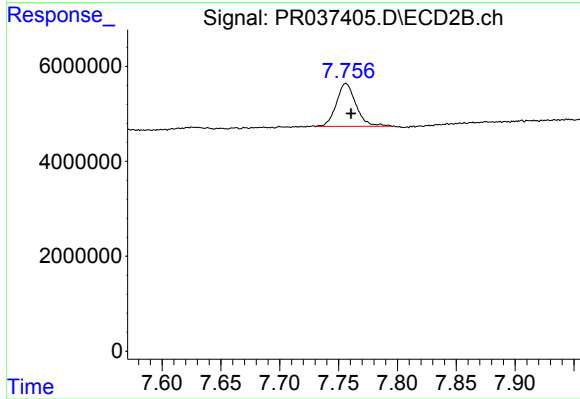

#44 AR-1268-4


R.T.: 7.756 min
Delta R.T.: -0.004 min
Response: 10498861
Conc: 28.94 ng/ml

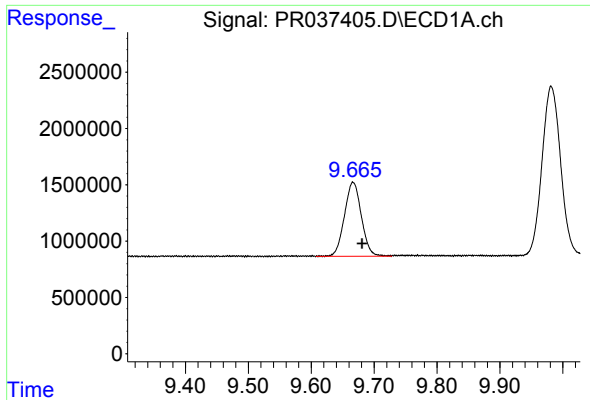

#45 AR-1268-5

R.T.: 9.666 min
Delta R.T.: -0.014 min
Response: 12285851
Conc: 26.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

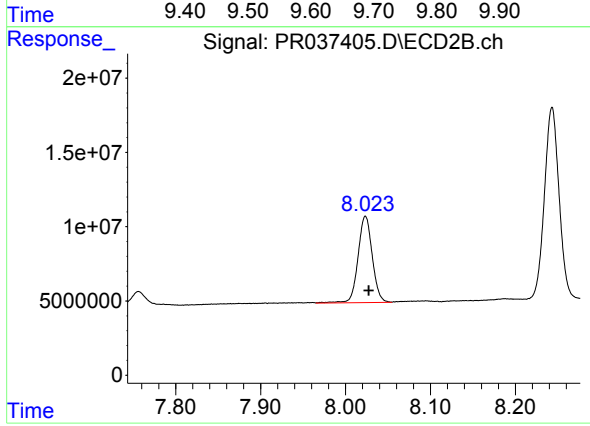

#45 AR-1268-5

R.T.: 8.024 min
Delta R.T.: -0.004 min
Response: 67713196
Conc: 26.61 ng/ml