

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051719\
 Data File : PR038013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2019 11:50
 Operator : SM\MA
 Sample : K2848-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 FK-GF-02-040-B

Manual Integrations
 APPROVED

Ankita
 5/20/2019 4:05:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 12:15:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun May 12 00:51:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.780	4.627	46643346	138.8E6	25.883	27.532
2) SA Decachlor...	8.768	10.387	23583259	64688763	12.361m	14.223
Target Compounds						
31) L7 AR-1260-1	6.321	7.369	27573861	66265925	229.766	267.755
32) L7 AR-1260-2	6.505	7.619	33399431	180.8E6	213.067	614.574 #
33) L7 AR-1260-3	6.660	7.978	22548011	49477571	170.551	226.614 #
34) L7 AR-1260-4	7.129	8.207	15939180	53520362	149.597	209.456 #
35) L7 AR-1260-5	7.368	8.535	40226111	99004024	143.188	190.572 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051719\
Data File : PR038013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2019 11:50
Operator : SM\MA
Sample : K2848-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
FK-GF-02-040-B


Manual Integrations
APPROVED

Ankita
5/20/2019 4:05:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 12:15:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun May 12 00:51:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

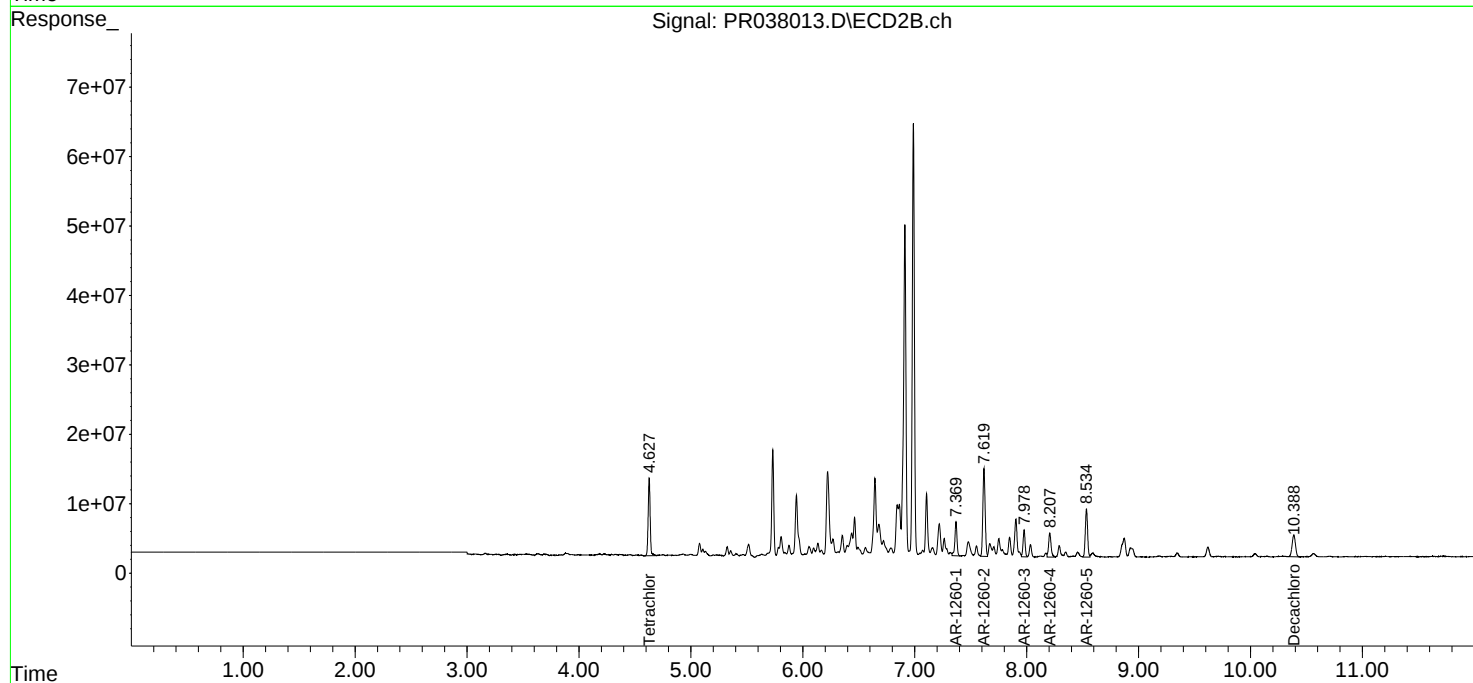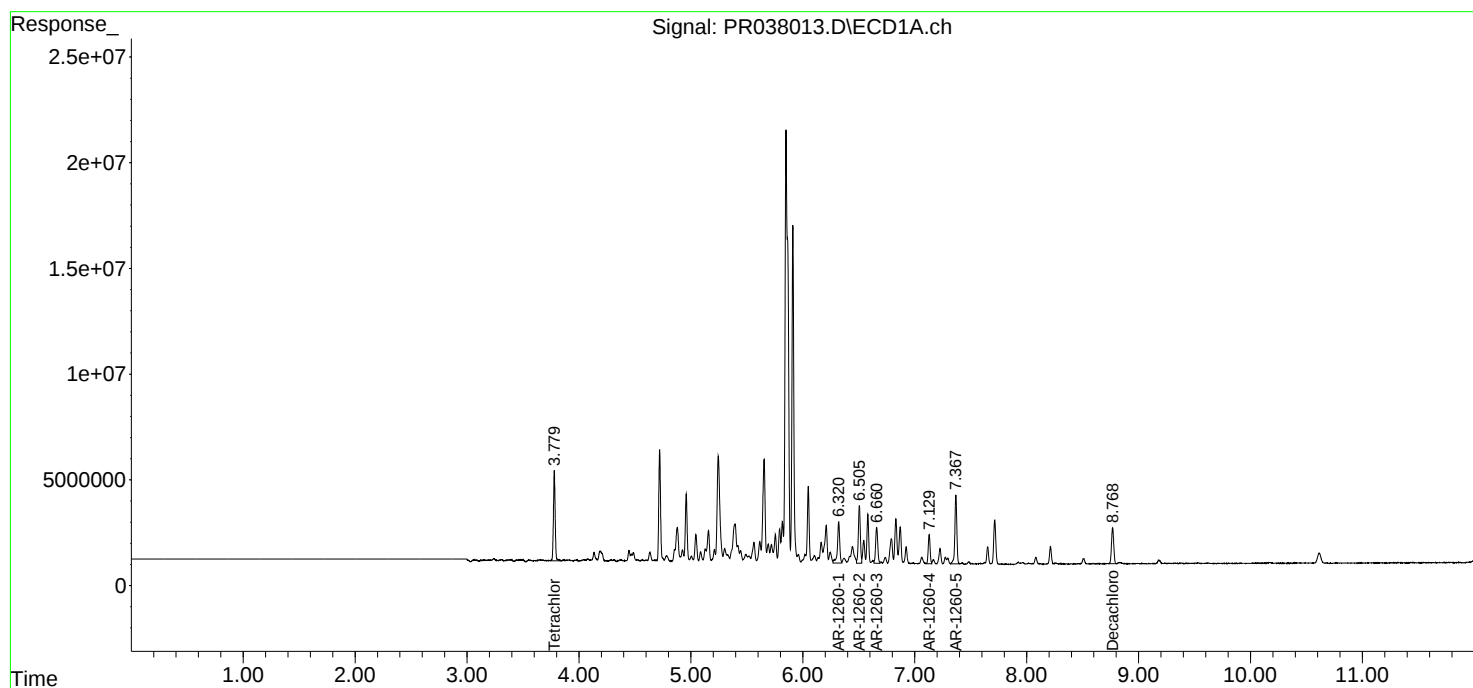

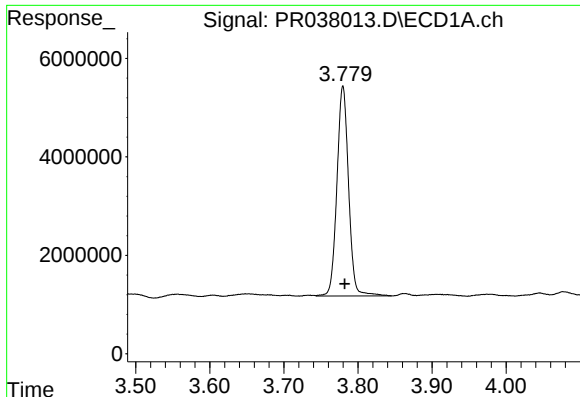


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 46643346
Conc: 25.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-GF-02-040-B


Manual Integrations
APPROVED

Ankita
5/20/2019 4:05:33 PM

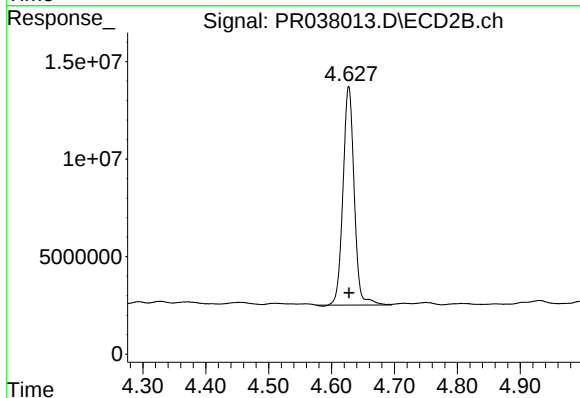


#1 Tetrachloro-m-xylene

R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 138839566
Conc: 27.53 ng/ml

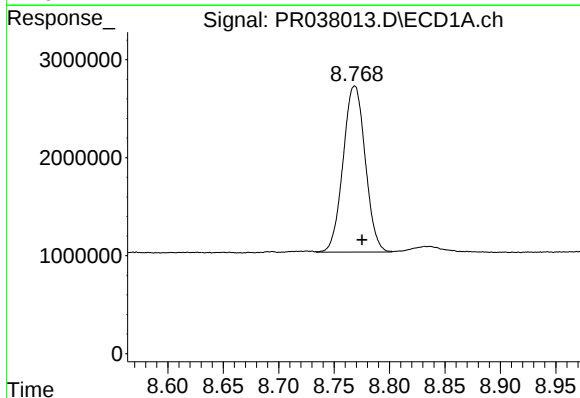


#2 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.007 min
Response: 23583259
Conc: 12.36 ng/ml m

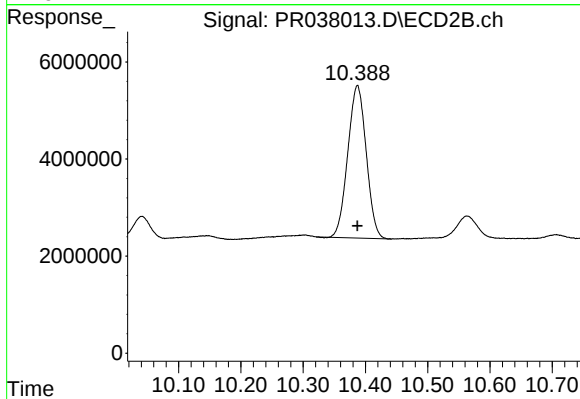

#2 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.000 min
Response: 64688763
Conc: 14.22 ng/ml

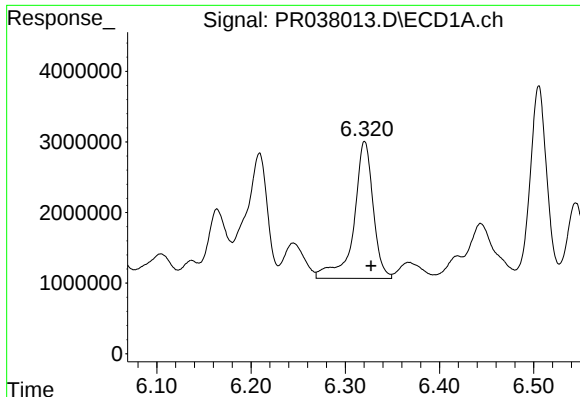


#31 AR-1260-1

R.T.: 6.321 min
Delta R.T.: -0.007 min
Response: 27573861
Conc: 229.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-GF-02-040-B


Manual Integrations
APPROVED

Ankita
5/20/2019 4:05:33 PM

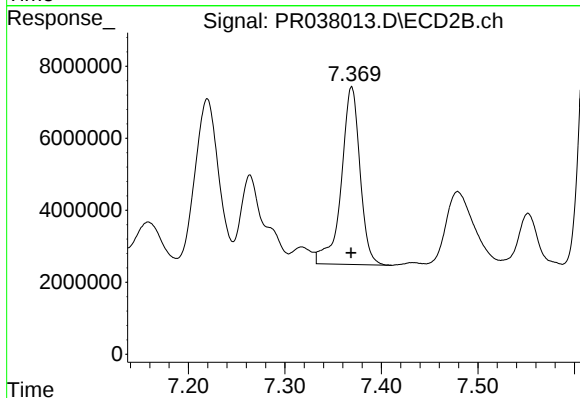


#31 AR-1260-1

R.T.: 7.369 min
Delta R.T.: 0.000 min
Response: 66265925
Conc: 267.75 ng/ml

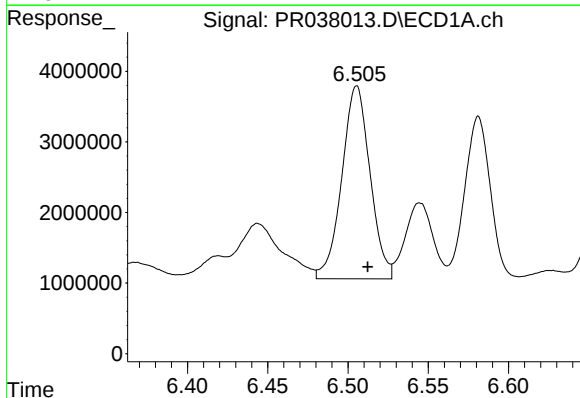


#32 AR-1260-2

R.T.: 6.505 min
Delta R.T.: -0.007 min
Response: 33399431
Conc: 213.07 ng/ml

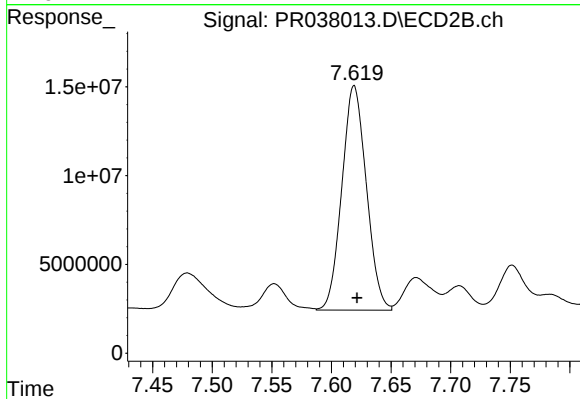

#32 AR-1260-2

R.T.: 7.619 min
Delta R.T.: -0.002 min
Response: 180768594
Conc: 614.57 ng/ml

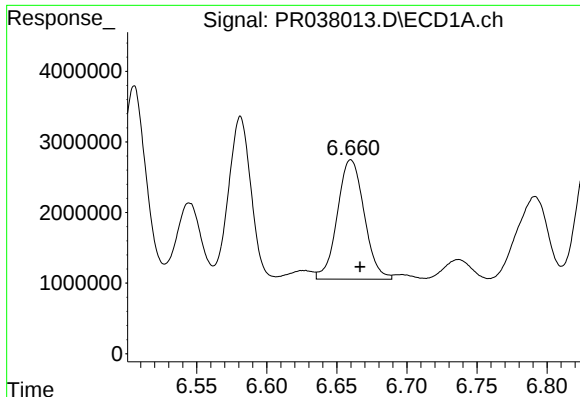


#33 AR-1260-3

R.T.: 6.660 min
Delta R.T.: -0.006 min
Response: 22548011
Conc: 170.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-GF-02-040-B


Manual Integrations
APPROVED

Ankita
5/20/2019 4:05:33 PM

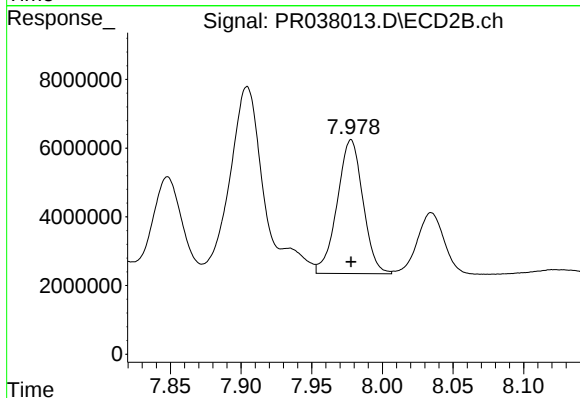


#33 AR-1260-3

R.T.: 7.978 min
Delta R.T.: 0.000 min
Response: 49477571
Conc: 226.61 ng/ml

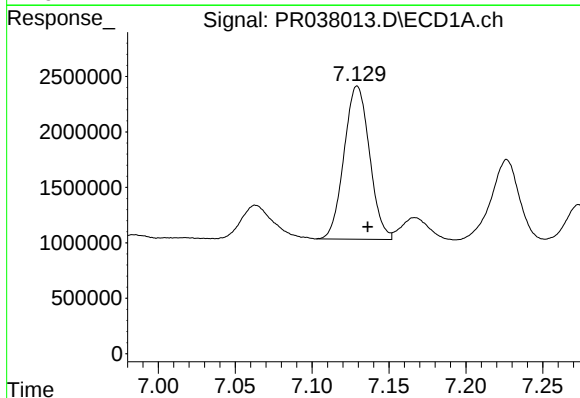


#34 AR-1260-4

R.T.: 7.129 min
Delta R.T.: -0.007 min
Response: 15939180
Conc: 149.60 ng/ml

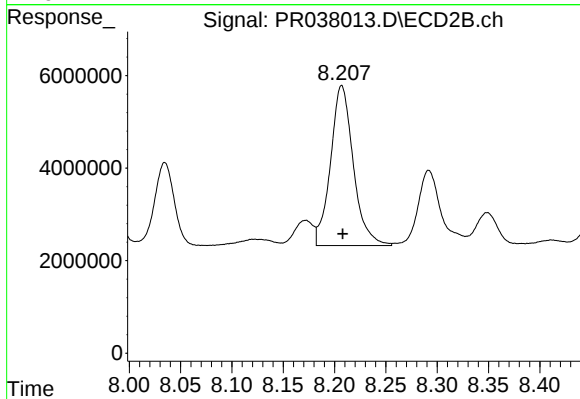

#34 AR-1260-4

R.T.: 8.207 min
Delta R.T.: -0.001 min
Response: 53520362
Conc: 209.46 ng/ml

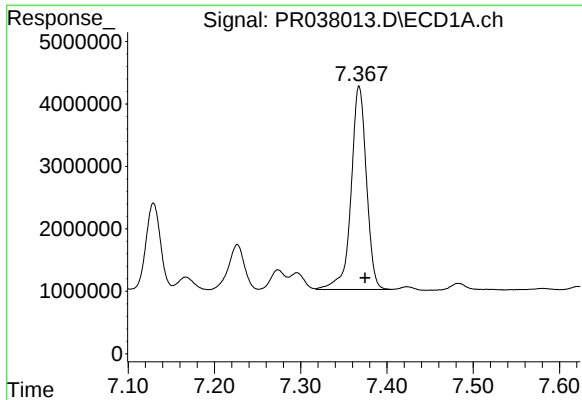


#35 AR-1260-5

R.T.: 7.368 min
Delta R.T.: -0.007 min
Response: 40226111
Conc: 143.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-GF-02-040-B

Manual Integrations
APPROVED

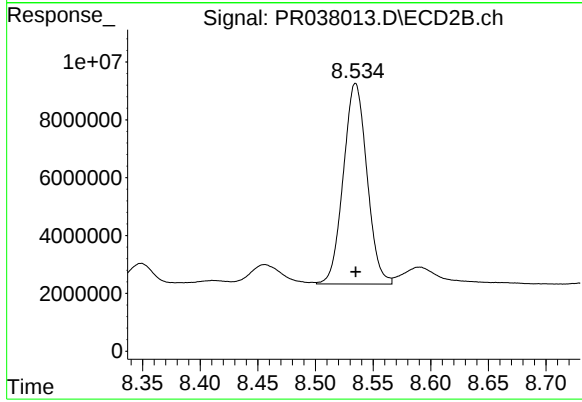

#35 AR-1260-5

R.T.: 8.535 min
Delta R.T.: 0.000 min
Response: 99004024
Conc: 190.57 ng/ml

Ankita
5/20/2019 4:05:33 PM