

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051719\
 Data File : PR038051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2019 01:14
 Operator : SM\MA
 Sample : K2866-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 RO-COMP-2

Manual Integrations
 APPROVED

Ankita
 5/20/2019 4:06:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 02:58:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun May 12 00:51:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.782	4.628	22980667	73630422	12.752	14.601
2) SA Decachlor...	8.762	10.382	31215155	79871211	16.361	17.561
Target Compounds						
31) L7 AR-1260-1	6.320	7.367	42025290	112.2E6	350.186	453.349 #
32) L7 AR-1260-2	6.505	7.619	55278169	158.0E6	352.640	537.277 #
33) L7 AR-1260-3	6.658	7.974	53279392	93657430	403.001	428.963
34) L7 AR-1260-4	7.128	8.199	32283666	179.7E6	302.998	703.299m#
35) L7 AR-1260-5	7.366	8.531	118.7E6	252.5E6	422.616	485.971

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051719\
Data File : PR038051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2019 01:14
Operator : SM\MA
Sample : K2866-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
RO-COMP-2


Manual Integrations
APPROVED

Ankita
5/20/2019 4:06:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 02:58:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun May 12 00:51:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

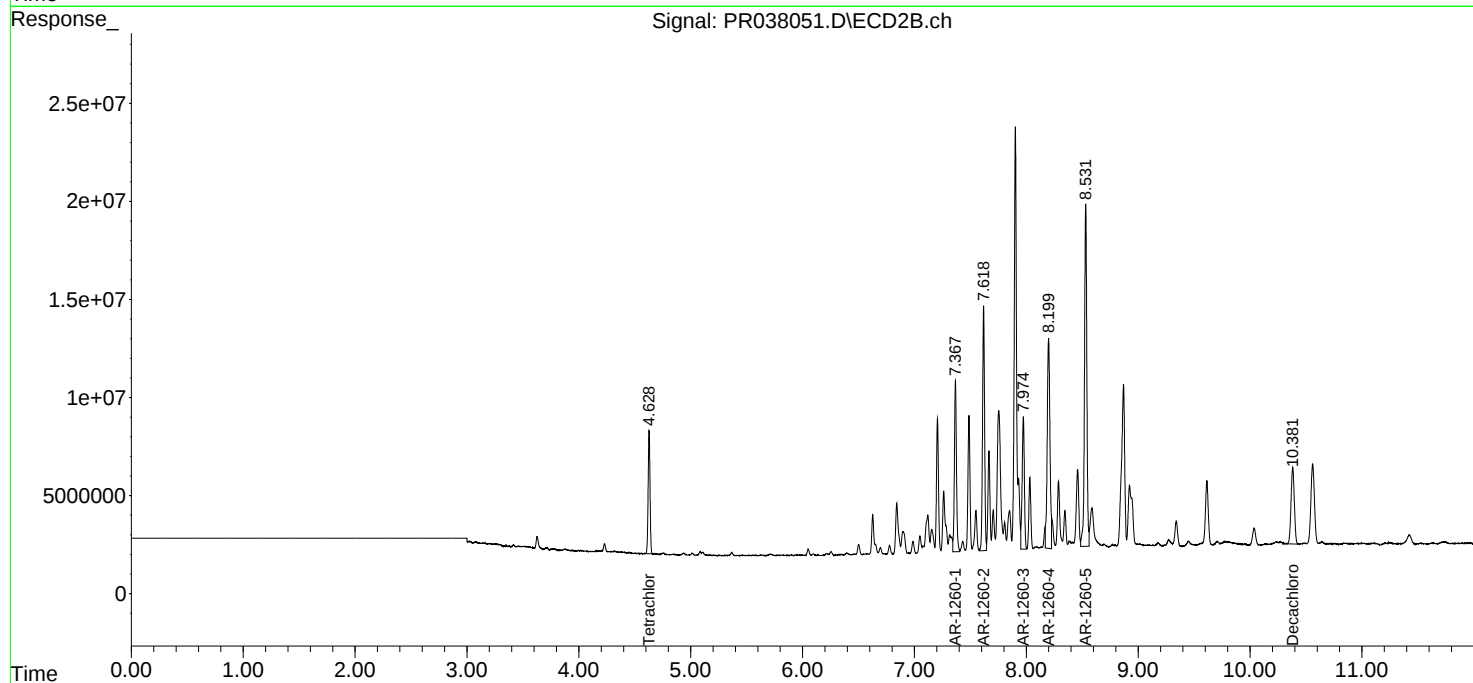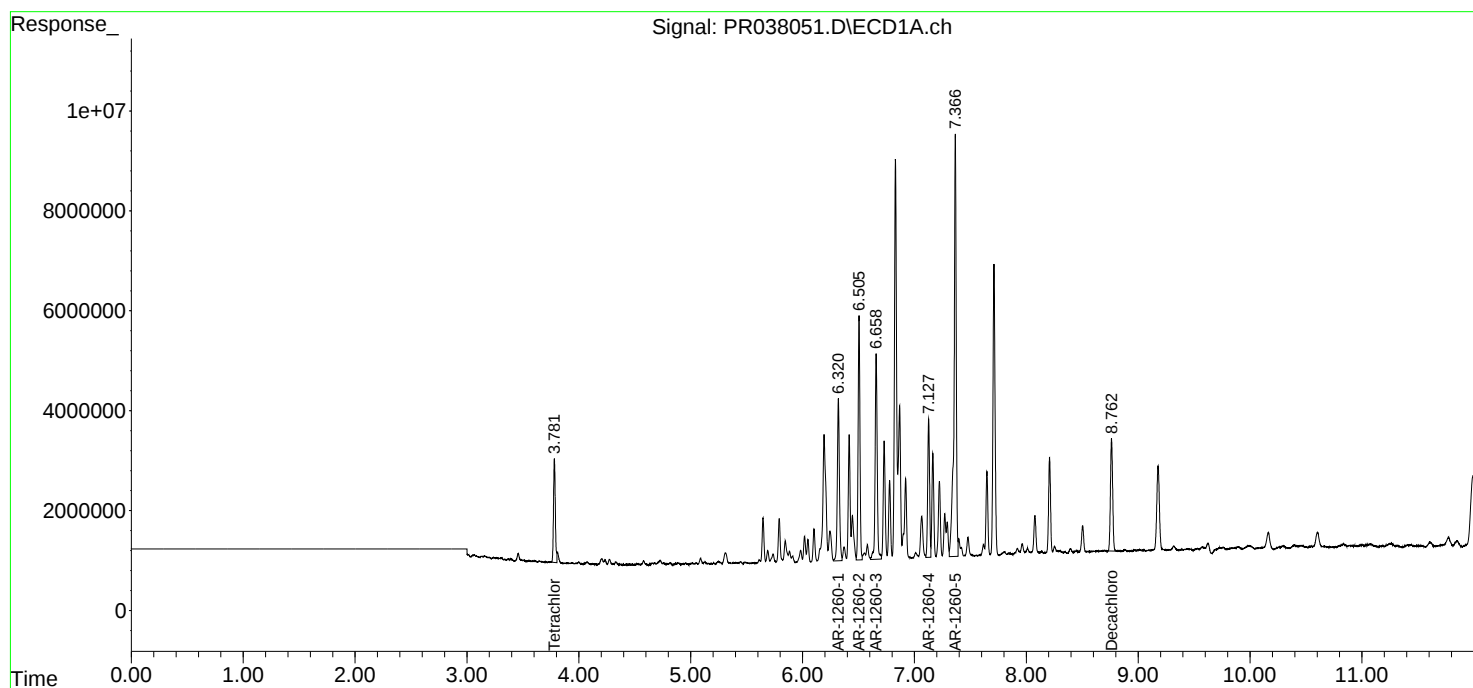

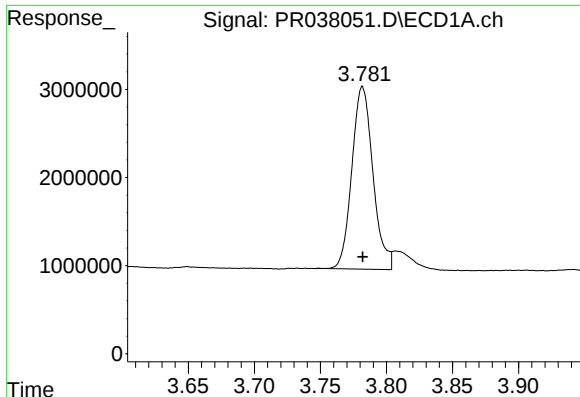


#1 Tetrachloro-m-xylene

R.T.: 3.782 min
Delta R.T.: 0.000 min
Response: 22980667
Conc: 12.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
RO-COMP-2


Manual Integrations
APPROVED

Ankita
5/20/2019 4:06:08 PM

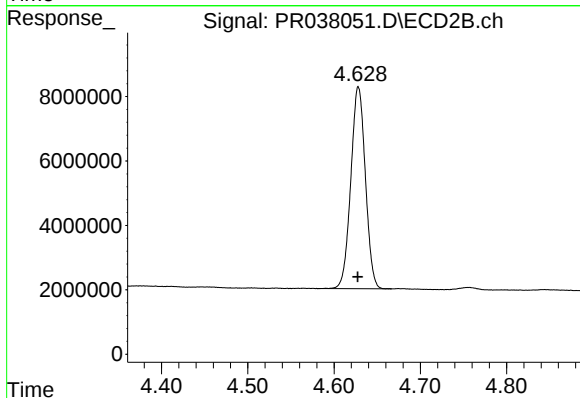


#1 Tetrachloro-m-xylene

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 73630422
Conc: 14.60 ng/ml

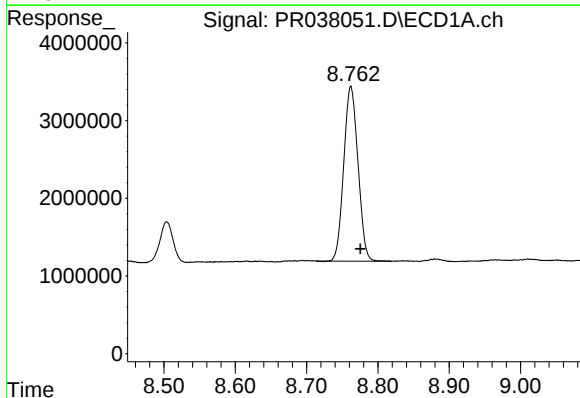


#2 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: -0.013 min
Response: 31215155
Conc: 16.36 ng/ml

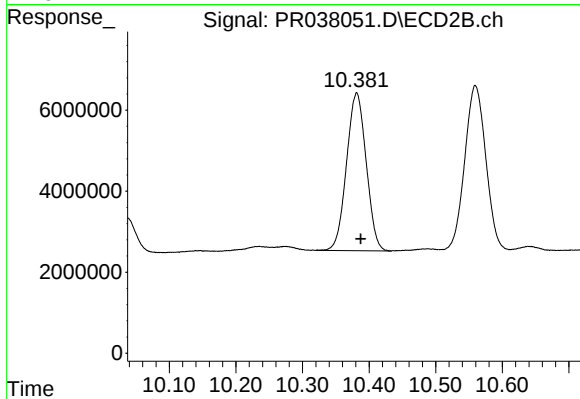

#2 Decachlorobiphenyl

R.T.: 10.382 min
Delta R.T.: -0.006 min
Response: 79871211
Conc: 17.56 ng/ml

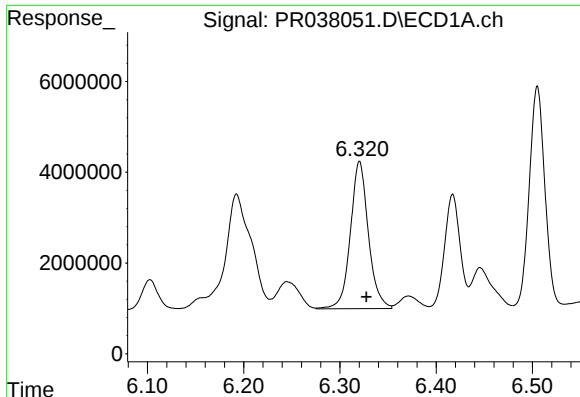


#31 AR-1260-1

R.T.: 6.320 min
Delta R.T.: -0.007 min
Response: 42025290
Conc: 350.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
RO-COMP-2


Manual Integrations
APPROVED

Ankita
5/20/2019 4:06:08 PM

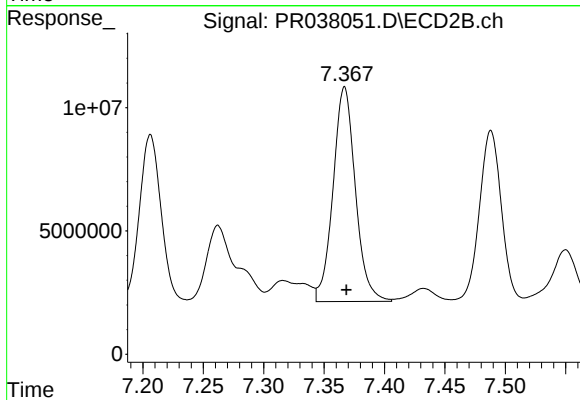


#31 AR-1260-1

R.T.: 7.367 min
Delta R.T.: -0.002 min
Response: 112198253
Conc: 453.35 ng/ml

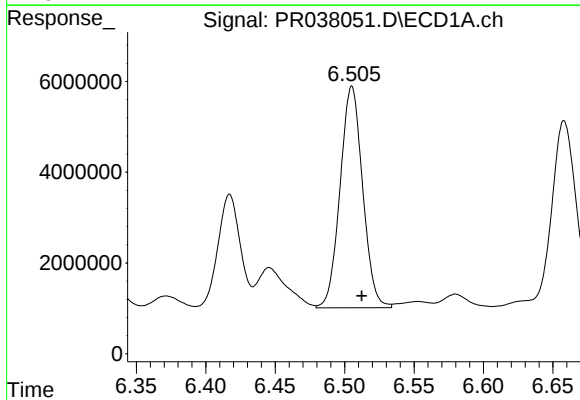


#32 AR-1260-2

R.T.: 6.505 min
Delta R.T.: -0.007 min
Response: 55278169
Conc: 352.64 ng/ml

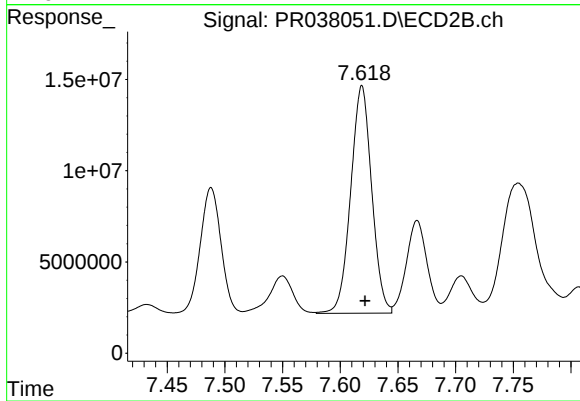

#32 AR-1260-2

R.T.: 7.619 min
Delta R.T.: -0.003 min
Response: 158032815
Conc: 537.28 ng/ml

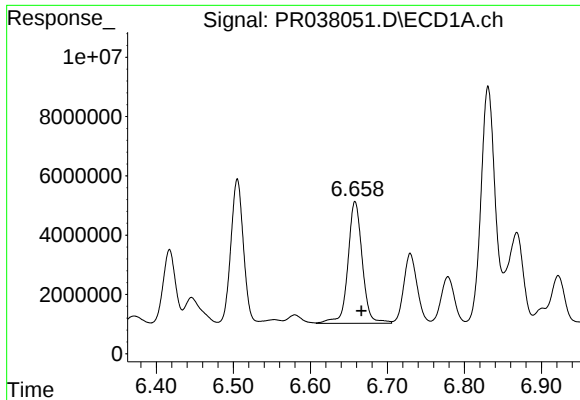


#33 AR-1260-3

R.T.: 6.658 min
Delta R.T.: -0.008 min
Response: 53279392
Conc: 403.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
RO-COMP-2


Manual Integrations
APPROVED

Ankita
5/20/2019 4:06:08 PM

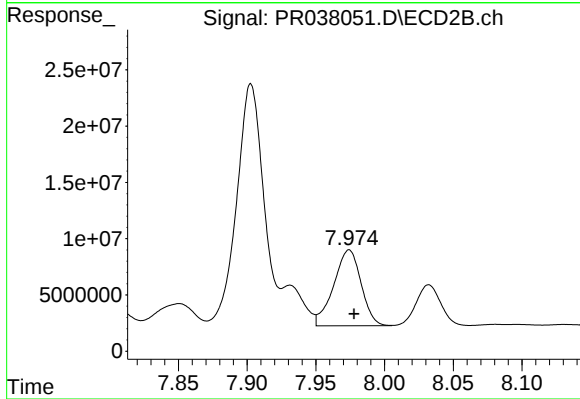


#33 AR-1260-3

R.T.: 7.974 min
Delta R.T.: -0.004 min
Response: 93657430
Conc: 428.96 ng/ml

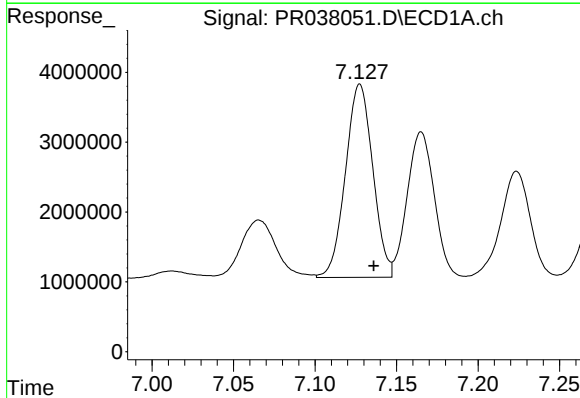


#34 AR-1260-4

R.T.: 7.128 min
Delta R.T.: -0.009 min
Response: 32283666
Conc: 303.00 ng/ml

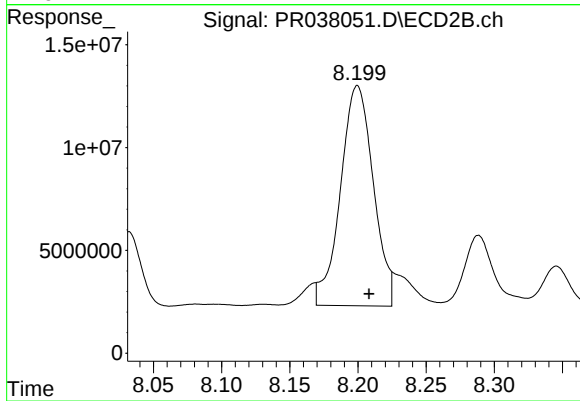

#34 AR-1260-4

R.T.: 8.199 min
Delta R.T.: -0.009 min
Response: 179707307
Conc: 703.30 ng/ml m

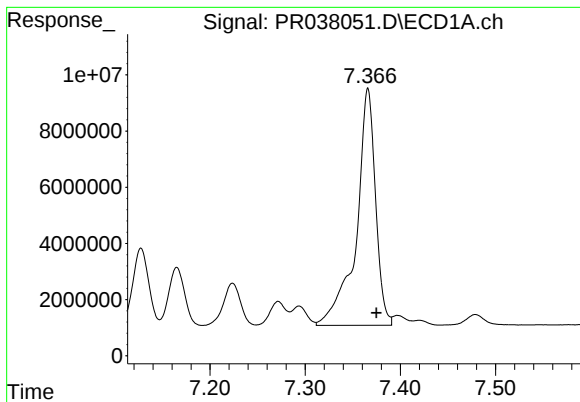


#35 AR-1260-5

R.T.: 7.366 min
Delta R.T.: -0.009 min
Response: 118726038
Conc: 422.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
RO-COMP-2

Manual Integrations
APPROVED

Ankita
5/20/2019 4:06:08 PM

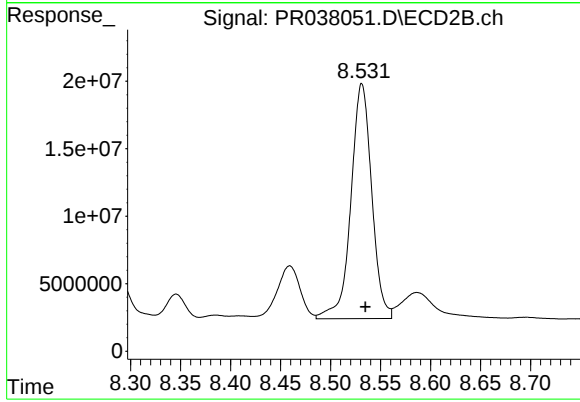

#35 AR-1260-5

R.T.: 8.531 min
Delta R.T.: -0.004 min
Response: 252466991
Conc: 485.97 ng/ml