

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052319\
 Data File : PR038255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2019 23:54
 Operator : SM\MA
 Sample : K2935-04RE
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PURGE-WATER-MUDRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 07:31:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 07:01:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.777	4.625	21449090	60646233	12.791	11.954
2)	SA Decachlor...	8.755	10.379	19698723	42683359	10.155	9.677
Target Compounds							
20)	L4 AR-1242-5	5.667	6.627	66704942	203.0E6	1061.753	1477.423 #
24)	L5 AR-1248-4	0.000	6.627	0	203.0E6	N.D.	788.020 #
25)	L5 AR-1248-5	5.667	6.627	66704942	203.0E6	770.669	832.968
26)	L6 AR-1254-1	5.667	6.627	66704942	203.0E6	455.284	759.661 #
28)	L6 AR-1254-3	0.000	7.217	0	28167981	N.D.	62.454 #
30)	L6 AR-1254-5	0.000	7.884	0	139.5E6	N.D.	402.511 #
31)	L7 AR-1260-1	0.000	7.376	0	10040827	N.D.	42.099 #
32)	L7 AR-1260-2	6.488	0.000	9677553	0	65.666	N.D. #
34)	L7 AR-1260-4	7.102	0.000	36554275	0	371.497	N.D. #
38)	L8 AR-1262-3	7.665	0.000	117.9E6	0	666.037	N.D. #
39)	L8 AR-1262-4	7.665	0.000	117.9E6	0	374.996	N.D. #
41)	L9 AR-1268-1	7.665	0.000	117.9E6	0	204.172	N.D. #
42)	L9 AR-1268-2	7.665	0.000	117.9E6	0	232.036	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052319\
Data File : PR038255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2019 23:54
Operator : SM\MA
Sample : K2935-04RE
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 07:31:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 07:01:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

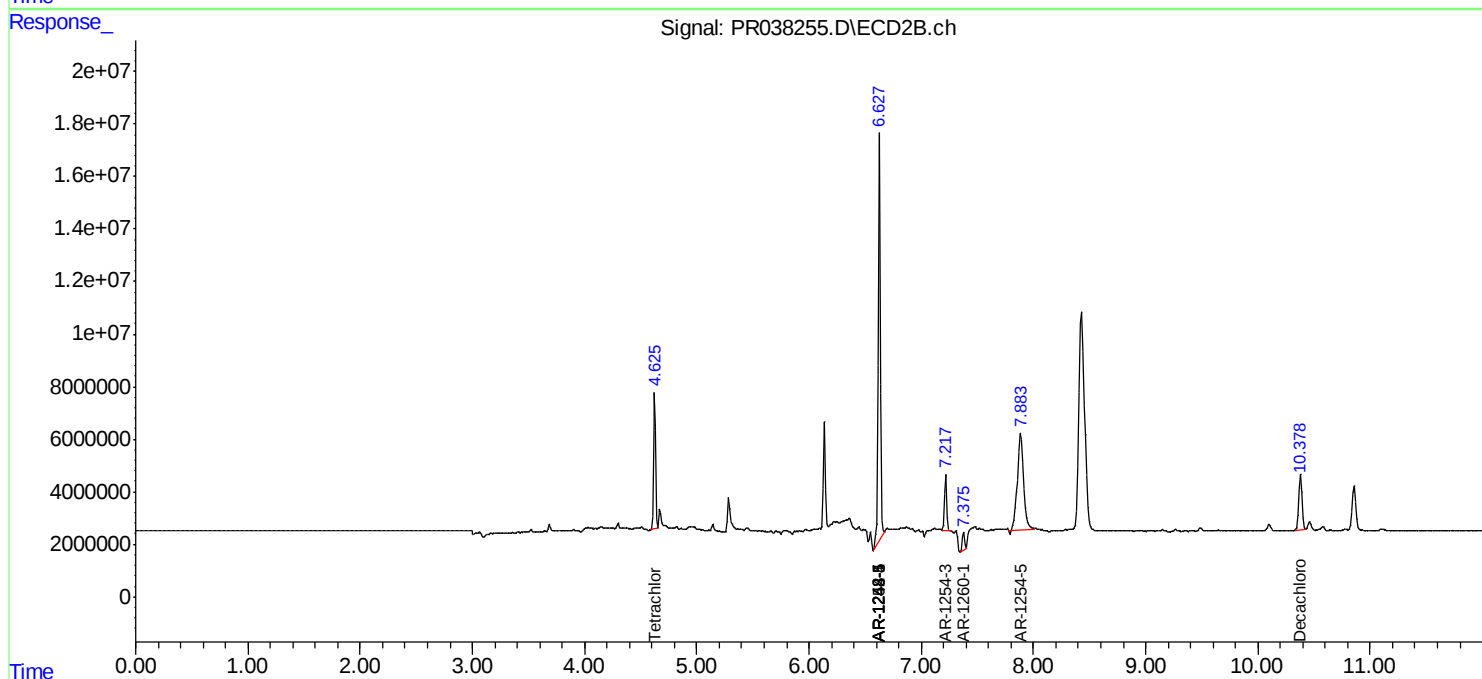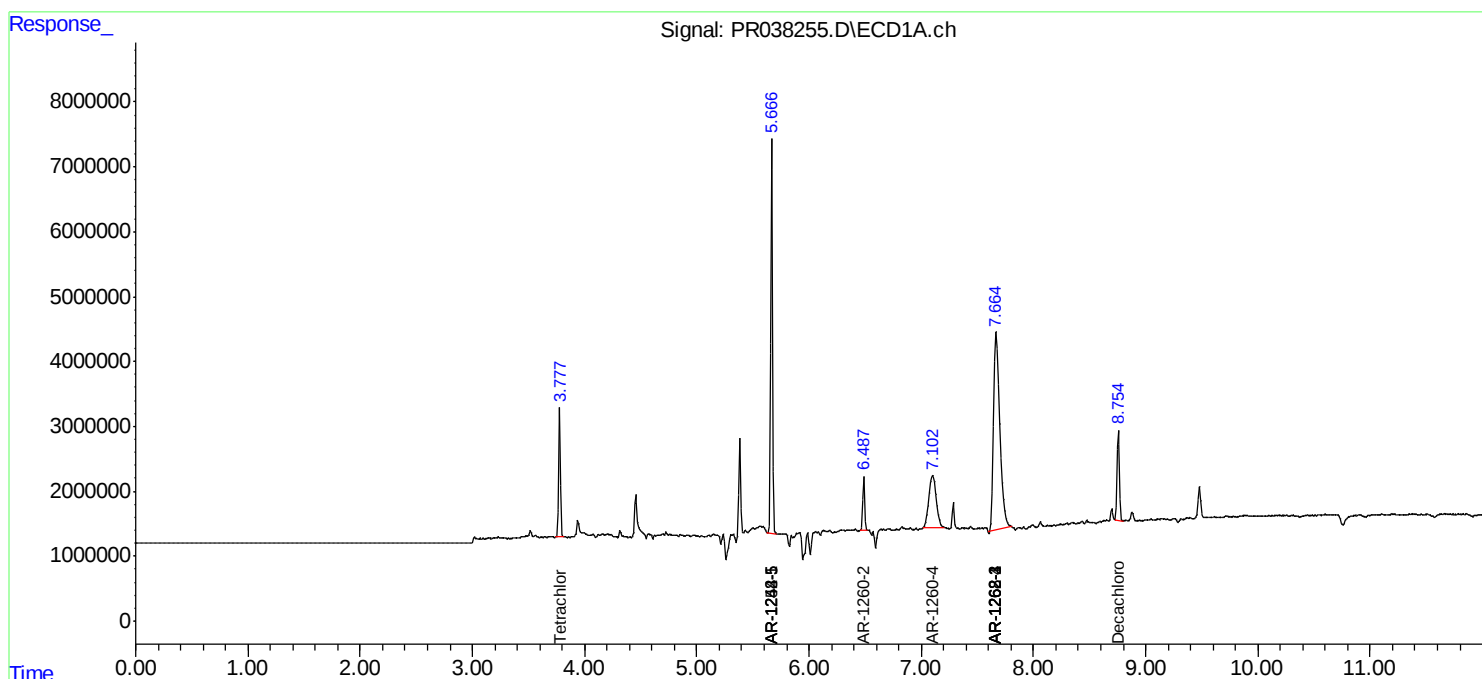


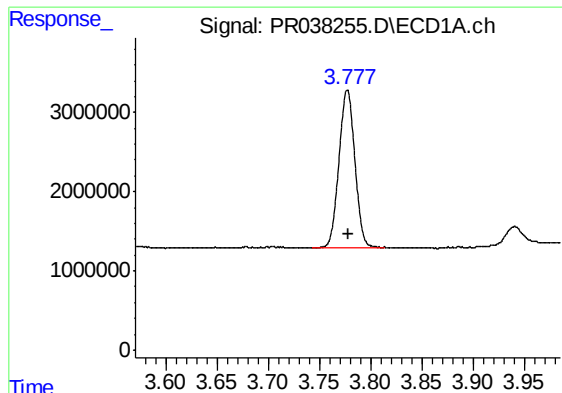

#1 Tetrachloro-m-xylene


R.T.: 3.777 min
Delta R.T.: 0.000 min
Response: 21449090
Conc: 12.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

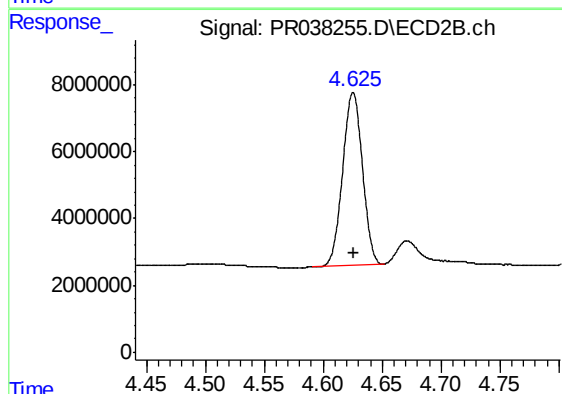


#1 Tetrachloro-m-xylene

R.T.: 4.625 min
Delta R.T.: 0.000 min
Response: 60646233
Conc: 11.95 ng/ml

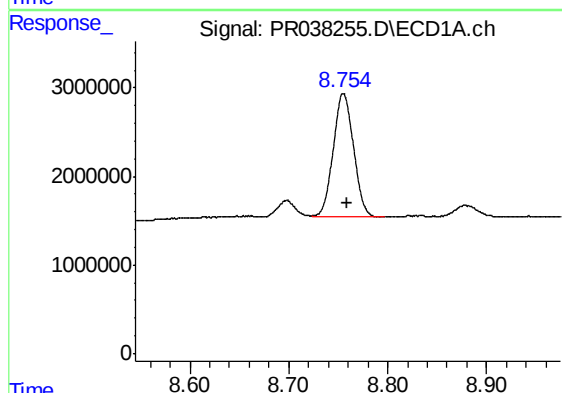


#2 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: -0.005 min
Response: 19698723
Conc: 10.15 ng/ml

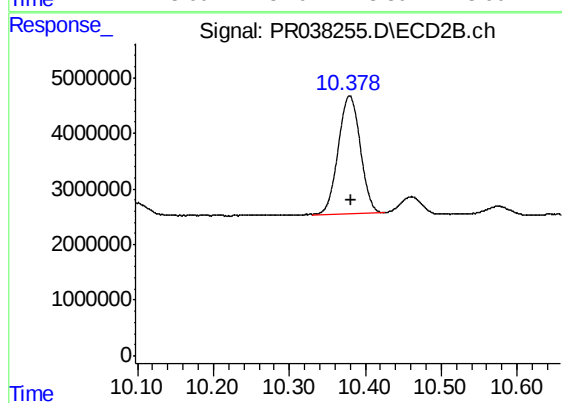

#2 Decachlorobiphenyl


R.T.: 10.379 min
Delta R.T.: -0.002 min
Response: 42683359
Conc: 9.68 ng/ml

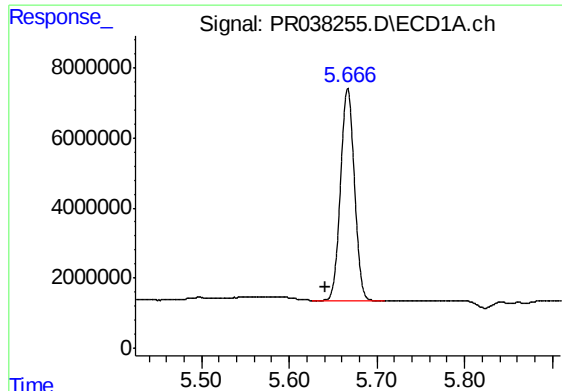

#20 AR-1242-5


R.T.: 5.667 min
Delta R.T.: 0.025 min
Response: 66704942
Conc: 1061.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

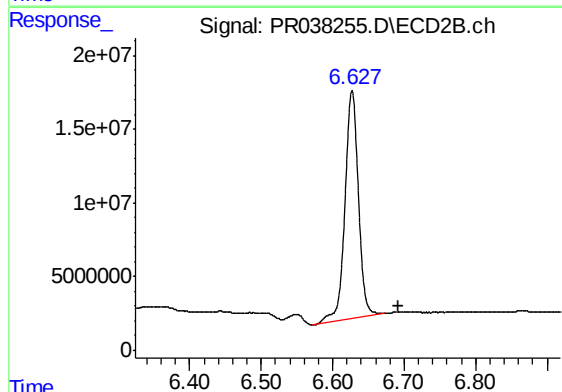


#20 AR-1242-5

R.T.: 6.627 min
Delta R.T.: -0.064 min
Response: 203014709
Conc: 1477.42 ng/ml

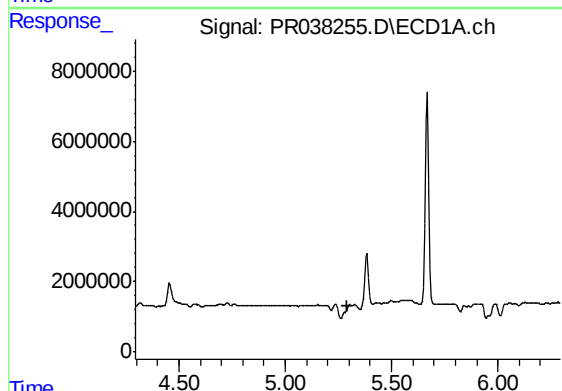


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.295 min
Response: 0
Conc: N.D.

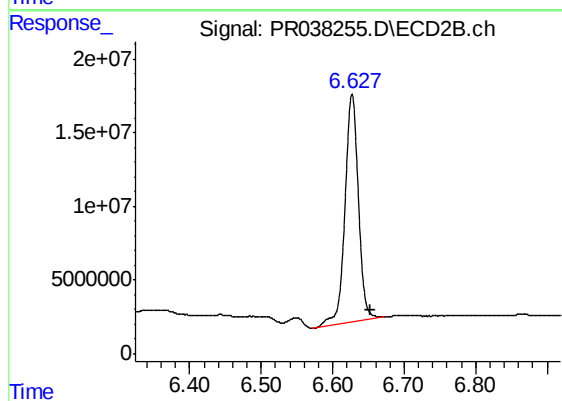

#24 AR-1248-4


R.T.: 6.627 min
Delta R.T.: -0.025 min
Response: 203014709
Conc: 788.02 ng/ml

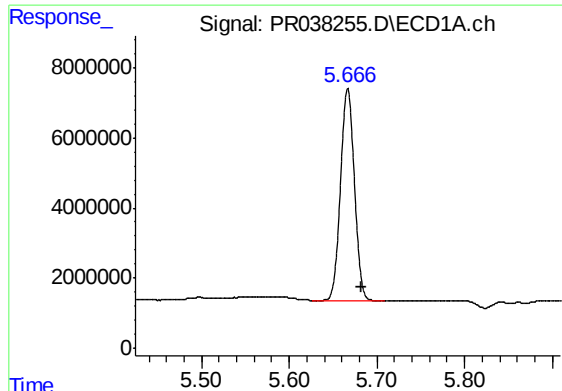

#25 AR-1248-5


R.T.: 5.667 min
Delta R.T.: -0.016 min
Response: 66704942
Conc: 770.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

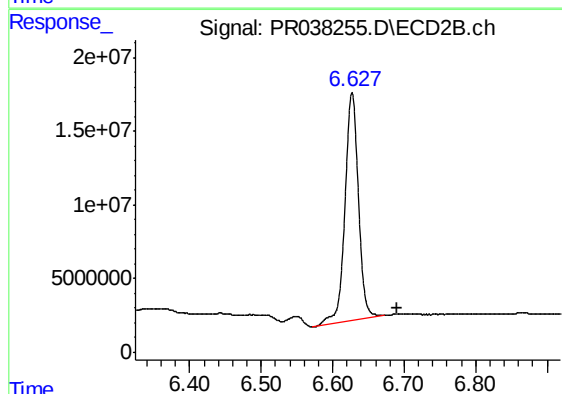


#25 AR-1248-5

R.T.: 6.627 min
Delta R.T.: -0.064 min
Response: 203014709
Conc: 832.97 ng/ml

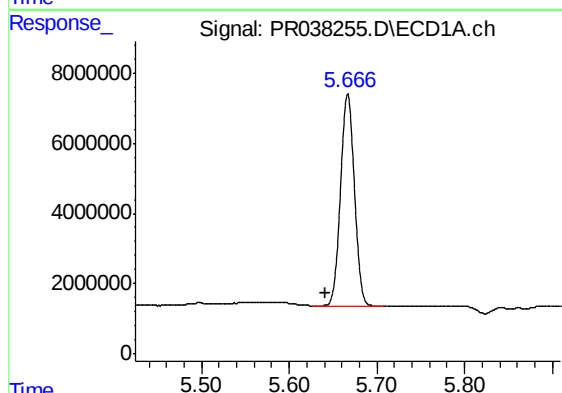


#26 AR-1254-1

R.T.: 5.667 min
Delta R.T.: 0.025 min
Response: 66704942
Conc: 455.28 ng/ml

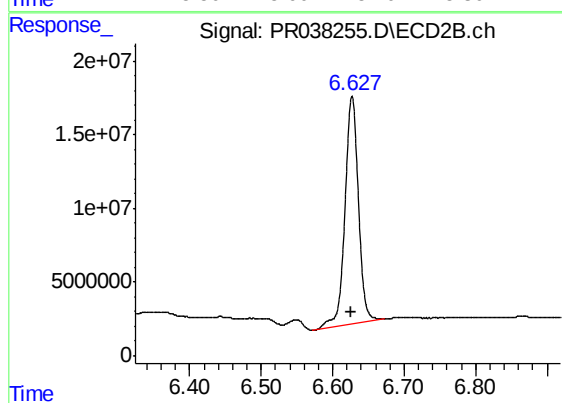

#26 AR-1254-1


R.T.: 6.627 min
Delta R.T.: 0.000 min
Response: 203014709
Conc: 759.66 ng/ml

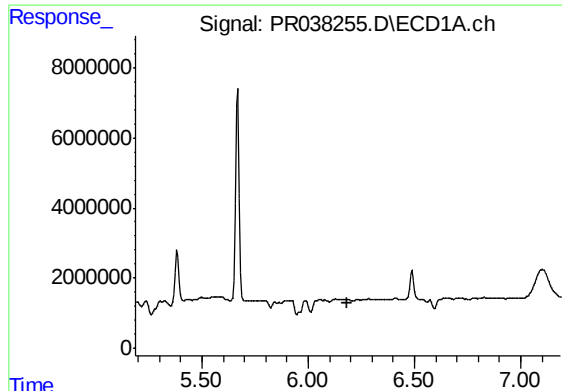

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

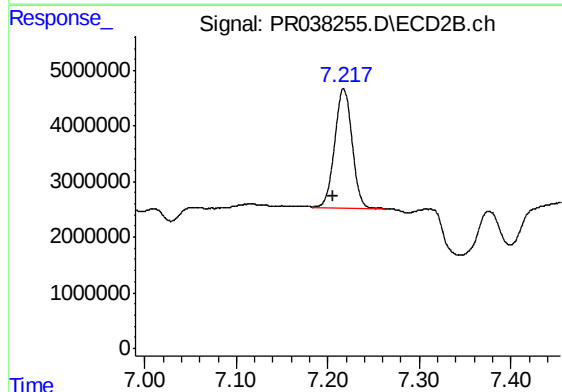


#28 AR-1254-3

R.T.: 7.217 min
Delta R.T.: 0.011 min
Response: 28167981
Conc: 62.45 ng/ml

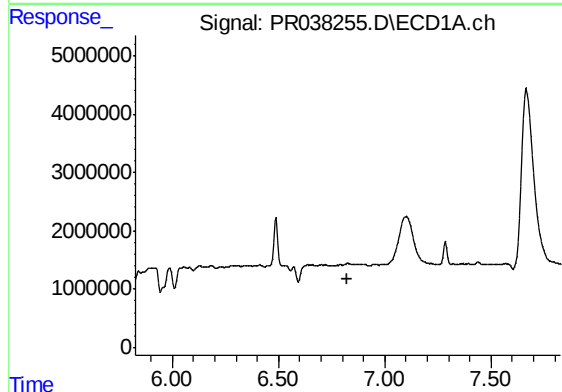


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.827 min
Response: 0
Conc: N.D.

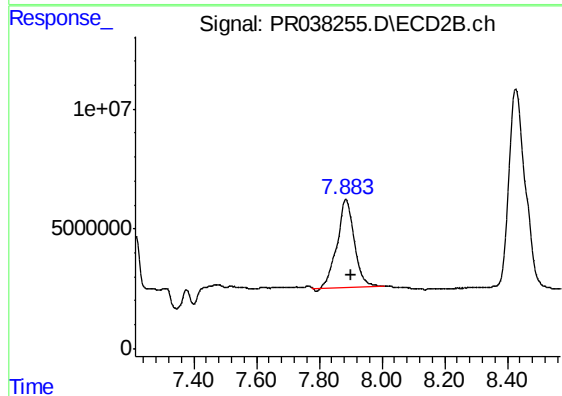

#30 AR-1254-5


R.T.: 7.884 min
Delta R.T.: -0.019 min
Response: 139456345
Conc: 402.51 ng/ml

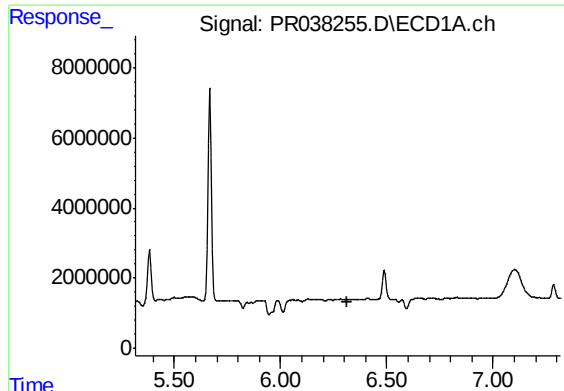

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

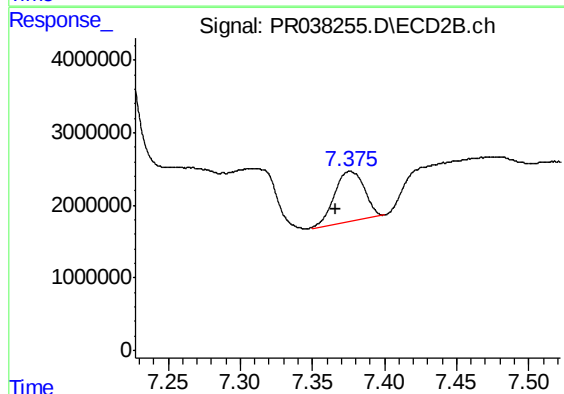


#31 AR-1260-1

R.T.: 7.376 min
Delta R.T.: 0.010 min
Response: 10040827
Conc: 42.10 ng/ml

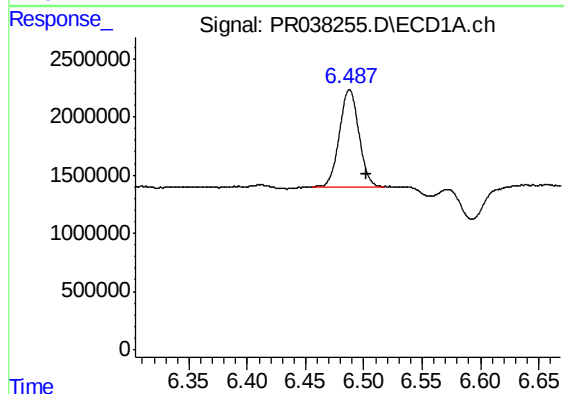


#32 AR-1260-2

R.T.: 6.488 min
Delta R.T.: -0.015 min
Response: 9677553
Conc: 65.67 ng/ml

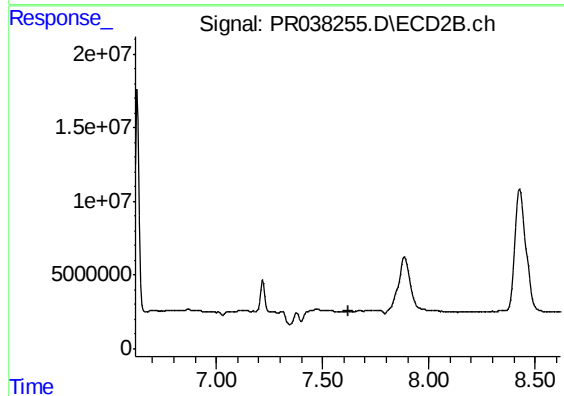

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.619 min
Response: 0
Conc: N.D.

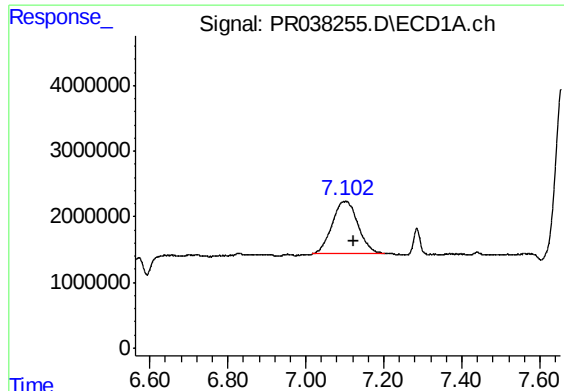

#34 AR-1260-4


R.T.: 7.102 min
Delta R.T.: -0.022 min
Response: 36554275
Conc: 371.50 ng/ml

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

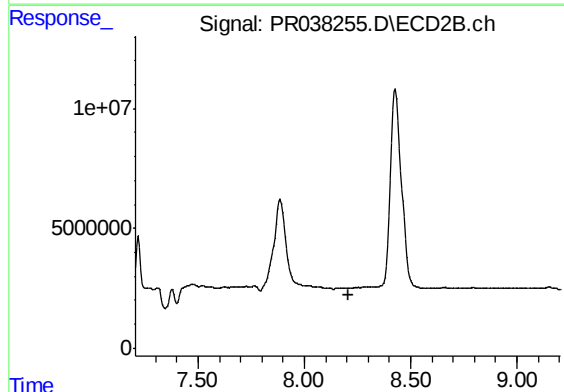


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.205 min
Response: 0
Conc: N.D.

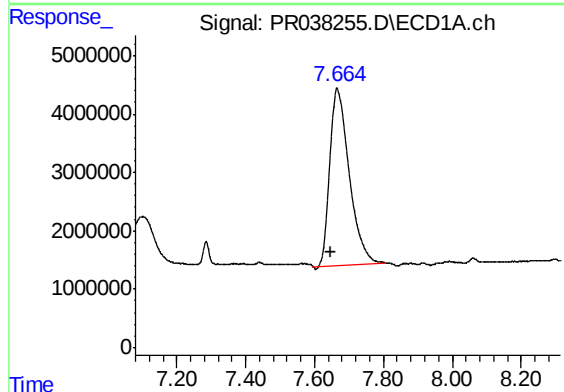


#38 AR-1262-3

R.T.: 7.665 min
Delta R.T.: 0.020 min
Response: 117880394
Conc: 666.04 ng/ml

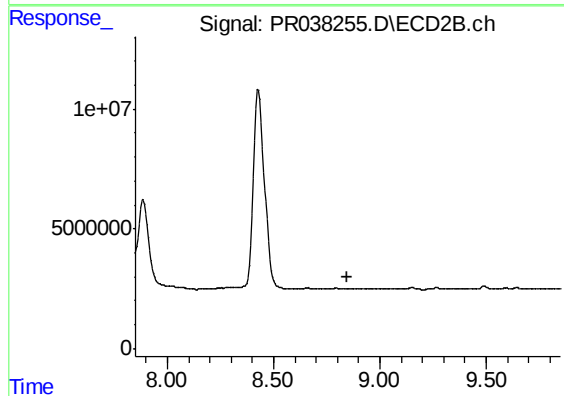

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.850 min
Response: 0
Conc: N.D.

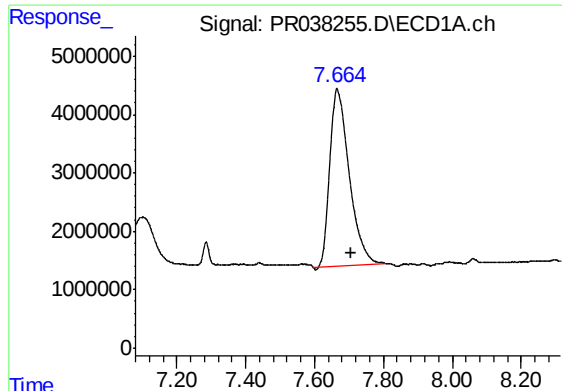

#39 AR-1262-4


R.T.: 7.665 min
Delta R.T.: -0.043 min
Response: 117880394
Conc: 375.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

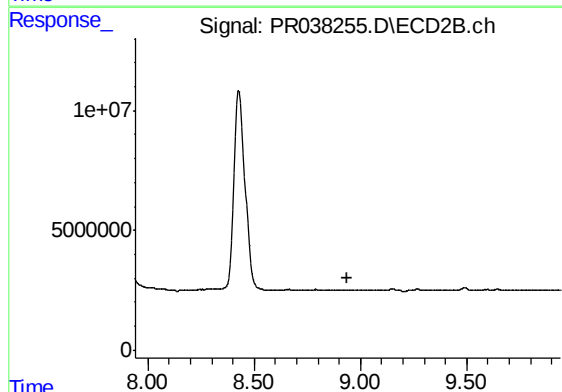


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.941 min
Response: 0
Conc: N.D.

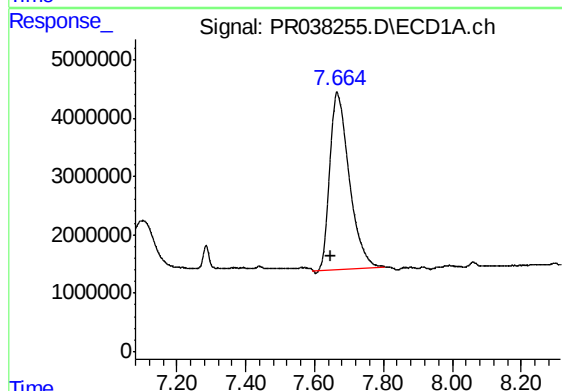


#41 AR-1268-1

R.T.: 7.665 min
Delta R.T.: 0.019 min
Response: 117880394
Conc: 204.17 ng/ml

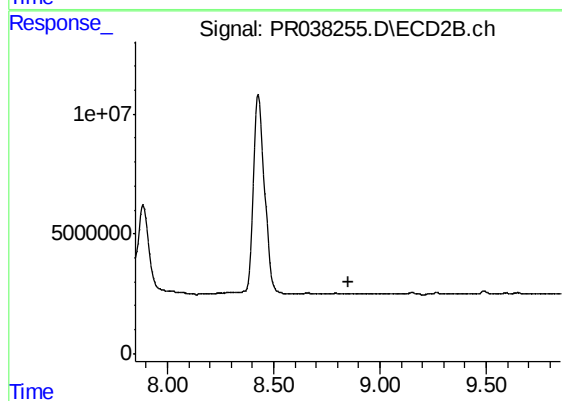

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

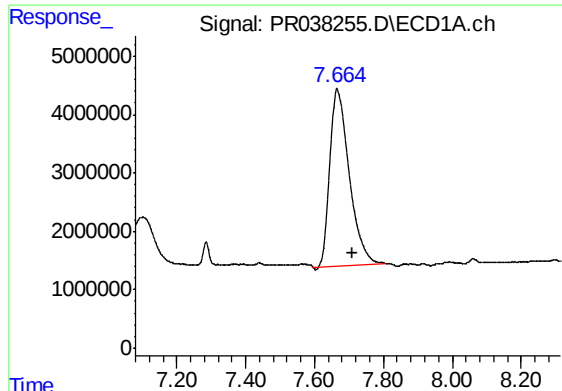

#42 AR-1268-2

R.T.: 7.665 min
Delta R.T.: -0.046 min
Response: 117880394
Conc: 232.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
PURGE-WATER-MUDRE

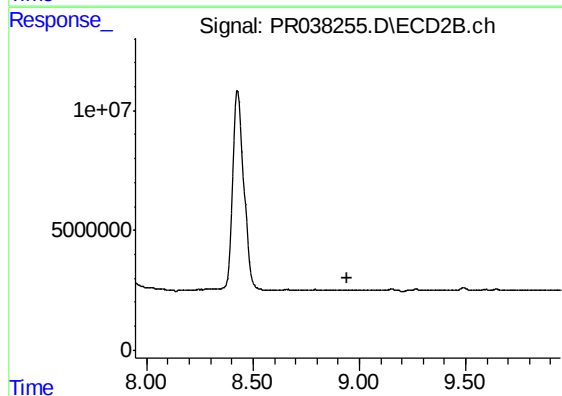

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.947 min
Response: 0
Conc: N.D.