

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052319\
 Data File : PR038237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2019 19:34
 Operator : SM\MA
 Sample : PB119968BS
 Misc :
 ALS Vial : 149 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PB119968BS

Manual Integrations
 APPROVED

Ankita
 5/24/2019 3:12:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 07:51:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 07:01:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.779	4.627	26618555	74315685	15.874	14.648
2) SA Decachlor...	8.756	10.380	36953283	81681259	19.049	18.518
Target Compounds						
31) L7 AR-1260-1	6.316	7.366	5255002	11808543	49.066	49.510
32) L7 AR-1260-2	6.501	7.618	8182239	12997835	55.520	45.440
33) L7 AR-1260-3	6.654	7.974	6949094	7842588	57.057m	36.845 #
34) L7 AR-1260-4	7.122	8.203	5074745	10261787	51.574m	41.470m
35) L7 AR-1260-5	7.361	8.530	11410025	20643199	41.880	40.256

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052319\
Data File : PR038237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2019 19:34
Operator : SM\MA
Sample : PB119968BS
Misc :
ALS Vial : 149 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
PB119968BS


Manual Integrations
APPROVED

Ankita
5/24/2019 3:12:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 07:51:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 07:01:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

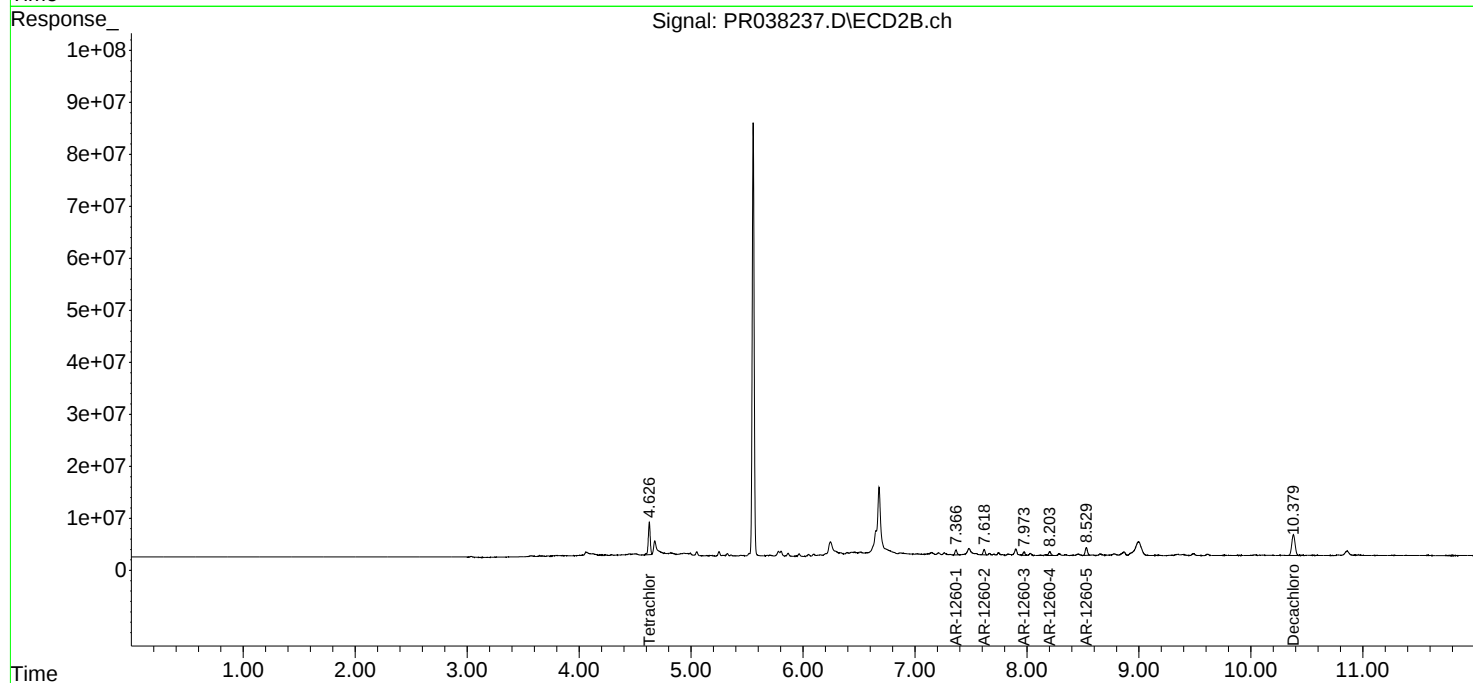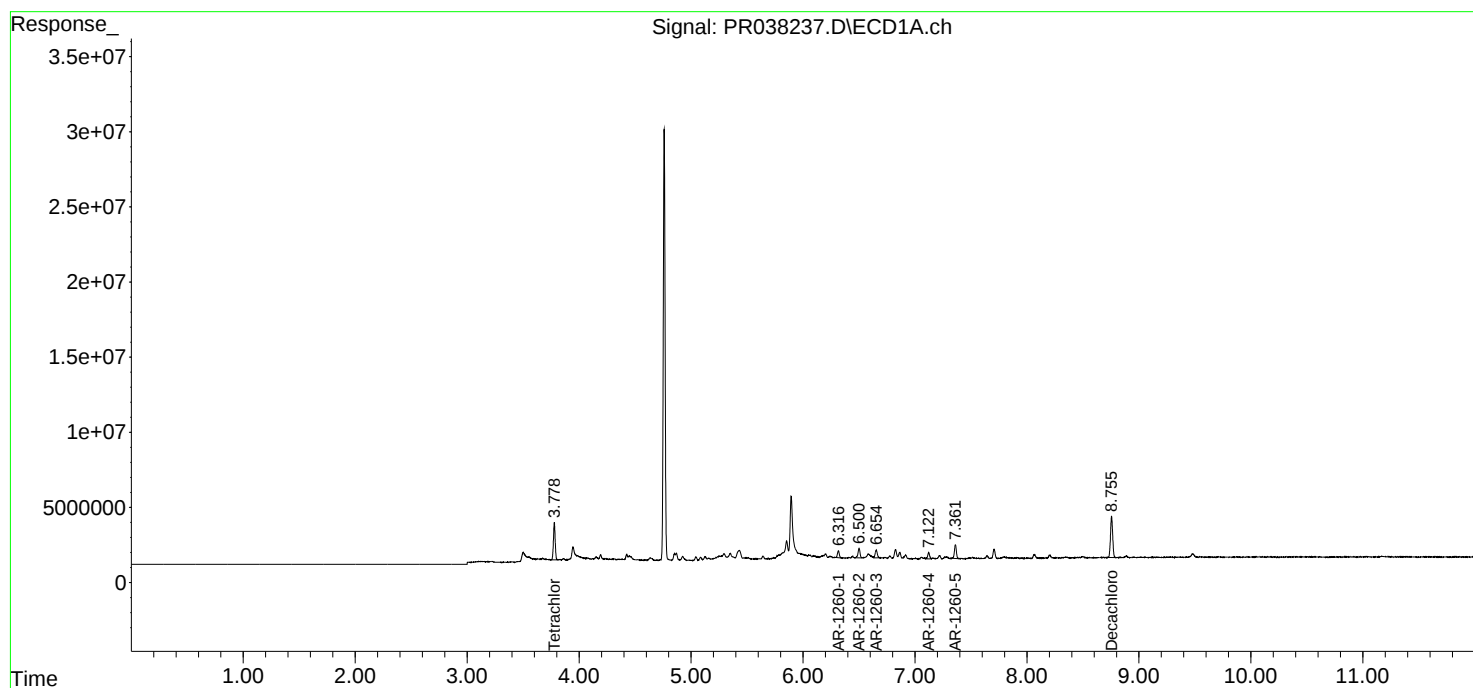

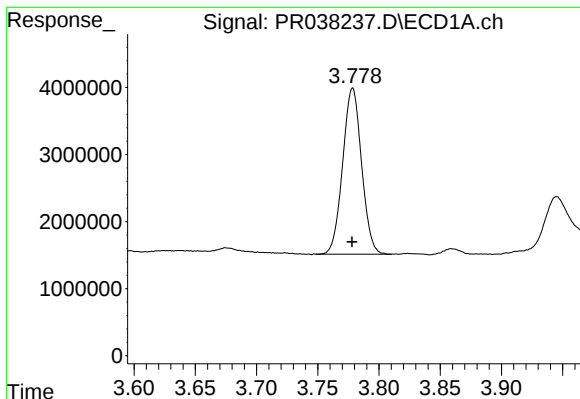


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 26618555
Conc: 15.87 ng/ml

Instrument :
ECD_R
ClientSampleId :
PB119968BS


Manual Integrations
APPROVED

Ankita
5/24/2019 3:12:36 PM

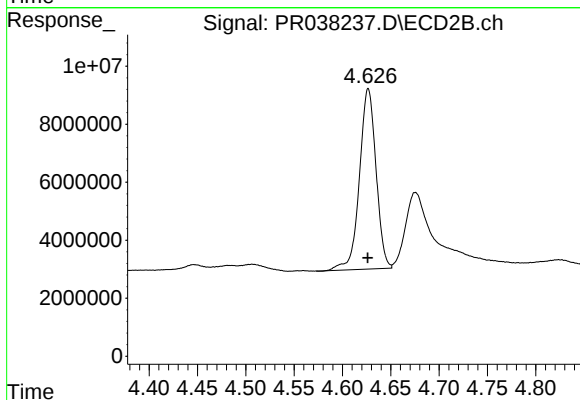


#1 Tetrachloro-m-xylene

R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 74315685
Conc: 14.65 ng/ml

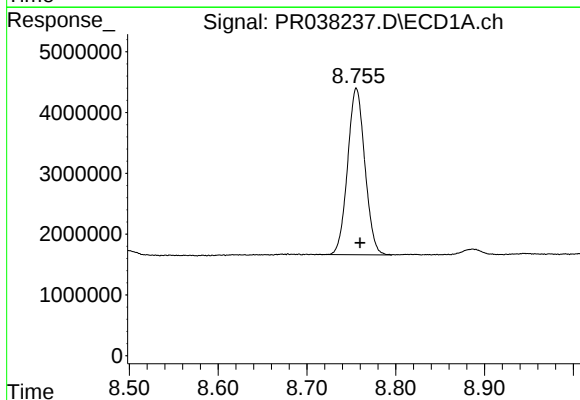


#2 Decachlorobiphenyl

R.T.: 8.756 min
Delta R.T.: -0.004 min
Response: 36953283
Conc: 19.05 ng/ml

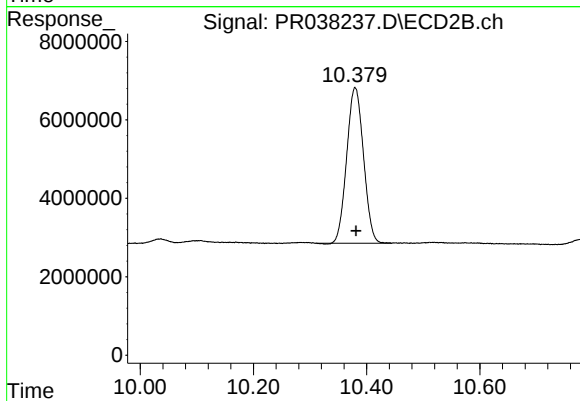

#2 Decachlorobiphenyl

R.T.: 10.380 min
Delta R.T.: -0.002 min
Response: 81681259
Conc: 18.52 ng/ml

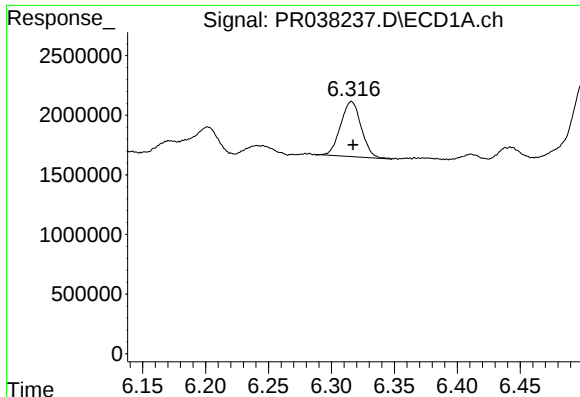


#31 AR-1260-1

R.T.: 6.316 min
Delta R.T.: -0.001 min
Response: 5255002
Conc: 49.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
PB119968BS


Manual Integrations
APPROVED

Ankita
5/24/2019 3:12:36 PM

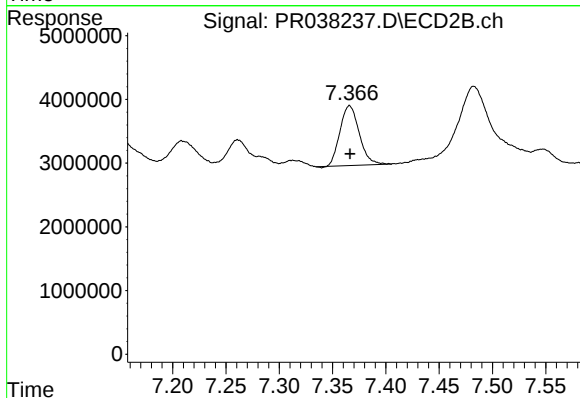


#31 AR-1260-1

R.T.: 7.366 min
Delta R.T.: 0.000 min
Response: 11808543
Conc: 49.51 ng/ml

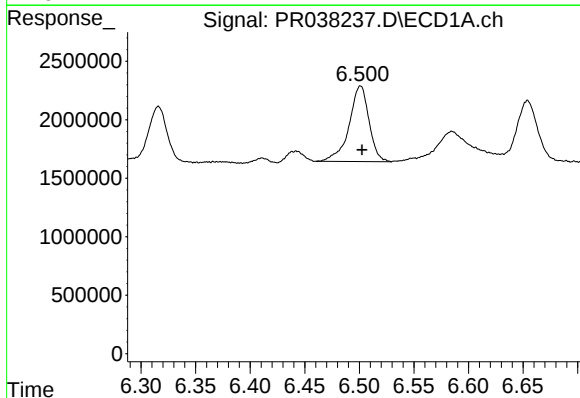


#32 AR-1260-2

R.T.: 6.501 min
Delta R.T.: -0.002 min
Response: 8182239
Conc: 55.52 ng/ml

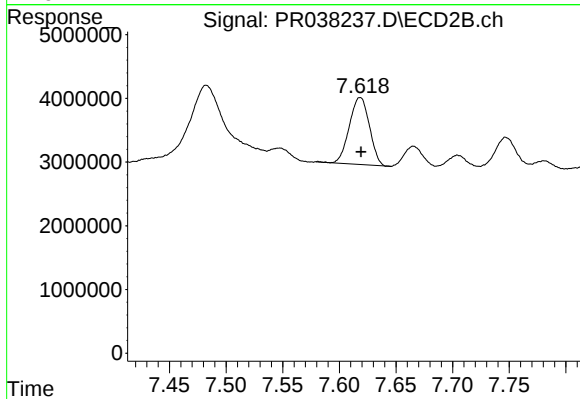

#32 AR-1260-2

R.T.: 7.618 min
Delta R.T.: 0.000 min
Response: 12997835
Conc: 45.44 ng/ml

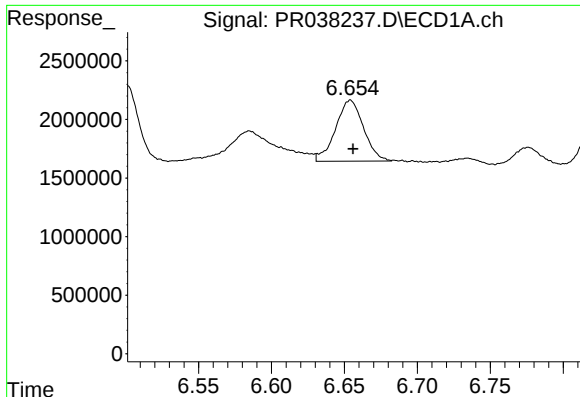


#33 AR-1260-3

R.T.: 6.654 min
Delta R.T.: -0.002 min
Response: 6949094
Conc: 57.06 ng/ml m

Instrument :
ECD_R
ClientSampleId :
PB119968BS


Manual Integrations
APPROVED

Ankita
5/24/2019 3:12:36 PM

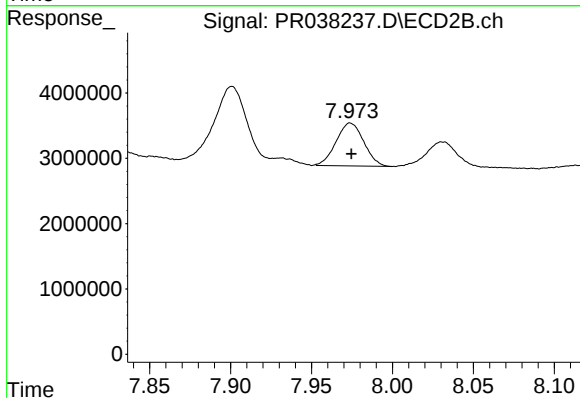


#33 AR-1260-3

R.T.: 7.974 min
Delta R.T.: 0.000 min
Response: 7842588
Conc: 36.84 ng/ml

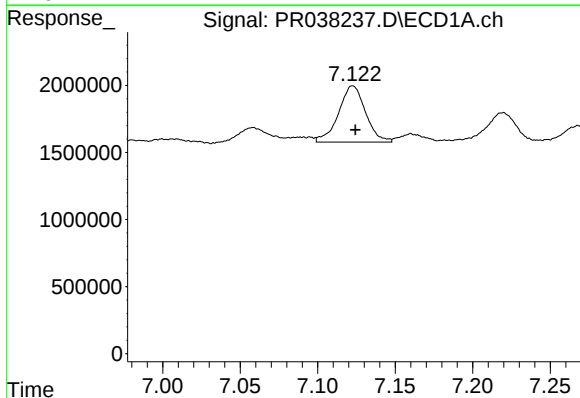


#34 AR-1260-4

R.T.: 7.122 min
Delta R.T.: -0.002 min
Response: 5074745
Conc: 51.57 ng/ml m

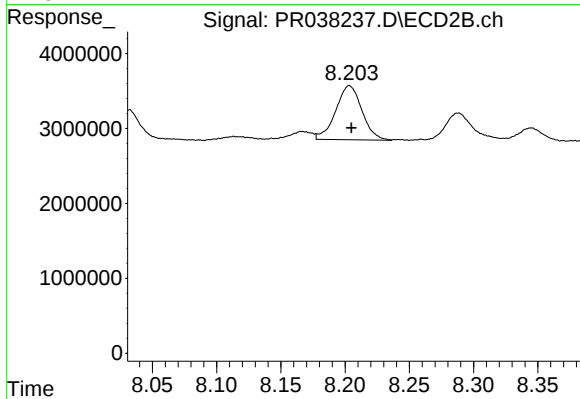

#34 AR-1260-4

R.T.: 8.203 min
Delta R.T.: -0.002 min
Response: 10261787
Conc: 41.47 ng/ml m

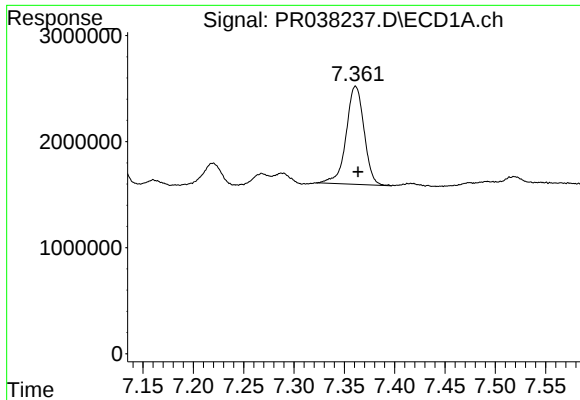


#35 AR-1260-5

R.T.: 7.361 min
Delta R.T.: -0.002 min
Response: 11410025
Conc: 41.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
PB119968BS

Manual Integrations
APPROVED

Ankita
5/24/2019 3:12:36 PM

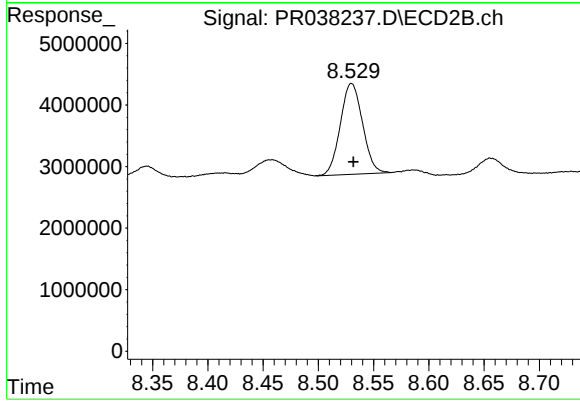

#35 AR-1260-5

R.T.: 8.530 min
Delta R.T.: -0.002 min
Response: 20643199
Conc: 40.26 ng/ml