

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR052319\  
 Data File : PR038255.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 May 2019 23:54  
 Operator : SM\MA  
 Sample : K2935-04RE  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 PURGE-WATER-MUDRE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 24 07:31:21 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR052319.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri May 24 07:01:56 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-------|--------|----------|----------|--------|--------|
| -----                       |       |        |          |          |        |        |
| System Monitoring Compounds |       |        |          |          |        |        |
| 1) SA Tetrachlo...          | 3.777 | 4.625  | 21449090 | 60646233 | 12.791 | 11.954 |
| 2) SA Decachlor...          | 8.755 | 10.379 | 19698723 | 42683359 | 10.155 | 9.677  |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR052319\  
Data File : PR038255.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 23 May 2019 23:54  
Operator : SM\MA  
Sample : K2935-04RE  
Misc :  
ALS Vial : 30 Sample Multiplier: 1

Instrument :  
ECD\_R  
ClientSampleId :  
PURGE-WATER-MUDRE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 24 07:31:21 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR052319.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri May 24 07:01:56 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

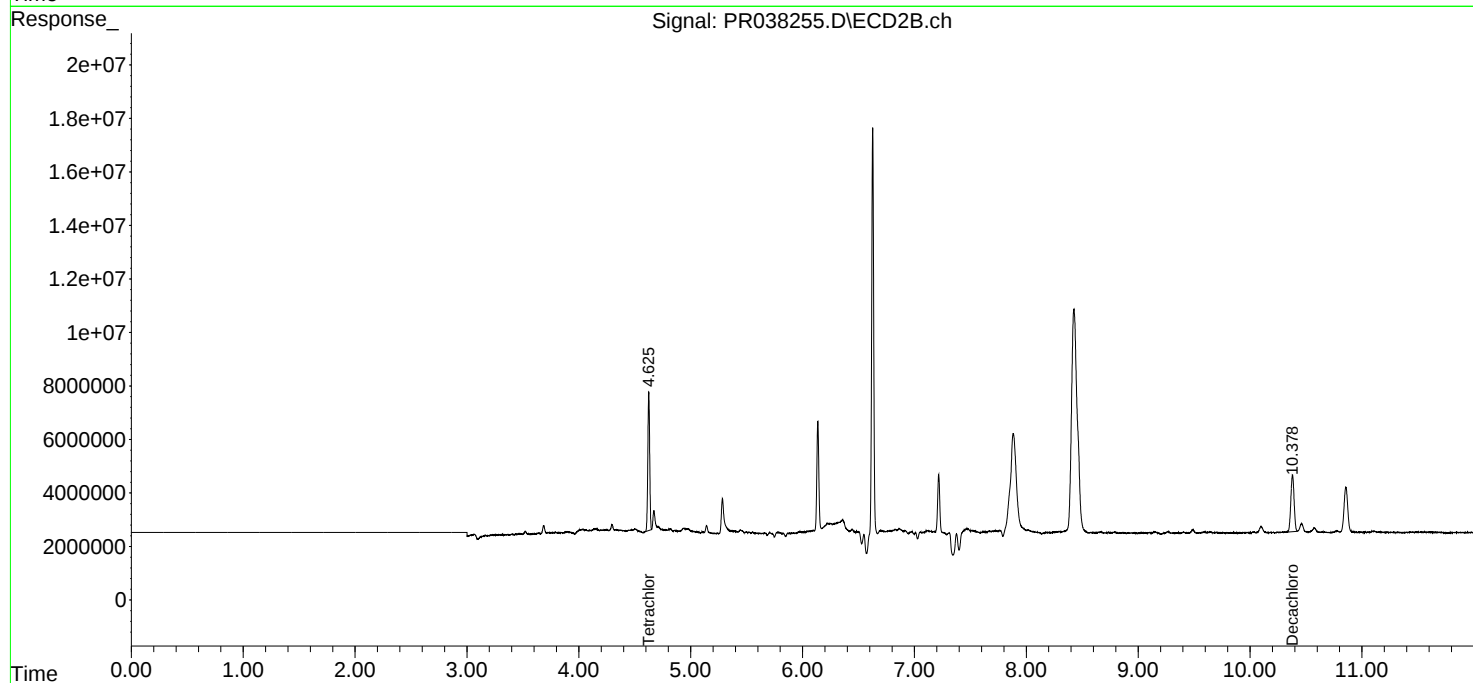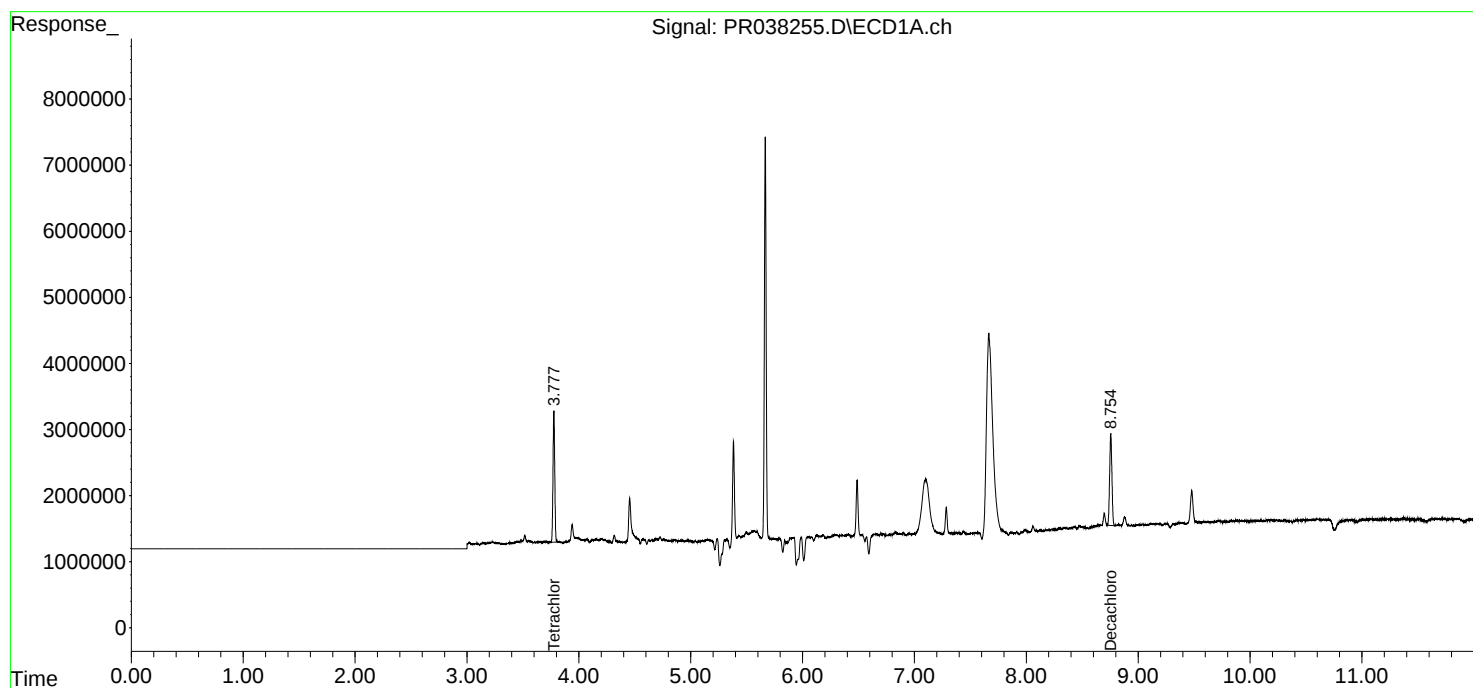


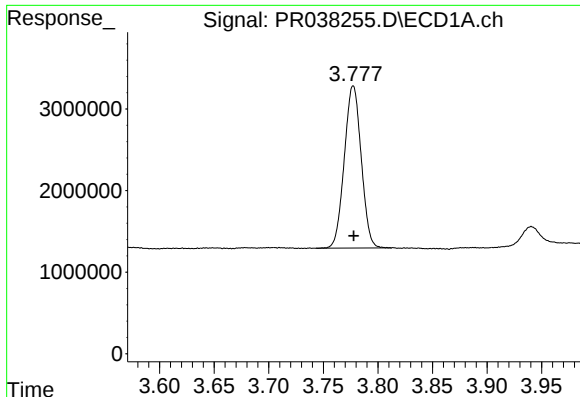

#1 Tetrachloro-m-xylene


R.T.: 3.777 min  
Delta R.T.: 0.000 min  
Response: 21449090  
Conc: 12.79 ng/ml

Instrument :  
ECD\_R  
ClientSampleId :  
PURGE-WATER-MUDRE

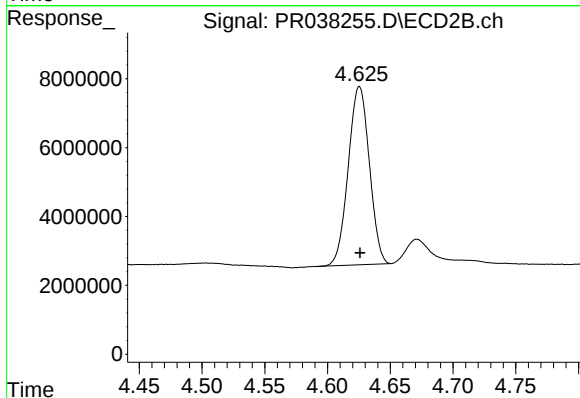


#1 Tetrachloro-m-xylene

R.T.: 4.625 min  
Delta R.T.: 0.000 min  
Response: 60646233  
Conc: 11.95 ng/ml

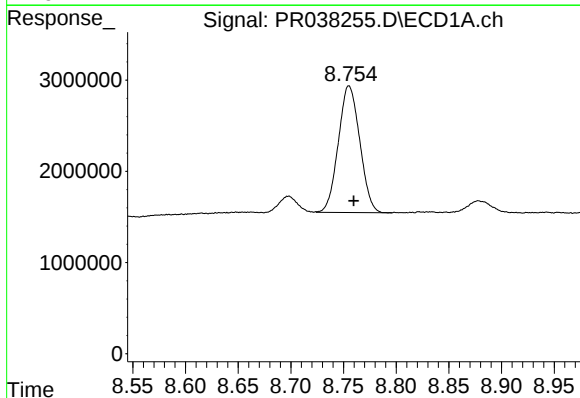

#2 Decachlorobiphenyl

R.T.: 8.755 min  
Delta R.T.: -0.005 min  
Response: 19698723  
Conc: 10.15 ng/ml

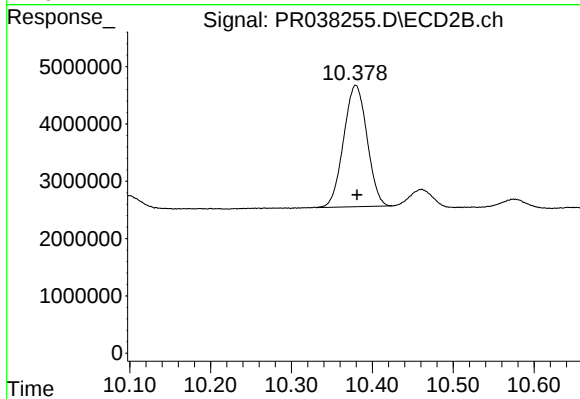

#2 Decachlorobiphenyl

R.T.: 10.379 min  
Delta R.T.: -0.002 min  
Response: 42683359  
Conc: 9.68 ng/ml