

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052819\
 Data File : PR038310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2019 11:50
 Operator : SM\MA
 Sample : K2994-15DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TP-6-SDL

Manual Integrations
 APPROVED

Ankita
 5/29/2019 2:09:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 13:37:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 07:01:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.780	4.627	17865077	47065191	10.654m	9.277
2)	SA Decachlor...	8.761	10.380	13992350	47594984	7.213m	10.790 #
Target Compounds							
31)	L7 AR-1260-1	6.317	7.366	39436347	117.3E6	368.219	491.716 #
32)	L7 AR-1260-2	6.500	7.617	99329277	184.9E6	673.990	646.566
33)	L7 AR-1260-3	6.657	7.974	50900438	169.4E6	417.931	795.784 #
34)	L7 AR-1260-4	7.125	8.204	58255014	171.8E6	592.039	694.343
35)	L7 AR-1260-5	7.364	8.530	179.5E6	459.9E6	658.935	896.803 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052819\
Data File : PR038310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2019 11:50
Operator : SM\MA
Sample : K2994-15DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
TP-6-SDL


Manual Integrations
APPROVED

Ankita
5/29/2019 2:09:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 13:37:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 07:01:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

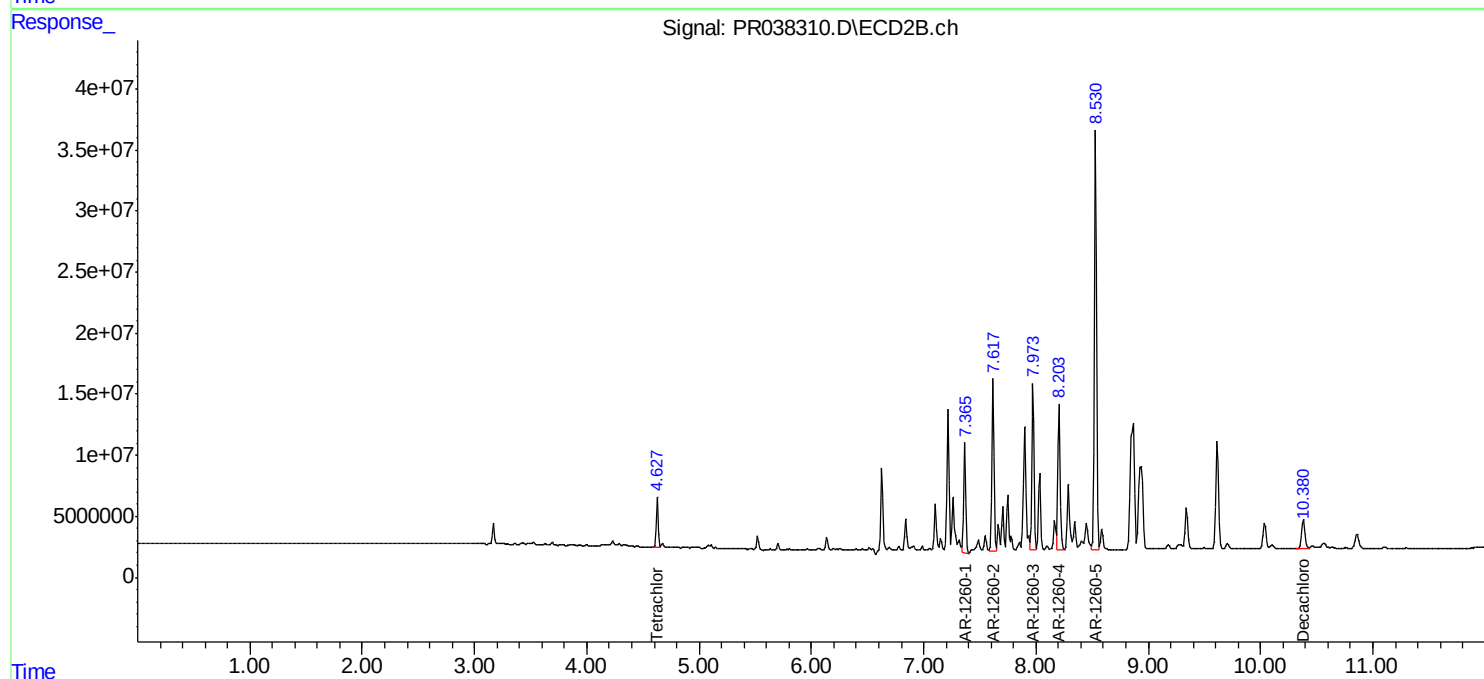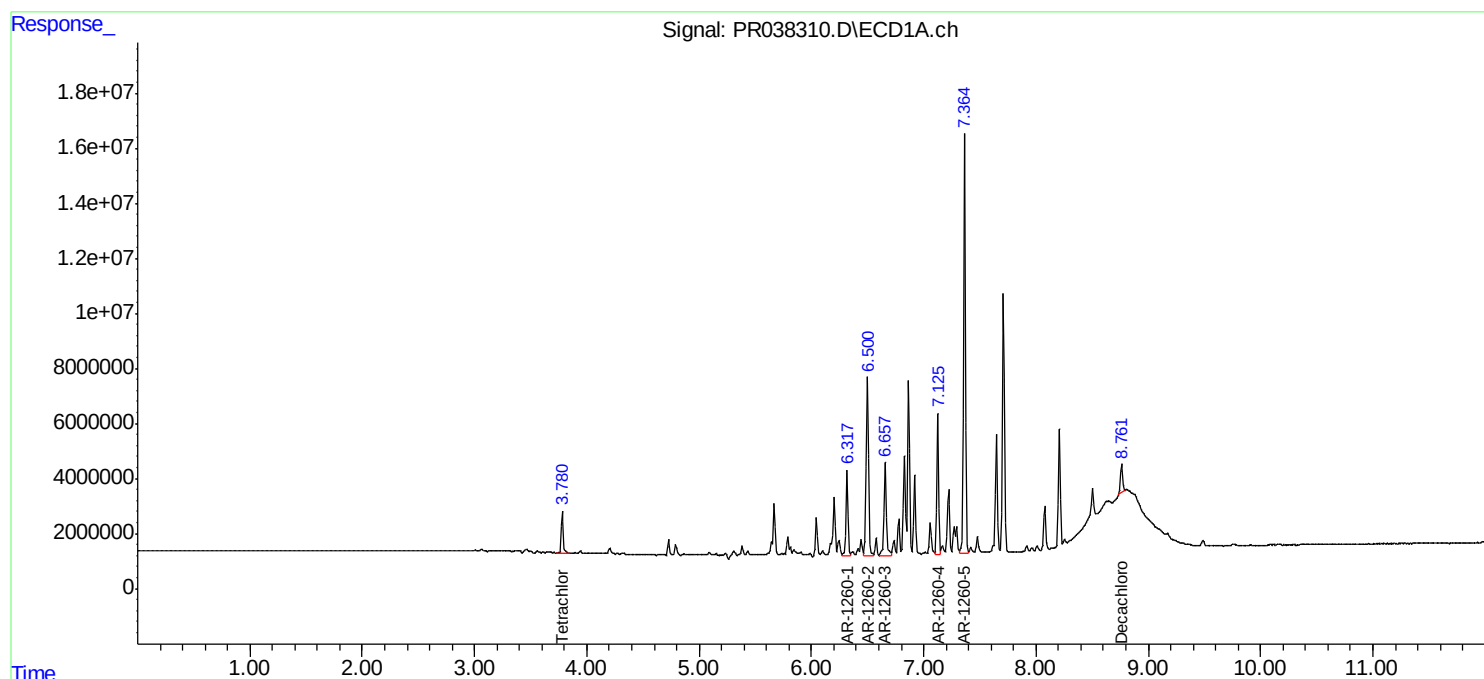

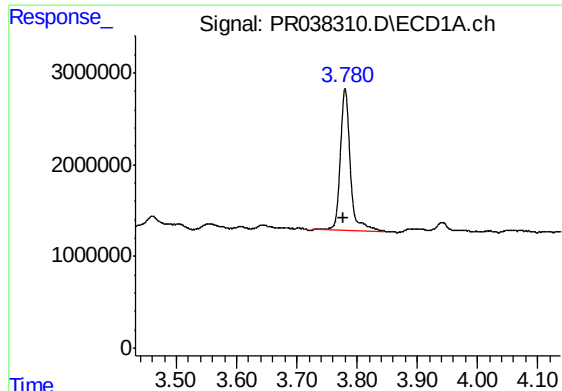


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: 0.002 min
Response: 17865077
Conc: 10.65 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TP-6-SDL


Manual Integrations
APPROVED

Ankita
5/29/2019 2:09:42 PM

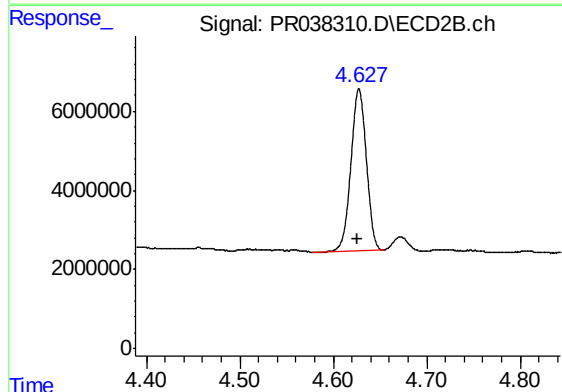


#1 Tetrachloro-m-xylene

R.T.: 4.627 min
Delta R.T.: 0.001 min
Response: 47065191
Conc: 9.28 ng/ml

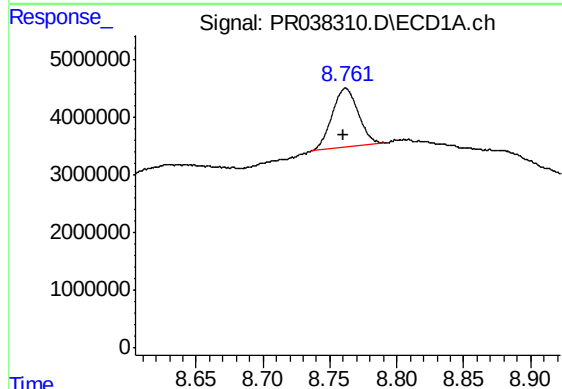


#2 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: 0.002 min
Response: 13992350
Conc: 7.21 ng/ml m

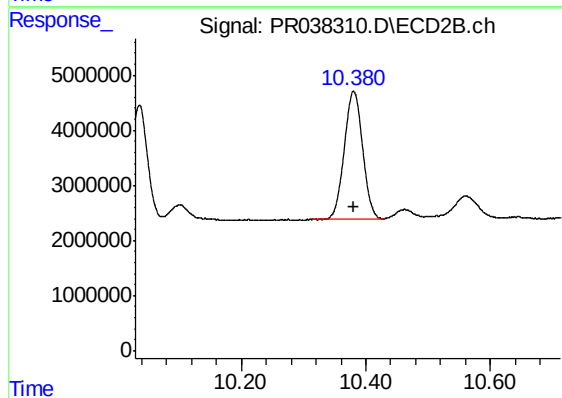

#2 Decachlorobiphenyl

R.T.: 10.380 min
Delta R.T.: -0.001 min
Response: 47594984
Conc: 10.79 ng/ml

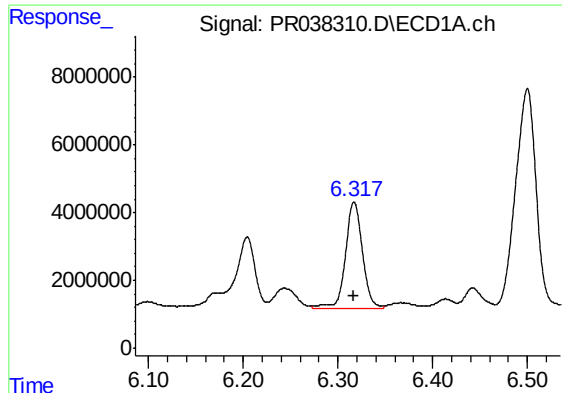


#31 AR-1260-1

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 39436347
Conc: 368.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-6-SDL


Manual Integrations
APPROVED

Ankita
5/29/2019 2:09:42 PM

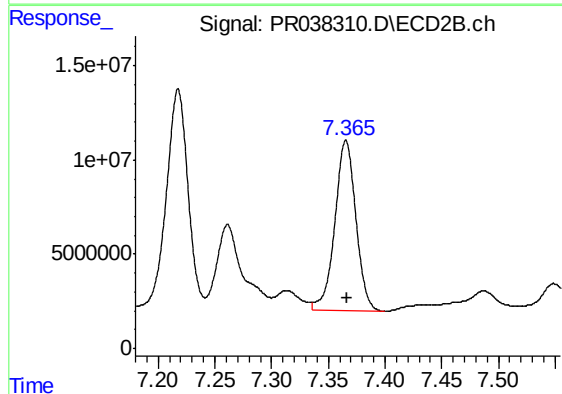


#31 AR-1260-1

R.T.: 7.366 min
Delta R.T.: 0.000 min
Response: 117277149
Conc: 491.72 ng/ml

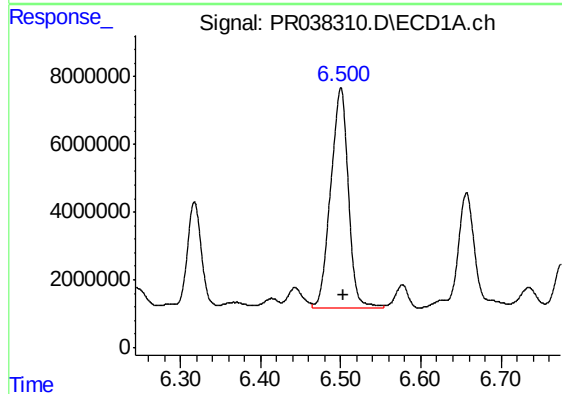


#32 AR-1260-2

R.T.: 6.500 min
Delta R.T.: -0.003 min
Response: 99329277
Conc: 673.99 ng/ml

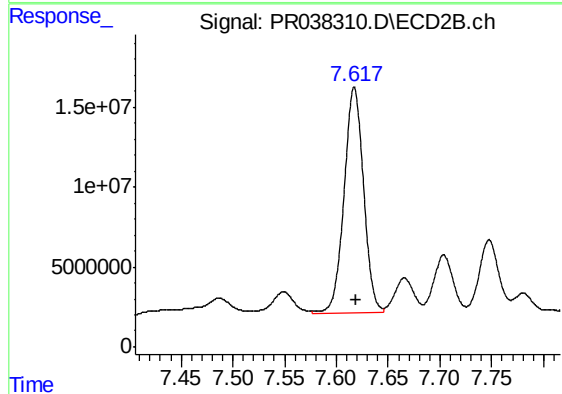

#32 AR-1260-2

R.T.: 7.617 min
Delta R.T.: -0.002 min
Response: 184948322
Conc: 646.57 ng/ml

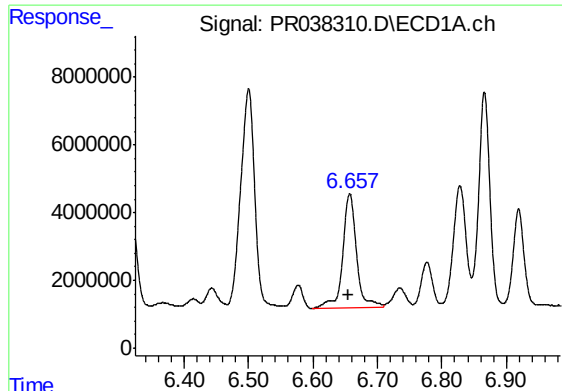


#33 AR-1260-3

R.T.: 6.657 min
Delta R.T.: 0.001 min
Response: 50900438
Conc: 417.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-6-SDL


Manual Integrations
APPROVED

Ankita
5/29/2019 2:09:42 PM

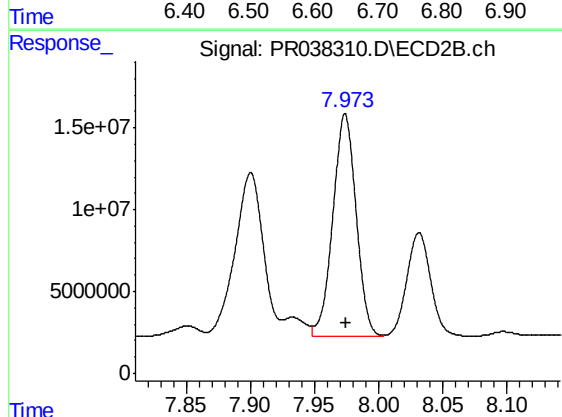


#33 AR-1260-3

R.T.: 7.974 min
Delta R.T.: 0.000 min
Response: 169386922
Conc: 795.78 ng/ml

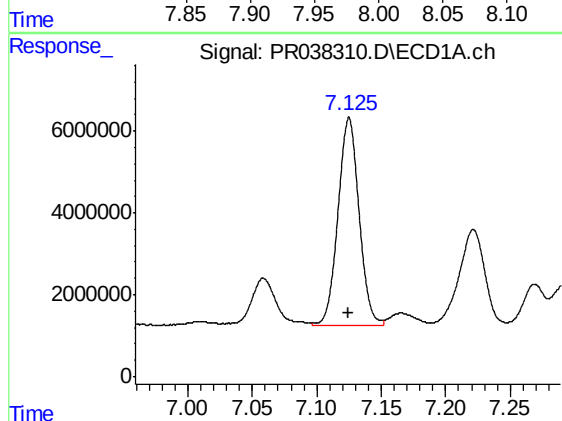


#34 AR-1260-4

R.T.: 7.125 min
Delta R.T.: 0.000 min
Response: 58255014
Conc: 592.04 ng/ml

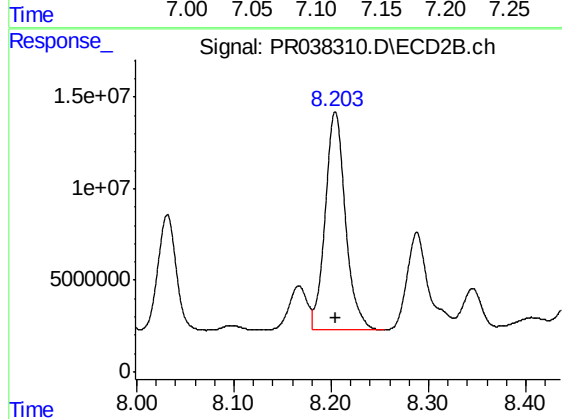

#34 AR-1260-4

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 171813692
Conc: 694.34 ng/ml

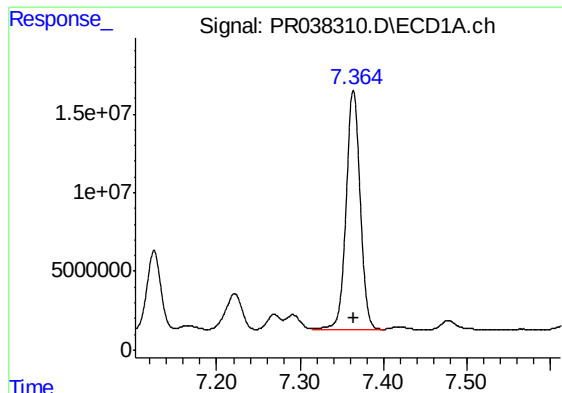


#35 AR-1260-5

R.T.: 7.364 min
Delta R.T.: 0.000 min
Response: 179523362
Conc: 658.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-6-SDL

Manual Integrations
APPROVED

Ankita
5/29/2019 2:09:42 PM

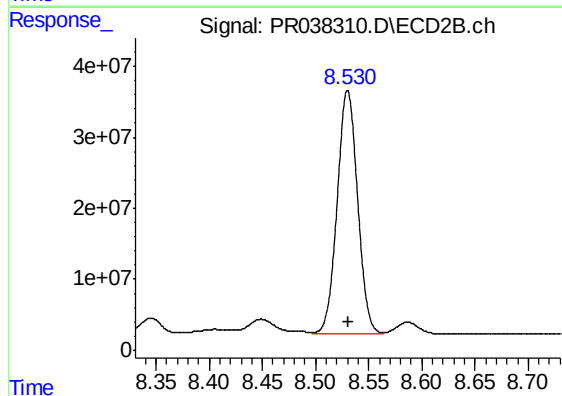

#35 AR-1260-5

R.T.: 8.530 min
Delta R.T.: -0.001 min
Response: 459876152
Conc: 896.80 ng/ml