

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052819\
 Data File : PR038320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2019 14:20
 Operator : SM\MA
 Sample : K3050-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 052319-SBOA-E-U-B

Manual Integrations
 APPROVED

Ankita
 5/29/2019 2:10:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 15:44:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 07:01:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.777	4.626	34474140	105.8E6	20.558m	20.852m
2) SA Decachlor...	8.759	10.380	28939316	80695469	14.918	18.294

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052819\
Data File : PR038320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2019 14:20
Operator : SM\MA
Sample : K3050-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
052319-SBOA-E-U-B


Manual Integrations
APPROVED

Ankita
5/29/2019 2:10:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 15:44:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 07:01:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

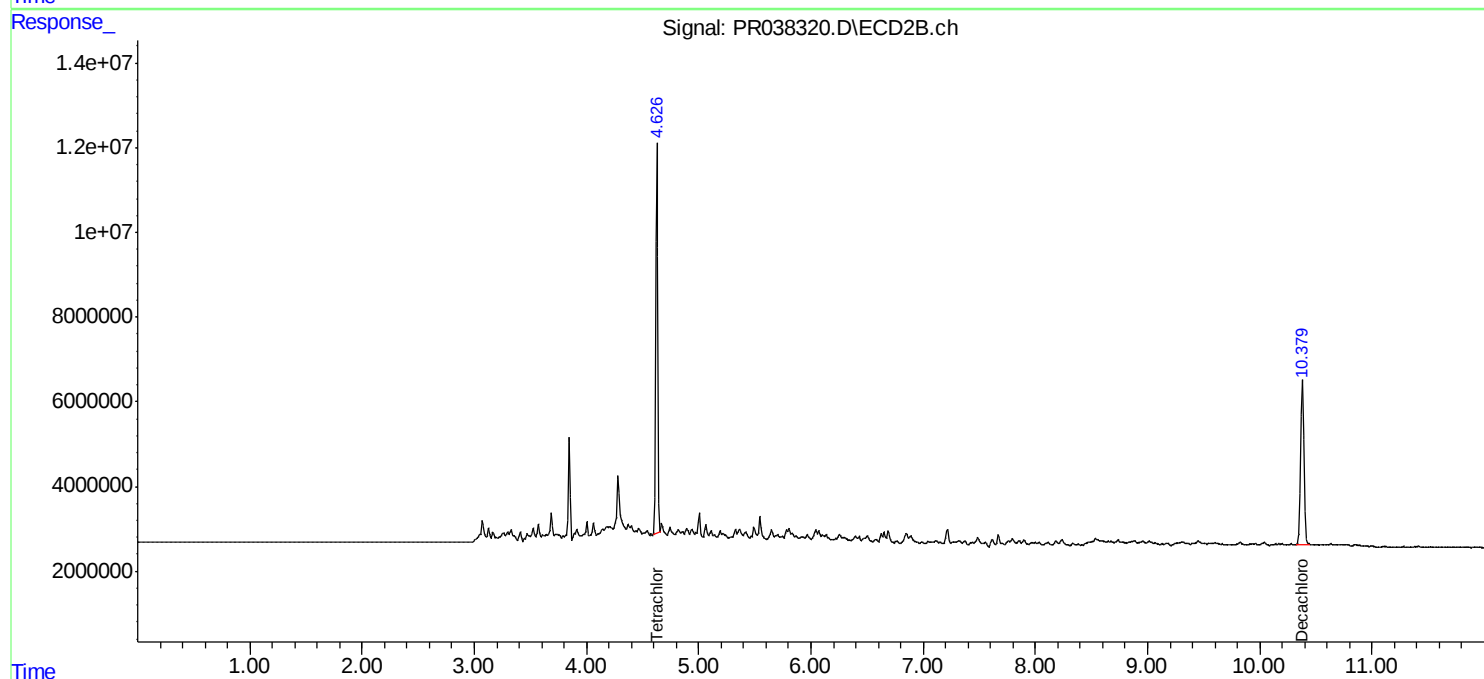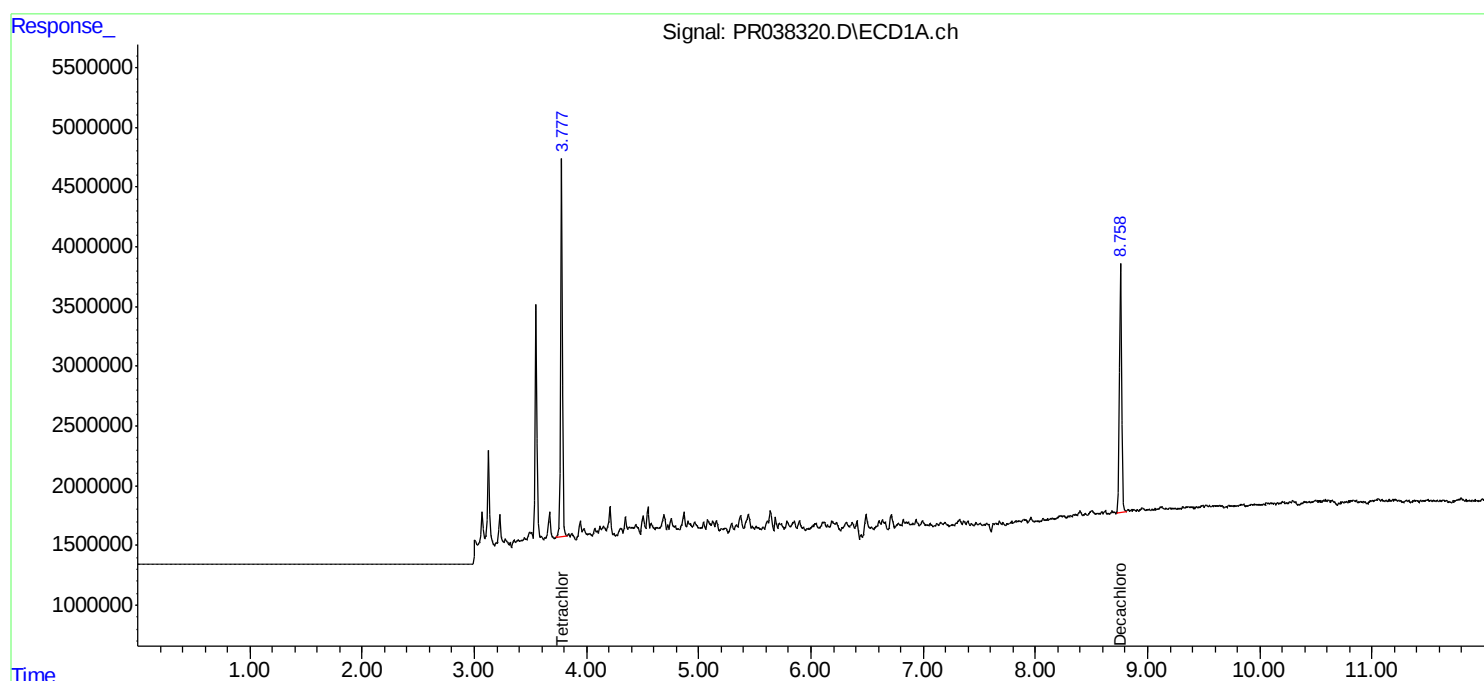

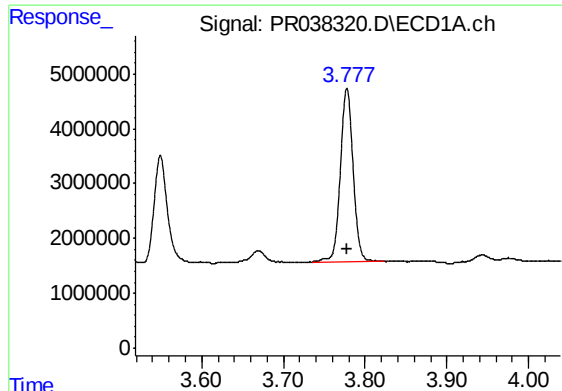


#1 Tetrachloro-m-xylene

R.T.: 3.777 min
Delta R.T.: 0.000 min
Response: 34474140
Conc: 20.56 ng/ml m

Instrument :
ECD_R
ClientSampleId :
052319-SBOA-E-U-B


Manual Integrations
APPROVED

Ankita
5/29/2019 2:10:48 PM

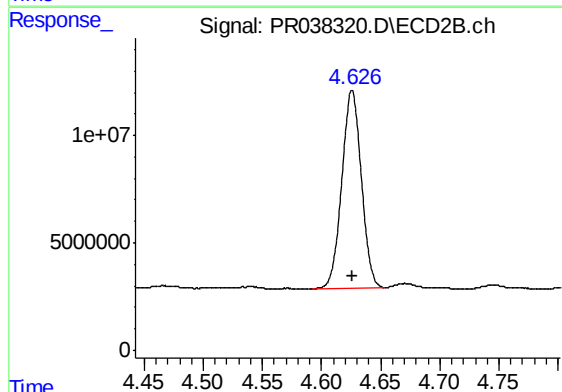


#1 Tetrachloro-m-xylene

R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 105794029
Conc: 20.85 ng/ml m

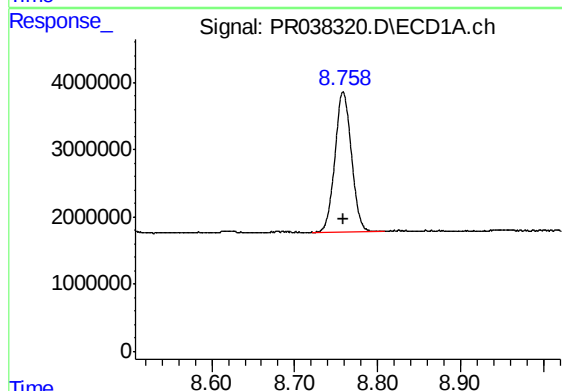

#2 Decachlorobiphenyl

R.T.: 8.759 min
Delta R.T.: 0.000 min
Response: 28939316
Conc: 14.92 ng/ml

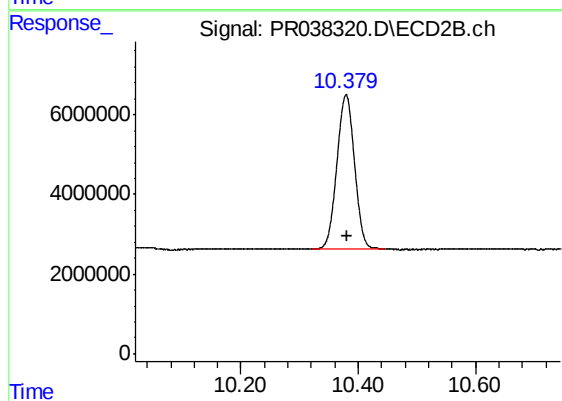

#2 Decachlorobiphenyl

R.T.: 10.380 min
Delta R.T.: -0.002 min
Response: 80695469
Conc: 18.29 ng/ml