

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR053119\
 Data File : PR038422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 20:14
 Operator : SM\MA
 Sample : K3111-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 FK-BPM-01-D1-D2-D1A-D2A

Manual Integrations
 APPROVED

Ankita
 6/3/2019 2:23:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 05:05:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR053019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 30 14:26:18 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.775	4.622	55108875	161.2E6	34.708	31.626
2) SA Decachlor...	8.752	10.375	40274690	108.8E6	25.624m	25.888

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR053119\
Data File : PR038422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 20:14
Operator : SM\MA
Sample : K3111-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
FK-BPM-01-D1-D2-D1A-D2A


Manual Integrations
APPROVED

Ankita
6/3/2019 2:23:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 05:05:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR053019.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 30 14:26:18 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

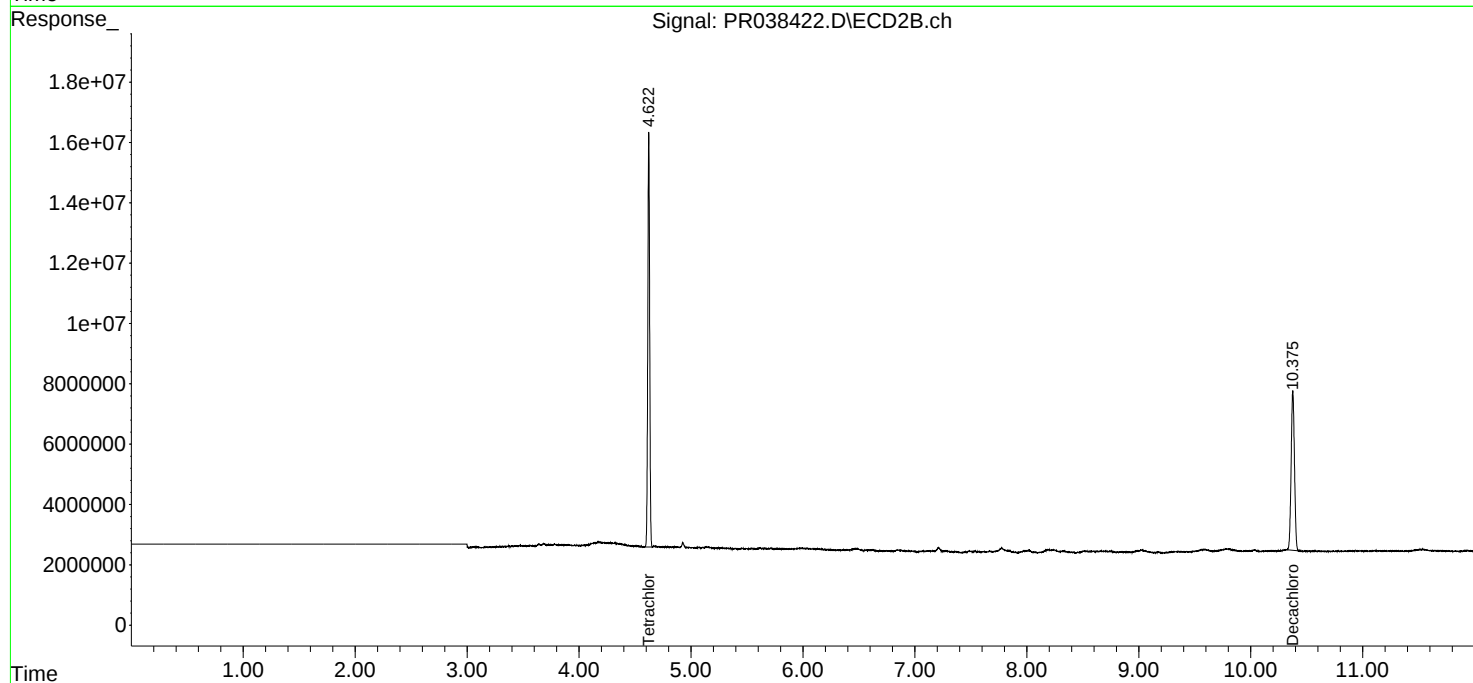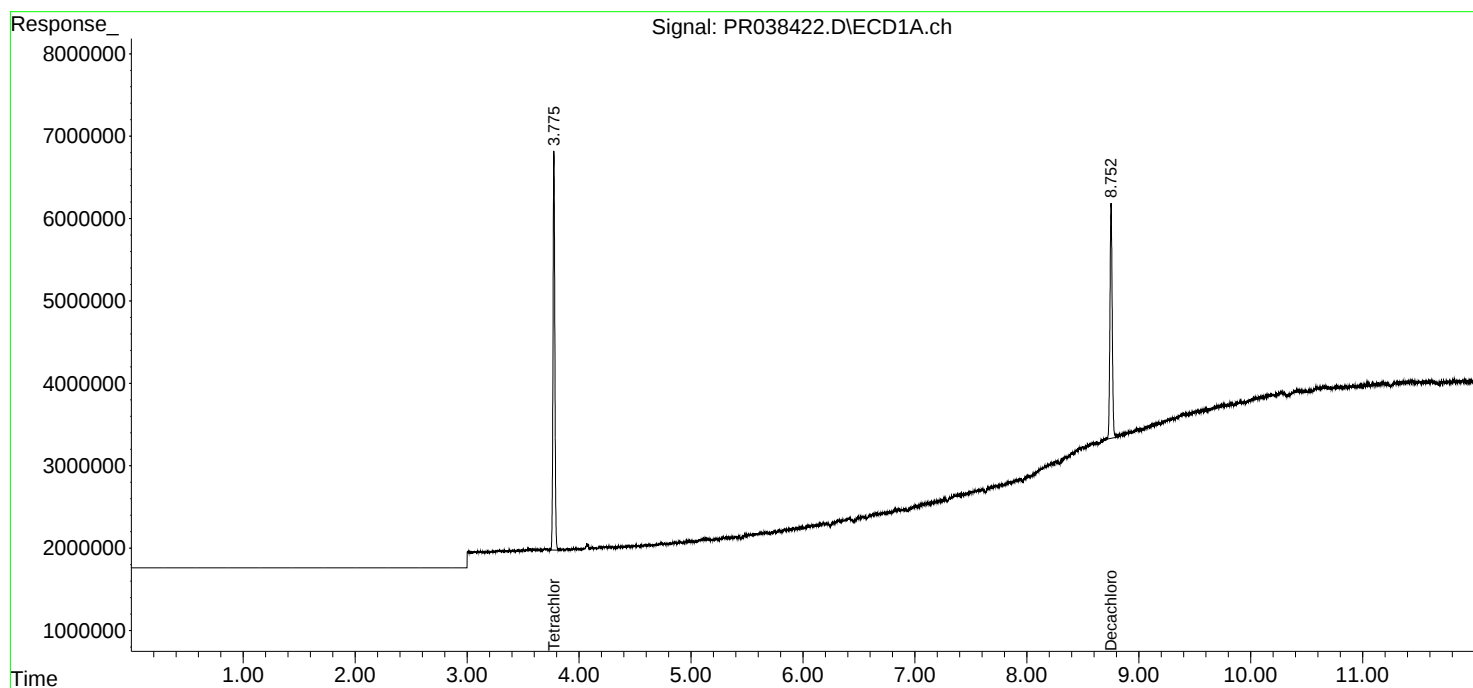

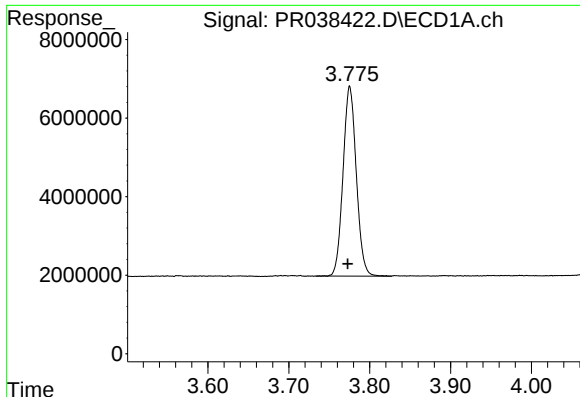


#1 Tetrachloro-m-xylene

R.T.: 3.775 min
Delta R.T.: 0.002 min
Response: 55108875
Conc: 34.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-BPM-01-D1-D2-D1A-D2A


Manual Integrations
APPROVED

Ankita
6/3/2019 2:23:38 PM

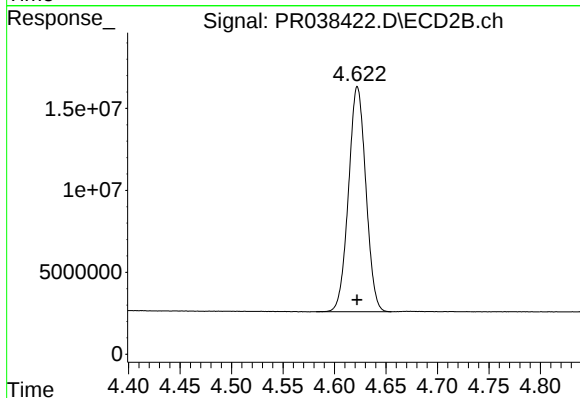


#1 Tetrachloro-m-xylene

R.T.: 4.622 min
Delta R.T.: 0.000 min
Response: 161202723
Conc: 31.63 ng/ml

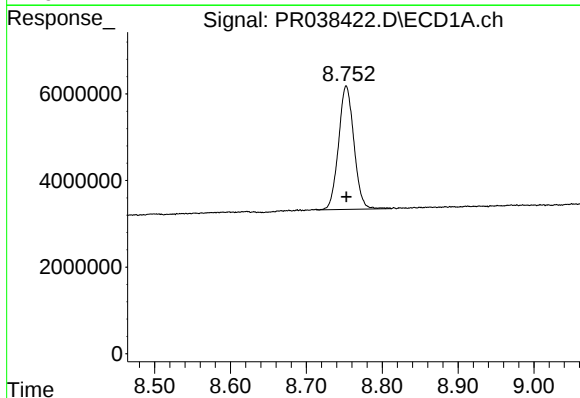

#2 Decachlorobiphenyl

R.T.: 8.752 min
Delta R.T.: 0.000 min
Response: 40274690
Conc: 25.62 ng/ml m

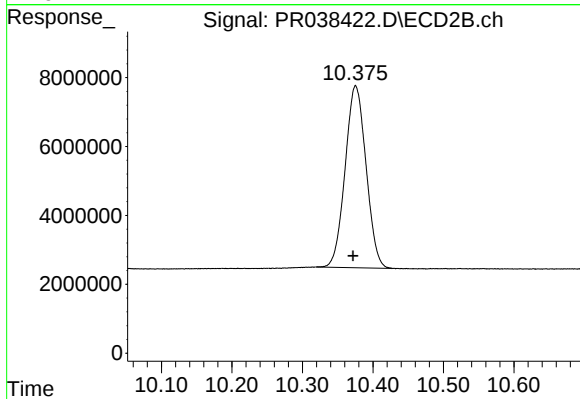

#2 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.004 min
Response: 108840296
Conc: 25.89 ng/ml