

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060619\
 Data File : PR038510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2019 09:49
 Operator : SM\MA
 Sample : K3097-23
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 0443-PR-6(PASSAIC)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 01:02:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 01:26:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.774	4.622	38005908	122.1E6	17.833	17.257
2)	SA Decachlor...	8.738	10.375	45523711	106.1E6	18.219	17.238

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060619\
Data File : PR038510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2019 09:49
Operator : SM\MA
Sample : K3097-23
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
0443-PR-6(PASSAIC)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 01:02:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060519.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 01:26:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

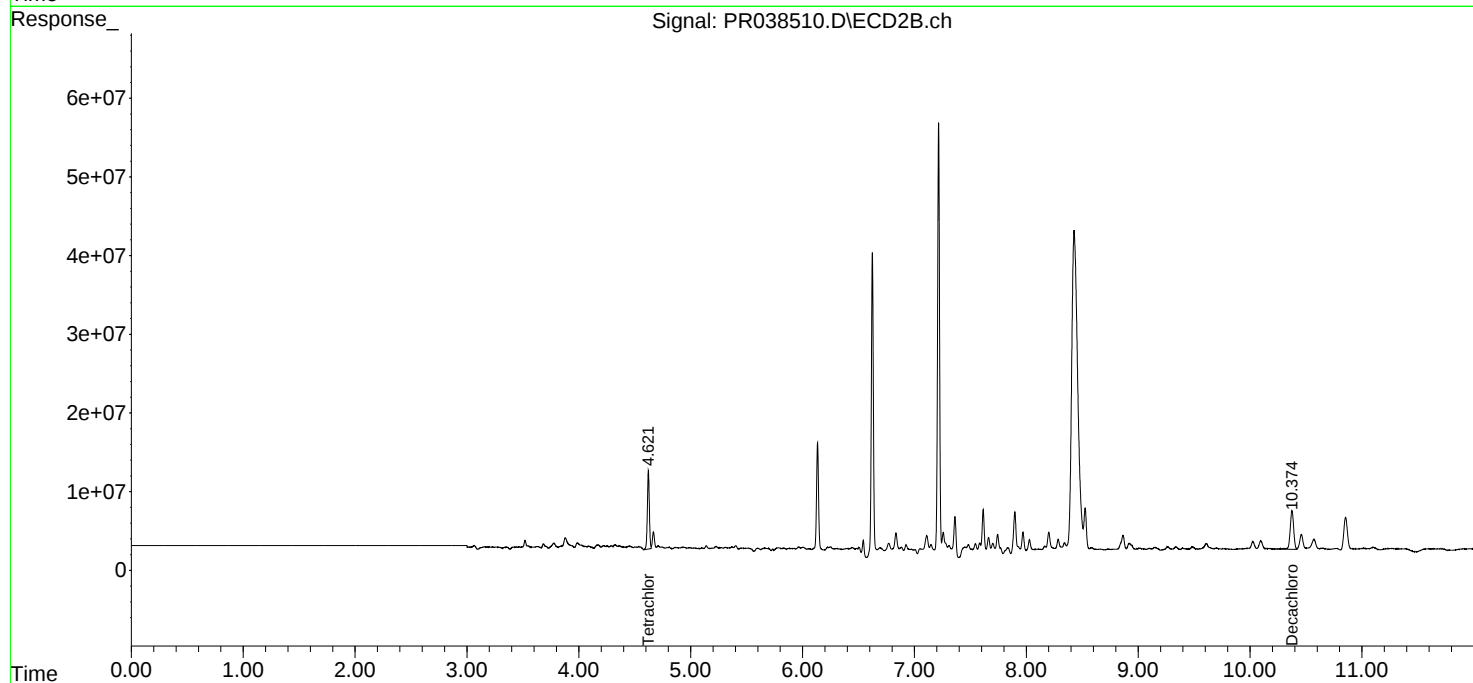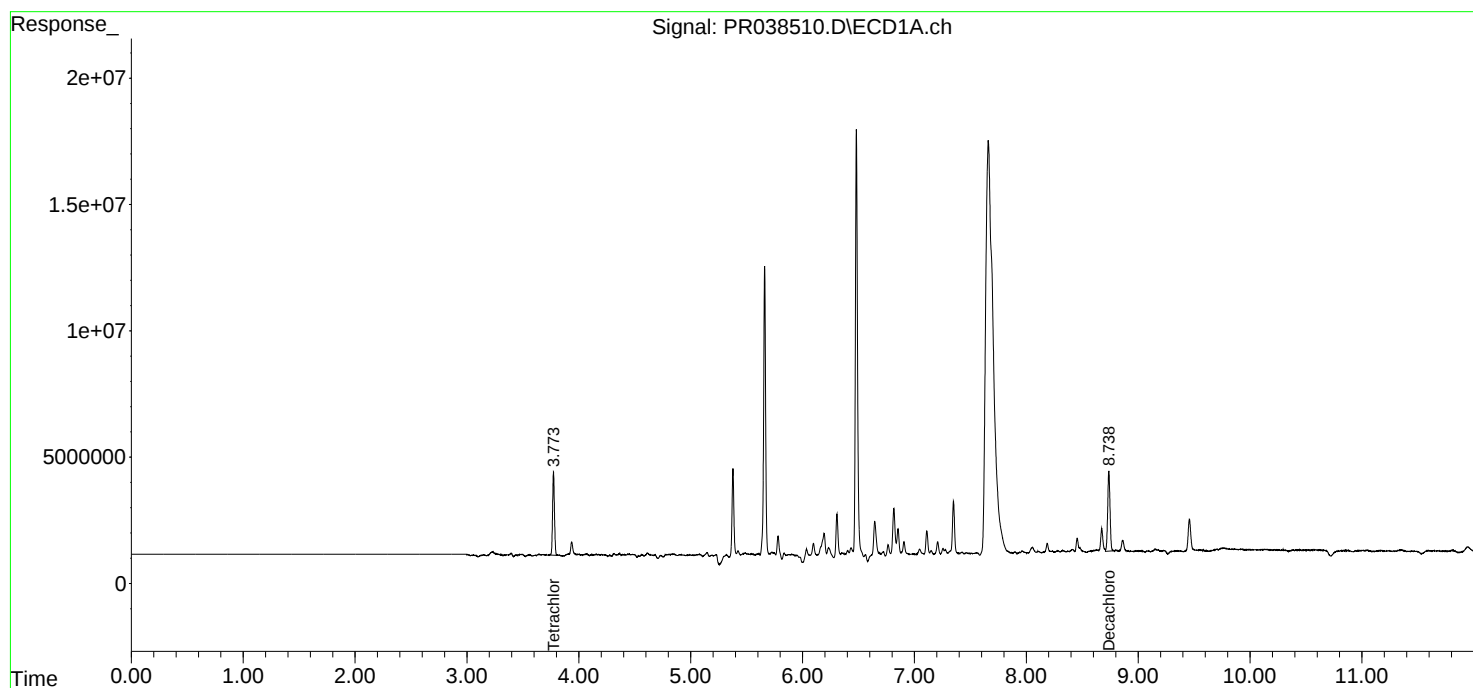


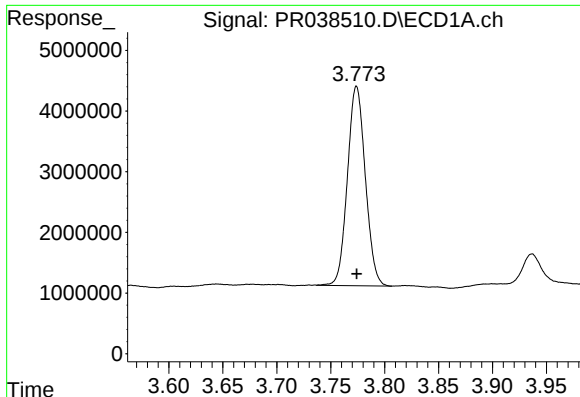

#1 Tetrachloro-m-xylene


R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 38005908
Conc: 17.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
0443-PR-6(PASSAIC)

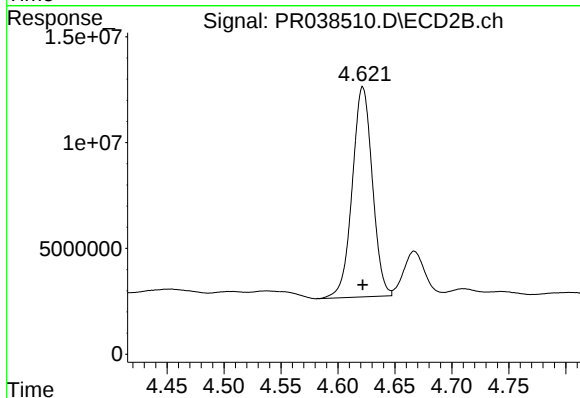


#1 Tetrachloro-m-xylene

R.T.: 4.622 min
Delta R.T.: 0.000 min
Response: 122079130
Conc: 17.26 ng/ml

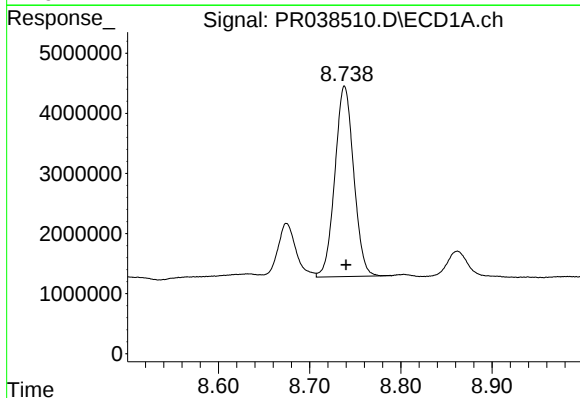

#2 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.002 min
Response: 45523711
Conc: 18.22 ng/ml

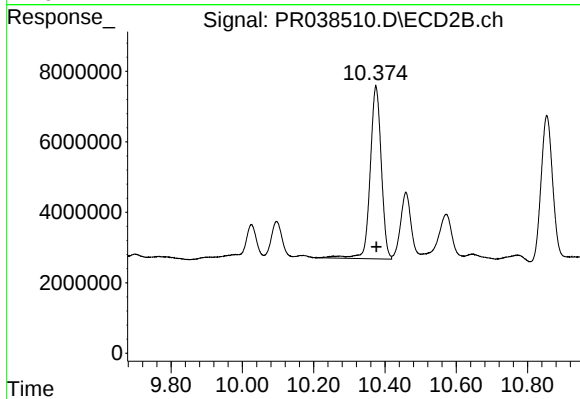

#2 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: -0.001 min
Response: 106077946
Conc: 17.24 ng/ml