

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060719\
 Data File : PR038587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2019 02:28
 Operator : SM\MA
 Sample : K3244-02
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 Q115-23A

Manual Integrations
 APPROVED

Ankita
 6/10/2019 2:59:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 04:23:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 01:26:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.774	4.620	39578149	124.3E6	18.571	17.575m
2) SA Decachlor...	8.731	10.370	24252565	69113542	9.706	11.231
Target Compounds						
31) L7 AR-1260-1	6.306	7.360	4071702	8999518	30.801m	26.190m
32) L7 AR-1260-2	6.490	7.612	4203111	82822430	24.644m	204.357 #
33) L7 AR-1260-3	6.642	7.967	4596254	6711668	30.443m	22.048 #
34) L7 AR-1260-4	7.109	8.195	1674959	13800033	12.958m	38.768m#
35) L7 AR-1260-5	7.346	8.525	4643699	8623325	13.626	11.865

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060719\
Data File : PR038587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2019 02:28
Operator : SM\MA
Sample : K3244-02
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
Q115-23A


Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 04:23:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060519.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 01:26:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

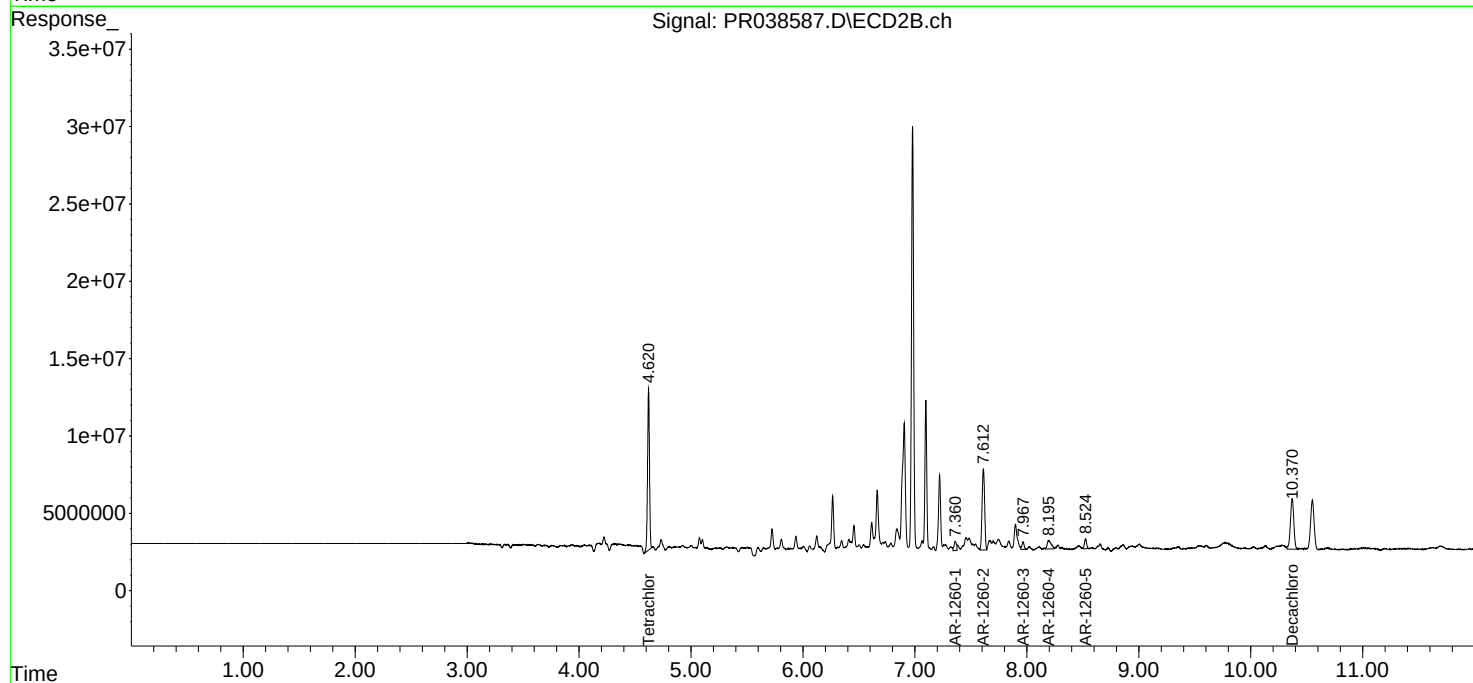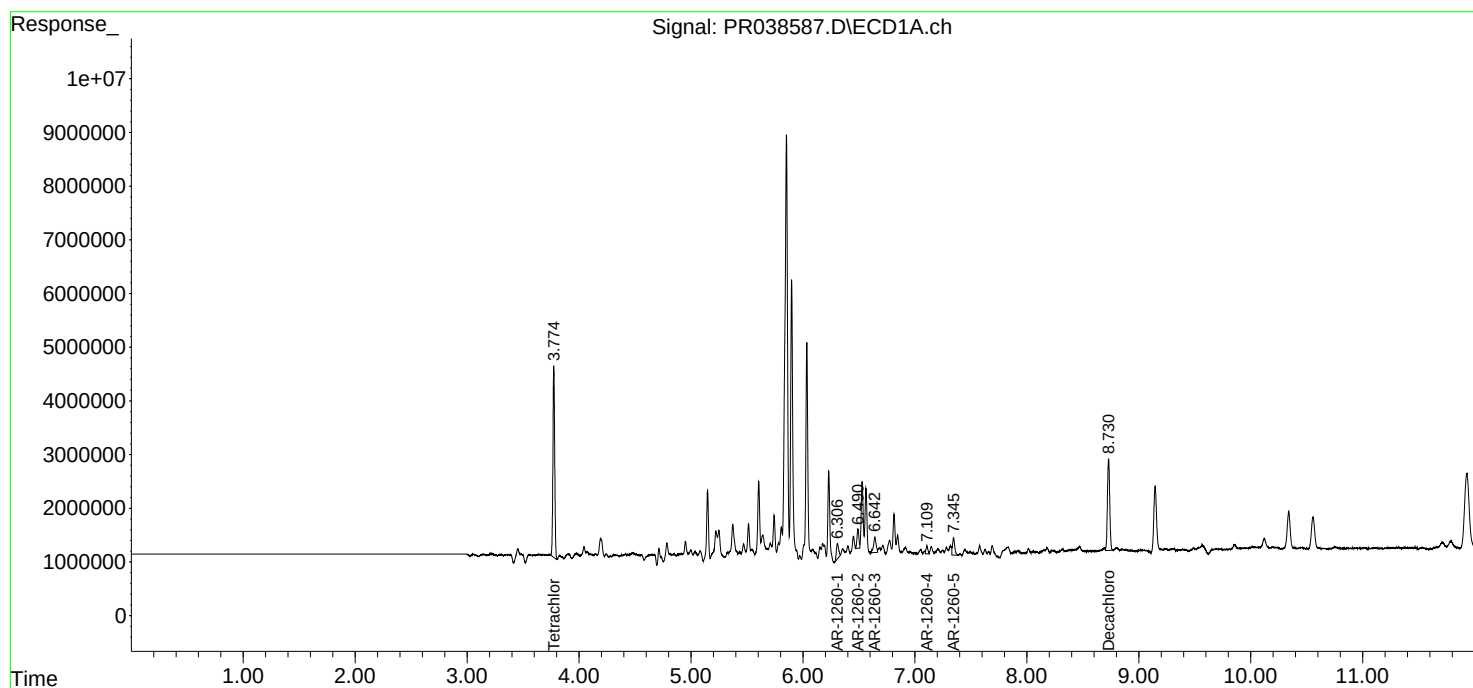

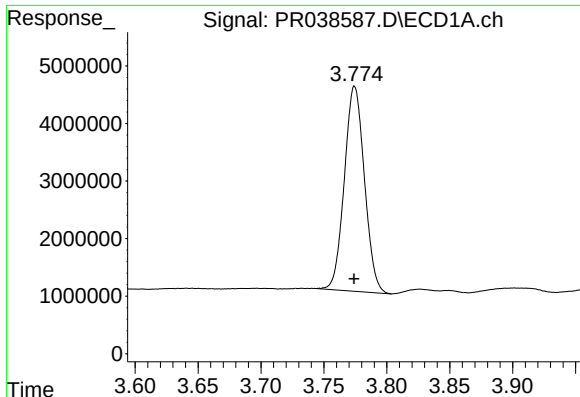


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 39578149
Conc: 18.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
Q115-23A


Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:46 PM

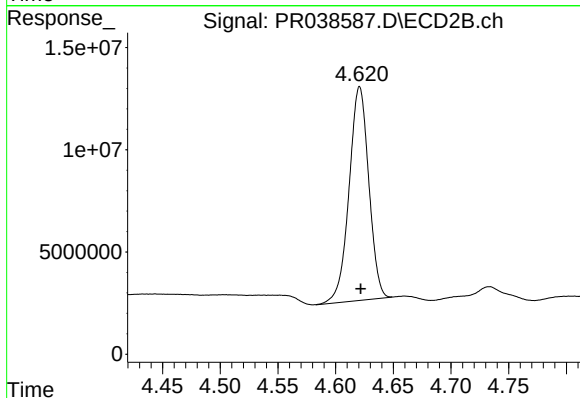


#1 Tetrachloro-m-xylene

R.T.: 4.620 min
Delta R.T.: -0.002 min
Response: 124332850
Conc: 17.58 ng/ml m

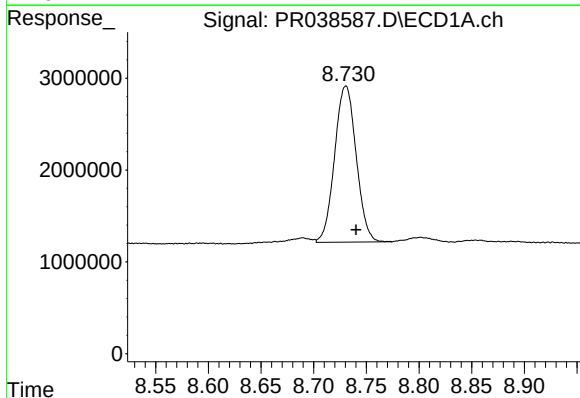


#2 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: -0.010 min
Response: 24252565
Conc: 9.71 ng/ml

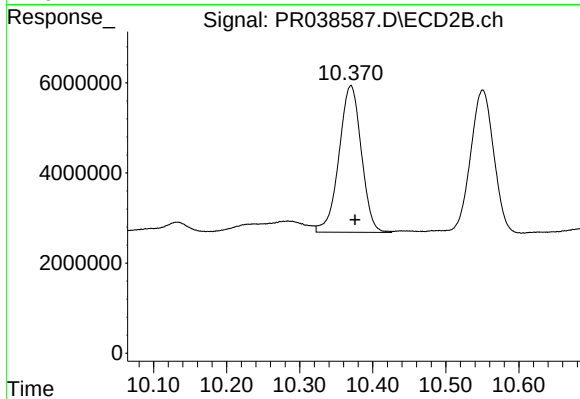

#2 Decachlorobiphenyl

R.T.: 10.370 min
Delta R.T.: -0.006 min
Response: 69113542
Conc: 11.23 ng/ml

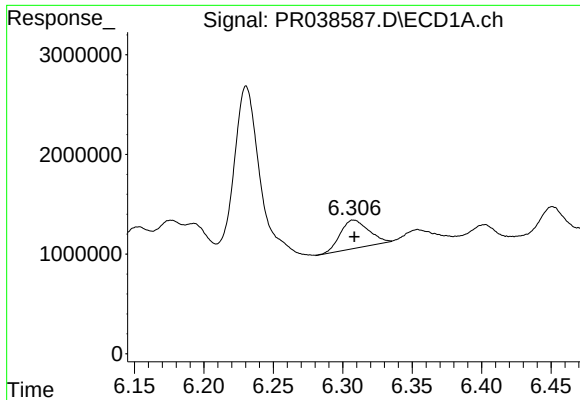


#31 AR-1260-1

R.T.: 6.306 min
Delta R.T.: -0.002 min
Response: 4071702
Conc: 30.80 ng/ml m

Instrument :
ECD_R
ClientSampleId :
Q115-23A


Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:46 PM

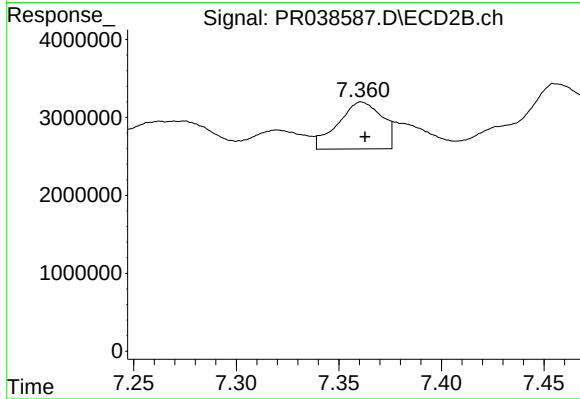


#31 AR-1260-1

R.T.: 7.360 min
Delta R.T.: -0.002 min
Response: 8999518
Conc: 26.19 ng/ml m

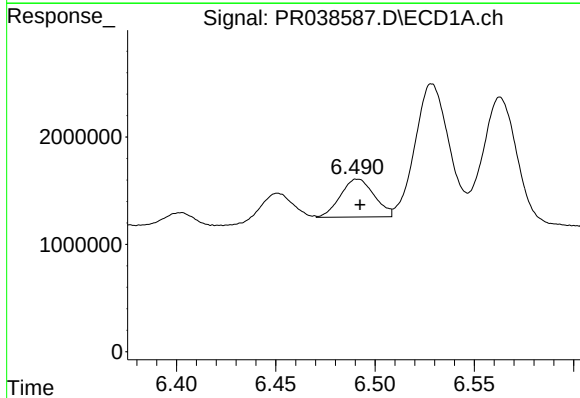


#32 AR-1260-2

R.T.: 6.490 min
Delta R.T.: -0.003 min
Response: 4203111
Conc: 24.64 ng/ml m

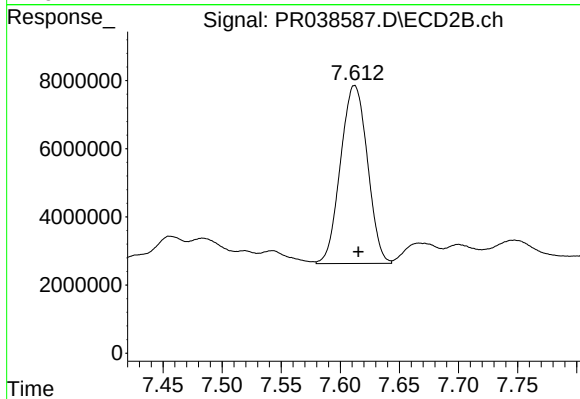

#32 AR-1260-2

R.T.: 7.612 min
Delta R.T.: -0.003 min
Response: 82822430
Conc: 204.36 ng/ml

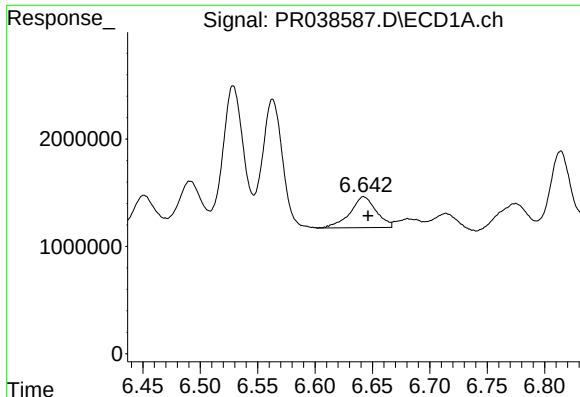


#33 AR-1260-3

R.T.: 6.642 min
Delta R.T.: -0.004 min
Response: 4596254
Conc: 30.44 ng/ml m

Instrument :
ECD_R
ClientSampleId :
Q115-23A


Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:46 PM

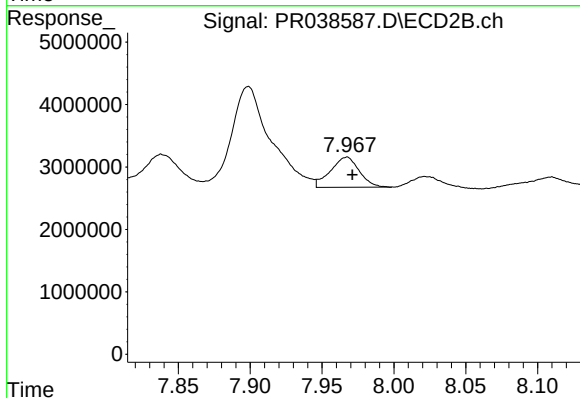


#33 AR-1260-3

R.T.: 7.967 min
Delta R.T.: -0.004 min
Response: 6711668
Conc: 22.05 ng/ml

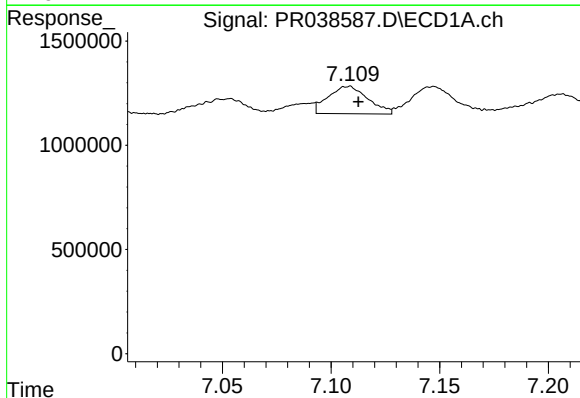


#34 AR-1260-4

R.T.: 7.109 min
Delta R.T.: -0.004 min
Response: 1674959
Conc: 12.96 ng/ml m

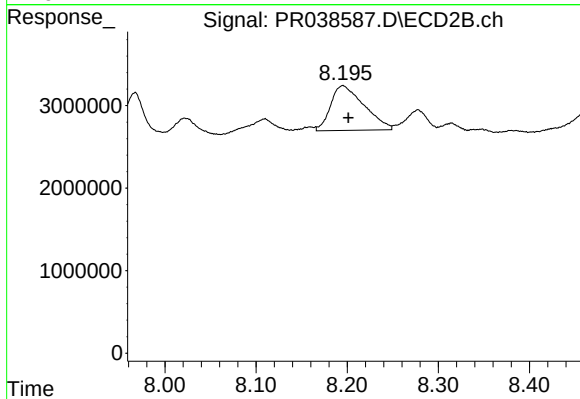

#34 AR-1260-4

R.T.: 8.195 min
Delta R.T.: -0.006 min
Response: 13800033
Conc: 38.77 ng/ml m

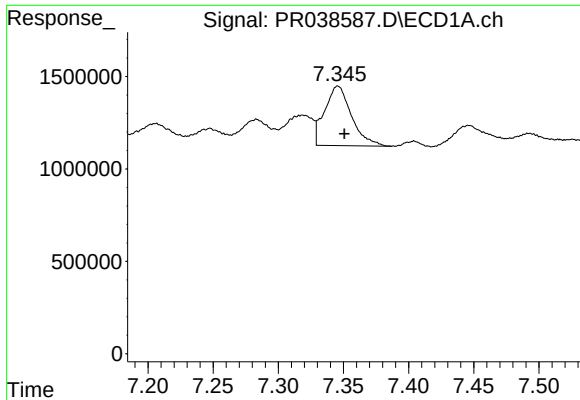


#35 AR-1260-5

R.T.: 7.346 min
Delta R.T.: -0.005 min
Response: 4643699
Conc: 13.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
Q115-23A

Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:46 PM

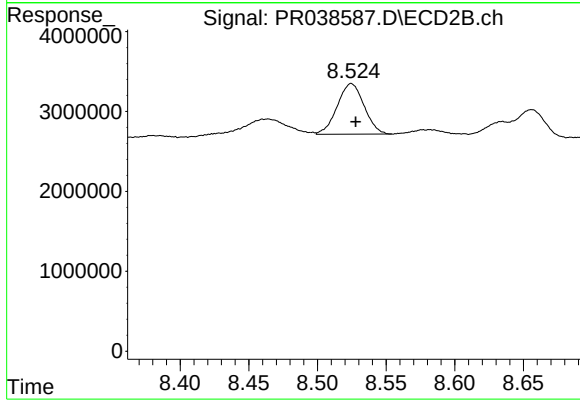

#35 AR-1260-5

R.T.: 8.525 min
Delta R.T.: -0.003 min
Response: 8623325
Conc: 11.86 ng/ml