

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060719\
 Data File : PR038588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2019 02:42
 Operator : SM\MA
 Sample : K3244-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 Q115-24A

Manual Integrations
 APPROVED

Ankita
 6/10/2019 2:59:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 04:24:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 01:26:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.774	4.621	44818050	141.3E6	21.030m	19.971m
2) SA Decachlor...	8.728	10.367	24013811	64734194	9.611m	10.519m
Target Compounds						
31) L7 AR-1260-1	6.306	7.361	4629152	12566845	35.018m	36.572
32) L7 AR-1260-2	6.491	7.609	5143802	112.3E6	30.160m	277.138 #
33) L7 AR-1260-3	6.641	7.965	4536089	8903313	30.045m	29.248
34) L7 AR-1260-4	7.108	8.195	1433587	14318820	11.091	40.225m#
35) L7 AR-1260-5	7.346	8.525	4933121	10650678	14.476	14.654

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060719\
Data File : PR038588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2019 02:42
Operator : SM\MA
Sample : K3244-05
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
Q115-24A


Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 04:24:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060519.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 01:26:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

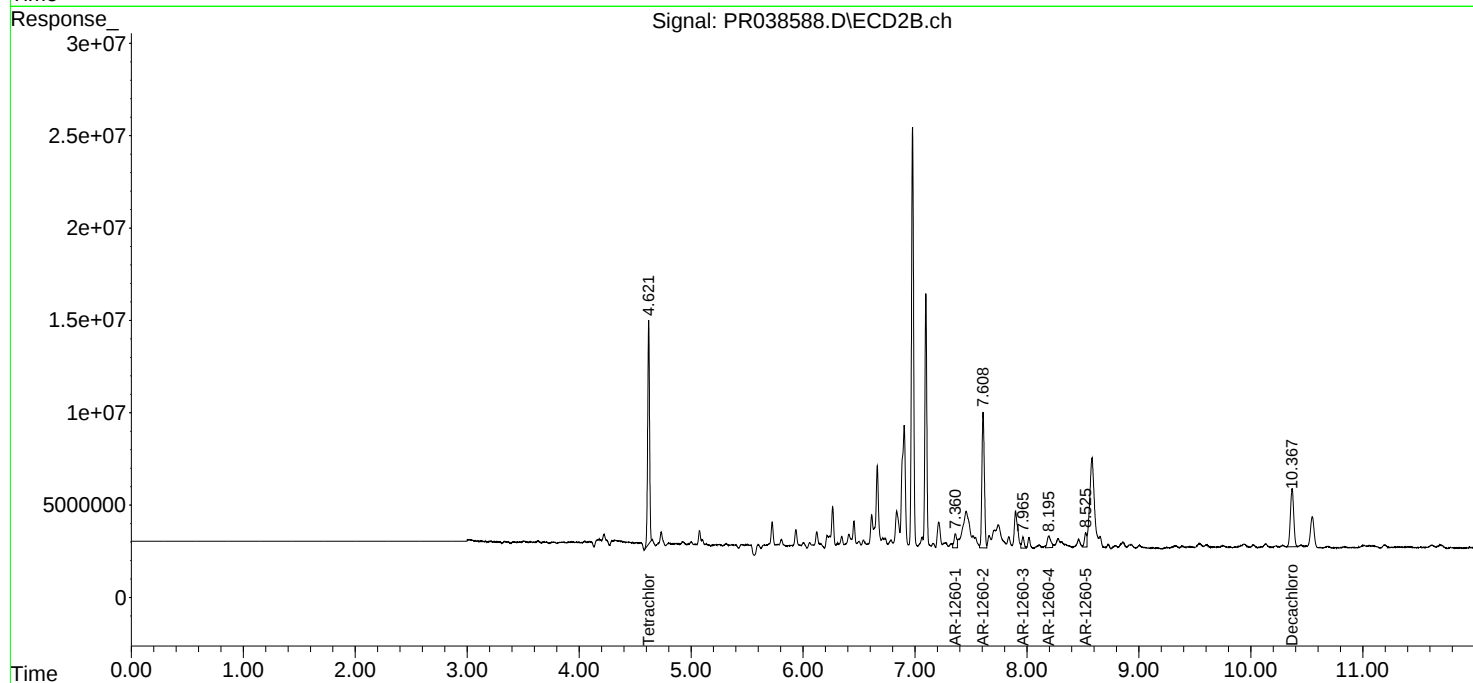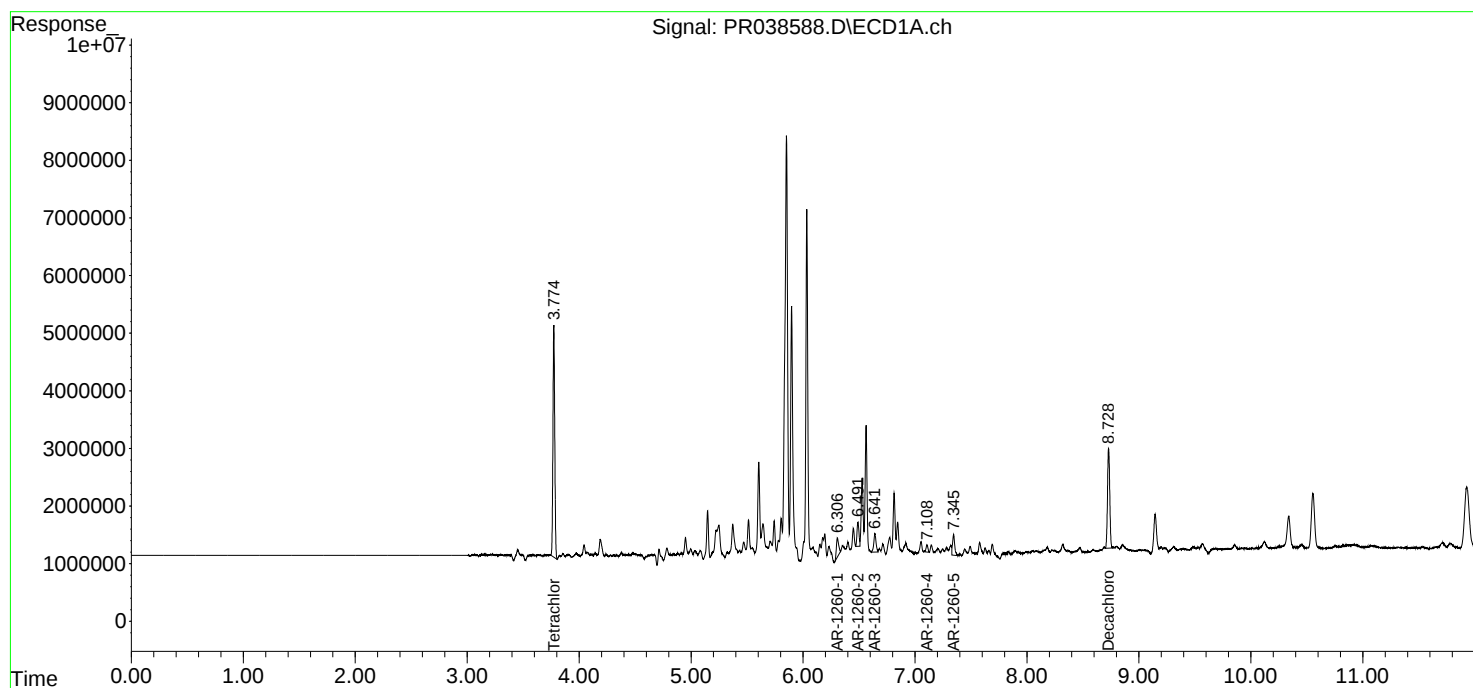

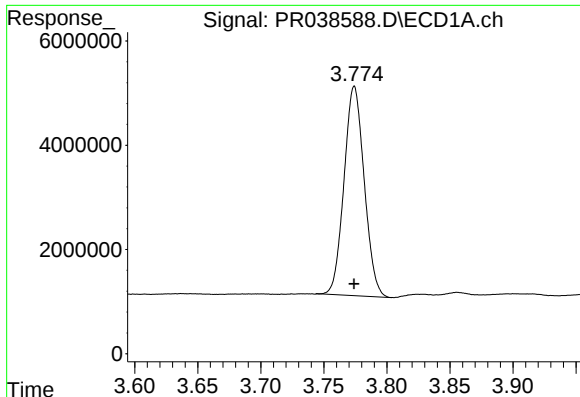


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: 0.000 min
Response: 44818050
Conc: 21.03 ng/ml m

Instrument :
ECD_R
ClientSampleId :
Q115-24A


Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:49 PM

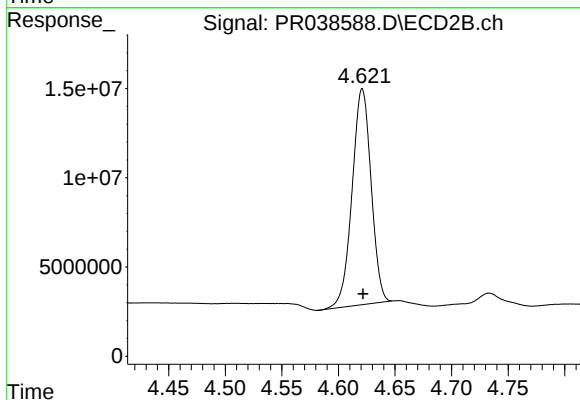


#1 Tetrachloro-m-xylene

R.T.: 4.621 min
Delta R.T.: -0.001 min
Response: 141278726
Conc: 19.97 ng/ml m

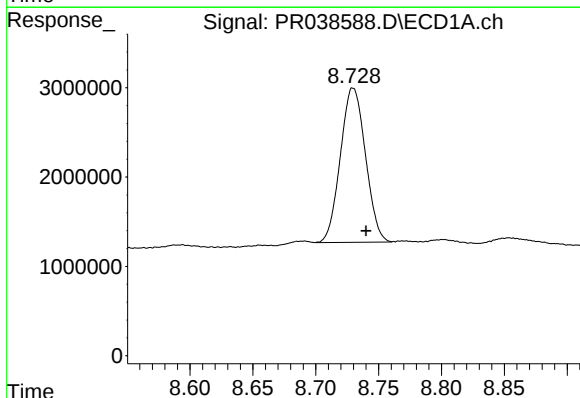


#2 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: -0.012 min
Response: 24013811
Conc: 9.61 ng/ml m

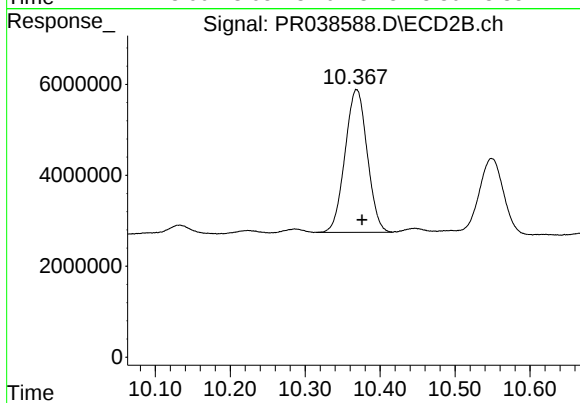

#2 Decachlorobiphenyl

R.T.: 10.367 min
Delta R.T.: -0.009 min
Response: 64734194
Conc: 10.52 ng/ml m

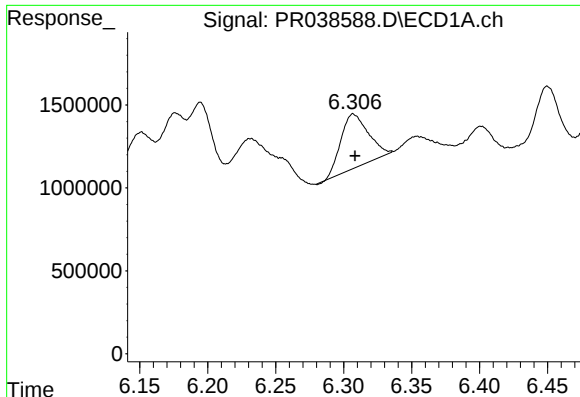


#31 AR-1260-1

R.T.: 6.306 min
Delta R.T.: -0.002 min
Response: 4629152
Conc: 35.02 ng/ml m

Instrument :
ECD_R
ClientSampleId :
Q115-24A


Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:49 PM

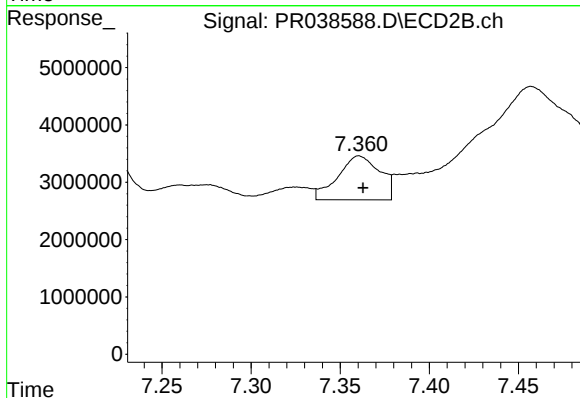


#31 AR-1260-1

R.T.: 7.361 min
Delta R.T.: -0.002 min
Response: 12566845
Conc: 36.57 ng/ml

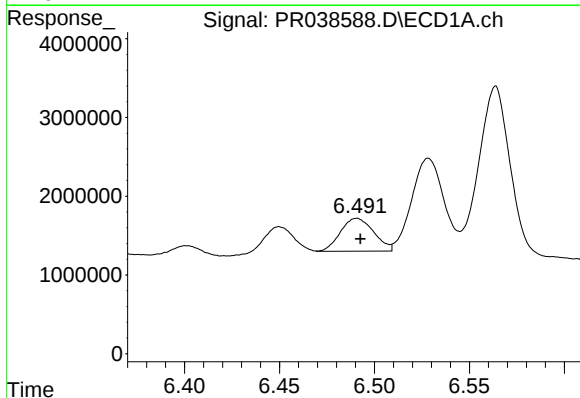


#32 AR-1260-2

R.T.: 6.491 min
Delta R.T.: -0.002 min
Response: 5143802
Conc: 30.16 ng/ml m

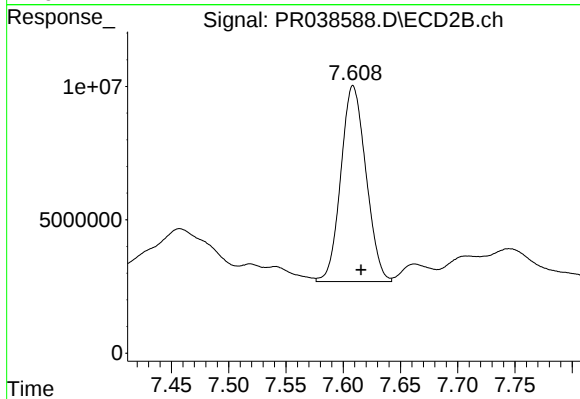

#32 AR-1260-2

R.T.: 7.609 min
Delta R.T.: -0.007 min
Response: 112319312
Conc: 277.14 ng/ml

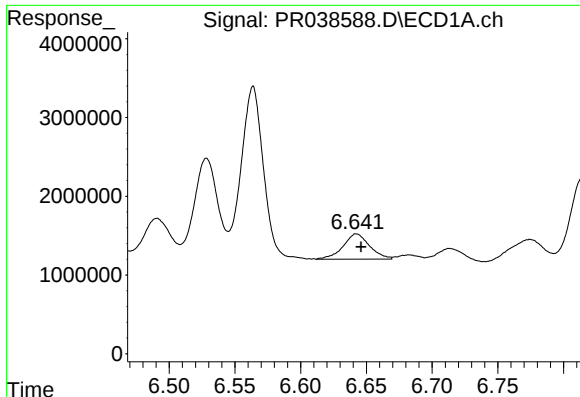


#33 AR-1260-3

R.T.: 6.641 min
Delta R.T.: -0.005 min
Response: 4536089
Conc: 30.04 ng/ml m

Instrument :
ECD_R
ClientSampleId :
Q115-24A


Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:49 PM

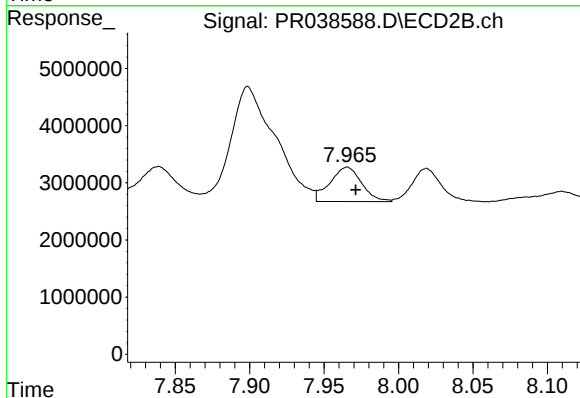


#33 AR-1260-3

R.T.: 7.965 min
Delta R.T.: -0.006 min
Response: 8903313
Conc: 29.25 ng/ml

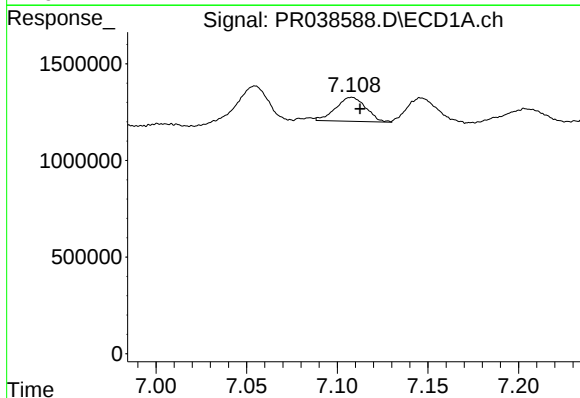


#34 AR-1260-4

R.T.: 7.108 min
Delta R.T.: -0.005 min
Response: 1433587
Conc: 11.09 ng/ml

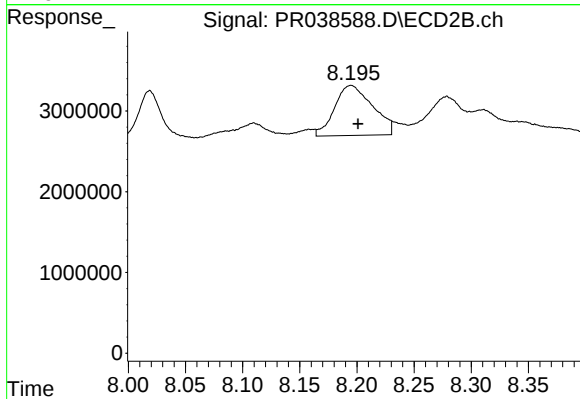

#34 AR-1260-4

R.T.: 8.195 min
Delta R.T.: -0.007 min
Response: 14318820
Conc: 40.22 ng/ml m

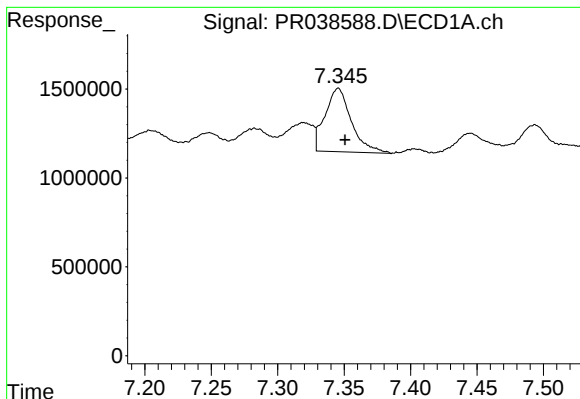


#35 AR-1260-5

R.T.: 7.346 min
Delta R.T.: -0.005 min
Response: 4933121
Conc: 14.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
Q115-24A

Manual Integrations
APPROVED

Ankita
6/10/2019 2:59:49 PM

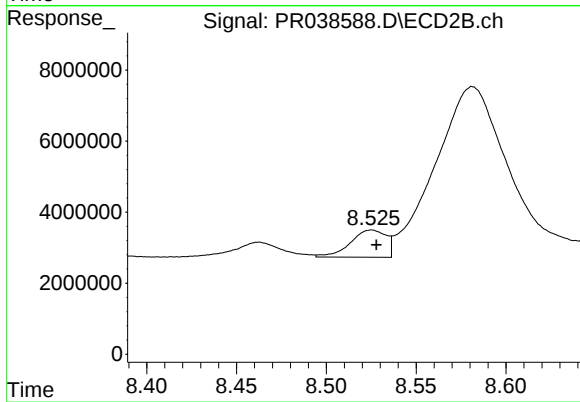

#35 AR-1260-5

R.T.: 8.525 min
Delta R.T.: -0.003 min
Response: 10650678
Conc: 14.65 ng/ml