

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060719\
 Data File : PR038591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2019 03:25
 Operator : SM\MA
 Sample : K3244-13
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 Q115-DUP6

Manual Integrations
 APPROVED

Ankita
 6/10/2019 3:00:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 04:26:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 01:26:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.775	4.621	36124455	113.6E6	16.950	16.062
2) SA Decachlor...	8.729	10.368	17089812	51860253	6.839m	8.427

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060719\
Data File : PR038591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2019 03:25
Operator : SM\MA
Sample : K3244-13
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
Q115-DUP6


Manual Integrations
APPROVED

Ankita
6/10/2019 3:00:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 04:26:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR060519.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 01:26:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

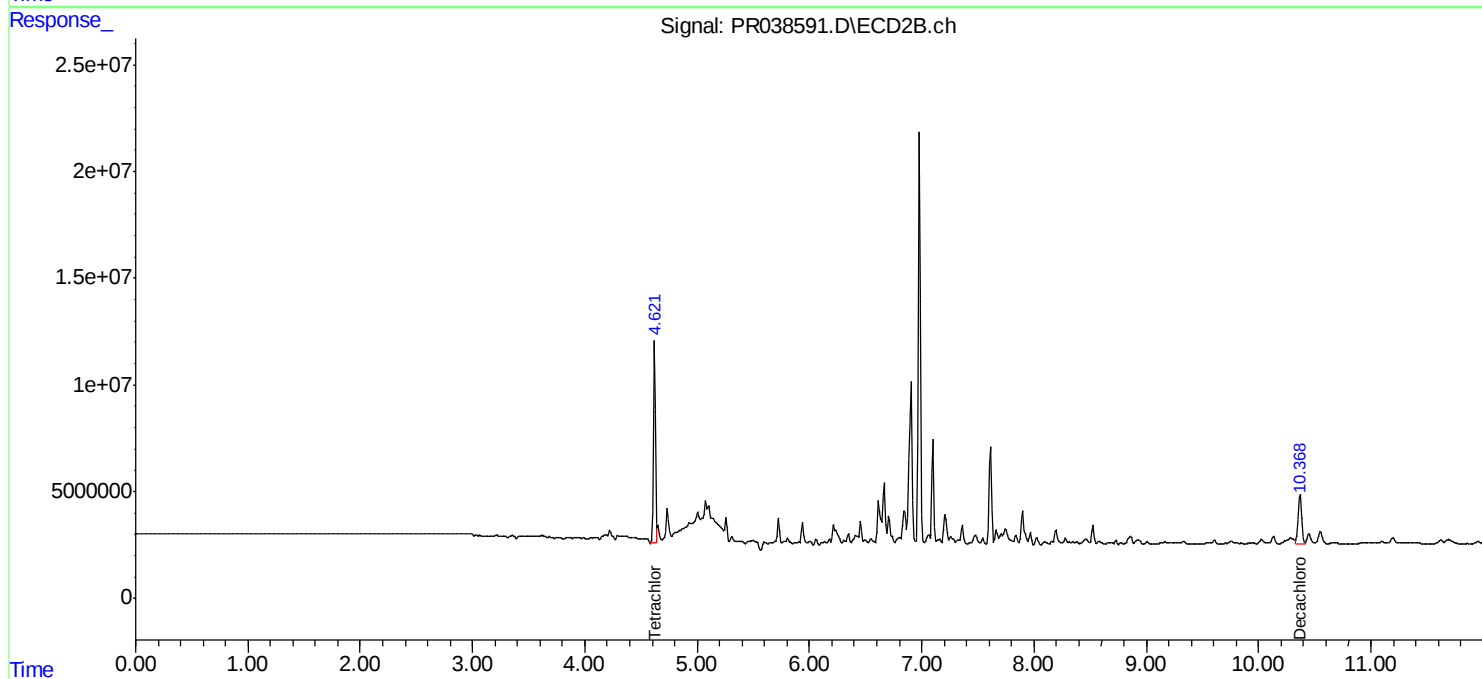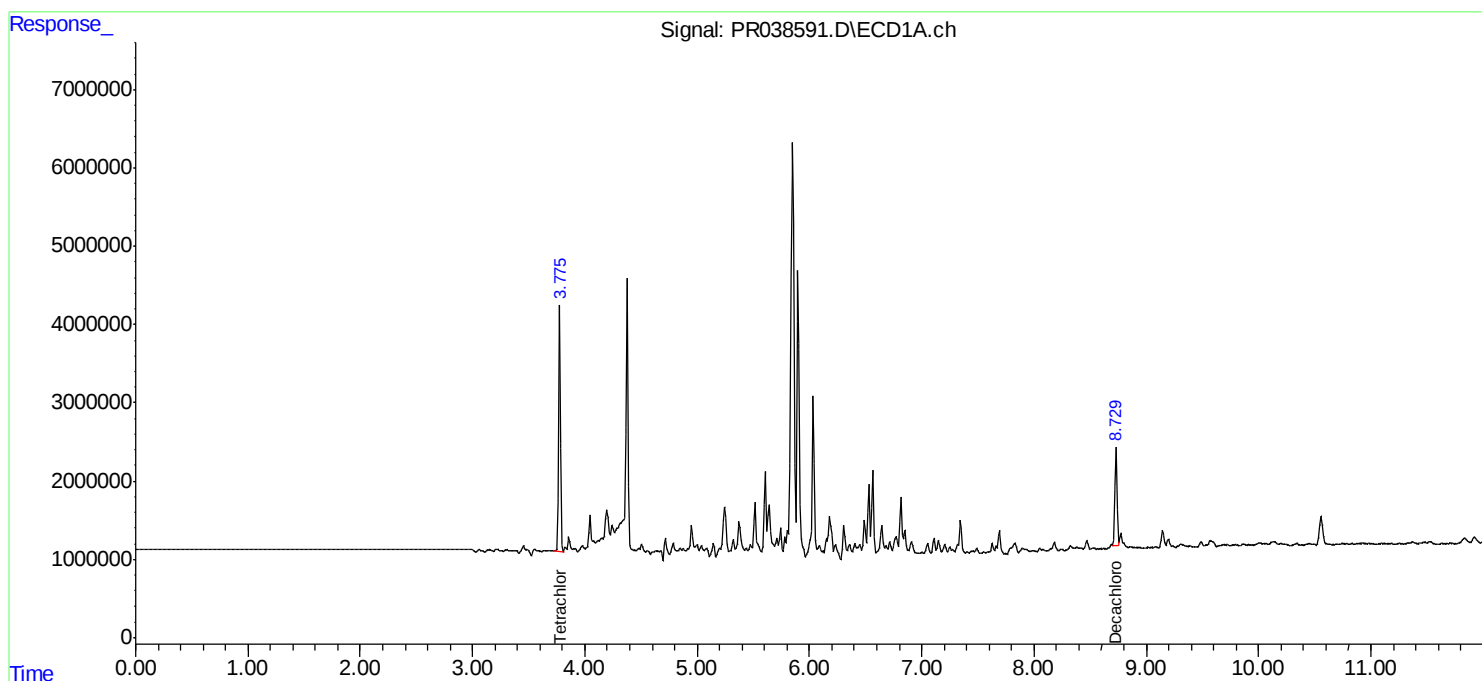

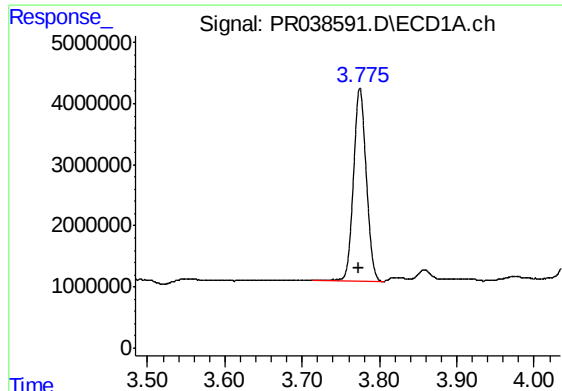


#1 Tetrachloro-m-xylene

R.T.: 3.775 min
Delta R.T.: 0.000 min
Response: 36124455
Conc: 16.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
Q115-DUP6


Manual Integrations
APPROVED

Ankita
6/10/2019 3:00:04 PM

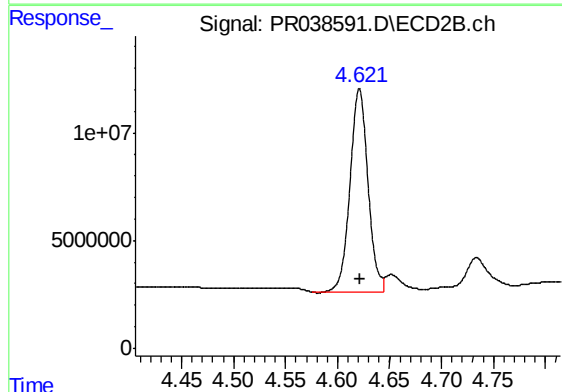


#1 Tetrachloro-m-xylene

R.T.: 4.621 min
Delta R.T.: 0.000 min
Response: 113626282
Conc: 16.06 ng/ml

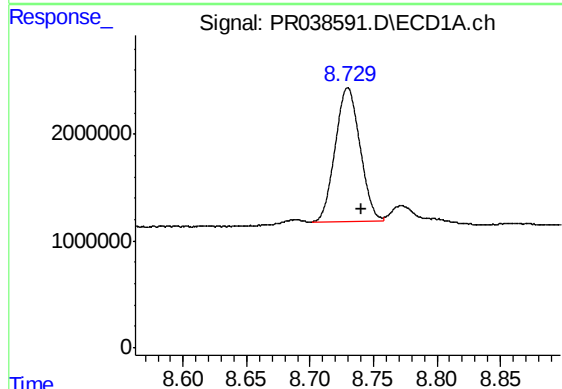

#2 Decachlorobiphenyl

R.T.: 8.729 min
Delta R.T.: -0.011 min
Response: 17089812
Conc: 6.84 ng/ml m

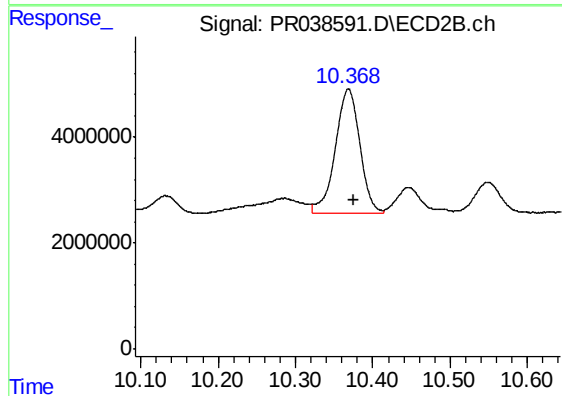

#2 Decachlorobiphenyl

R.T.: 10.368 min
Delta R.T.: -0.007 min
Response: 51860253
Conc: 8.43 ng/ml