

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061120\
 Data File : PQ048360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2020 20:41
 Operator : AJ\MA
 Sample : L2965-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MASON-BRICK-COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 08:10:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 10 03:52:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.296	4.291	126.2E6	61655432	14.771	14.927
2)	SA Decachlor...	11.566	9.656	154.0E6	91951114	16.607	20.544
Target Compounds							
3)	L1 AR-1016-1	6.626	5.556	47063433	15022407	157.587	96.569 #
4)	L1 AR-1016-2	6.650	5.576	60387095	21881425	147.861	103.432 #
5)	L1 AR-1016-3	6.717	5.769	42637303	13619903	168.665	125.391 #
6)	L1 AR-1016-4	6.826	5.818	39257537	12157887	190.324	135.995 #
7)	L1 AR-1016-5	7.140	6.051	45585939	11463321	230.514	117.324 #
8)	L2 AR-1221-1	5.537	4.550	24706727	7482302	276.591	173.613 #
9)	L2 AR-1221-2	5.651	4.648	21346192	11155512	313.101	342.124
10)	L2 AR-1221-3	5.735	4.739	32312749	17373821	153.752	170.533
11)	L3 AR-1232-1	5.735	4.739	32312749	17373821	191.473	212.905
12)	L3 AR-1232-2	6.306	5.576	69780784	21881425	814.550	256.251 #
13)	L3 AR-1232-3	6.650	5.769	60387095	13619903	360.832	315.816
14)	L3 AR-1232-4	6.826	5.865	39257537	13909675	462.690	354.846
15)	L3 AR-1232-5	6.915	6.051	67455007	11463321	1064.577	293.892 #
16)	L4 AR-1242-1	6.626	5.556	47063433	15022407	207.893	130.393 #
17)	L4 AR-1242-2	6.650	5.576	60387095	21881425	195.612	138.848 #
18)	L4 AR-1242-3	6.717	5.769	42637303	13619903	222.609	165.988 #
19)	L4 AR-1242-4	6.826	5.865	39257537	13909675	247.590	172.077 #
20)	L4 AR-1242-5	7.611	6.431	61068977	32608192	359.408	304.713
21)	L5 AR-1248-1	6.626	5.556	47063433	15022407	271.173	170.062 #
22)	L5 AR-1248-2	6.915	5.818	67455007	12157887	303.261	108.372 #
23)	L5 AR-1248-3	7.140	5.865	45585939	13909675	186.811	122.246 #
24)	L5 AR-1248-4	7.570	6.051	63580768	11463321	229.889	84.505 #
25)	L5 AR-1248-5	7.611	6.474	61068977	23319312	232.294	169.481 #
26)	L6 AR-1254-1	7.541	6.431	49607047	32608192	165.601	138.017
27)	L6 AR-1254-2	7.779	6.588	60704819	8889579	131.177	43.346 #
28)	L6 AR-1254-3	8.155	7.011	27859238	11186829	57.161	33.333 #
29)	L6 AR-1254-4	8.450	7.249	19212144	9830522	50.743	44.762
30)	L6 AR-1254-5	8.881	7.674	18093337	21952561	45.270	75.146 #
31)	L7 AR-1260-1	8.320	7.154	5937752	7482829	17.708	37.258 #
32)	L7 AR-1260-2	8.580	7.343	25779804	3518142	64.262	14.205 #
33)	L7 AR-1260-3	8.964	7.499	39193024	4409819	124.040	19.558 #
34)	L7 AR-1260-4	9.199	7.983	5111755	1841997	13.852	9.595 #
35)	L7 AR-1260-5	9.556	8.229	5477040	1939707	6.449	4.058 #
36)	L8 AR-1262-1	8.964	7.674	39193024	21952561	90.342	155.122 #
37)	L8 AR-1262-2	9.556	8.229	5477040	1939707	6.602	3.680 #
38)	L8 AR-1262-3	9.889	8.551	5794789	170.9E6	14.959	794.636 #
39)	L8 AR-1262-4	10.024	8.551	11202134	170.9E6	24.712	444.024 #
40)	L8 AR-1262-5	0.000	9.088	0	3110573	N.D.	16.935 #
41)	L9 AR-1268-1	9.889	8.551	5794789	170.9E6	5.109	249.029 #
42)	L9 AR-1268-2	10.024	8.551	11202134	170.9E6	10.259	269.000 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061120\
 Data File : PQ048360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2020 20:41
 Operator : AJ\MA
 Sample : L2965-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1


Instrument :
 ECD_R
 ClientSampleId :
 MASON-BRICK-COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 08:10:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 10 03:52:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	10.251	8.797	-40338	1863070	N.D.	3.519 #
44) L9	AR-1268-4	0.000	9.088	0	3110573	N.D.	13.351 #
45) L9	AR-1268-5	11.191	9.369	4215849	11563397	1.324	6.605 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

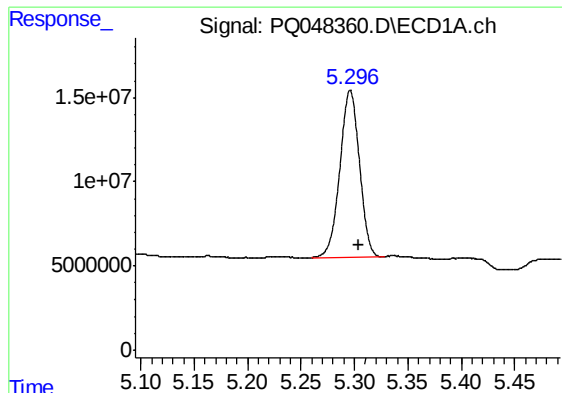

#1 Tetrachloro-m-xylene


R.T.: 5.296 min
Delta R.T.: -0.008 min
Response: 126223067
Conc: 14.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

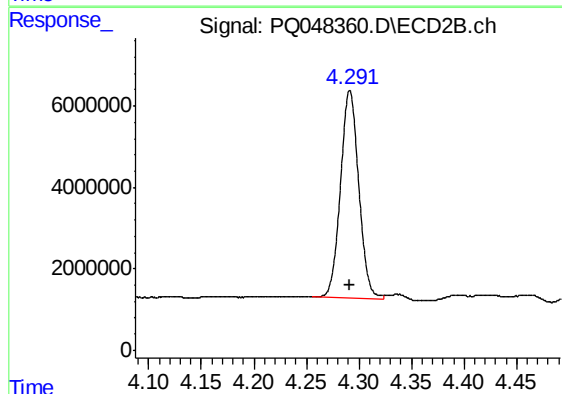


#1 Tetrachloro-m-xylene

R.T.: 4.291 min
Delta R.T.: 0.000 min
Response: 61655432
Conc: 14.93 ng/ml

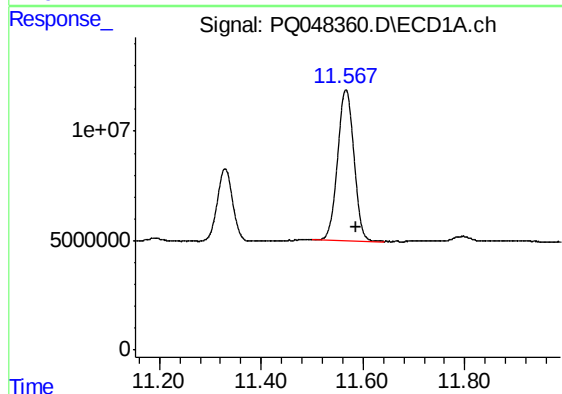


#2 Decachlorobiphenyl

R.T.: 11.566 min
Delta R.T.: -0.020 min
Response: 153989602
Conc: 16.61 ng/ml

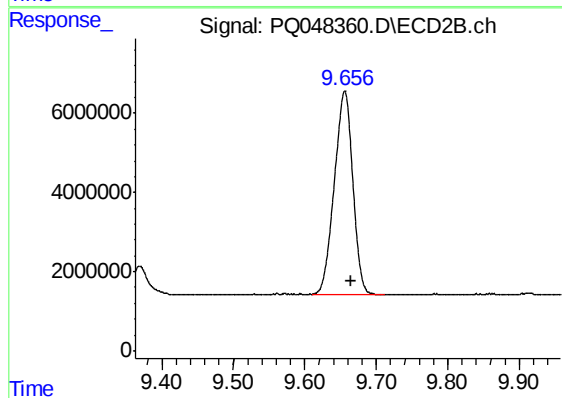

#2 Decachlorobiphenyl


R.T.: 9.656 min
Delta R.T.: -0.009 min
Response: 91951114
Conc: 20.54 ng/ml



#3 AR-1016-1


R.T.: 6.626 min
Delta R.T.: -0.009 min
Response: 47063433
Conc: 157.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#3 AR-1016-1

R.T.: 5.556 min
Delta R.T.: -0.001 min
Response: 15022407
Conc: 96.57 ng/ml




#4 AR-1016-2

R.T.: 6.650 min
Delta R.T.: -0.009 min
Response: 60387095
Conc: 147.86 ng/ml

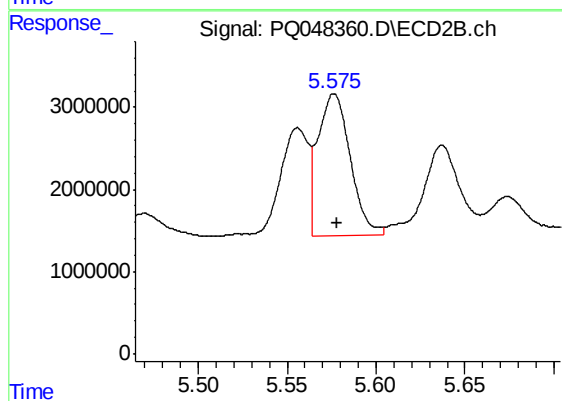

#4 AR-1016-2


R.T.: 5.576 min
Delta R.T.: -0.002 min
Response: 21881425
Conc: 103.43 ng/ml

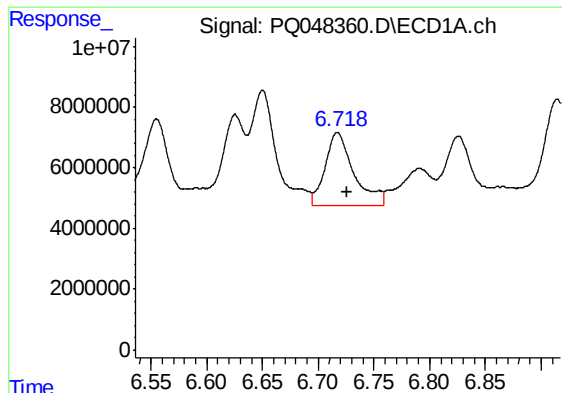

#5 AR-1016-3


R.T.: 6.717 min
Delta R.T.: -0.008 min
Response: 42637303
Conc: 168.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

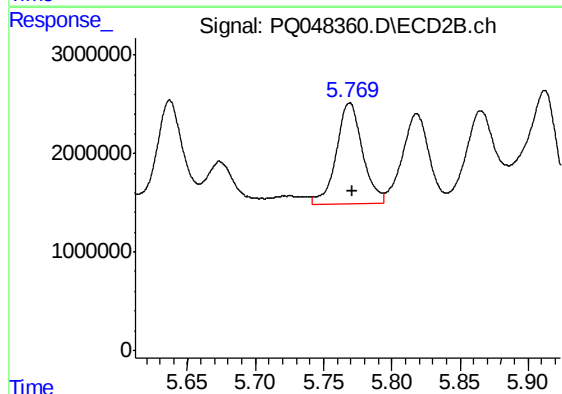


#5 AR-1016-3

R.T.: 5.769 min
Delta R.T.: -0.002 min
Response: 13619903
Conc: 125.39 ng/ml

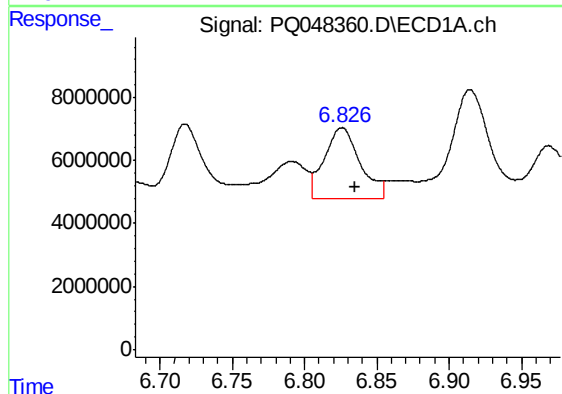


#6 AR-1016-4

R.T.: 6.826 min
Delta R.T.: -0.008 min
Response: 39257537
Conc: 190.32 ng/ml

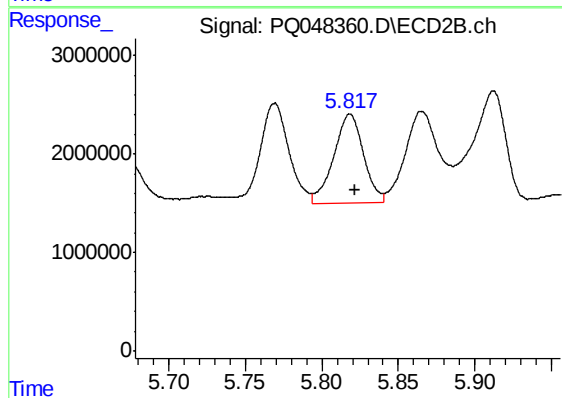

#6 AR-1016-4


R.T.: 5.818 min
Delta R.T.: -0.003 min
Response: 12157887
Conc: 136.00 ng/ml



#7 AR-1016-5


R.T.: 7.140 min
Delta R.T.: -0.010 min
Response: 45585939
Conc: 230.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#7 AR-1016-5

R.T.: 6.051 min
Delta R.T.: -0.002 min
Response: 11463321
Conc: 117.32 ng/ml




#8 AR-1221-1

R.T.: 5.537 min
Delta R.T.: -0.016 min
Response: 24706727
Conc: 276.59 ng/ml

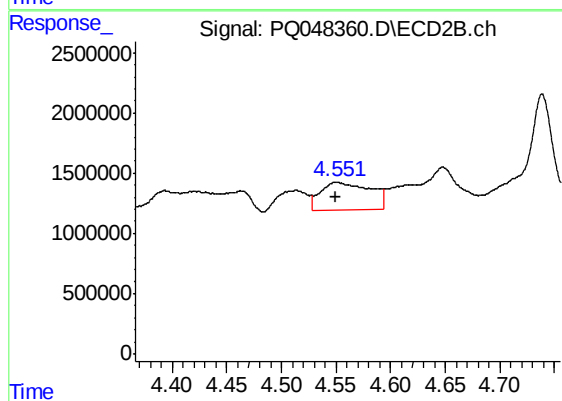

#8 AR-1221-1


R.T.: 4.550 min
Delta R.T.: 0.000 min
Response: 7482302
Conc: 173.61 ng/ml



#9 AR-1221-2


R.T.: 5.651 min
Delta R.T.: -0.002 min
Response: 21346192
Conc: 313.10 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

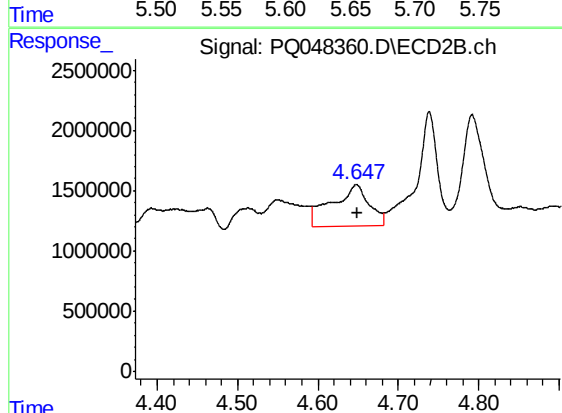


#9 AR-1221-2

R.T.: 4.648 min
Delta R.T.: -0.002 min
Response: 11155512
Conc: 342.12 ng/ml

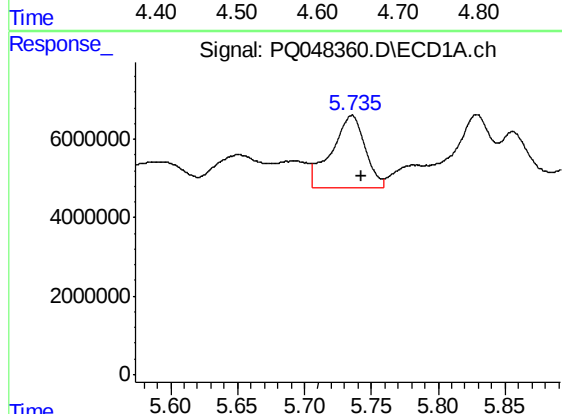


#10 AR-1221-3

R.T.: 5.735 min
Delta R.T.: -0.007 min
Response: 32312749
Conc: 153.75 ng/ml

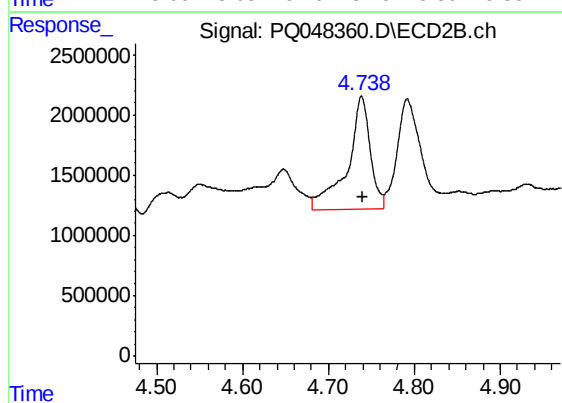

#10 AR-1221-3


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 17373821
Conc: 170.53 ng/ml



#11 AR-1232-1


R.T.: 5.735 min
Delta R.T.: -0.007 min
Response: 32312749
Conc: 191.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#11 AR-1232-1

R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 17373821
Conc: 212.90 ng/ml




#12 AR-1232-2

R.T.: 6.306 min
Delta R.T.: -0.031 min
Response: 69780784
Conc: 814.55 ng/ml

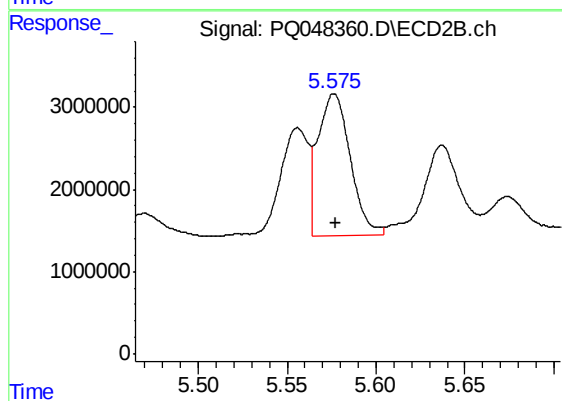

#12 AR-1232-2


R.T.: 5.576 min
Delta R.T.: 0.000 min
Response: 21881425
Conc: 256.25 ng/ml



#13 AR-1232-3


R.T.: 6.650 min
Delta R.T.: -0.008 min
Response: 60387095
Conc: 360.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#13 AR-1232-3

R.T.: 5.769 min
Delta R.T.: -0.002 min
Response: 13619903
Conc: 315.82 ng/ml




#14 AR-1232-4

R.T.: 6.826 min
Delta R.T.: -0.009 min
Response: 39257537
Conc: 462.69 ng/ml

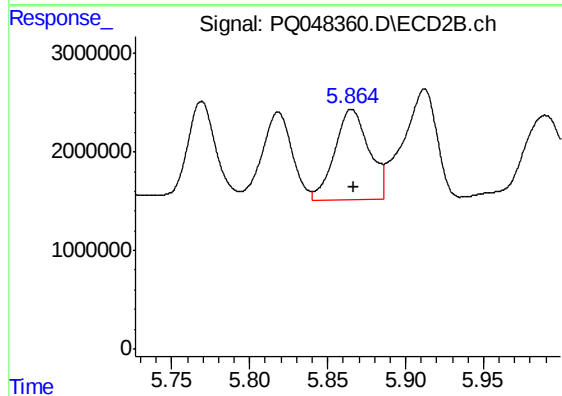

#14 AR-1232-4


R.T.: 5.865 min
Delta R.T.: -0.001 min
Response: 13909675
Conc: 354.85 ng/ml



#15 AR-1232-5


R.T.: 6.915 min
Delta R.T.: -0.014 min
Response: 67455007
Conc: 1064.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

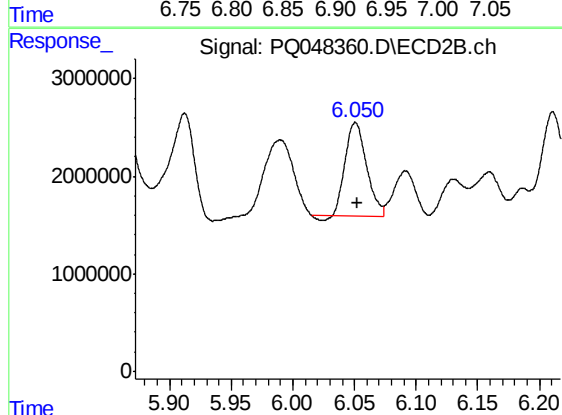


#15 AR-1232-5

R.T.: 6.051 min
Delta R.T.: -0.002 min
Response: 11463321
Conc: 293.89 ng/ml

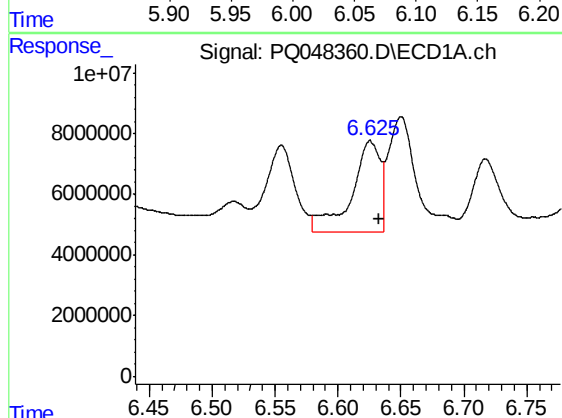


#16 AR-1242-1

R.T.: 6.626 min
Delta R.T.: -0.007 min
Response: 47063433
Conc: 207.89 ng/ml

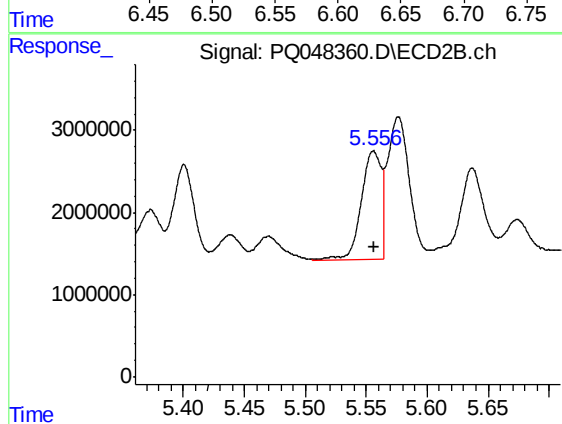

#16 AR-1242-1


R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 15022407
Conc: 130.39 ng/ml



#17 AR-1242-2


R.T.: 6.650 min
Delta R.T.: -0.007 min
Response: 60387095
Conc: 195.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#17 AR-1242-2

R.T.: 5.576 min
Delta R.T.: 0.000 min
Response: 21881425
Conc: 138.85 ng/ml




#18 AR-1242-3

R.T.: 6.717 min
Delta R.T.: -0.008 min
Response: 42637303
Conc: 222.61 ng/ml

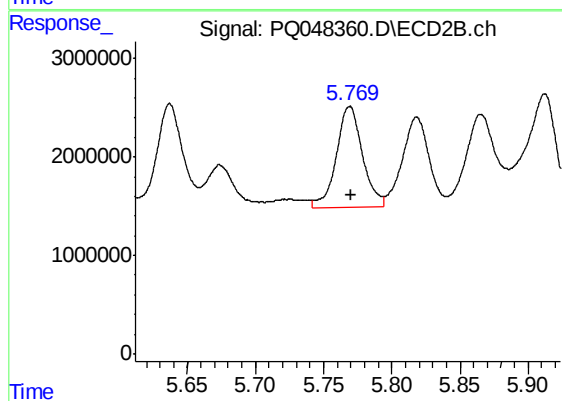

#18 AR-1242-3


R.T.: 5.769 min
Delta R.T.: -0.002 min
Response: 13619903
Conc: 165.99 ng/ml



#19 AR-1242-4


R.T.: 6.826 min
Delta R.T.: -0.008 min
Response: 39257537
Conc: 247.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#19 AR-1242-4

R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 13909675
Conc: 172.08 ng/ml




#20 AR-1242-5

R.T.: 7.611 min
Delta R.T.: -0.008 min
Response: 61068977
Conc: 359.41 ng/ml

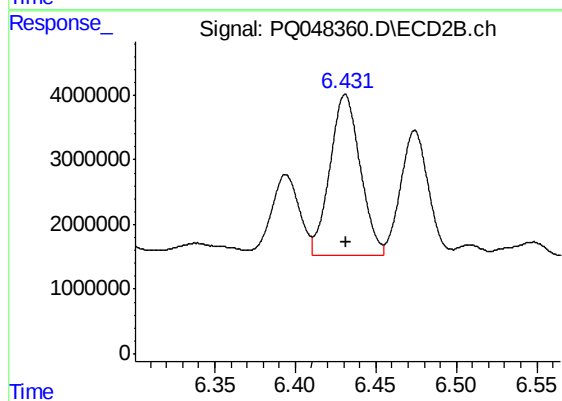

#20 AR-1242-5


R.T.: 6.431 min
Delta R.T.: 0.000 min
Response: 32608192
Conc: 304.71 ng/ml



#21 AR-1248-1


R.T.: 6.626 min
Delta R.T.: -0.007 min
Response: 47063433
Conc: 271.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#21 AR-1248-1

R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 15022407
Conc: 170.06 ng/ml




#22 AR-1248-2

R.T.: 6.915 min
Delta R.T.: -0.013 min
Response: 67455007
Conc: 303.26 ng/ml

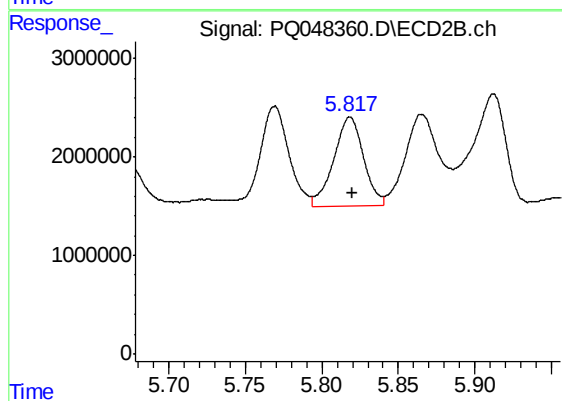

#22 AR-1248-2


R.T.: 5.818 min
Delta R.T.: -0.002 min
Response: 12157887
Conc: 108.37 ng/ml



#23 AR-1248-3


R.T.: 7.140 min
Delta R.T.: -0.009 min
Response: 45585939
Conc: 186.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#23 AR-1248-3

R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 13909675
Conc: 122.25 ng/ml




#24 AR-1248-4

R.T.: 7.570 min
Delta R.T.: -0.009 min
Response: 63580768
Conc: 229.89 ng/ml

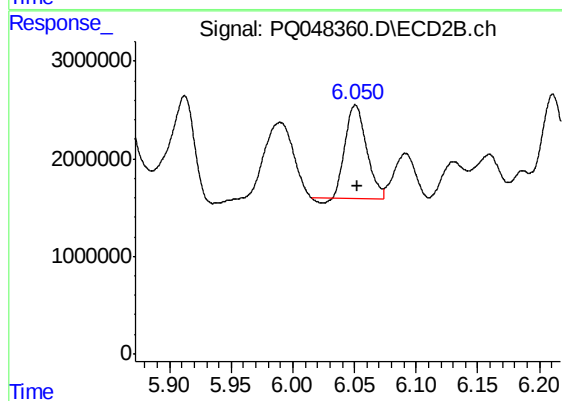

#24 AR-1248-4


R.T.: 6.051 min
Delta R.T.: -0.001 min
Response: 11463321
Conc: 84.51 ng/ml



#25 AR-1248-5


R.T.: 7.611 min
Delta R.T.: -0.008 min
Response: 61068977
Conc: 232.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#25 AR-1248-5

R.T.: 6.474 min
Delta R.T.: -0.001 min
Response: 23319312
Conc: 169.48 ng/ml




#26 AR-1254-1

R.T.: 7.541 min
Delta R.T.: -0.007 min
Response: 49607047
Conc: 165.60 ng/ml

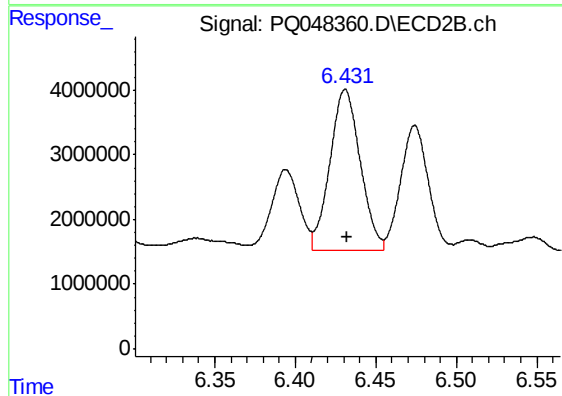

#26 AR-1254-1


R.T.: 6.431 min
Delta R.T.: -0.001 min
Response: 32608192
Conc: 138.02 ng/ml



#27 AR-1254-2


R.T.: 7.779 min
Delta R.T.: 0.002 min
Response: 60704819
Conc: 131.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#27 AR-1254-2

R.T.: 6.588 min
Delta R.T.: -0.002 min
Response: 8889579
Conc: 43.35 ng/ml




#28 AR-1254-3

R.T.: 8.155 min
Delta R.T.: -0.008 min
Response: 27859238
Conc: 57.16 ng/ml

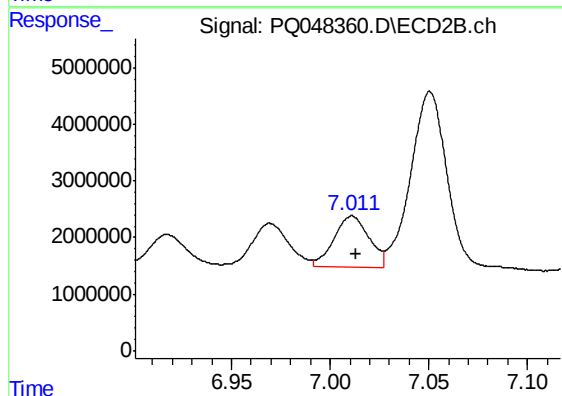

#28 AR-1254-3


R.T.: 7.011 min
Delta R.T.: -0.002 min
Response: 11186829
Conc: 33.33 ng/ml

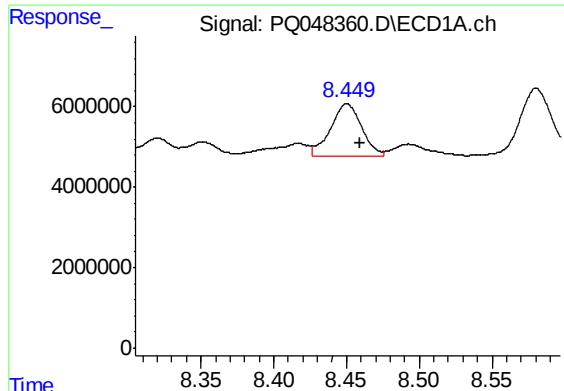

#29 AR-1254-4


R.T.: 8.450 min
Delta R.T.: -0.009 min
Response: 19212144
Conc: 50.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

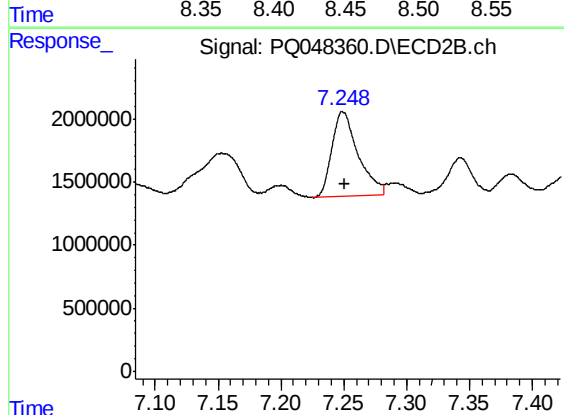


#29 AR-1254-4

R.T.: 7.249 min
Delta R.T.: -0.002 min
Response: 9830522
Conc: 44.76 ng/ml

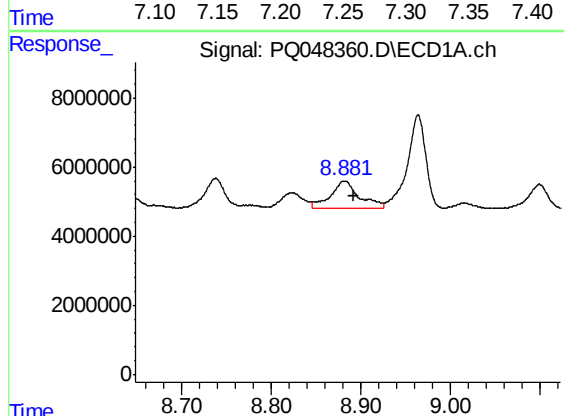


#30 AR-1254-5

R.T.: 8.881 min
Delta R.T.: -0.010 min
Response: 18093337
Conc: 45.27 ng/ml

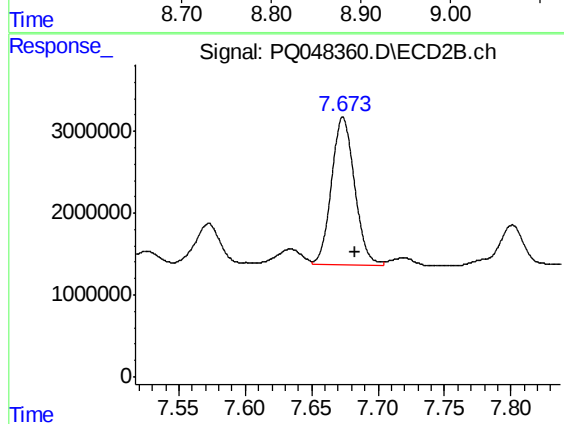

#30 AR-1254-5


R.T.: 7.674 min
Delta R.T.: -0.009 min
Response: 21952561
Conc: 75.15 ng/ml

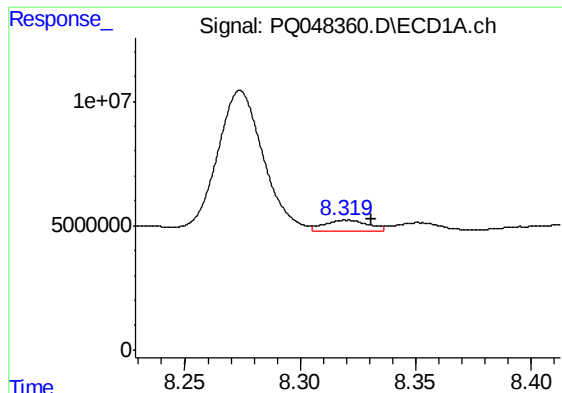

#31 AR-1260-1


R.T.: 8.320 min
Delta R.T.: -0.011 min
Response: 5937752
Conc: 17.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#31 AR-1260-1

R.T.: 7.154 min
Delta R.T.: 0.002 min
Response: 7482829
Conc: 37.26 ng/ml




#32 AR-1260-2

R.T.: 8.580 min
Delta R.T.: -0.015 min
Response: 25779804
Conc: 64.26 ng/ml

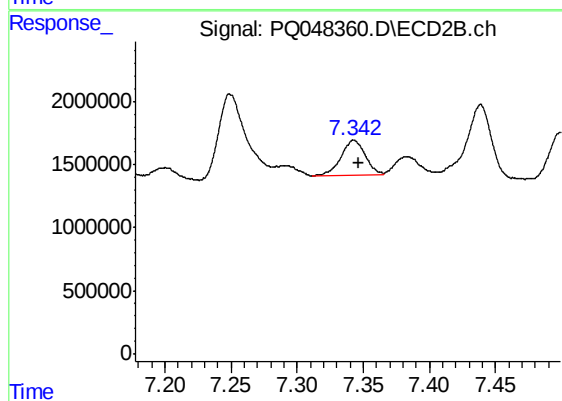

#32 AR-1260-2


R.T.: 7.343 min
Delta R.T.: -0.004 min
Response: 3518142
Conc: 14.20 ng/ml

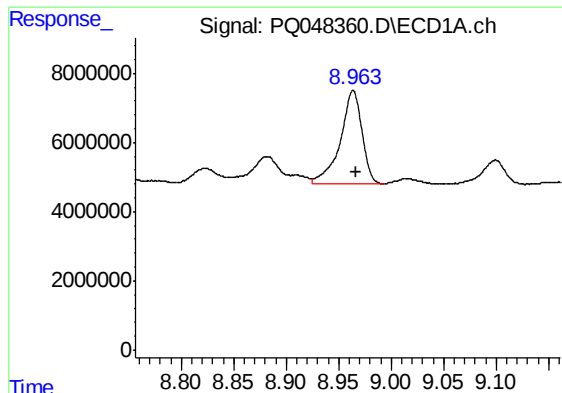

#33 AR-1260-3


R.T.: 8.964 min
Delta R.T.: -0.003 min
Response: 39193024
Conc: 124.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

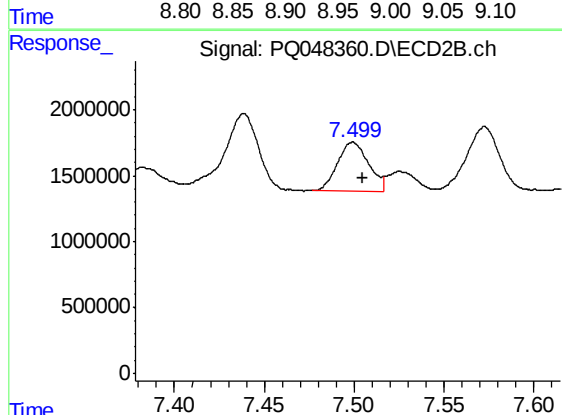


#33 AR-1260-3

R.T.: 7.499 min
Delta R.T.: -0.005 min
Response: 4409819
Conc: 19.56 ng/ml

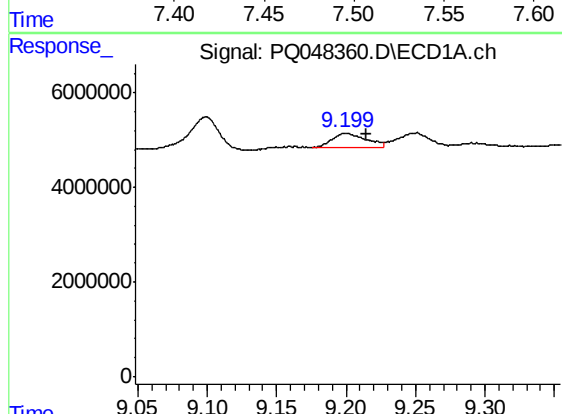


#34 AR-1260-4

R.T.: 9.199 min
Delta R.T.: -0.015 min
Response: 5111755
Conc: 13.85 ng/ml

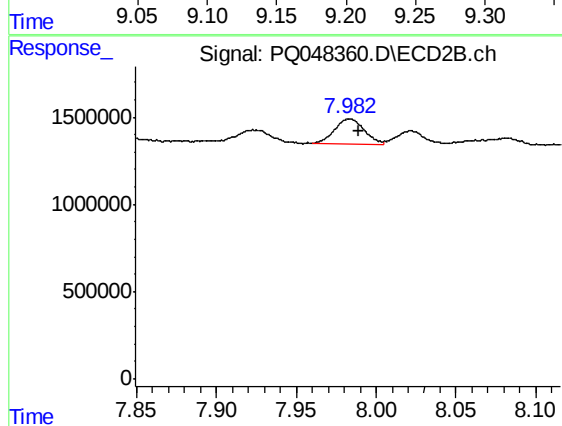

#34 AR-1260-4


R.T.: 7.983 min
Delta R.T.: -0.006 min
Response: 1841997
Conc: 9.60 ng/ml



#35 AR-1260-5


R.T.: 9.556 min
Delta R.T.: -0.012 min
Response: 5477040
Conc: 6.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#35 AR-1260-5

R.T.: 8.229 min
Delta R.T.: -0.005 min
Response: 1939707
Conc: 4.06 ng/ml

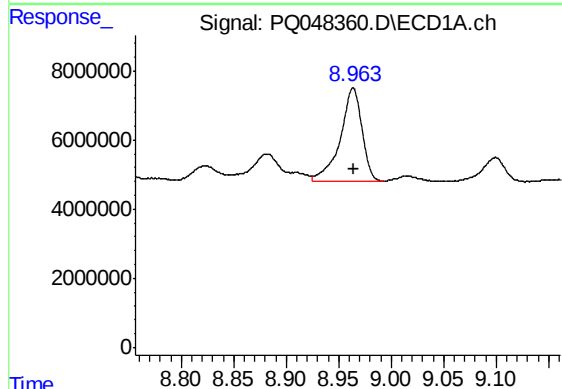


#36 AR-1262-1

R.T.: 8.964 min
Delta R.T.: 0.000 min
Response: 39193024
Conc: 90.34 ng/ml

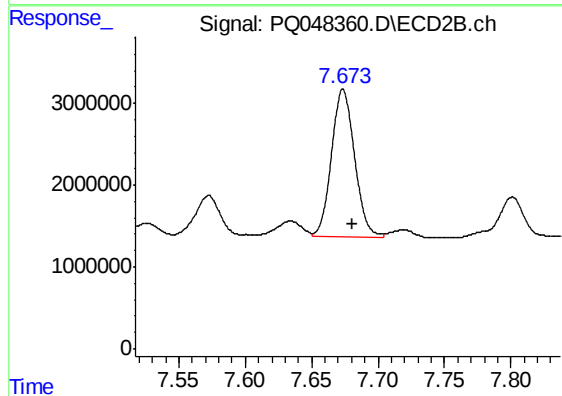

#36 AR-1262-1


R.T.: 7.674 min
Delta R.T.: -0.007 min
Response: 21952561
Conc: 155.12 ng/ml



#37 AR-1262-2


R.T.: 9.556 min
Delta R.T.: -0.010 min
Response: 5477040
Conc: 6.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#37 AR-1262-2

R.T.: 8.229 min
Delta R.T.: -0.003 min
Response: 1939707
Conc: 3.68 ng/ml

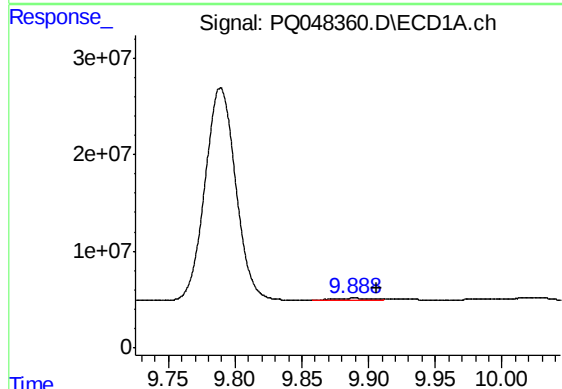


#38 AR-1262-3

R.T.: 9.889 min
Delta R.T.: -0.017 min
Response: 5794789
Conc: 14.96 ng/ml

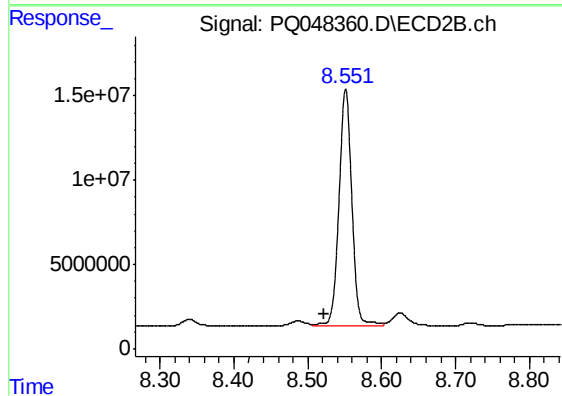

#38 AR-1262-3


R.T.: 8.551 min
Delta R.T.: 0.030 min
Response: 170906439
Conc: 794.64 ng/ml



#39 AR-1262-4


R.T.: 10.024 min
Delta R.T.: 0.016 min
Response: 11202134
Conc: 24.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

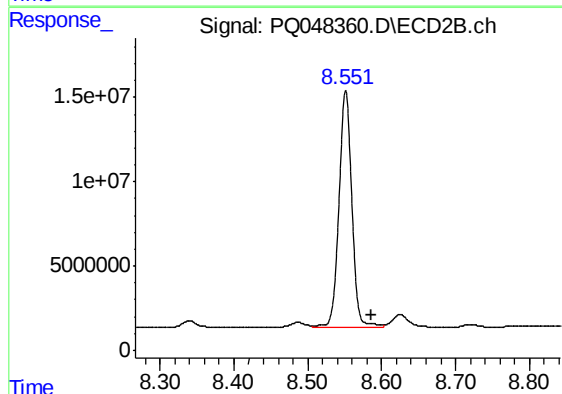


#39 AR-1262-4

R.T.: 8.551 min
Delta R.T.: -0.034 min
Response: 170906439
Conc: 444.02 ng/ml




#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 10.746 min
Response: 0
Conc: N.D.

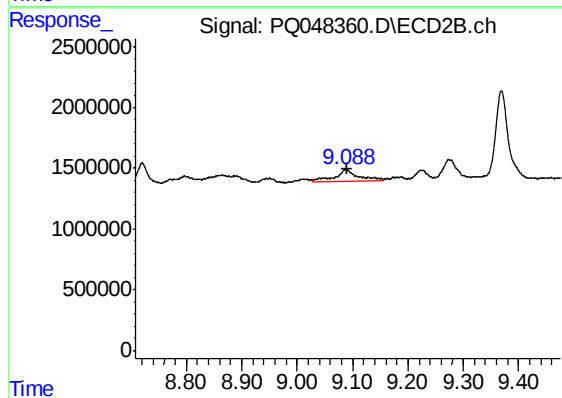

#40 AR-1262-5


R.T.: 9.088 min
Delta R.T.: -0.003 min
Response: 3110573
Conc: 16.94 ng/ml

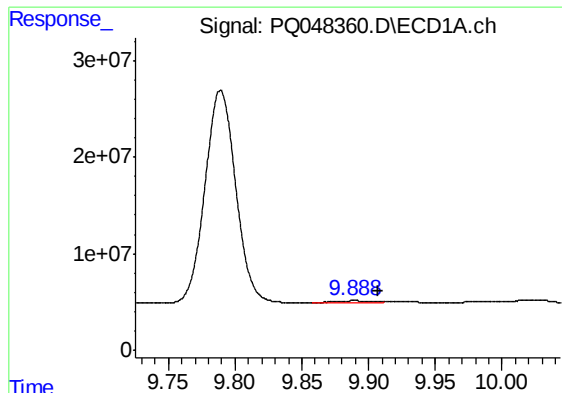

#41 AR-1268-1


R.T.: 9.889 min
Delta R.T.: -0.018 min
Response: 5794789
Conc: 5.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

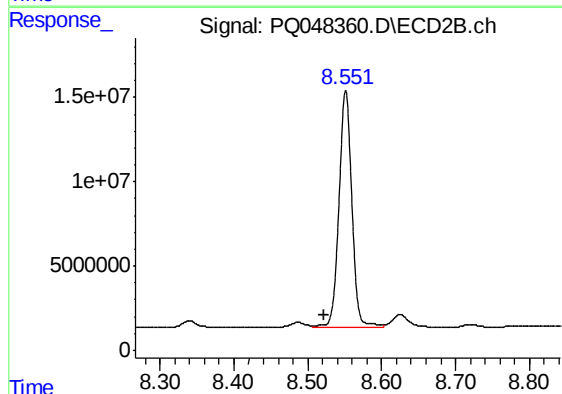


#41 AR-1268-1

R.T.: 8.551 min
Delta R.T.: 0.029 min
Response: 170906439
Conc: 249.03 ng/ml




#42 AR-1268-2

R.T.: 10.024 min
Delta R.T.: 0.011 min
Response: 11202134
Conc: 10.26 ng/ml

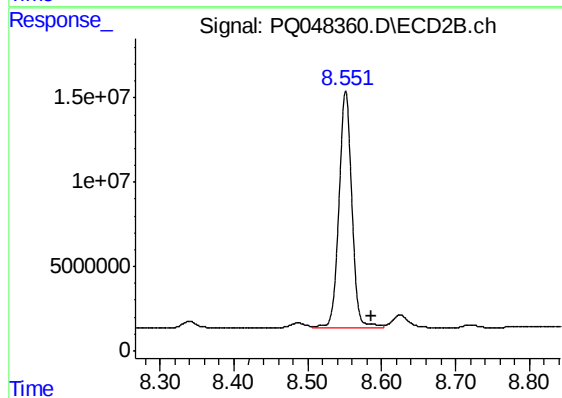

#42 AR-1268-2


R.T.: 8.551 min
Delta R.T.: -0.036 min
Response: 170906439
Conc: 269.00 ng/ml



#43 AR-1268-3


R.T.: 10.251 min
Delta R.T.: -0.013 min
Response: -40338
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1




#43 AR-1268-3

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 1863070
Conc: 3.52 ng/ml




#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 10.748 min
Response: 0
Conc: N.D.

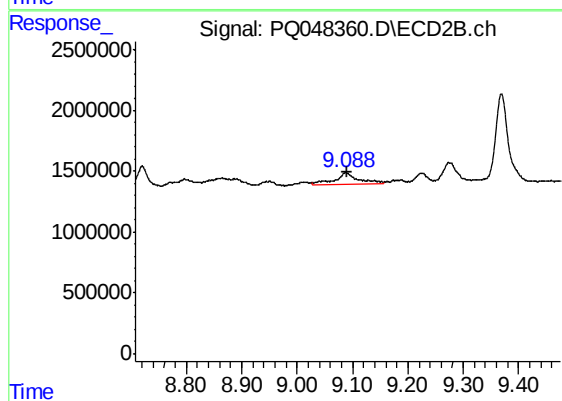

#44 AR-1268-4


R.T.: 9.088 min
Delta R.T.: -0.004 min
Response: 3110573
Conc: 13.35 ng/ml

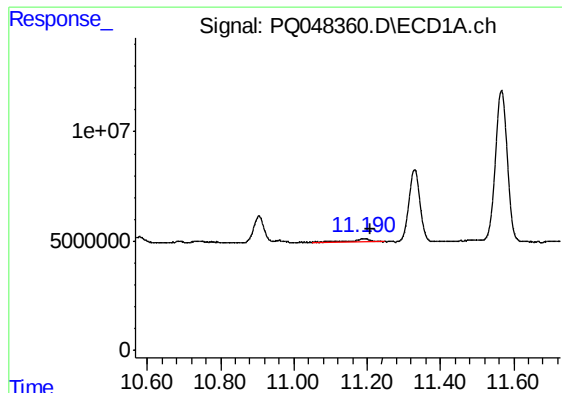

#45 AR-1268-5

R.T.: 11.191 min
Delta R.T.: -0.017 min
Response: 4215849
Conc: 1.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MASON-BRICK-COMP-1

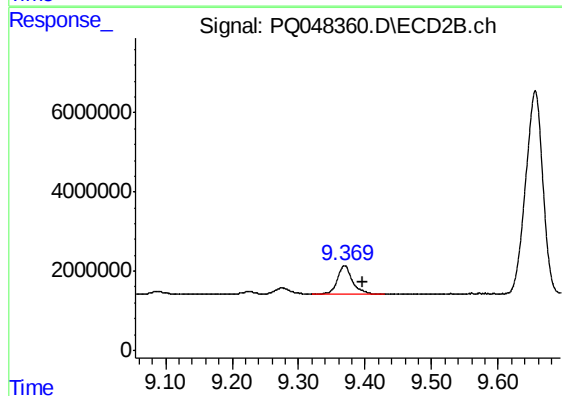

#45 AR-1268-5

R.T.: 9.369 min
Delta R.T.: -0.028 min
Response: 11563397
Conc: 6.60 ng/ml