

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062019\
 Data File : PR038831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 21:12
 Operator : SM\AJ
 Sample : K3438-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 FK-SF-01-005-A

Manual Integrations
 APPROVED

Ankita
 6/21/2019 9:18:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 04:43:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 12 02:00:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.770	4.618	36342928	116.9E6	24.908	23.450
2)	SA Decachlor...	8.720	10.363	50498419	142.6E6	22.131	23.012m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062019\
Data File : PR038831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 21:12
Operator : SM\AJ
Sample : K3438-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
FK-SF-01-005-A


Manual Integrations
APPROVED

Ankita
6/21/2019 9:18:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 04:43:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061119.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 12 02:00:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

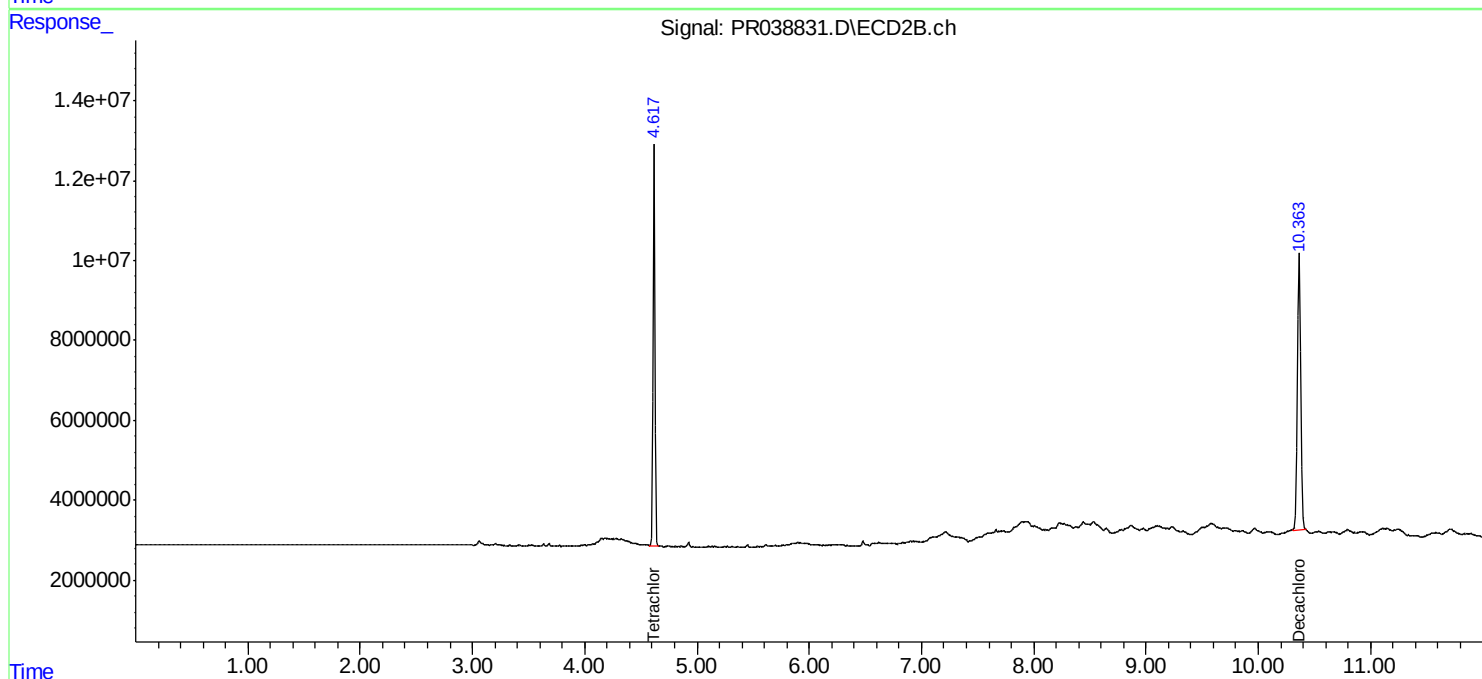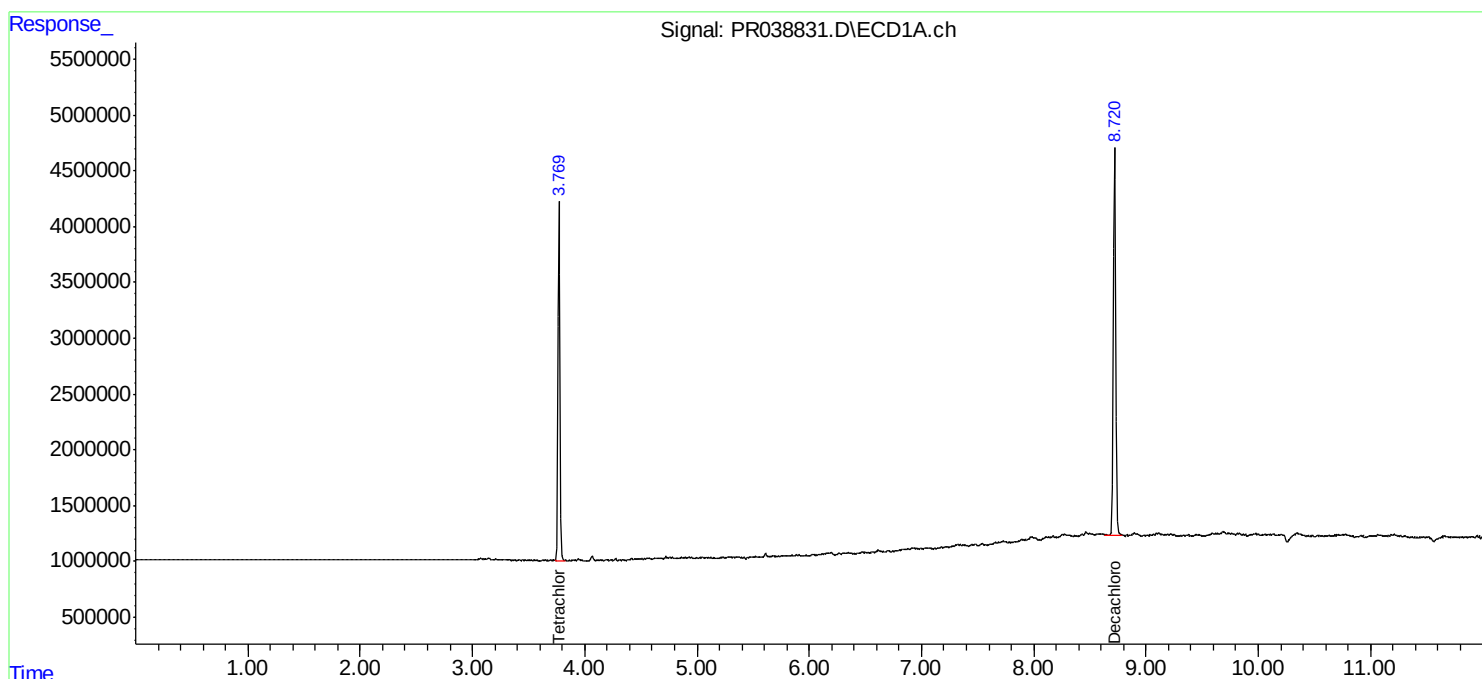

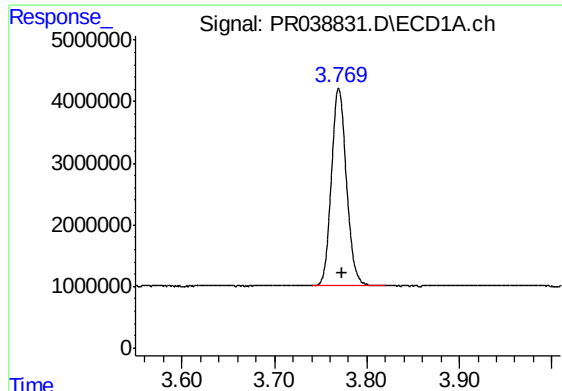


#1 Tetrachloro-m-xylene

R.T.: 3.770 min
Delta R.T.: -0.003 min
Response: 36342928
Conc: 24.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-SF-01-005-A


Manual Integrations
APPROVED

Ankita
6/21/2019 9:18:27 AM

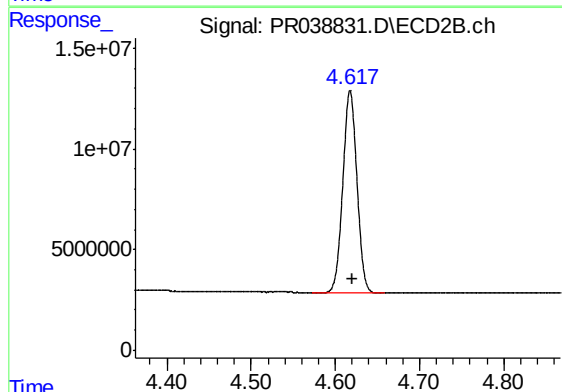


#1 Tetrachloro-m-xylene

R.T.: 4.618 min
Delta R.T.: -0.003 min
Response: 116910088
Conc: 23.45 ng/ml

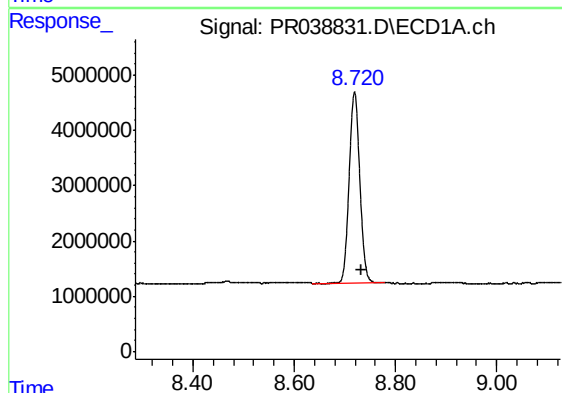

#2 Decachlorobiphenyl

R.T.: 8.720 min
Delta R.T.: -0.012 min
Response: 50498419
Conc: 22.13 ng/ml

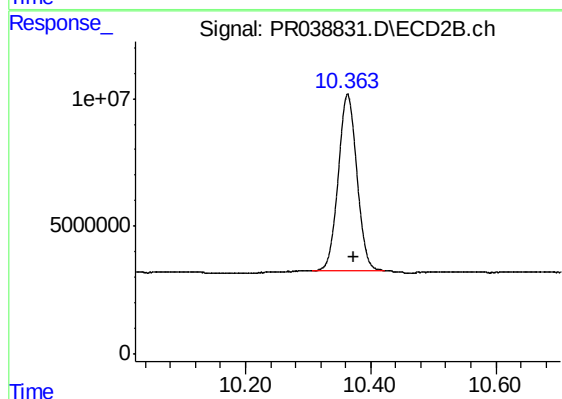

#2 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: -0.010 min
Response: 142631810
Conc: 23.01 ng/ml m