

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062218\
 Data File : PR029141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 12:26
 Operator : UA/SM
 Sample : J3415-03
 Misc :
 ALS Vial : 116 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 SB-34COMP

Manual Integrations
 APPROVED

UGO
 6/15/2018 5:13:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 12:41:11 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 06 14:28:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.574	3.720	490.3E6	892.4E6	19.864	18.303
2) SA Decachlor...	10.350	8.668	368.0E6	699.5E6	17.304	12.269m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062218\
Data File : PR029141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 12:26
Operator : UA/SM
Sample : J3415-03
Misc :
ALS Vial : 116 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
SB-34COMP


Manual Integrations
APPROVED

UGO
6/15/2018 5:13:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 12:41:11 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR061018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 06 14:28:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

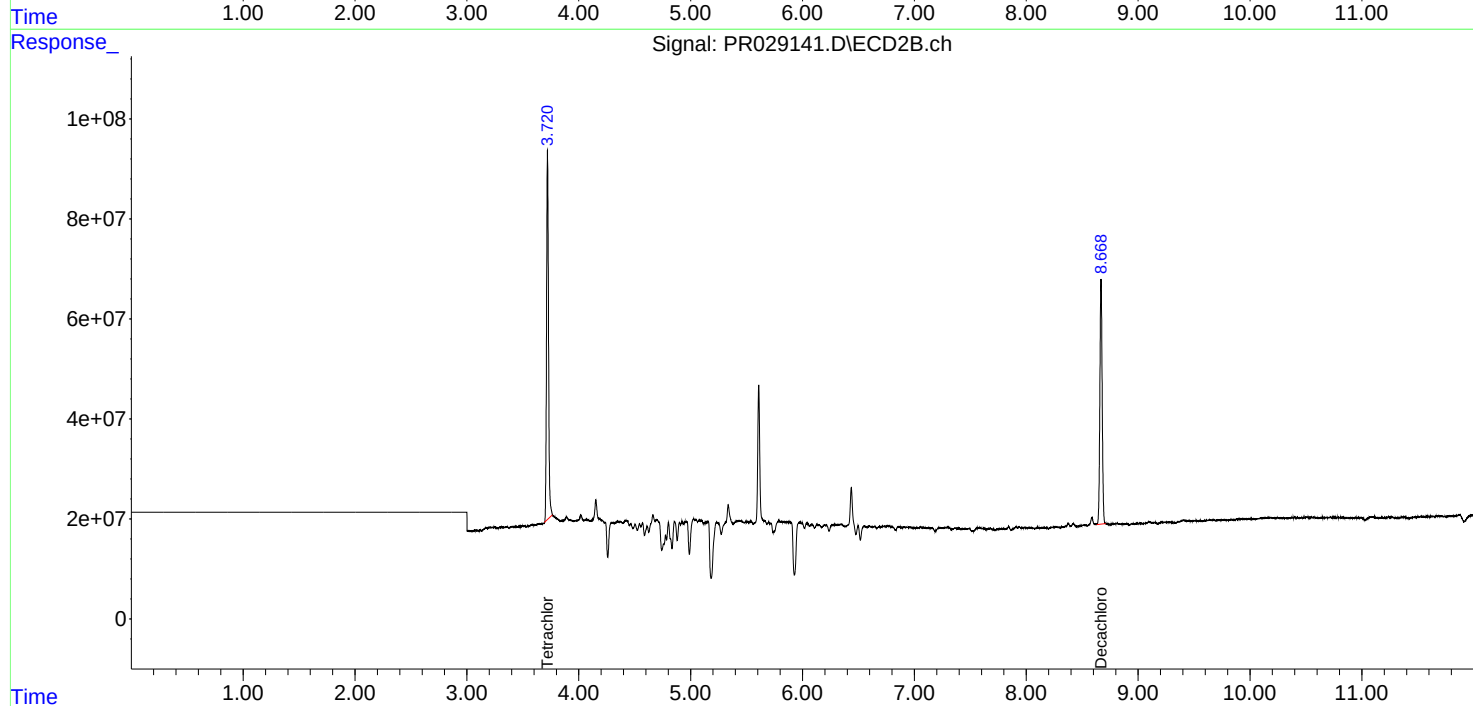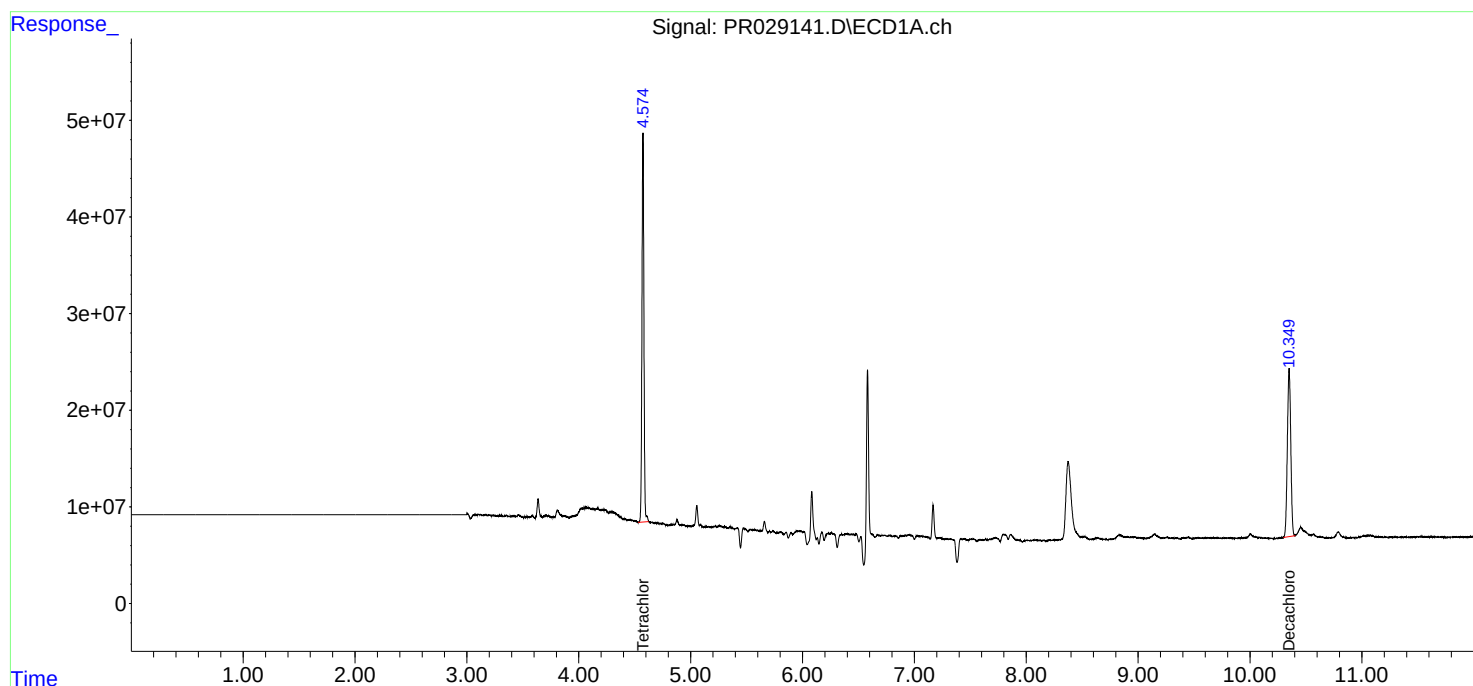

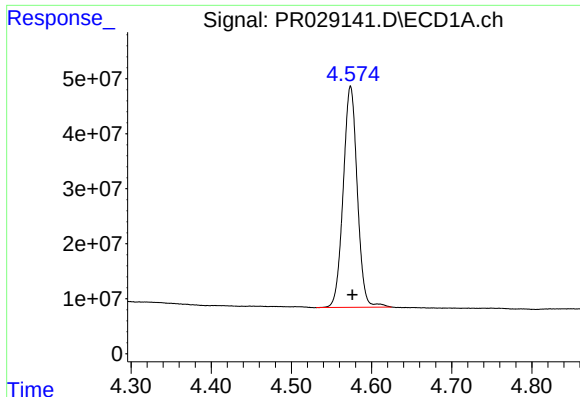


#1 Tetrachloro-m-xylene

R.T.: 4.574 min
Delta R.T.: -0.002 min
Response: 490265719
Conc: 19.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
SB-34COMP


Manual Integrations
APPROVED

UGO
6/15/2018 5:13:39 PM

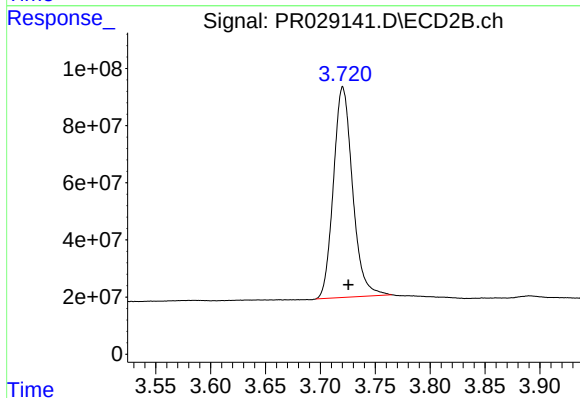


#1 Tetrachloro-m-xylene

R.T.: 3.720 min
Delta R.T.: -0.005 min
Response: 892432243
Conc: 18.30 ng/ml

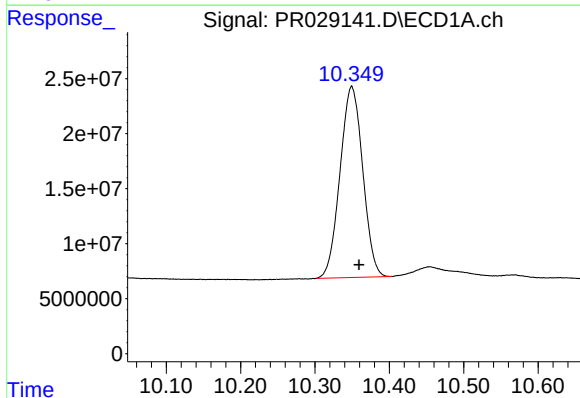

#2 Decachlorobiphenyl

R.T.: 10.350 min
Delta R.T.: -0.010 min
Response: 367971454
Conc: 17.30 ng/ml

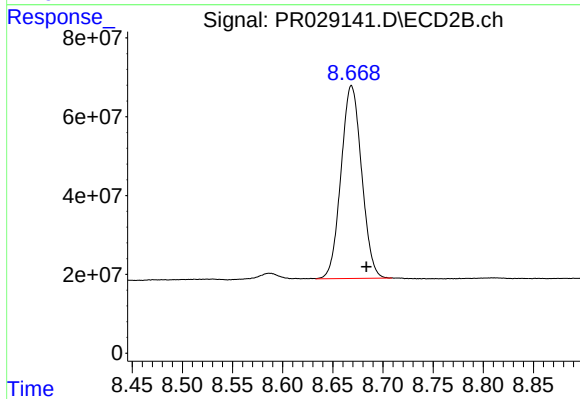

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.015 min
Response: 699528788
Conc: 12.27 ng/ml m