

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062718\
 Data File : PR029416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 16:28
 Operator : UA/SM
 Sample : J3611-05
 Misc :
 ALS Vial : 141 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 N-1366-WATER

Manual Integrations
 APPROVED

ugo
 6/27/2018 2:37:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:13:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 23 04:10:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.570	3.720	301.9E6	551.5E6	13.118	11.666
2) SA Decachlor...	10.349	8.664	200.3E6	134.0E6	7.155	6.787

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062718\
Data File : PR029416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 16:28
Operator : UA/SM
Sample : J3611-05
Misc :
ALS Vial : 141 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
N-1366-WATER


Manual Integrations
APPROVED

ugo
6/27/2018 2:37:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:13:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 23 04:10:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

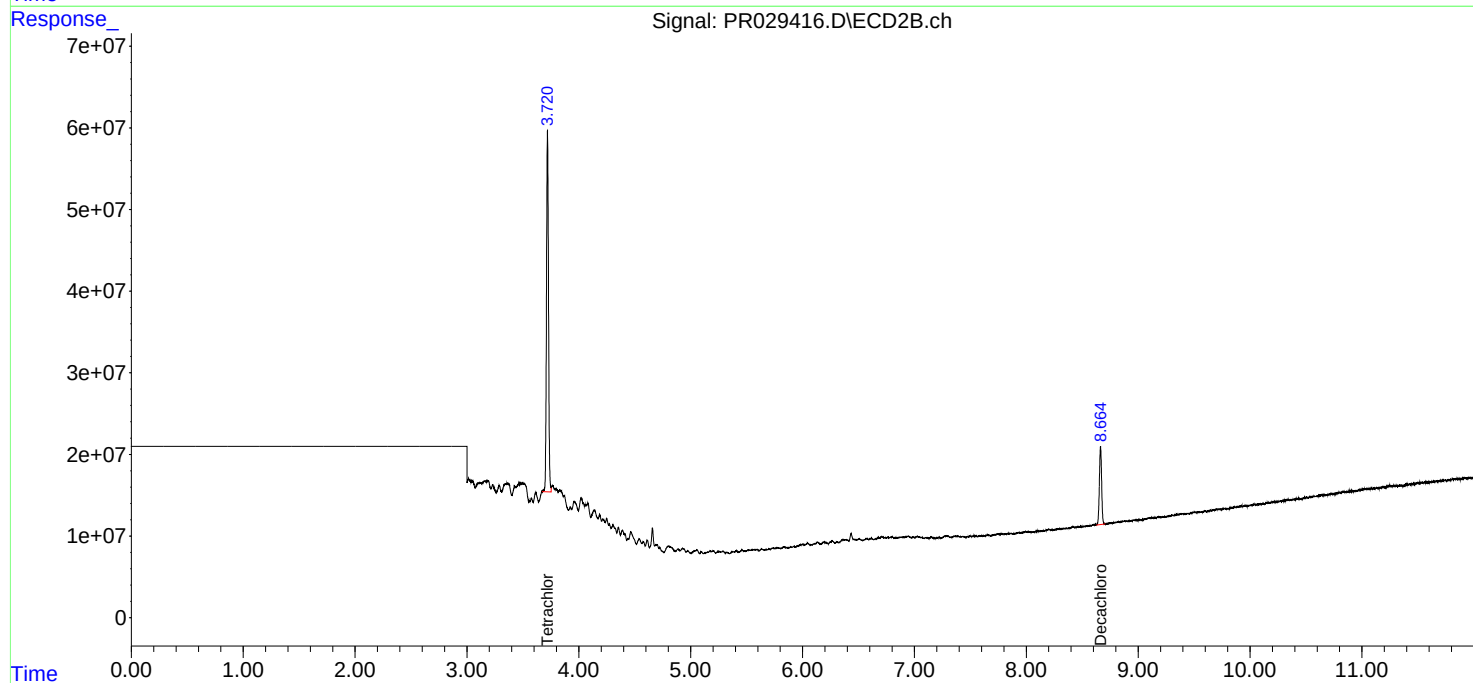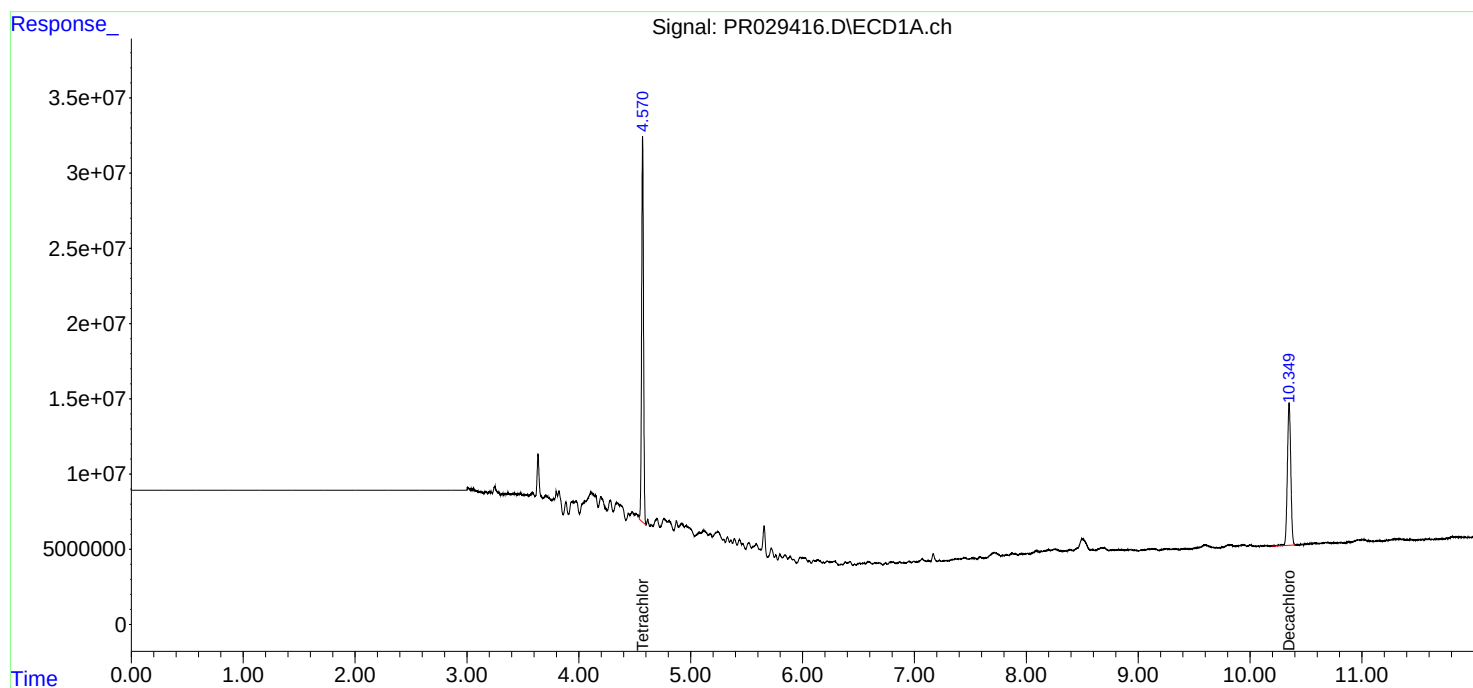

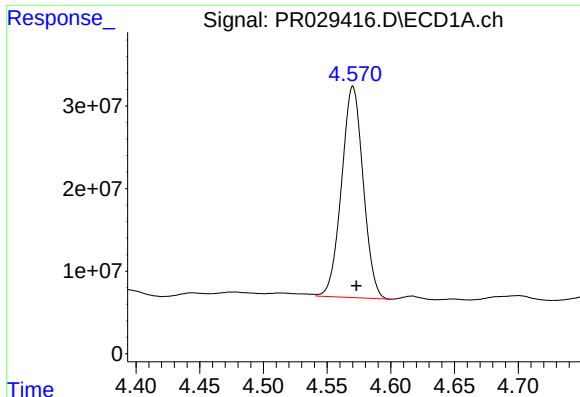


#1 Tetrachloro-m-xylene

R.T.: 4.570 min
Delta R.T.: -0.003 min
Response: 301917799
Conc: 13.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
N-1366-WATER


Manual Integrations
APPROVED

ugo
6/27/2018 2:37:11 PM

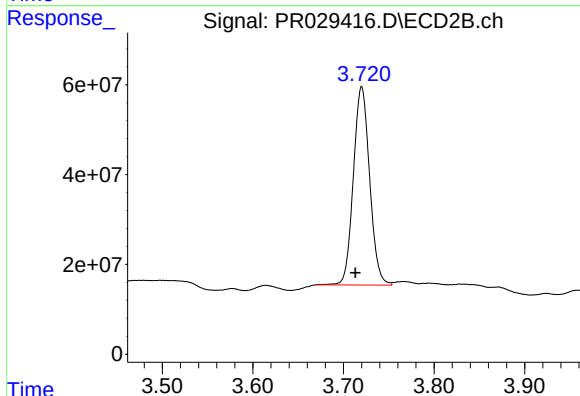


#1 Tetrachloro-m-xylene

R.T.: 3.720 min
Delta R.T.: 0.007 min
Response: 551516497
Conc: 11.67 ng/ml

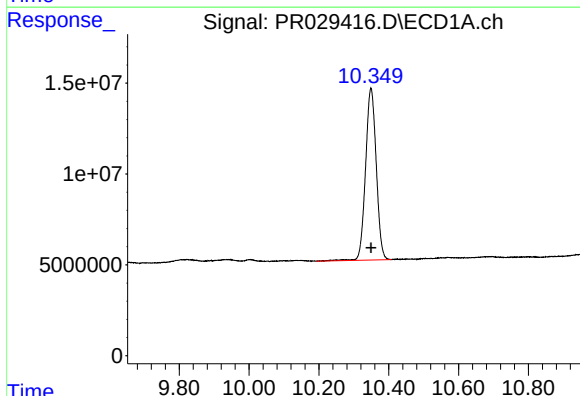

#2 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: 0.000 min
Response: 200322794
Conc: 7.16 ng/ml

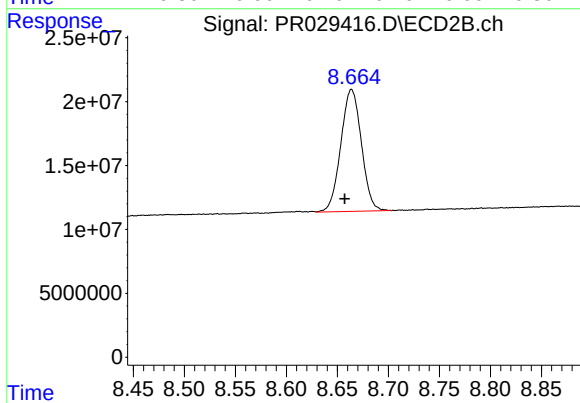

#2 Decachlorobiphenyl

R.T.: 8.664 min
Delta R.T.: 0.007 min
Response: 134044193
Conc: 6.79 ng/ml