

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062918\
 Data File : PR029488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 14:28
 Operator : UA/SM
 Sample : J3627-23 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 26KV-CC-12

Manual Integrations
 APPROVED

ugo
 6/27/2018 2:42:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 15:26:26 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 23 08:41:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.573	3.715	40280716	69601241	1.750	1.472m
2) SA Decachlor...	10.345	8.654	53665595	42468527	1.917m	2.150

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062918\
Data File : PR029488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 14:28
Operator : UA/SM
Sample : J3627-23 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
26KV-CC-12


Manual Integrations
APPROVED

ugo
6/27/2018 2:42:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 15:26:26 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 23 08:41:26 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

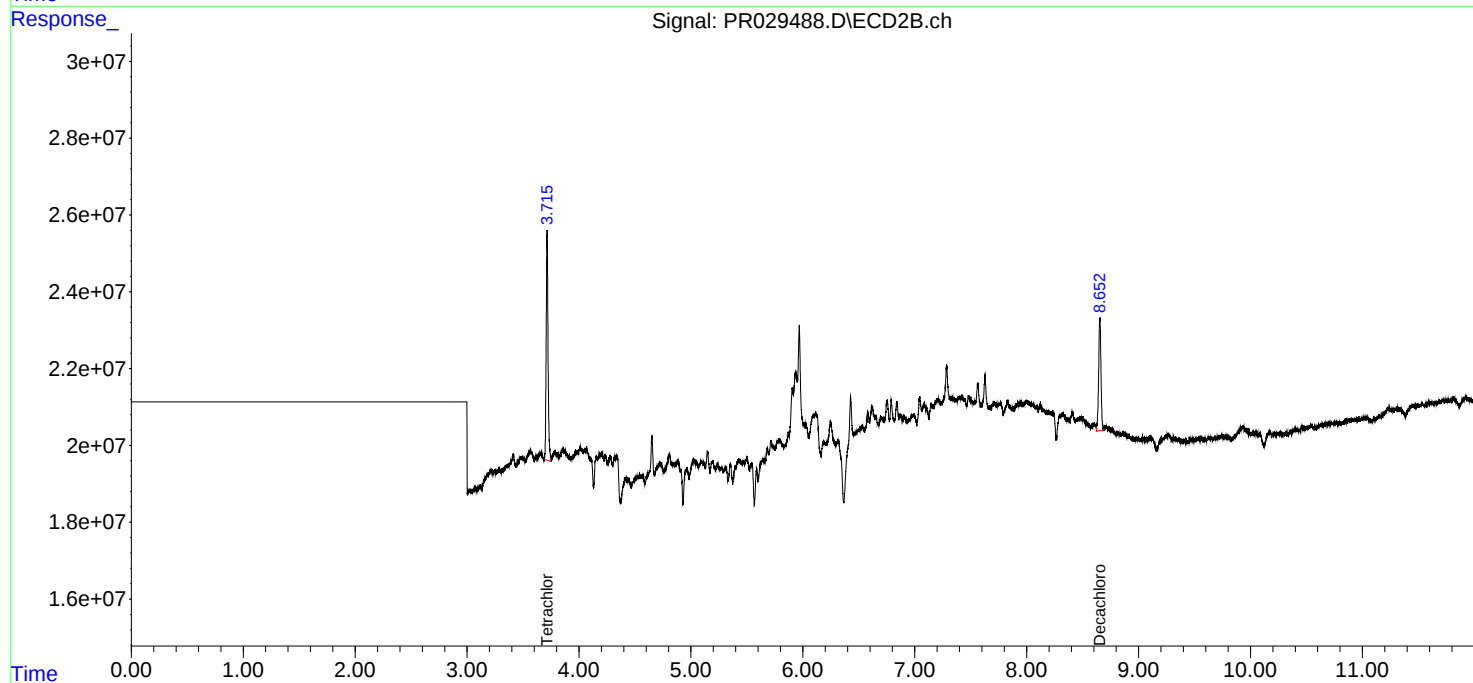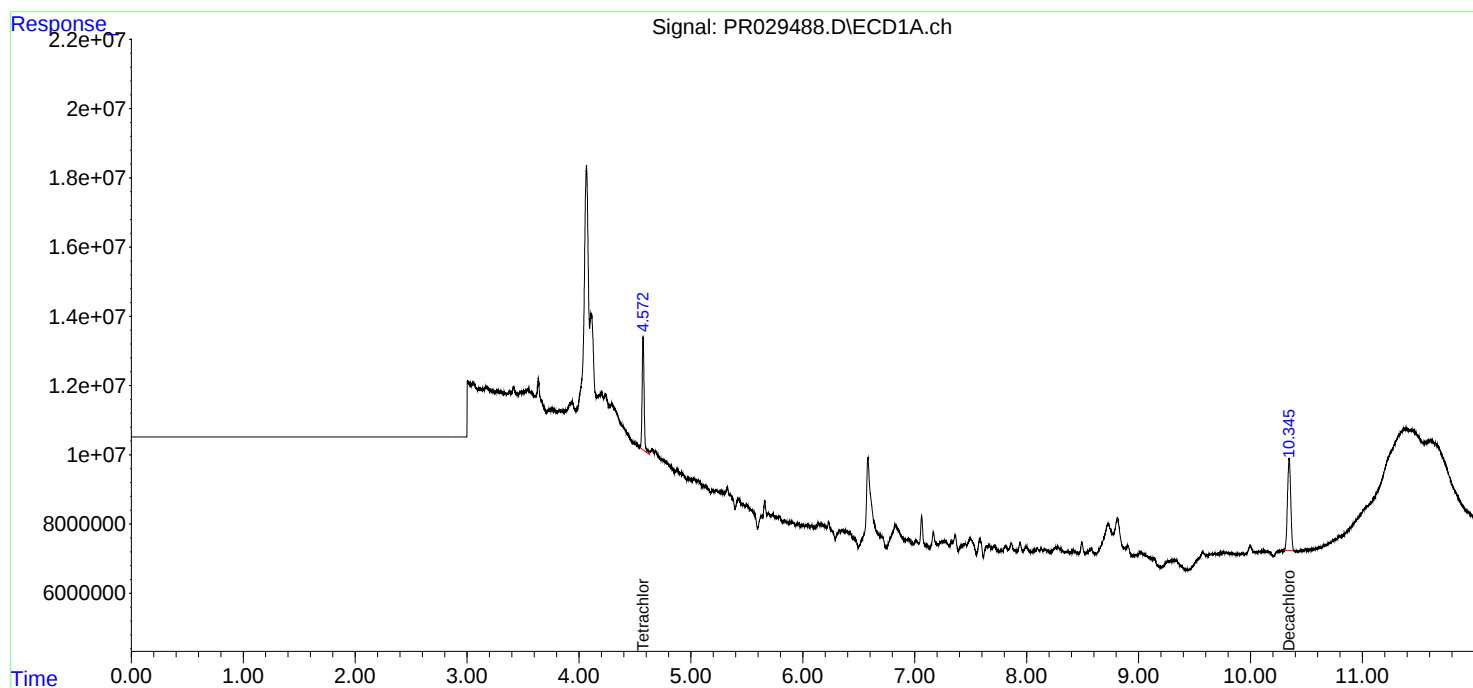

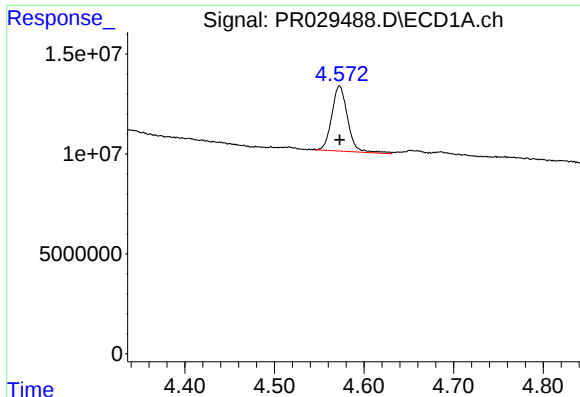


#1 Tetrachloro-m-xylene

R.T.: 4.573 min
Delta R.T.: 0.000 min
Response: 40280716
Conc: 1.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
26KV-CC-12


Manual Integrations
APPROVED

ugo
6/27/2018 2:42:21 PM

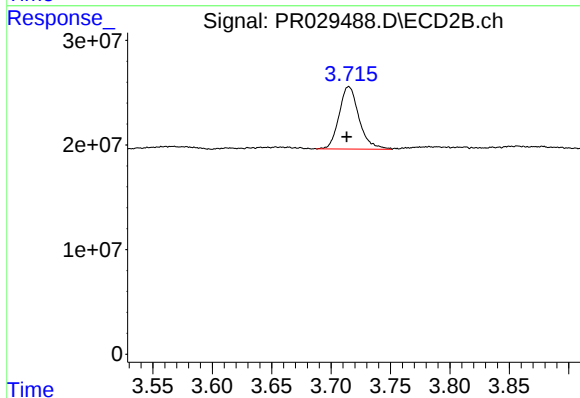


#1 Tetrachloro-m-xylene

R.T.: 3.715 min
Delta R.T.: 0.001 min
Response: 69601241
Conc: 1.47 ng/ml m

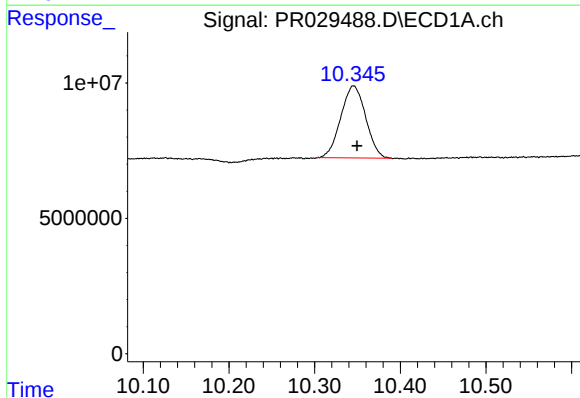

#2 Decachlorobiphenyl

R.T.: 10.345 min
Delta R.T.: -0.004 min
Response: 53665595
Conc: 1.92 ng/ml m

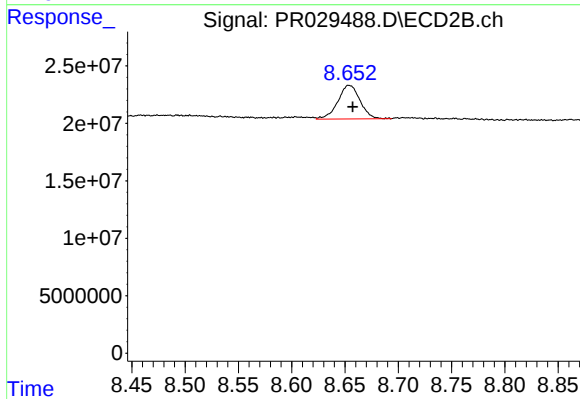

#2 Decachlorobiphenyl

R.T.: 8.654 min
Delta R.T.: -0.003 min
Response: 42468527
Conc: 2.15 ng/ml