

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062918\
 Data File : PR029490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 14:57
 Operator : UA/SM
 Sample : J3627-27 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 26KV-CC-14

Manual Integrations
 APPROVED

ugo
 6/27/2018 2:42:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 15:27:00 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 23 08:41:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.567	3.718	36092261	63310647	1.568m	1.339m
2) SA Decachlor...	10.335	8.652	55193158	40799557	1.971m	2.066m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR062918\
Data File : PR029490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 14:57
Operator : UA/SM
Sample : J3627-27 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
26KV-CC-14


Manual Integrations
APPROVED

ugo
6/27/2018 2:42:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 15:27:00 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 23 08:41:26 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

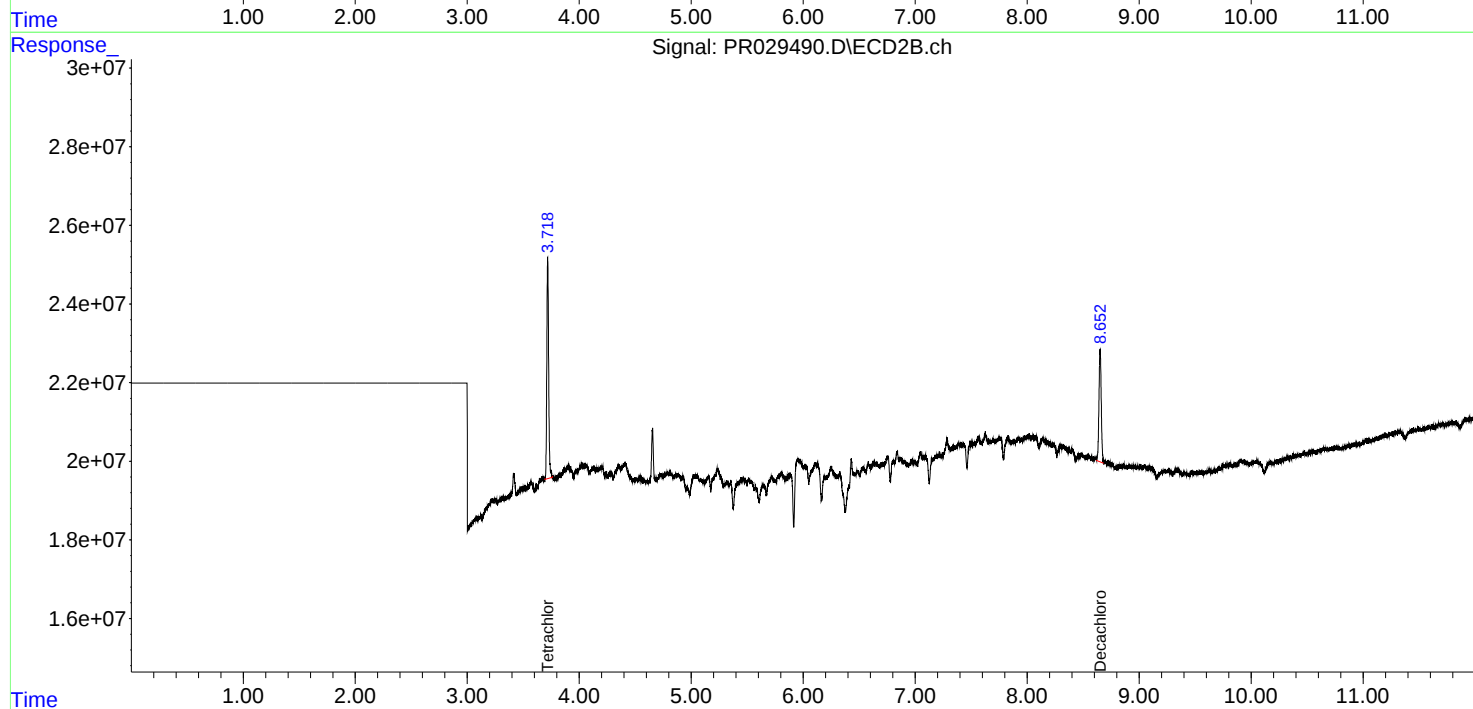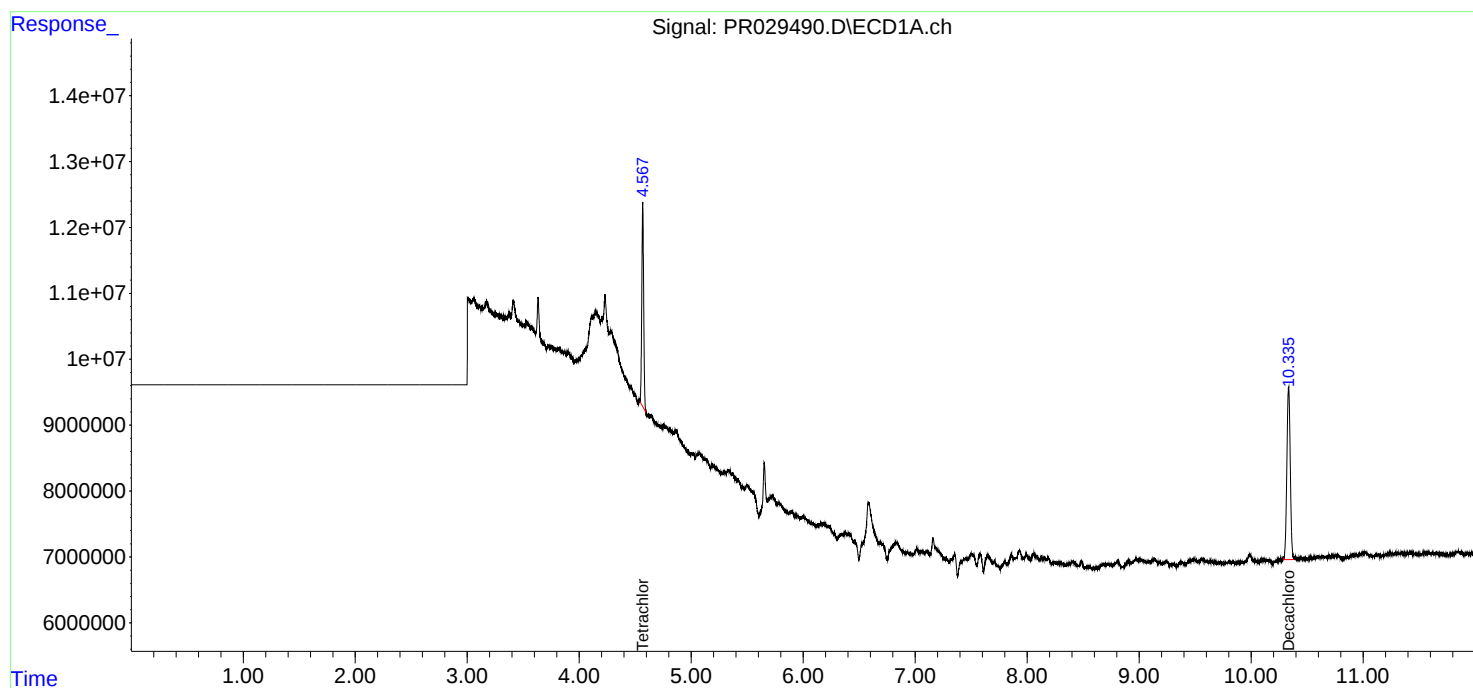

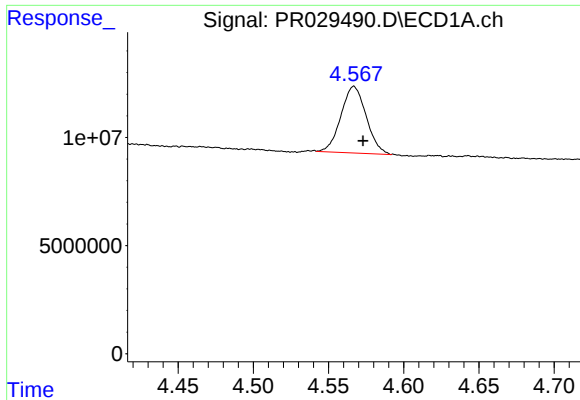


#1 Tetrachloro-m-xylene

R.T.: 4.567 min
Delta R.T.: -0.006 min
Response: 36092261
Conc: 1.57 ng/ml m

Instrument :
ECD_R
ClientSampleId :
26KV-CC-14


Manual Integrations
APPROVED

ugo
6/27/2018 2:42:29 PM

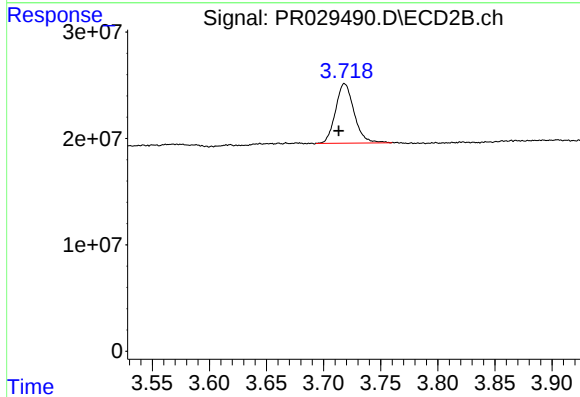


#1 Tetrachloro-m-xylene

R.T.: 3.718 min
Delta R.T.: 0.004 min
Response: 63310647
Conc: 1.34 ng/ml m

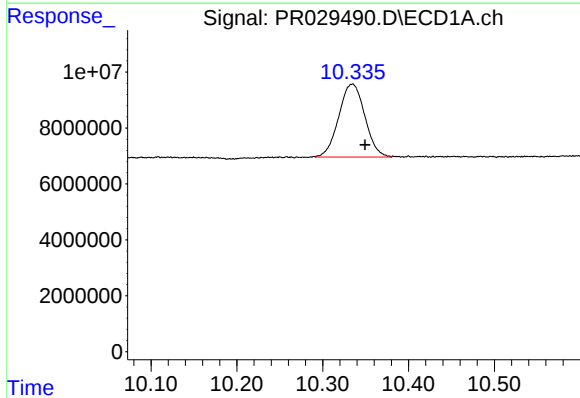

#2 Decachlorobiphenyl

R.T.: 10.335 min
Delta R.T.: -0.014 min
Response: 55193158
Conc: 1.97 ng/ml m

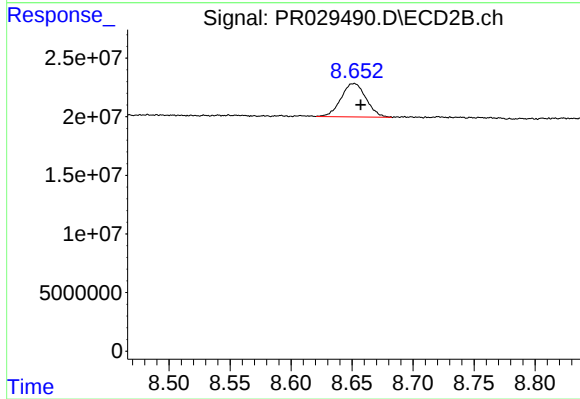

#2 Decachlorobiphenyl

R.T.: 8.652 min
Delta R.T.: -0.005 min
Response: 40799557
Conc: 2.07 ng/ml m