

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR070218\
 Data File : PR029707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2018 14:52
 Operator : UA/SM
 Sample : J3729-04
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 02B-METAL-TO-GLASS-CAULK

Manual Integrations
 APPROVED

mohammad
 7/3/2018 4:26:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 05:14:20 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 23 08:41:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.568	3.717	423.5E6	1096.1E6	18.399	23.185 #
2) SA Decachlor...	10.332	8.644	466.6E6	385.5E6	16.665	19.521m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR070218\
Data File : PR029707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2018 14:52
Operator : UA/SM
Sample : J3729-04
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
02B-METAL-TO-GLASS-CAULK


Manual Integrations
APPROVED

mohammad
7/3/2018 4:26:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 05:14:20 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_R\Method\PR062718.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 23 08:41:26 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

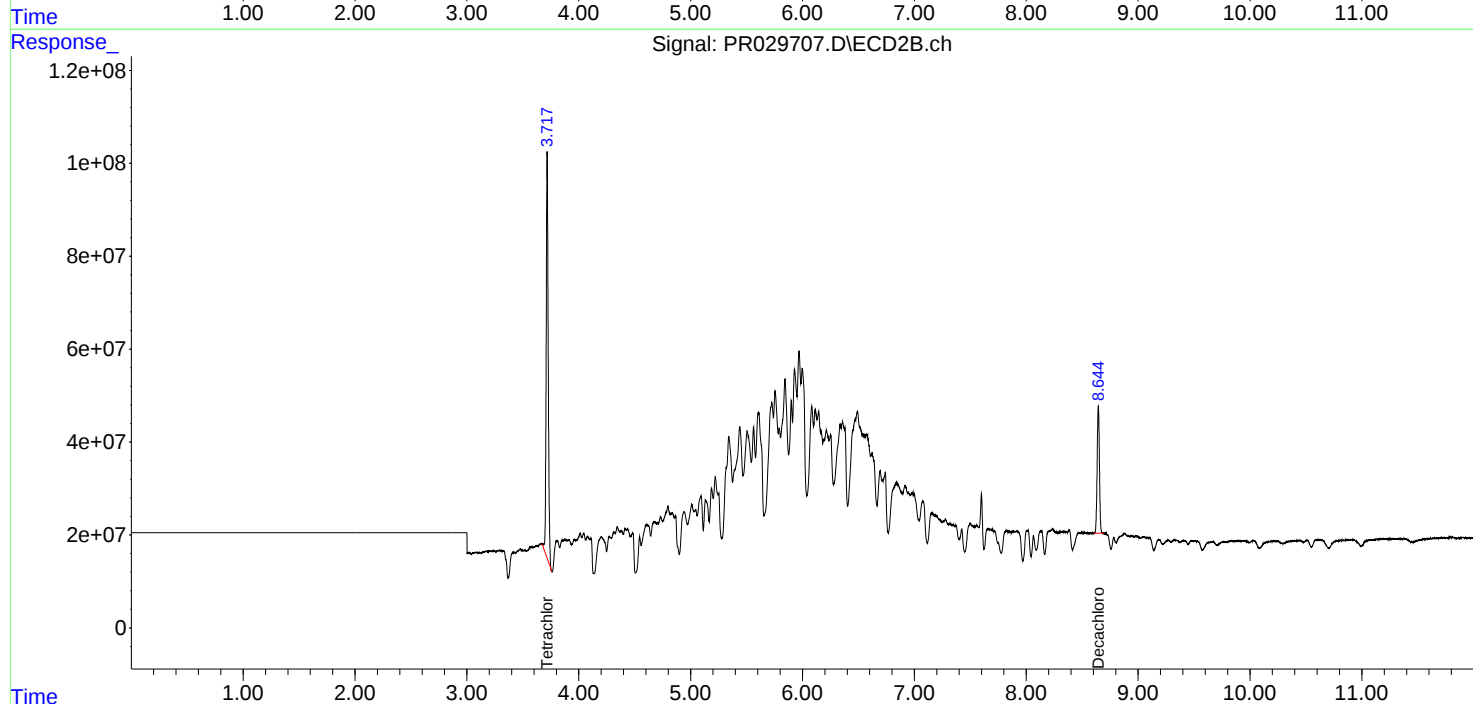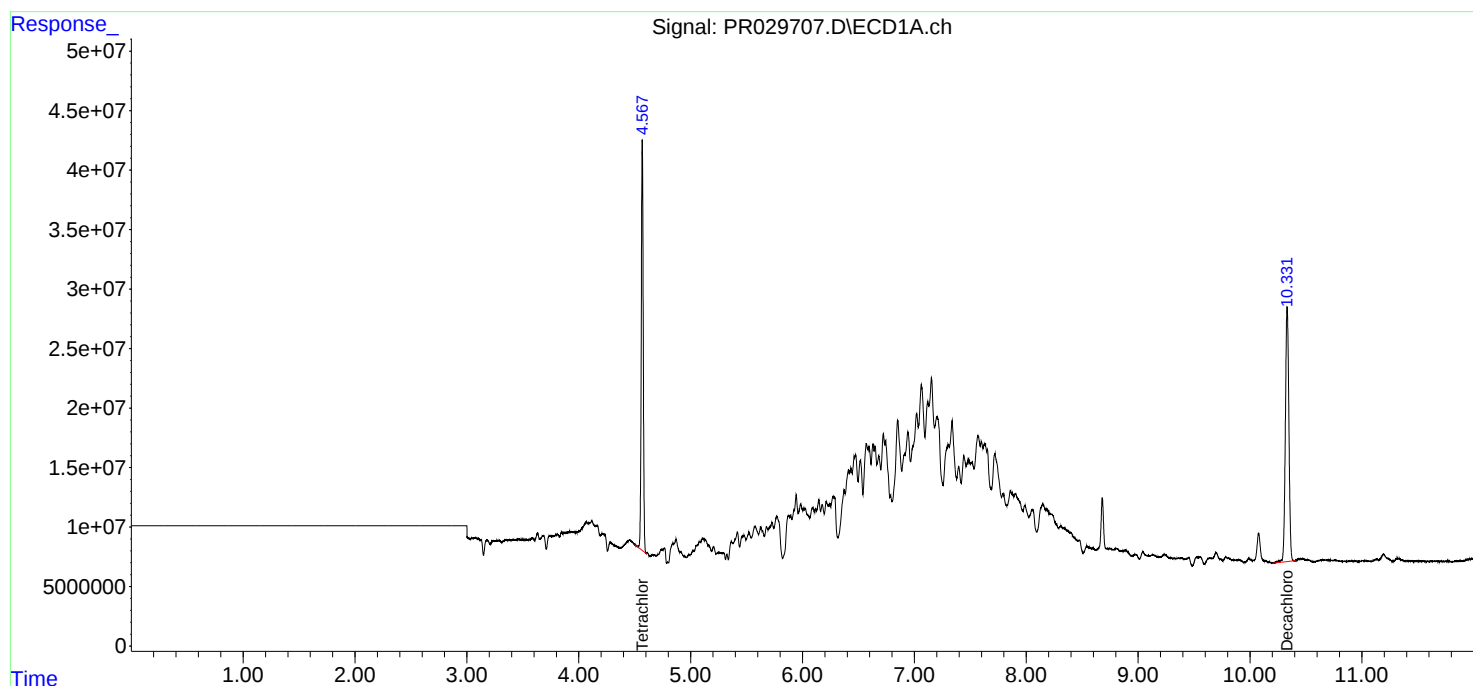

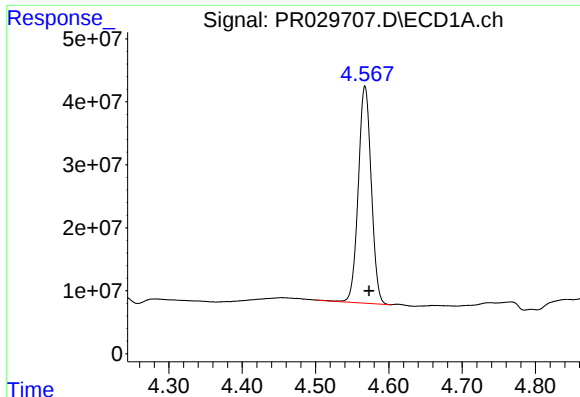


#1 Tetrachloro-m-xylene

R.T.: 4.568 min
Delta R.T.: -0.005 min
Response: 423455002
Conc: 18.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
02B-METAL-TO-GLASS-CAULK


Manual Integrations
APPROVED

mohammad
7/3/2018 4:26:33 PM

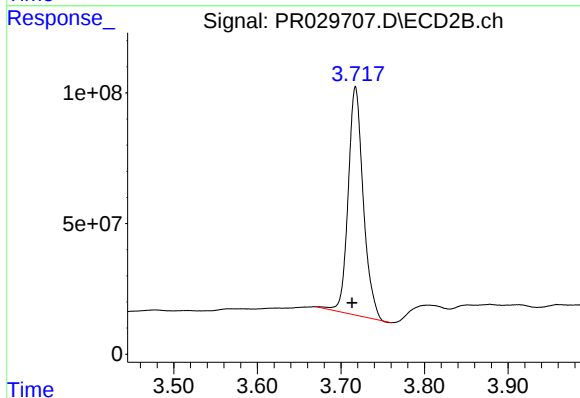


#1 Tetrachloro-m-xylene

R.T.: 3.717 min
Delta R.T.: 0.004 min
Response: 1096086734
Conc: 23.19 ng/ml

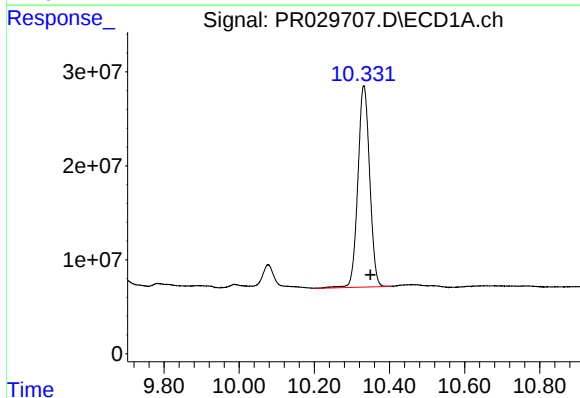

#2 Decachlorobiphenyl

R.T.: 10.332 min
Delta R.T.: -0.018 min
Response: 466553741
Conc: 16.67 ng/ml

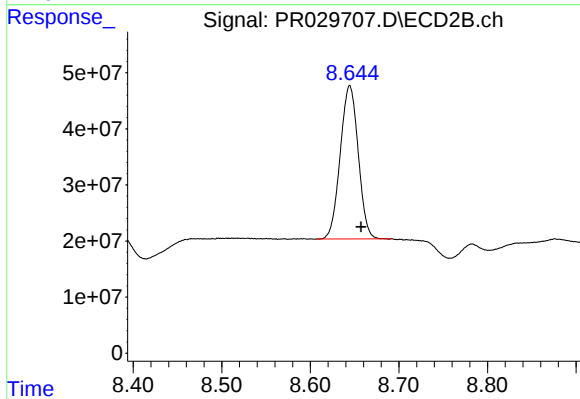

#2 Decachlorobiphenyl

R.T.: 8.644 min
Delta R.T.: -0.013 min
Response: 385532675
Conc: 19.52 ng/ml m