

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071119\
 Data File : PR039266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 02:36
 Operator : SM\AJ
 Sample : K3751-01
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MANHOLE-TEST-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 07:35:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 12 04:20:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.761	4.607	59446156	241.7E6	21.777	25.050
2) SA Decachlor...	8.699	10.342	28577793	104.2E6	13.676	15.221
Target Compounds						
9) L2 AR-1221-2	4.056	0.000	704374	0	39.240	N.D. #
33) L7 AR-1260-3	6.620	0.000	7490751	0	55.825	N.D. #
35) L7 AR-1260-5	7.326	0.000	24172841	0	90.617	N.D. #
37) L8 AR-1262-2	7.326	0.000	24172841	0	71.059	N.D. #
39) L8 AR-1262-4	0.000	8.957	0	118.3E6	N.D.	253.242 #
42) L9 AR-1268-2	0.000	8.957	0	118.3E6	N.D.	129.828 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071119\
Data File : PR039266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 02:36
Operator : SM\AJ
Sample : K3751-01
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 07:35:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071119.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 12 04:20:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

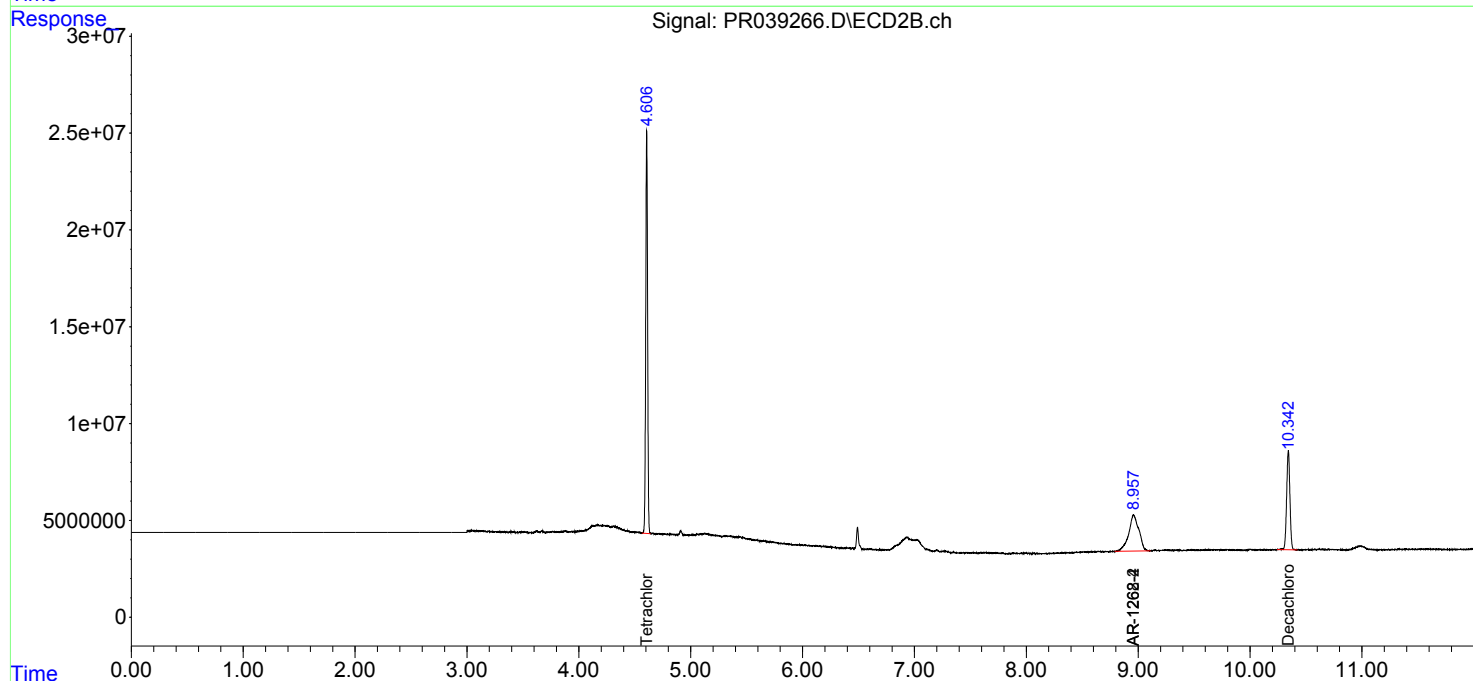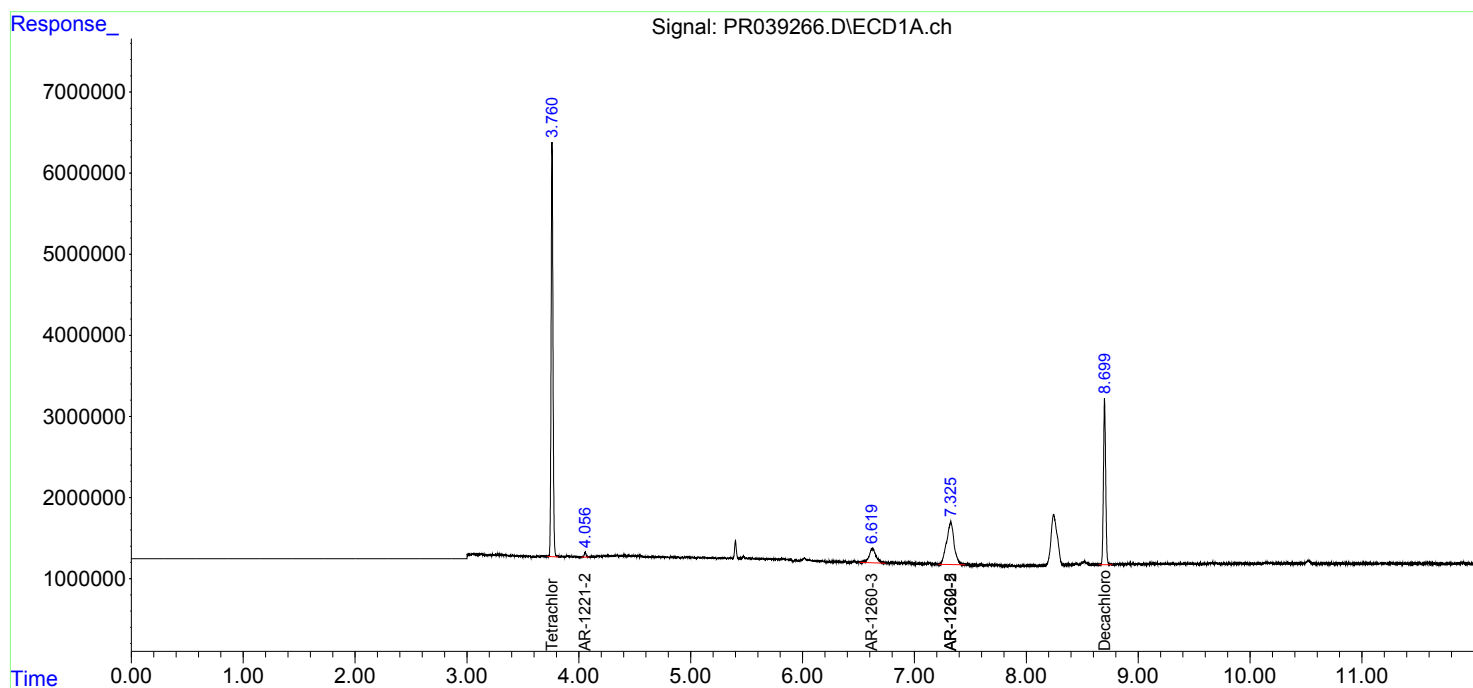


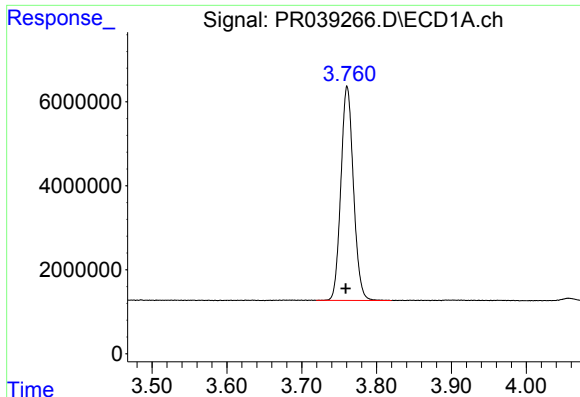

#1 Tetrachloro-m-xylene


R.T.: 3.761 min
Delta R.T.: 0.002 min
Response: 59446156
Conc: 21.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PIT

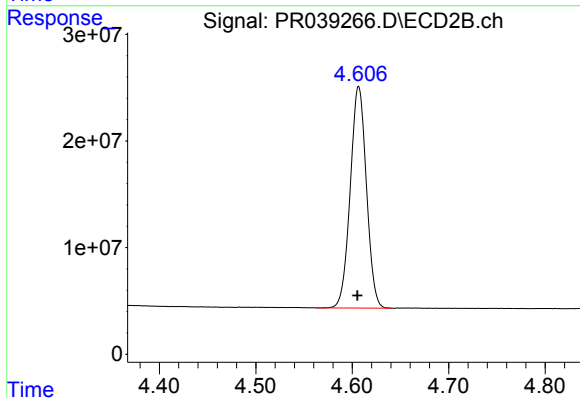


#1 Tetrachloro-m-xylene

R.T.: 4.607 min
Delta R.T.: 0.001 min
Response: 241684833
Conc: 25.05 ng/ml

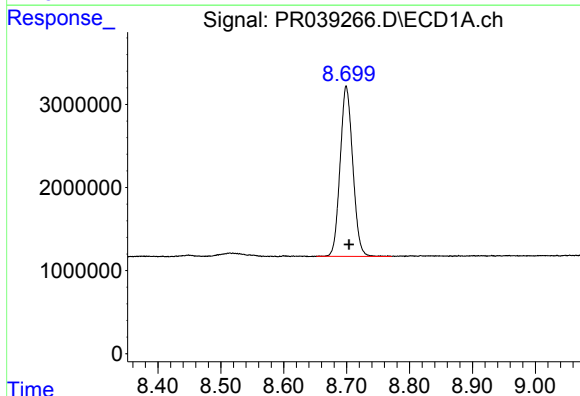


#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: -0.004 min
Response: 28577793
Conc: 13.68 ng/ml

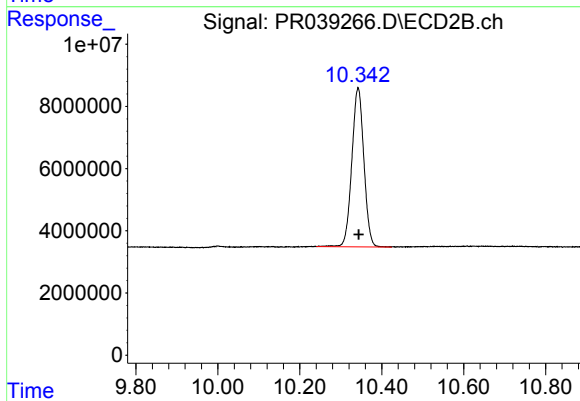

#2 Decachlorobiphenyl


R.T.: 10.342 min
Delta R.T.: -0.002 min
Response: 104152997
Conc: 15.22 ng/ml

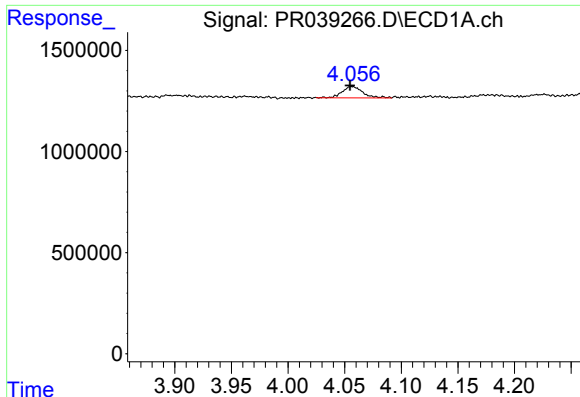

#9 AR-1221-2


R.T.: 4.056 min
Delta R.T.: 0.002 min
Response: 704374
Conc: 39.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PIT

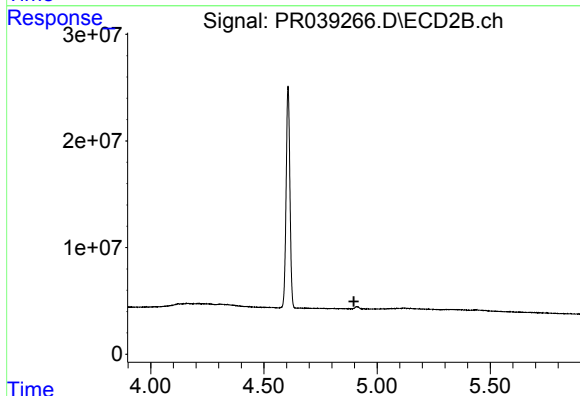


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.897 min
Response: 0
Conc: N.D.

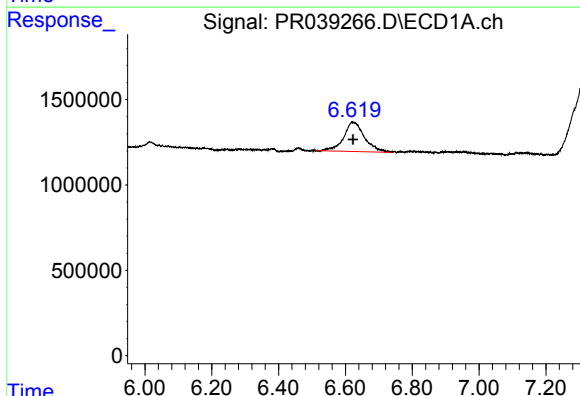


#33 AR-1260-3

R.T.: 6.620 min
Delta R.T.: -0.003 min
Response: 7490751
Conc: 55.83 ng/ml

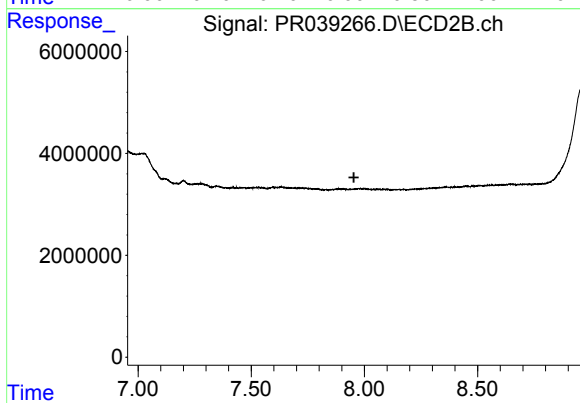

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

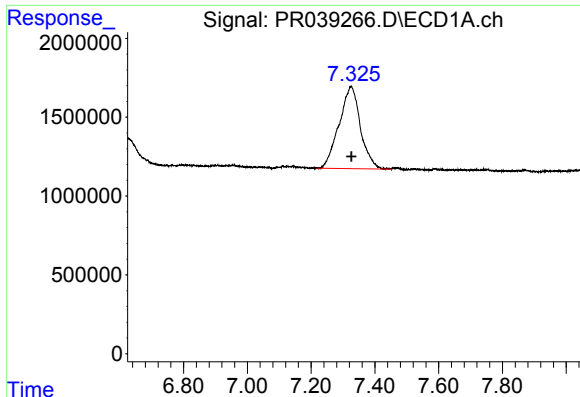

#35 AR-1260-5


R.T.: 7.326 min
Delta R.T.: 0.000 min
Response: 24172841
Conc: 90.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PIT

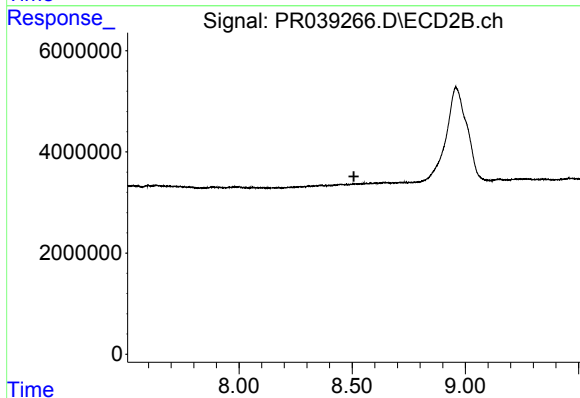


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.508 min
Response: 0
Conc: N.D.

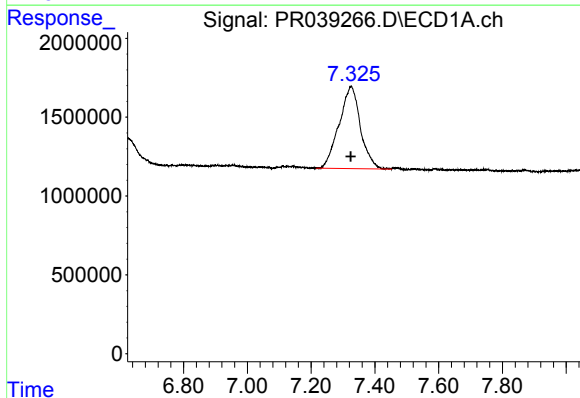


#37 AR-1262-2

R.T.: 7.326 min
Delta R.T.: 0.001 min
Response: 24172841
Conc: 71.06 ng/ml

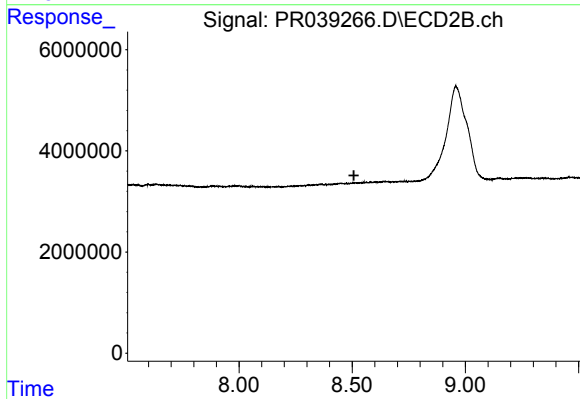

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.508 min
Response: 0
Conc: N.D.

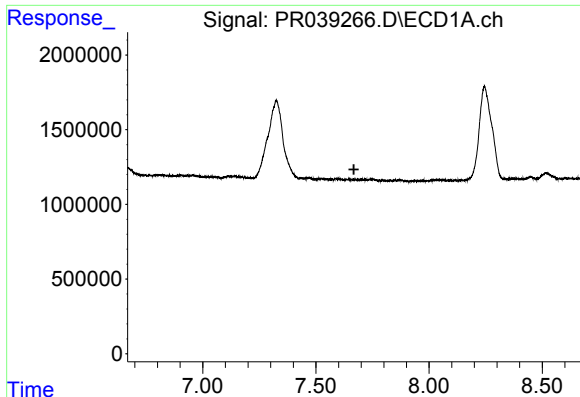

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 7.668 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PIT

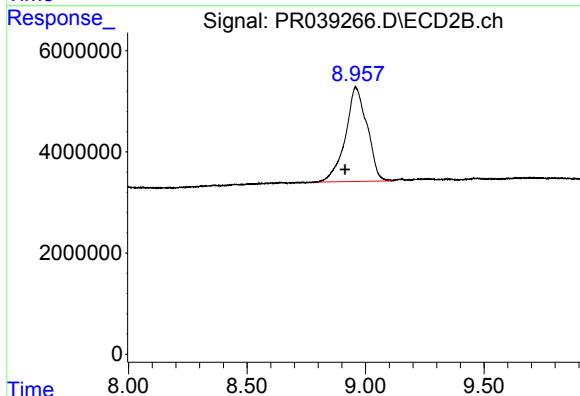


#39 AR-1262-4

R.T.: 8.957 min
Delta R.T.: 0.043 min
Response: 118329711
Conc: 253.24 ng/ml

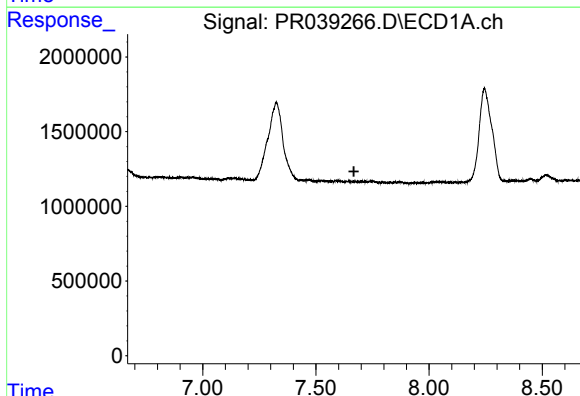

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 7.668 min
Response: 0
Conc: N.D.

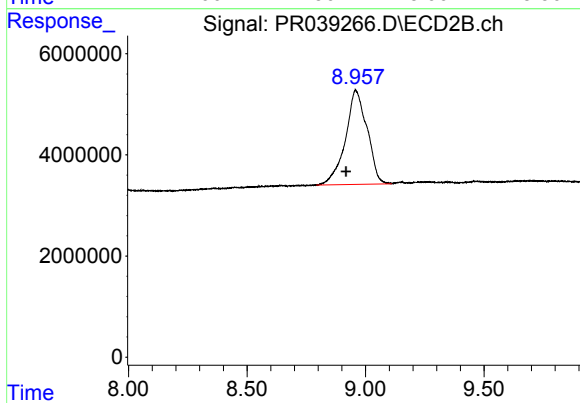

#42 AR-1268-2

R.T.: 8.957 min
Delta R.T.: 0.039 min
Response: 118329711
Conc: 129.83 ng/ml