

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071119\
 Data File : PR039268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 03:05
 Operator : SM\AJ
 Sample : K3751-03
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 DUCT-BANK-TEST-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 16:35:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 12 04:20:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.761	4.607	56626144	231.8E6	20.744	24.028
2) SA Decachlor...	8.701	10.342	31369179	113.8E6	15.012	16.630

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071119\
Data File : PR039268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 03:05
Operator : SM\AJ
Sample : K3751-03
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
DUCT-BANK-TEST-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 16:35:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071119.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 12 04:20:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

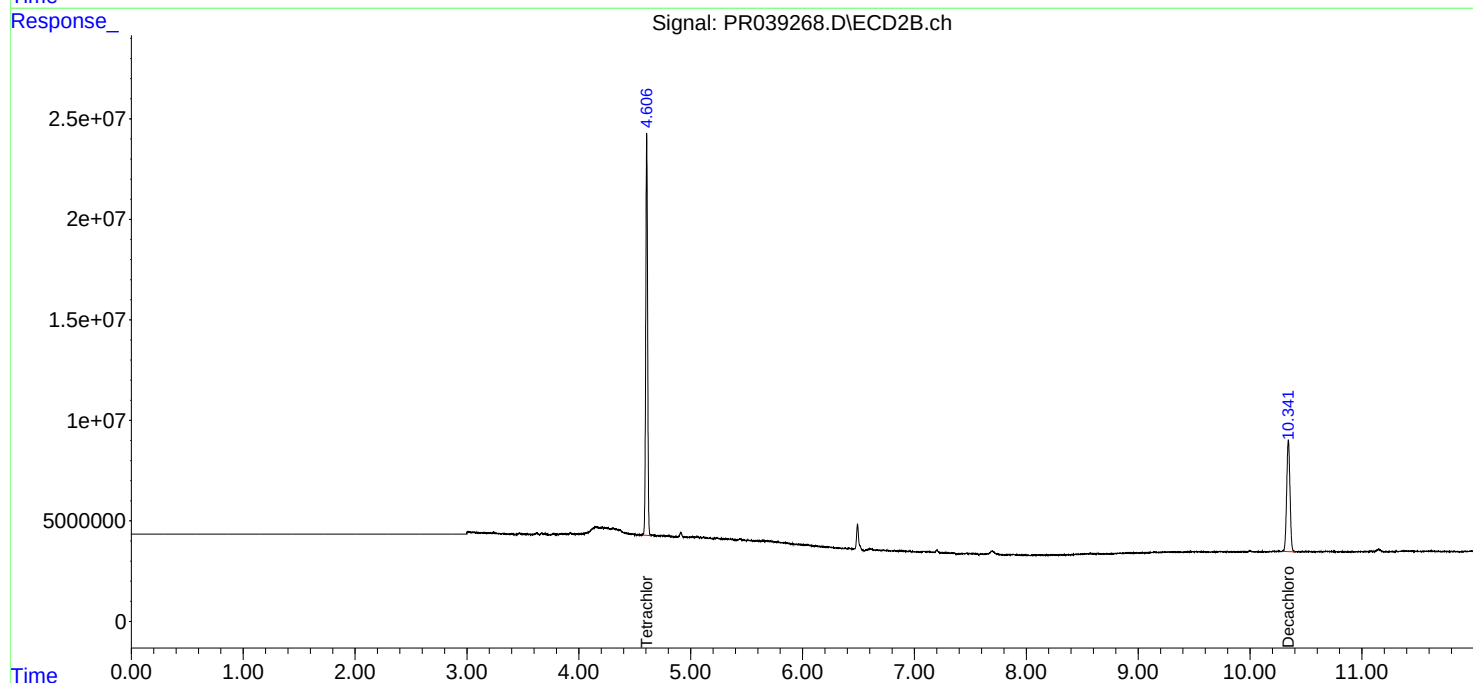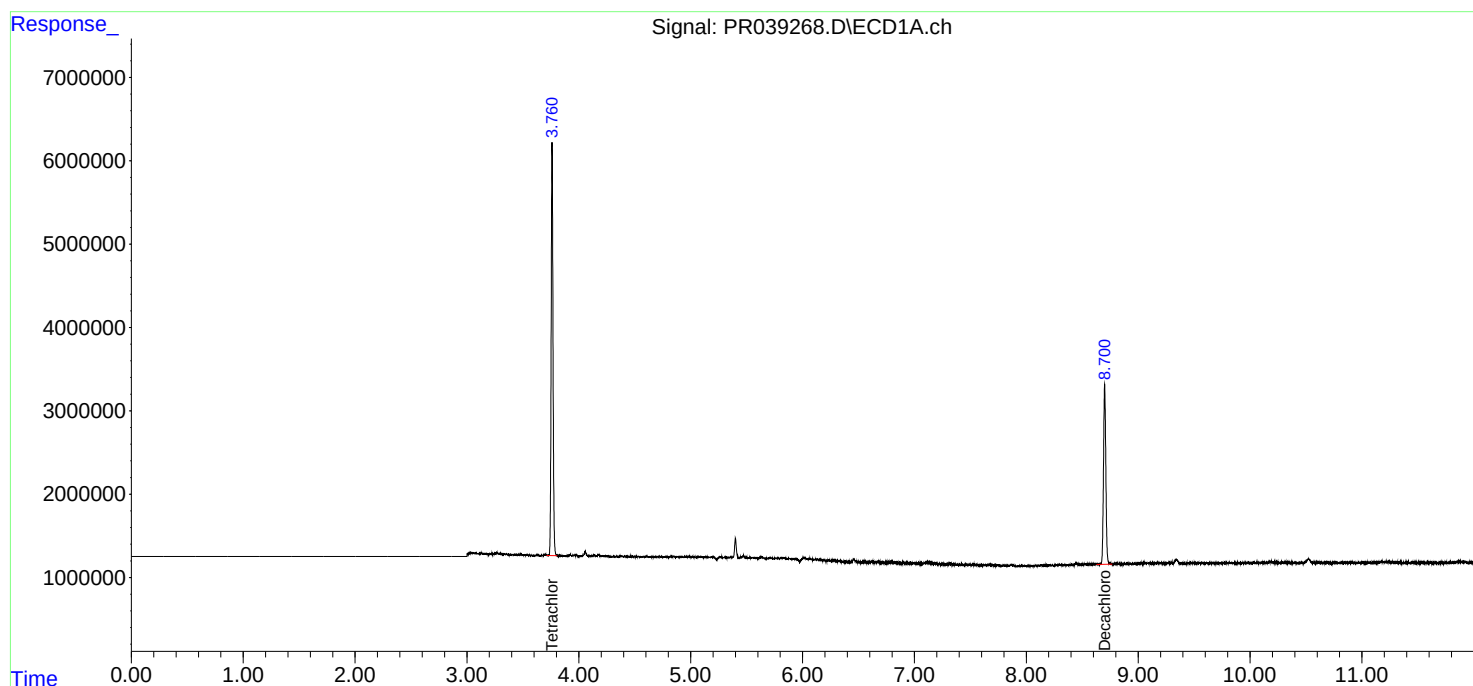


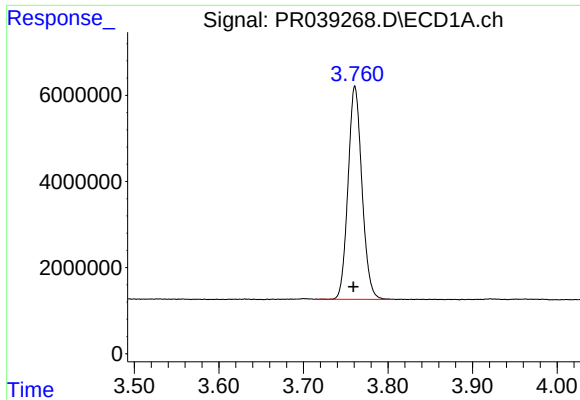

#1 Tetrachloro-m-xylene


R.T.: 3.761 min
Delta R.T.: 0.002 min
Response: 56626144
Conc: 20.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
DUCT-BANK-TEST-PIT

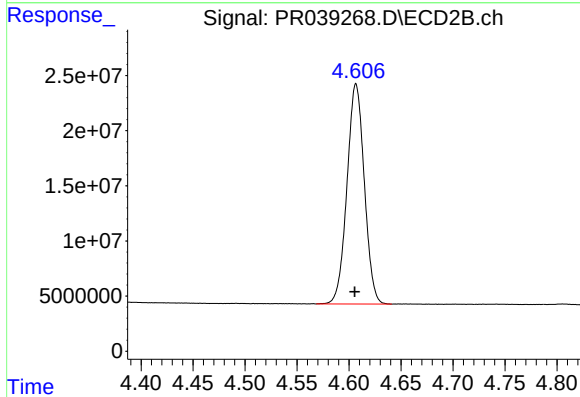


#1 Tetrachloro-m-xylene

R.T.: 4.607 min
Delta R.T.: 0.001 min
Response: 231824461
Conc: 24.03 ng/ml

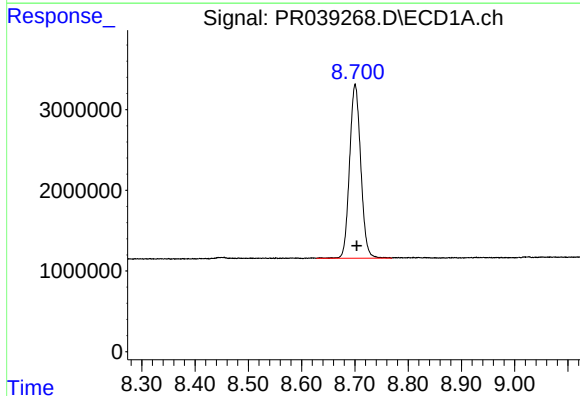

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.003 min
Response: 31369179
Conc: 15.01 ng/ml

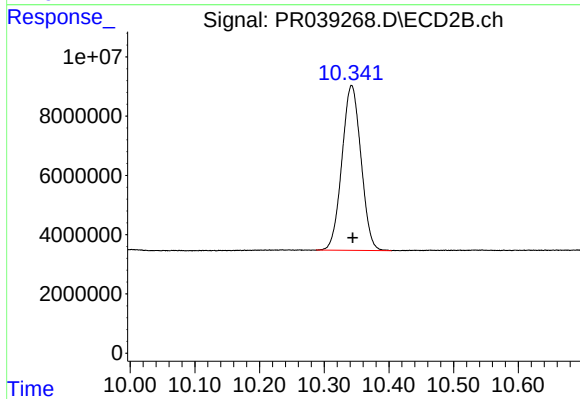

#2 Decachlorobiphenyl

R.T.: 10.342 min
Delta R.T.: -0.002 min
Response: 113798392
Conc: 16.63 ng/ml