

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071819\
 Data File : PR039398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 17:35
 Operator : SM\AJ
 Sample : K3751-01MS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MANHOLE-TEST-PITMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 01:32:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.760	4.604	55458205	227.2E6	35.805	35.128
2)	SA Decachlor...	8.702	10.342	49811823	180.5E6	20.370	21.094
Target Compounds							
3)	L1 AR-1016-1	4.830	5.760	23008063	95479582	382.605	381.700
4)	L1 AR-1016-2	4.847	5.782	33204861	137.1E6	338.022	375.729
5)	L1 AR-1016-3	5.020	5.844	17672892	79318304	355.754	360.336
6)	L1 AR-1016-4	5.061	5.943	14355274	68372128	359.021	365.491
7)	L1 AR-1016-5	5.270	6.232	14899875	67234404	273.912	366.314 #
9)	L2 AR-1221-2	4.056	4.896	2535447	9913401	199.742	214.551
10)	L2 AR-1221-3	4.131	4.972	10896343	41919659	275.066	278.063
11)	L3 AR-1232-1	4.131	4.972	10896343	41919659	366.904	381.305
12)	L3 AR-1232-2	4.847	5.496	33204861	84264125	899.519	1405.854 #
13)	L3 AR-1232-3	5.020	5.782	17672892	137.1E6	967.961	1057.016
14)	L3 AR-1232-4	5.103	5.943	15523369	68372128	974.284	1020.923
15)	L3 AR-1232-5	5.270	6.029	14899875	50509146	826.607	1108.276 #
16)	L4 AR-1242-1	4.830	5.760	23008063	95479582	435.462	444.353
17)	L4 AR-1242-2	4.847	5.782	33204861	137.1E6	381.015	438.578
18)	L4 AR-1242-3	5.020	5.844	17672892	79318304	406.023	416.135
19)	L4 AR-1242-4	5.103	5.943	15523369	68372128	360.490	426.028
20)	L4 AR-1242-5	5.617	6.669	14024017	10291570	224.431	54.581 #
21)	L5 AR-1248-1	4.830	5.760	23008063	95479582	531.602	558.471
22)	L5 AR-1248-2	5.061	6.029	14355274	50509146	228.849	215.059
23)	L5 AR-1248-3	5.103	6.232	15523369	67234404	237.782	243.275
24)	L5 AR-1248-4	5.270	6.641	14899875	15983957	181.759	47.631 #
25)	L5 AR-1248-5	5.617	6.669	14024017	10291570	160.509	32.060 #
26)	L6 AR-1254-1	5.617	6.604	14024017	54898941	106.037	171.452 #
27)	L6 AR-1254-2	5.761	6.818	14982919	54655235	127.907	106.805
28)	L6 AR-1254-3	6.172	7.185	37471755	19465511	181.345	32.437 #
29)	L6 AR-1254-4	6.382	7.465	5198850	30194332	33.958	69.770 #
30)	L6 AR-1254-5	6.794	7.879	52407923	170.5E6	281.311	362.723 #
31)	L7 AR-1260-1	6.286	7.344	37172864	117.9E6	324.363	324.641
32)	L7 AR-1260-2	6.470	7.596	47600361	135.9E6	315.629	310.695
33)	L7 AR-1260-3	6.622	7.951	41221155	84390747	306.287	248.662
34)	L7 AR-1260-4	7.088	8.181	30433769	107.8E6	254.270	265.313
35)	L7 AR-1260-5	7.326	8.507	75351491	210.9E6	250.727	246.587
36)	L8 AR-1262-1	6.884	7.951	14520149	84390747	153.174	121.522
37)	L8 AR-1262-2	7.326	8.507	75351491	210.9E6	154.884	153.836
38)	L8 AR-1262-3	7.605	8.843	14640909	141.4E6	80.615	157.003 #
39)	L8 AR-1262-4	7.670	8.898	46567915	72844253	130.888	108.496
40)	L8 AR-1262-5	8.160	9.583	15358679	48916869	94.179	99.928
41)	L9 AR-1268-1	7.605	8.843	14640909	141.4E6	27.117	89.754 #
42)	L9 AR-1268-2	7.670	8.898	46567915	72844253	94.015	49.658 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071819\
 Data File : PR039398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 17:35
 Operator : SM\AJ
 Sample : K3751-01MS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MANHOLE-TEST-PITMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 01:32:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.160	9.583	15358679	48916869	85.971	92.329
45) L9	AR-1268-5	8.450	10.002	4819694	17641770	3.550	4.113



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071819\
Data File : PR039398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 17:35
Operator : SM\AJ
Sample : K3751-01MS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 01:32:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 02:56:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

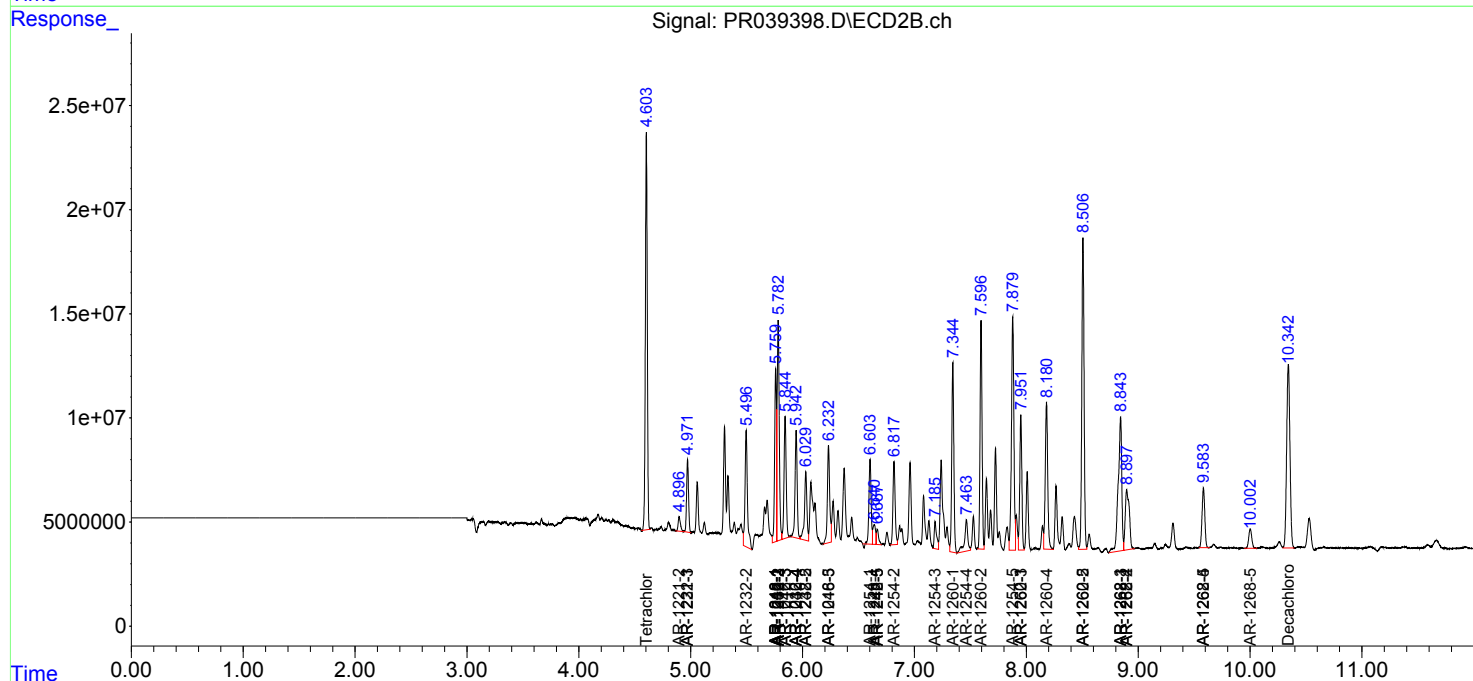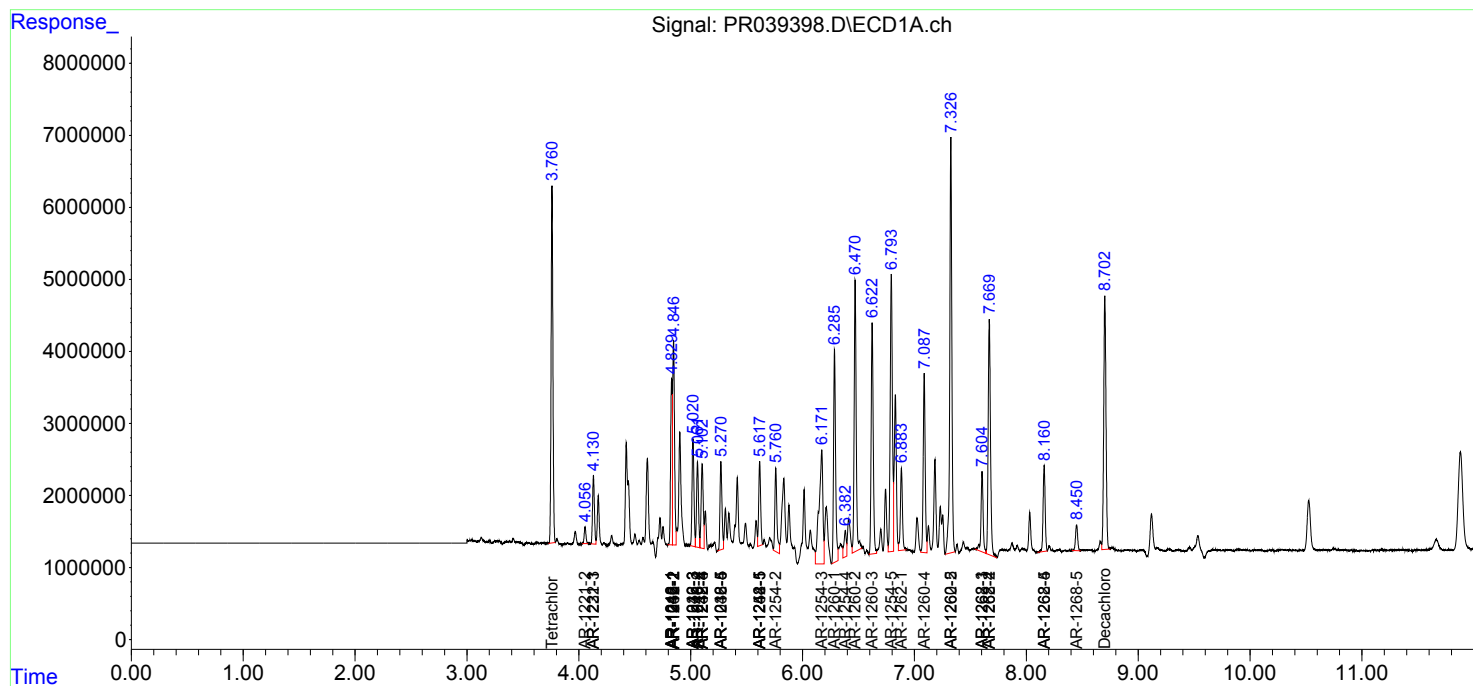


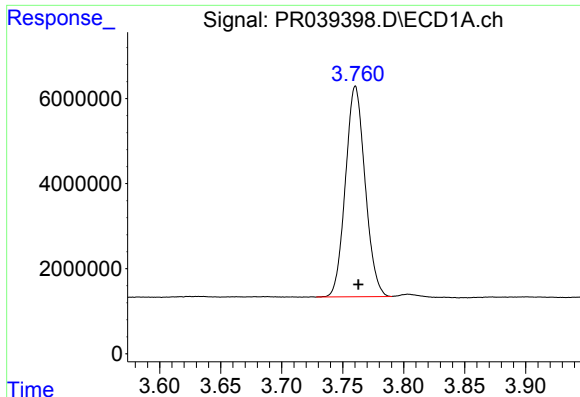

#1 Tetrachloro-m-xylene


R.T.: 3.760 min
Delta R.T.: -0.003 min
Response: 55458205
Conc: 35.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

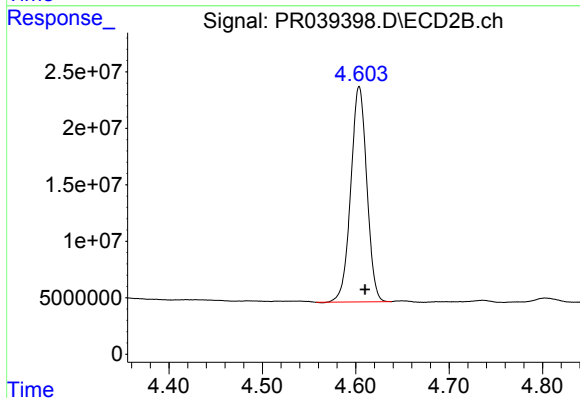


#1 Tetrachloro-m-xylene

R.T.: 4.604 min
Delta R.T.: -0.006 min
Response: 227179410
Conc: 35.13 ng/ml

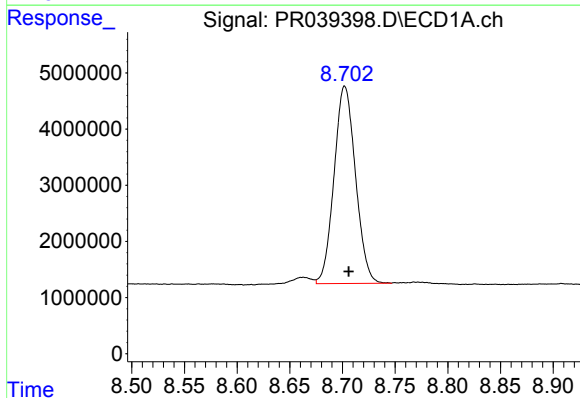


#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.004 min
Response: 49811823
Conc: 20.37 ng/ml

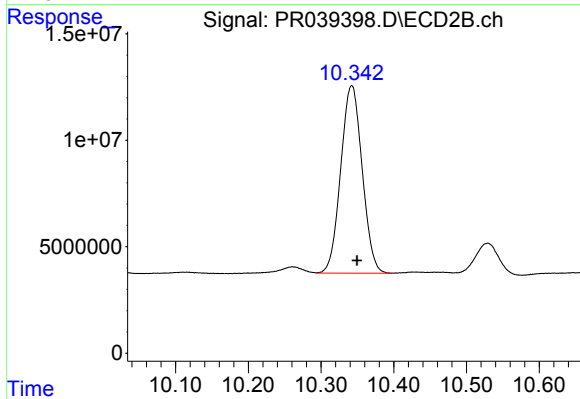

#2 Decachlorobiphenyl


R.T.: 10.342 min
Delta R.T.: -0.007 min
Response: 180516731
Conc: 21.09 ng/ml

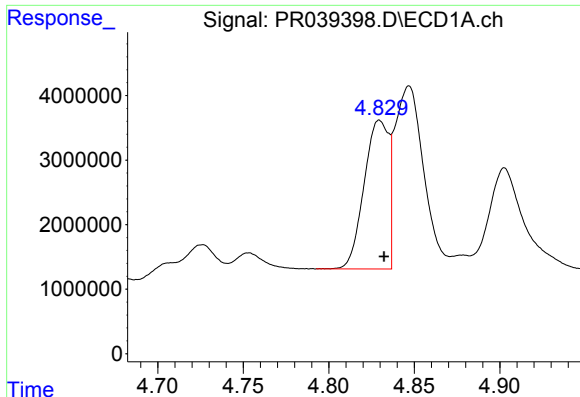

#3 AR-1016-1


R.T.: 4.830 min
Delta R.T.: -0.003 min
Response: 23008063
Conc: 382.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

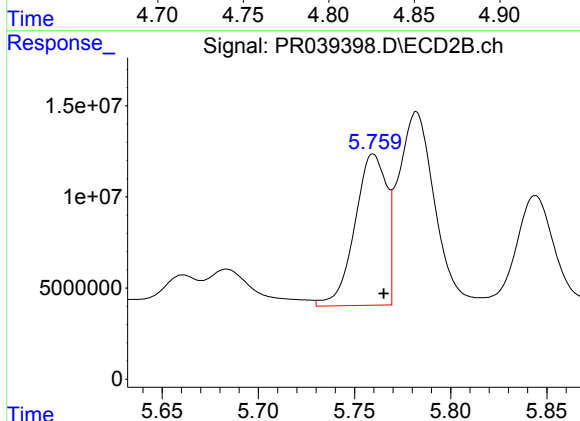


#3 AR-1016-1

R.T.: 5.760 min
Delta R.T.: -0.005 min
Response: 95479582
Conc: 381.70 ng/ml

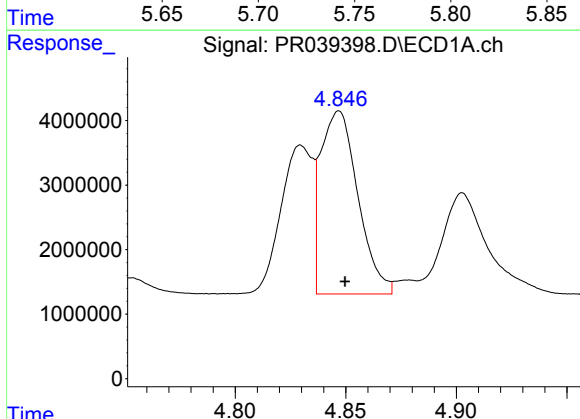


#4 AR-1016-2

R.T.: 4.847 min
Delta R.T.: -0.003 min
Response: 33204861
Conc: 338.02 ng/ml

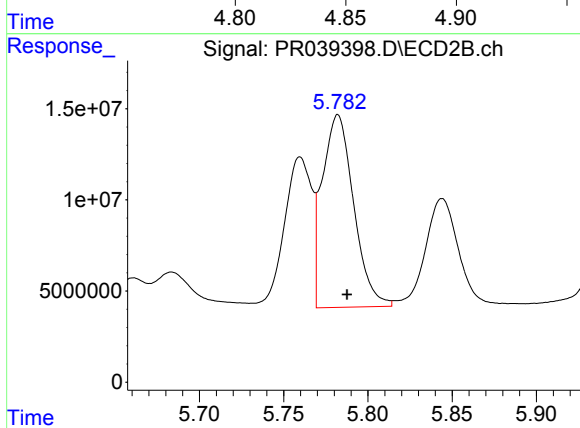

#4 AR-1016-2


R.T.: 5.782 min
Delta R.T.: -0.006 min
Response: 137086798
Conc: 375.73 ng/ml

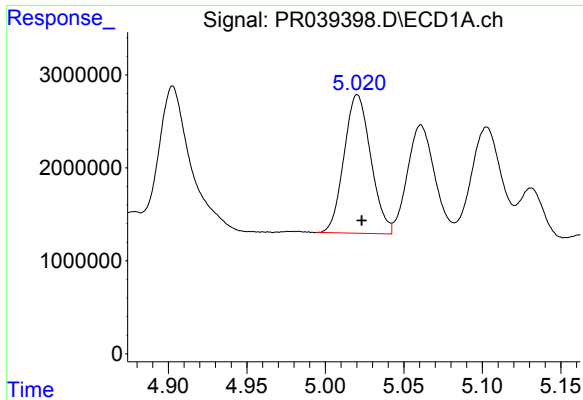

#5 AR-1016-3


R.T.: 5.020 min
Delta R.T.: -0.003 min
Response: 17672892
Conc: 355.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

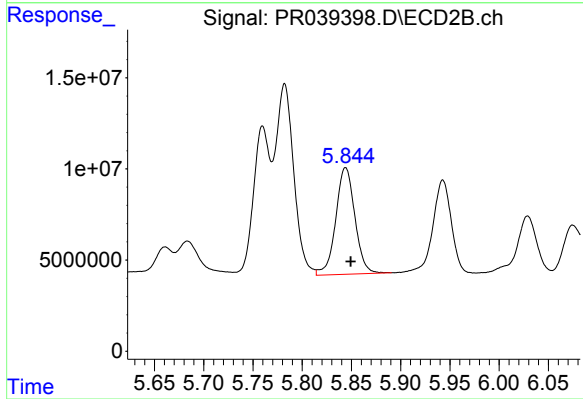


#5 AR-1016-3

R.T.: 5.844 min
Delta R.T.: -0.005 min
Response: 79318304
Conc: 360.34 ng/ml

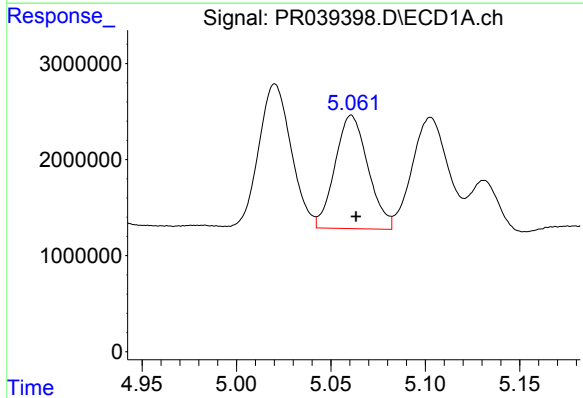


#6 AR-1016-4

R.T.: 5.061 min
Delta R.T.: -0.002 min
Response: 14355274
Conc: 359.02 ng/ml

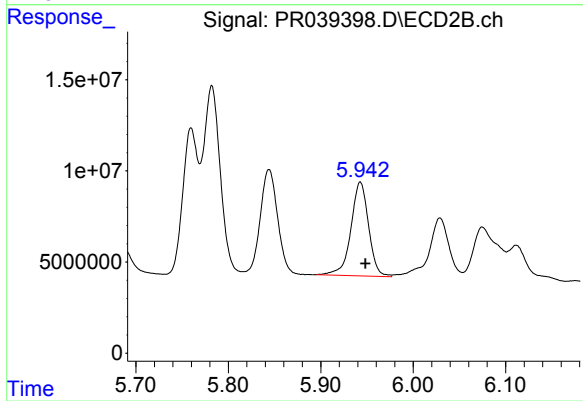

#6 AR-1016-4


R.T.: 5.943 min
Delta R.T.: -0.006 min
Response: 68372128
Conc: 365.49 ng/ml

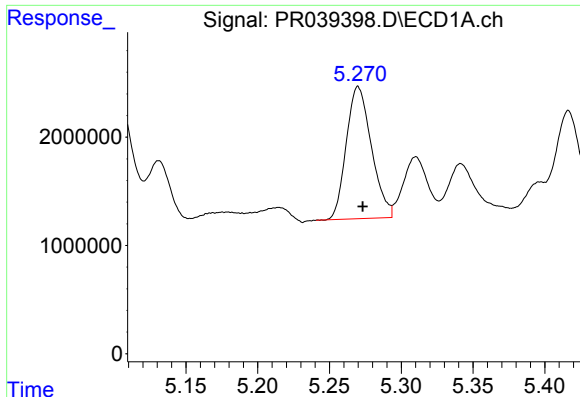

#7 AR-1016-5


R.T.: 5.270 min
Delta R.T.: -0.003 min
Response: 14899875
Conc: 273.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

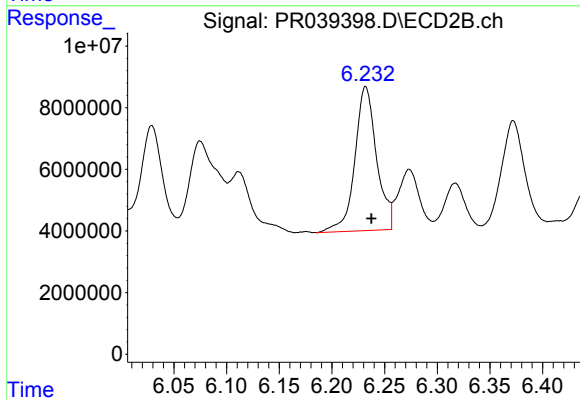


#7 AR-1016-5

R.T.: 6.232 min
Delta R.T.: -0.005 min
Response: 67234404
Conc: 366.31 ng/ml

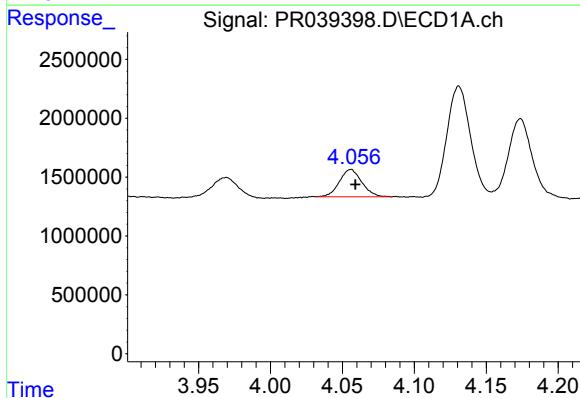


#9 AR-1221-2

R.T.: 4.056 min
Delta R.T.: -0.003 min
Response: 2535447
Conc: 199.74 ng/ml

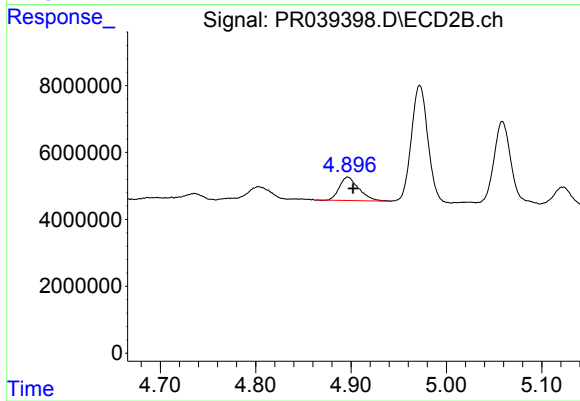

#9 AR-1221-2


R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 9913401
Conc: 214.55 ng/ml

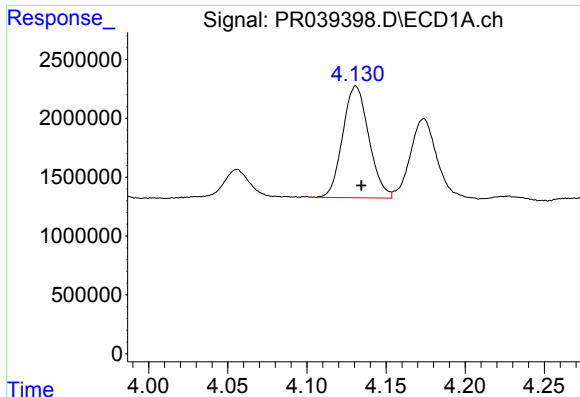

#10 AR-1221-3


R.T.: 4.131 min
Delta R.T.: -0.003 min
Response: 10896343
Conc: 275.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

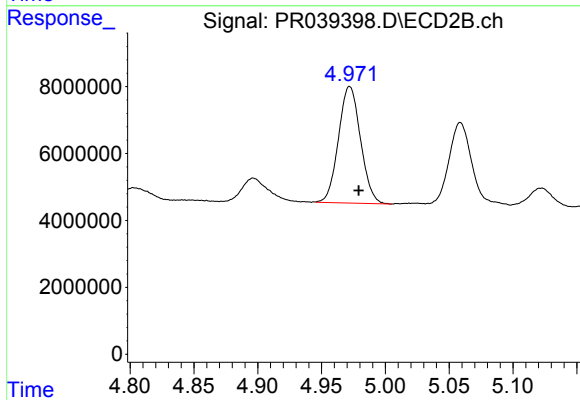


#10 AR-1221-3

R.T.: 4.972 min
Delta R.T.: -0.007 min
Response: 41919659
Conc: 278.06 ng/ml

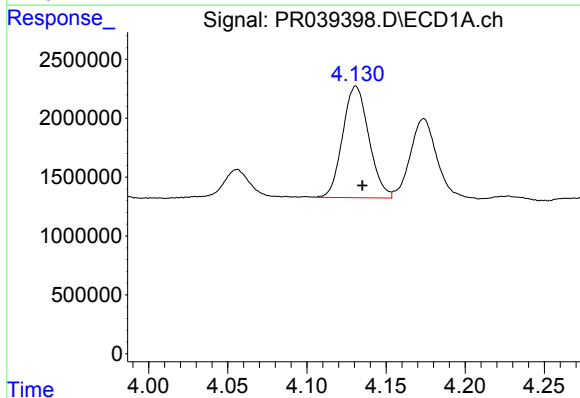


#11 AR-1232-1

R.T.: 4.131 min
Delta R.T.: -0.004 min
Response: 10896343
Conc: 366.90 ng/ml

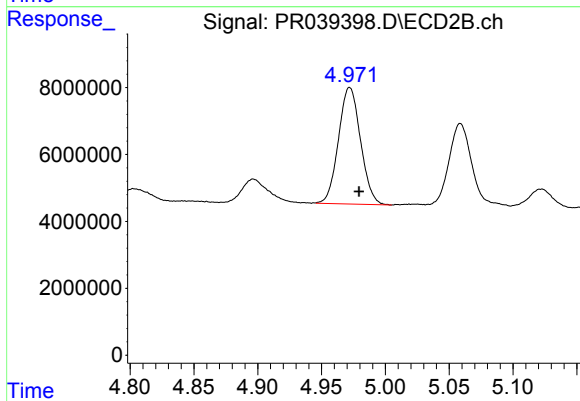

#11 AR-1232-1


R.T.: 4.972 min
Delta R.T.: -0.007 min
Response: 41919659
Conc: 381.30 ng/ml

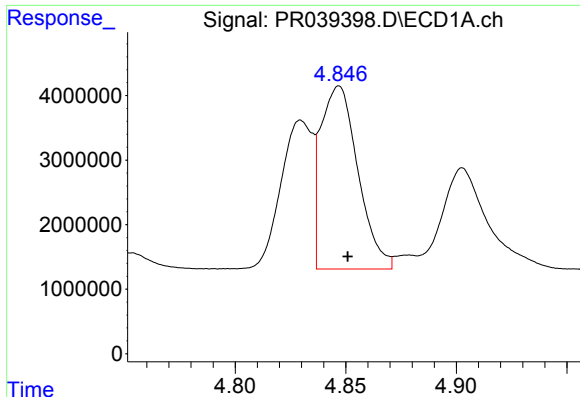

#12 AR-1232-2


R.T.: 4.847 min
Delta R.T.: -0.004 min
Response: 33204861
Conc: 899.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

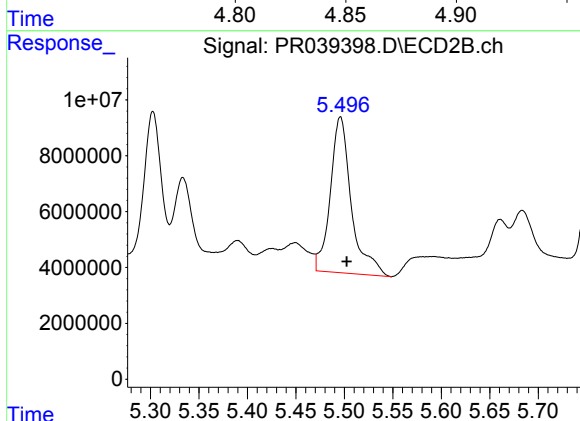


#12 AR-1232-2

R.T.: 5.496 min
Delta R.T.: -0.006 min
Response: 84264125
Conc: 1405.85 ng/ml

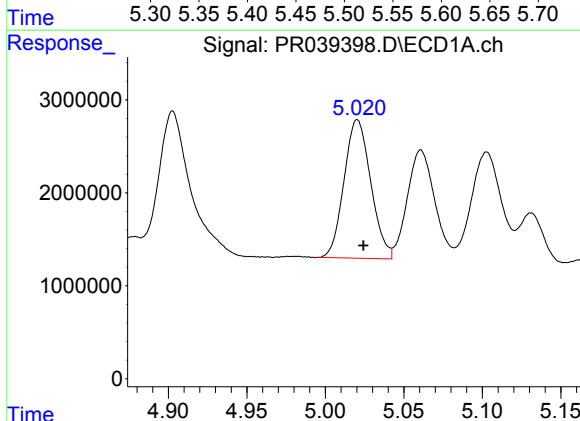


#13 AR-1232-3

R.T.: 5.020 min
Delta R.T.: -0.004 min
Response: 17672892
Conc: 967.96 ng/ml

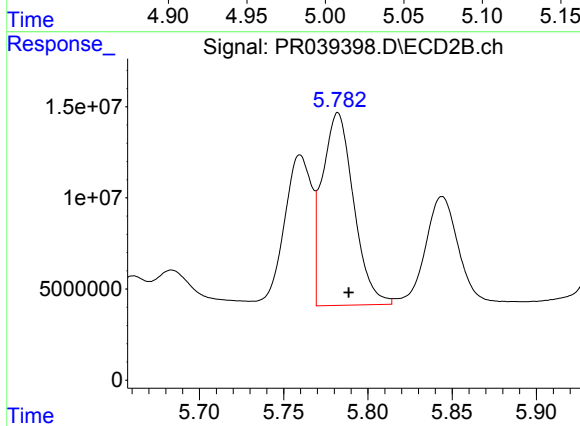

#13 AR-1232-3


R.T.: 5.782 min
Delta R.T.: -0.006 min
Response: 137086798
Conc: 1057.02 ng/ml

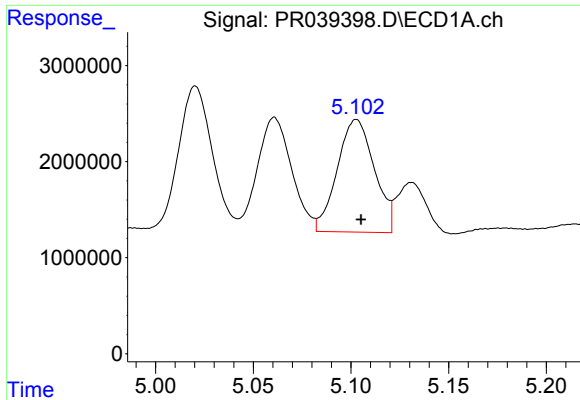

#14 AR-1232-4


R.T.: 5.103 min
Delta R.T.: -0.002 min
Response: 15523369
Conc: 974.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

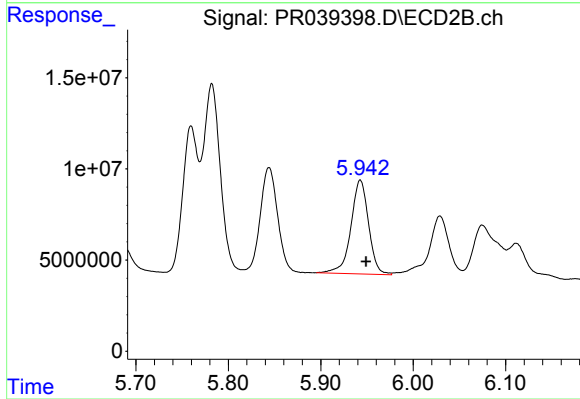


#14 AR-1232-4

R.T.: 5.943 min
Delta R.T.: -0.006 min
Response: 68372128
Conc: 1020.92 ng/ml

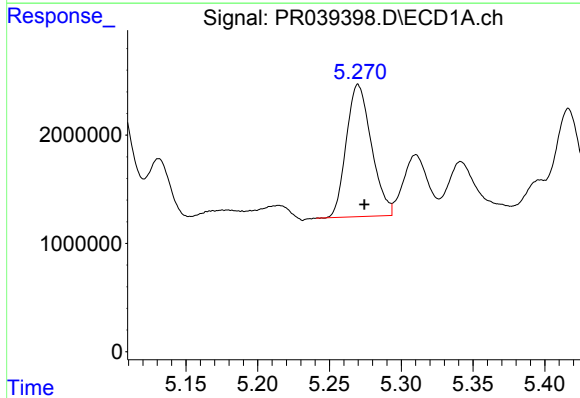


#15 AR-1232-5

R.T.: 5.270 min
Delta R.T.: -0.004 min
Response: 14899875
Conc: 826.61 ng/ml

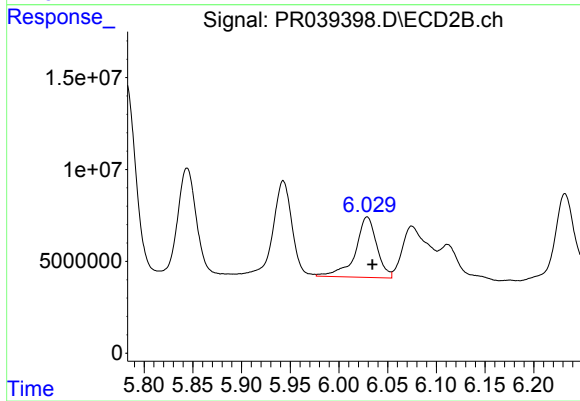

#15 AR-1232-5


R.T.: 6.029 min
Delta R.T.: -0.005 min
Response: 50509146
Conc: 1108.28 ng/ml

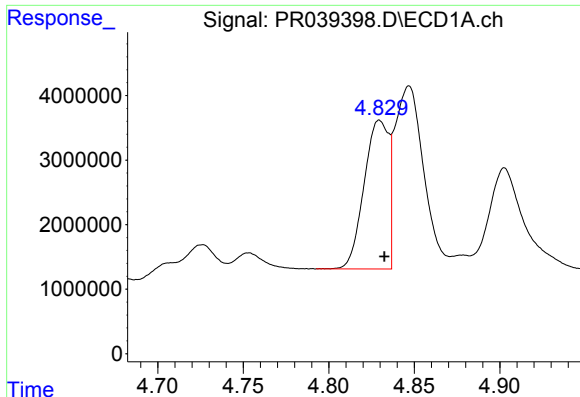

#16 AR-1242-1


R.T.: 4.830 min
Delta R.T.: -0.003 min
Response: 23008063
Conc: 435.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

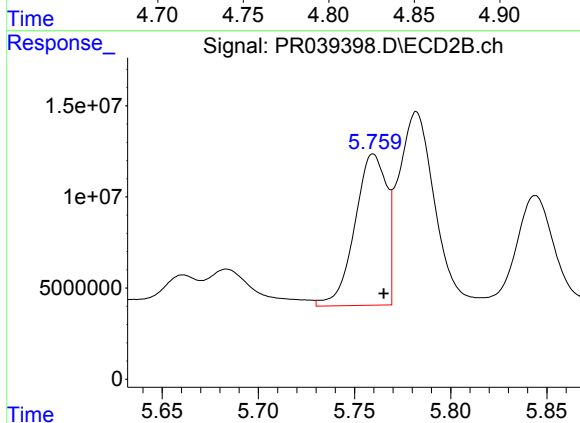


#16 AR-1242-1

R.T.: 5.760 min
Delta R.T.: -0.005 min
Response: 95479582
Conc: 444.35 ng/ml

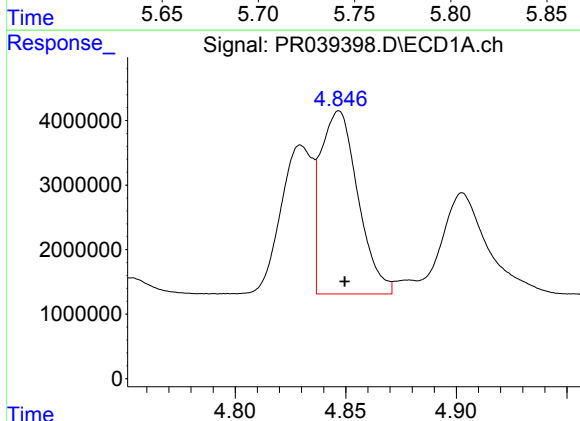


#17 AR-1242-2

R.T.: 4.847 min
Delta R.T.: -0.003 min
Response: 33204861
Conc: 381.02 ng/ml

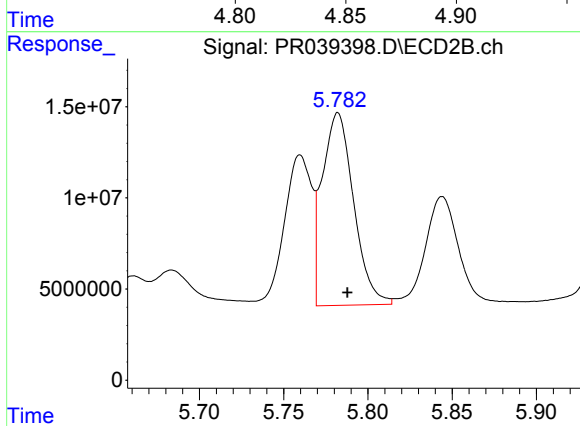

#17 AR-1242-2


R.T.: 5.782 min
Delta R.T.: -0.006 min
Response: 137086798
Conc: 438.58 ng/ml

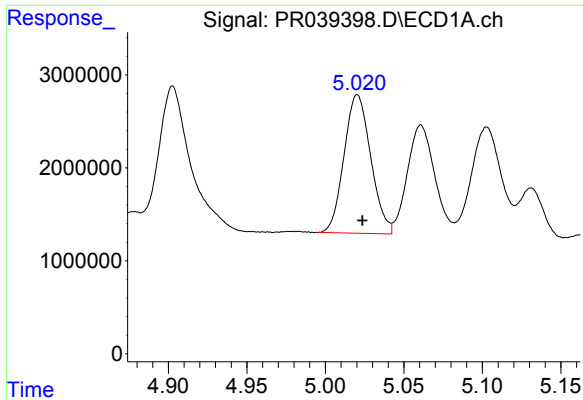

#18 AR-1242-3


R.T.: 5.020 min
Delta R.T.: -0.003 min
Response: 17672892
Conc: 406.02 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

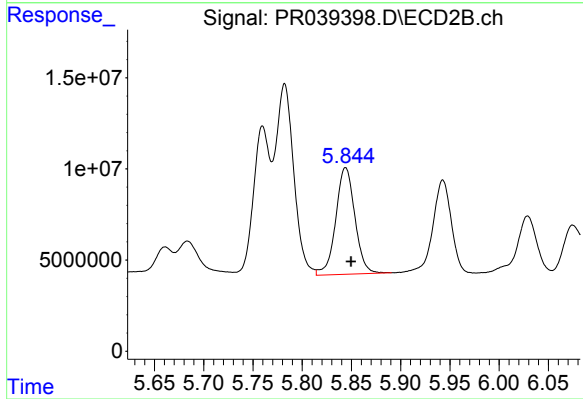


#18 AR-1242-3

R.T.: 5.844 min
Delta R.T.: -0.006 min
Response: 79318304
Conc: 416.14 ng/ml

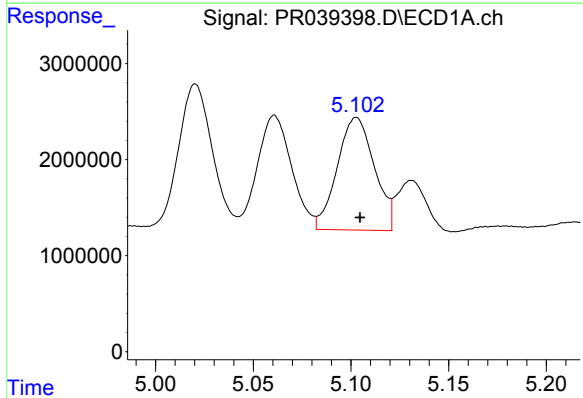


#19 AR-1242-4

R.T.: 5.103 min
Delta R.T.: -0.002 min
Response: 15523369
Conc: 360.49 ng/ml

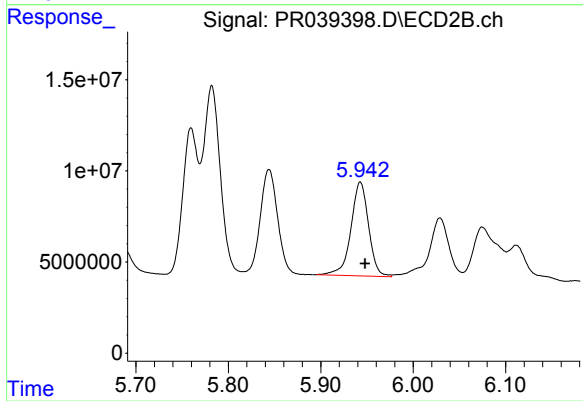

#19 AR-1242-4


R.T.: 5.943 min
Delta R.T.: -0.005 min
Response: 68372128
Conc: 426.03 ng/ml

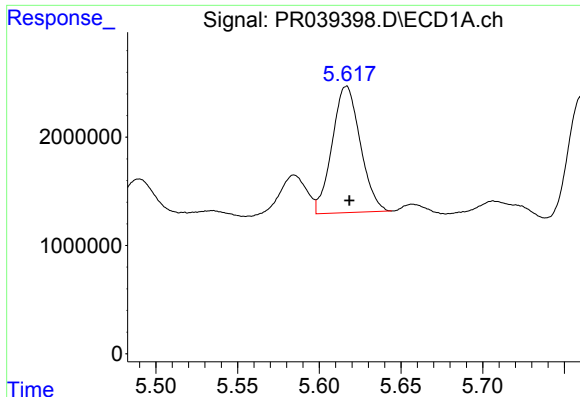

#20 AR-1242-5


R.T.: 5.617 min
Delta R.T.: -0.002 min
Response: 14024017
Conc: 224.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

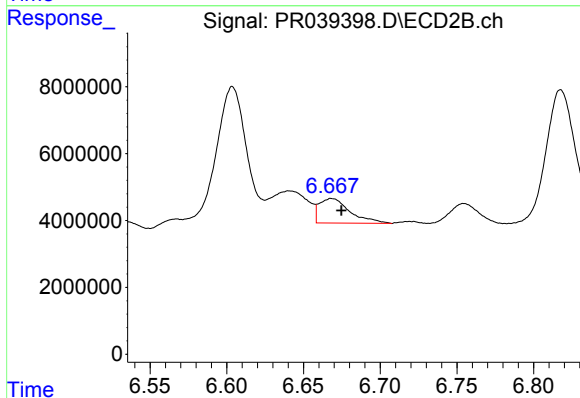


#20 AR-1242-5

R.T.: 6.669 min
Delta R.T.: -0.006 min
Response: 10291570
Conc: 54.58 ng/ml

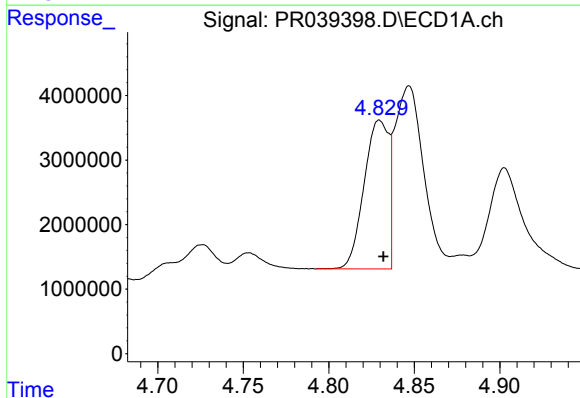


#21 AR-1248-1

R.T.: 4.830 min
Delta R.T.: -0.002 min
Response: 23008063
Conc: 531.60 ng/ml

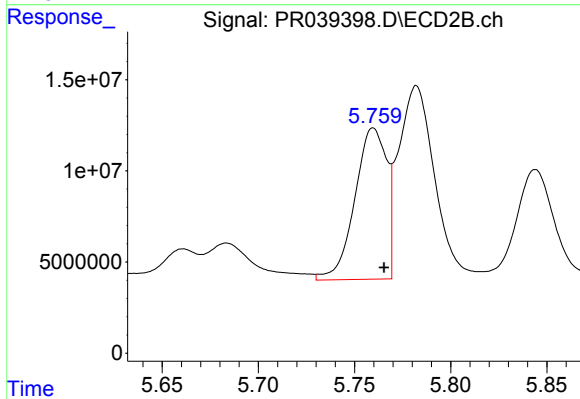

#21 AR-1248-1


R.T.: 5.760 min
Delta R.T.: -0.006 min
Response: 95479582
Conc: 558.47 ng/ml

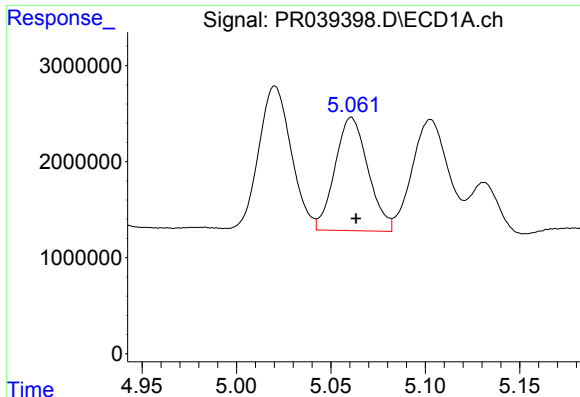

#22 AR-1248-2


R.T.: 5.061 min
Delta R.T.: -0.003 min
Response: 14355274
Conc: 228.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

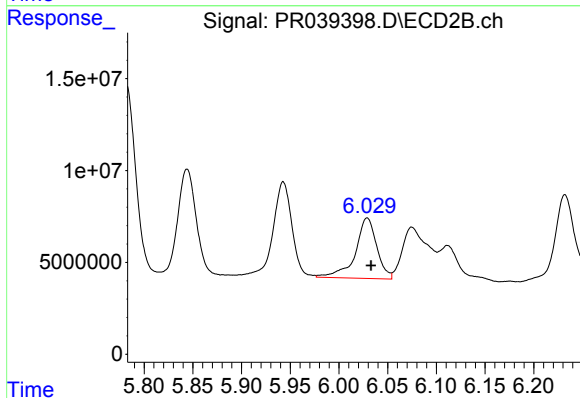


#22 AR-1248-2

R.T.: 6.029 min
Delta R.T.: -0.004 min
Response: 50509146
Conc: 215.06 ng/ml

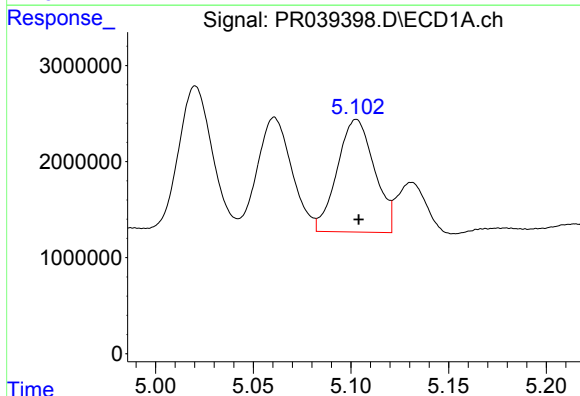


#23 AR-1248-3

R.T.: 5.103 min
Delta R.T.: -0.001 min
Response: 15523369
Conc: 237.78 ng/ml

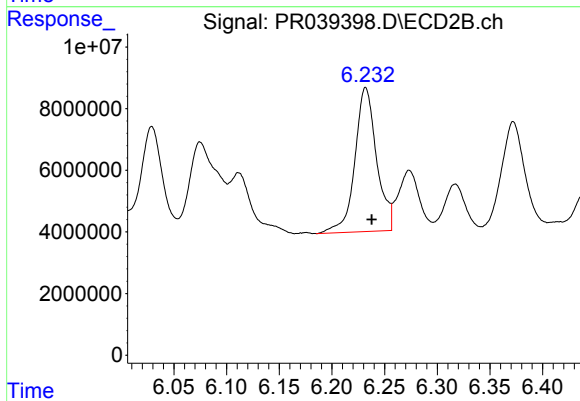

#23 AR-1248-3


R.T.: 6.232 min
Delta R.T.: -0.006 min
Response: 67234404
Conc: 243.28 ng/ml

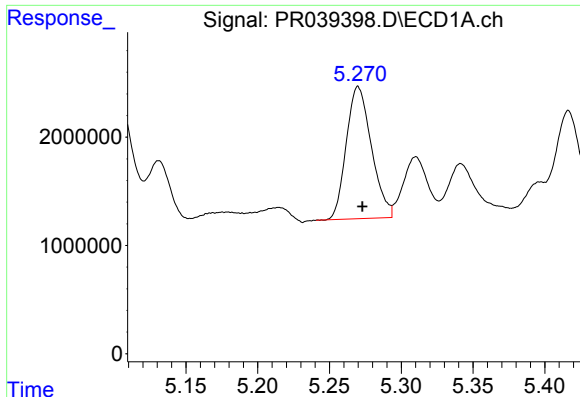

#24 AR-1248-4


R.T.: 5.270 min
Delta R.T.: -0.003 min
Response: 14899875
Conc: 181.76 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

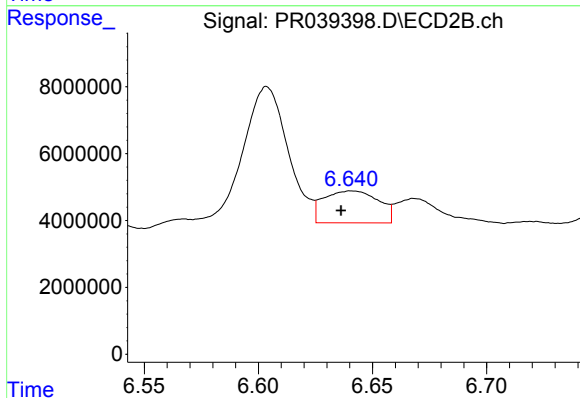


#24 AR-1248-4

R.T.: 6.641 min
Delta R.T.: 0.005 min
Response: 15983957
Conc: 47.63 ng/ml

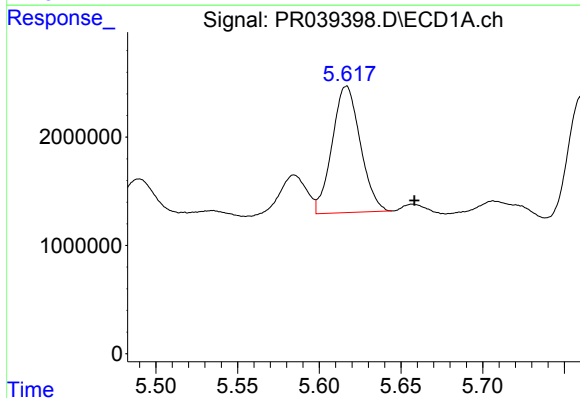


#25 AR-1248-5

R.T.: 5.617 min
Delta R.T.: -0.042 min
Response: 14024017
Conc: 160.51 ng/ml

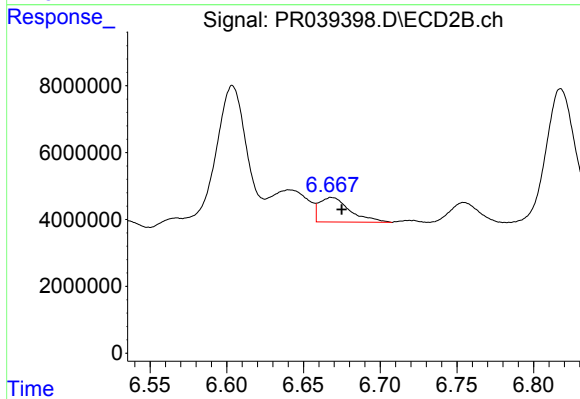

#25 AR-1248-5


R.T.: 6.669 min
Delta R.T.: -0.006 min
Response: 10291570
Conc: 32.06 ng/ml

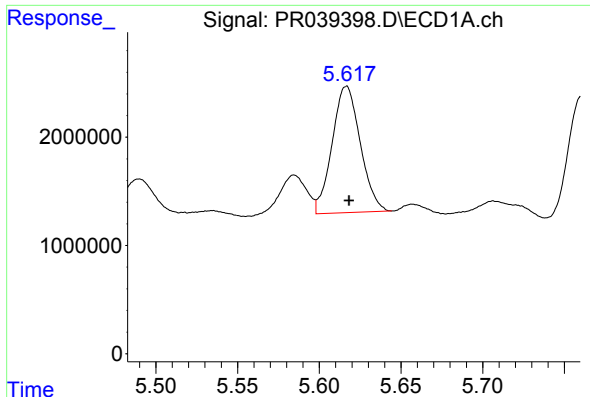

#26 AR-1254-1


R.T.: 5.617 min
Delta R.T.: -0.002 min
Response: 14024017
Conc: 106.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

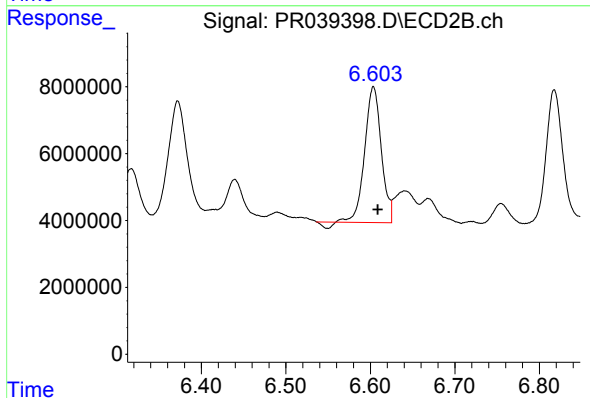


#26 AR-1254-1

R.T.: 6.604 min
Delta R.T.: -0.005 min
Response: 54898941
Conc: 171.45 ng/ml

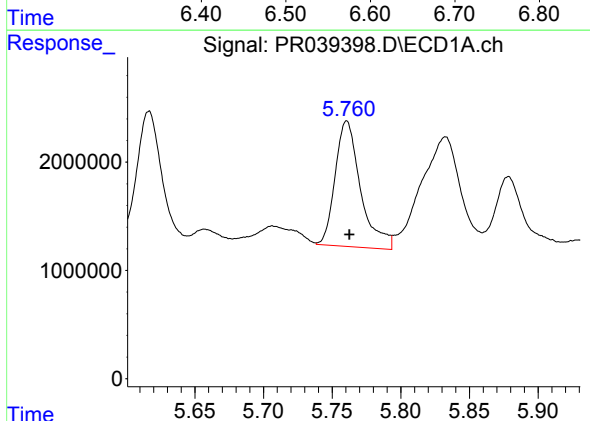


#27 AR-1254-2

R.T.: 5.761 min
Delta R.T.: -0.002 min
Response: 14982919
Conc: 127.91 ng/ml

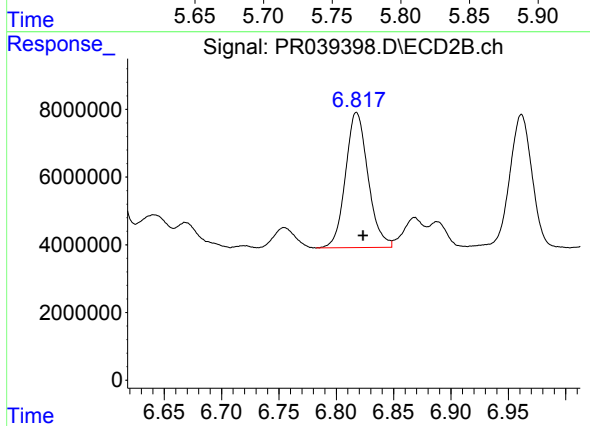

#27 AR-1254-2


R.T.: 6.818 min
Delta R.T.: -0.006 min
Response: 54655235
Conc: 106.81 ng/ml

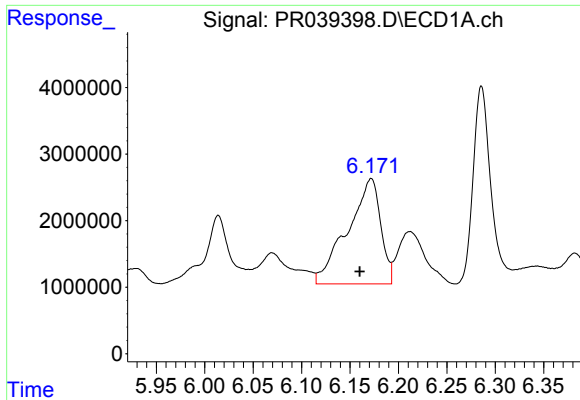

#28 AR-1254-3


R.T.: 6.172 min
Delta R.T.: 0.012 min
Response: 37471755
Conc: 181.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

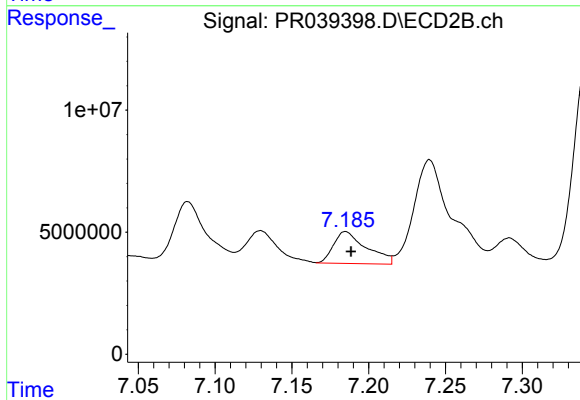


#28 AR-1254-3

R.T.: 7.185 min
Delta R.T.: -0.004 min
Response: 19465511
Conc: 32.44 ng/ml

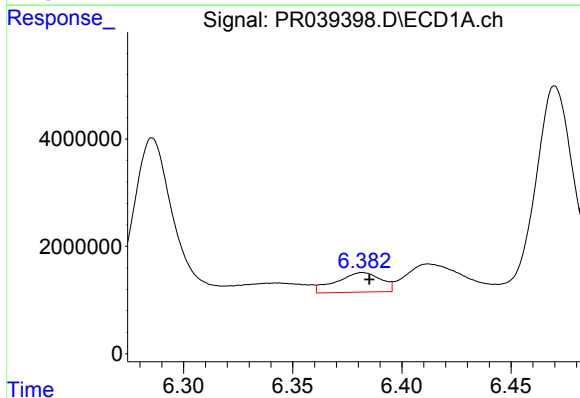


#29 AR-1254-4

R.T.: 6.382 min
Delta R.T.: -0.003 min
Response: 5198850
Conc: 33.96 ng/ml

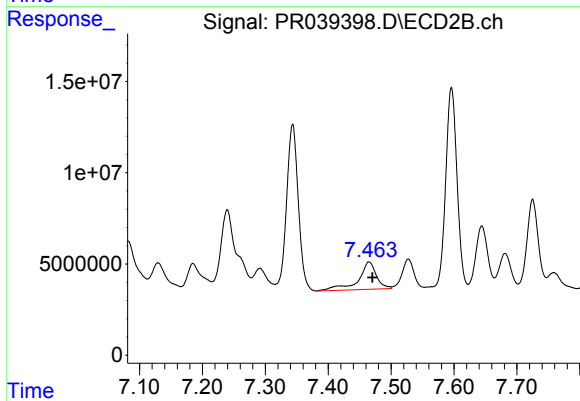

#29 AR-1254-4


R.T.: 7.465 min
Delta R.T.: -0.005 min
Response: 30194332
Conc: 69.77 ng/ml

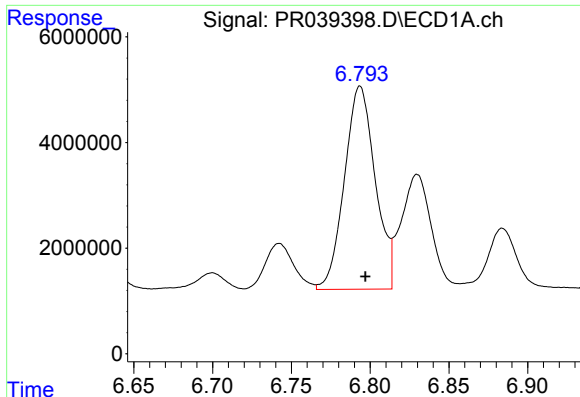

#30 AR-1254-5


R.T.: 6.794 min
Delta R.T.: -0.003 min
Response: 52407923
Conc: 281.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

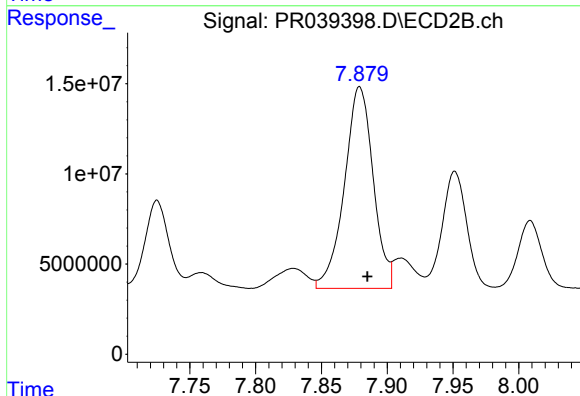


#30 AR-1254-5

R.T.: 7.879 min
Delta R.T.: -0.006 min
Response: 170469924
Conc: 362.72 ng/ml

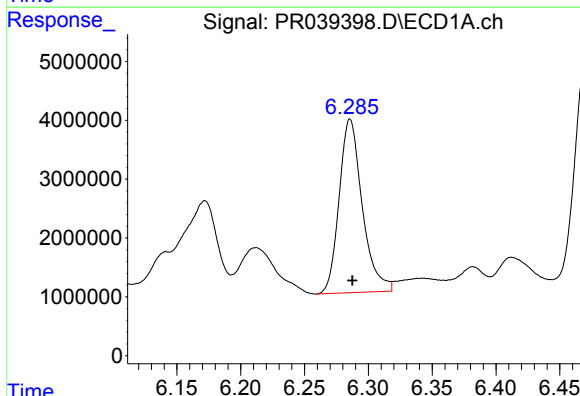


#31 AR-1260-1

R.T.: 6.286 min
Delta R.T.: -0.002 min
Response: 37172864
Conc: 324.36 ng/ml

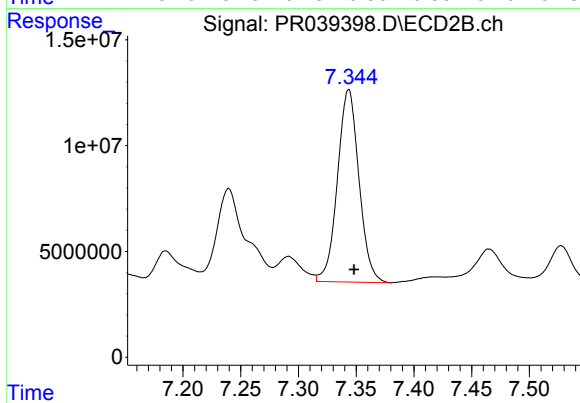

#31 AR-1260-1


R.T.: 7.344 min
Delta R.T.: -0.005 min
Response: 117886855
Conc: 324.64 ng/ml

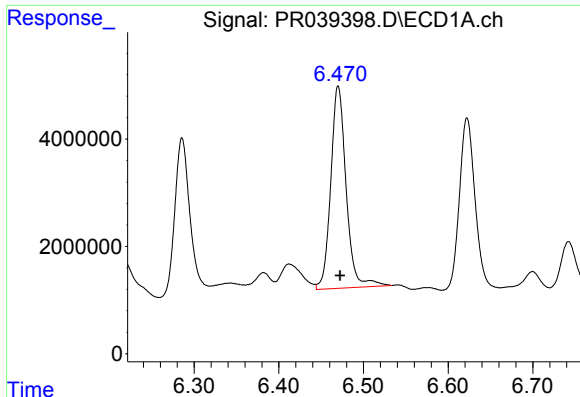

#32 AR-1260-2


R.T.: 6.470 min
Delta R.T.: -0.002 min
Response: 47600361
Conc: 315.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

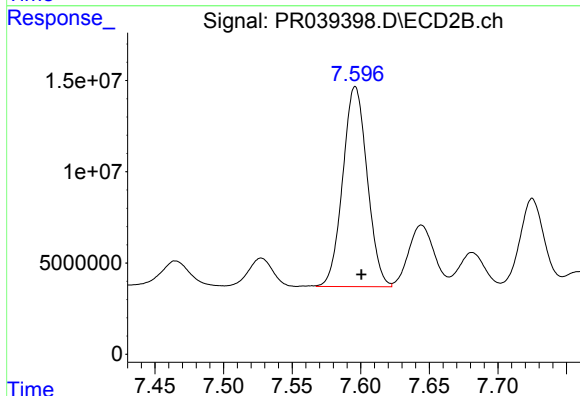


#32 AR-1260-2

R.T.: 7.596 min
Delta R.T.: -0.004 min
Response: 135899341
Conc: 310.70 ng/ml

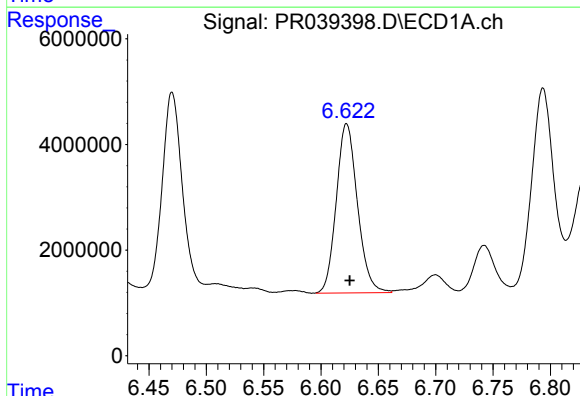


#33 AR-1260-3

R.T.: 6.622 min
Delta R.T.: -0.003 min
Response: 41221155
Conc: 306.29 ng/ml

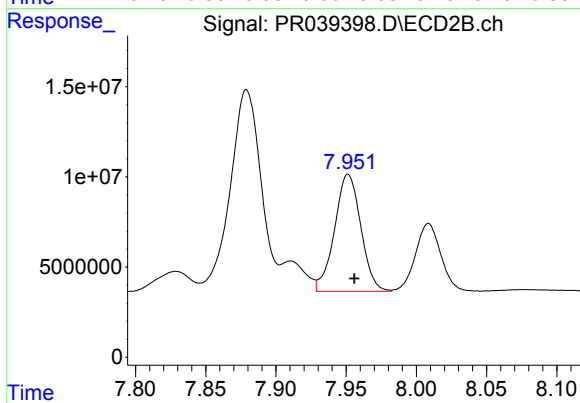

#33 AR-1260-3


R.T.: 7.951 min
Delta R.T.: -0.005 min
Response: 84390747
Conc: 248.66 ng/ml

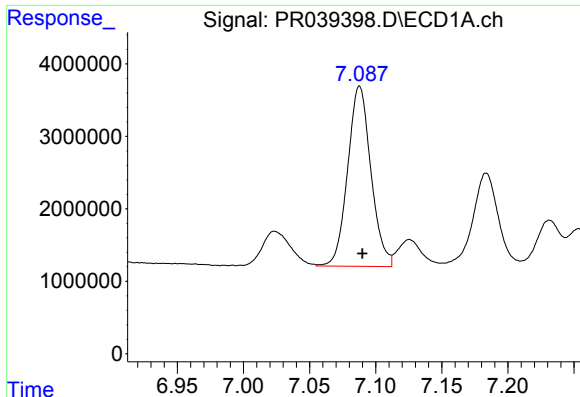

#34 AR-1260-4


R.T.: 7.088 min
Delta R.T.: -0.002 min
Response: 30433769
Conc: 254.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

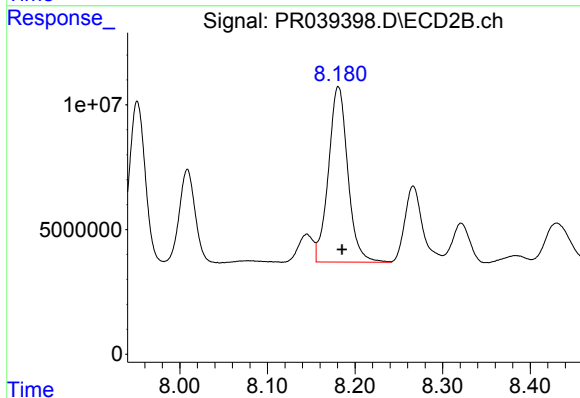


#34 AR-1260-4

R.T.: 8.181 min
Delta R.T.: -0.004 min
Response: 107816970
Conc: 265.31 ng/ml

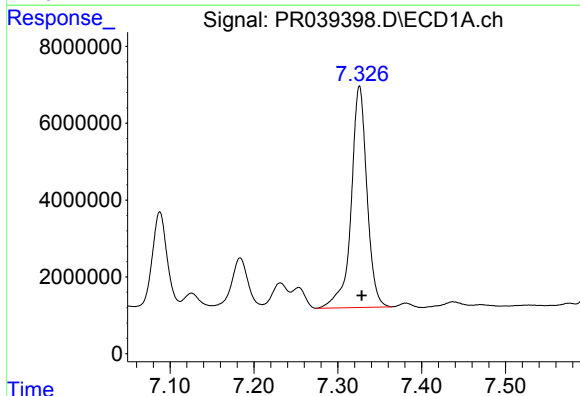


#35 AR-1260-5

R.T.: 7.326 min
Delta R.T.: -0.003 min
Response: 75351491
Conc: 250.73 ng/ml

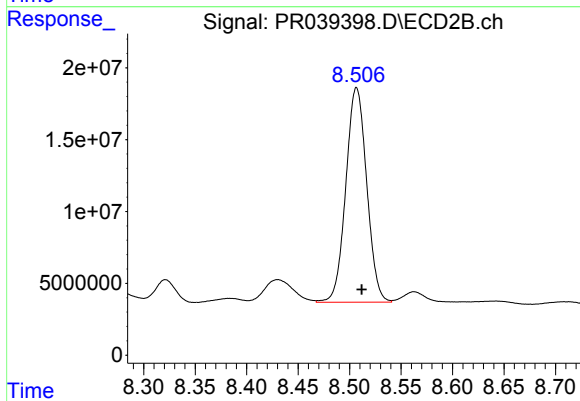

#35 AR-1260-5


R.T.: 8.507 min
Delta R.T.: -0.005 min
Response: 210868185
Conc: 246.59 ng/ml

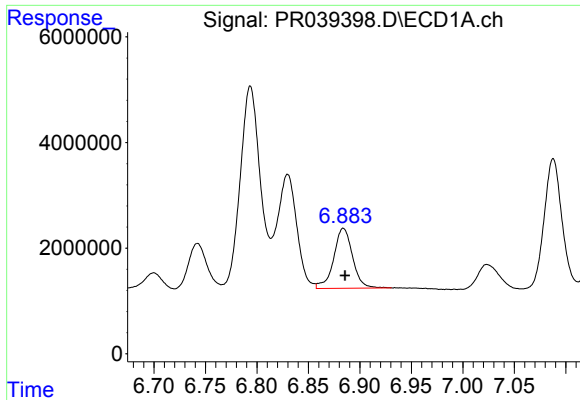

#36 AR-1262-1


R.T.: 6.884 min
Delta R.T.: -0.002 min
Response: 14520149
Conc: 153.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

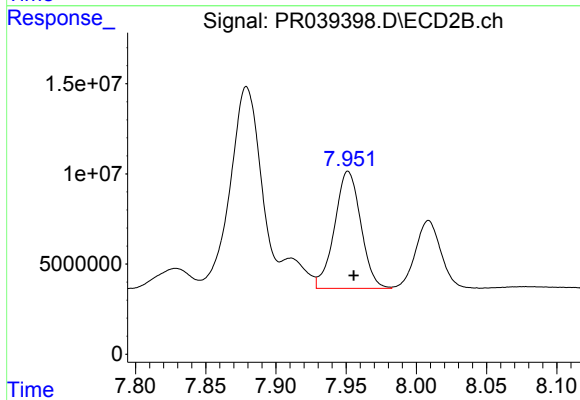


#36 AR-1262-1

R.T.: 7.951 min
Delta R.T.: -0.004 min
Response: 84390747
Conc: 121.52 ng/ml

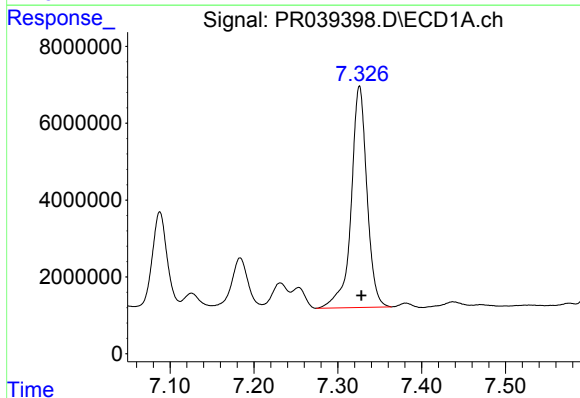


#37 AR-1262-2

R.T.: 7.326 min
Delta R.T.: -0.002 min
Response: 75351491
Conc: 154.88 ng/ml

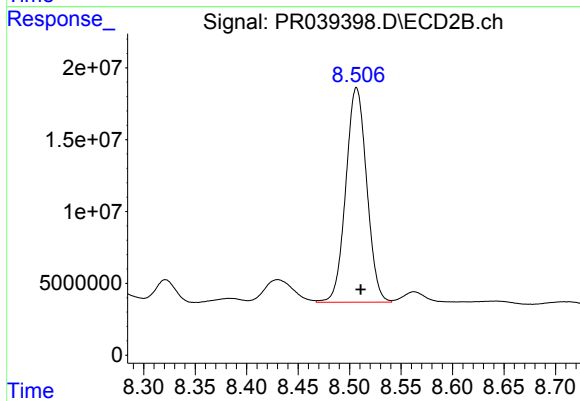

#37 AR-1262-2


R.T.: 8.507 min
Delta R.T.: -0.004 min
Response: 210868185
Conc: 153.84 ng/ml

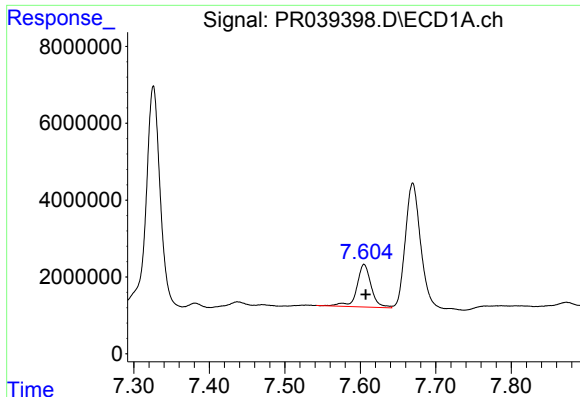

#38 AR-1262-3


R.T.: 7.605 min
Delta R.T.: -0.002 min
Response: 14640909
Conc: 80.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

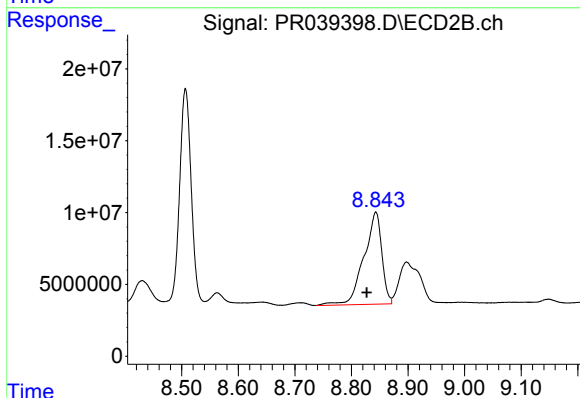


#38 AR-1262-3

R.T.: 8.843 min
Delta R.T.: 0.016 min
Response: 141427125
Conc: 157.00 ng/ml

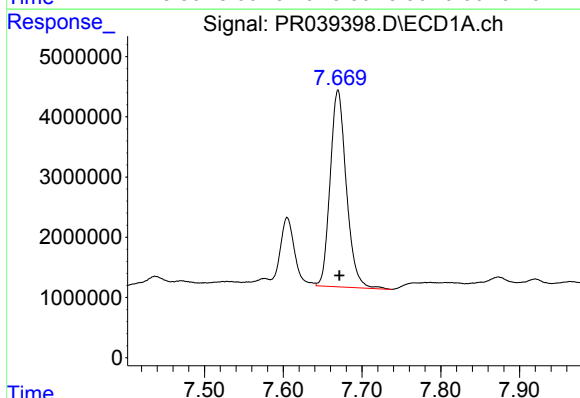


#39 AR-1262-4

R.T.: 7.670 min
Delta R.T.: -0.002 min
Response: 46567915
Conc: 130.89 ng/ml

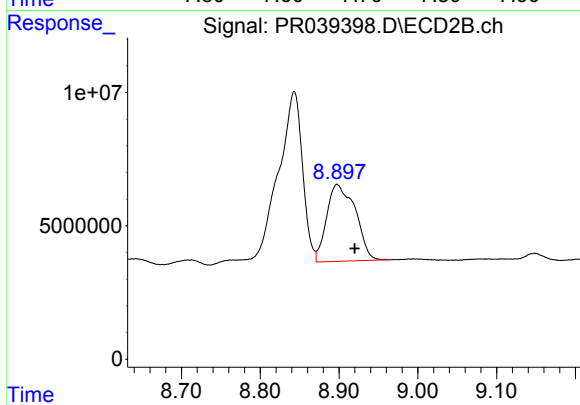

#39 AR-1262-4


R.T.: 8.898 min
Delta R.T.: -0.022 min
Response: 72844253
Conc: 108.50 ng/ml

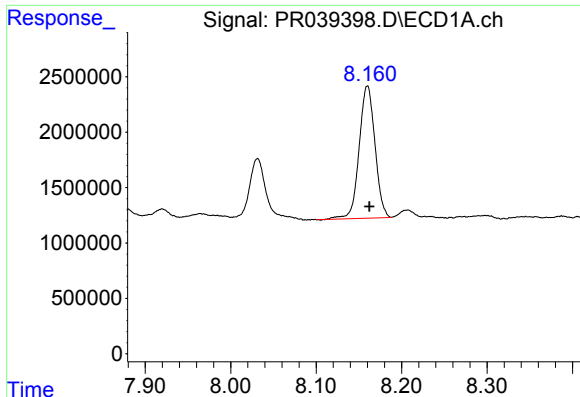

#40 AR-1262-5


R.T.: 8.160 min
Delta R.T.: -0.002 min
Response: 15358679
Conc: 94.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

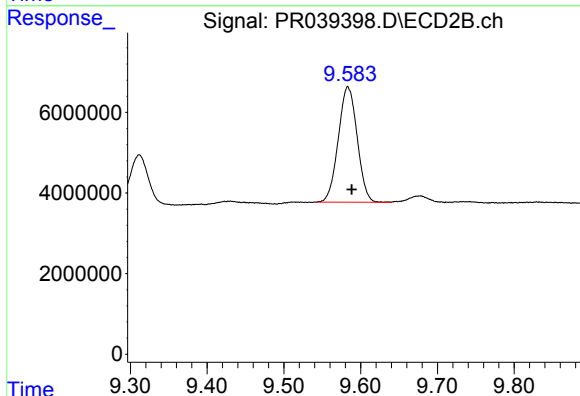


#40 AR-1262-5

R.T.: 9.583 min
Delta R.T.: -0.005 min
Response: 48916869
Conc: 99.93 ng/ml

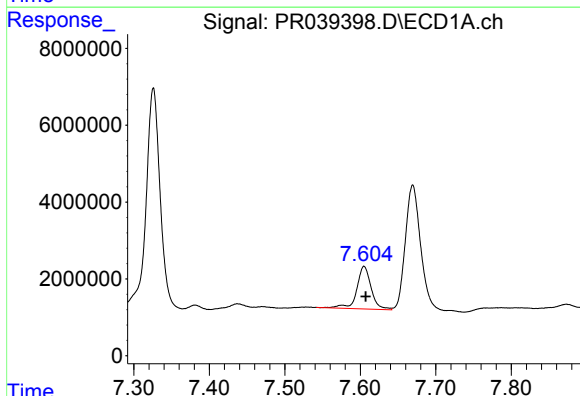


#41 AR-1268-1

R.T.: 7.605 min
Delta R.T.: -0.002 min
Response: 14640909
Conc: 27.12 ng/ml

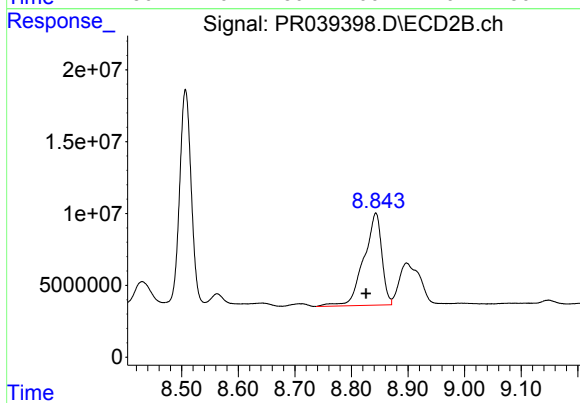

#41 AR-1268-1


R.T.: 8.843 min
Delta R.T.: 0.017 min
Response: 141427125
Conc: 89.75 ng/ml

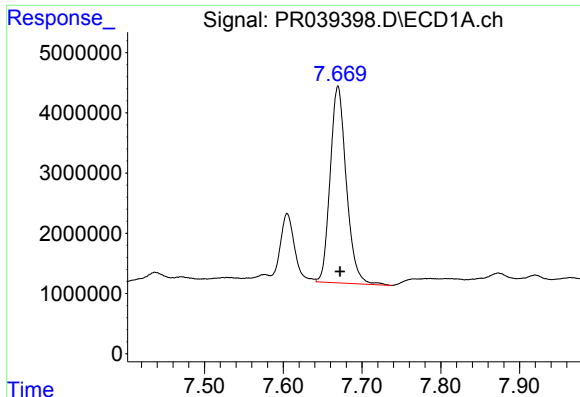

#42 AR-1268-2


R.T.: 7.670 min
Delta R.T.: -0.003 min
Response: 46567915
Conc: 94.02 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

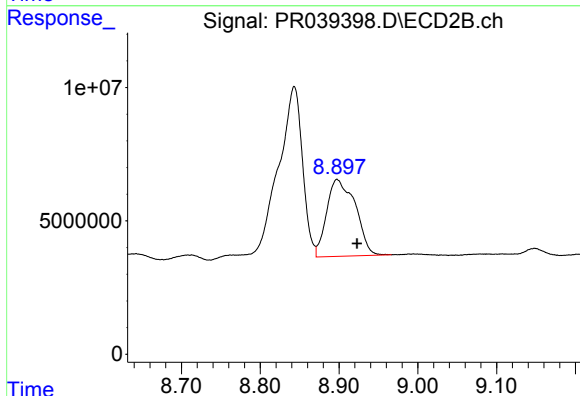


#42 AR-1268-2

R.T.: 8.898 min
Delta R.T.: -0.025 min
Response: 72844253
Conc: 49.66 ng/ml

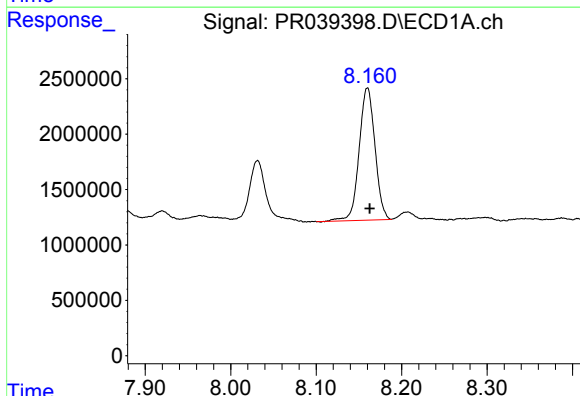


#44 AR-1268-4

R.T.: 8.160 min
Delta R.T.: -0.003 min
Response: 15358679
Conc: 85.97 ng/ml

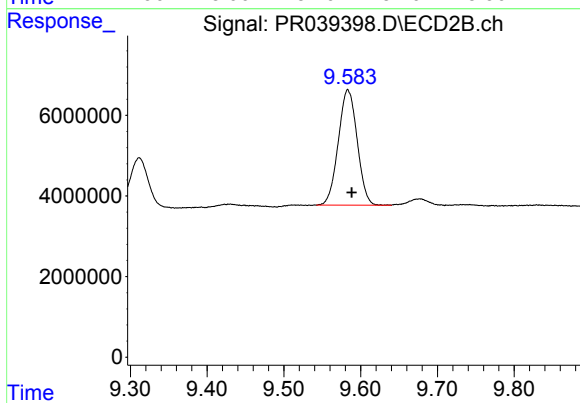

#44 AR-1268-4


R.T.: 9.583 min
Delta R.T.: -0.005 min
Response: 48916869
Conc: 92.33 ng/ml

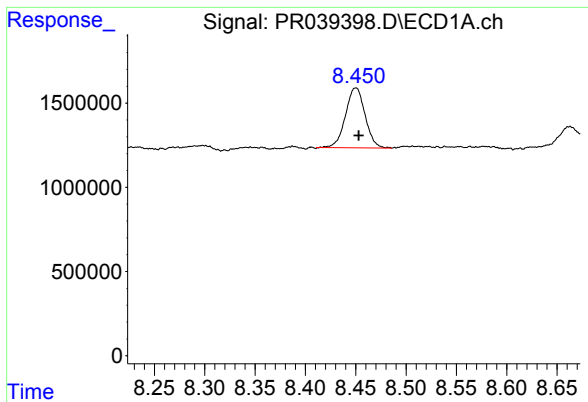

#45 AR-1268-5

R.T.: 8.450 min
Delta R.T.: -0.003 min
Response: 4819694
Conc: 3.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMS

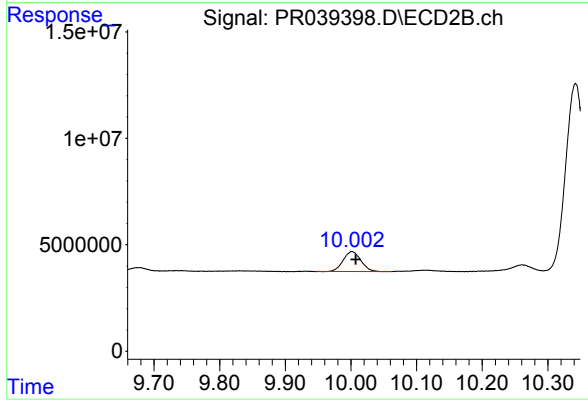

#45 AR-1268-5

R.T.: 10.002 min
Delta R.T.: -0.006 min
Response: 17641770
Conc: 4.11 ng/ml