

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071819\
 Data File : PR039399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 17:49
 Operator : SM\AJ
 Sample : K3751-01MSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MANHOLE-TEST-PITMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 01:32:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.759	4.605	50729690	209.9E6	32.752	32.461
2)	SA Decachlor...	8.696	10.340	49941857	194.0E6	20.424	22.673
Target Compounds							
3)	L1 AR-1016-1	4.827	5.760	20676839	91843533	343.839	367.164
4)	L1 AR-1016-2	4.843	5.782	31879169	131.0E6	324.527	358.981
5)	L1 AR-1016-3	5.017	5.844	16439364	75057134	330.923	340.977
6)	L1 AR-1016-4	5.058	5.942	13281700	64761915	332.172	346.192
7)	L1 AR-1016-5	5.266	6.232	14222222	64660437	261.455	352.290 #
9)	L2 AR-1221-2	4.054	4.897	2452826	9529068	193.233	206.233
10)	L2 AR-1221-3	4.128	4.973	10128087	39133768	255.672	259.583
11)	L3 AR-1232-1	4.128	4.973	10128087	39133768	341.035	355.964
12)	L3 AR-1232-2	4.843	5.496	31879169	79794999	863.606	1331.291 #
13)	L3 AR-1232-3	5.017	5.782	16439364	131.0E6	900.400	1009.901
14)	L3 AR-1232-4	5.099	5.942	14471453	64761915	908.264	967.016
15)	L3 AR-1232-5	5.266	6.028	14222222	49165286	789.013	1078.788 #
16)	L4 AR-1242-1	4.827	5.760	20676839	91843533	391.340	427.431
17)	L4 AR-1242-2	4.843	5.782	31879169	131.0E6	365.803	419.028
18)	L4 AR-1242-3	5.017	5.844	16439364	75057134	377.684	393.780
19)	L4 AR-1242-4	5.099	5.942	14471453	64761915	336.062	403.533
20)	L4 AR-1242-5	5.613	6.668	12947485	9519482	207.202	50.486 #
21)	L5 AR-1248-1	4.827	5.760	20676839	91843533	477.739	537.203
22)	L5 AR-1248-2	5.058	6.028	13281700	49165286	211.734	209.337
23)	L5 AR-1248-3	5.099	6.232	14471453	64660437	221.669	233.962
24)	L5 AR-1248-4	5.266	6.641	14222222	15488080	173.492	46.153 #
25)	L5 AR-1248-5	5.613	6.668	12947485	9519482	148.187	29.654 #
26)	L6 AR-1254-1	5.613	6.603	12947485	53467669	97.897	166.982 #
27)	L6 AR-1254-2	5.757	6.816	13021913	53496199	111.166	104.541
28)	L6 AR-1254-3	6.168	7.183	30384251	18544831	147.045	30.903 #
29)	L6 AR-1254-4	6.378	7.464	2234292	31557992	14.594	72.921 #
30)	L6 AR-1254-5	6.790	7.878	49850933	168.2E6	267.586	357.855 #
31)	L7 AR-1260-1	6.282	7.342	32366871	117.0E6	282.427	322.258
32)	L7 AR-1260-2	6.467	7.595	43122448	135.0E6	285.936	308.542
33)	L7 AR-1260-3	6.618	7.950	38423644	84268382	285.500	248.301
34)	L7 AR-1260-4	7.083	8.179	29441780	114.1E6	245.982	280.876
35)	L7 AR-1260-5	7.321	8.505	72628802	239.0E6	241.667	279.519
36)	L8 AR-1262-1	6.880	7.950	13836004	84268382	145.957	121.346
37)	L8 AR-1262-2	7.321	8.505	72628802	239.0E6	149.287	174.381
38)	L8 AR-1262-3	7.601	8.840	13990251	143.2E6	77.033	158.978 #
39)	L8 AR-1262-4	7.665	8.895	45298369	73880938	127.320	110.040
40)	L8 AR-1262-5	8.154	9.581	15383590	51423829	94.332	105.049
41)	L9 AR-1268-1	7.601	8.840	13990251	143.2E6	25.912	90.883 #
42)	L9 AR-1268-2	7.665	8.895	45298369	73880938	91.452	50.365 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071819\
 Data File : PR039399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 17:49
 Operator : SM\AJ
 Sample : K3751-01MSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MANHOLE-TEST-PITMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 01:32:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.154	9.581	15383590	51423829	86.111	97.060
45) L9	AR-1268-5	8.444	9.999	4913694	17891654	3.619	4.171



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071819\
Data File : PR039399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 17:49
Operator : SM\AJ
Sample : K3751-01MSD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 01:32:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 02:56:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

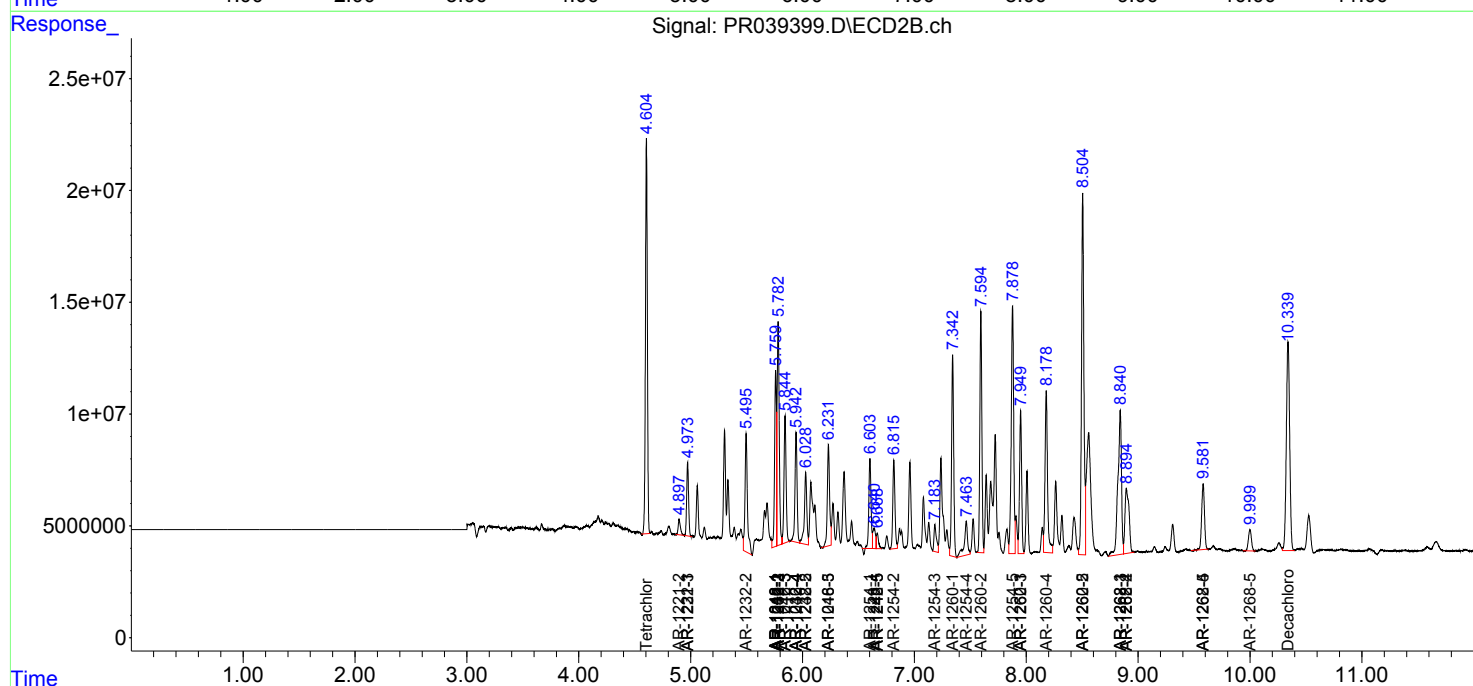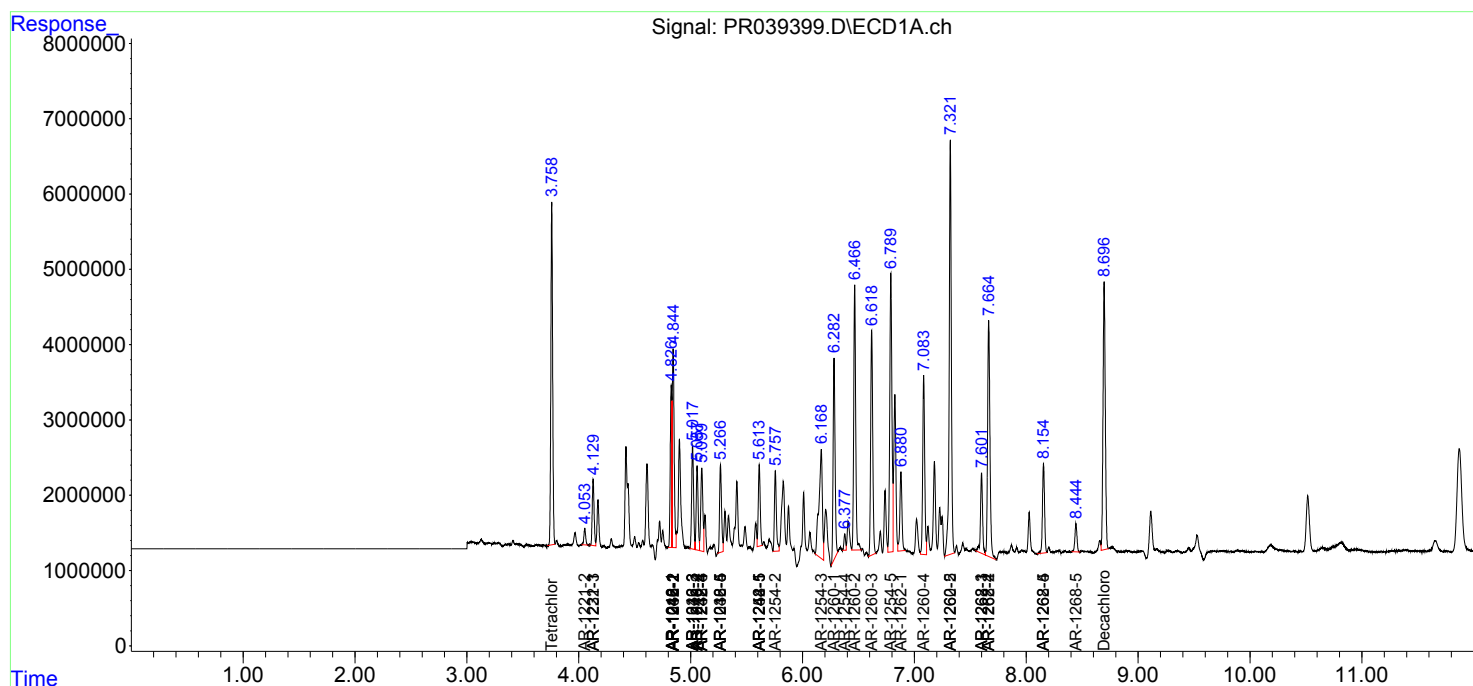


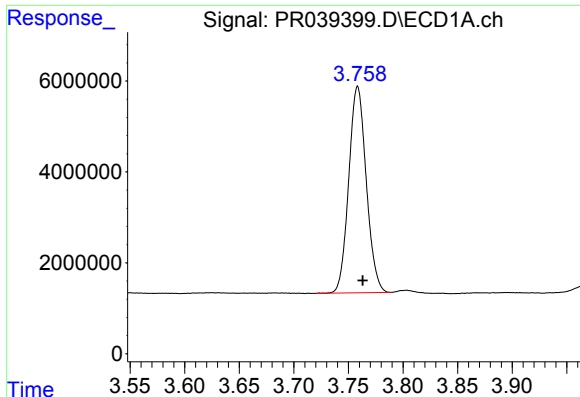

#1 Tetrachloro-m-xylene


R.T.: 3.759 min
Delta R.T.: -0.004 min
Response: 50729690
Conc: 32.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

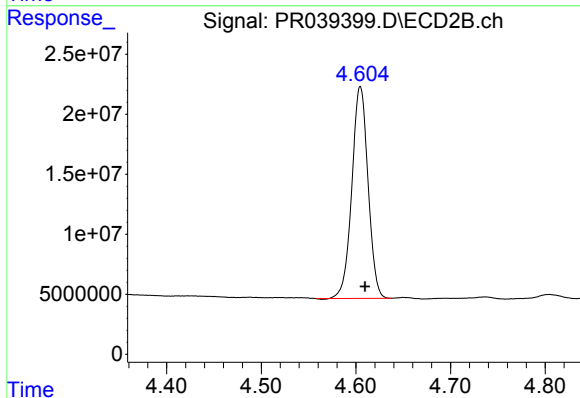


#1 Tetrachloro-m-xylene

R.T.: 4.605 min
Delta R.T.: -0.005 min
Response: 209935322
Conc: 32.46 ng/ml

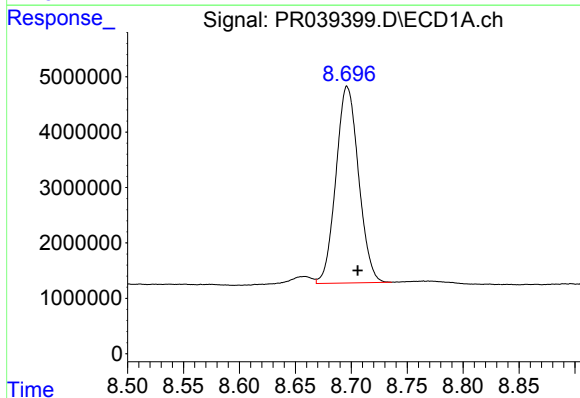


#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: -0.010 min
Response: 49941857
Conc: 20.42 ng/ml

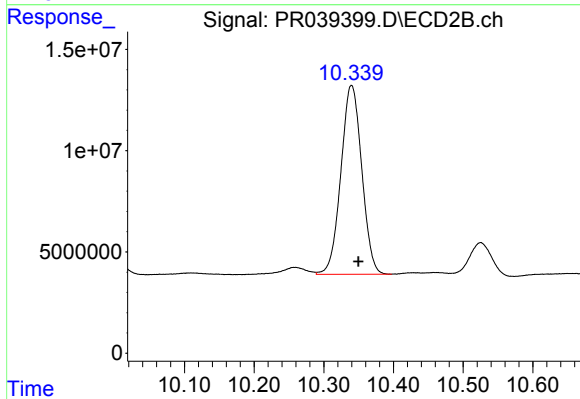

#2 Decachlorobiphenyl


R.T.: 10.340 min
Delta R.T.: -0.010 min
Response: 194033486
Conc: 22.67 ng/ml

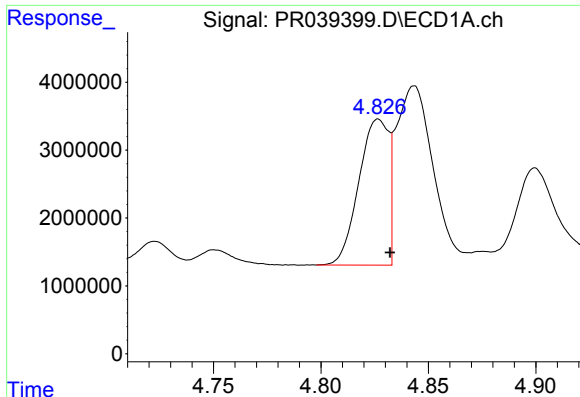

#3 AR-1016-1


R.T.: 4.827 min
Delta R.T.: -0.006 min
Response: 20676839
Conc: 343.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

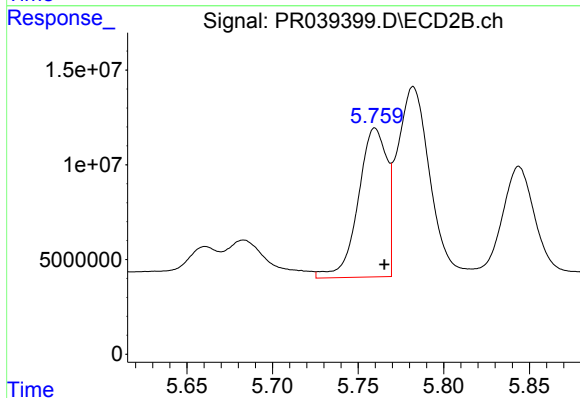


#3 AR-1016-1

R.T.: 5.760 min
Delta R.T.: -0.005 min
Response: 91843533
Conc: 367.16 ng/ml

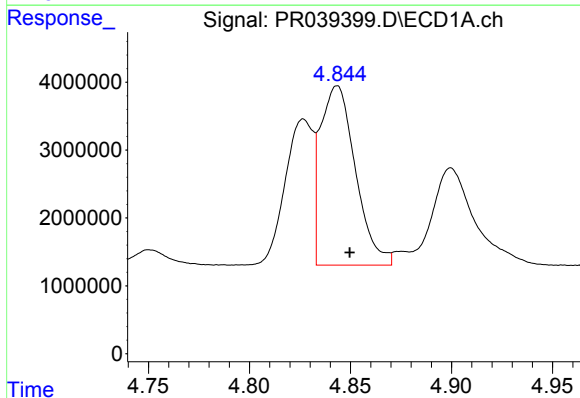


#4 AR-1016-2

R.T.: 4.843 min
Delta R.T.: -0.006 min
Response: 31879169
Conc: 324.53 ng/ml

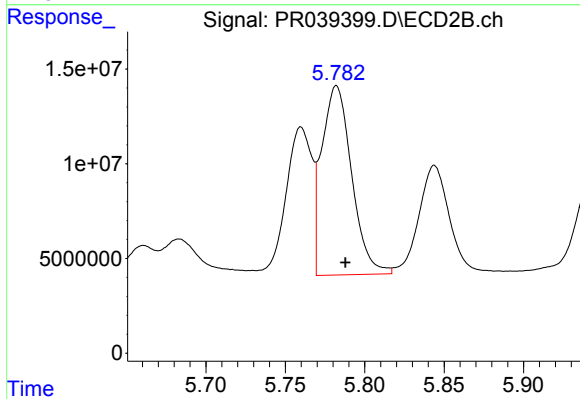

#4 AR-1016-2


R.T.: 5.782 min
Delta R.T.: -0.006 min
Response: 130976267
Conc: 358.98 ng/ml

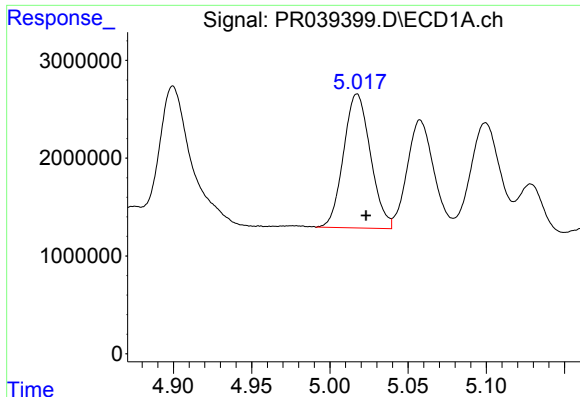

#5 AR-1016-3


R.T.: 5.017 min
Delta R.T.: -0.006 min
Response: 16439364
Conc: 330.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

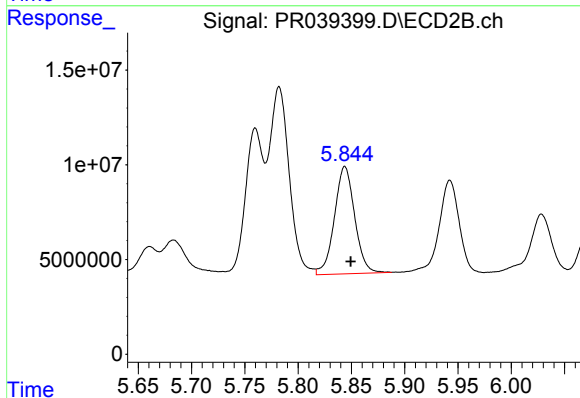


#5 AR-1016-3

R.T.: 5.844 min
Delta R.T.: -0.005 min
Response: 75057134
Conc: 340.98 ng/ml

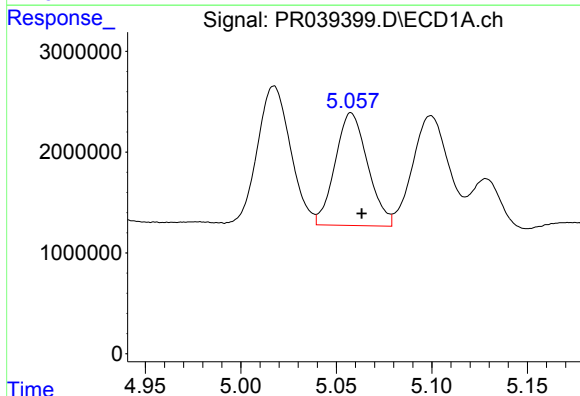


#6 AR-1016-4

R.T.: 5.058 min
Delta R.T.: -0.006 min
Response: 13281700
Conc: 332.17 ng/ml

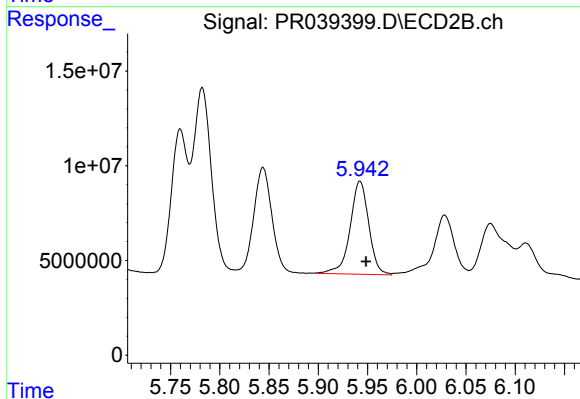

#6 AR-1016-4


R.T.: 5.942 min
Delta R.T.: -0.006 min
Response: 64761915
Conc: 346.19 ng/ml

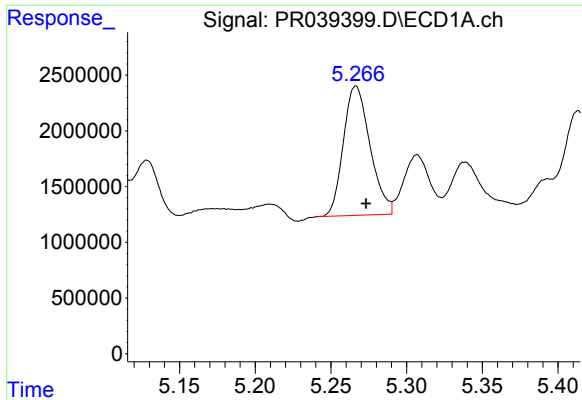

#7 AR-1016-5


R.T.: 5.266 min
Delta R.T.: -0.007 min
Response: 14222222
Conc: 261.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

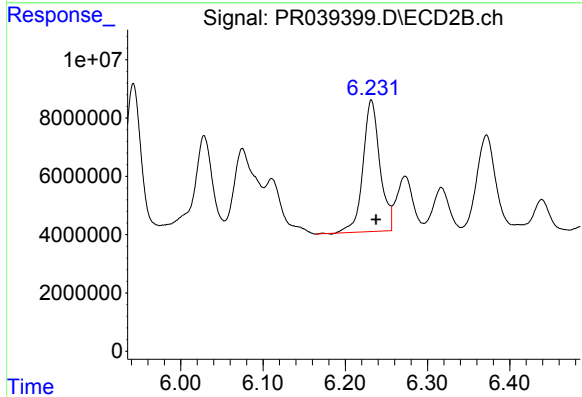


#7 AR-1016-5

R.T.: 6.232 min
Delta R.T.: -0.006 min
Response: 64660437
Conc: 352.29 ng/ml

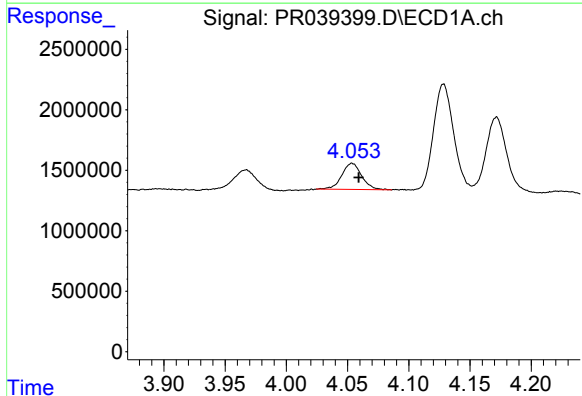


#9 AR-1221-2

R.T.: 4.054 min
Delta R.T.: -0.006 min
Response: 2452826
Conc: 193.23 ng/ml

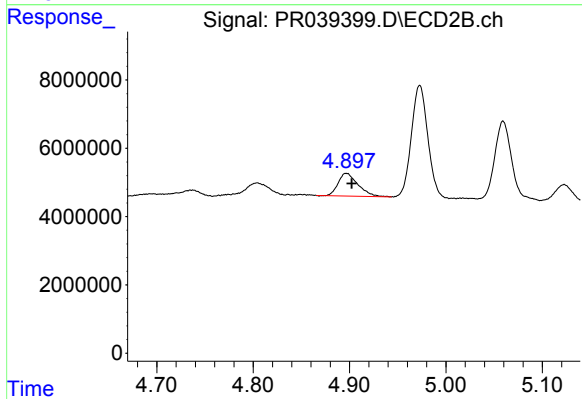

#9 AR-1221-2


R.T.: 4.897 min
Delta R.T.: -0.006 min
Response: 9529068
Conc: 206.23 ng/ml

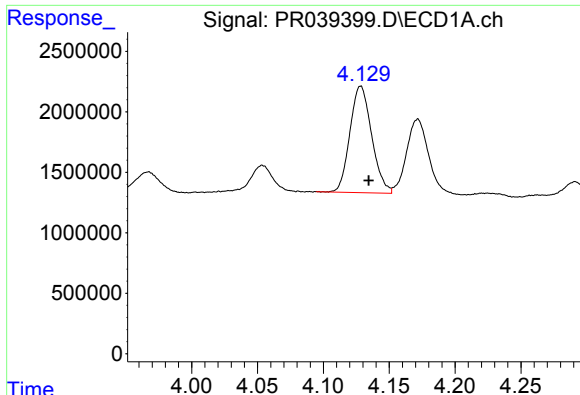

#10 AR-1221-3


R.T.: 4.128 min
Delta R.T.: -0.006 min
Response: 10128087
Conc: 255.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

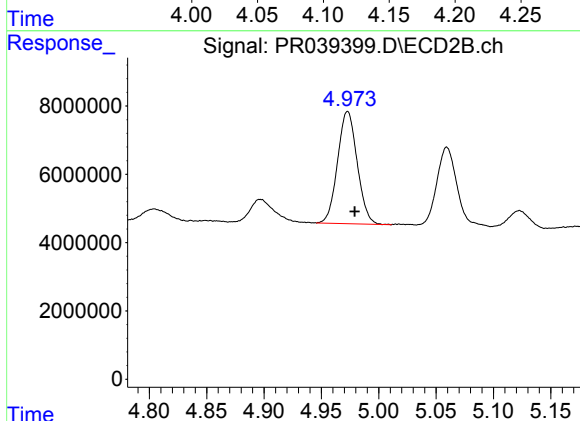


#10 AR-1221-3

R.T.: 4.973 min
Delta R.T.: -0.006 min
Response: 39133768
Conc: 259.58 ng/ml

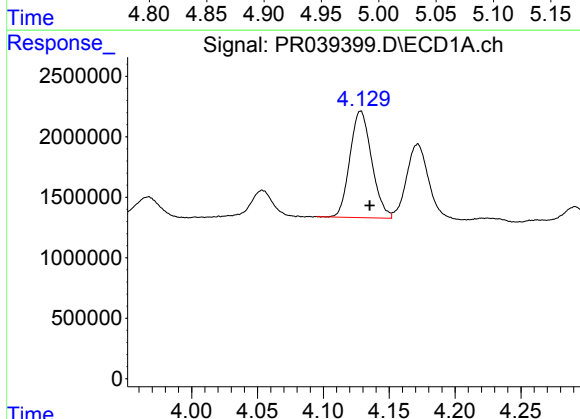


#11 AR-1232-1

R.T.: 4.128 min
Delta R.T.: -0.007 min
Response: 10128087
Conc: 341.03 ng/ml

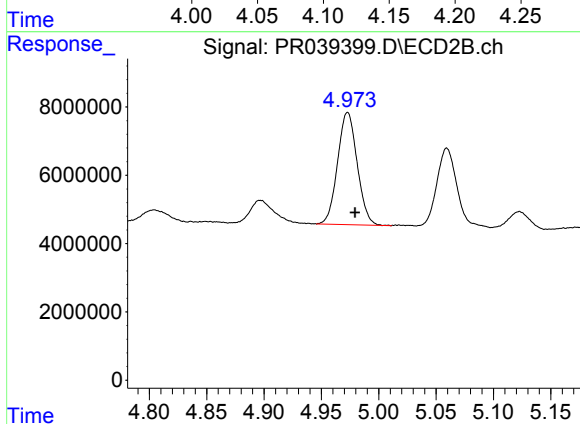

#11 AR-1232-1


R.T.: 4.973 min
Delta R.T.: -0.007 min
Response: 39133768
Conc: 355.96 ng/ml

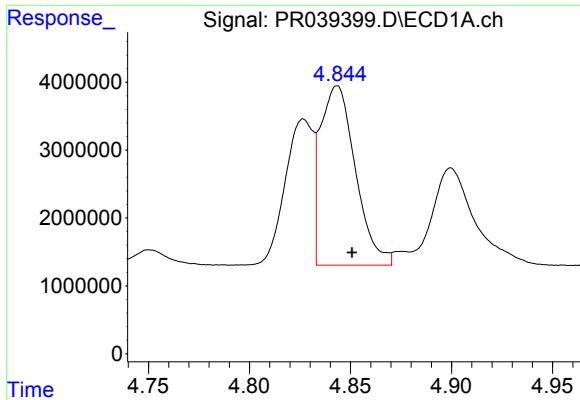

#12 AR-1232-2


R.T.: 4.843 min
Delta R.T.: -0.007 min
Response: 31879169
Conc: 863.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

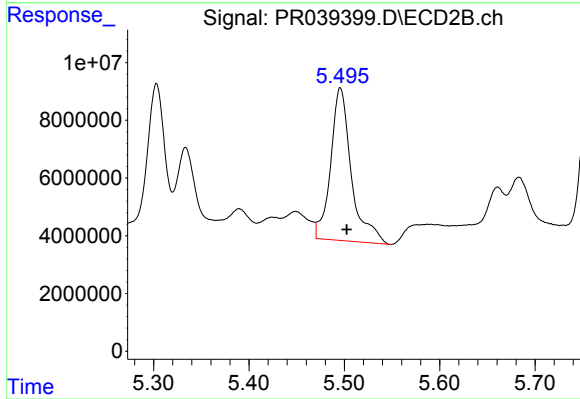


#12 AR-1232-2

R.T.: 5.496 min
Delta R.T.: -0.007 min
Response: 79794999
Conc: 1331.29 ng/ml

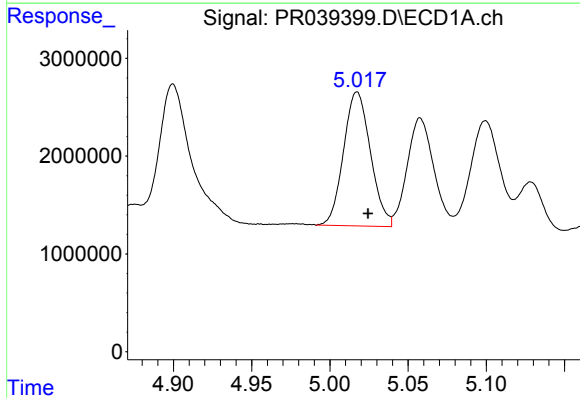


#13 AR-1232-3

R.T.: 5.017 min
Delta R.T.: -0.007 min
Response: 16439364
Conc: 900.40 ng/ml

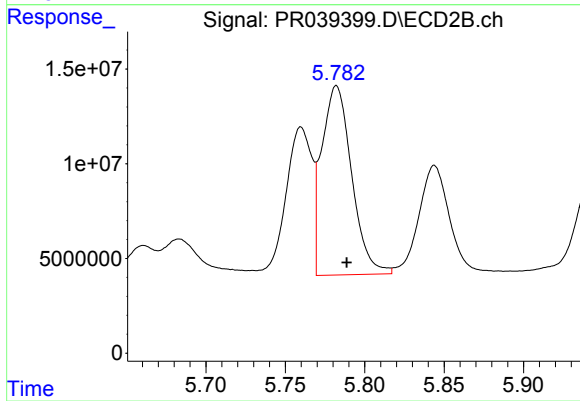

#13 AR-1232-3


R.T.: 5.782 min
Delta R.T.: -0.006 min
Response: 130976267
Conc: 1009.90 ng/ml

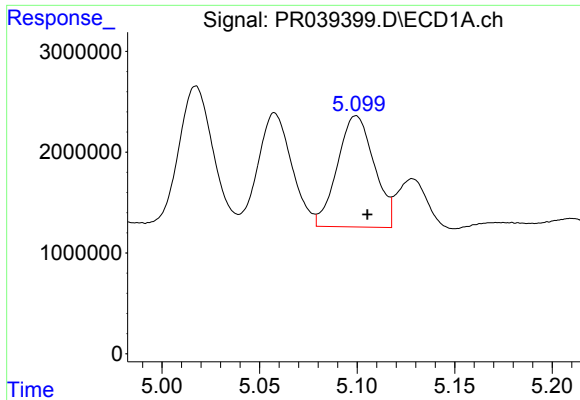

#14 AR-1232-4


R.T.: 5.099 min
Delta R.T.: -0.006 min
Response: 14471453
Conc: 908.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

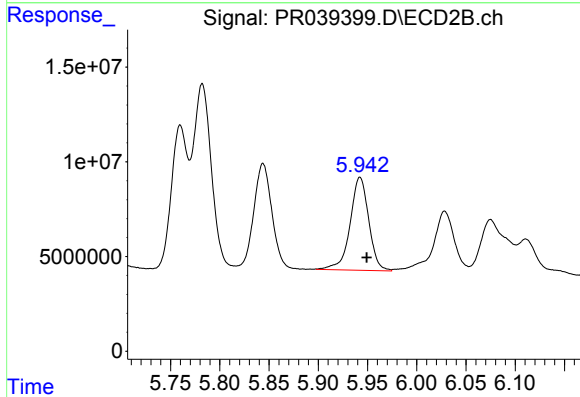


#14 AR-1232-4

R.T.: 5.942 min
Delta R.T.: -0.007 min
Response: 64761915
Conc: 967.02 ng/ml

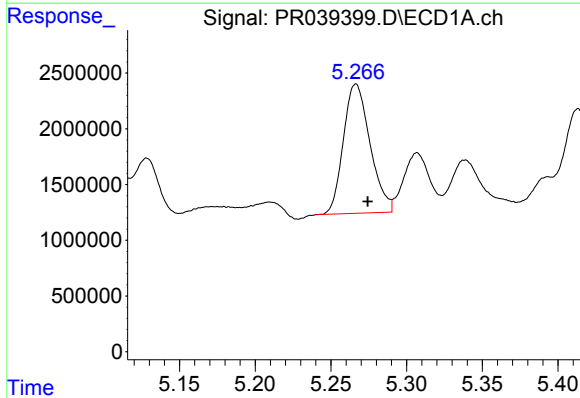


#15 AR-1232-5

R.T.: 5.266 min
Delta R.T.: -0.008 min
Response: 14222222
Conc: 789.01 ng/ml

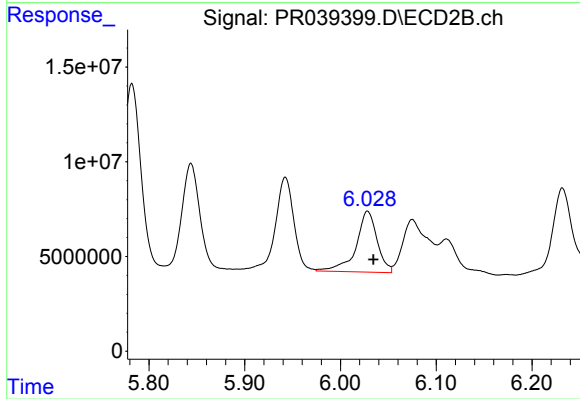

#15 AR-1232-5


R.T.: 6.028 min
Delta R.T.: -0.006 min
Response: 49165286
Conc: 1078.79 ng/ml

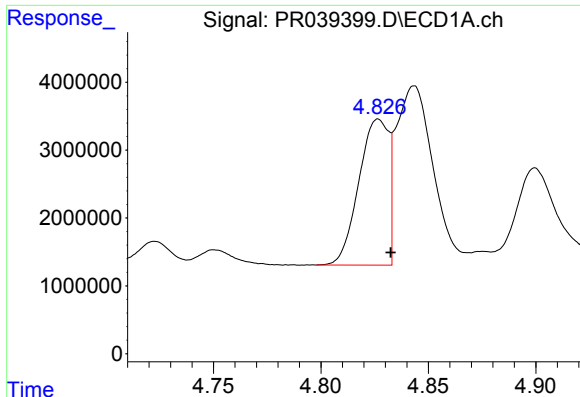

#16 AR-1242-1


R.T.: 4.827 min
Delta R.T.: -0.006 min
Response: 20676839
Conc: 391.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

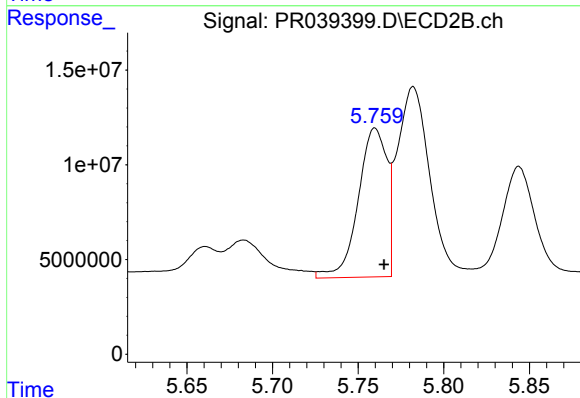


#16 AR-1242-1

R.T.: 5.760 min
Delta R.T.: -0.005 min
Response: 91843533
Conc: 427.43 ng/ml

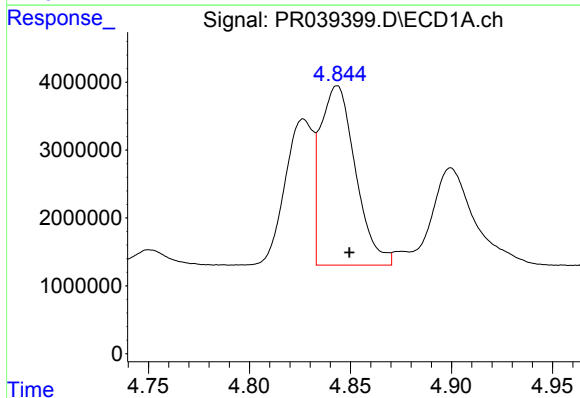


#17 AR-1242-2

R.T.: 4.843 min
Delta R.T.: -0.006 min
Response: 31879169
Conc: 365.80 ng/ml

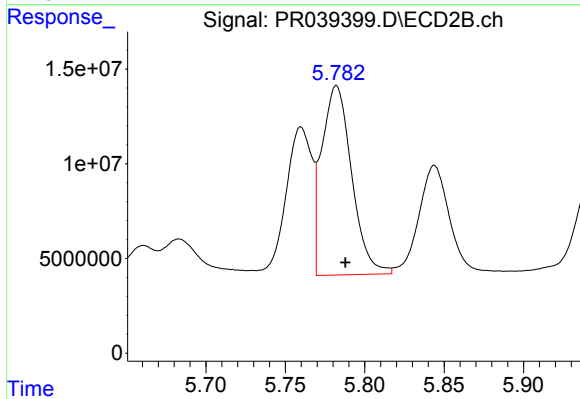

#17 AR-1242-2


R.T.: 5.782 min
Delta R.T.: -0.006 min
Response: 130976267
Conc: 419.03 ng/ml

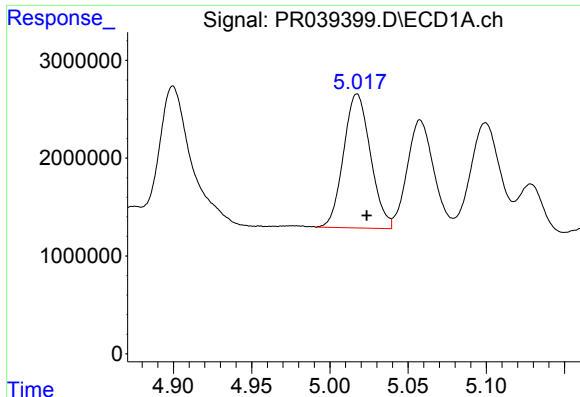

#18 AR-1242-3


R.T.: 5.017 min
Delta R.T.: -0.006 min
Response: 16439364
Conc: 377.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

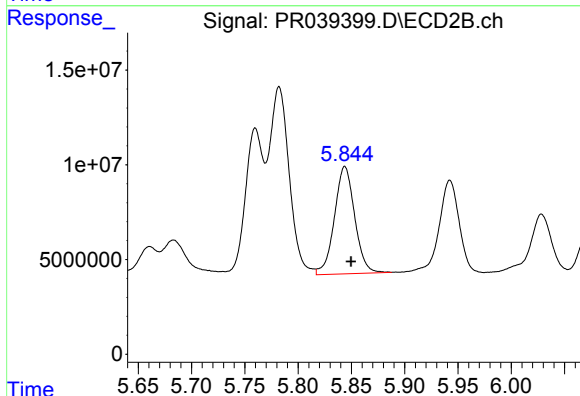


#18 AR-1242-3

R.T.: 5.844 min
Delta R.T.: -0.006 min
Response: 75057134
Conc: 393.78 ng/ml

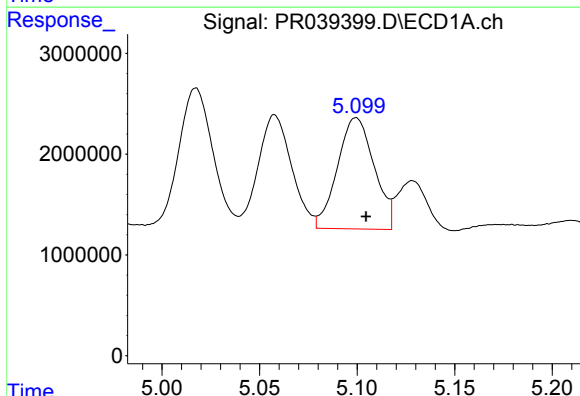


#19 AR-1242-4

R.T.: 5.099 min
Delta R.T.: -0.005 min
Response: 14471453
Conc: 336.06 ng/ml

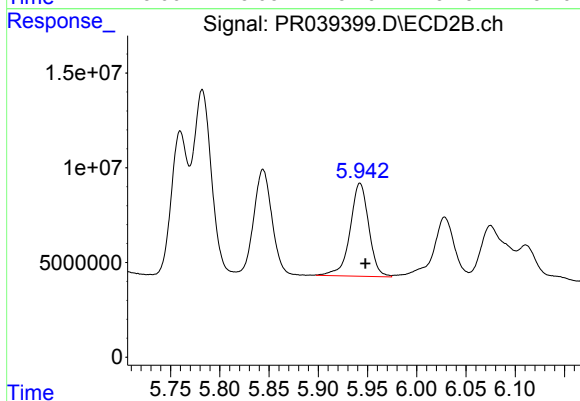

#19 AR-1242-4


R.T.: 5.942 min
Delta R.T.: -0.006 min
Response: 64761915
Conc: 403.53 ng/ml

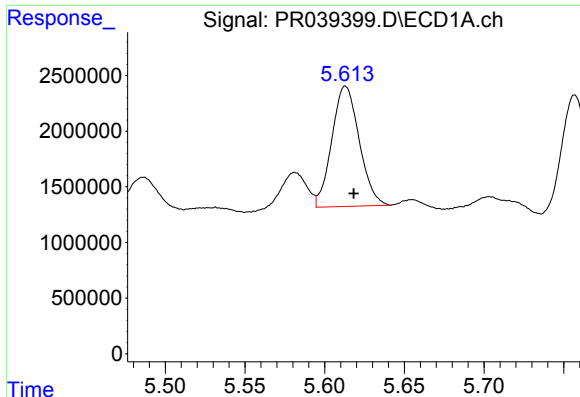

#20 AR-1242-5


R.T.: 5.613 min
Delta R.T.: -0.005 min
Response: 12947485
Conc: 207.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

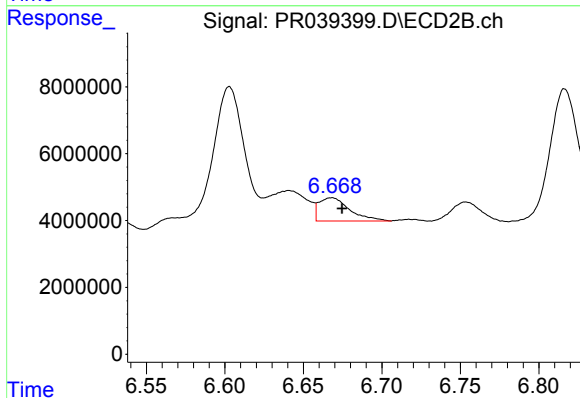


#20 AR-1242-5

R.T.: 6.668 min
Delta R.T.: -0.006 min
Response: 9519482
Conc: 50.49 ng/ml

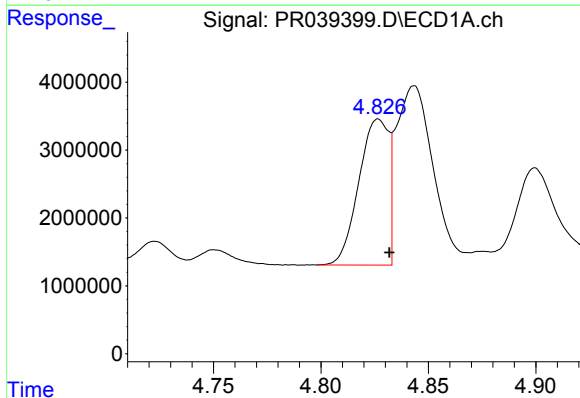


#21 AR-1248-1

R.T.: 4.827 min
Delta R.T.: -0.005 min
Response: 20676839
Conc: 477.74 ng/ml

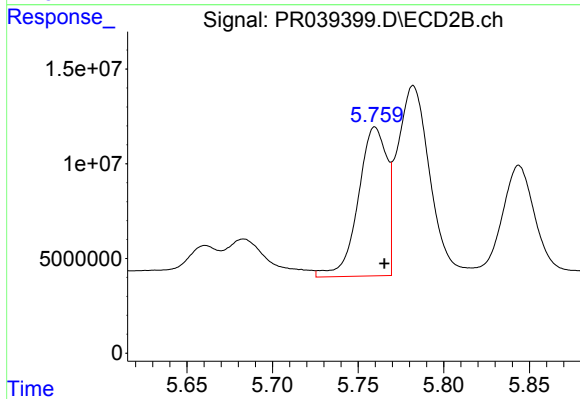

#21 AR-1248-1


R.T.: 5.760 min
Delta R.T.: -0.005 min
Response: 91843533
Conc: 537.20 ng/ml

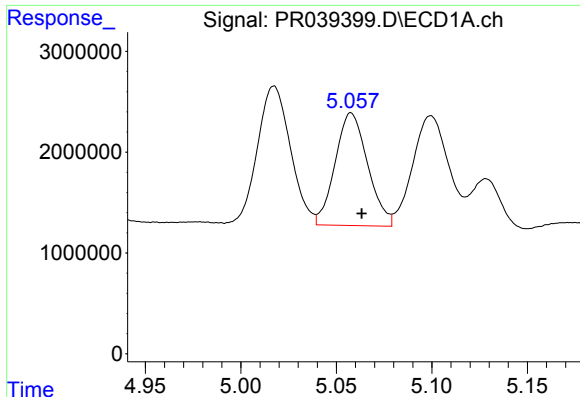

#22 AR-1248-2


R.T.: 5.058 min
Delta R.T.: -0.006 min
Response: 13281700
Conc: 211.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

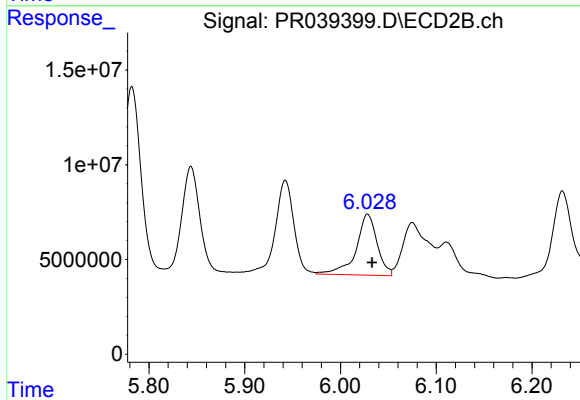


#22 AR-1248-2

R.T.: 6.028 min
Delta R.T.: -0.005 min
Response: 49165286
Conc: 209.34 ng/ml

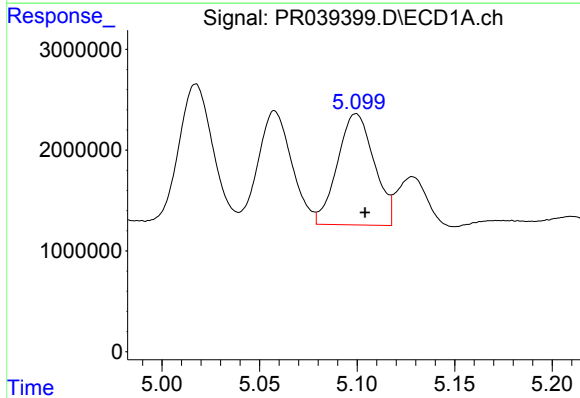


#23 AR-1248-3

R.T.: 5.099 min
Delta R.T.: -0.005 min
Response: 14471453
Conc: 221.67 ng/ml

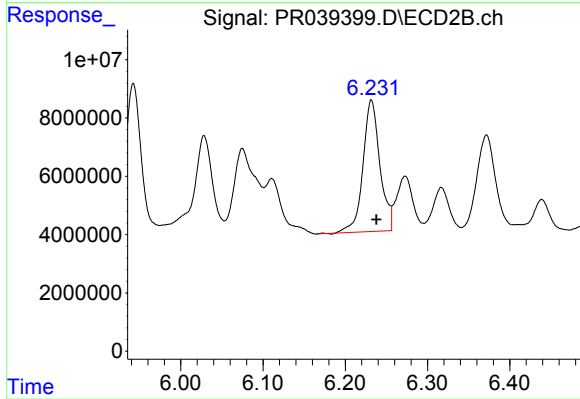

#23 AR-1248-3


R.T.: 6.232 min
Delta R.T.: -0.006 min
Response: 64660437
Conc: 233.96 ng/ml

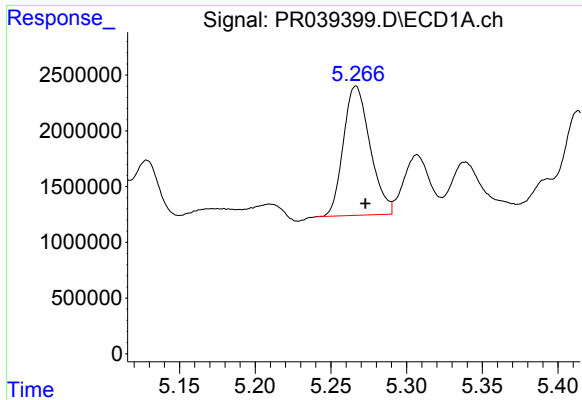

#24 AR-1248-4


R.T.: 5.266 min
Delta R.T.: -0.006 min
Response: 1422222
Conc: 173.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

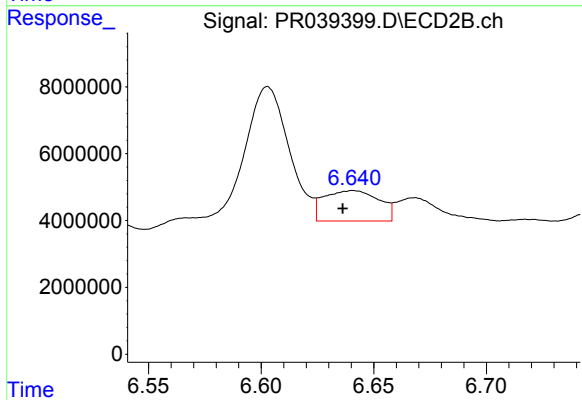


#24 AR-1248-4

R.T.: 6.641 min
Delta R.T.: 0.005 min
Response: 15488080
Conc: 46.15 ng/ml

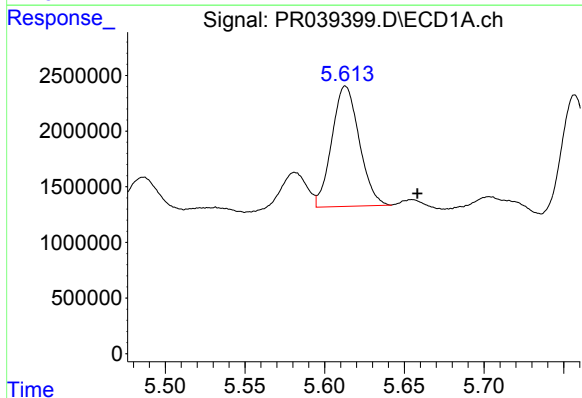


#25 AR-1248-5

R.T.: 5.613 min
Delta R.T.: -0.045 min
Response: 12947485
Conc: 148.19 ng/ml

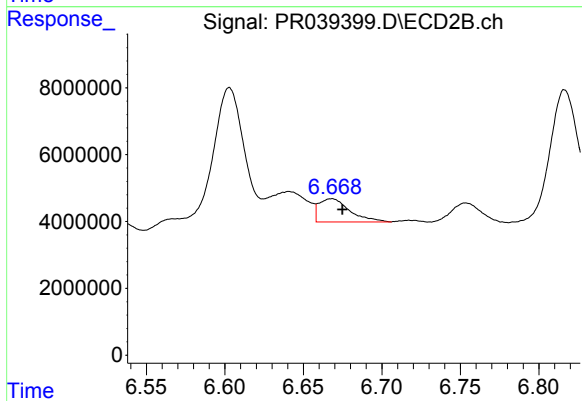

#25 AR-1248-5


R.T.: 6.668 min
Delta R.T.: -0.007 min
Response: 9519482
Conc: 29.65 ng/ml

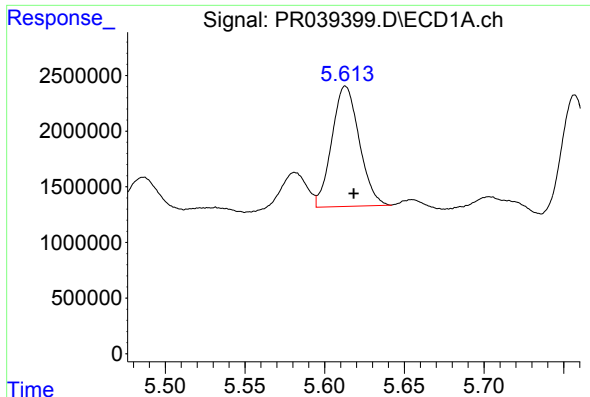

#26 AR-1254-1


R.T.: 5.613 min
Delta R.T.: -0.005 min
Response: 12947485
Conc: 97.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

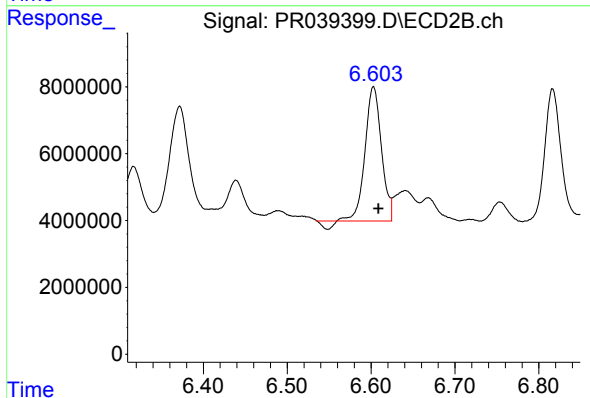


#26 AR-1254-1

R.T.: 6.603 min
Delta R.T.: -0.006 min
Response: 53467669
Conc: 166.98 ng/ml

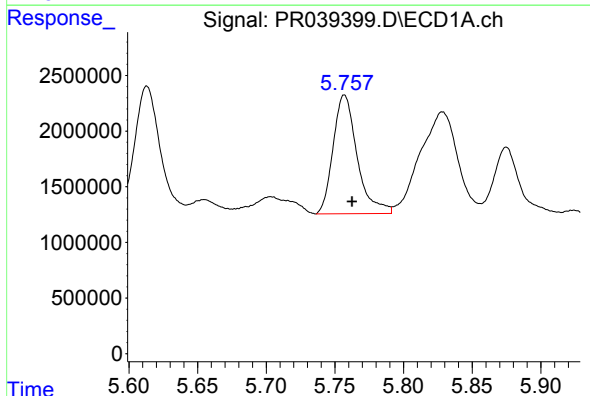


#27 AR-1254-2

R.T.: 5.757 min
Delta R.T.: -0.006 min
Response: 13021913
Conc: 111.17 ng/ml

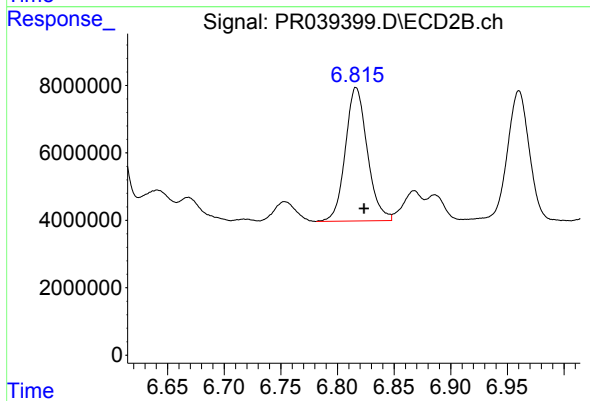

#27 AR-1254-2


R.T.: 6.816 min
Delta R.T.: -0.007 min
Response: 53496199
Conc: 104.54 ng/ml

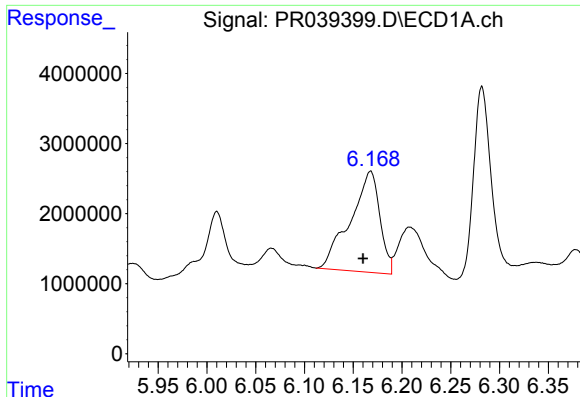

#28 AR-1254-3


R.T.: 6.168 min
Delta R.T.: 0.008 min
Response: 30384251
Conc: 147.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

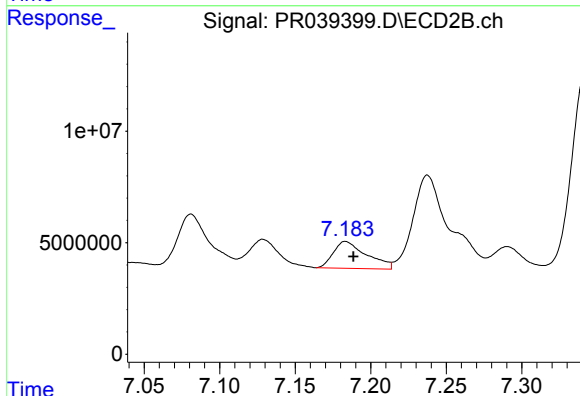


#28 AR-1254-3

R.T.: 7.183 min
Delta R.T.: -0.005 min
Response: 18544831
Conc: 30.90 ng/ml

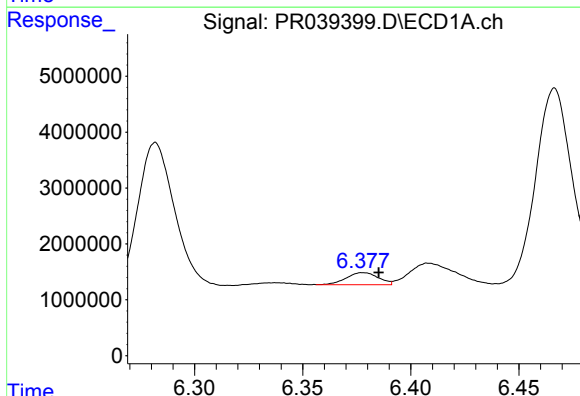


#29 AR-1254-4

R.T.: 6.378 min
Delta R.T.: -0.007 min
Response: 2234292
Conc: 14.59 ng/ml

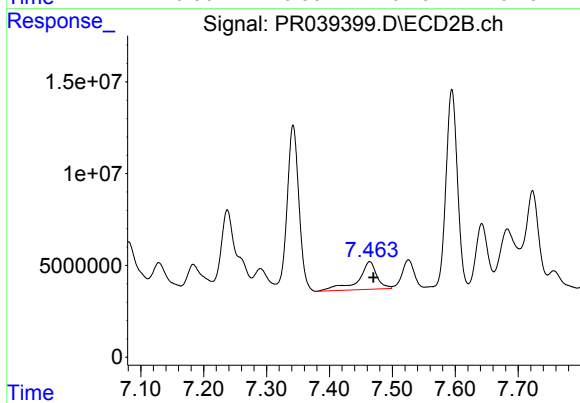

#29 AR-1254-4


R.T.: 7.464 min
Delta R.T.: -0.006 min
Response: 31557992
Conc: 72.92 ng/ml

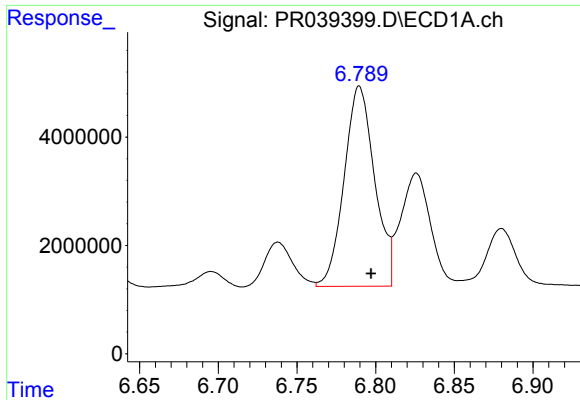

#30 AR-1254-5


R.T.: 6.790 min
Delta R.T.: -0.007 min
Response: 49850933
Conc: 267.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

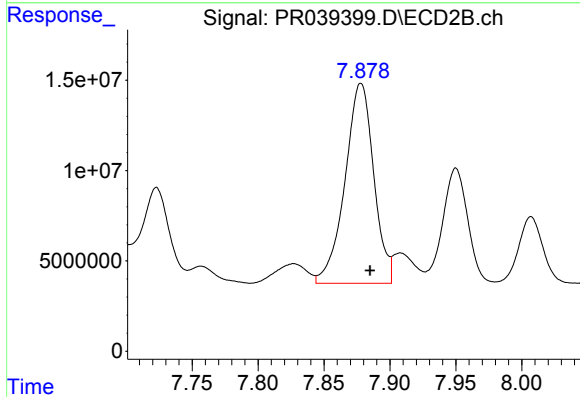


#30 AR-1254-5

R.T.: 7.878 min
Delta R.T.: -0.007 min
Response: 168182039
Conc: 357.85 ng/ml

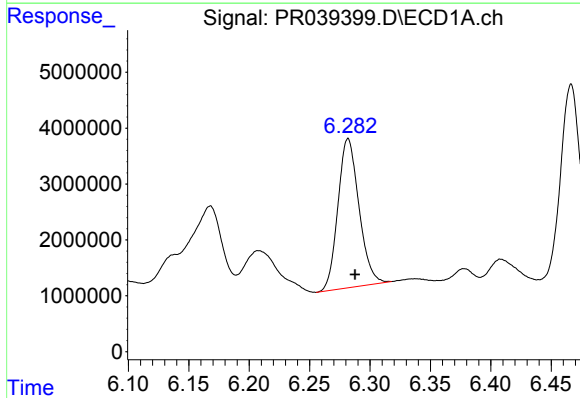


#31 AR-1260-1

R.T.: 6.282 min
Delta R.T.: -0.006 min
Response: 32366871
Conc: 282.43 ng/ml

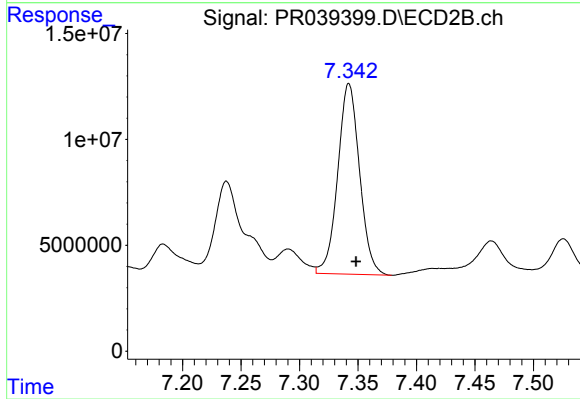

#31 AR-1260-1


R.T.: 7.342 min
Delta R.T.: -0.006 min
Response: 117021344
Conc: 322.26 ng/ml

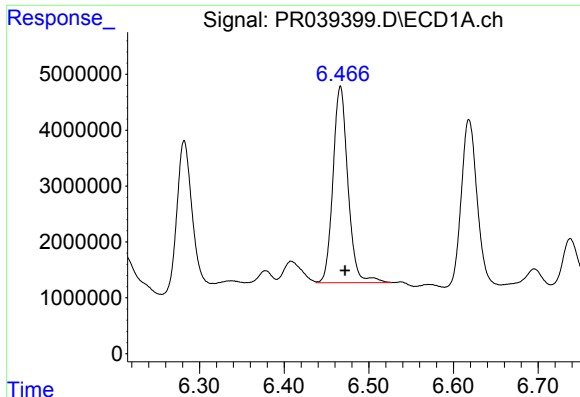

#32 AR-1260-2


R.T.: 6.467 min
Delta R.T.: -0.006 min
Response: 43122448
Conc: 285.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

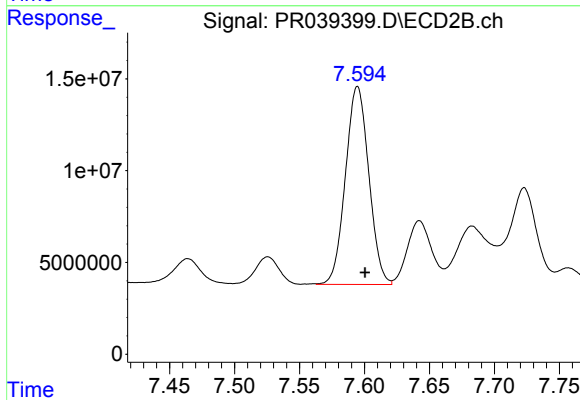


#32 AR-1260-2

R.T.: 7.595 min
Delta R.T.: -0.006 min
Response: 134957358
Conc: 308.54 ng/ml

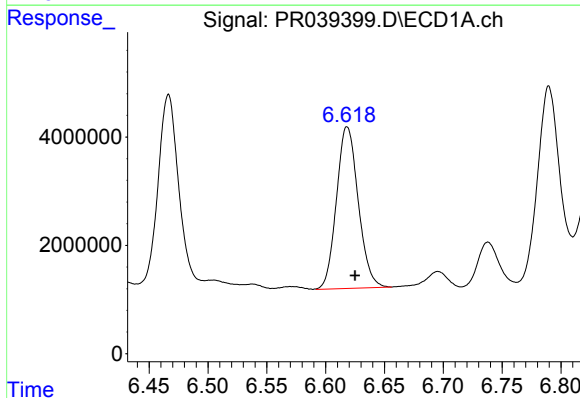


#33 AR-1260-3

R.T.: 6.618 min
Delta R.T.: -0.007 min
Response: 38423644
Conc: 285.50 ng/ml

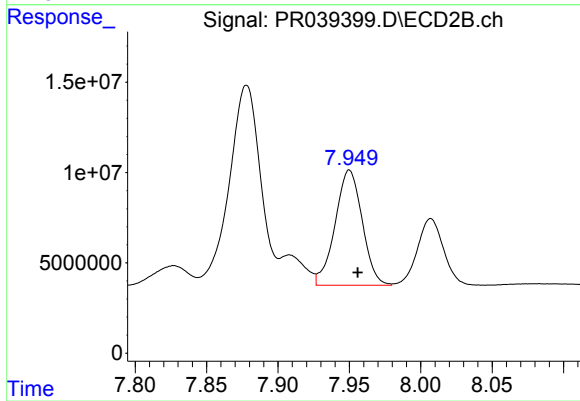

#33 AR-1260-3


R.T.: 7.950 min
Delta R.T.: -0.006 min
Response: 84268382
Conc: 248.30 ng/ml

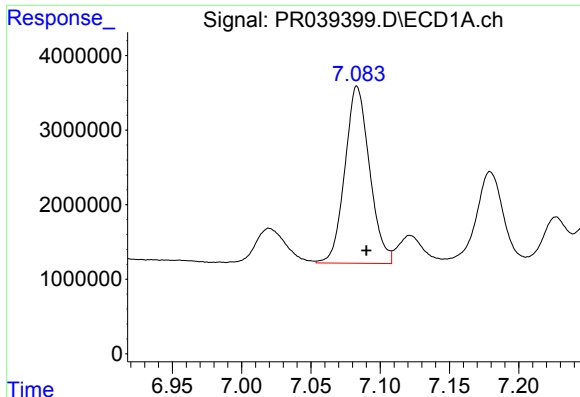

#34 AR-1260-4


R.T.: 7.083 min
Delta R.T.: -0.007 min
Response: 29441780
Conc: 245.98 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

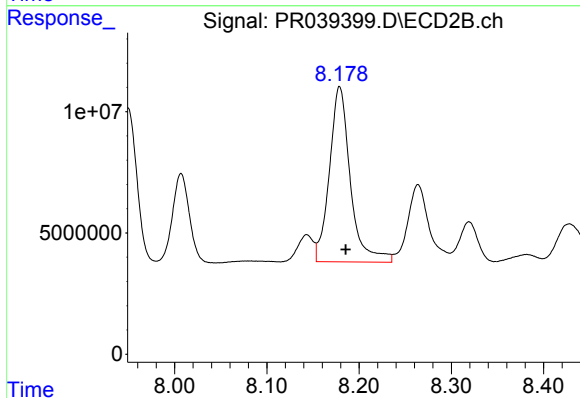


#34 AR-1260-4

R.T.: 8.179 min
Delta R.T.: -0.007 min
Response: 114141290
Conc: 280.88 ng/ml

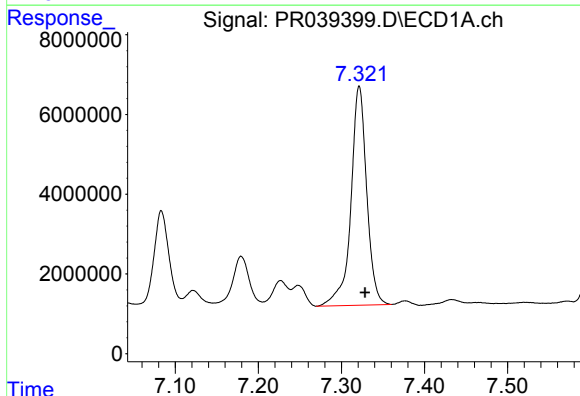


#35 AR-1260-5

R.T.: 7.321 min
Delta R.T.: -0.007 min
Response: 72628802
Conc: 241.67 ng/ml

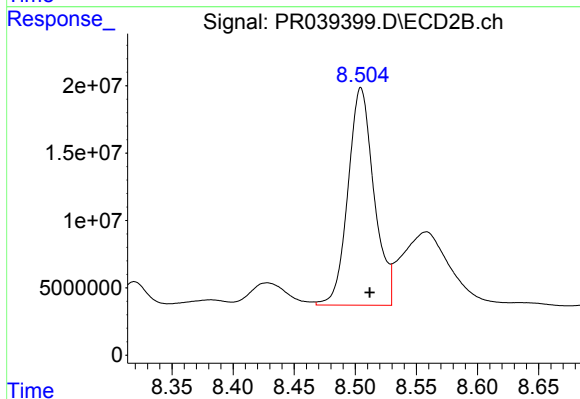

#35 AR-1260-5


R.T.: 8.505 min
Delta R.T.: -0.007 min
Response: 239030346
Conc: 279.52 ng/ml

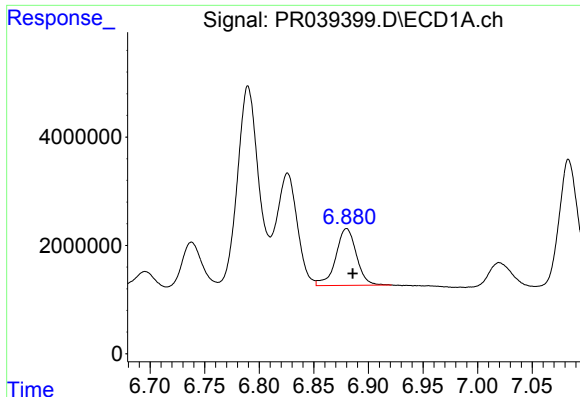

#36 AR-1262-1


R.T.: 6.880 min
Delta R.T.: -0.006 min
Response: 13836004
Conc: 145.96 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

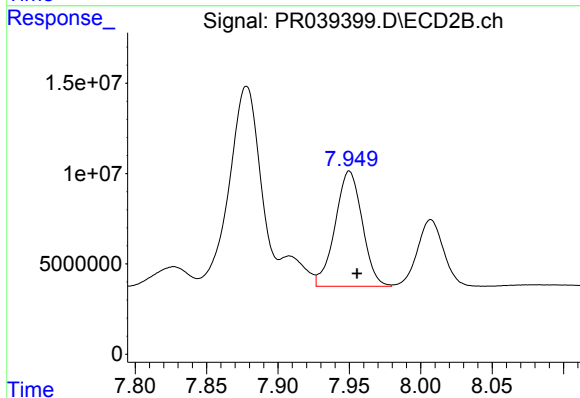


#36 AR-1262-1

R.T.: 7.950 min
Delta R.T.: -0.005 min
Response: 84268382
Conc: 121.35 ng/ml

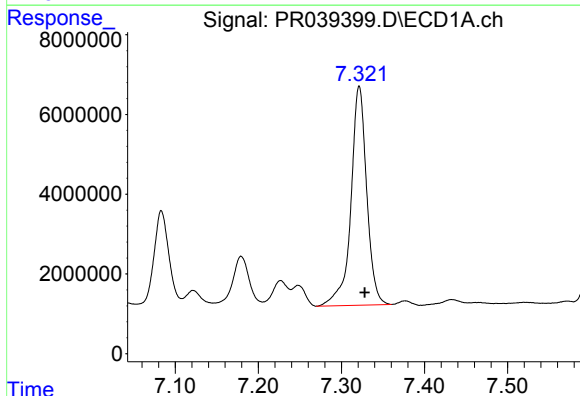


#37 AR-1262-2

R.T.: 7.321 min
Delta R.T.: -0.006 min
Response: 72628802
Conc: 149.29 ng/ml

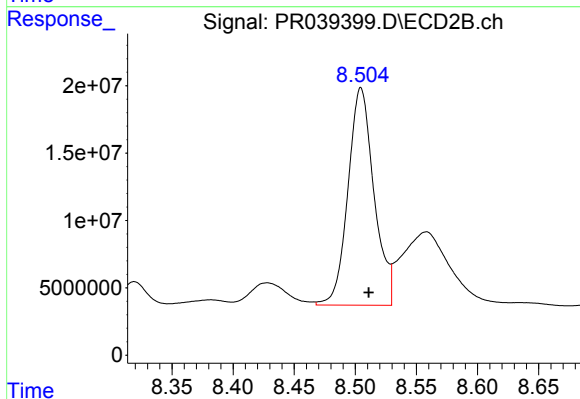

#37 AR-1262-2


R.T.: 8.505 min
Delta R.T.: -0.006 min
Response: 239030346
Conc: 174.38 ng/ml

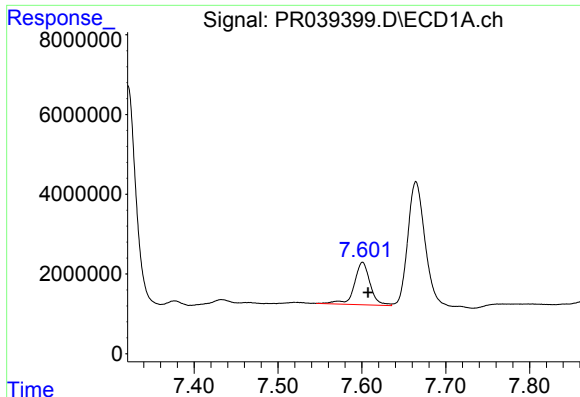

#38 AR-1262-3


R.T.: 7.601 min
Delta R.T.: -0.007 min
Response: 13990251
Conc: 77.03 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

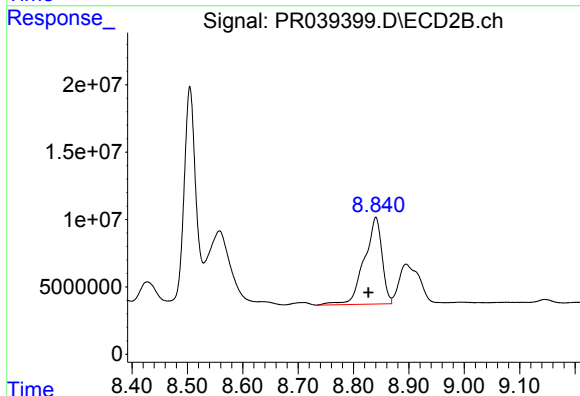


#38 AR-1262-3

R.T.: 8.840 min
Delta R.T.: 0.013 min
Response: 143206308
Conc: 158.98 ng/ml

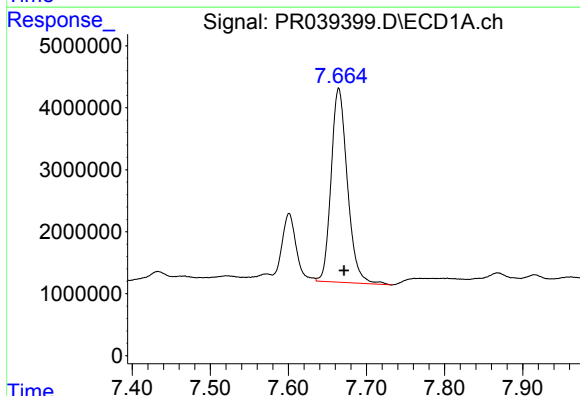


#39 AR-1262-4

R.T.: 7.665 min
Delta R.T.: -0.007 min
Response: 45298369
Conc: 127.32 ng/ml

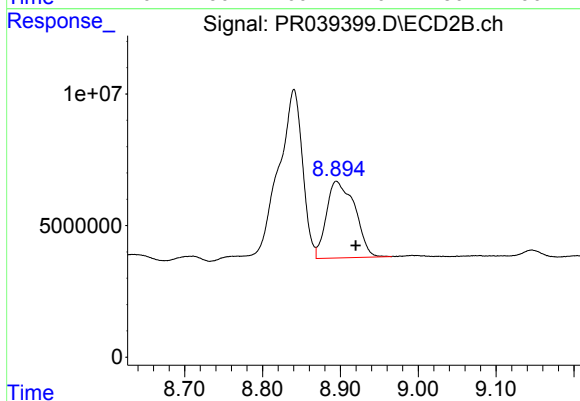

#39 AR-1262-4


R.T.: 8.895 min
Delta R.T.: -0.025 min
Response: 73880938
Conc: 110.04 ng/ml

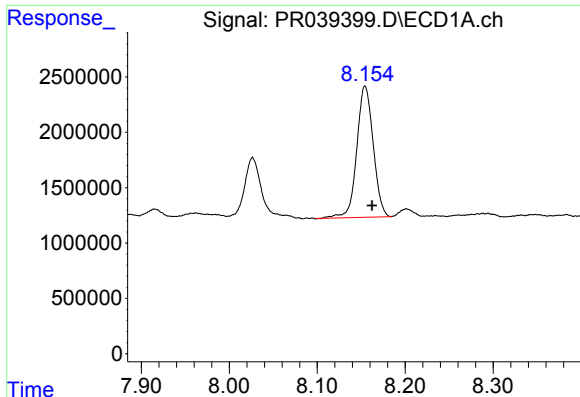

#40 AR-1262-5


R.T.: 8.154 min
Delta R.T.: -0.008 min
Response: 15383590
Conc: 94.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

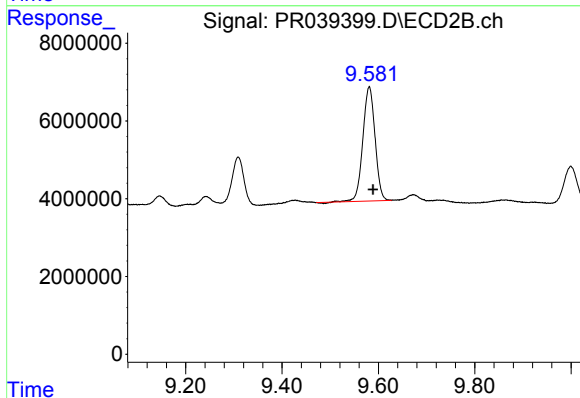


#40 AR-1262-5

R.T.: 9.581 min
Delta R.T.: -0.007 min
Response: 51423829
Conc: 105.05 ng/ml

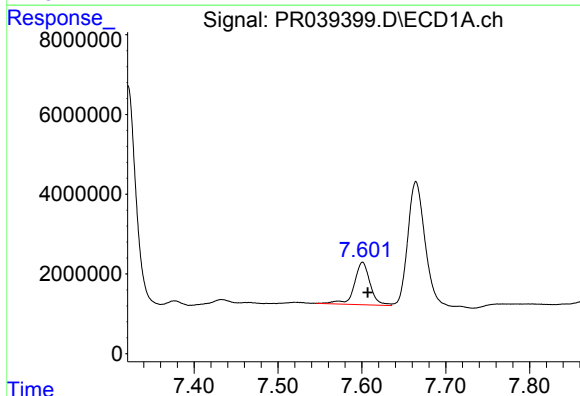


#41 AR-1268-1

R.T.: 7.601 min
Delta R.T.: -0.006 min
Response: 13990251
Conc: 25.91 ng/ml

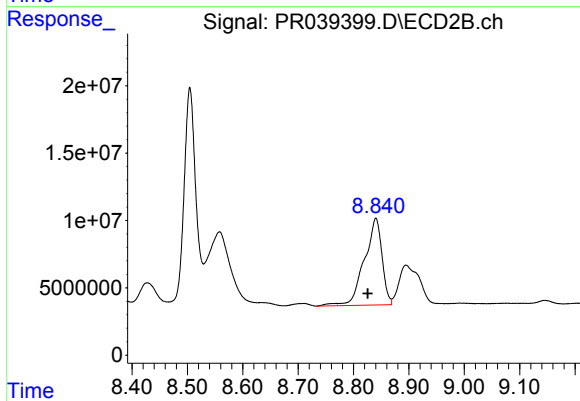

#41 AR-1268-1


R.T.: 8.840 min
Delta R.T.: 0.015 min
Response: 143206308
Conc: 90.88 ng/ml

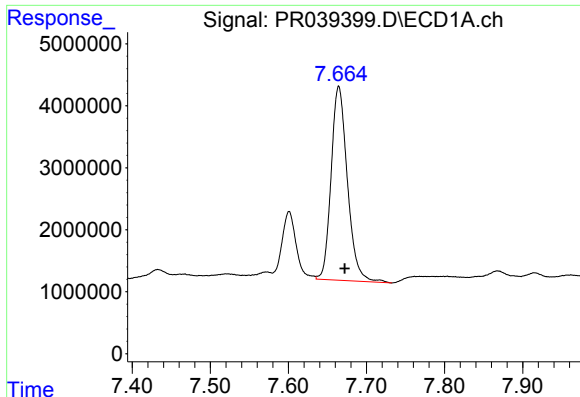

#42 AR-1268-2


R.T.: 7.665 min
Delta R.T.: -0.008 min
Response: 45298369
Conc: 91.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

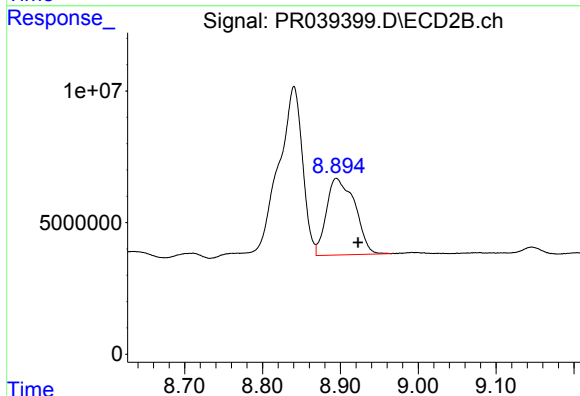


#42 AR-1268-2

R.T.: 8.895 min
Delta R.T.: -0.028 min
Response: 73880938
Conc: 50.36 ng/ml

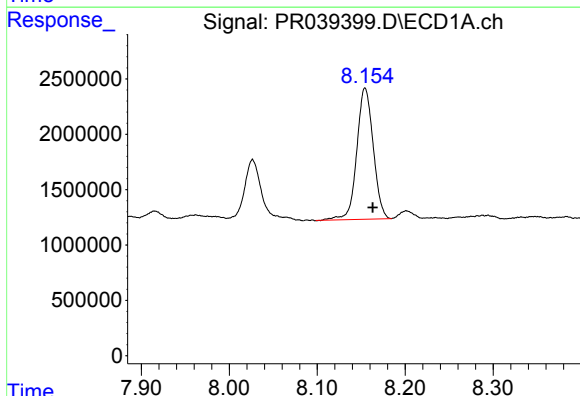


#44 AR-1268-4

R.T.: 8.154 min
Delta R.T.: -0.009 min
Response: 15383590
Conc: 86.11 ng/ml

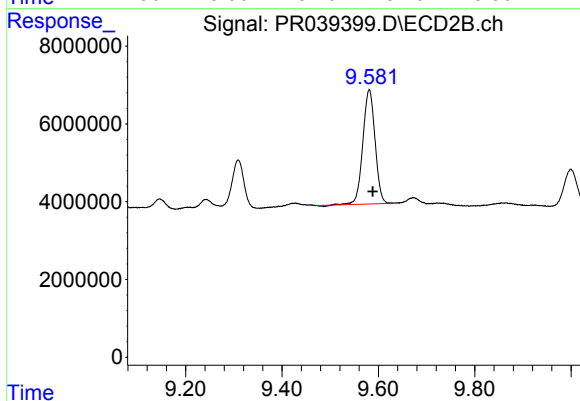

#44 AR-1268-4


R.T.: 9.581 min
Delta R.T.: -0.007 min
Response: 51423829
Conc: 97.06 ng/ml

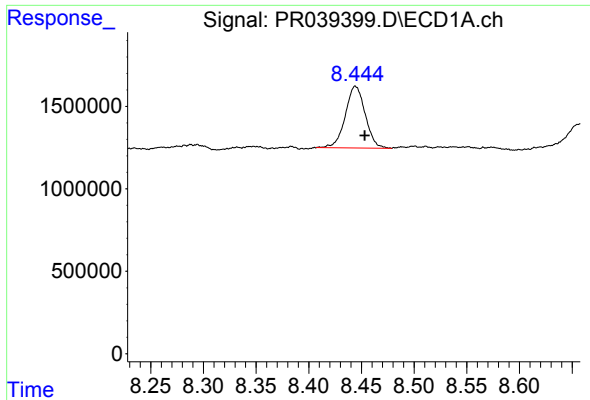

#45 AR-1268-5

R.T.: 8.444 min
Delta R.T.: -0.009 min
Response: 4913694
Conc: 3.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MANHOLE-TEST-PITMSD

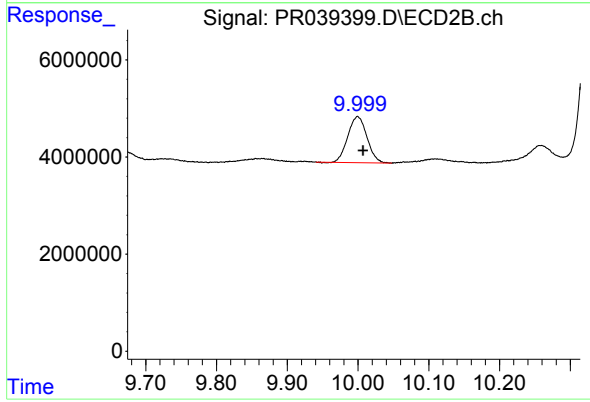

#45 AR-1268-5

R.T.: 9.999 min
Delta R.T.: -0.008 min
Response: 17891654
Conc: 4.17 ng/ml