

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071819\
 Data File : PR039412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 21:46
 Operator : SM\AJ
 Sample : K3885-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 S10-03-S

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:53:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 01:38:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 16 02:56:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.757	4.603	34697384	139.7E6	22.401	21.600
2)	SA Decachlor...	8.697	10.340	41991290	150.6E6	17.172	17.594
Target Compounds							
26)	L6 AR-1254-1	5.618	6.607	2467990	3566844	18.661m	11.139m#
27)	L6 AR-1254-2	5.757	6.816	1329313	26169992	11.348m	51.141 #
28)	L6 AR-1254-3	6.154	7.189	3290579	19971382	15.925m	33.280 #
29)	L6 AR-1254-4	6.378	7.464	2342963	8837159	15.304m	20.420 #
30)	L6 AR-1254-5	6.789	7.878	3953032	13019483	21.219m	27.703 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR071819\
Data File : PR039412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 21:46
Operator : SM\AJ
Sample : K3885-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
S10-03-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:53:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 01:38:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071519.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 16 02:56:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

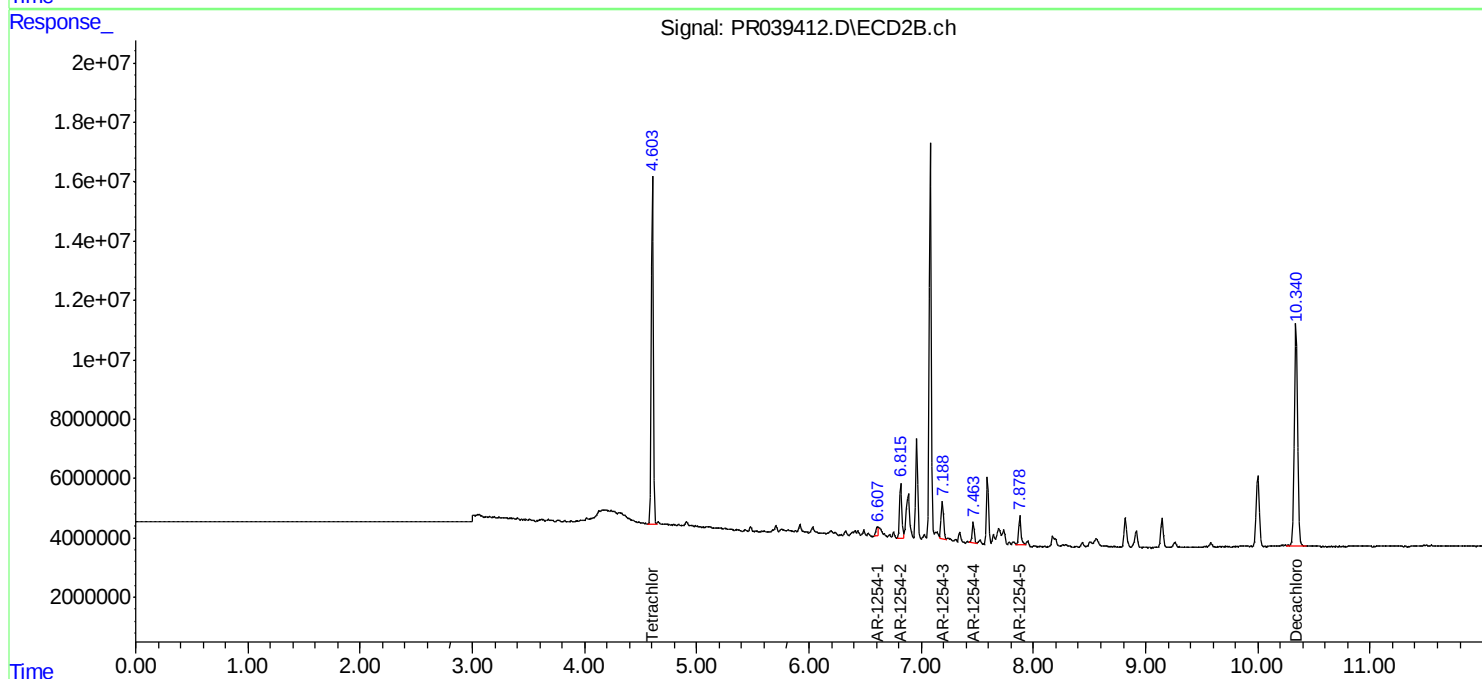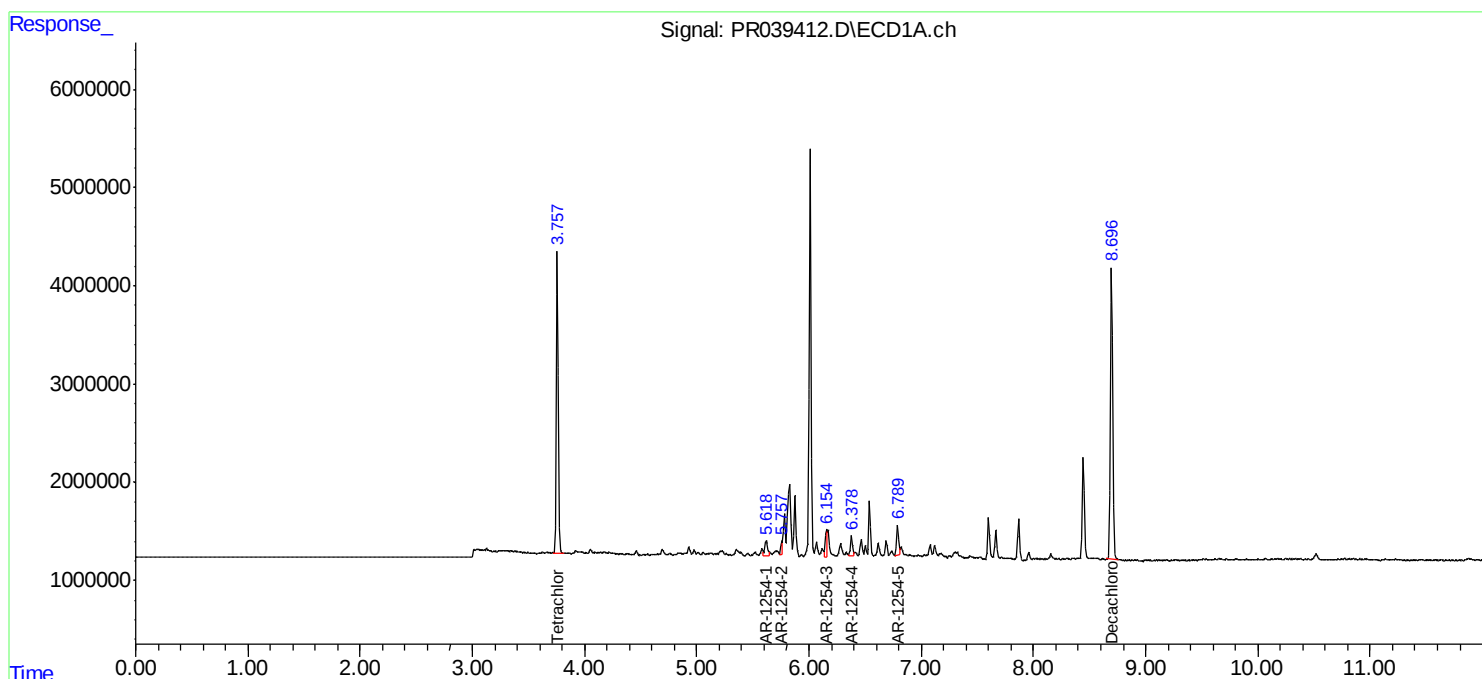

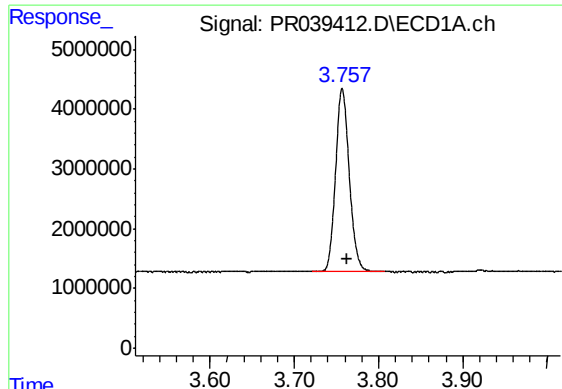


#1 Tetrachloro-m-xylene

R.T.: 3.757 min
Delta R.T.: -0.006 min
Response: 34697384
Conc: 22.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
S10-03-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:53:00 AM

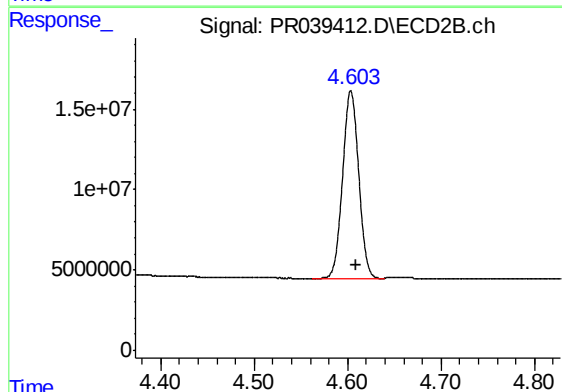


#1 Tetrachloro-m-xylene

R.T.: 4.603 min
Delta R.T.: -0.006 min
Response: 139692448
Conc: 21.60 ng/ml

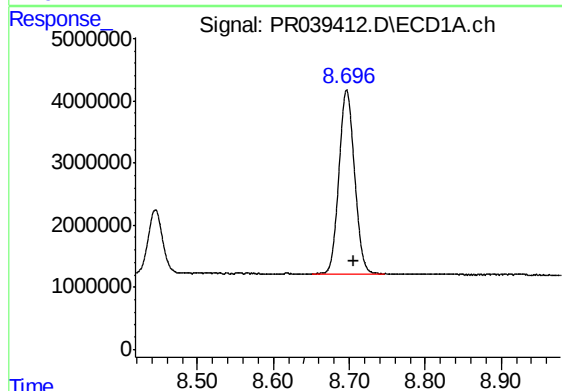


#2 Decachlorobiphenyl

R.T.: 8.697 min
Delta R.T.: -0.009 min
Response: 41991290
Conc: 17.17 ng/ml

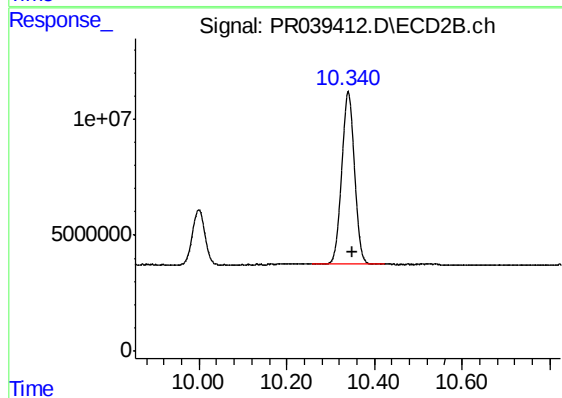

#2 Decachlorobiphenyl

R.T.: 10.340 min
Delta R.T.: -0.009 min
Response: 150563718
Conc: 17.59 ng/ml

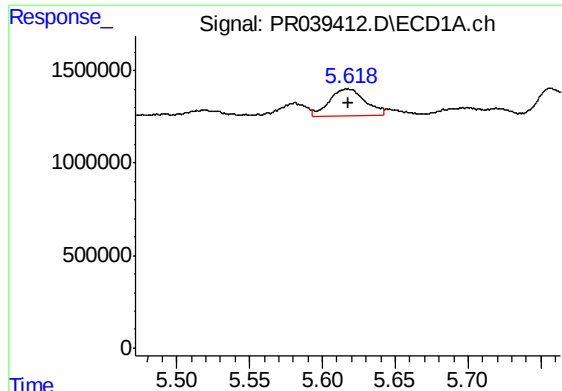


#26 AR-1254-1

R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 2467990
Conc: 18.66 ng/ml m

Instrument :
ECD_R
ClientSampleId :
S10-03-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:53:00 AM

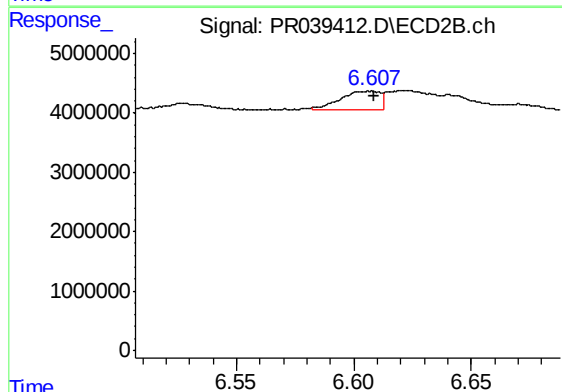


#26 AR-1254-1

R.T.: 6.607 min
Delta R.T.: -0.001 min
Response: 3566844
Conc: 11.14 ng/ml m

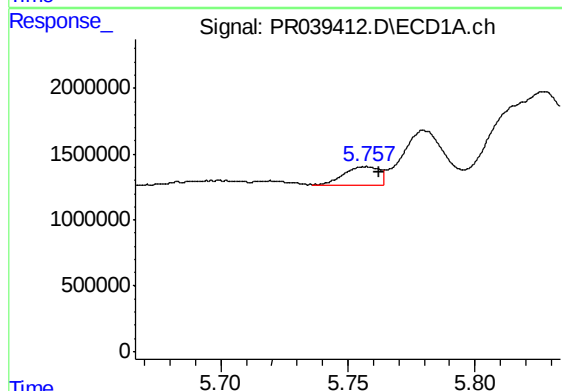


#27 AR-1254-2

R.T.: 5.757 min
Delta R.T.: -0.005 min
Response: 1329313
Conc: 11.35 ng/ml m

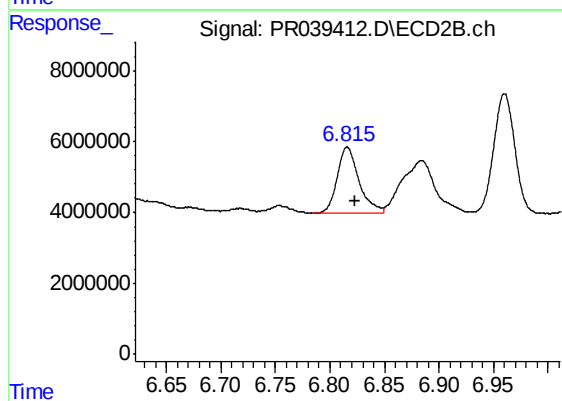

#27 AR-1254-2

R.T.: 6.816 min
Delta R.T.: -0.008 min
Response: 26169992
Conc: 51.14 ng/ml

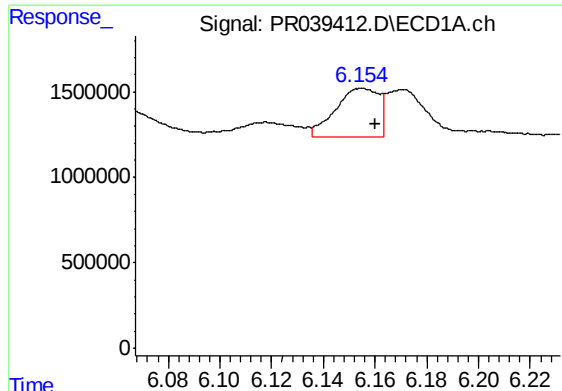


#28 AR-1254-3

R.T.: 6.154 min
Delta R.T.: -0.006 min
Response: 3290579
Conc: 15.92 ng/ml m

Instrument :
ECD_R
ClientSampleId :
S10-03-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:53:00 AM

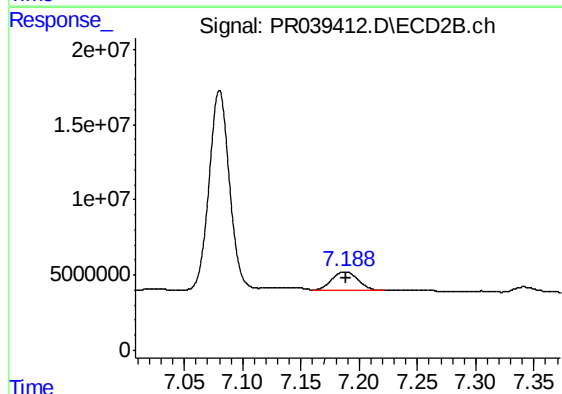


#28 AR-1254-3

R.T.: 7.189 min
Delta R.T.: 0.000 min
Response: 19971382
Conc: 33.28 ng/ml

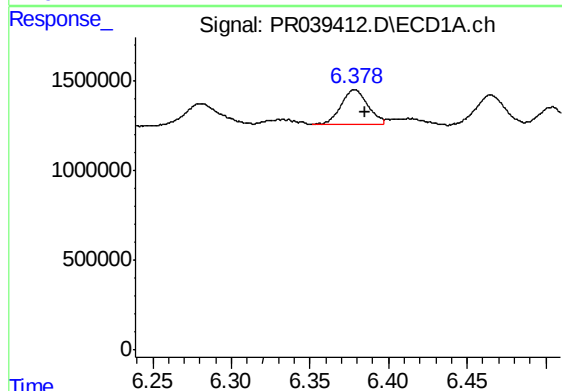


#29 AR-1254-4

R.T.: 6.378 min
Delta R.T.: -0.008 min
Response: 2342963
Conc: 15.30 ng/ml m

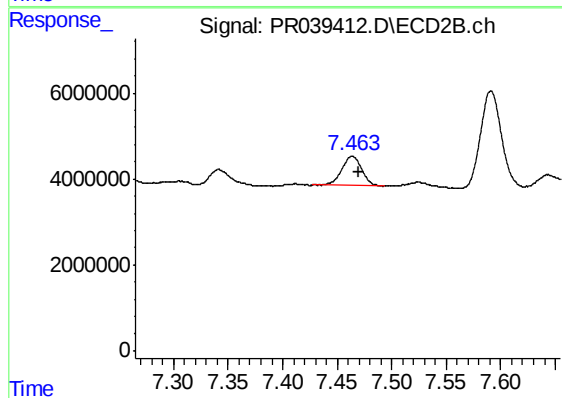

#29 AR-1254-4

R.T.: 7.464 min
Delta R.T.: -0.006 min
Response: 8837159
Conc: 20.42 ng/ml

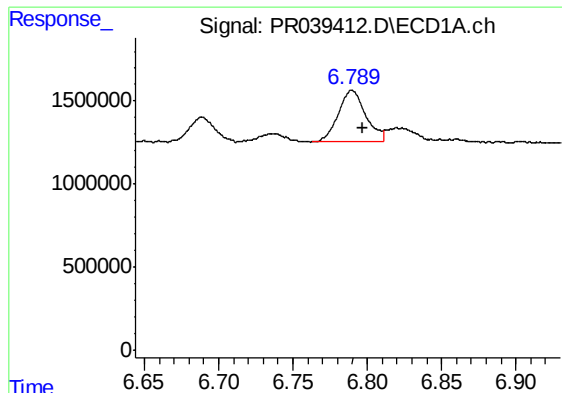


#30 AR-1254-5

R.T.: 6.789 min
Delta R.T.: -0.008 min
Response: 3953032
Conc: 21.22 ng/ml m

Instrument :
ECD_R
ClientSampleId :
S10-03-S

Manual Integrations
APPROVED

Ankita
7/21/2019 11:53:00 AM

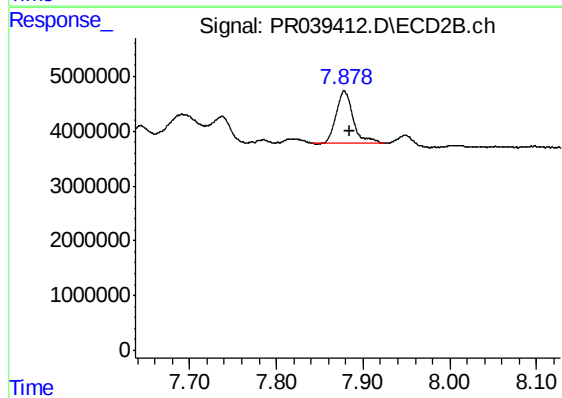

#30 AR-1254-5

R.T.: 7.878 min
Delta R.T.: -0.007 min
Response: 13019483
Conc: 27.70 ng/ml