

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072018\
Data File : PR030465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2018 15:09
Operator : SM\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
ECD_R
LabSampleId :
AR1660312

Manual Integrations
APPROVED

Sohil
7/21/2018 11:05:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 03:09:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071318CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 18 11:23:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

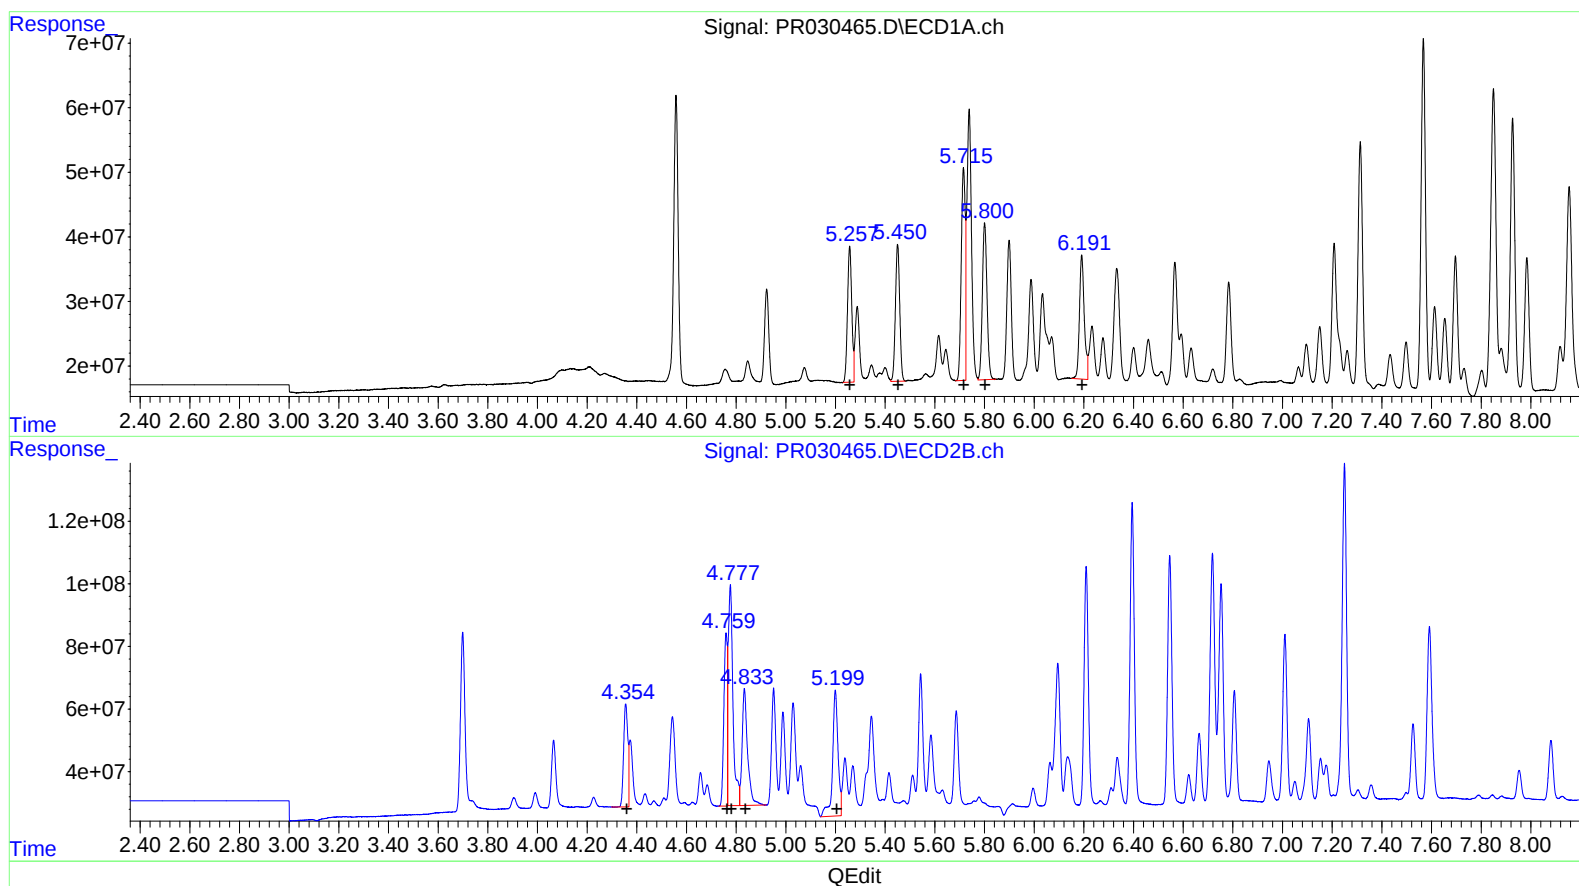

(3) AR-1016-1 (L1)
R.T. Response Conc
5.26 250807372 398.56
5.45 255909872 417.54
5.72 369748641 403.25
5.80 316356345 405.64
6.19 259342131 410.34

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
4.36 388056222 359.69
4.76 527873653 354.25
4.78 939333901 372.12
4.83 572435025 371.50
5.20 614581163 470.97

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072018\
Data File : PR030465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2018 15:09
Operator : SM\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
ECD_R
LabSampleId :
AR1660312

Manual Integrations
APPROVED

Sohil
7/21/2018 11:05:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 03:09:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071318CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 18 11:23:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

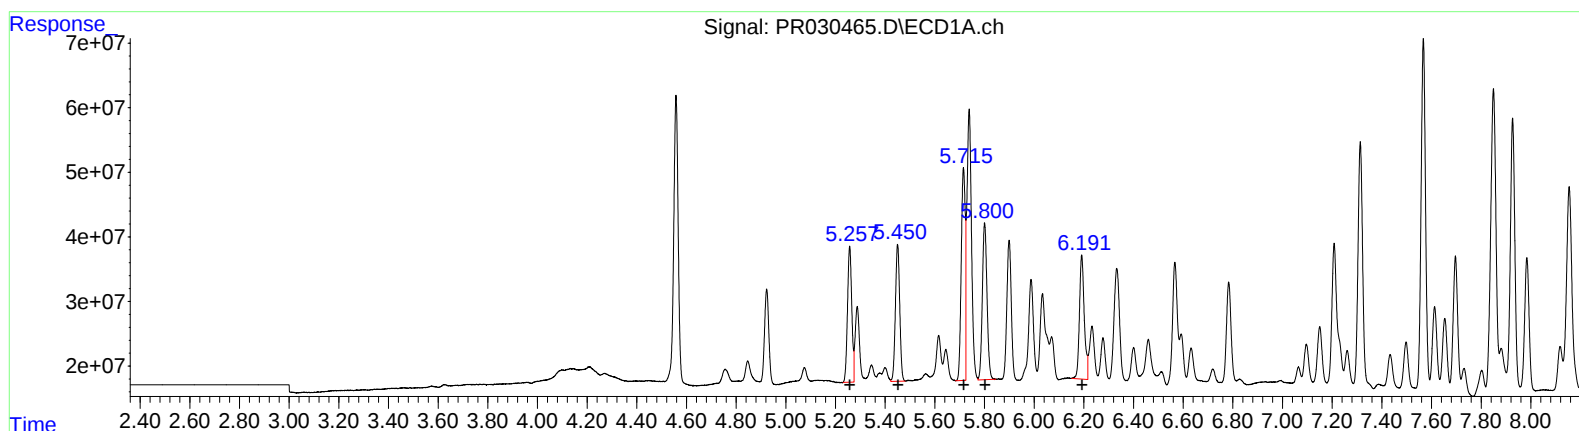

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
5.26 250807372 398.56
5.45 255909872 417.54
5.72 369748641 403.25
5.80 316356345 405.64
6.19 259342131 410.34

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
4.36 388056222 359.69
4.76 527873653 354.25
4.78 939333901 372.12
4.83 572435025 371.50
5.20 480691051 368.36

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072018\
Data File : PR030465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2018 15:09
Operator : SM\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
ECD_R
LabSampleId :
AR1660312

Manual Integrations
APPROVED

Sohil
7/21/2018 11:05:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 03:09:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071318CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 18 11:23:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

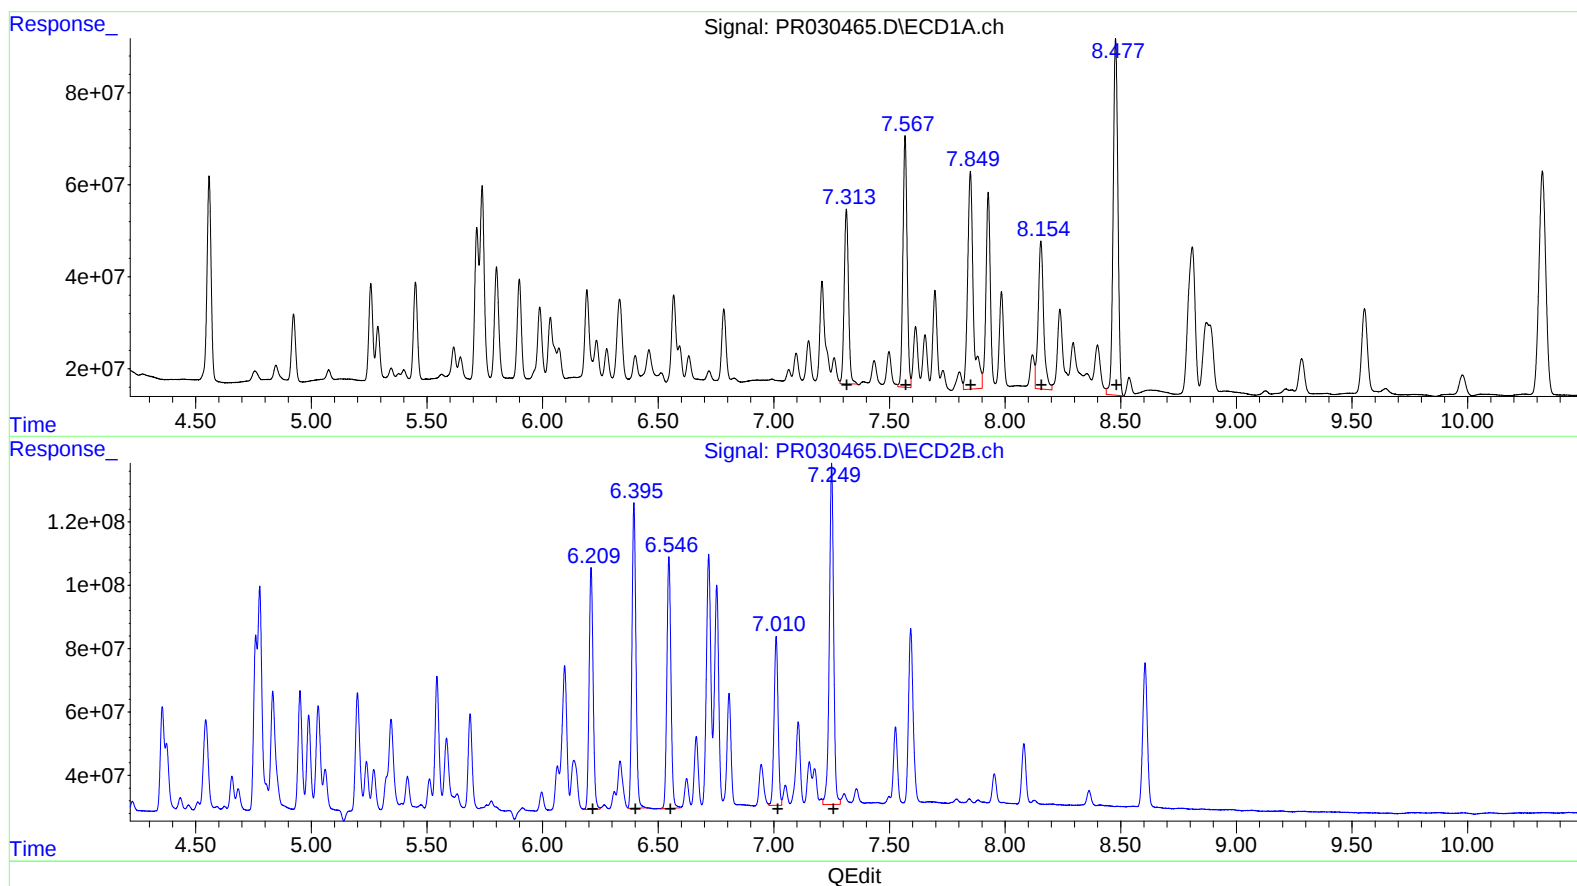

(31) AR-1260-1 (L7)
R.T. Response Conc
7.31 492503673 406.65
7.57 686224978 420.49
7.85 803236287 455.47
8.15 521501901 468.99
8.48 1108895016 444.73

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.21 915987871 433.74
6.40 1143269631 464.99
6.55 969962730 469.58
7.01 640735577 463.80
7.25 1384178932 441.97

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072018\
Data File : PR030465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2018 15:09
Operator : SM\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
ECD_R
LabSampleId :
AR1660312

Manual Integrations
APPROVED

Sohil
7/21/2018 11:05:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 03:09:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071318CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 18 11:23:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

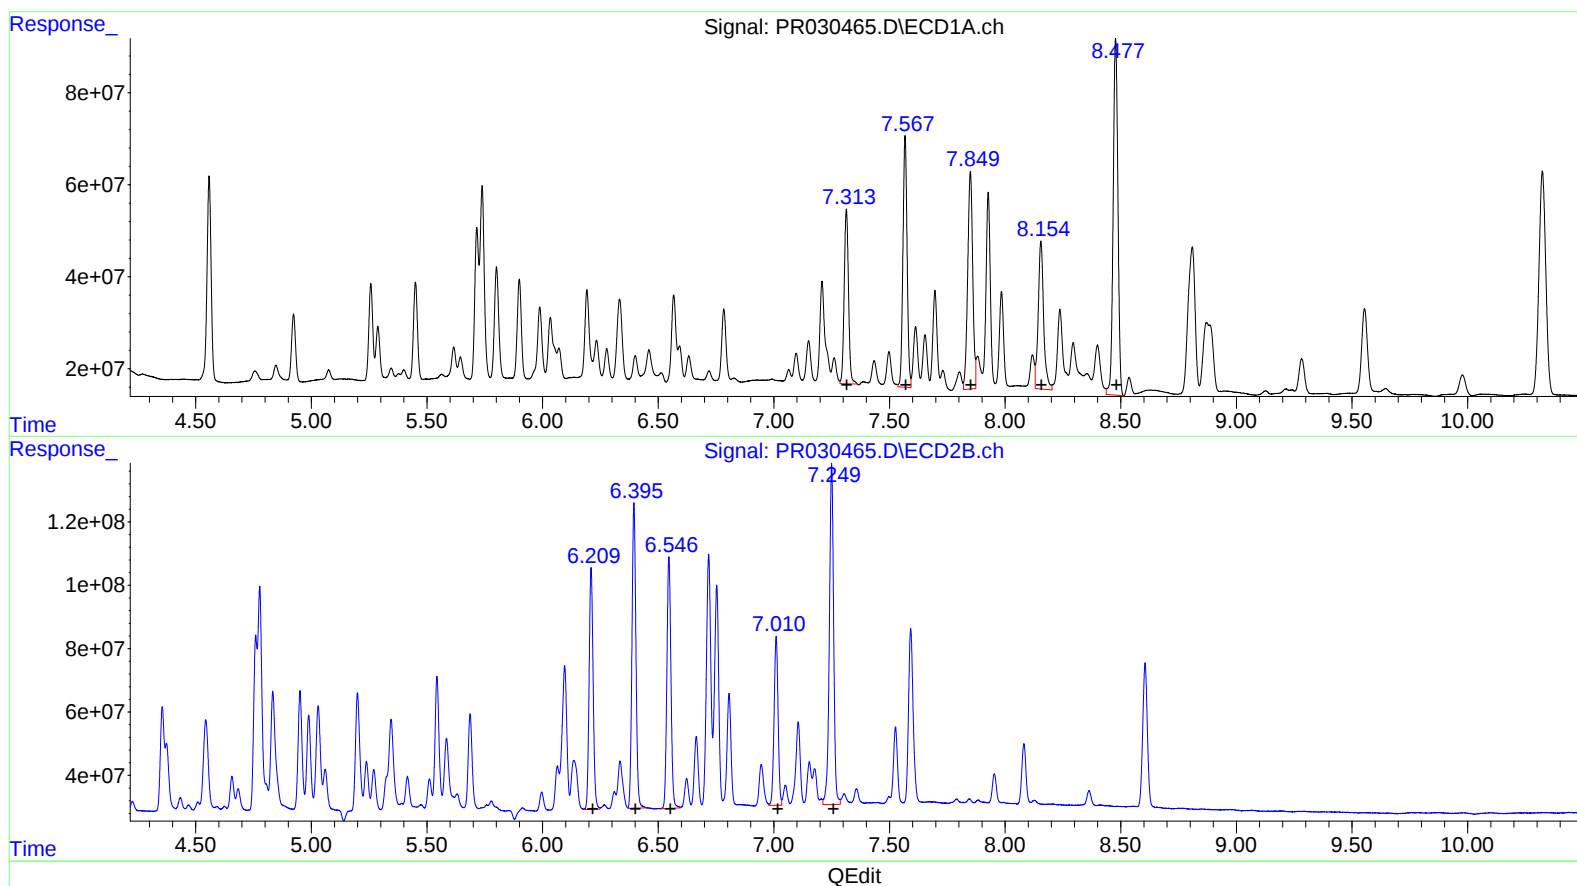

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
7.31 492503673 406.65
7.57 686224978 420.49
7.85 709592907 402.37
8.15 521501901 468.99
8.48 1108895016 444.73

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.21 915987871 433.74
6.40 1143269631 464.99
6.55 969962730 469.58
7.01 640735577 463.80
7.25 1384178932 441.97

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072018\
 Data File : PR030465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2018 15:09
 Operator : SM\MA
 Sample : AR1660CCC400
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_R
 LabSampleId :
 AR1660312

Manual Integrations
 APPROVED

Sohil
 7/21/2018 11:05:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 03:09:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR071318CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 18 11:23:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.558	3.699	554.8E6	691.6E6	19.711	19.231
2) SA Decachlor...	10.323	8.605	1001.0E6	629.3E6	44.671	41.171
Target Compounds						
3) L1 AR-1016-1	5.257	4.356	250.8E6	388.1E6	398.556	359.692
4) L1 AR-1016-2	5.450	4.760	255.9E6	527.9E6	417.541	354.255
5) L1 AR-1016-3	5.716	4.777	369.7E6	939.3E6	403.246	372.118
6) L1 AR-1016-4	5.801	4.833	316.4E6	572.4E6	405.642	371.503
7) L1 AR-1016-5	6.192	5.199	259.3E6	480.7E6	410.340	368.365m)
31) L7 AR-1260-1	7.314	6.210	492.5E6	916.0E6	406.645	433.741
32) L7 AR-1260-2	7.567	6.395	686.2E6	1143.3E6	420.488	464.987
33) L7 AR-1260-3	7.849	6.546	709.6E6	970.0E6	402.369m)	469.580
34) L7 AR-1260-4	8.155	7.010	521.5E6	640.7E6	468.988	463.796
35) L7 AR-1260-5	8.478	7.250	1108.9E6	1384.2E6	444.732	441.967

} 35 07/23/18

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.