

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072319\
 Data File : PR039614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2019 12:54
 Operator : SM\AJ
 Sample : K3941-03DL 4X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 K580-S3DL

Manual Integrations
 APPROVED

Ankita
 7/23/2019 5:14:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 13:44:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 22 14:03:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.755	4.602	9832068	39778278	4.097	3.968
2) SA Decachlor...	8.696	10.337	100.6E6	376.0E6	40.489	40.047
Target Compounds						
31) L7 AR-1260-1	6.279	7.339	72474937	242.0E6	497.320	545.324
32) L7 AR-1260-2	6.465	7.592	123.3E6	334.7E6	669.488	610.504
33) L7 AR-1260-3	6.616	7.948	76415926	169.4E6	461.260	404.119
34) L7 AR-1260-4	7.081	8.175	62752228	252.3E6	451.433	523.005
35) L7 AR-1260-5	7.319	8.502	164.1E6	438.9E6	475.598	427.959

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072319\
Data File : PR039614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2019 12:54
Operator : SM\AJ
Sample : K3941-03DL 4X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
K580-S3DL


Manual Integrations
APPROVED

Ankita
7/23/2019 5:14:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 13:44:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 22 14:03:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

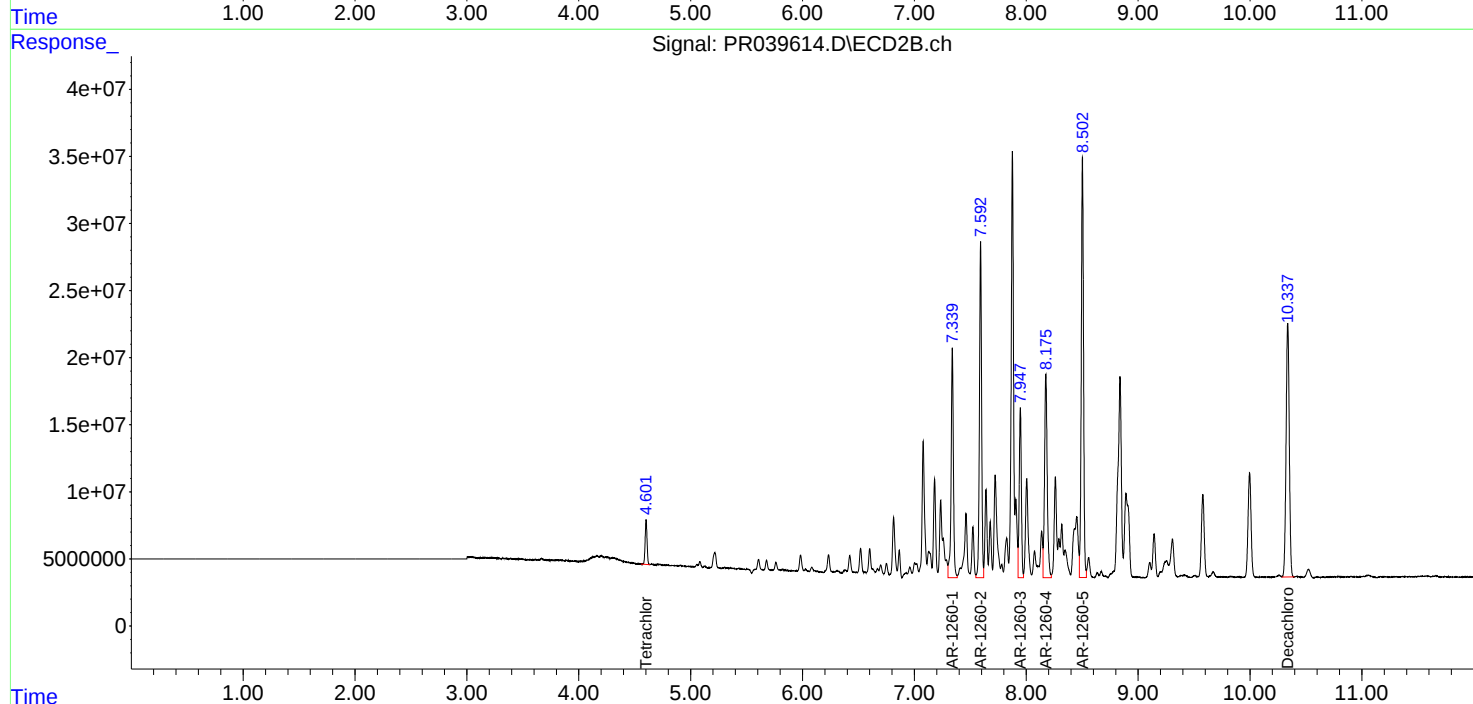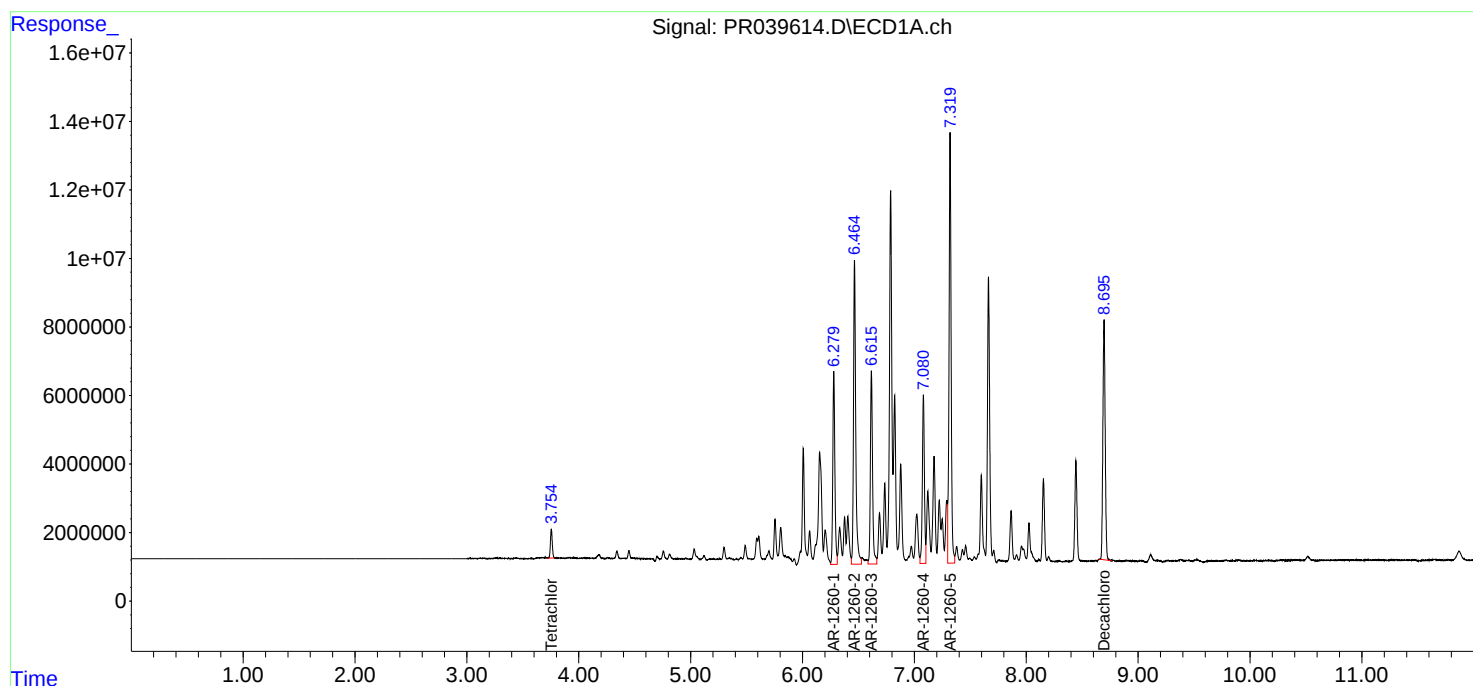

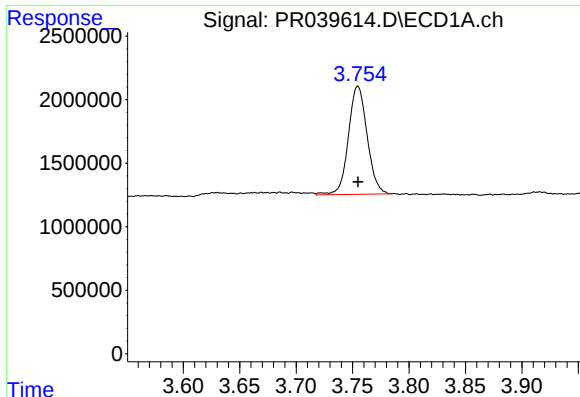


#1 Tetrachloro-m-xylene

R.T.: 3.755 min
Delta R.T.: 0.000 min
Response: 9832068
Conc: 4.10 ng/ml

Instrument :
ECD_R
ClientSampleId :
K580-S3DL


Manual Integrations
APPROVED

Ankita
7/23/2019 5:14:09 PM

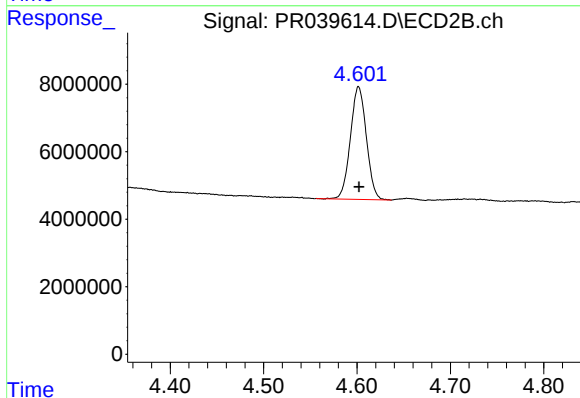


#1 Tetrachloro-m-xylene

R.T.: 4.602 min
Delta R.T.: 0.000 min
Response: 39778278
Conc: 3.97 ng/ml

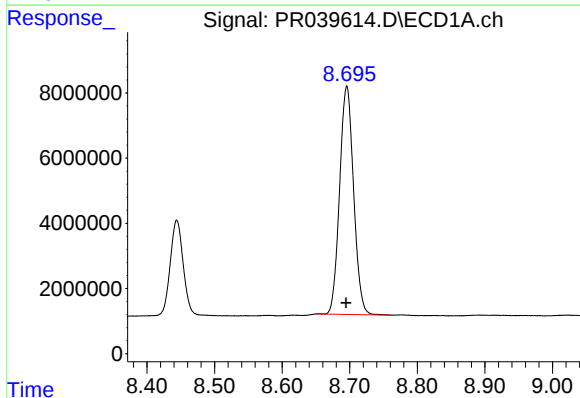


#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: 0.000 min
Response: 100598531
Conc: 40.49 ng/ml

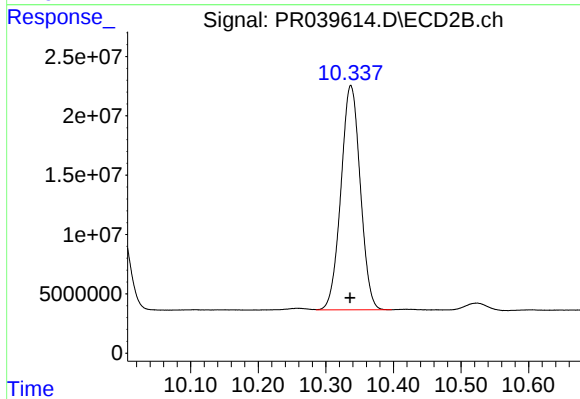

#2 Decachlorobiphenyl

R.T.: 10.337 min
Delta R.T.: 0.001 min
Response: 375954556
Conc: 40.05 ng/ml

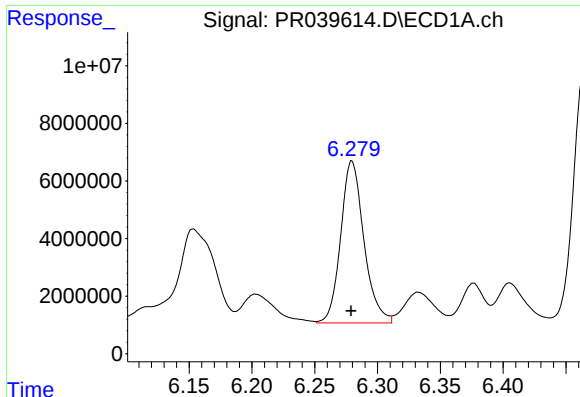


#31 AR-1260-1

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 72474937
Conc: 497.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
K580-S3DL


Manual Integrations
APPROVED

Ankita
7/23/2019 5:14:09 PM

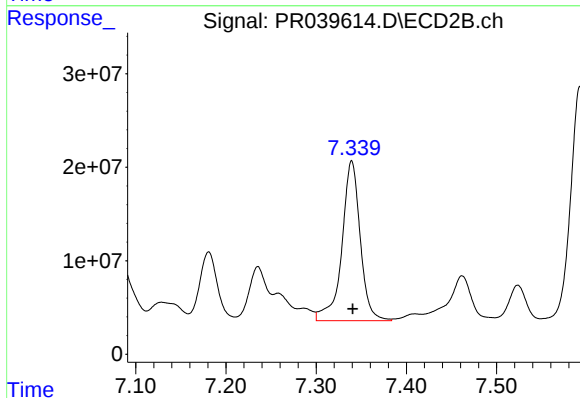


#31 AR-1260-1

R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 241971151
Conc: 545.32 ng/ml

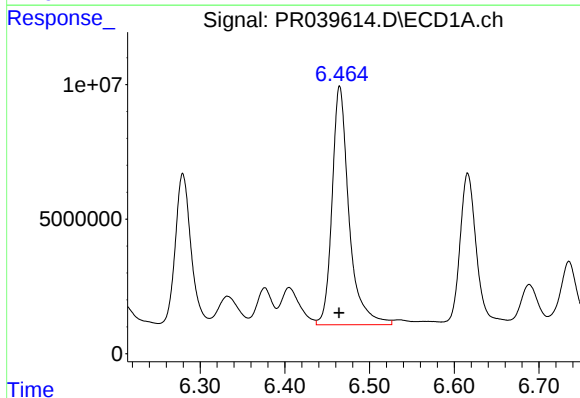


#32 AR-1260-2

R.T.: 6.465 min
Delta R.T.: 0.000 min
Response: 123261878
Conc: 669.49 ng/ml

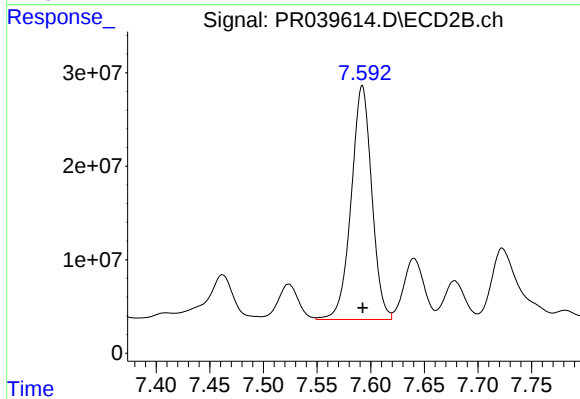

#32 AR-1260-2

R.T.: 7.592 min
Delta R.T.: 0.000 min
Response: 334654986
Conc: 610.50 ng/ml

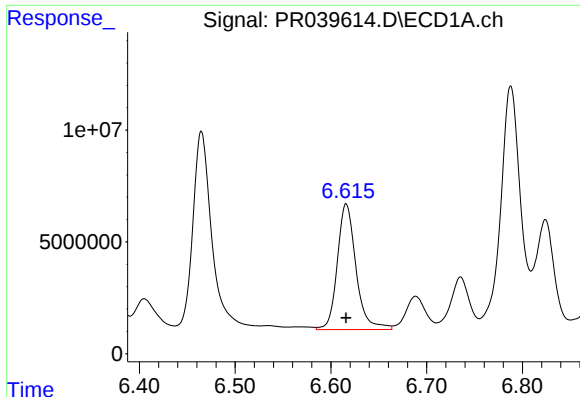


#33 AR-1260-3

R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 76415926
Conc: 461.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
K580-S3DL


Manual Integrations
APPROVED

Ankita
7/23/2019 5:14:09 PM

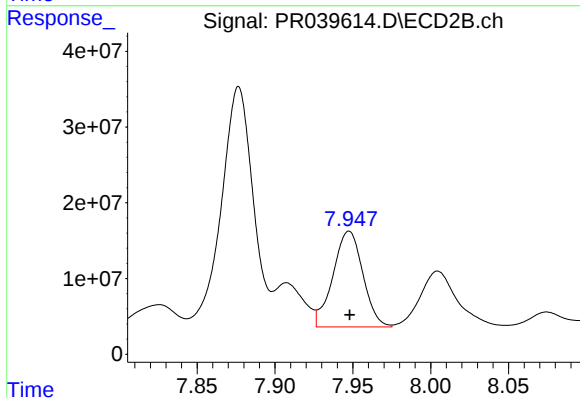


#33 AR-1260-3

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 169422655
Conc: 404.12 ng/ml

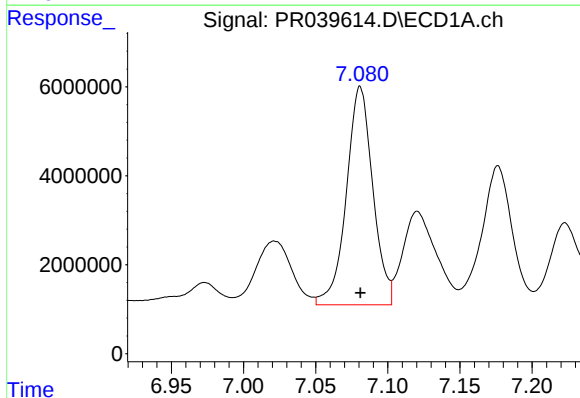


#34 AR-1260-4

R.T.: 7.081 min
Delta R.T.: 0.000 min
Response: 62752228
Conc: 451.43 ng/ml

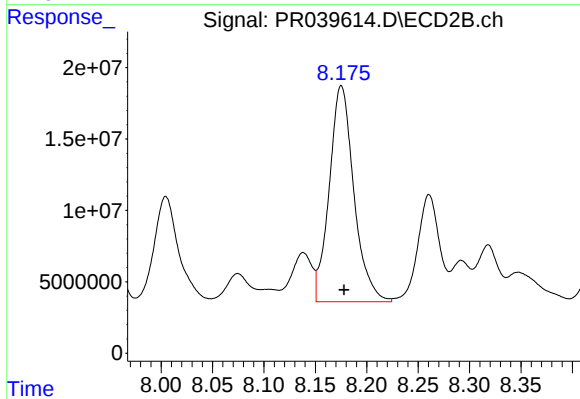

#34 AR-1260-4

R.T.: 8.175 min
Delta R.T.: -0.003 min
Response: 252345936
Conc: 523.01 ng/ml

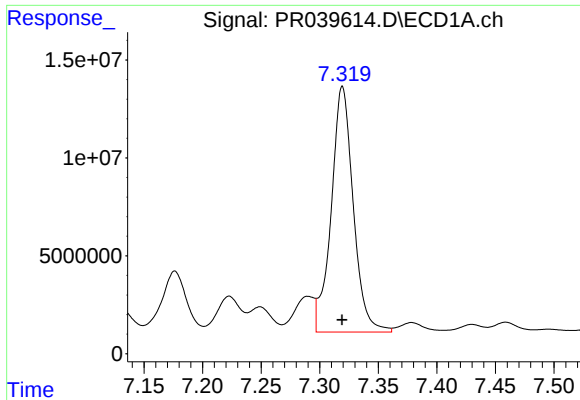


#35 AR-1260-5

R.T.: 7.319 min
Delta R.T.: 0.000 min
Response: 164077164
Conc: 475.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
K580-S3DL

Manual Integrations
APPROVED

Ankita
7/23/2019 5:14:09 PM

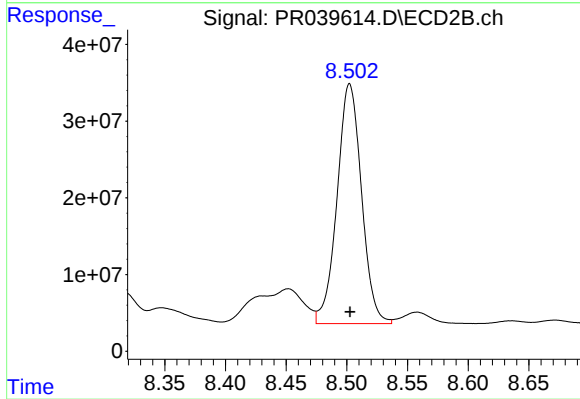

#35 AR-1260-5

R.T.: 8.502 min
Delta R.T.: 0.000 min
Response: 438947210
Conc: 427.96 ng/ml