

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072719\
 Data File : PR039791.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 18:18
 Operator : SM\AJ
 Sample : K4000-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Ankita
 7/29/2019 8:59:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 01:25:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 22 14:03:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.756	4.601	52136169	193.0E6	21.724m	19.254
2) SA Decachlor...	8.690	10.329	35529058	136.5E6	14.300	14.543

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072719\
Data File : PR039791.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 18:18
Operator : SM\AJ
Sample : K4000-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Ankita
7/29/2019 8:59:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:25:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 22 14:03:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

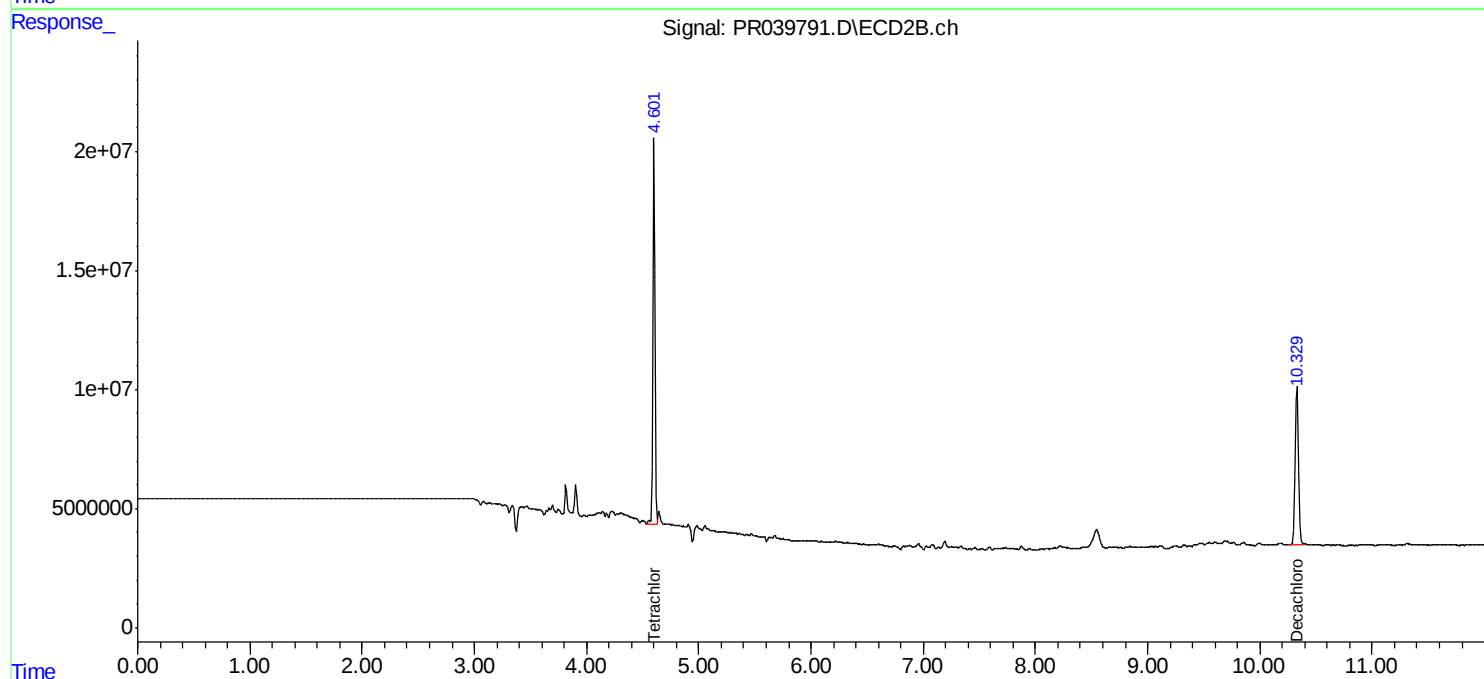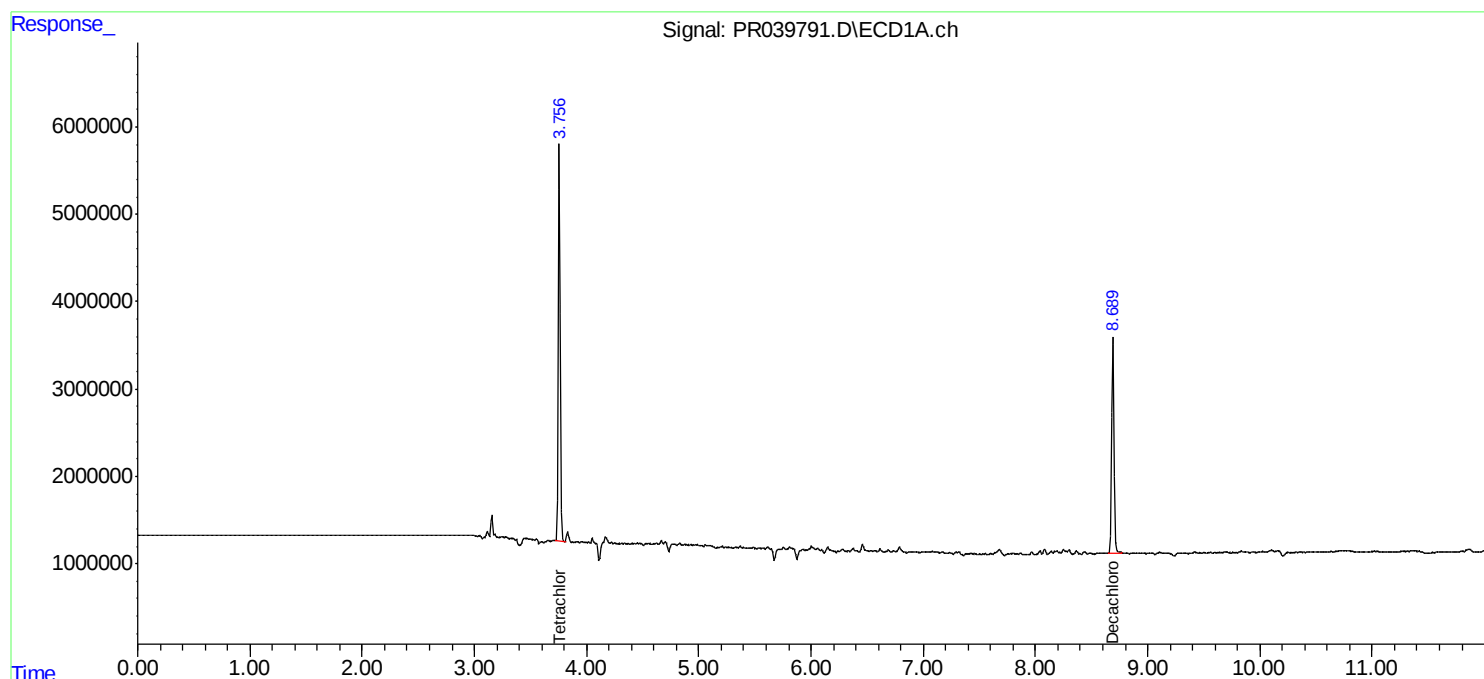

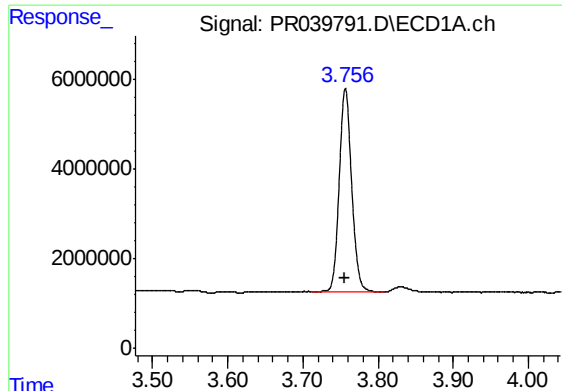


#1 Tetrachloro-m-xylene

R.T.: 3.756 min
Delta R.T.: 0.001 min
Response: 52136169
Conc: 21.72 ng/ml m

Instrument :
ECD_R
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Ankita
7/29/2019 8:59:54 AM

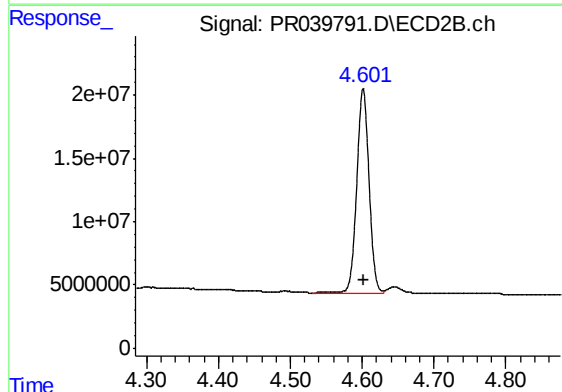


#1 Tetrachloro-m-xylene

R.T.: 4.601 min
Delta R.T.: 0.000 min
Response: 193011525
Conc: 19.25 ng/ml

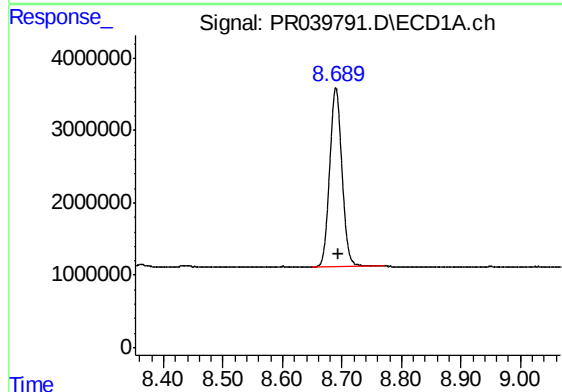

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.005 min
Response: 35529058
Conc: 14.30 ng/ml

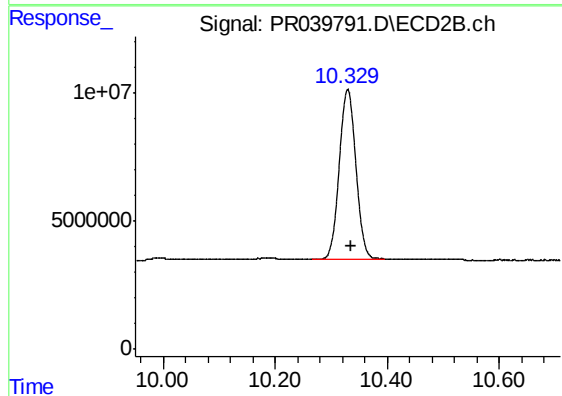

#2 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: -0.006 min
Response: 136524478
Conc: 14.54 ng/ml