

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072719\
Data File : PR039792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 18:33
Operator : SM\AJ
Sample : K4000-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:26:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 22 14:03:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.757	4.601	59408826	228.9E6	24.754	22.836
2) SA Decachlor...	8.689	10.330	41375731	155.9E6	16.653	16.604

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072719\
Data File : PR039792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 18:33
Operator : SM\AJ
Sample : K4000-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:26:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 22 14:03:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

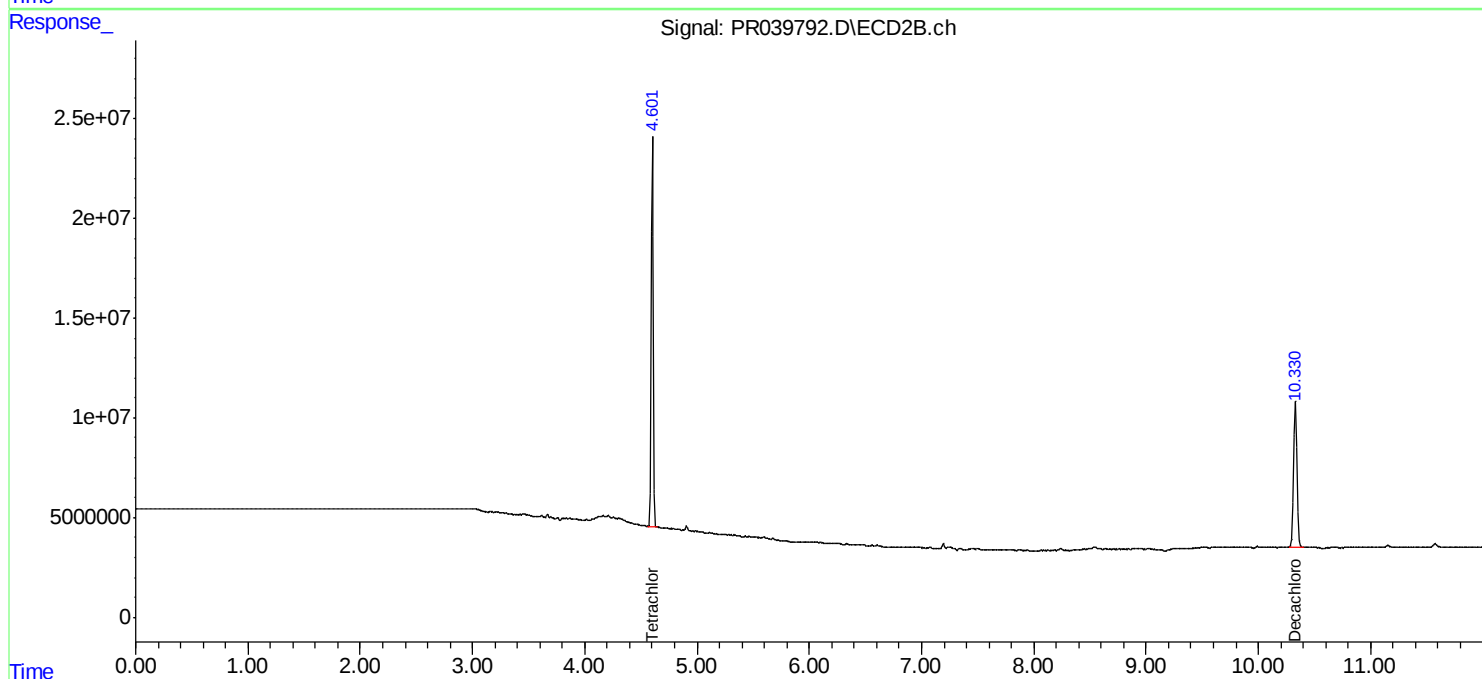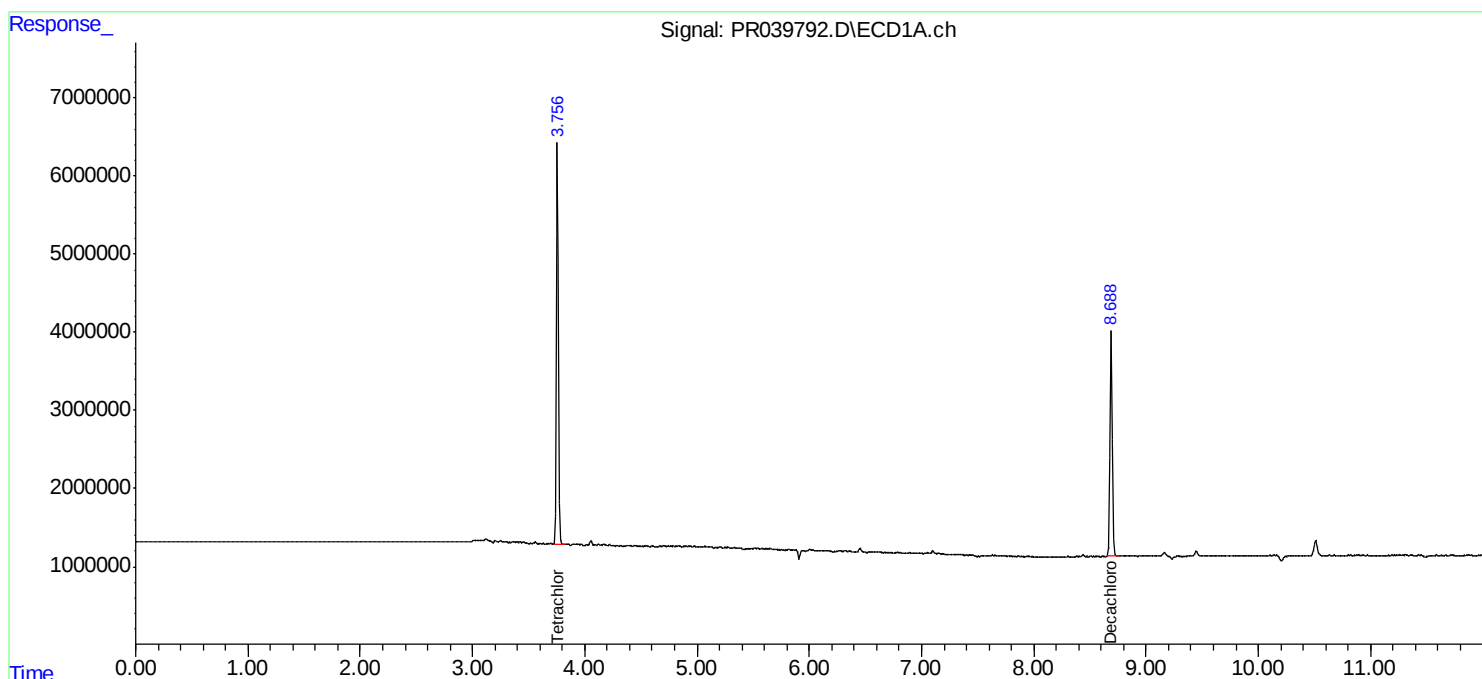


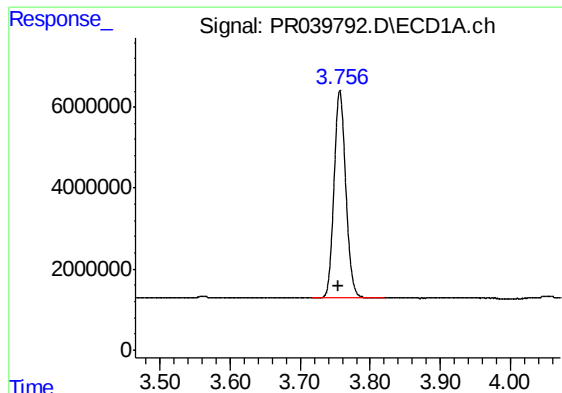

#1 Tetrachloro-m-xylene


R.T.: 3.757 min
Delta R.T.: 0.002 min
Response: 59408826
Conc: 24.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-2

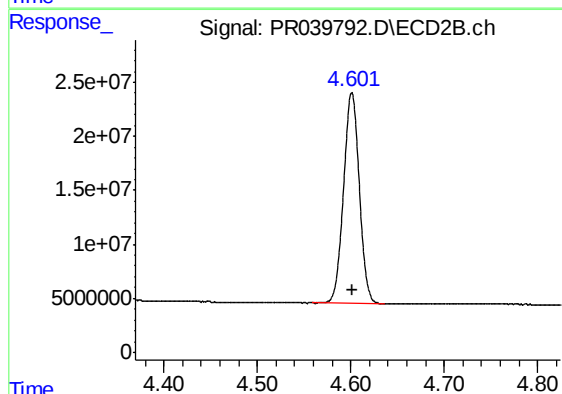


#1 Tetrachloro-m-xylene

R.T.: 4.601 min
Delta R.T.: 0.000 min
Response: 228914191
Conc: 22.84 ng/ml

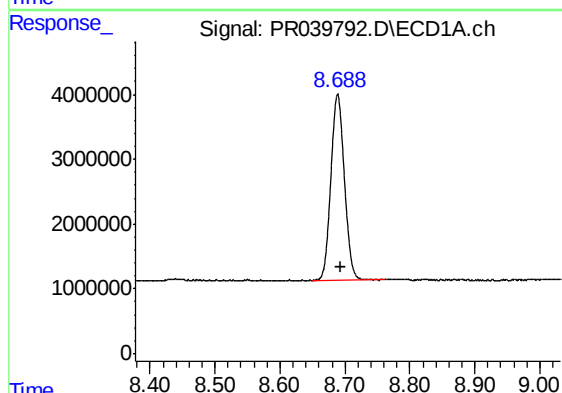

#2 Decachlorobiphenyl

R.T.: 8.689 min
Delta R.T.: -0.006 min
Response: 41375731
Conc: 16.65 ng/ml

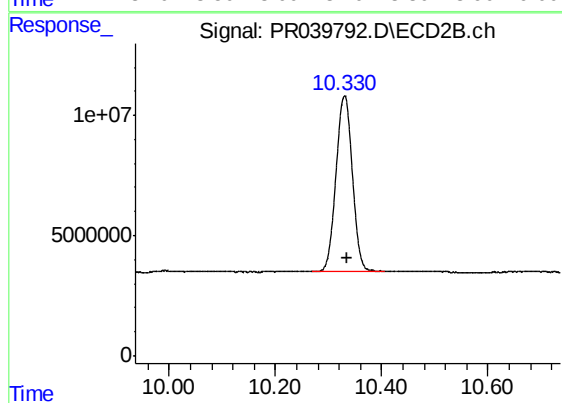

#2 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: -0.006 min
Response: 155875160
Conc: 16.60 ng/ml