

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072719\
Data File : PR039793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 18:47
Operator : SM\AJ
Sample : K4000-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:26:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 22 14:03:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.756	4.601	58554774	230.6E6	24.398	23.001
2) SA Decachlor...	8.689	10.330	41493262	153.8E6	16.700	16.383

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072719\
Data File : PR039793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 18:47
Operator : SM\AJ
Sample : K4000-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:26:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 22 14:03:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

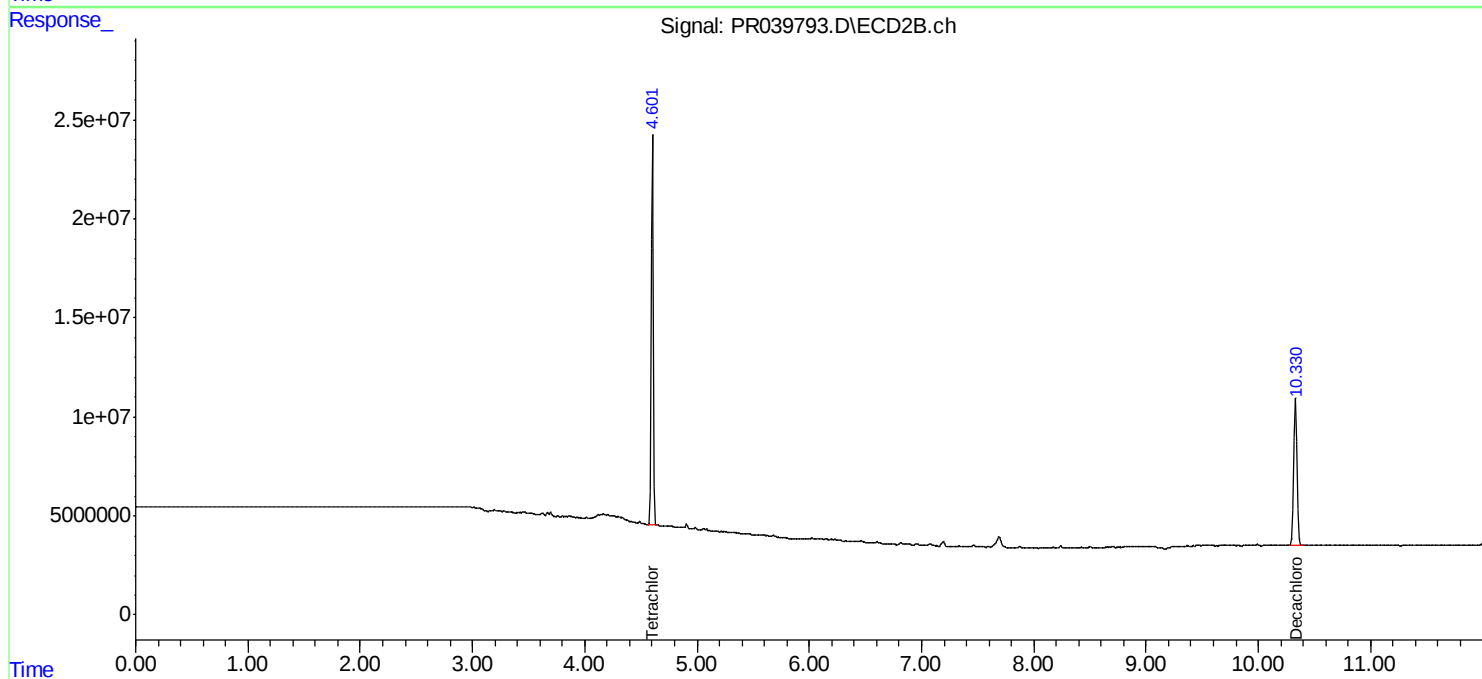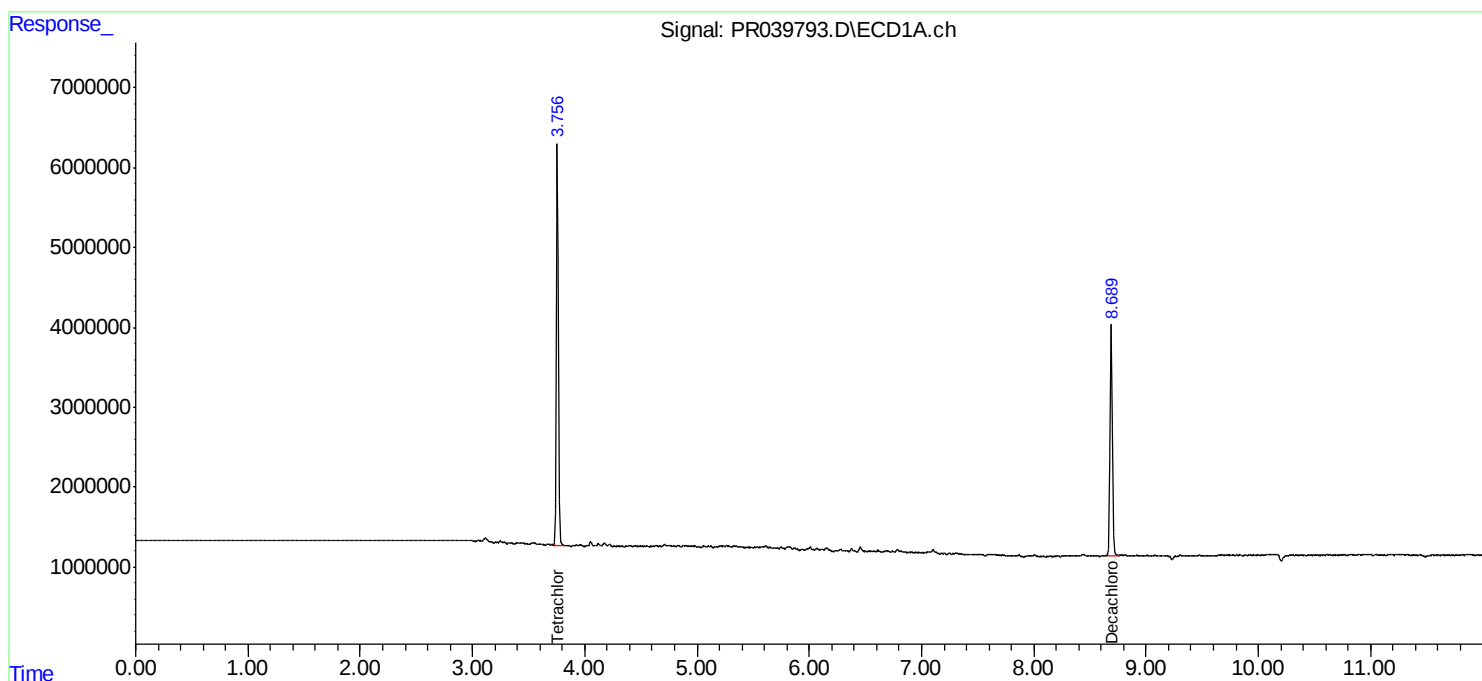


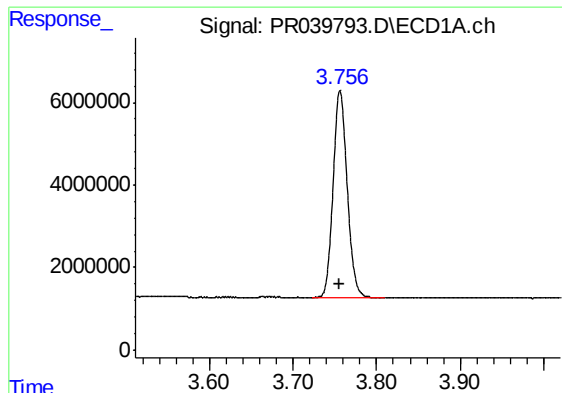

#1 Tetrachloro-m-xylene


R.T.: 3.756 min
Delta R.T.: 0.001 min
Response: 58554774
Conc: 24.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-3

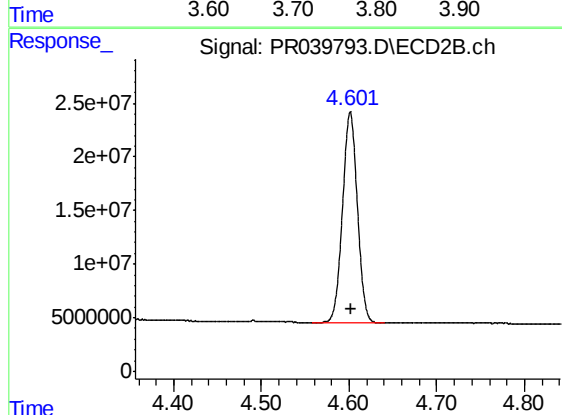


#1 Tetrachloro-m-xylene

R.T.: 4.601 min
Delta R.T.: 0.000 min
Response: 230564980
Conc: 23.00 ng/ml

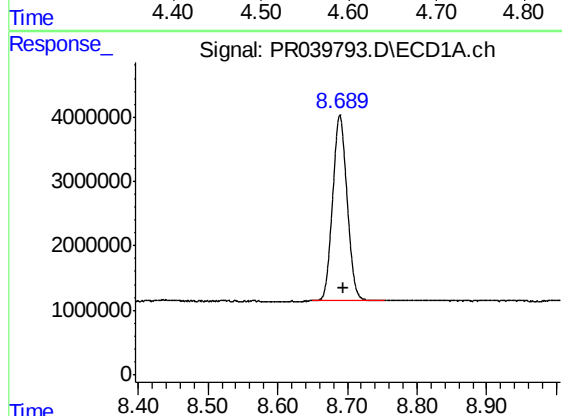

#2 Decachlorobiphenyl

R.T.: 8.689 min
Delta R.T.: -0.006 min
Response: 41493262
Conc: 16.70 ng/ml

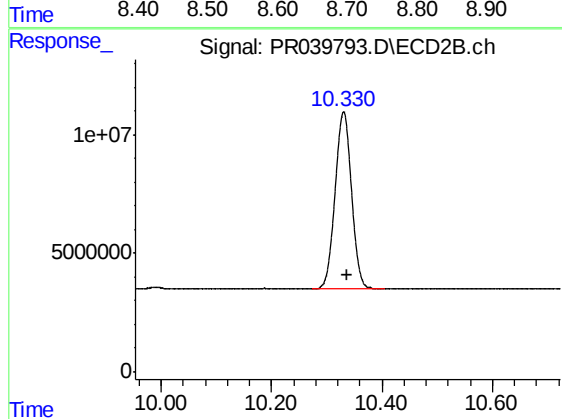

#2 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: -0.005 min
Response: 153799694
Conc: 16.38 ng/ml