

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072719\
 Data File : PR039806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 22:39
 Operator : SM\AJ
 Sample : K3992-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 55-ST-19

Manual Integrations
 APPROVED

Ankita
 7/29/2019 9:00:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 01:31:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 22 14:03:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.756	4.601	39433062	158.0E6	16.431m	15.766
2) SA Decachlor...	8.688	10.329	30676016	115.4E6	12.346	12.296

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR072719\
Data File : PR039806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 22:39
Operator : SM\AJ
Sample : K3992-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
55-ST-19


Manual Integrations
APPROVED

Ankita
7/29/2019 9:00:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:31:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 22 14:03:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

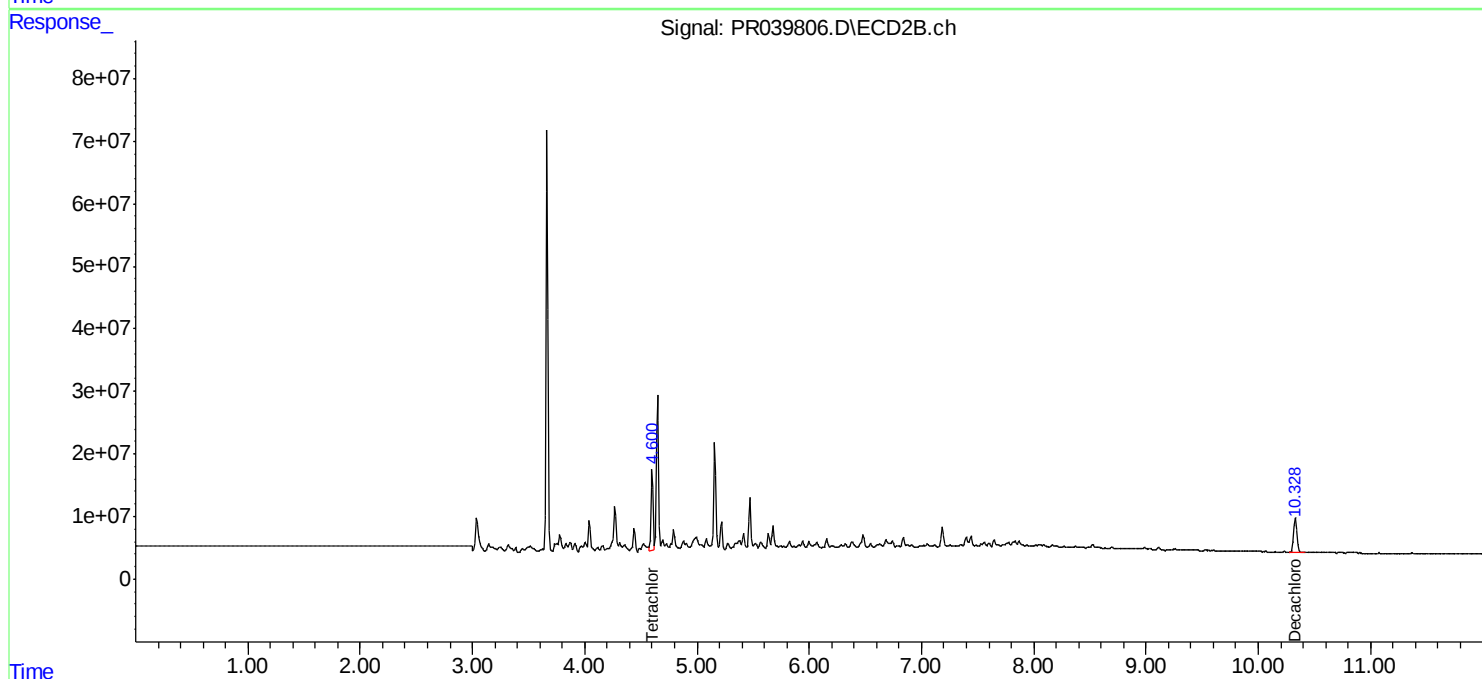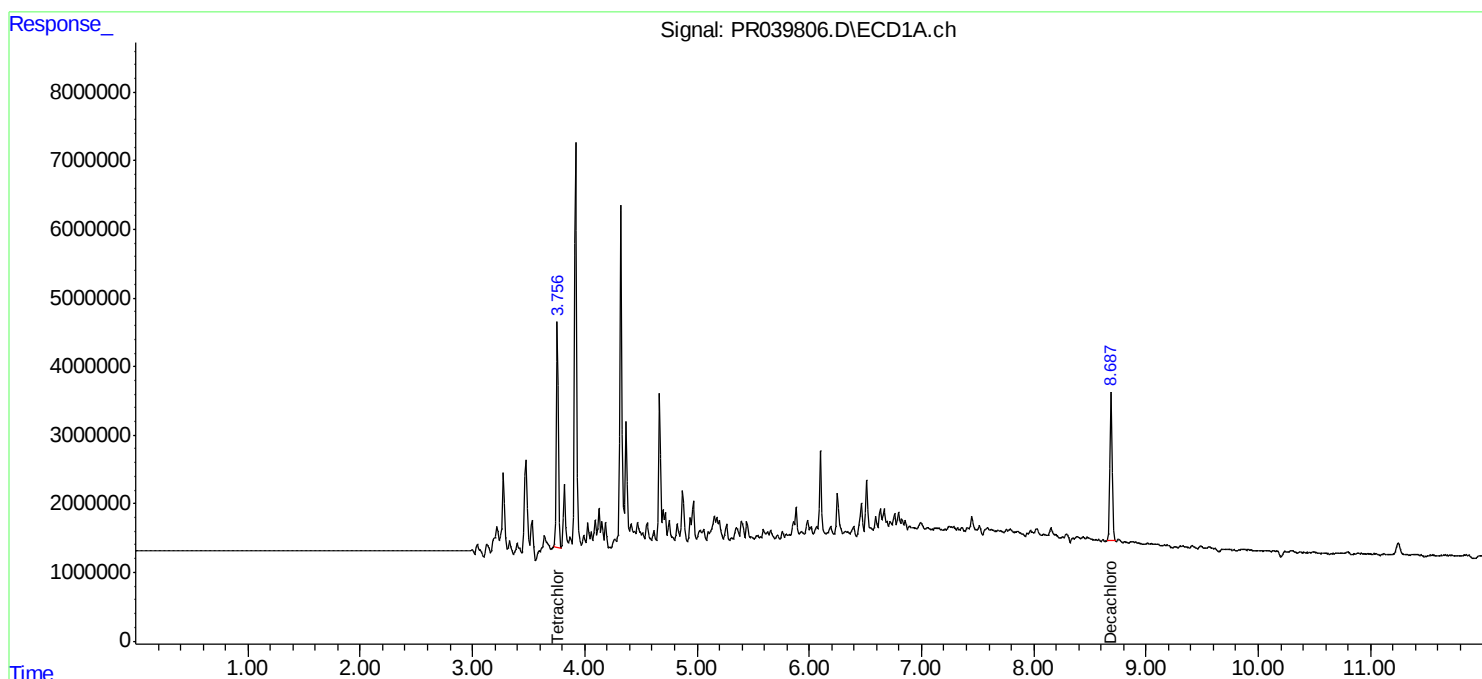

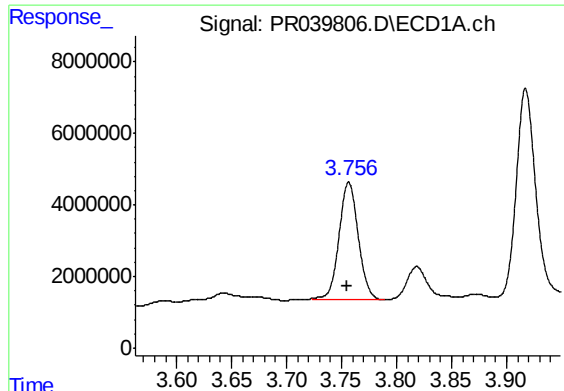


#1 Tetrachloro-m-xylene

R.T.: 3.756 min
Delta R.T.: 0.000 min
Response: 39433062
Conc: 16.43 ng/ml m

Instrument :
ECD_R
ClientSampleId :
55-ST-19


Manual Integrations
APPROVED

Ankita
7/29/2019 9:00:00 AM

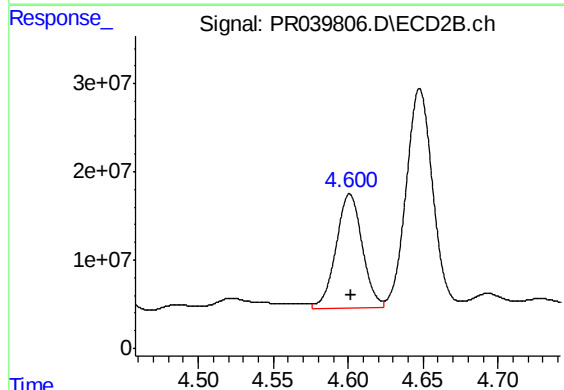


#1 Tetrachloro-m-xylene

R.T.: 4.601 min
Delta R.T.: -0.001 min
Response: 158038126
Conc: 15.77 ng/ml

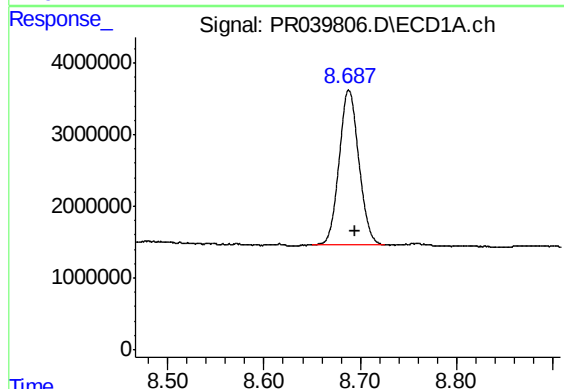

#2 Decachlorobiphenyl

R.T.: 8.688 min
Delta R.T.: -0.007 min
Response: 30676016
Conc: 12.35 ng/ml

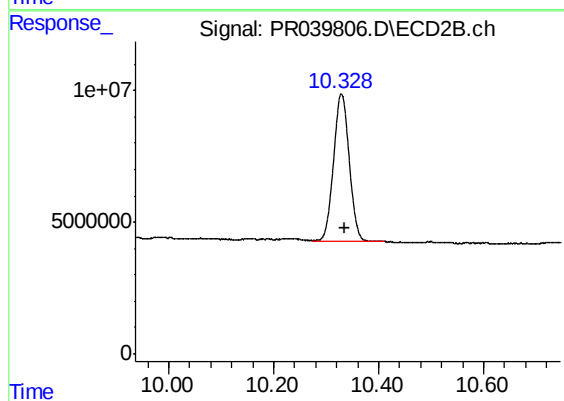

#2 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: -0.007 min
Response: 115435870
Conc: 12.30 ng/ml