

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081119\
 Data File : PR040264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2019 10:47
 Operator : SM\AJ
 Sample : K4245-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 COMP-26

Manual Integrations
 APPROVED

Ankita
 8/14/2019 10:03:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 02:00:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR081019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 10 07:38:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.750	4.591	51628984	210.8E6	21.544m	20.251
2)	SA Decachlor...	8.676	10.310	31625214	147.8E6	12.996	16.875 #
Target Compounds							
31)	L7 AR-1260-1	6.266	7.324	15514131	56719780	134.854m	155.254
32)	L7 AR-1260-2	6.447	7.576	23743633	83783910	164.891m	184.159
33)	L7 AR-1260-3	6.601	7.932	11500705	28448504	85.175m	82.721
34)	L7 AR-1260-4	7.066	8.160	6083531	32889870	53.881	83.654 #
35)	L7 AR-1260-5	7.305	8.486	20330525	60276909	72.130	70.360

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081119\
Data File : PR040264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2019 10:47
Operator : SM\AJ
Sample : K4245-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
COMP-26


Manual Integrations
APPROVED

Ankita
8/14/2019 10:03:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 02:00:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR081019.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 10 07:38:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

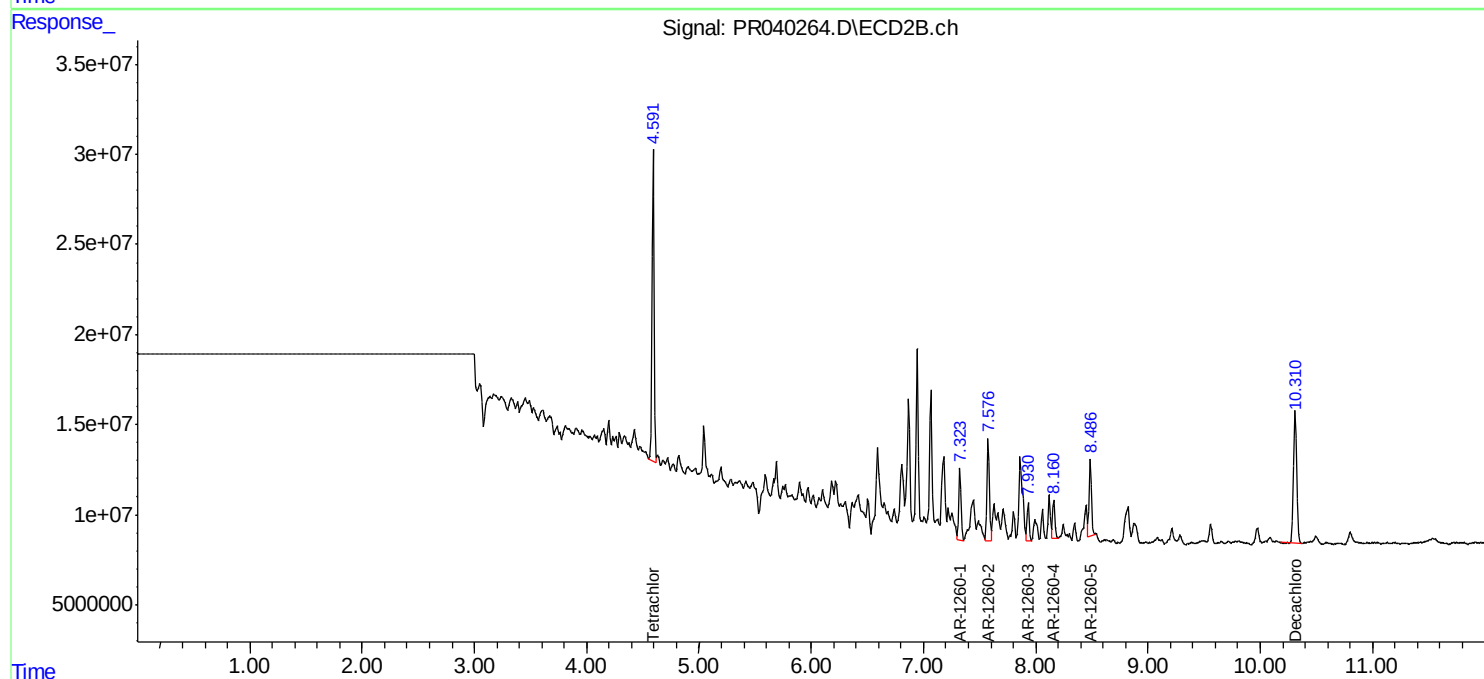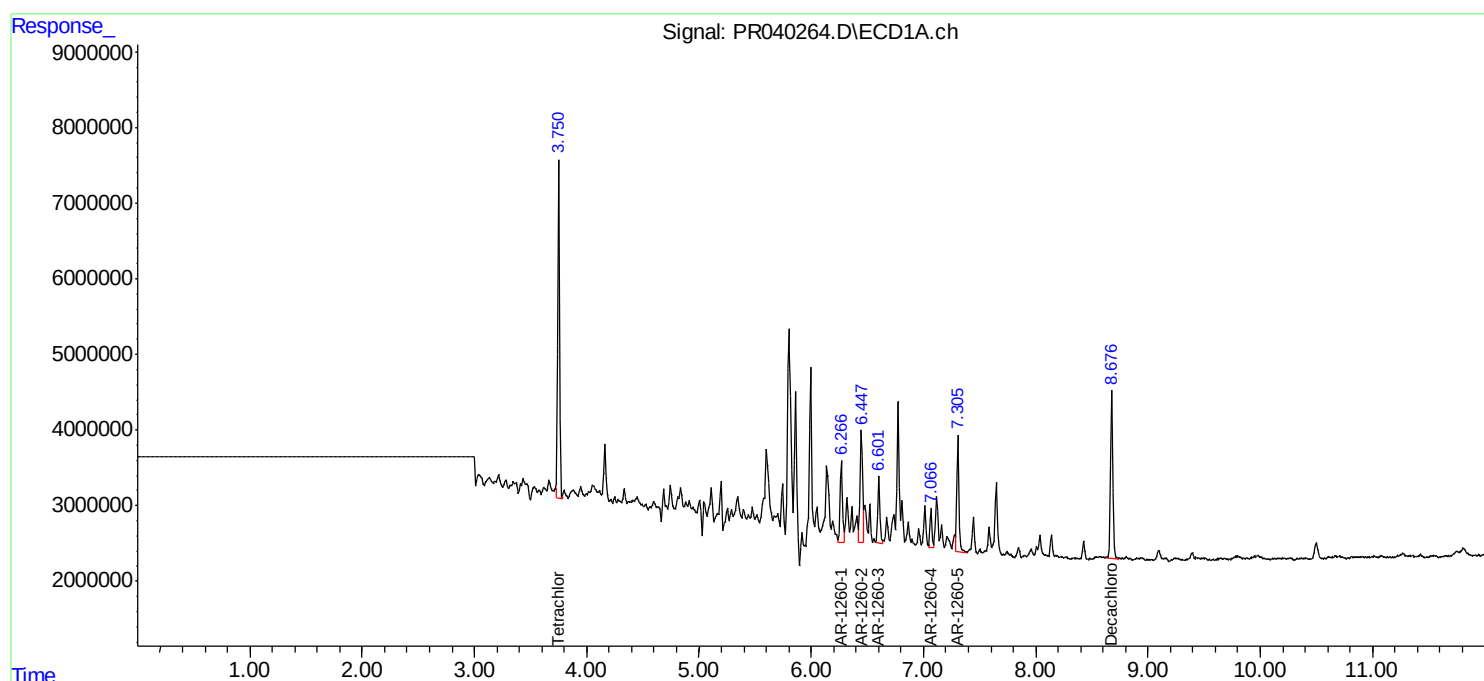

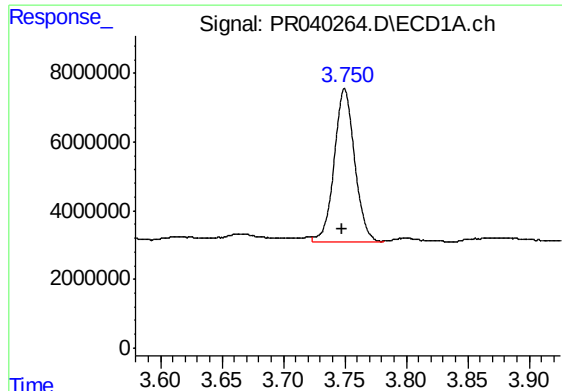


#1 Tetrachloro-m-xylene

R.T.: 3.750 min
Delta R.T.: 0.002 min
Response: 51628984
Conc: 21.54 ng/ml m

Instrument :
ECD_R
ClientSampleId :
COMP-26


Manual Integrations
APPROVED

Ankita
8/14/2019 10:03:50 AM

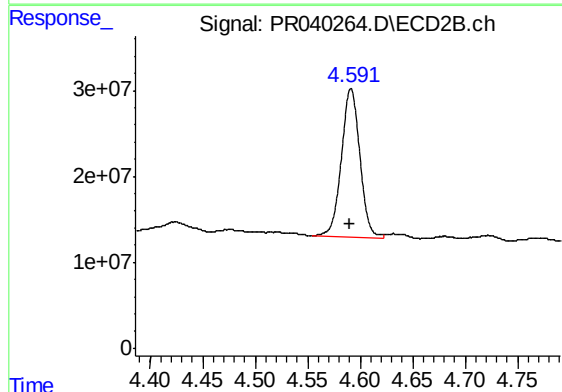


#1 Tetrachloro-m-xylene

R.T.: 4.591 min
Delta R.T.: 0.001 min
Response: 210839263
Conc: 20.25 ng/ml

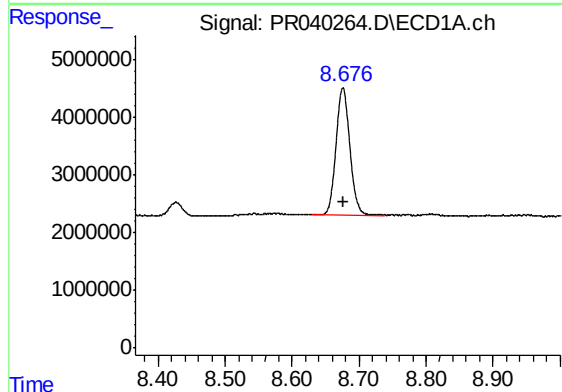


#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.002 min
Response: 31625214
Conc: 13.00 ng/ml

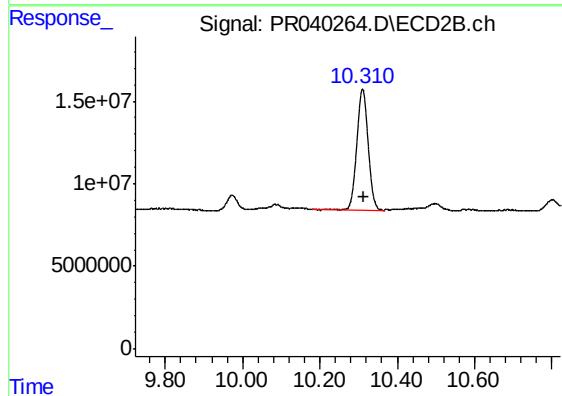

#2 Decachlorobiphenyl

R.T.: 10.310 min
Delta R.T.: -0.004 min
Response: 147788707
Conc: 16.88 ng/ml

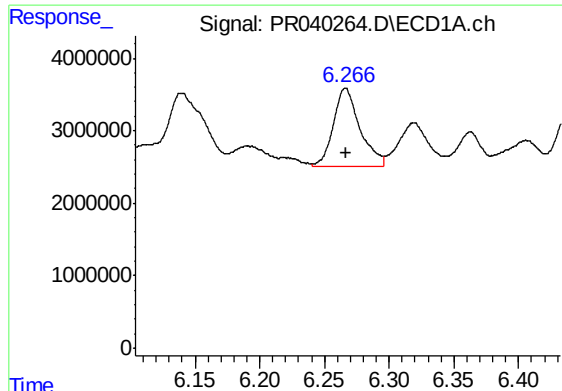


#31 AR-1260-1

R.T.: 6.266 min
Delta R.T.: 0.000 min
Response: 15514131
Conc: 134.85 ng/ml m

Instrument :
ECD_R
ClientSampleId :
COMP-26


Manual Integrations
APPROVED

Ankita
8/14/2019 10:03:50 AM

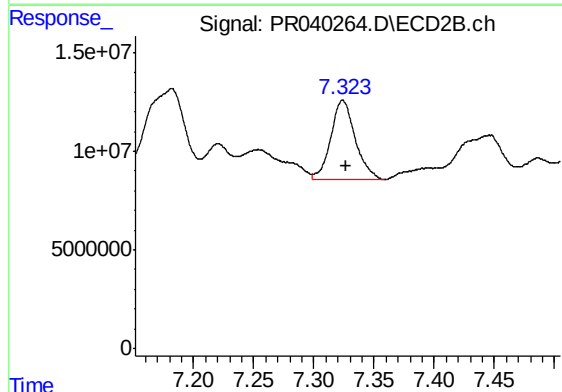


#31 AR-1260-1

R.T.: 7.324 min
Delta R.T.: -0.003 min
Response: 56719780
Conc: 155.25 ng/ml

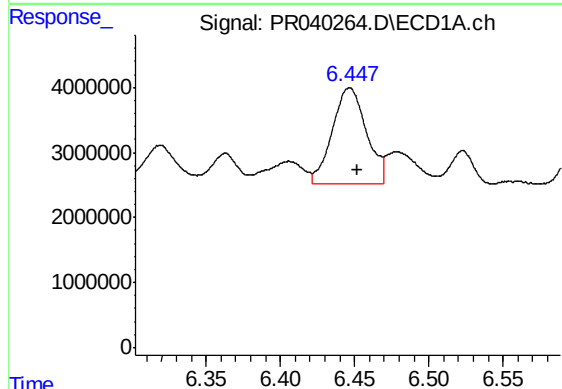


#32 AR-1260-2

R.T.: 6.447 min
Delta R.T.: -0.005 min
Response: 23743633
Conc: 164.89 ng/ml m

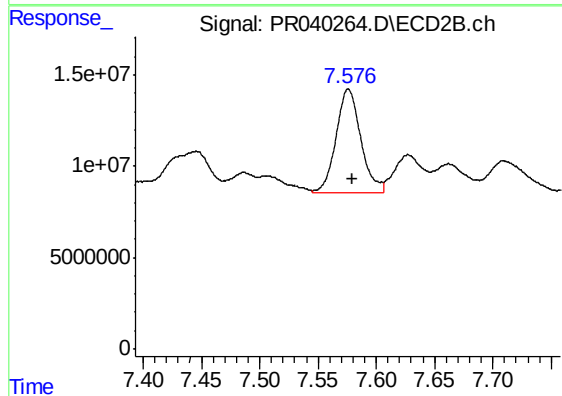

#32 AR-1260-2

R.T.: 7.576 min
Delta R.T.: -0.003 min
Response: 83783910
Conc: 184.16 ng/ml

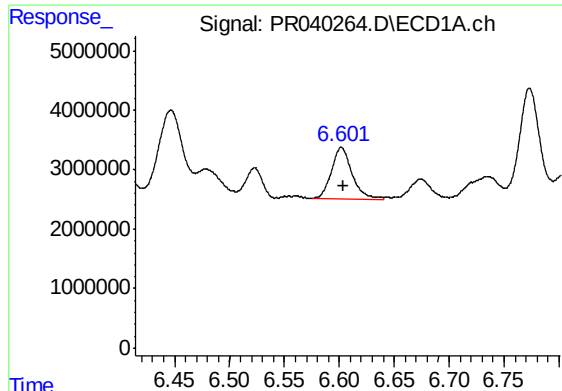


#33 AR-1260-3

R.T.: 6.601 min
Delta R.T.: -0.002 min
Response: 11500705
Conc: 85.18 ng/ml m

Instrument :
ECD_R
ClientSampleId :
COMP-26


Manual Integrations
APPROVED

Ankita
8/14/2019 10:03:50 AM

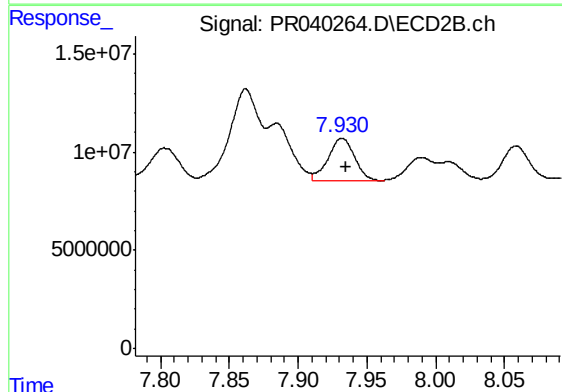


#33 AR-1260-3

R.T.: 7.932 min
Delta R.T.: -0.003 min
Response: 28448504
Conc: 82.72 ng/ml

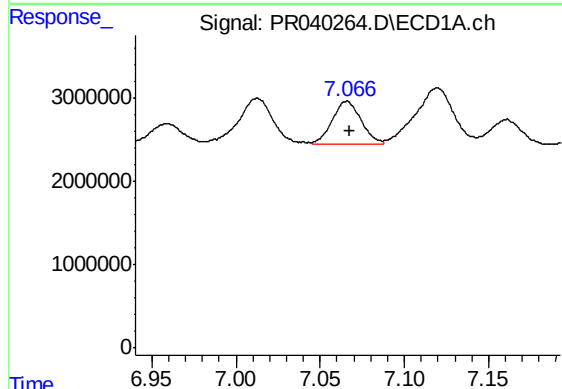


#34 AR-1260-4

R.T.: 7.066 min
Delta R.T.: -0.002 min
Response: 6083531
Conc: 53.88 ng/ml

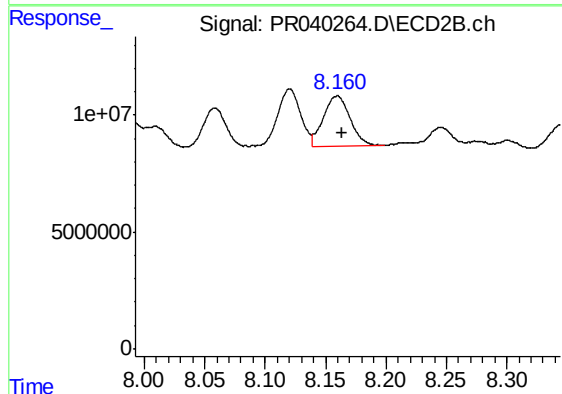

#34 AR-1260-4

R.T.: 8.160 min
Delta R.T.: -0.004 min
Response: 32889870
Conc: 83.65 ng/ml

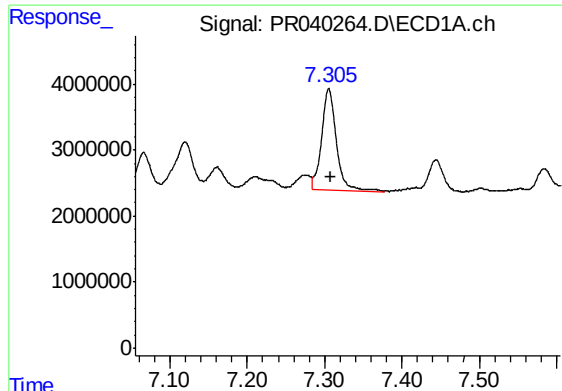


#35 AR-1260-5

R.T.: 7.305 min
Delta R.T.: -0.002 min
Response: 20330525
Conc: 72.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
COMP-26

Manual Integrations
APPROVED

Ankita
8/14/2019 10:03:50 AM

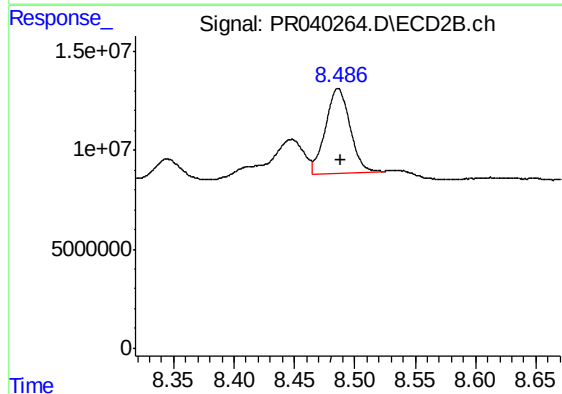

#35 AR-1260-5

R.T.: 8.486 min
Delta R.T.: -0.002 min
Response: 60276909
Conc: 70.36 ng/ml